



1.Основной блок




















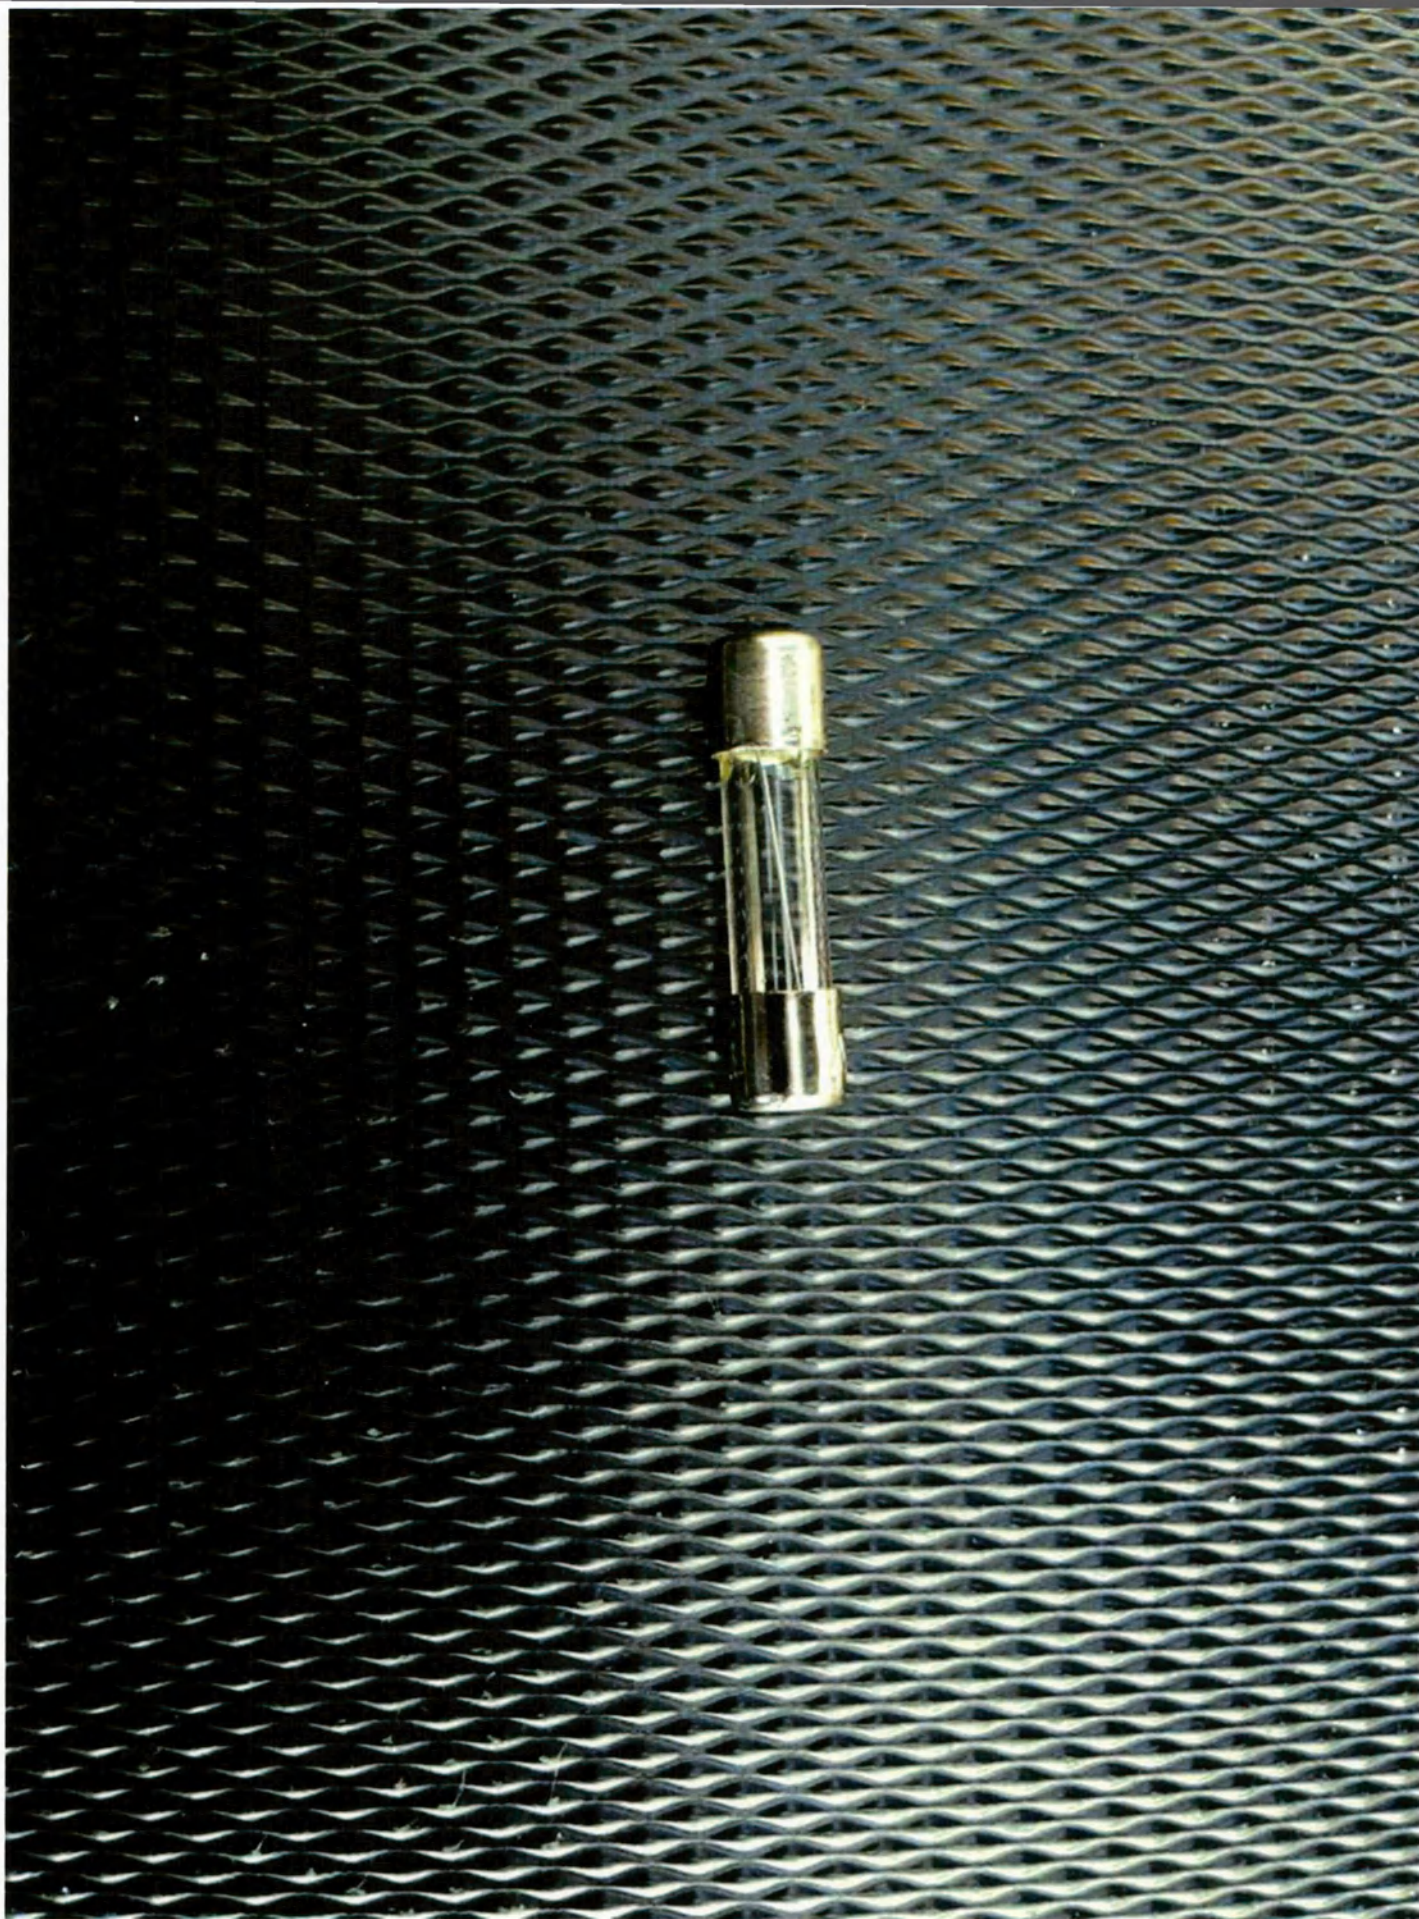

6.Предохранители






7. Чехол защитный



INSTRUCTION MANUAL

OPHTHALMOLOGIC ULTRASONIC
DIAGNOSTIC DEVICE
UD-8000 with accessories

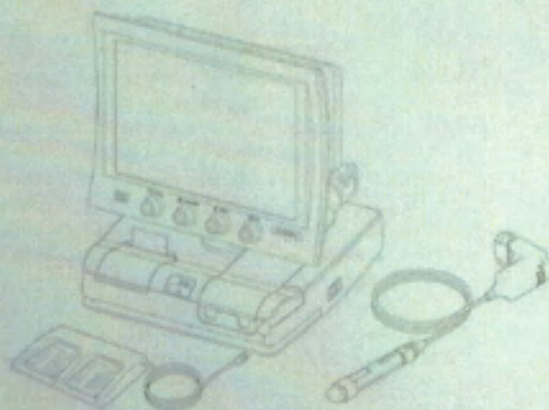

Read this manual thoroughly before using the instrument to ensure proper and safe operation. Contact Tomey Corporation or our local distributor if you have any questions or you encounter any problems during operation.

Note

- Always follow the operation procedures described in this manual.
- Keep this manual in a readily accessible location while operating this software.
- Contact our local distributor if you lose this manual.

TOMEY GMBH
Am Weicheelgarten 19a
D-91058 Erlangen-Tengenlohe
Tel. 091 31 / 77 71-0, Fax: 720
www.tomey.de

TOMEY
769A9090-0C

Dr. Zita von Glatz
Regulatory Affairs Manager

8.Руководство пользователя









OPERATOR MANUAL

DATA Transfer Software

In order to use this software properly, please be sure to read through this manual before using this software.

For any questions, please feel free to get in touch with your local distributors or us.

Note Do not use this software in any way other than described in this manual.


Note Users shall assume full responsibility for any data stored and application of any computed data by using this software.

Note Keep this manual in a place where you can refer at any time during use.

Note In case you have lost this manual, please get in touch with your local distributor to obtain another copy.

TOMEY GMBH
Am Walchgraben 19a
D-91058 Erlangen-Tenneltal
Tel. 091 31 9771-0, Fax -20
www.tomey.de

IA. Zita von Glatz
-Regulatory Affairs Manager-



941E9900-0Q

10. Справочник DATA Transfer






11.Бумага для принтера





12. Гель ультразвуковой, 250 мл.




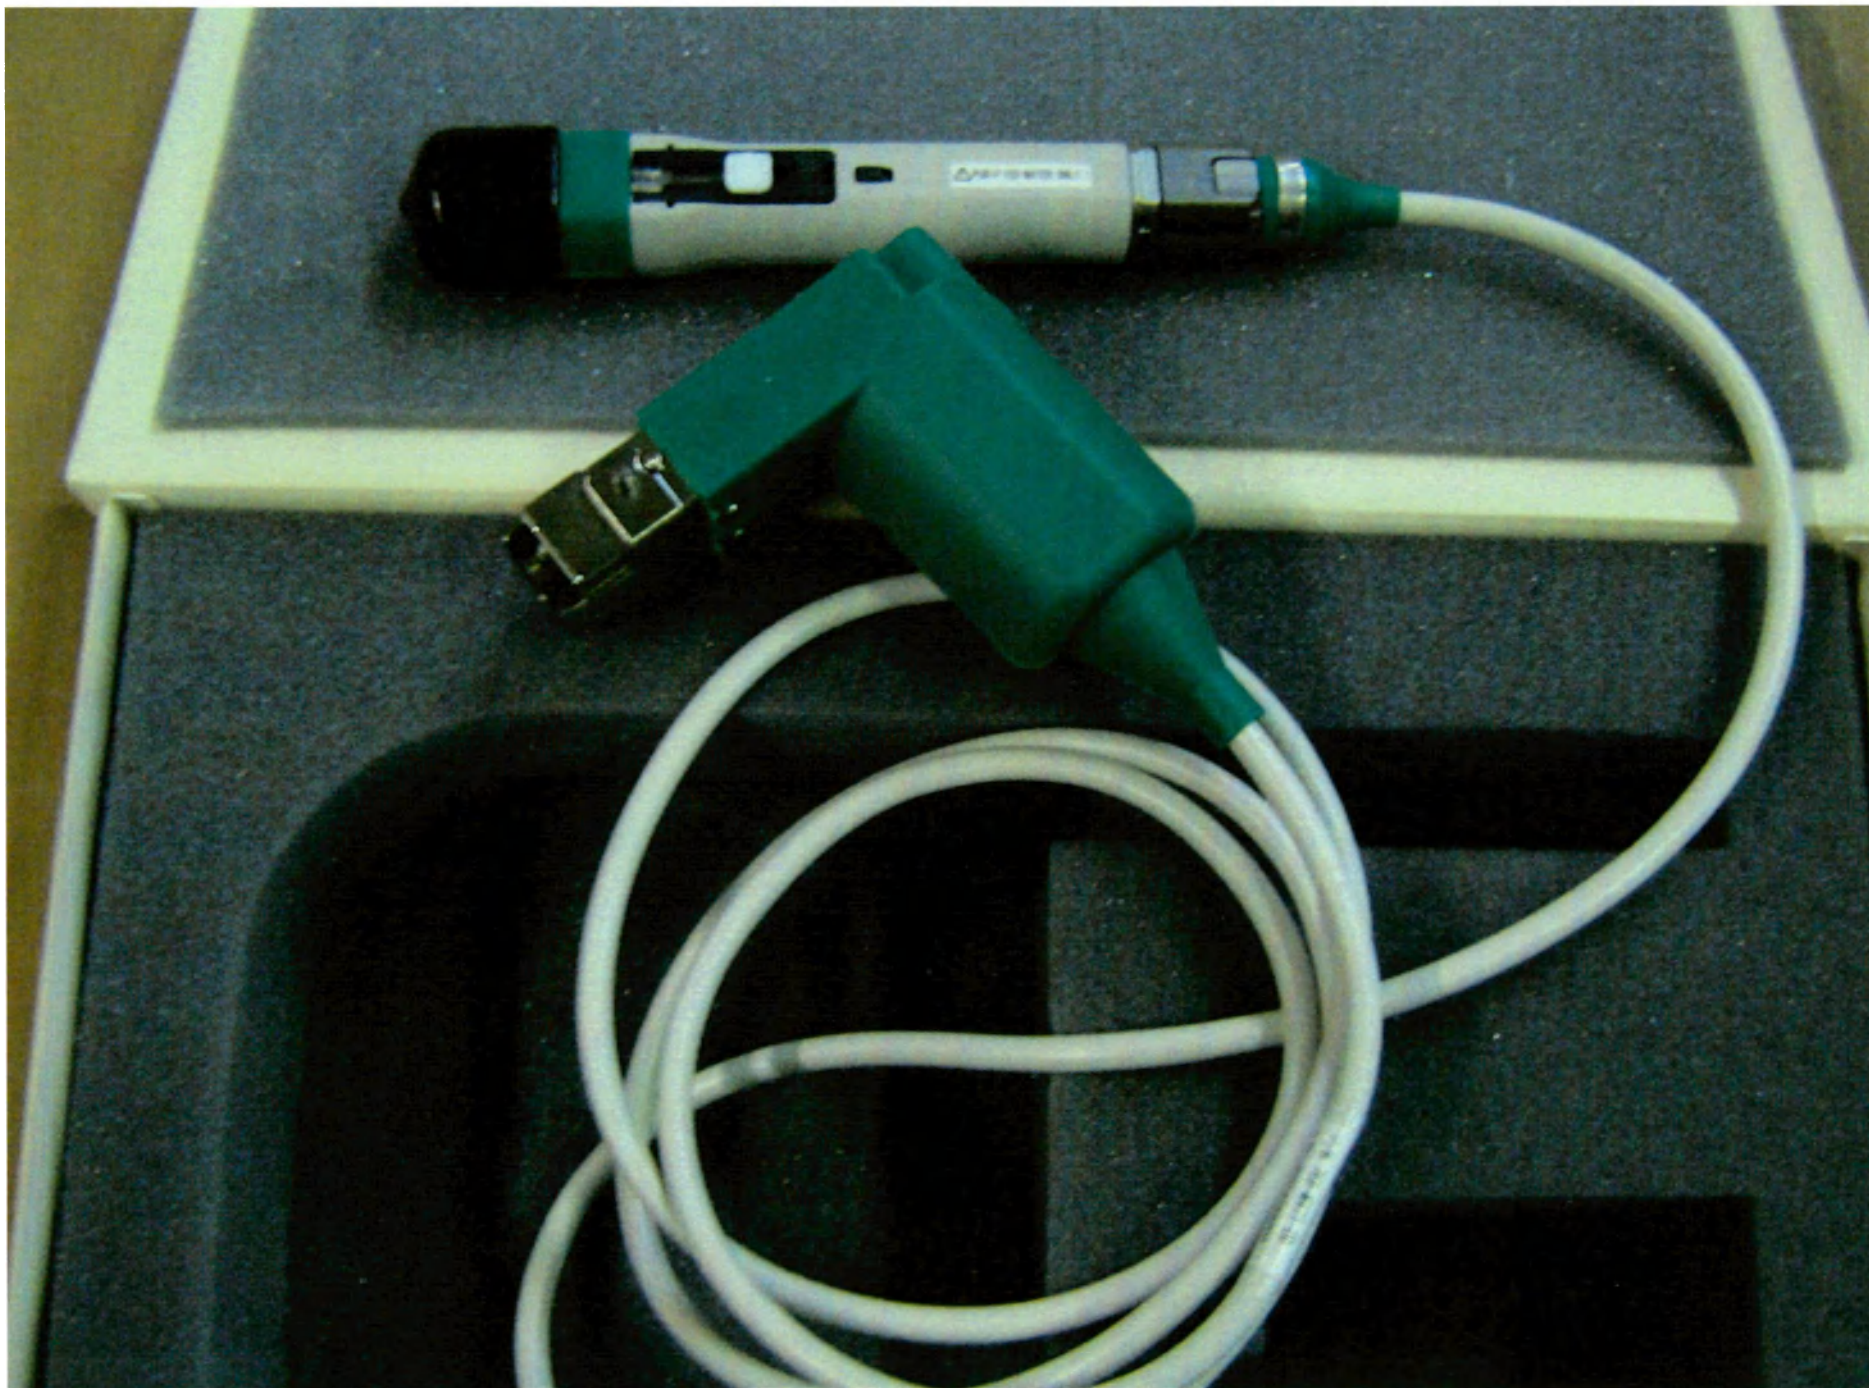








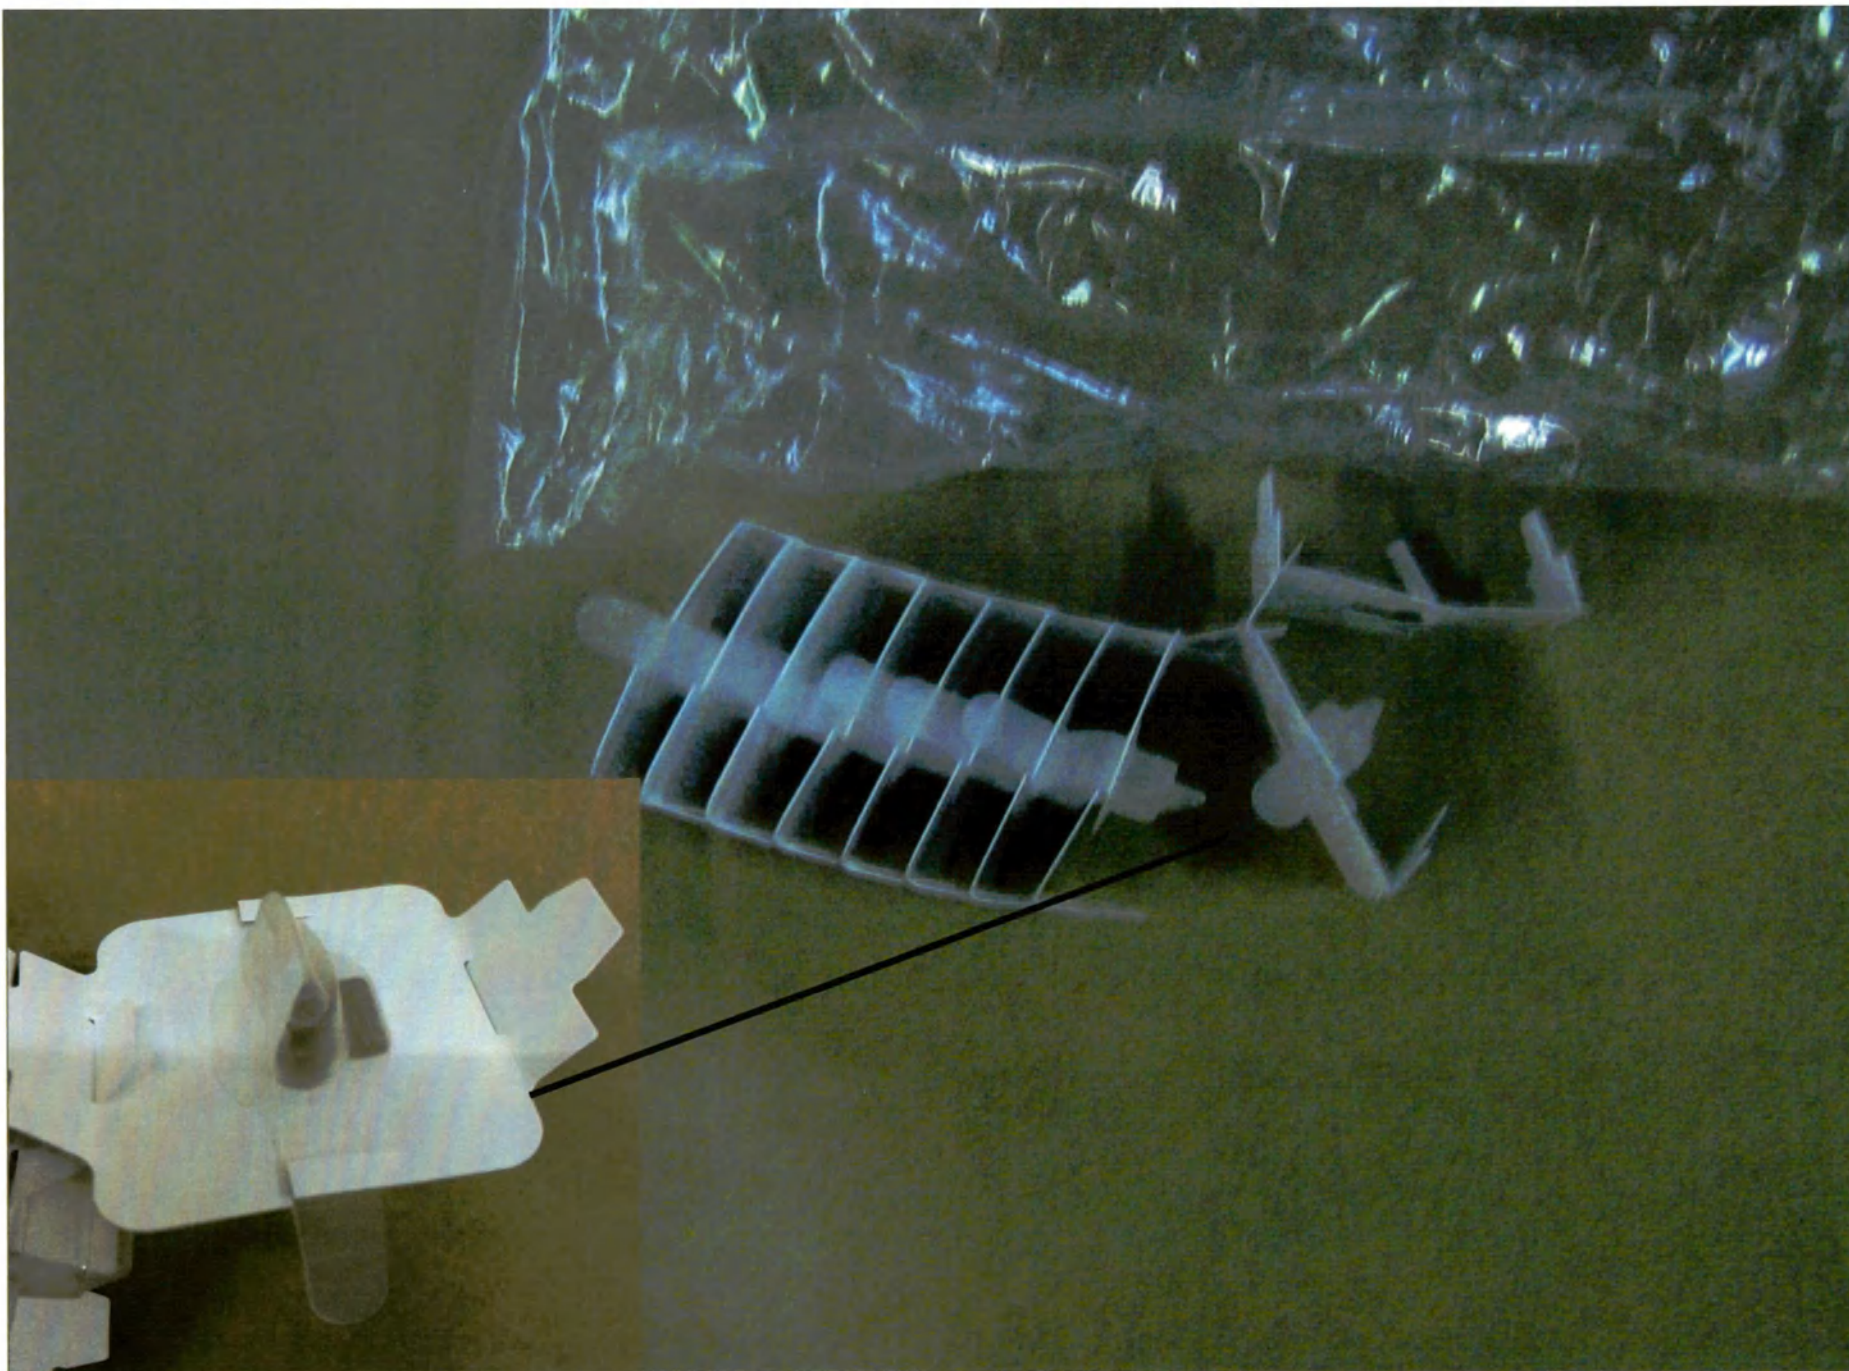

15.Колпачки мембранные



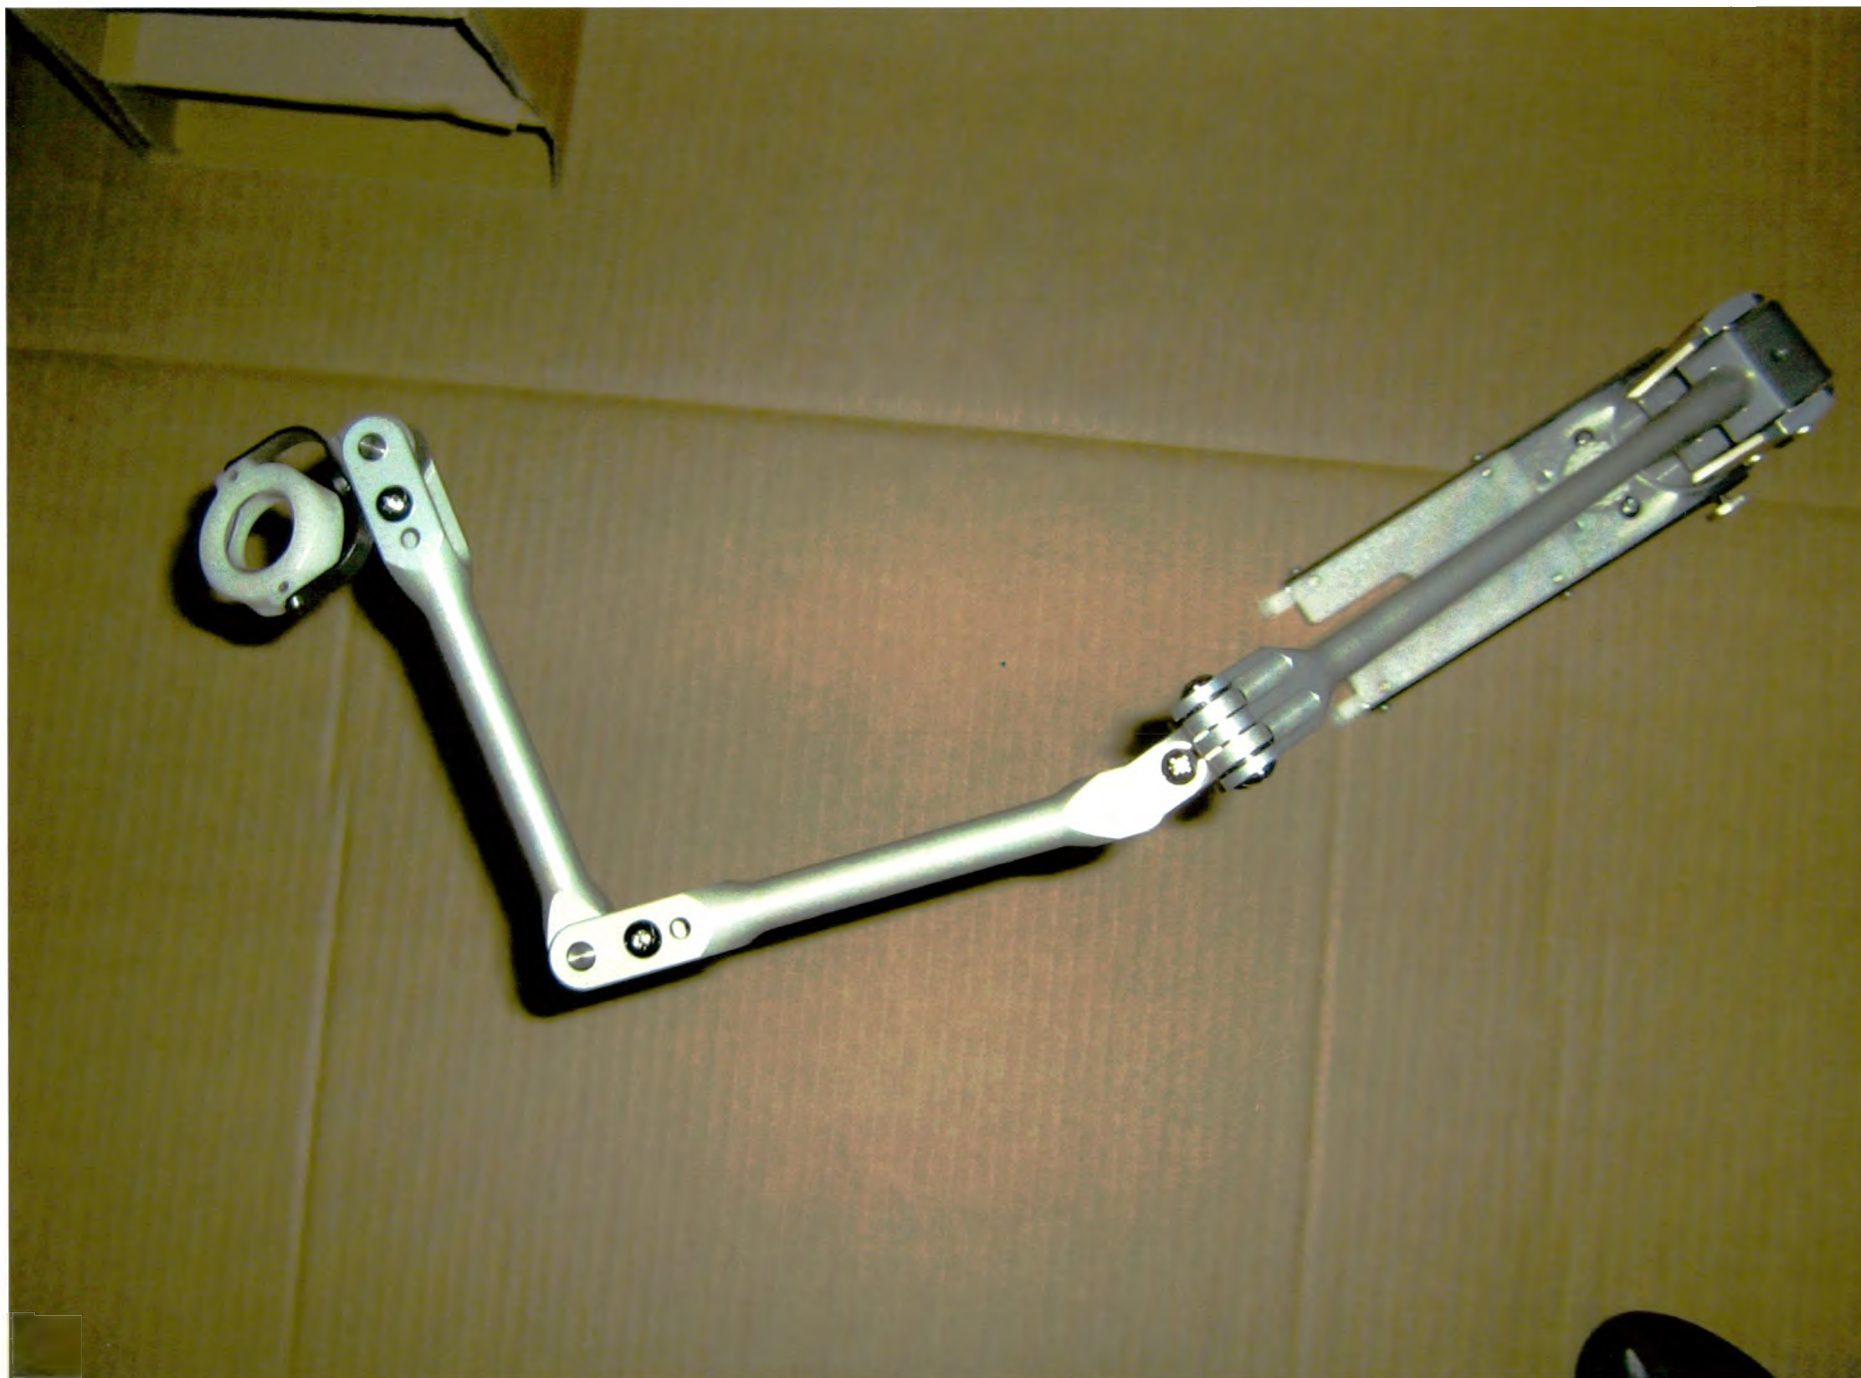

16.Рука-держатель датчика

