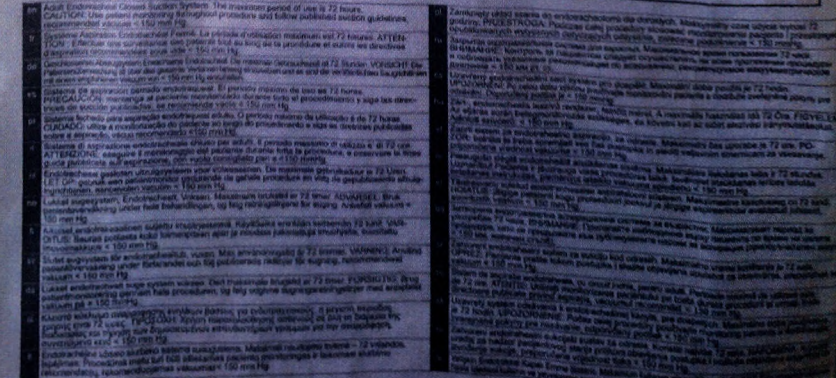


**Фотографические изображения медицинского изделия:
Система закрытая аспирационная для взрослых TrachSeal,
варианты исполнения**

1. Система закрытая аспирационная эндотрахеальная для взрослых TrachSeal. 72 часа, размер катетера 3,3 мм (10Fr);



Intersurgical Ltd.
 Crane House, Motby Millers Lane,
 Wokingham, Berkshire, RG41 2RZ, UK
 T: +44 (0)118 9656 300 F: +44 (0)118 9656 350
 info@intersurgical.com www.intersurgical.com

Deutschland 00241 911063 info@intermagical.de	España T. 91 620 78 18 info@intermagical.es
France 01 48 78 72 30 info@intermagical.fr	Portugal T. 21 410 89 50 info@intermagical.pt
Italia 0038 26496 info@intermagical.it	Niederlande T. 0412 443440 info@intermagical.nl

Литва
T. 267 08611
info@interengrad.lt

Россия
T. 260 771 0809
info@interengrad.ru

Украина
T. 420 27 001 1914
info@interengrad.ua

[illegible][illegible]



2. Система закрытая аспирационная эндотрахеальная для взрослых TrachSeal, 72 часа, размер катетера 4,0 мм (12Fr);

TrachSeal™ Adult Endotracheal Closed Suction System 72 hours


4.0 mm (12Fr)
x 540 mm (21.3 in)

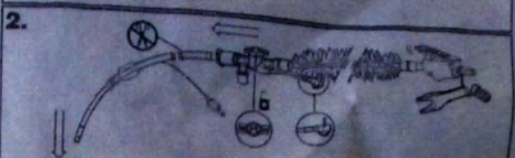
REF 3720000
LOT 341578
2017-05

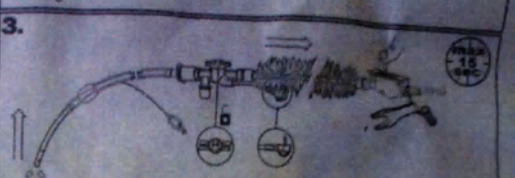
0 30267 087852

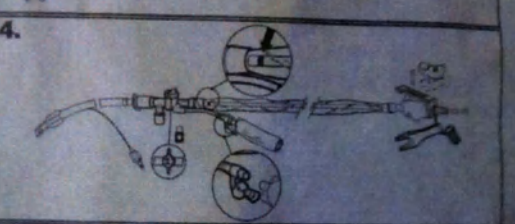
3720000-3-A

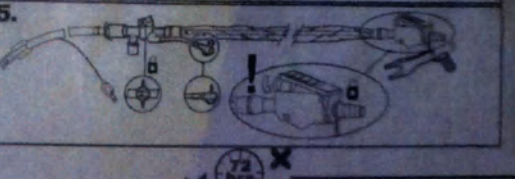
CE 0120
STERILE EO Rx ONLY


1. 

2. 

3. 

4. 

5. 

6. 

INTERSURGICAL

Intersurgical Ltd.
Central Medical Supply Division, Unit 1
The Parkway, Frimley, Surrey GU10 2PH, UK
Tel: +44 (0)1832 254000 Fax: +44 (0)1832 254001
Email: info@intersurgical.com



TrachSeal™ Adult Endotracheal Closed Suction System 72 hours

47 mm (14F)
x 540 mm (21.3 in)

REF 3720001

LOT 341579

2017-05










3720001-3-A



CE
0120


STERILE EO Rx ONLY

[illegible]

INTERSURGICAL
COMPLETE RESPIRATORY SYSTEMS

Intersurgical Ltd.
Crane House, Molly Millars Lane,
Wokingham, Berkshire, RG40 2BZ, UK
T: +44 (0)118 9656 200 F: +44 (0)118 9656 216
info@intersurgical.com www.intersurgical.com





5.3 mm (16F)
x 540 mm (21.3 in)

REF 3720002

LOT 341580

2017-05



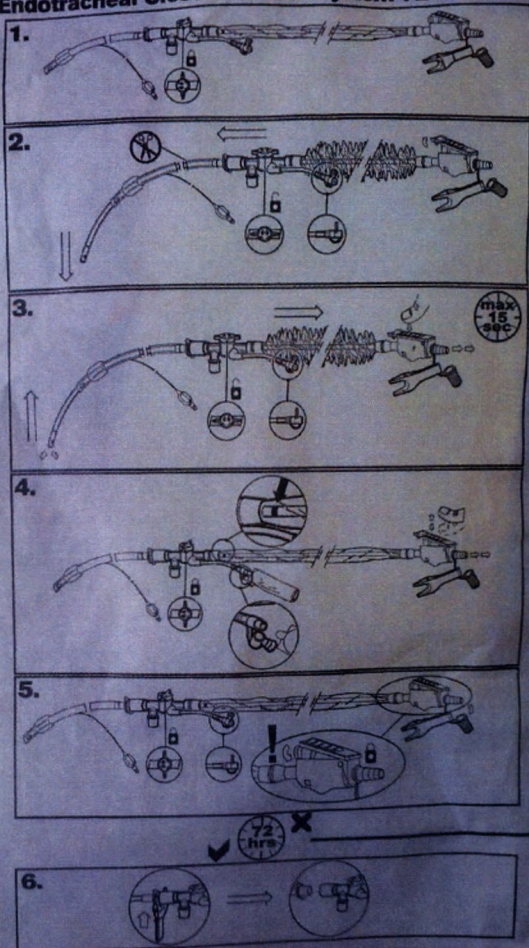
5 030267 097873 >

3720002-3-A



CE
0120

STERILE EO Rx ONLY

[illegible][illegible]

INTERSURGICAL
SUNGLASS REPAIR/REPLACEMENT SYSTEMS

Intersurgical Ltd.
Crane House, Mody Millers Lane,
Wokingham, Berkshire, RG43 2RZ, UK
E +44 (0)118 9086 300 F +44 (0)118 9086 356
E info@intersurgical.co.uk www www.intersurgical.co.uk

France	Portugal
T. 01 48 76 72 30	T. 21 210 00 00
Italy	Spain
T. 02 55 55 55	T. 91 666 78 16

Lietens
T. 307 4451
info@lietens.org.za

Puison
T. 010 771 8405
info@puison.org.za

Christa Engelbrecht
T. 420 772 1774

Talman
T. 010 2390 1234
info@talman.org.za

South Africa
T. 011 444 7890
info@sa.org.za

Malaysia
T. 03 222 0191





5. Система закрытая аспирационная эндотрахеальная для взрослых TrachSeal, 24 часа, размер катетера 3,3 мм (10Fr);

TrachSeal™ Adult Endotracheal Closed Suction System 24 hours

3.3 mm (10F)
x 540 mm (21.3 in)

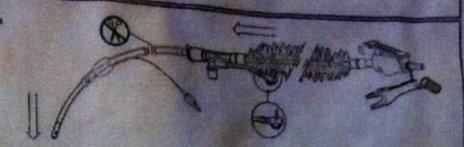
REF 3240003
LOT 341573
2017-05

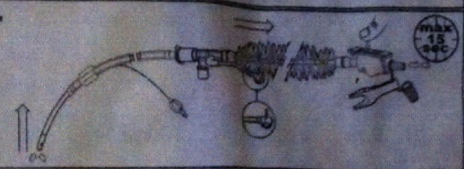
030267 116259

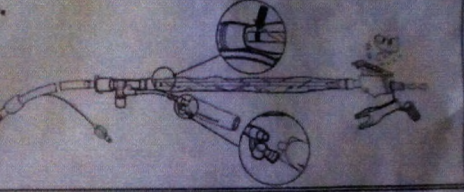
3240003-3-A

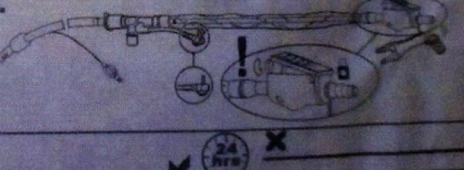
CE 0120
STERILE EO Rx ONLY


1. 

2. 

3. 

4. 

5. 

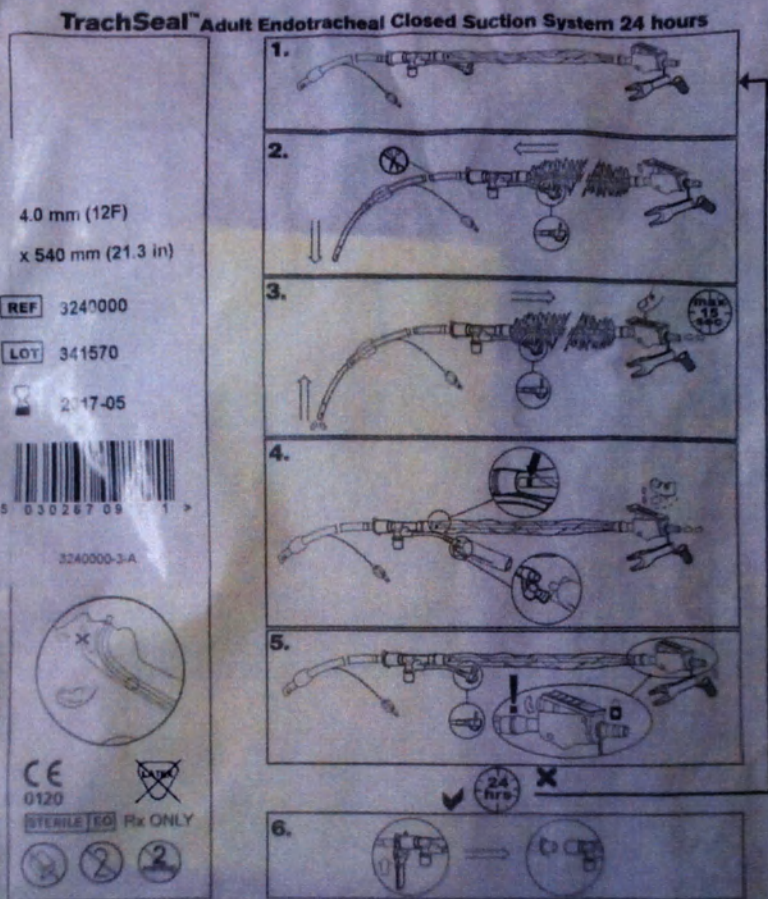
6. 

24 hrs

INTERMEDICAL



6. Система закрытая аспирационная эндотрахеальная для взрослых TrachSeal, 24 часа, размер катетера 4,0 мм (12Fr);



INDICATIONS: TrachSeal is indicated for the closed suction of secretions from the endotracheal tube of patients who are intubated and require suctioning. TrachSeal is not intended for use in patients who are not intubated or who are not on mechanical ventilation.

CONTRAINDICATIONS: TrachSeal is contraindicated for use in patients who are not intubated or who are not on mechanical ventilation. TrachSeal is also contraindicated for use in patients who have a known or suspected tracheal obstruction or who have a known or suspected tracheal injury.

WARNINGS: TrachSeal is a single-use device. Do not reuse TrachSeal. TrachSeal is not to be used in patients who are not intubated or who are not on mechanical ventilation. TrachSeal is not to be used in patients who have a known or suspected tracheal obstruction or who have a known or suspected tracheal injury.

PRECAUTIONS: TrachSeal is a single-use device. Do not reuse TrachSeal. TrachSeal is not to be used in patients who are not intubated or who are not on mechanical ventilation. TrachSeal is not to be used in patients who have a known or suspected tracheal obstruction or who have a known or suspected tracheal injury.

ADVERSE REACTIONS: TrachSeal is a single-use device. Do not reuse TrachSeal. TrachSeal is not to be used in patients who are not intubated or who are not on mechanical ventilation. TrachSeal is not to be used in patients who have a known or suspected tracheal obstruction or who have a known or suspected tracheal injury.

HOW TO USE: TrachSeal is a single-use device. Do not reuse TrachSeal. TrachSeal is not to be used in patients who are not intubated or who are not on mechanical ventilation. TrachSeal is not to be used in patients who have a known or suspected tracheal obstruction or who have a known or suspected tracheal injury.

INTERSURGICAL

INTERSURGICAL, Inc.
10000 W. 16th Ave., Suite 100
Denver, CO 80202, USA
Tel: 303.755.1000
Fax: 303.755.1001
Email: info@intersurgical.com
Website: www.intersurgical.com



Indications	Contraindications	Side effects	Precautions
1. Acute and chronic inflammation of the respiratory tract.	1. Hypersensitivity to the active substance.	1. Allergic reactions.	1. Use with caution in patients with renal and hepatic impairment.
2. Prevention of infection in patients with immunodeficiency.	2. Pregnancy and lactation.	2. Nausea, vomiting.	2. Avoid contact with eyes and mucous membranes.
3. Treatment of infection in patients with immunodeficiency.	3. History of allergic reactions to similar products.	3. Headache, dizziness.	3. Use with caution in patients with cardiovascular disease.
4. Prevention of infection in patients with immunodeficiency.	4. History of allergic reactions to similar products.	4. Rash, itching.	4. Use with caution in patients with diabetes.
5. Treatment of infection in patients with immunodeficiency.	5. History of allergic reactions to similar products.	5. Stomach pain, diarrhea.	5. Use with caution in patients with epilepsy.
6. Prevention of infection in patients with immunodeficiency.	6. History of allergic reactions to similar products.	6. Fatigue, weakness.	6. Use with caution in patients with hypertension.
7. Treatment of infection in patients with immunodeficiency.	7. History of allergic reactions to similar products.	7. Increased body temperature.	7. Use with caution in patients with low blood pressure.
8. Prevention of infection in patients with immunodeficiency.	8. History of allergic reactions to similar products.	8. Decreased appetite.	8. Use with caution in patients with heart failure.
9. Treatment of infection in patients with immunodeficiency.	9. History of allergic reactions to similar products.	9. Increased body temperature.	9. Use with caution in patients with kidney disease.
10. Prevention of infection in patients with immunodeficiency.	10. History of allergic reactions to similar products.	10. Decreased appetite.	10. Use with caution in patients with liver disease.

7. Система закрытая аспирационная эндотрахеальная для взрослых TrachSeal. 24 часа, размер катетера 4,7 мм (14Fr);

TrachSeal™ Adult Endotracheal Closed Suction System 24 hours

4.7 mm (14F)
x 540 mm (21.3 in)

REF 3240001


LOT 341571


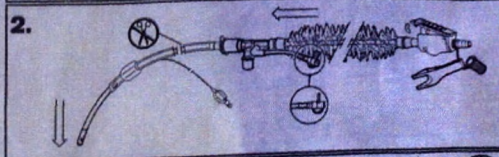
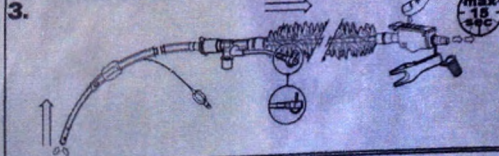
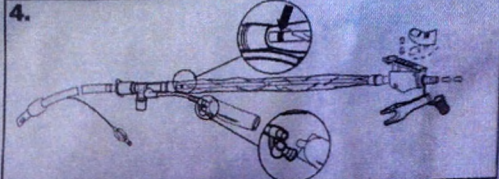
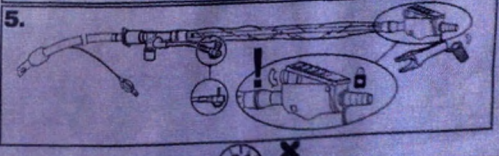

2017-05



5 030267 097807 >

3240001-3-A

Adult Endotracheal Closed Suction System. This system is used for 24 hours.

CAUTION: Use only as intended. Do not use for anything other than the intended purpose. Do not use for anything other than the intended purpose. Do not use for anything other than the intended purpose.

System Description: The system consists of a catheter, a connector, and a suction unit. The catheter is inserted into the trachea through the endotracheal tube. The connector is attached to the catheter and the suction unit. The suction unit is connected to the suction source.

Indications: The system is used for the removal of secretions from the trachea of patients who are intubated. It is used for the removal of secretions from the trachea of patients who are intubated.

Contraindications: The system is not used for the removal of secretions from the trachea of patients who are not intubated. It is not used for the removal of secretions from the trachea of patients who are not intubated.

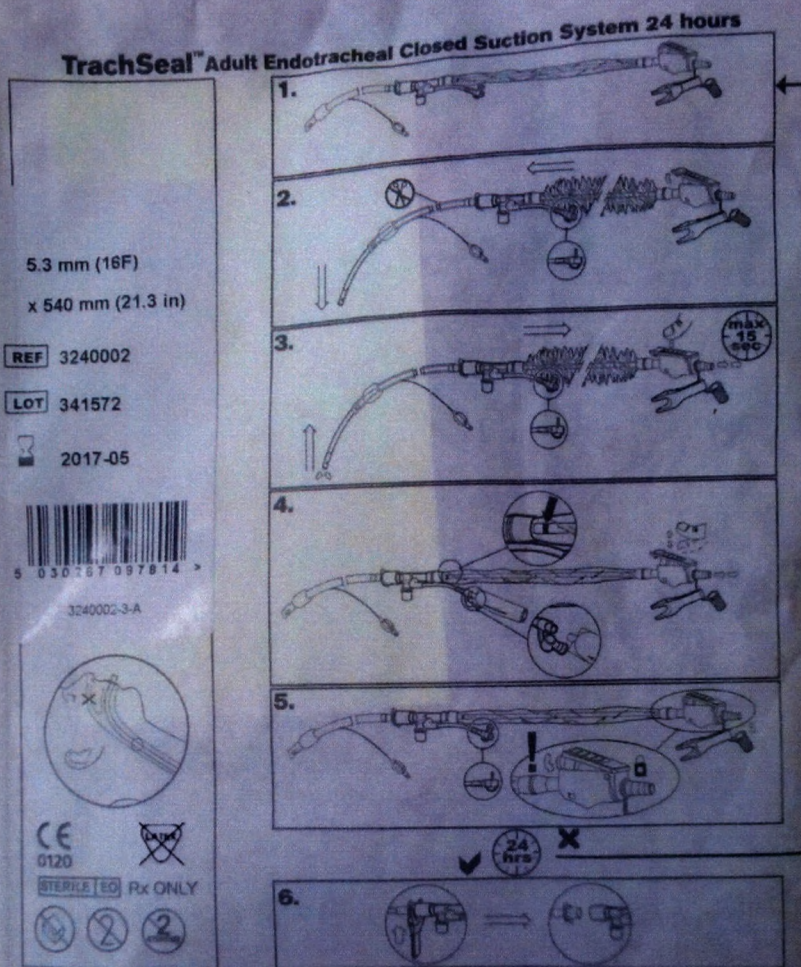
Warnings: Do not use the system for anything other than the intended purpose. Do not use the system for anything other than the intended purpose. Do not use the system for anything other than the intended purpose.

Instructions for Use: 1. Unpack the system. 2. Prepare the catheter. 3. Insert the catheter into the trachea. 4. Secure the catheter. 5. Connect to the suction unit. 6. Final setup and operation.

Intersurgical Ltd.
Crane House, Sandy, Bedfordshire, MK43 0JQ, UK
T: +44 (0)1525 530000 F: +44 (0)1525 530001
info@intersurgical.com www.intersurgical.com



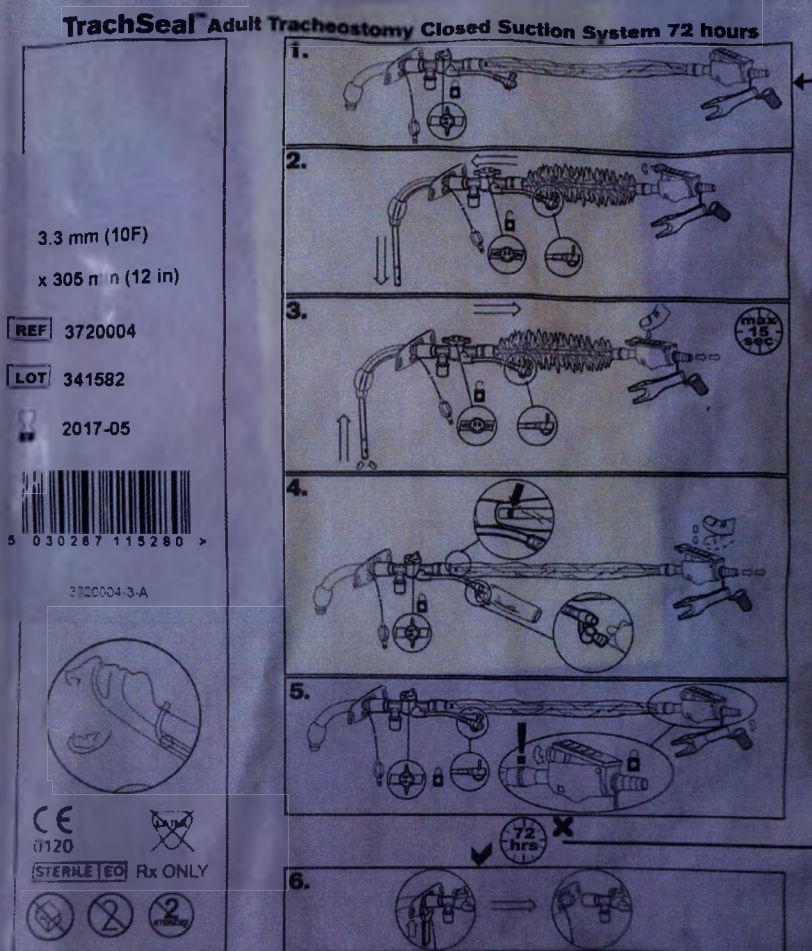
8. Система закрытая аспирационная эндотрахеальная для взрослых TrachSeal, 24 часа, размер катетера 5,3 мм (16Fr);

[illegible]

Ⓢ INTERSURGICAL

International Ltd.
 Crown House, Shady Grove Lane,
 Washington, D.C. 20787, U.S.A.
 Tel: (202) 776-1100. Fax: (202) 776-1101
 Email: info@washington.edu



[illegible]

 INTERSURGICAL A Division of Becton Dickinson	Distribution Tel: 02021 810000 address@intersurgical.co.uk	France Tel: 01 695 75 16 info@intersurgical.fr	Germany Tel: 089 8814 info@intersurgical.de	Spain Tel: 91 550 0000 info@intersurgical.es	USA Tel: 800 445 2222 info@intersurgical.com	Website for Intersurgical in Spain www.intersurgical.es
	Intersurgical Ltd. Crane House, Millers Lane, Westborough, Leicestershire, LE15 2RQ, UK E: info@intersurgical.com F: +44 (0)1533 606 200 www.intersurgical.com	Italy Tel: 02 46 46 72 90 info@intersurgical.it	Portugal Tel: 21 41 41 41 30 info@intersurgical.pt	Sweden Tel: 08 77 77 0000 info@intersurgical.se	Switzerland Tel: 052 72 72 72 72 info@intersurgical.ch	UK Tel: 01533 606 200 info@intersurgical.com



10. Система закрытая аспирационная трахеостомическая для взрослых TrachSeal, 72 часа, размер катетера 4,0 мм (12Fr);

TrachSeal™ Adult Tracheostomy Closed Suction System 72 hours

4.0 mm (12Fr)
x 305 mm (12 in)

REF 3720005
LOT 34 1583
20 17-05





3720005-2-A


0120

STERILE EO Rx ONLY





1. Assemble the system as shown in the diagram. The maximum period of use is 72 hours.

2. Insert the catheter into the tracheostomy tube. The catheter should be inserted to a depth of 10 cm.

3. Connect the suction tubing to the catheter. The suction tubing should be connected to the catheter at a depth of 10 cm.

4. Check the system for leaks. The system should be checked for leaks at the connection points.

5. Suction the patient's secretions. The suction should be performed at a depth of 10 cm.

6. Remove the system. The system should be removed at the end of the 72-hour period.

Adult Tracheostomy Closed Suction System. The maximum period of use is 72 hours.

CAUTION: Use patient monitoring throughout procedure and follow published suction guidelines.

System description: Tracheostomy Form, Adult. The catheter is inserted into the tracheostomy tube. The catheter is inserted to a depth of 10 cm. The catheter is connected to the suction tubing. The suction tubing is connected to the catheter at a depth of 10 cm.

Indications: The system is used for the suctioning of secretions from the tracheostomy tube. The system is used for the suctioning of secretions from the tracheostomy tube.

Contraindications: The system is not to be used for the suctioning of secretions from the tracheostomy tube. The system is not to be used for the suctioning of secretions from the tracheostomy tube.

Warnings: The system is not to be used for the suctioning of secretions from the tracheostomy tube. The system is not to be used for the suctioning of secretions from the tracheostomy tube.

Precautions: The system is not to be used for the suctioning of secretions from the tracheostomy tube. The system is not to be used for the suctioning of secretions from the tracheostomy tube.

Instructions for use: The system is used for the suctioning of secretions from the tracheostomy tube. The system is used for the suctioning of secretions from the tracheostomy tube.

Storage: The system is stored in a sterile container. The system is stored in a sterile container.

Disposal: The system is disposed of in a biohazard container. The system is disposed of in a biohazard container.



11. Система закрытая аспирационная трахеостомическая для взрослых TrachSeal. 72 часа, размер катетера 4,7 мм (14Fr);

TrachSeal™ Adult Tracheostomy Closed Suction System 72 hours

4.7 mm (14F)
x 305 mm (12 in)

REF 3720006

LOT 341584

2017-05

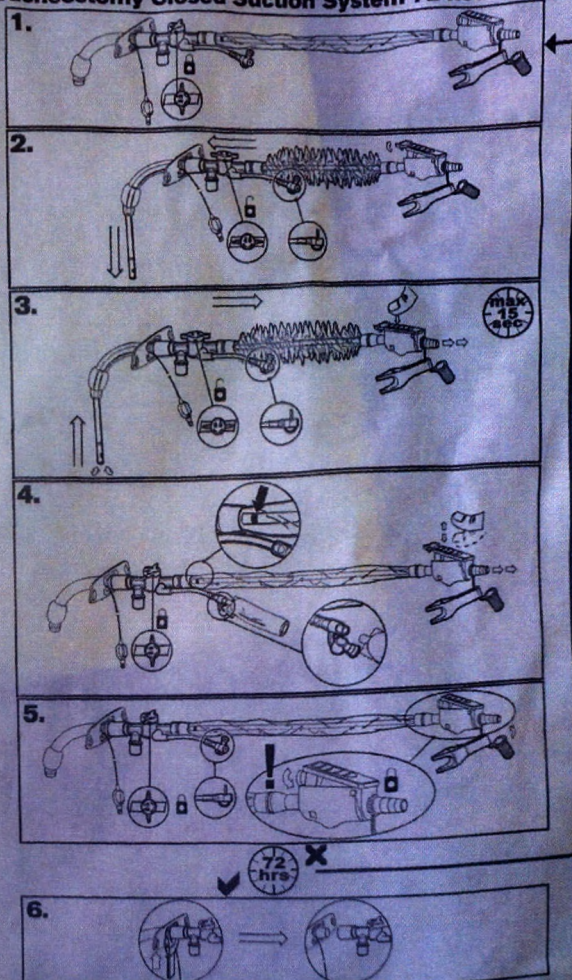



3720006-3-A



CE 0120

STERILE EO Rx ONLY



Adult Tracheostomy Closed Suction System. The maximum period of use is 72 hours.
CAUTION: Use patient monitoring throughout procedure and follow published suction guidelines, recommended vacuum: ≤ 150 mm Hg.

Systeme d'aspiration Trachéostomique Fermée. Durée: La période d'utilisation maximale est 72 heures. **ATTENTION:** Effectuer une surveillance des patients tout au long de la procédure et suivre les directives d'aspiration recommandées, sous vide: ≤ 150 mm Hg.

Systeme de aspiración cerrada de traqueostomía. El periodo máximo de uso es 72 horas. **PRECAUCIÓN:** Vigilancia al paciente durante todo el procedimiento y seguir las directrices de aspiración recomendadas, en succión máxima: ≤ 150 mm Hg.

Systeme de aspirazione tracheostomica chiusa per 72 ore. **ATTENZIONE:** Assicurare il monitoraggio del paziente durante tutta la procedura, e osservare la linea della sifonatura nel corso stesso, così come consigliata, sotto ≤ 150 mm Hg.

Tracheostomie gesloten afzuigstelsel voor maximaal 72 uur. **LET OP:** Gebruik het patiënt continu toezicht gedurende de gehele procedure en volg de gepubliceerde afzuigrichtlijnen, afzuigspanning maximaal ≤ 150 mm Hg.

Lakaitis succion sistem, Traqueostomía, Máximo: Máximo periodo de uso 72 horas. **PRECAUCIÓN:** Seguimiento constante del paciente durante toda la intervención, y observar la línea de succión durante el procedimiento, así como se recomienda, bajo ≤ 150 mm Hg.

Aspirator, tracheostomica sistem, Aspirations, Maximum: Maximum period of use 72 hours. **CAUTION:** Patient monitoring throughout procedure and follow published suction guidelines, recommended vacuum: ≤ 150 mm Hg.

Adult Tracheostomy Closed Suction System. The maximum period of use is 72 hours. **ATTENTION:** Use patient monitoring throughout procedure and follow published suction guidelines, recommended vacuum: ≤ 150 mm Hg.

Systeme d'aspiration Trachéostomique Fermée. Durée: La période d'utilisation maximale est 72 heures. **ATTENTION:** Effectuer une surveillance des patients tout au long de la procédure et suivre les directives d'aspiration recommandées, sous vide: ≤ 150 mm Hg.

Systeme de aspiración cerrada de traqueostomía. El periodo máximo de uso es 72 horas. **PRECAUCIÓN:** Vigilancia al paciente durante todo el procedimiento y seguir las directrices de aspiración recomendadas, en succión máxima: ≤ 150 mm Hg.

Systeme de aspirazione tracheostomica chiusa per 72 ore. **ATTENZIONE:** Assicurare il monitoraggio del paziente durante tutta la procedura, e osservare la linea della sifonatura nel corso stesso, così come consigliata, sotto ≤ 150 mm Hg.

Tracheostomie gesloten afzuigstelsel voor maximaal 72 uur. **LET OP:** Gebruik het patiënt continu toezicht gedurende de gehele procedure en volg de gepubliceerde afzuigrichtlijnen, afzuigspanning maximaal ≤ 150 mm Hg.

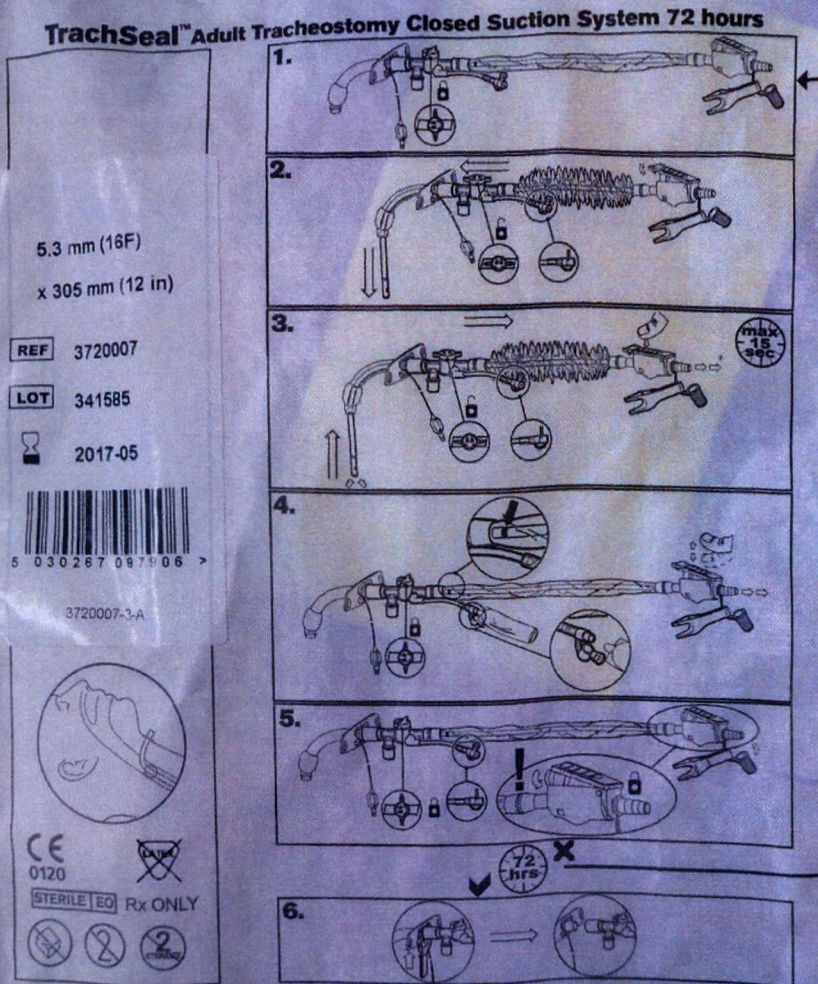
Lakaitis succion sistem, Traqueostomía, Máximo: Máximo periodo de uso 72 horas. **PRECAUCIÓN:** Seguimiento constante del paciente durante toda la intervención, y observar la línea de succión durante el procedimiento, así como se recomienda, bajo ≤ 150 mm Hg.

Aspirator, tracheostomica sistem, Aspirations, Maximum: Maximum period of use 72 hours. **CAUTION:** Patient monitoring throughout procedure and follow published suction guidelines, recommended vacuum: ≤ 150 mm Hg.

INTERSURGICAL
Distributed in the USA by Intersurgical Inc.
Distributed in the UK by Intersurgical Ltd.
Distributed in the EU by Intersurgical GmbH.
Distributed in the RU by Intersurgical OOO.



12. Система закрытая аспирационная трахеостомическая для взрослых TrachSeal. 72 часа, размер катетера 5,3 мм (16Fr);



Adult Tracheostomy Closed Suction System. The maximum period of use is 72 hours. **CAUTION:** Use before expiration. **WARNING:** Do not use if the package is damaged or if the system is not assembled correctly. **REF 3720007**. **LOT 341585**. **2017-05**. **5 030267 097906**. **3720007-3-A**.

1. Insert the catheter into the tracheostomy tube. **2.** Connect the catheter to the suction device. **3.** Adjust the suction level. **4.** Monitor the system. **5.** Disconnect the system. **6.** Reconnect the system.

CAUTION: Do not use if the package is damaged or if the system is not assembled correctly. **WARNING:** Do not use if the package is damaged or if the system is not assembled correctly. **REF 3720007**. **LOT 341585**. **2017-05**. **5 030267 097906**. **3720007-3-A**.

1. Insert the catheter into the tracheostomy tube. **2.** Connect the catheter to the suction device. **3.** Adjust the suction level. **4.** Monitor the system. **5.** Disconnect the system. **6.** Reconnect the system.

CAUTION: Do not use if the package is damaged or if the system is not assembled correctly. **WARNING:** Do not use if the package is damaged or if the system is not assembled correctly. **REF 3720007**. **LOT 341585**. **2017-05**. **5 030267 097906**. **3720007-3-A**.

1. Insert the catheter into the tracheostomy tube. **2.** Connect the catheter to the suction device. **3.** Adjust the suction level. **4.** Monitor the system. **5.** Disconnect the system. **6.** Reconnect the system.

CAUTION: Do not use if the package is damaged or if the system is not assembled correctly. **WARNING:** Do not use if the package is damaged or if the system is not assembled correctly. **REF 3720007**. **LOT 341585**. **2017-05**. **5 030267 097906**. **3720007-3-A**.

INTERSURGICAL Ltd. **Crane House, Moll's Mill Lane, Wokingham, Berkshire RG41 2BZ, UK**. **T: +44 (0)118 9530 300 F: +44 (0)118 9530 306**. **info@intersurgical.com**. **www.intersurgical.com**.

1. Insert the catheter into the tracheostomy tube. **2.** Connect the catheter to the suction device. **3.** Adjust the suction level. **4.** Monitor the system. **5.** Disconnect the system. **6.** Reconnect the system.

CAUTION: Do not use if the package is damaged or if the system is not assembled correctly. **WARNING:** Do not use if the package is damaged or if the system is not assembled correctly. **REF 3720007**. **LOT 341585**. **2017-05**. **5 030267 097906**. **3720007-3-A**.

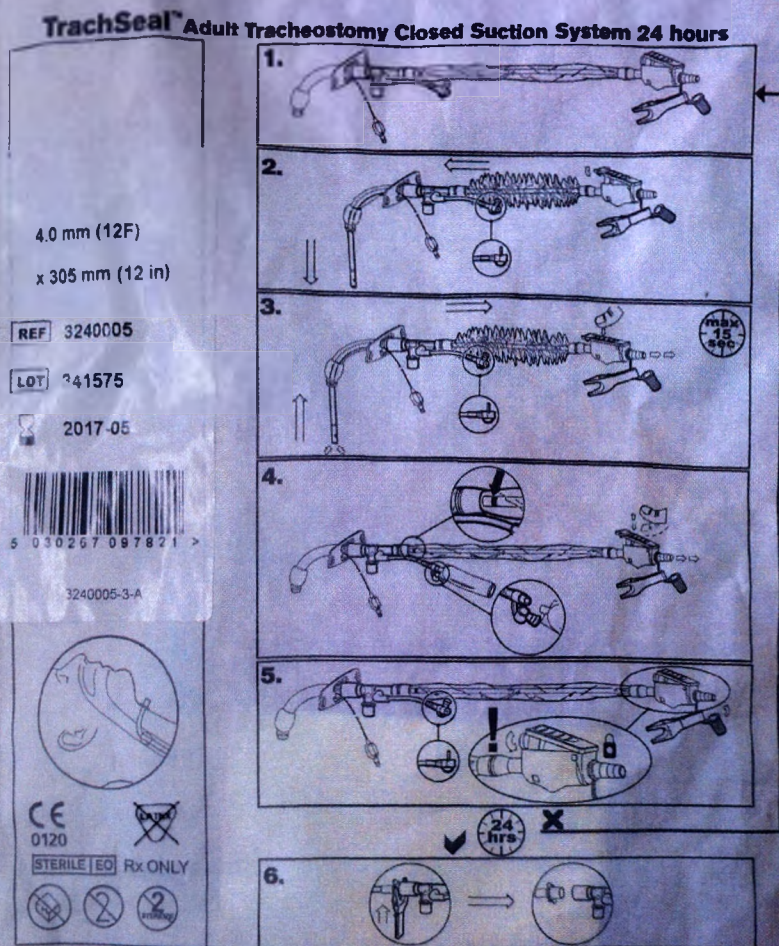
1. Insert the catheter into the tracheostomy tube. **2.** Connect the catheter to the suction device. **3.** Adjust the suction level. **4.** Monitor the system. **5.** Disconnect the system. **6.** Reconnect the system.

CAUTION: Do not use if the package is damaged or if the system is not assembled correctly. **WARNING:** Do not use if the package is damaged or if the system is not assembled correctly. **REF 3720007**. **LOT 341585**. **2017-05**. **5 030267 097906**. **3720007-3-A**.





14. Система закрытая аспирационная трахеостомическая для взрослых TrachSeal, 24 часа, размер катетера 4,0 мм (12Fr);



4.0 mm (12F)
x 305 mm (12 in)

REF 3240005

LOT 341575

2017-05



5 030267 097821 >

3240005-3-A



CE
0120

STEP

Amos 1

CAUTION
REACTIVE

QUESTIONS

105

CLINICAL
EVIDENCE

ATTENTION

LIST OF
WRITERS

1000

12

Published by
Quintessence Publishing

1989

Trachemys
superciliosa
pennsylvanica

IN

interu
Crane b

Wokingham
44 (0)118 9
www...

1998, 1999, 2000, 2001, 2002, 2003, 2004, 2005, 2006, 2007, 2008, 2009, 2010, 2011, 2012, 2013, 2014, 2015, 2016, 2017, 2018, 2019, 2020, 2021, 2022, 2023, 2024, 2025, 2026, 2027, 2028, 2029, 2030, 2031, 2032, 2033, 2034, 2035, 2036, 2037, 2038, 2039, 2040, 2041, 2042, 2043, 2044, 2045, 2046, 2047, 2048, 2049, 2050, 2051, 2052, 2053, 2054, 2055, 2056, 2057, 2058, 2059, 2060, 2061, 2062, 2063, 2064, 2065, 2066, 2067, 2068, 2069, 2070, 2071, 2072, 2073, 2074, 2075, 2076, 2077, 2078, 2079, 2080, 2081, 2082, 2083, 2084, 2085, 2086, 2087, 2088, 2089, 2090, 2091, 2092, 2093, 2094, 2095, 2096, 2097, 2098, 2099, 2100, 2101, 2102, 2103, 2104, 2105, 2106, 2107, 2108, 2109, 2110, 2111, 2112, 2113, 2114, 2115, 2116, 2117, 2118, 2119, 2120, 2121, 2122, 2123, 2124, 2125, 2126, 2127, 2128, 2129, 2130, 2131, 2132, 2133, 2134, 2135, 2136, 2137, 2138, 2139, 2140, 2141, 2142, 2143, 2144, 2145, 2146, 2147, 2148, 2149, 2150, 2151, 2152, 2153, 2154, 2155, 2156, 2157, 2158, 2159, 2160, 2161, 2162, 2163, 2164, 2165, 2166, 2167, 2168, 2169, 2170, 2171, 2172, 2173, 2174, 2175, 2176, 2177, 2178, 2179, 2180, 2181, 2182, 2183, 2184, 2185, 2186, 2187, 2188, 2189, 2190, 2191, 2192, 2193, 2194, 2195, 2196, 2197, 2198, 2199, 2200, 2201, 2202, 2203, 2204, 2205, 2206, 2207, 2208, 2209, 2210, 2211, 2212, 2213, 2214, 2215, 2216, 2217, 2218, 2219, 2220, 2221, 2222, 2223, 2224, 2225, 2226, 2227, 2228, 2229, 2230, 2231, 2232, 2233, 2234, 2235, 2236, 2237, 2238, 2239, 2240, 2241, 2242, 2243, 2244, 2245, 2246, 2247, 2248, 2249, 2250, 2251, 2252, 2253, 2254, 2255, 2256, 2257, 2258, 2259, 2260, 2261, 2262, 2263, 2264, 2265, 2266, 2267, 2268, 2269, 2270, 2271, 2272, 2273, 2274, 2275, 2276, 2277, 2278, 2279, 2280, 2281, 2282, 2283, 2284, 2285, 2286, 2287, 2288, 2289, 2290, 2291, 2292, 2293, 2294, 2295, 2296, 2297, 2298, 2299, 2300, 2301, 2302, 2303, 2304, 2305, 2306, 2307, 2308, 2309, 2310, 2311, 2312, 2313, 2314, 2315, 2316, 2317, 2318, 2319, 2320, 2321, 2322, 2323, 2324, 2325, 2326, 2327, 2328, 2329, 2330, 2331, 2332, 2333, 2334, 2335, 2336, 2337, 2338, 2339, 2340, 2341, 2342, 2343, 2344, 2345, 2346, 2347, 2348, 2349, 2350, 2351, 2352, 2353, 2354, 2355, 2356, 2357, 2358, 2359, 2360, 2361, 2362, 2363, 2364, 2365, 2366, 2367, 2368, 2369, 2370, 2371, 2372, 2373, 2374, 2375, 2376, 2377, 2378, 2379, 2380, 2381, 2382, 2383, 2384, 2385, 2386, 2387, 2388, 2389, 2390, 2391, 2392, 2393, 2394, 2395, 2396, 2397, 2398, 2399, 2400, 2401, 2402, 2403, 2404, 2405, 2406, 2407, 2408, 2409, 2410, 2411, 2412, 2413, 2414, 2415, 2416, 2417, 2418, 2419, 2420, 2421, 2422, 2423, 2424, 2425, 2426, 2427, 2428, 2429, 2430, 2431, 2432, 2433, 2434, 2435, 2436, 2437, 2438, 2439, 2440, 2441, 2442, 2443, 2444, 2445, 2446, 2447, 2448, 2449, 2450, 2451, 2452, 2453, 2454, 2455, 2456, 2457, 2458, 2459, 2460, 2461, 2462, 2463, 2464, 2465, 2466, 2467, 2468, 2469, 2470, 2471, 2472, 2473, 2474, 2475, 2476, 2477, 2478, 2479, 2480, 2481, 2482, 2483, 2484, 2485, 2486, 2487, 2488, 2489, 2490, 2491, 2492, 2493, 2494, 2495, 2496, 2497, 2498, 2499, 2500, 2501, 2502, 2503, 2504, 2505, 2506, 2507, 2508, 2509, 2510, 2511, 2512, 2513, 2514, 2515, 2516, 2517, 2518, 2519, 2520, 2521, 2522, 2523, 2524, 2525, 2526, 2527, 2528, 2529, 2530, 2531, 2532, 2533, 2534, 2535, 2536, 2537, 2538, 2539, 2540, 2541, 2542, 2543, 2544, 2545, 2546, 2547, 2548, 2549, 2550, 2551, 2552, 2553, 2554, 2555, 2556, 2557, 2558, 2559, 2560, 2561, 2562, 2563, 2564, 2565, 2566, 2567, 2568, 2569, 2570, 2571, 2572, 2573, 2574, 2575, 2576, 2577, 2578, 2579, 2580, 2581, 2582, 2583, 2584, 2585, 2586, 2587, 2588, 2589, 2590, 2591, 2592, 2593, 2594, 2595, 2596, 2597, 2598, 2599, 2600, 2601, 2602, 2603, 2604, 2605, 2606, 2607, 2608, 2609, 2610, 2611, 2612, 2613, 2614, 2615, 2616, 2617, 2618, 2619, 2620, 2621, 2622, 2623, 2624, 2625, 2626, 2627, 2628, 2629, 2630, 2631, 2632, 2633, 2634, 2635, 2636, 2637, 2638, 2639, 2640, 2641, 2642, 2643, 2644, 2645, 2646, 2647, 2648, 2649, 2650, 2651, 2652, 2653, 2654, 2655, 2656, 2657, 2658, 2659, 2660, 2661, 2662, 2663, 2664, 2665, 2666, 2667, 2668, 2669, 2670, 2671, 2672, 2673, 2674, 2675, 2676, 2677, 2678, 2679, 26

1

WWW

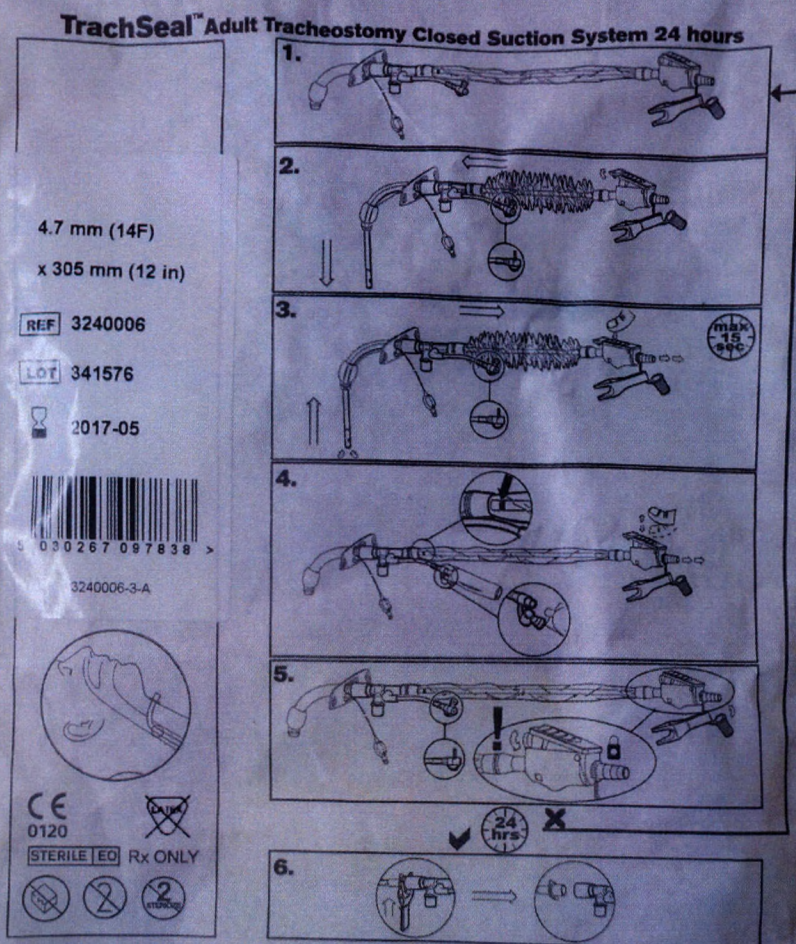
24. **Handwritten:** *Handwritten: 24. 11. 1974*
 25. **Handwritten:** *Handwritten: 25. 11. 1974*
 26. **Handwritten:** *Handwritten: 26. 11. 1974*
 27. **Handwritten:** *Handwritten: 27. 11. 1974*
 28. **Handwritten:** *Handwritten: 28. 11. 1974*
 29. **Handwritten:** *Handwritten: 29. 11. 1974*
 30. **Handwritten:** *Handwritten: 30. 11. 1974*
 31. **Handwritten:** *Handwritten: 31. 11. 1974*
 32. **Handwritten:** *Handwritten: 32. 11. 1974*
 33. **Handwritten:** *Handwritten: 33. 11. 1974*
 34. **Handwritten:** *Handwritten: 34. 11. 1974*
 35. **Handwritten:** *Handwritten: 35. 11. 1974*
 36. **Handwritten:** *Handwritten: 36. 11. 1974*
 37. **Handwritten:** *Handwritten: 37. 11. 1974*
 38. **Handwritten:** *Handwritten: 38. 11. 1974*
 39. **Handwritten:** *Handwritten: 39. 11. 1974*
 40. **Handwritten:** *Handwritten: 40. 11. 1974*
 41. **Handwritten:** *Handwritten: 41. 11. 1974*
 42. **Handwritten:** *Handwritten: 42. 11. 1974*
 43. **Handwritten:** *Handwritten: 43. 11. 1974*
 44. **Handwritten:** *Handwritten: 44. 11. 1974*
 45. **Handwritten:** *Handwritten: 45. 11. 1974*
 46. **Handwritten:** *Handwritten: 46. 11. 1974*
 47. **Handwritten:** *Handwritten: 47. 11. 1974*
 48. **Handwritten:** *Handwritten: 48. 11. 1974*
 49. **Handwritten:** *Handwritten: 49. 11. 1974*
 50. **Handwritten:** *Handwritten: 50. 11. 1974*
 51. **Handwritten:** *Handwritten: 51. 11. 1974*
 52. **Handwritten:** *Handwritten: 52. 11. 1974*
 53. **Handwritten:** *Handwritten: 53. 11. 1974*
 54. **Handwritten:** *Handwritten: 54. 11. 1974*
 55. **Handwritten:** *Handwritten: 55. 11. 1974*
 56. **Handwritten:** *Handwritten: 56. 11. 1974*
 57. **Handwritten:** *Handwritten: 57. 11. 1974*
 58. **Handwritten:** *Handwritten: 58. 11. 1974*
 59. **Handwritten:** *Handwritten: 59. 11. 1974*
 60. **Handwritten:** *Handwritten: 60. 11. 1974*
 61. **Handwritten:** *Handwritten: 61. 11. 1974*
 62. **Handwritten:** *Handwritten: 62. 11. 1974*
 63. **Handwritten:** *Handwritten: 63. 11. 1974*
 64. **Handwritten:** *Handwritten: 64. 11. 1974*
 65. **Handwritten:** *Handwritten: 65. 11. 1974*
 66. **Handwritten:** *Handwritten: 66. 11. 1974*
 67. **Handwritten:** *Handwritten: 67. 11. 1974*
 68. **Handwritten:** *Handwritten: 68. 11. 1974*
 69. **Handwritten:** *Handwritten: 69. 11. 1974*
 70. **Handwritten:** *Handwritten: 70. 11. 1974*
 71. **Handwritten:** *Handwritten: 71. 11. 1974*
 72. **Handwritten:** *Handwritten: 72. 11. 1974*
 73. **Handwritten:** *Handwritten: 73. 11. 1974*
 74. **Handwritten:** *Handwritten: 74. 11. 1974*
 75. **Handwritten:** *Handwritten: 75. 11. 1974*
 76. **Handwritten:** *Handwritten: 76. 11. 1974*
 77. **Handwritten:** *Handwritten: 77. 11. 1974*
 78. **Handwritten:** *Handwritten: 78. 11. 1974*
 79. **Handwritten:** *Handwritten: 79. 11. 1974*
 80. **Handwritten:** *Handwritten: 80. 11. 1974*
 81. **Handwritten:** *Handwritten: 81. 11. 1974*
 82. **Handwritten:** *Handwritten: 82. 11. 1974*
 83. **Handwritten:** *Handwritten: 83. 11. 1974*
 84. **Handwritten:** *Handwritten: 84. 11. 1974*
 85. **Handwritten:** *Handwritten: 85. 11. 1974*
 86. **Handwritten:** *Handwritten: 86. 11. 1974*
 87. **Handwritten:** *Handwritten: 87. 11. 1974*
 88. **Handwritten:** *Handwritten: 88. 11. 1974*
 89. **Handwritten:** *Handwritten: 89. 11. 1974*
 90. **Handwritten:** *Handwritten: 90. 11. 1974*
 91. **Handwritten:** *Handwritten: 91. 11. 1974*
 92. **Handwritten:** *Handwritten: 92. 11. 1974*
 93. **Handwritten:** *Handwritten: 93. 11. 1974*
 94. **Handwritten:** *Handwritten: 94. 11. 1974*
 95. **Handwritten:** *Handwritten: 95. 11. 1974*
 96. **Handwritten:** *Handwritten: 96. 11. 1974*
 97. **Handwritten:** *Handwritten: 97. 11. 1974*
 98. **Handwritten:** *Handwritten: 98. 11. 1974*
 99. **Handwritten:** *Handwritten: 99. 11. 1974*
 100. **Handwritten:** *Handwritten: 100. 11. 1974*

32-33-34-35-36-37-38-39-40-41-42-43-44-45-46-47-48-49-50-51-52-53-54-55-56-57-58-59-60-61-62-63-64-65-66-67-68-69-70-71-72-73-74-75-76-77-78-79-80-81-82-83-84-85-86-87-88-89-90-91-92-93-94-95-96-97-98-99-100-101-102-103-104-105-106-107-108-109-110-111-112-113-114-115-116-117-118-119-120-121-122-123-124-125-126-127-128-129-130-131-132-133-134-135-136-137-138-139-140-141-142-143-144-145-146-147-148-149-150-151-152-153-154-155-156-157-158-159-160-161-162-163-164-165-166-167-168-169-170-171-172-173-174-175-176-177-178-179-180-181-182-183-184-185-186-187-188-189-190-191-192-193-194-195-196-197-198-199-200-201-202-203-204-205-206-207-208-209-210-211-212-213-214-215-216-217-218-219-220-221-222-223-224-225-226-227-228-229-230-231-232-233-234-235-236-237-238-239-240-241-242-243-244-245-246-247-248-249-250-251-252-253-254-255-256-257-258-259-260-261-262-263-264-265-266-267-268-269-270-271-272-273-274-275-276-277-278-279-280-281-282-283-284-285-286-287-288-289-290-291-292-293-294-295-296-297-298-299-300-301-302-303-304-305-306-307-308-309-310-311-312-313-314-315-316-317-318-319-320-321-322-323-324-325-326-327-328-329-330-331-332-333-334-335-336-337-338-339-340-341-342-343-344-345-346-347-348-349-350-351-352-353-354-355-356-357-358-359-360-361-362-363-364-365-366-367-368-369-370-371-372-373-374-375-376-377-378-379-380-381-382-383-384-385-386-387-388-389-390-391-392-393-394-395-396-397-398-399-400-401-402-403-404-405-406-407-408-409-410-411-412-413-414-415-416-417-418-419-420-421-422-423-424-425-426-427-428-429-430-431-432-433-434-435-436-437-438-439-440-441-442-443-444-445-446-447-448-449-450-451-452-453-454-455-456-457-458-459-460-461-462-463-464-465-466-467-468-469-470-471-472-473-474-475-476-477-478-479-480-481-482-483-484-485-486-487-488-489-490-491-492-493-494-495-496-497-498-499-500-501-502-503-504-505-506-507-508-509-510-511-512-513-514-515-516-517-518-519-520-521-522-523-524-525-526-527-528-529-530-531-532-533-534-535-536-537-538-539-540-541-542-543-544-545-546-547-548-549-550-551-552-553-554-555-556-557-558-559-560-561-562-563-564-565-566-567-568-569-570-571-572-573-574-575-576-577-578-579-580-581-582-583-584-585-586-587-588-589-590-591-592-593-594-595-596-597-598-599-600-601-602-603-604-605-606-607-608-609-610-611-612-613-614-615-616-617-618-619-620-621-622-623-624-625-626-627-628-629-630-631-632-633-634-635-636-637-638-639-640-641-642-643-644-645-646-647-648-649-650-651-652-653-654-655-656-657-658-659-660-661-662-663-664-665-666-667-668-669-670-671-672-673-674-675-676-677-678-679-680-681-682-683-684-685-686-687-688-689-690-691-692-693-694-695-696-697-698-699-700-701-702-703-704-705-706-707-708-709-710-711-712-713-714-715-716-717-718-719-720-721-722-723-724-725-726-727-728-729-730-731-732-733-734-735-736-737-738-739-740-741-742-743-744-745-746-747-748-749-750-751-752-753-754-755-756-757-758-759-760-761-762-763-764-765-766-767-768-769-770-771-772-773-774-775-776-777-778-779-780-781-782-783-784-785-786-787-788-789-790-791-792-793-794-795-796-797-798-799-800-801-802-803-804-805-806-807-808-809-810-811-812-813-814-815-816-817-818-819-820-821-822-823-824-825-826-827-828-829-830-831-832-833-834-835-836-837-838-839-840-841-842-843-844-845-846-847-848-849-850-851-852-853-854-855-856-857-858-859-860-861-862-863-864-865-866-867-868-869-870-871-872-873-874-875-876-877-878-879-880-881-882-883-884-885-886-887-888-889-890-891-892-893-894-895-896-897-898-899-900-901-902-903-904-905-906-907-908-909-910-911-912-913-914-915-916-917-918-919-920-921-922-923-924-925-926-927-928-929-930-931-932-933-934-935-936-937-938-939-940-941-942-943-944-945-946-947-948-949-950-951-952-953-954-955-956-957-958-959-960-961-962-963-964-965-966-967-968-969-970-971-972-973-974-975-976-977-978-979-980-981-982-983-984-985-986-987-988-989-990-991-992-993-994-995-996-997-998-999-1000-1001-1002-1003-1004-1005-1006-1007-1008-1009-1010-1011-1012-1013-1014-1015-1016-1017-1018-1019-1020-1021-1022-1023-1024-1025-1026-1027-1028-1029-1030-1031-1032-1033-1034-1035-1036-1037-1038-1039-1040-1041-1042-1043-1044-1045-1046-1047-1048-1049-1050-1051-1052-1053-1054-1055-1056-1057-

 Intersurgical Ltd. Crane House, Mully Millers Lane, Hemel Hempstead, Herts, SG9 6UN, UK T: +44 (0)1462 865030 F: +44 (0)1462 865638 info@intersurgical.com www.intersurgical.com	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de	Representative T: 01 900 79 19 19 F: 01 900 79 19 19 E: info@intersurgical.fr	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de
	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de	Representative T: 00491 511000 F: 00491 511001 E: info@intersurgical.de



15. Система закрытая аспирационная трахеостомическая для взрослых TrachSeal, 24 часа, размер катетера 4,7 мм (14Fr);



Adult Tracheostomy Closed Suction System, the maximum period of use is 24 hours.
CAUTION: Use patient monitoring throughout procedure and follow published suction guidelines.
TENTATIVE: L'efficacité d'une aspiration des patients doit être surveillée tout au long de la procédure et suivre les directives d'aspiration recommandées sous vide ≤ 150 mm Hg.

1. Insert the catheter into the tracheostomy tube. 2. Connect the catheter to the suction device. 3. Adjust the suction pressure. 4. Monitor the patient's condition. 5. Disconnect the catheter from the suction device. 6. Remove the catheter from the tracheostomy tube.

1. Insérer le cathéter dans le tube de trachéostomie. 2. Brancher le cathéter sur l'appareil d'aspiration. 3. Régler la pression d'aspiration. 4. Surveiller l'état du patient. 5. Débrancher le cathéter de l'appareil d'aspiration. 6. Retirer le cathéter du tube de trachéostomie.

1. Insertar el catéter en el tubo de traqueostomía. 2. Conectar el catéter al dispositivo de succión. 3. Ajustar la presión de succión. 4. Monitorizar al paciente. 5. Desconectar el catéter del dispositivo de succión. 6. Retirar el catéter del tubo de traqueostomía.

1. Einfügen des Katheters in das Tracheostomierohr. 2. Anschließen des Katheters an das Sauggerät. 3. Einstellen des Saugdrucks. 4. Überwachen des Patienten. 5. Abtrennen des Katheters vom Sauggerät. 6. Entfernen des Katheters aus dem Tracheostomierohr.

1. Вставить катетер в трахеостомическую трубку. 2. Подключить катетер к устройству для отсасывания. 3. Настроить давление отсасывания. 4. Наблюдать за состоянием пациента. 5. Отсоединить катетер от устройства для отсасывания. 6. Удалить катетер из трахеостомической трубки.

INTERSURGICAL
InterSurgical Ltd.
Crane House, Muddy Millers Lane,
Warrington, Cheshire, W9 3RZ, UK
T: +44 (0)194 6650 200 F: +44 (0)194 6650 250
info@intersurgical.com www.intersurgical.com

Deutschland T: 0241 92 00 00
F: 0241 92 00 01
E: info@intersurgical.de
www.intersurgical.de

France T: 02 47 86 11 11
F: 02 47 86 11 12
E: info@intersurgical.fr
www.intersurgical.fr

Italy T: 02 87 11 11 11
F: 02 87 11 11 12
E: info@intersurgical.it
www.intersurgical.it

Spain T: 91 55 55 55
F: 91 55 55 56
E: info@intersurgical.es
www.intersurgical.es

Sweden T: 08 77 77 77
F: 08 77 77 78
E: info@intersurgical.se
www.intersurgical.se

Switzerland T: 058 11 11 11
F: 058 11 11 12
E: info@intersurgical.ch
www.intersurgical.ch





1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30	31	32	33	34	35	36	37	38	39	40	41	42	43	44	45	46	47	48	49	50	51	52	53	54	55	56	57	58	59	60	61	62	63	64	65	66	67	68	69	70	71	72	73	74	75	76	77	78	79	80	81	82	83	84	85	86	87	88	89	90	91	92	93	94	95	96	97	98	99	100
1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30	31	32	33	34	35	36	37	38	39	40	41	42	43	44	45	46	47	48	49	50	51	52	53	54	55	56	57	58	59	60	61	62	63	64	65	66	67	68	69	70	71	72	73	74	75	76	77	78	79	80	81	82	83	84	85	86	87	88	89	90	91	92	93	94	95	96	97	98	99	100

107818100 2-11-12

В документе пронумеровано,
прошнуровано и скреплено печатью

33 (тридцать три) листа(ов)

Генеральный директор ЗАО «ИНТЕРСЕДЖИКАЛ»

Парастаев Г. К.

