

ЗАО «СЭЙДЖ»

Россия, 121069, Москва,
ул. Малая Никитская, д. 20/9, стр.2



ZAO «SAGE»

Malaya Nikitskaya, 20/9, bld. 2
Moscow, 121069, Russia

Tel.: +7(095) 234 3945/46, 795 0360/61 Fax: 234 3947

Internet: <http://www.sagemed.ru> E-mail: info@sagemed.ru

Исх № _____

ПОДТВЕРЖДАЮ

Генеральный директор

ЗАО "СЭЙДЖ"

Овтемел Григори



» декабря 2015 г.

Фотографические изображения

Медицинское изделие:

Проводник урологический RocaWire

в различных исполнениях

Производитель:

"ROCAMED FRANCE"

1. Проводник RocaWire нитиноловый с гидрофильным покрытием (Картонная коробка)



ROCAMED

www.rocamed-urology.com

REF ROWP3510ST

Catalog Number

Nitinol RocaWire Curved tip

Fil guide • Cable guida


Filo guida • Geleidedraad

Fio guida • Проволоочный проводник

0.035" 150 cm



(01)03700512972006(1) 2016-10 R130835



Quantity Per Box

STERILE EO

Sterilized Using Ethylene Oxide



Consult Instructions For Use



Do Not Reuse

This device is not to be used with natural latex

LOT

R130835

Batch Code



2016-10

Use By

Caution: Federal (USA) law restricts this device to sale by or on the order of a physician.

In the USA: Distributed by ROCAMED Inc. Inc. PROMEPLA S.A.M. and its affiliates - 2010 Corporate Ridge, Suite 200, Midvale, VA 22102 Tel: 804 505 8022 E-mail: sales@rocamed-usa.com

Manufactured by PROMEPLA S.A.M. 3 Avenue Albert II - 98000 MONACO Tel: +377 97 98 42 43 Fax: +377 92 05 81 50

Out of the USA: Distributed by ROCAMED S.A.M. 3 Avenue Albert II - 98000 MONACO Tel: +377 97 98 42 43

CE 0459 Manufactures

ROCAMED France 21 de Sugères - Allée de Stockholm 33370 SIGNES FRANCE Tel: +33 484 902 100

1. Проводник
RocaWire
нитиноловый с
гидрофильным
покрытием
(Стерильный
пакет с
изделием)
Фото 1.

ROCAMED www.rocamed-urology.com

REF ROWP3510ST

Catalog Number

Nitinol RocaWire Curved tip

Fil guide • Cable guida
Filo guida • Geleidedraad
Fio guida • Проволоочный проводник



(01)03700512962007(17)161000(10)R130835

0.035" 150 cm

LOT R130835

Batch Code

2016-10

Use By

STERILE EO

Sterilized Using Ethylene Oxide



This device is not
made with natural
rubber latex



Consult Instructions
For Use



Do Not Reuse

Caution : Federal (USA) law restricts this device to sale by or on the order of a physician

In the USA: Distributed by ROCAMED Inc for PROMEPLA S.A.M.
and its affiliates • 2010 Corporate Ridge, Suite 700, McLean, VA 22102
Tel: 804 525 882 2 E-mail: sales@rocamed-us.com

Manufactured by PROMEPLA S.A.M.
9 avenue Albert II - 98000 MONACO
Tel: +377 97 98 42 43 Fax: +377 92 05 61 50

Out of the USA: Distributed by ROCAMED S.A.M.
9 avenue Albert II - 98000 MONACO
Tel: +377 97 98 42 43



Manufacturer

ROCAMED France - ZI de Signes
Allée de Stockholm - 83870 SIGNES FRANCE
Tel: +33 494 902 100

REF ROWP3510ST

Number

LOT R130835

Use By **2016-10**

REF ROWP3510ST

R130835

2016-10

REF ROWP3510ST

Number

LOT R130835


Use By **2016-10**

REF ROWP3510ST

R130835

Use By **2016-10**

1. Проводник
RocaWire
нителиловый с
гидрофильным
покрытием
(Стерильный
пакет с
изделием)
Фото 2.

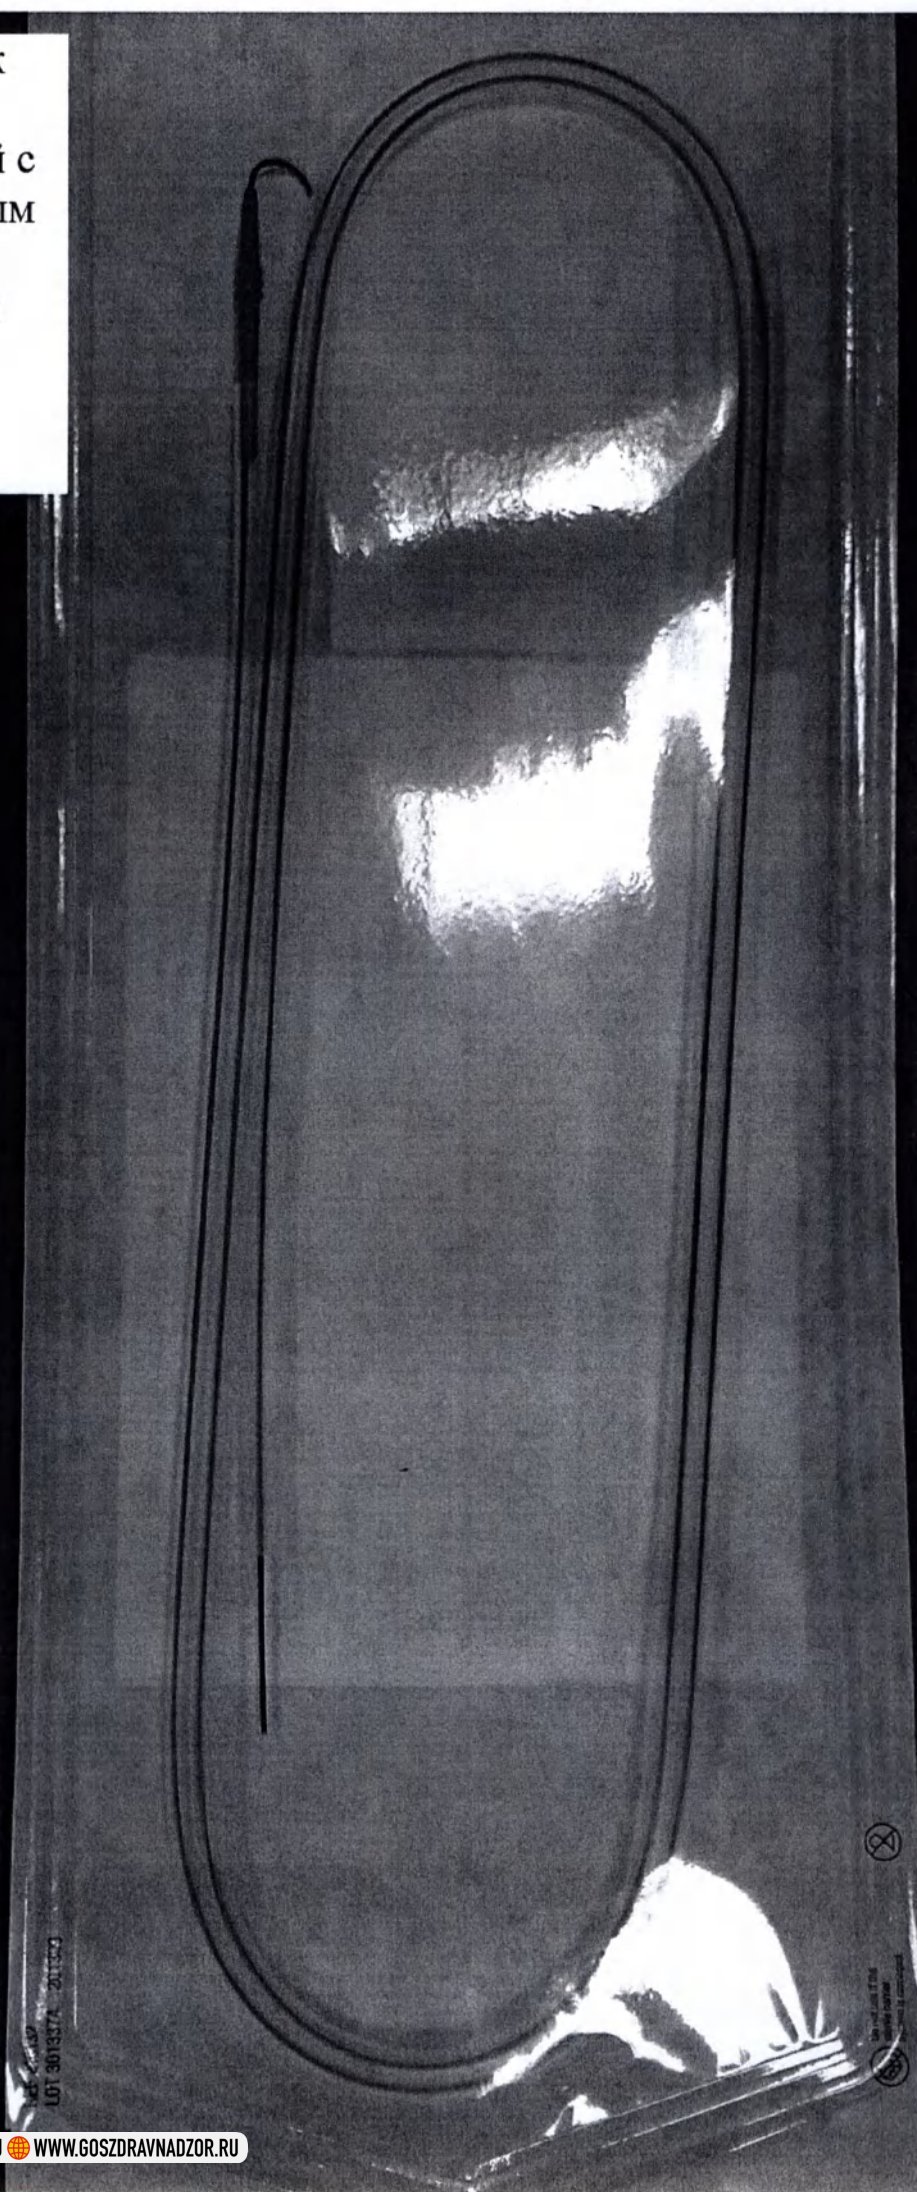

2. Проводник RocaWire STIFF нитиноловый с гидрофильным покрытием
(Картонная коробка)



ROCAMED www.rocamed-ortho.fr

Nitinol RocaWire Stiff
Fil guide : Guide guide
Fil guide : Guide guide
Fil guide : Guide guide

REF ROWP3502ST
Catalog Number

0.035" 150 cm

LOT R150554
Batch Code

2018/05
Use By

STERILE EO
Sterilized Using Ethylene Oxide

Do Not Reuse

CE

ROCAMED France - ZI de Sighe - Allée de Stockholm - 83070 SIGHE - FRANCE
Manufactured by ROCAMED S.A.M. - 9 Avenue Albert II - 98000 MONACO - tel +377 57 98 42 43

Quantity Per Box
x10

Barcode
(01)03700512571988(17)170100(10)R150554

Caution This device is not made with natural rubber latex

Consult Instructions For Use

2. Проводник RocaWire STIFF
 нитиноловый с гидрофильным
 покрытием
 (Стерильный пакет с изделием)
 Фото 1.

REF ROWP3502ST
 Catalog Number

0.035" 150 cm

ROCAMED www.rocamed-urology.com

Nitinol RocaWire Stiff


Fil guide - Cable guide
 Filo guida - Cabelodguida
 Filo guia - Проводниковый проводник



(01)03700512961987(17)180500(10)R150554

LOT R150554
 Batch Code

Use By 2018/05



STERILE EO
 Sterilized Using Ethylene Oxide

This device is not
 made with natural
 rubber latex

Caution / Federal (USA) law restricts this device to sale by or on the order of a physician

In the USA: Distributed by ROCAMED Inc. for PROMEPILA S.A.M.
 9 avenue Albert II - 2010 Corporate Ridge, Suite 700, McLean, VA 22102
 Tel: (703) 905 8822 E-mail: sales@rocamed-usa.com

Out of the USA: Distributed by ROCAMED S.A.M.
 9 avenue Albert II - 98000 MONACO
 Tel: +377 97 36 42 43




ROCAMED France - 21 de Signes
 Aisle de Stockholm - 82879 SIGNES FRANCE
 Tel: +33 494 902 100

REF ROWP3502ST
 Catalog Number
LOT R150554
 Batch Code
 Use By 2018/05

REF ROWP3502ST
 Catalog Number
LOT R150554
 Batch Code
 Use By 2018/05

REF ROWP3502ST
 Catalog Number
LOT R150554
 Batch Code
 Use By 2018/05

2. Проводник RocaWire STIFF
нитиноловый с гидрофильным
покрытием (стерильный пакет с
изделием) Фото 2.

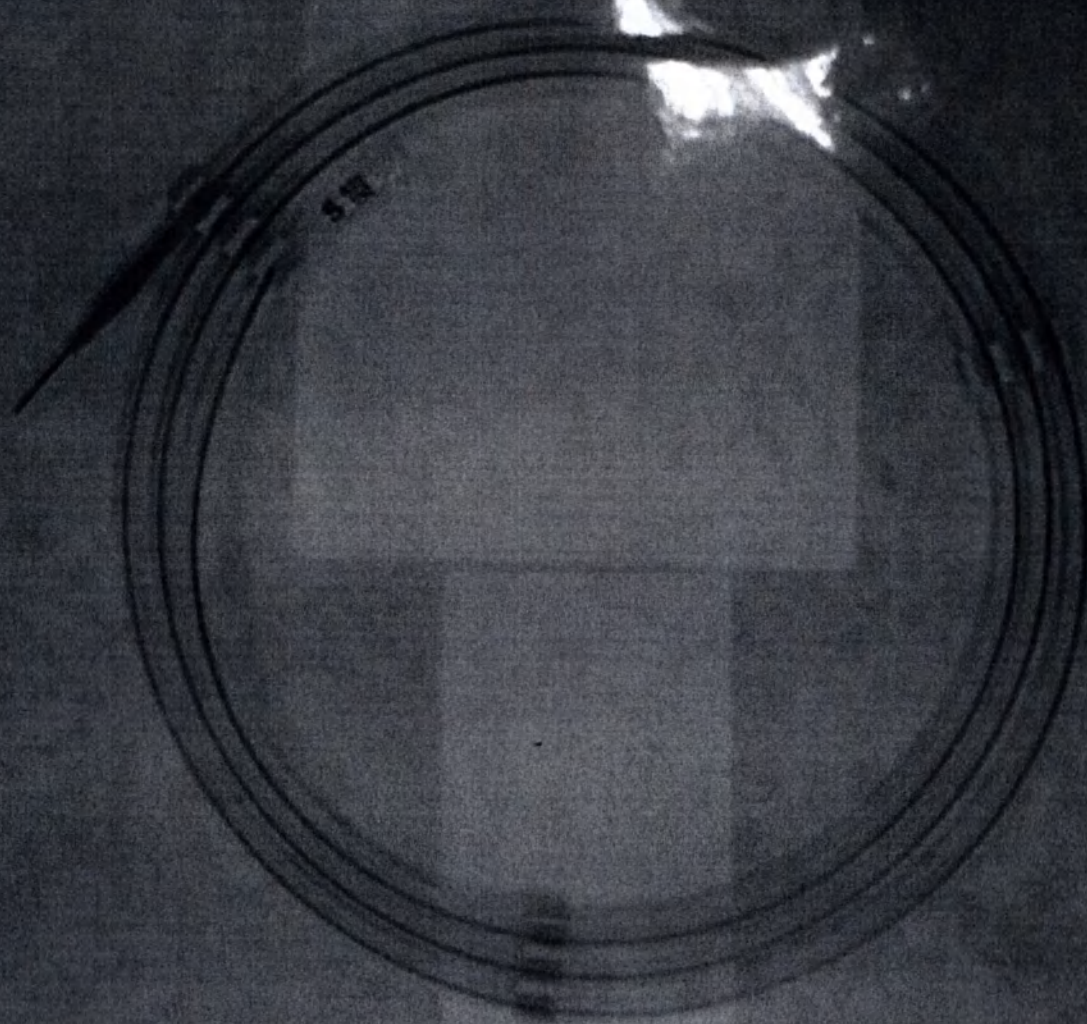

3. Проводник RosaWire стальной с покрытием из ПТФЭ (картонная коробка)

ROCAMED

www.rocamed-urolgy.com


PTFE-coated RocaWire
Curved tip




(01)03700512972051(17)170200(10)R140212

STERILE EO

Sterilized Using Ethylene Oxide




Consult Instructions
For Use



This device is not
made with natural
rubber latex




Do Not Reuse



Quantity Per Box

LOT R140212

Batch Code





2017-02

Use By

Caution : Federa, (USA) law restricts this device to sale by or on the order of a physician

In the USA: Distributed by ROCAMED Inc. for PROMEPLA S.A.M.
and its affiliates - 2010 Corporate Ridge, Suite 700, McLean, VA 22102
Tel: 804 525 8822 E-mail: sales@rocamed-us.com

Manufactured by PROMEPLA S.A.M.
9 avenue Albert II - 98000 MONACO
Tel: +377 97 98 42 43 Fax: +377 92 05 61 50



Manufacturer

ROCAMED France
ZI de Signes - Allée de Stockholm
83570 SIGNES FRANCE
Tel: +33 494 902 100

Out of the USA: Distributed by
ROCAMED S.A.M.
9 avenue Albert II - 98000 MONACO
Tel: +377 97 98 42 43

REF ROWG3510ST

Catalog Number

0.035" 150 cm



3. Проводник RosaWire стальной с покрытием из ПТФЭ (стерильный пакет с изделием) Фото 1.

ROCAMED
www.rocamed.ru

REF ROWG3S10ST
Lottery Number

PTFE-coated RocaWire
Curved tip

0.035" 150 cm


(01) 0027 0000 12962902(17) 17E2004 103041-002-12

STERILE EO
Sterilized using Ethylene Oxide



This device is not
reusable with heat
labelling system


Consult instructions
For use

2 Use Max Force

LOT R140212
Batch Code


2017-02
Use By


Conformé à la norme
EN ISO 13485

ROCAMED France - 28 rue de la
Liberté - 92000 Nanterre - France
Tél : +33 (0)1 47 35 10 00 - Fax : +33 (0)1 47 35 10 01

ROCAMED Inc. 10000 Highway 7
Suite 100 - Richmond, BC V6X 1A6
Canada
Tél : +1 (604) 271-1111 - Fax : +1 (604) 271-1112

REF ROWG3S10ST
Lottery Number


LOT R140212
Batch Code


2017-02
Use By


This device is not
reusable with heat
labelling system


Consult instructions
For use

2 Use Max Force


Conformé à la norme
EN ISO 13485

ROCAMED France - 28 rue de la
Liberté - 92000 Nanterre - France
Tél : +33 (0)1 47 35 10 00 - Fax : +33 (0)1 47 35 10 01

ROCAMED Inc. 10000 Highway 7
Suite 100 - Richmond, BC V6X 1A6
Canada
Tél : +1 (604) 271-1111 - Fax : +1 (604) 271-1112

3. Проводник
RocaWire
стальной с
покрытием из
ПТФЭ
(стерильный
пакет с
изделием)
Фото 2.



Проводник RocaWire стальной с покрытием из
ФЭ для нефростомии
(тонная коробка)



ROCAMED
www.rocamed-urology.com

Nephro RocaWire

Fil guide pour néphrostomie • Cable guide pour néphrostomie
Filr guida per nefrostomia • Guida di guida per nefrostomia
Filr guida para nefrostomia • /Гидроурологический спонгиоз для нефростомии

0.035" 100 cm



(01)03700512572075(17)161200(10)R131105



Quantity Per Box

STERILE EO

Sterilizing Ethylene Oxide



Consult Instructions For Use



This device is not made with natural rubber latex



Do Not Reuse

LOT R131105
Batch Code

Use By 2016-12



ROCAMED France - ZI de Signes
Allée de Stockholm - 83870 SIGNES - FRANCE

Distribue par / Distributed by **ROCAMED S.A.M.** - 3 avenue Albert II - 98000 MONACO - tel +377 57 58 42 43

Проводник RocaWire стальной с
крытием из ПТФЭ для нефростомии
в стерильном пакете с изданием Фото 1.

ROCAMED www.rocamed-urology.com

REF ROWS3500ST
Catalog Number

Nephro RocaWire

Fil guide pour nephrostomie - Cable guia para nefrostomia
Filo guida per nefrostomia - Geleidedraad voor nefrostomie
Fio guia para nefrostomia - Проводочный проводник для нефростомии

0.035" 100 cm



(01)03700512962076(17)161200(10)R131105

LOT R131105

Batch Code

2016-12

Use By

STERILE EO

Sterilized Using Ethylene Oxide



This device is not
made with natural
rubber latex



Consult Instructions
For Use



Do Not Reuse

CE 0459

Manufacturer

ROCAMED France - ZI de Signes
Allée de Stockholm - 83870 SIGNES - FRANCE

Distribué par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

REF ROWS3500ST

Catalog Number

LOT R131105

Batch Code

Use By 2016-12

REF ROWS3500ST

Catalog Number

LOT R131105

Batch Code

Use By 2016-12

REF ROWS3500ST

Catalog Number

LOT R131105

Batch Code

Use By 2016-12

REF ROWS3500ST

Catalog Number

LOT R131105

Batch Code

Use By 2016-12

4. Проводник RosaWire стальной с покрытием из ПТФЭ для нефростомии (стерильный пакет с изделием) Фото 2.



Проводник RocaWire RIO TRACER нитиноловый с
покрытием из ПТФЭ, с гидрофильным наконечником
(картонная коробка)



ROCAMED www.rocamed-urology.com

RocaWire Rio Tracer™

guide - Cable guide
guide - Geländeguide
Rio guide - Позиционный проводник

REF ROWR3502ST
Catalog Number

3.035" 150 cm

LOT R150551
Batch Code

Quantity Per Box
x10

STERILE EO
Sterilized Using Ethylene Oxide

Do Not Reuse

Use By 2018-05

(61)03700512975250(17)180500(10)R150551

Caution: Federal (USA) law restricts this device to sale by or on the order of a physician.

Manufactured by: PROMEPLA S.A.M.
9 Avenue Albert II - 98000 MONACO
Tel: +377 97 98 42 43 Fax: +377 92 05 61 50

ROCAMED France
ZI de Signes - Allée de Stockholm
63070 SIGNES FRANCE
Tel: +33 454 302 100

Manufacturer

CE 0459

For the USA: Distributed by
ROCAMED S.A.M.
9 Avenue Albert II - 98000 MONACO
Tel: +377 97 98 42 43

5. Проводник RocaWire RIO TRACER
 нитиноловый с покрытием из ПТФЭ, с
 гидрофильным наконечником
 (стерильный пакет с изделием) Фото 1.

ROCAMED www.rocamed-urology.com

RocaWire Rio Tracer™

Fil guide - Cable guide
 Filo guida - Gebiedelraad
 Filo guida - Гидрофильный проводник



(01)0370051296525(17)180500(10)R150551

STERILE EO
 Sterilized Using Ethylene Oxide

 This device is not
 made with natural
 rabbit skin.

 Consult Instructions
 For Use

 Do Not Reuse

REF R150551
 Catalog Number
LOT R150551
 Batch Code
 Use By 2018-05

0.035" 150 cm

REF R150551
 Catalog Number
LOT R150551
 Batch Code
 Use By 2018-05

Caution: Federal (USA) law restricts this device to sale by or on the order of a physician

In the USA: Distributed by ROCAMED Inc. for PROMEPLA S.A.M.
 20100 Corporate Center Drive, Suite 700, McLean, VA 22102
 Tel: 804 525 5822 E-mail: sales@rocamed-us.com

Out of the USA: Distributed by ROCAMED S.A.M.
 9 avenue Albert II - 98000 MONACO
 Tel. +377 97 96 42 43

Manufactured by PROMEPLA S.A.M.
 9 avenue Albert II - 98000 MONACO
 Tel: +377 97 96 42 43 Fax: +377 92 06 61 50

CE 0459

Manufacturer

ROCAMED France - ZI de Signes
 Allée de Stockholm - 83870 SIGNES FRANCE
 Tel. +33 494 902 100


REF R150551
 Catalog Number
LOT R150551
 Batch Code
 Use By 2018-05

REF R150551
 Catalog Number
LOT R150551
 Batch Code
 Use By 2018-05

REF R150551
 Catalog Number
LOT R150551
 Batch Code
 Use By 2018-05

REF R150551
 Catalog Number
LOT R150551
 Batch Code
 Use By 2018-05

8. Проводник RocaWire RIO TRACER
нителиновый с покрытием из ПТФЭ, с
гидрофильным наконечником
(стерильный пакет с изделием) Фото 2.

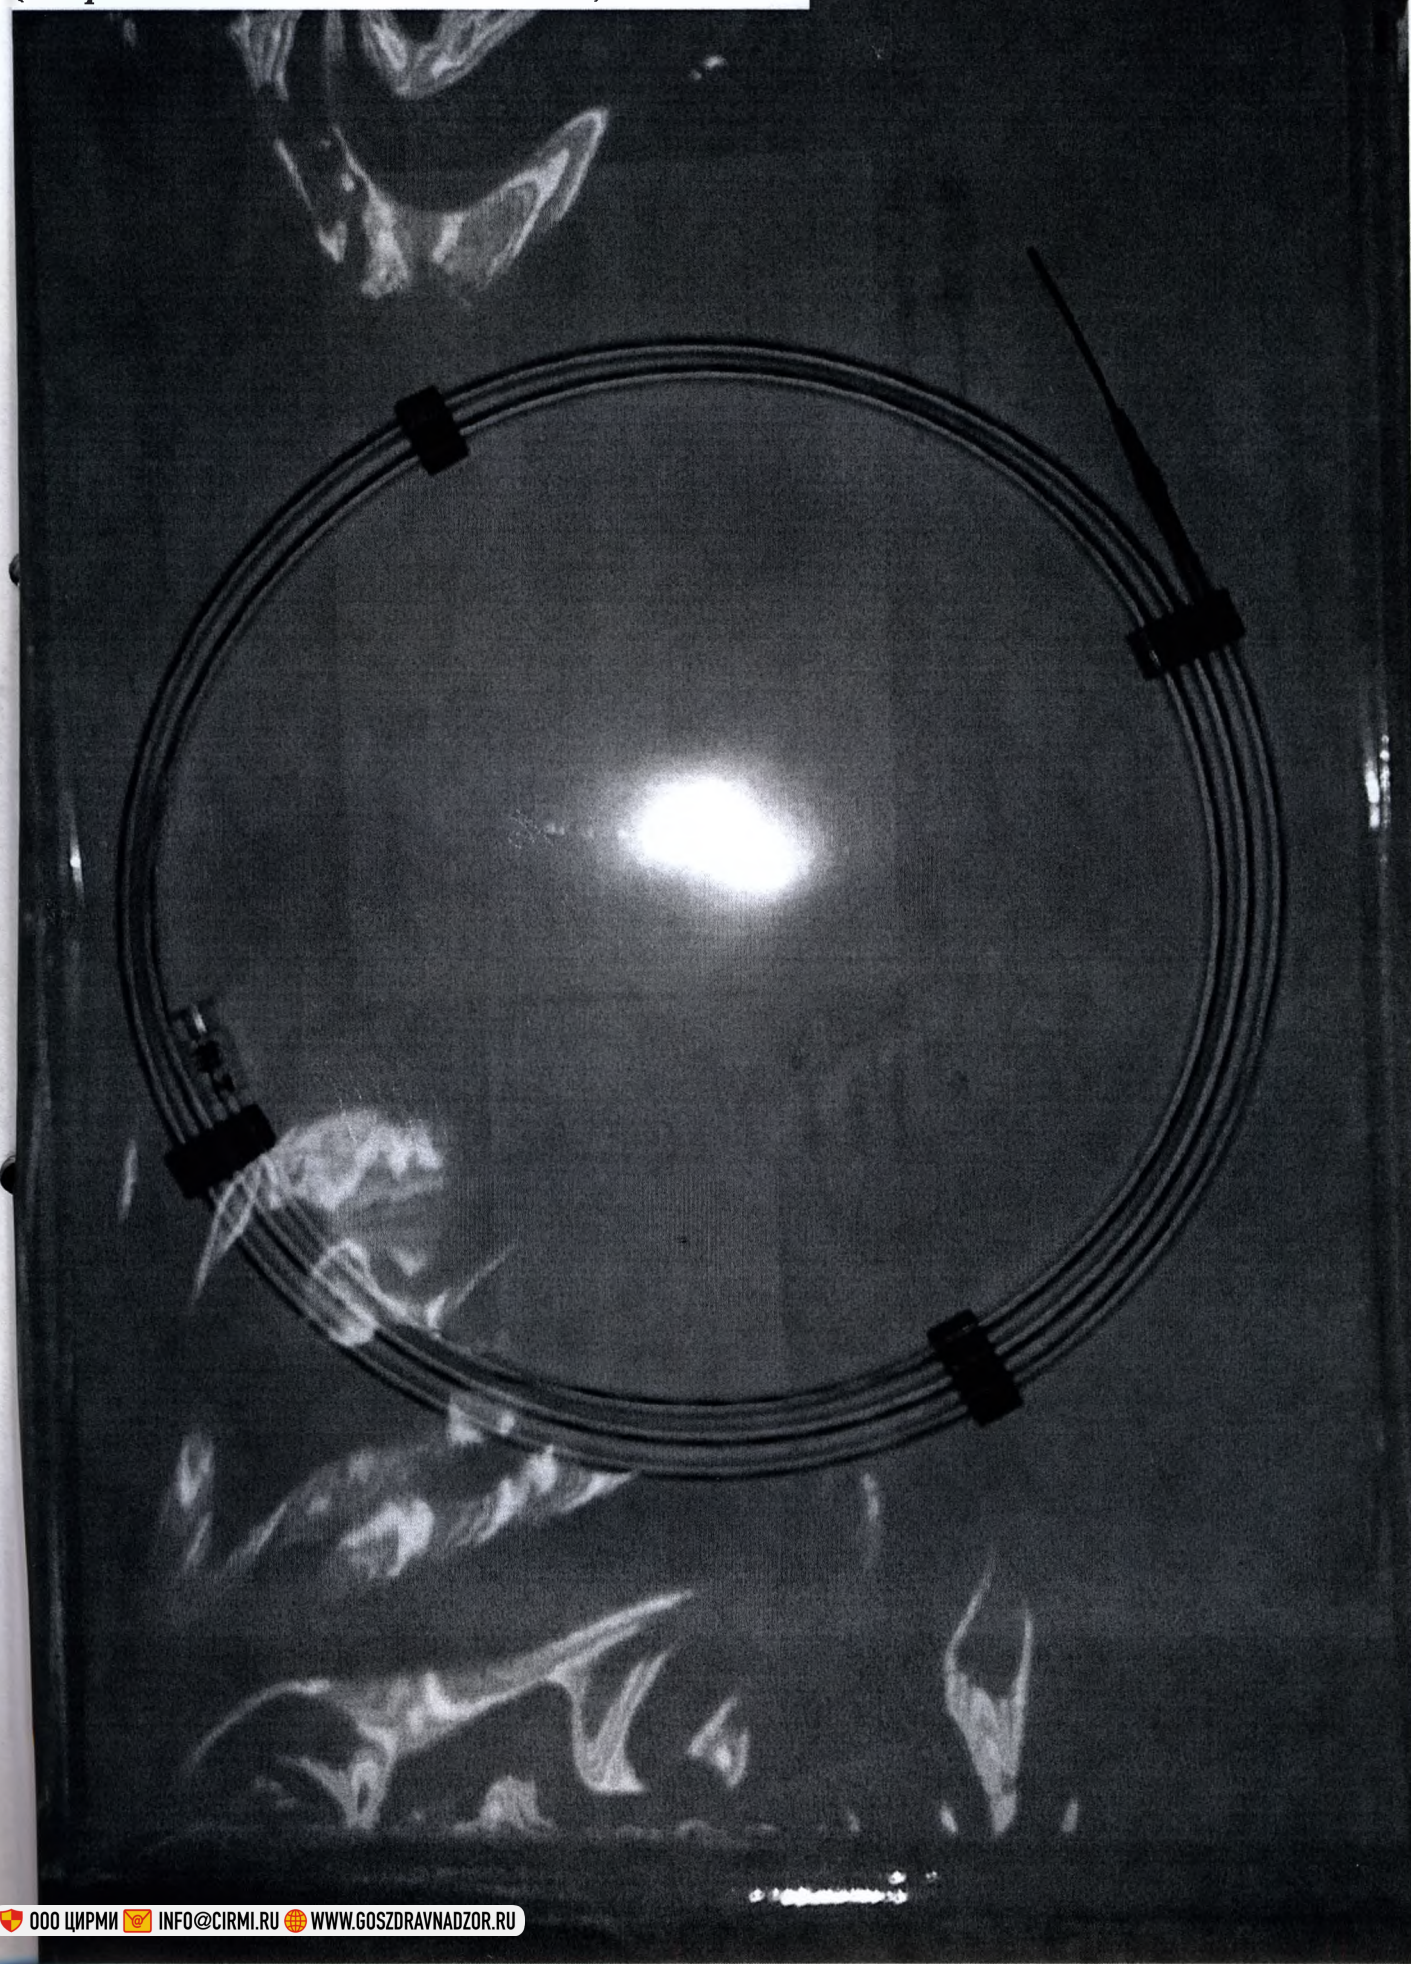

Всего пронумеровано,
прошнуровано и
скреплено печатью
16 листа (ов)

