



ПОДТВЕРЖДАЮ
Генеральный директор
ЗАО «Трейдомед Инвест»

« 18 » 07 _____ Сутягин С.А.
2016 г.



**Фотографические изображения
на медицинское изделие**
«Прибор ручной диагностический для офтальмо и ретиноскопии
с принадлежностями»



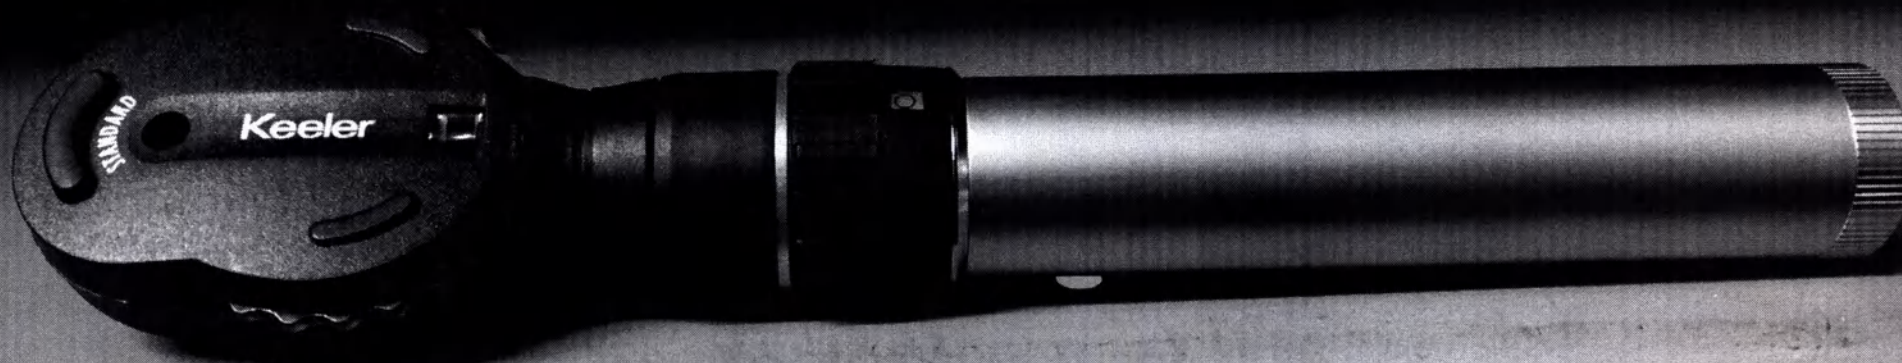

1126-P-1006|2FC-C01|902|A
3.5v Standard Ophth in Cas
2FC-C01 Bin: A EA FGDS 902


1126-P-1006
SLIMLINE 3.6V STANDARD OPHTH IN CASE



Keeler
A PALMA COMPANY
2016-03
2.8V PRACTITIONER OPHTH IN CASE

REF 1127-P-1005
LOT 160330




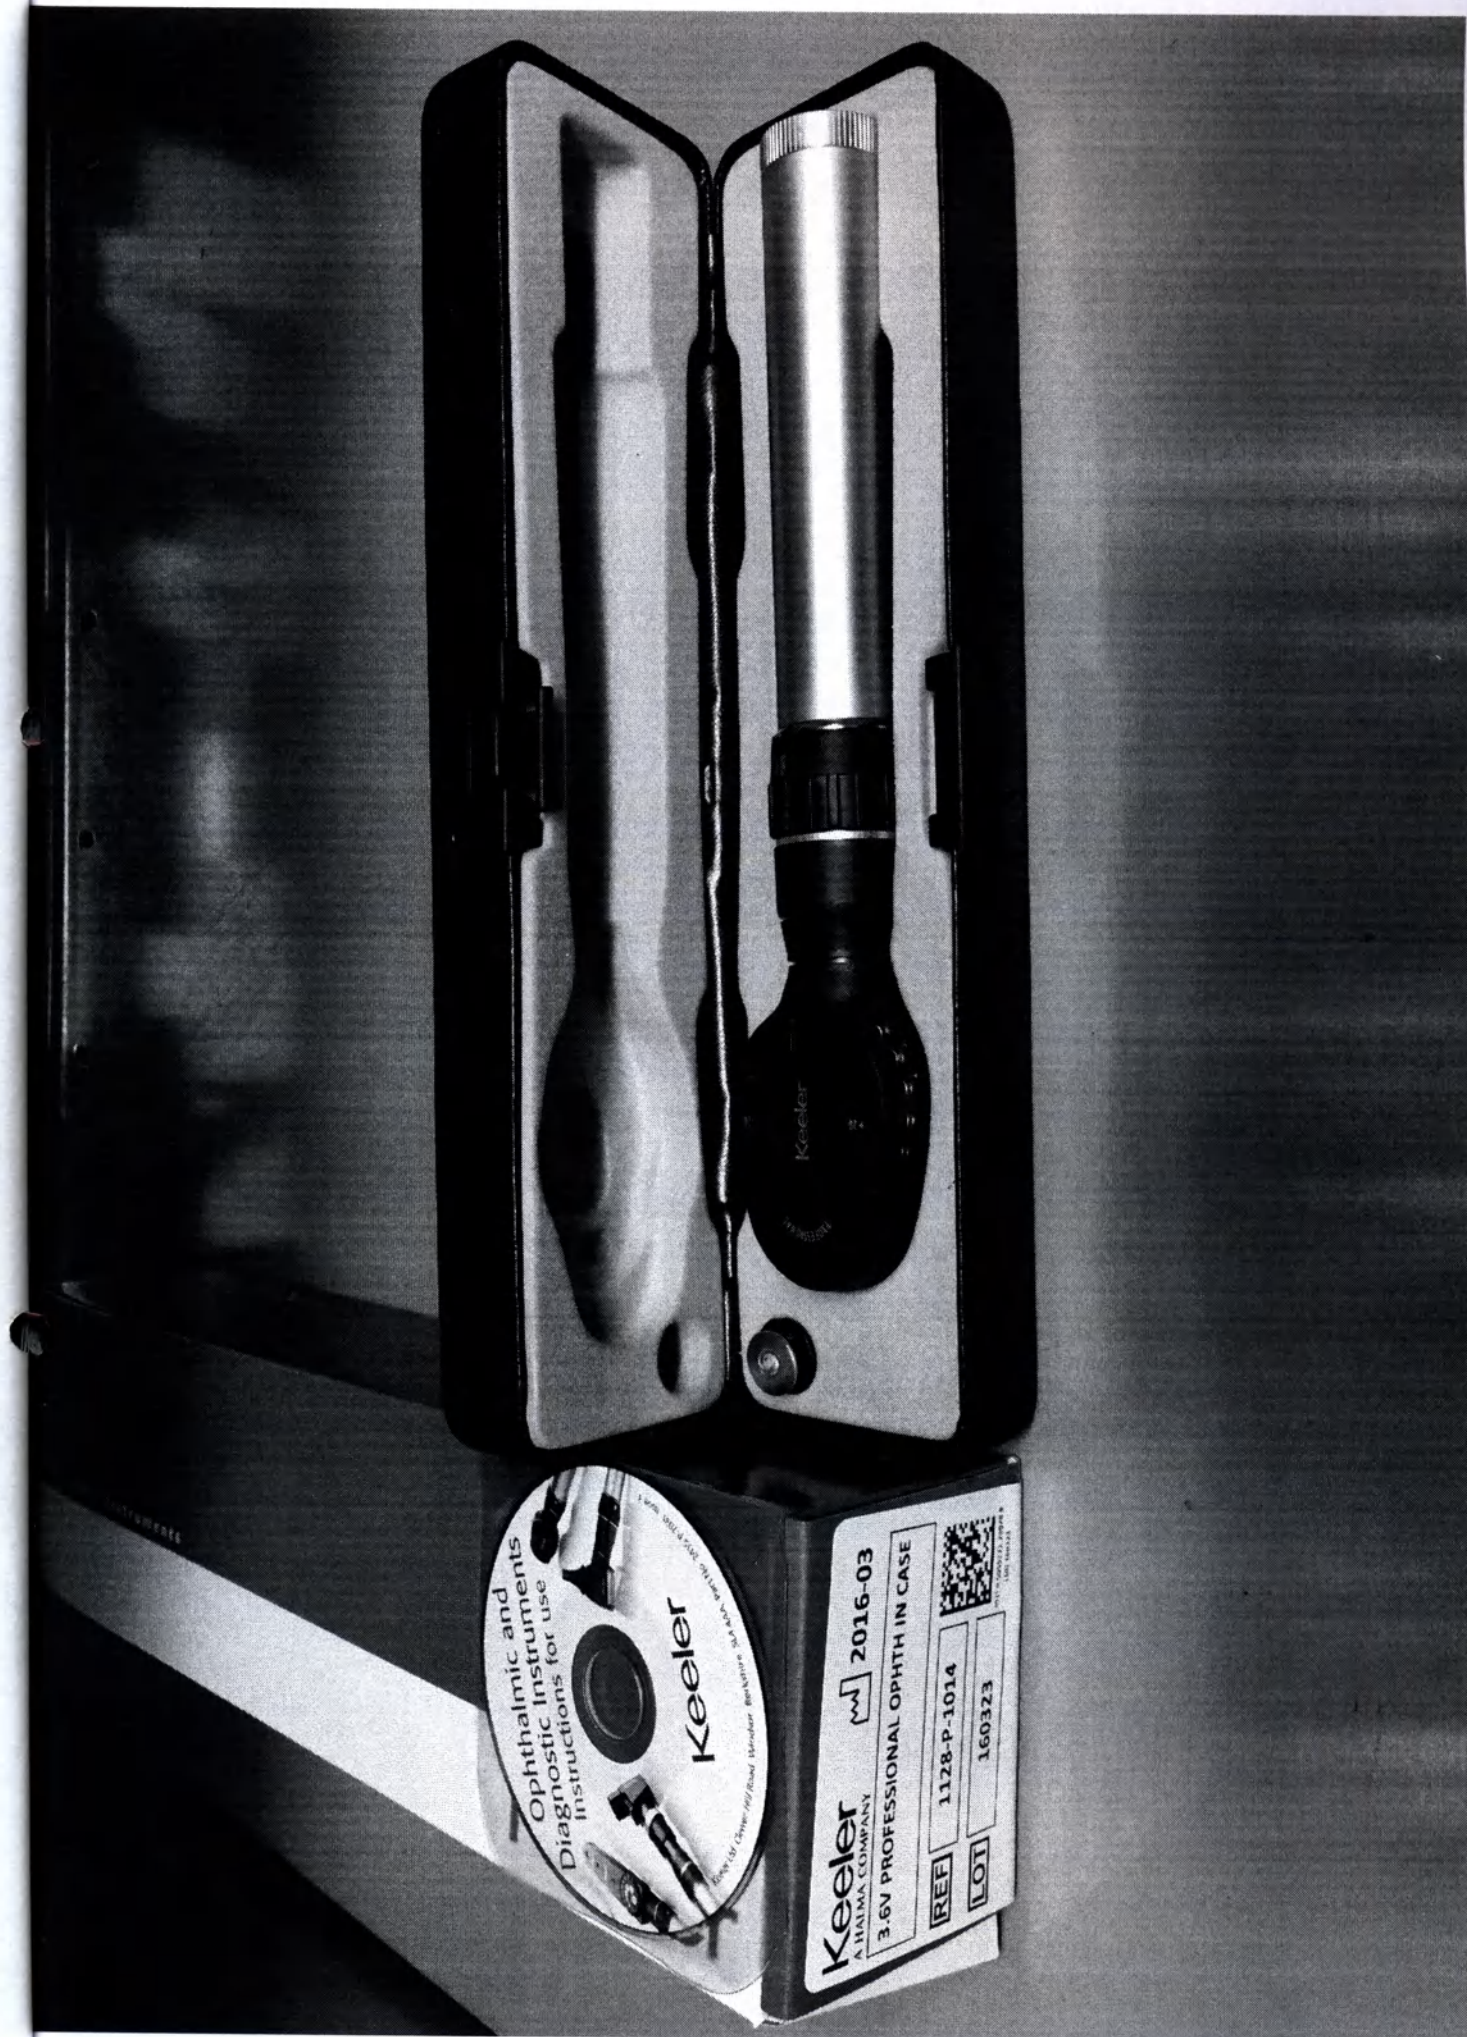








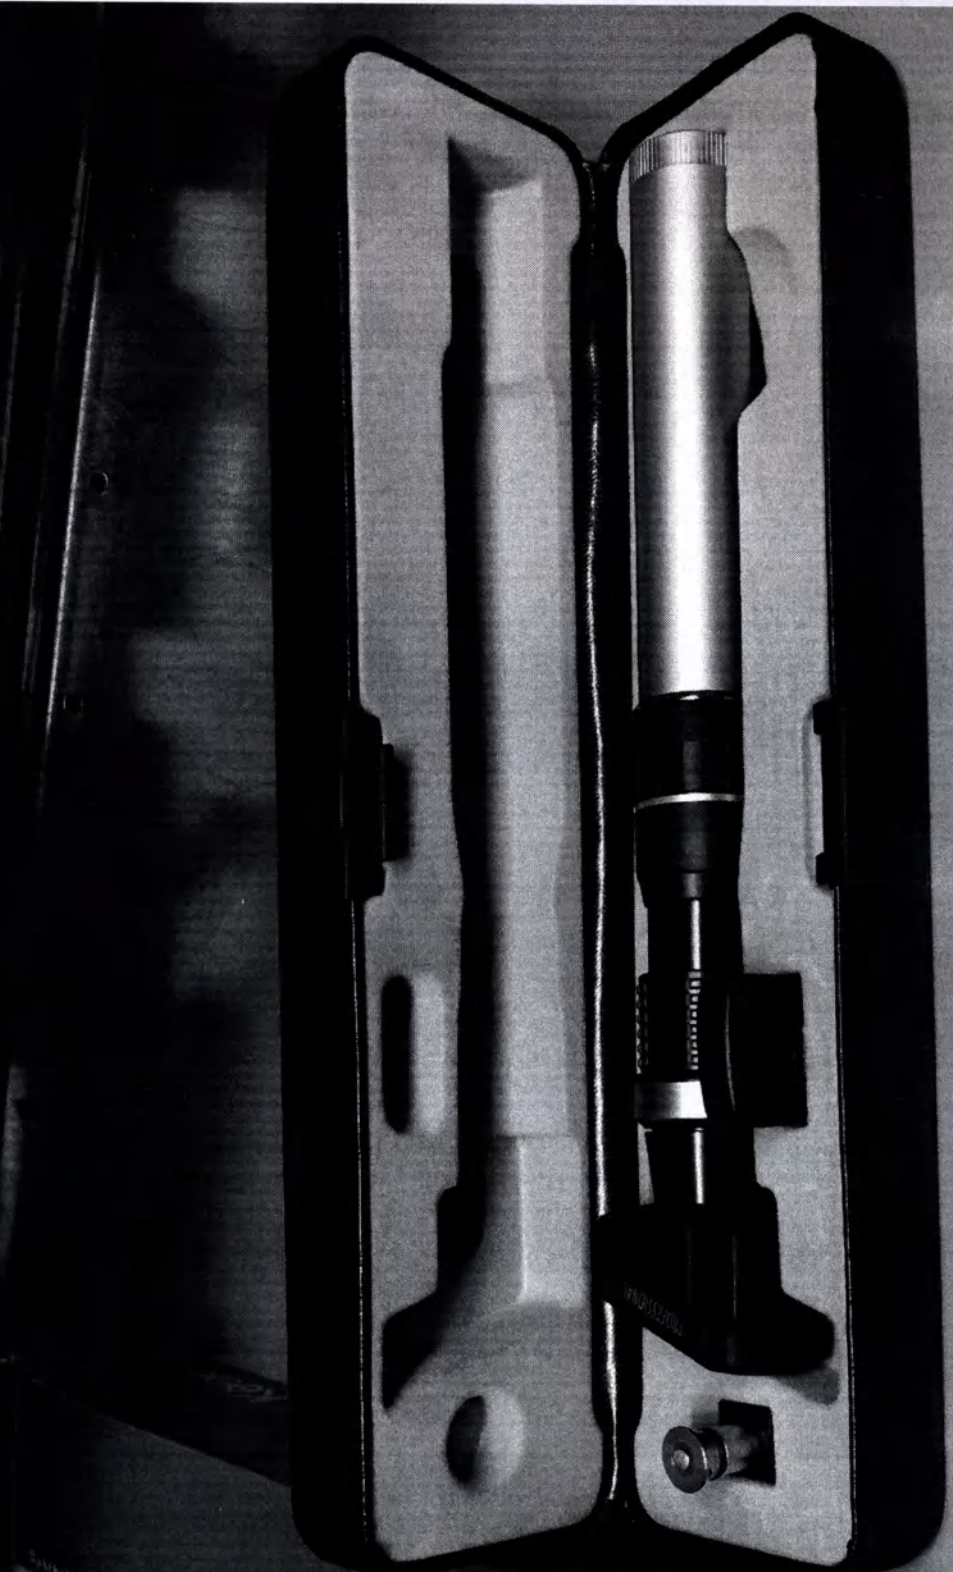





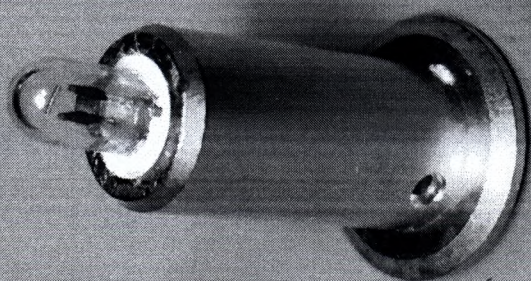






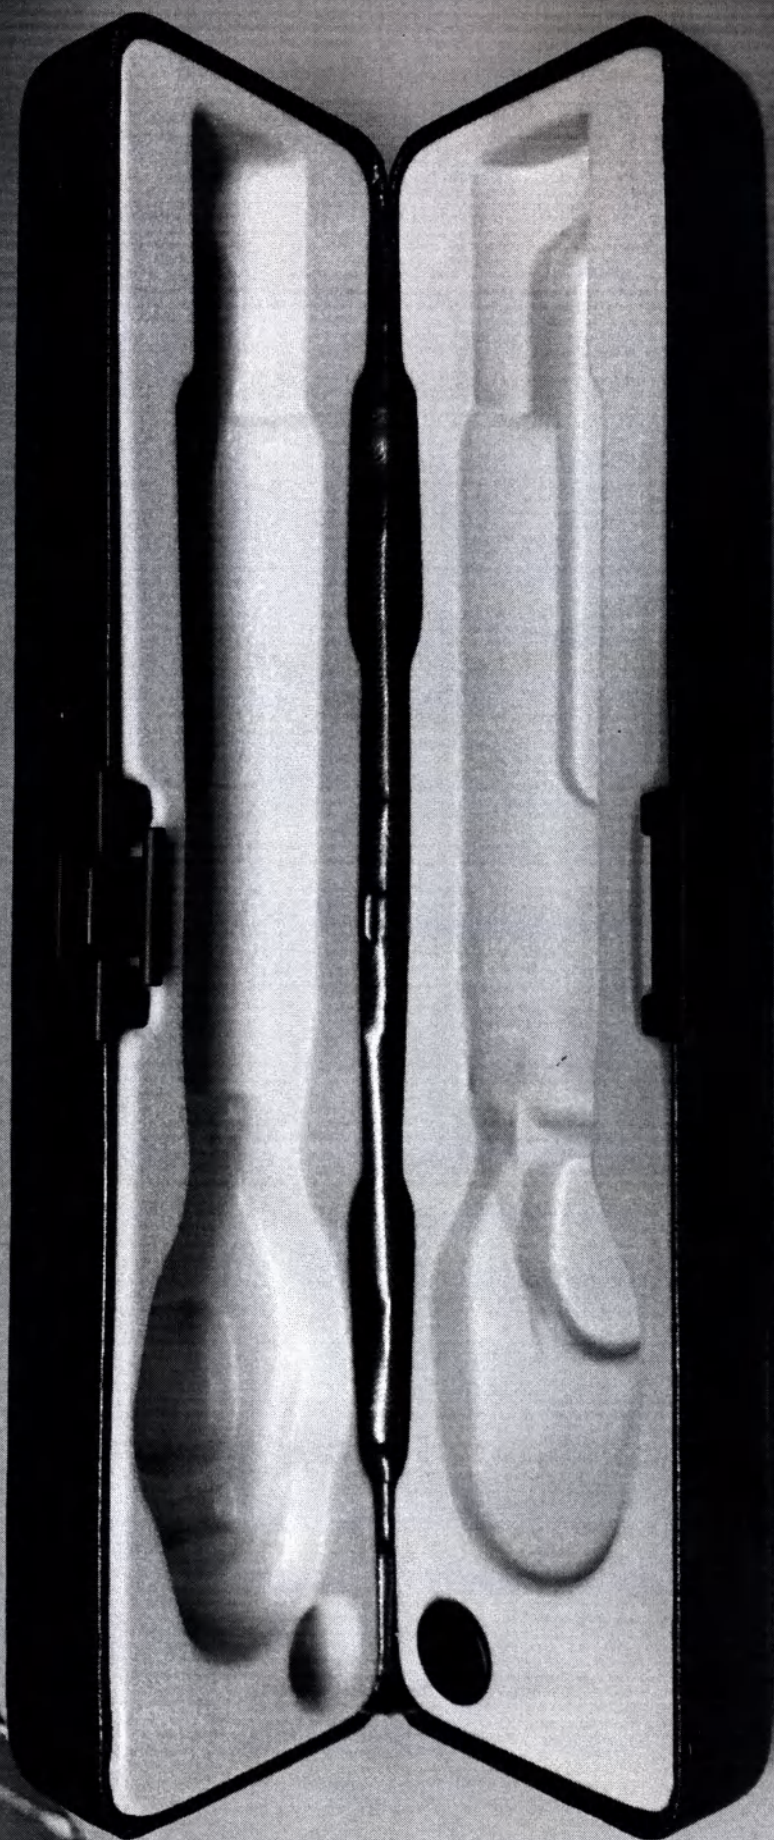

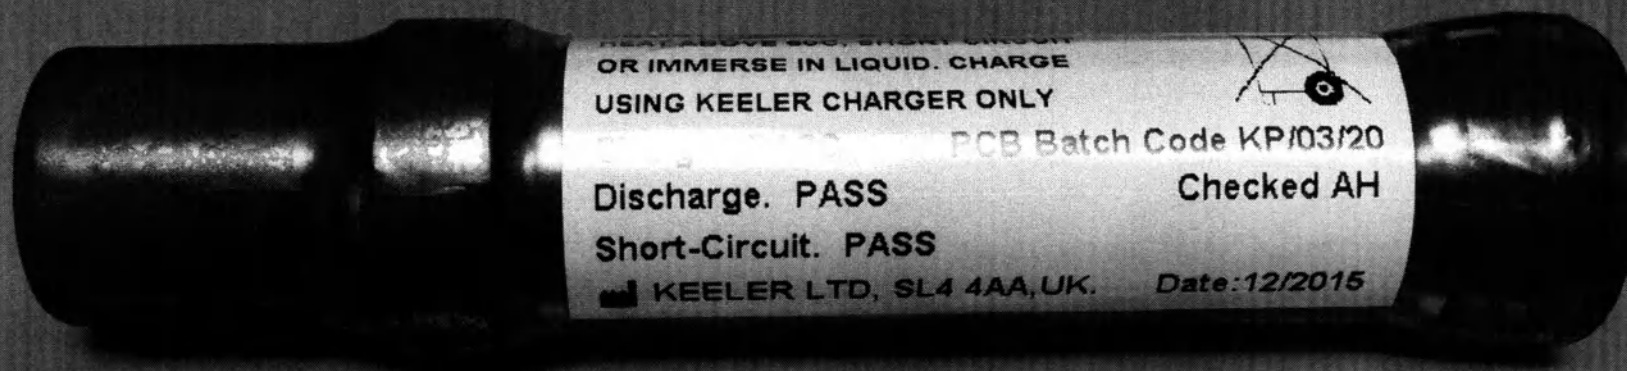

NEVER REMOVE GEL, EXPOSE TO SUN
OR IMMERSE IN LIQUID. CHARGE
USING KEELER CHARGER ONLY



PCB Batch Code KP/03/20

Discharge. PASS

Checked AH

Short-Circuit. PASS

KEELER LTD, SL4 4AA, UK.

Date: 12/2015



Keeler
A HALMA COMPANY

2016-03

LITHIUM DOUBLE CHARGER

REF 1941-P-1368

SN 168066

(01) 0 5055272 70277
(21) 168066

CE

RoHS
CONSULT
INSTRUCTIONS
FOR USE

FRAGILE

DO NOT USE IF
PACKAGE IS
DAMAGED

MADE IN
THE UK


Keeler Ltd., Clewer Hill Rd.,
Windsor, Berkshire SL4 4AA

10% 95

-40°C

KEEP DRY



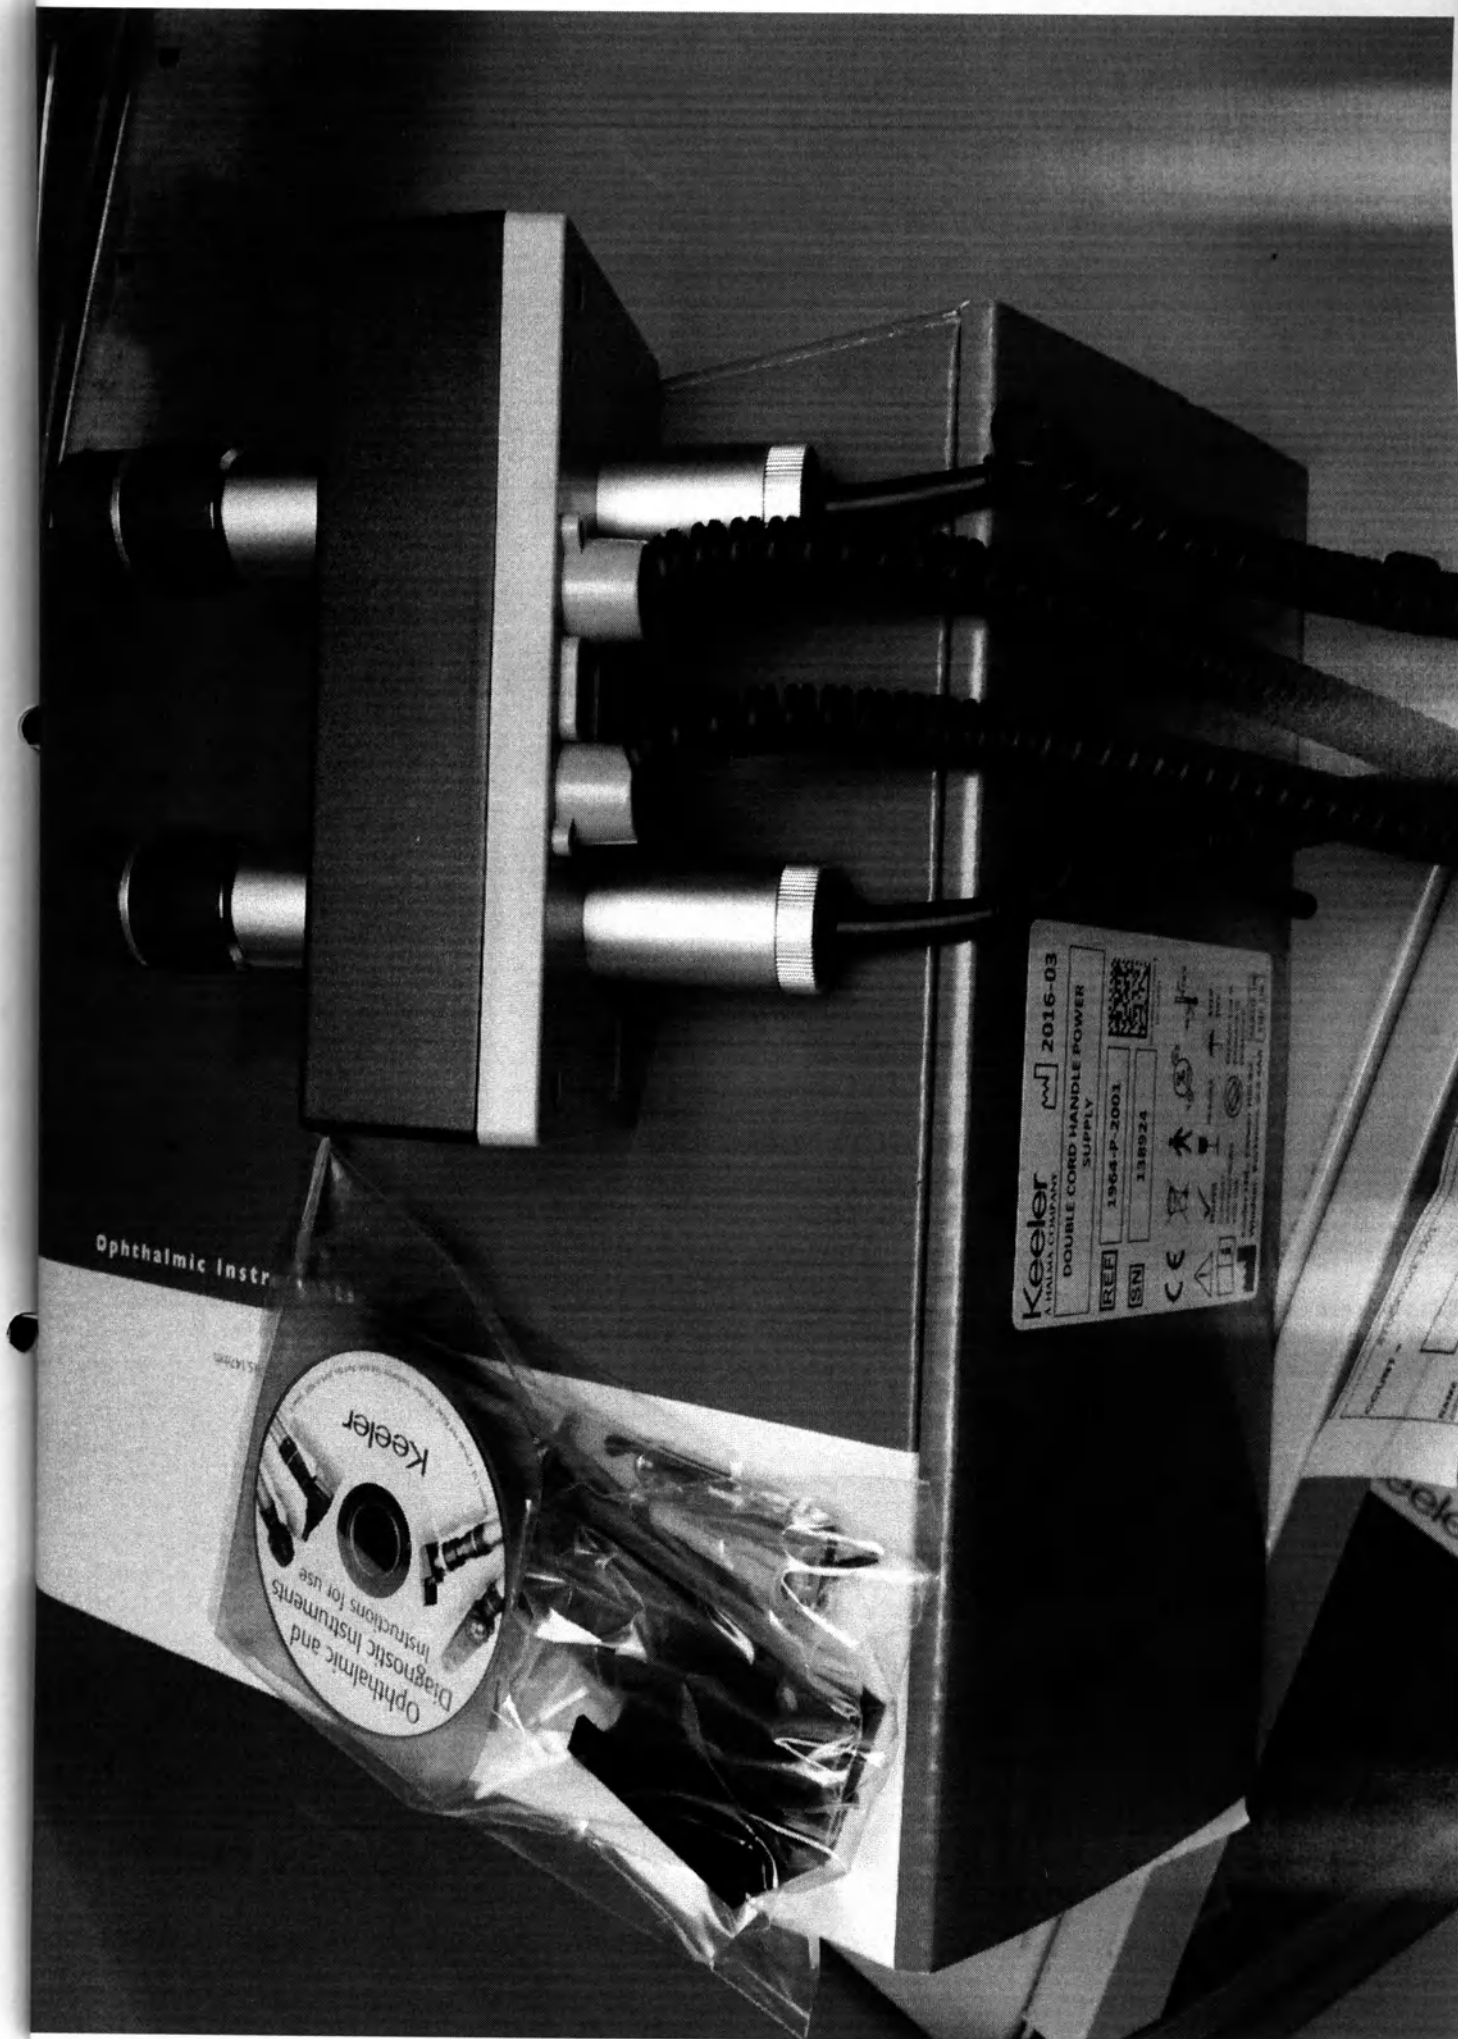

Keeler
A HALLAM COMPANY
2016-03
DOUBLE CORD HANDLE POWER
SUPPLY
REF 1964-P-2001
SN 138924
CE
WEEE
RoHS
FSC
Recycling symbol
Keeler
1964-P-2001
138924
1964-P-2001
138924

Ophthalmic Instr

Keeler
Ophthalmic and
Diagnostic Instruments
for use











Диагностические ручные приборы

Офтальмоскоп / ретиноскоп / отоскоп

Руководство по эксплуатации



Keeler

24 листа




ПОДТВЕРЖДАЮ
Генеральный директор
ЗАО «Трейдомед Инвест»

 Сутягин С.А.
«28» ноября 2016

**Фотографические изображения
на принадлежности**

«Сетевой штекер» и «Сетевой адаптер питания»

к медицинскому изделию
«Прибор ручной диагностический для офтальмо и ретиноскопии
с принадлежностями»

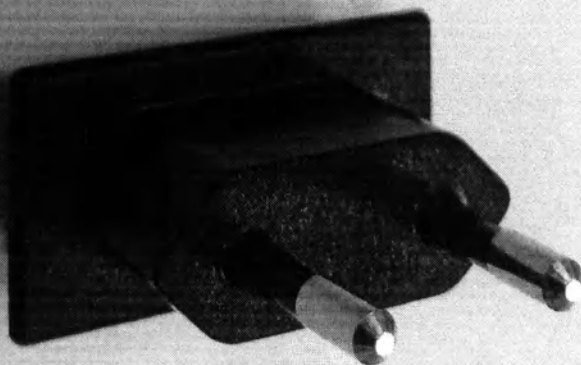

FIT MAINS INPUT PLUG BEFORE USE
AC/DC ADAPTER EP29-32777
Type: FW7362M/12 Made in Germany

Input: 100-240V~/ 50-60Hz/ 700mA
Output: 12V~/ 2.5A

CAUTION: 
RISK OF ELECTRICAL SHOCK
DRY LOCATION USE ONLY

 **Keeler**

220-240V Q02748 



IP40

T40/F



100V



TÜV Rheinland
Keeler YNA










120V



For I.T. and Medical Equipment

Class 2

C  US
E143128

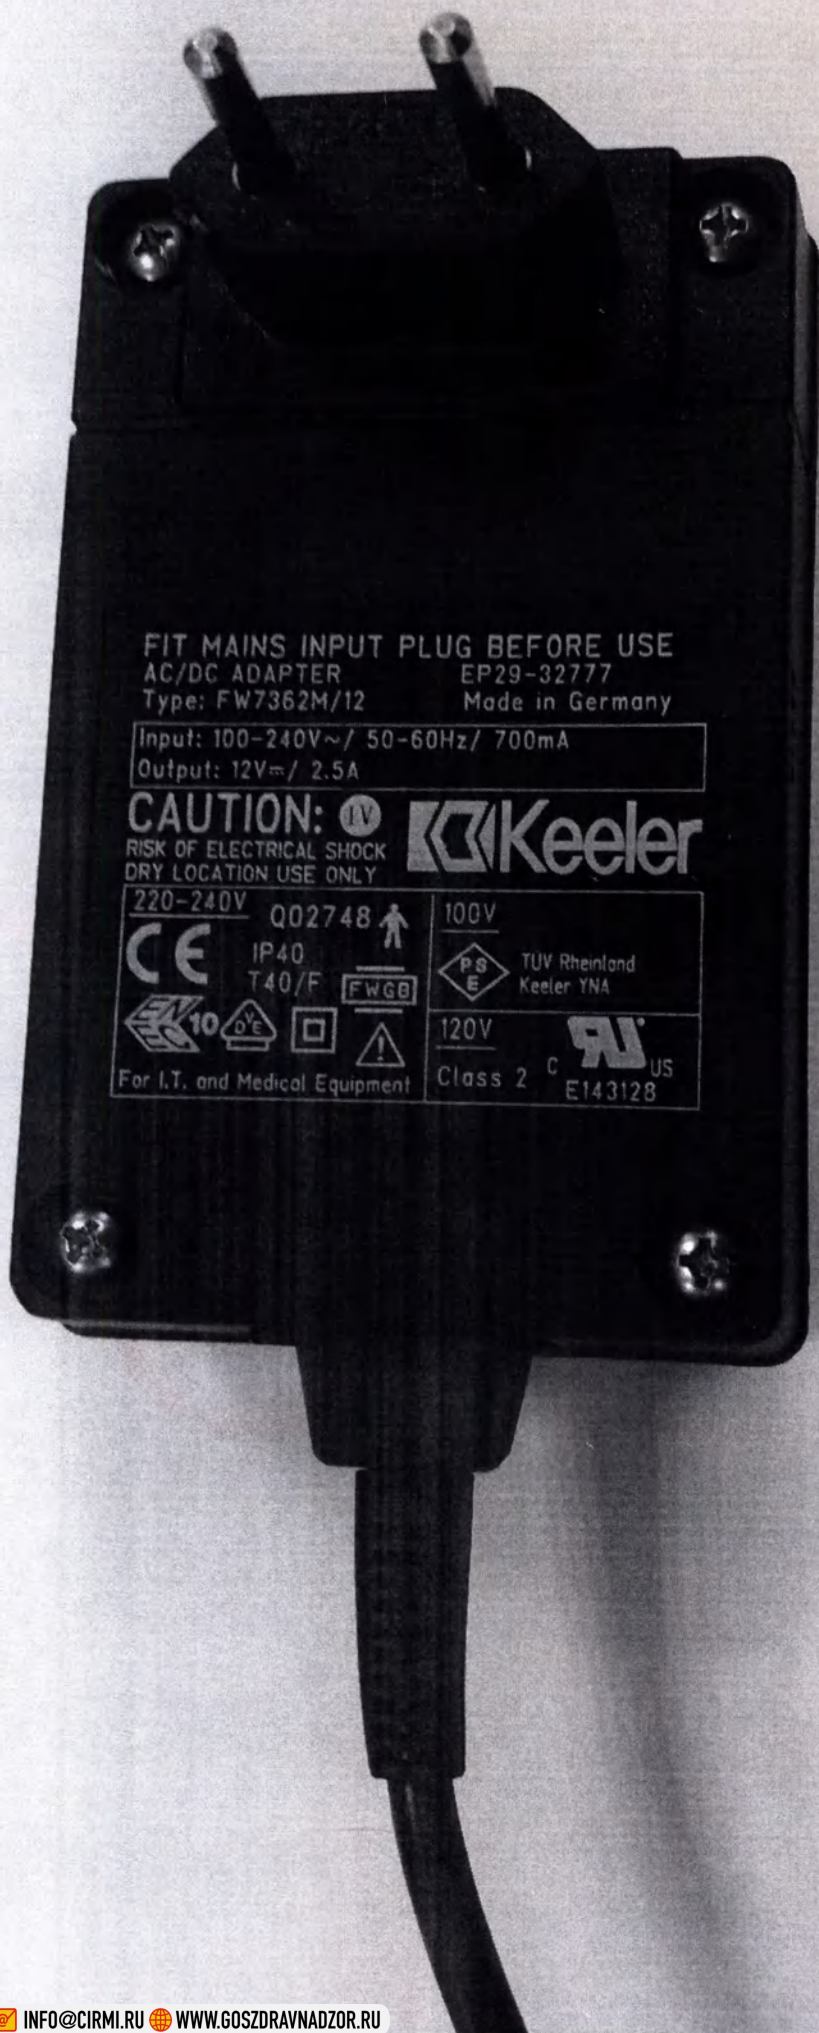

FIT MAINS INPUT PLUG BEFORE USE

AC/DC ADAPTER

EP29-32777

Type: FW7362M/12

Made in Germany

Input: 100-240V~/ 50-60Hz/ 700mA

Output: 12V~/ 2.5A

CAUTION:



RISK OF ELECTRICAL SHOCK
DRY LOCATION USE ONLY

Keeler

220-240V



Q02748



IP40

T40/F

FWGB

100V



TUV Rheinland
Keeler YNA



120V

Class 2

C



US

E143128

For I.T. and Medical Equipment

4 листа

