

ООО «Терумо Рус»



Бизнес-Центр «Северная Башня»
123317, Москва, Россия,
ул.Тестовская, д.10, 2-ой под., 13-й этаж,
Tel.: +7 495 988 4740
Fax: +7 495 988 4739


www.terumo-europe.com

ПОДТВЕРЖДАЮ
Генеральный директор
ООО «Терумо Рус»
Уэно Минору




**Фотографические изображения медицинского изделия:
Комплект Spectra Optia для тромбоцитов и плазмы**

2017

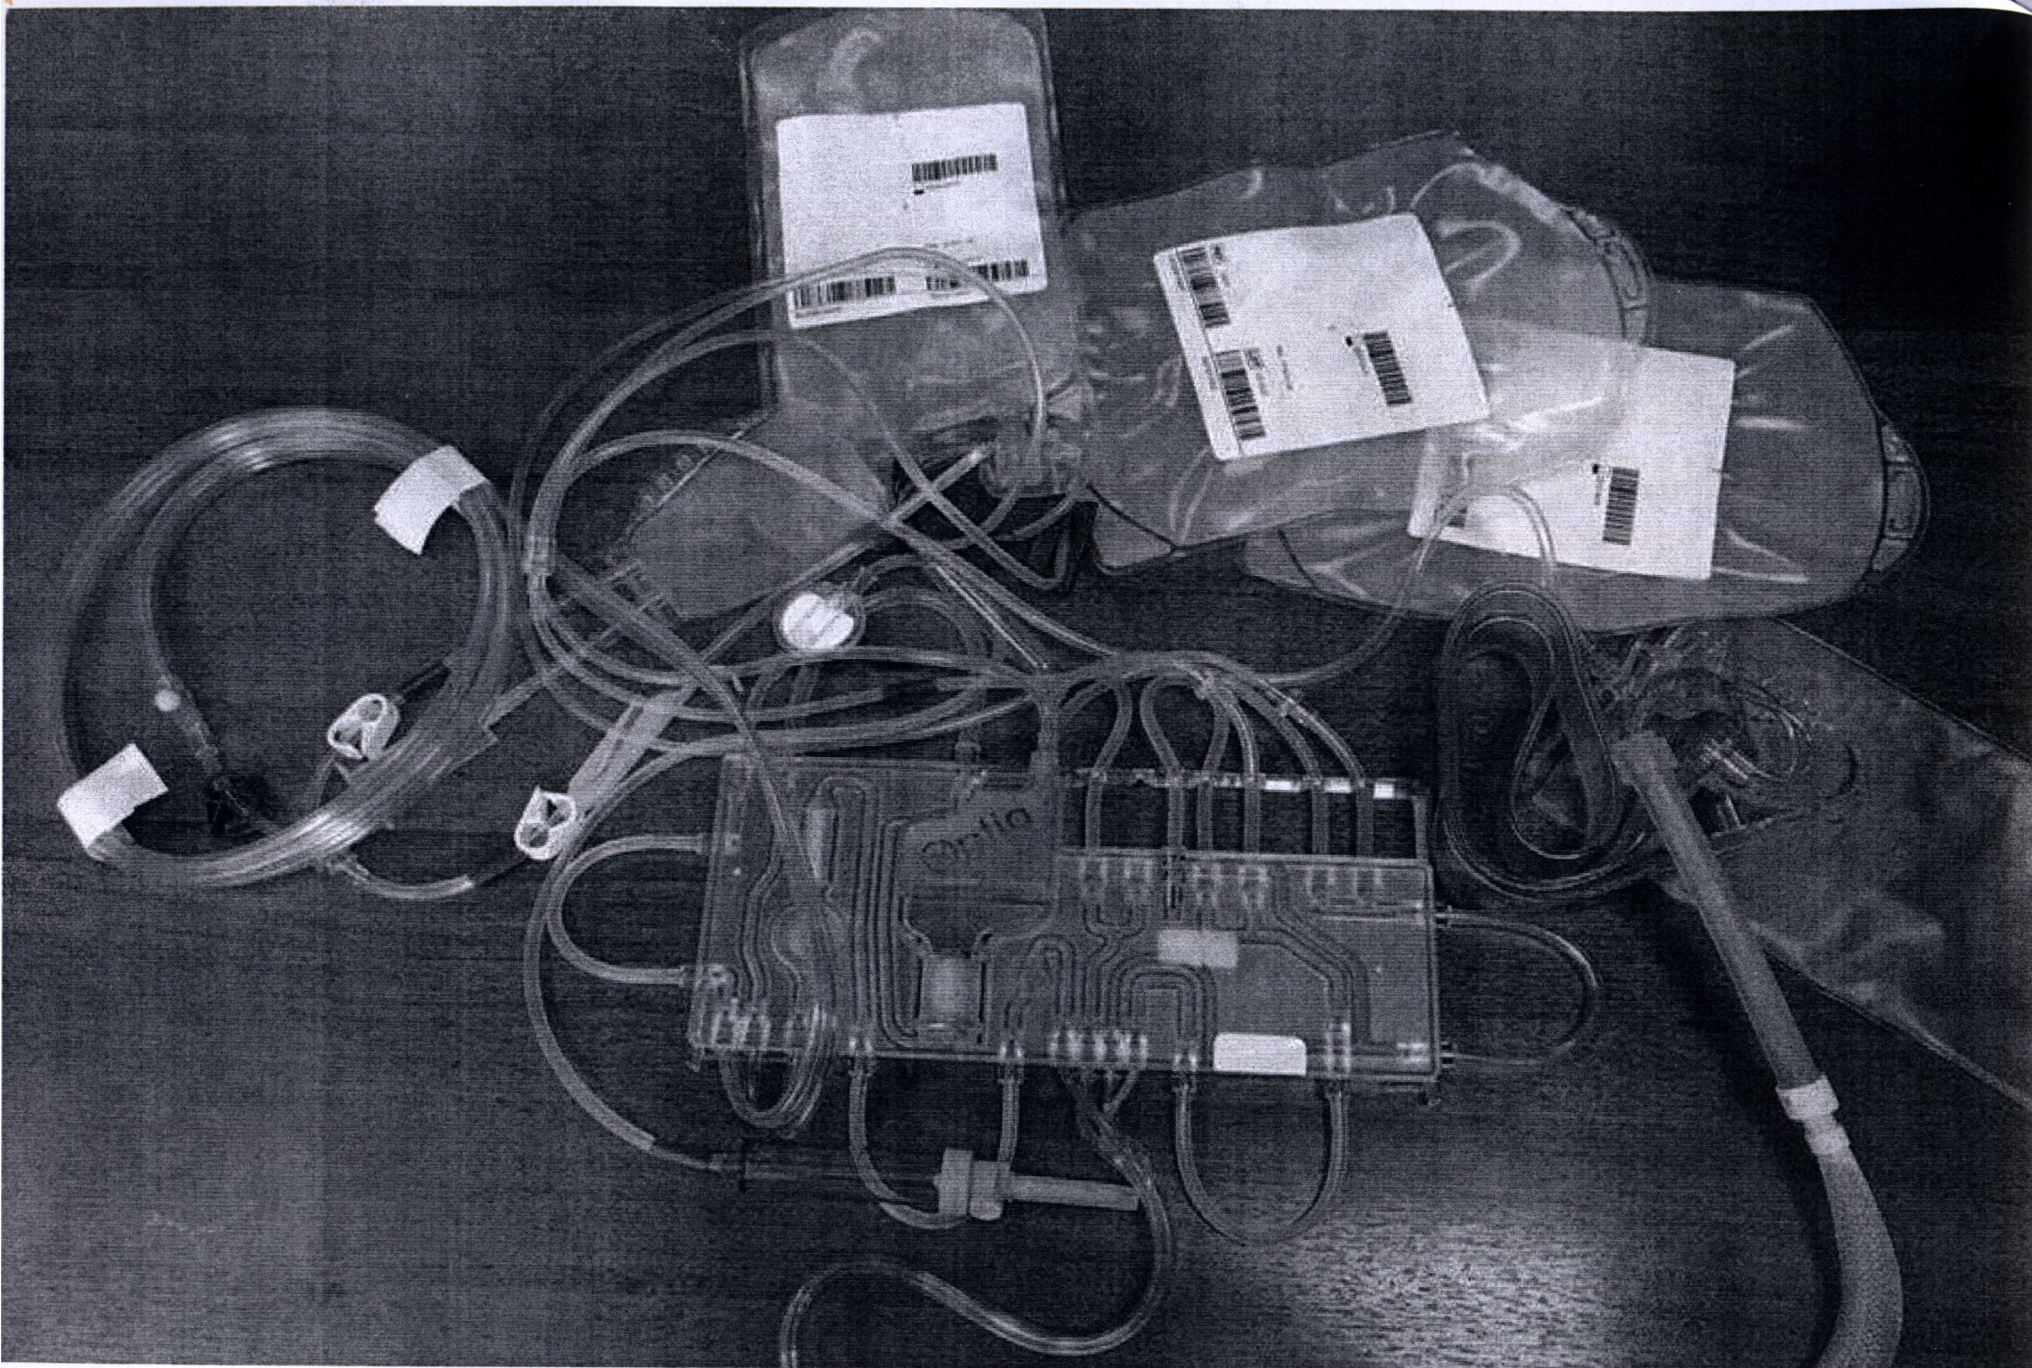

Комплект Spectra Optia для тромбоцитов и плазмы – общий вид

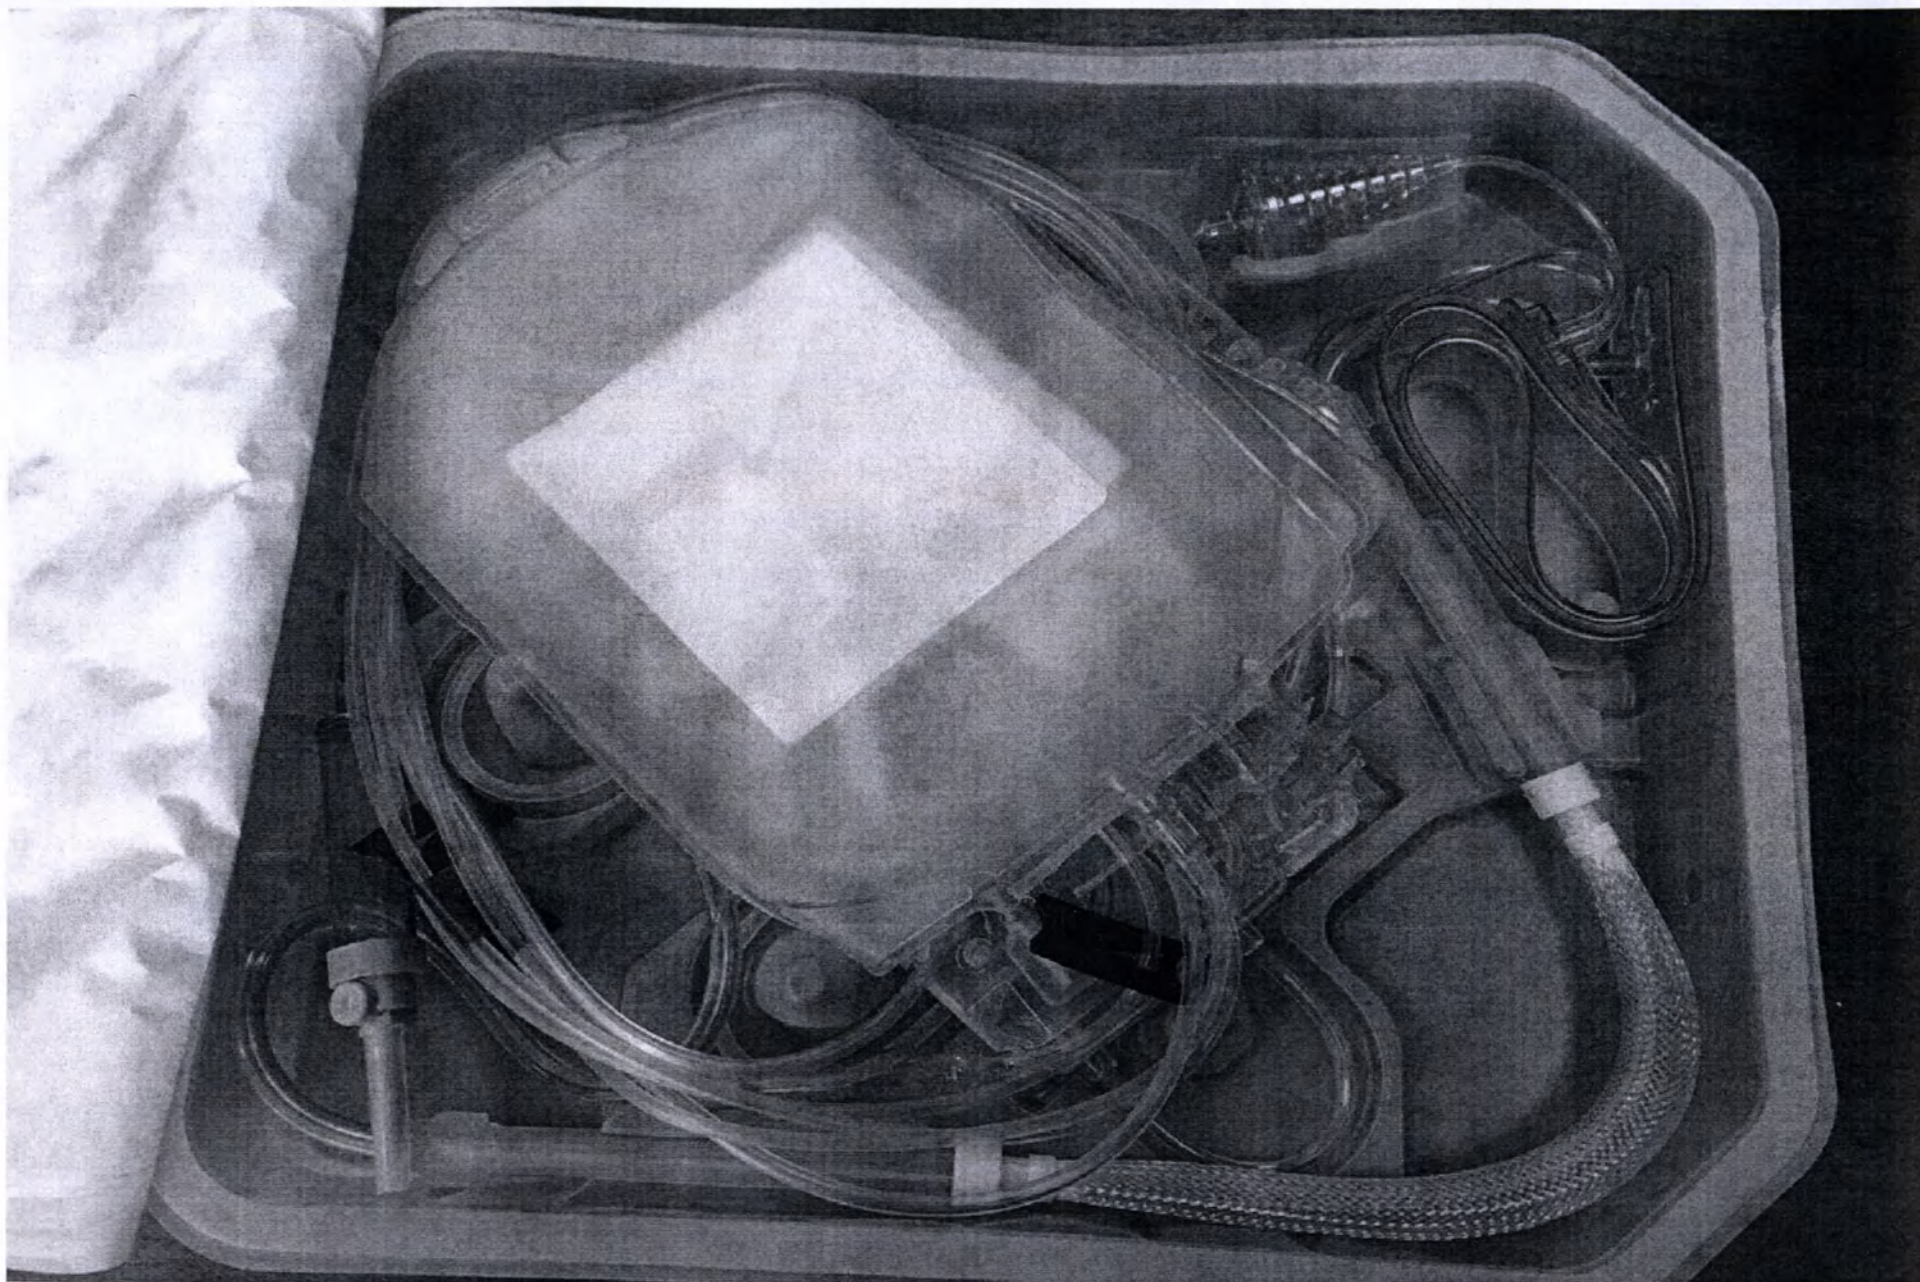

Комплект Spectra Optia для тромбоцитов и плазмы в лотке со вскрытой крышкой

Spectra Optia®
APHERESIS SYSTEM

Starch and non-synthetic food particles. Do not use the sac if the end caps are not in place. Read instructions for use before application. Sterilized with ethylene oxide. Intended for single use only. Do not reinsert.

MANUFACTURE DATE MM 2016-09-18

CATALOG NO. **REF** 10400

LOT NO. 09Y3118









TERUMOBCT

Copyright © 1994 by Creative Arts
Lanham, MD 20640
Made in USA

011580220563104006
0115710061101013322

© 2000 Blackwell Science Ltd *Journal of Internal Medicine* 247: 391–397

also is provided by the electronic database and is available to all members of the participating agencies.

[illegible]

0633 442182, 07471 967166, 074845 509099, 07484 57464, 07483 317.50 7042,
07483 159 709275, 07483 709194, 07483 3016, 07483 305014, 07483 32,
07483 531658, 07483 717008, 07483 3399, 07483 4073, 07483 334934, 07483
07483 74, 07483 67155, 07483 874449, 07483 71, 07483 331554, 07483
07483 710000, 07483 701443, 07483 710000, 07483 710000, 07483 35-0000, 710011,
07483 710000, 07483 710000, 07483 710000, 07483 710000, 07483 710000, 07483 710000


Journal of Interpersonal Violence 26(10)

[illegible][illegible][illegible]

Copyright © 2004 John Wiley & Sons, Ltd.
J. Polym. Sci. Part A: Polym. Chem. 42: 1035–1044 (2004)

Комплект Spectra Optia для тромбоцитов и плазмы – Индивидуальная стерильная упаковка

Spectra Optia® Platelet, Plasma Set
 Kit de collecte Plaquettes + Plasma Spectra Optia®
 Circuito per piastrine e plasma Spectra Optia®
 Spectra Optia® Thrombozyten-, Plasma-Set
 Equipo Spectra Optia® para plaquetas y plasma
 Conjunto de plasma e plaquetas Spectra Optia®
 Set Spectra Optia® pro trombocyty a plazmu
 Spectra Optia® trombocyt, plasmasæt
 Spectra Optia® -trombosyytti, plasmasetti
 Σει Spectra Optia® αιμοπεταλίων, πλάσματος
 Spectra Optia® blodplate- og plasmasæt
 Zestaw do pobierania płytek krwi i osocza do systemu Spectra Optia®
 Комплект Spectra Optia® для тромбоцитов и плазмы
 Spectra Optia® Trombocyt- och plasmasæt
 Spectra Optia® Trombosit, Plazma Seti





Sterile and non-pyrogenic fluid pathway. Do not use the set if the end caps are not in place. Read instructions for use before application. Sterilized with ethylene oxide. Intended for single use only. Do not resterilize.

EXPIRY DATE  2017-09-01

MANUFACTURE DATE  2015-09-18

CATALOG NO. **REF** 10400

LOT NO. 09Y3118




CE 0086



TERUMO BCT

10811 W. Collins Ave.
 Lakewood, CO 80215
 MADE IN USA



TPN - 777815-167

Комплект Spectra Optia для тромбоцитов и плазмы – Маркировка индивидуальной стерильной упаковки



Всего пронумеровано,
прошнуровано и
скреплено печатью
5 листа (ов)

29793