

ЗАО «СЭЙДЖ»

Россия, 121069, Москва,
ул. Малая Никитская, д. 20/9, стр.2



ЗАО «SAGE»

Malaya Nikitskaya, 20/9, bld. 2
Moscow, 121069, Russia

Tel.: +7(095) 234 3945/46, 795 0360/61 Fax: 234 3947

Internet: <http://www.sagemed.ru>, E-mail: info@sagemed.ru

Исх № _____

ПОДТВЕРЖДАЮ

Генеральный директор
ЗАО "СЭЙДЖ"
Озтемел Грегори



» декабря 2015 г.


Фотографические изображения

Медицинское изделие:

Стент RocaJJ мочеточниковый в наборах
в различных исполнениях

Производитель:

"ROCAMED FRANCE"

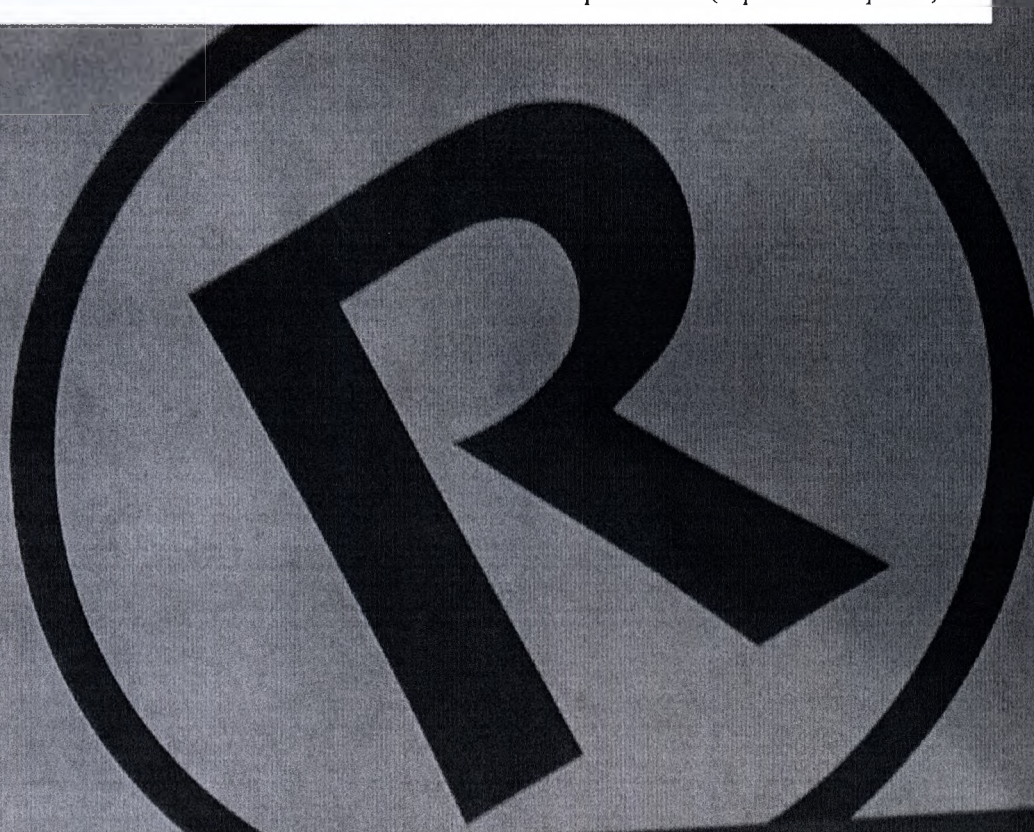

ROCAMED www.rocamed-surgical.com **REF** ROJP0624ST
Casting Number

RocaJJ Silicone - STANDARD KIT, Unilateral JJ Stent

6FR 24cm

Unilateral RocaJJ Wire 0.035"

Connectable - 43cm

x1 Quantity Per Box

STERILE EO This device is not made with natural rubber latex

LOT E010203

Use By 2017-01

CE ROCAMED Filippine - 21 de Siguan - Aldea de Stockholmen - 83879 SIGNES FRANCE

5065 Manufacture

Distributed and Distributed by ROCAMED S.A.R.L. - 9 Avenue Albert 1^{er} - 93000 NOGENT - FR +337 57 88 42 43

REF ROJP0624ST Casting Number LOT E010203 Batch Code Use By 2017-01	REF ROJP0624ST Casting Number LOT E010203 Batch Code Use By 2017-01
--	--

1. Стент RocaJJ мочеточниковый силиконовый в наборе Standart (маркировка коробки)

ROCAMED www.rocamed-urology.com

RocaJJ Silicone - STANDARD KIT: Ureteral JJ Stent

REF ROJP06248T
Catalog Number

6FR
24cm

Nitinol RocaWire 0.038"

Connectable - 40cm



(01)03700612072039(17)170100(10)E010203

STERILE **EO**
Sterilized Using Ethylene Oxide

 Consult Instructions For Use

 This device is not made with natural rubber latex

 Do Not Reuse

LOT E010203
Batch Code


 2017-01
Use By

CE  ROCAMED France - ZI de Signes - Allée de Blockholm - 83870 SIGNES FRANCE
0459 Manufacturer

Distribué par / Distributed by ROCAMED S.A.S. - 9 avenue Albert II - 83000 MONACO - tel (377) 87 00 82 43

REF ROJP06248T Catalog Number LOT E010203 Batch Code Use By  2017-01	REF ROJP06248T Catalog Number LOT E010203 Batch Code Use By  2017-01
REF ROJP06248T Catalog Number LOT E010203 Batch Code Use By  2017-01	REF ROJP06248T Catalog Number LOT E010203 Batch Code Use By  2017-01

1. Стент RocaJJ мочеточниковый силиконовый в наборе Standart (стерильный пакет с изделием) Фото 1.

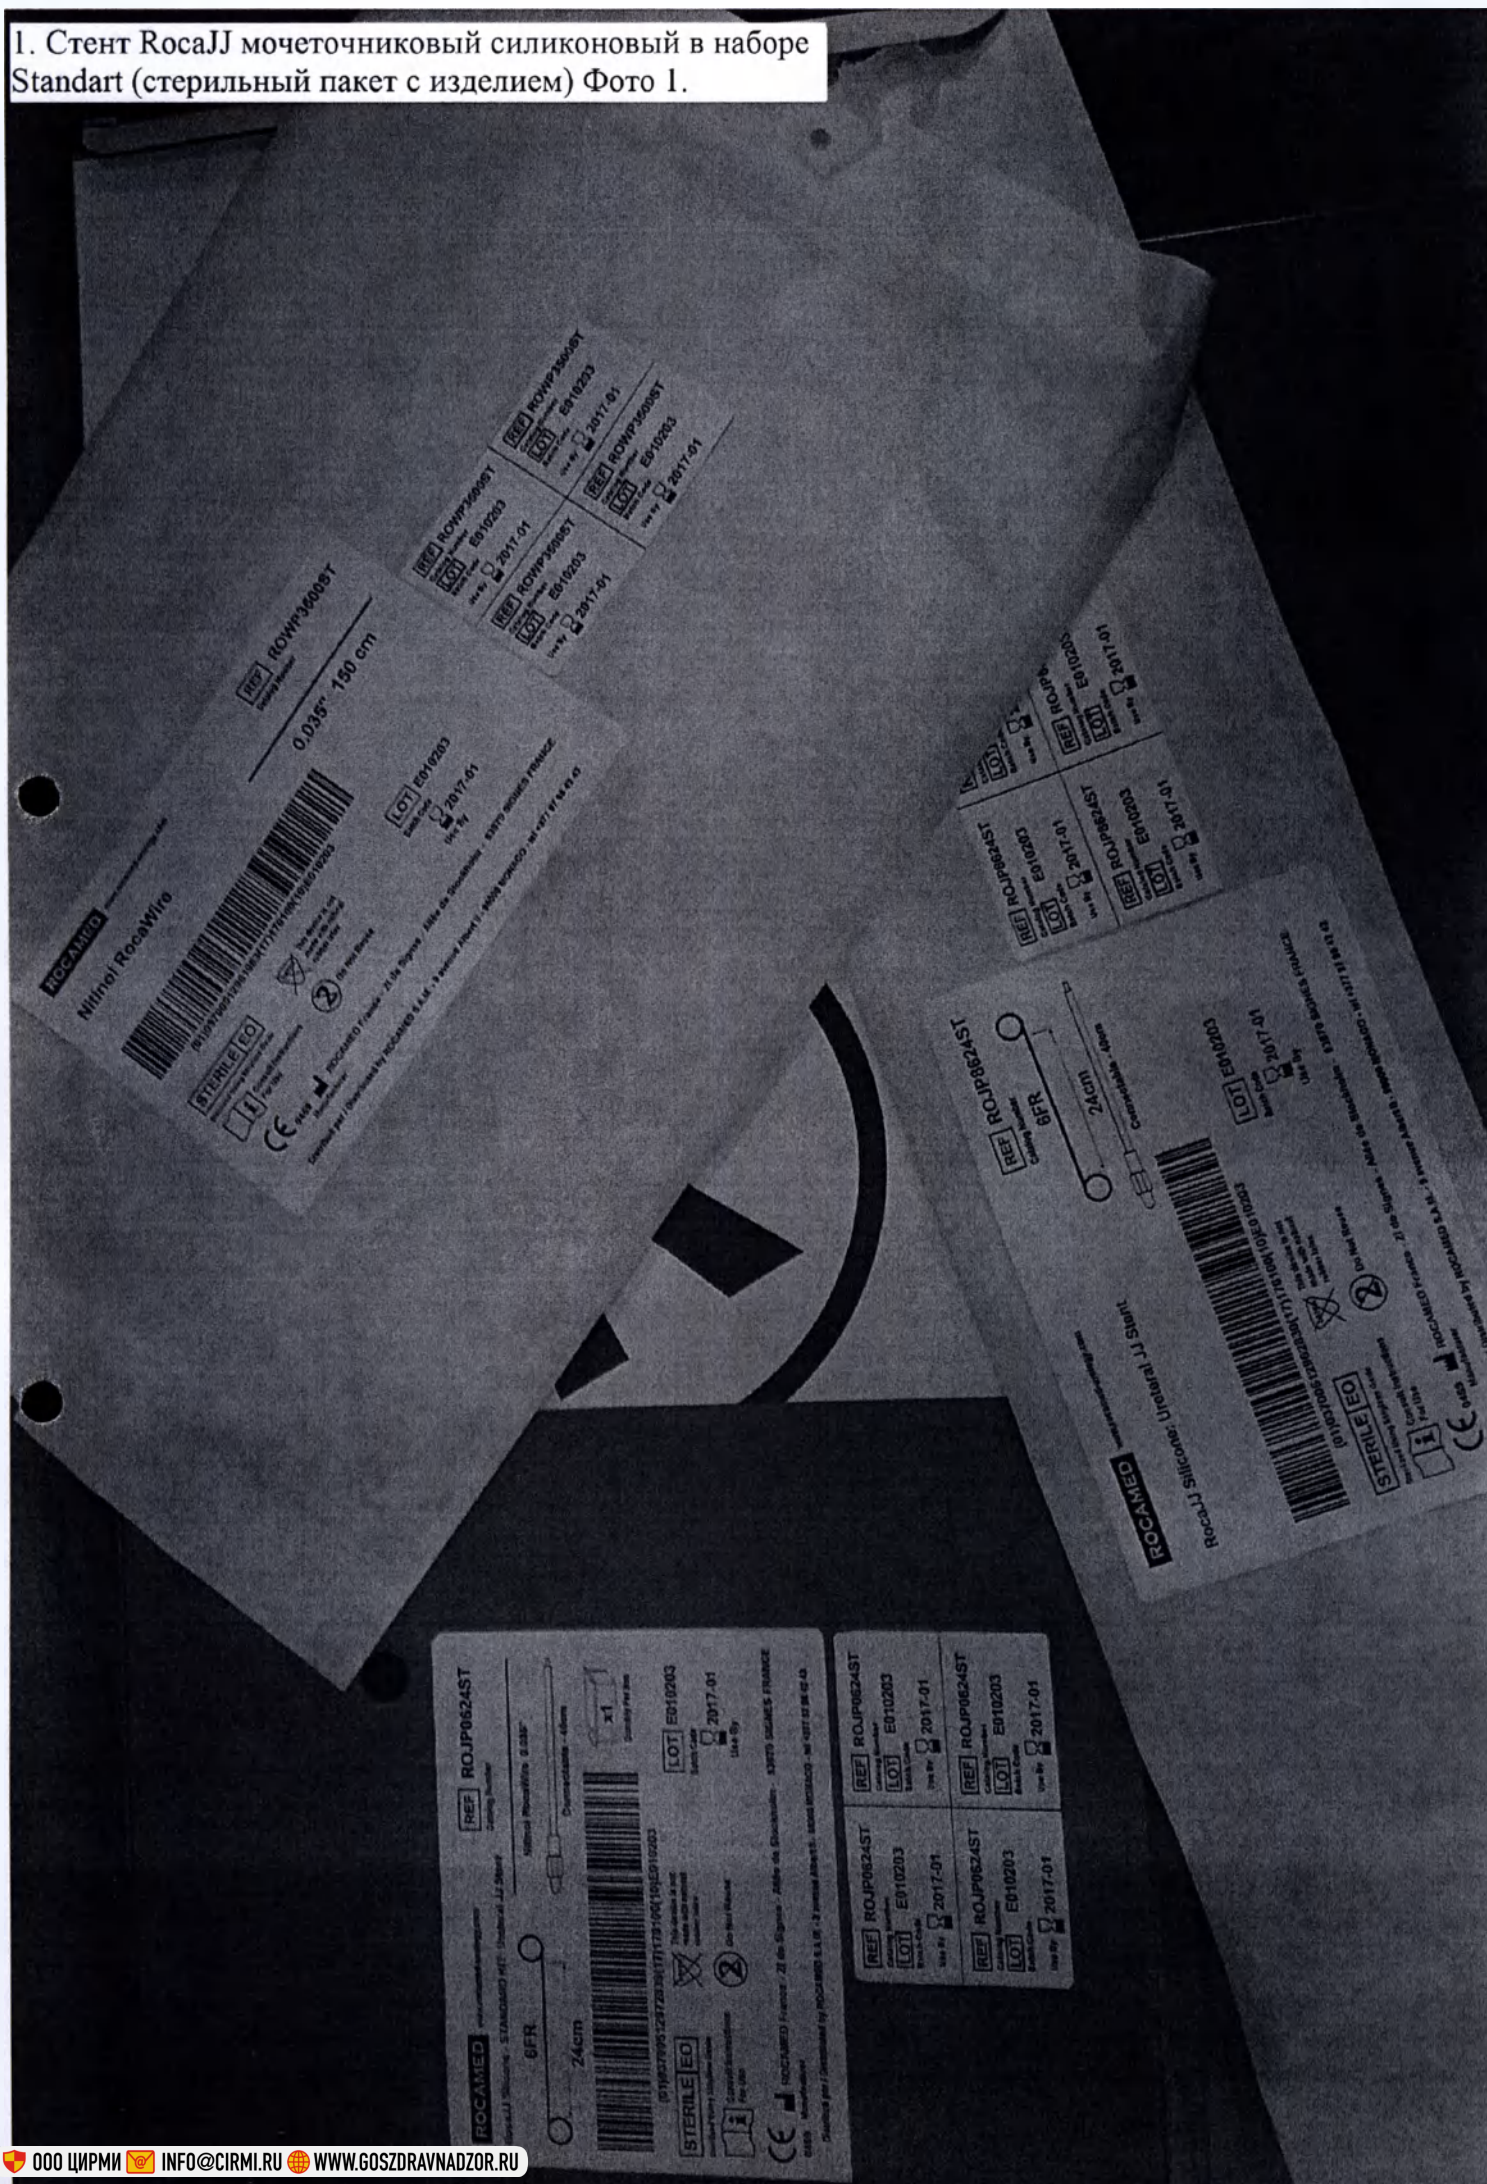

1. Стент RocaJJ мочеточниковый силиконовый в наборе Standart (стерильный пакет с изделием) Фото 2.

Толкатель подсоединяемый

JJ-стент силиконовый

Проводник RocaWire стандартный
нитиноловый с гидрофильным покрытием



Use By 2017-09

2. Стент RocaJJ мочеточниковый силиконовый в наборе STIFF
(маркировка картонной коробки)

ROCAMED

www.rocamed-urology.com

REF ROJP9630ST

Catalog Number


RocaJJ Silicone - STIFF KIT: Ureteral JJ Stent

6FR



30cm


RocaWire Nitinol 0.035"



Connectable - 40cm



(01)03700512974017(17)170900(10)R140954



Quantity Per Box

STERILE EO

Sterilized Using Ethylene Oxide



This device is not
made with natural
rubber latex

LOT R140954

Batch Code



Consult Instructions
For Use



Do Not Reuse



2017-09

Use By



0459



ROCAMED France - ZI de Signes - Allée de Stockholm - 83870 SIGNES FRANCE
Manufacturer

Distribué par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

REF ROJP9630ST

Catalog Number

LOT R140954

Batch Code

Use By 2017-09

REF ROJP9630ST

Catalog Number

LOT R140954

Batch Code

Use By 2017-09

REF ROJP9630ST

Catalog Number

LOT R140954

Batch Code

Use By 2017-09

REF ROJP9630ST


Catalog Number

LOT R140954


Batch Code

Use By 2017-09

2. Стент RocaJJ мочеточниковый силиконовый в наборе STIFF (стерильный пакет с изделием) Фото 1.

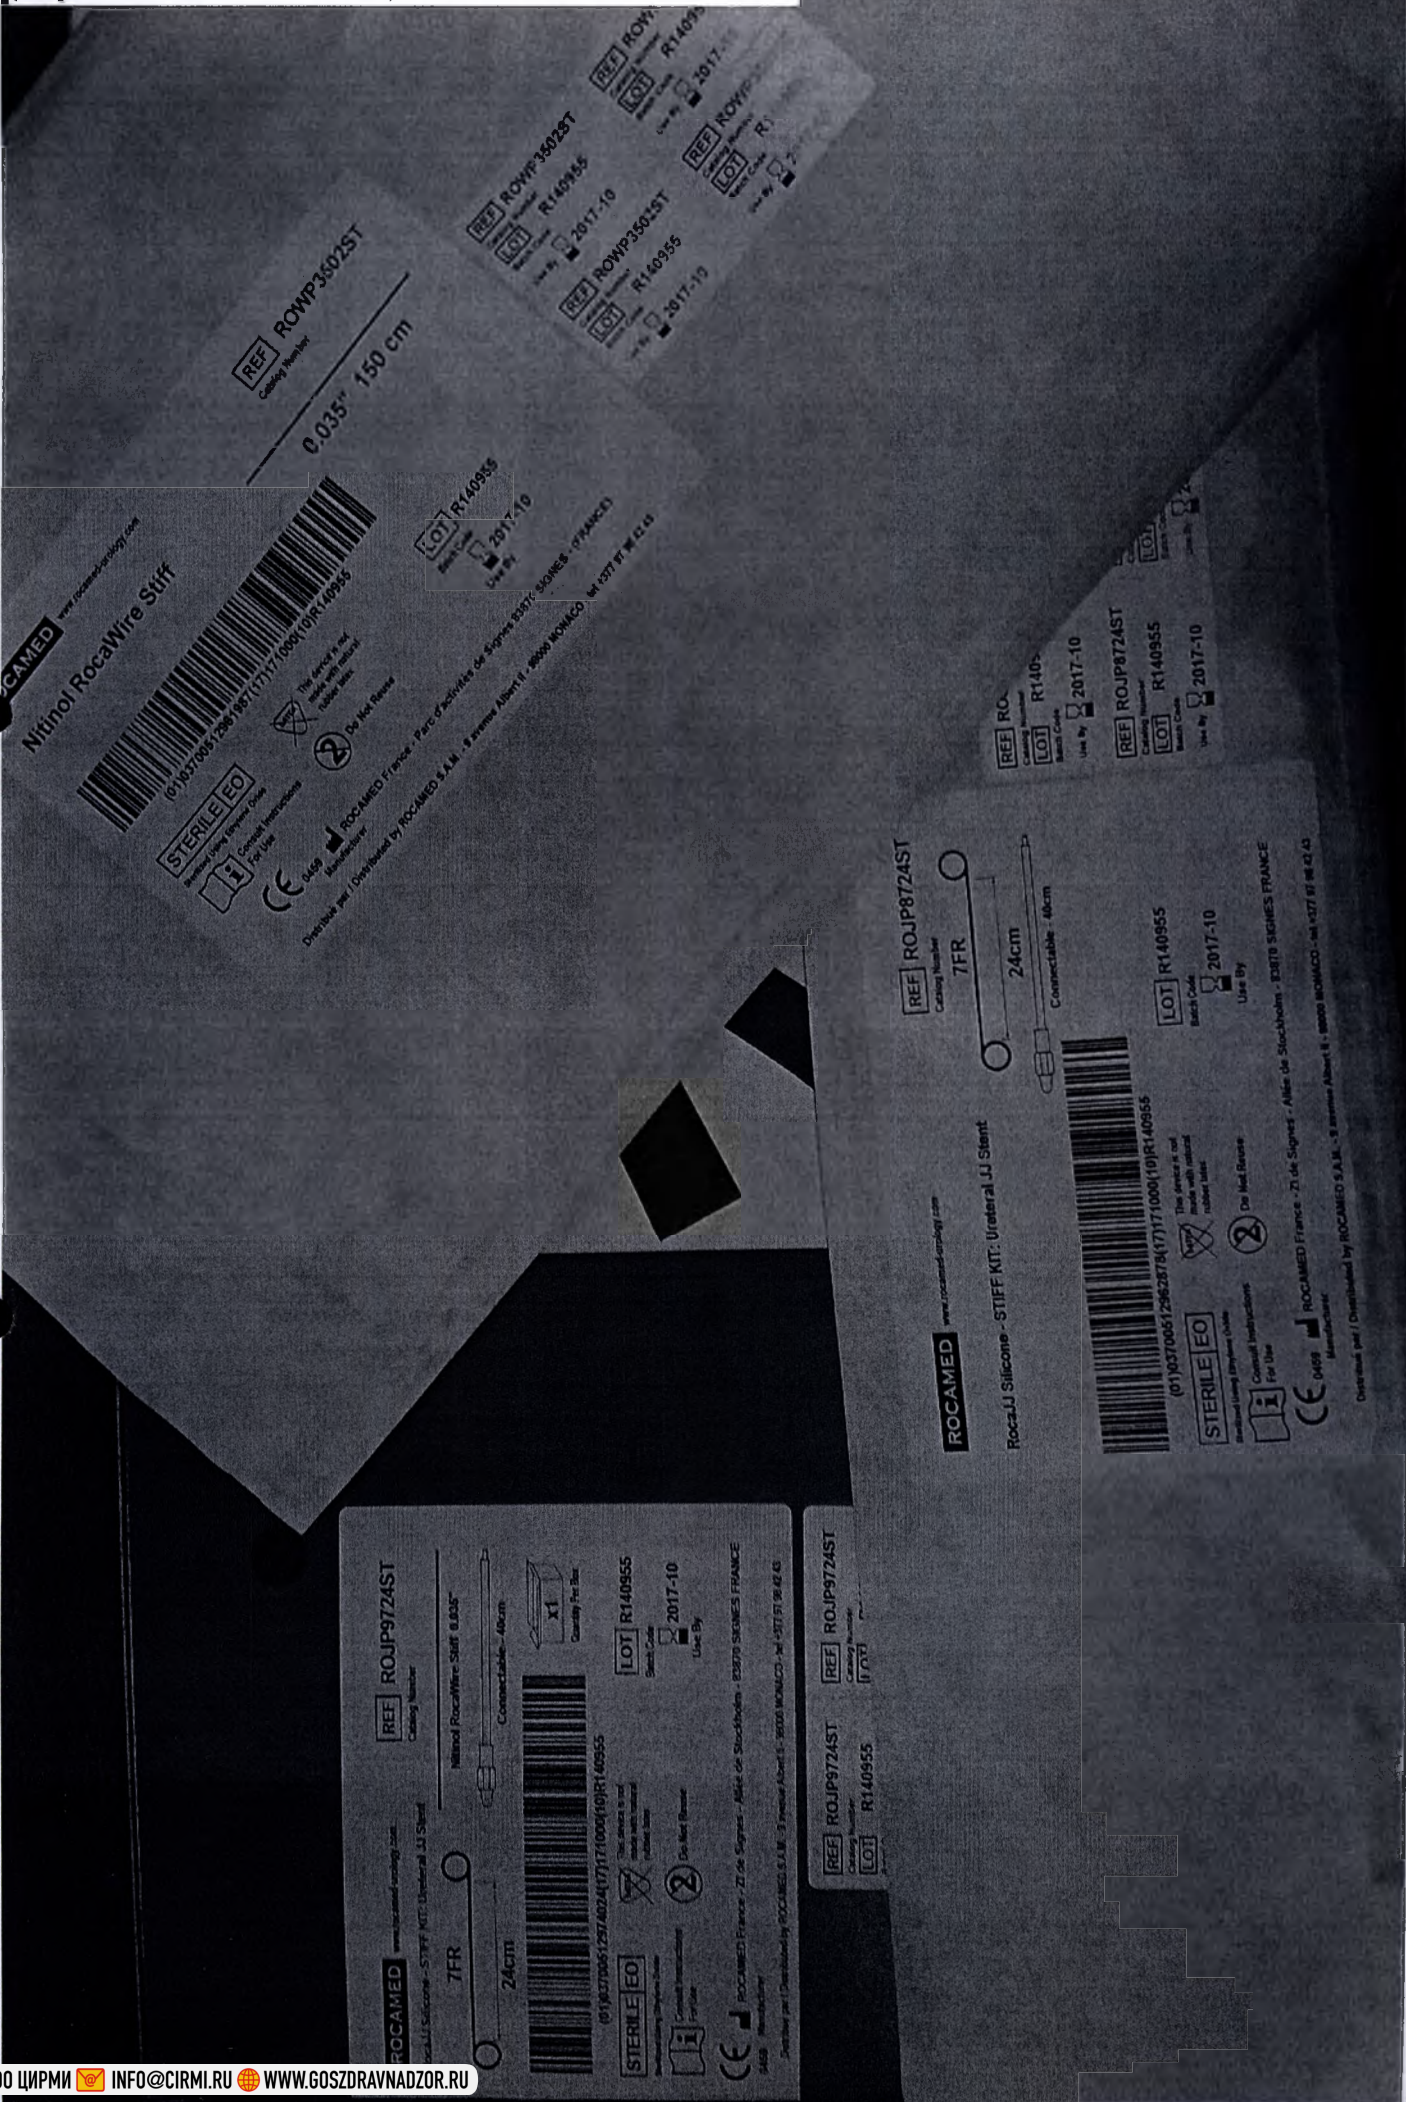

2. Стент RocaJJ мочеточниковый силиконовый в наборе STIFF (стерильный пакет с изделием) Фото 2.

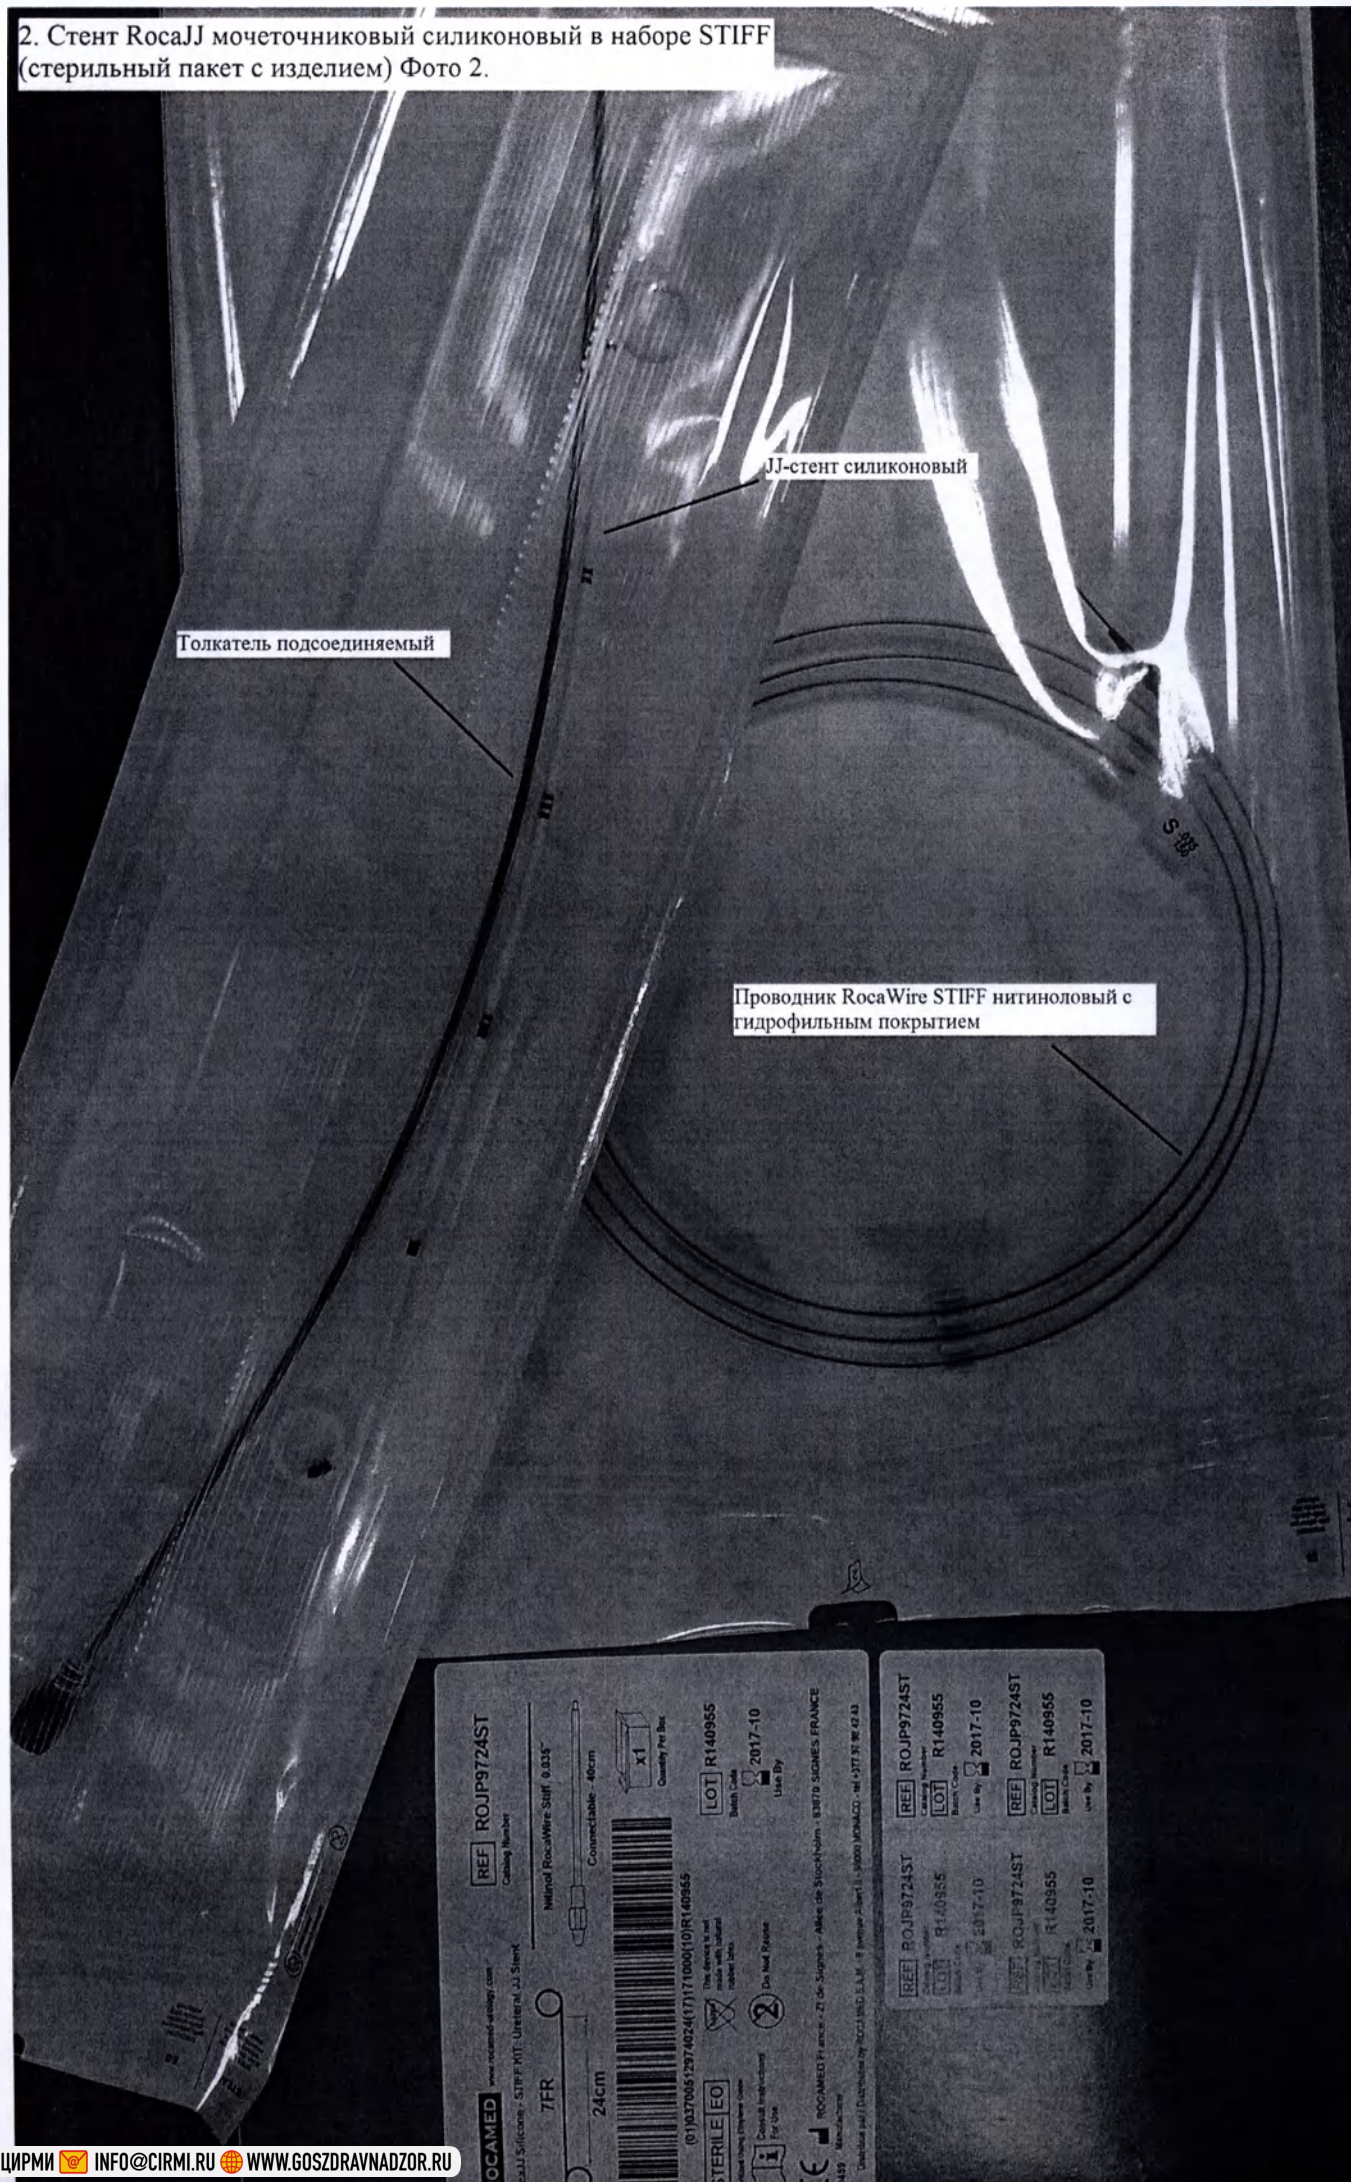

Голкатель подсоединяемый

JJ-стент силиконовый

Проводник RocaWire STIFF нитиноловый с гидрофильным покрытием

ROCAMED www.rocamed-surgery.com RocaJJ Silicone - STIFF KIT - Ureteral JJ Stent		REF ROJP9724ST Catalog Number	
Nitinol RocaWire Stiff 0.035" Connectable 40cm x1 Quantity Per Box		LOT R140955 Batch Code Use By 2017-10	
7FR 24cm (01037065)2374024(17)17100010(R)140955 STERILE EO Sterilized using Ethylene Oxide Do not use if tamper seal is broken Do not use if tamper seal is broken		REF ROJP9724ST LOT R140955 Batch Code Use By 2017-10	
ROCAMED France - ZI de Sogues - Allée de Stockholm - 83870 SORGES FRANCE 0439 - Manufacture Distributed by: Dispositifs by ROC MED S.A.S. - 8 Avenue Albert 1 ^{er} - 93000 NOGENT - FR (377 91 82 42)		REF ROJP9724ST LOT R140955 Batch Code Use By 2017-10	

3. Стент RocaJJ мочеточниковый полиуретановый в наборе STIFF
(картонная коробка)




REF ROJG9630ST

Catalog Number

Nitinol RocaWire Stiff 0.035"

Connectable - 40cm



x1

Quantity Per Box

LOT R150437

Batch Code

2018-04

Use By

This device is not
made with natural
rubber latex

Do Not Reuse

STERILE EO
Consult Instructions
For Use

Read Using Eyeglass Reader

0459 ROCAMED France - Zi des Signes - Aïsse de Stockholm - 93870 SIGNES FRANCE

Distribue par / Distributed by ROCAMED S.A.M. - 9 Avenue Albert N. - 92000 MONACO - tel +3377 97 98 42 43

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

2018-04

Use By

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

2018-04

Use By

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

2018-04

Use By

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

2018-04

Use By

3. Стент RocaJJ мочеточниковый полиуретановый в наборе STIFF (маркировка картонной коробки)

ROCAMED

www.rocamed-urology.com

REF ROJG9630ST

Catalog Number

**RocaJJ Soft - STIFF KIT :
Ureteral JJ Stent**

Tuteur Urétéral • Tutor uretral

Stent urétéral • Ureterstent

Stent ureteral • Мочеточниковый стент

Nitinol RocaWire Stiff 0.035"


Connectable - 40cm

6FR

30cm



(01)03700512973706(17)180400(10)R150437



Quantity Per Box

STERILE EO

Sterilized Using Ethylene Oxide



Consult Instructions
For Use



This device is not
made with natural
rubber latex



Do Not Reuse

LOT R150437

Batch Code



2018-04

Use By



0459

Manufacturer



ROCAMED France - ZI de Signes - Allée de Stockholm - 83870 SIGNES FRANCE

Distribué par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

Use By 2018-04

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

Use By 2018-04

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

Use By 2018-04

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

Use By 2018-04

3. Стент RocaJJ мочеточниковый полиуретановый в наборе STIFF (стерильный пакет с изделием) Фото 2.

Проводник RocaWire STIFF нитиноловый с гидрофильным покрытием

Толкатель подсоединяемый с рентгенконтрастным кольцом

JJ-стент полиуретановый

REF ROJG9630S

Catalog Number

Nitinol RocaWire Stiff 0.035"

Connectable - 40cm

6FR

30cm



Quantity Per Box

LOT R150437

Batch Code

2018-04

Use By



10(10)R150437

This device is not made with natural rubber latex

Do Not Reuse

gries - Aliso de Stockholm - 83370 SIGNES FRANCE

2 rue de la Chapelle - 59000 MONACO - tel +377 97 96 42 43

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

2018-04

Use By

REF ROJG9630ST

Catalog Number

LOT R150437

Batch Code

2018-04

Use By

4. Стент RocaJJ мочеточниковый полиуретановый в наборе Simple (картонная коробка)



ROCAMED www.rocamed-urlogy.com

RocaJJ Soft - SIMPLE KIT: Ureteral JJ Stent

7FR

24cm

sample - 40cm

PTFE-Coated RocaWire 0.035"

(01)03700512573348(17)170500(10)R140118

STERILE EO

Standard Using Englebert Guide

Disinfect Instructions For Use

CE

000 ЦРПМИ

REF ROJS0724ST
Catalog Number

LOT R140118
Batch Code

Use By 2017-05

REF ROJS0724ST
Catalog Number

LOT R140118
Batch Code

Use By 2017-05

This device is not made with natural rubber latex

2 Dis Not Reuse

(01)03700512573348(17)170500(10)R140118

RocaJJ Soft - SIMPLE KIT: Ureteral JJ Stent

7FR

24cm

sample - 40cm

PTFE-Coated RocaWire 0.035"

(01)03700512573348(17)170500(10)R140118

STERILE EO

Standard Using Englebert Guide

Disinfect Instructions For Use

CE

000 ЦРПМИ

4. Стент RocaJJ мочеточниковый полиуретановый
в наборе Simple (маркировка картонной коробки)

ROCAMED

www.rocamed-urology.com

RocaJJ Soft - SIMPLE KIT: Ureteral JJ Stent

REF

ROJS0724ST

Catalog Number

7FR

PTFE-Coated RocaWire 0.035"

24cm

simple - 40cm



(01)03700512973348(17)170500(10)R140118

STERILE EO

Sterilized Using Ethylene Oxide



This device is not
made with natural
rubber latex

LOT

R140118

Batch Code



Consult Instructions
For Use



Do Not Reuse



2017-05

Use By



0459



ROCAMED France - ZI de Signes - Allée de Stockholm - 83870 SIGNES FRANCE
Manufacturer

Distribué par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

REF

ROJS0724ST

Catalog Number

LOT

R140118

Batch Code

Use By



2017-05

REF

ROJS0724ST

Catalog Number

LOT

R140118

Batch Code

Use By



2017-05

REF

ROJS0724ST

Catalog Number

LOT

R140118

Batch Code

Use By



2017-05

REF

ROJS0724ST

Catalog Number

LOT

R140118

Batch Code

Use By



2017-05

4. Стент RocaJJ мочеточниковый полиуретановый в наборе Simple (стерильный пакет с изделием) Фото 1.

ROCAMED www.rocamed.com

RocaJJ Soft: Uniflexal JJ Stent

REF ROJS724ST
Casting Number
7FR

24cm
simple 40cm

(01)03700512973348(17)170500(10)R140118

STERILE EO

Uniflexal Using Ethylene Oxide

Conform Instructions For Use

CE

LOT R140118
Batch Code
2017-05
Use By

ROCAMED France - 23 rue Sigisbert - 93700 Nogent-sur-Marne
Distribué par / Distributed by ROCAMED S.A.M. - 1 rue de la République - 93700 Nogent-sur-Marne

ROCAMED www.rocamed.com

RocaJJ Soft: Simple JJ Stent

REF ROJS724ST
Casting Number
7FR

24cm
simple 40cm

(01)03700512973348(17)170500(10)R140118

STERILE EO

Uniflexal Using Ethylene Oxide

Conform Instructions For Use

CE

LOT R140118
Batch Code
2017-05
Use By

ROCAMED France - 23 rue Sigisbert - 93700 Nogent-sur-Marne
Distribué par / Distributed by ROCAMED S.A.M. - 1 rue de la République - 93700 Nogent-sur-Marne

ROCAMED www.rocamed.com

RocaJJ Soft: Uniflexal JJ Stent

REF ROJS724ST
Casting Number
7FR

24cm
simple 40cm

(01)03700512973348(17)170500(10)R140118

STERILE EO

Uniflexal Using Ethylene Oxide

Conform Instructions For Use

CE

LOT R140118
Batch Code
2017-05
Use By

ROCAMED France - 23 rue Sigisbert - 93700 Nogent-sur-Marne
Distribué par / Distributed by ROCAMED S.A.M. - 1 rue de la République - 93700 Nogent-sur-Marne

ROCAMED www.rocamed.com

RocaJJ Soft: Uniflexal JJ Stent

REF ROJS724ST
Casting Number
7FR

24cm
simple 40cm

(01)03700512973348(17)170500(10)R140118

STERILE EO

Uniflexal Using Ethylene Oxide

Conform Instructions For Use

CE

LOT R140118
Batch Code
2017-05
Use By

ROCAMED France - 23 rue Sigisbert - 93700 Nogent-sur-Marne
Distribué par / Distributed by ROCAMED S.A.M. - 1 rue de la République - 93700 Nogent-sur-Marne

4. Стент RocaJJ мочеточниковый полиуретановый в наборе Simple (стерильный пакет с изделием) Фото 2.

Толкатель простой с рентгенконтрастным кольцом

JJ-стент полиуретановый

Проводник RocaWire
стальной с покрытием
из ПТФЭ

5. Стент RocaJJ мочеточниковый полиуретановый в наборе ЕСО (без проводника)
(картонная коробка)




ROCAMED

www.rocamed-urology.com

RocaJJ Soft - ECO KIT: Ureteral JJ Stent


6FR




30cm

REF ROJS9630ST
Catalog Number

sample - 40cm

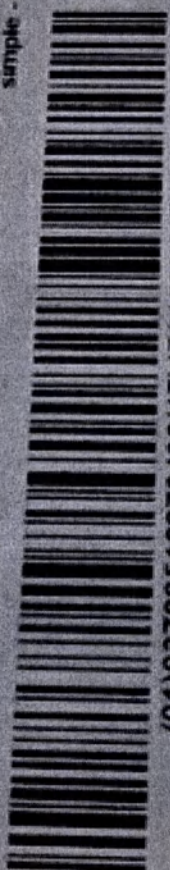


(01)03700512973492(17)170400(10)R140421




Quantity Per Box

STERILE EO


Sterilized Using Ethylene Oxide



This device is not
made with natural
rubber latex



Consult Instructions
For Use



Do Not Reuse

LOT R140421

Batch Code

2017-04

Use By



0459



ROCAMED France - Parc d'activités de Signes 83870 SIGNES - (FRANCE)

Manufacturer

Distribué par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43



ROCAMED www.rocamed-urology.com
 Soft - ECO KIT: Uniferal JJ Stent
 6FR
 20cm
 sample - 40cm
 x1
 Quantity Per Box
 LOT R140421
 Batch Code
 Use By 2017-04
 This device is not made with natural rubber latex.
 Do Not Reuse
 Consult Instructions For Use
 ROCAMED France - Parc d'activités de Signes 83870 SIGNES - (FRANCE)
 Distributeur par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43


ROCAMED www.rocamed-urology.com
 RocaJJ Soft - ECO KIT: Uniferal JJ Stent
 6FR
 30cm
 sample - 40cm
 LOT R140421
 Batch Code
 Use By 2017-04
 This device is not made with natural rubber latex.
 Do Not Reuse
 Consult Instructions For Use
 ROCAMED France - Parc d'activités de Signes 83870 SIGNES - (FRANCE)
 Distributeur par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

REF ROJS9630ST
 Catalog Number
 LOT R140421
 Batch Code
 Use By 2017-04
 REF ROJS9630ST
 Catalog Number
 LOT R140421
 Batch Code
 Use By 2017-04

REF ROJS9630ST
 Catalog Number
 LOT R140421
 Batch Code
 Use By 2017-04
 REF ROJS9630ST
 Catalog Number
 LOT R140421
 Batch Code
 Use By 2017-04

5. Стент RocaJJ мочеточниковый полиуретановый в наборе ECO (без проводника) (стерильный пакет с изделием) Фото 1.

5. Стент RosaJJ мочеточниковый полиуретановый в наборе ECO (без проводника) (стерильный пакет с изделием) Фото 2.

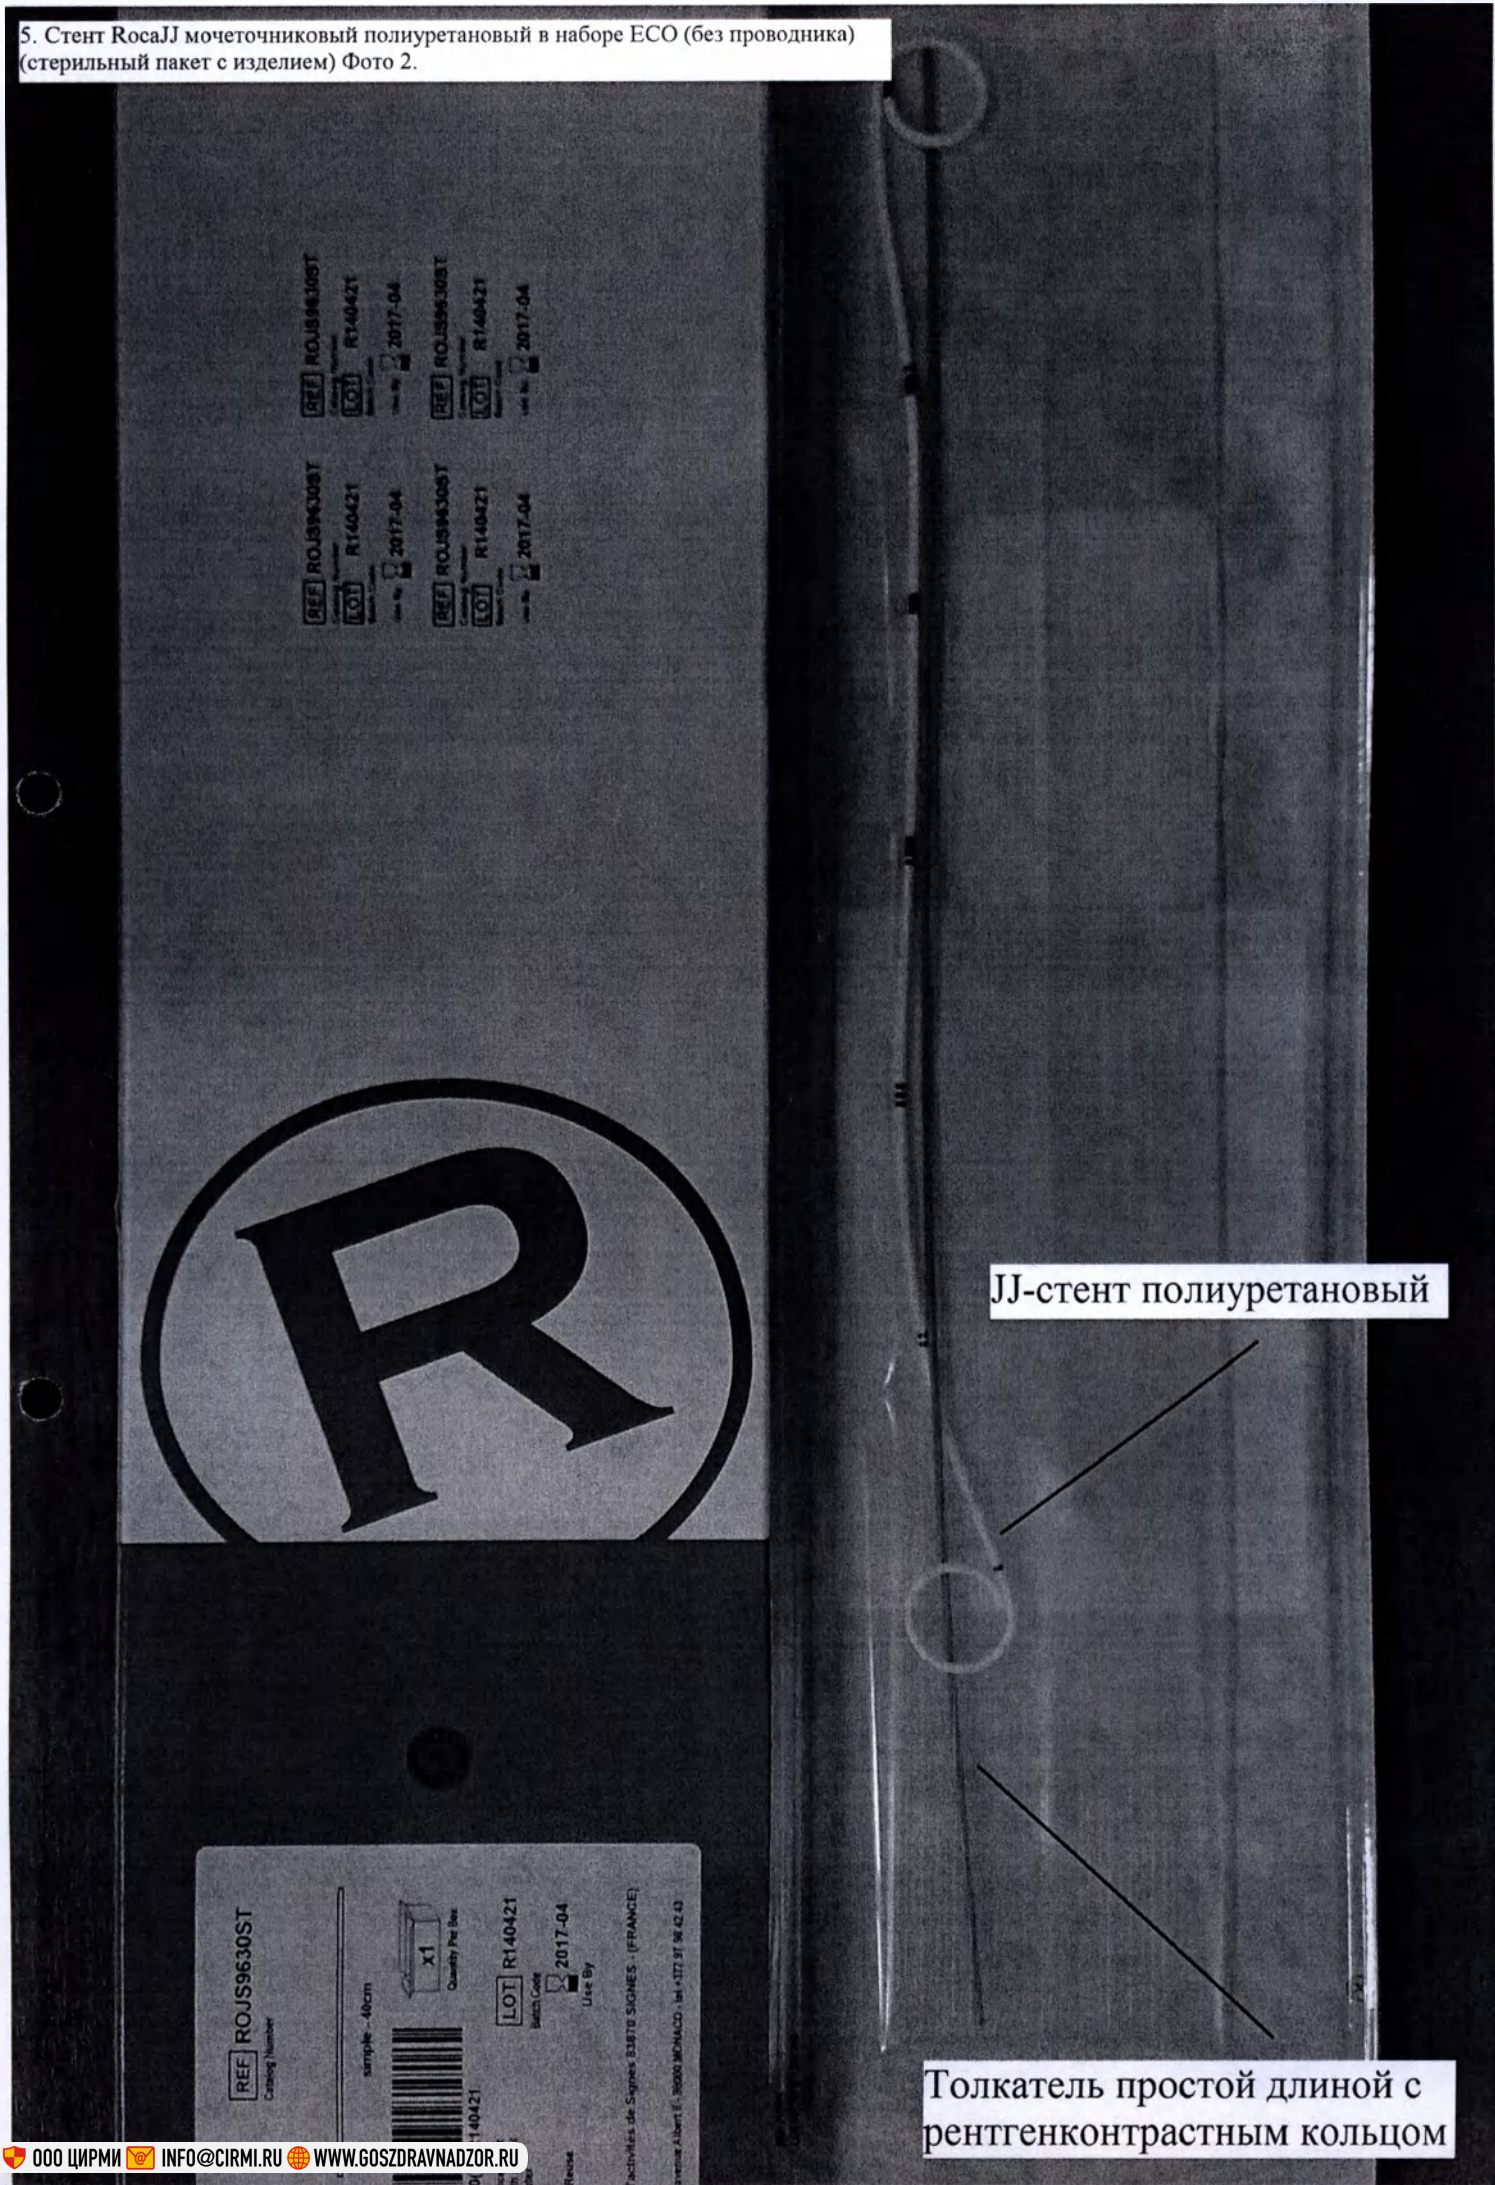

JJ-стент полиуретановый

Толкатель простой длиной с рентгенконтрастным кольцом

ROCAMED www.rocamed-urology.com

SimpleJ Stent Set

REF ROJG4790ST


Catalog Number

7FR 90cm

PTFE-Coated RocaWire 0.035"



(01)03700512973249(17)170800(10)R140802



Quantity Per Box

STERILE EO

Using Ethylene Oxide



This device is not
made with natural
rubber latex

LOT R140802

Batch Code



2017-08

Use By



Do Not Reuse

Consult Instructions
For Use

0455 ROCAMED France - Parc d'activités de Signes 83870 SIGNES - (FRANCE)

Manufacturer

Distributed by / Distributed by ROCAMED DAM - 9 Avenue Albert II - 98 000 MONACO - tel +377 97 98 42 43

REF ROJG4790ST

Catalog Number

LOT R140802

Batch Code

Use By 2017-08

REF ROJG4790ST

Catalog Number

LOT R140802

Batch Code

Use By 2017-08

REF ROJG4790ST

Catalog Number

LOT R140802

Batch Code

Use By 2017-08

REF ROJG4790ST

Catalog Number

LOT R140802

Batch Code

Use By 2017-08

6. Стент RocaJJ мочеточниковый полиуретановый простой в наборе (маркировка картонной коробки)

ROCAMED

www.rocamed-urology.com

REF


ROJG4790ST

Catalog Number

SimpleJ Stent Set

7FR 90cm

PTFE-Coated RocaWire 0.035"

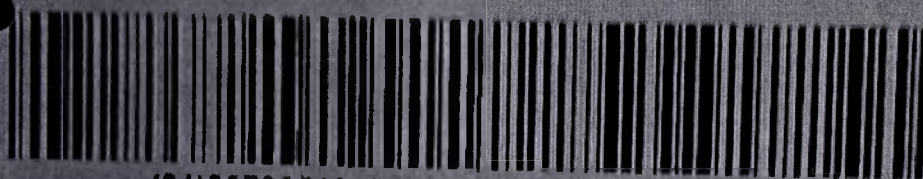

(01)03700512973249(17)170800(10)R140802

STERILE EO

Sterilized Using Ethylene Oxide



Consult Instructions
For Use



This device is not
made with natural
rubber latex



2 Do Not Reuse

LOT

R140802

Batch Code



2017-08

Use By



0459



ROCAMED France - Parc d'activités de Signes 83870 SIGNES - (FRANCE)
Manufacturer

Distribué par / Distributed by **ROCAMED SAM** - 9 Avenue Albert II - 98 000 MONACO - tel +377 97 98 42 43

REF

ROJG4790ST

Catalog Number

LOT

R140802

Batch Code

Use By



2017-08

REF

ROJG4790ST

Catalog Number

LOT

R140802

Batch Code

Use By



2017-08

REF

ROJG4790ST

Catalog Number

LOT

R140802

Batch Code

Use By



2017-08

REF

ROJG4790ST

Catalog Number

LOT

R140802

Batch Code

Use By



2017-08

6. Стент RocaJJ мочеточниковый полиуретановый простой в наборе (стерильный пакет с изделием) Фото 1.

ROCAMED www.rocamed.com

SimpleJ Stent:
Unilateral Simple J Stent

REF: ROJG8790ST
Casting Number

7FR 90cm

STERILE EO
Not Sterile to be used
made with natural
rubber latex
For Use

LOT: R140802
Batch Code
2017-08
Use By

CE 0459 ROCAMED France - Parc d'activités de Signes 53875 SIGNES
Manufacture

Distributed per / Distributeur by ROCAMED SAS - 9 Avenue Albert II - 98 500 MOU

Barcode: (07)03700512963240(17)170800(10)R140802

ROCAMED www.rocamed.com

SimpleJ Stent Set

7FR 90cm

PTFE-Coated RocaWire 0.035"

STERILE EO
Not Sterile to be used
made with natural
rubber latex
For Use

LOT: R140802
Batch Code
2017-08
Use By

CE 0459 ROCAMED France - Parc d'activités de Signes 53875 SIGNES (FR)
Manufacture

Distributed per / Distributeur by ROCAMED SAS - 9 Avenue Albert II - 98 500 MOU

Barcode: (07)03700512963240(17)170800(10)R140802

ROCAMED www.rocamed.com

SimpleJ Stent Set

7FR 90cm

PTFE-Coated RocaWire 0.035"

STERILE EO
Not Sterile to be used
made with natural
rubber latex
For Use

LOT: R140802
Batch Code
2017-08
Use By

CE 0459 ROCAMED France - Parc d'activités de Signes 53875 SIGNES (FR)
Manufacture

Distributed per / Distributeur by ROCAMED SAS - 9 Avenue Albert II - 98 500 MOU

Barcode: (07)03700512963240(17)170800(10)R140802

ROCAMED www.rocamed.com

SimpleJ Stent Set

7FR 90cm

PTFE-Coated RocaWire 0.035"

STERILE EO
Not Sterile to be used
made with natural
rubber latex
For Use

LOT: R140802
Batch Code
2017-08
Use By

CE 0459 ROCAMED France - Parc d'activités de Signes 53875 SIGNES (FR)
Manufacture

Distributed per / Distributeur by ROCAMED SAS - 9 Avenue Albert II - 98 500 MOU

Barcode: (07)03700512963240(17)170800(10)R140802

ROCAMED www.rocamed.com

SimpleJ Stent Set

7FR 90cm

PTFE-Coated RocaWire 0.035"

STERILE EO
Not Sterile to be used
made with natural
rubber latex
For Use

LOT: R140802
Batch Code
2017-08
Use By

CE 0459 ROCAMED France - Parc d'activités de Signes 53875 SIGNES (FR)
Manufacture

Distributed per / Distributeur by ROCAMED SAS - 9 Avenue Albert II - 98 500 MOU

Barcode: (07)03700512963240(17)170800(10)R140802

ROCAMED www.rocamed.com

SimpleJ Stent Set

7FR 90cm

PTFE-Coated RocaWire 0.035"

STERILE EO
Not Sterile to be used
made with natural
rubber latex
For Use


LOT: R140802
Batch Code
2017-08
Use By

CE 0459 ROCAMED France - Parc d'activités de Signes 53875 SIGNES (FR)
Manufacture

Distributed per / Distributeur by ROCAMED SAS - 9 Avenue Albert II - 98 500 MOU

Barcode: (07)03700512963240(17)170800(10)R140802

6. Стент RocaJJ мочеточниковый полиуретановый простой в наборе (стерильный пакет с изделием) Фото 2.

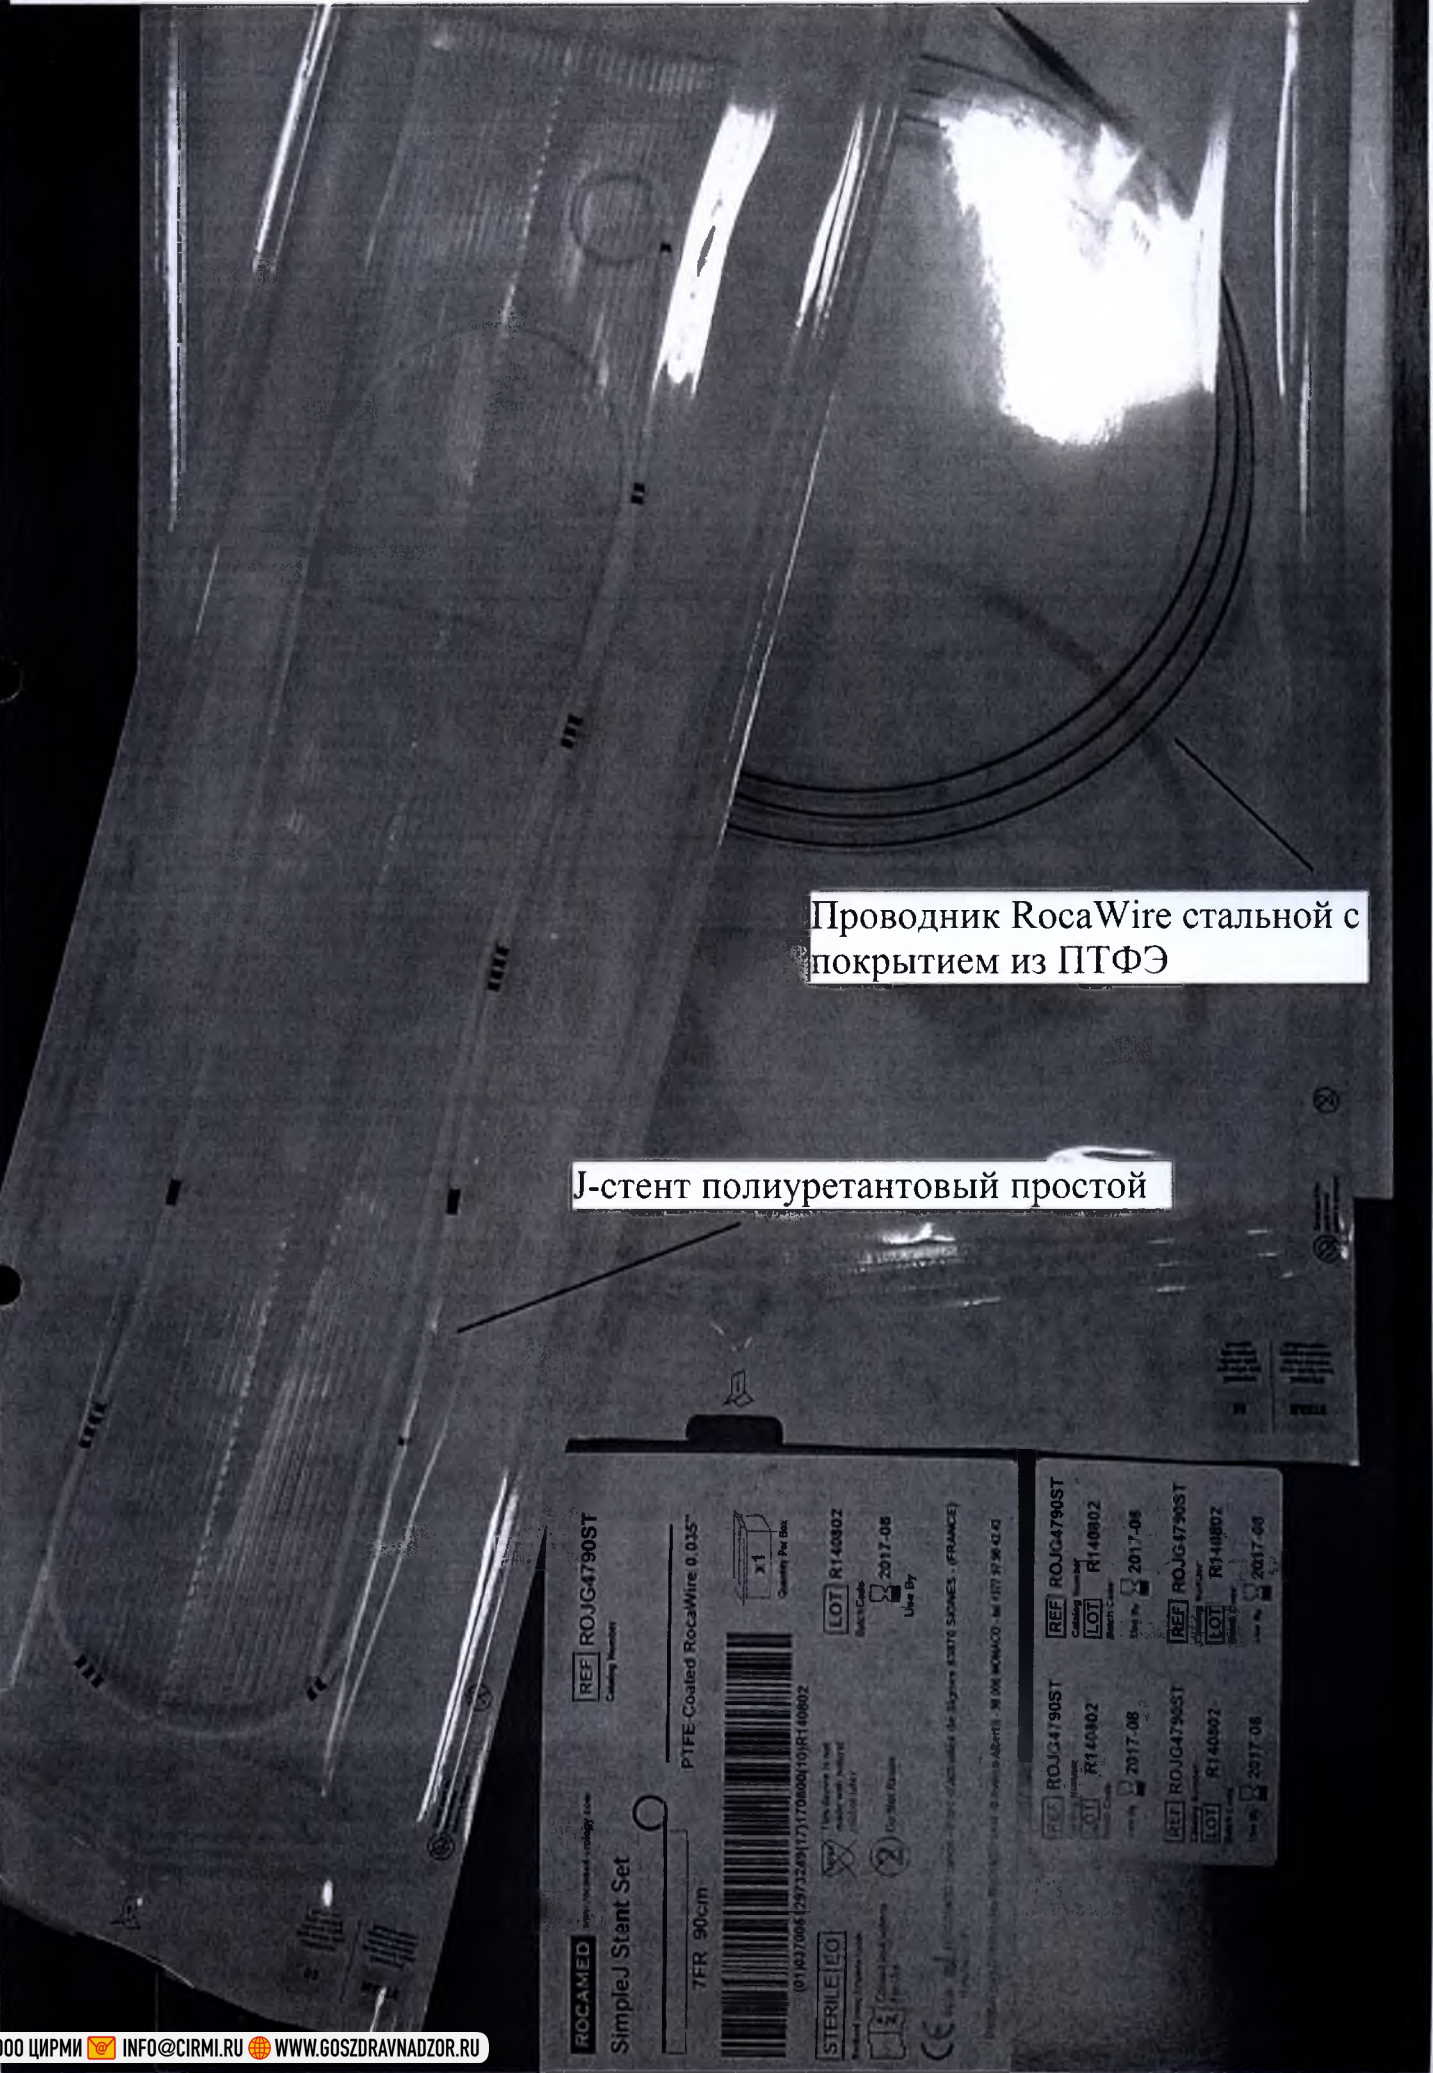

7. Стент RocaJJ полиуретановый опухолевый (для нижней трети мочеоточника) в наборе (картонная коробка)



OCAMED www.rocamed-urology.com

REF ROJG1726ST
Catalog Number

RocaWire Nitinol 0.035"

simple - 40cm

7FR

26cm

x1

Quantity Per Box

LOT R150560

Batch Code

2018/05

Use By

STERILE EO

Sterilized Using Ethylene Oxide

Consult Instructions For Use

Do Not Reuse

This device is not made with natural rubber latex

(01)03700512973126(17)180500(10)R150560

Stent tumoral avec partie renforcée - Stent tumoral con parte reforzada
Stent tumoral con parte rinforzata - Tumorstent met versterkt deel
Stent tumoral con parte reforçada - Опухолевый стент с армированной частью

0459

ROCAMED France - ZI de Signes - Allée de Stockholm - 83870 SIGNES FRANCE

Manufactured

Distribué par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

REF ROJG1726ST
Catalog Number

LOT R150560

Batch Code

Use By 2018/05

REF ROJG1726ST
Catalog Number

LOT R150560

Batch Code

Use By 2018/05

7. Стент RocaJJ полиуретановый опухолевый
(для нижней трети мочеточника) в наборе
(маркировка картонной коробки)

ROCAMED

www.rocamed-urology.com

RocaJJ Tumor Stent Set

Low part / Partie basse

Stent tumoral avec partie renforcée • Stent tumoral con parte reforzada

Stent tumorale con parte rinforzata • Tumorstent met versterkt deel

Stent tumoral com parte reforçada • Опухолевый стент с армированной частью

REF ROJG1726ST

Catalog Number

RocaWire Nitinol 0.035"

simple - 40cm

7FR

26cm



(01)03700512973126(17)180500(10)R150560

STERILE EO

Sterilized Using Ethylene Oxide



This device is not
made with natural
rubber latex



Consult Instructions
For Use



Do Not Reuse

LOT R150560

Batch Code



2018/05

Use By



0459



ROCAMED France - ZI de Signes - Allée de Stokholm - 83870 SIGNES FRANCE

Manufacturer

Distribué par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

REF ROJG1726ST

Catalog Number

LOT R150560

Batch Code

Use By



2018/05

REF ROJG1726ST

Catalog Number

LOT R150560

Batch Code

Use By



2018/05

REF ROJG1726ST

Catalog Number

LOT R150560

Batch Code

Use By



2018/05

REF ROJG1726ST

Catalog Number

LOT R150560

Batch Code

Use By



2018/05

7. Стент RocaJJ полиуретановый опухолевый (для нижней трети мочеточника) в наборе (стерильный пакет с изделием) Фото 2.

Стент опухолевый полиуретановый с усиленной нижней частью

Проводник RocaWire стандартный нитиноловый с гидрофильным покрытием

Толкатель простой

ROCAMED www.rocamed.com

Low part / partie basse

Stent tunnel with polyurethane - Stent tunnel con parte inferior
Stent tunnel con parte inferior - Stent tunnel mit unterer Teil
Stent tunnel con parte inferior - Stent tunnel mit unterer Teil

REF: ROJG1726ST
Casting Number
RocaWire Nitinol 0.033"

Length - 40cm
7FR

26cm

Quantity Per Box
LOT R150560
Batch Code
2018/05
Use By

STERILE EO

This device is not made with natural rubber latex

Do Not Reuse

Consult Instructions For Use

CE

ROCAMED France - 21 de Signes - 68100 - 3377 97 96 42 47

Distributed by ROCAMED S.A.M. - 9 avenue Albert 6 - 36000 MONTAIGU - M. 3377 97 96 42 47

REF: ROJG1726ST
Casting Number
LOT R150560
Batch Code
2018/05
Use By


REF: ROJG1726ST
Casting Number
LOT R150560
Batch Code
2018/05
Use By

8. Стент RocaJJ полиуретановый опухолевый (для средней трети мочеточника) в наборе (картонная коробка)

ROCAMED

www.rocamed-urology.com


RocaJJ Tumor Stent Set
Middle part / Partie médiane

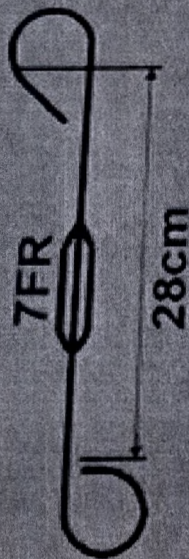

REF ROJG2728ST
Catalog Number

RocaWire Nitinol 0.035"

simple - 40cm

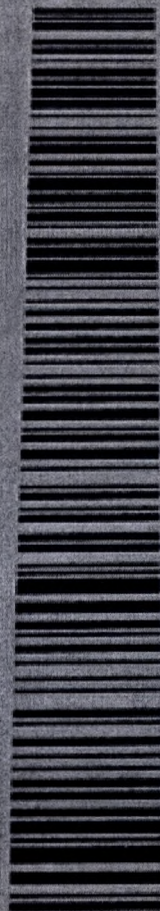

(01)03700512973171(17)171000(10)R141048

~~Latex~~ This device is not made with natural rubber latex.

LOT R141048


Batch Code

2017-10

Use By

STERILE EO

Sterilized Using Ethylene Oxide



Consult Instructions

For Use

2 Do Not Reuse

ROCAMED France - ZI de Signes - Allée de Stockholm - 83870 SIGNES - FRANCE


CE 0459



ROCAMED France - ZI de Signes - Allée de Stockholm - 83870 SIGNES - FRANCE

Manufacturer

Distribue par / Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 98 42 43



Quantity Per Box

3. Стент RocaJJ полиуретановый опухолевый (для средней трети мочеочника) в наборе (стерильный пакет с изделием) Фото 1.

sample - 40cm

28cm

1PK

Quantity Per Box

LOT R141048

Batch Code

Use By 2017-10

Do Not Reuse

Consult Instructions For Use

ROCAMED France - ZI de Sigres - Allée de Stockholm - 83870 SIONNES - FRANCE

0459 1458

Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 96 42 43

0103700512963171171000101R141048

STERILE EO

This device is not made with natural rubber latex

Do Not Reuse

Consult Instructions For Use

ROCAMED France - ZI de Sigres - Allée de Stockholm - 83870 SIONNES - FRANCE

0459 1458

Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 96 42 43

ROCAMED www.rocamed-urology.com

Nitinol RocaWire

0.035" 150 cm



(0103700512963171171000101R141048)

STERILE EO

This device is not made with natural rubber latex

Consult Instructions For Use

Do Not Reuse

CE

ROCAMED France - ZI de Sigres - Allée de Stockholm - 83870 SIONNES - FRANCE

Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 96 42 43

ROCAMED www.rocamed-urology.com

RocaJJ Tumor Stent
Middle part
Partie médiane

REF ROJG6728ST

Lot Number

7FR

28cm

sample - 40cm

(0103700512963171171000101R141048)

STERILE EO

This device is not made with natural rubber latex

Consult Instructions For Use

Do Not Reuse

CE

ROCAMED France - ZI de Sigres - Allée de Stockholm - 83870 SIONNES - FRANCE

Distributed by ROCAMED S.A.M. - 9 avenue Albert II - 98000 MONACO - tel +377 97 96 42 43

REF ROJG2728ST

REF ROJG2728ST

REF ROJG2728ST

REF ROJG2728ST

REF ROWP3500ST

REF ROWP3500ST

REF ROWP3500ST

REF ROWP3500ST


REF ROJG6728ST

REF ROJG6728ST

REF ROJG6728ST

REF ROJG6728ST


8. Стент RosaJJ полиуретановый опухолевый (для средней трети мочеточника) в наборе (стерильный пакет с изделием) Фото 2.



Проводник RosaWire стандартный нитиноловый с гидрофильным покрытием

[illegible]

9. Стент RocaJJ полиуретановый опухолевый (для верхней трети мочеточника) в наборе (картонная коробка)

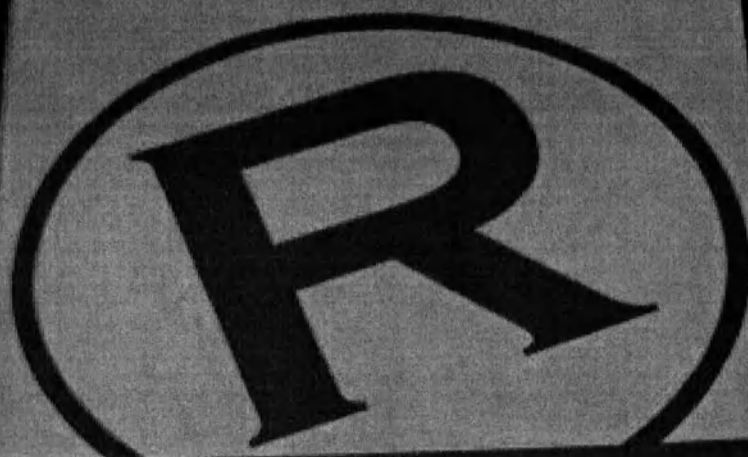

ROCAMED

www.rocamed-urology.com

RocaJJ Tumor Stent Set
Upper part / Partie haute

7FR

26cm

REF ROJG3726ST
Catalog Number

RocaWire Nitinol 0.035"

simple - 40cm

LOT R140415
Batch Code

2017-04
Use By

STERILE EO
Sterilized Using Ethylene Oxide

CE 0459
Manufacturer

(01)03700512973201(17)170400(10)R140415

~~Latex~~ This device is not made with natural rubber latex

~~2~~ Do Not Reuse

Consult Instructions For Use

CE 0459 **ROCAMED France** - ZI de Signet - Allée de Stockholm - 53870 SIGNES - FRANCE

Distribué par / Distributed by **ROCAMED S.A.M.** - 9 Avenue Albert II - 98000 MONACO - tel +377 97 98 42 43

9. Стент RocaJJ полиуретановый опухолевый (для верхней трети мочеточника) в наборе (стерильный пакет с изделием) Фото 1.



REF ROJG3726ST
Casting Number
LOT R140415
Batch Code
Use By 2017-04

REF ROJG3726ST
Casting Number
LOT R140415
Batch Code
Use By 2017-04

REF ROWP3500ST
Casting Number
LOT R140415
Batch Code
Use By 2017-04

REF ROWP3500ST
Casting Number
LOT R140415
Batch Code
Use By 2017-04


REF ROJG7726ST
Casting Number
LOT R140415
Batch Code
Use By 2017-04

REF ROJG7726ST
Casting Number
LOT R140415
Batch Code
Use By 2017-04

ROCAMED www.rocamed-urology.com

Nitinol RocaWire

0.035" 150 cm



(01)0370065 296120(17)170400(10)R140415

STERILE EO
This device is not
made with natural
rubber latex.
Do Not Remove
For Use

LOT R140415
Batch Code
Use By 2017-04



ROCAMED France - 21 rue Sigisbert - 33870 STOMES - FRANCE


Distributed by / Distribué par ROCAMED S.A.S. - 3 Avenue Albert I^{er} - 98000 MONACO - tel +377 97 96 42 42

REF ROJG3726ST

Casting Number

RocaWire Nitinol 0.035"

sample - 48cm



(01)0370065 296120(17)170400(10)R140415

LOT R140415
Batch Code
Use By 2017-04

Quantity Per Box

x1

STERILE EO

This device is not
made with natural
rubber latex.

Do Not Remove
For Use

Consult Instructions
For Use

ROCAMED France - 21 rue Sigisbert - 33870 STOMES - FRANCE

Distributed by / Distribué par ROCAMED S.A.S. - 3 Avenue Albert I^{er} - 98000 MONACO - tel +377 97 96 42 42

ROCAMED www.rocamed-urology.com

RocaJJ Tumor Stent
Upper part
Partie haute

REF ROJG7726ST

Casting Number

7FR

26cm

sample - 48cm



(01)0370065 296120(17)170400(10)R140415

STERILE EO
This device is not
made with natural
rubber latex.
Do Not Remove
For Use


LOT R140415
Batch Code
Use By 2017-04



ROCAMED France - 21 rue Sigisbert - 33870 STOMES - FRANCE

Distributed by / Distribué par ROCAMED S.A.S. - 3 Avenue Albert I^{er} - 98000 MONACO - tel +377 97 96 42 42

9. Стент RocaJJ полиуретановый опухолевый (для верхней трети мочеточника) в наборе (стерильный пакет с изделием) Фото 2.

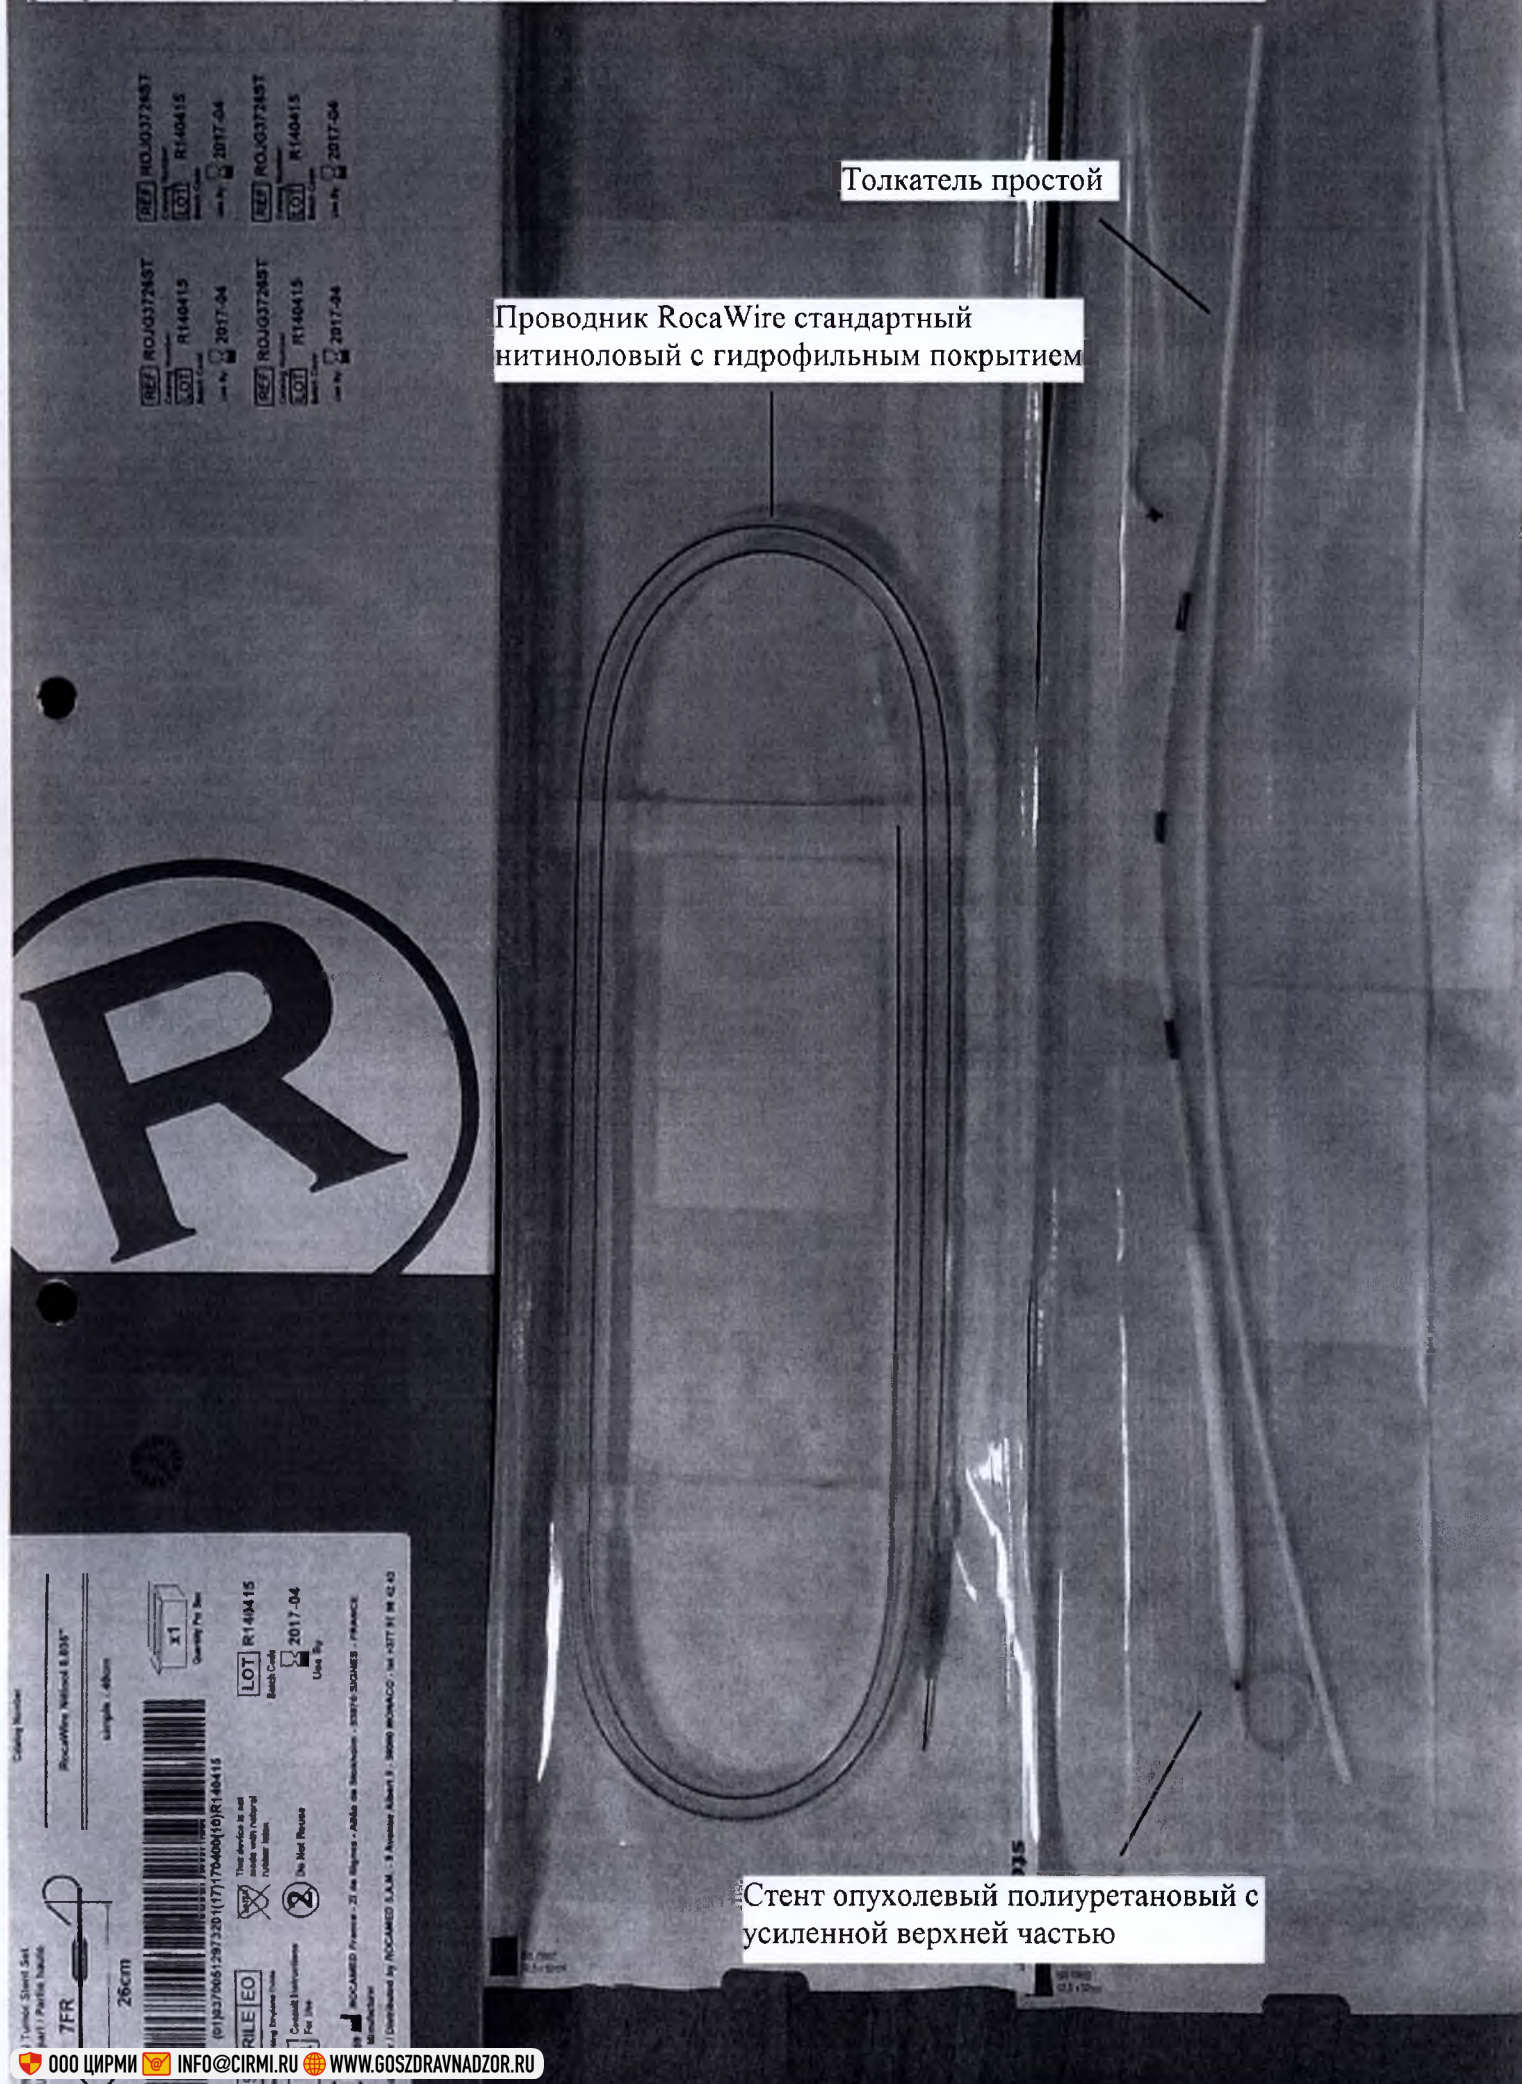

Толкатель простой

Проводник RocaWire стандартный
нитиноловый с гидрофильным покрытием

Стент опухолевый полиуретановый с
усиленной верхней частью



Всего пронумеровано,
протнуровано и
скреплено печатью
34 листа (ов)

