



Фотографические изображения медицинского изделия

**Аппарат усиленной наружной контрпульсации EECР LUMENAIR, с
принадлежностью**




Общий вид

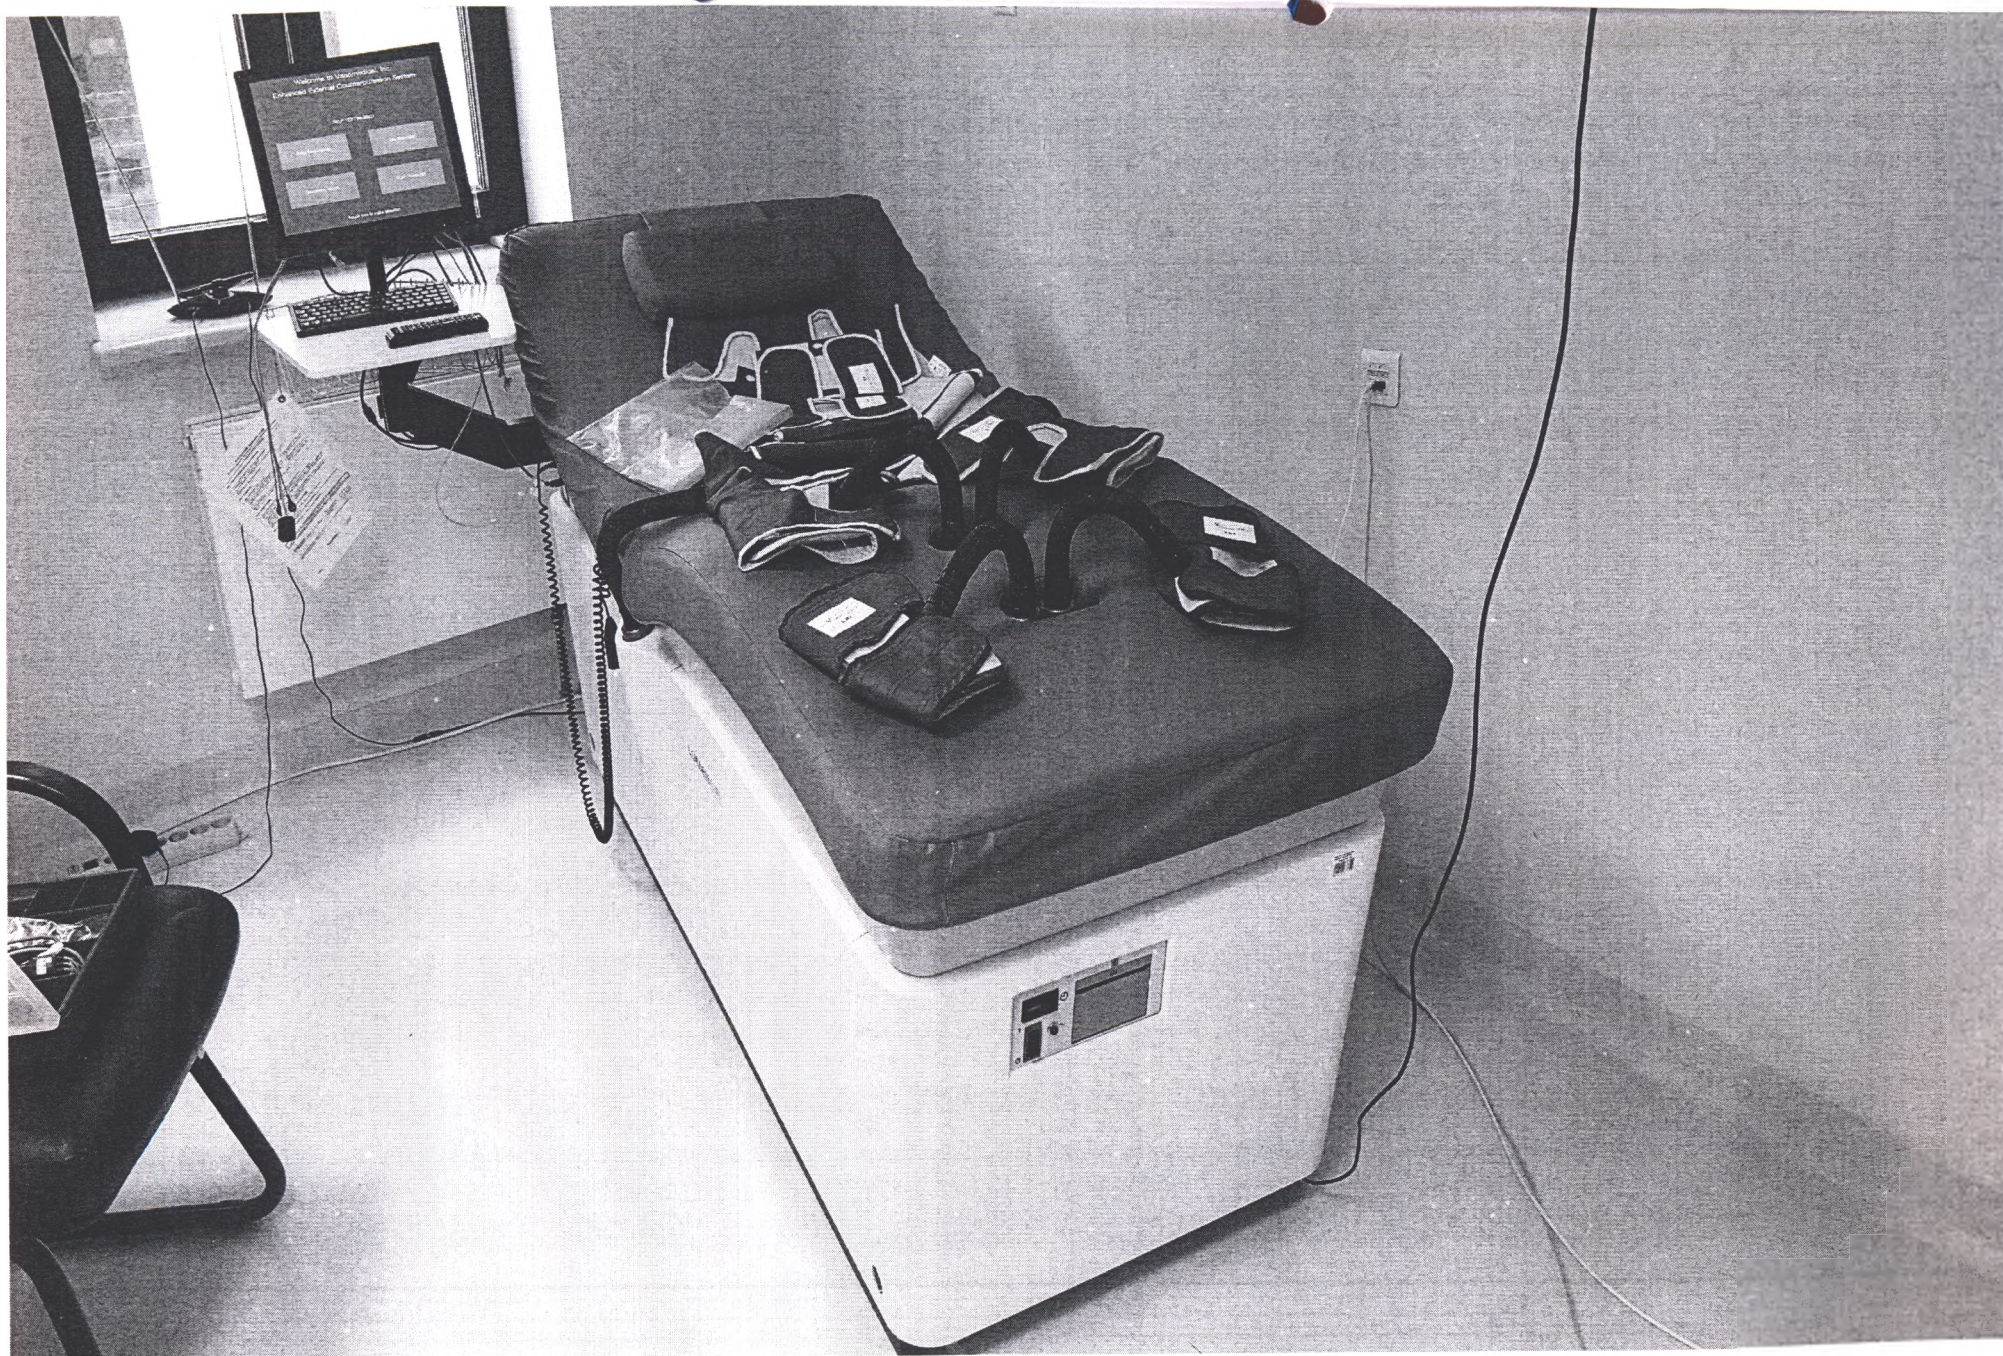


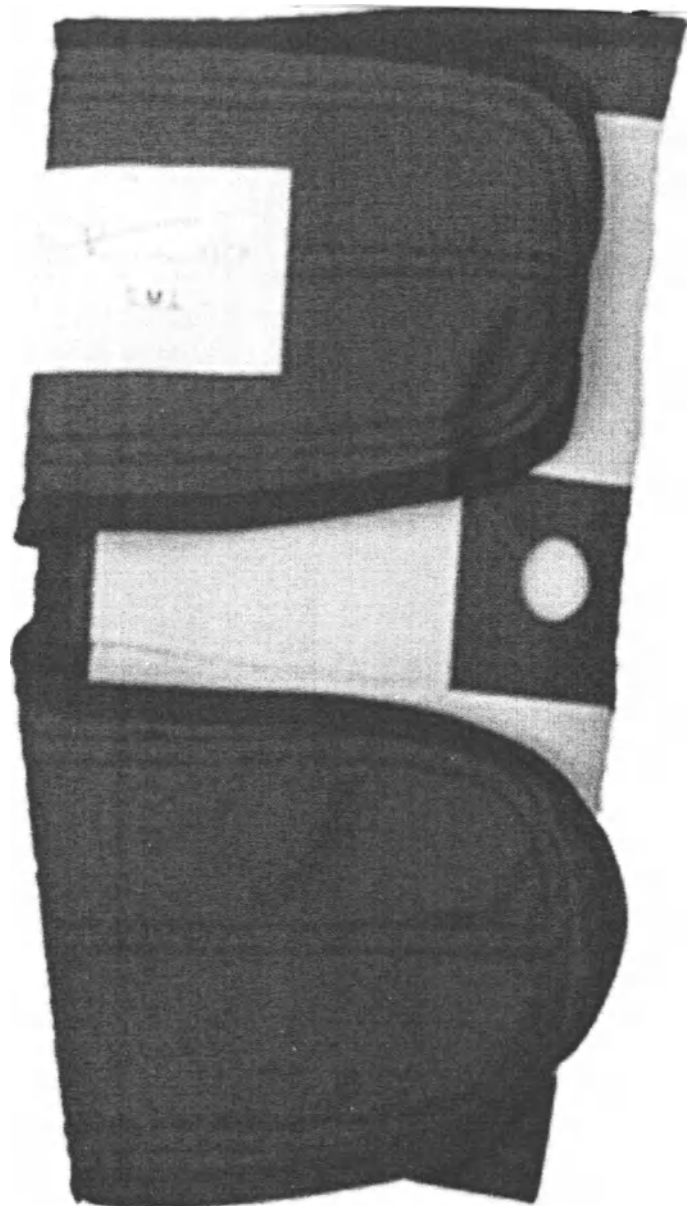


Наружная часть манжеты для голени (все типоразмеры)

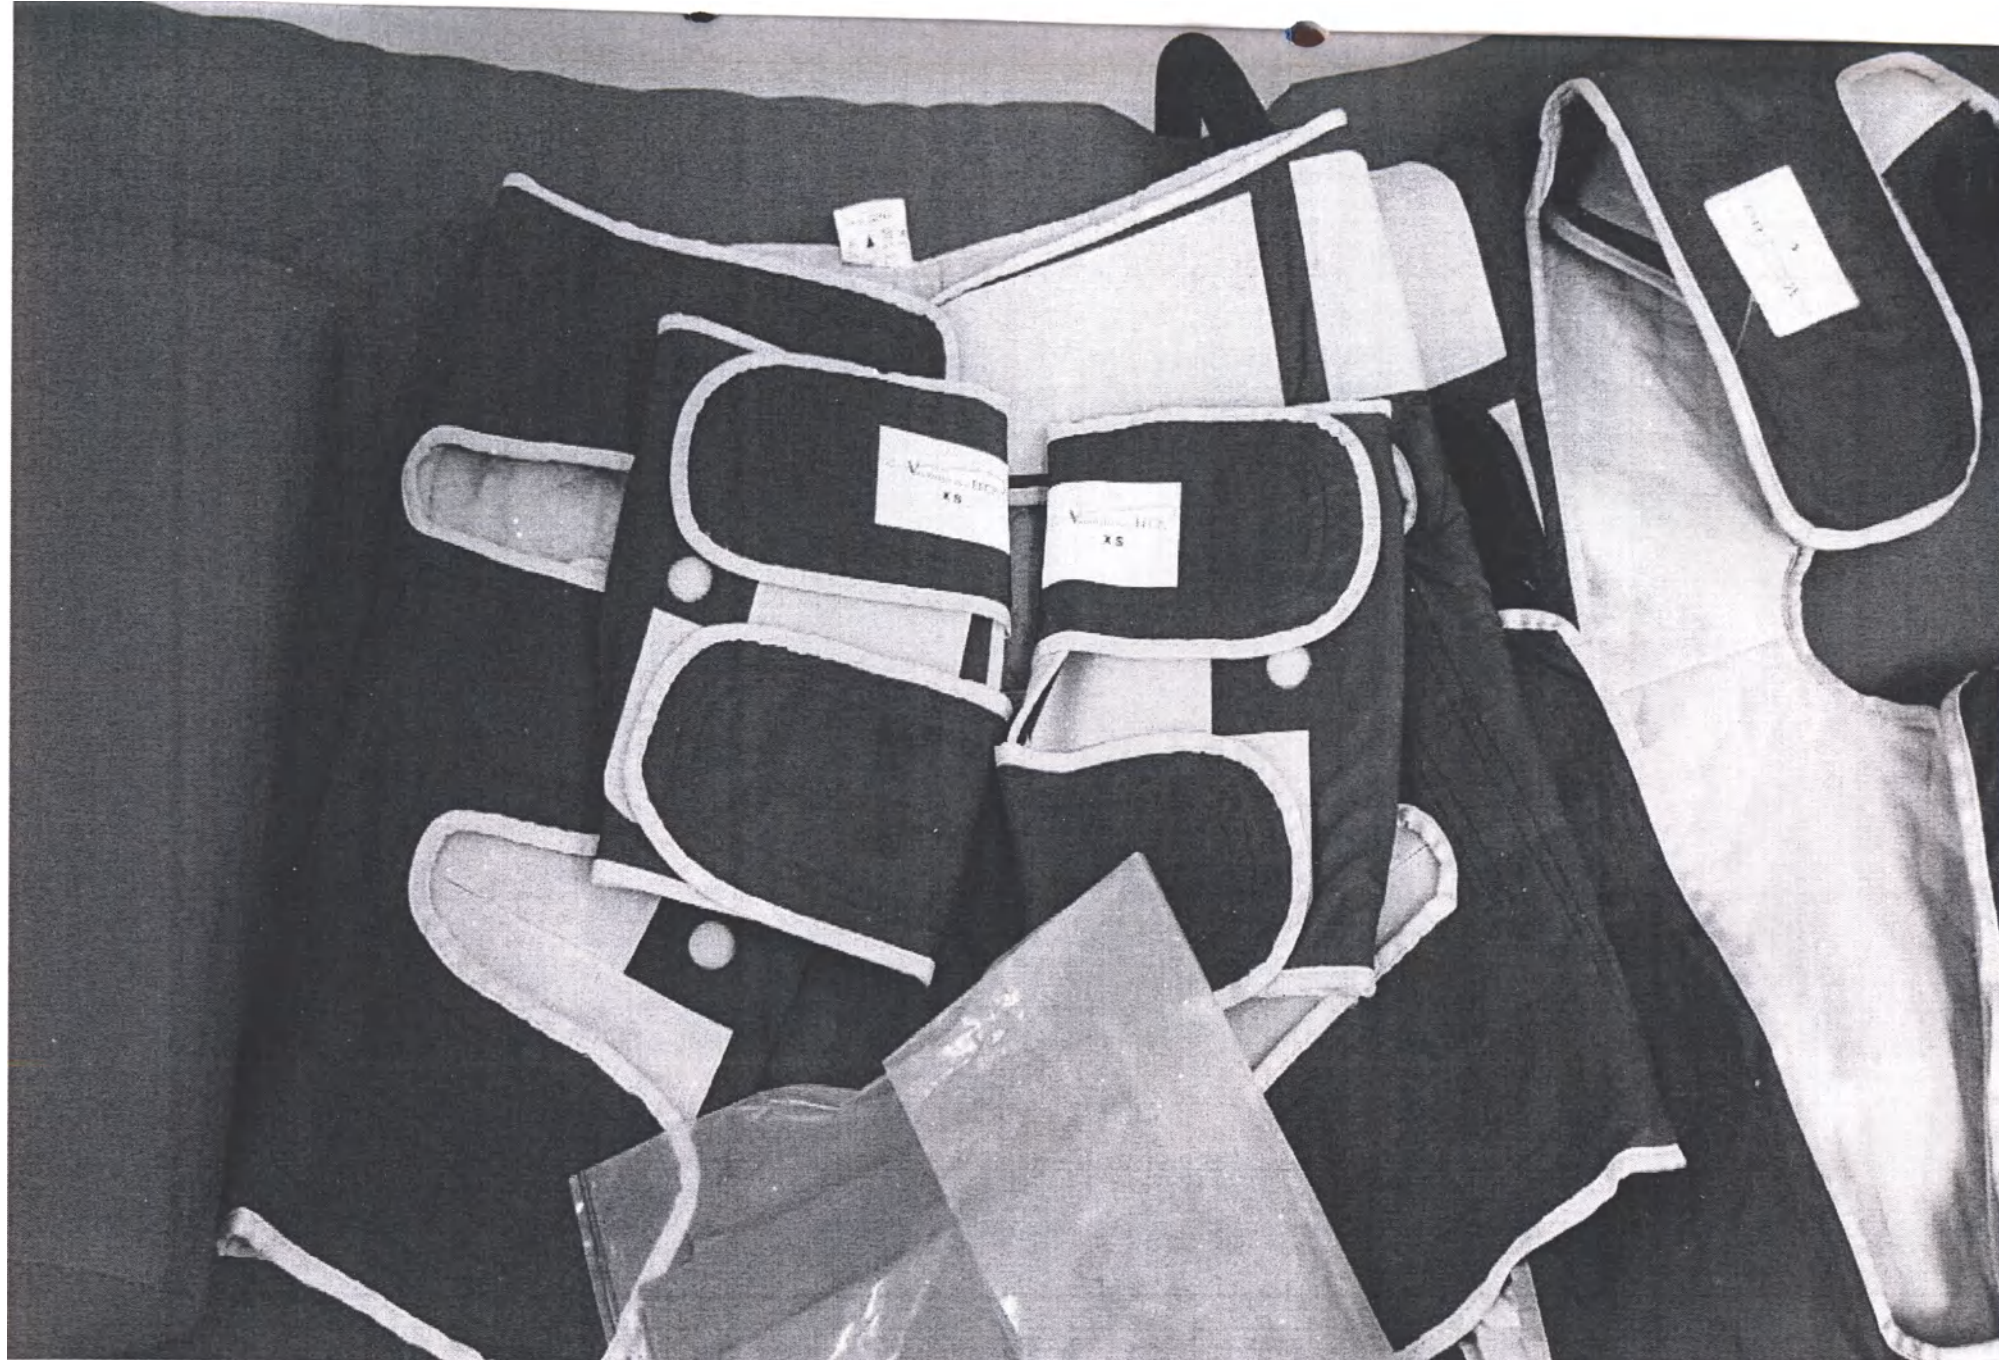

Наружная часть манжеты для бедра (все типоразмеры)

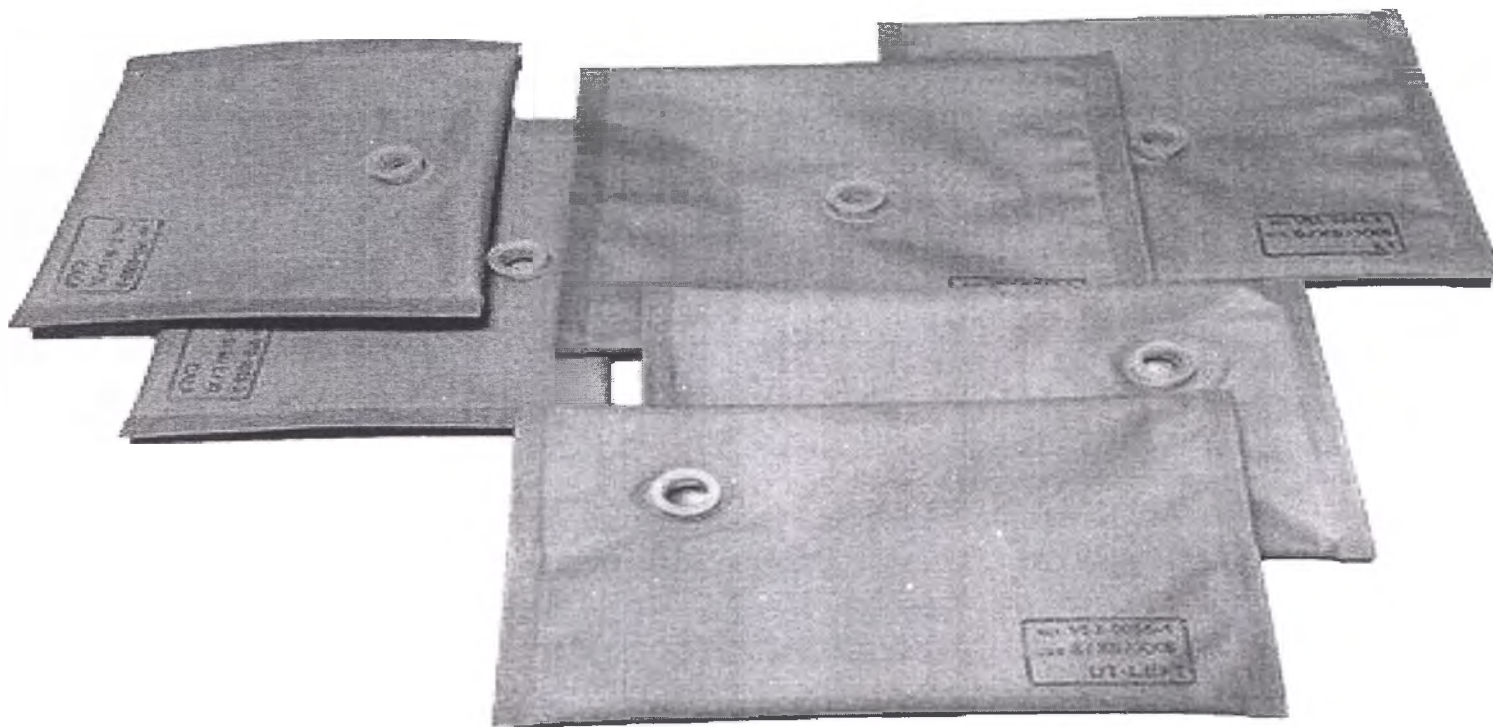

Воздушные камеры манжеты для бедра/голени (все типоразмеры)

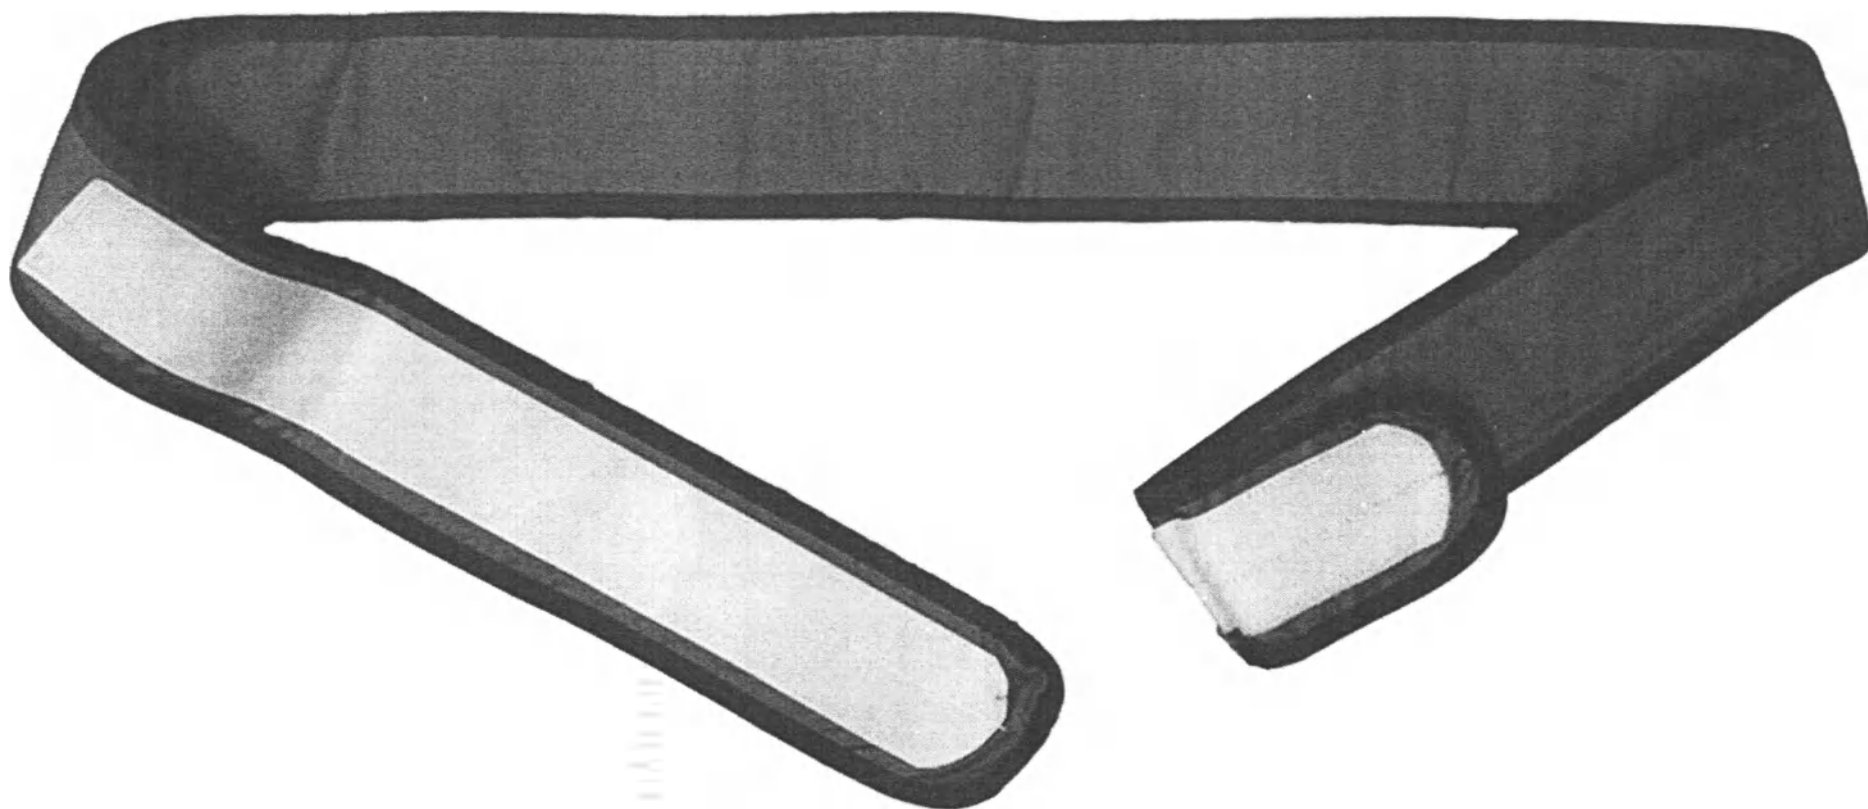


Ремень для закрепления лодыжек пациента








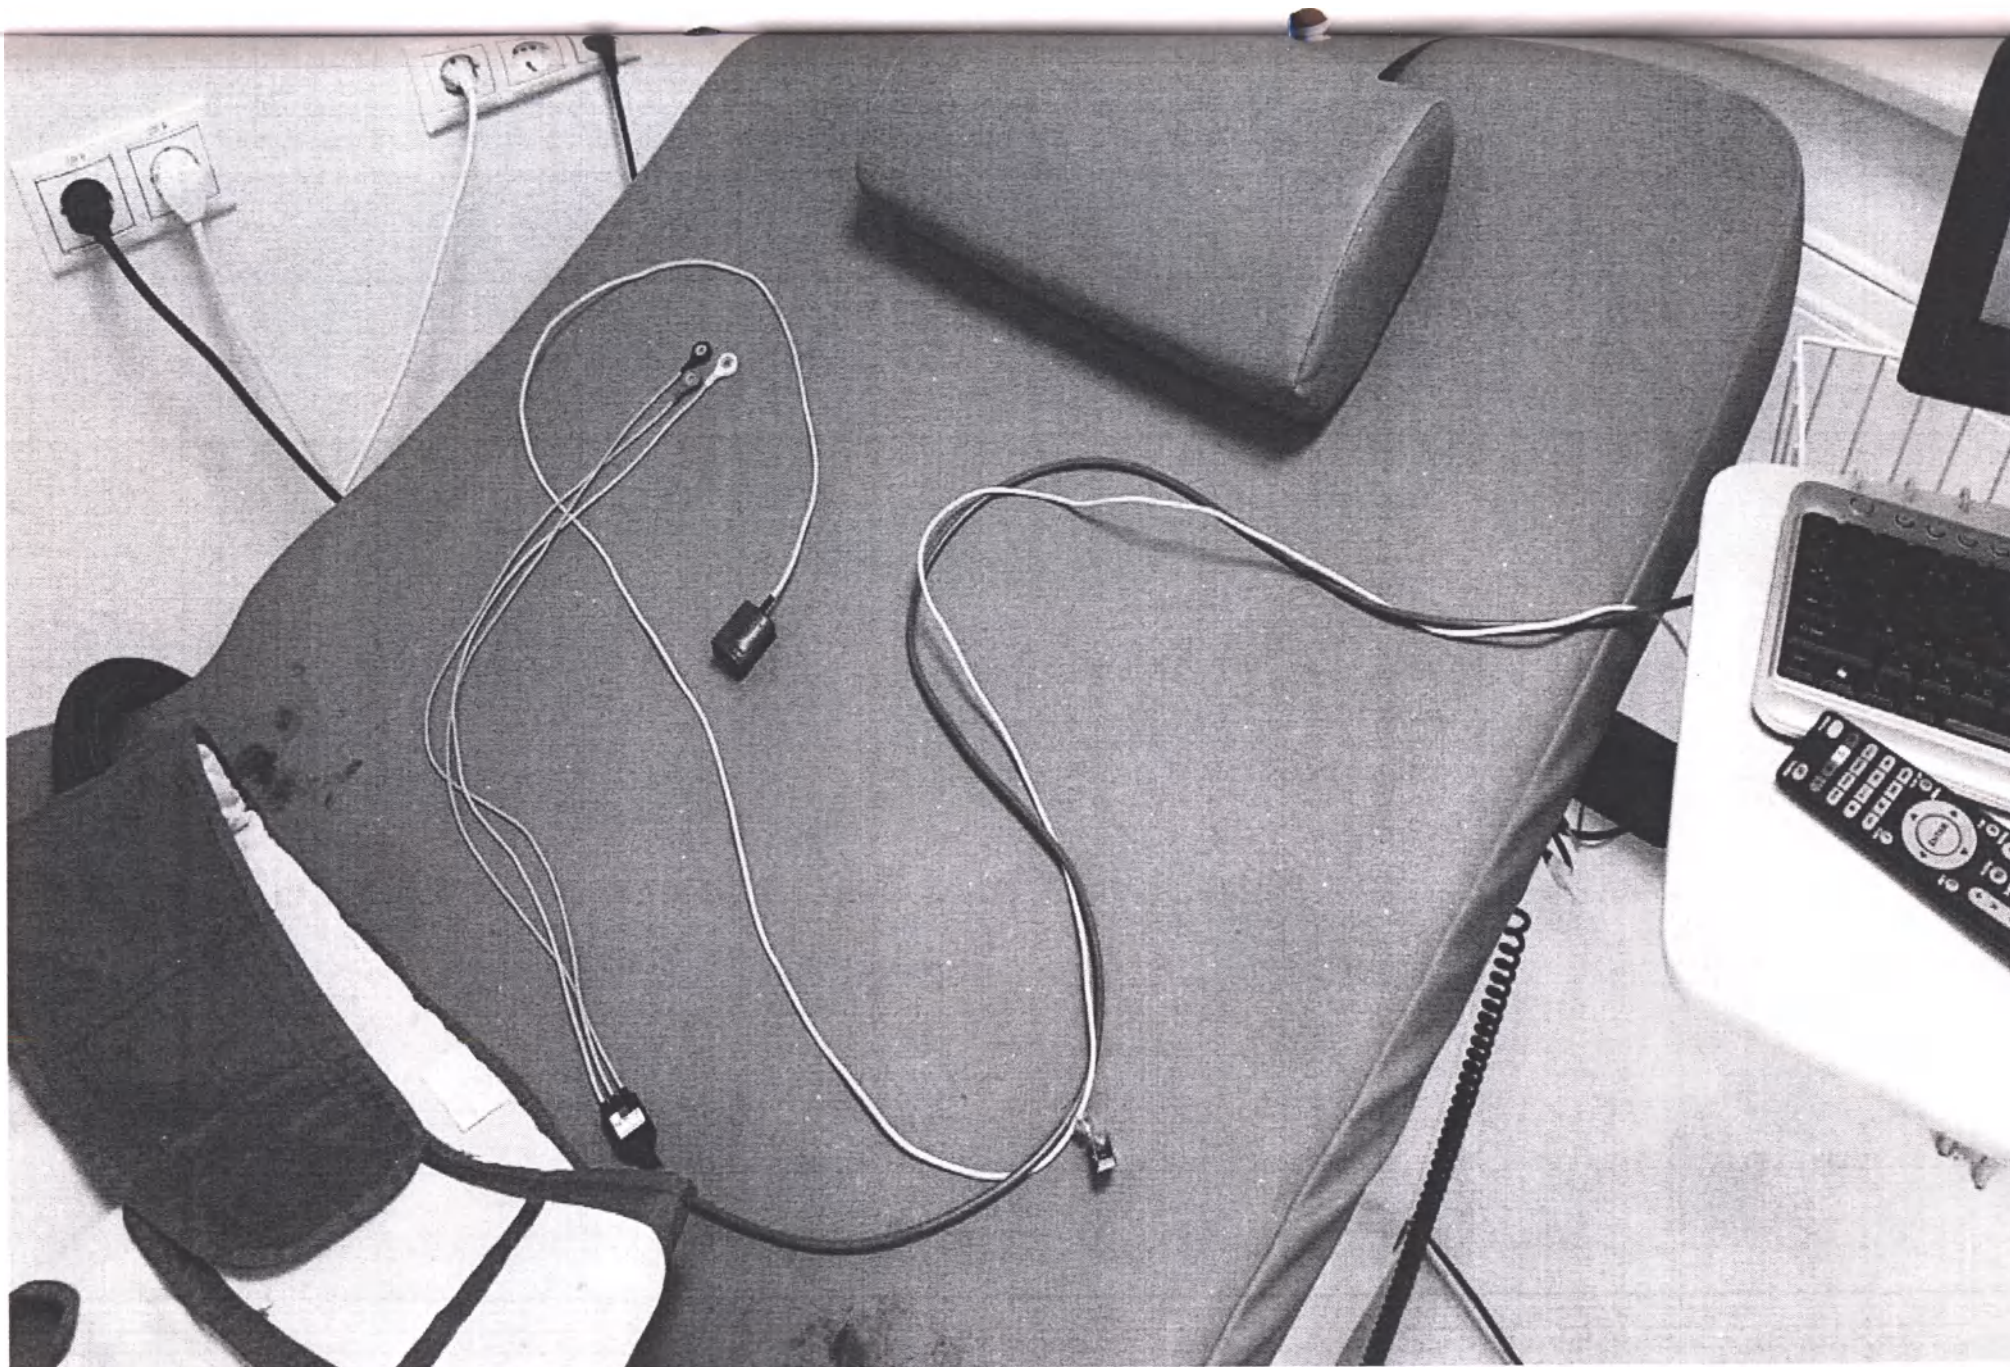


ЭКГ кабель пациента, основной




ЭКГ кабель пациента, основной

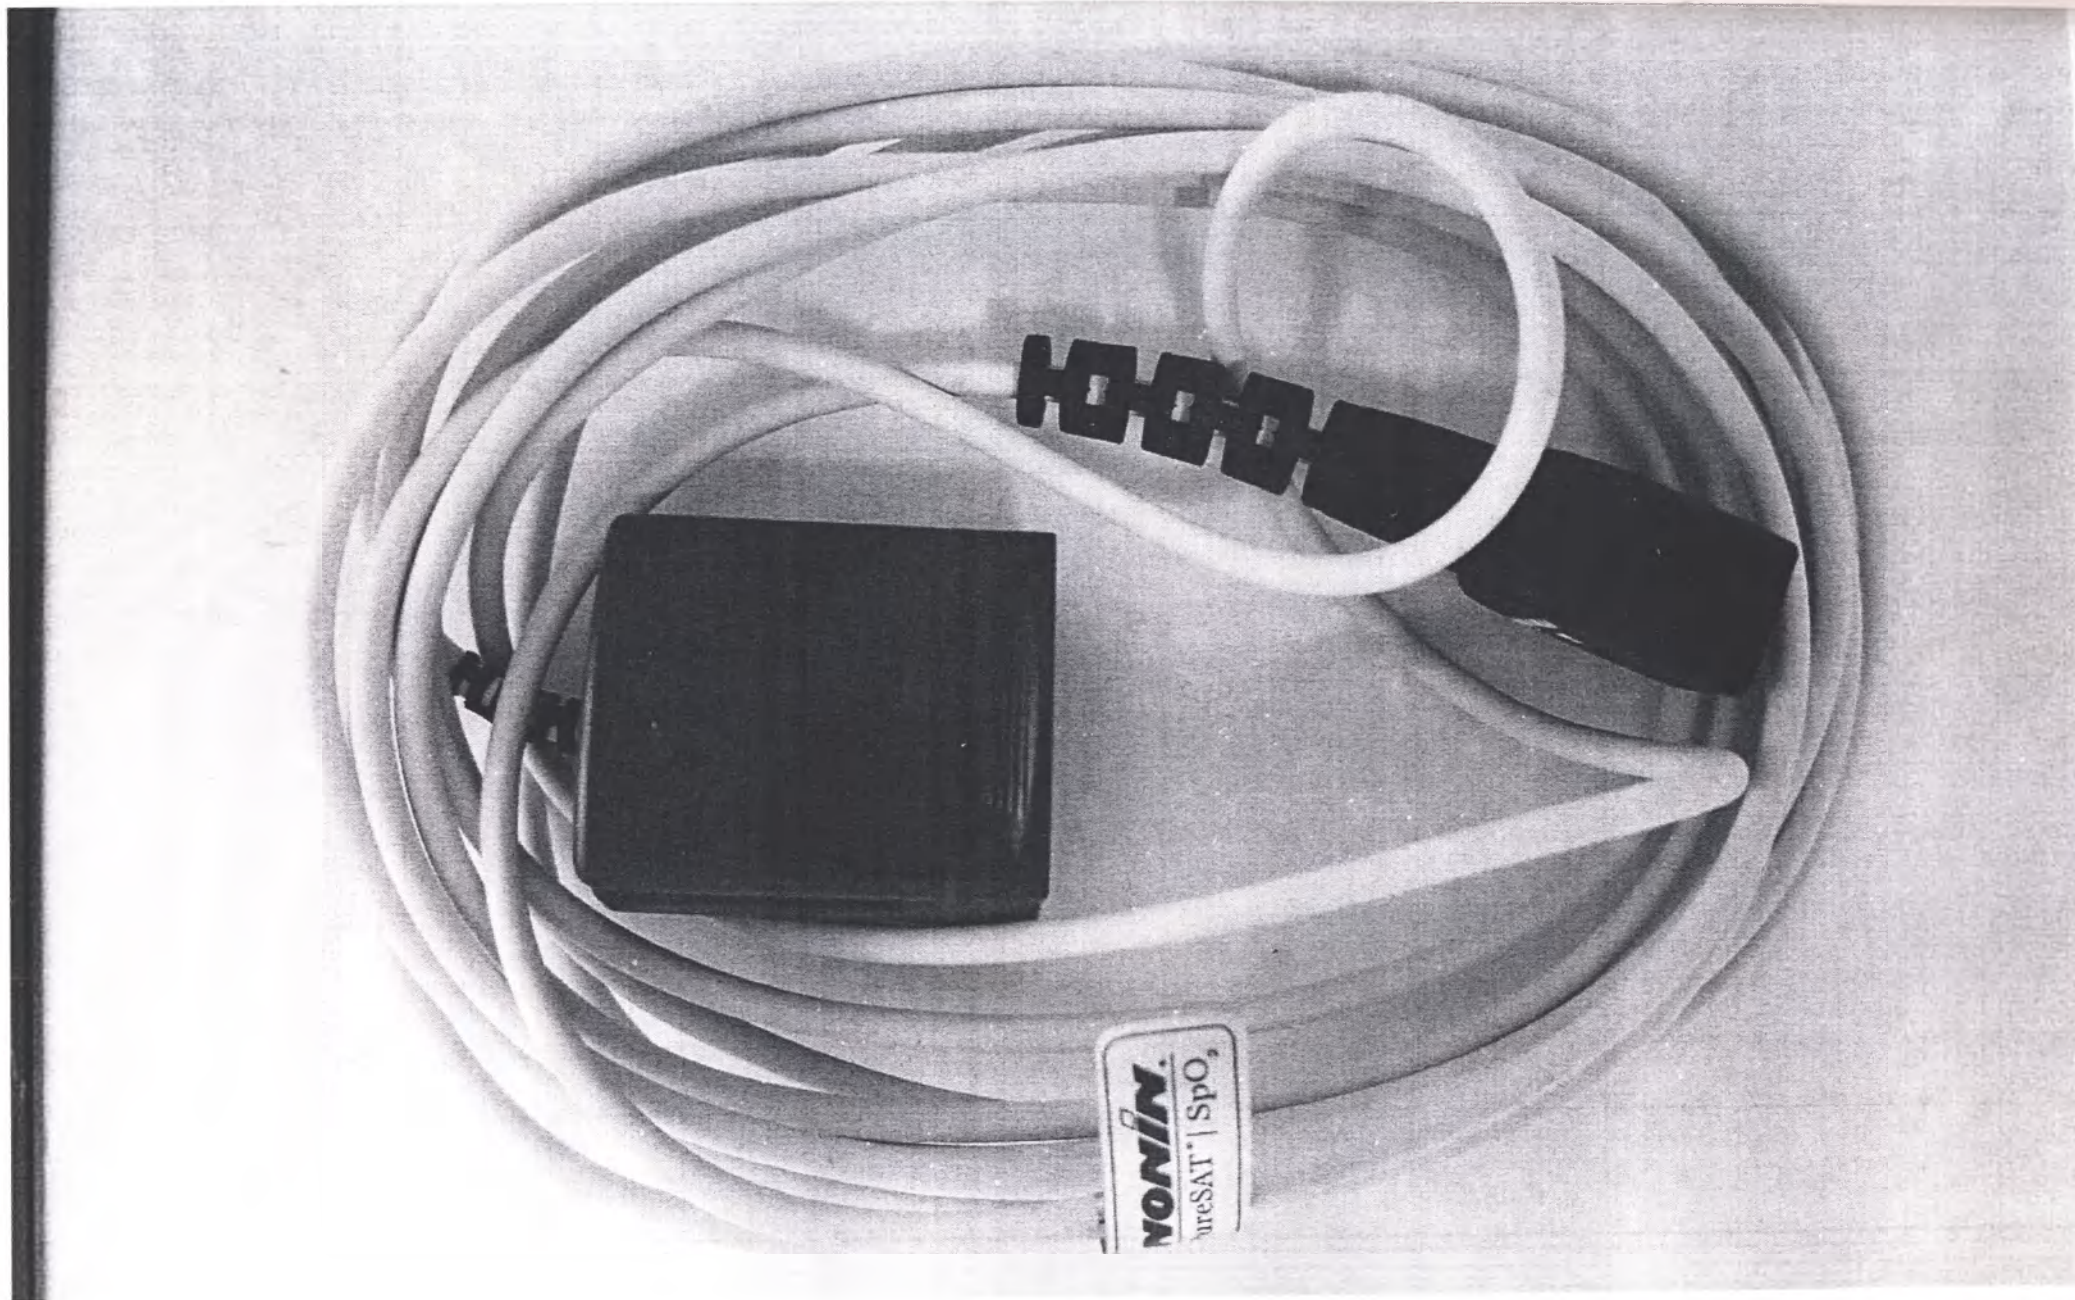


Датчик SpO₂ с кабелем, 8000AA-3, производства фирмы "Nonin", США (РУ ФСР 2012/13343 от 10.04.2015)

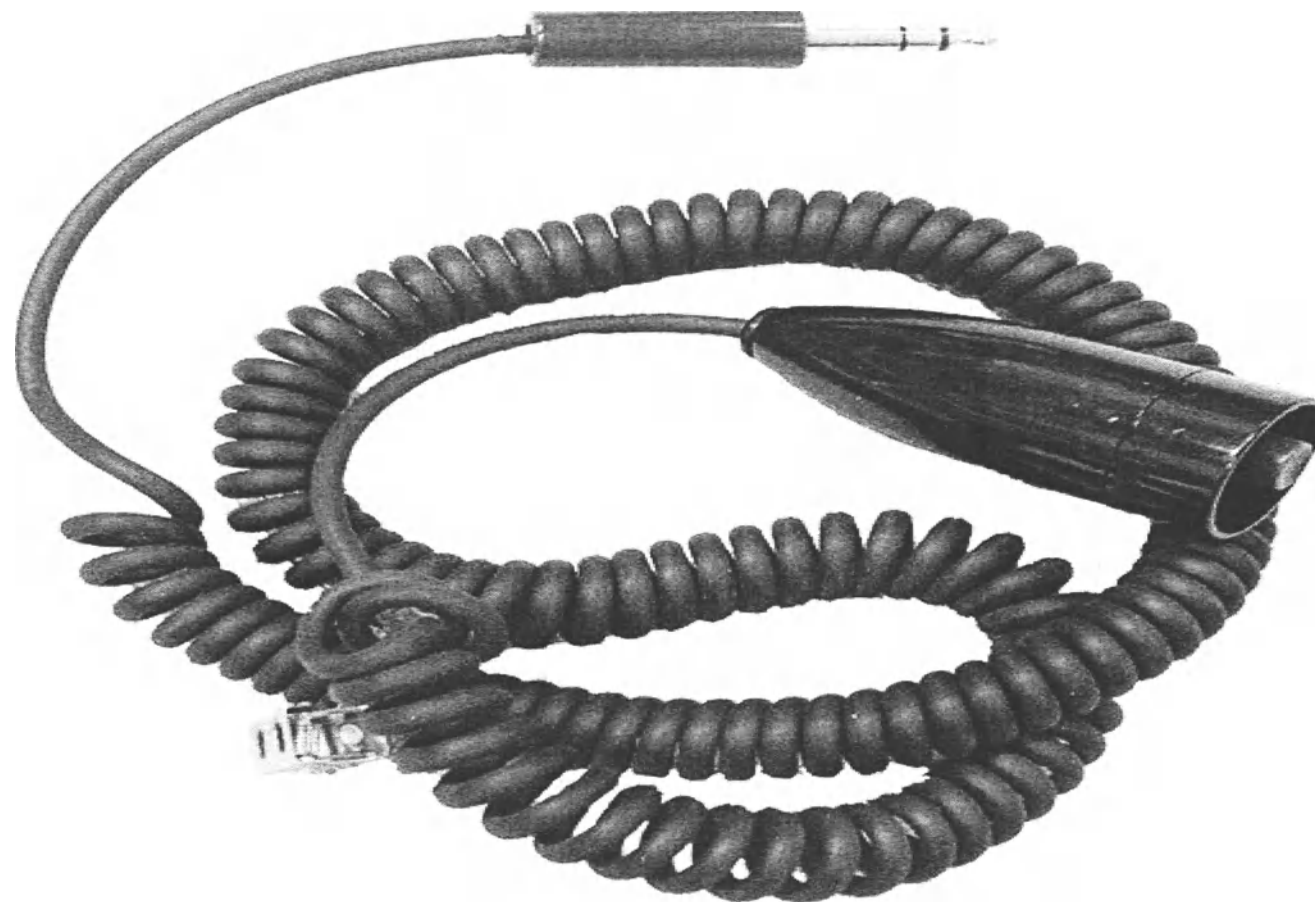

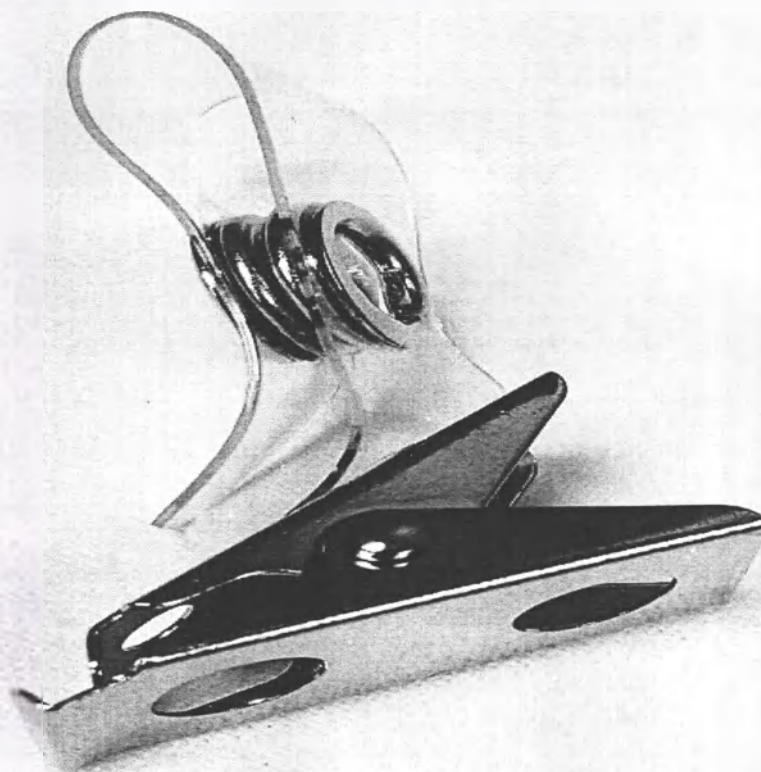

VASOMEDICAL INC. ЕЕСР
NaturalBypass.com

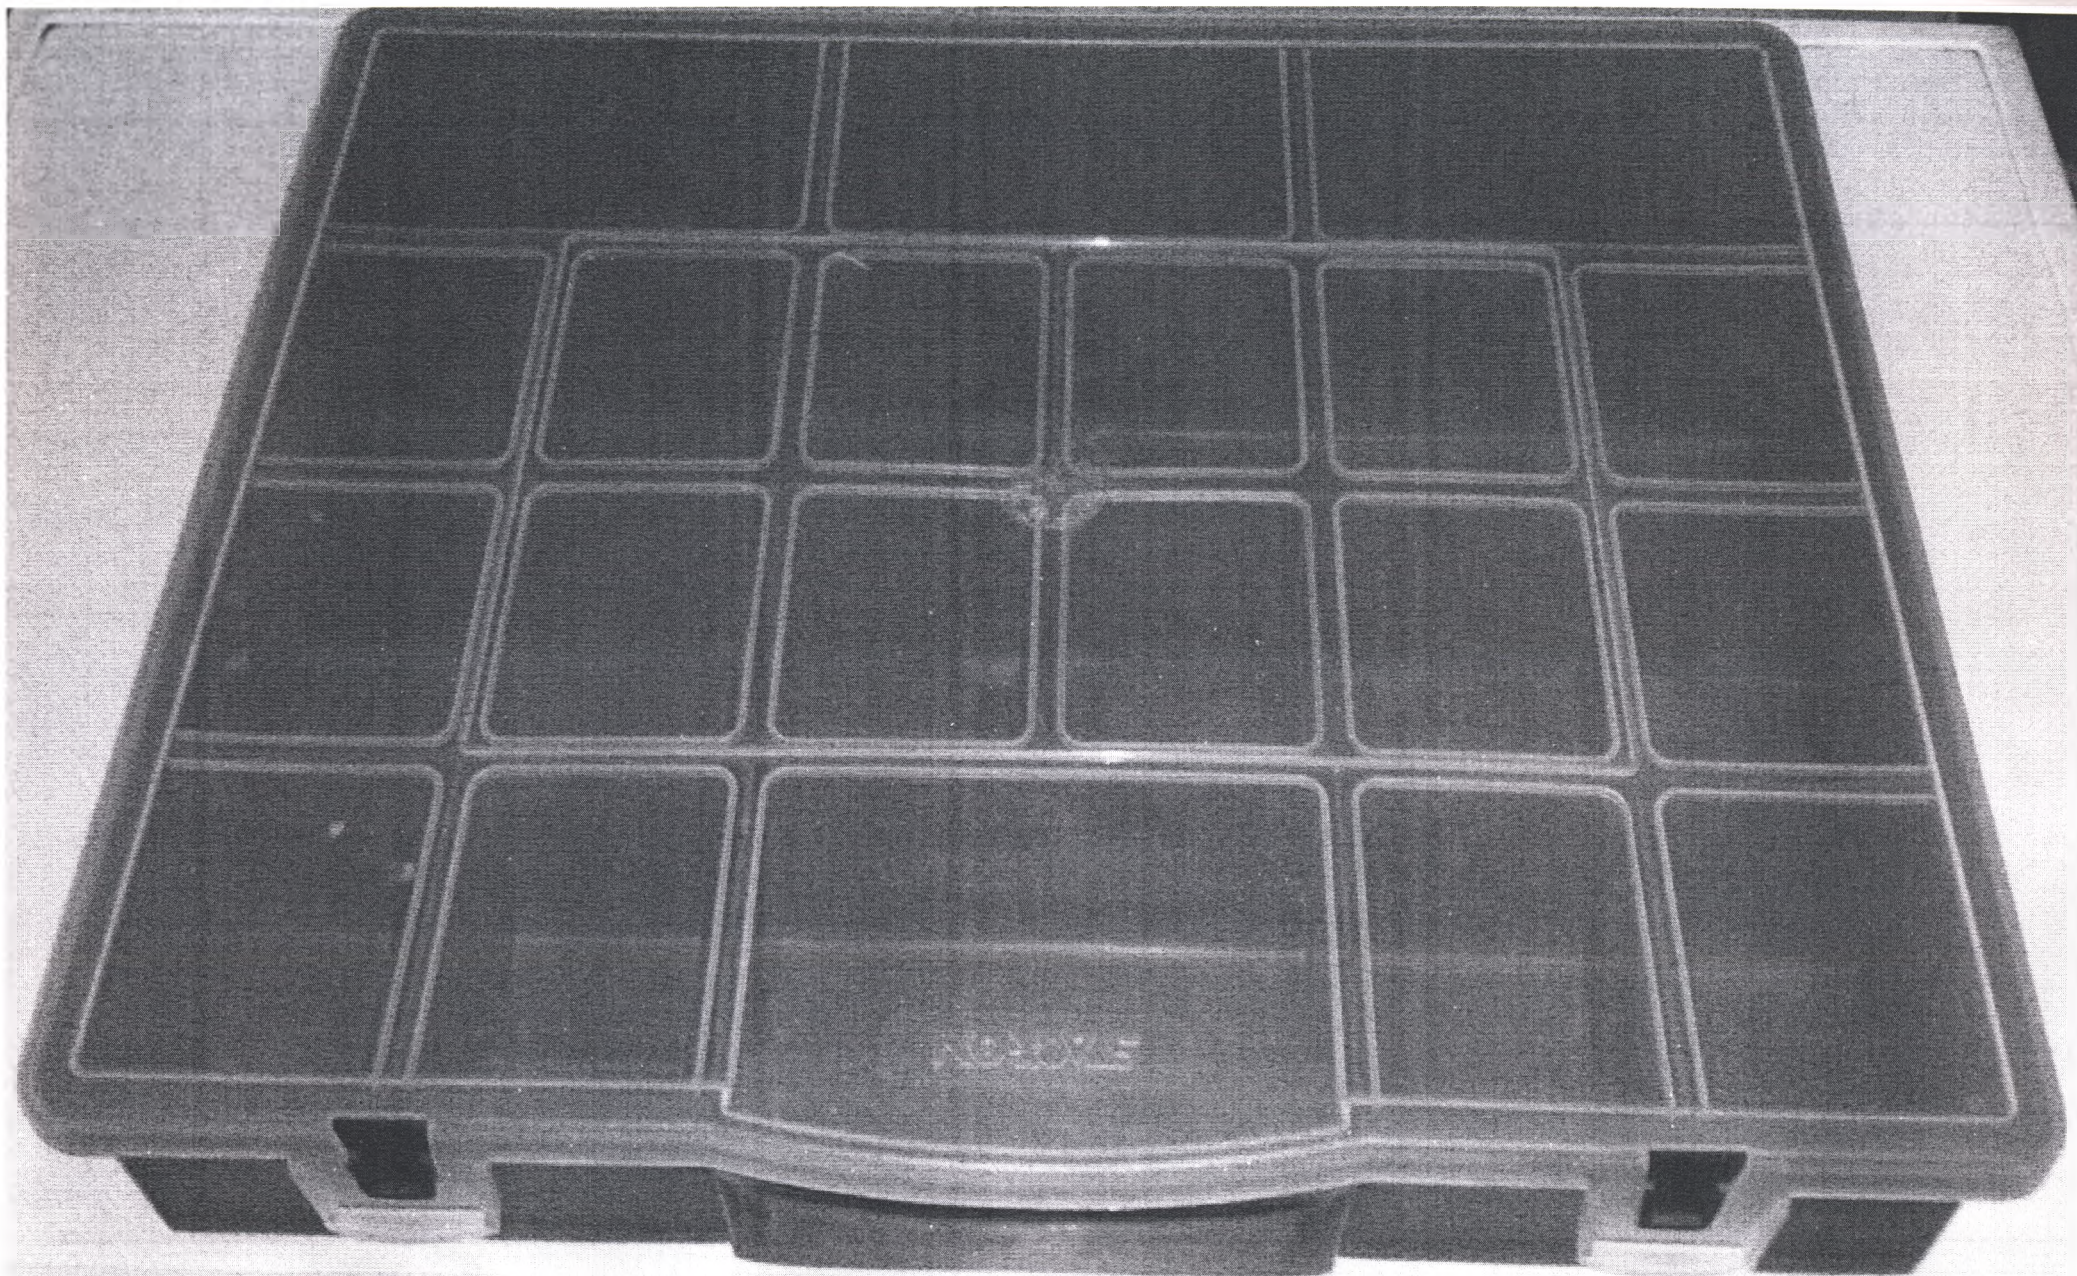

ВНЕШНИЙ ОТДЕЛ
ПОСЛАНИИ
ОБЩЕСТВЕННО-ПРАВОВЫЙ
СЕКТОР
ПОСЛАНИИ
ПОСЛАНИИ

ВНЕШНИЙ ОТДЕЛ
ПОСЛАНИИ
ОБЩЕСТВЕННО-ПРАВОВЫЙ
СЕКТОР
ПОСЛАНИИ
ПОСЛАНИИ

Cuff Assembly Guide

Placement & Application Recommendations for Achieving Optimal Cuff During Delivery of EECPT[®] Therapy

1. Position the bladders and cuffs aligning the bladder inlets with cuff inlet openings. [Fig. 1]
 - Upper thigh/buttocks bladders lie across the buttock with the bladder inlet on the upper buttock side of the cuff. [Fig. 1- a]
 - Lower thigh bladders are positioned to lie lengthwise at the inner aspect of the thigh with the bladder inlet in the center. [Fig. 1- b]
 - Calf bladders lie lengthwise on the lower leg, covering the calf muscle. The bladder inlet is inserted into the cuff. [Fig. 1- c]
2. Fold the upper thigh/buttocks cuffs in half exposing the lining. Position bladders on the lining. [Fig. 2]
3. Open the hook and loop binding. [Fig. 3]
 - Insert upper thigh/buttocks bladders positioning the bladders as indicated in Fig. 1- a, 2- a.
 - Insert the lower thigh bladders positioning the bladders as indicated in Fig. 1- b, 2- b.
4. After inserting the bladders, check to be sure they are lying flat, without wrinkles or creases. Secure the bindings and smooth out wrinkles of the cuff lining.
5. Repeat steps 1-4 for the opposite side of the upper thigh/ buttocks cuffs.
6. Open the hook and loop binding for the calf cuff and insert the bladder inlet side first. [Fig. 5] Position the bladders as indicated in Fig. 1- c, 2- c, 5- c. *Inserted correctly, the bladder will be positioned facing the opening/ strap side of the cuffs.* Smooth out wrinkles and creases and secure the bindings. Repeat this step for the opposite calf cuff.

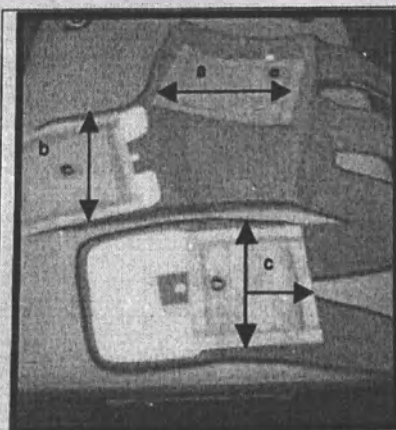


Fig. 1

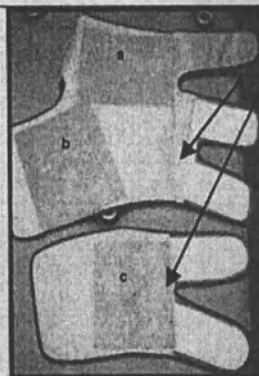


Fig. 2

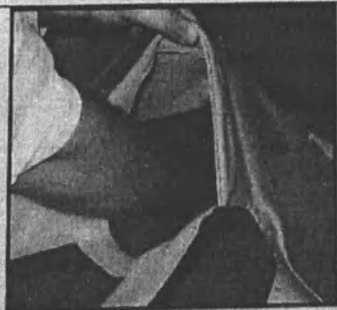


Fig. 3

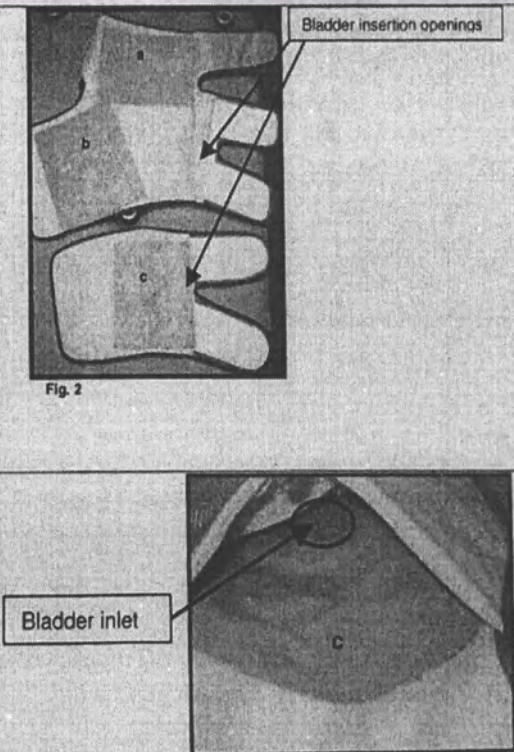


Fig. 5

