

Катетер баллонный OPN NC



ВЕО NC High Pressure 24 mm


Inflation Compliance: Do not exceed Rated Burst Pressure (RBP)

Preload (mmHg) Ø Diameter [mm]


	1.5	2.0	2.5	3.0	3.5	4.0
10	1.53	2.02	2.50	3.00	3.52	4.03
12	1.56	2.06	2.54	3.04	3.57	4.10
14	1.58	2.10	2.57	3.07	3.61	4.17
16	1.59	2.11	2.60	3.11	3.65	4.22
18	1.62	2.13	2.63	3.17	3.69	4.27
20	1.64	2.16	2.67	3.22	3.73	4.33
22	1.67	2.19	2.70	3.26	3.77	4.37
24	1.72	2.22	2.73	3.30	3.81	4.43
RBP	2.22	2.73	3.30	3.81	4.37	4.93

ПРИНАДЛЕЖНОСТИ

Шприц-манометр 96346 (40 атм)

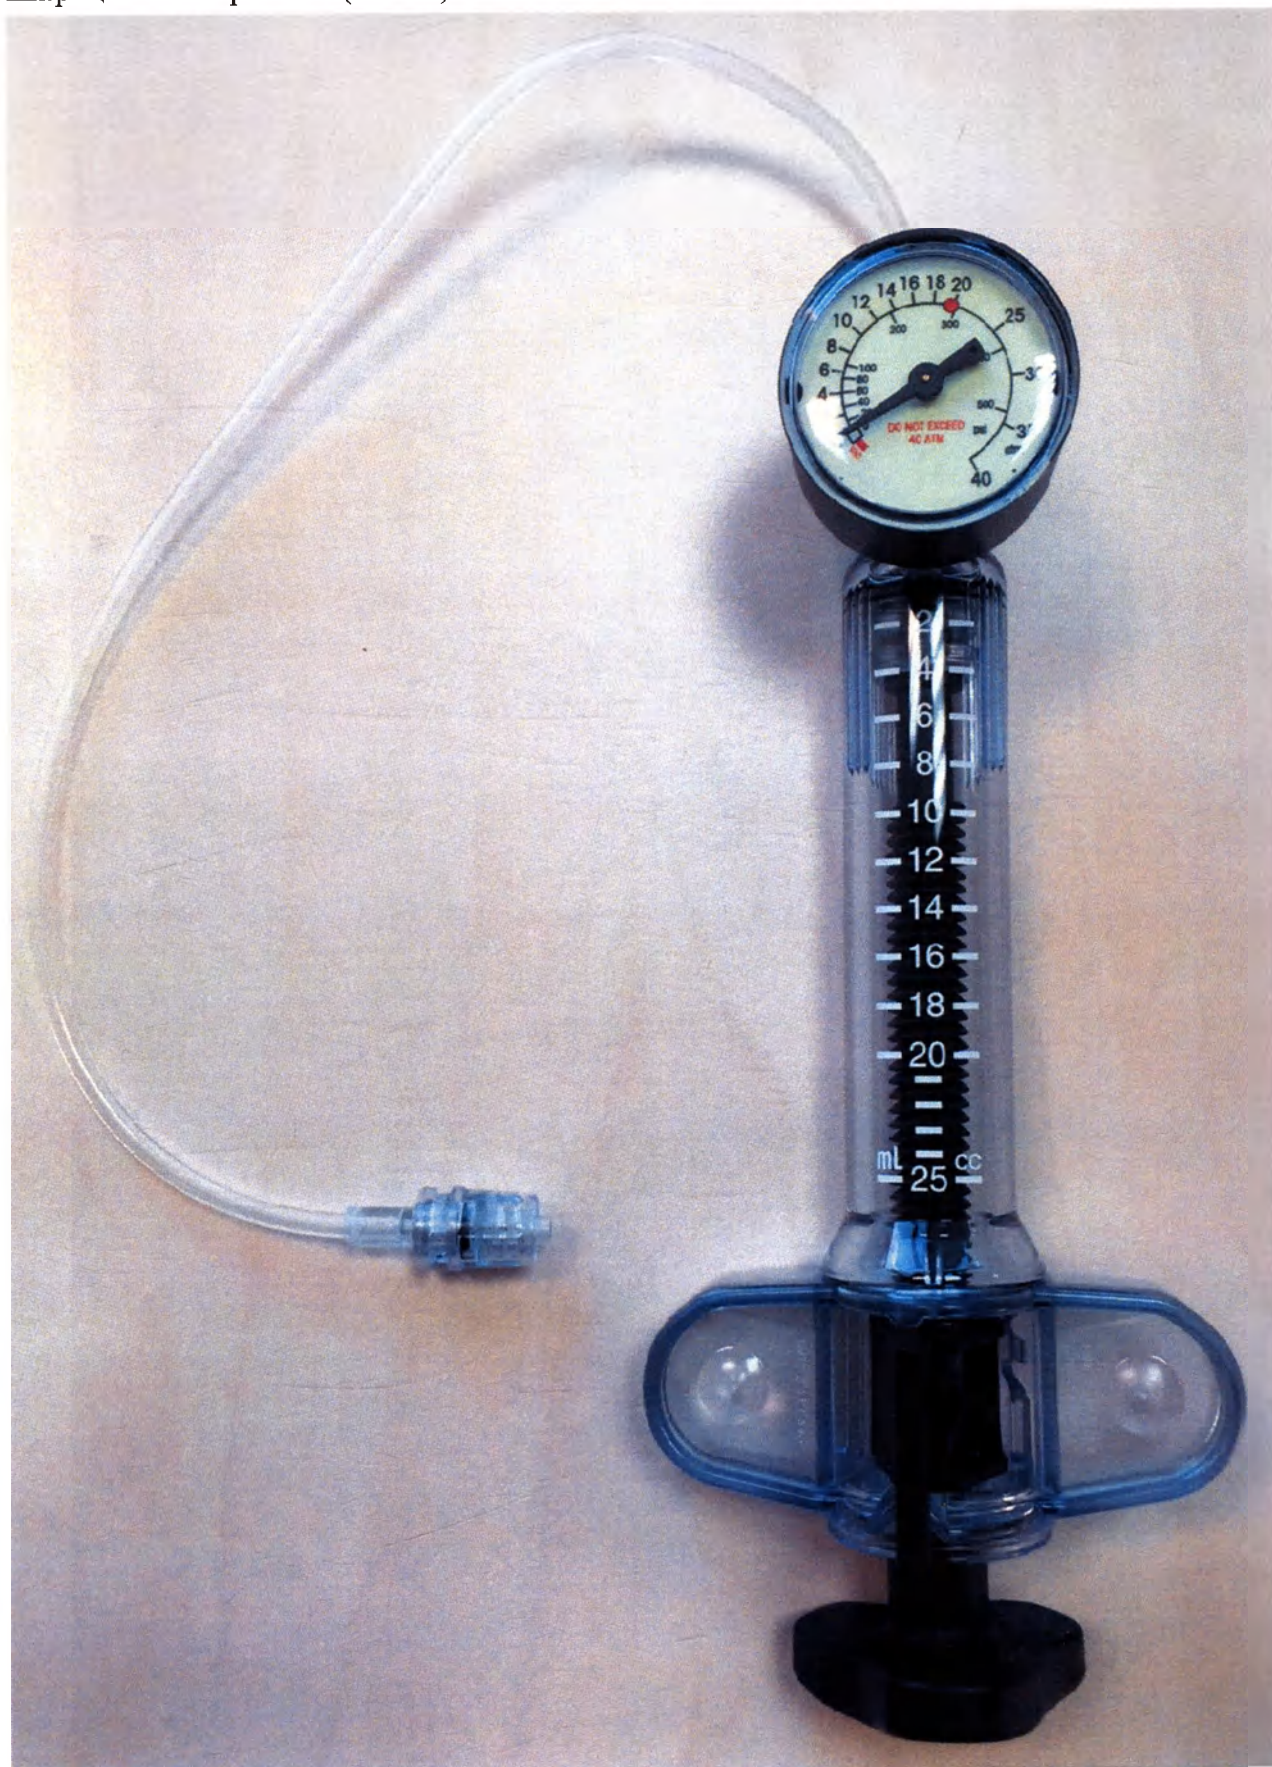

Шприц-манометр 96463 (55 атм)

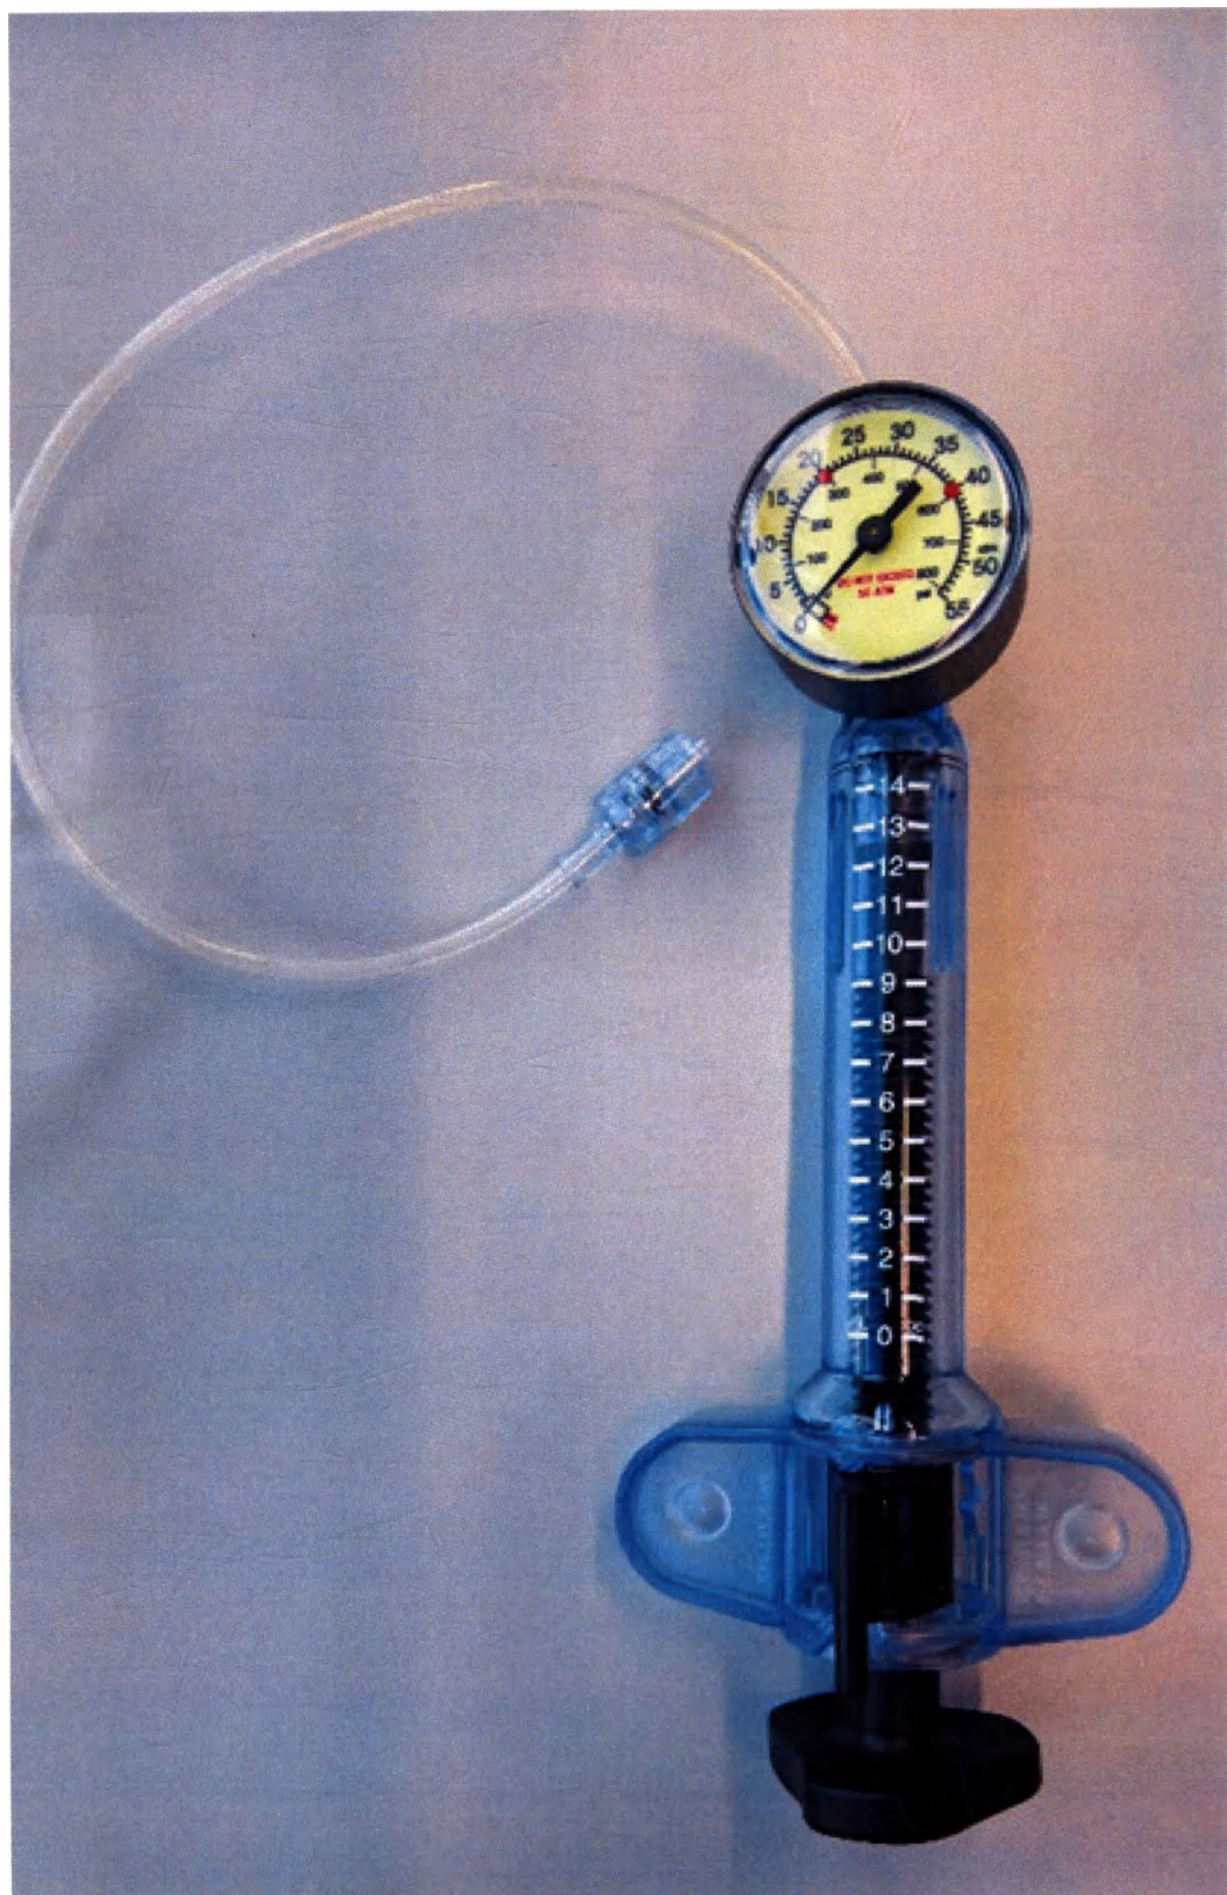



Оборотень 21.10.

Прошито и
пронумеровано 4 листов