



лет успеха!

Генеральный дилер предприятий: "CHIRANA s.r.o." "CHIRASTAR KDT" "BEING Foshan" в РОССИИ
Официальный дилер предприятий: "Chirana-Dental" "TECNO-GAZ" "Ekom" "Bien-Air"
Авторизованный сервисный центр. Российский центр обучения сервисных инженеров.
Склад оборудования и запасных частей.

ООО фирма "Соло". Адрес: 620137 г. Екатеринбург ул. Блюхера 75 корпус 1, помещение 3-17
Расч./счет 40702810616540008584 в УРАЛЬСКИЙ БАНК СБЕРБАНКА РФ г. Екатеринбург
Кор/счет 30101810500000000674 БИК 046577674 ИНН 6659005033 КПП 667001001
ОГРН 1026602952760 Код по ОКПО 25027715 Код по ОКОНХ 19320/71500, 80400/95300
Тел/факс (343) 351-76-16, 351-76-12, 351-76-13, 351-76-14
E-mail: mail@solo-trade.ru www.solo-trade.ru www.solo-chirana.ru www.beingfoshan.ru

Фотографические изображения медицинского изделия

«Система ультразвукового сканирования SONON 300C, SONON 300L с принадлежностями»

Производитель:

Healcerion Co., Ltd

804ho, 38-21, Digital-ro 31-gil, Guro-gu, Seoul, 08376, Korea



Сканер SONON 300C



Сканер SONON 300C




Сканер SONON 300C



Сканер SONON 300C



Сканер SONON 300C

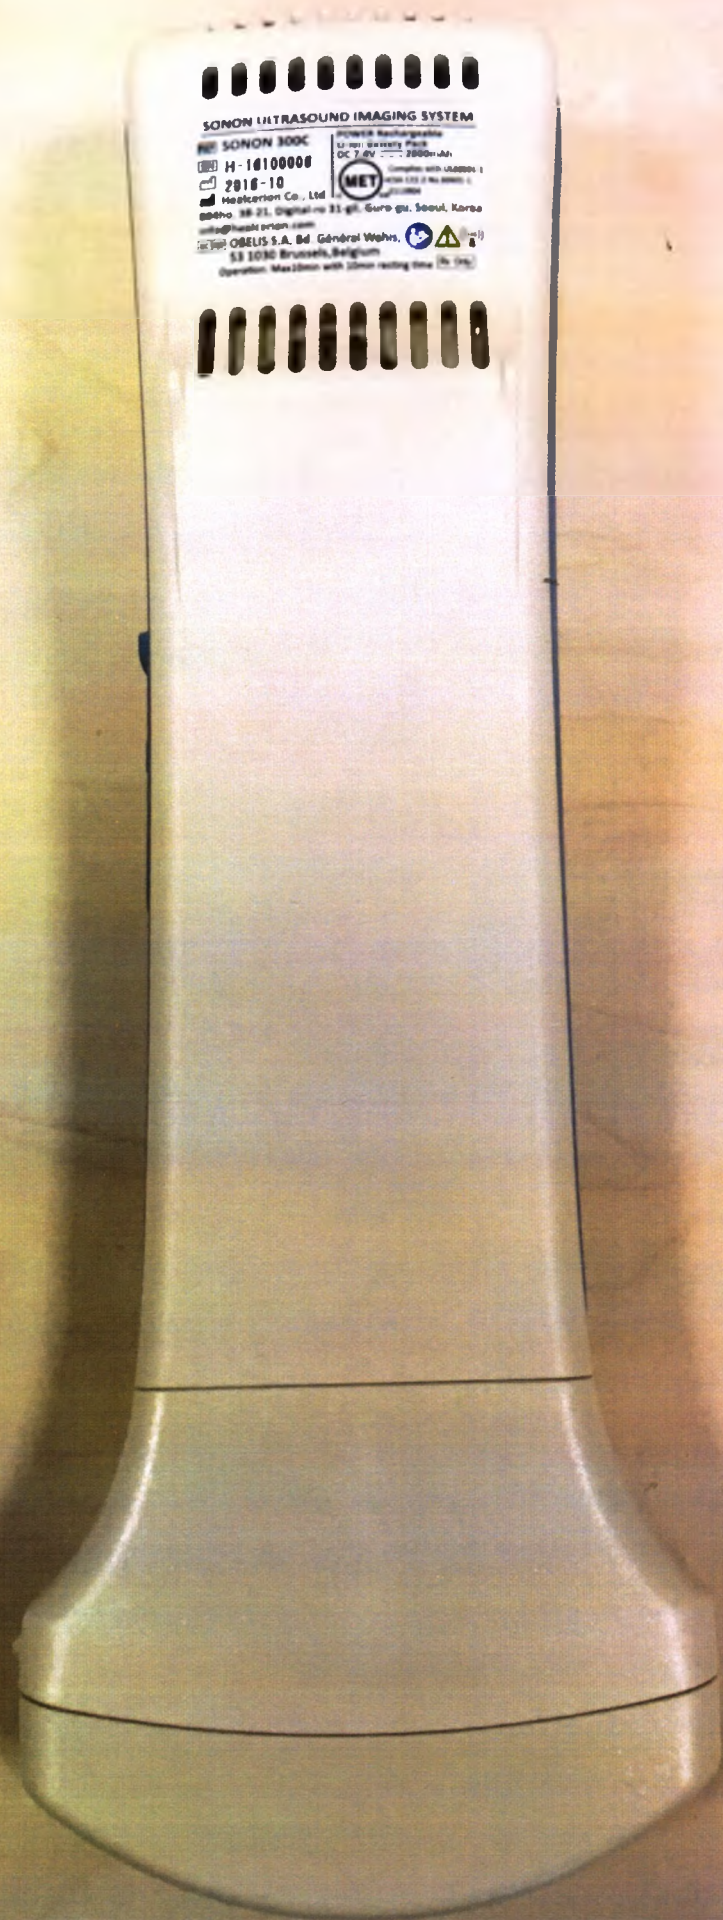

SONON ULTRASOUND IMAGING SYSTEM

SONON 300C

H-10100000

2010-10

Mediscan Co., Ltd.

2010-10-21, Digital no. 31-gil, Guro-gu, Seoul, Korea

mediscan@mediscan.com

OBELIS S.A. Bd Général Weyts,

53 1030 Brussels, Belgium

Operation: Max 20min with 20min cooling time (No. 104)

Powerful Rechargeable
12-lead Battery Pack
DC 7.0V 2000mAh

Complies with IEC60601-1

CE Mark

RoHS

WEEE

REACH

EN 60601-1

EN 60601-1-2

EN 60601-1-3

EN 60601-1-4

EN 60601-1-5

EN 60601-1-6

EN 60601-1-7

EN 60601-1-8

EN 60601-1-9

EN 60601-1-10

EN 60601-1-11

EN 60601-1-12

EN 60601-1-13

EN 60601-1-14

EN 60601-1-15

EN 60601-1-16

EN 60601-1-17

EN 60601-1-18

EN 60601-1-19

EN 60601-1-20

EN 60601-1-21

EN 60601-1-22

EN 60601-1-23

EN 60601-1-24

EN 60601-1-25

EN 60601-1-26

EN 60601-1-27

EN 60601-1-28

EN 60601-1-29

EN 60601-1-30

EN 60601-1-31

EN 60601-1-32

EN 60601-1-33

EN 60601-1-34

EN 60601-1-35

EN 60601-1-36

EN 60601-1-37

EN 60601-1-38

EN 60601-1-39

EN 60601-1-40

EN 60601-1-41

EN 60601-1-42

EN 60601-1-43

EN 60601-1-44

EN 60601-1-45

EN 60601-1-46

EN 60601-1-47

EN 60601-1-48

EN 60601-1-49

EN 60601-1-50

EN 60601-1-51

EN 60601-1-52

EN 60601-1-53

EN 60601-1-54

EN 60601-1-55

EN 60601-1-56

EN 60601-1-57

EN 60601-1-58

EN 60601-1-59

EN 60601-1-60

EN 60601-1-61

EN 60601-1-62

EN 60601-1-63

EN 60601-1-64

EN 60601-1-65

EN 60601-1-66

EN 60601-1-67

EN 60601-1-68

EN 60601-1-69

EN 60601-1-70

EN 60601-1-71

EN 60601-1-72

EN 60601-1-73

EN 60601-1-74

EN 60601-1-75

EN 60601-1-76

EN 60601-1-77

EN 60601-1-78

EN 60601-1-79

EN 60601-1-80

EN 60601-1-81

EN 60601-1-82

EN 60601-1-83

EN 60601-1-84

EN 60601-1-85

EN 60601-1-86

EN 60601-1-87

EN 60601-1-88

EN 60601-1-89

EN 60601-1-90

EN 60601-1-91

EN 60601-1-92

EN 60601-1-93

EN 60601-1-94

EN 60601-1-95

EN 60601-1-96

EN 60601-1-97

EN 60601-1-98

EN 60601-1-99

EN 60601-1-100

EN 60601-1-101

EN 60601-1-102

EN 60601-1-103

EN 60601-1-104

EN 60601-1-105

EN 60601-1-106

EN 60601-1-107

EN 60601-1-108

EN 60601-1-109

EN 60601-1-110

EN 60601-1-111

EN 60601-1-112

EN 60601-1-113

EN 60601-1-114

EN 60601-1-115

EN 60601-1-116

EN 60601-1-117

EN 60601-1-118

EN 60601-1-119

EN 60601-1-120

EN 60601-1-121

EN 60601-1-122

EN 60601-1-123

EN 60601-1-124

EN 60601-1-125

EN 60601-1-126

EN 60601-1-127

EN 60601-1-128

EN 60601-1-129

EN 60601-1-130

EN 60601-1-131

EN 60601-1-132

EN 60601-1-133

EN 60601-1-134

EN 60601-1-135

EN 60601-1-136

EN 60601-1-137

EN 60601-1-138

EN 60601-1-139

EN 60601-1-140

EN 60601-1-141

EN 60601-1-142

EN 60601-1-143

EN 60601-1-144

EN 60601-1-145

EN 60601-1-146

EN 60601-1-147

EN 60601-1-148

EN 60601-1-149

EN 60601-1-150

EN 60601-1-151

EN 60601-1-152

EN 60601-1-153

EN 60601-1-154

EN 60601-1-155

EN 60601-1-156

EN 60601-1-157

EN 60601-1-158

EN 60601-1-159

EN 60601-1-160

EN 60601-1-161

EN 60601-1-162

EN 60601-1-163

EN 60601-1-164

EN 60601-1-165

EN 60601-1-166

EN 60601-1-167

EN 60601-1-168

EN 60601-1-169

EN 60601-1-170

EN 60601-1-171

EN 60601-1-172

EN 60601-1-173

EN 60601-1-174

EN 60601-1-175

EN 60601-1-176

EN 60601-1-177

EN 60601-1-178

EN 60601-1-179

EN 60601-1-180

EN 60601-1-181

EN 60601-1-182

EN 60601-1-183

EN 60601-1-184

EN 60601-1-185

EN 60601-1-186

EN 60601-1-187

EN 60601-1-188

EN 60601-1-189

EN 60601-1-190

EN 60601-1-191

EN 60601-1-192

EN 60601-1-193

EN 60601-1-194

EN 60601-1-195

EN 60601-1-196

EN 60601-1-197

EN 60601-1-198

EN 60601-1-199

EN 60601-1-200

EN 60601-1-201

EN 60601-1-202

EN 60601-1-203

EN 60601-1-204

EN 60601-1-205

EN 60601-1-206

EN 60601-1-207

EN 60601-1-208

EN 60601-1-209

EN 60601-1-210

EN 60601-1-211

EN 60601-1-212

EN 60601-1-213

EN 60601-1-214

EN 60601-1-215

EN 60601-1-216

EN 60601-1-217

EN 60601-1-218

EN 60601-1-219

EN 60601-1-220

EN 60601-1-221

EN 60601-1-222

EN 60601-1-223

EN 60601-1-224

EN 60601-1-225

EN 60601-1-226

EN 60601-1-227

EN 60601-1-228

EN 60601-1-229

EN 60601-1-230

EN 60601-1-231

EN 60601-1-232

EN 60601-1-233

EN 60601-1-234

EN 60601-1-235

EN 60601-1-236

EN 60601-1-237

EN 60601-1-238

EN 60601-1-239

EN 60601-1-240

EN 60601-1-241

EN 60601-1-242

EN 60601-1-243

EN 60601-1-244

EN 60601-1-245

EN 60601-1-246

EN 60601-1-247

SONON ULTRASOUND IMAGING SYSTEM

REF SONON 300C

SN H-16100006

2016-10

Healcerion Co., Ltd

804ho, 38-21, Digital-ro 31-gil, Guro-gu, Seoul, Korea

info@healcerion.com

EC REP OBELIS S.A, Bd. Général Wahis,
53 1030 Brussels, Belgium

Operation: Max10min with 10min resting time **Rx Only**

POWER Rechargeable
Li-ion Battery Pack
DC 7.4V --- 2600mAh



Complies with UL60601-1

CSA C22.2 No.60601-1

vs E113904





Сканер SONON 300L







Сканер SONON 300L

SONON ULTRASOUND IMAGING SYSTEM

300L

SN H-17060089

2017-06


Healcerion Co., Ltd

**804ho, 38-21, Digital-ro 31-gil, Guro-gu
Seoul 08376, REPUBLIC OF KOREA**

**EC REP OBELIS S.A, Bd. Général Wahis,
53 1030 Brussets, Belgium**

Operation: Max10min with 10min resting time


**POWER Rechargeable
Li-ion Battery Pack
DC 7.4V --- 2600mAh**



Сканер SONON 300L



Упаковка Системы ультразвукового сканирования SONON

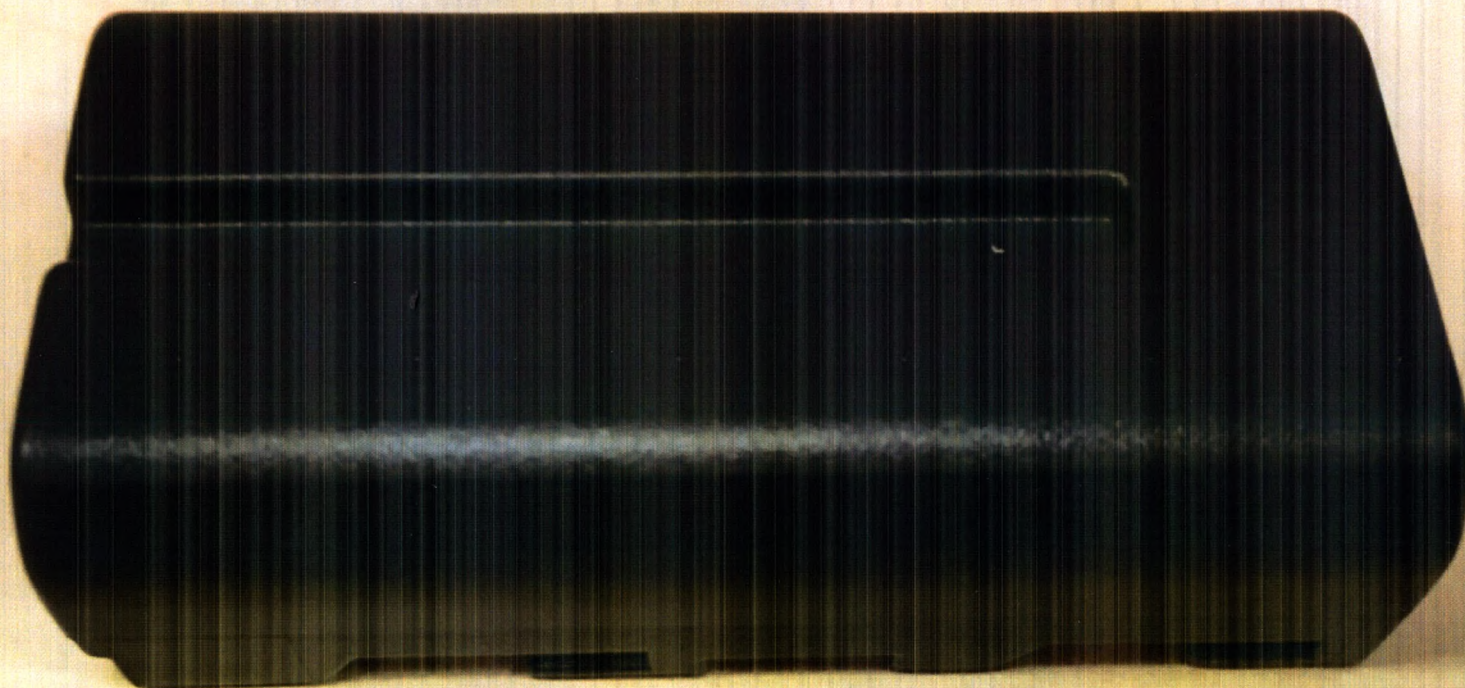


Аккумуляторная батарея



Аккумуляторная батарея



Аккумуляторная батарея

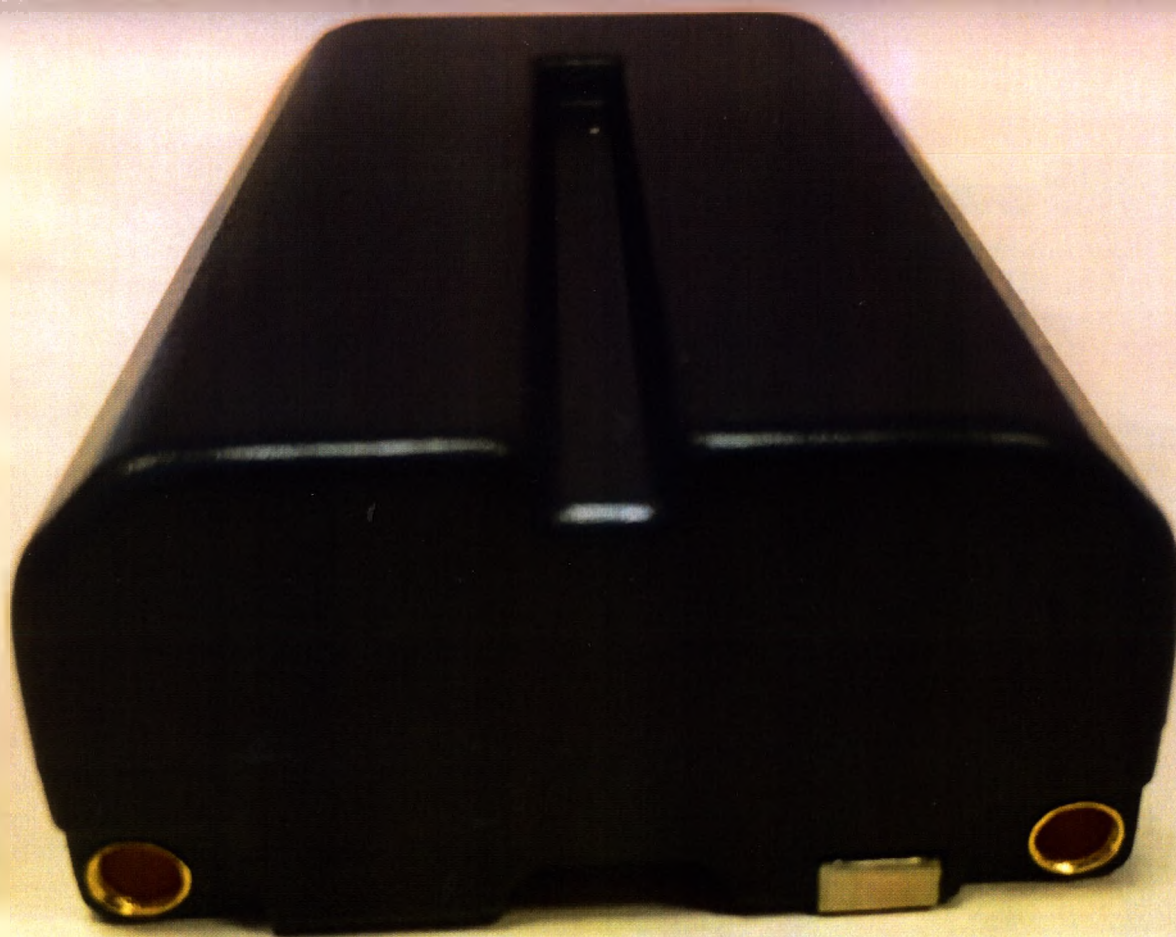

Аккумуляторная батарея



HEALCERION

MODEL : MBP-2S1PSD26

Rechargeable Lithium-ion Battery
DC7.4V $\equiv$ 2600mAh /19.24Wh

Be sure that the power is turned off
when the battery is inserted.

Made in Korea



MH59945



2ICR19/65



ZH12017-13005



MFG. mPLUS Electronics Co.,Ltd.



CAUTION Date : 2016.11


S/N : AK16000813

Replace with batteries which are fit to
standard specification provided by only
manufacturing company.

To reduce the risk of explosion, do not
disassemble, and avoid flame or watery
material in disposing of batteries.

Recycle or dispose of used batteries
should be processed as stipulated by
local regulations.


Аккумуляторная батарея

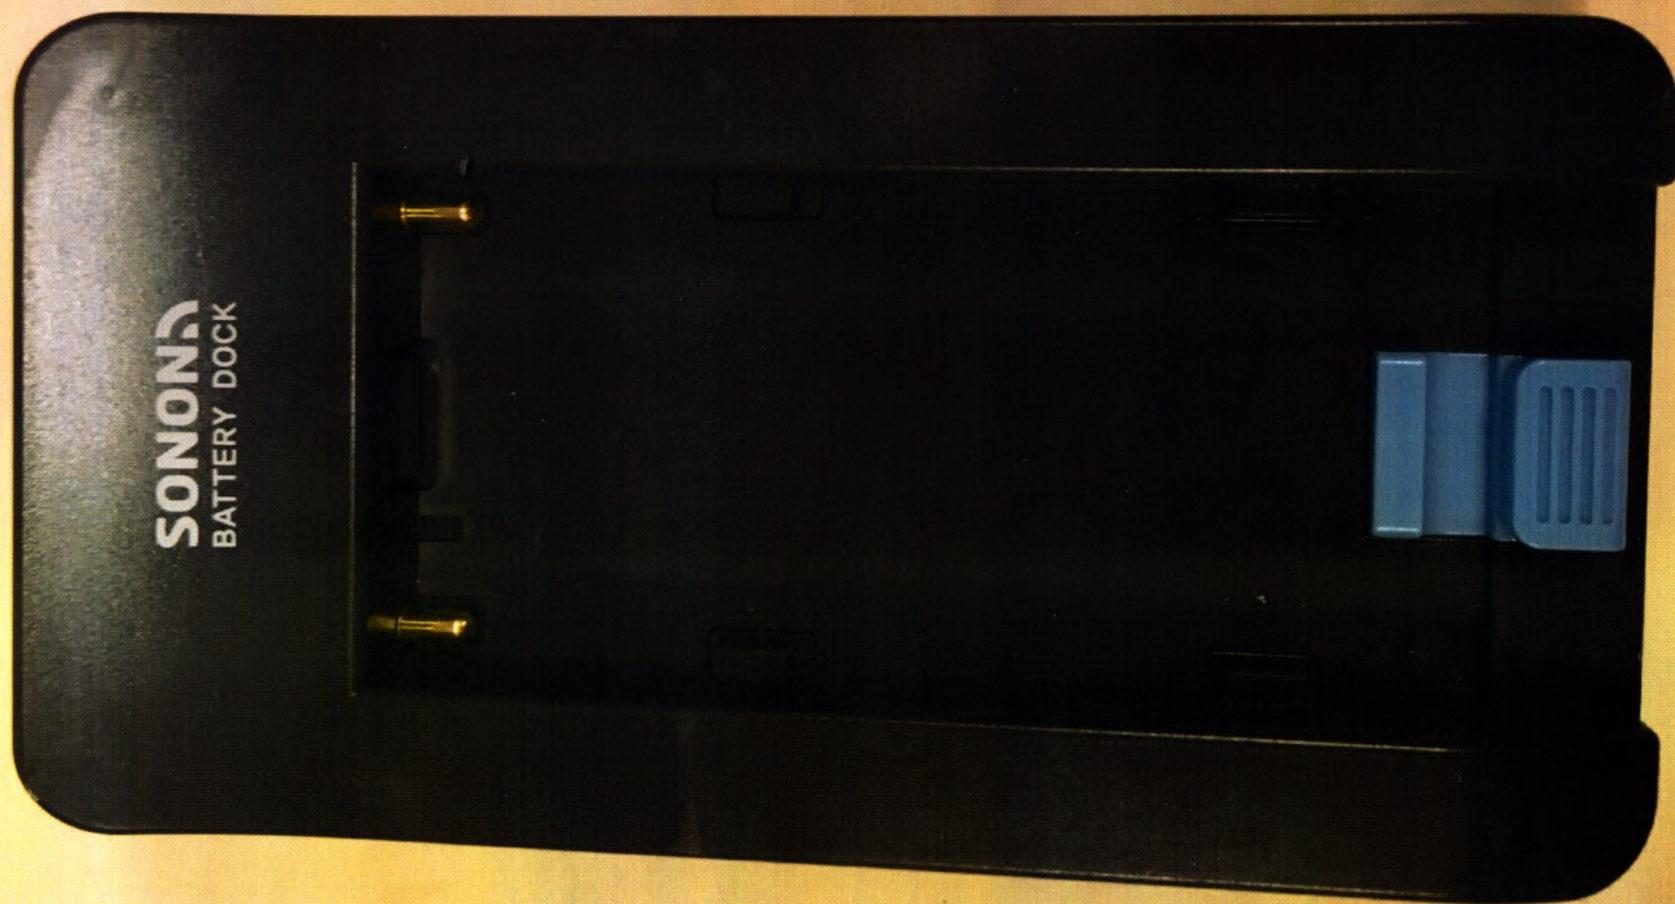

Зарядное устройство SONON



Зарядное устройство SONON

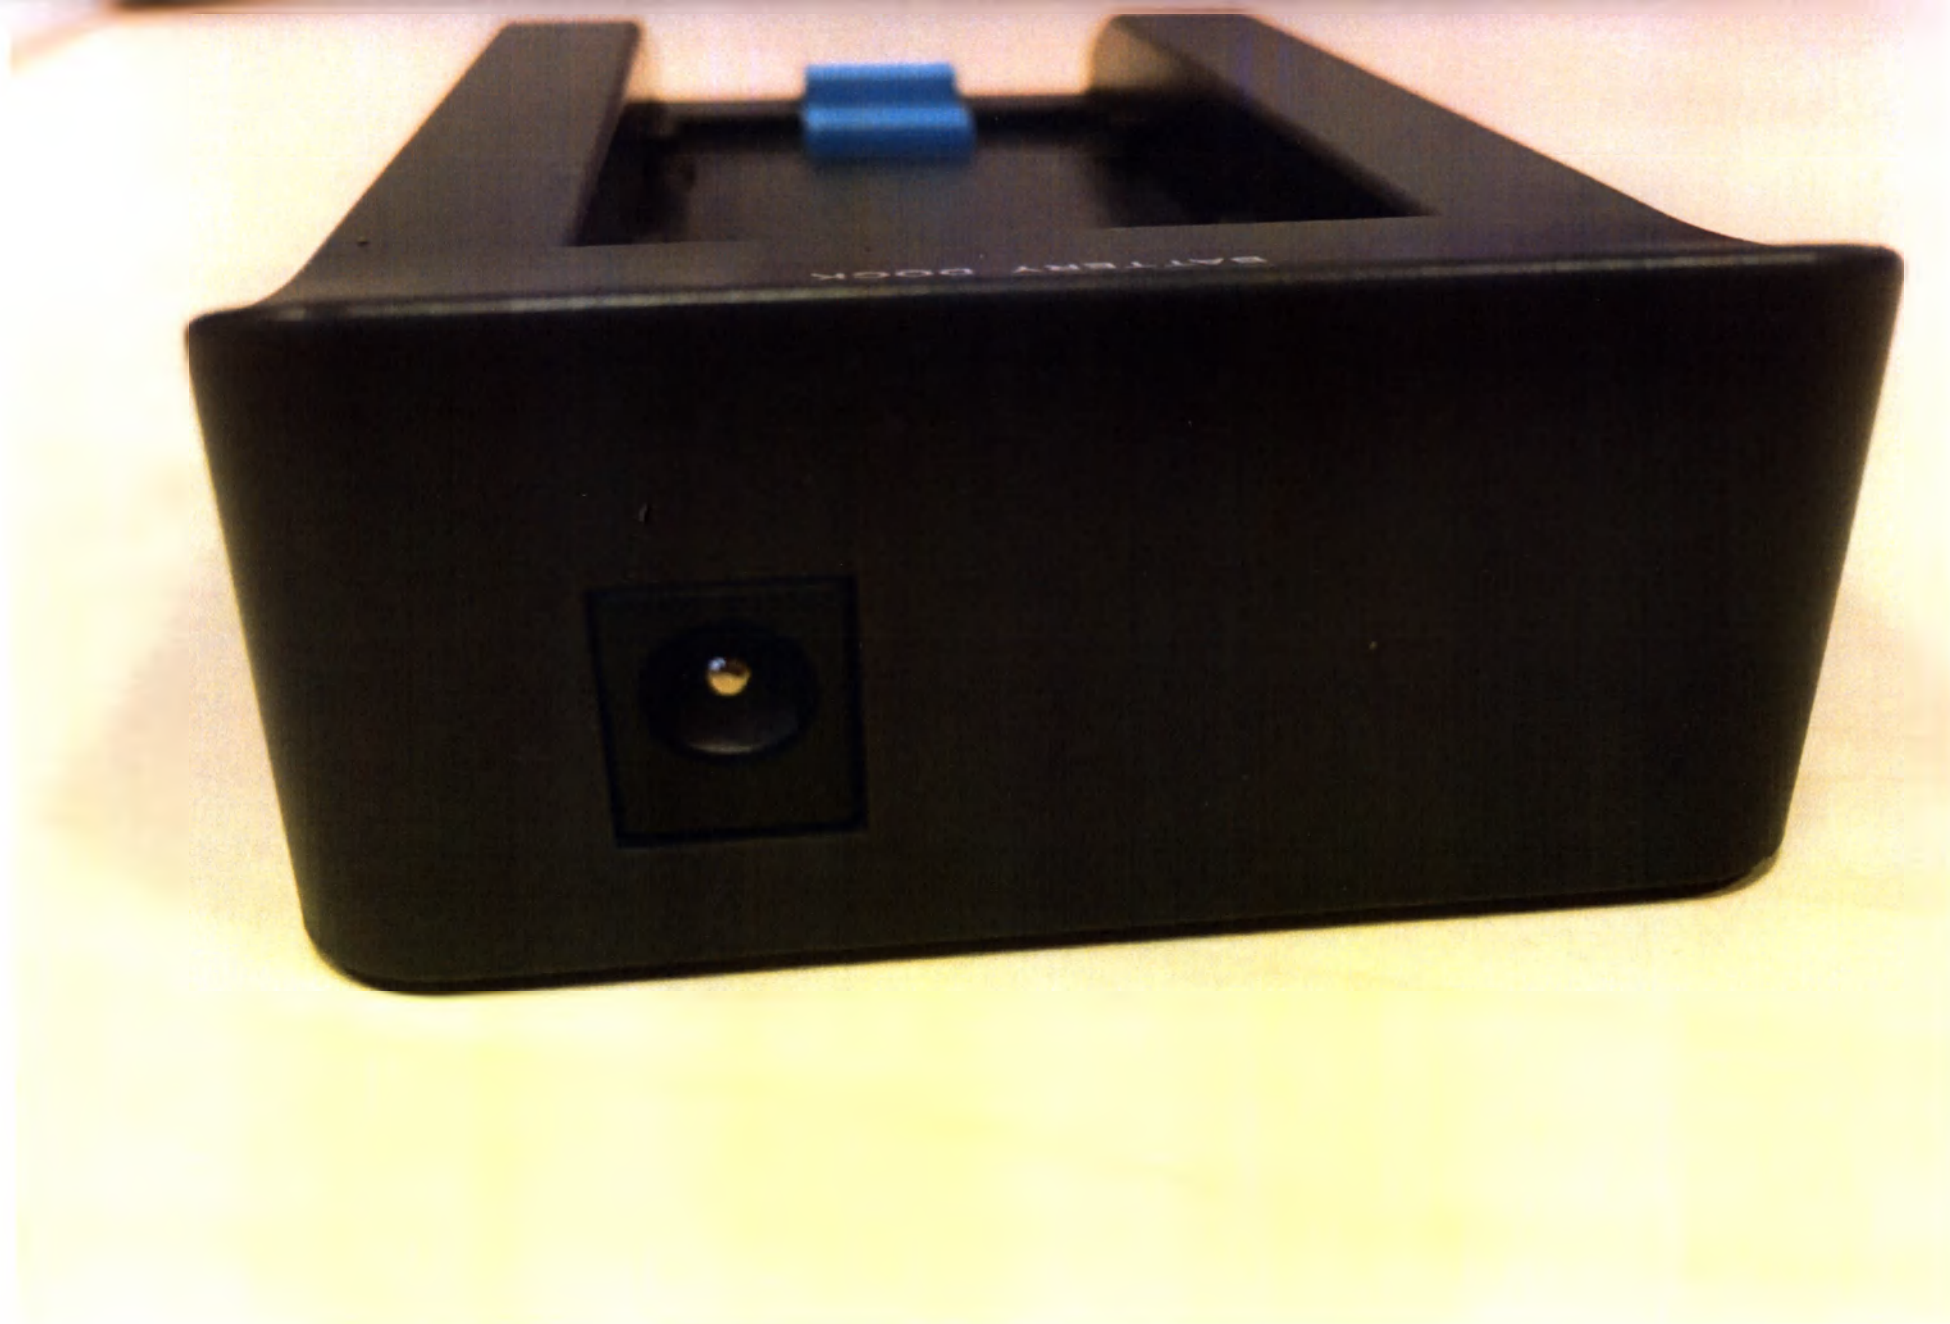

Зарядное устройство SONON

Зарядное устройство SONON



MADE IN KOREA

Model : DOCK 300C

Input Power : DC8.4V $\approx$ 1.5A

Output Power : DC8.4V $\approx$ 1.5A

Healcerion Co., Ltd

804ho, 38-21, Digital-ro 31-gil, Guro-gu,
Seoul, 08376, REPUBLIC of KOREA

TEL : +82-70-7582-6326



17060067



- 7. Select the power supply cord that is listed by country and suitable for country regulation.
- 8. Locate near an area accessible to a properly grounded outlet receptacle.
- 9. This battery charger is for use only with the battery types and ratings indicated on the base of the unit. Any other application may cause fire or damage.
- 10. The outlet shall be installed near the equipment and shall be easily accessible.

680 - 5044 REV. C



Charger Adaptor



SONON
Wireless Mobile Ultrasound Device



WIDE RANGE BATTERY CHARGER

INSTALLATION INSTRUCTION


1. This product is intended for indoor use only.
2. Not protected against the ingress of water.
3. Need to be protected from excessive force or shock.
4. Do not pull output plug with excessive force.
5. No user serviceable part inside.
6. Use only rated input and output range which indicated on the bottom of the equipment.
7. Select the power supply cord that is listed by country and suitable for country regulation.
8. Locate near an area accessible to a properly grounded outlet receptacle.
9. This battery charger is for use only with the battery types and ratings as indicated on the base of the unit. Any other application may cause injury or damage.
10. The socket-outlet shall be installed near the equipment and shall be easily accessible.

680 - 5044 REV. C

Адаптер переменного тока для зарядного устройства SONON



Адаптер переменного тока для зарядного устройства SONON

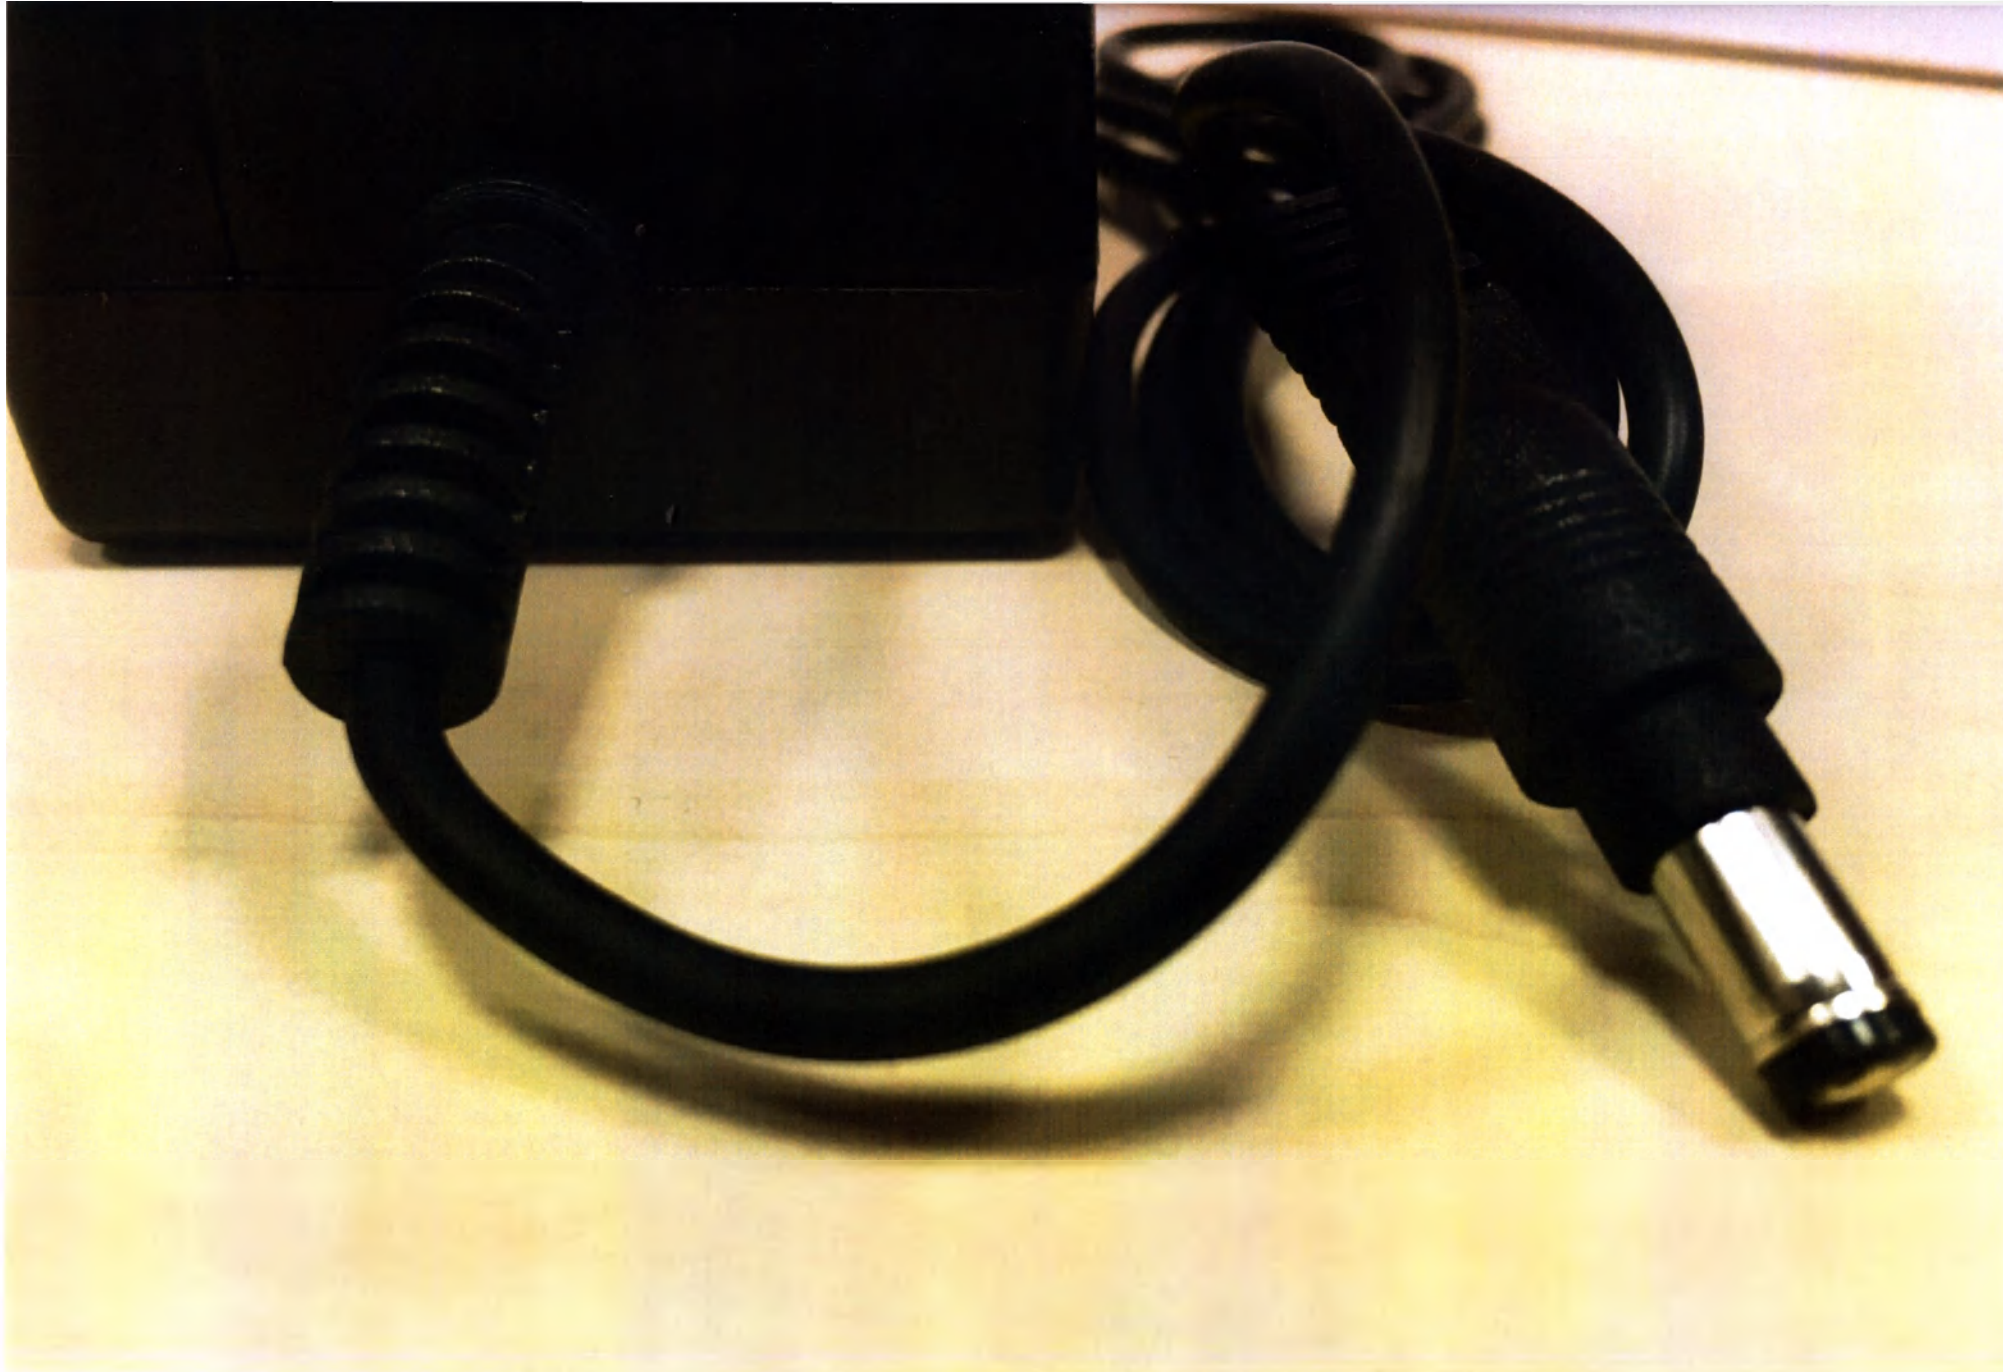



Адаптер переменного тока для зарядного устройства SONON



Шнур питания



Шнур питания

Шнур питания





Адаптер сетевой для SONON

I. T. E. POWER SUPPLY

직류전원장치

MODEL BPI010S05N07

INPUT : 100-240 V~, 50-60 Hz, 0.3 A

OUTPUT : +5 V $\equiv$, 2.0 A




LISTED

31KG

E300305

I.T.E. POWER SUPPLY



모델명 : BPI010S05N07

최저소비효율기준 만족제품

KTL SU10316-11011



Indoor, Dry
Location
Use Only



Refer To
Instructions



Double
Insulated



DATE CODE

C 1725 / REV A / RoHS

BridgePower Corp.

MANUFACTURED BY Wendeng Jeil Electronics

CUSTOMER SERVICE NO.: 82-31-299-1234

MADE IN CHINA

Адаптер сетевой для SONON




Адаптер сетевой для SONON



Адаптер сетевой для SONON



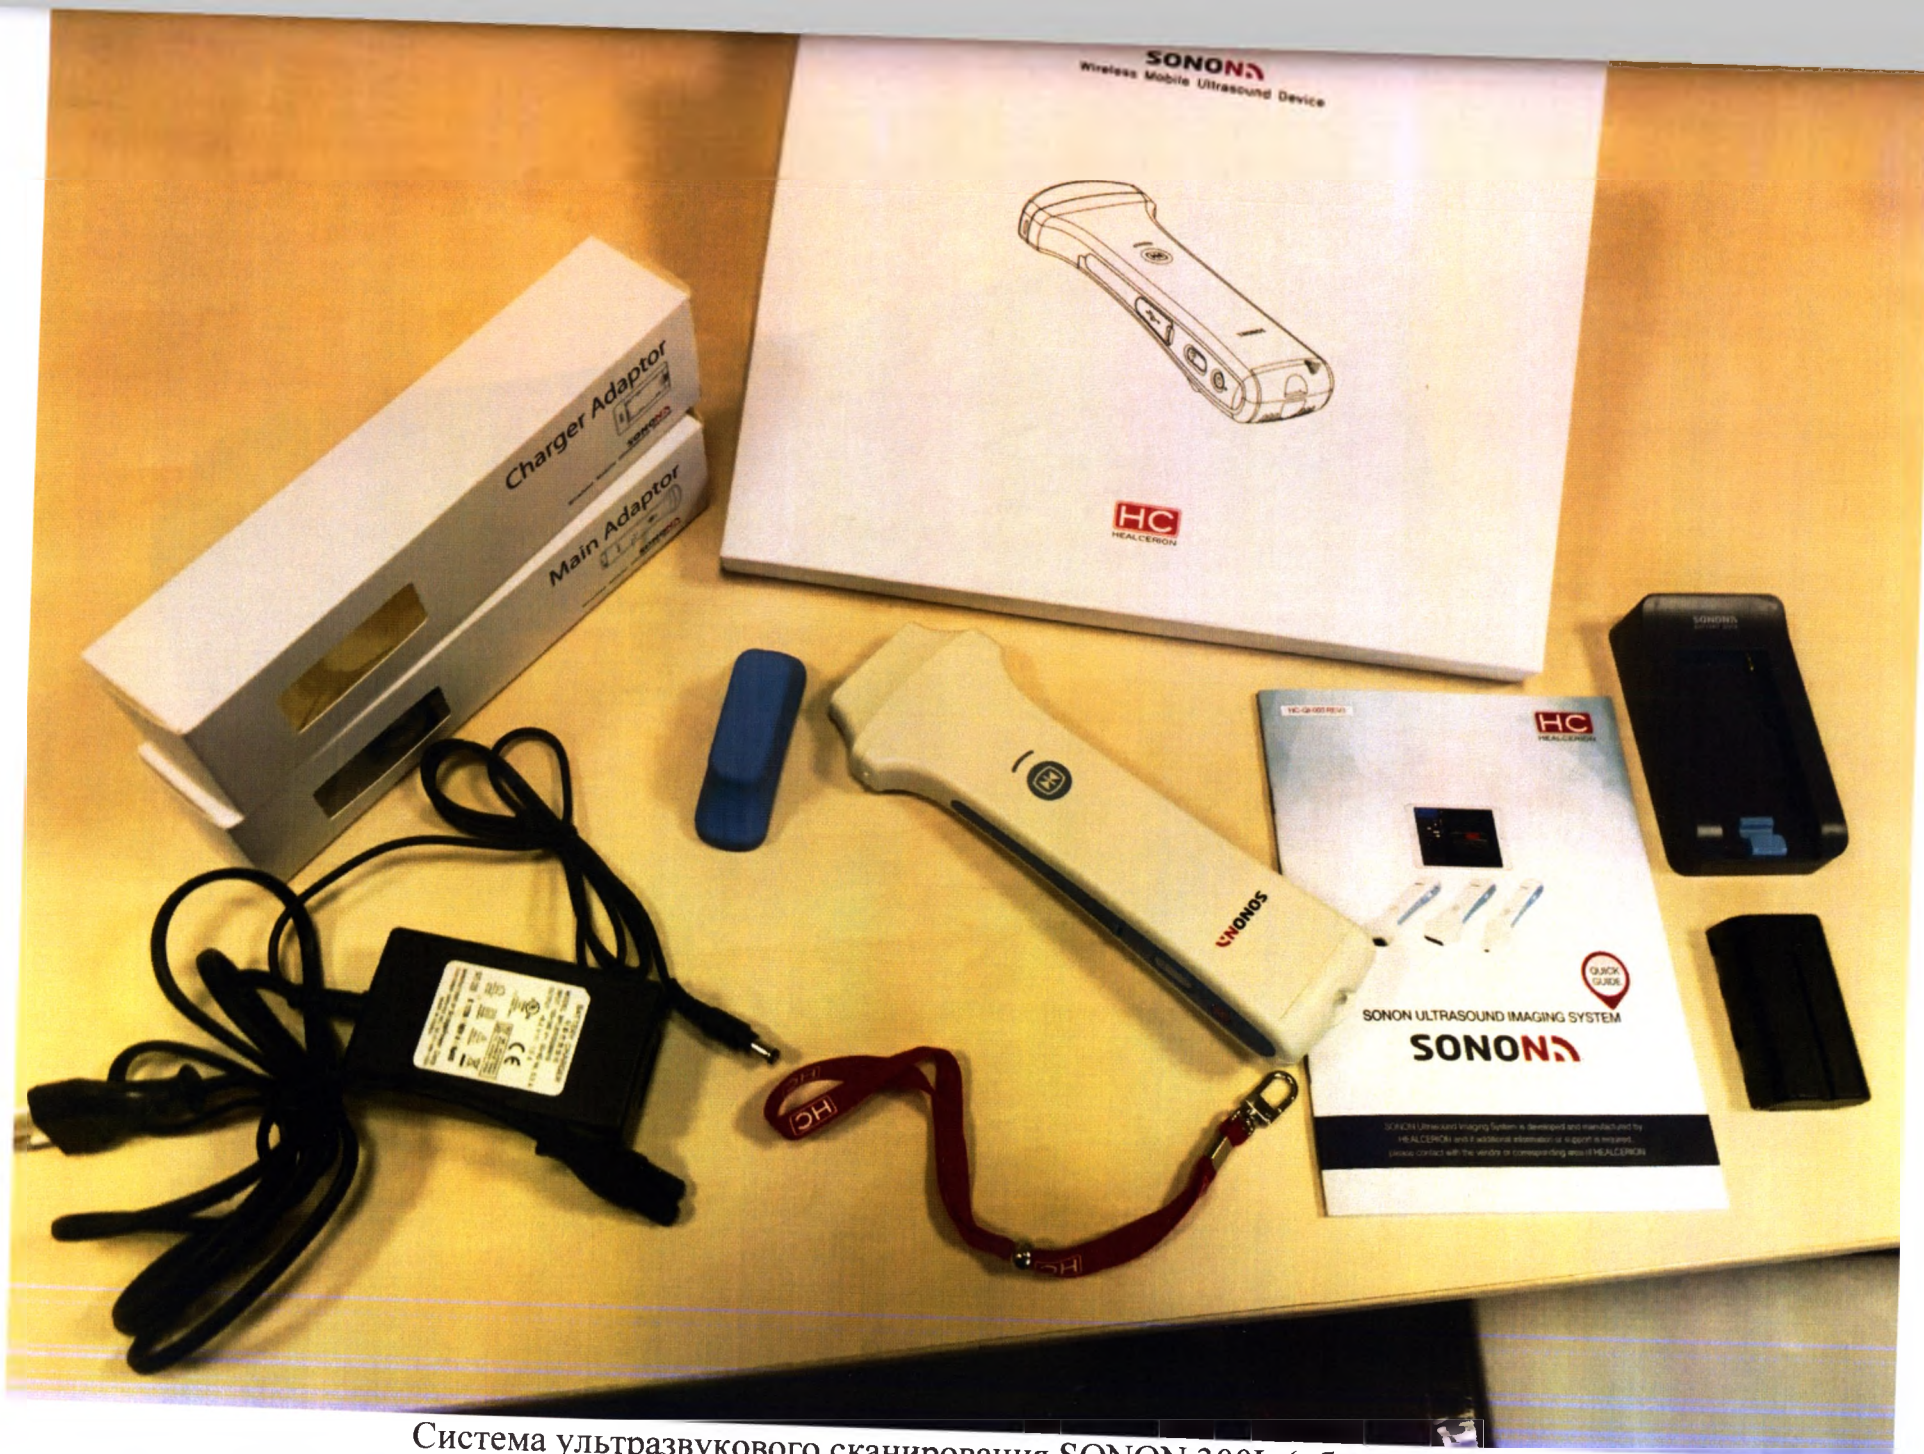


Система ультразвукового сканирования SONON 300L (общий вид)







Крепление для SONON

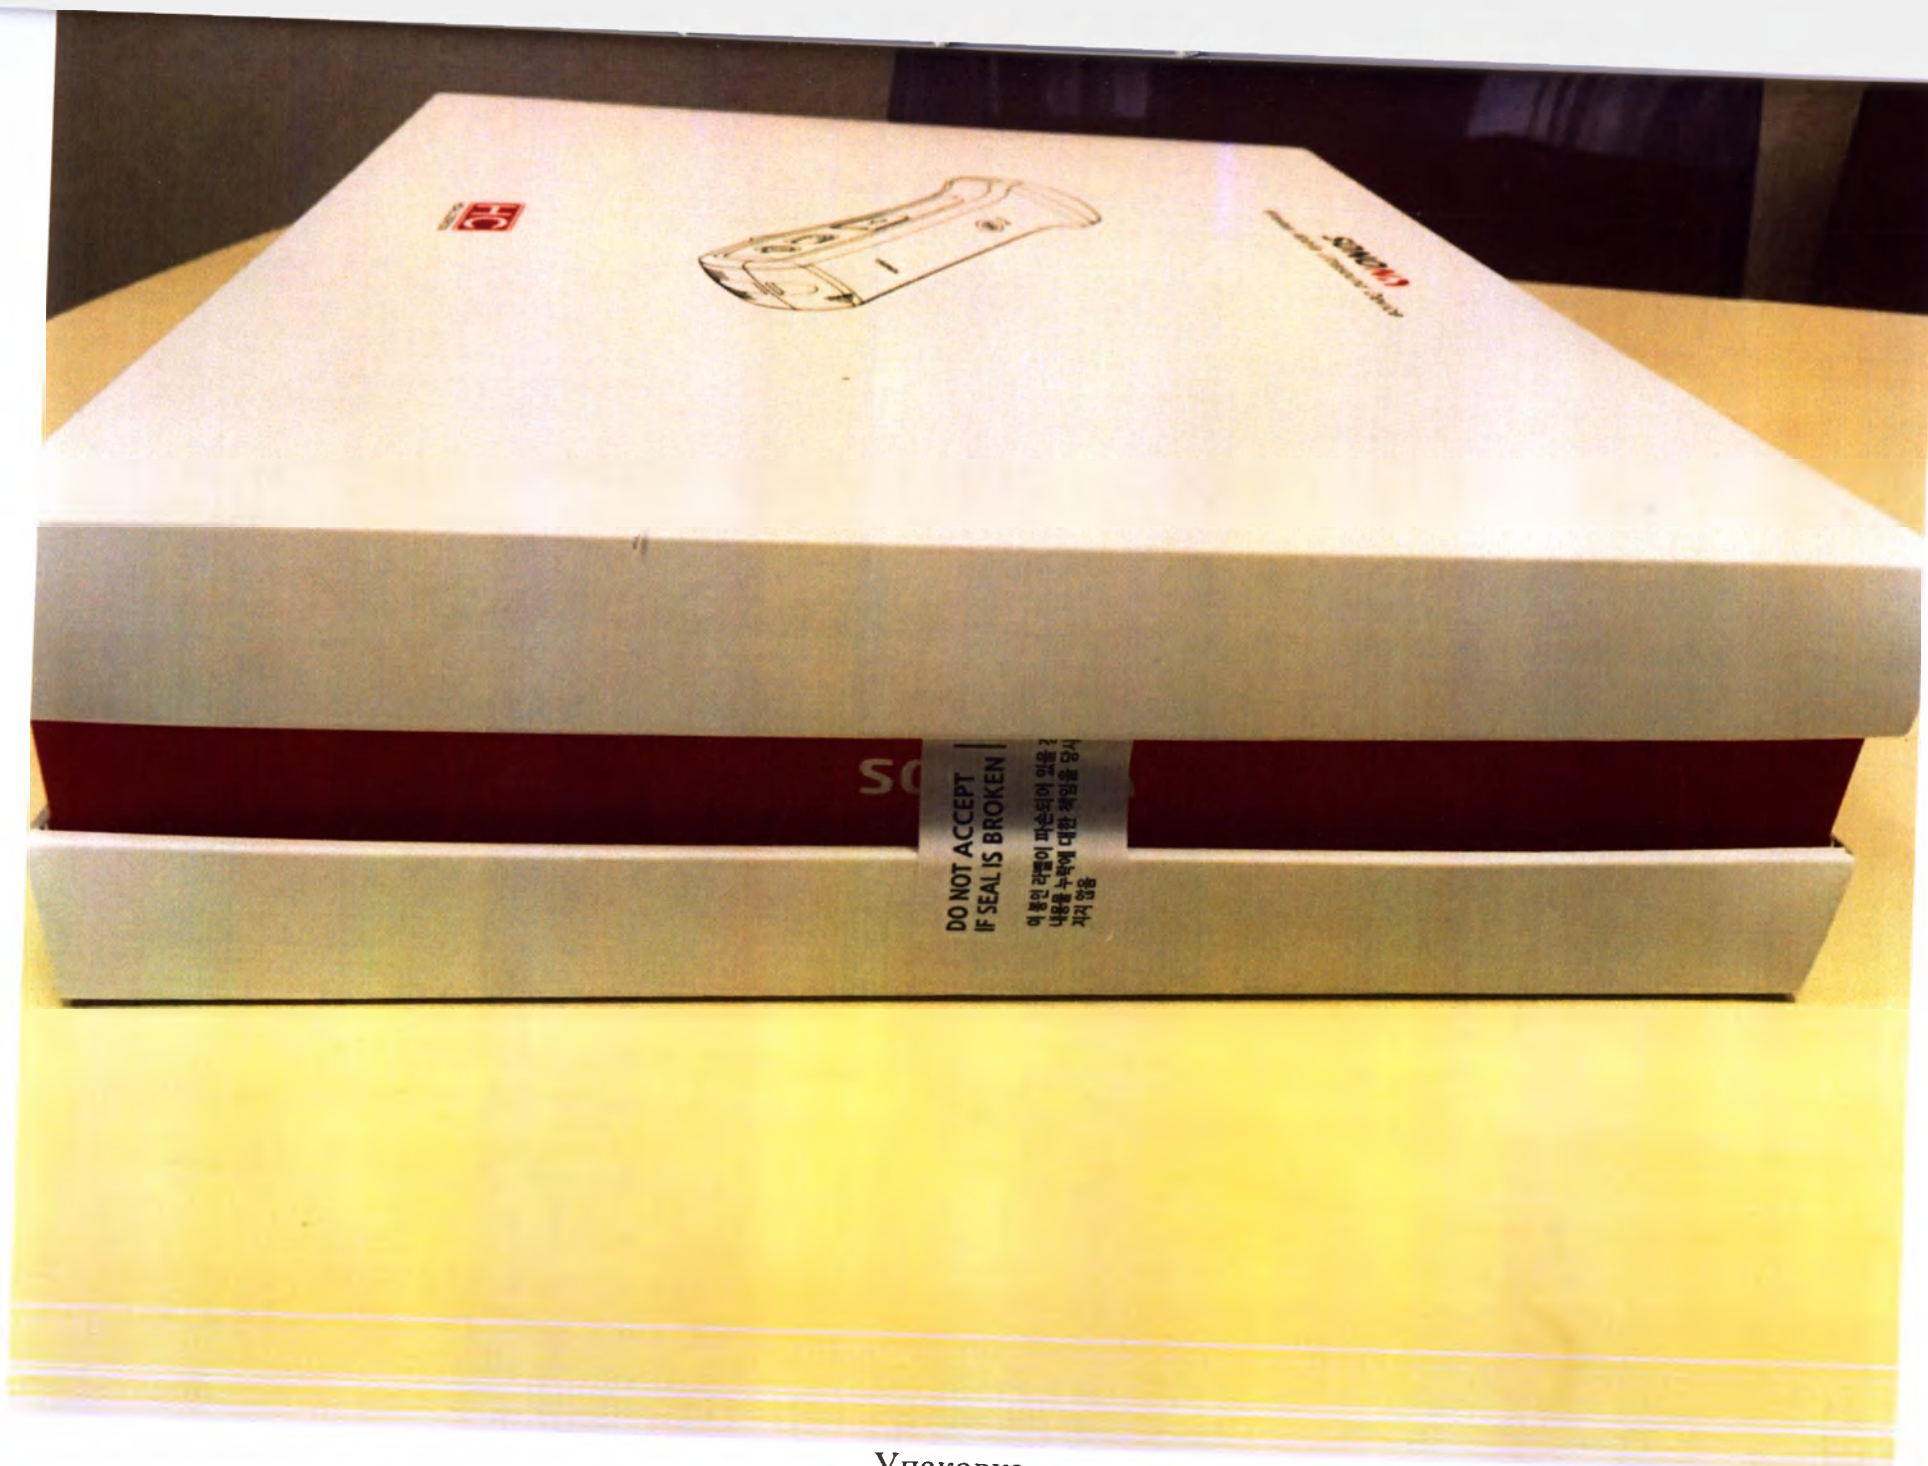

Упаковка



SONON ULTRASOUND IMAGING SYSTEM

CE 0123
Made in Korea



SONON 300C



H-16100006




2016-10



Healcerion Co., Ltd

804ho, 38-21, Digital-ro 31-gil, Guro-gu, Seoul, Korea



OBELIS S.A, Bd. Général Wahis, 53 1030 Brussels, Belgium

POWER Rechargeable Li-ion Battery

DC 7.4V  2600mAh

Operation: Max10min with 10min resting time



Rx Only



SONON ULTRASOUND IMAGING SYSTEM

CE 0123
Made in Korea

REF 300L


SN H-17060089

2017-06



Healcerion Co., Ltd

804ho, 38-21, Digital-ro 31-gil, Guro-gu, Seoul, 08376, REPUBLIC of KOREA



OBELIS S.A, Bd. Général Wahis, 53 1030 Brussels, Belgium

POWER Rechargeable Li-ion Battery

DC 7.4V, 2600mAh

Operation: Max 10min with 10min resting time



Rx Only

Пронумеровано, прошито и
скреплено печатью

43 (Соловьев) лист (12)

М.П.

(Шемят А.А.)

Расшифровка подписи