

Фотографические изображения медицинского изделия

Степлер циркулярный в вариантах исполнения

Производства

**Jiangsu Brightness Medical Devices Co., Ltd
*No. 66, Heshuan Road, Zhonglou Economic, Development Area,
Changzhou 213013, China***




Disposable Circular Stapler

CE 0197

REF

- | | |
|------|-------------------------------------|
| DH17 | ☐ |
| DH19 | ☐ |
| DH21 | ☐ |
| DH24 | ☐ |
| DH26 | ☐ |
| DH29 | ☐ |
| DH32 | ☒ |
| DH34 | ☐ |

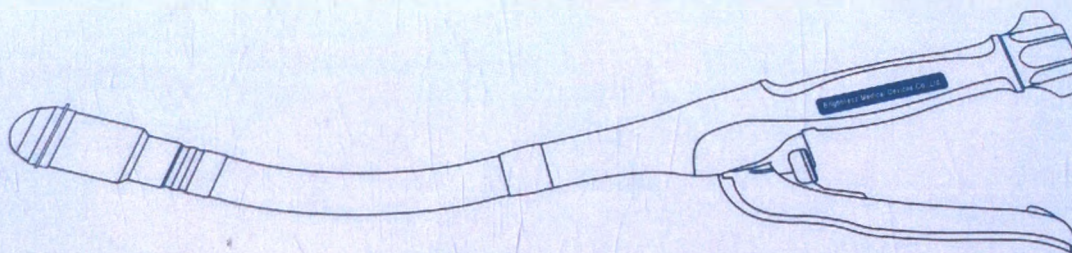

Disposable Circular Stapler
Suturatrice circolare monouso
Einweg Zirkular Stapler
la circulaire disponible d'agrafeuse
Disposable Circulaire Stapler
GRAPADORA CIRCULAR DESECHABLE
Agrafador Circular Descartável



STERILE EO



DH17
DH19

DH21
DH24
DH26

DH29
DH32
DH34



Brightness

Disposable Circular Stapler

LOT

18110FG210



20181101



20231031



INSTRUCTIONS FOR USE

DH

Model DH Curved Stapler
Circular Stapler with implantable titanium staples

REF	DH-17	DH-24	DH-32
	DH-19	DH-26	DH-34
	DH-21	DH-29	

CC certifies the Product from their Technical Data sheet.

Check the supplier on their Features

[illegible]

Read instructions carefully prior to use.



Standard using Ethernet Cable
 Monthly guaranteed internet package speeds to 10Mbps



Simple and easy.




Удлиняющий держатель



Disposable Circular Stapler

CE 0197

REF	
DH17	☐
DH19	☐
DH21	☒
DH24	☐
DH26	☐
DH29	☐
DH32	☐
DH34	☐

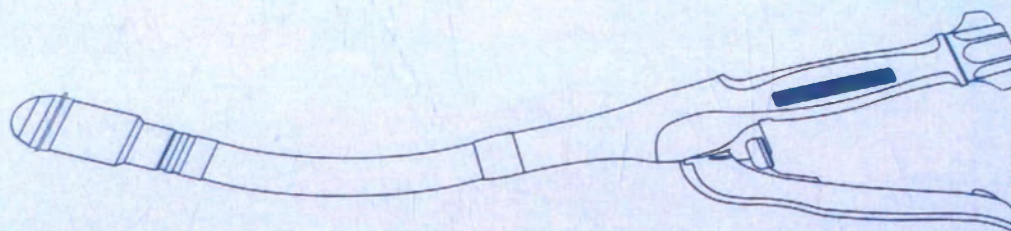

STERILE EO



Disposable Circular Stapler
Suturatrice circolare monouso
Einweg Zirkular Stapler
la circulaire disponible d'agrafeuse
Disposable Circulaire Stapler
GRAPADORA CIRCULAR DESECHABLE
Agrafador Circular Descartável

DH17
DH19

DH21
DH24
DH26

DH29
DH32
DH34

021

ер циркулярный D (DП-21)



Brightness

Disposable Circular Stapler

LOT

18110K2110



20181101



20231031



INSTRUCTIONS FOR USE

H

Model DH Curved Stapler
Circular Stapler with Implantable Titanium Staples

REF

04-17 04-24 04-32
04-19 04-26 04-34
04-21 04-28 04-36

100% Satisfaction
 24/7 Support
 100% Satisfaction

1800 800-451-1111
 1800 800-451-1111
 1800 800-451-1111

Best of the South and Southeast

[illegible]

1

100

11



дер циркулярный ДН (ДН-21)



Brightness Circular Stapler 21mm



Удлиняющий держатель



Disposable Double-handle Circular Stapler


CE 0197

REF

- SGH17 ☐
- SGH19 ☐
- SGH21 ☐
- SGH24 ☐
- SGH26 ☐
- SGH29 ☐
- SGH32 ☒
- SGH34 ☐



STERILE EO

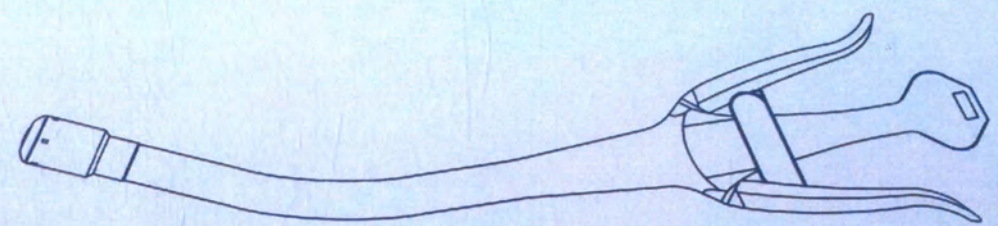

SGH17 ☐
SGH19 ☐

SGH21 ☐
SGH24 ☐
SGH26 ☐

SGH29 ☐
SGH32 ☒
SGH34 ☐



Ø32

Стapлер циркулярный ДН (SGH-32)



Disposable Double-handle Circular Stapler

LOT

1811SH3210



20181101



20231031

Φ32



(Notes)
Full the products in response, trying and also determine their safe. No liability.

ADD
FAX
CE 0197

Jiangsu Brightness Medical Devices Co., Ltd.
No. 88 Huaihai Road Zhongshan Economic Development Area,
Cangshan, Suzhou 215131 China

Mingqi Limited
Add: 211 Fuzhou Road, Suzhou, China
Tel: +86 512 2988460
Fax: +86 512 2988460
E-mail: info@mingqi.com
Website: www.mingqi.com

Модернизация (СН 32)



Удлиняющий держатель

инструкция по применению

Инструкция по применению

Степлер циркулярный в вариантах исполнения



Disposable Double-handle Circular Stapler

CE 0197

REF

- SGH17 ☐
- SGH19 ☐
- SGH21 ☐
- SGH24 ☐
- SGH26 ☒
- SGH29 ☐
- SGH32 ☐
- SGH34 ☐



STERILE EO





Brightness

Disposable Double-handle Circular Stapler

LOT

1811942610



20181101



20231031

[illegible]

Instruction of Disposable Double-Handle Circular Stapler

[Product Name] Disposable Double-Handle Circular Stapler
[Product Specification] SGH26 (10, 20, 24, 26, 28, 32, M)
[Main Technical Index]

Disposable Double-Handle Circular Stapler is equipped by shell, cartridge, shaft, active handle, safety button, adjusting handle, spring, mating ring and connection tube. Modelist: small and round body are made by ABS (polyacrylonitrile-butadiene-styrene), adjusting handle and most of cartridge are made by PA or YAL. Chamber Double Handle New gunst feature available. Connects a cross and/or 3 (4) tips. Its leakage and safety. Safety release should be done enough. Lock system should be opened and closed freely. Keep use safety. The spring should be elastic enough, and can release after compression. Anesthesia connection tube is used to protect the shaft during using the device and it is made by polypropylene.




1. Shell
2. Cartridge
3. Shaft
4. Safety Button
5. Active handle
6. Adjusting handle
7. Safety Release

[Application]
Used in the surgical operation of small organs, stomach and intestine.

[Usage]
Disposable double-handle circular stapler is single use only, open the sterile package and take it out, rotate the active handle anticlockwise, or clockwise to lock and off.



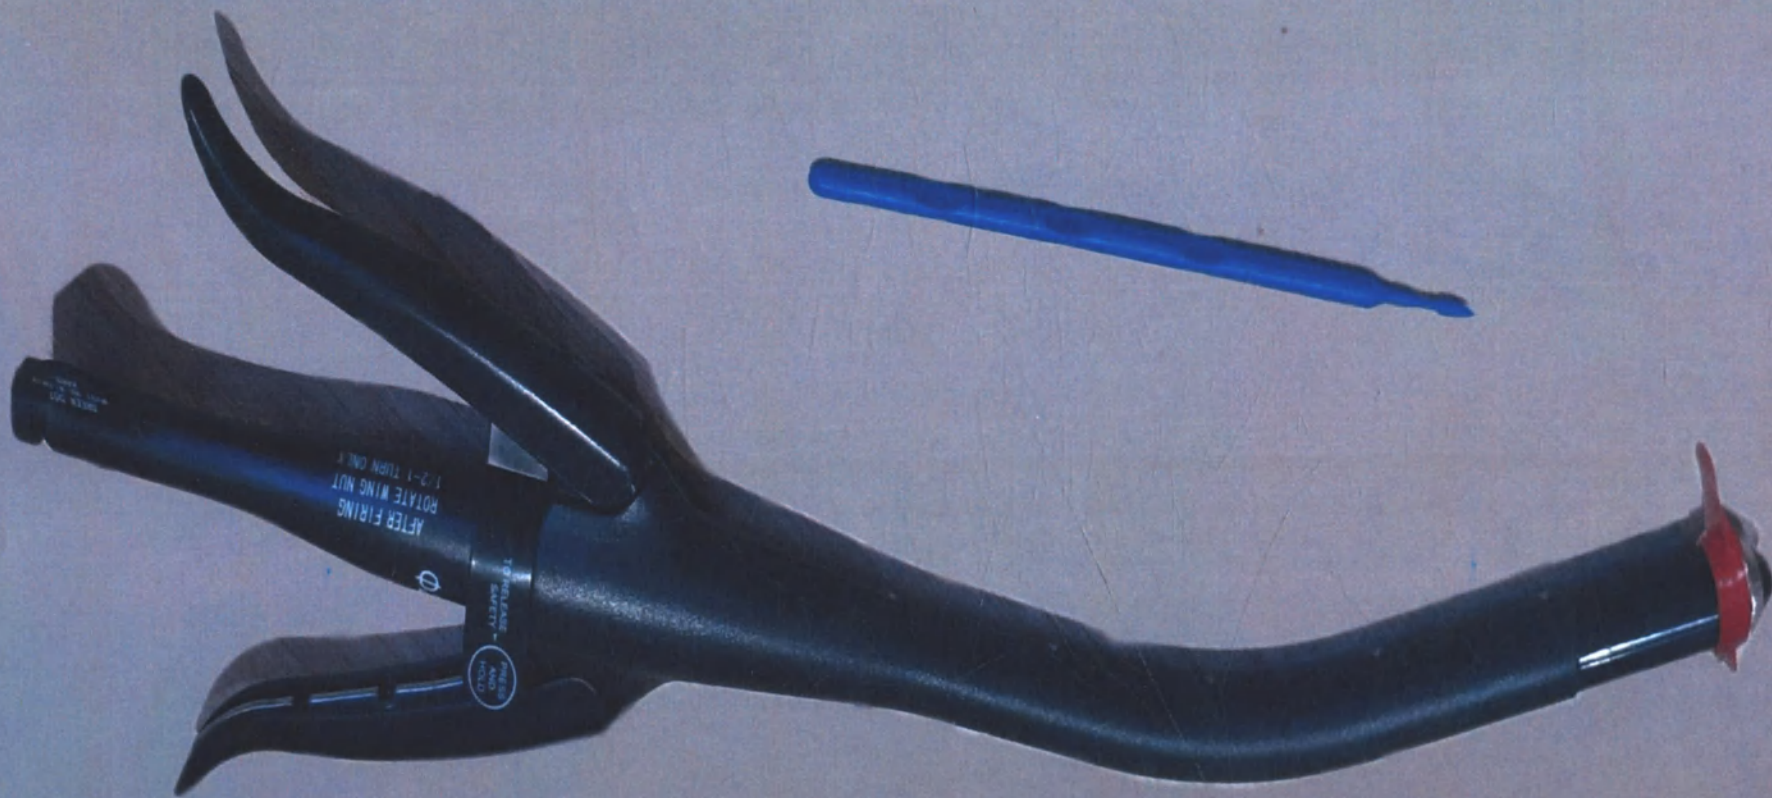

циркулярный ДП (SGH-21)



Disposable Double-handle Circular Stapler

CE 0197

REF

- SGH17 ☐
- SGH19 ☐
- SGH21 ☒
- SGH24 ☐
- SGH26 ☐
- SGH29 ☐
- SGH32 ☐
- SGH34 ☐



STERILE EO

2

SGH17 ☐
SGH19 ☐

SGH21 ☒
SGH24 ☐
SGH26 ☐

SGH29 ☐
SGH32 ☐
SGH34 ☐



Disposable Double-handle Circular Stapler

LOT

1811S/2110



20181101



20231031

Φ21

Instruction of Disposable Double-Handle Circular Stapler

[Product Name] Disposable Double-Handle Circular Stapler
[Product Specification] SGH1716, 21, 24, 26, 28, 32, 34

[Main Technical Index]

Disposable Double-Handle Circular Stapler is constituted by work cartridge, shaft, active handle, safety button, adjusting handle, round knife, stapler, cutting ring and connection tube. Material shell and round knife are made by 30Cr19Ni10 stainless steel, active handle, safety button, adjusting handle and end of cartridge are made by ABS plastic, connection tube is made by polypropylene, staples are made by TAI or TAI. Character: Stapler should have good sealing property. Clearness stress reinforced 3.8Mpa. No leakage and leak: index window should be clear enough. Lock system should be correct and closed tightly. Some use safety: The spring should be elastic enough, and it can operate after compression. Hold-down, connection rate is used to prevent the pinching during making the purse, and it is made by polypropylene.



1. Shaft
2. Cartridge
3. Shell
4. Safety button
5. Active handle
6. Adjusting handle
7. Safety shield

[Application]

Used in the surgical operation of oesophagus, stomach and duodenum.


[Usage]

Disposable double handle circular stapler is single use only. Open the sterile package and take it out, rotate the active handle anticlockwise, in order to take the shell off.



Бер циркулярный ДН (SGH-21)

[illegible]

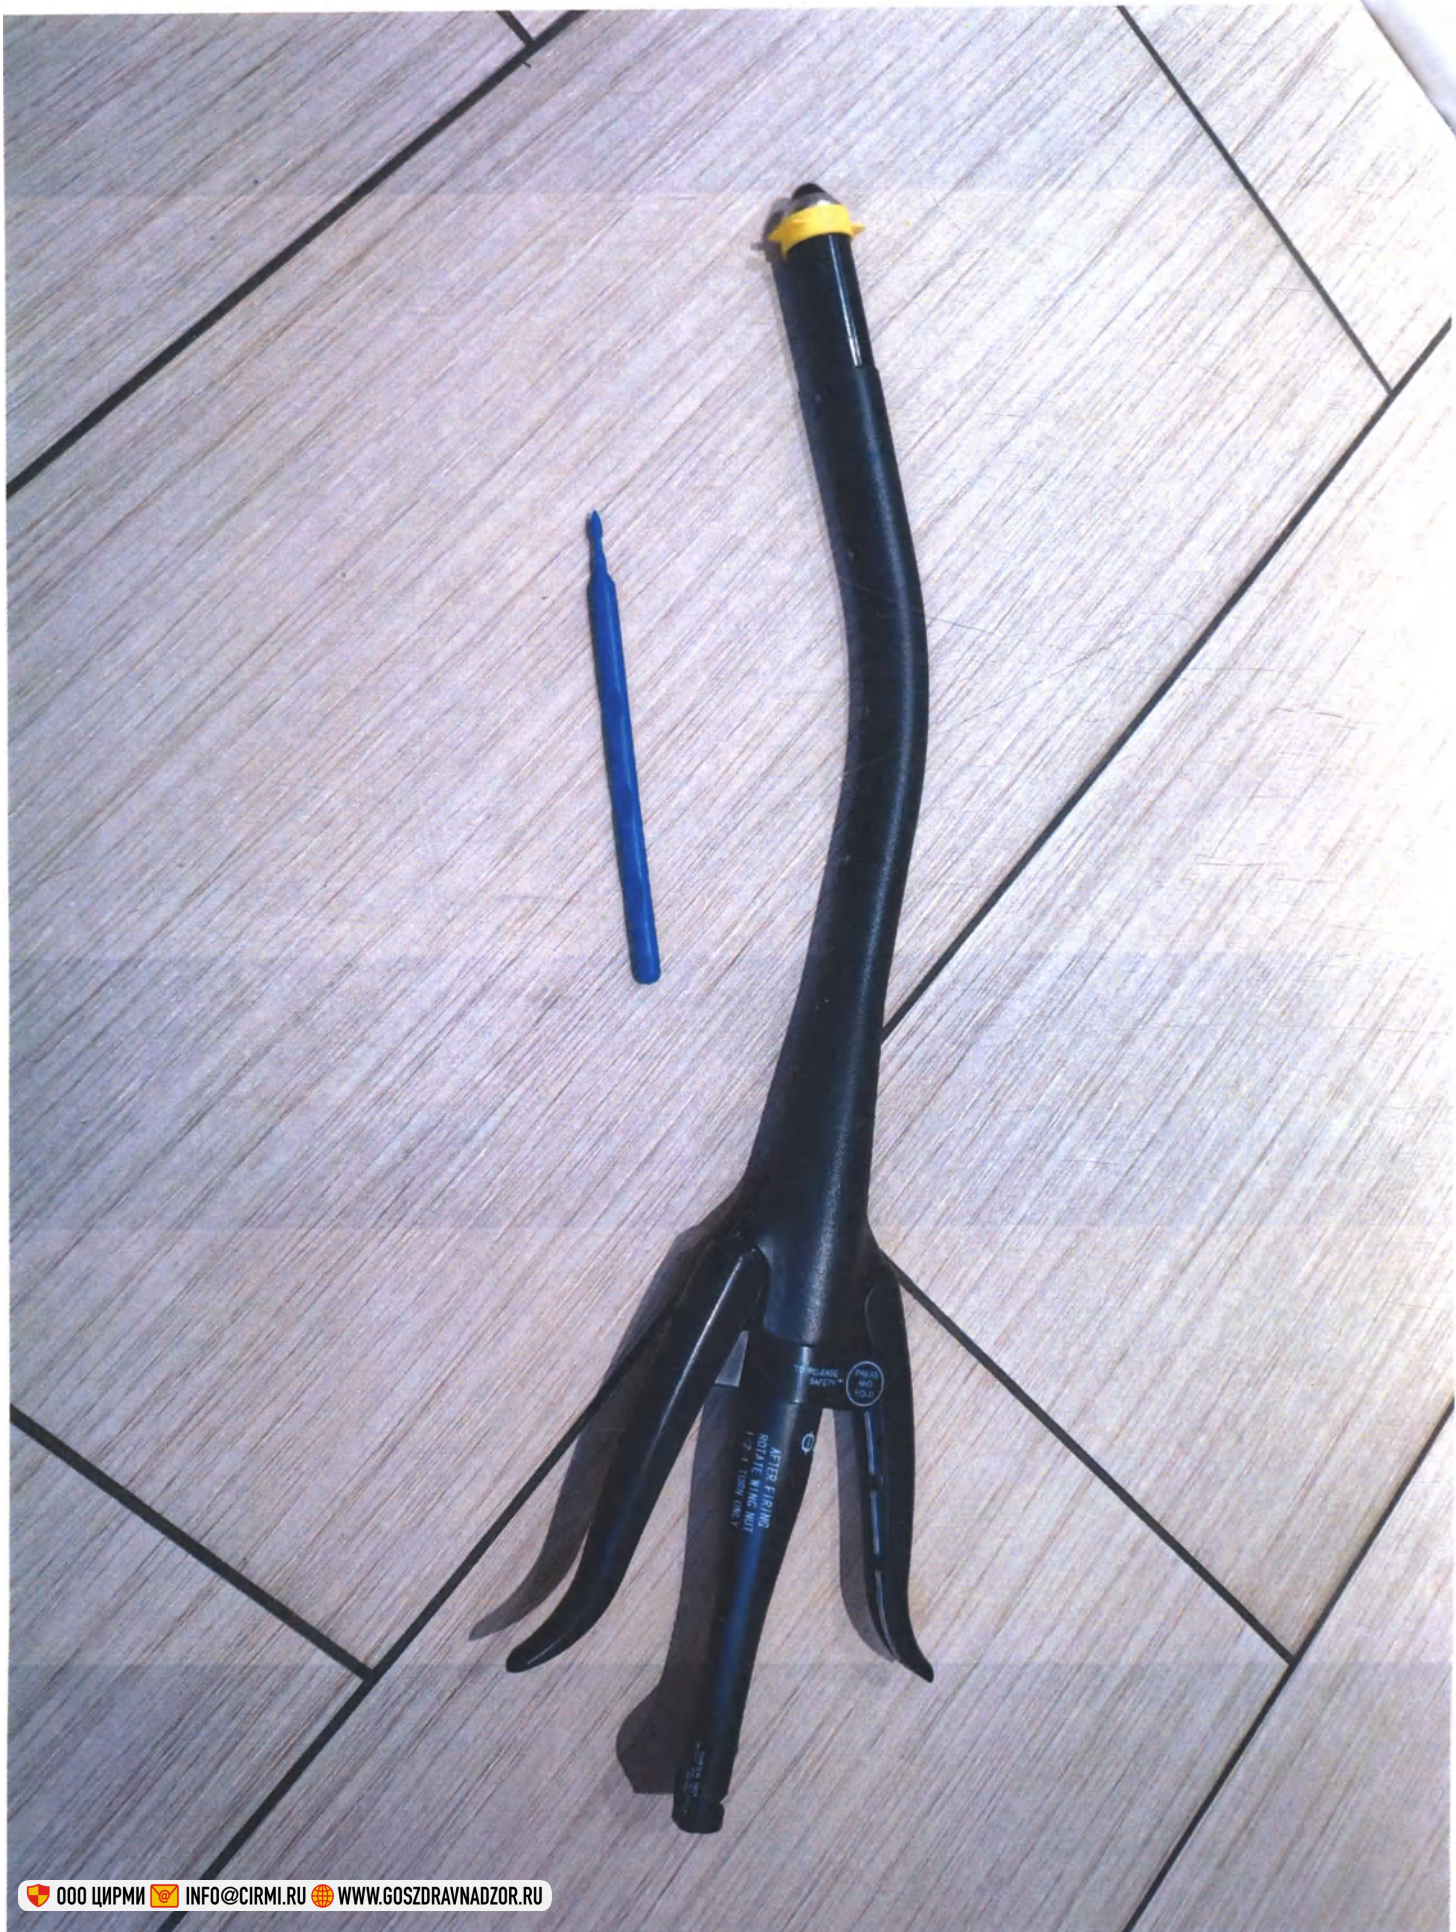

Инструкция по применению

Степлер циркулярный в вариантах исполнения

ПРОШИТО
Листов 26

