

**«УТВЕРЖДАЮ»**

Директор

ООО «Ортус-МС»

Я.Ю. Макаров

2019 г.



**ФОТОГРАФИЧЕСКИЕ ИЗОБРАЖЕНИЯ МЕДИЦИНСКОГО ИЗДЕЛИЯ:**

«Анализатор зрительной функции iTrace, с принадлежностями»

**Производства:**


Tracey Technologies Corporation (Трейси Текнолоджиз Корпорейшн), 16720 Hedgecroft Drive, Houston, TX, 77060, USA (16720 Хеджкрофт-Драйв, г. Хьюстон, штат Техас, 77060 США)

# **I. Анализатор зрительной функции iTrace, в составе:**

## **1. Блок сбора данных (БСД);**



## 2. Програмное обеспечение;

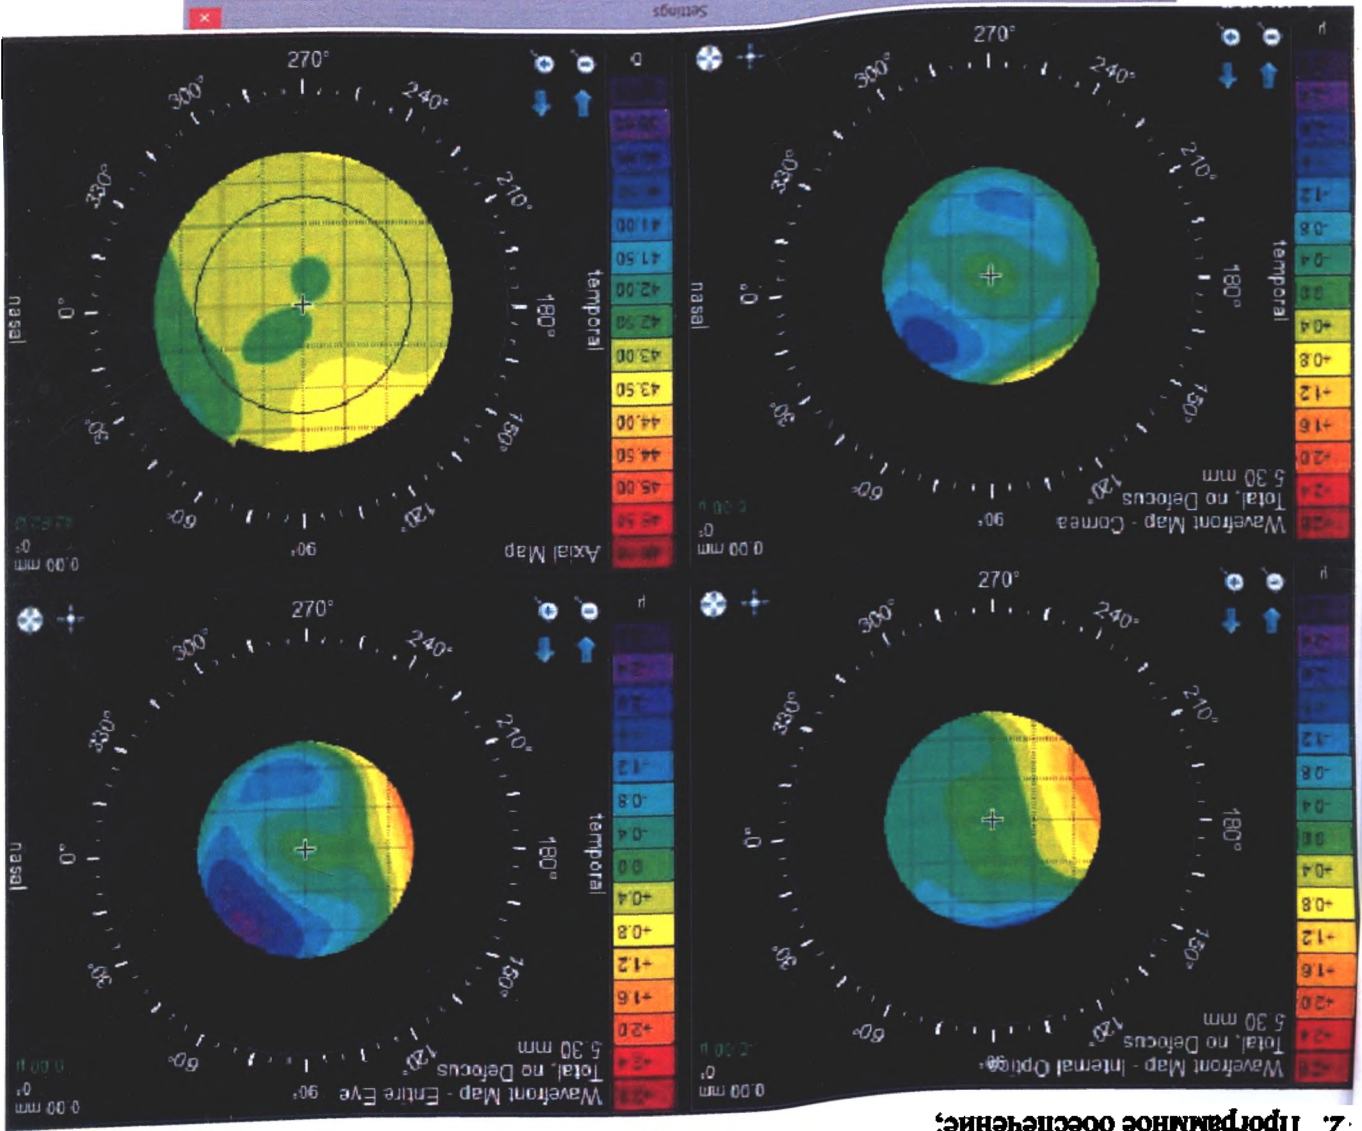

The screenshot shows the 'Settings' dialog box of a software application. The dialog box is divided into several sections:


- Wavefront Map:** Contains checkboxes for 'Wavefront Map', 'Wavefront Map - Cornea', 'Wavefront Map - Entire Eye', and 'Wavefront Map - Internal Optical'. The 'Wavefront Map' checkbox is checked.
- Advanced Settings:** Contains checkboxes for 'Advanced Settings', 'Wavefront Map', 'Wavefront Map - Cornea', 'Wavefront Map - Entire Eye', and 'Wavefront Map - Internal Optical'. The 'Advanced Settings' checkbox is checked.
- Export Data:** Contains checkboxes for 'Export Data', 'Wavefront Map', 'Wavefront Map - Cornea', 'Wavefront Map - Entire Eye', and 'Wavefront Map - Internal Optical'. The 'Export Data' checkbox is checked.
- Export Log:** Contains checkboxes for 'Export Log', 'Wavefront Map', 'Wavefront Map - Cornea', 'Wavefront Map - Entire Eye', and 'Wavefront Map - Internal Optical'. The 'Export Log' checkbox is checked.
- Wavefront Map:** Contains checkboxes for 'Wavefront Map', 'Wavefront Map - Cornea', 'Wavefront Map - Entire Eye', and 'Wavefront Map - Internal Optical'. The 'Wavefront Map' checkbox is checked.

The dialog box also includes a 'Settings' button at the bottom right and a 'Cancel' button at the bottom left.

Выносной блок питания;



4. Сетевой кабель;

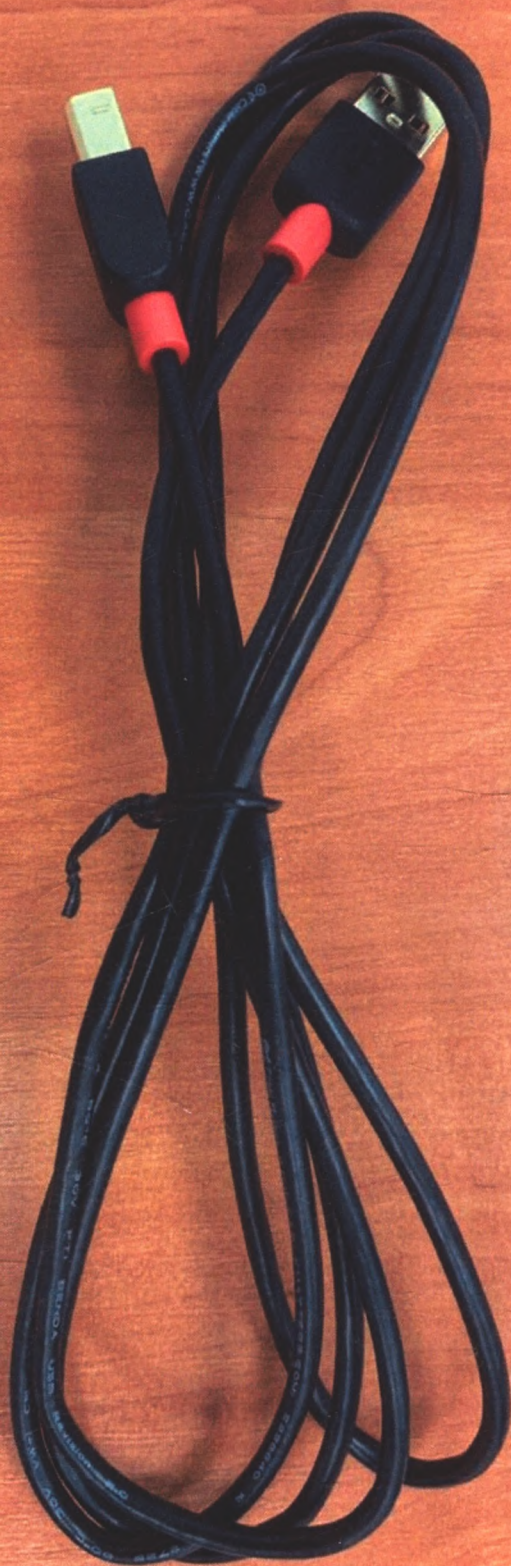

5. Калибровочный инструмент №1;



6. Калибровочный инструмент №2.




II. Принадлежности

- 1. Противопылевой чехол;




**iTrace™**  
COMBINATION RAY TRACING  
ABERROMETER/TOPOGRAPHER


2. Комплект оборудования со стороны пациента в составе:
- Основание;

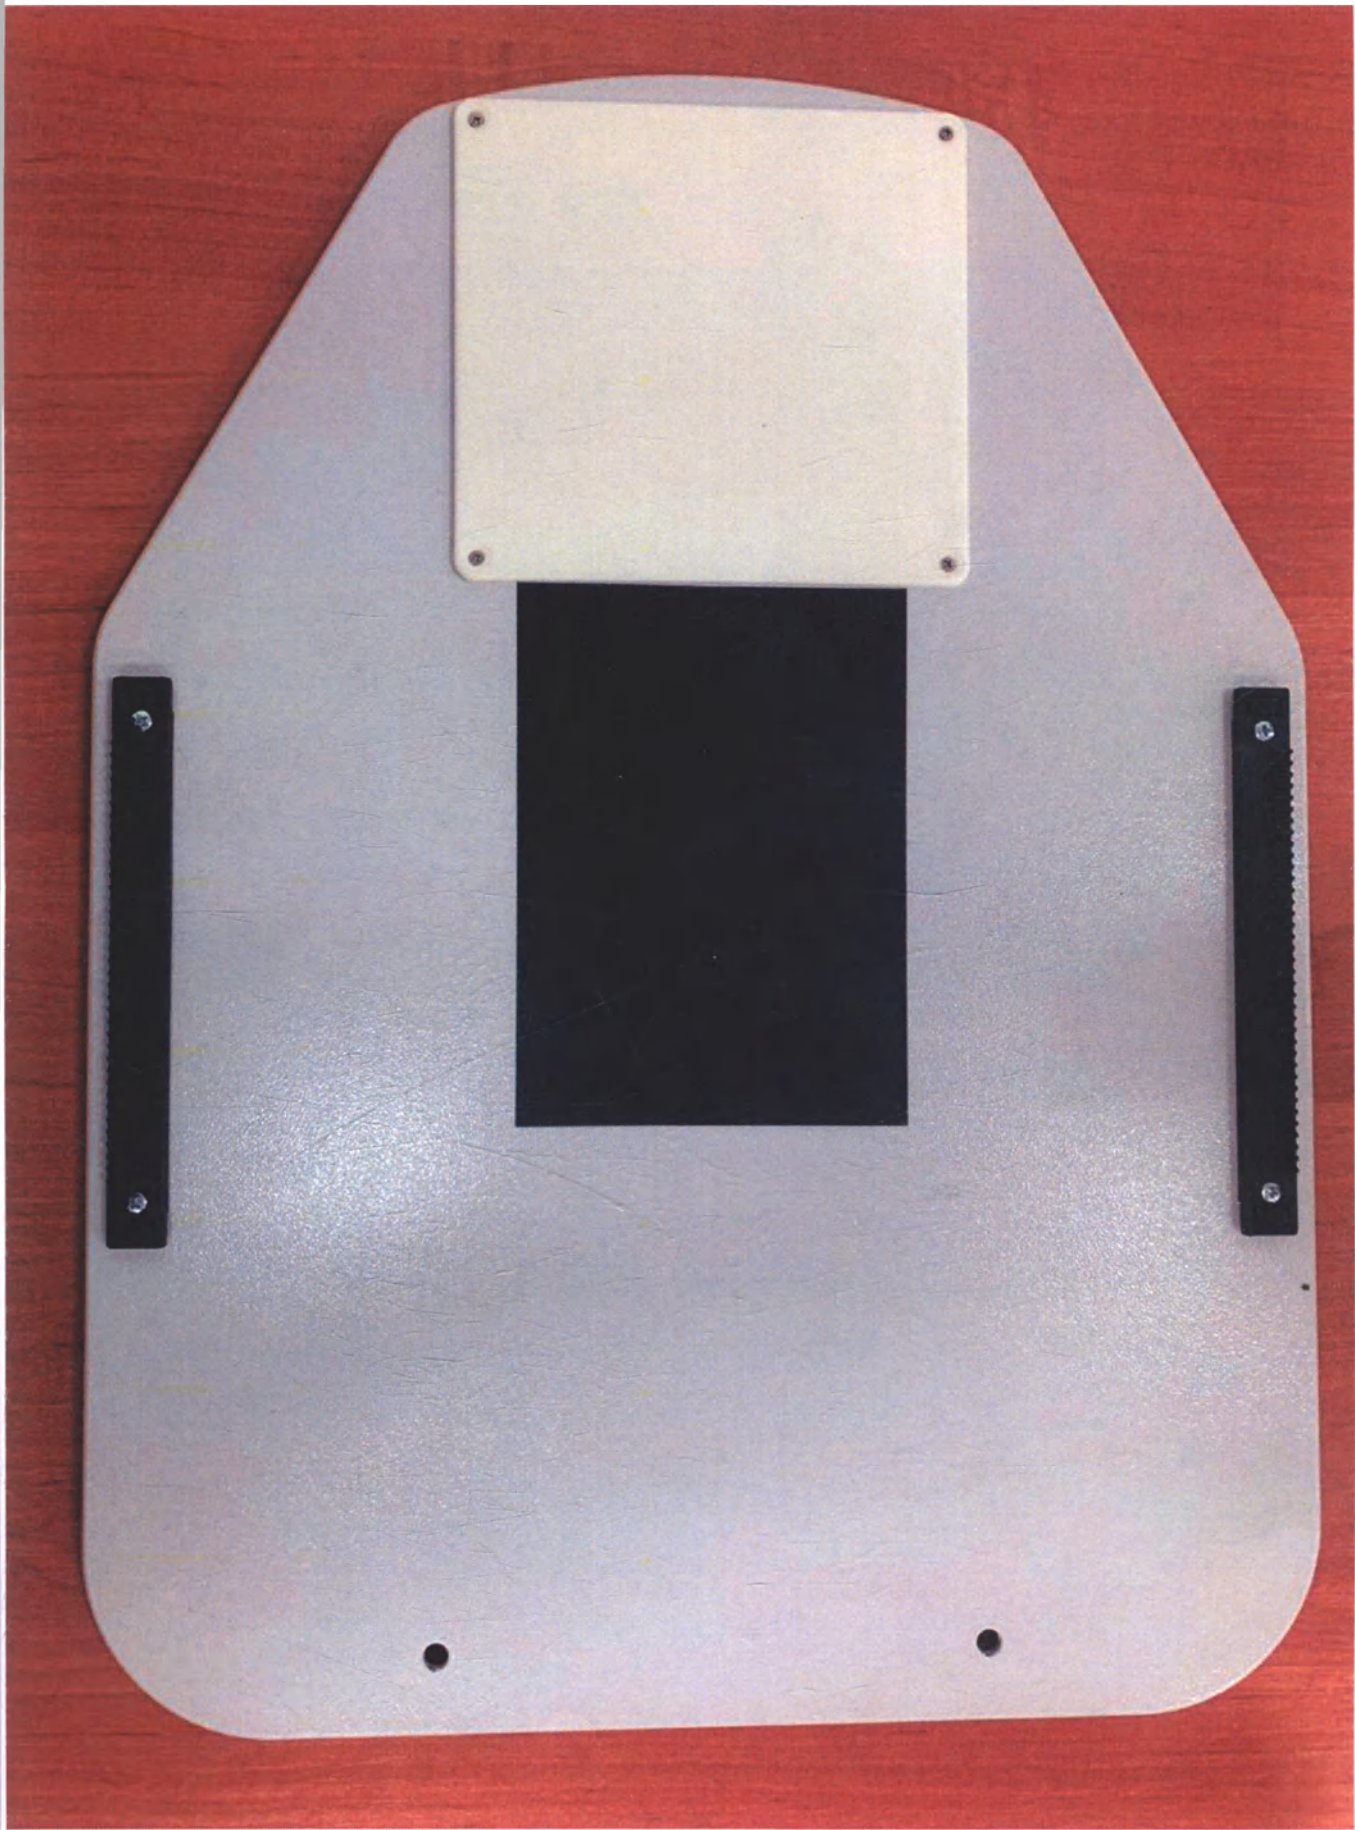

– Упор для подбородка;

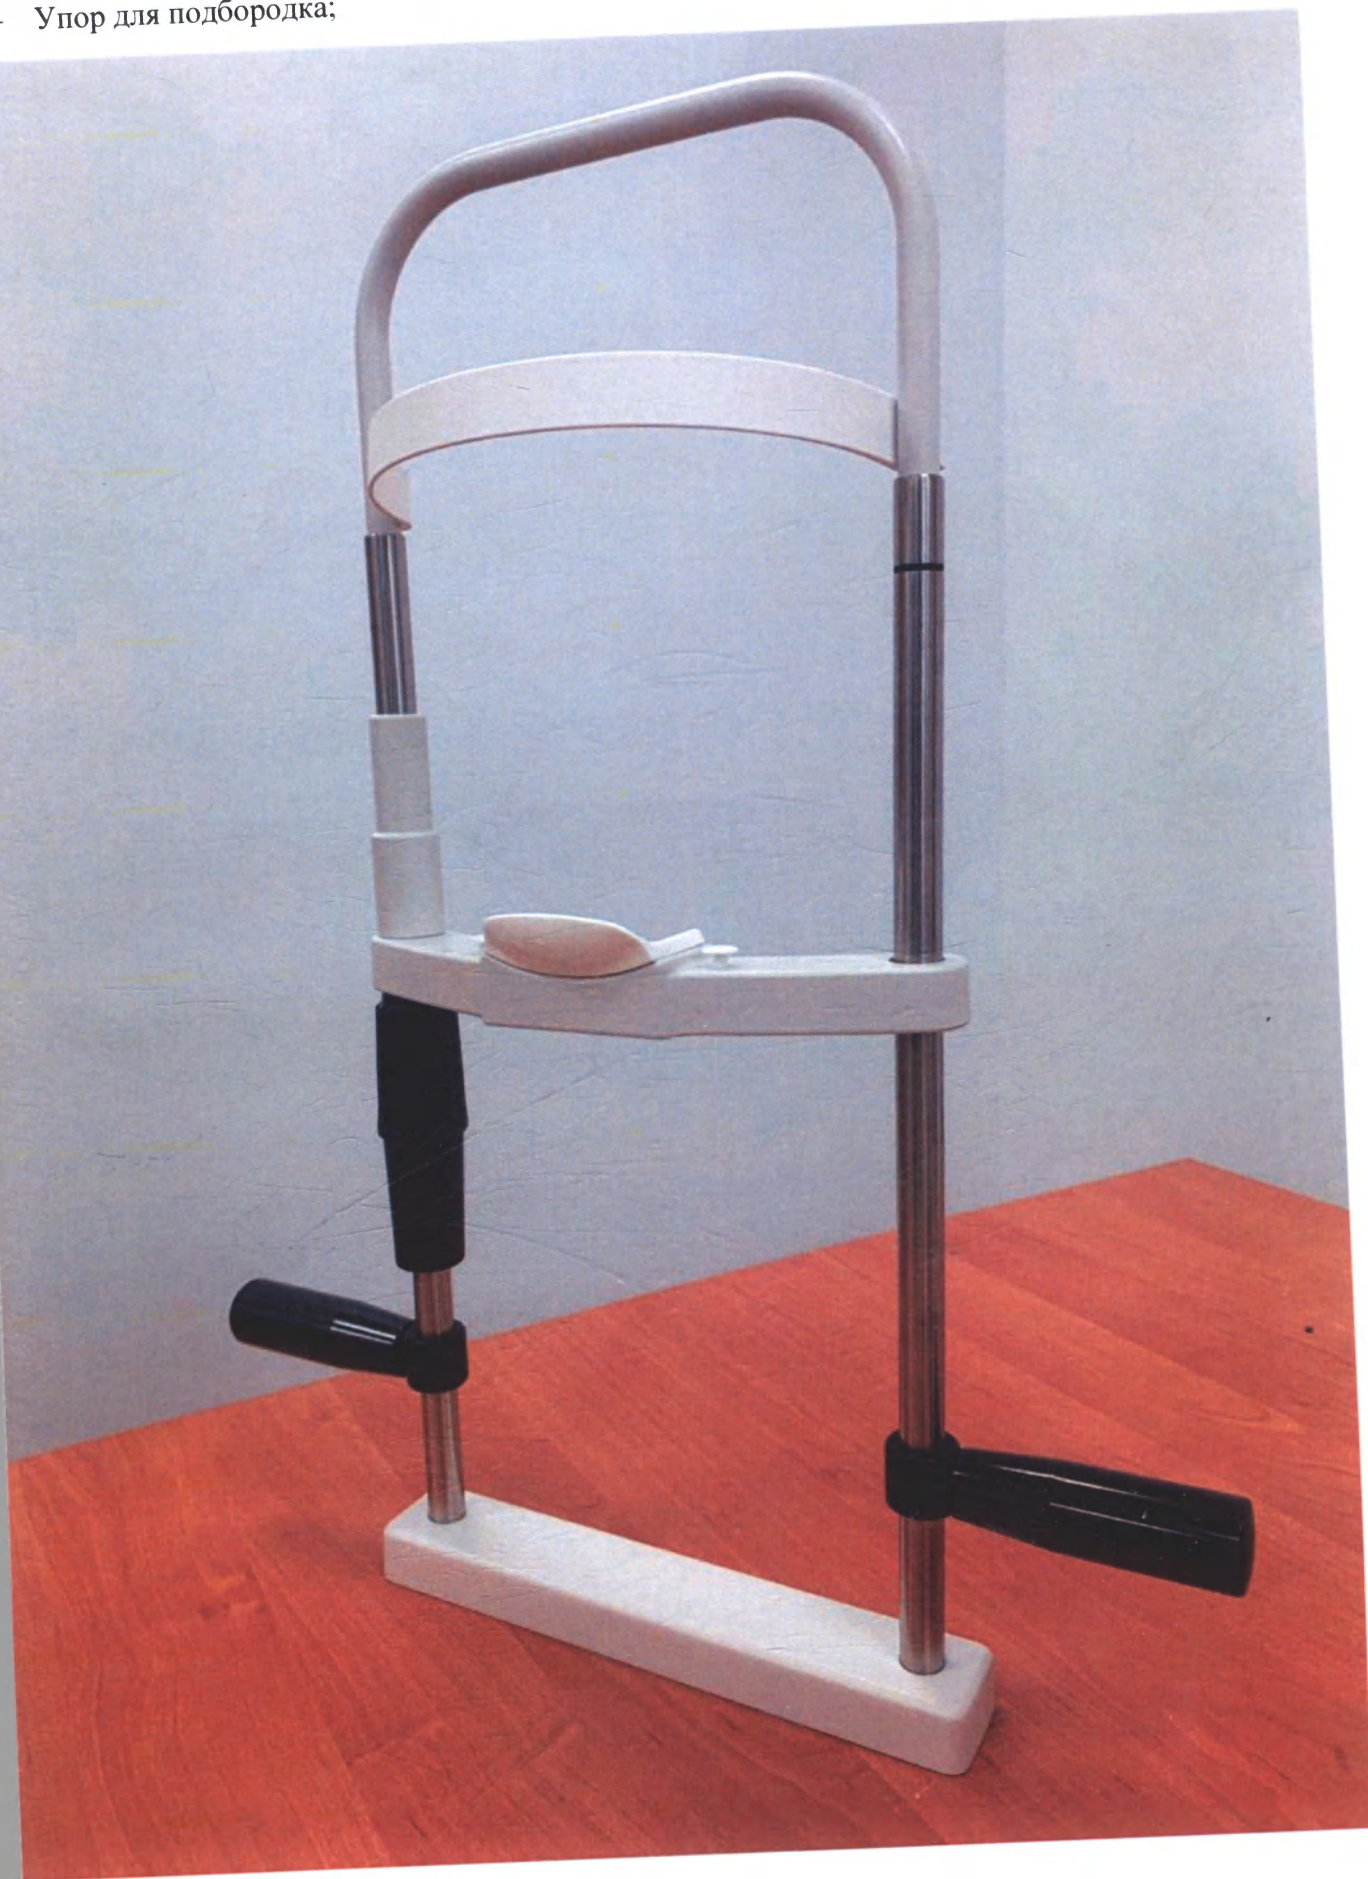


– Установочные винты;

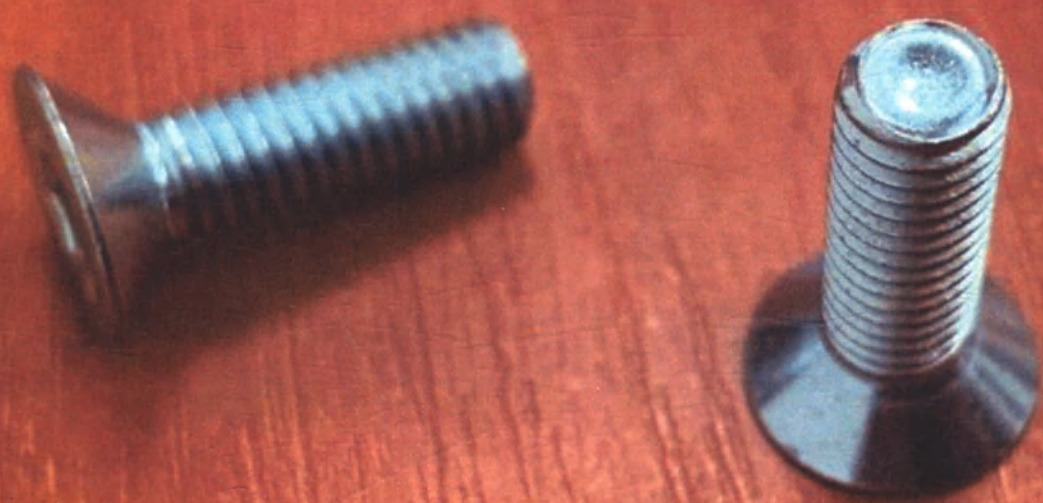

**TRACEY**<sup>TM</sup>  
TECHNOLOGIES

CLASS 1 LASER PRODUCT



Tracey Technologies  
16720 Hedgecroft Dr., Ste 208  
Houston, TX 77060, USA  
www.traceytechnologies.com

12-18

SN

3975

REF Tracey-VFA  
Visual Function Analyzer  
Model: iTrace

LB001F

EC REP

EMERGO EUROPE  
Prinsesgracht 20  
2514 AP, The Hague  
The Netherlands  
Phone: +31 70 345 8570  
Fax: +31 70 345 7289



CE 24V ~ 2.5A  
0120



прошито, пронумеровано 700 ) листов

Директор \_\_\_\_\_ /Макаров Я.Ю./

