



**ЦЕНТР
ПОДТВЕРЖДЕНИЯ
СООТВЕТСТВИЯ**

**Общество с ограниченной
ответственностью
«Центр Подтверждения Соответствия»
123308, г. Москва, ул. Мневники, дом
3, корпус 1
ИНН/КПП 7725790126/773401001
ОГРН 1137746368869
Тел/факс +7 495 532 92 10,
эл. почта: info@ctrps.ru**

**Фотографические изображения медицинского изделия
«Катетер внутрисердечный ультразвуковой Ultra ICE
Plus» с принадлежностями**

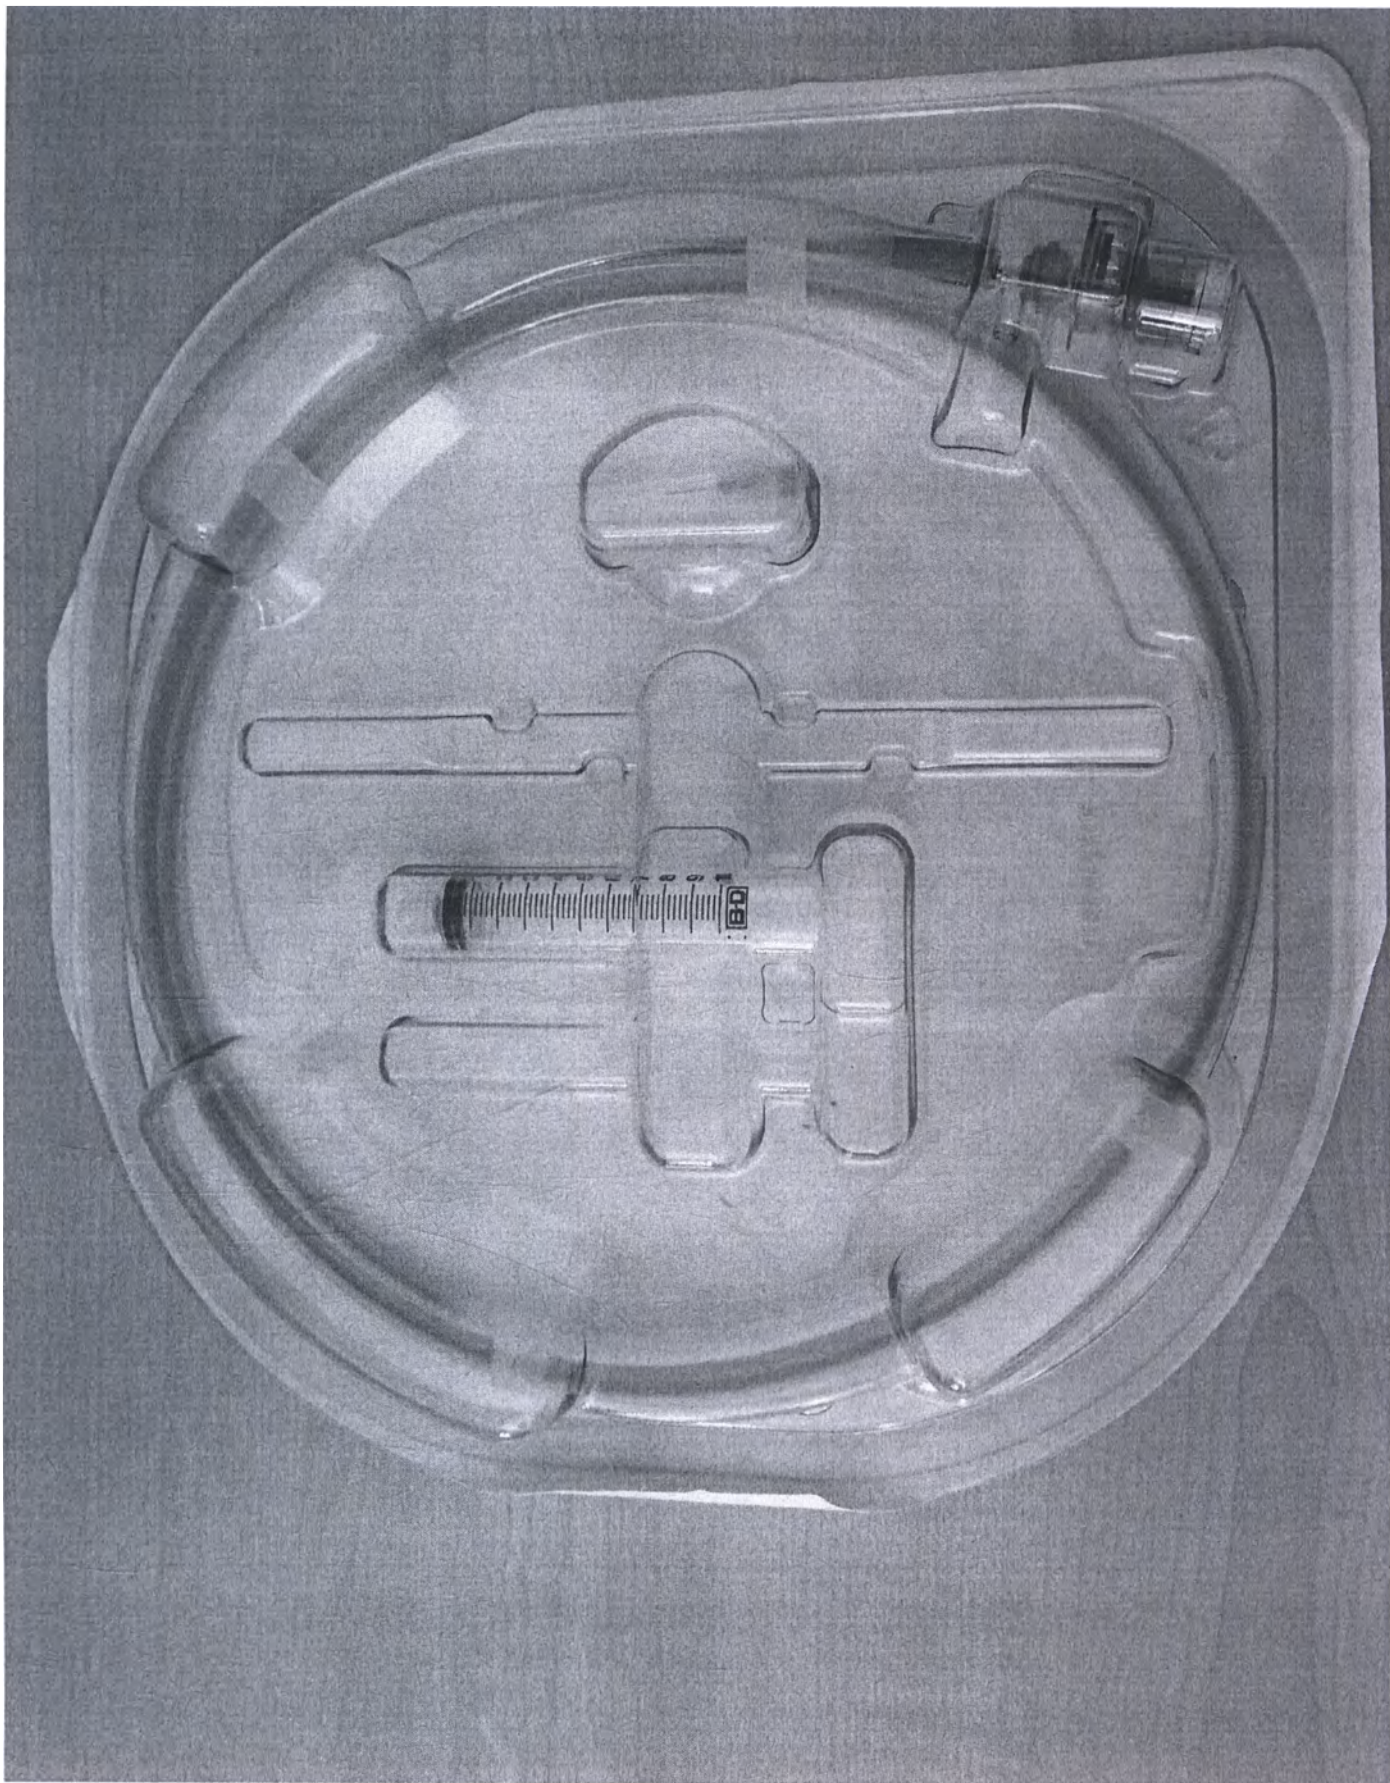


Рис.1. Общий вид медицинского изделия с комплектующими в первичной упаковке (катетер со шприцом и иглой)

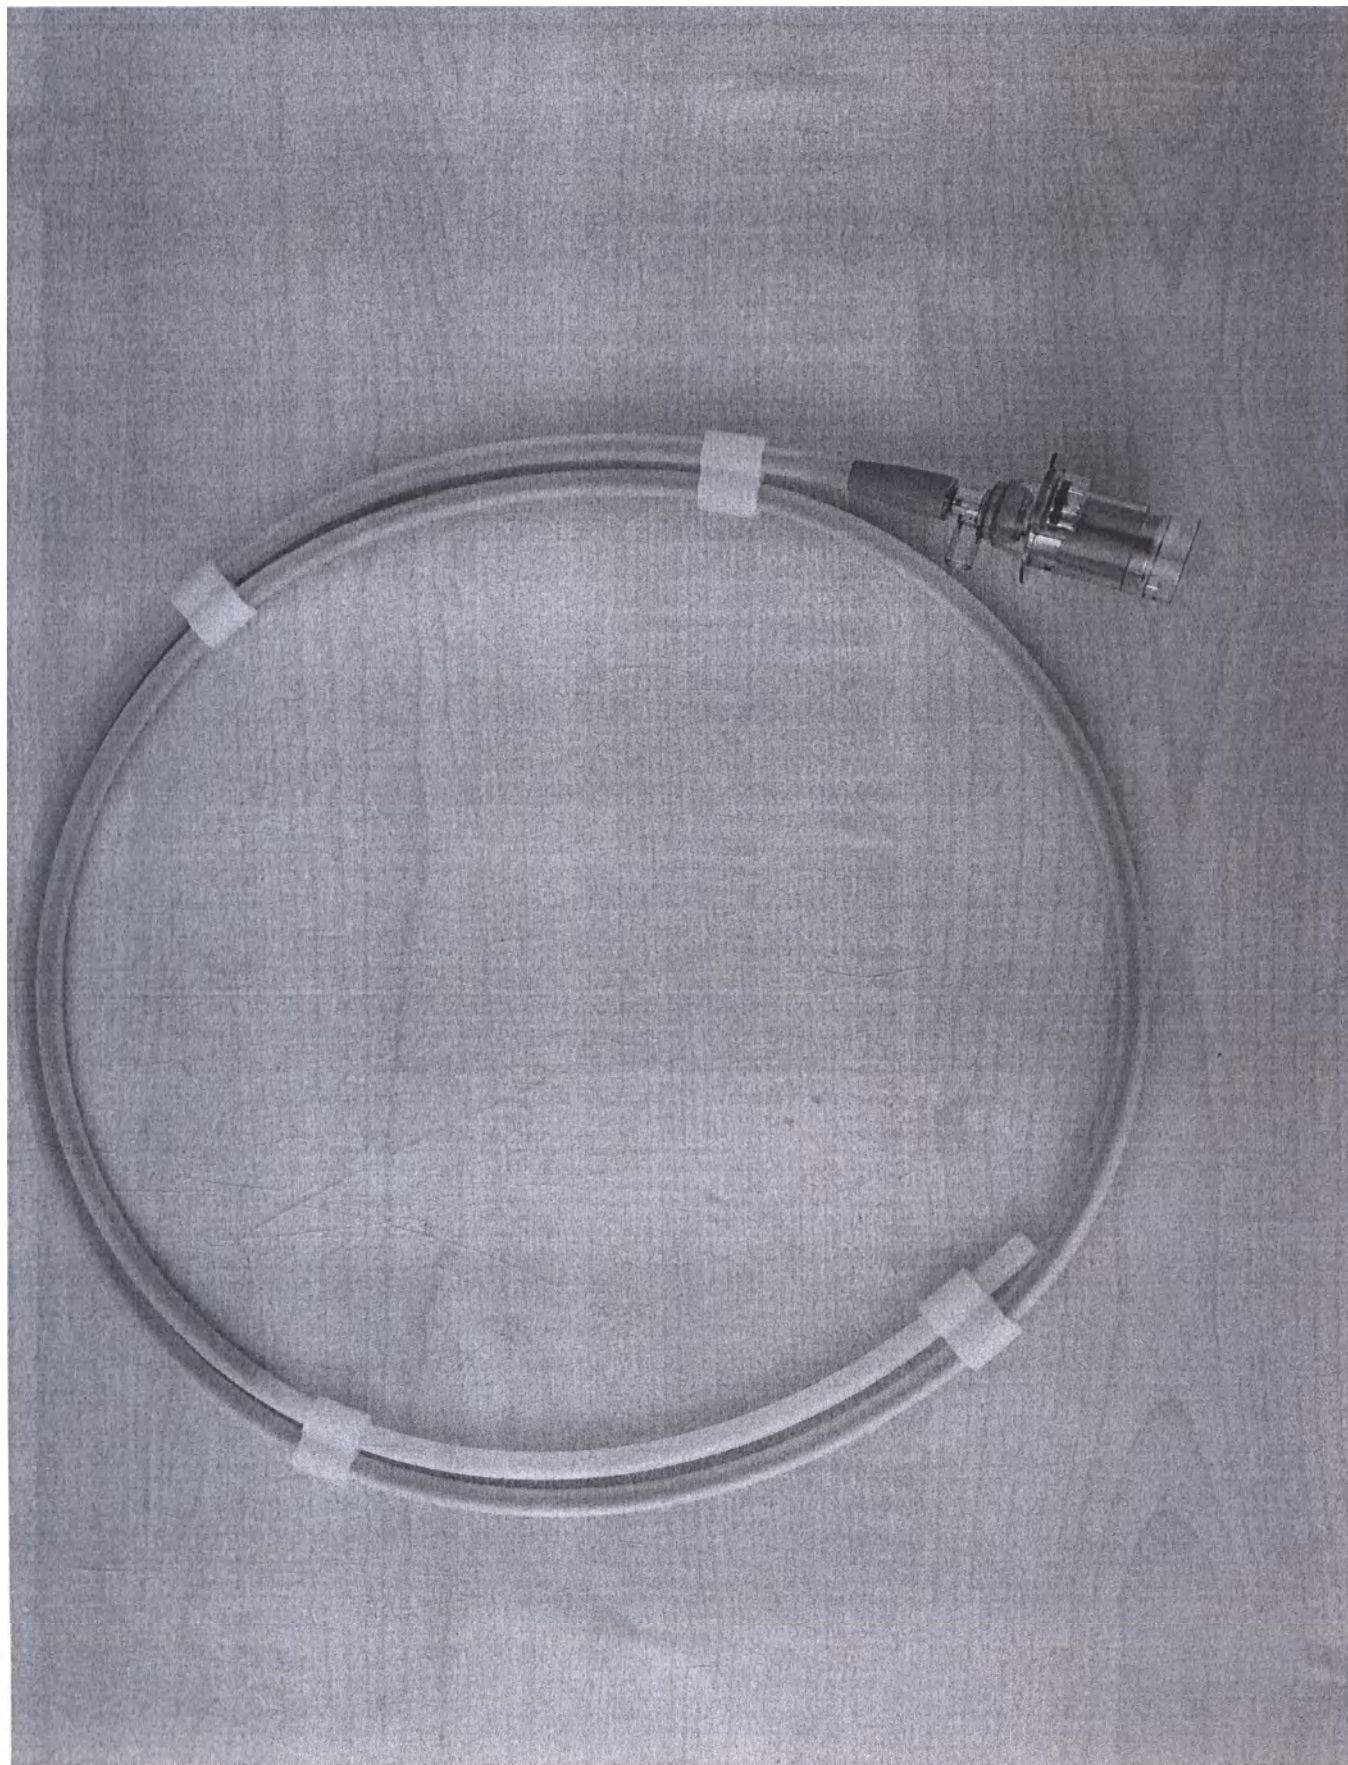


Рис.2. Катетер Ultra ICE Plus в защитной оболочке

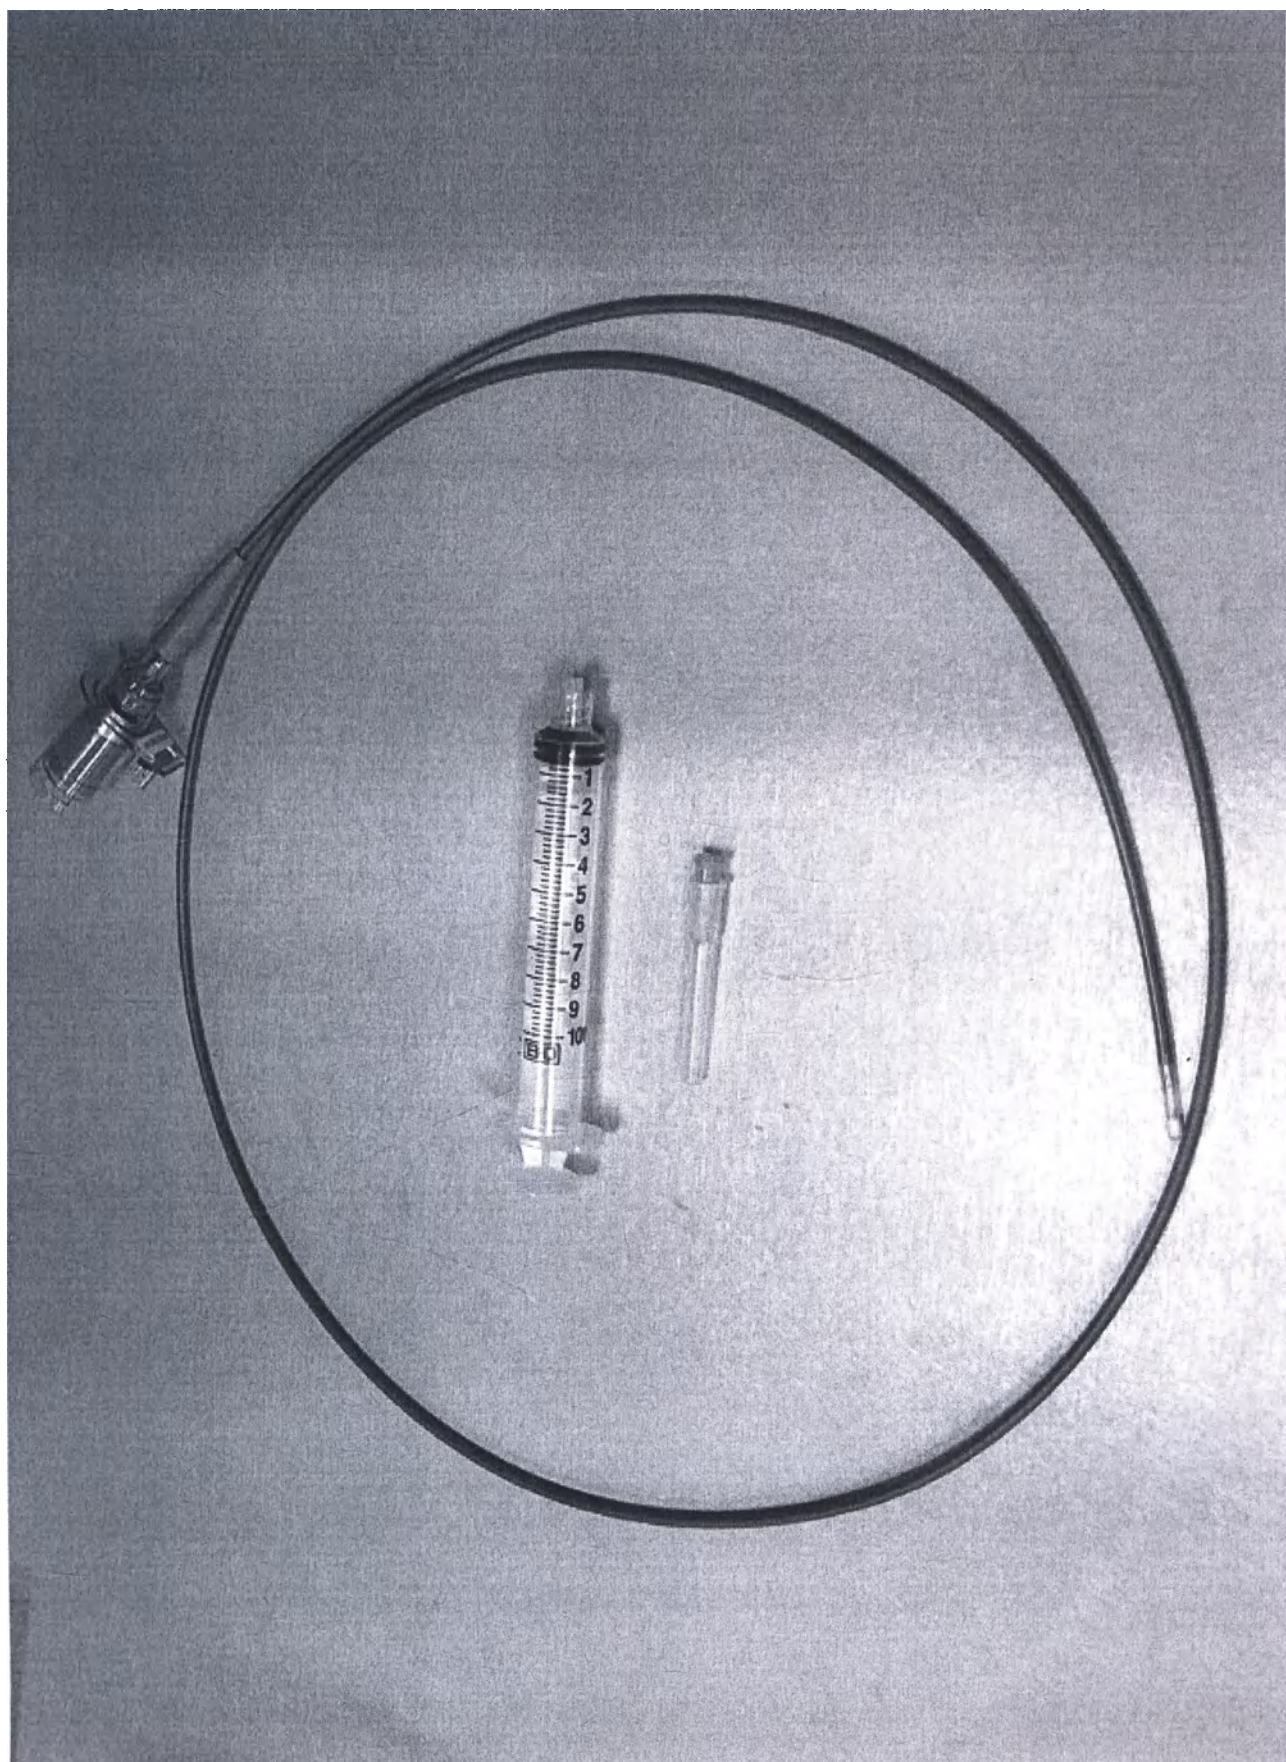


Рис.3. Катетер Ultra ICE Plus со шприцом 10 мл и промывочной иглой

Boston Scientific



EC REP EU Authorized Representative

Boston Scientific Limited
Ballybarr Business Park
Galway
IRELAND

Legal Manufacturer

Boston Scientific Corporation
881 Boston Scientific Way
Marlborough, MA 01758
USA
USA Customer Service: 800-272-1001

Rx ONLY



Consult instructions for use.



Do not use if package is damaged.



For single use only. Do not reuse.



Do Not Resterilize

Boston Scientific


Ultra ICE™ Plus

9MHz

IntraCardiac Echo Catheter

Cateter para ecografia intracardíaca, Cathéter d'echographie intracardiaque, Intrakardialer Echokardiographie-Katheter, Catetere per ecografia intracardíaca, Intracardiac echokatheter, イントラカーディアック・エコー・カテーテル/V, Kateter til akkardiografi, Evokardiograf-kateter, Kardiograf-kateter, Cateter Echografic Intracardiac, Intrakardialis echokateter, Kateter pro intrakardialni echokardiografii, Cevnik do echokardiografije v intrakardijalni, Intrakardial ultrahd kateter (ekokardiografii), IntraKardiyak Eko Kateteri, Sydämsinsäätin ultraäänikatetri, Cateter de ecografie intracardiacă, Внутрисердечный эхокардиографический катетер, Kateter na intrakardialnu echokardiografiju

Contents (1)



9F (3.00mm) Recommended Introducer Sheath



Includes Flushing Needle (1) with Luer Fitting



(1) Includes Syringe

Tip Style: Rounded Tip

Estilo de la punta: punta redondeada, Type d'extrémité: Extrémité arrondie, Spitzenausführung: Abgerundete Spitze, Stile della punta: tonda, Tipstørrelse: afrundet tip, チップ種類: 丸型チップ, Spisstype: Rund spids, Tuncoc dipov: Zrpolovukuseto dipo, Tipo de Ponta: Ponta Arredondada, Spatsauformung: Avrundad spets, Csica típusa: legördültyűtűtű csúcs, Tip hrotu: kulaty hrot, Rodzaj końcówki: końcówka zaokrąglona, Spisstype: avrundat spiss, Uç Stili: Yuvarlak uçlu, Uç Karan malis: pyöristetty kärki, Tip varti: Värilastic, Тип наконечника: закругленный наконечник, Typ hrotu: zaoblený hrot

GTIN

08714729904373

LOT

23572588

REF Catalog No.

M00499100

Use By

2021-03-31

STERILE R

Sterilized using irradiation.



91102823-01A

CE 0344

Made in COSTA RICA
2546 First Street
Propark
El Coyoil, Alajuela
COSTA RICA

This product may be protected by one or more patents.
Patent information can be obtained at
<http://www.bostonscientific.com/patents>

Boston Scientific
Ultra ICE™ Plus
8.5F (2.82mm) x 110cm
GTIN 08714729904373
REF M00499100
LOT 23572588



Boston Scientific
Ultra ICE™ Plus
8.5F (2.82mm) x 110cm
GTIN 08714729904373
REF M00499100
LOT 23572588



Boston Scientific
Ultra ICE™ Plus
8.5F (2.82mm) x 110cm

GTIN 08714729904373
REF M00499100
LOT 23572588



10106714729904373 17321033111023572588

GS1

Рис.4. Маркировка производителя на первичной упаковке катетера Ultra ICE Plus со шприцом 10 мл и промывочной иглой

Boston Scientific



EC REP EU Authorized Representative
Boston Scientific Limited
Ballybrit Business Park
Galway
IRELAND

Legal Manufacturer
Boston Scientific Corporation
200 Boston Scientific Way
Marlborough, MA 01752
USA
USA Customer Service 888-272-1001

Rx ONLY

Consult instructions for use.

Do not use if package is damaged.

For single use only. Do not reuse.

Do Not Resterilize

Boston Scientific


Ultra ICE™ Plus

9MHz

IntraCardiac Echo Catheter

Cateter para ecografia intracardíaca, Cathéter d'échographie intracardiaque, Intrakardialer Echokardiographie-Katheter, Catetere per ecografia intracardíaca, Intracardiale echokatheter, イントラカーディアック・エコー・カテーテル, Катетер для эхોકардиографіі, Ενδοκαρδιακός καθετήρ, Ecokardiografni kateter, Cateter Ecografico Intracardíaco, Intrakardiális echokatóter, Katētris pro intrakardiālīni echokardiografijai, Cewnik do echokardiografii wewnatrzsercowej, Intrakardiāls ultrāldiķatērs (ekokardiogrāfi), Intra Kardiak Eko Kateteri, Sydämsstisläinen ultraäänikatetri, Cateter de ecografie intracardiacă, Внутрисердечный эхографический катетер, Katēter na intrakardiālu echokardiografiju

Contents (1)



9F (3.00mm) Recommended Introducer Sheath

(1) Includes Syringe

Includes Flushing Needle with Luer Fitting

Tip Style: Rounded Tip

Castillo de la punta: punta redondeada, Type d'extrémité: Extrémité arrondie, Spitzenausführung: Abgerundete Spitze, Stile della punta: tonda, Tipüvveering: afgeronde tip, チップ種類: 丸型チップ, Spidestyle: Rønd spids, Топос άκρου: Στρογγυλεμένο άκρο, Tipo de Ponta: Ponta Arredondada, Spätsuförmming: Avrundad spåts, Csőcsúspont: lekörömölött csúcs, Typ hrotu: kulatý hrot, Rodzaj końcówki: końcówka zaokrąglona, Spisatyp: avrundat spiss, Uç Stili: Yuvarlanmış Uç, Kāņien mali: pyēnāstetty kārkis, Tip vdrf: Vdrf stētic, Тип наконечника: закругленный наконечник, Typ hrotu: zaoblony hrot

GTIN

08714729904373

LOT

23572588

REF

Catalog No.

M00499100

Use By

2021-03-31

STERILE R

Sterilized using irradiation



91102823-01A

CE 0344

Made in COSTA RICA
2546 First Street
Propark
El Coyol, Alajuela
COSTA RICA

This product may be protected by one or more patents.
Patent information can be obtained at
<http://www.bostonscientific.com/patents>

Boston Scientific
Ultra ICE™ Plus
8.5F (2.82mm) x 110cm
GTIN 08714729904373
REF M00499100
LOT 23572588



Boston Scientific
Ultra ICE™ Plus
8.5F (2.82mm) x 110cm
GTIN 08714729904373
REF M00499100
LOT 23572588



Boston Scientific
Ultra ICE™ Plus
8.5F (2.82mm) x 110cm

GTIN 08714729904373
REF M00499100
LOT 23572588



(01)08714729904373.17(21)03311(10)23572588

GS1

Рис.5. Маркировка производителя на вторичной упаковке катетера Ultra ICE Plus со шприцом 10 мл и промывочной иглой

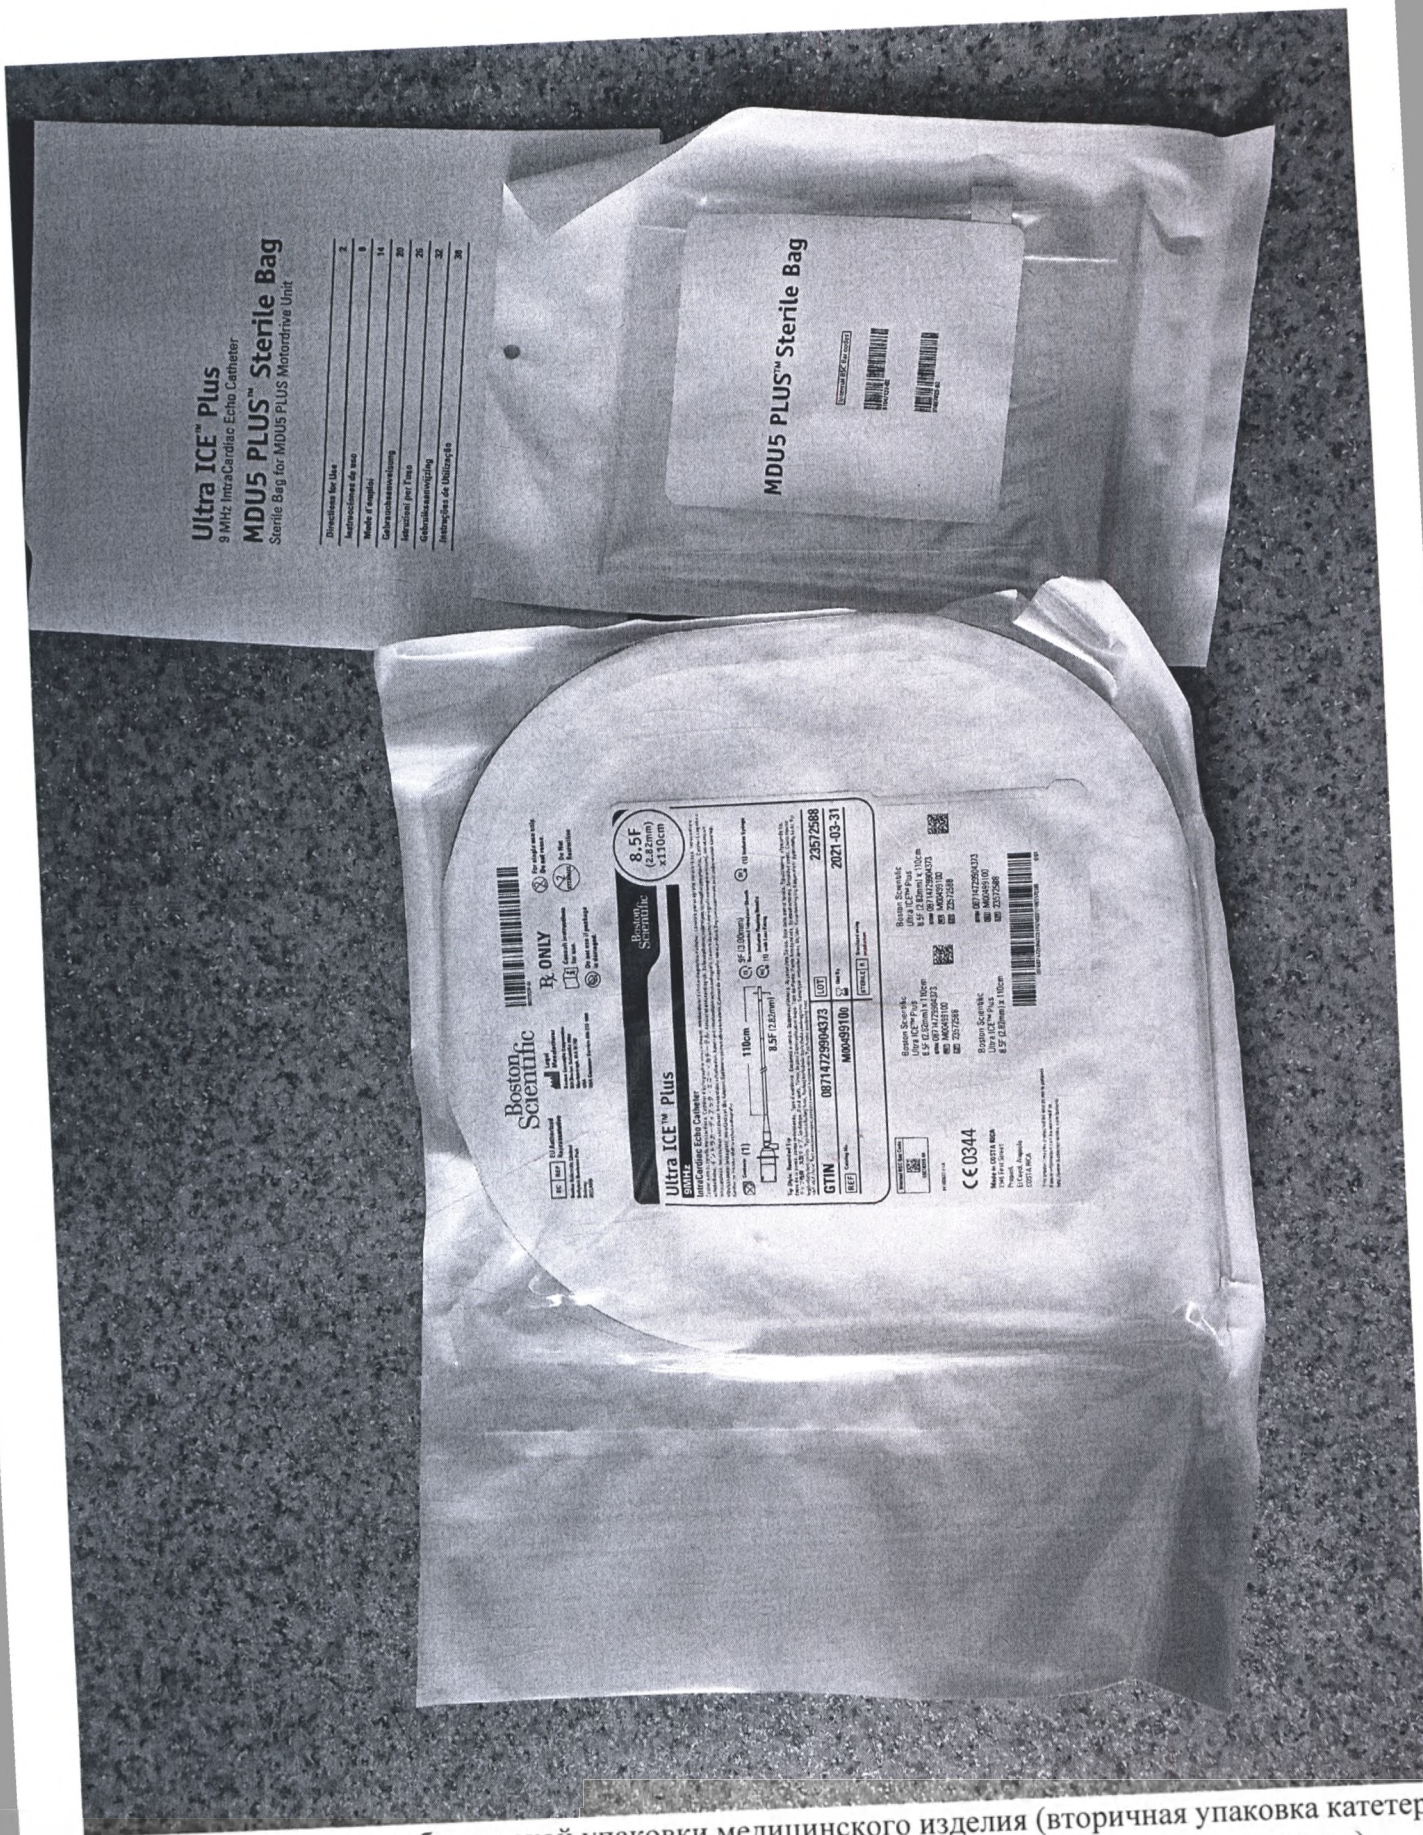


Рис. 7. Содержимое потребительской упаковки медицинского изделия (вторичная упаковка катетера, пакет стерильный MDU5 PLUS в первичной упаковке, эксплуатационная документация)



Рис. 8. Пакет стерильный MDU5 PLUS

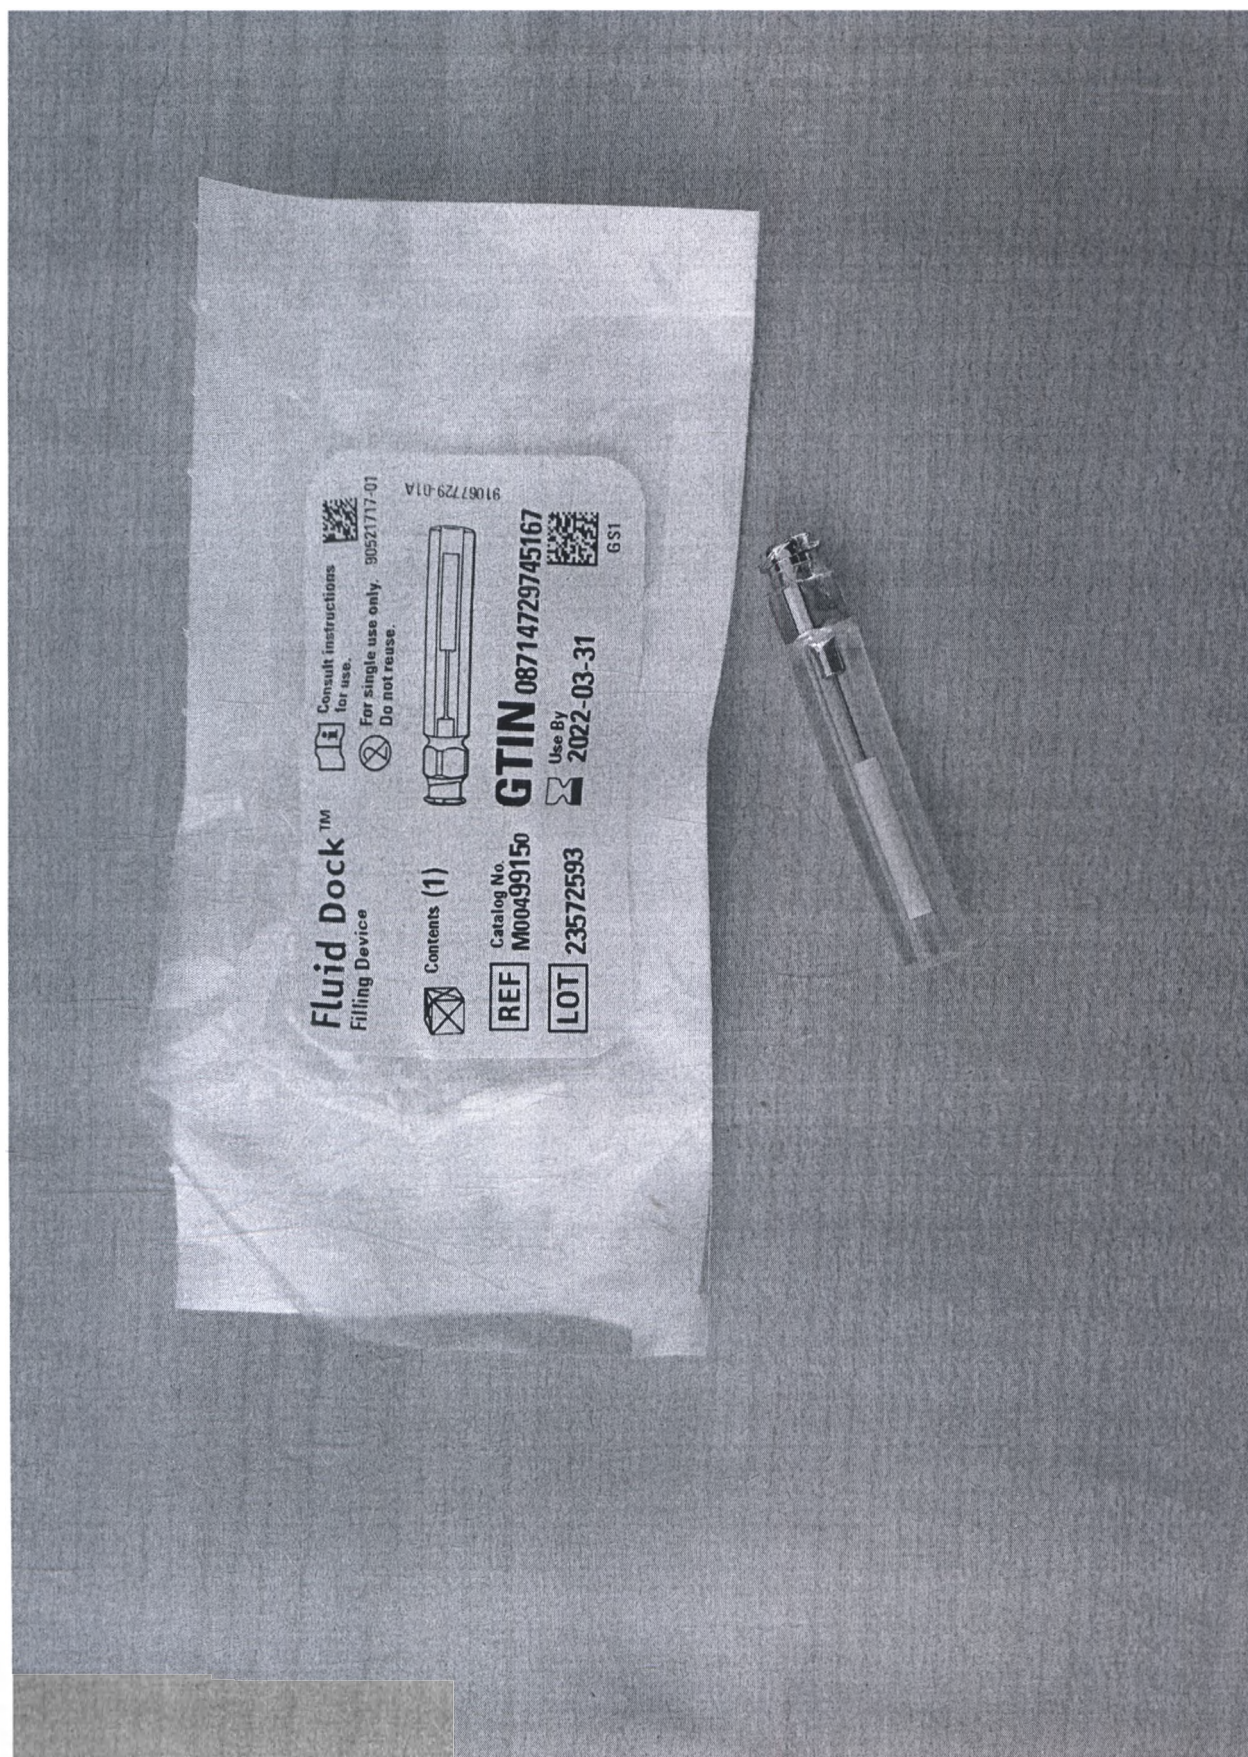


Рис. 9. Устройство для заполнения катетера для ультразвуковых исследований Fluid Dock с первичной упаковкой

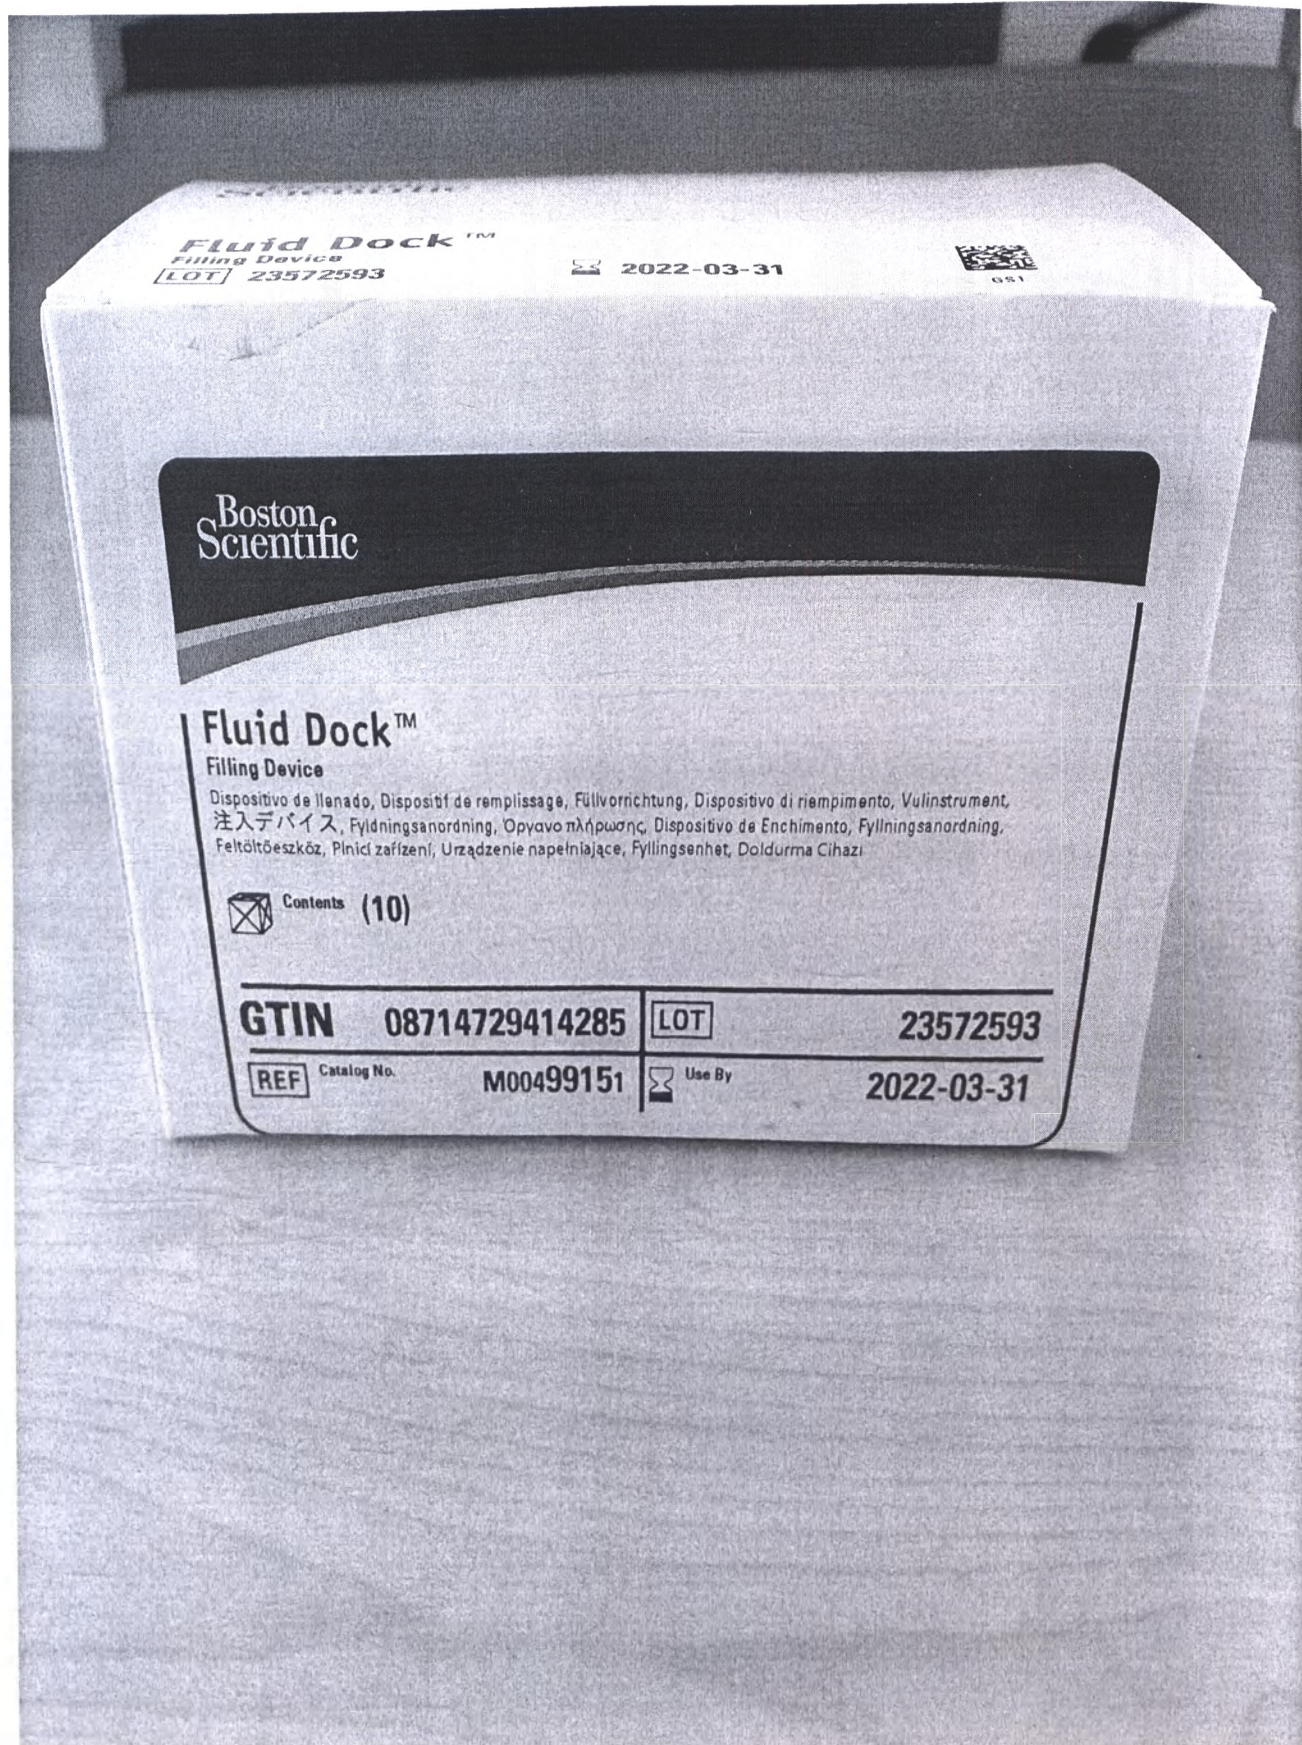


Рис. 10. Вторичная упаковка устройства для заполнения катетера для ультразвуковых исследований Fluid Dock