






OmniView ^{CE} ₂₄₆₀
MULTIPLE BAND LIGATOR

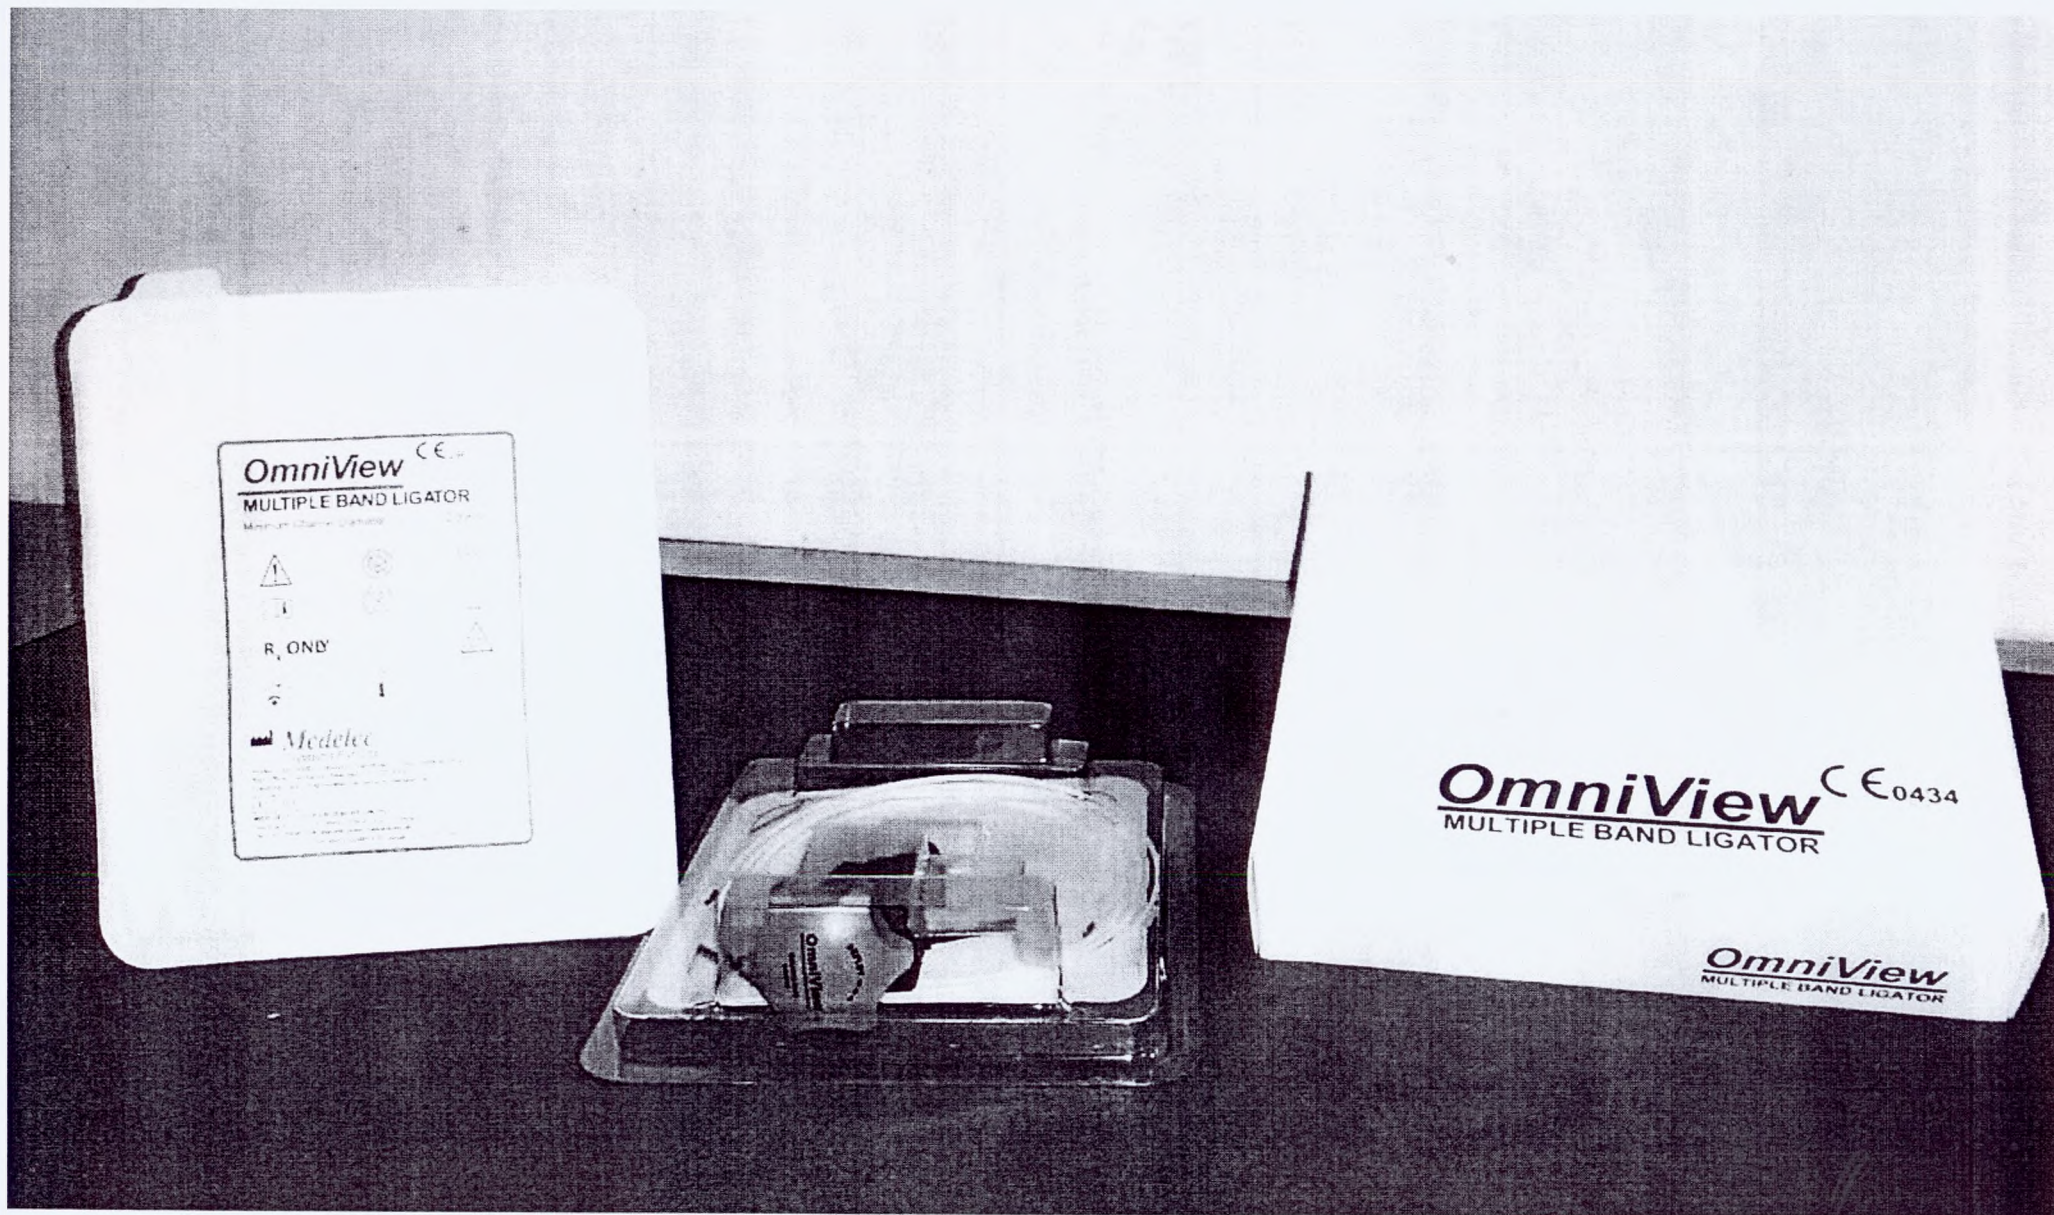


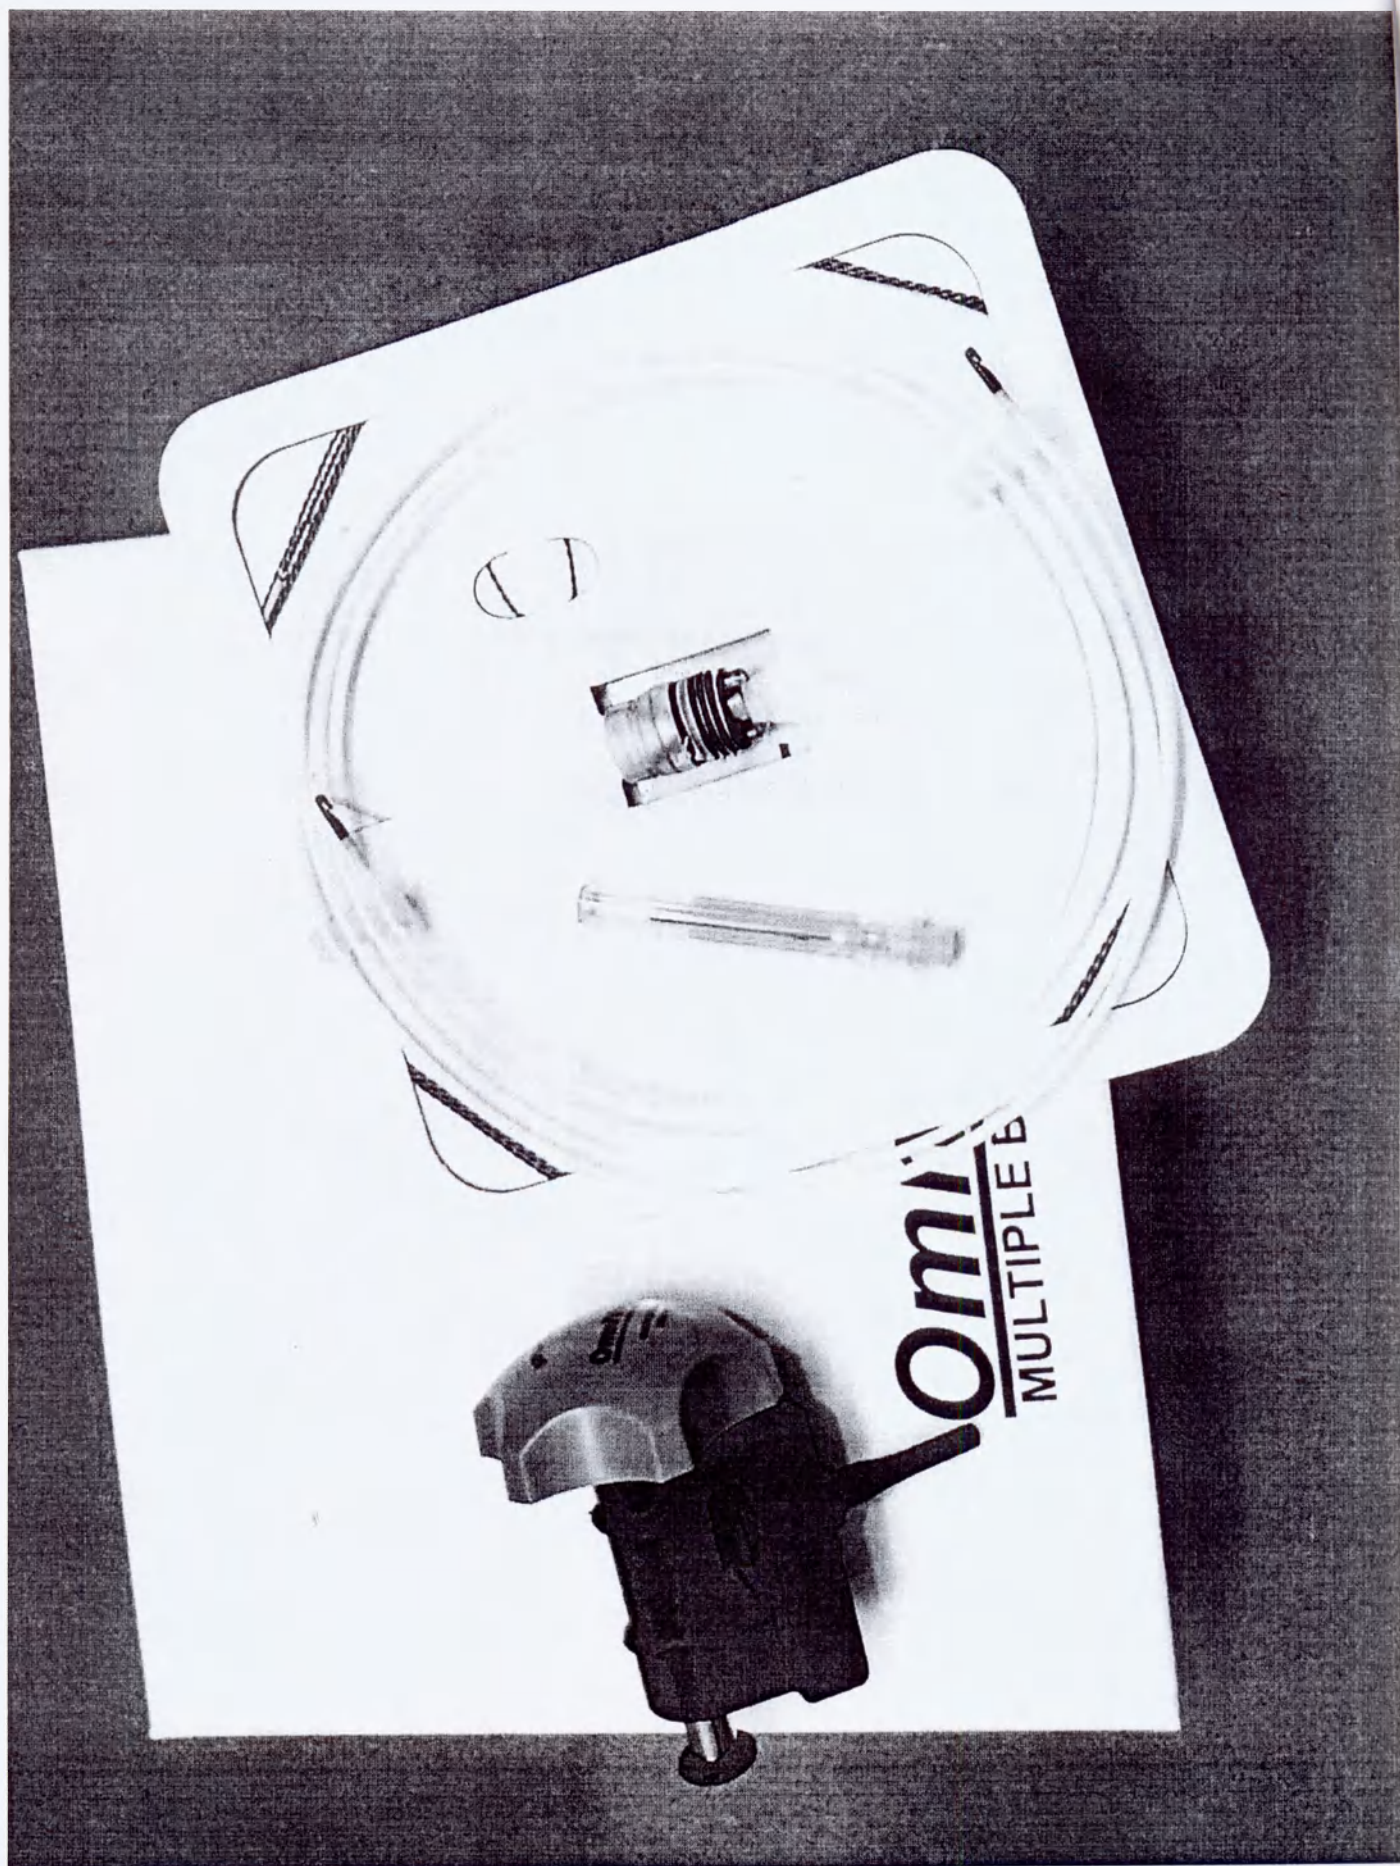

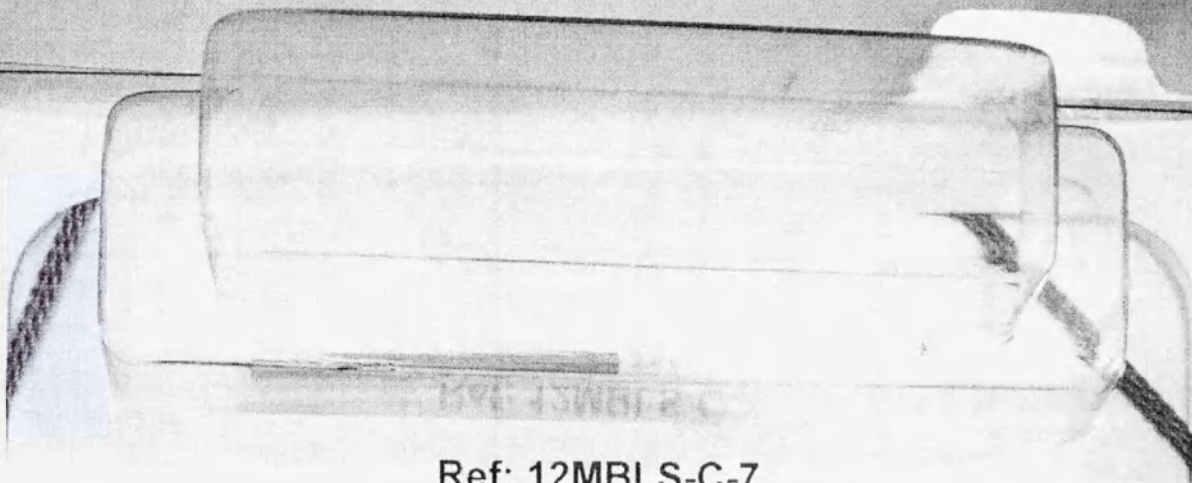


Ref: 12MBLS-C-7
Endoscope Diameter
9.5~13.0 mm

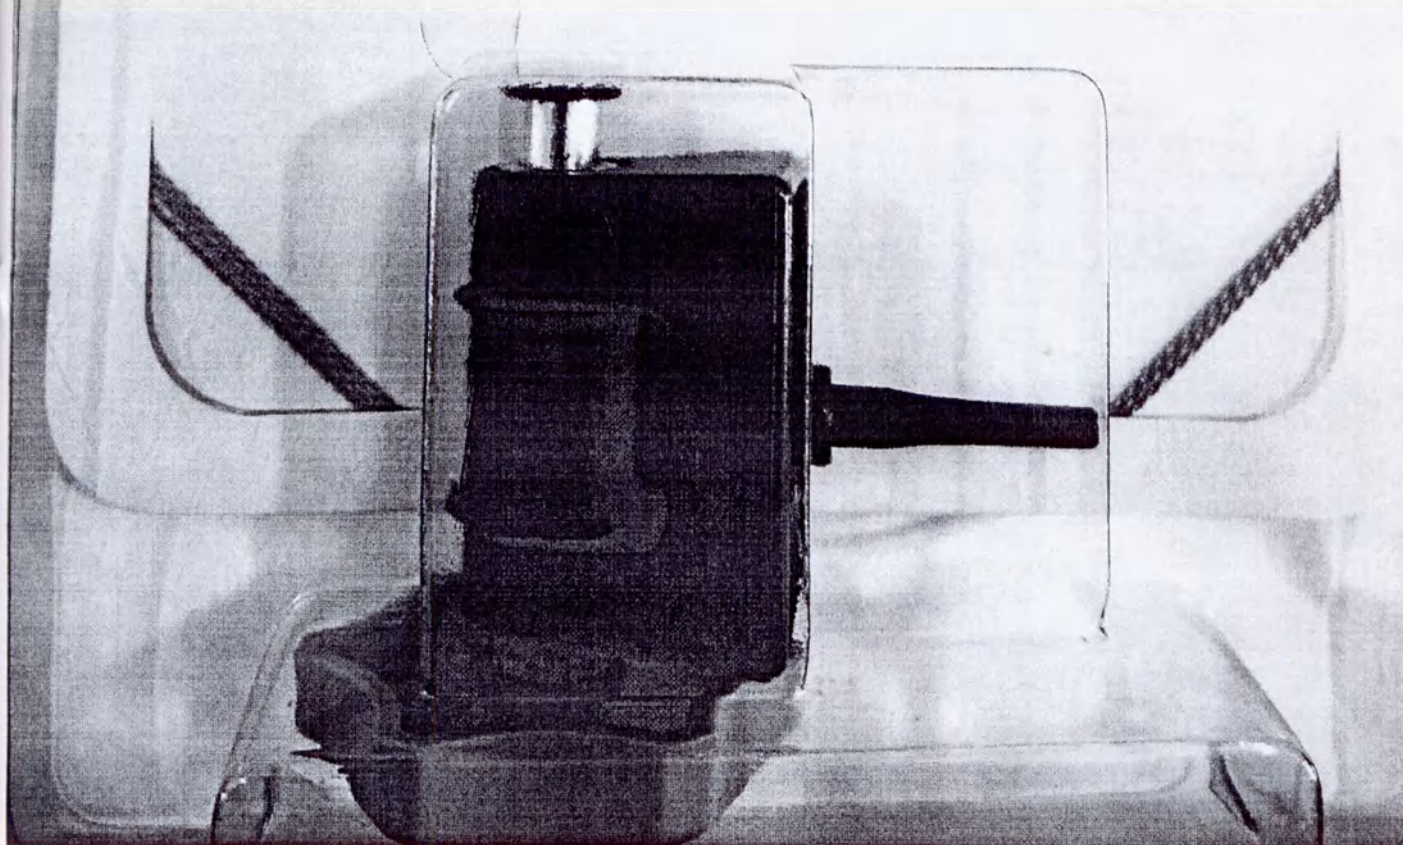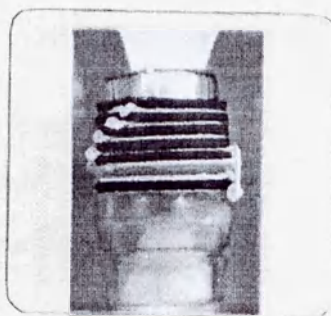


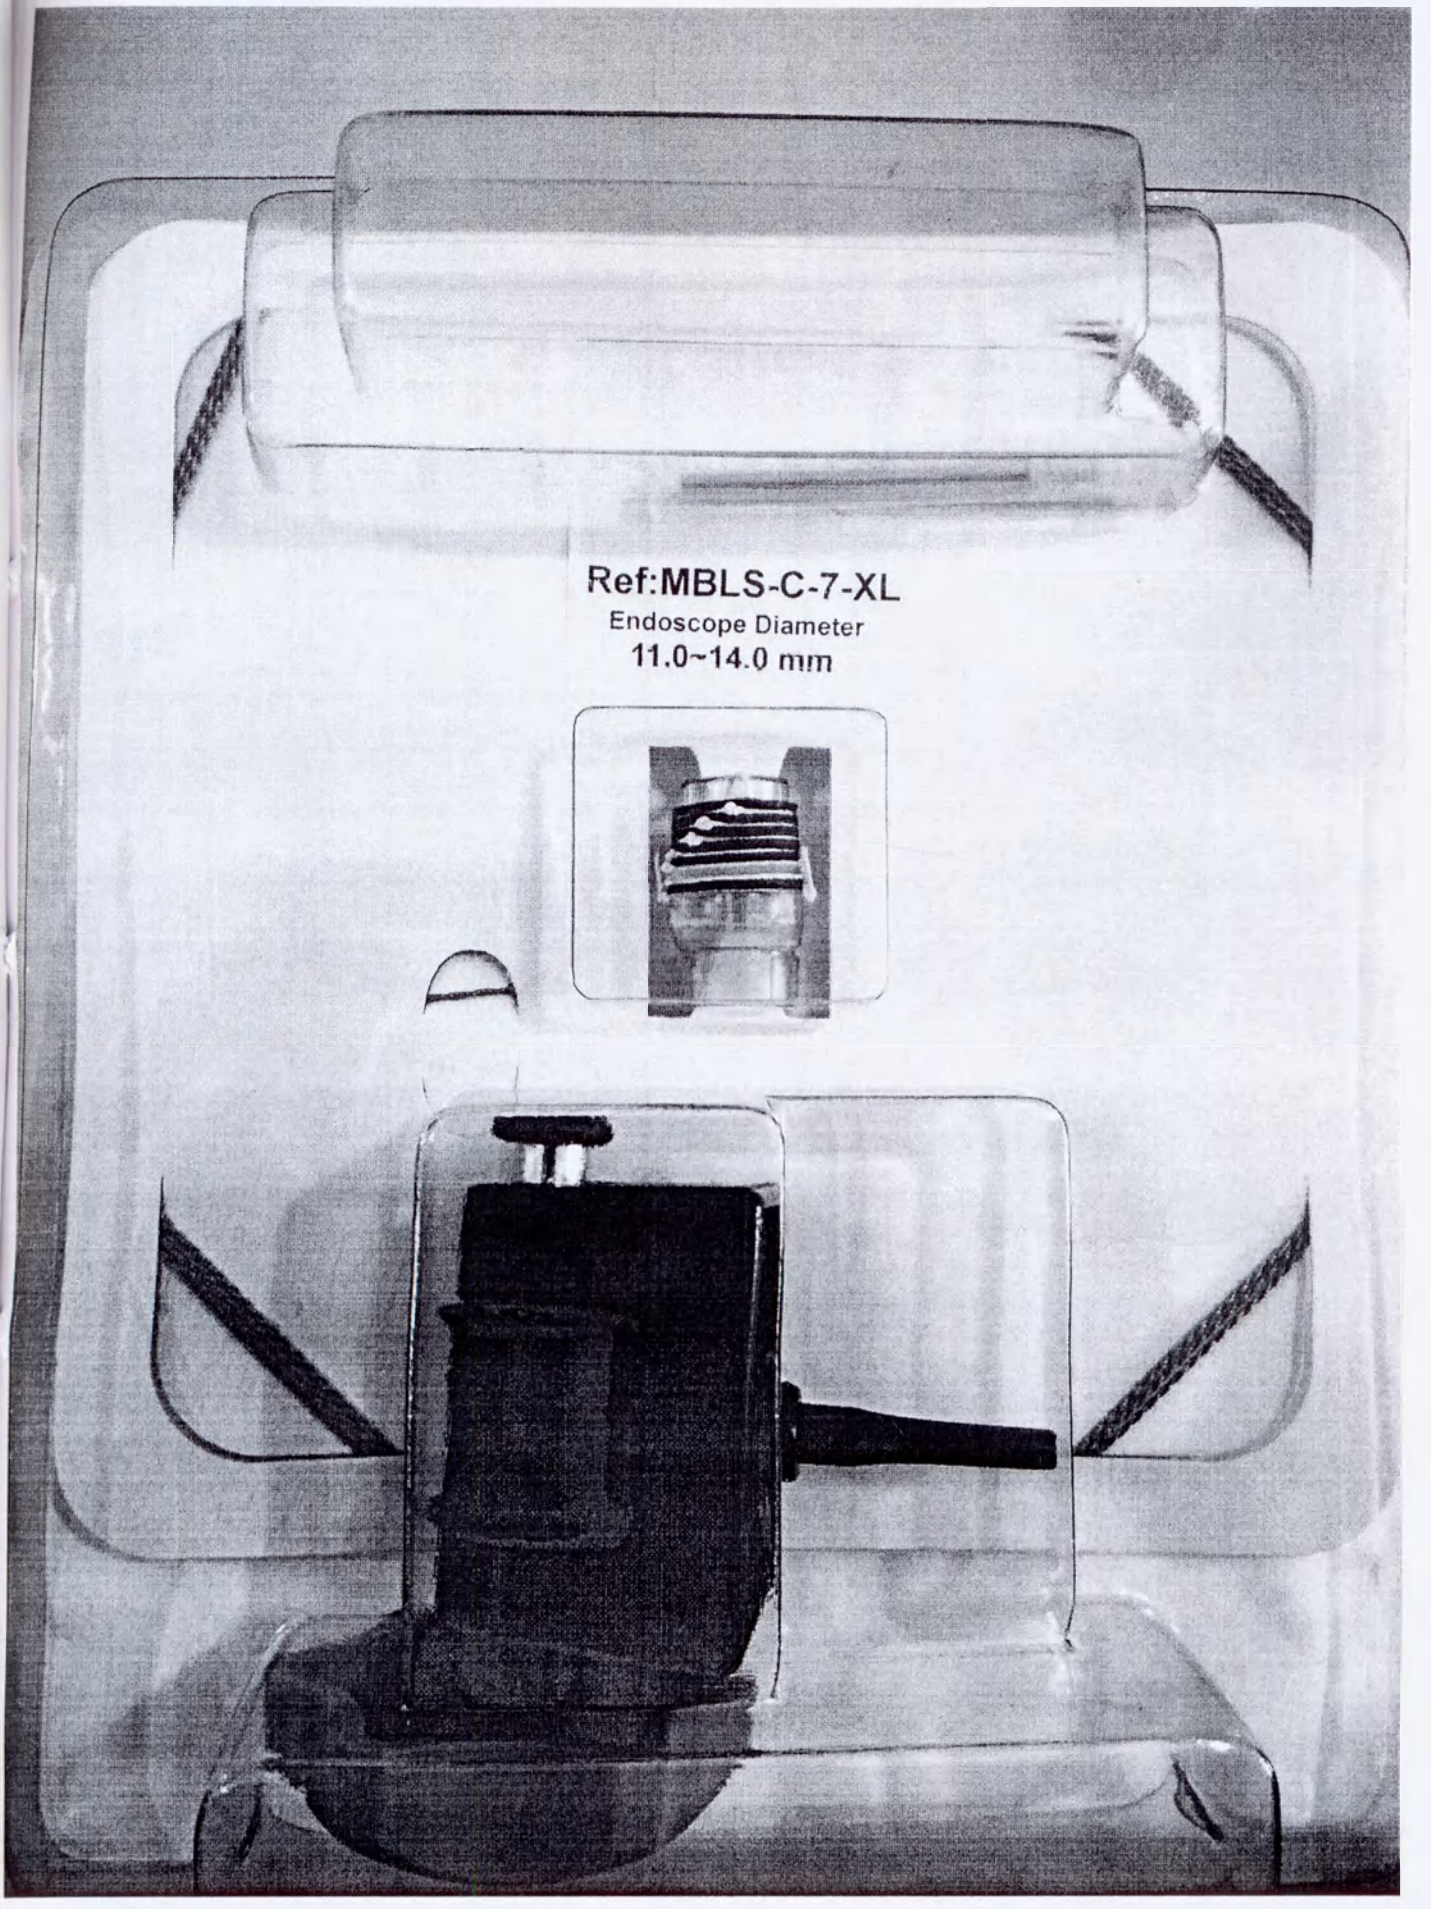

Ref:MBLS-C-7-XL
Endoscope Diameter
11.0~14.0 mm

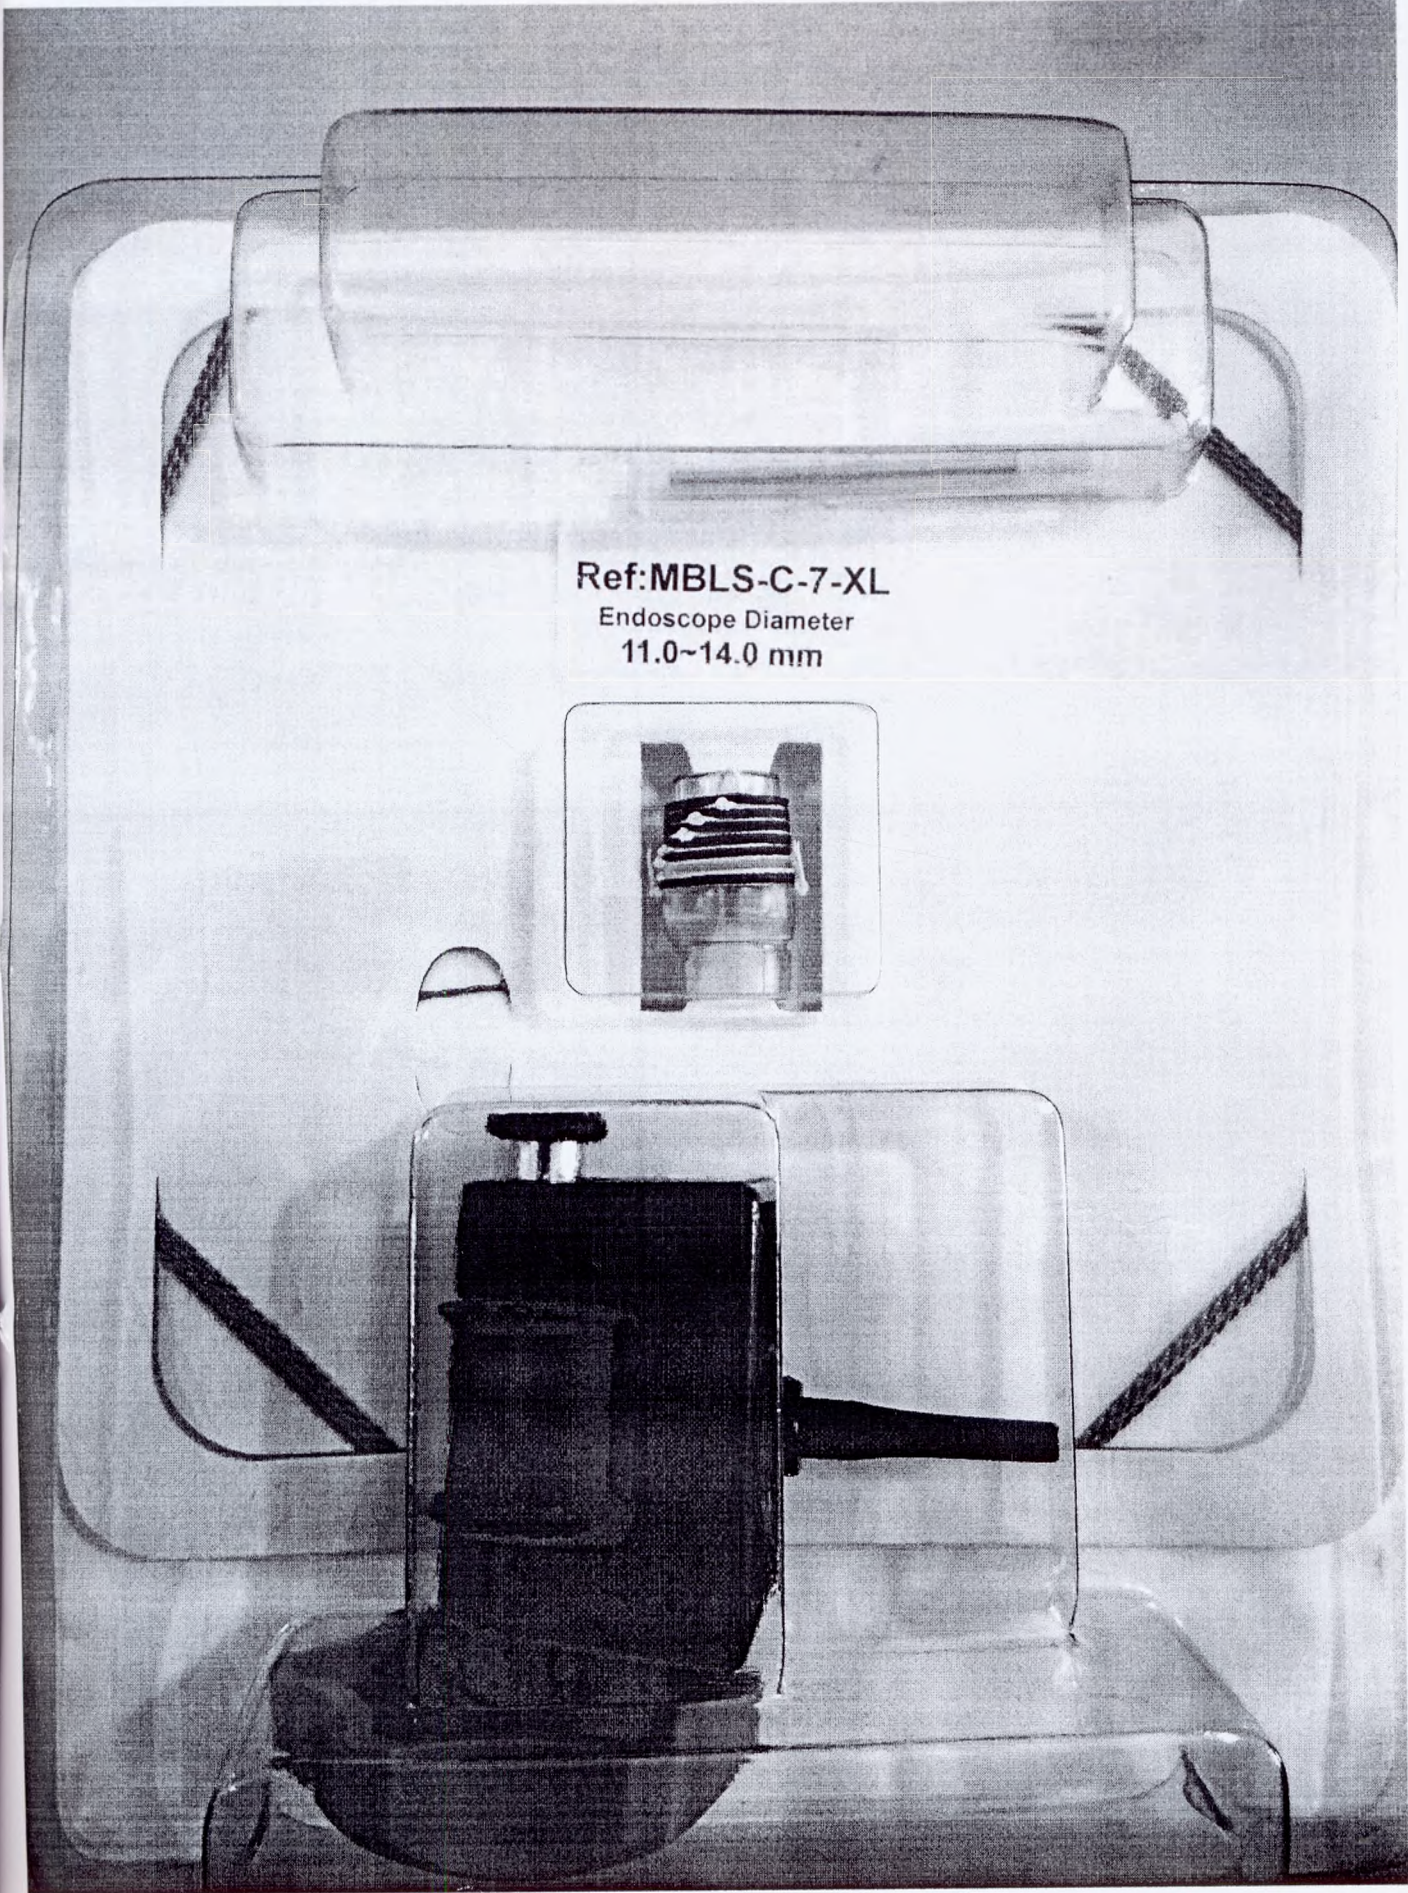



Ref:MBLS-C-7-XL
Endoscope Diameter
11.0~14.0 mm

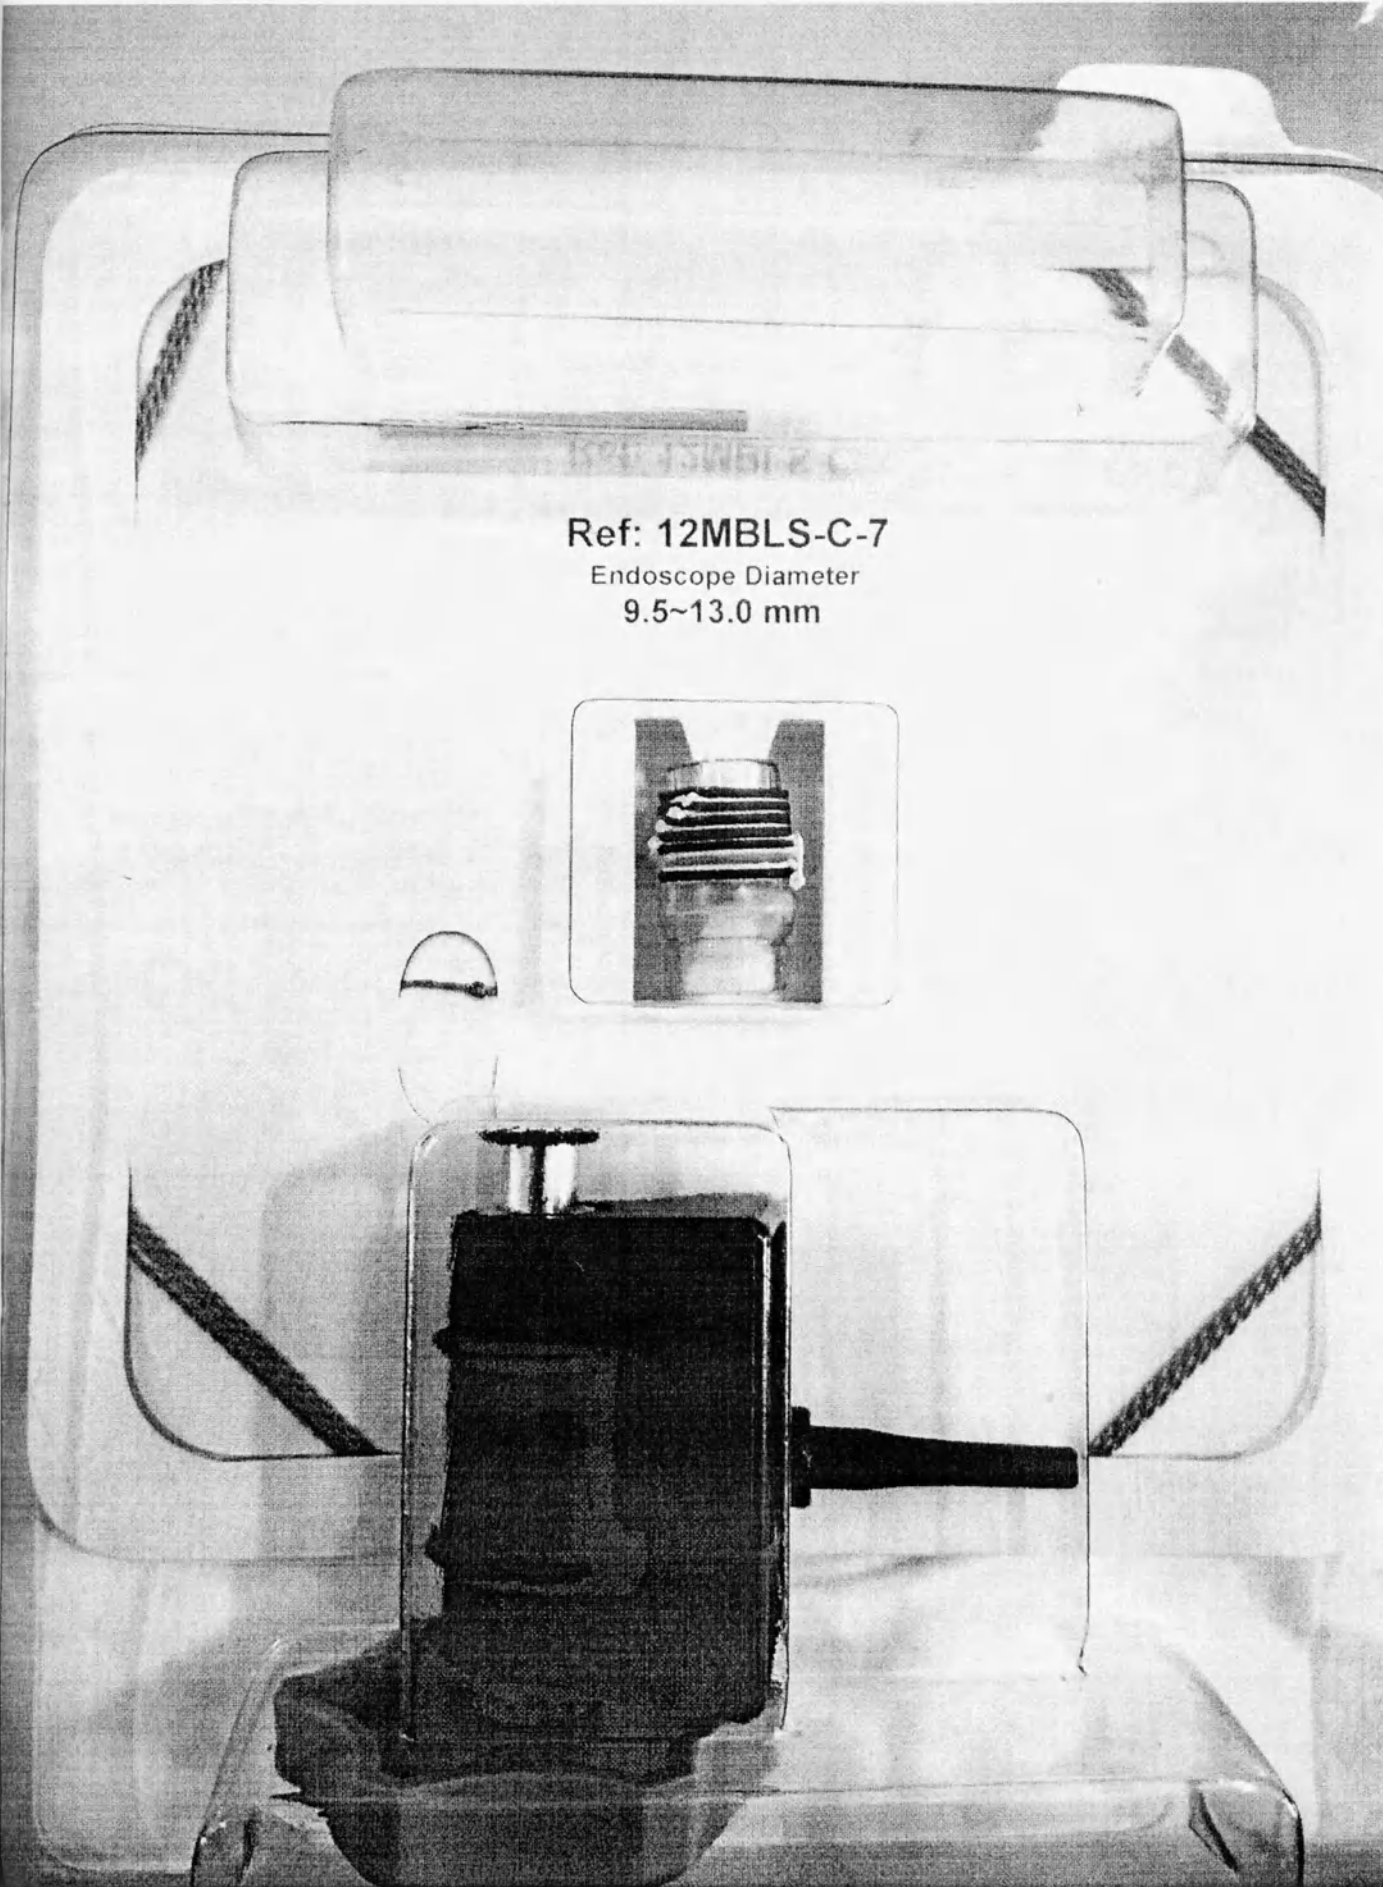

Ref: 12MBLS-C-7

Endoscope Diameter
9.5~13.0 mm

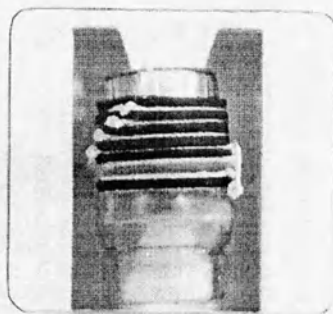


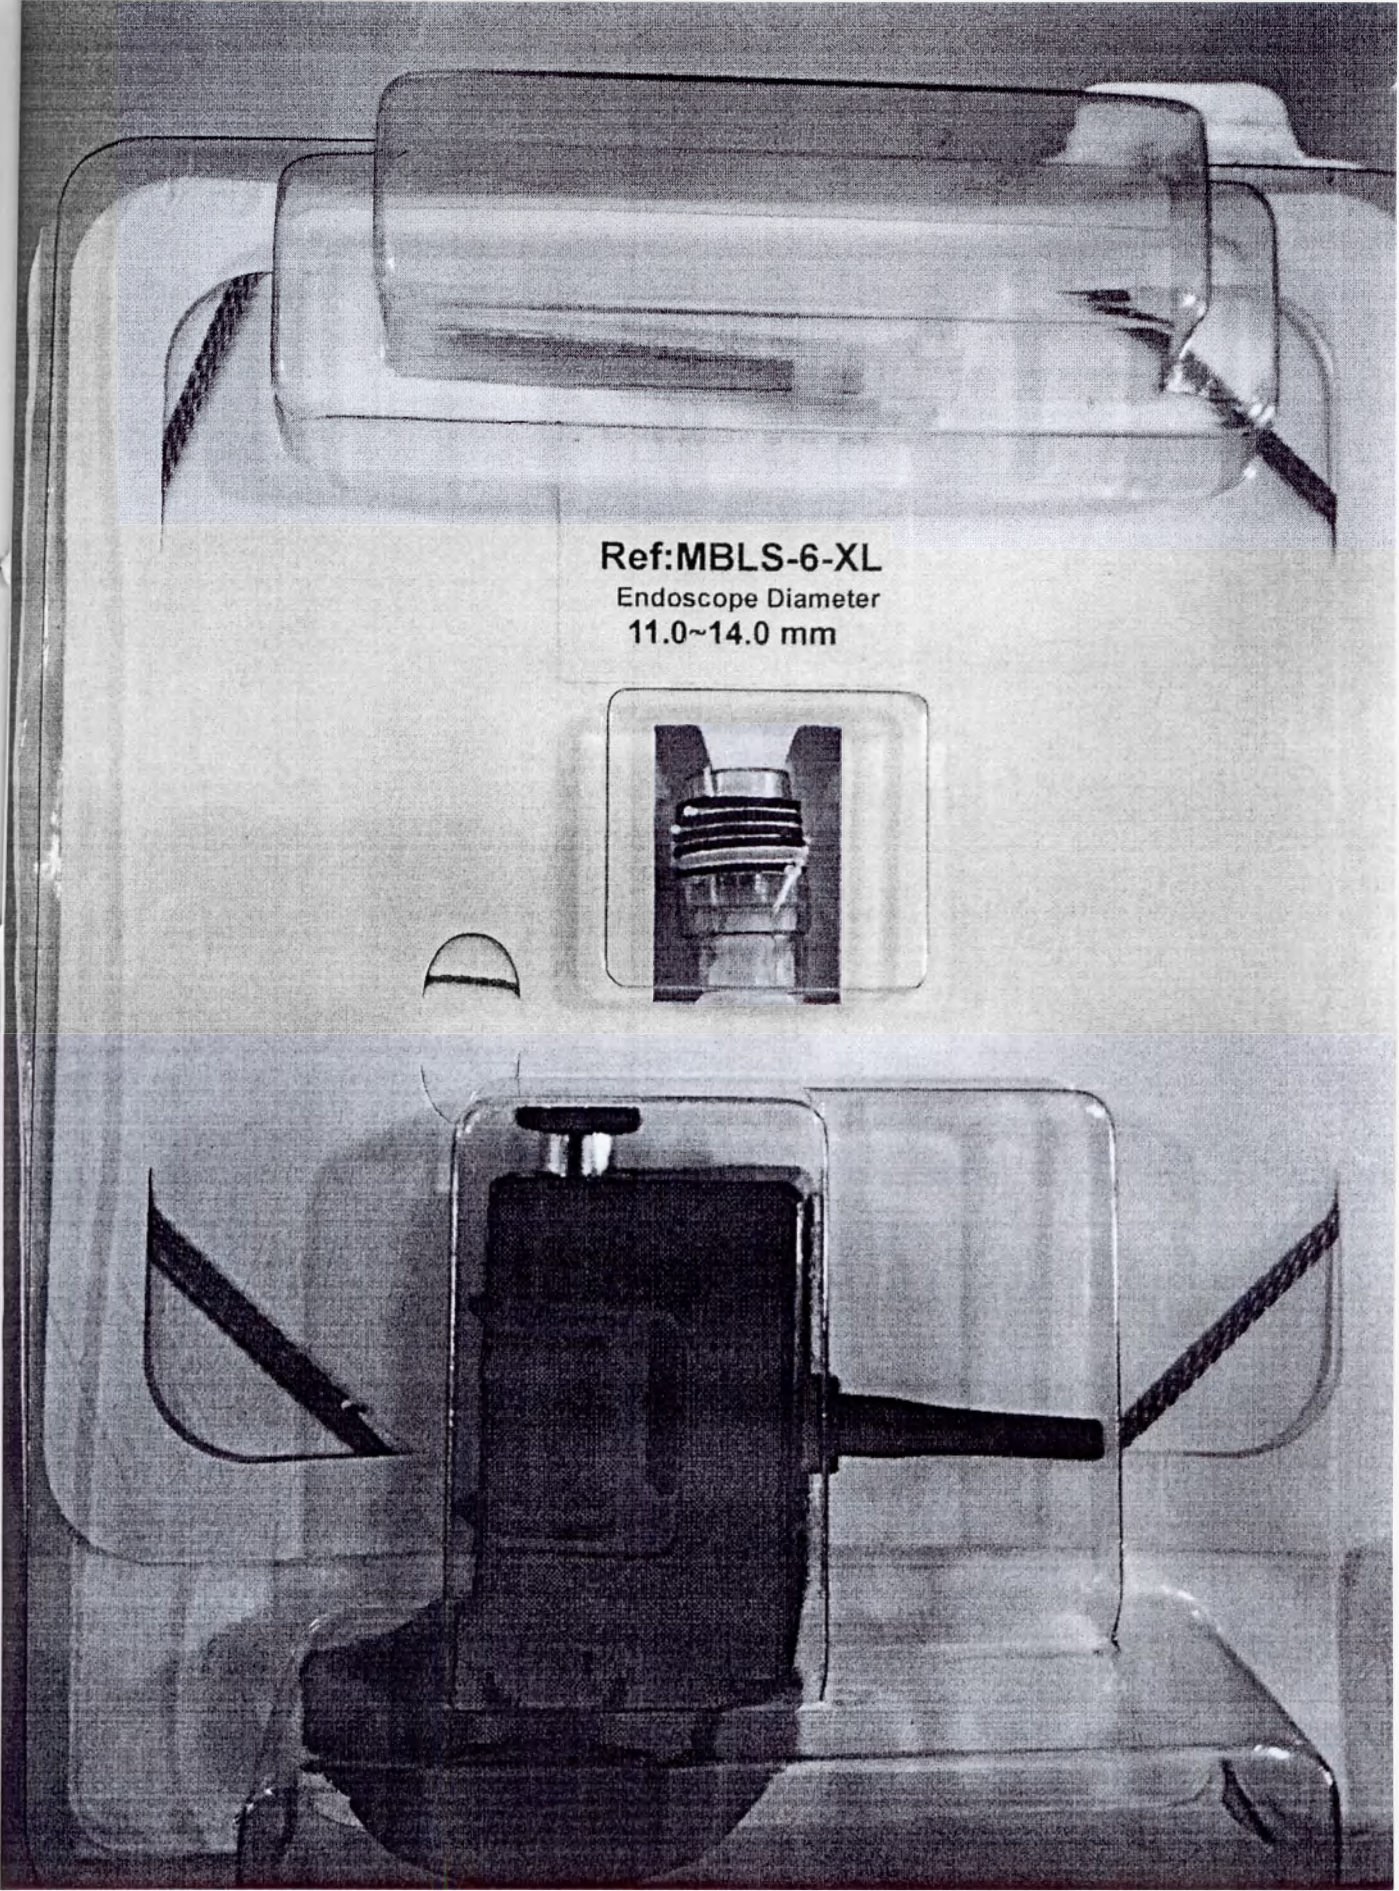


The image shows an endoscope, model MBL-6-XL, inside its clear plastic carrying case. The case is open, revealing the endoscope's handle at the top and its long, flexible shaft extending downwards. A small, square inset window in the center of the case provides a magnified view of the distal tip of the endoscope, which features a series of concentric rings and a central channel. The case is secured with black straps on the sides. The background is a plain, light-colored surface.

Ref:MBLS-6-XL

Endoscope Diameter
11.0~14.0 mm

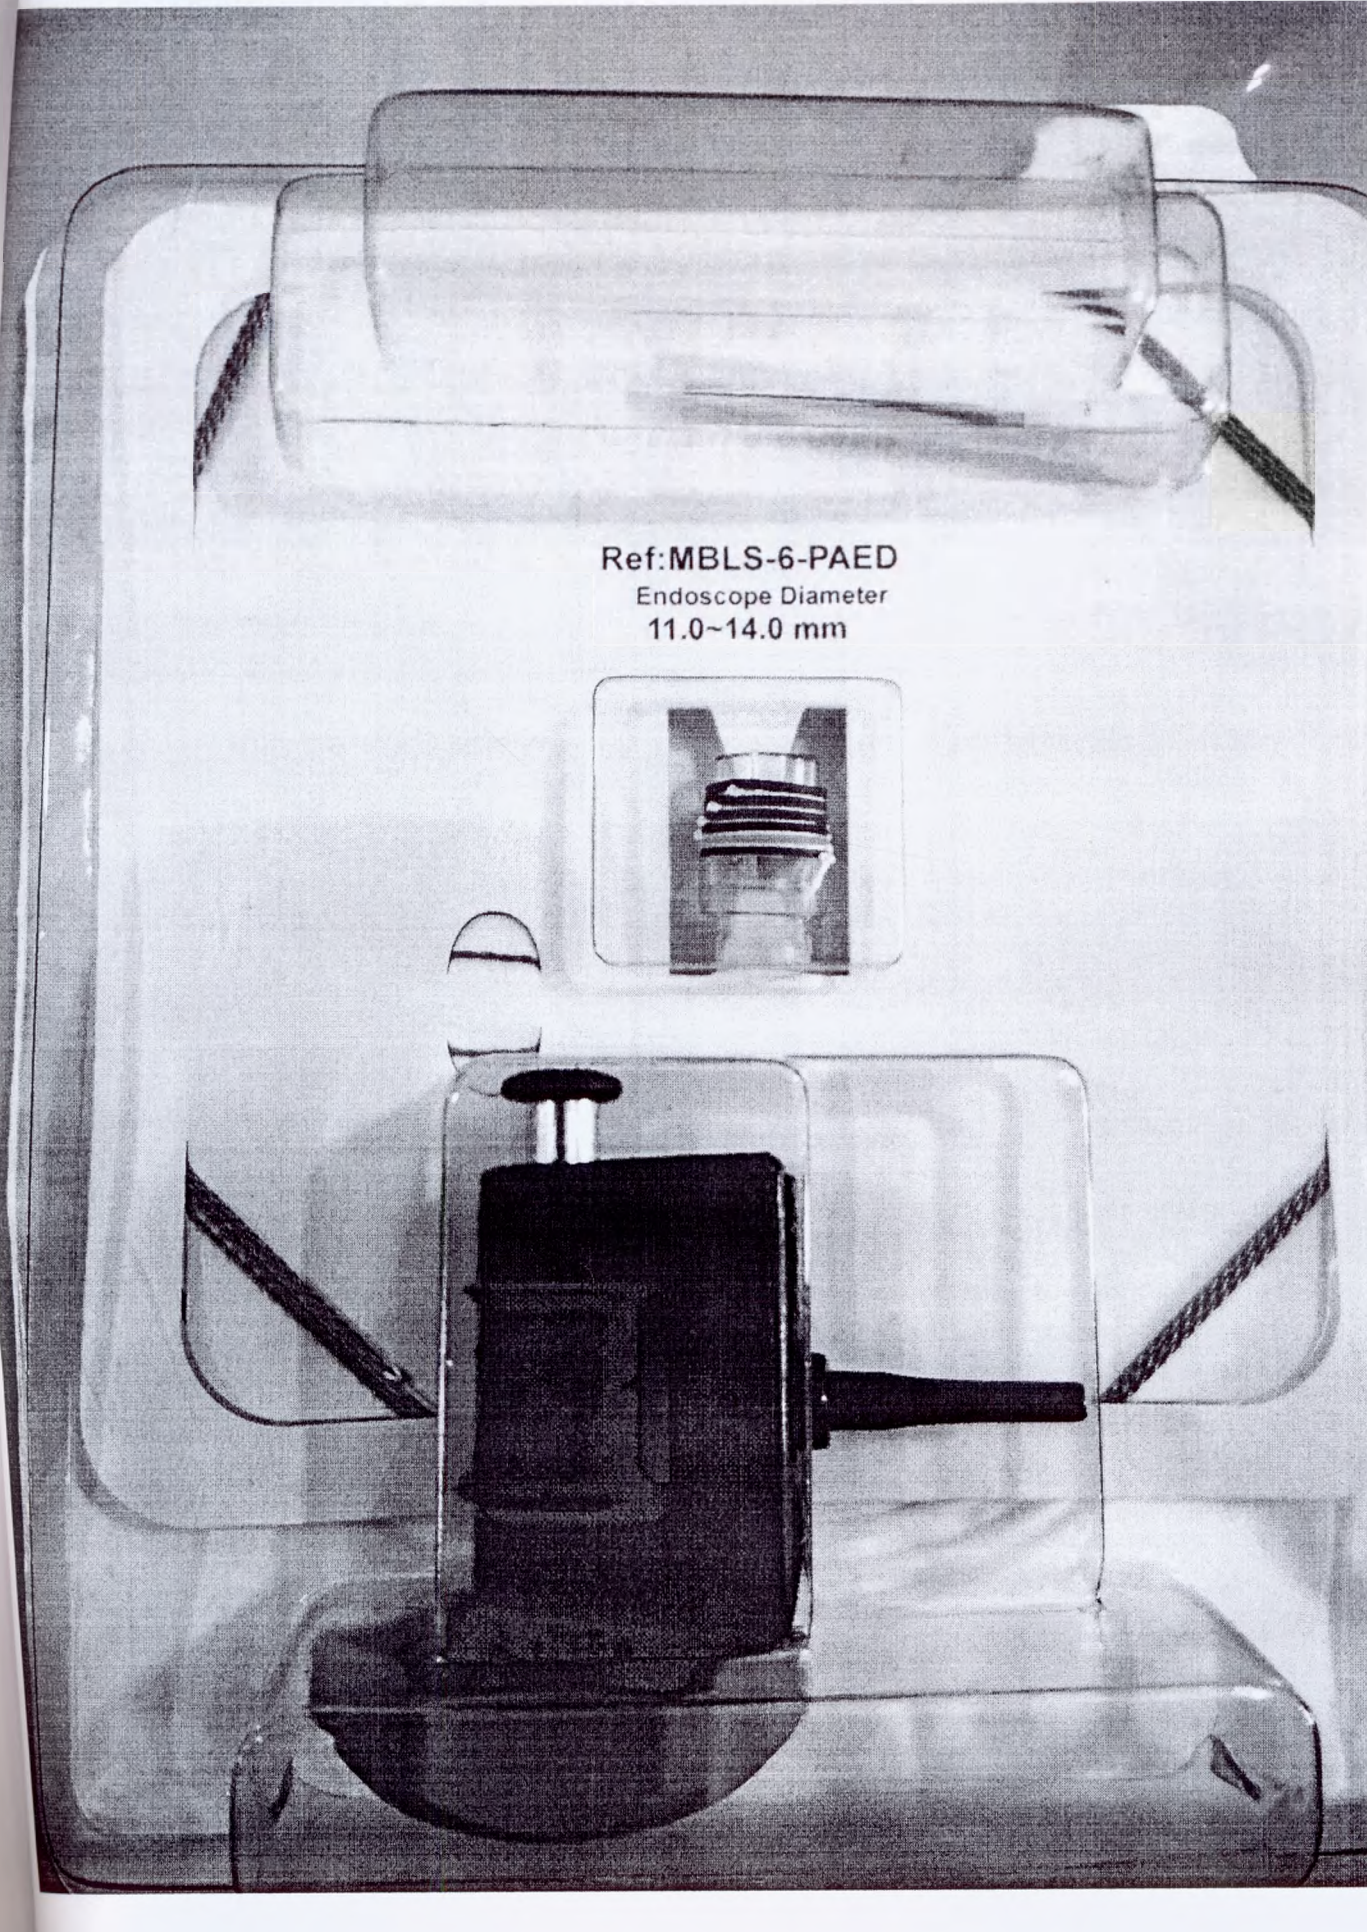

Ref:MBLS-6-PAED
Endoscope Diameter
11.0~14.0 mm

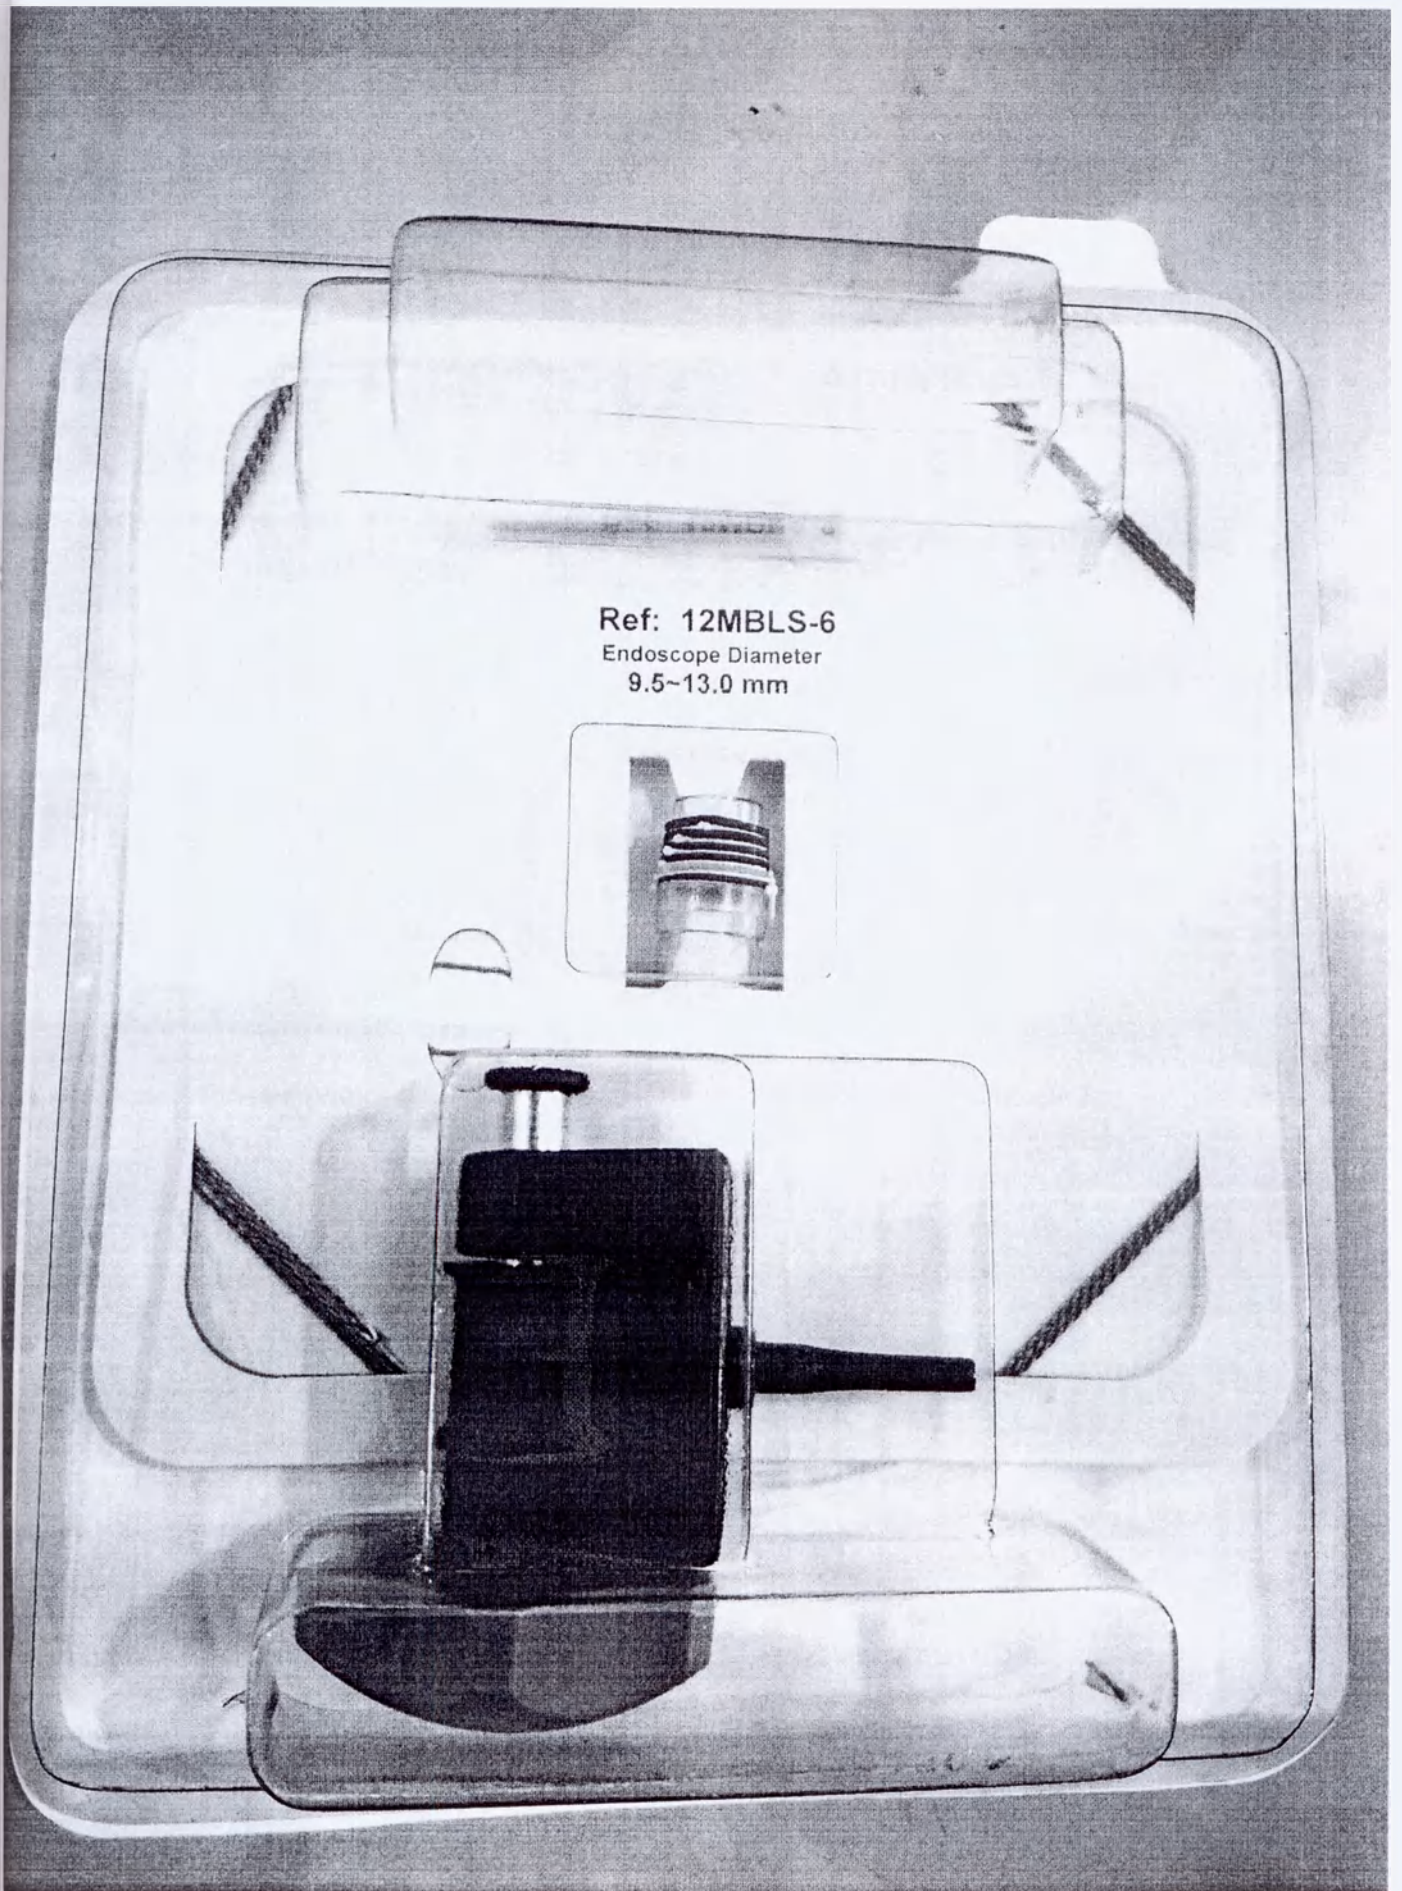

Ref: 12MBLS-6
Endoscope Diameter
9.5~13.0 mm

MULTI BAND LIGATOR

REF	12MBLS-6	Scope Dia.	CE 2460 Rx Only
LOT	2017/1004	9.5~13.0 mm	NON STERILE
	2019/04	Min Ch Dia.	
	2017/10	2.8 mm	
		No of Bands	
		6	
		Quantity	
		1	

MULTI BAND LIGATOR	MULTI BAND LIGATOR	MULTI BAND LIGATOR
REF 12MBLS-6	REF 12MBLS-6	REF 12MBLS-6
LOT 2017/1004	LOT 2017/1004	LOT 2017/1004
2019/04	2019/04	2019/04
8 908007 150129	8 908007 150129	8 908007 150129



MED DEVICES LIFESCIENCES LIMITED
The Black Church, St. Mary's Place, Dublin - 7, Ireland
Tel: +35 37668 01106. Email: info@meddevices.net

Specially manufactured for:
Endoskopie, W. Haag KG, Germany by:

Medelec CE 2460
SYSTEMS PVT. LTD
D-9 KALINDI COLONY, RING ROAD, NEW DELHI 110 065, INDIA
Tel: +91-11-26844289, 26827952
website: www.medelec.net, e-mail: info@medelec.net

MED DEVICES LIFESCIENCES LIMITED
The Black Church, St. Mary's Place
Dublin - 7, Ireland
Tel: +35 37668 01106
Email: info@meddevices.net

Маркировка: Устройство для эндоскопического лигирования (Multiple Band Ligator) в варианте исполнения 12MBLS-6

OmniView

CE 2460

MULTIPLE BAND LIGATOR

Minimum Channel Diameter : 2.8 mm



R_X ONLY



Medelec
Systems Pvt. Ltd.

Works: 129B, HSIIDC, Sector 31, Faridabad 121003, Haryana, INDIA
Reg. Office: D-9 Kalindi, New Delhi 110065, INDIA
Customer Care: info@medelec.net, website: medelec.net

EC REP

MED DEVICES LIFESCIENCES LIMITED

20-22 Wenlock Road, London, N1 7GU, U.K.
Contact: (+44 - 84552 80533), E-mail: info@meddevices.net

Ref: MSPL/LAB/MBLS-TH, Issue# 01, Date 15/12/2017, Rev. 03

OmniView

CE 2460

MULTIPLE BAND LIGATOR

Minimum Channel Diameter : 2.8 mm



R_X ONLY



Medelec
Systems Pvt. Ltd.

Works: 129B, HSIIDC, Sector 31, Faridabad 121003, Haryana, INDIA
Reg. Office: D-9 Kalindi, New Delhi 110065, INDIA
Customer Care: info@medelec.net, website: medelec.net

EC REP

MED DEVICES LIFESCIENCES LIMITED

20-22 Wenlock Road, London, N1 7GU, U.K.
Contact: (+44 - 84552 80533), E-mail: info@meddevices.net

Ref: MSPL/LAB/MBLS-TH, Issue# 01, Date 15/12/2017, Rev. 03

OmniView

CE 2460

MULTIPLE BAND LIGATOR

Minimum Channel Diameter : 2.8 mm



R_X ONLY



Medelec
Systems Pvt. Ltd.

Works: 129B, HSIIDC, Sector 31, Faridabad 121003, Haryana, INDIA
Reg. Office: D-9 Kalindi, New Delhi 110065, INDIA
Customer Care: info@medelec.net, website: medelec.net

EC REP

MED DEVICES LIFESCIENCES LIMITED

20-22 Wenlock Road, London, N1 7GU, U.K.
Contact: (+44 - 84552 80533), E-mail: info@meddevices.net

Ref: MSPL/LAB/MBLS-TH, Issue# 01, Date 15/12/2017, Rev. 03

OmniView

CE 2460

MULTIPLE BAND LIGATOR

Minimum Channel Diameter : 2.8 mm



R_X ONLY



Medelec
Systems Pvt. Ltd.

Works: 129B, HSIIDC, Sector 31, Faridabad 121003, Haryana, INDIA
Reg. Office: D-9 Kalindi, New Delhi 110065, INDIA
Customer Care: info@medelec.net, website: medelec.net


EC REP


MED DEVICES LIFESCIENCES LIMITED


20-22 Wenlock Road, London, N1 7GU, U.K.
Contact: (+44 - 84552 80533), E-mail: info@meddevices.net

Ref: MSPL/LAB/MBLS-TH, Issue# 01, Date 15/12/2017, Rev. 03

5 pkt. 20.02.18

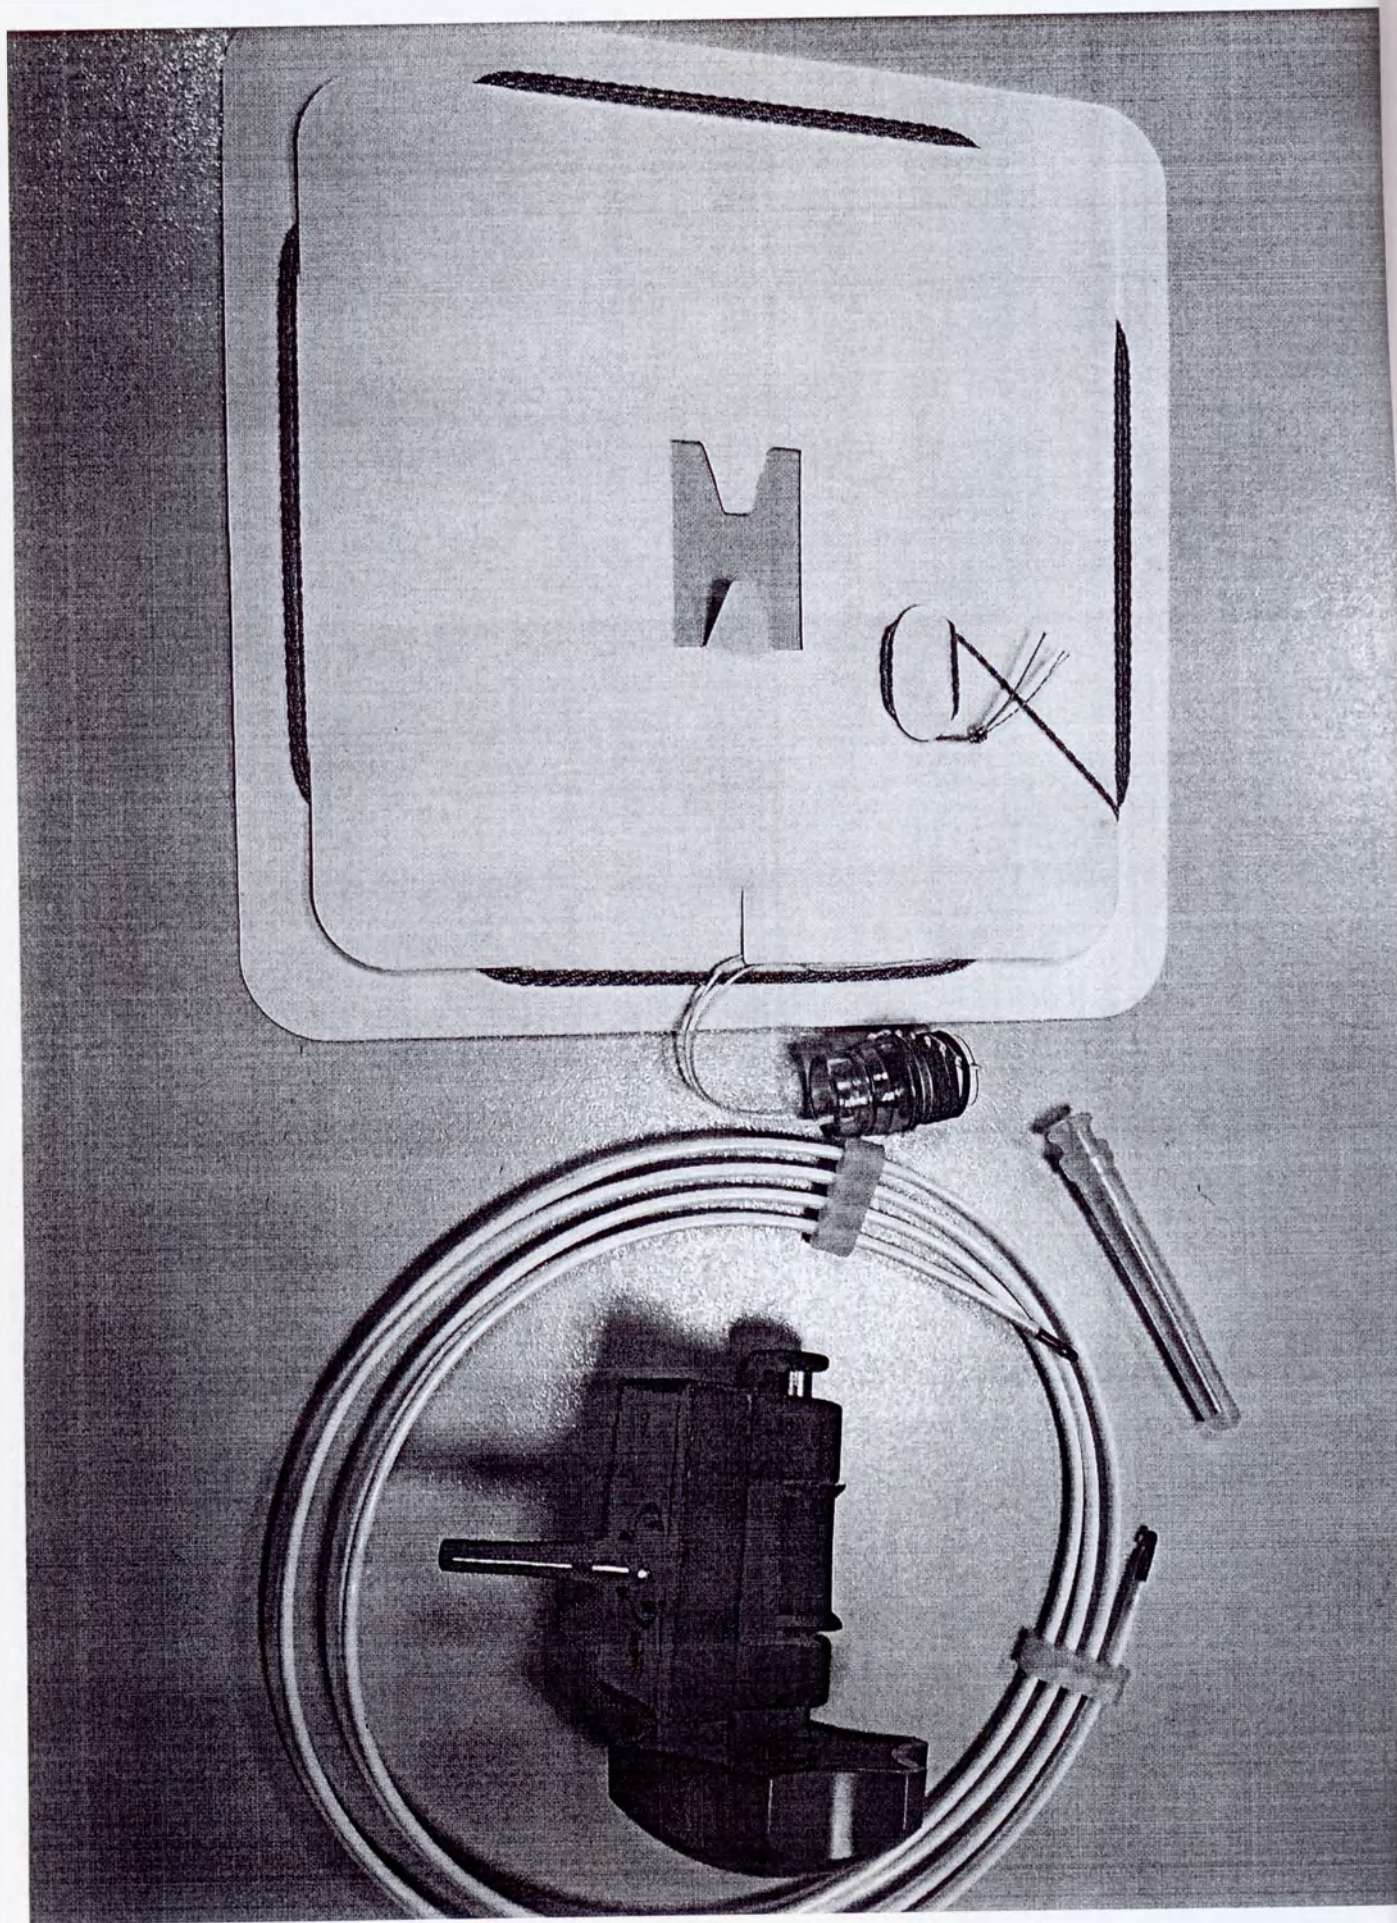

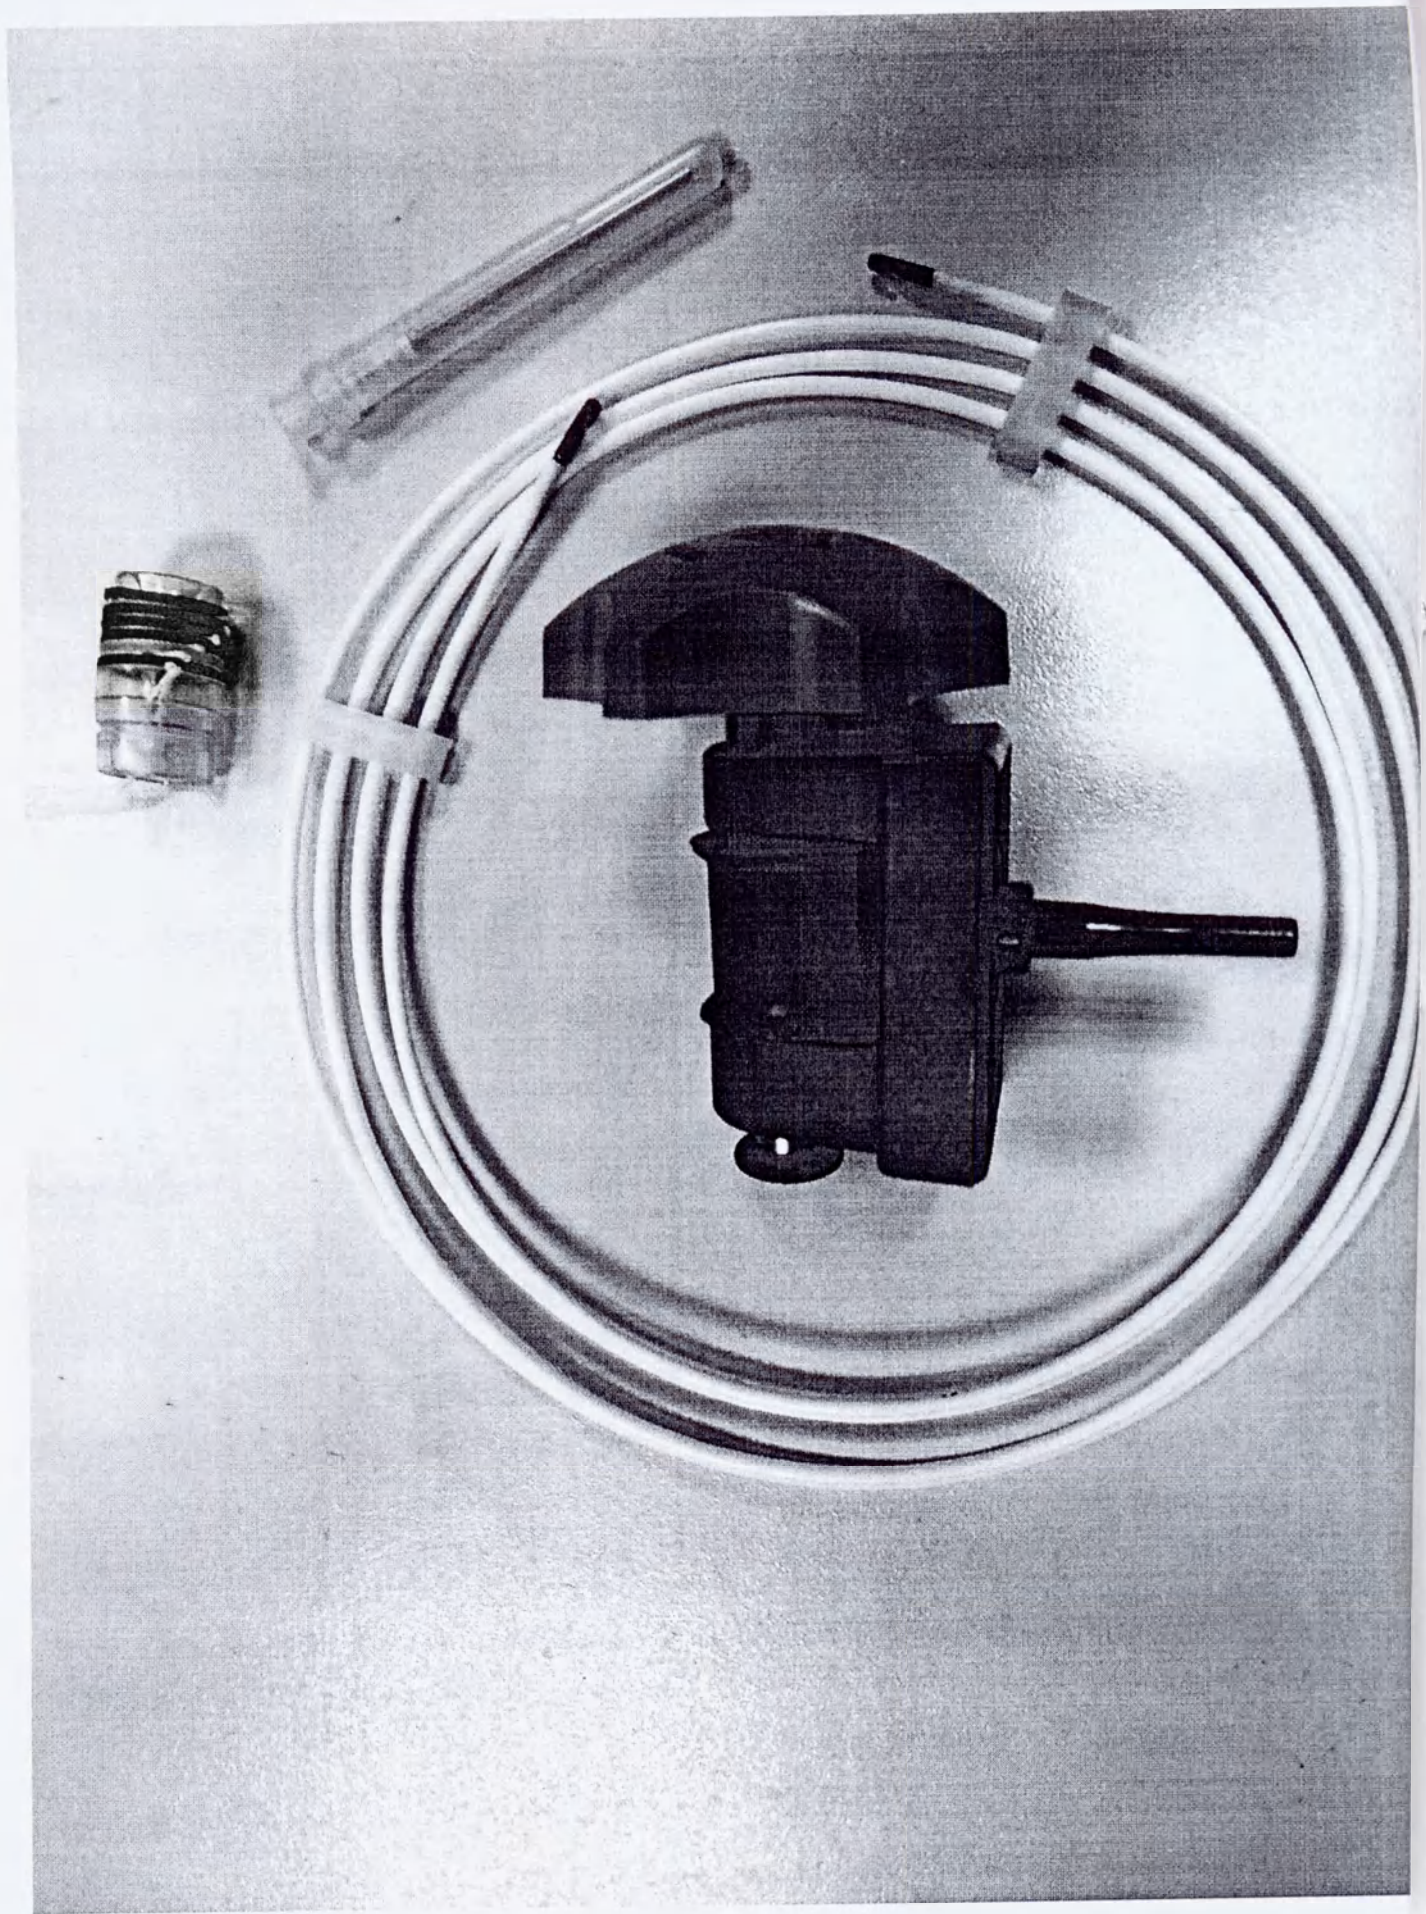

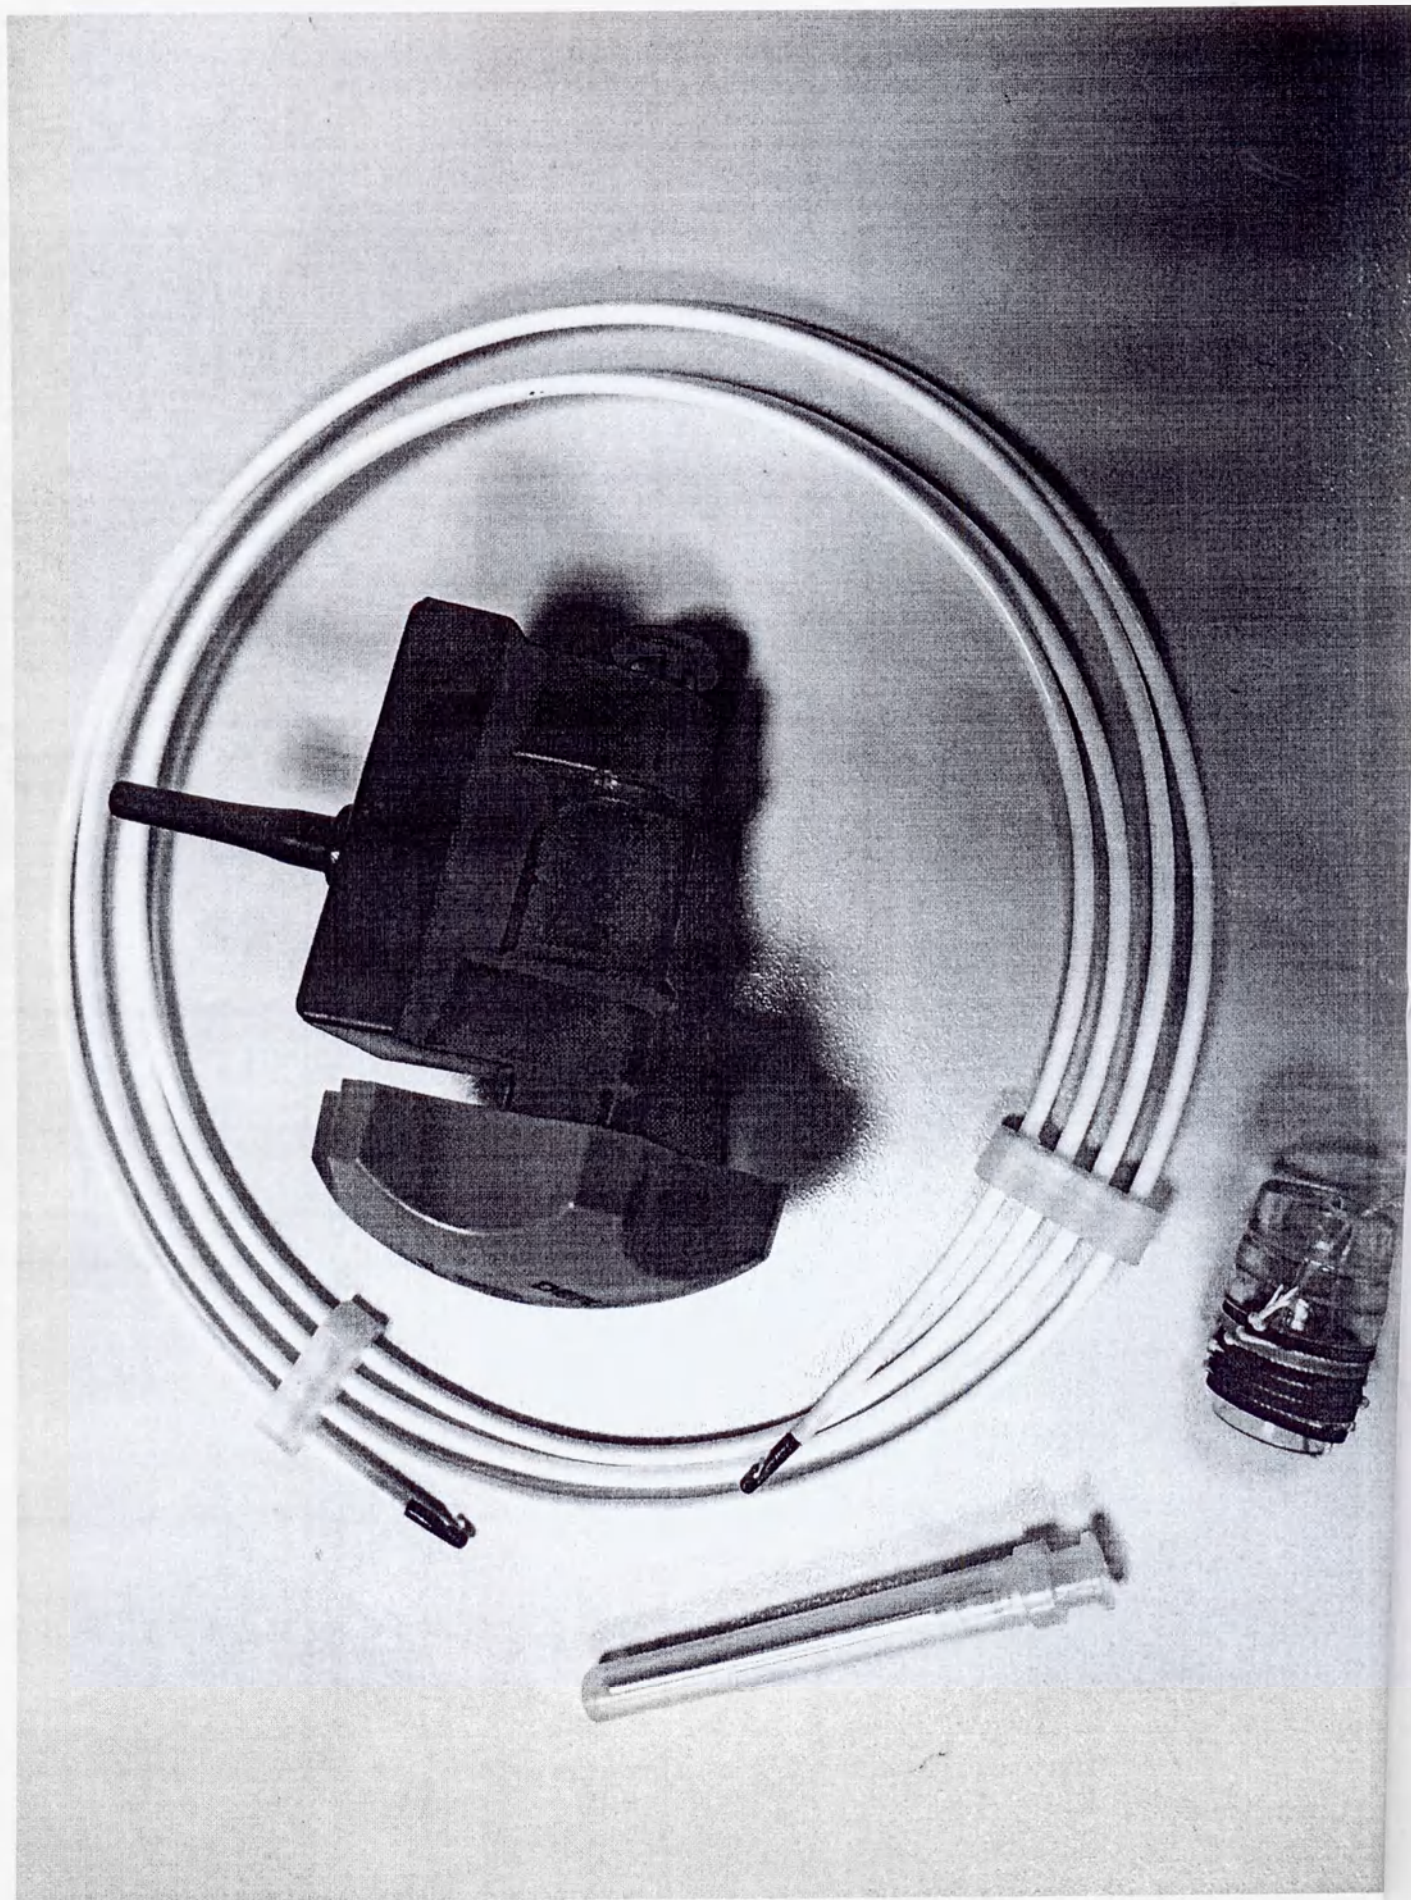

КОПИЯ ВЕРНА
ДИРЕКТОР
ООО «ДЕЛГА-МЕДИС»
ШАЛАЕВ В. В.

Итого в документе
прошито и пронумеровано

15 (Пятнадцать) листов

Директор ООО «Делга-Медис»

В.В. Шалаев

