

**Фотографические изображения медицинского изделия «Электрод
биполярный ELRA», производства «СТАРмед Ко., Лтд.», Корея,
«STARmed Co., Ltd.», B-1403, DAEBANG TRIPLAON, 158, Haneulmaeul-
ro, Ilsandong-gu, Goyang-si, Gyeonggi-do, Republic of Korea. Тел.: +82(506)-
816-3546 Факс: +82(506)-816-4546 E-mail: Info@STARmed4u.com)**



ELRA
[Bipolar type] **Electrode**

REF 7-4B18L

Ground Pad

18mm
178mm

LOT 7NEL7518RJ17007

2018-10-24 2021-10-23

STERILE EO

CE 0120

EMERGO EUROPE
Prinsessegracht 20 2514 AP The Hague The Netherlands

STARMed Co., Ltd.
2-1-401, DAEJANG TRIPLACK, 191, Haeundae-dong,
Busanjin-gu, Gyeongsang-si, Gyeongsang-do, Republic of Korea

TEL: +82-506-810-3046 FAX: +82-506-816-4546


ST-LS-306(1)(Rev.3)
MADE IN KOREA

Barcode 1: 1108809306762399
Barcode 2: 1108809306762399
Barcode 3: 1108809306762399
Barcode 4: 1108809306762399

ELRA Electrode
E. O. G

ELRA
Electrode
[Bipolar type]

REF 7-4B18L

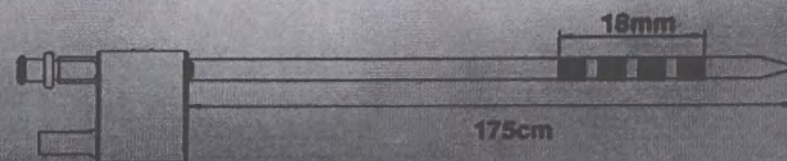

LOT 7NEL7518RJ17007

2018-10-24 2021-10-23



STERILE EO



CE
0120

EC REP

EMERGO EUROPE

Prinsesgracht 20 2514 AP The Hague The Netherlands




Starkind Co., Ltd

TEL: +82-506-816-3546 FAX: +82-506-816-4546

B-1403, DAEBANG TRIPLAON, 158, Haneulmaeul-ro,
Tisandong-gu, Goyang-si, Gyeonggi-do, Republic of Korea.

ST-LB-250(Rev.9)
MADE IN KOREA

ELRA *Electrode*
[Bipolar type] **REF 7-4B18L**



LOT 7NEL7518RJ17007
2018-10-24 2021-10-23
STERILE EO
CE 0120
EMERGO EUROPE
Prinsengracht 20 2514 AP The Hague The Netherlands
STARmed Co., Ltd. TEL: +82-506-816-2546 FAX: +82-506-816-4546
B-1463, GMSANG TRUPJACH, 158, Hwangnam-d-m, Seongdong-gu, Gwangju-si, Gyeonggi-do, Republic of Korea
ST-4-B-298(10/Rev. 8)
MADE IN KOREA

Global distributor

TaeWoong
MEDICAL

Manufacturer

STARmed




CE
0120

Инструкция по применению на медицинское изделие:

«Электрод биполярный ELRA»


Производства: «СТАРмед Ко., Лтд.», Корея («STARmed Co., Ltd.»)

2. Электрод биполярный ELRA 7-2B11L (в первичной упаковке)

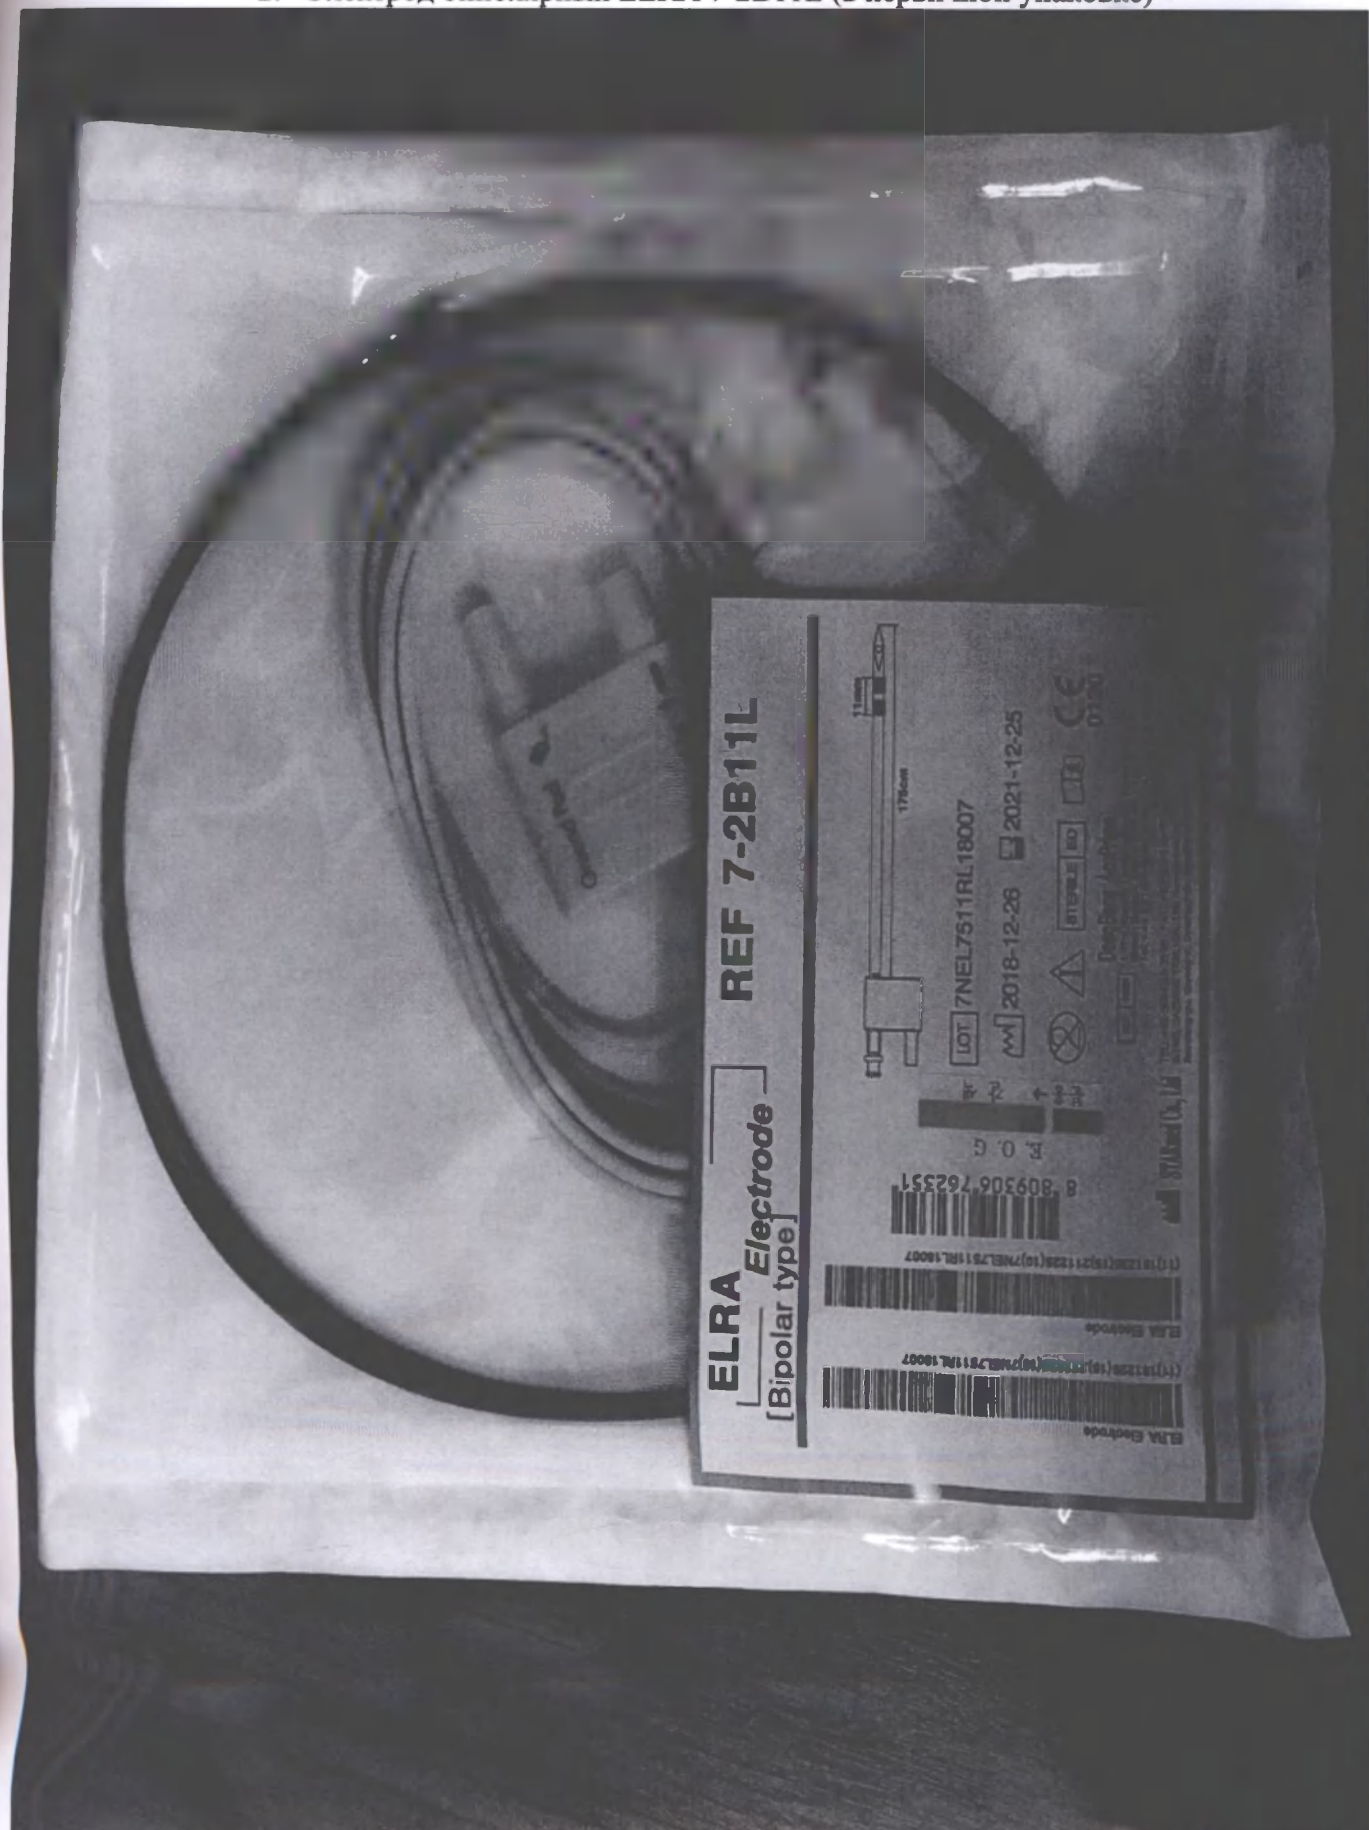

ELRA *Electrode*
[Bipolar type]

REF 7-2B11L



8 809306 762351

(1) 101220 (10) 211220 (10) 77NEL7911ML10007

ELRA Electrode

LOT 7NEL7511RL18007

2018-12-26 2021-12-25

STERILE ISO 1

CE 0120

Disposing Acrylic

1 The Product Name, Intended Patient Use, and the lot number are printed on the electrode.

Tel: +82-506-316-3546 FAX: +82-506-315-4546

10-103, DAEJANG TOWER, 158, Yeosu-ro, Yeosu-si, Jeollanam-do, Korea

2021-12-26 (10) 211220 (10) 77NEL7911ML10007

ELRA Electrode

GLOBAL Co., Ltd

Global distributor


ToeWoong
MEDICAL

3. Электрод биполярный ELRA 7-2B22L (в первичной упаковке)



ELRA
Electrode
[Bipolar type]

REF 7-2B22L



LOT 7NEL7522SA22005

2019-01-29 2022-01-28

STERILE EO 0120

DongBang AcuPrime
1 The Forum Units, Haverock Road East
Marsh Barton, Exeter EX2 8PU, UK
Tel: +44 (0)1392 829500 Fax: +44 (0)1392 823232

STARmed Co., Ltd
TEL: +82-506-816-1546 FAX: +82-506-816-4545
B-1401, DAIZANG TROPLEAK 119, Haeundae-dong, Busan-gu,
Daejeon-gi, Chungcheong-do, Republic of Korea

ST-LB-096(11)(Rev.0)
MADE IN KOREA

ELRA Electrode (01)08809306762375
(11)180129(15)220128(10)7NEL7522SA22005
ELRA Electrode (11)180129(15)220128(10)7NEL7522SA22005

Global distributor

TaeWoong
MEDICAL




Manufacturer





ELRA REF 7-4B33L


Electrode
[Bipolar type]



LOT 7NEL7533RG03005

2018.07.10 2021.07.10

8 809306 762412

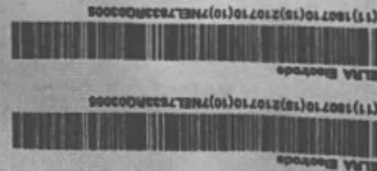

Disposable Acupuncture

The Electrode is Sterile and Single-Use Only

For Use with the ELRA 7-4B33L Electrode


Manufactured by: ELRA, Inc., 10000 El Camino Real, Suite 100, San Diego, CA 92121, USA

ELRA *Electrode*
[Bipolar type]

REF 7-4B33L



8 809306 762412

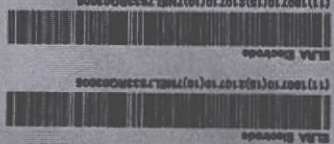

LOT 7NEL7533RG03005

2018.07.10 2021.07.10

STERILE

CE 0120

Disinfecting Instructions

1. The Electrode must be disinfected before use.


2. The Electrode must be disinfected in a solution of 1% sodium hypochlorite for 10 minutes.


3. The Electrode must be rinsed with sterile water before use.

4. The Electrode must be stored in its original packaging until use.


Manufacturer
STARmed

Global distributor
Toshiba

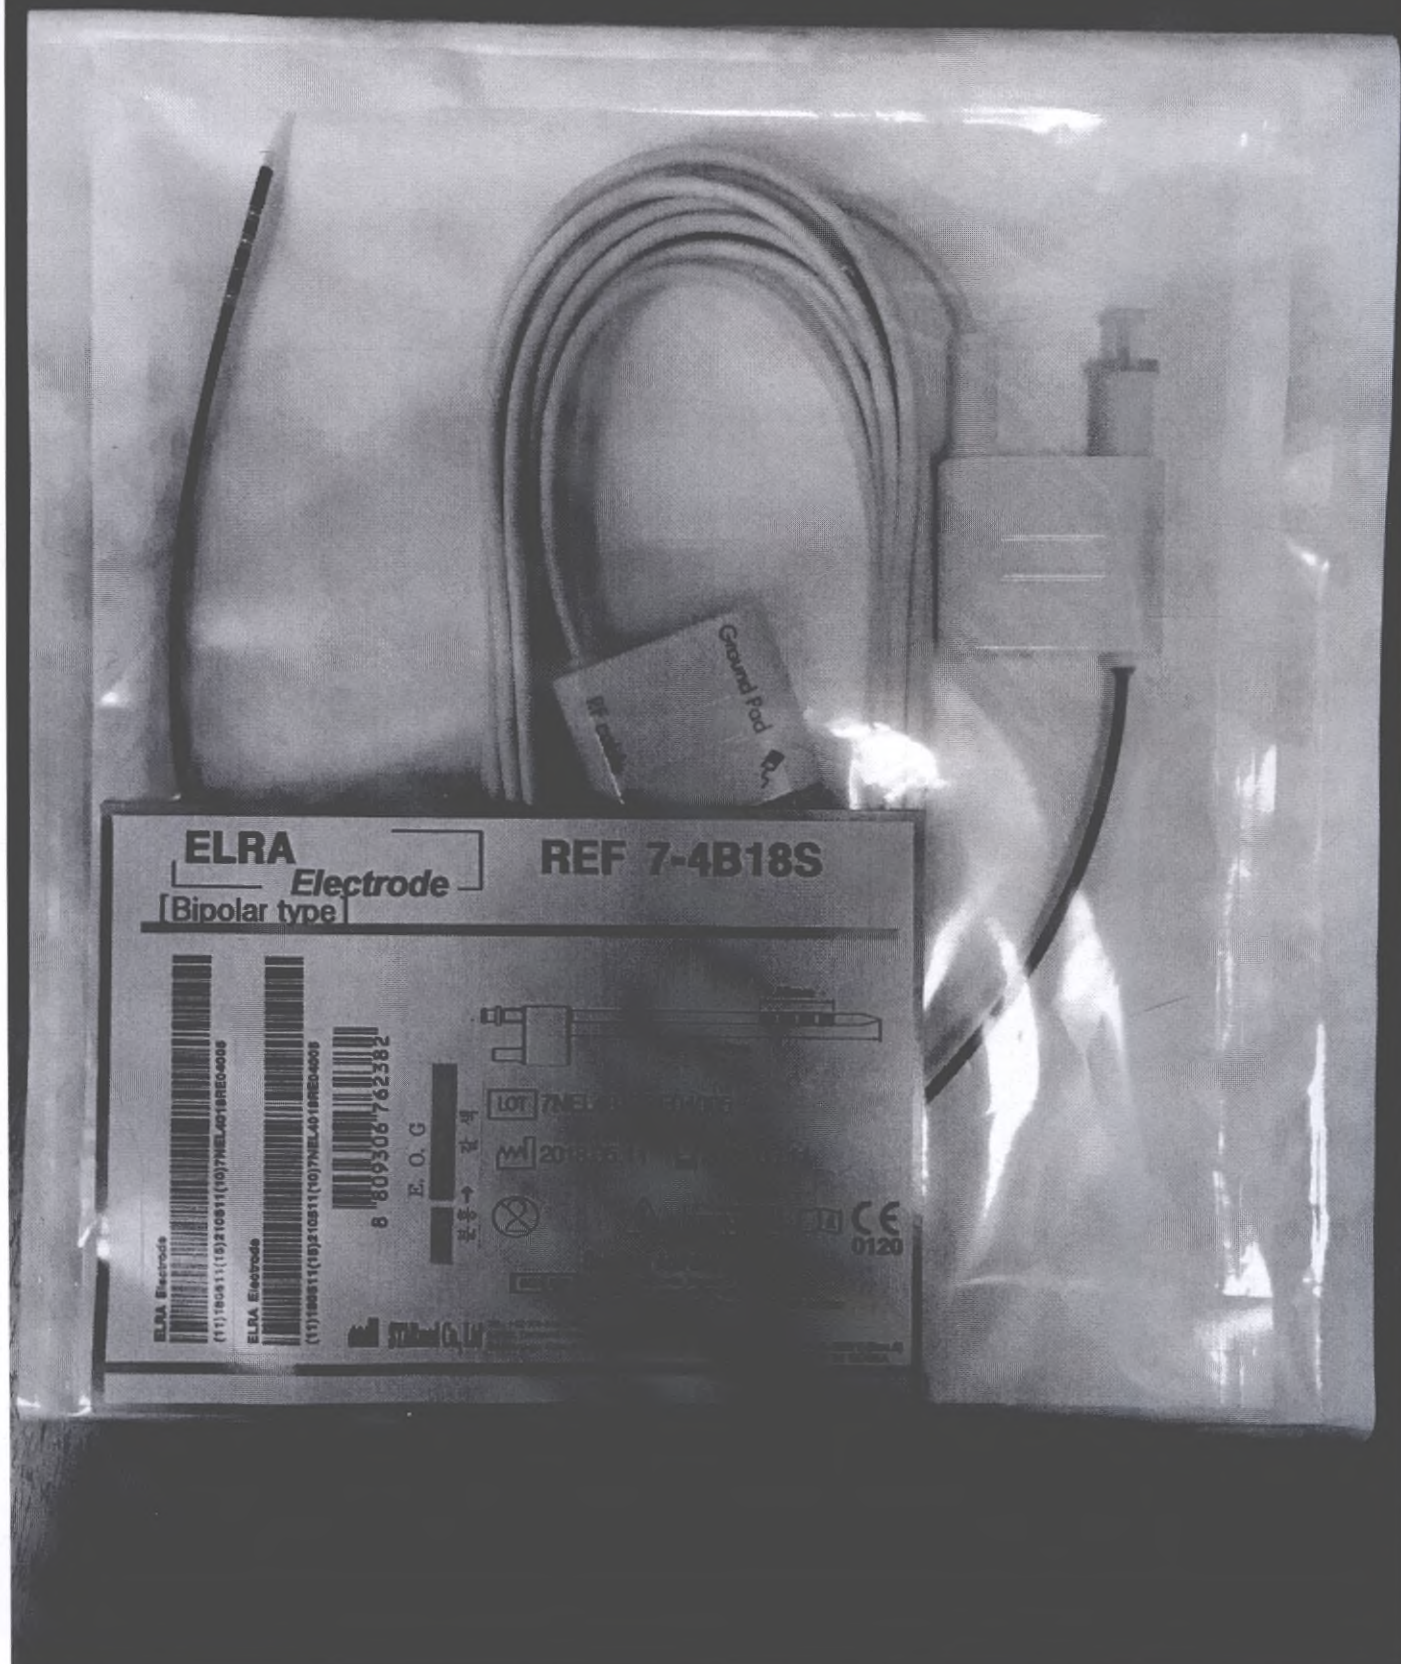

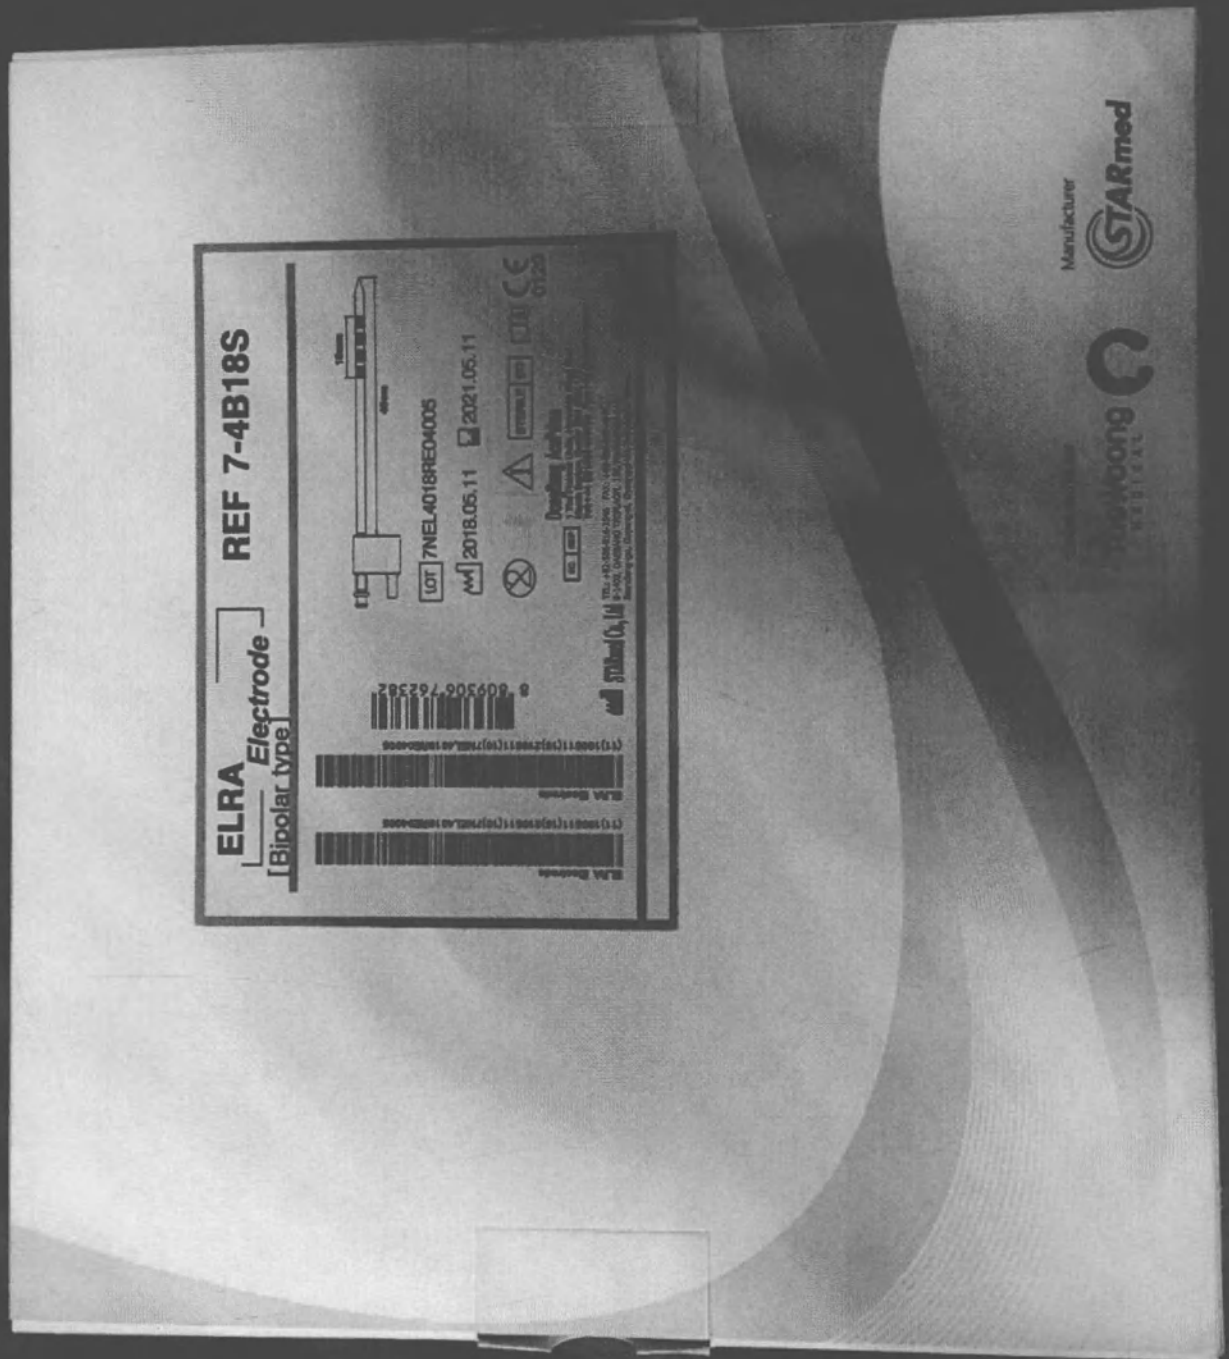




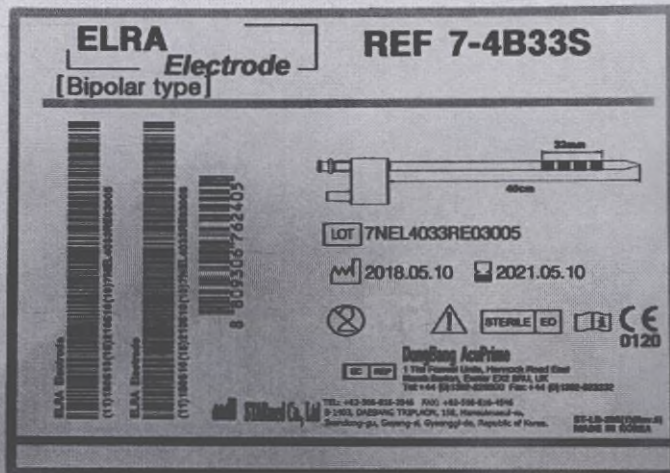

TaeWoong
MEDICAL

Manufacturer



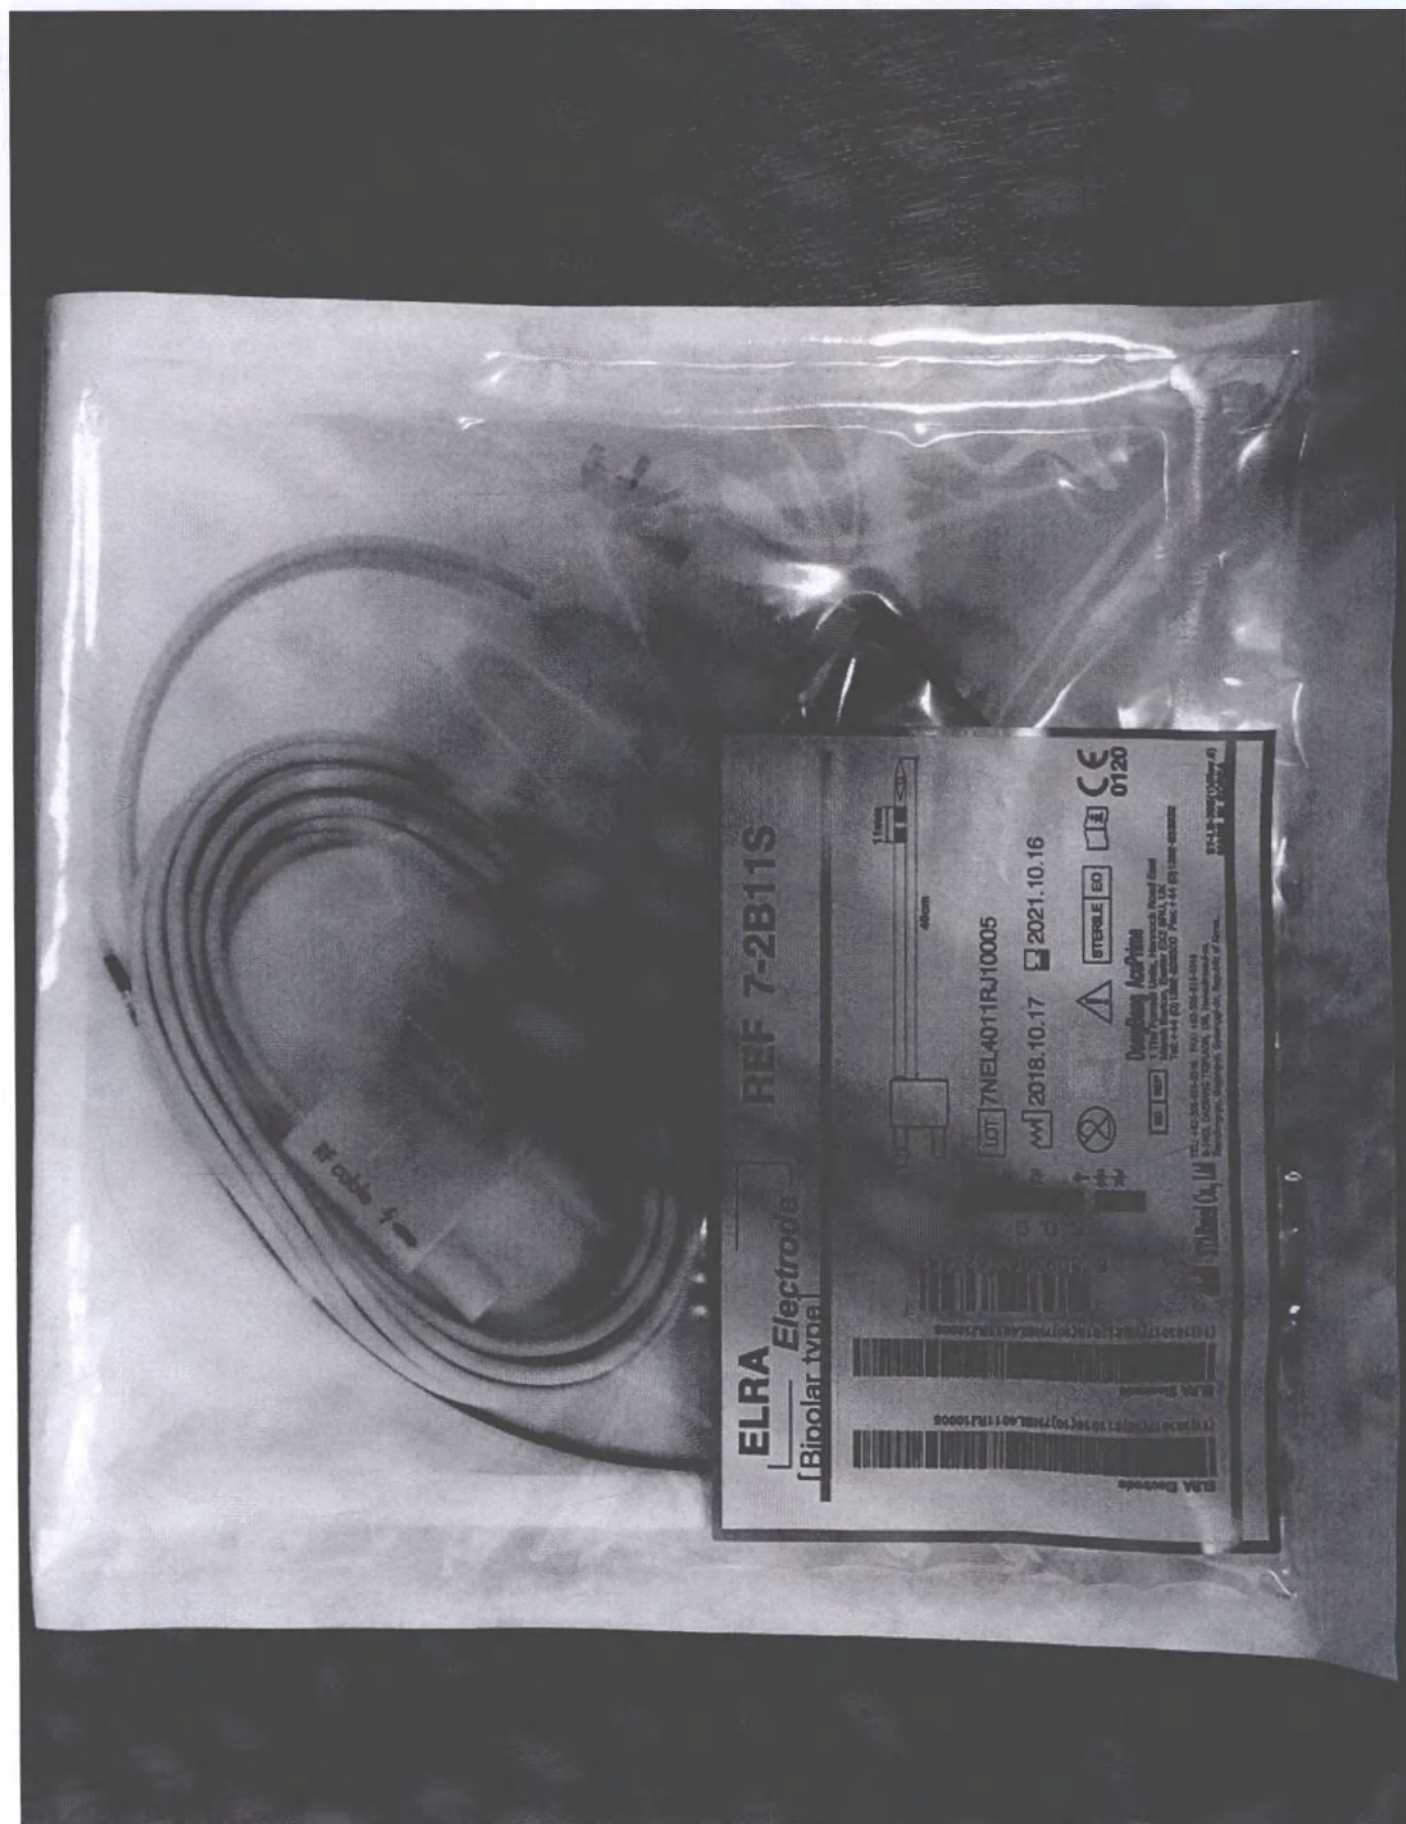

ELRA

Electrode

[Bipolar type]

REF 7-2B11S




ELRA Electrode
(11)719 1017 (10)51 1016 (10)719EL.A11RJ 10005



ELRA Electrode
(11)719 1017 (10)51 1016 (10)719EL.A11RJ 10005



8 809306 762344



LOT 7NEL4011RJ10005

2018.10.17 2021.10.16

STERILE EO

CE 0120

DongBang AcaPrime

1 The Forum Units, Hancock Road East
Mangrove, Eastern DSD (RJ), LBN
Tel +64 (0)3 508 40500 Fax +64 (0)3 508 40500

Tel: +82-506-816-3346 Fax: +82-506-816-4346
9-1401, DAEWANG TRUPHASE, 130, Hamsaemul-ro,
Bundang-gu, Gyeonggi-do, Republic of Korea.

ST-4LB-206 (Yellow-A)
MADE IN KOREA

Global distributor

TaeWoong
MEDICAL

Manufacturer

STARmed

8. Электрод биполярный ELRA 7-2B22S (в первичной упаковке)




ELRA
Electrode
[Bipolar type]

REF 7-2B22S



(11)100416(10)7NEL4022RD10002
(11)100416(10)7NEL4022RD10002



40cm

LOT 7NEL4022RD10002

2018.04.16 2021.04.16

STERILE EO

DongBang Acupoint

1 The Foremost Units, Hancock Road East
Shatin District, New Territories, HONG KONG, CHINA
Tel: +854 (85) 590-820000 Fax: +854 (85) 590-820032

TEL: +82-506-616-2546 FAX: +82-506-616-6546
D-1403, DAEJANG TROOP, 15th, Hwangnam-dong,
Daejeon-gu, Gyeonggi-do, Gyeonggi-do, Republic of Korea.

SY-418-200(11)(Rev.0)
MADE IN KOREA

Global distributor

TheWoong
MEDICAL

Manufacturer

STARmed

Генеральный директор
ООО Группа Компаний СМТ



Симчук И.П.

Прошито и пронумеровано 20 (двадцать) лист 06