

Наименование изделия «Система дентальной имплантации ОКСИ (DentalImplantSystem OXY)»

(Имплантат Модель _____)

Размер _____

Код продукта (REF) _____

Номер партии (LOT) _____

Дата изготовления _____


Дата истечения срока годности _____

Внимание! Изделие для использования только в стоматологии. Внимательно прочитайте инструкцию по применению. Не используйте если упаковка повреждена.

Уполн.пред. в РФ: ООО «АГАТА» 450059, респ. Башкортостан, г. Уфа, пр.Октября, дом 33/1, кв.28

Производитель «Биомекс.р.д.(Biomecs.r.l.)», Италия, Виа Национале Норд, 21/а, 23823 Колико(ЛК)

Р.У. _____



Наименование изделия «Система дентальной имплантации ОКСИ (DentalImplantSystem OXY)»

(компонент)

Код продукта (REF) _____

Номер партии (LOT) _____

Дата изготовления _____

Уполн.пред. в РФ: ООО «АГАТА» 450059, респ. Башкортостан, г. Уфа, пр.Октября, дом 33/1, кв.28

Производитель «Биомекс.р.д.(Biomecs.r.l.)», Италия, Виа Национале Норд, 21/а, 23823 Колико(ЛК)

Р.У. _____



Наименование изделия «Система дентальной имплантации ОКСИ (DentalImplantSystem OXY)»
(инструмент)

Код продукта (REF) _____

Номер партии (LOT) _____


Дата изготовления _____

Уполн.пред. в РФ: ООО «АГАТА» 450059, респ. Башкортостан, г. Уфа, пр.Октября, дом 33/1, кв.28
Производитель «Биомекс.р.л.(Biomecs.r.l.)», Италия, Виа Национале Норд, 21/а, 23823 Колико(ЛК)

Р.У. _____

REF

LOT



0051

Директор _____



Зиганшин Ф.С.

Пропущено
и учтено



Имплантат K1 (Implant K1)



1

Имплантат ПСК (Implant PSK)



2

Имплантат ИИТ ЭКСТРАШОРТ (Implant INT EXTRA SHORT)



Имплантат ИНТ ПС МИКРО (Implant INT PS MICRO)



4

Имплантат ИИТ ПС НОРМО (Implant INT PS NORMO)




5

Имплантат НЬЮ КЛАССИК МИКРО (Implant INT CLASSIC MICRO)




6

Имплантат НЬЮ КЛАСИК НОРМО (Implant INT CLASSIC NORMO)

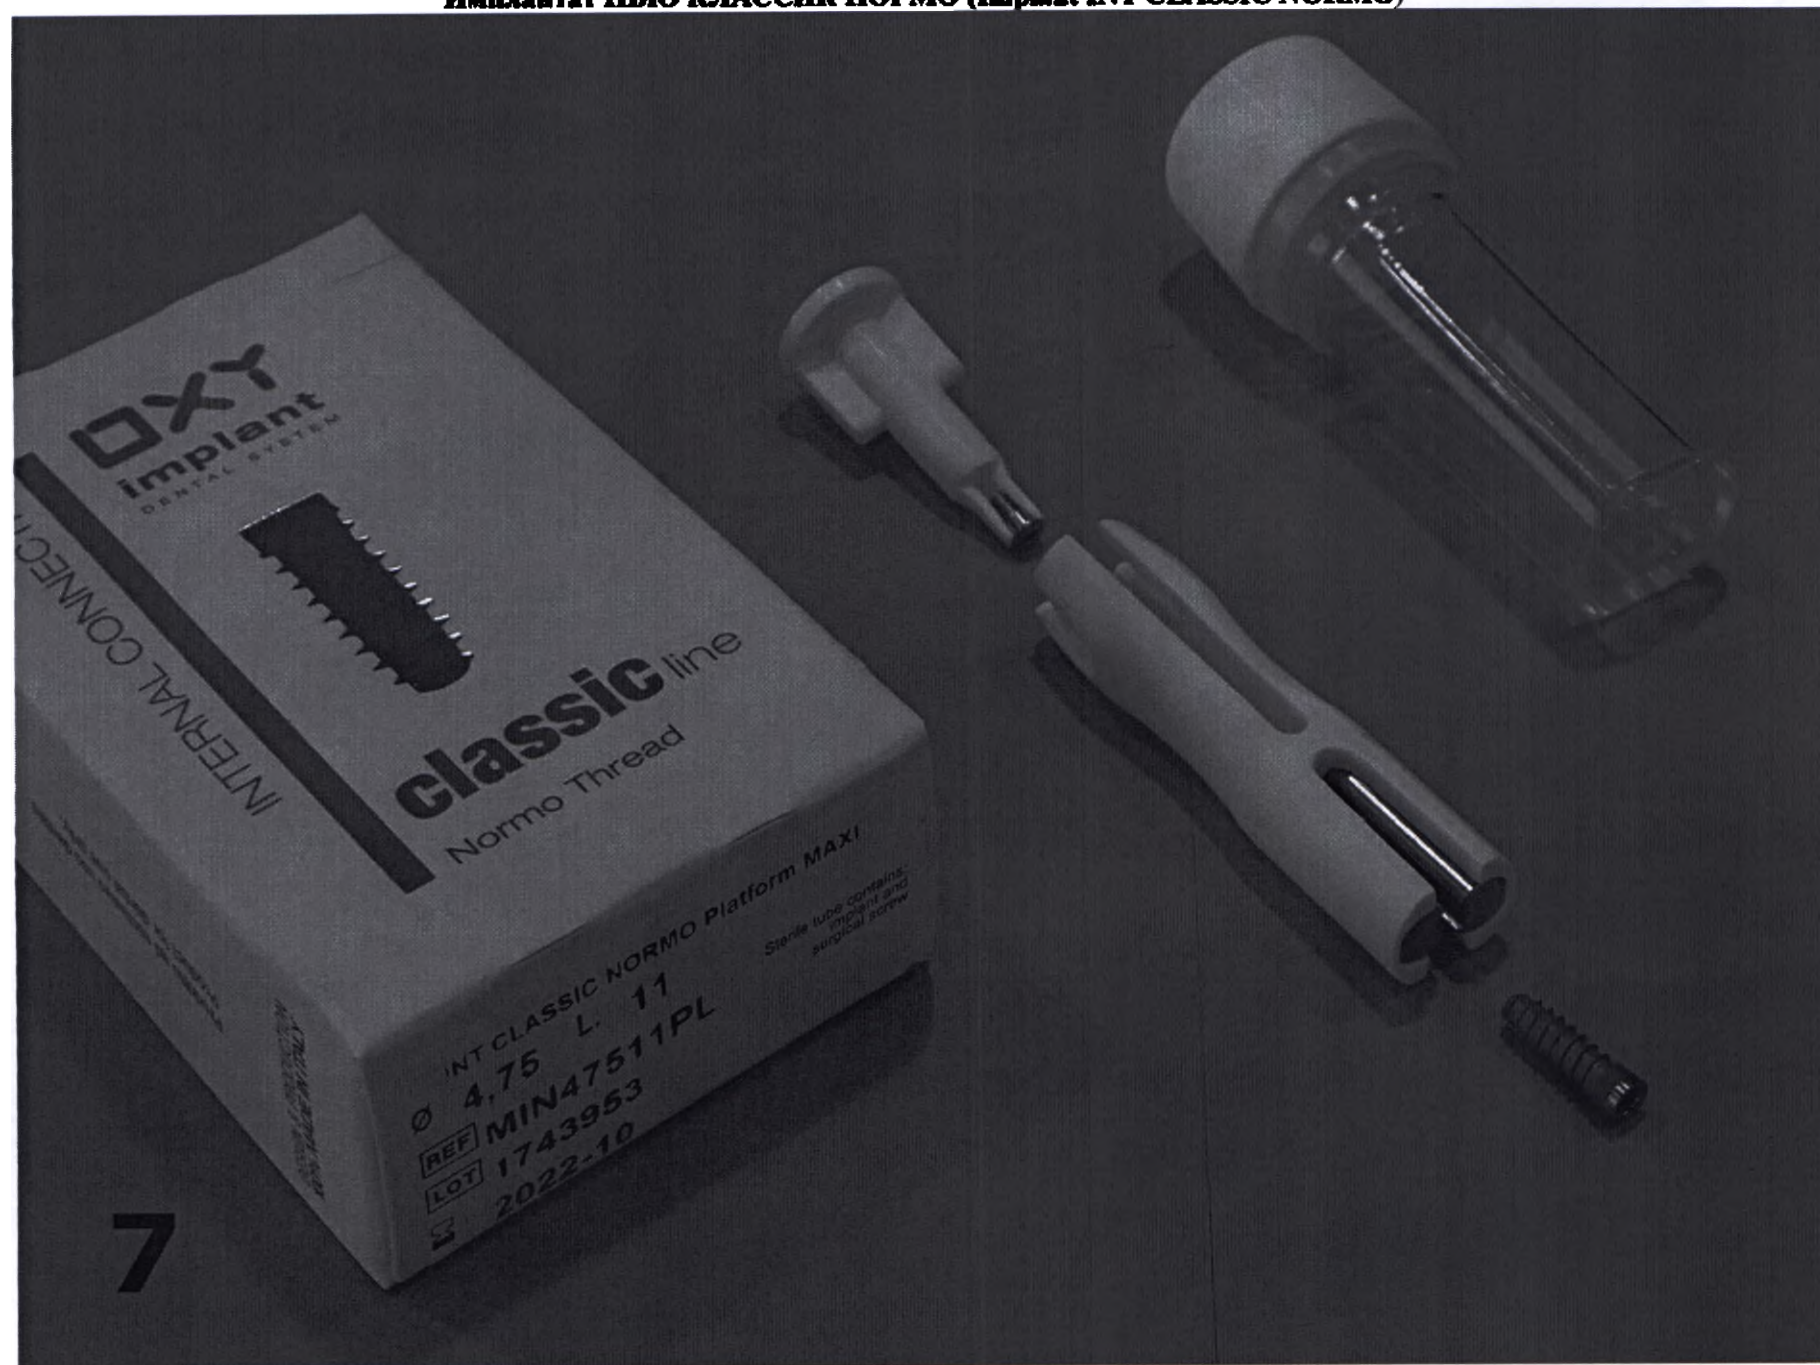

7

Имплантат МИКРО ФИКС (IMPLANT MICRO FIX)

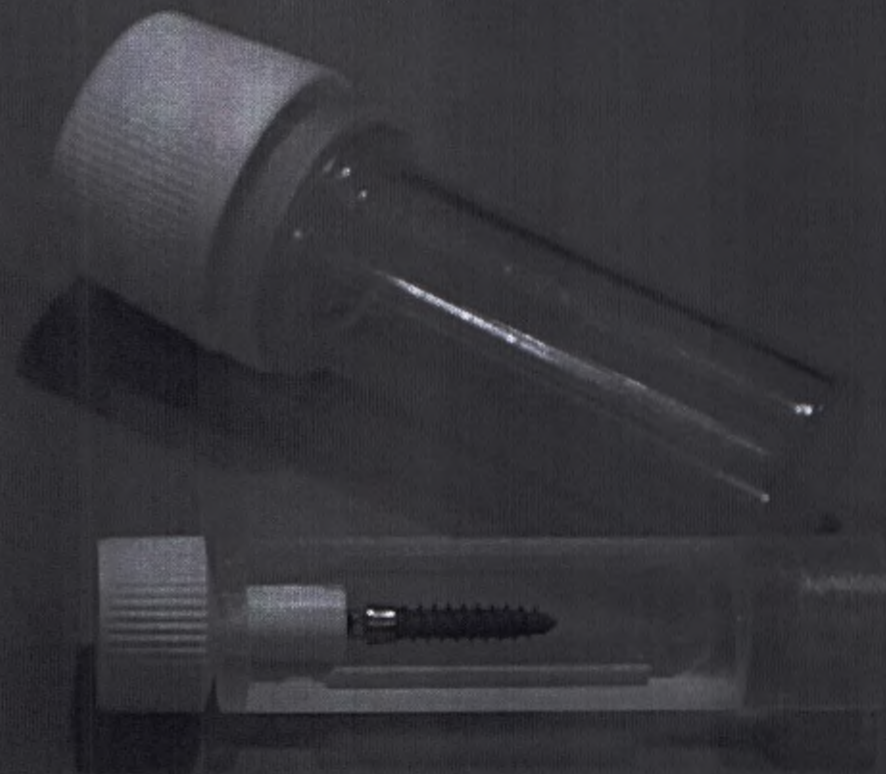

Имплантат МИКРО ФИКС СФЕР (IMPLANT MICRO FIX SPHERE)



9

формирователь десны конический (healing abutment conical)

HEALING ABUTMENT
STD Conical D5 H3

REF



K1HAR5030

LOT




1739378

2 units



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0434

CAUTIONS

Read instructions for use and file prosthesis system carefully

BIO-MEC S.R.L.
Via Nazionale Nord 21a
23123 Colico (LC)-ITALY

10



трансфер слепочный для открытой ложки конический (imp. coping transfer open tray conical)

IMP. COPING TRANSFER
OPEN TRAY STD Conical

REF



K ICTR

LOT



1742999



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and the prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



11

трансфер слепочный для закрытой ложки конический (imp. coping transfer closed tray conical)

IMP. COPING TRANSF.
CL. TRAY STD Conical

REF



K1SNPTR

LOT



1744485



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.

Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



12

oxyimplant.com

LAB ANALOGUE
MINI CONICAL

REF

K1LABN

LOT

1779334



DO NOT USE IF PACKAGE
IS DAMAGED



CE

CAUTIONS
Read instructions for use and fit prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



13

абатмент прямой конический (straight abutment conical)

oxyimplant.com

STRAIGHT ABUT. K1
REGULAR H3 D.4,5

REF

LOT



DO NOT USE IF PACKAGE
IS DAMAGED



ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo di impianto protesico
Read instructions for use and file prosthesis system carefully



K1STR30

F1635071

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

14

абатмент фрезеруемый конический (milling abutment conical)

MILLING ABUT. K1
REGULAR -WIDE

REF



K1STRCNC

LOT



1845620



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

15

oxyimplant.com

PREMILLED ABUT.
ANTIR.NARROW K1

REF
LOT

K1MI N60

1637782

DO NOT USE IF PACKAGE IS DAMAGED

ATTENZIONE - CAUTION
L'egge attenzione to istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and the prosthesis system carefully

CE 0434

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



16

абатмент угловой 15° конический (angled abutment 15° conical)

oximplant.com

ANG ABUT. 15°

REGULAR K1

REF



K1ANR1530

LOT



F1635075



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0434

BIOMEC S.R.L.
Via Nazionale Nord 21a
23023 Colico (LC)-ITALY



ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and file prosthesis system carefully

17

абатмент угловой 25° конический (angled abutment 25° conical)

oximplant.com

ANG ABUT. 25°
NARROW H4 K1

REF



K1ANN2540

LOT



1637729



DO NOT USE IF PACKAGE
IS DAMAGED



0434

ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



18

oxyimplant.com

UNIVERSAL BASE
STD Conical D 5 H2

CAUTIONS
Read instructions for use and file prosthesis system carefully

REF

LOT

K1ESTR20

1638073

DO NOT USE IF PACKAGE IS DAMAGED

CE 0434

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC) ITALY

19

абатмент шаровидный конический (ball abutment conical)

20

eximplant.com
BALL ABUTMENT STD
CONICAL H3 D 2.25

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



0434

LOT

1637132



K1BALLR30



REF



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



абатмент окси лок конический (oxy loc abut. conical)

OXY LOC K1
REGULAR H1

REF



LOCK1R10

LOT



1844802



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC) ITALY



ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully

22

TEMPORARY ABUT.
ROT. STD CONICAL
Non Act.

REF

K1TMPRR



LOT

1844804



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051




BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and fit the prosthesis system carefully



абатмент временный антиротационный конический неактивный (temporary abut. ant. conical non act.)

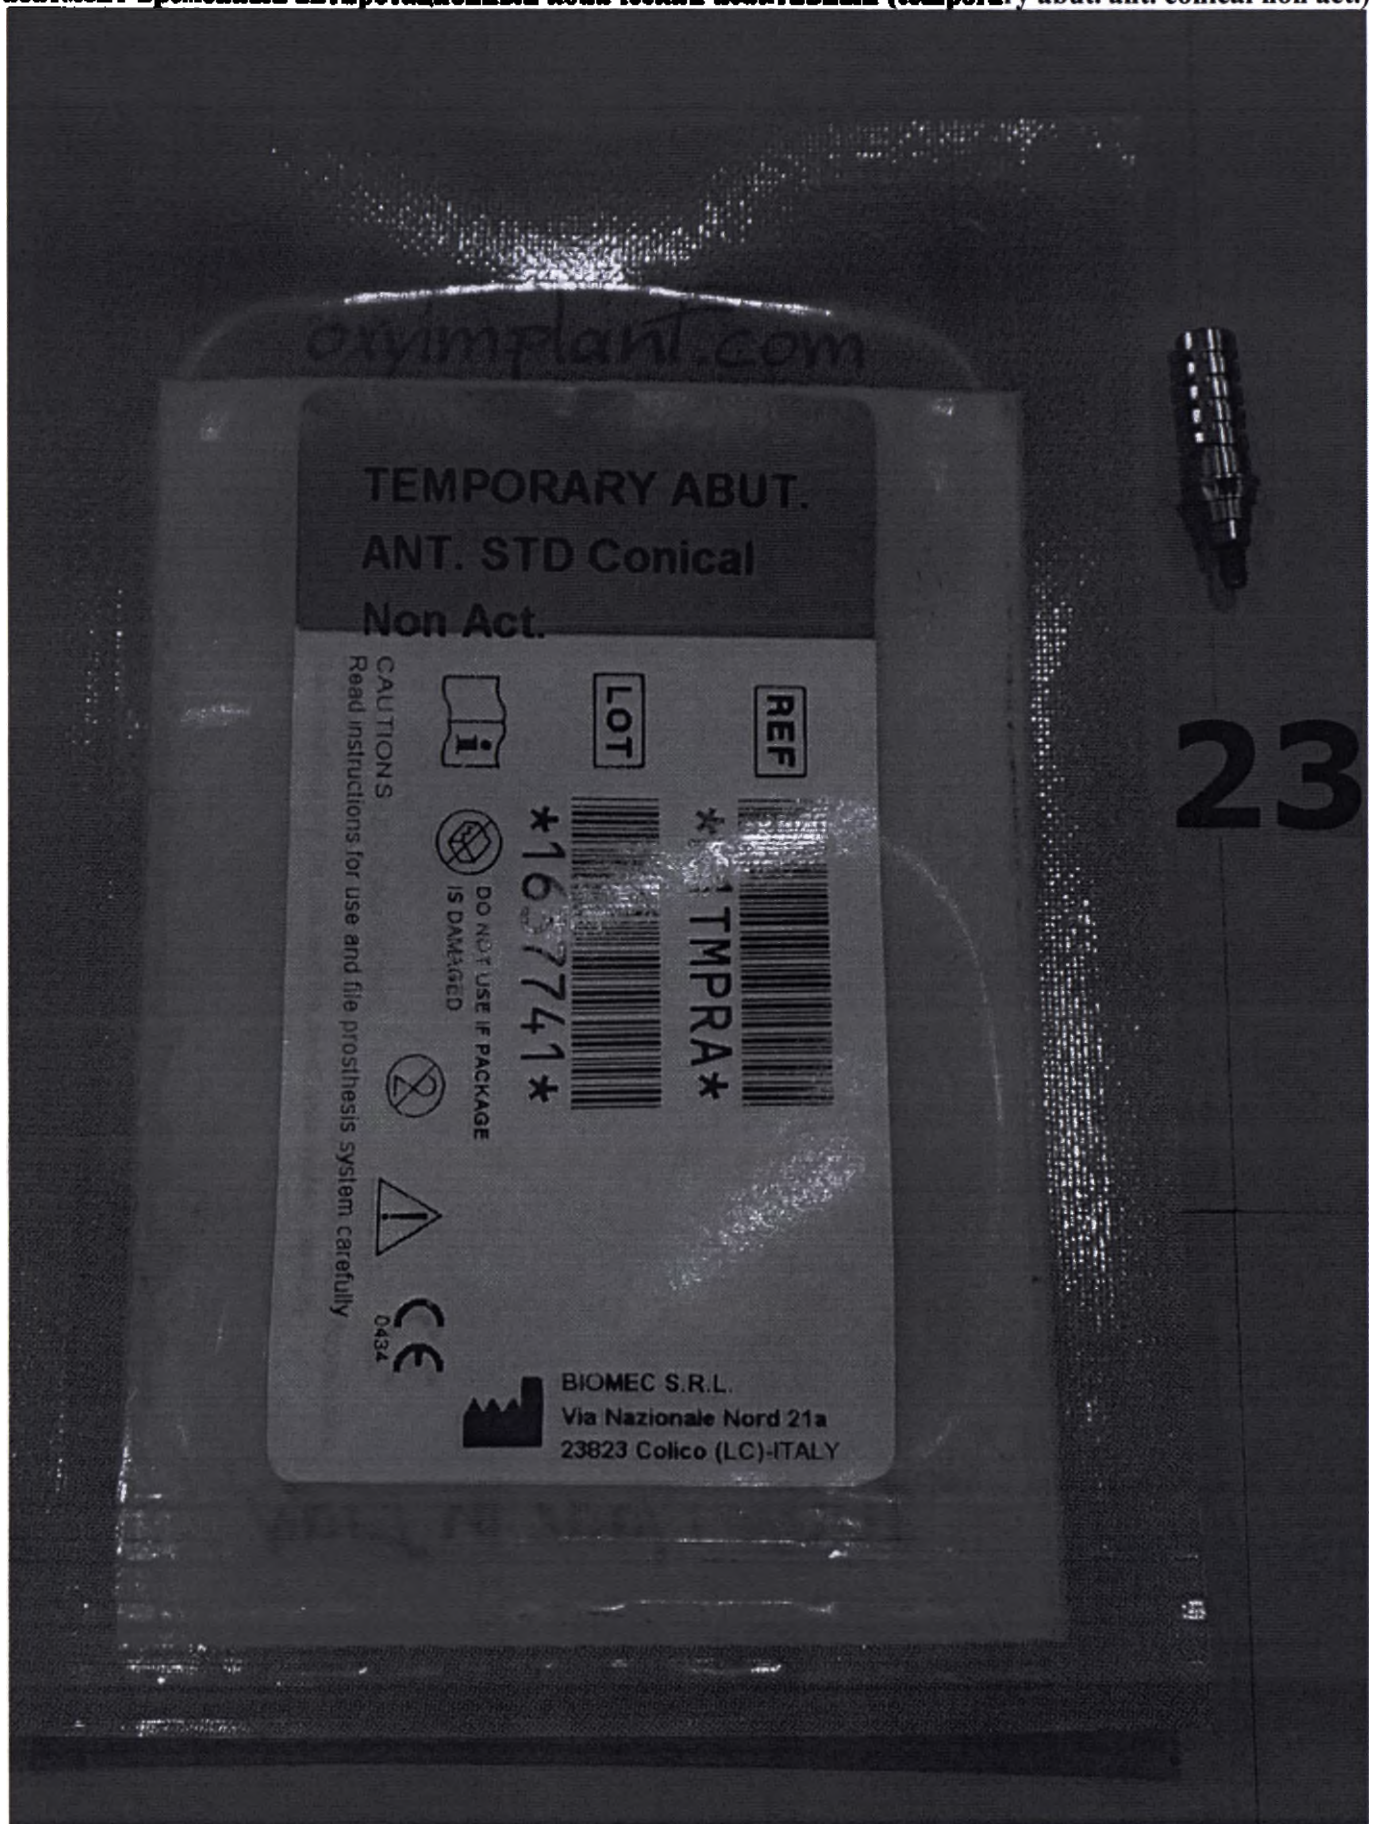

абатмент выжигаемый ротационный конический неактивный (castable abut. rot. conical non act.)

oxyimplant.com

**CASTABLE ABUTMENT
K1 REGULAR ROT.**

REF

LOT



K1CASTR



1638060



DO NOT USE IF PACKAGE
IS DAMAGED

ATTENZIONE - CAUTIONS


Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and the prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

24


абатмент выжигаемый антиротационный конический неактивный (castable abut. ant. conical non act.)

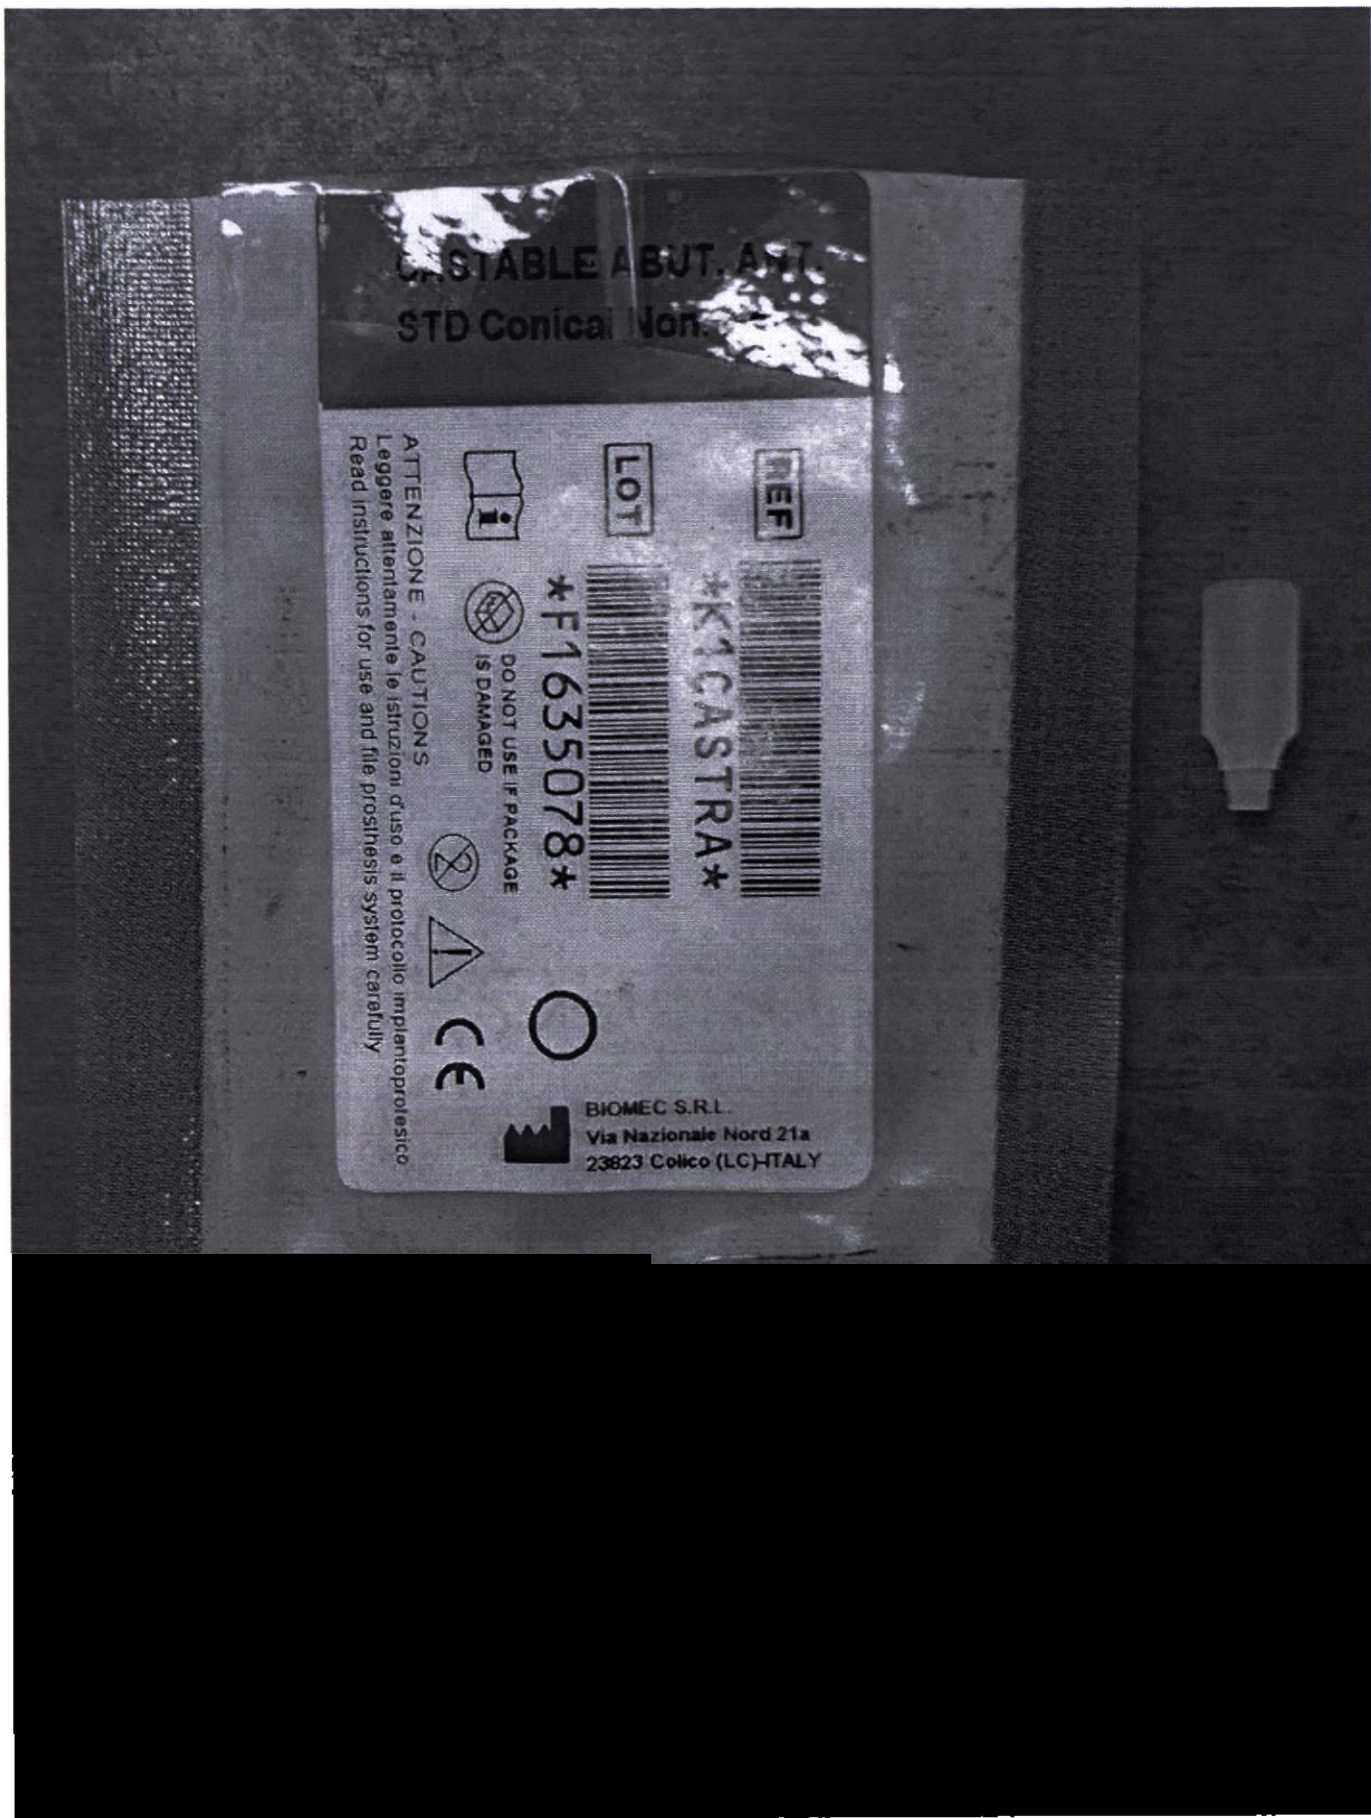

абатмент фрезеруемый конический неактивный (milling abut. conical non act.)



основание прямое или коническое (straight base ils conical)

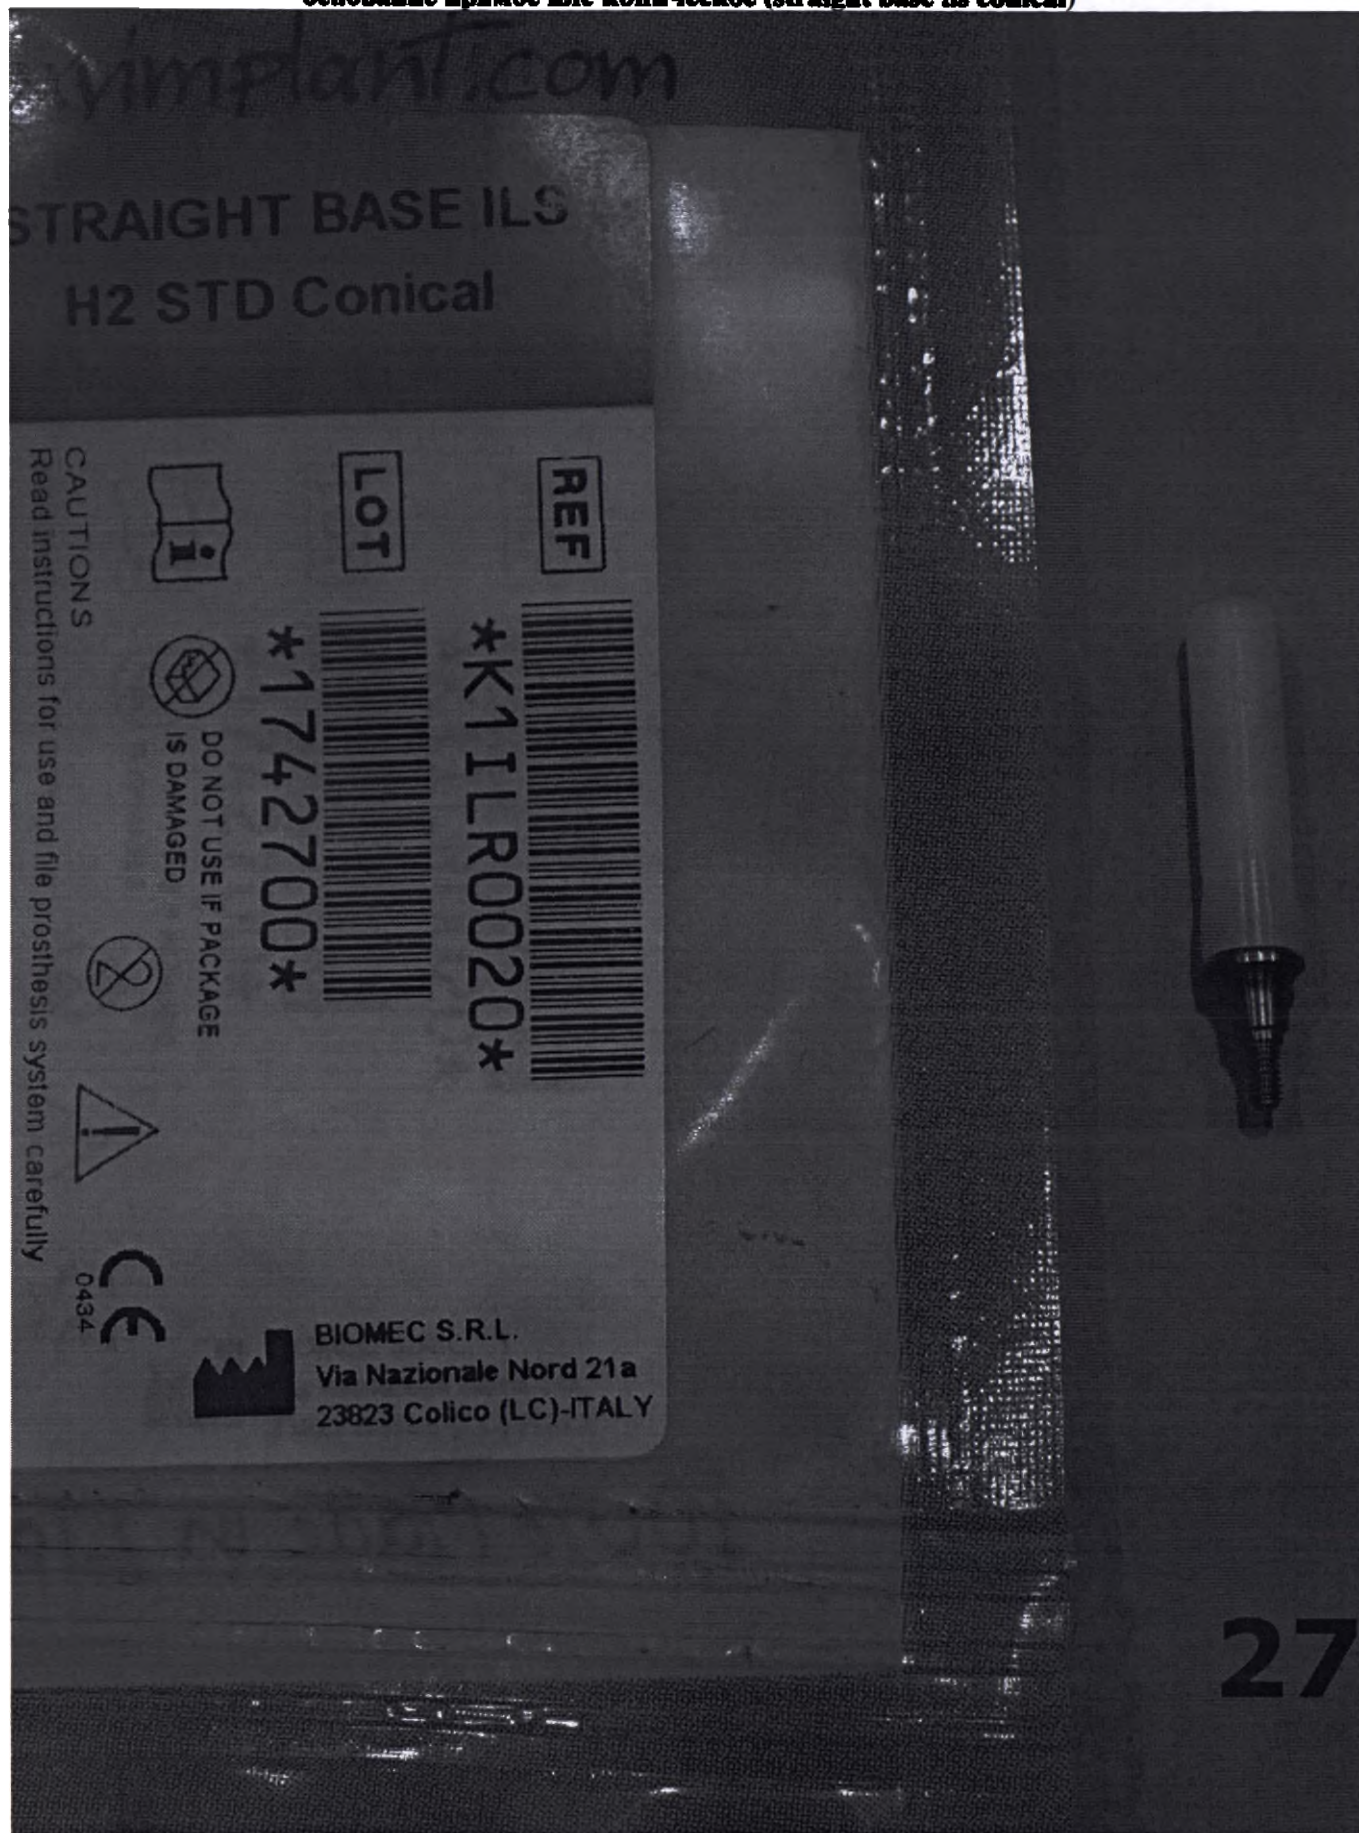

основание угловое 17° илс коническое (angled base 17° ils conical)

ANGLED BASE 17°
ILS H2 STD Conical

REF



K1ILR1720

LOT



1744298



DO NOT USE IF PACKAGE
IS DAMAGED



0051

CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

основание угловое 35° или коническое (angled base 35° ils conical)

ANGLED BASE 35°
ILS H3 STD Conical

REF

K1ILR3530

LOT

1744300



DO NOT USE IF PACKAGE
IS DAMAGED



0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

29

копачок заживляющий илс (healing cap ils)

HEALING CAP ILS

REF

ILHC

LOT

1744094

2 Units



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



30

трансфер слепочный илс (imp. coping transfer ils)

IMP. COPING
TRANSFER ILS

REF



ILT

LOT



1743740



DO NOT USE IF PACKAGE
IS DAMAGED

2 Units



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



31

аналог илс (analogue ils)

32

ANALOGUE ILS

REF



ILA

LOT



1744083



DO NOT USE IF PACKAGE
IS DAMAGED

2 Units



CE

CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



абатмент временный для основания илс (temporary for ils base)

TEMPORARY FOR
ILS BASE

REF

LOT

ILTA

1847402



DO NOT USE IF PACKAGE
IS DAMAGED



2 Units



CAUTIONS
Read instructions for use and file prosthesis system carefully.

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

33

TITANIUM COVER FOR ILS BASE

CAUTIONS



DO NOT USE IF PACKAGE
IS DAMAGED



2 Units



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

LOT

REF

17433365



ILCT*



колпачок хромокобальтовый для основания илс (cocr cover for ils base)

COCR COVER FOR ILS BASE

REF

LOT

ILCC

1844524



DO NOT USE IF PACKAGE
IS DAMAGED



2 Units



CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

35

абатмент выжигаемый для основания илс (castable for ils base)

36

CASTABLE FOR
ILS BASE

REF



ILCA

LOT



1845450



DO NOT USE IF PACKAGE
IS DAMAGED

2 Units



BIOMECC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS

Read instructions for use and file prosthesis system carefully



CE

SCAN BODY ILS



DO NOT USE IF PACKAGE
IS DAMAGED

1845629



SCANILS*



ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

37

аналог цифровой илс (digital analogue ils) ADIL

DIGITAL ANALOGUE
ILS

REF



ADIL

LOT



1743617



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



CE

BIOMEC S.R.L.

Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



основание титановое ротационное cad-cam коническое (titanium base cad/cam rot. conical non act.)

TIT. BASE CAD/CAM
ROT. MINI Conical
Non Act.

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



LOT

1637742



REF

K1BTRN



BIOMEC S.p.A.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

39

основание титановое антиротационное cad-cam коническое неактивное (titanium base cad/cam ant. conical non act.) K1BTNN K1BTNR

TIT. BASE CAD/CAM
ANT. MINI Conical
Non Act.

CAUTIONS

Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED




CE

0434

LOT

K1BTNN



REF



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

40

основание хромокобальтовое ротационное cad-cam коническое неактивное (coCr base cad/cam rot. Conical non act.)

CoCr BASE CAD/CAM ROT. STD Conical Non Act.

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



LOT

17740523



REF

K1BCRR



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

41



основание хромокобальтовое антиротационное cad-cam коническое неактивное
(coCr base cad/cam ant. Conical non act.) \

42

CoCr BASE CAD/CAM
ANT. STD Conic
Non Act.

REF

K1BCNR

LOT

1844520



DO NOT USE IF PACKAGE
IS DAMAGED



0051



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and file prosthesis system carefully

абатмент выжигаемый для титанового/хромокобальтового основания cad/cam ротационный
(castable abut. For ti/coCr base cad/cam rot.)

43

CASTABLE ABUT.
FOR TI/COCR BASE
CAD/CAM ROT. MINI

CAUTIONS
Read instructions for use and file prosthetic



DO NOT USE IF PACKAGE
IS DAMAGED




LOT

REF

1743519



CBZ220

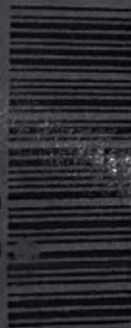

BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

основание титановое окси бас ротационное cad/cam коническое (titanium oxy bas cad/cam rot. Conical)

TIT. OXY BAS CAD/CAM
ROT. MINI CONICAL

REF

K1CBTRN

LOT

1846737



DO NOT USE IF PACKAGE
IS DAMAGED



0051

CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

44

основание титановое окси бас антиротационное cad/cam коническое (titanium oxy bas cad/cam ant. Conical)



основание хромокобальтовое оксид бас ротационное cad/cam коническое (cocr oxy baz cad/cam rot. Conical)



основание хромокобальтовое окси бас антиротационное cad/cam коническое

(CoCr oxy bas cad/cam ant. Conical)

CoCr OXY BAS CAD/
CAM ANT. STD Conical

REF



K1CBCNR

LOT



1742695



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0434

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS

Read instructions for use and file prosthesis system carefully

47

48

TORX SCREW FOR OXY BAS MINI CONICAL

REF



NDS102000

LOT



1851455



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

50


SCAN BODY MINI
Conical CAD-CAM

REF



SCANK1N

LOT

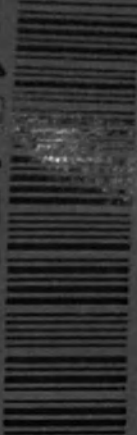

1743934



DO NOT USE IF PACKAGE
IS DAMAGED



ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il presente modulo impiantoprotesico
Read instructions for use and file prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



аналог цифровой конический (digital analogue conical)

DIGITAL ANALOGUE MINI CONICAL

REF



ADK1N

LOT



143939



DO NOT USE IF PACKAGE
IS DAMAGED



CE

CAUTION
Read instructions for use and fit prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт для слепочного трансфера открытая ложка конический (imp. Coping transfer screw open tray conical)

IMP. COPING TRANSFER
SCREW OPEN TRAY MINI
CONICAL

REF

LOT



K1ICSN30



1740382



CAUTIONS

Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



CE



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт для слепочного трансфера закрытая ложка конический (imp. Coping transfer screw closed tray conical)

IMP. COPING TRANSFER SCREW
STD CONICAL CLOSED TRAY

REF

K1ICSRC

LOT

1850533



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a



PLASTIC CAP FOR
CLOSED TRAY
IMP. COPING

REF



SNAP

LOT



1845095



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.

Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт фиксирующий для абатмента конический (abutment screw conical) K1SCWN K1SCWRW

ABUTMENT SCREW
STD CONICAL

REF



K1SCWRW

LOT



1744304



DO NOT USE IF PACKAGE
IS DAMAGED

5 Units



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт для универсального основания конический (universal base screw conical)

UNIVERSAL BASE SCREW D4 H2 STD CONICAL

REF



K1ESSWR20

LOT



1847834



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



абатмент выжигаемый ротационный для универсального основания конический
(castable rot. For universal base conical)

CASTABLE ROT. FOR UNIVERSAL BASE

REF

LOT



CAUTIONS
Read instructions for use and file prosthesis system carefully

K1NCESR



1848354



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

абатмент выжигаемый антиротационный для универсального основания конический
(castable ant. For universal base conical)

CASTABLE ANT.FOR
UNIVERSAL BASE MINI

REF

K1NCESN

LOT

1846732



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and the prosthesis system carefully

абатмент ротационный пээк для универсального основания конический
(peek rot. Abut. For universal base mini conical)

PEEK ROT.ABUT.FOR
UNIVERSAL BASE MINI

REF

K1NPEKR



LOT



1846730



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and file prosthesis system carefully

абатмент антитротационный пэж для универсального основания конический
(peek ant. Abut. For universal base conical)


PEEK ANT. ABUT. FOR
UNIVERSAL BASE MINI

REF



K1NPEKN



LOT

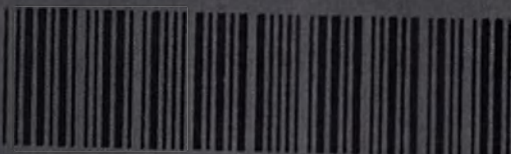

1846729



DO NOT USE IF PACKAGE
IS DAMAGED



ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.

Via Nazionale Nord 21a

23823 Colico (LC)-ITALY



абатмент хромокобальтовый ротационный для универсального основания конический
(cocr rot. Abut. For universal base conical)

**COCR ROT.ABUT.FOR
UNIVERSAL BASE
MINI CONICAL**

REF

K1NCROR

LC

184728



DO NOT
IS DAMAGE

PACKAGE



ATTENZIONE - CAUTIONS
Leggere attentamente l'istruzione
Read instructions for use and file

prothesis system carefully
d'uso e il protocollo impiantoprotesico

BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

абатмент хромокобальтовый антиротационный для универсального основания конический
(cocr ant. Abut. For universal base conical)

OCR ANT.ABUT.FOR
UNIVERSAL BASE
INI CONICAL

ATTENZIONE - CAUTIONS



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

REF

K1NCRD



1050*

винт слепочного трансфера илс (imp. Coping transfer screw ils)

IMP. COPING TRANSFER SCREW FOR ILS

REF



ILTS

LOT



1743741



DO NOT USE IF PACKAGE
IS DAMAGED

5 units



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



ВИНТ ДЛЯ УГЛОВОГО ОСНОВАНИЯ ИЛС КОНИЧЕСКИЙ (screw for angled base ils conical)

SCREW FOR ANGLED
BASE ILS STD CONICAL

REF



K1ILRS

LOT



1734538



DO NOT USE IF PACKAGE
IS DAMAGED

2 Units



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт фиксирующий илс (fixing screw ils)

FIXING SCREW ILS

REF



ILPS

LOT



1952269



DO NOT USE IF PACKAGE
IS DAMAGED



0051

5 Units

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully

аналог микро фикс (micro fix analogue)

oxyimplant.com

MICROFIX ANALOGUE

REF

IAXP02

LOT

1739115

CAUTIONS
Read instructions for use and the prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



CE



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



абатмент выжигаемый антиротационный/трансфер для микрофикс (castable ant. / i.c. transfer micro fix)

oxyimplant.com

CASTABLE ANT.
I.C. TRANSFER
MICRO FIX

CAUTION
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC) ITALIA

LOT

1739119



REF

NUXPR01



аналог микро фикс сфера (micro fix sphere analogue)

oxyimplant.com

**MICRO FIX SPHERE
ANALOGUE**

REF



221AXP01

LOT



1636213



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



абатмент выжигаемый антиротационный / трансфер для микрофикс сфер
(castable ant. / i.e. transfer micro fix sphere)

oxyimplant.com

CASTABLE ANT.
I.C. TRANSFER
MICROFIX SPHERE

REF

LOT

22NUXP01

F1634806



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMECC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and file prosthesis system carefully

формирователь десны INT (healing abutment int)

HEALING ABUTMENT
H3 mm INT STD

REF



HAIN3430

LOT



1744478



DO NOT USE IF PACKAGE
IS DAMAGED

2 units



CE
0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



ATTENZIONE! - CAUTIONS
Read instructions for use and fit prosthesis system carefully

анатомический формирователь десны нит (anatomical healing abut. Int)

oxyimplant.com

ANATOMICAL HEALING
ABUT. H. 6 INT MINI

REF

LOT

ANA1N460

F1633153



DO NOT USE IF PACKAGE
IS DAMAGED



2 units

CAUTIONS
Read instructions for use and the prosthesis system carefully



BIOHEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

трансфер слепочный для открытой ложки инт (imp. coping transfer open tray int)

IMP. COPING TRANSF.
OPEN TRAY INT STD

IMP

PTIN3400


LOT

17740771



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS
Read instructions for use and file prosthesis system carefully



CE



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

трансфер анатомический слепочный для открытой ложки нит
(anatomical imp. Coping transfer open tray int)

ANATOMICAL IMP.
COPING TRANSFER
OPEN TRAY INT

REF



APT5

LOT



F1739887



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

трансфер слепочный для закрытой ложки инт (imp. coping transfer closed tray int)

MP. COPING TRANSFER
CLOSED TRAY INT MINI

REF



*TCIN2000

LOT



1741893



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



CE

BIOMED 2011

Via Nazionale 21a
23823 Colico (LC)-ITALY

трансфер слепочный для закрытой ложки snap-он нит (imp. Coping transfer closed tray snap-on Int)

IMP. COPING TRANSF.
CLOSED TRAY SNAP
INT STD

REF

LOT




DO NOT USE IF PACKAGE
IS DAMAGED

1844776



PUIN3400




CE



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



трансфер анатомический пластиковый пулл-ап нит (anatomical plastic transfer pull up int)

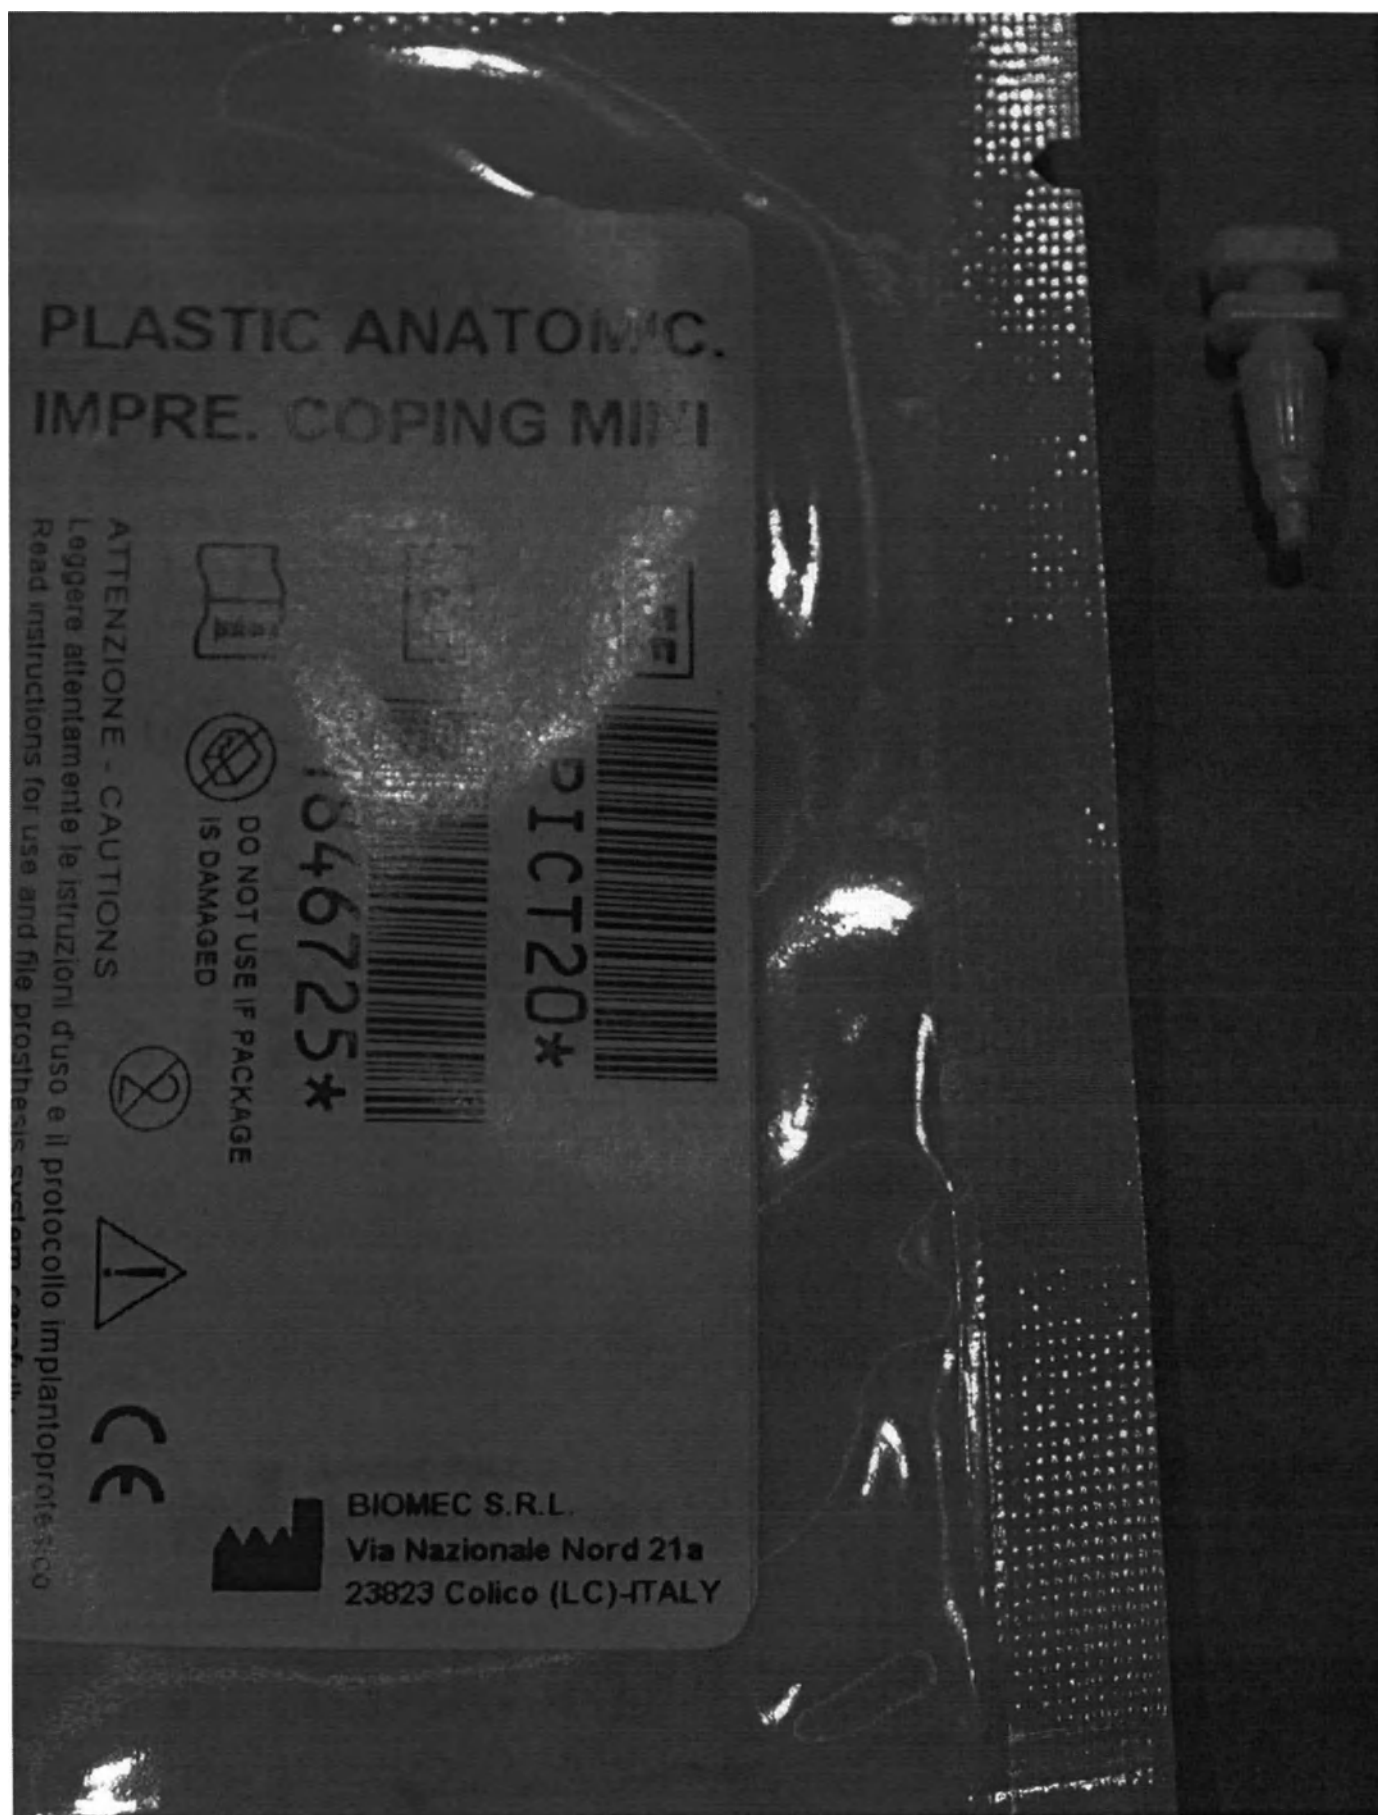

аналог лабораторный инт (laboratory analogue int)

LAB ANALOGUE
INT STD

REF



IAIN3400

LOT




1845445



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMECC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

абатмент выжигаемый ротационный ннт (castable abutment rot. Int)

CASTABLE ABUTMENT
ROT. INT STD

CAUTIONS
Read instructions for use and file properly



DO NOT USE IF PACKAGING
IS DAMAGED

LOT

*17740842



REF

RUIN3400



ITALIA S.R.L.
Via Nazionale Nord 21a
28039 Colico (LC)-ITALY

абатмент выжигаемый антиротационный INT (castable abutment ant. Int)

CASTABLE ABUTMENT
ANT. INT STD

REF

NUIIN3400

LOT

1743304



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and the orthosis system carefully

абатмент временный ротационный ннт (temporary abutment rot. Int)

TEMPORARY ABUT.
ROT. INT STD

REF


LOT

*RUINT34C

F1632656



DO NOT USE IF PACKAGE
IS DAMAGED



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and file prosthesis system carefully

Prosthesis system carefully

абатмент временный антиротационный инт (temporary ant. abutment int)

TEMPORARY ANT.
ABUTMENT INT STD

CAUTIONS
Read instructions for use and the prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



LOT

1744097



REF

NUINT3400



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



абатмент фрезеруемый инт (milling abutment int)

MILLING ABUTMENT INT MINI

REF

LOT

NIN20NC

1844686



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and file prosthesis system carefully

абатмент прямой инт (straight abutment int)

STRAIGHT ABUTMENT
INT MINI H 1,5

REF

STIN2015PS

LOT

1743970



DO NOT USE IF PACKAGE
IS DAMAGED



0051

CAUTIONS
Read instructions for use and fit prostheses system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

абатмент угловой 15° инт (angled abutment 15° int)

ANGLED ABUT.

15° H 2,5 MINI INT

REF

LOT

A2IN2015

1847059



DO NOT USE IF PACKAGE
IS DAMAGED



CE

0051



BIOMECH S.R.L.

Via Nazionale Nord 21a

23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and file prosthesis system carefully

абатмент угловой 25° инт (angled abutment 25° int)

ANGLED ABUTMENT 25° INT STD H.2,5

REF



A2IN3425


LOT



741913



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0434

CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

89

абатмент прямой анатомический (straight anatomical abut.)


STRAIGHT ANAT.
ABUTMENT MINI

REF

LOT



A341N425

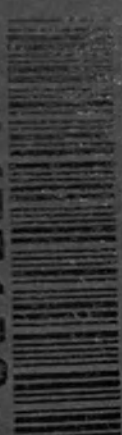

F1633150



DO NOT USE IF PACKAGE
IS DAMAGED



0434



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and file prosthesis system carefully



абатмент угловой анатомический 15° инт (angled anat. abut. 15° int)

ANGLED ANAT. ABUT.
15° H 2,5 INT MINI

REF

A15AIN425

LOT

1744076



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and file prosthesis system carefully

абатмент угловой анатомический 25° инт (angled anatomic abut. 25° int)

ANGLED ANATOMICAL
ABUT. 25° INT STD

REF

A25A1N525

LOT

F1633106



DO NOT USE IF PACKAGE
IS DAMAGED




CE

0434

ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesi
Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

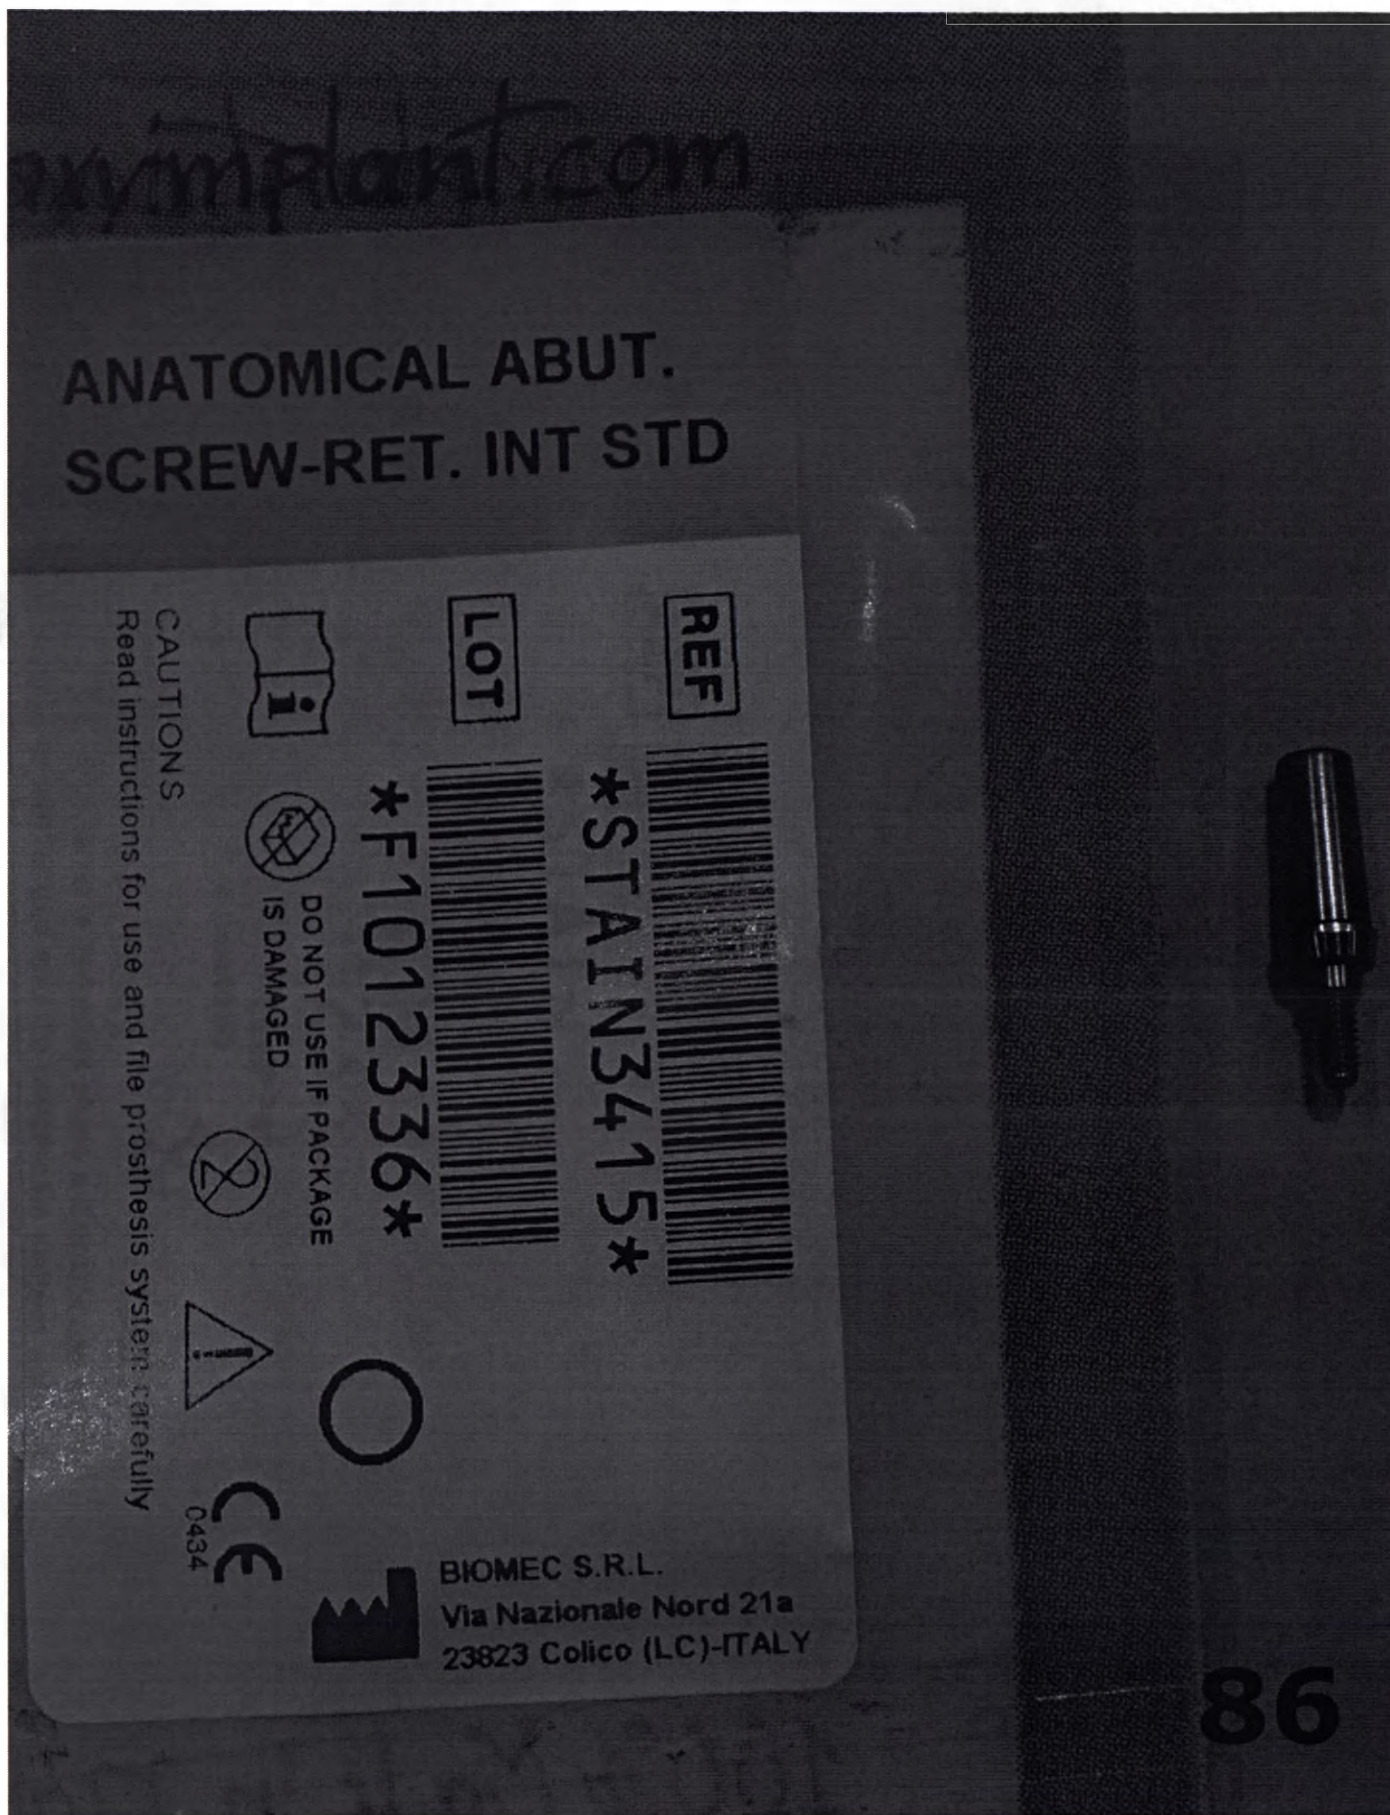

абатмент шаровидный инт (ball abutment int)

eximplant.com

BALL ABUTMENT
INT MINI H.2,5

REF



22BAIN2025

LOT



1740902



DO NOT USE IF PACKAGE
IS DAMAGED



0051

UNITEC S.R.L.

Viale Nord 21a

23052 Caluso (LC)-ITALY


CAUTIONS

Read instructions for use and file prosthesis system carefully

абатмент оксилок инт (oxy loc abut. Int)


OXY LOC INT MINI H2

REF

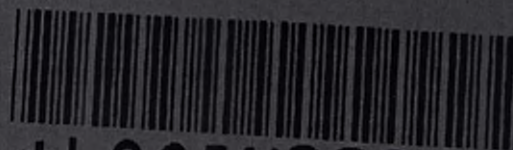

LOCIN2020


LOT

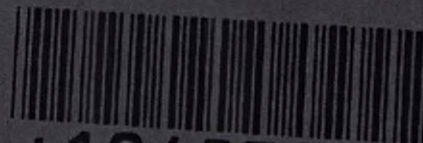

1845321



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

основание универсальное инт (universal base int)

2winimplant.com

UNIVERSAL BASE
INT STD H.1,5

REF



BBI13415

LOT



F163477



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0434

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS

Read instructions for use and file prosthesis system carefully

AESTHETIC ABUT.
INT STD H.1,5

REF


AAIN3415

LOT

1636885




DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

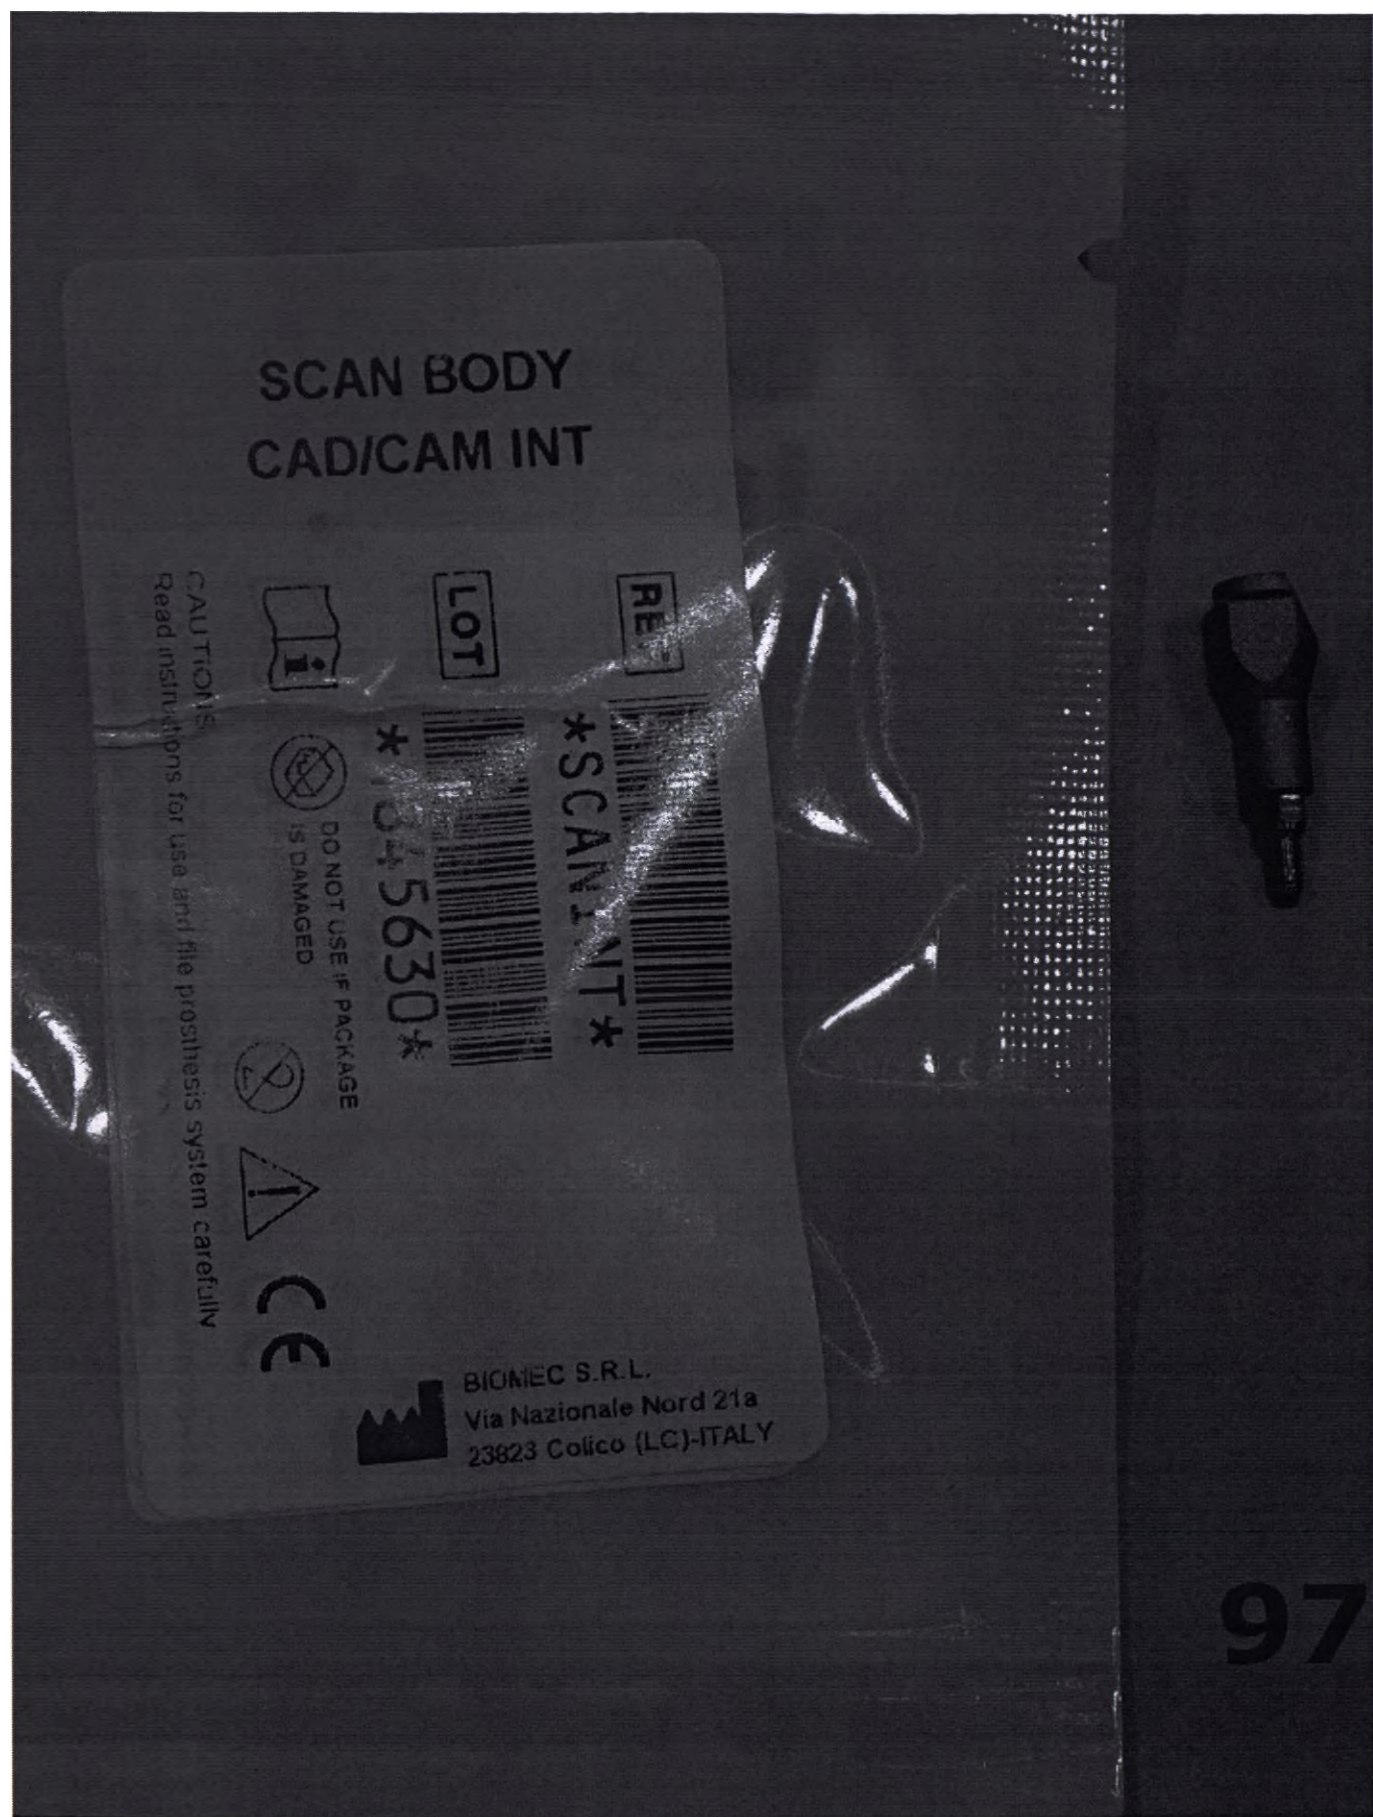

DIGITAL ANALOGUE CAD/CAM INT

REF

LOT

ADINT

1743618




DO NOT USE IF PACKAGE
IS DAMAGED



BIONE S.R.L.
Via Mazzini 21a
23823 Conco (LC) ITALY

CAUTIONS
Read instructions for use and file prosthesis system carefully


основание титановое антиротационное cad/cam мнт (titanium base cad/cam ant. Int)

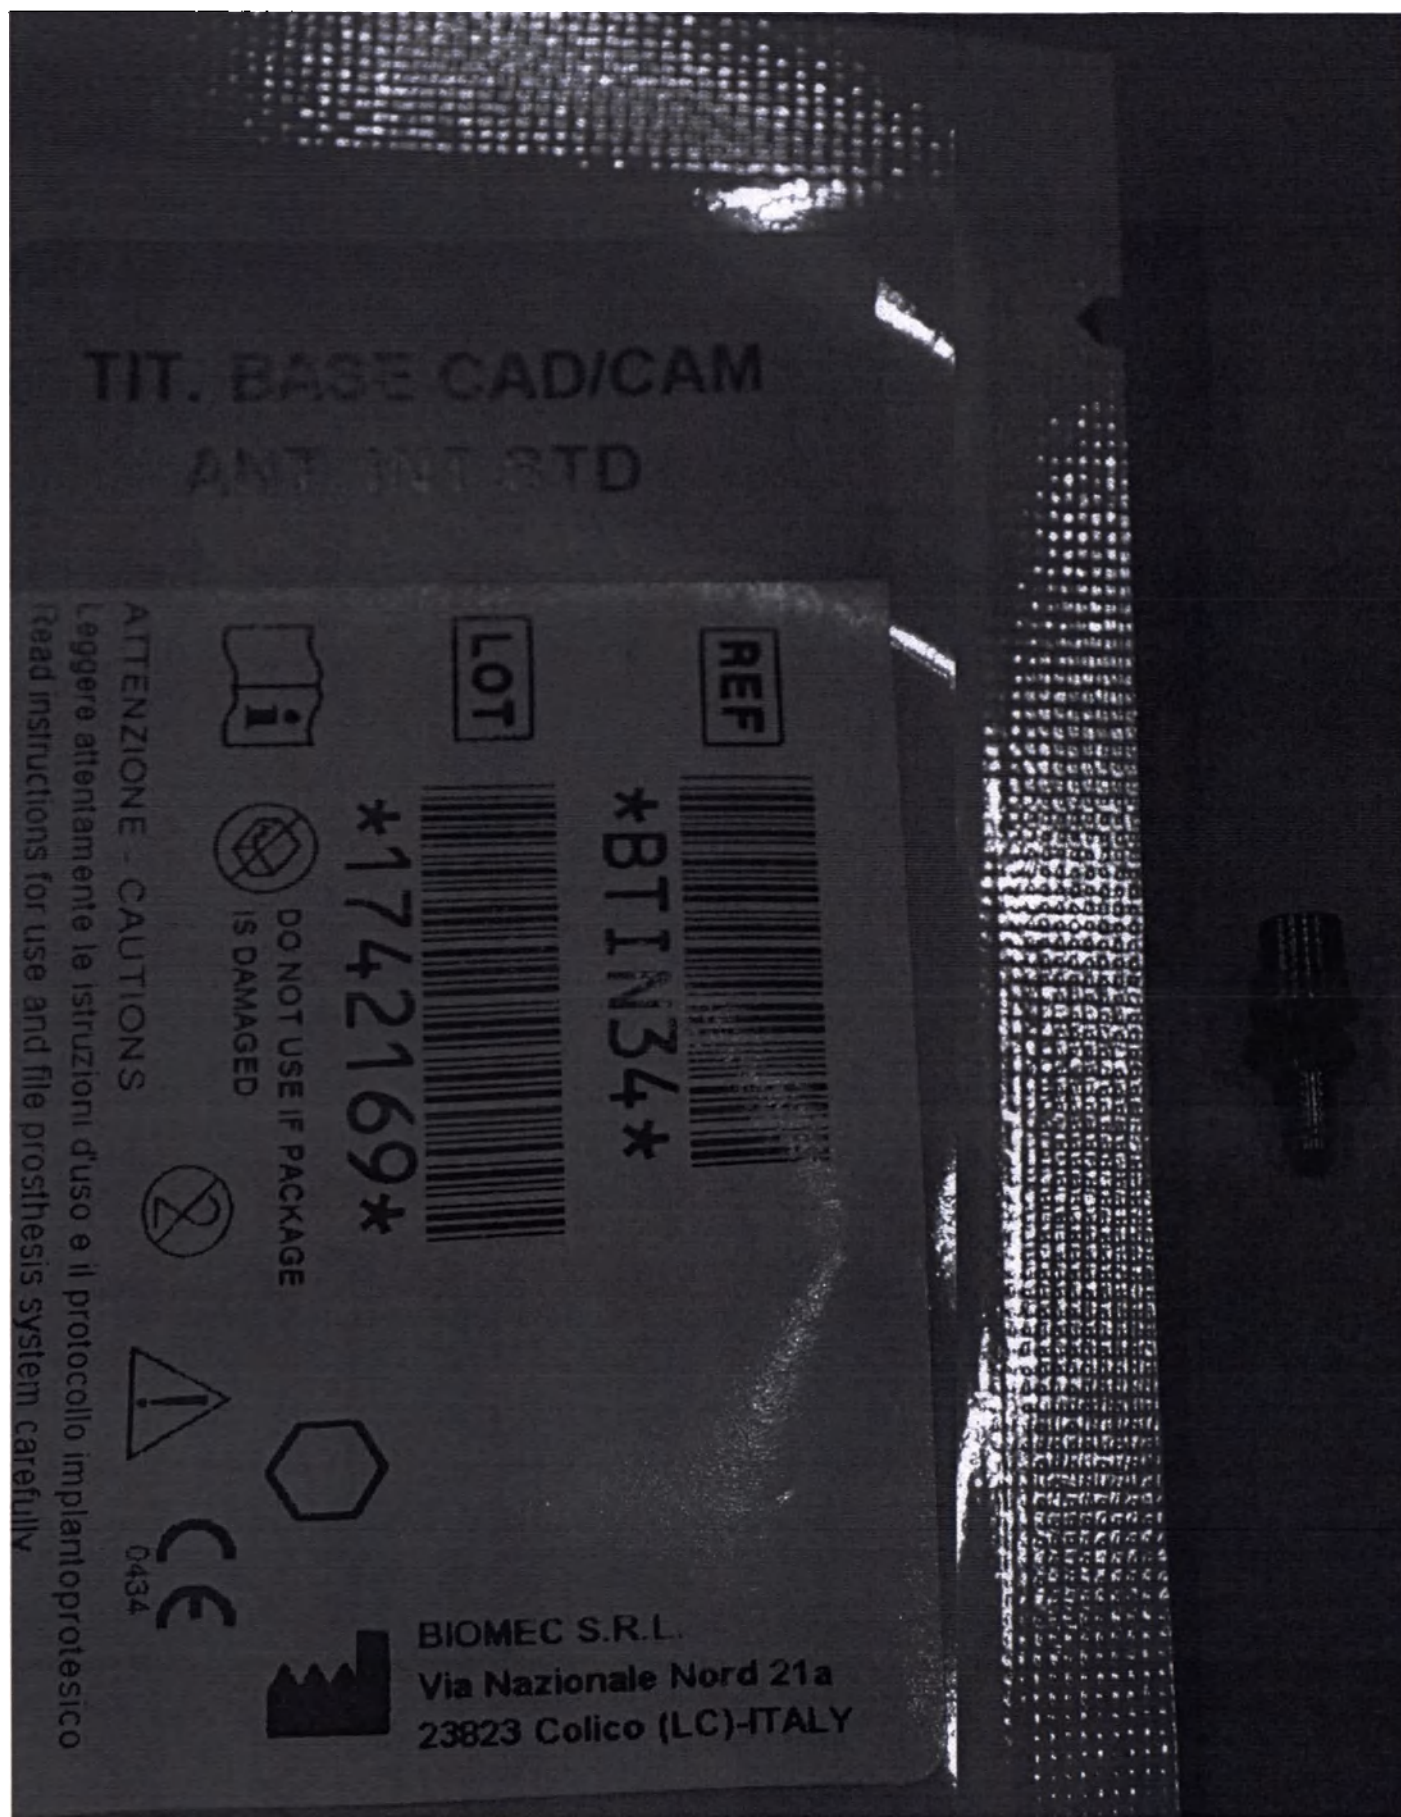


основание титановое ротационное cad/cam лит (titanium base cad/cam rot. Int)



основание хромокобальтовое антиротационное cad/cam нит (coCr base cad/cam ant. Int)

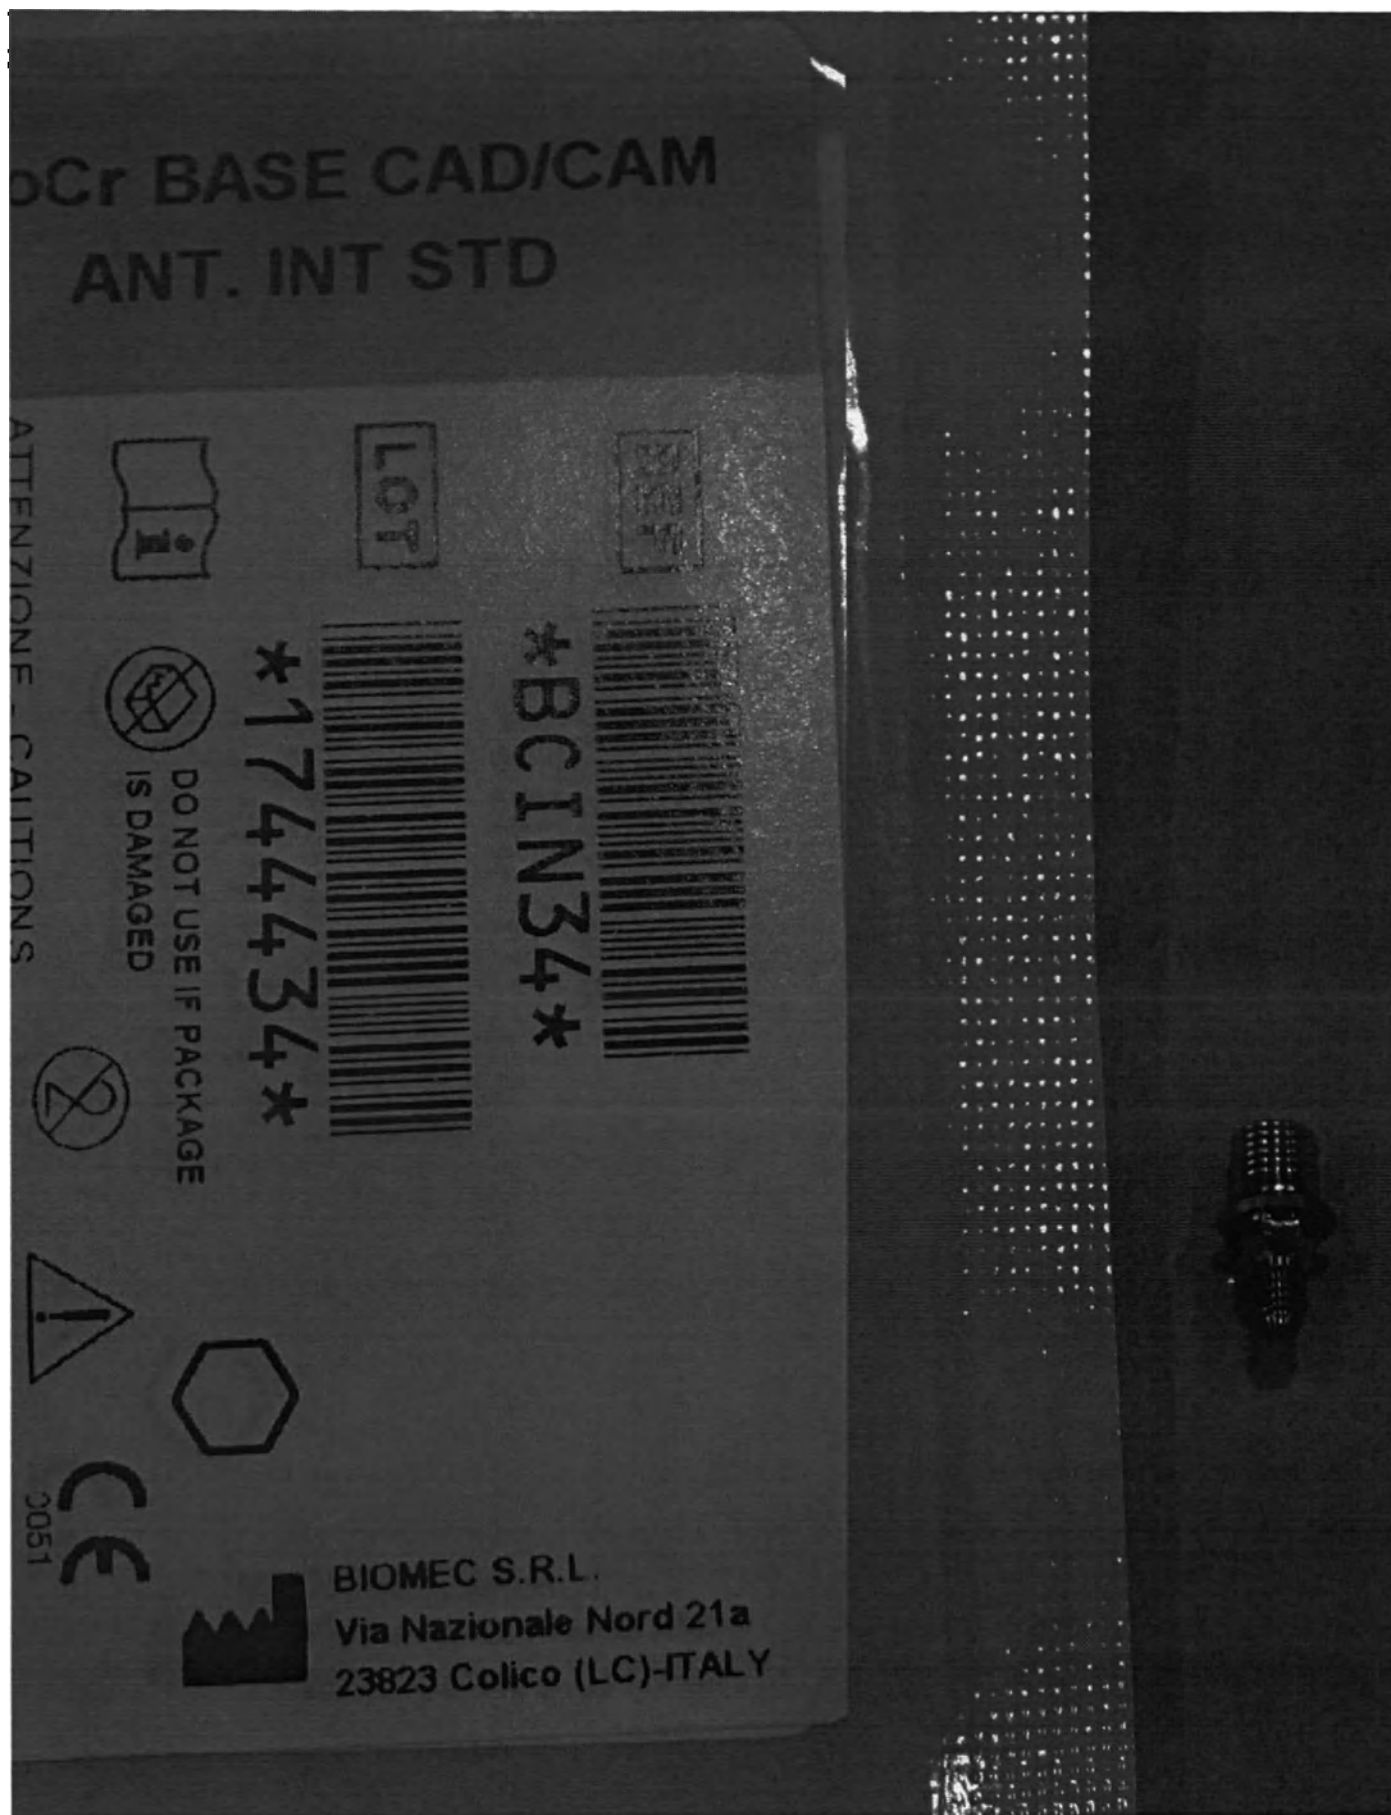

основание хромокобальтовое ротационное cad/cam штт (cocr base cad/cam rot. Int)

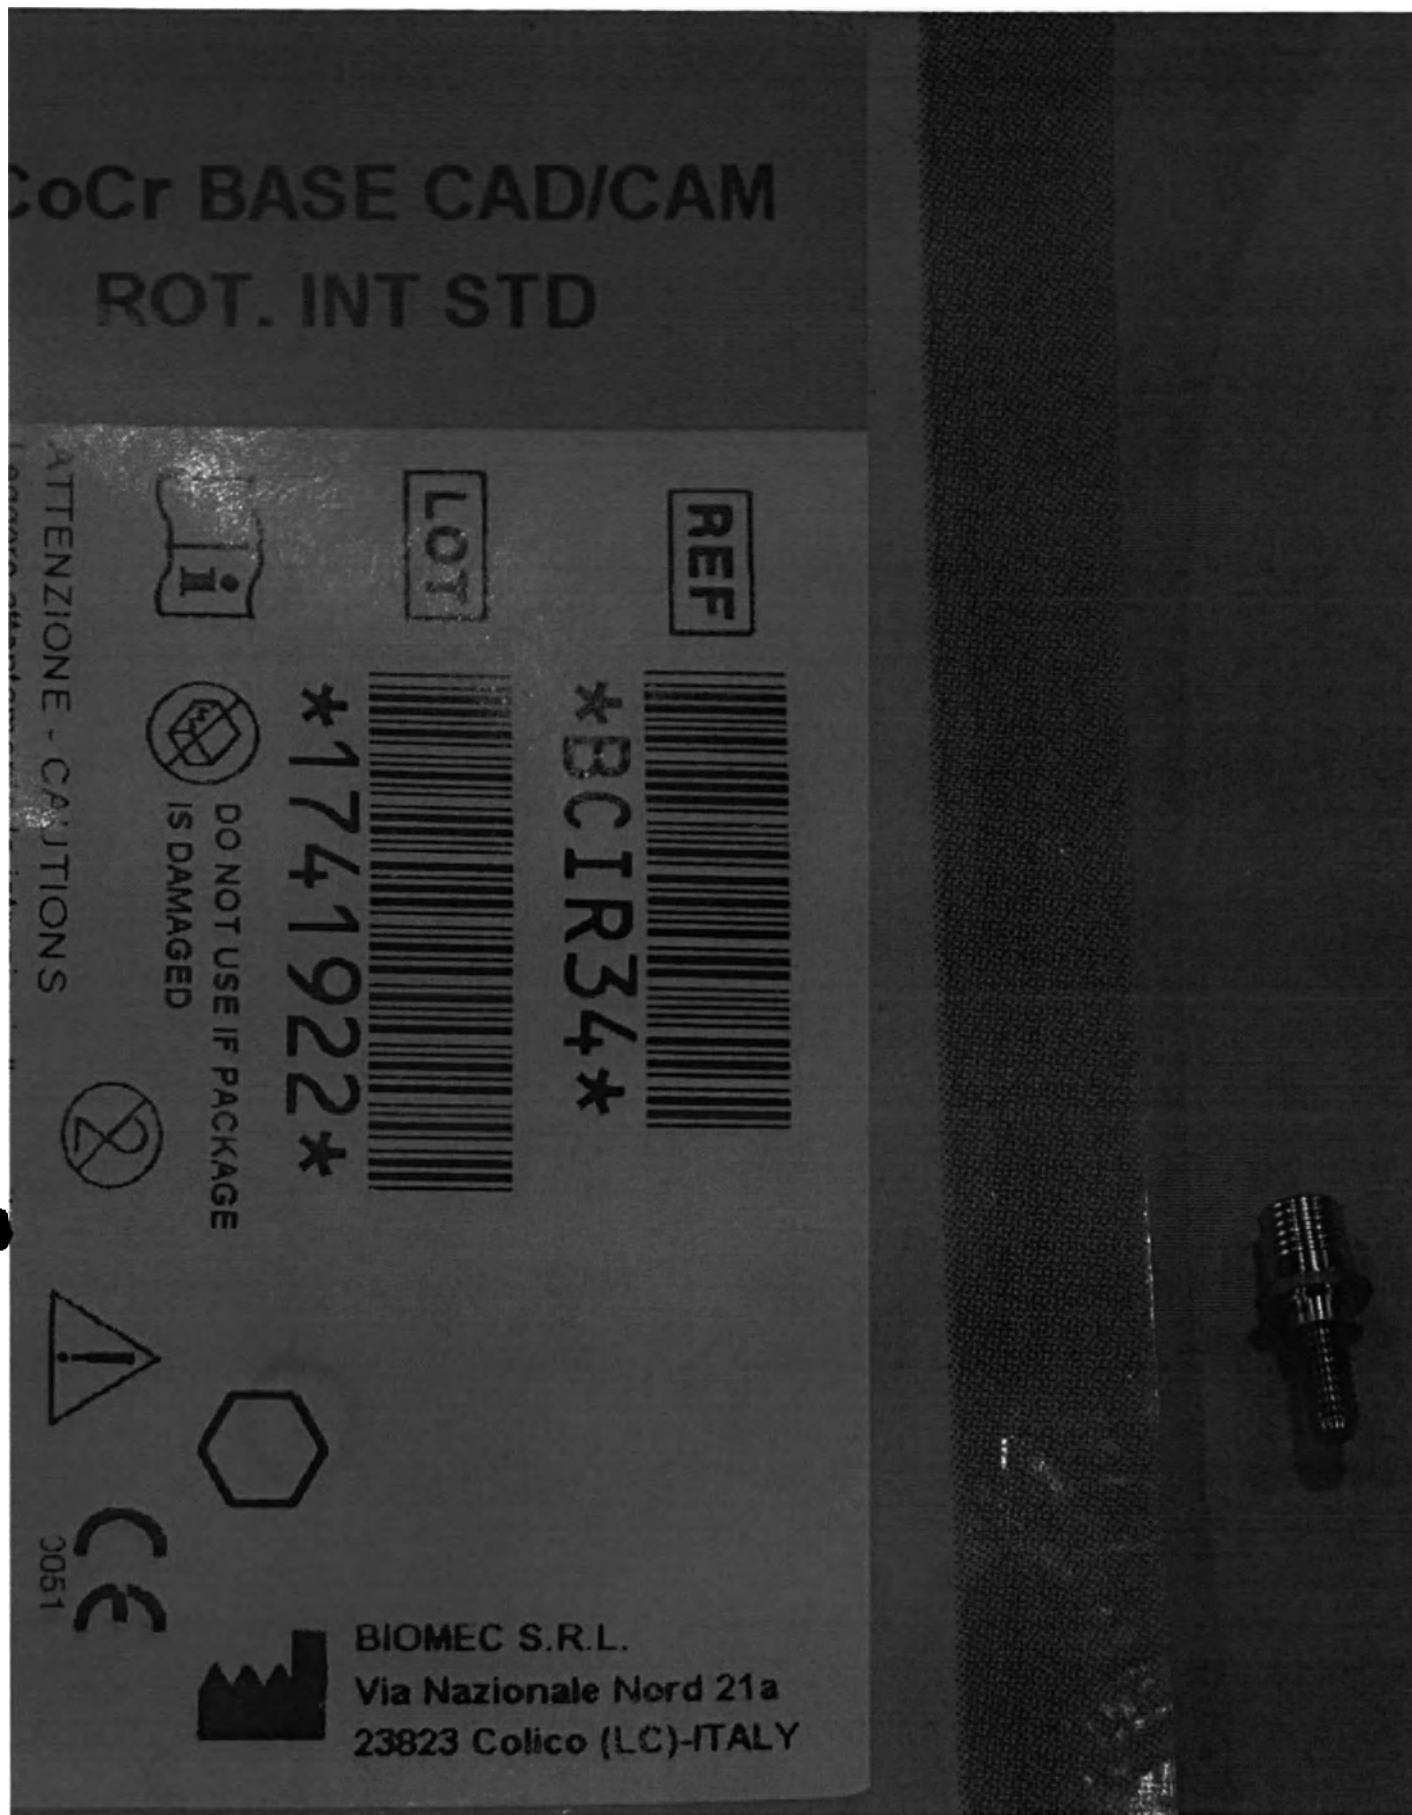

основание прямое илс нмт (straight base ils int)

STRAIGHT BASE ILS H2 INT MINI

REF

LOT

LA1002020*

17744102



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMECC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

основание угловое 17° илс инт (angled base 17° ils int)

ANGLED BASE 17°
ILS H3 INT STD

REF

ILS H3 INT STD 173430

LOT

1845053



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



основание угловое 35° или INT (angled base 35° или int)

ANGLED BASE 35°
ILS H4 INT STD

REF




ILAI353440


LOT



F1633467



DO NOT USE IF PACKAGE
IS DAMAGED



0434

CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

комплект лабораторных абатментов инт (lab abutment set int) INLAB

REF



INLAB


LOT



1846722



DO NOT USE IF PACKAGE
IS DAMAGED



CE

ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт для лабораторного абатмента инт (lab abutment screw int)

LAB ABUTMENT
SCREW STD/MAXI

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



CE


5 units



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

LOT

F1011623




REF

LBEL3400



указатель хирургический направления имплантатов (direction guide)

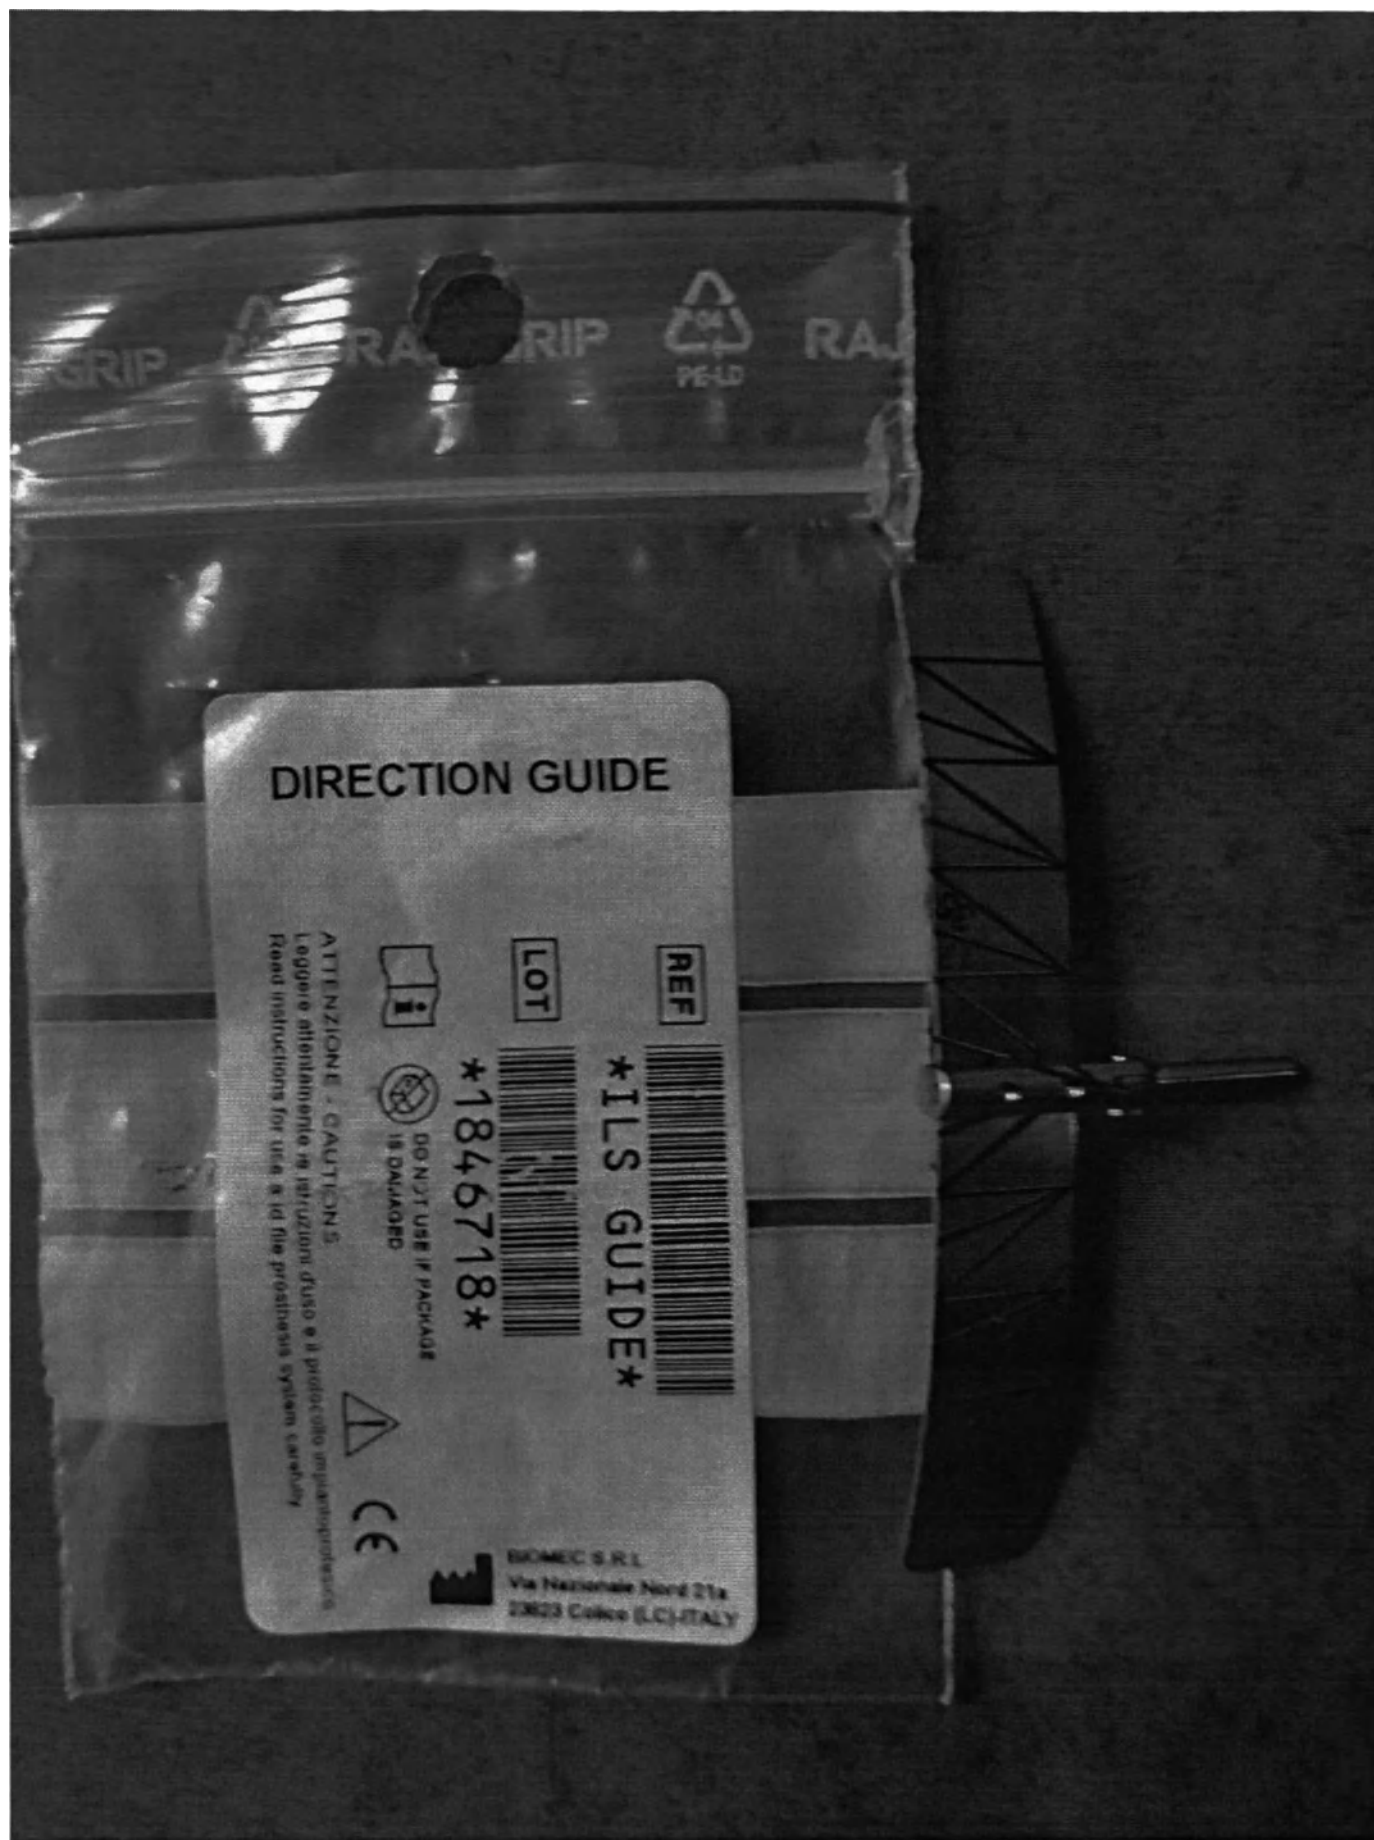

винт для слепочного трансфера инт (imp. Coping transfer screw int)

MP. COPING TRANSFER SCREW INT

REF



LTSS3400

LOT



F1633136



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт фиксирующий для абатмента м2 (abutment screw m2)

ABUTMENT SCREW M2

REF



DSEI3400

LOT




1849972



DO NOT USE IF PACKAGE
IS DAMAGED

5 units



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.

Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



абатмент выжигаемый для универсального основания int (castable abut. For int universal base)

CASTABLE ABUT. FOR
UNIVERSAL BASE INT

CAUTIONS
Read instructions for use and the prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



LOT

1953148



REF

CB



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

винт фиксирующий для универсального основания (universal base screw)



абатмент ротационный выжигаемый для эстетического абатмента (rot. Castable for aesthetic abut.)

ROT. CASTABLE FOR
AESTHETIC ABUT. STD

REF

LOT

NCA0034

1743003



DO NOT USE IF PACKAGE
IS DAMAGED



CE

ATTENZIONE - CAUTIONS
Léggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and the prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

абатмент антиротационный выжигаемый для эстетического абатмента
(ant. Castable for aesthetic abut.)



винт фиксирующий для эстетического абатмента (aesthetic abutment screw)

AESTHETIC ABUTMENT SCREW

REF



DSAA0030

LOT



1743735



DO NOT USE IF PACKAGE
IS DAMAGED

5 units



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



винт для углового основания ИЛС ИНТ (its angled base screw int)

**SCREW FOR ANGLED
BSE ILS INT**

REF



ILAS

LOT



F1527684



DO NOT USE IF PACKAGE
IS DAMAGED



2 Units

BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



CAUTIONS

Read instructions for use and file prosthesis system carefully

контейнер титановый для шаровидного абатмента (titanium cover for ball abut.)

TITANIUM COVER FOR MINI BALL ABUTMENT

REF



MBE10018

LOT



1742698



DO NOT USE IF PACKAGE
IS DAMAGED



2 units



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico

контейнер титановый с пластиковым колпачком для шаровидного абатмента (
titanium cover with plastic cap for ball abut.)

**TITANIUM COVER +
RETENTION CAP SOFT
FOR BALL ABUT.**

CAUTIONS
Read instructions for use and file prosthesis system carefully



LOT

REF




DO NOT USE IF PACKAGE
IS DAMAGED

1847592



22PBET0010T



CE



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

контейнер титановый для окси лок (titanium cover for oxyloc)

TITANIUM COVER FOR OXY LOC

REF



CTLOC

LOT



1744435



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

RETENTION CAP FOR HARD BALL ABUT.

REF

CN005

LOT

1952042



DO NOT USE IF PACKAGE
IS DAMAGED



5 units



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and fit the prosthesis system carefully

колпачок ретенционный мягкий для шаровидного абатмента (retention cap soft for ball abut.)

RETENTION CAP SOFT FOR BALL ABUT.

REF



CND006

LOT



1951989



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully




5 units



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

Read instructions for use and file prosthesis system carefully

колпачок ретенционный экстрамягкий для шаровидного абатмента
(retention cap extrasoft for ball abut.)

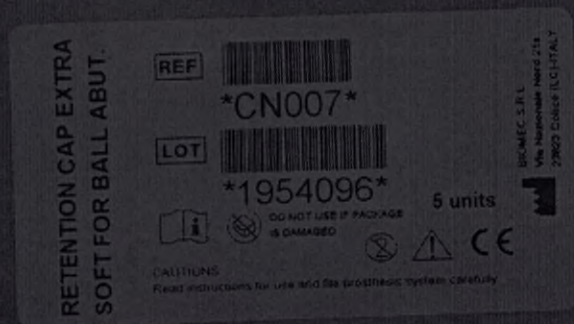

RETENTION CAP FOR OXY LOC EXTRASOFT

REF

LOT



CN098



1858316

5 units



CAUTIONS
Read instructions for use and the prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



RETENTION CAP FOR OXY LOC SOFT

REF

LOT



CN097



1959129



DO NOT USE IF PACKAGE
IS DAMAGED



5 units



BIOMECH S.R.L

Via Nazionale Nord 21a

23823 Colico (LC)-ITALY

CAUTIONS
Read instructions for use and file prosthesis system carefully

колпачок ретенционный для оксилок стандарт (retention cap for oxyloc standard)

колпачок ретенционный для окси лок лабораторный (retention cap for oxy loc
laboratory)

RETENTION CAP FOR
OXY LOC LABORATORY

REF



CN100

LOT



1959127

5 units



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

колпачок ретенционный для шаровидного абатмента мини конический (retention cap
for ball abut. Mini conical)

RETENTION CAP FOR
BALL ABUT. MINI


CONICAL

REF



CN011

LOT



1953960

5 units



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and fit prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
20021 Celico (LC) ITALY

сверло пилотное D 1.8 (pilot drill D 1.8) SID01S SID01L



PILOT DRILL
D. 2,3 LONG

LOT


SIDOOL



1846914



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale
23823 Colico (LC)

128

сверло калиброванное начальное (initial grad. Drill)



INITIAL GRADUATED
DRILL D.2,30 mm

REF



IGSD230

LOT



1850744




DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis syst

сверло калиброванное конечное (final grad. Drill)

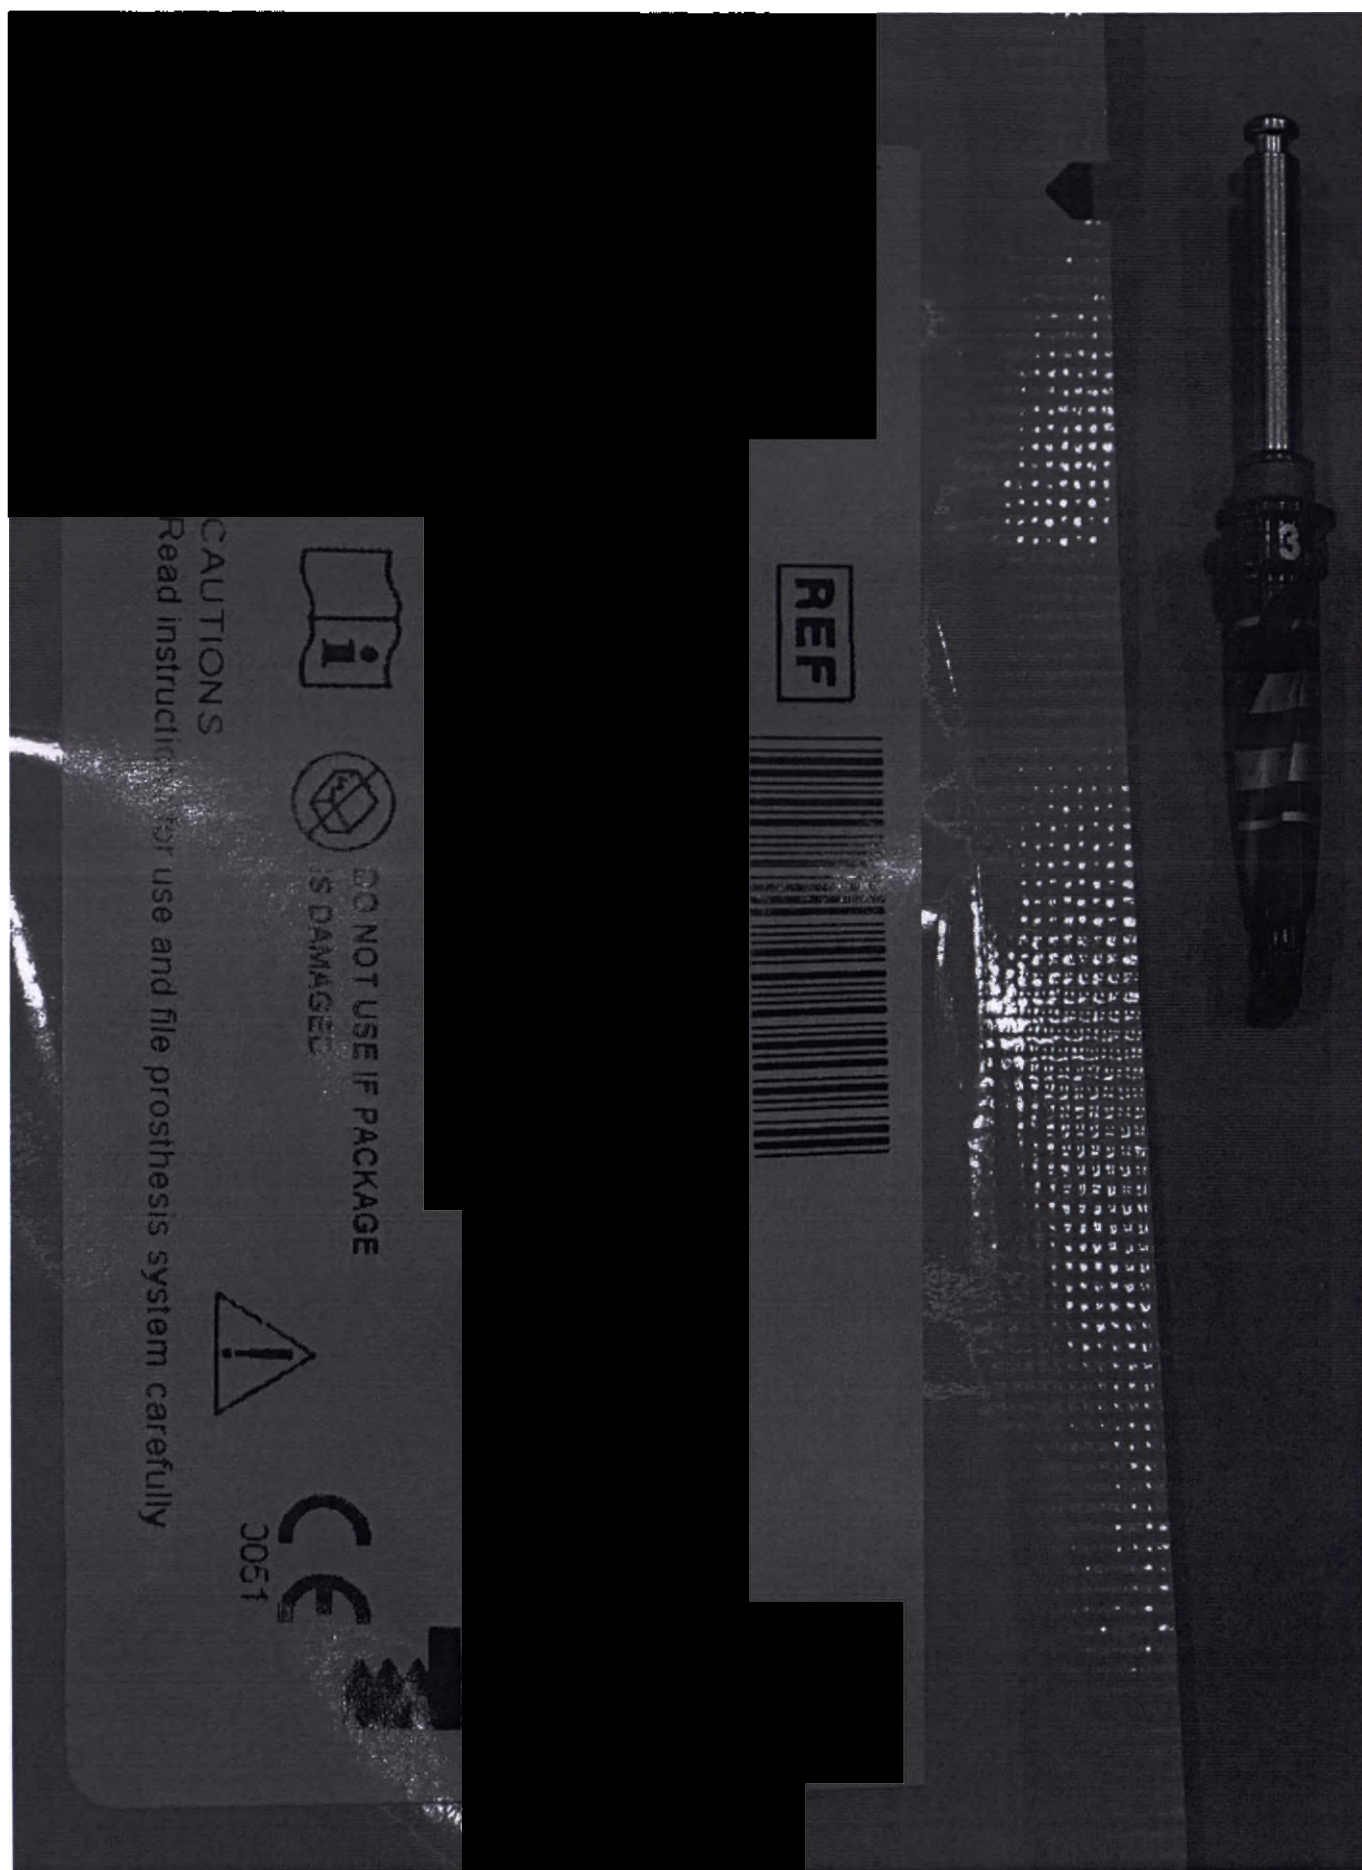

CALIBRATED STOP

L. 5,5

REF

LOT

EST4055T

1847103



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS
Read instructions for use and file prosthesis system carefully




HOMEC S.R.L.
Via Nazario Nord 21a
23623 Colico (LC)-ITALY

131

сверло кортикальное пс/ккс (countersink drill ps/cls) STDPSILS

COUNTERSINK DRILL PS/CLS

REF

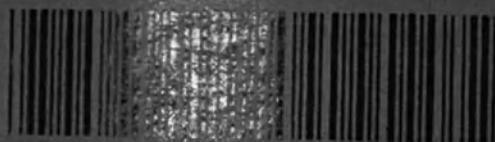

STDPSILS

LOT



F1633360



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



CE
0434

BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



TISSUE PUNCH
STD/K1 NARROW

REF



MPU34

LOT



1847105



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and the prosthesis system carefully




CE
0051



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



133

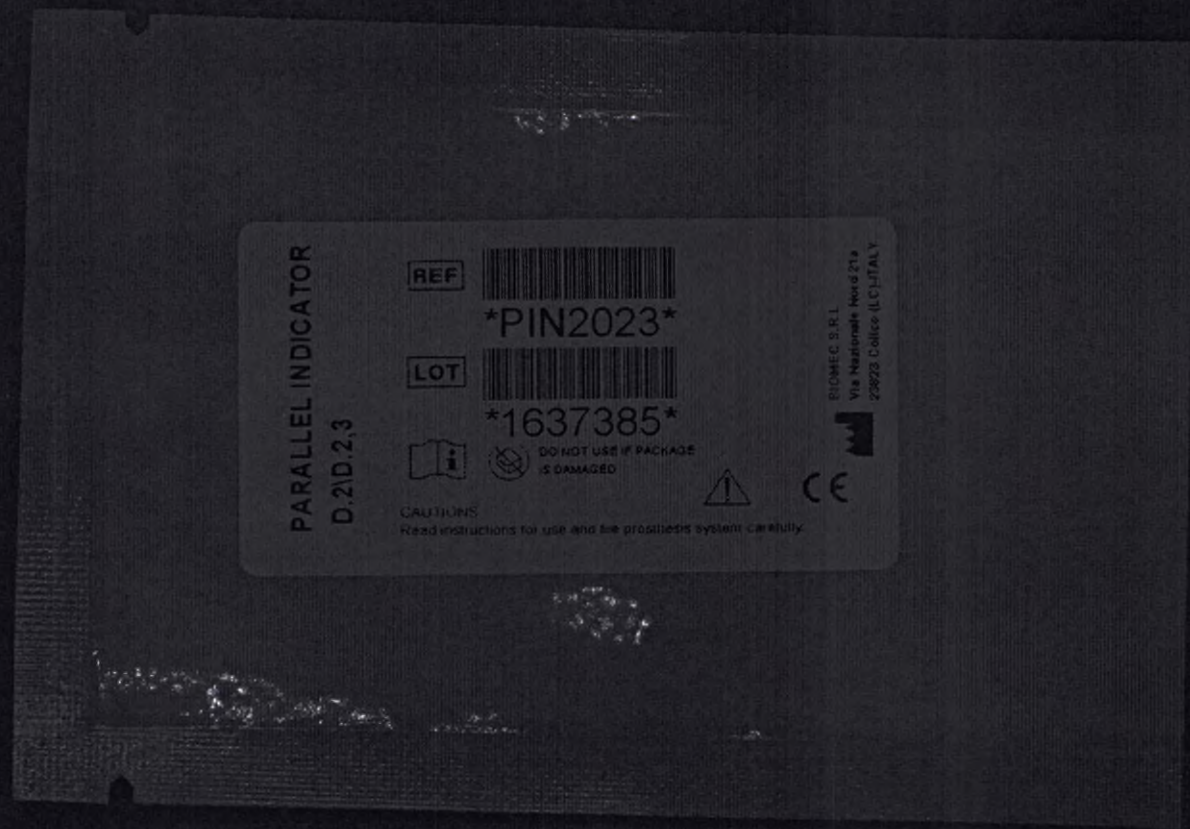

DRILL EXTENSION

REF



DEXT


LOT



1847107



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



135



CAUTIONS

Read instructions for use and file prosthesis system carefully

костный экспандер механический - ручной, микро (bone tap mec - man micro)

BONE TAP MEC-MAN D 4 MICRO

REF

LOT

TDLT400

1847108



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS


Read instructions for use and all



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



костный экспандер механический - ручной, нормо (bone tap mec - man normo)

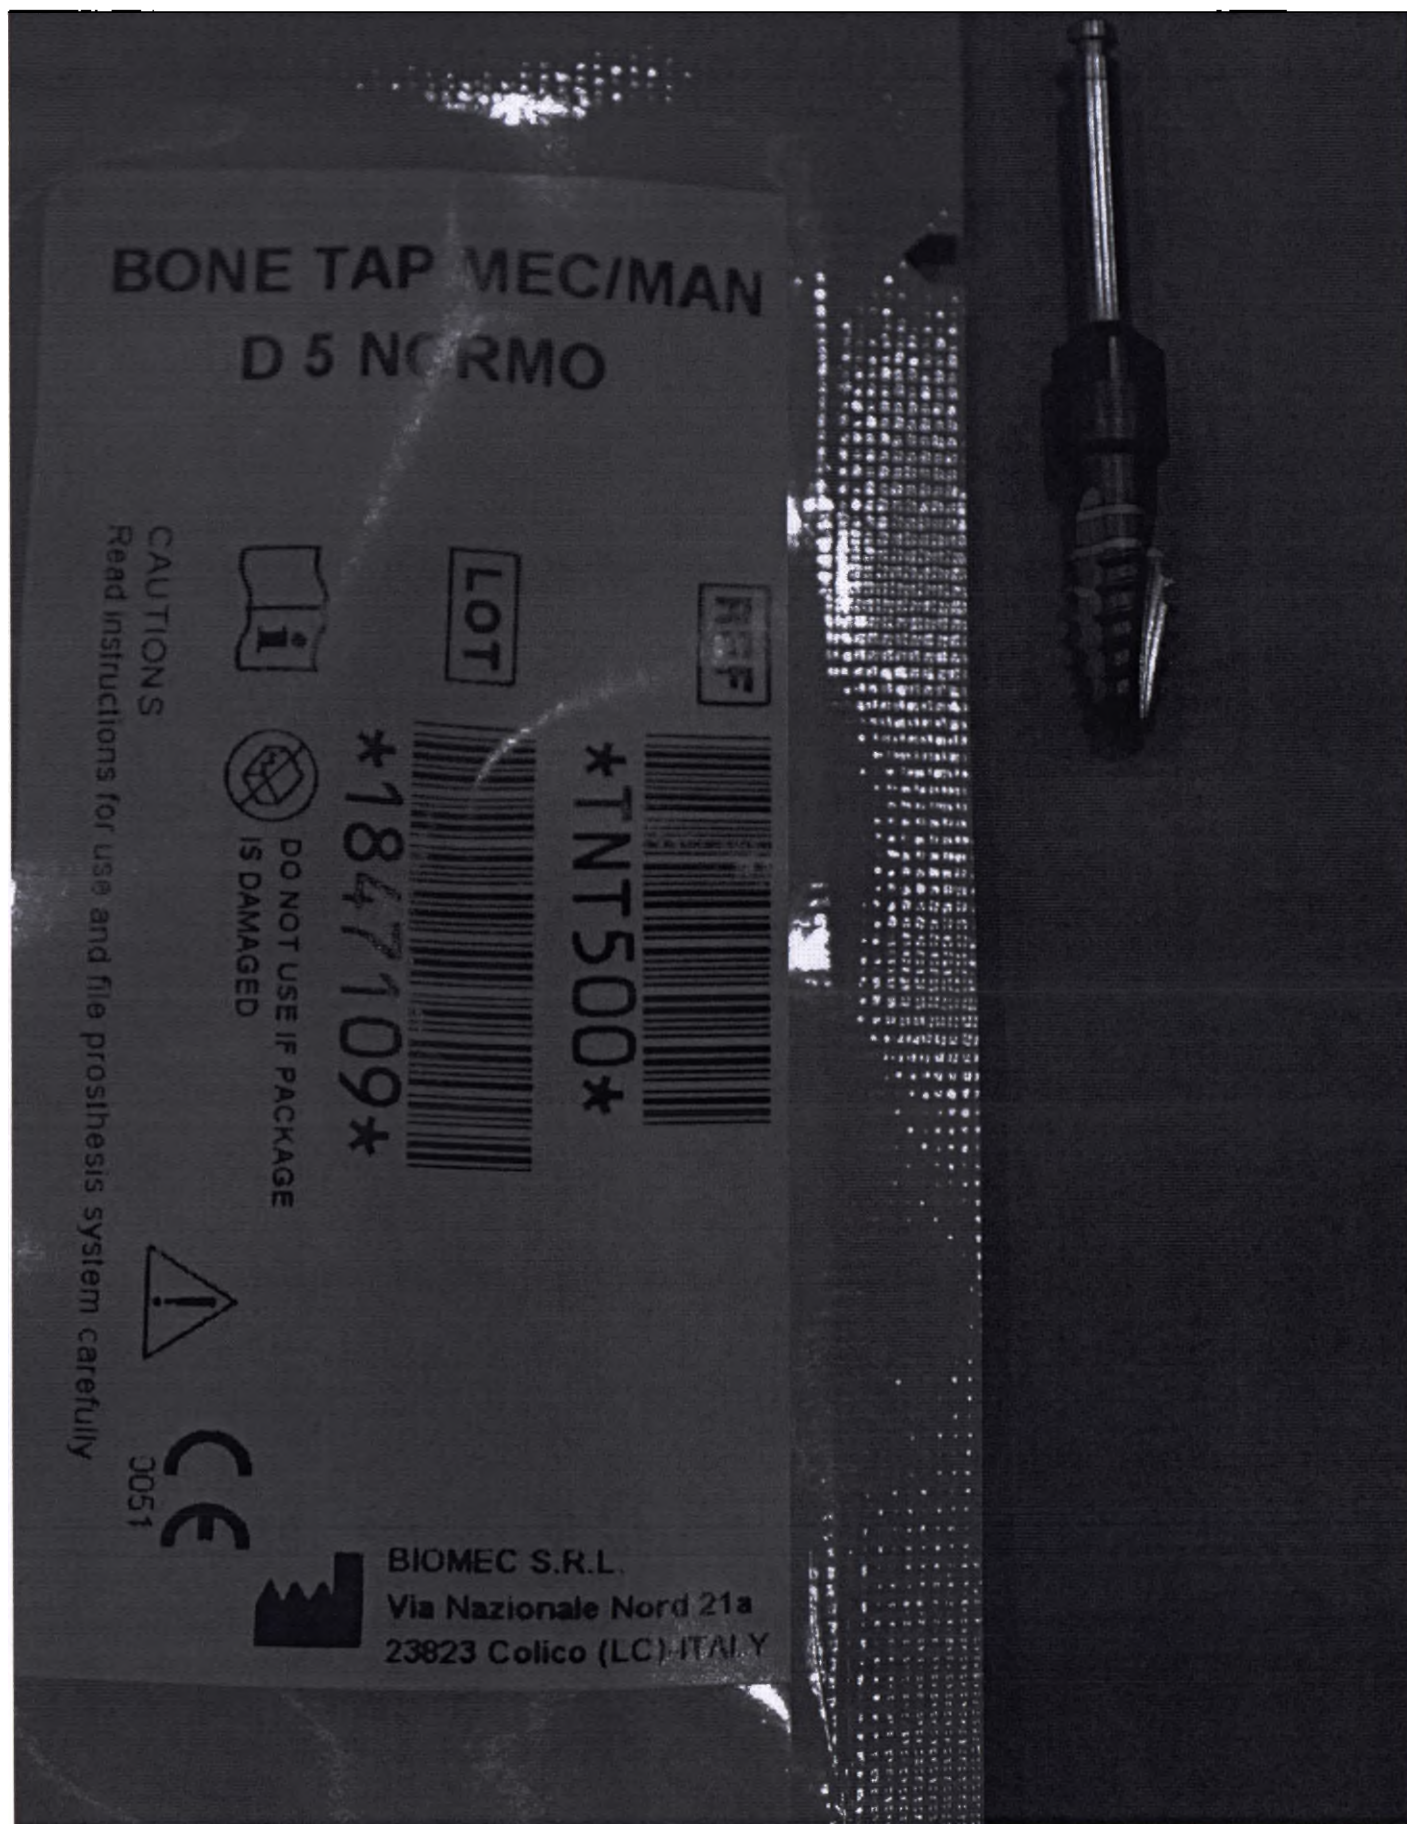

костный экспандер - ручной, классик микро (man. Bone tap classic micro)

MAN. BONE TAP CLASSIC D 3,3 MICRO

REF

TAP330PF

#847110*



DO NOT OPEN PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and the prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



костный экспандер - ручной, классик нормо (ман. Bone tap classic normo)

MEC. BONE TAP
CLASSIC MICRO
D.3,30

CAUTION:
Read instructions for use with the product and follow safety
Do not use if package is damaged

REF

LOT

1741899

MTAP330PF*

CE

BIOMEC S.R.L.
Via Nazionale Nord 21a
20123 Corso (L.C.) ITALY

MEC. BONE TAP
CLASSIC NORMO
D.3,75

CAUTION
Read instructions for use and the pressure system carefully



LOT

REF



DO NOT USE IF PACKAGING IS DAMAGED

1741900



MTAP375PL



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

сверло пилотное для экстрашорт (pilot drill for extrashort)

PILOT DRILL D 2,5 FOR EXTRASHORT

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



LOT

1847112



REF

EXSID00



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



сверло для экстрашорт (drill extrashort)

DRILL EXTRASHORT D 4,5

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



LOT

1847113



REF

EXFGSD450



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



ограничитель сверла для экстрашорт (extrashort stop)

EXTRASHORT STOP L 8



LOT

REF



DO NOT USE IF PACKAGE
IS DAMAGED

1847114



ESSTE08



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

костный экспандер ручной микро для экстрашорт (man. Bone tap extrashort micro)

**MAN. BONE TAP
EXTRASHORT
D.5,75 MICRO**

REF

LOT



**DO NOT USE IF PACKAGE
IS DAMAGED**

1847115



EXTAP575PF



CAUTIONS
Read instructions for use and file prosthesis system carefully



**BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY**



мукотом для микро (tissue punch for micro)

TISSUE PUNCH FOR MICRO

REF



MPU10

LOT



1847116



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully.



0051

BIOMEC S.R.L.
Via Nazionale Nord 241
23823 Colico (LC)-ITALY



MEC. INSERTER INT LONG

REF

LOT

LMEIT



1847117



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS



BIDMEC S.R.L.
Via Nazionale Nord 21a
23823 Conco (LC)-ITALY



DRIVER INSERTER INT EXTRALONG

CAUTIONS
Read instructions, ISO 10000 and EN 15000




LOT

REF



DO NOT REUSE THIS PACKAGE

18471103

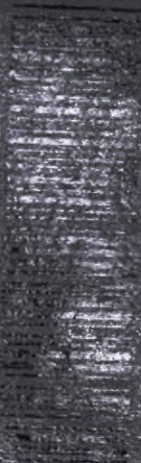

*E132



BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



отвертка механическая для винтов (mec. Screwdriver for screws)

MEC. SCREWDRIVER FOR SCREWS EXTRALONG

REF



MEELSD

LOT



1847119



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS



CE
0051

BIOMECH S.R.L.

Via Nazionale Nord 219

отвертка ручная для винтов (man. Screwdriver for screws)

MAN. SCREWDRIVER FOR SCREWS EXTRALONG D8

REF

LOT



ELMSD8



1847120



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



ключ механический для прямого абатмента и/или эстетического абатмента (mec. Driver for its straight base/aesthetic abut.)



ключ механический для имплантата микро фикс (mec. Driver for micro fix implant)



153

MEC. DRIVER FOR
MICRO FIX IMPLANT

REF



MAXP

LOT



1741343



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully




CE
0434

BIOMEC S.R.L.

153

ключ механический для шаровидного абатмента / микро фикс сфир (mec. Driver for ball abut. /micro fix sphere)

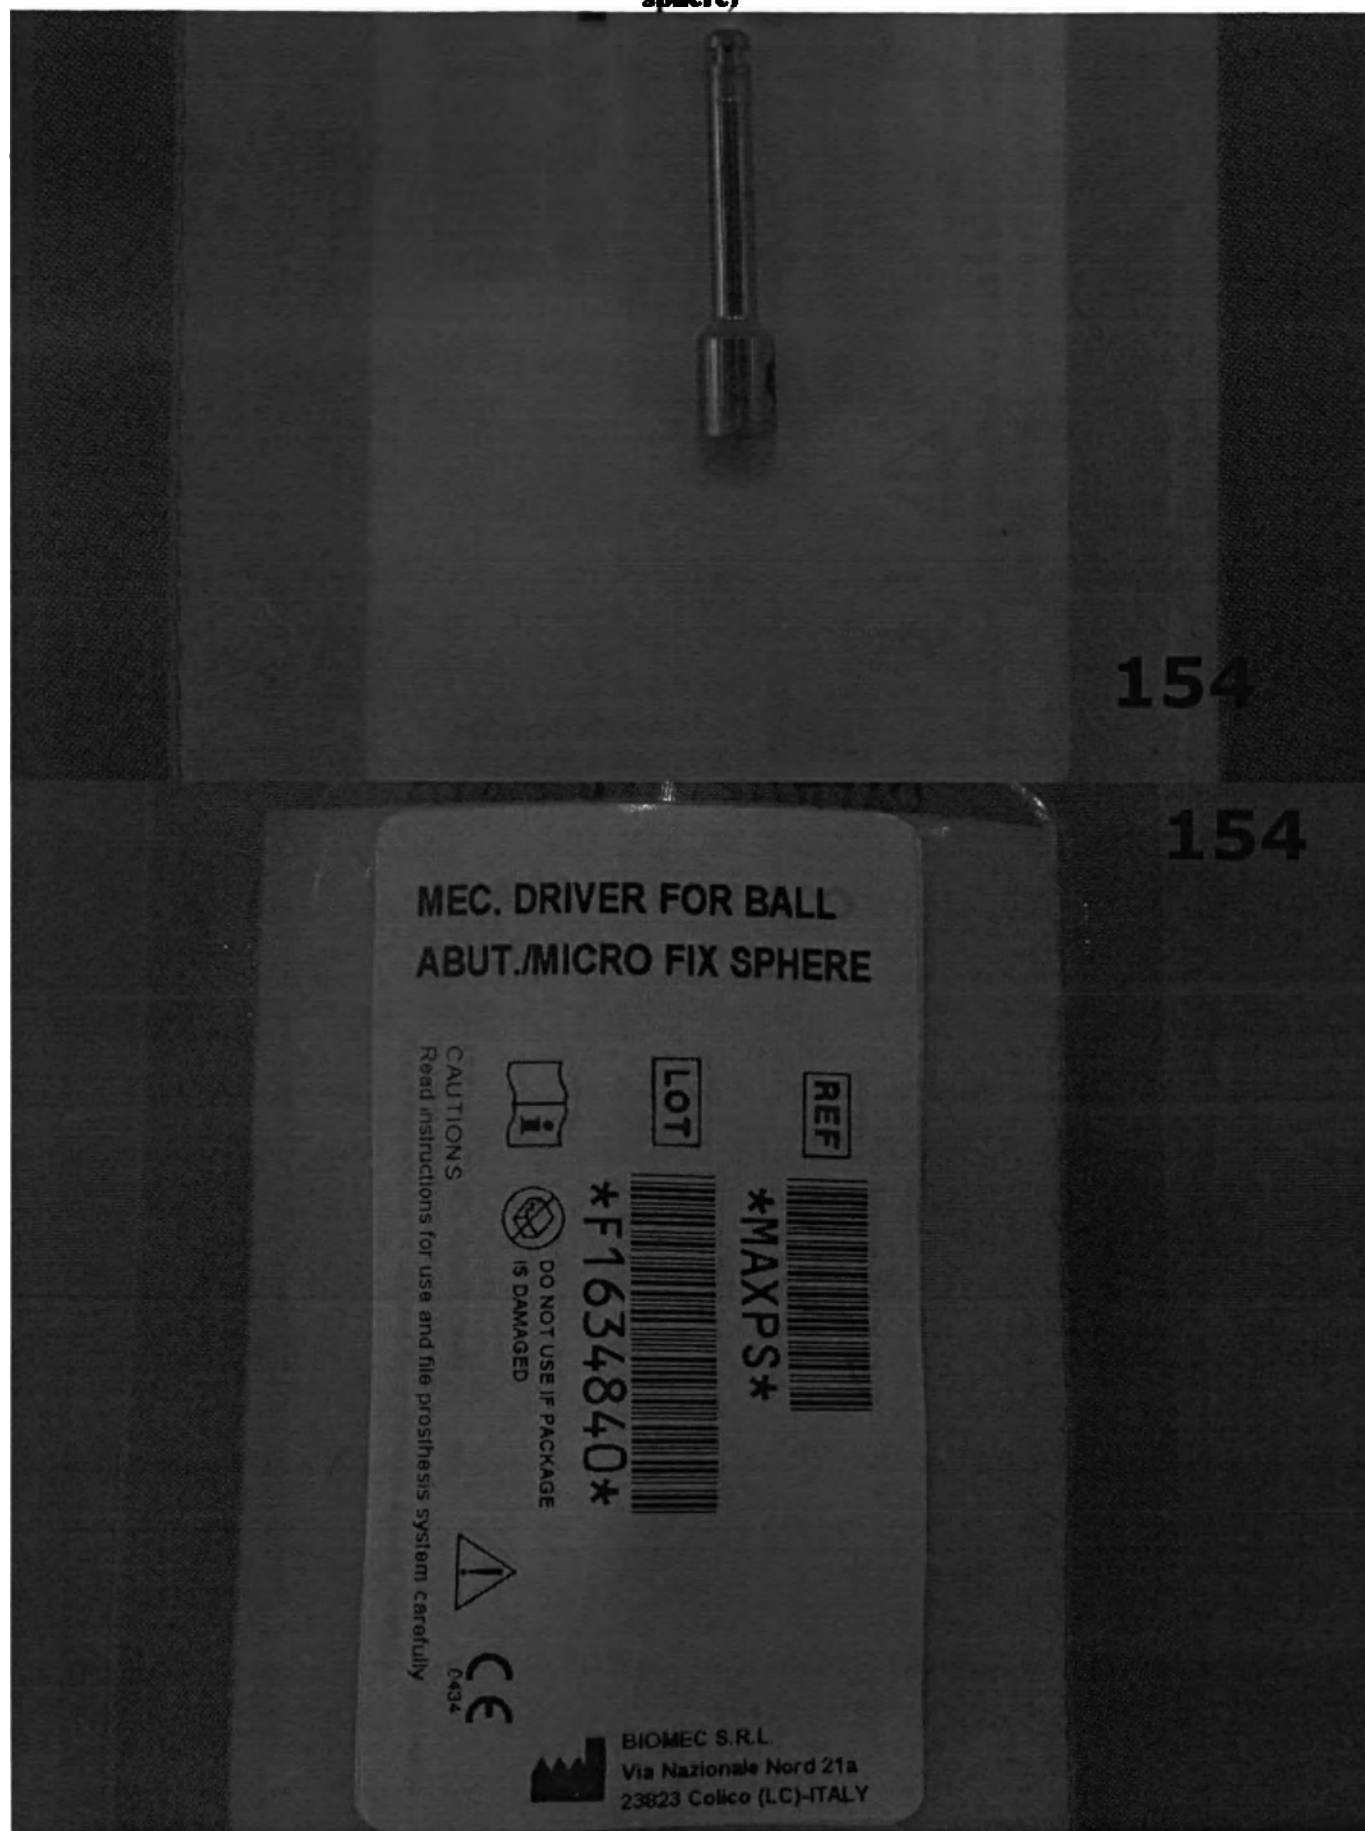

ключ ручной для прямого абатмента илс (man. Driver for ILS straight bases)



ключ ручной для имплантата микрофикс (man. Driver for micro fix implant)



156

DESIGN & PRODUCTION
100% MADE IN ITALY
www.oxvimplant.com

MAN. DRIVER FOR
MICROFIX IMPLANT

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



CE

LOT

1846771



REF

MFDD8



156

BIOMECH S.R.L.
Via Nazionale Nord 21a

ключ ручной для шаровидного абатмента / абатмента микро фикс сфер (man. Driver for ball abut. /micro fix sphere)



MAN. DRIVER FOR BALL
ABUT. / MICROFIX SPHERE

CAUTIONS
Read instructions for use and file prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED

LOT

1850958



REF

MBDD8



CE



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

157

ключ ручной для костного экспандера (man. Driver for bone taps)



DESIGN & PRODUCTION
100% MADE IN ITALY


158

MAN. DRIVER FOR
BONE TAPS

ATTENZIONE - CAUTIONS
Leggere attentamente le istruzioni d'uso e il protocollo impiantoprotesico
Read instructions for use and the prosthesis system carefully



DO NOT USE IF PACKAGE
IS DAMAGED



LOT

1848132



REF

CMRC8



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

158

глубиномер (depth gauge)



ключ прямой (straight key)

160

STRAIGHT KEY

REF



DEK

LOT



1847129



DO NOT OPEN IF PACKAGE IS DAMAGED

CAUTIONS


Read instructions for use and file preparation system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Celico (LC)-ITALY



ключ-трещотка реверсивный (reverse ratchet)



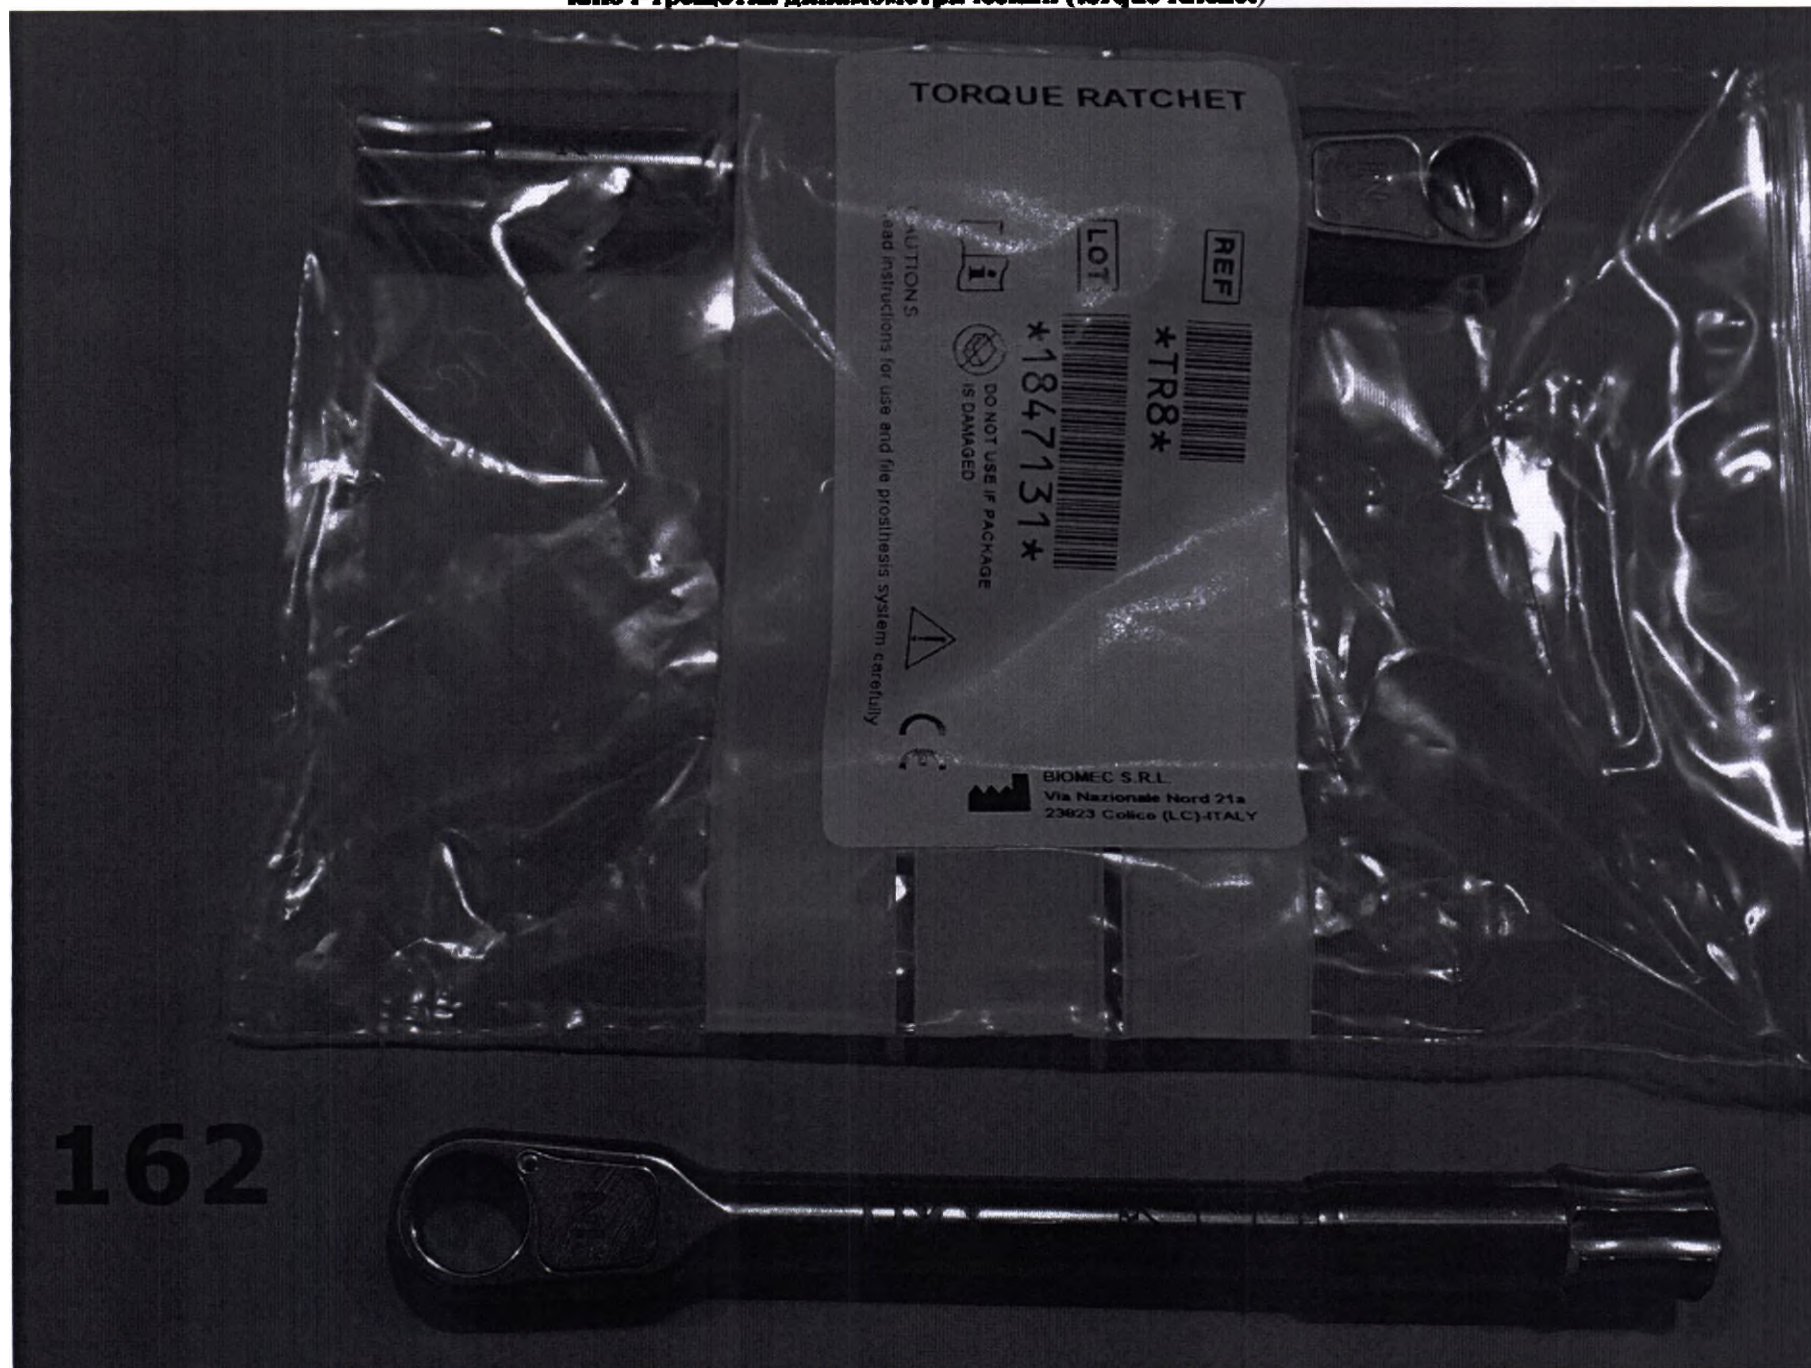

162

ключ-трещотка ручной (lever key)



сверло пилотное к1 (pilot drill k1)

PILOT DRILL SHORT D2

REF



*K1LD

LOT



1847133



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file procedures carefully

BICMEC S.R.L.
Via Montebello, No. 21a
20129 Milano (Italy)



сверло начальное к1 (initial drill k1)

INITIAL DRILL K1

D 2,3 H 15

REF

LOT



K1ID150



1347134



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and the synthesis sy

сверло заключительное k1 (final drill k1)

FINAL DRILL K1 NARROW H7



LOT




DO NOT USE IF PACKAGE
IS DAMAGED

1847135



K1FDN070

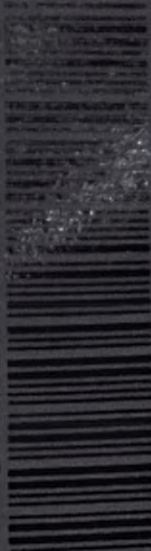

Via Nazionale Nord 211

сверло кортикальное (countersink drill)

COUNTERSINK DRILL WIDE



REF




DO NOT USE IF PACKAGE
IS DAMAGED

1847136



1CSDW

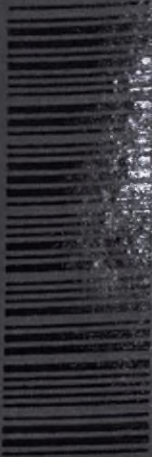

BIOMECH S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC) ITALY



костный экспандер механический/ручной k1 (bone tap mec/man k1)

BONE TAP MEC/MAN K1 REGULAR

REF

LOT



K1TAPR



1847137



DO NOT USE IF PACKAGE
IS DAMAGED

CASETAPRIS

Read instructions for use and file prosthesis system carefully



CE
3051



BIOMECH S.R.L.

Via Nazionale Nord 21a

23823 Colico (LC) ITALY



MEC. INSERTER STD CONICAL LONG


169

CAUTIONS
Read instructions for use and file prosthesis system carefully




LOT

REF



DO NOT USE IF PACKAGE
IS DAMAGED

1847140*

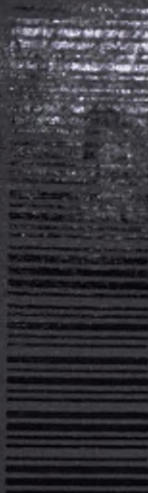

MEC INRL*



CE
0051



BIOMECC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY





индикатор направления винтовой конический (parallel ind. Screwable conical)

171

PARALLEL INDICATOR
SCREW-RET.
MINI CONICAL



LOT

REF



DO NOT USE IF PACKAGE
IS DAMAGED

1847142



K1SWPN



BIOMEC S.R.L.
Via Nazionale Nord 21a
23923 Colico (LC) ITALY

ключ для извлечения абамента конический (abut. Removal driver conical)

ABUT. REMOVAL DRIVER STD CONICAL

172

REF



K1ARDR

LOT



1847143



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.

Via Nazionale Nord 21a

23823 CORNO (LC)-ITALY



сверло для пина оге (pin drill ogs)

173



REF



IOMEC S.R.L.
Via Nazionale Nord 21a
3823 Colico (LC)-ITALY

IS DAMAGED



for use and file pro

174

FIXING PIN FOR TEMPLATE OGS

REF

LOT

PINGS



1847145



DO NOT USE IF PACKAGE
IS DAMAGED



3051

CAUTIONS
Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Repubblica
23823 Colico (LC) ITALY



175



TISSUE PUNCH OGS

REF



TPGS

LOT



1847146



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



сверло для подготовки кости орс (bone level drill ogs)


176

BONE LEVEL DRILL OGS


REF



LOT

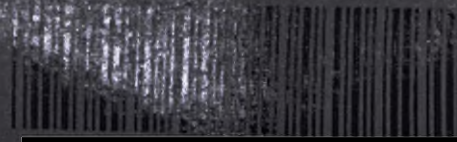

CAUTIONS

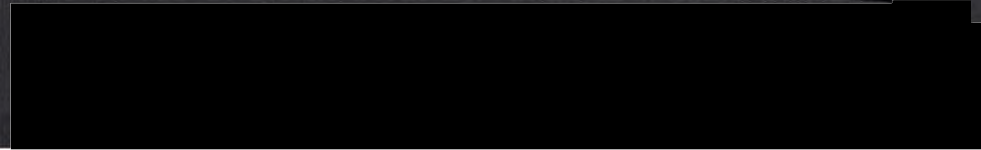

CE
0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



сверло пилотное/контрзакладное инт орс (pilot/countersink drill int ogs)

PILOT/COUNTERSINK DRILL INT OGS

177

REF

LOT



CGGS



1847148



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



CE
0051



сверло к1 пилотное огс (k1 pilot drill ogs)

178

K1 PILOT DRILL OGS

REF



K10GSPD

LOT



1847149



DO NOT USE IF PACKAGE
IS DAMAGED



0051

CAUTIONS

Read instructions for use and file prosthesis system carefully



179

INITIAL DRILL INT
OGS D 2,3 H 8,5

REF

LOT



SD23085G



1847150



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



CE
3051



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



сверло заключительное нит орс (final drill int ogs)

180

FINAL DRILL INT
OGS D 3,8 H 15

CAUTIONS
Read instructions for use and file prosthesis regularly



LOT

REF



DO NOT USE IF PACKAGE
IS DAMAGED

1847404



SD38150GS



CE
2051



BIOFEC S.R.L.
Via Nazionale Nord 21a
23823 Colla (LC)-ITALY




181



MOUNTER OGS INT

REF




G128

LOT



347152



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.

Via Nazionale Nord 21a
23823 Colico (LC)-ITALY




182



**MOUNTER OGS
K1 REGULAR**

REF

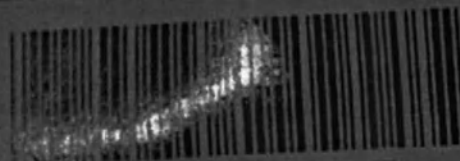


K10GSMR

LOT



1847153



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



MOUNTER REMOVAL INT



LOT

21



DO NOT USE IF PACKAGE
IS DAMAGED

1847154



GMSE



CE

CAUTIONS
Read instructions for use and file prosthesis system carefully



DRIVER CONVERTER

4X4


184

REF



MAEX

LOT

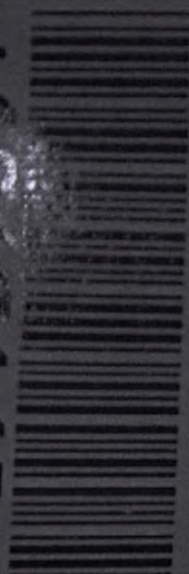

1847165



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully.



BIOMECC S.R.L.

Via Nazionale Nord 21a

23823 Colico (LC)-ITALY



185

TEMPLATE SLEEVE

REF



CGS

LOT



1847156



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthetic system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



186

FIXING PIN SLEEVE

REF



CPINGS

LOT



1847157



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



калибратор зубочелюстной (bite gauge)

187

BITE GAUGE

REF



BITEGAUGEPS

LOT



1847158



DO NOT USE IF PACKAGE
IS DAMAGED



CAUTIONS

Read instructions for use and file prosthesis system carefully



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



188

CAUTIONS
Read instructions for use and the instructions for the system carefully

REF

LOT

BMCIL

1847159

DO NOT USE IF PACKAGE
IS DAMAGED

CE 0051

BIOMECC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



мельница коническая костная (conical bone mill)

CONICAL BONE MILL

D 6,5

189

REF

LOT

BMCON

1847160



DO NOT USE IF PACKAGE
IS DAMAGED



CE
3051

BIOMEC S.R.L.



CAUTIONS
Read instructions for use and file prosthesis system carefully.

ВИНТ ДЛЯ КОСТНОЙ МЕЛЬНИЦЫ INT (bone mill screw int)



GBMSINT



1847161



DO NOT USE IF PACKAGE
IS DAMAGED

IONS

Instructions for use and file prosthesis system carefully



BIOMECH S.R.L.
Via Nazionale Nord 21a

BONE MILL SCREW K1 REGULAR

191

REF

LOT



K1BMS



1847162



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis



BIOMECC S.R.L.

Via Nazionale Nord 21a

23823 Colico (LC)-ITALY

сверло калиброванное ogc k1 (calibrated drill ogs k1)

CALIBRATED DRILL OGS K1 REG. H 11,5

192

REF

LOT



K10GSR115



*1847103+



DO NOT USE IF PACKAGE
IS DAMAGED

CAUTIONS

Read instructions for use and file prosthesis system carefully



CE
3051



BIOMECH S.R.L.

Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



сверло кортикальное k1 ogs (countersink drill k1 ogs)

COUNTERSINK DRILL K1 OGS

193

CAUTIONS
Read instructions for use and file prosthesis system carefully




LOT

REF



DO NOT USE IF PACKAGE
IS DAMAGED

118+7164

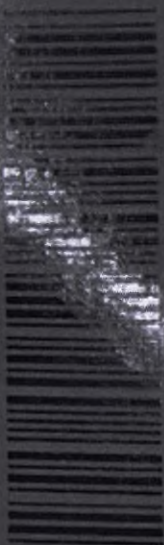

K1OGSCS



0051



BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



MAN. DRIVER CONVERTER 4X4

REF



SMRC8

LOT



1847155



DO NOT USE IF PACKAGE
IS DAMAGED


CAUTIONS

Read instructions for use and file prosthesis system carefully



CE

пин для фиксации мембраны (membrane fixing pin)

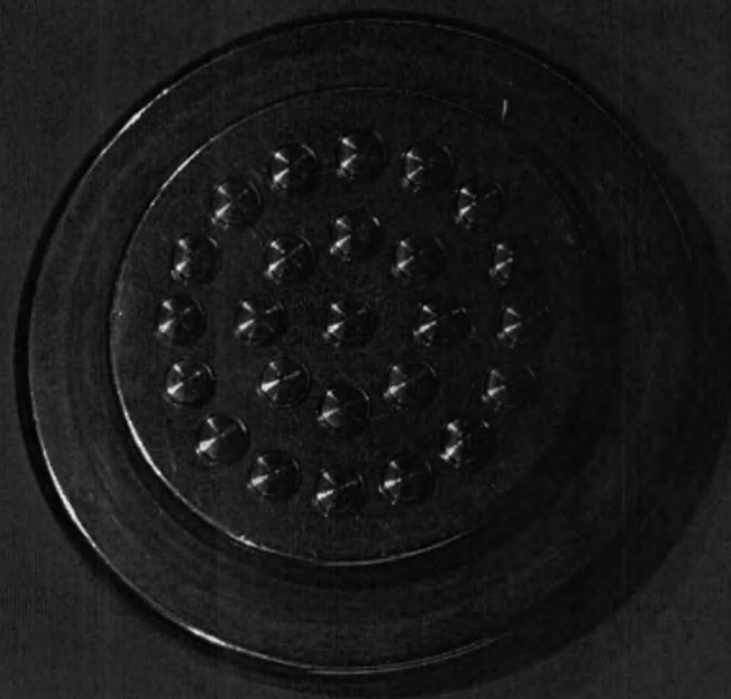

MEMBRANE FIXING
PIN H3

REF



P130-C

LOT



1847871



DO NOT USE IF PACKAGE
IS DAMAGED

STERILIZZARE
PRIMA DELL'USO

25 units

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully




0051


отвертка механическая для основания окси бас (mec. screwdriver for oxy bas) MESD




TROGSK1

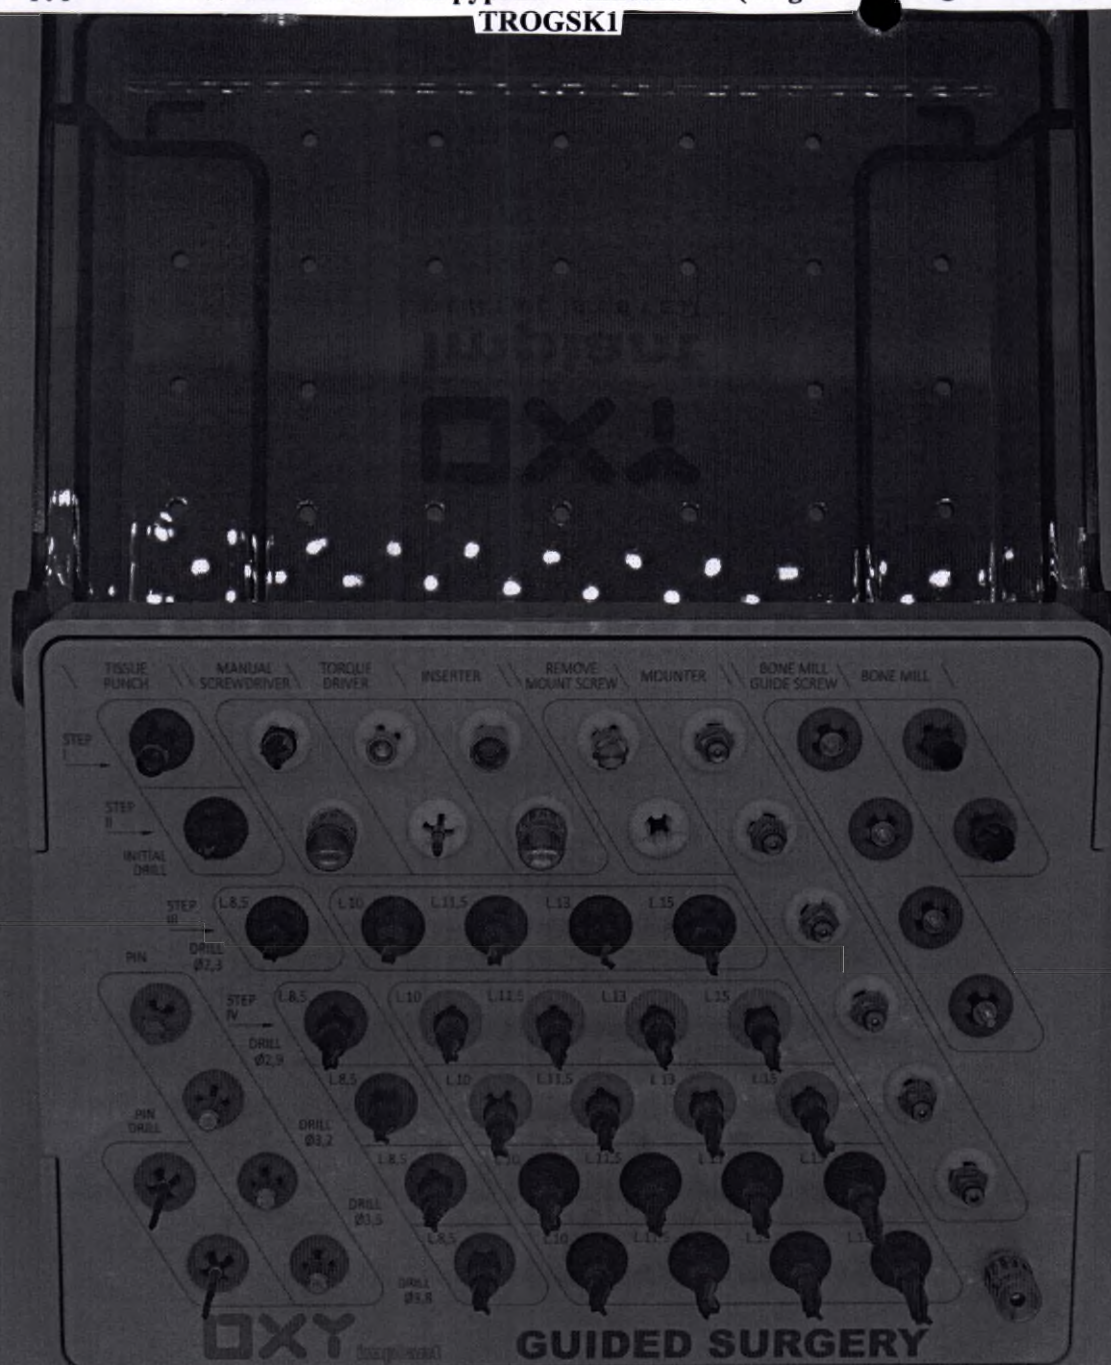


- комплект хирургический для шаблоновой хирургии - "nc" - "классик" (surgical kit for guided surgery - ps - classic) TRGUIDEPSILS

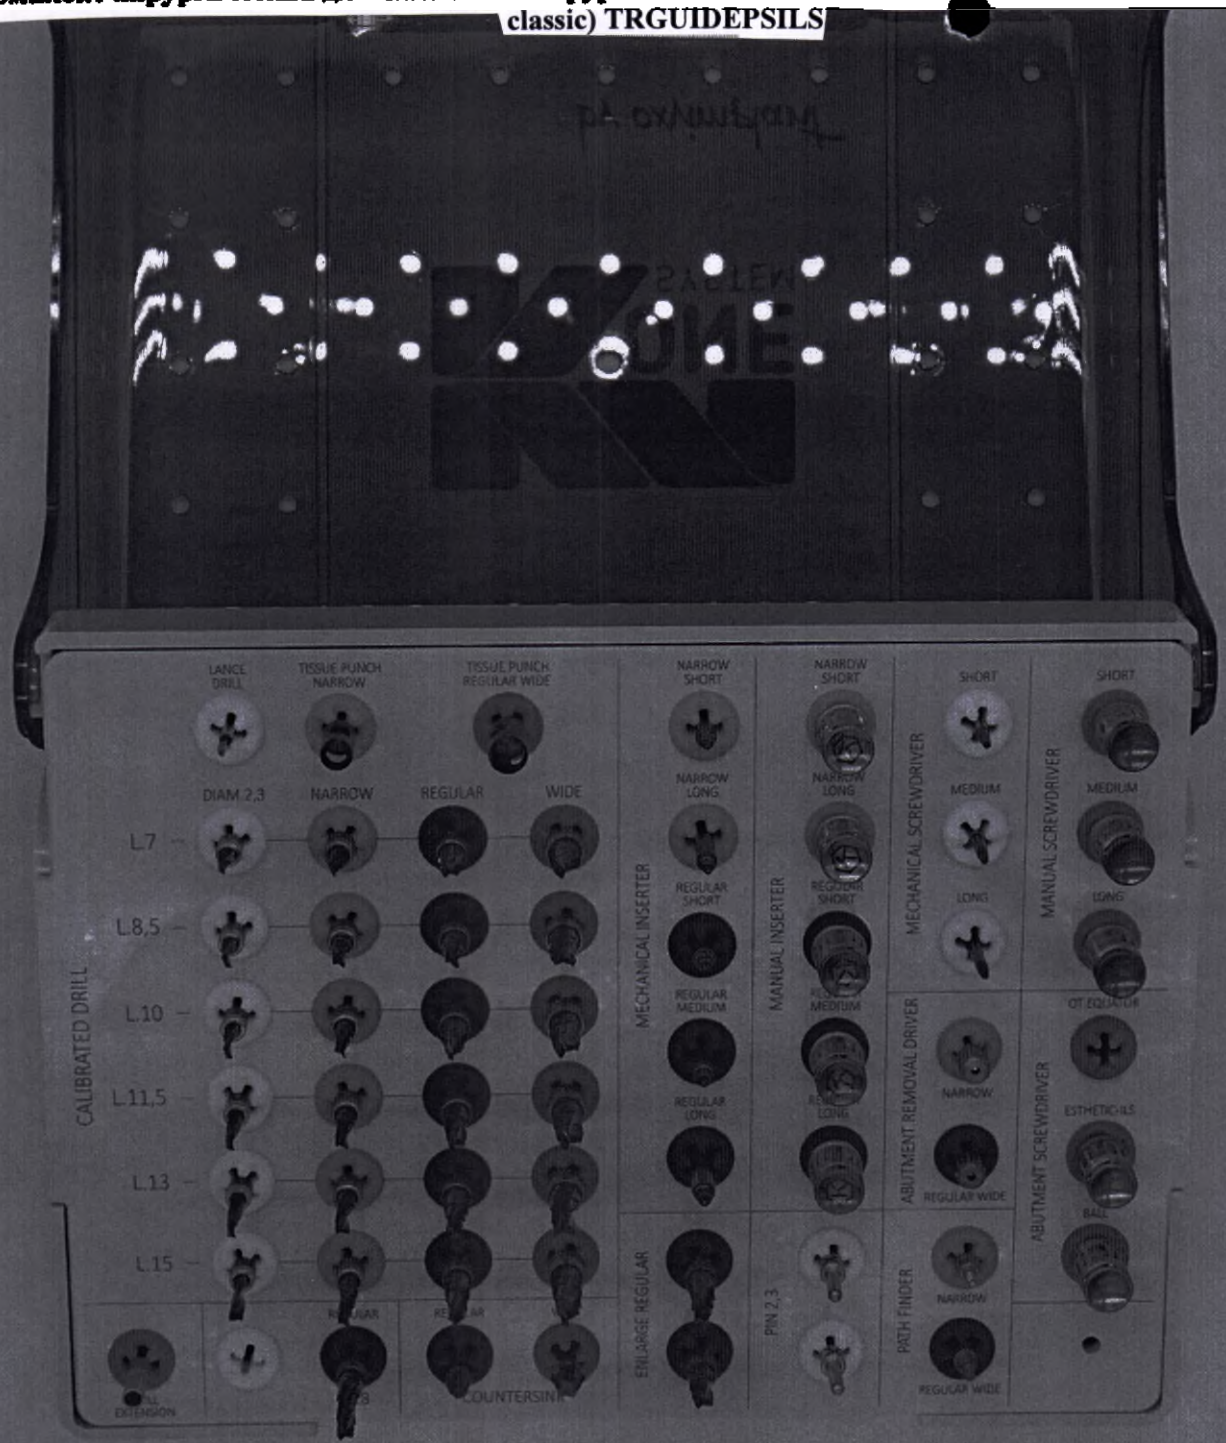




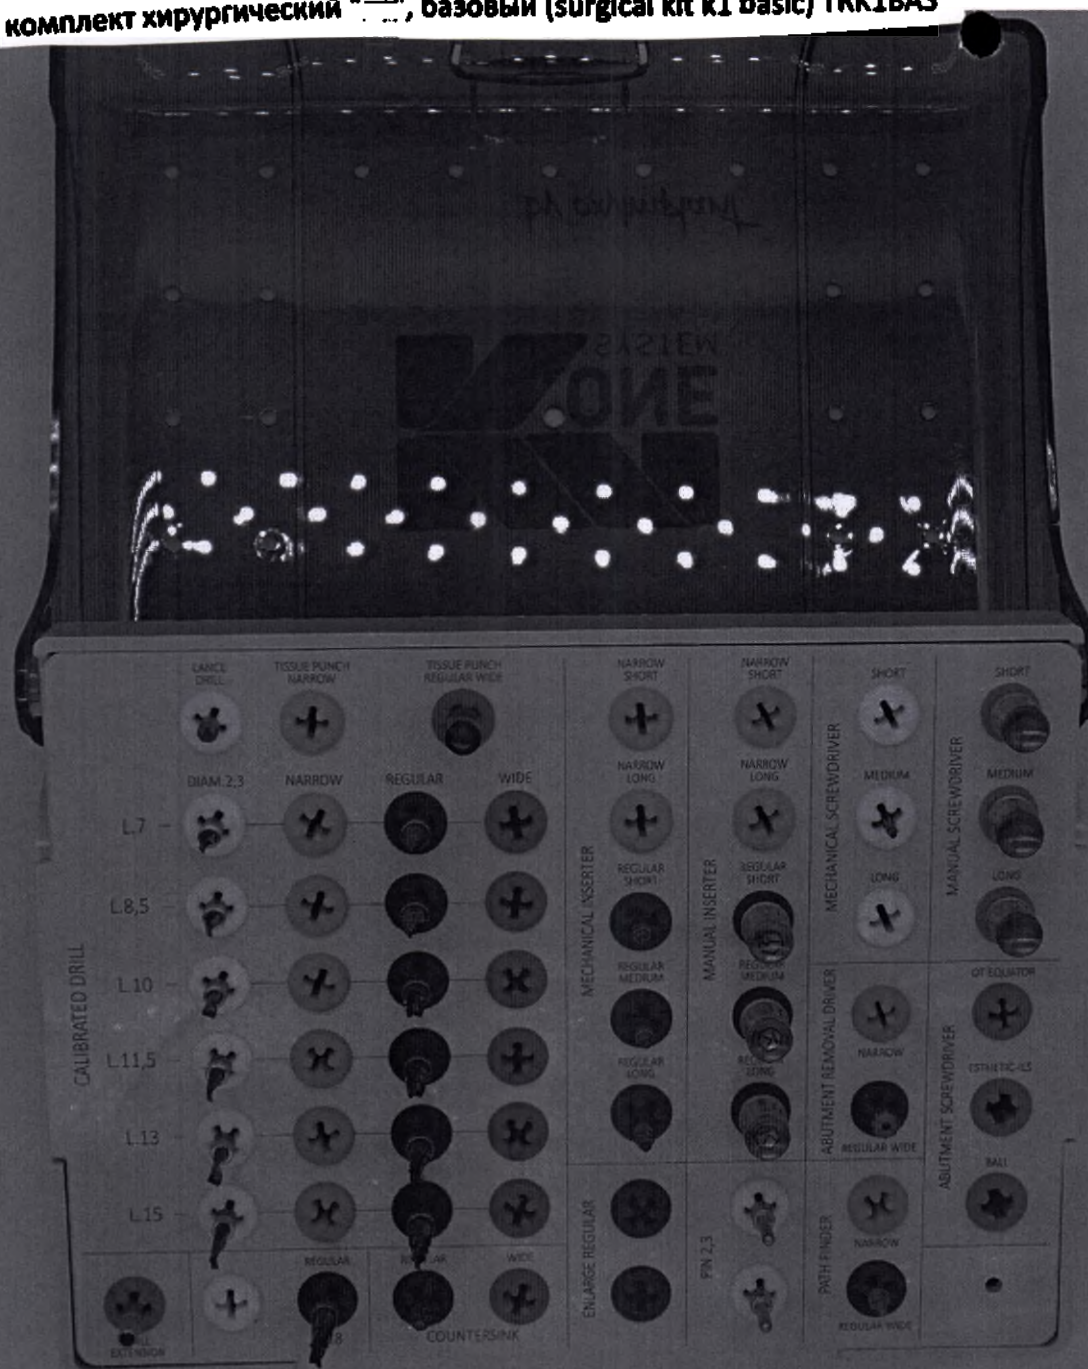

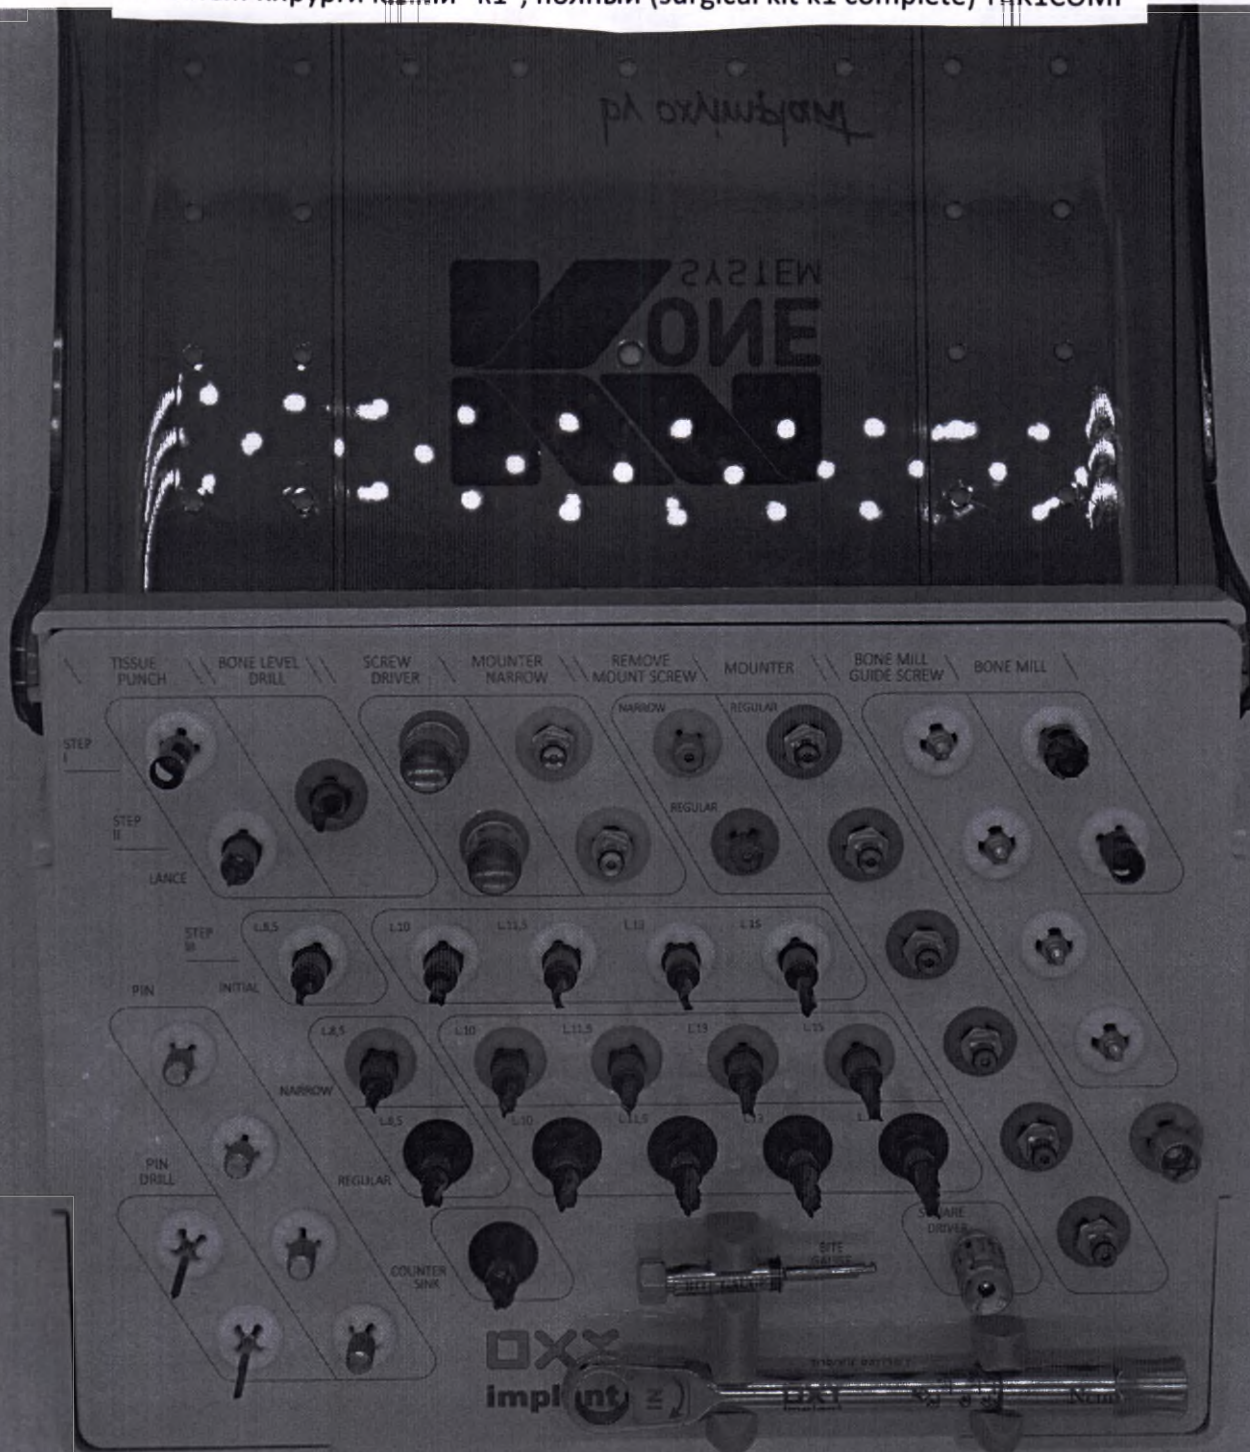

комплект хирургический "микро" (surgical kit micro) TRMICRO:

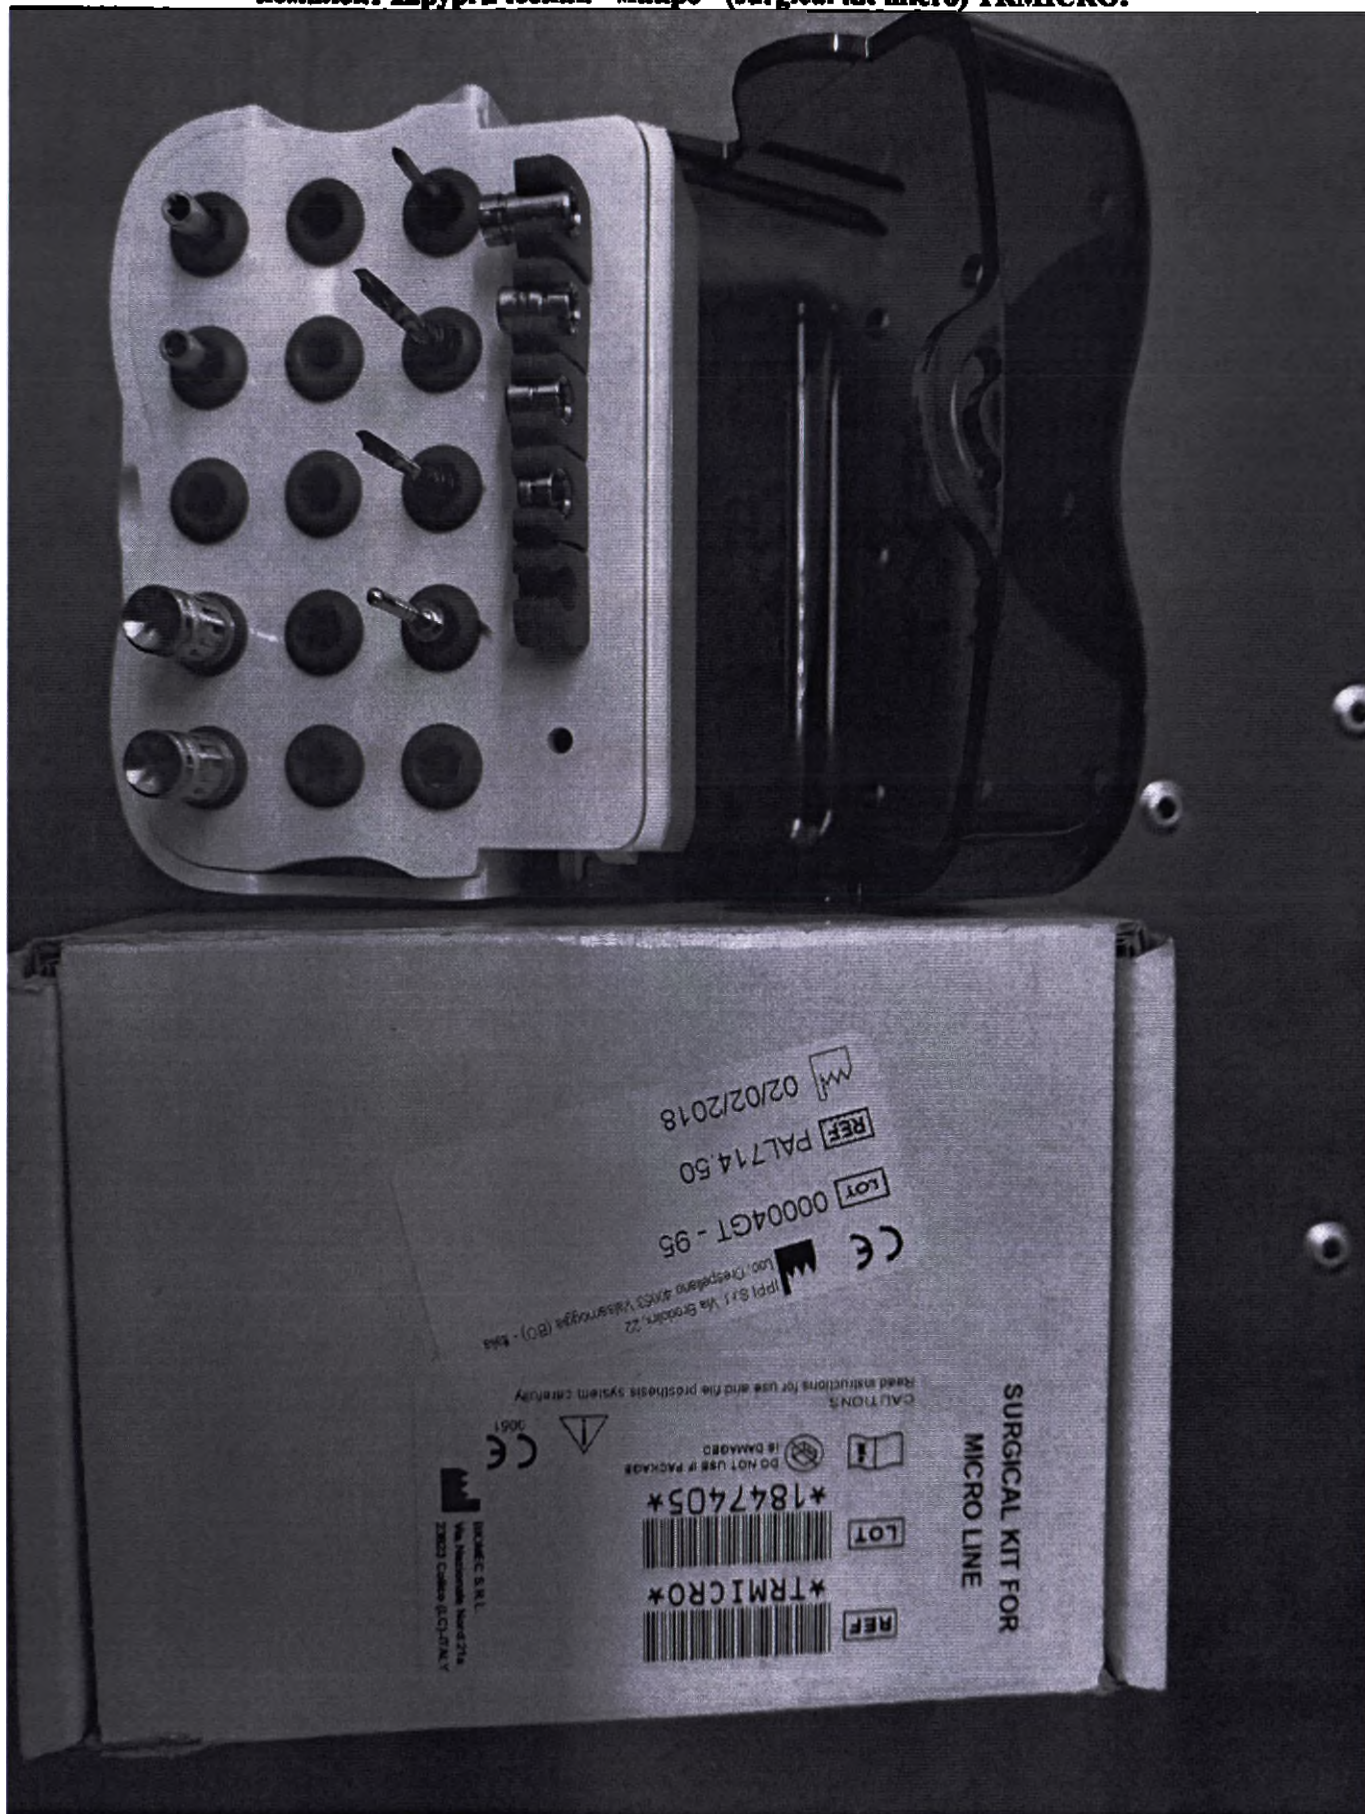

комплект хирургический "экстрашорт" (surgical kit extra short) TREXS:

SURGICAL KIT
EXTRA SHORT

REF



TREXS

LOT



1951807-5



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY



CAUTIONS

Read instructions for use and file prosthesis system carefully

200



- комплект хирургический для шаблонной хирургии - "пск" (surgical kit for guided surgery - psk)
TRGUIDEPSK:

SUGICAL KIT FOR
GUIDED SURGERY PSK

REF



TRGUIDEPSK

LOT



1850969-3



DO NOT USE IF PACKAGE
IS DAMAGED



CE
0051

BIOMEC S.R.L.
Via Nazionale Nord 21a
23823 Colico (LC)-ITALY

ATTENZIONE - CAUTIONS

Leggere attentamente le istruzioni d'uso e il protocollo implantoprotesico
Read instructions for use and file prosthesis system carefully



- комплект хирургический для ортопедии/протезирования (surgical kit prosthetic phase) TREIPROS:

**SURGICAL KIT
PROSTHETIC PHASE**

REF



TREIPROS

LOT



1851591-5



DO NOT USE IF PACKAGE
IS DAMAGED



CE
3051

BIOMECC S.R.L.
Via Nazionale Nord 21a
23023 Colico (LC)-ITALY

CAUTIONS

Read instructions for use and file prosthesis system carefully

CE
IPPI S.r.l. Via Brodolini, 22
Loc. Crespellano 40053 Valsamoggia (bo)
24GT-95

204





Пропіснн куновороно и шпроніста (ор)
дфкскініці
Ці
10.04.2020