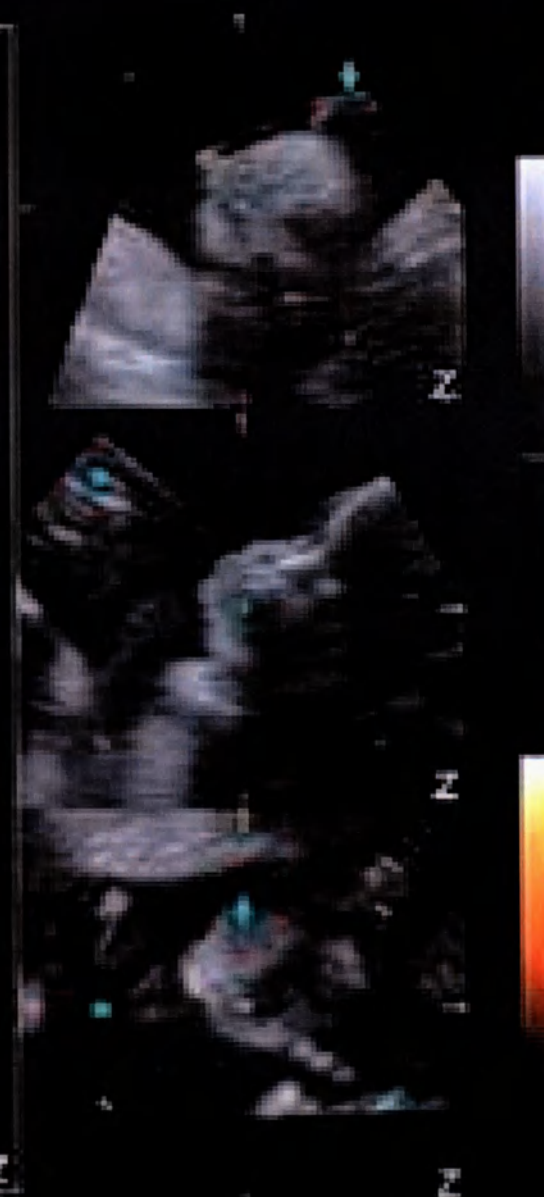



Фотографические изображения принадлежностей для медицинского изделия:
«Система ультразвуковая диагностическая ACUSON X600 с принадлежностями»

C6F2
C6
Surface
Opacity
Opacity 70
DR 35
Contrast 56
Brightness 54
Smooth 45
LowTh 66
Map A
Tint 50
1.7 vps



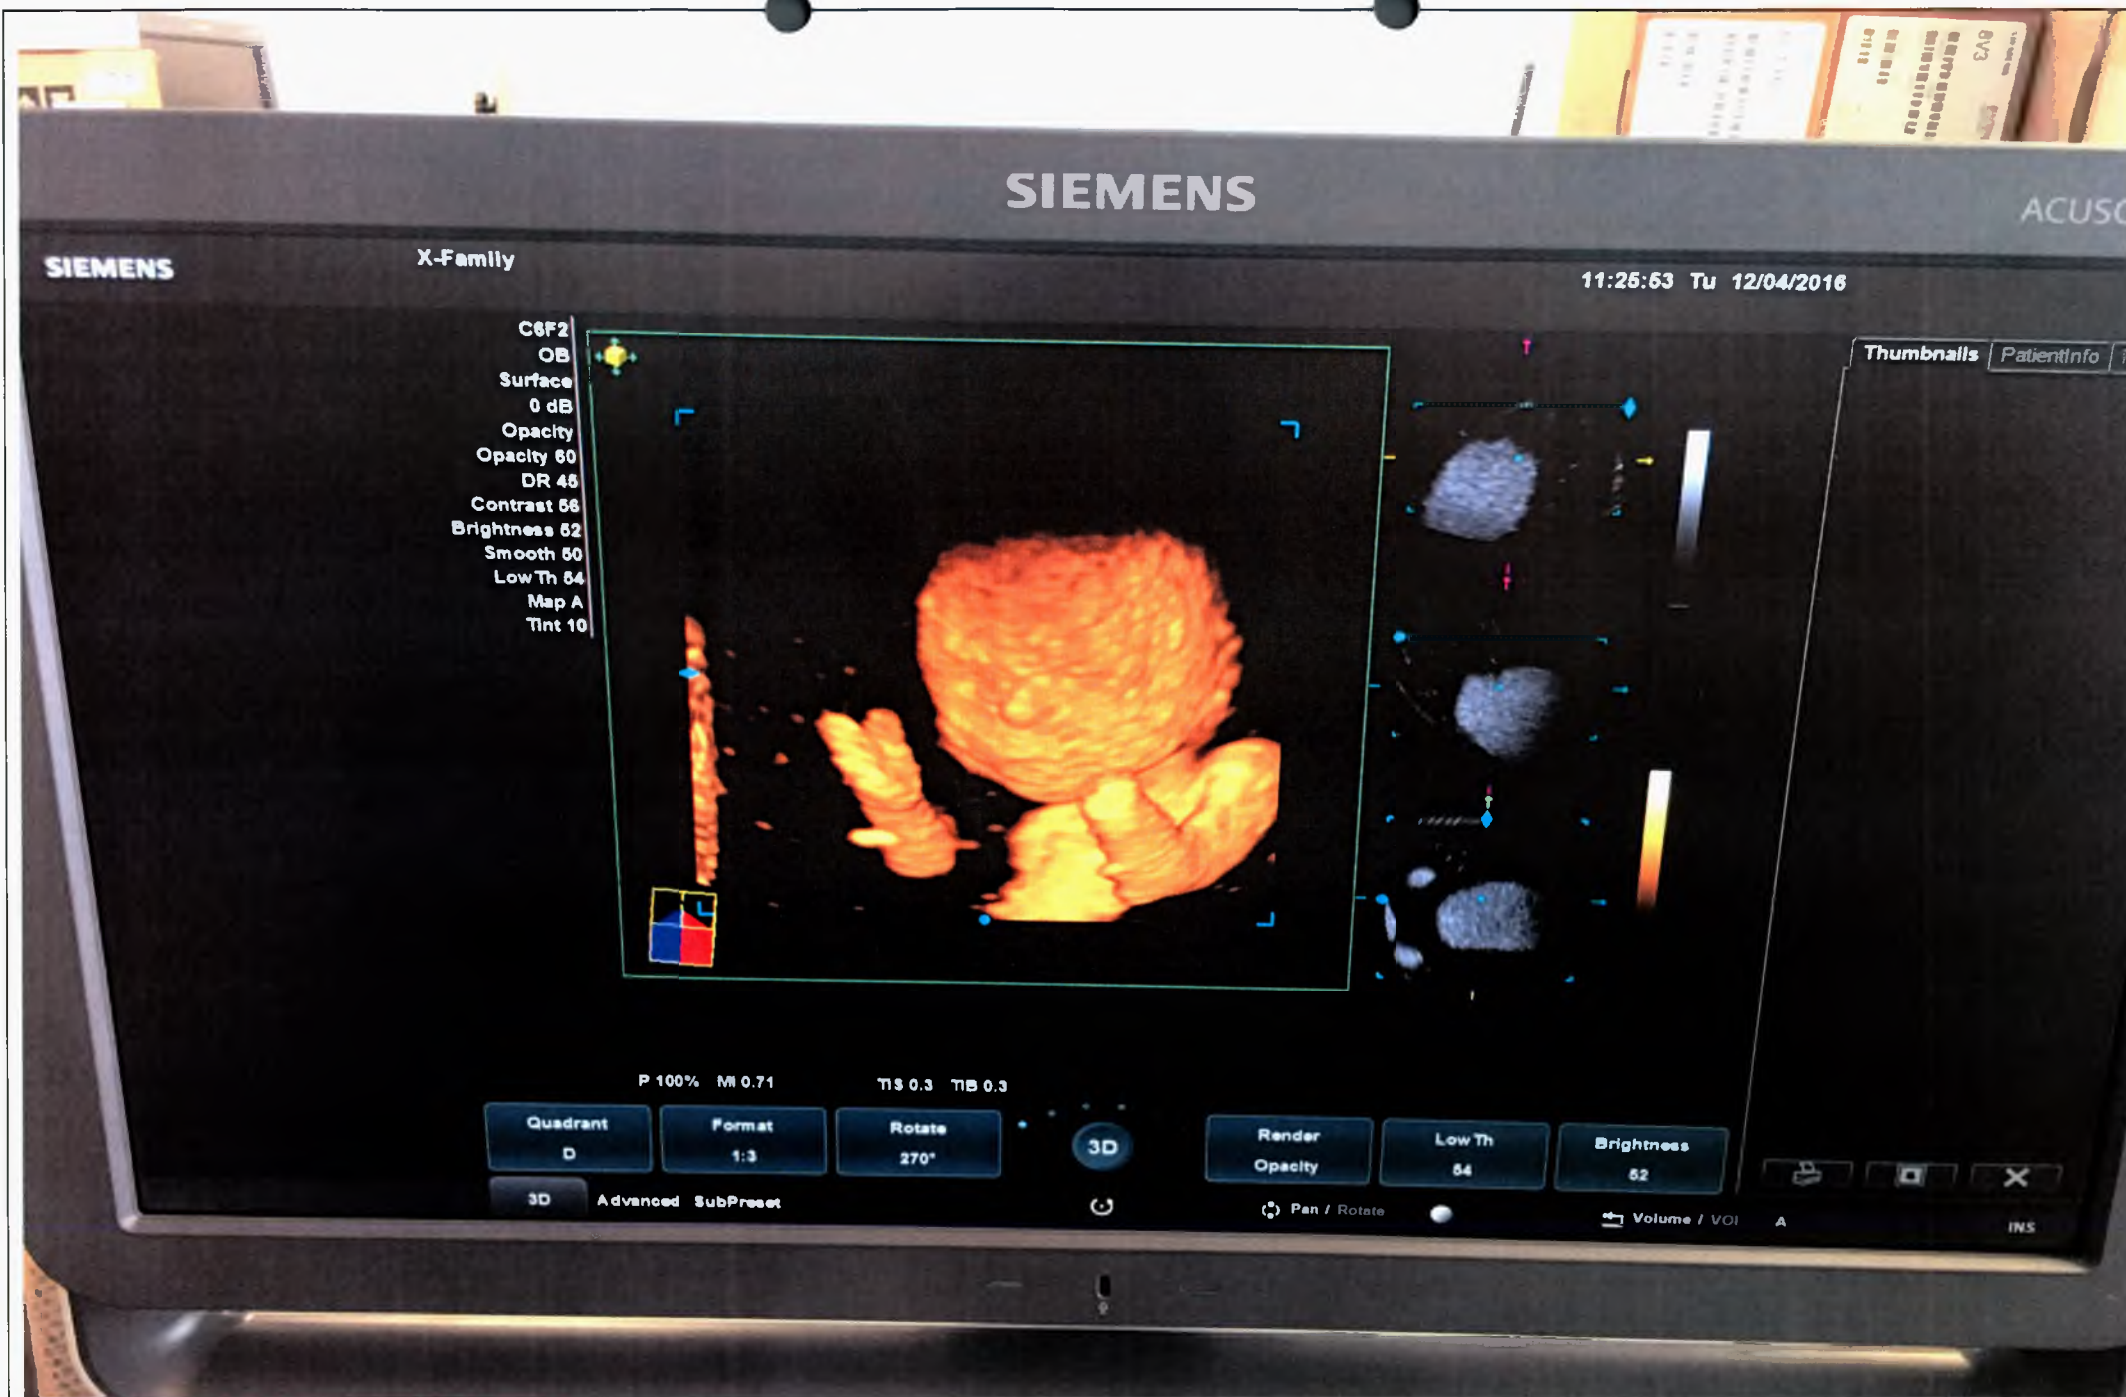


Рисунок 7. Лицензионный ключ для функции трехмерной визуализации
ООО ЦРМИ INFO@CIRMI.RU WWW.GOSZDRAVNADZOR.RU

Configuration

System Options

- Local Host

Site Info

System

Routing

Hardware

DNS

- Service

Mail

FTP

AutoTransfers

→ Licensing and Components

- Virus Protection

SolidCore

→ [License Details](#)

[Select New License File](#)

Available Features


Feature	Version	Expire Date	Required	Status
fourSight_4D_imaging_X600	1.0	permanent	no	available
Advanced_fourSight_X600	1.0	permanent	no	available
US_System_License_X600	1.0	permanent	no	available
SyngoLite_US_X600	1.0	permanent	no	available
US_Stress_Echo_X600	1.0	15-jun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

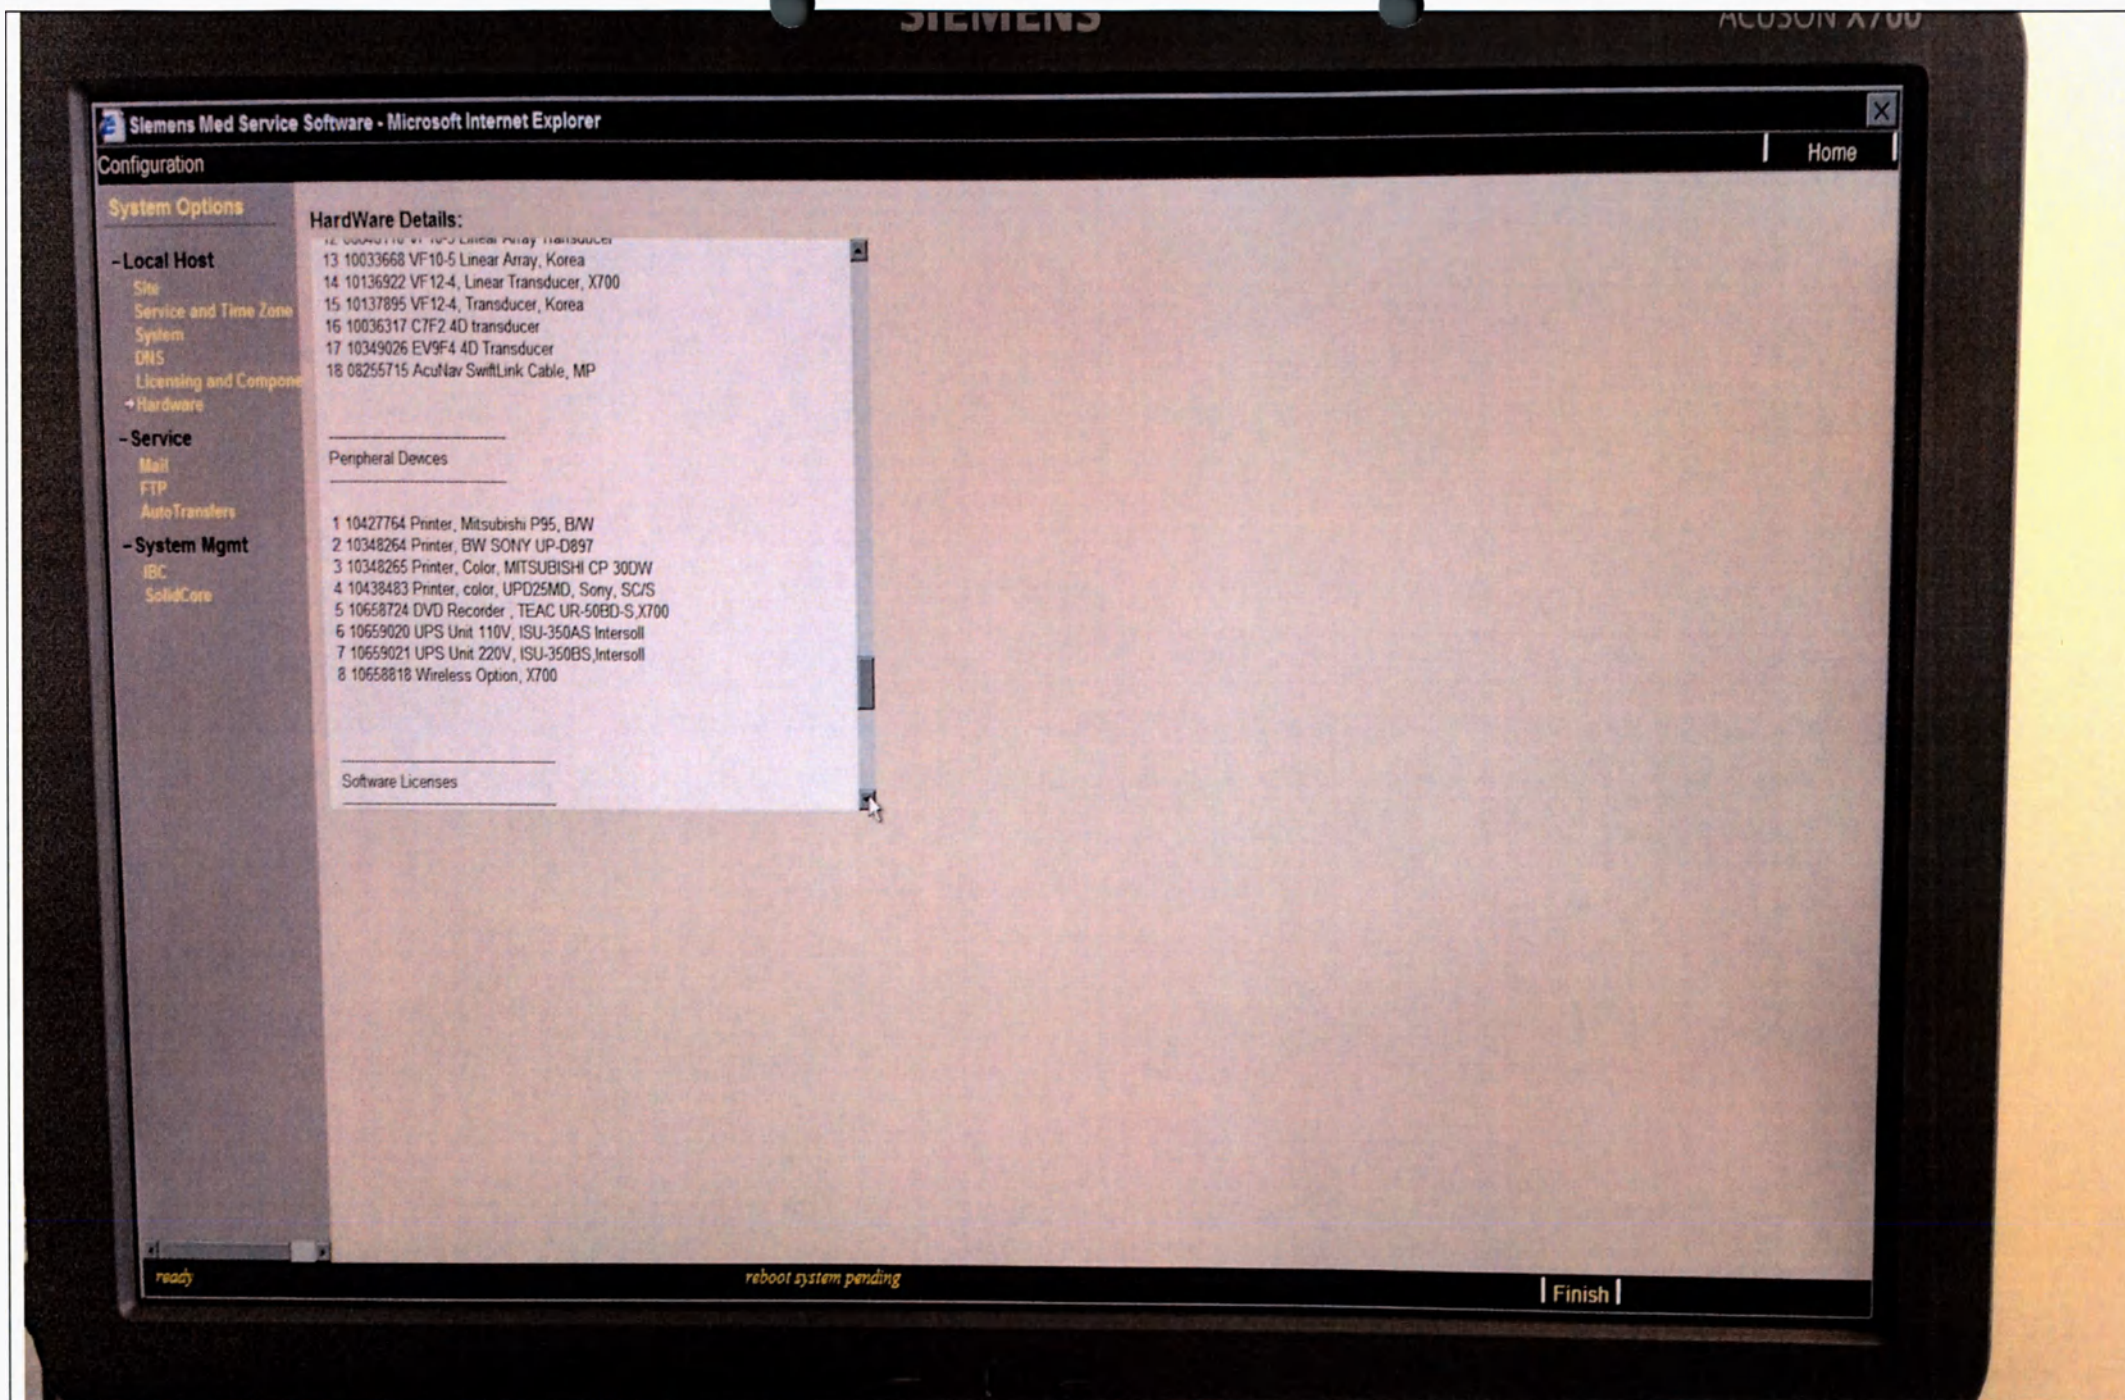



Presets

- General 1
- General 2
- Peripheral
- Customize Keys
- Display
- Exam Configuration
- User-Defined Exam List
- Text Annotation
- Pictogram List
- M & R Configuration
- Summary
- Service
- Stress Echo
- SieScape
- CAI
- Wireless
- DICOM**
- DIMAQ Utility
- Clip Capture
- Network Export
- Authorization
- Archive
- Printer

DICOM

Local Host | Storage Server | Worklist Server | MPPS Server | B/W Printer | Color Printer | Query/Retrieve |

Local Host

☒ Show network status

Alias:

Default

☒ Default

AE Title:

Default

Host Name:

Default

MAC Address:

00-19-0F-23-2C-DE

New

Edit

Delete

☐ DHCP☐ Mapping Application☒ Fixed IP address

IP Address:

192

168

0

1

Subnet Mask:

255

255

255

0

Default Gateway:

0

0

0

0

Media Type

HardwareDefault

Duplex Mode

HardwareDefault

Save

Cancel

Configuration

System Options

- Local Host

Site Info

System

Routing

Hardware

DNS

- Service

Mail

FTP

AutoTransfers

→ Licensing and Components

- Virus Protection

SolidCore

→ License Details

Select New License File

Available Features

Feature	Version	Expire Date	Required	Status
DICOM_SR_Vascular_X600	1.0	permanent	no	available
US_DICOM_SR_Card_X600	1.0	permanent	no	available
US_Freehand_3D_X600	1.0	permanent	no	available
DICOM_SR_OB_GYN_X600	1.0	permanent	no	available
fourSight_4D_Imaging_X600	1.0	permanent	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

Configuration

System Options

- Local Host

Site Info

System

Routing

Hardware

DNS

- Service

Mail

FTP

AutoTransfers

➔ **Licensing and Components**

- Virus Protection

SolidCore

➔ License Details

Select New License File

Available Features

Feature	Version	Expire Date	Required	Status
DICOM_SR_Vascular_X600	1.0	permanent	no	available
US_DICOM_SR_Card_X600	1.0	permanent	no	available
US_Freehand_3D_X600	1.0	permanent	no	available
DICOM_SR_OB_GYN_X600	1.0	permanent	no	available
fourSight_4D_Imaging_X600	1.0	permanent	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

Configuration

System Options

- Local Host

Site Info

System

Routing

Hardware

DNS

- Service

Mail

FTP

AutoTransfers

→ Licensing and Components

- Virus Protection

SolidCore

→ License Details

Select New License File

Available Features

Feature	Version	Expire Date	Required	Status
DICOM_SR_Vascular_X600	1.0	permanent	no	available
US_DICOM_SR_Card_X600	1.0	permanent	no	available
US_Freehand_3D_X600	1.0	permanent	no	available
DICOM_SR_OB_GYN_X600	1.0	permanent	no	available
fourSight_4D_Imaging_X600	1.0	permanent	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

Configuration

System Options

- Local Host

Site Info

System

Routing

Hardware

DNS

- Service

Mail

FTP

AutoTransfers

⇒ Licensing and Components

- Virus Protection

SolidCore

⇒ License Details

[Select New License File](#)

Available Features

Feature	Version	Expire Date	Required	Status
AXIUS_EF_X600	1.0	15-jun-2016	no	available
CLARIFY_VE_X600	1.0	15-jun-2016	no	available
ARTERIAL_HEALTH_PACKAGE_X600	1.0	15-jun-2016	no	available
US_ALH_X600	1.0	15-jun-2016	no	available
US_Syngo Auto OB X600	1.0	15-jun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

Configuration

System Options

- Local Host

Site Info
System
Routing
Hardware
DNS

- Service

Mail
FTP
AutoTransfers

➔ Licensing and Components

- Virus Protection

SolidCore

➔ License Details

Select New License File

Available Features

Feature	Version	Expire Date	Required	Status
US_ALH_X600	1.0	15-jun-2016	no	available
US_Syngo_Auto_OB_X600	1.0	15-jun-2016	no	available
Contrast_Agent_Image_X600	1.0	15-jun-2016	no	available
US_Security_VP_X600	1.0	15-jun-2016	no	available
US_SieScape_X600	1.0	15-jun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

Configuration

System Options

-Local Host

Site Info
System
Routing
Hardware
DNS

-Service

Mail
FTP
AutoTransfers

→ Licensing and Components

-Virus Protection

SolidCore

→ License Details

[Select New License File](#)

Available Features

Feature	Version	Expire Date	Required	Status
US_ALH_X600	1.0	15-jun-2016	no	available
US_Syngo_Auto_OB_X600	1.0	15-jun-2016	no	available
Contrast_Agent_Image_X600	1.0	15-jun-2016	no	available
US_Security_VP_X600	1.0	15-jun-2016	no	available
US_SieScape_X600	1.0	15-jun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

Configuration

System Options

-Local Host

Site Info
System
Routing
Hardware
DNS

-Service

Mail
FTP
AutoTransfers

➔ Licensing and Components

-Virus Protection

SolidCore

➔ License Details

[Select New License File](#)

Available Features

Feature	Version	Expire Date	Required	Status
US_ALH_X600	1.0	15-jun-2016	no	available
US_Syngo_Auto_OB_X600	1.0	15-jun-2016	no	available
Contrast_Agent_Image_X600	1.0	15-jun-2016	no	available
US_Security_VP_X600	1.0	15-jun-2016	no	available
US_SieScape_X600	1.0	15-jun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\License.dat"

Рисунок 18. Лицензионный ключ для функции автоматического акушерского исследования

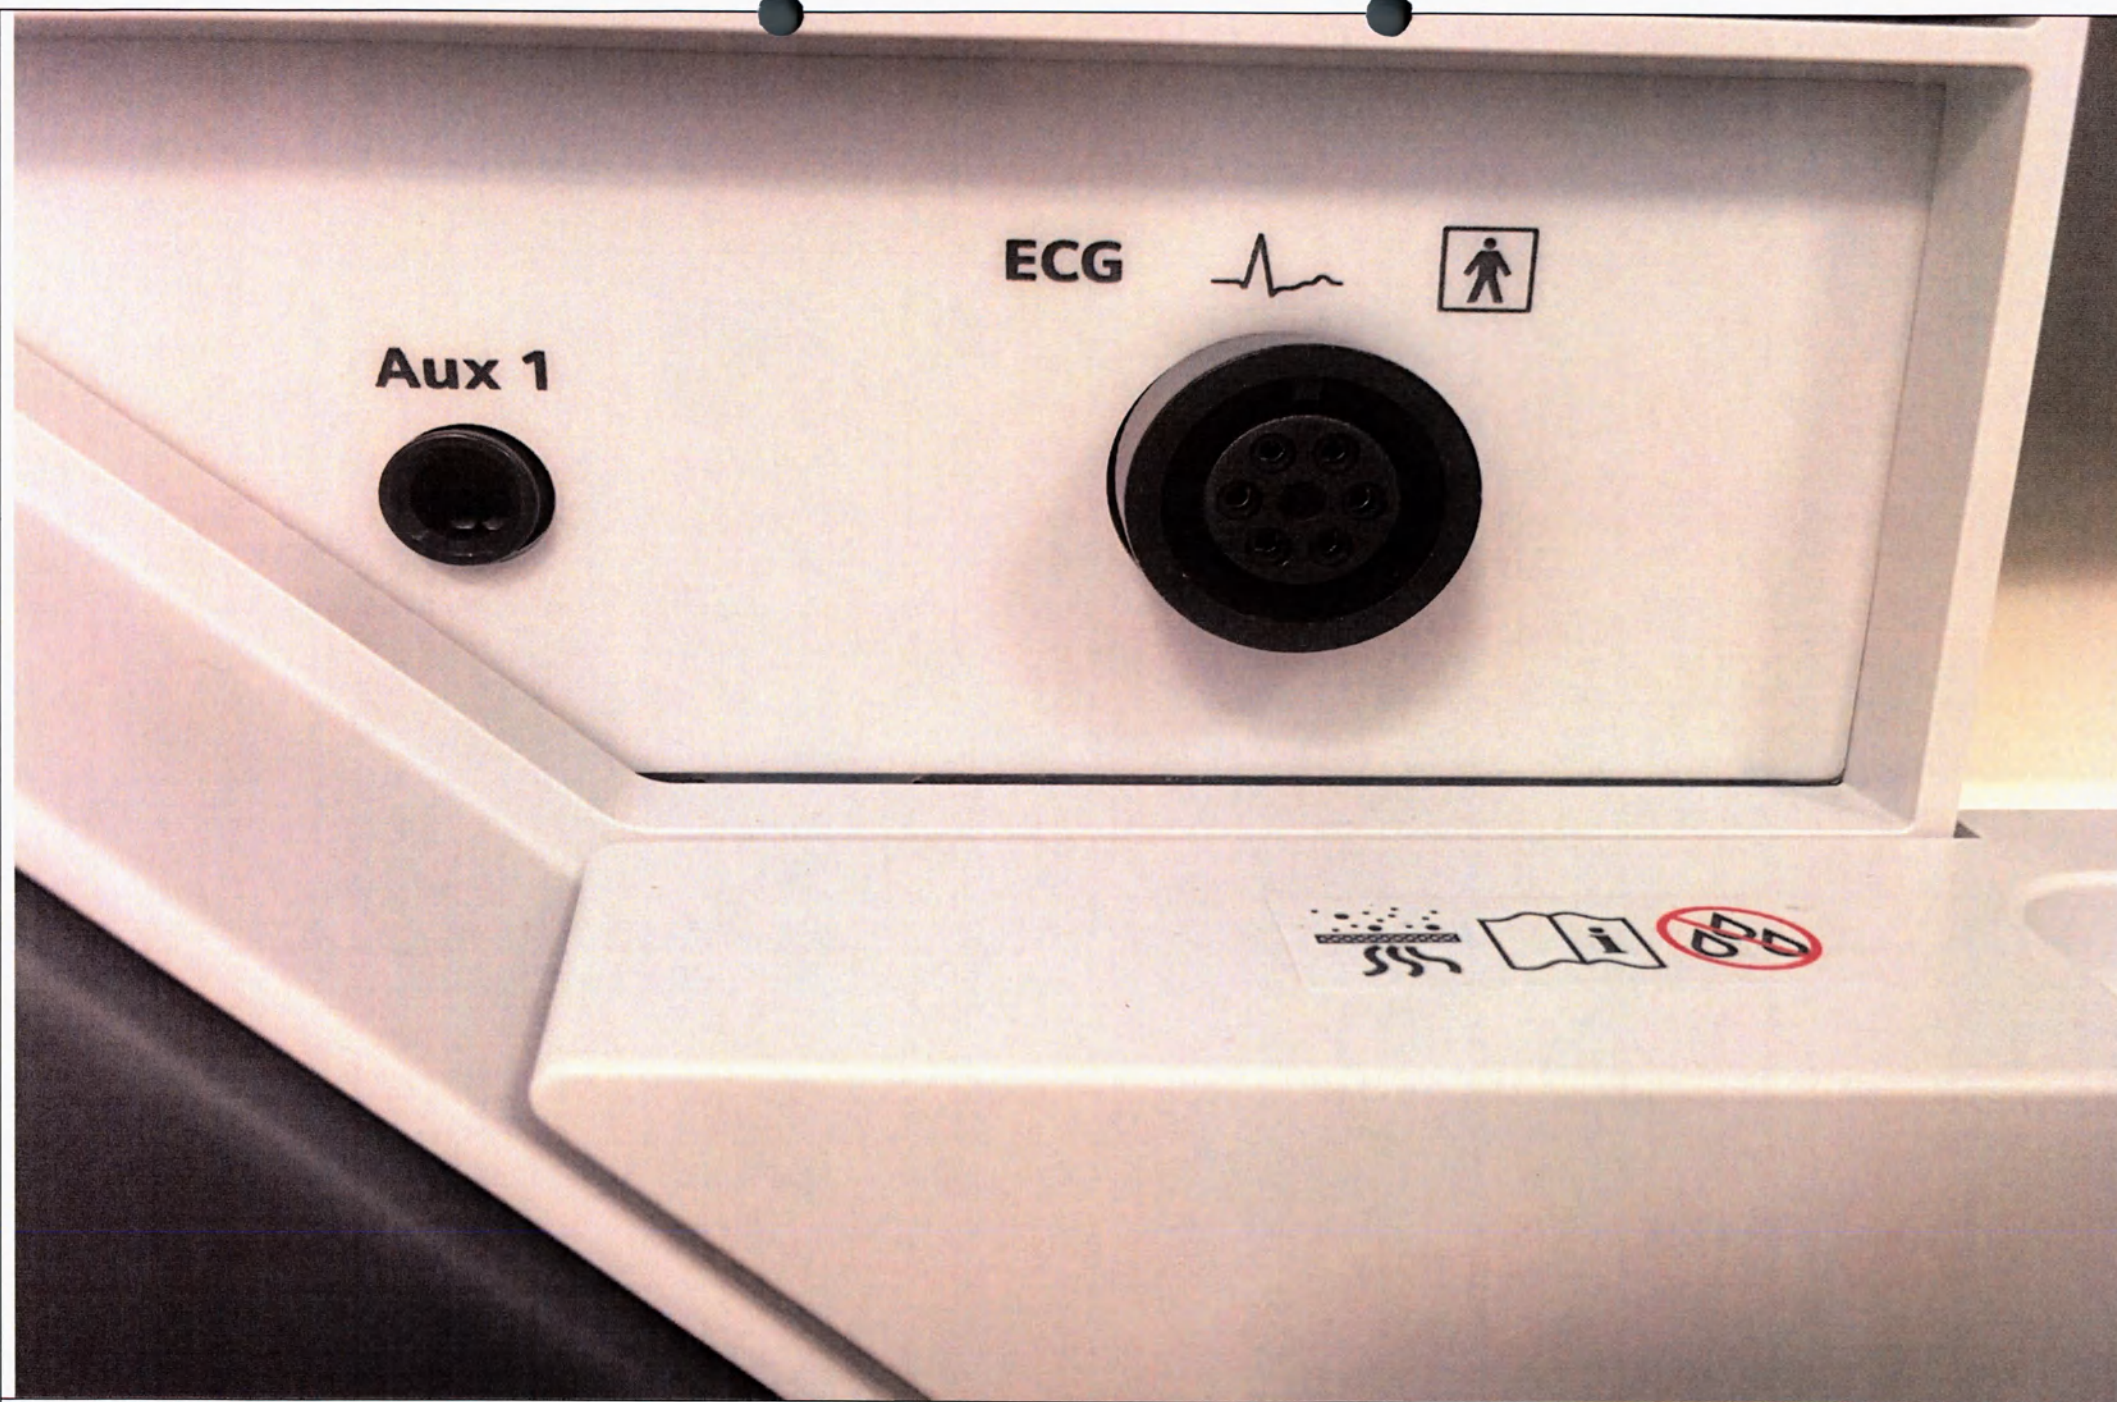


Рисунок 19. Модуль физиологический для синхронизации с ЭКГ





Рисунок 20. Модуль для сердечно - сосудистых исследований


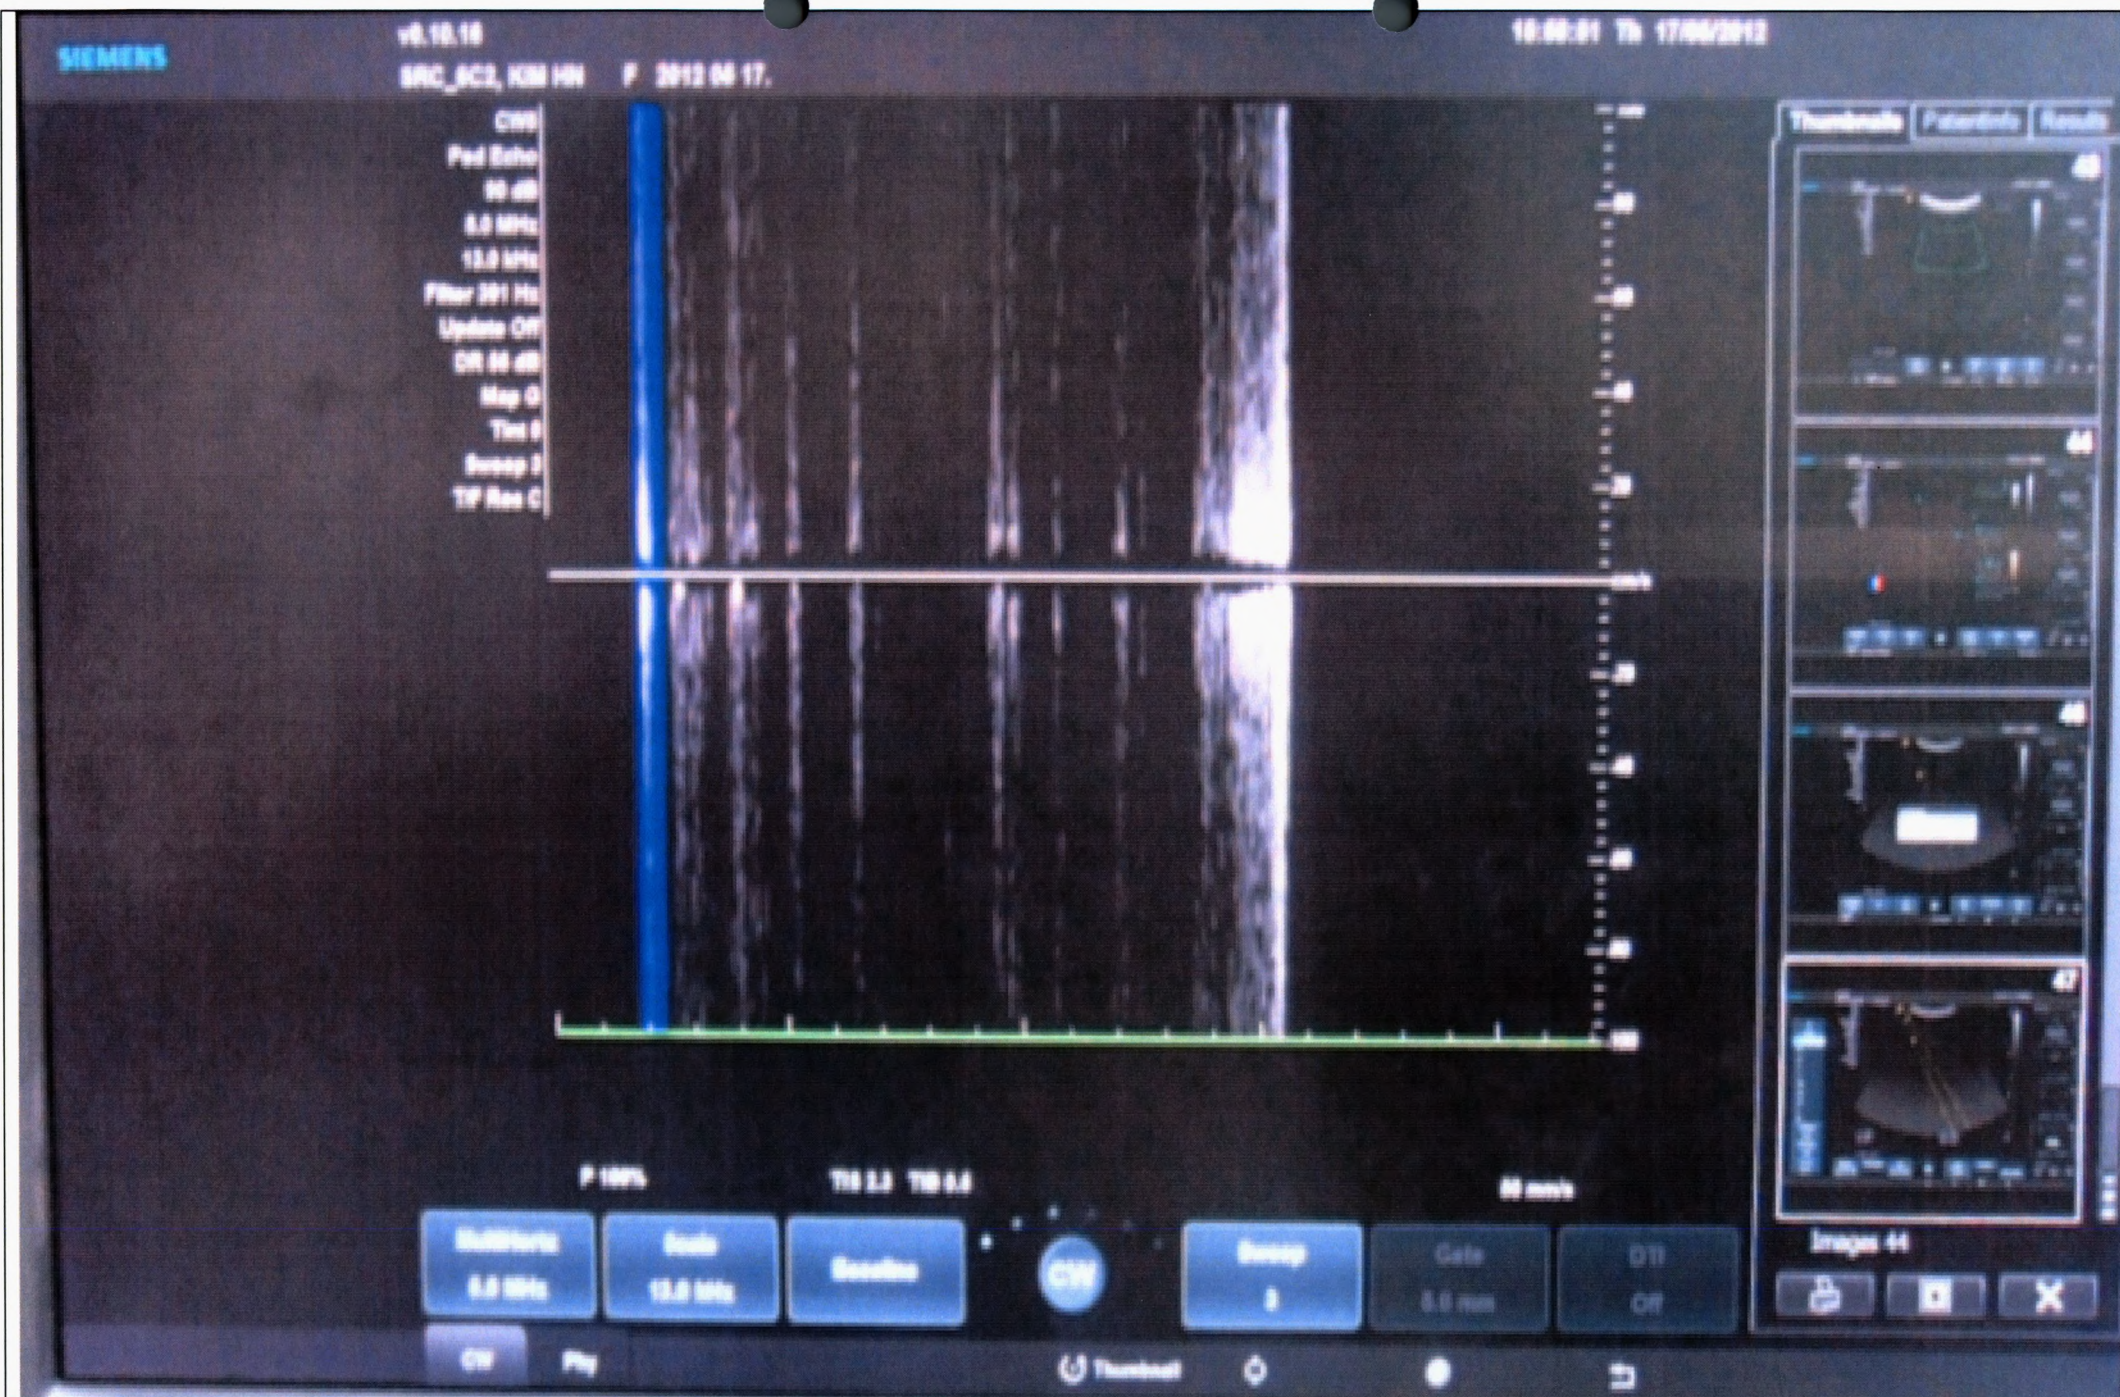


Рисунок 21. Лицензионный ключ для функции постоянно - волнового доплера

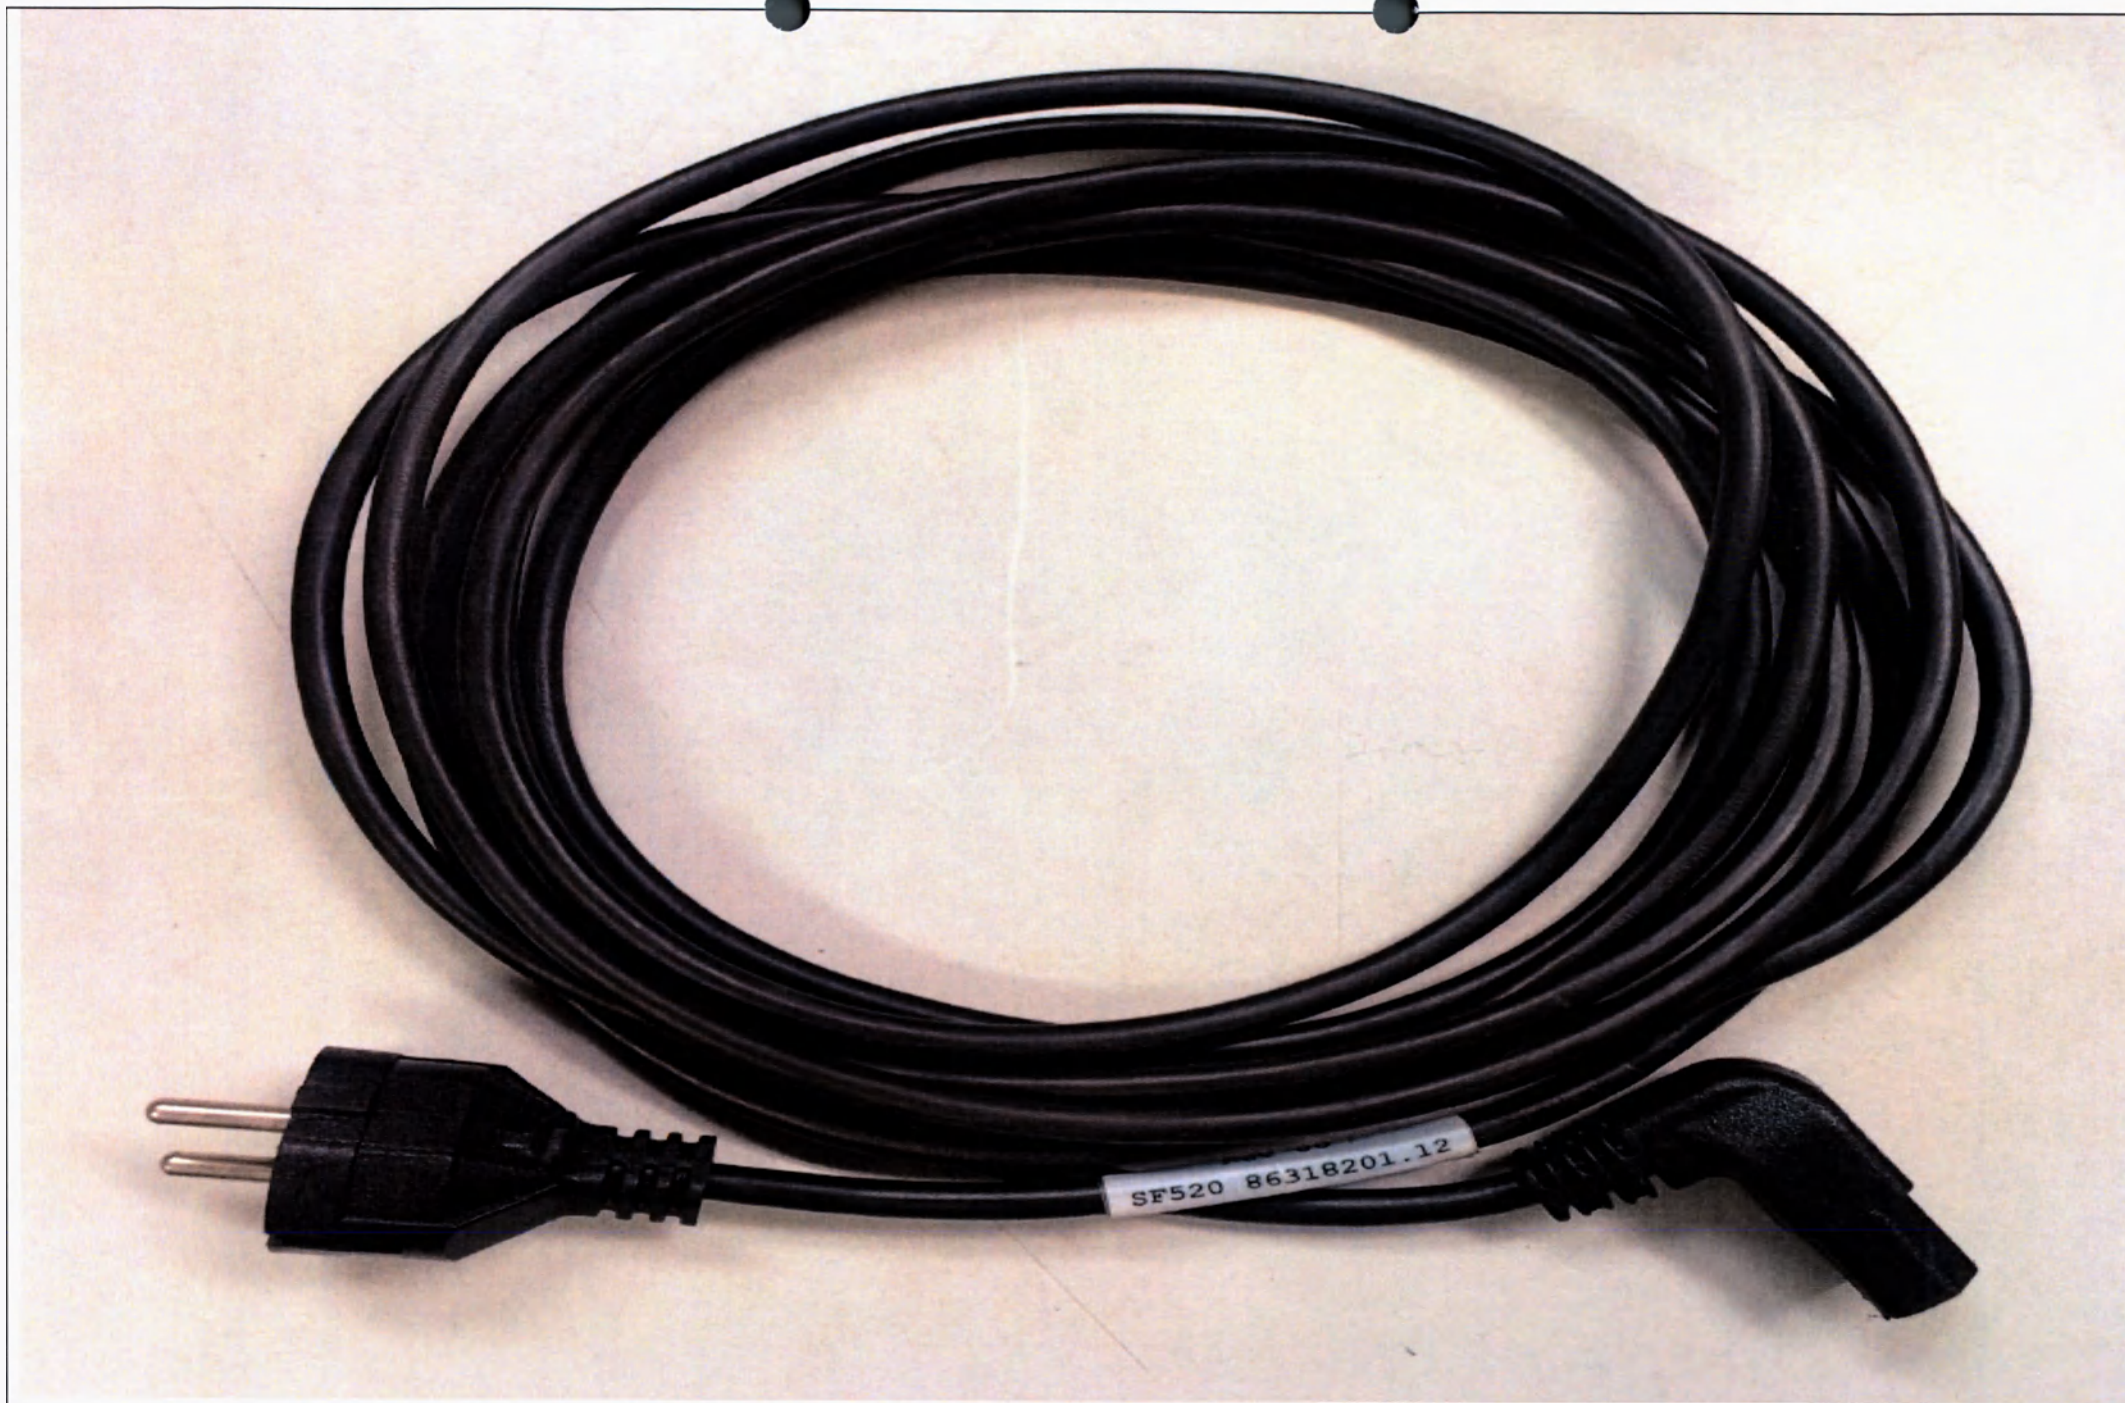

Configuration

System Options

- Local Host

Site Info

System

Routing

Hardware

DNS

- Service

Mail

FTP

AutoTransfers

⇒ Licensing and Components

- Virus Protection

SolidCore

⇒ License Details

[Select New License File](#)

Available Features


Feature	Version	Expire Date	Required	Status
AXIUS_EF_X600	1.0	15-jun-2016	no	available
CLARIFY_VE_X600	1.0	15-jun-2016	no	available
ARTERIAL_HEALTH_PACKAGE_X600	1.0	15-jun-2016	no	available
US_ALH_X600	1.0	15-jun-2016	no	available
US Syngo Auto OB X600	1.0	15-iun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

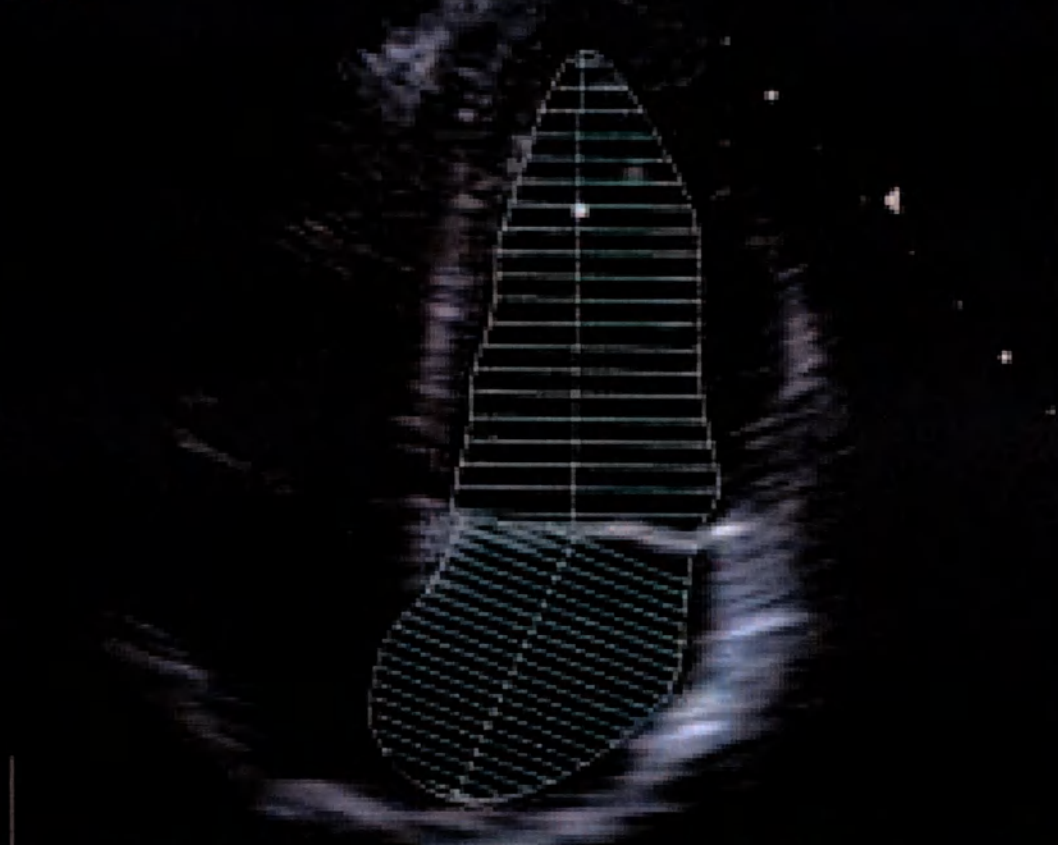4
ED
A4C13
ES

	EF%	EDV (ml)	ESV (ml)	HR (bpm)
LV	58	94.0	39.3	78
LA	73	8.7	32.0	

Cycle: ◀ 2 ▶

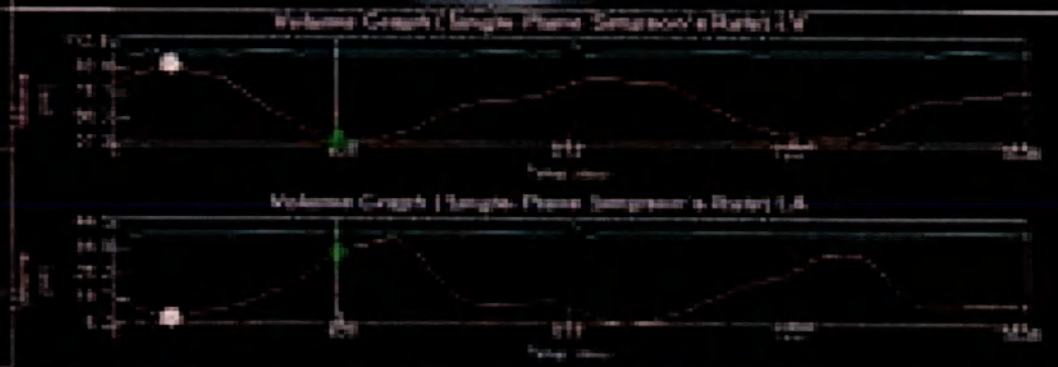


Рисунок 24. Лицензионный ключ для опции автоматического исследования левых отделов сердца

Configuration

System Options

- Local Host

Site Info
System
Routing
Hardware
DNS

- Service

Mail
FTP
AutoTransfers
→ Licensing and Components

- Virus Protection

SolidCore

↪ License Details

Select New License File

Available Features

Feature	Version	Expire Date	Required	Status
fourSight_4D_Imaging_X600	1.0	permanent	no	available
Advanced_fourSight_X600	1.0	permanent	no	available
US_System_License_X600	1.0	permanent	no	available
SyngoLite_US_X600	1.0	permanent	no	available
US_Stress_Echo_X600	1.0	15-jun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

Configuration

System Options

-Local Host

Site Info
System
Routing
Hardware
DNS

-Service

Mail
FTP

AutoTransfers

➔ Licensing and Components

-Virus Protection

SolidCore

➔ License Details

[Select New License File](#)

Available Features


Feature	Version	Expire Date	Required	Status
AXIUS_EF_X600	1.0	15-jun-2016	no	available
CLARIFY_VE_X600	1.0	15-jun-2016	no	available
ARTERIAL_HEALTH_PACKAGE_X600	1.0	15-jun-2016	no	available
US_ALH_X600	1.0	15-jun-2016	no	available
US_Syngo_Auto_OB_X600	1.0	15-jun-2016	no	available

Feature Details

Features with errors: 0

Missing required features: 0

LM_LICENSE_FILE = C:\syngo_lite\config\Licensing\license.dat"

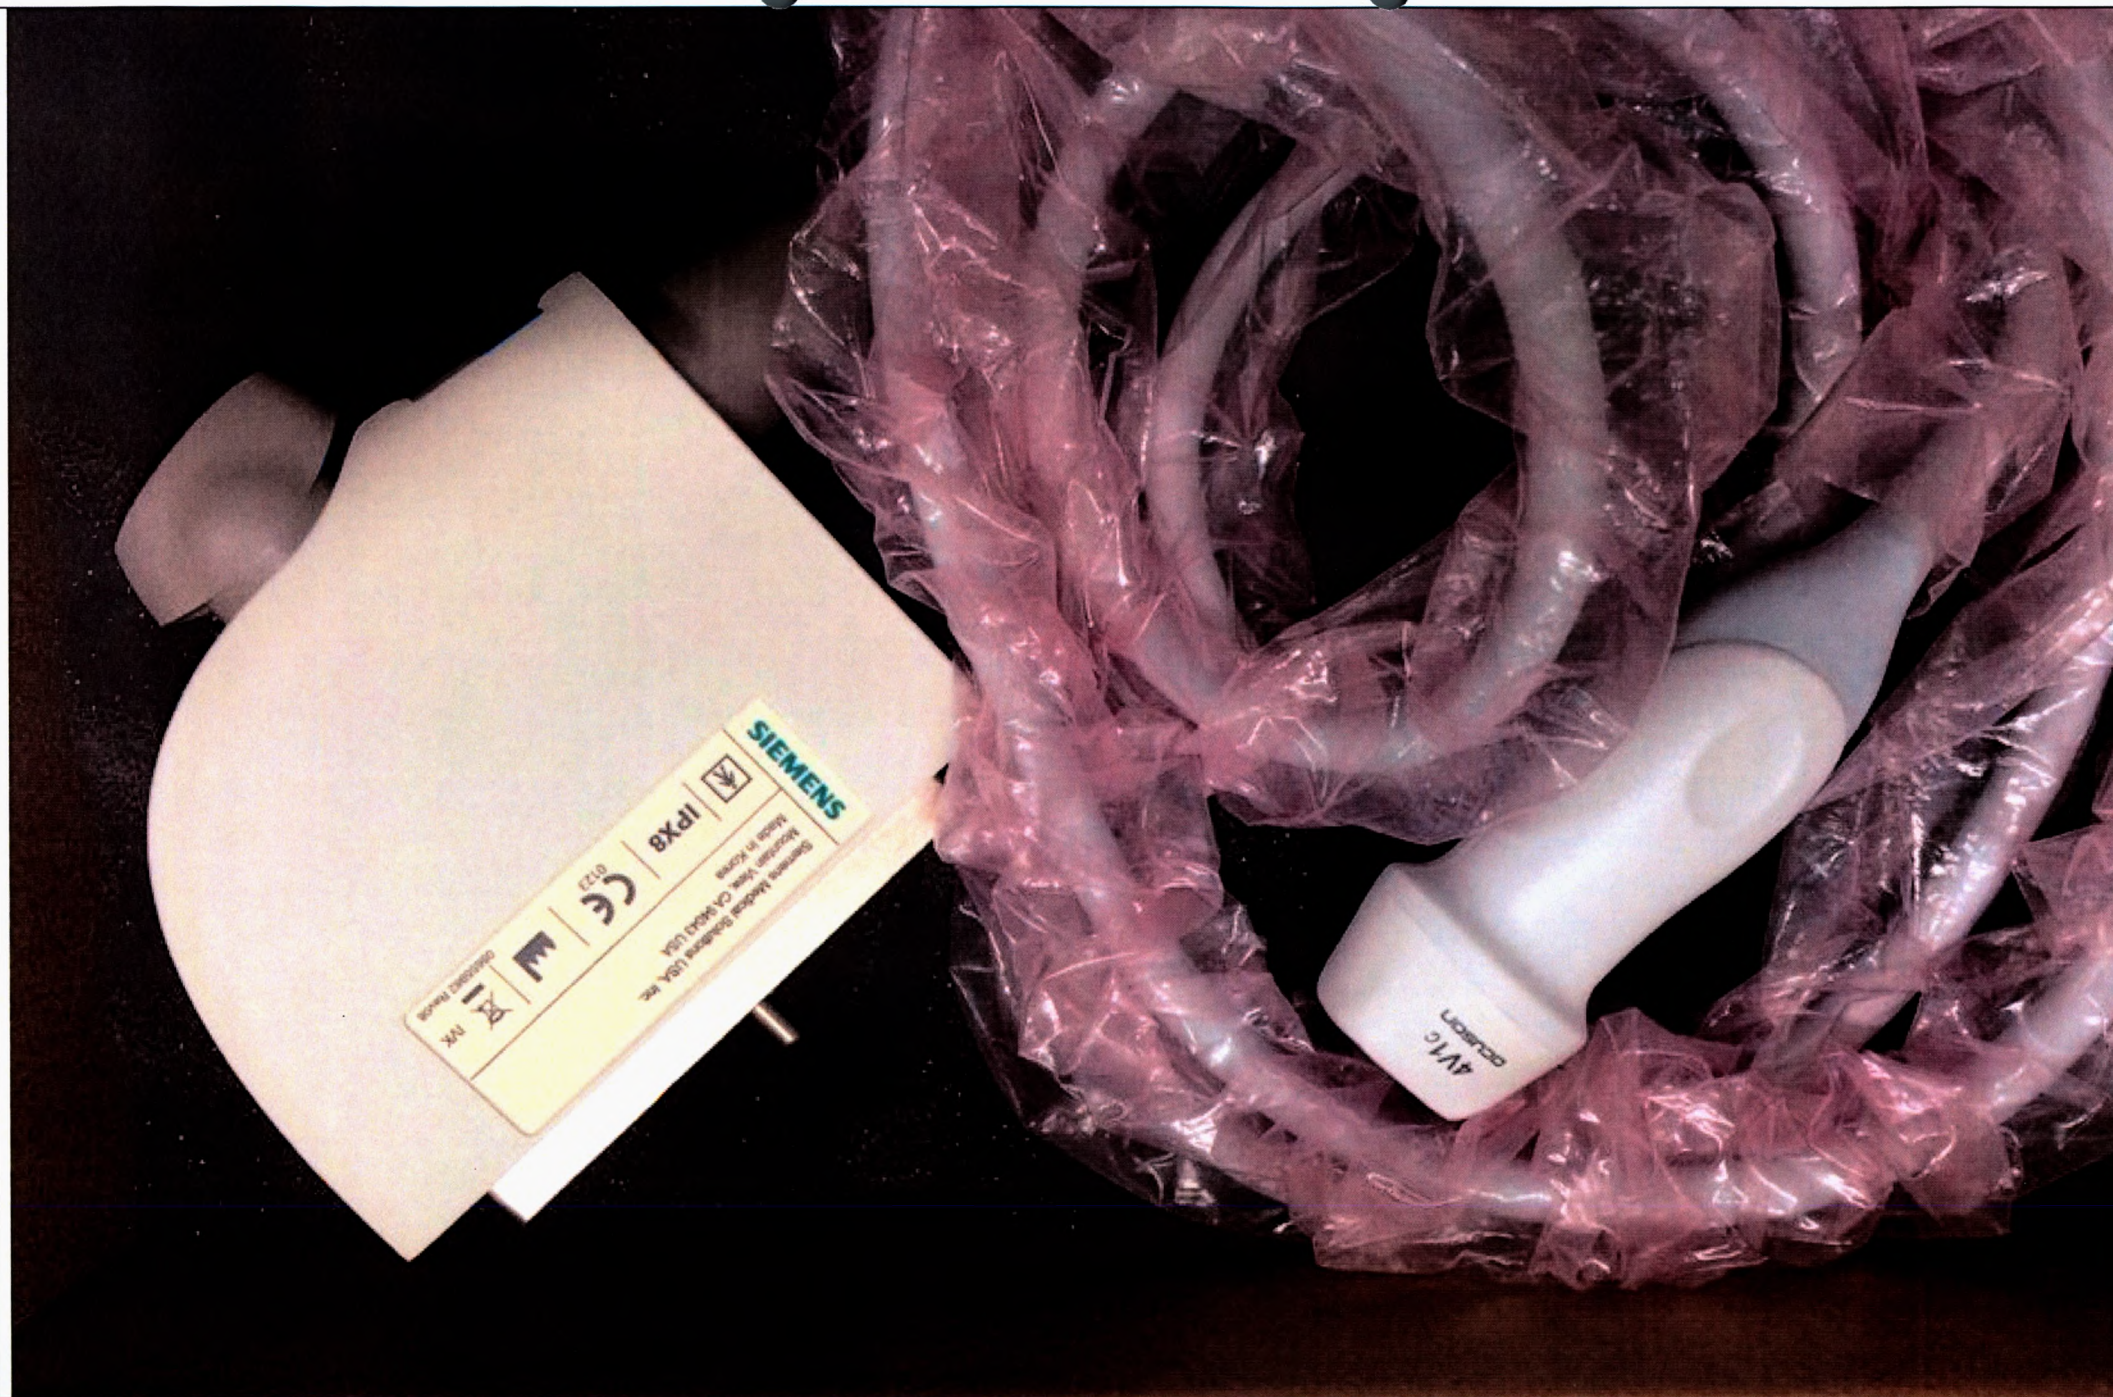

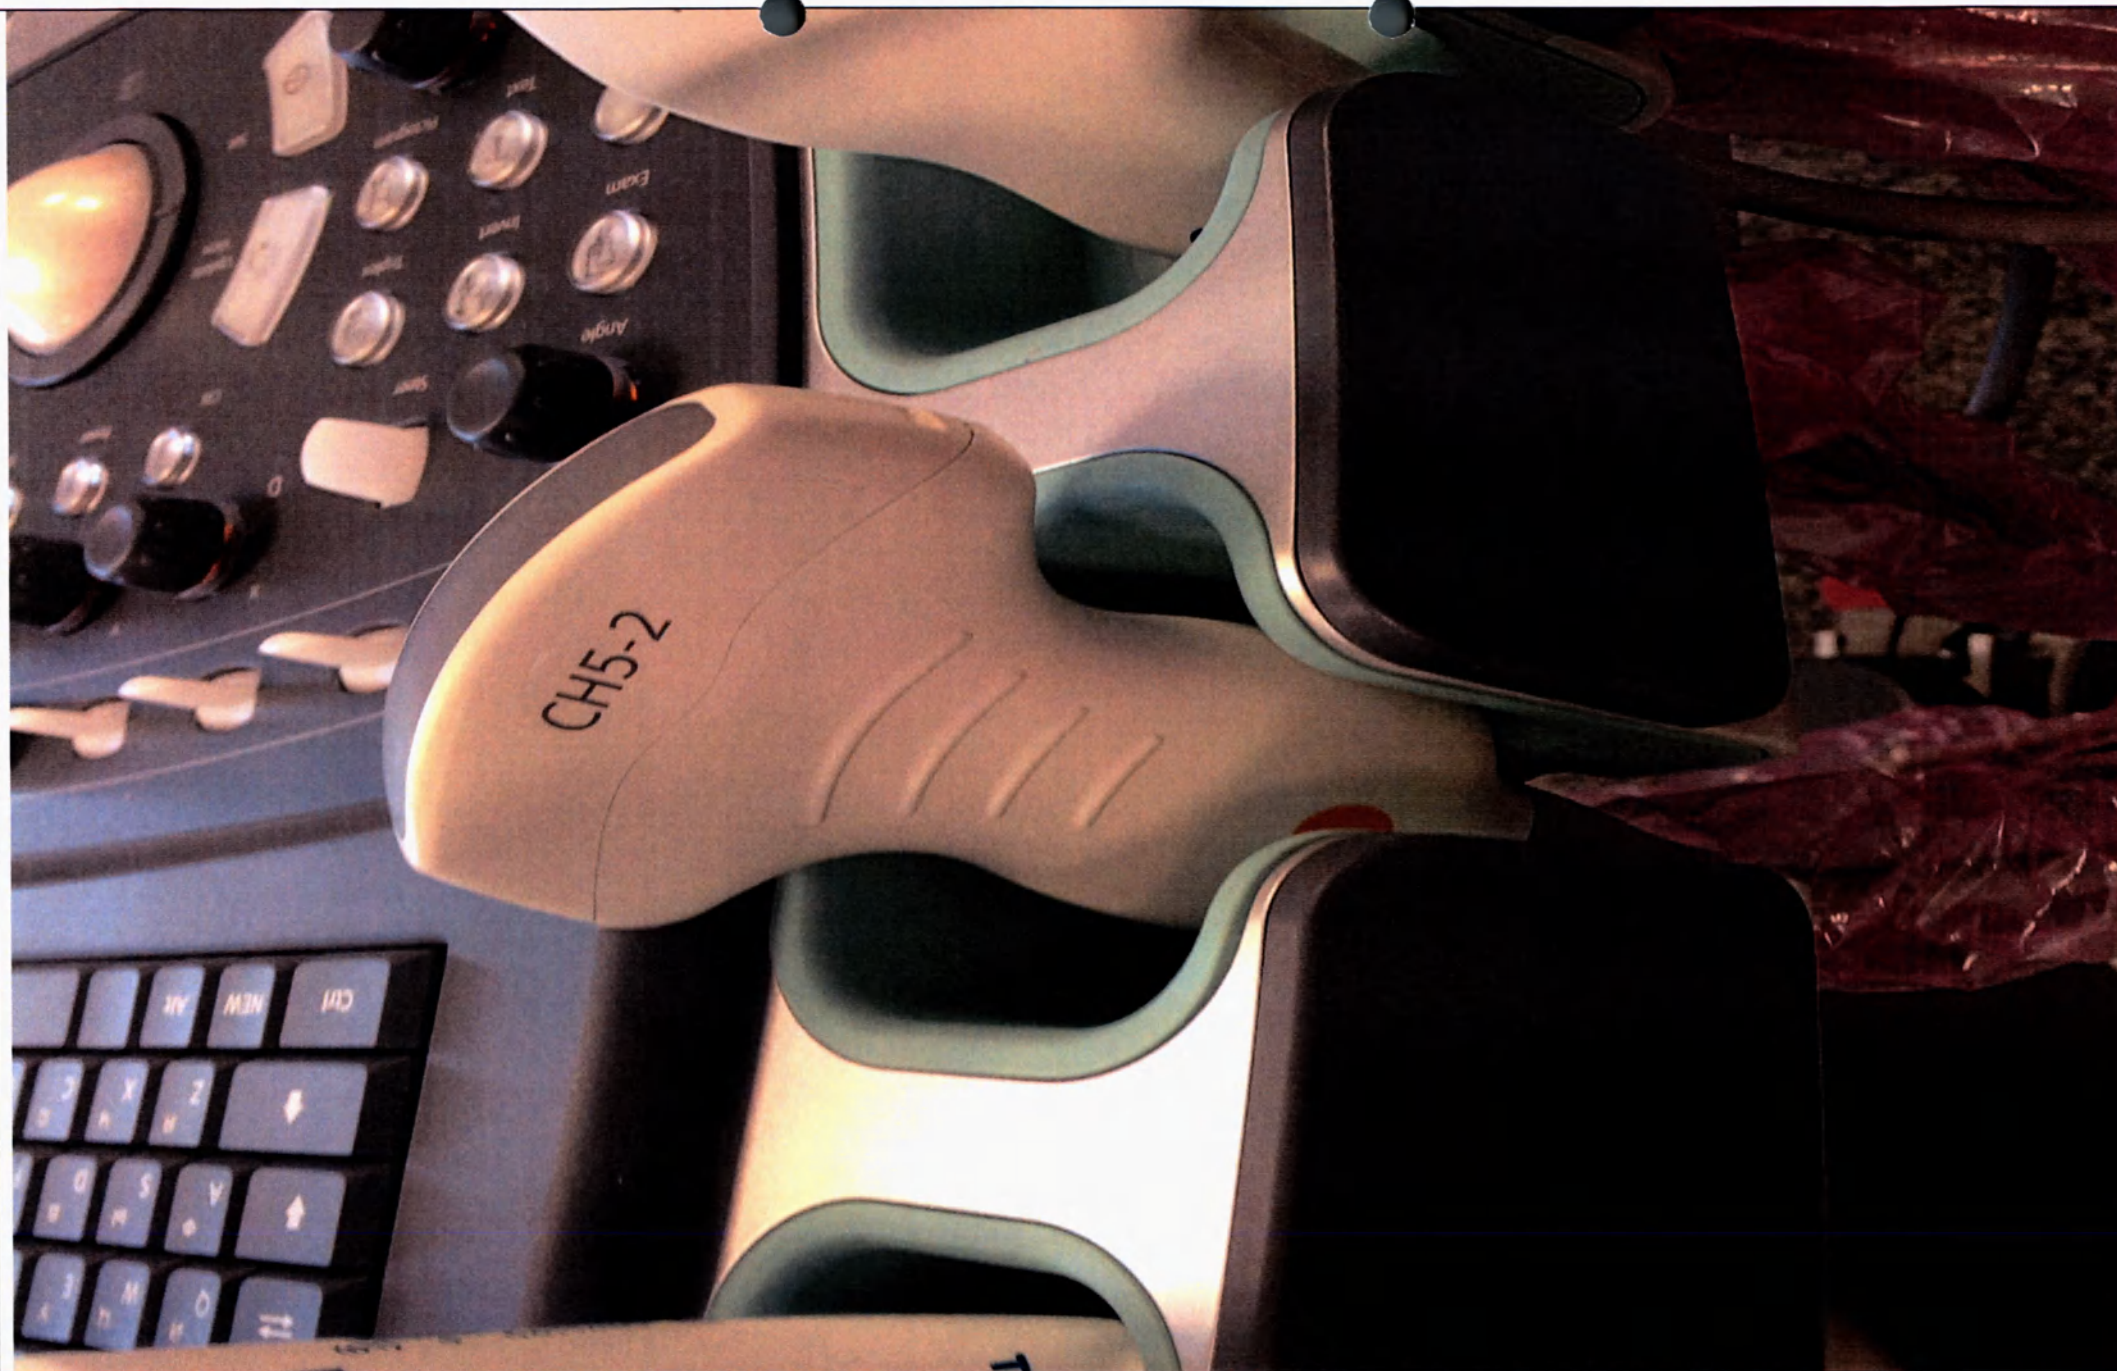


Рисунок 28. Датчик конвексный матричный CH5-2, для сканирования органов брюшной полости, забрюшинного пространства, почек

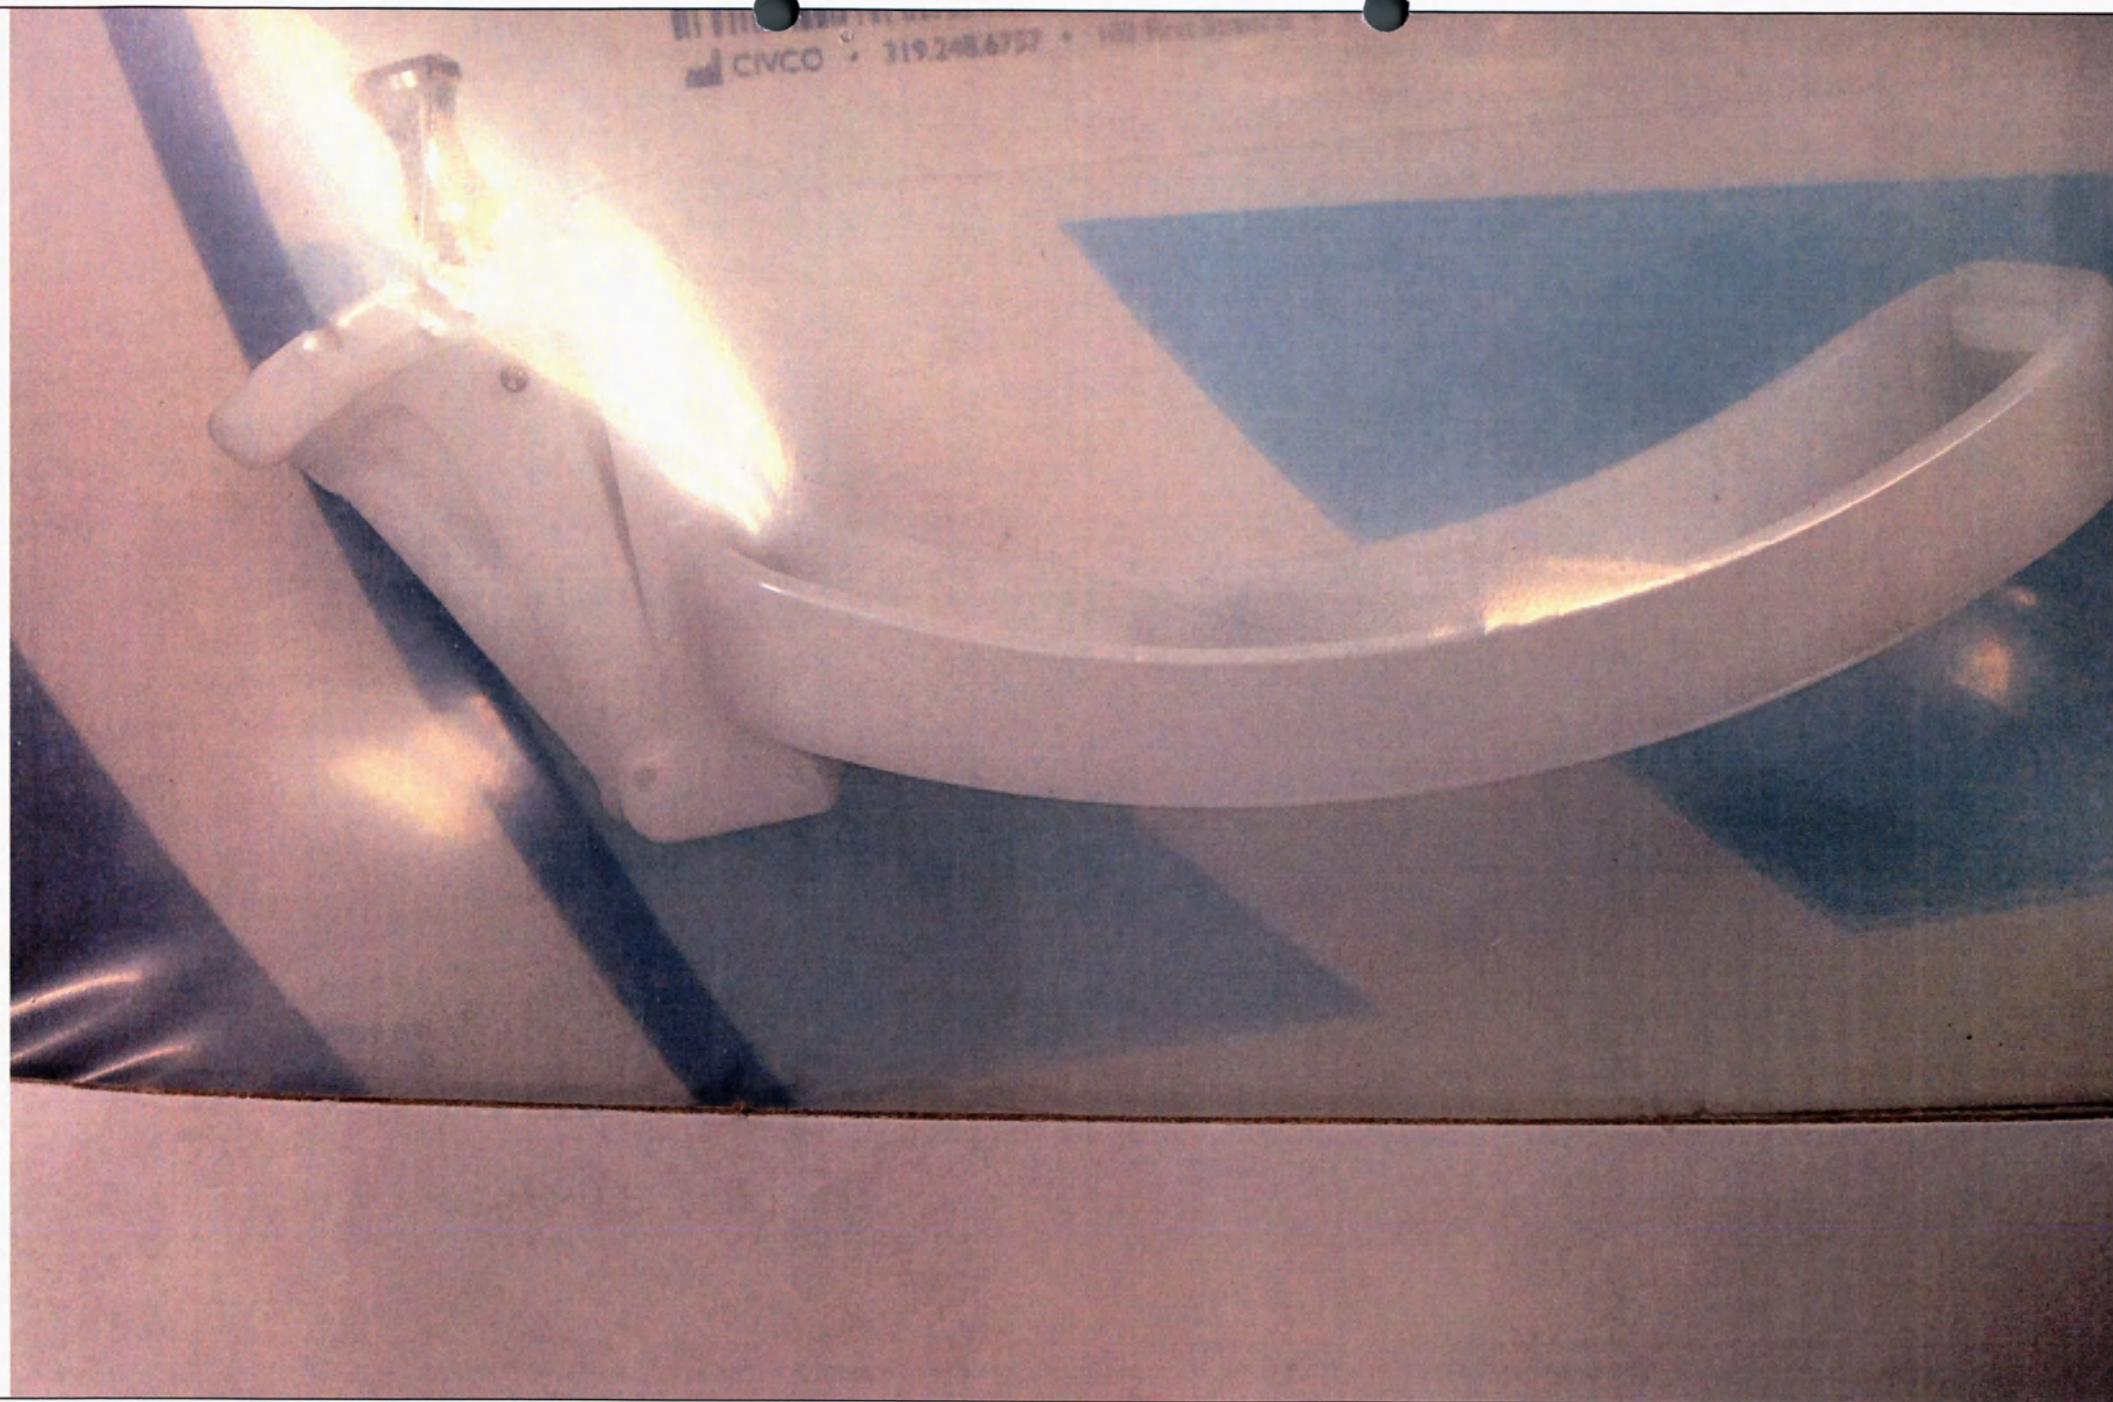


Рисунок 29. Адаптер иглопроводника для конвексного датчика CH5-2

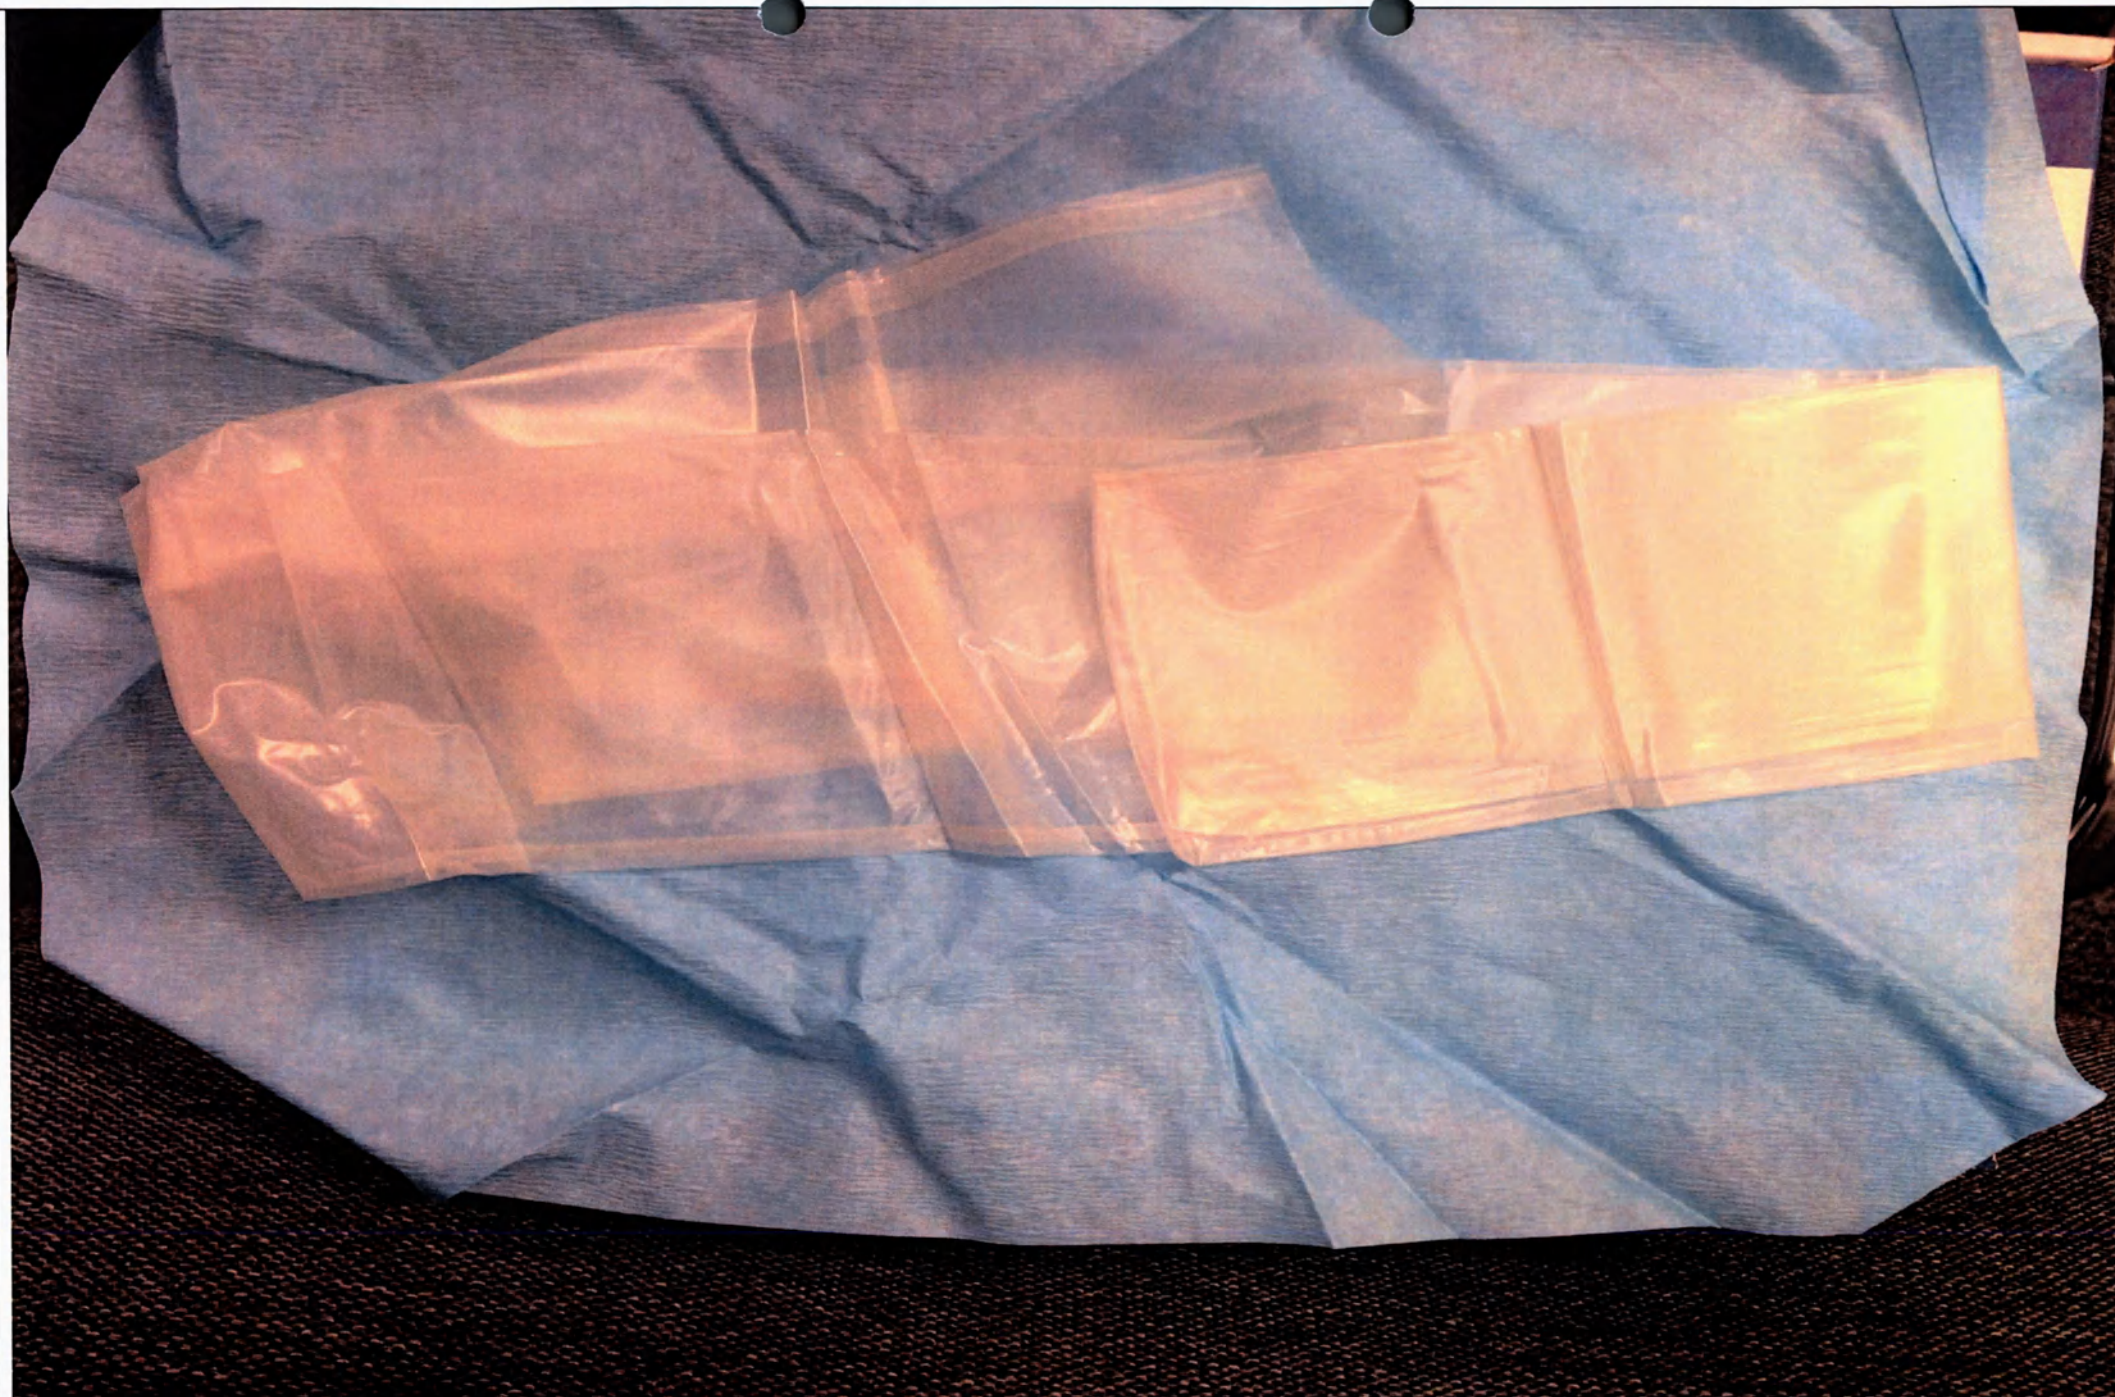


Рисунок 30. Защитные одноразовые чехлы для датчика CH5-2



Рисунок 31. Датчик конвексный матричный C6-2, для сканирования органов брюшной полости, для акушерско-гинекологических исследований



Рисунок 32. Защитные одноразовые чехлы для датчика С6-2

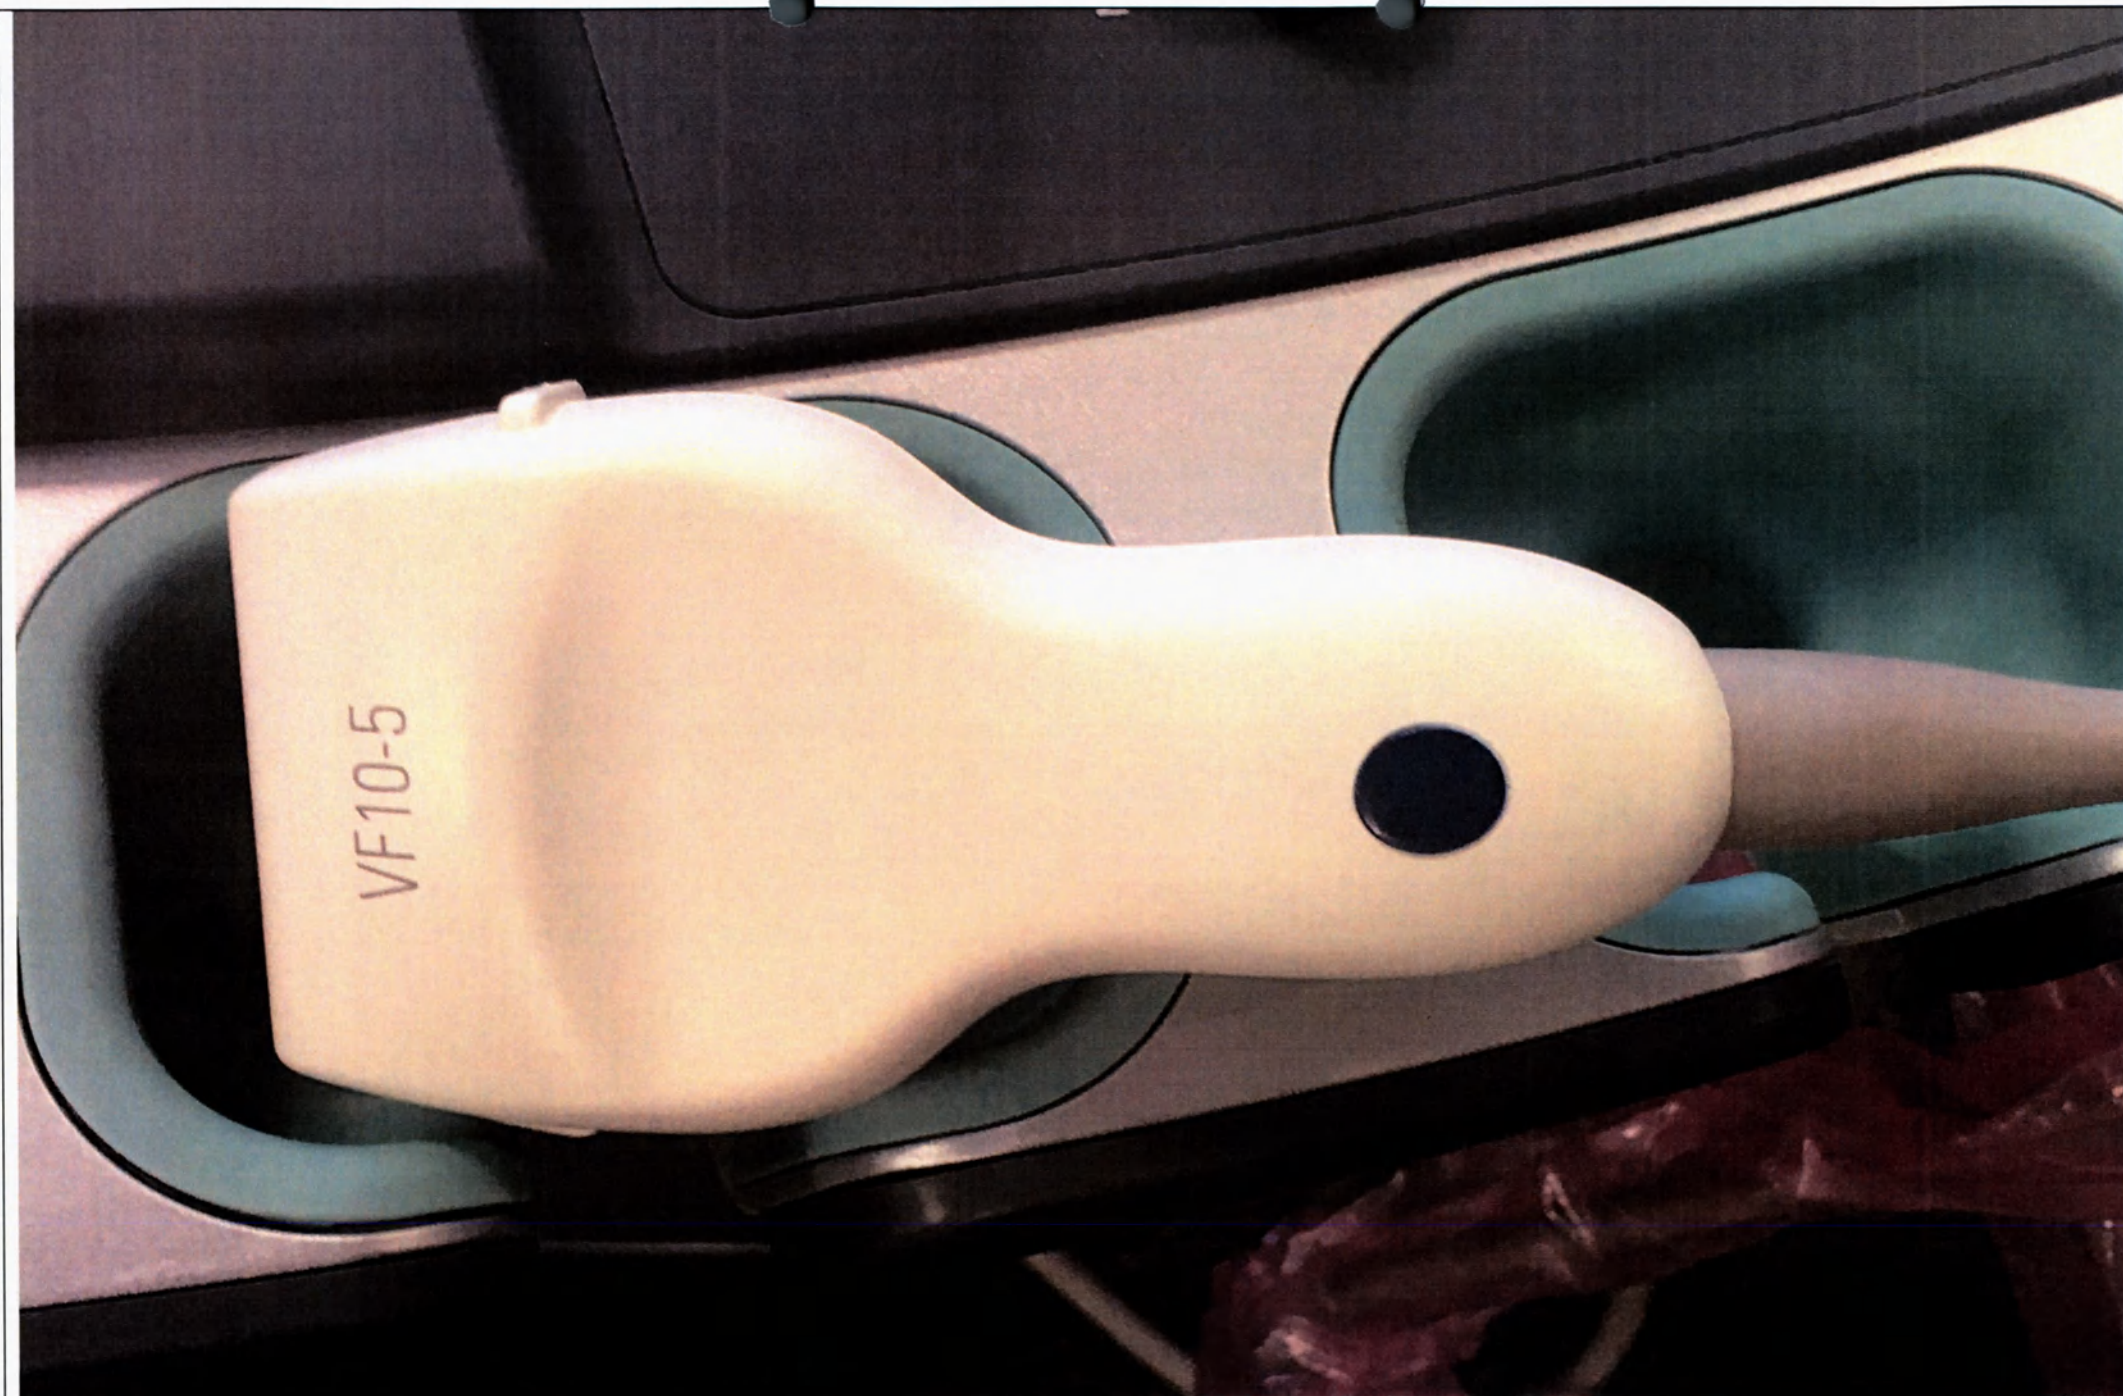


Рисунок 33. Латчик пинейный матричный VF10-5, для сканирования поверхностно-расположенных органов и тканей: щитовидной железы, молочных желез, для
ООО ЦИРМИ ✉ info@cirmi.ru 🌐 www.goszdravnadzor.ru
Федеральное государственное учреждение «Центральный институт радиационной медицины»



Рисунок 34. Адаптер иглопроводника для линейного датчика VF10-5



Рисунок 35. Защитные одноразовые чехлы для датчика VF10-5, не более 10 шт

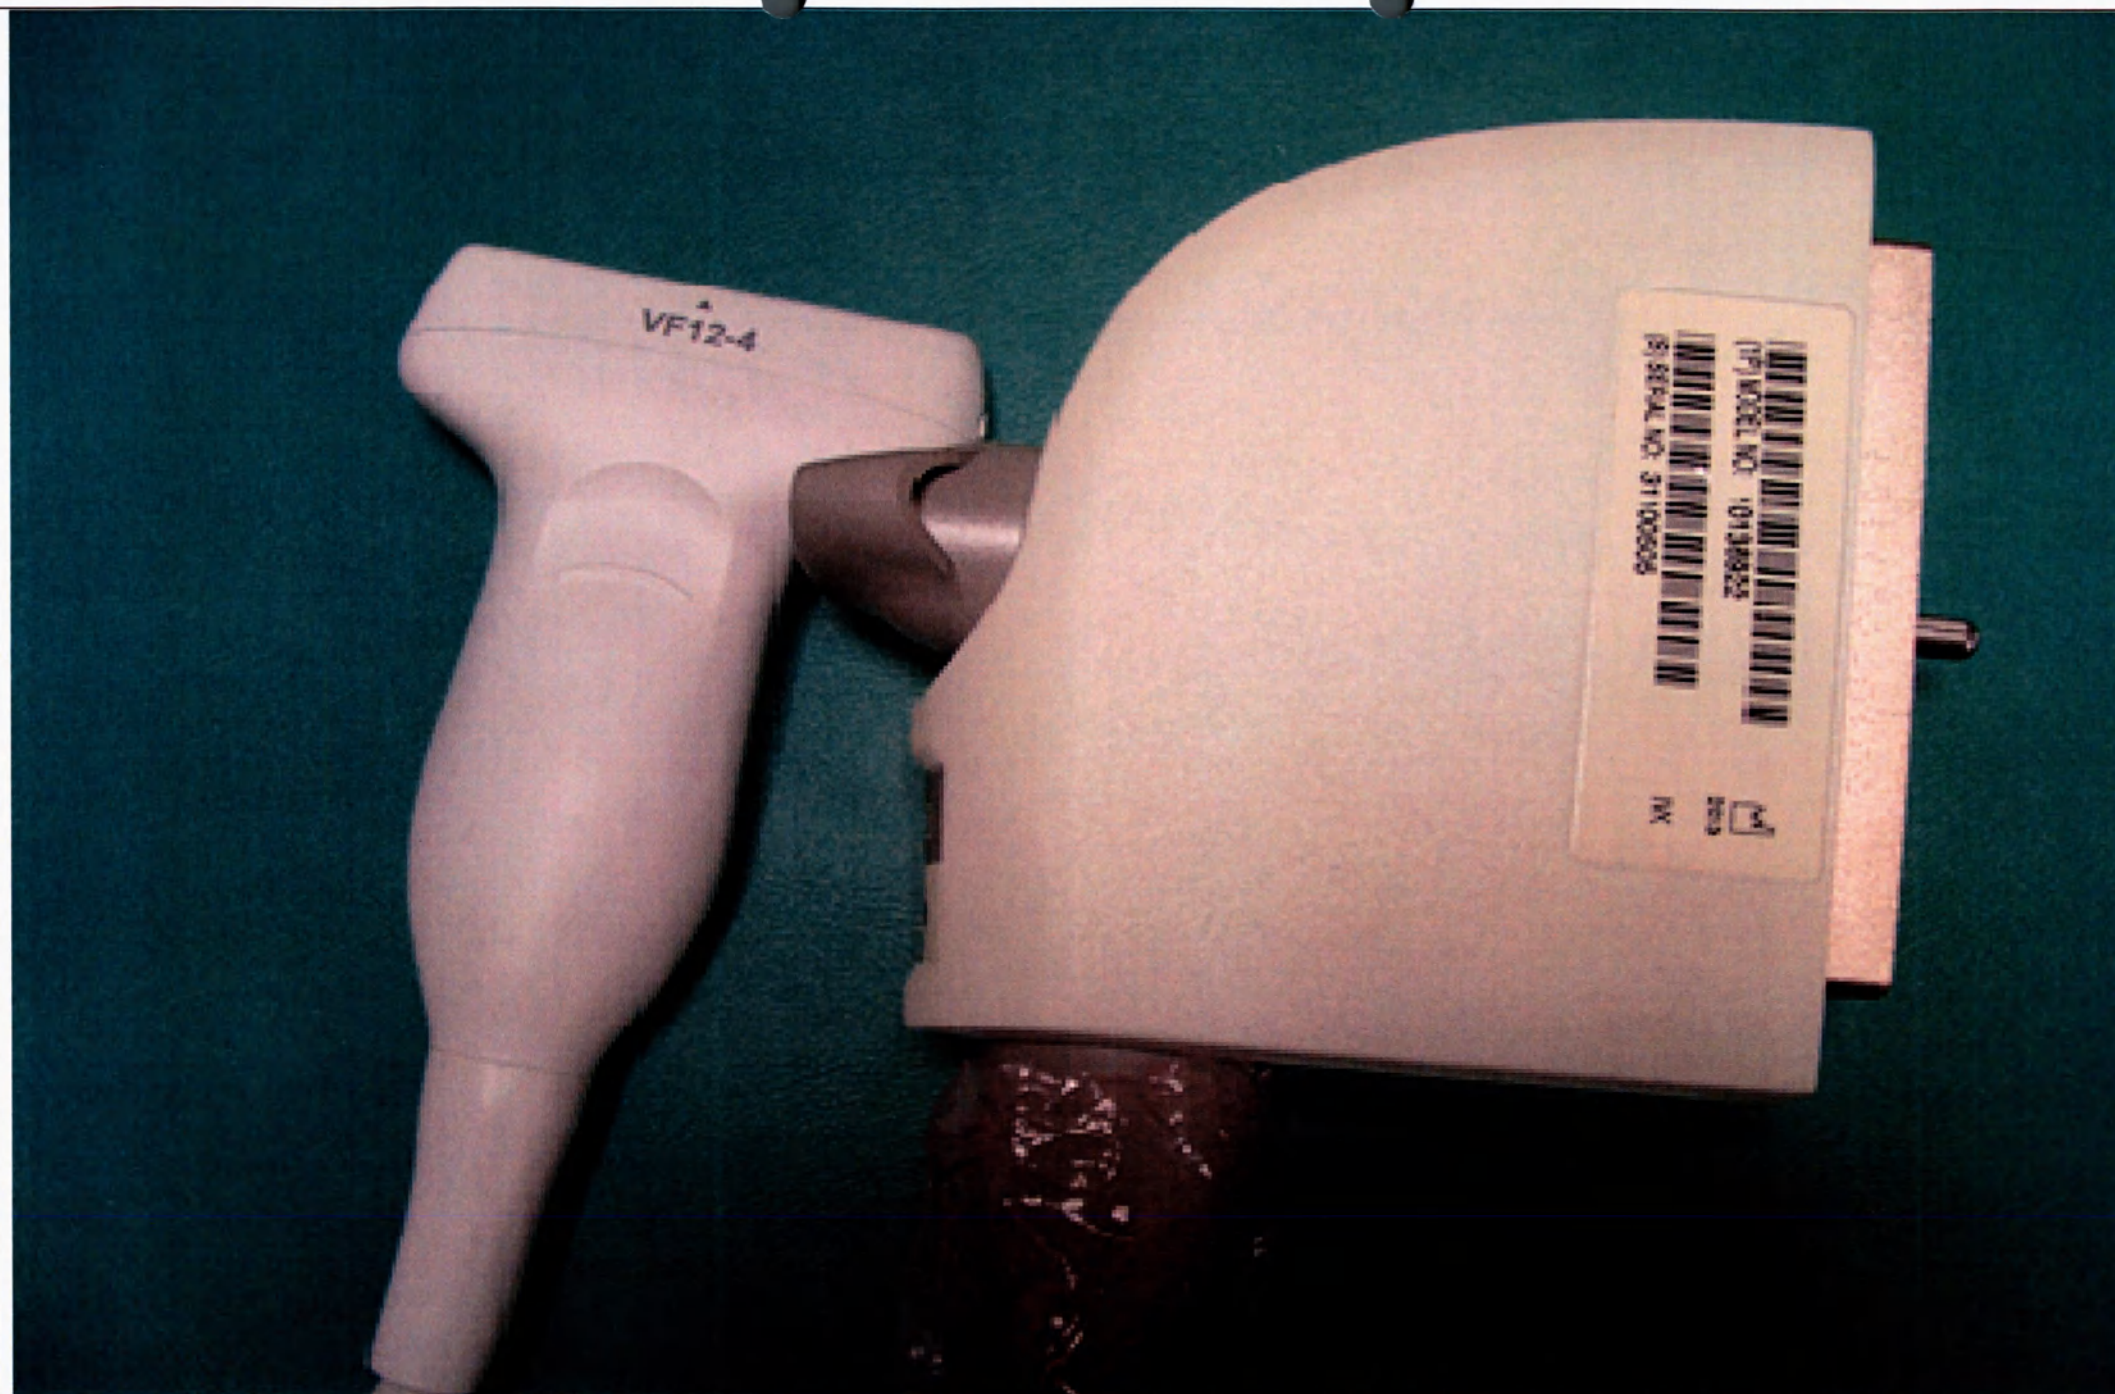


Рисунок 26. Датчик линейный, модель VF12-4, для сканирования поверхностно-расположенных органов и тканей



Рисунок 37. Адаптер иглопроводника одноразовый для линейного датчика VF12-4

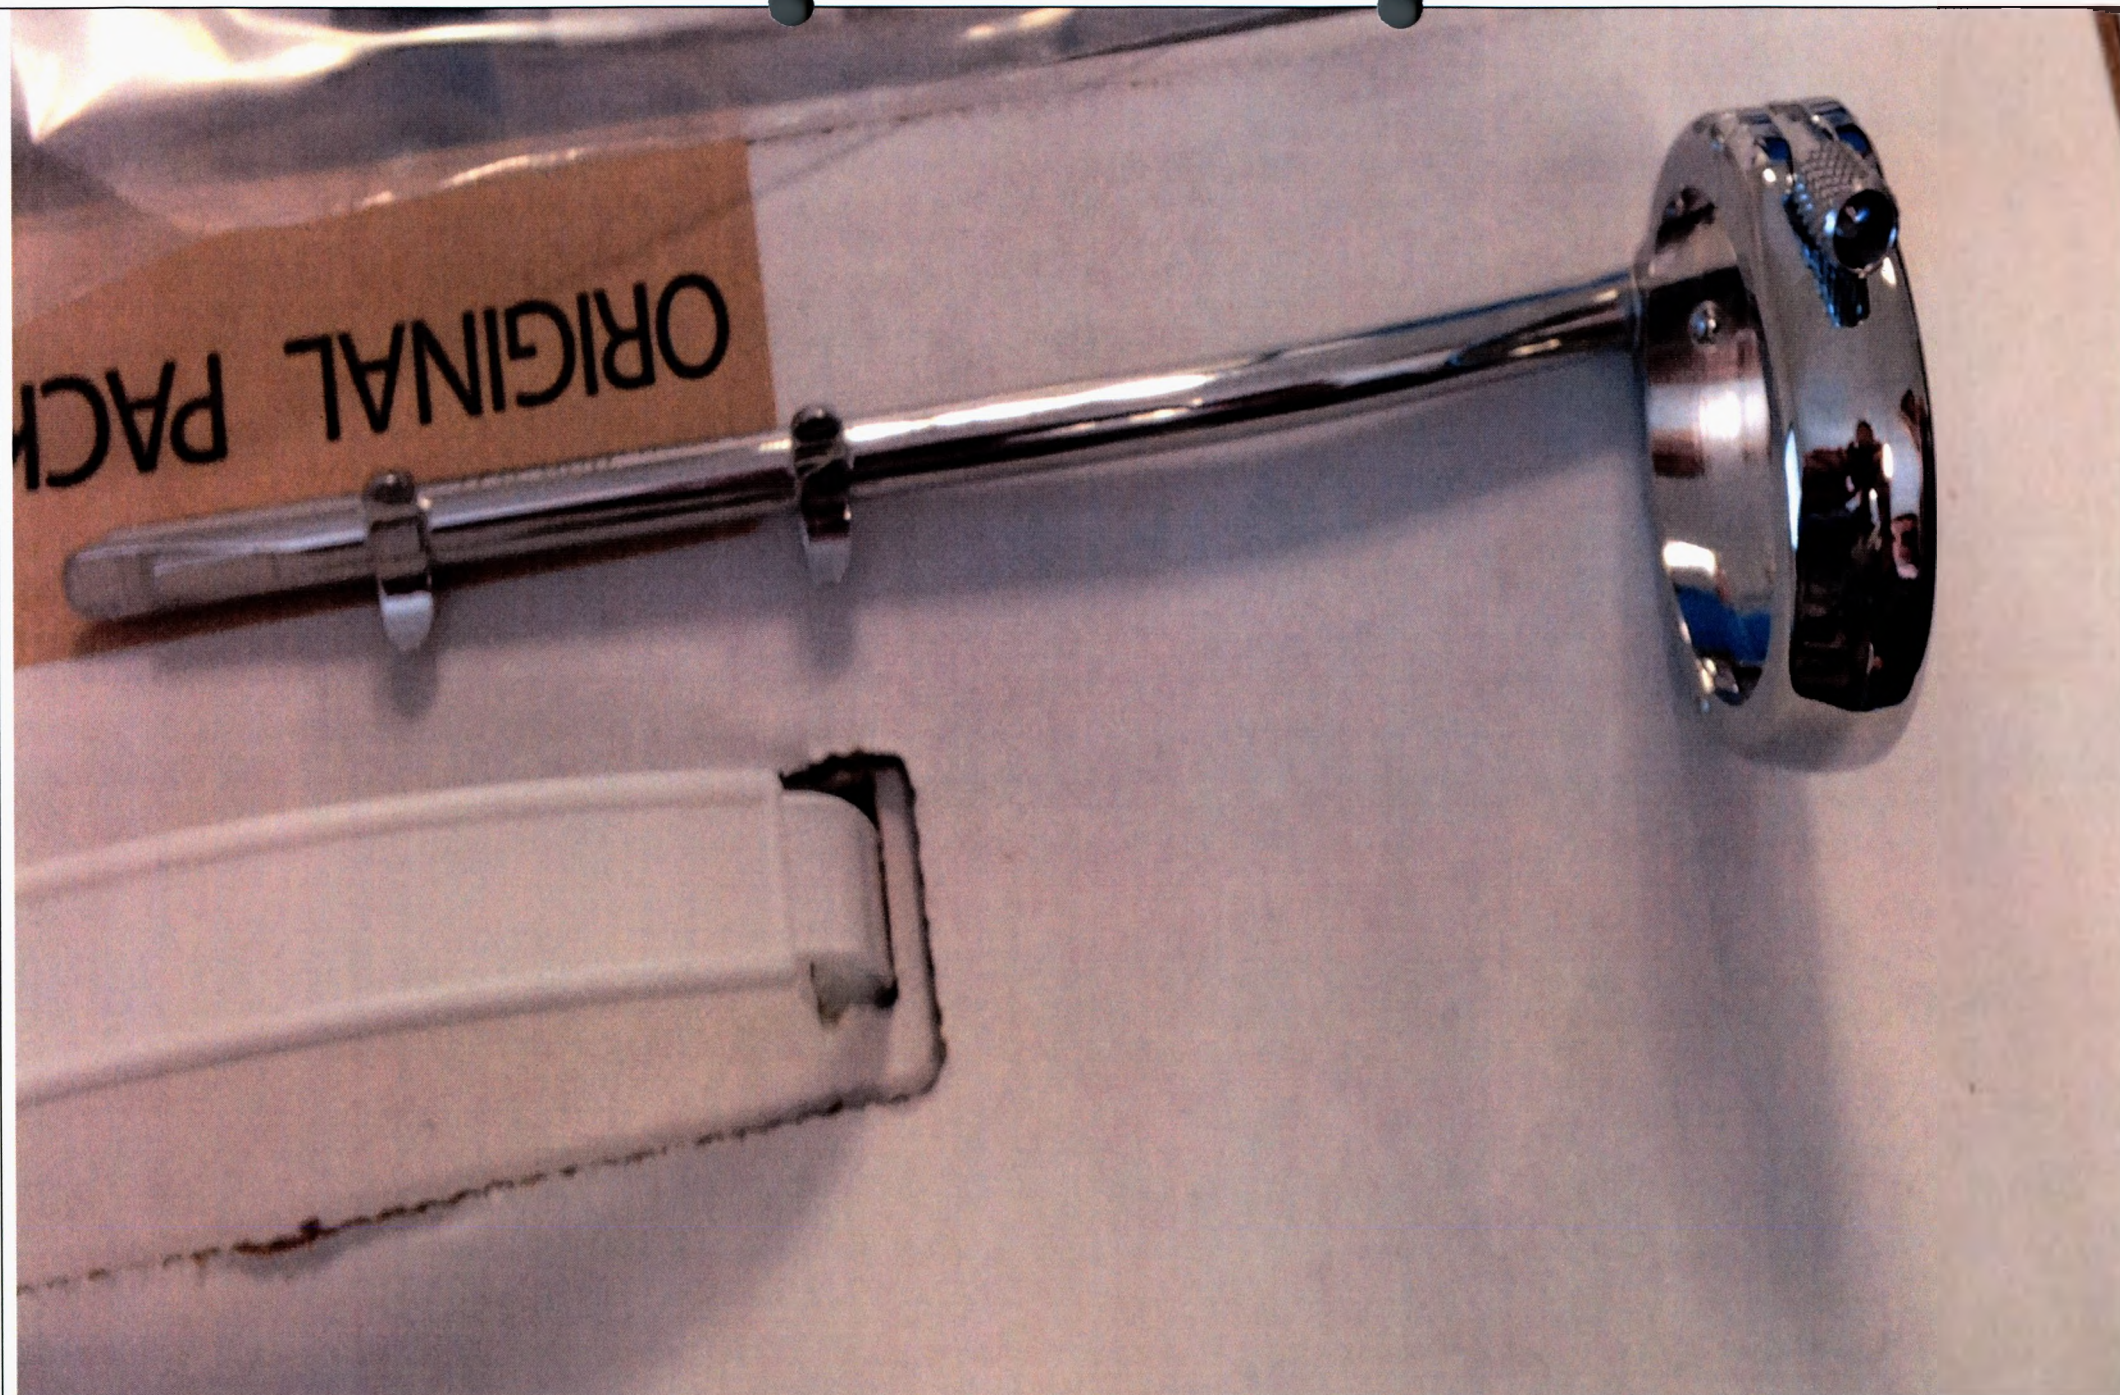


Рисунок 38. Адаптер иглопроводника многоразовый для линейного датчика VF12-4



Рисунок 39. Датчик конвексный высокочастотный с поддержкой функции четырехмерной визуализации C8F3 для акушерских трансабдоминальных исследований



Рисунок 40. Датчик конвексный с поддержкой функции четырехмерной визуализации C6F2 для акушерских трансабдоминальных исследований.



Рисунок 41. Датчик микроконвексный с поддержкой функции четырехмерной визуализации EV9F3 для акушерских трансвагинальных исследований



Рисунок 42. Адаптер иглопроводника многоразовый для датчика EV9F3

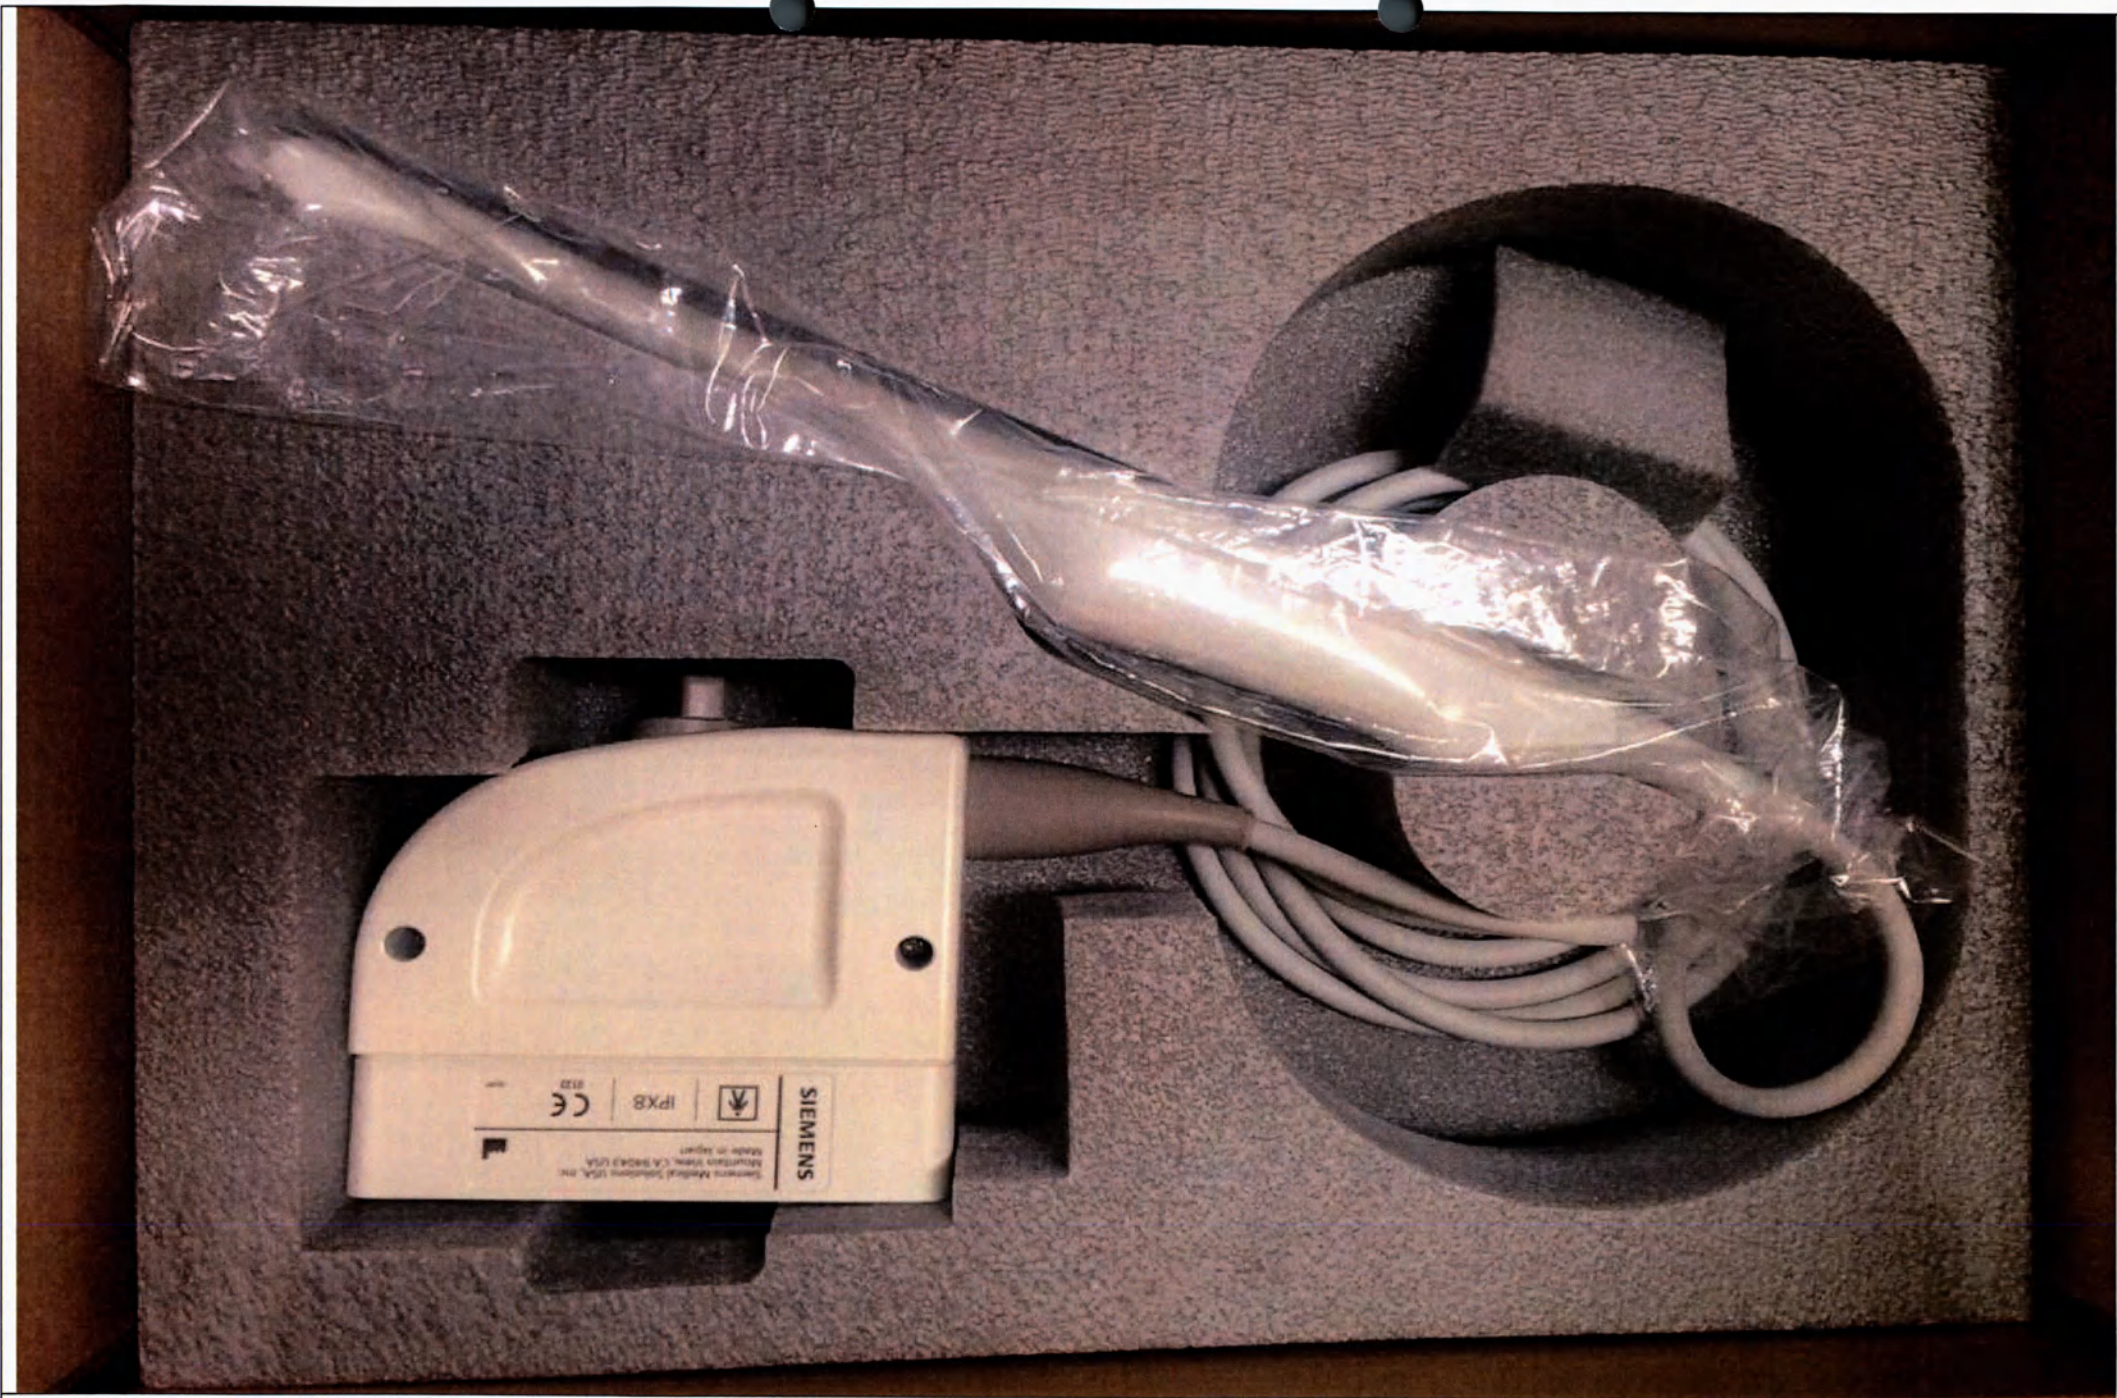


Рисунок 43. Датчик микроконвексный, универсальный эндополостной EC9-4w для акушерско-гинекологических и урологических исследований.

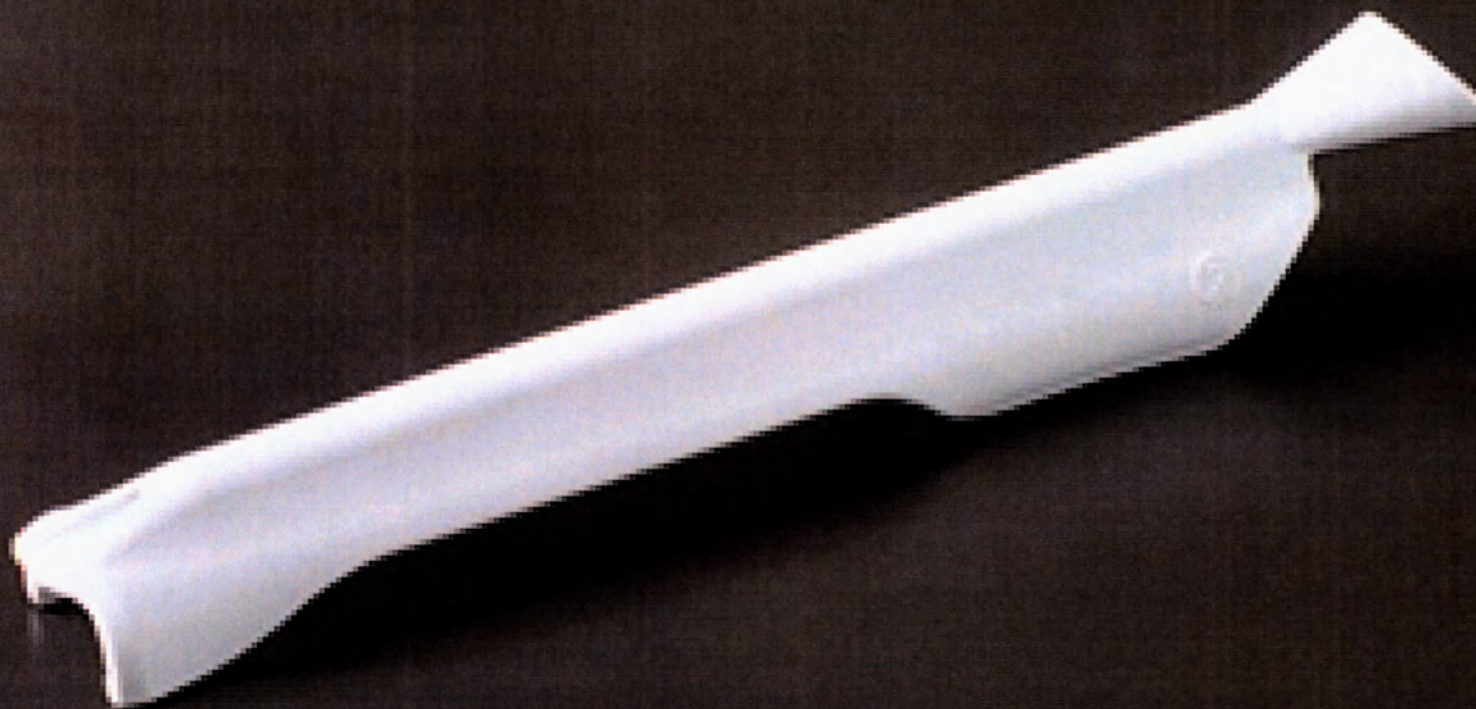


Рисунок 44. Адаптер иглопроводника одноразовый для датчика EC9-4w



Рисунок 45. Адаптер иглопроводника многоразовый для датчика EC9-4w

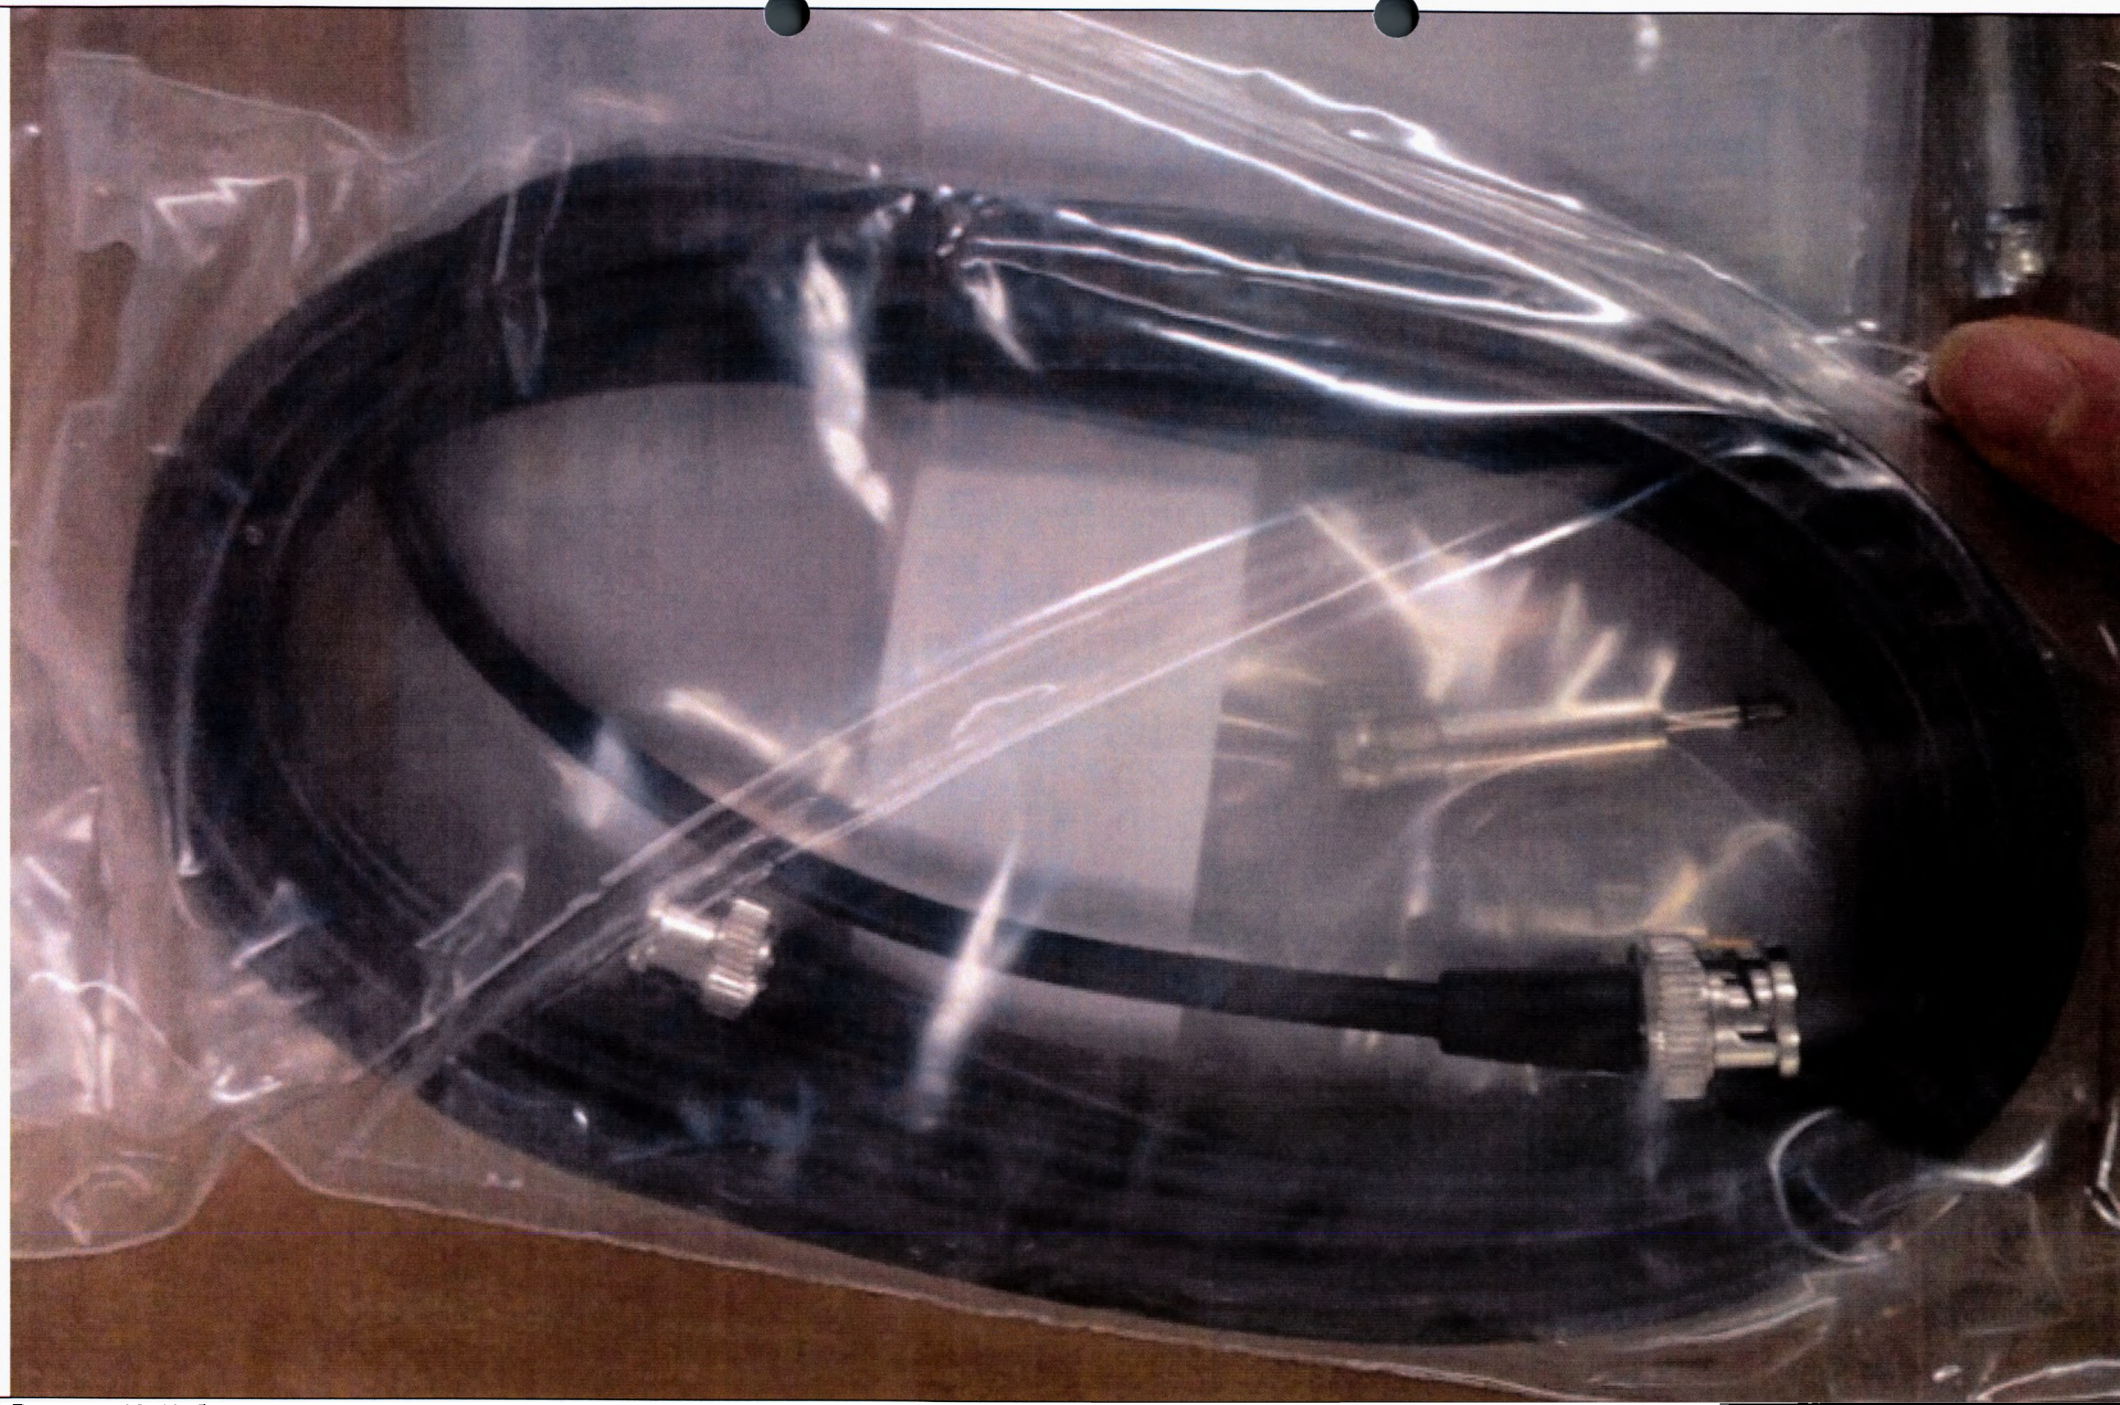


Рисунок 46. Кабель адаптера для стресс-эхокардиографии, европейского образца.



Рисунок 47. Датчик непрерывно-волновой CW2.

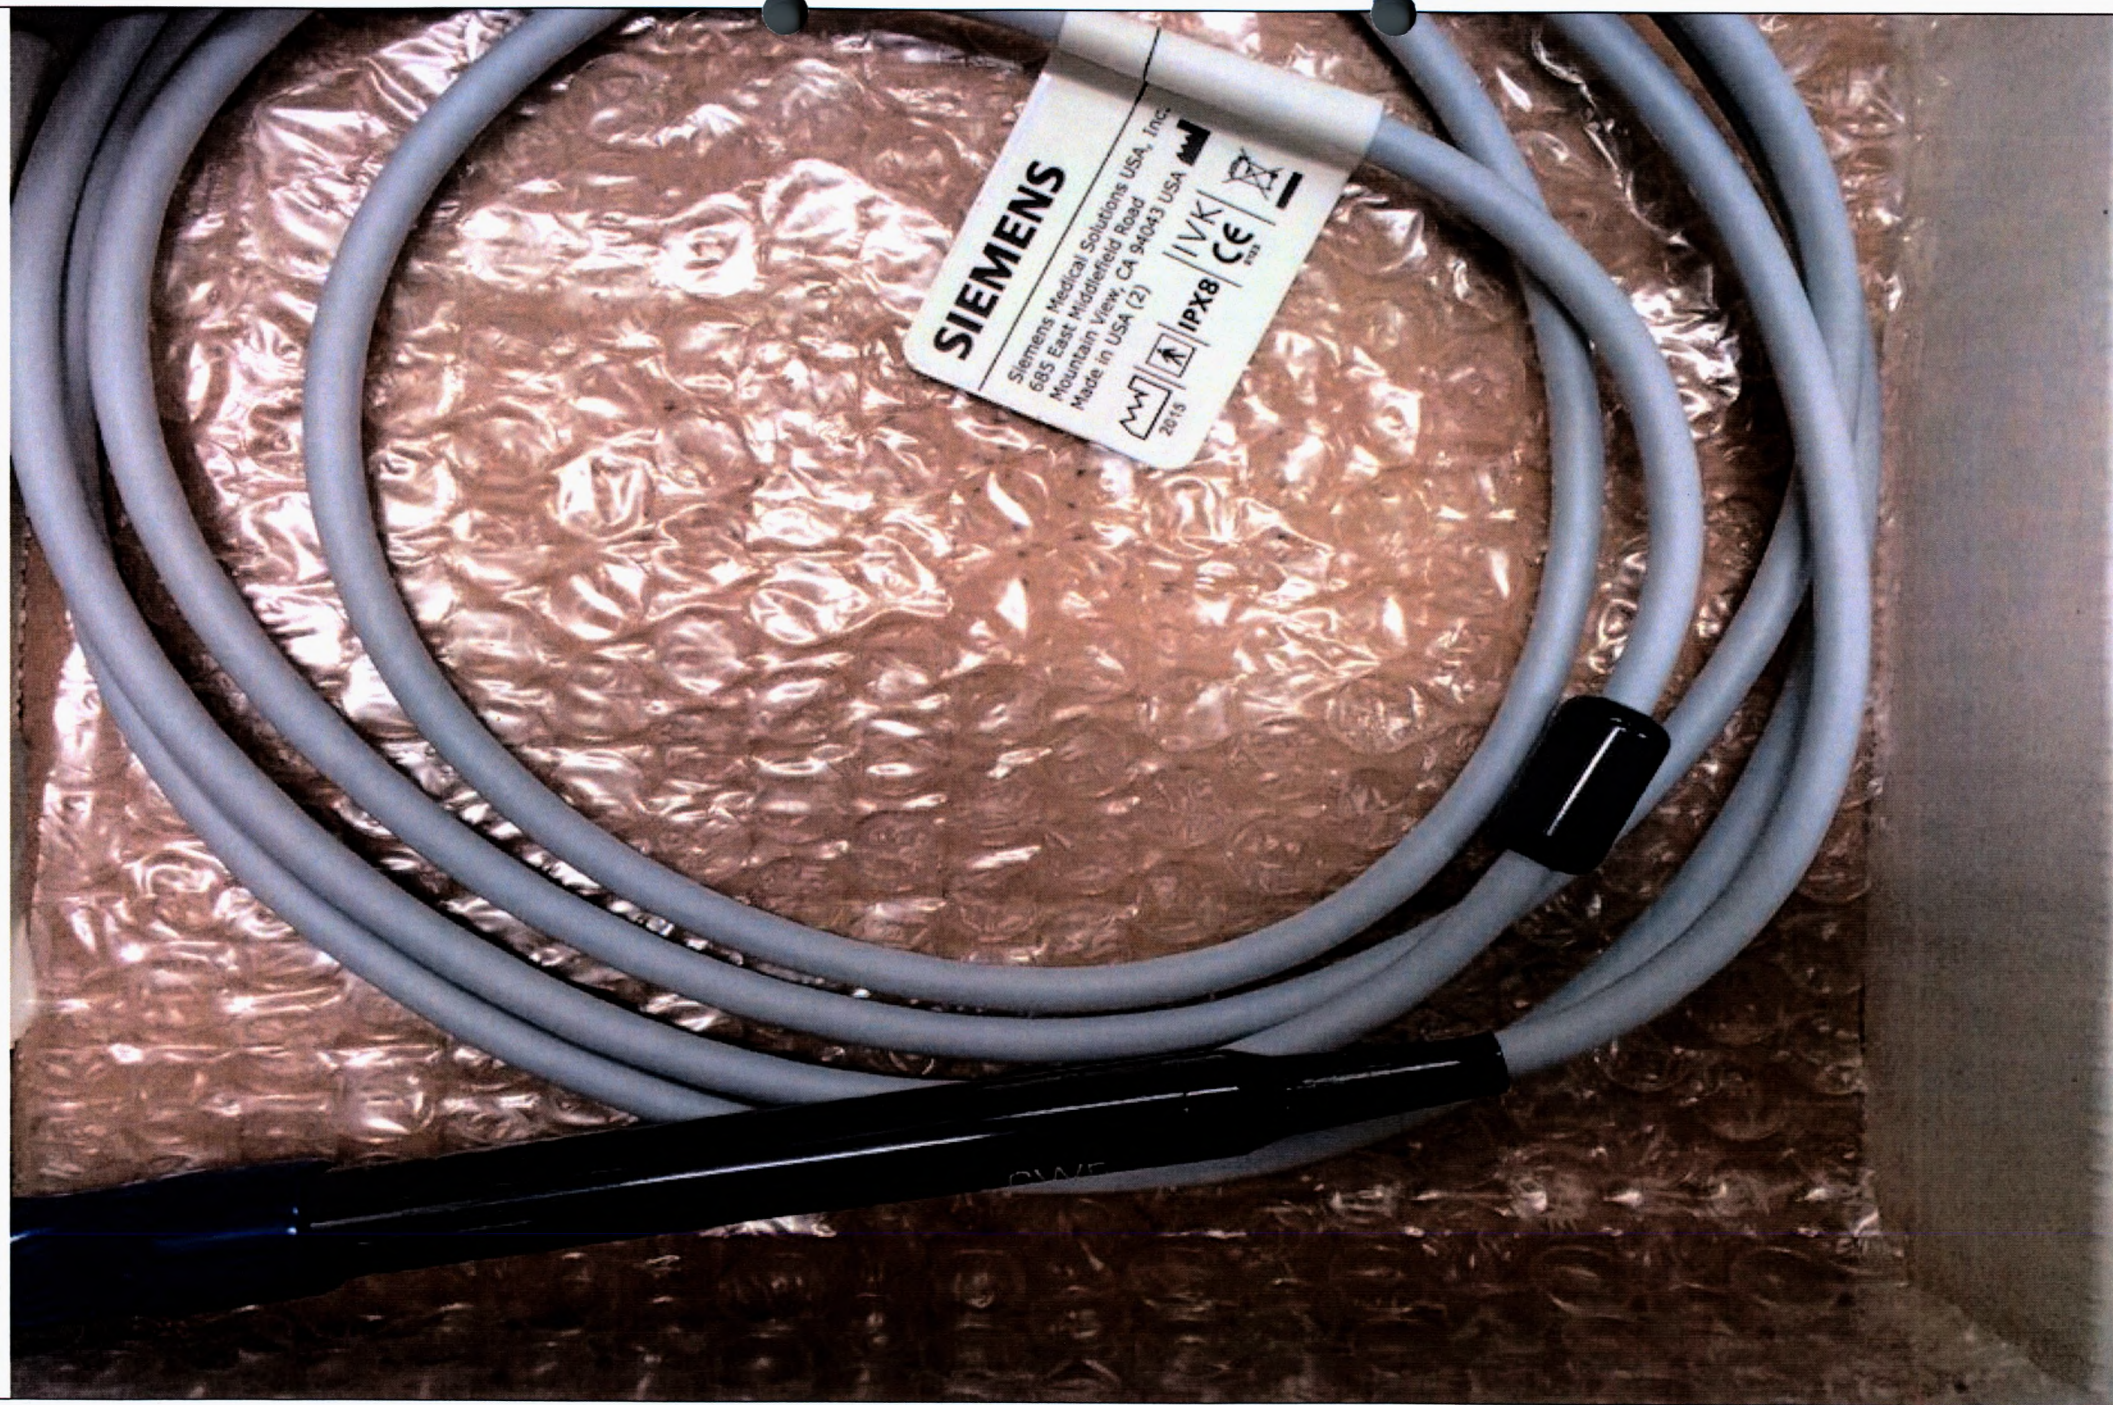


Рисунок 48. Датчик непрерывно-волновой CW5

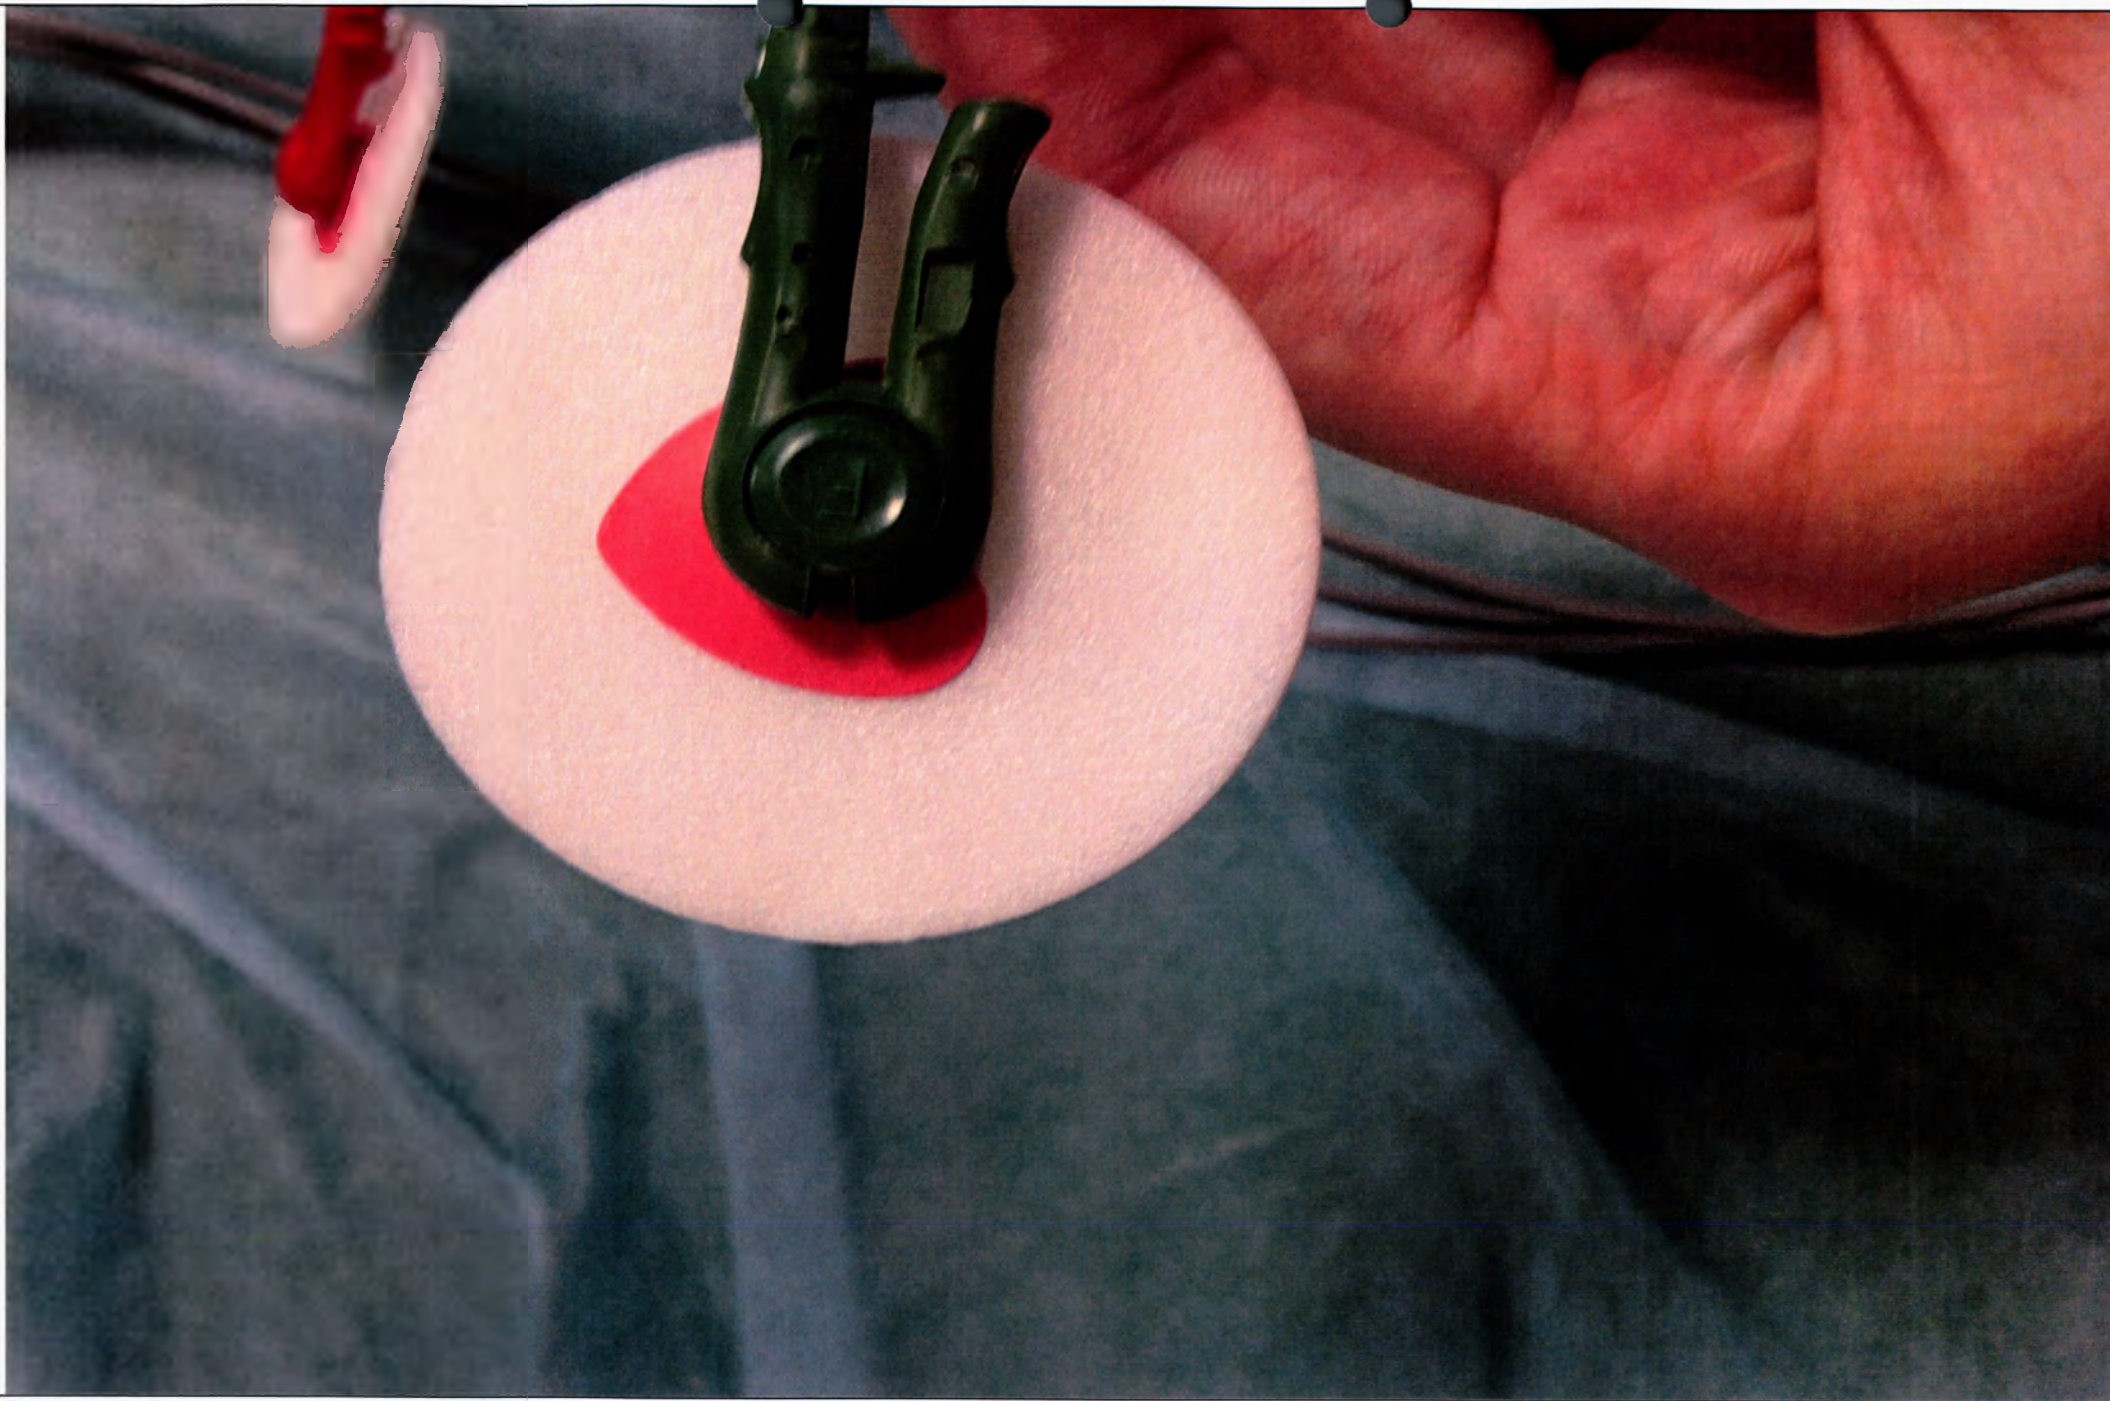


Рисунок 49. Одноразовые электроды ЭКГ



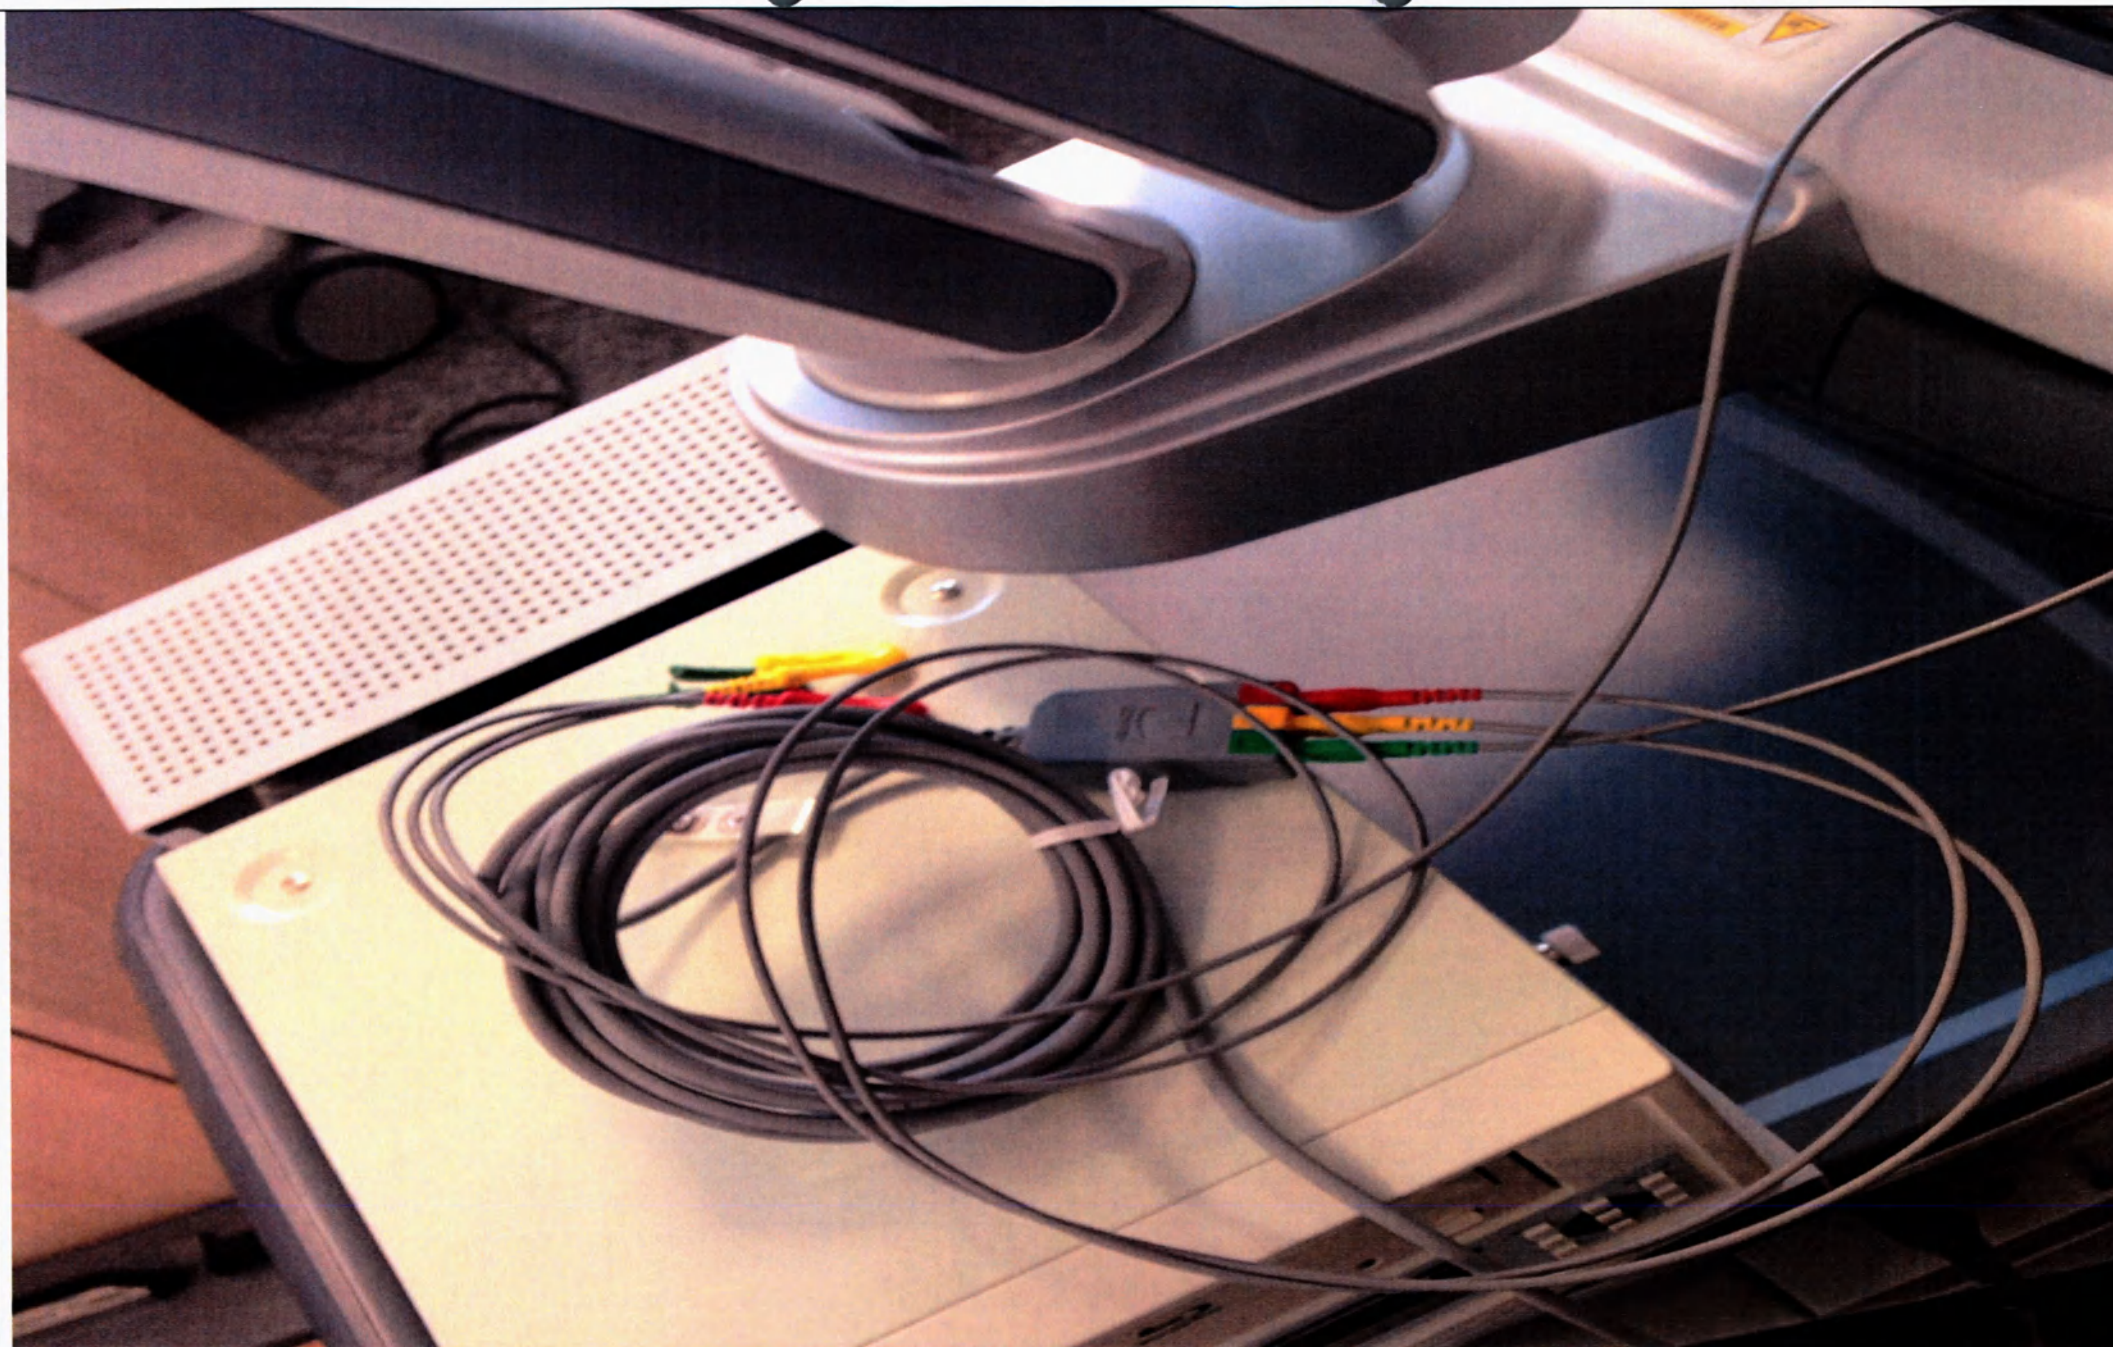


Рисунок 51. Кабель ЭКГ на 3 отведения

Всего
прошито/пронумеровано
56 листа (ов)

ООО «Сиенс»

