

NS-60YG

+3.00

(ϕ T)

(ϕ B)

BN



A-Constant (est)

STERILE



: 13.0mm

: 6.0mm

: PBS01368



: 2024-01

: 119.7

Intended placement : PC

Lens material : SOFT ACRYL/Y

Loop material : SOFT ACRYL/Y



(01) 04987669570302 (17) 240100 (21) PBS01368

CE
0344

78400-P355-00

Manufacturer: NIDEK CO. LTD.

EyeCee

CE
0123



SN : PBS01368

NS-60YG

BAUSCH+LOMB

+3.00

OT : 13.0mm

OB : 8.0mm

78400-P206-C0

24042 Chisaki, France
 TEL: (33) 01 49 60 97 97



NIDEK CO., LTD.
 34-14, Masushima, Hiroshi-cho,
 Gamagori, Aichi 443-0035
 Japan



A-Constant (est)

: 118.7



ONE INTRAOCULAR LENS

OPEN HERE

Линза интраокулярная заднекамерная псевдофакичная EyeCee® One preloaded



BAUSCH+LOMB



STERILE EO

EC REP: NIDEK S.A.,
Europarc 13, rue Auguste Perret,
94042 Créteil, France

 **NIDEK CO., LTD.,**
34-14, Maehama, Hiroishi-cho,
Gamagori, Aichi 443-0038, Japan

CE
0344

EyeCee is a trademark of Bausch & Lomb Incorporated or its affiliates.
© Bausch & Lomb Incorporated.

78400-P534-D0 AW 1800408



Manufacturer: NIDEK CO., LTD



(21)PFX38574

SZ-1 BAUSCH+LOMB +22.00

(ϕ B) : 6.0mm

(ϕ T) : 13.0mm

SN PFX38574

EyeCee preloaded

78400-P376-B0

EyeCee
ONE
PRELOADED

SZ-1

BAUSCH+LOMB



BAUSCH+LOMB 76400-9377-00

Manufacturer: NIDEK CO., LTD.

EyeCee PRELOADED

(φB): 8.0mm (φT): 13.0mm

SZ-1 PFX38574

(01)04987695550(1)724000021PFX38574

BAUSCH+LOMB

Manufacturer: NIDEK CO., LTD.

EyeCee PRELOADED

(φB): 8.0mm (φT): 13.0mm

SZ-1 PFX3857

(01)04987695550(1)724000021PFX38574

BAUSCH+LOMB

Manufacturer: NIDEK CO., LTD.

EyeCee PRELOADED

(φB): 8.0mm (φT): 13.0mm

SZ-1 PFX3857

(01)04987695550(1)724000021PFX38574

BAUSCH+LOMB

Manufacturer: NIDEK CO., LTD.

EyeCee PRELOADED

(φB): 8.0mm (φT): 13.0mm

SZ-1 PFX3857

(01)04987695550(1)724000021PFX38574

BAUSCH+LOMB

NIDEK CO., LTD., 34-14 Mashima, Hiroishi-cho,
Gamagori, Aichi 443-0038, Japan

EC REP

NIDEK S.A., Europe: 13, rue Auguste Perret,
94042 Créteil, France

AW 1600795



Manufacturer: NIDEK CO., LTD.



(21)PFX38574
SZ-1 BAUSCH+LOMB +22.00
(φB): 8.0mm (φT): 13.0mm
PFX38574 EyeCee PRELOADED
76400-9377-00

CE
SAA

EyeCee
PRELOADED
ONE
SZ-1

Product Information

Indications
The EyeCee SZ-1 contact lens is designed for use in the correction of myopia (nearsightedness) in both eyes. It is a soft, flexible, preloaded contact lens. It is made of a special material that allows it to be worn for extended periods of time without causing discomfort. It is also designed to provide clear vision and comfort throughout the day.

Contraindications
The EyeCee SZ-1 contact lens should not be worn by individuals who have any of the following conditions:
1. Active eye infection or inflammation.
2. Recent eye surgery or trauma.
3. Allergic reactions to contact lenses or eye drops.
4. Dry eye syndrome or other conditions that affect the tear film.
5. Any other condition that may affect the health of the eye.

Warnings
The EyeCee SZ-1 contact lens should be worn as directed by the manufacturer. It should not be worn for extended periods of time without giving the eyes a rest. It should not be worn while sleeping or during activities that require a high degree of visual acuity. It should not be worn if it causes discomfort or if it does not provide clear vision.

Directions for Use
1. Wash your hands thoroughly with soap and water before handling the contact lens.
2. Remove the contact lens from its packaging and inspect it for damage or debris.
3. Place the contact lens on the eye and blink several times to settle it.
4. Remove the contact lens by pulling on the temple of the frame or by using the contact lens removal tool.
5. Clean the contact lens with a mild, non-alkaline detergent and rinse it with sterile water.
6. Store the contact lens in its case with a drop of sterile water or contact lens solution.

Precautions
The EyeCee SZ-1 contact lens should be worn as directed by the manufacturer. It should not be worn for extended periods of time without giving the eyes a rest. It should not be worn while sleeping or during activities that require a high degree of visual acuity. It should not be worn if it causes discomfort or if it does not provide clear vision.

Линза интраокулярная заднекамерная псевдофакичная EyeCee® One crystal



EyeCee[®] crystal

01

NS-60G

+1.00

(φT)

(φB)

301

8

A-Combined (net)

07000000



: 13.0mm

: 6.0mm

: MFS00551

: 2022-04

: 119.7

Intended placement : PC

Lens material : SOFT ACRYL

Loop material : SOFT ACRYL



(01)04987669301630(17)220400(21)MFS00551

CE
0344

NIDEK CO., LTD.
34-14, Mashima, Higashi
Gamagori, Aichi 440
Japan

Manufacturer: NIDEK CO., LTD.

EyeCee crystal 0123



SN : NFS00901

NS-606

+1.00

13.00

6.00




Линза интраокулярная заднекамерная псевдофакичная EyeCee® One crystal preloaded



EyeCee®
ONE CRYSTAL PRELOADED

SZ-1C

BAUSCH+LOMB

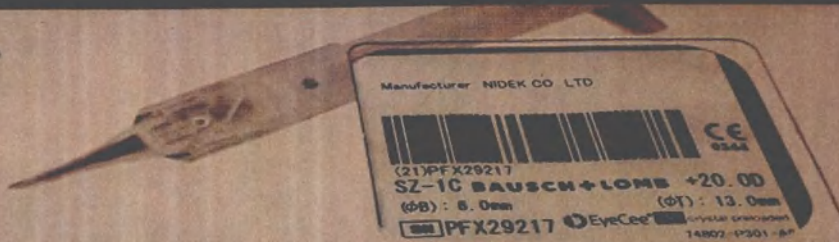

BAUSCH+LOMB



STERILE EO

EC REP: NIDEK S.A.,
Europarc 13, rue Auguste Perret,
94 042 Créteil, France

 **NIDEK CO., LTD.,**
34-14, Maehama, Hiroishi-cho,
Gamagori, Aichi 443-0038, Japan

CE
0344

EyeCee is a trademark of Bausch & Lomb Incorporated or its affiliates.
© Bausch & Lomb Incorporated.

74802-P502-80

AW 1800413



Manufacturer: NIDEK CO., LTD.



(21)PFX29217



SZ-1C BAUSCH+LOMB +20.00

(ϕ B) : 6.0mm

(ϕ T) : 13.0mm

SN PFX29217 EyeCee crystal preloaded

74802-P301-A0

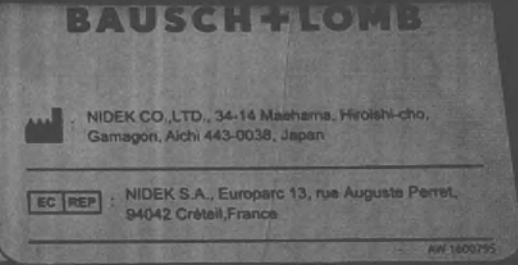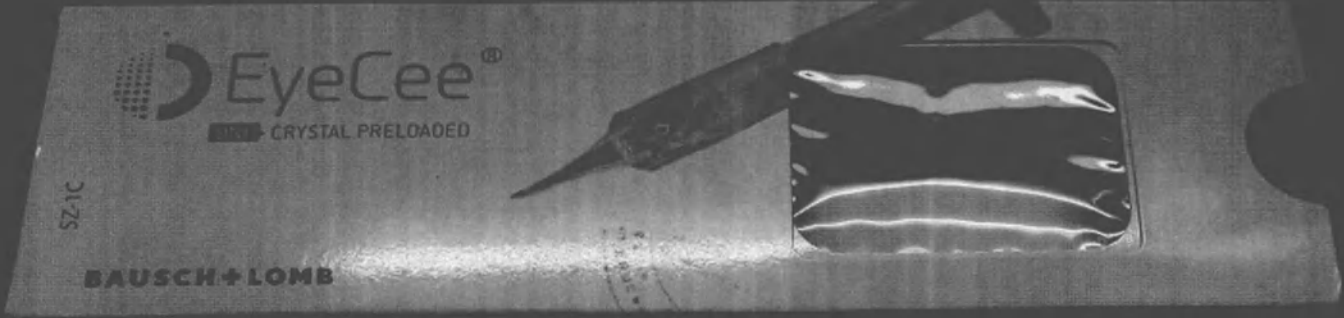

Method of Distribution
The EyeCee lens must be inserted in the eye as follows:

1. Preparation of the eye.
2. Insertion of the lens.
3. Removal of the lens.

Preparation of the eye
The eye must be prepared for the insertion of the lens. The eye must be washed with water and then with a solution of 3% hydrogen peroxide. The eye must be dried with a clean, dry cloth. The eye must be examined for any signs of infection or irritation. If any signs of infection or irritation are present, the eye must be treated with an appropriate eye drop before the lens is inserted.

Insertion of the lens
The lens must be inserted into the eye as follows:

1. The lens must be held between the thumb and index finger of the right hand.
2. The lens must be moved towards the eye.
3. The lens must be inserted into the eye.
4. The lens must be moved away from the eye.
5. The lens must be held between the thumb and index finger of the right hand.
6. The lens must be moved towards the eye.
7. The lens must be inserted into the eye.
8. The lens must be moved away from the eye.
9. The lens must be held between the thumb and index finger of the right hand.
10. The lens must be moved towards the eye.
11. The lens must be inserted into the eye.
12. The lens must be moved away from the eye.
13. The lens must be held between the thumb and index finger of the right hand.
14. The lens must be moved towards the eye.
15. The lens must be inserted into the eye.
16. The lens must be moved away from the eye.
17. The lens must be held between the thumb and index finger of the right hand.
18. The lens must be moved towards the eye.
19. The lens must be inserted into the eye.
20. The lens must be moved away from the eye.
21. The lens must be held between the thumb and index finger of the right hand.
22. The lens must be moved towards the eye.
23. The lens must be inserted into the eye.
24. The lens must be moved away from the eye.
25. The lens must be held between the thumb and index finger of the right hand.
26. The lens must be moved towards the eye.
27. The lens must be inserted into the eye.
28. The lens must be moved away from the eye.
29. The lens must be held between the thumb and index finger of the right hand.
30. The lens must be moved towards the eye.
31. The lens must be inserted into the eye.
32. The lens must be moved away from the eye.
33. The lens must be held between the thumb and index finger of the right hand.
34. The lens must be moved towards the eye.
35. The lens must be inserted into the eye.
36. The lens must be moved away from the eye.
37. The lens must be held between the thumb and index finger of the right hand.
38. The lens must be moved towards the eye.
39. The lens must be inserted into the eye.
40. The lens must be moved away from the eye.
41. The lens must be held between the thumb and index finger of the right hand.
42. The lens must be moved towards the eye.
43. The lens must be inserted into the eye.
44. The lens must be moved away from the eye.
45. The lens must be held between the thumb and index finger of the right hand.
46. The lens must be moved towards the eye.
47. The lens must be inserted into the eye.
48. The lens must be moved away from the eye.
49. The lens must be held between the thumb and index finger of the right hand.
50. The lens must be moved towards the eye.
51. The lens must be inserted into the eye.
52. The lens must be moved away from the eye.
53. The lens must be held between the thumb and index finger of the right hand.
54. The lens must be moved towards the eye.
55. The lens must be inserted into the eye.
56. The lens must be moved away from the eye.
57. The lens must be held between the thumb and index finger of the right hand.
58. The lens must be moved towards the eye.
59. The lens must be inserted into the eye.
60. The lens must be moved away from the eye.
61. The lens must be held between the thumb and index finger of the right hand.
62. The lens must be moved towards the eye.
63. The lens must be inserted into the eye.
64. The lens must be moved away from the eye.
65. The lens must be held between the thumb and index finger of the right hand.
66. The lens must be moved towards the eye.
67. The lens must be inserted into the eye.
68. The lens must be moved away from the eye.
69. The lens must be held between the thumb and index finger of the right hand.
70. The lens must be moved towards the eye.
71. The lens must be inserted into the eye.
72. The lens must be moved away from the eye.
73. The lens must be held between the thumb and index finger of the right hand.
74. The lens must be moved towards the eye.
75. The lens must be inserted into the eye.
76. The lens must be moved away from the eye.
77. The lens must be held between the thumb and index finger of the right hand.
78. The lens must be moved towards the eye.
79. The lens must be inserted into the eye.
80. The lens must be moved away from the eye.
81. The lens must be held between the thumb and index finger of the right hand.
82. The lens must be moved towards the eye.
83. The lens must be inserted into the eye.
84. The lens must be moved away from the eye.
85. The lens must be held between the thumb and index finger of the right hand.
86. The lens must be moved towards the eye.
87. The lens must be inserted into the eye.
88. The lens must be moved away from the eye.
89. The lens must be held between the thumb and index finger of the right hand.
90. The lens must be moved towards the eye.
91. The lens must be inserted into the eye.
92. The lens must be moved away from the eye.
93. The lens must be held between the thumb and index finger of the right hand.
94. The lens must be moved towards the eye.
95. The lens must be inserted into the eye.
96. The lens must be moved away from the eye.
97. The lens must be held between the thumb and index finger of the right hand.
98. The lens must be moved towards the eye.
99. The lens must be inserted into the eye.
100. The lens must be moved away from the eye.

Прошито и пронумеровано и
скреплено печатью 8 листа (ов)
Должность: Директор по регистрации в
России и странах СНГ Козлова Т.В.
Подпись Т.В. Козлова МП
« 27 » Август 2020 г.

