

УТВЕРЖДАЮ
Менеджер по регистрации и
контролю качества
ООО "Страйкер"
Моисеева А.В.




(Подпись)

28.09.2020

(Дата)



Фотографические изображения медицинского изделия
Система архивирования и управления данными Connected OR Hub

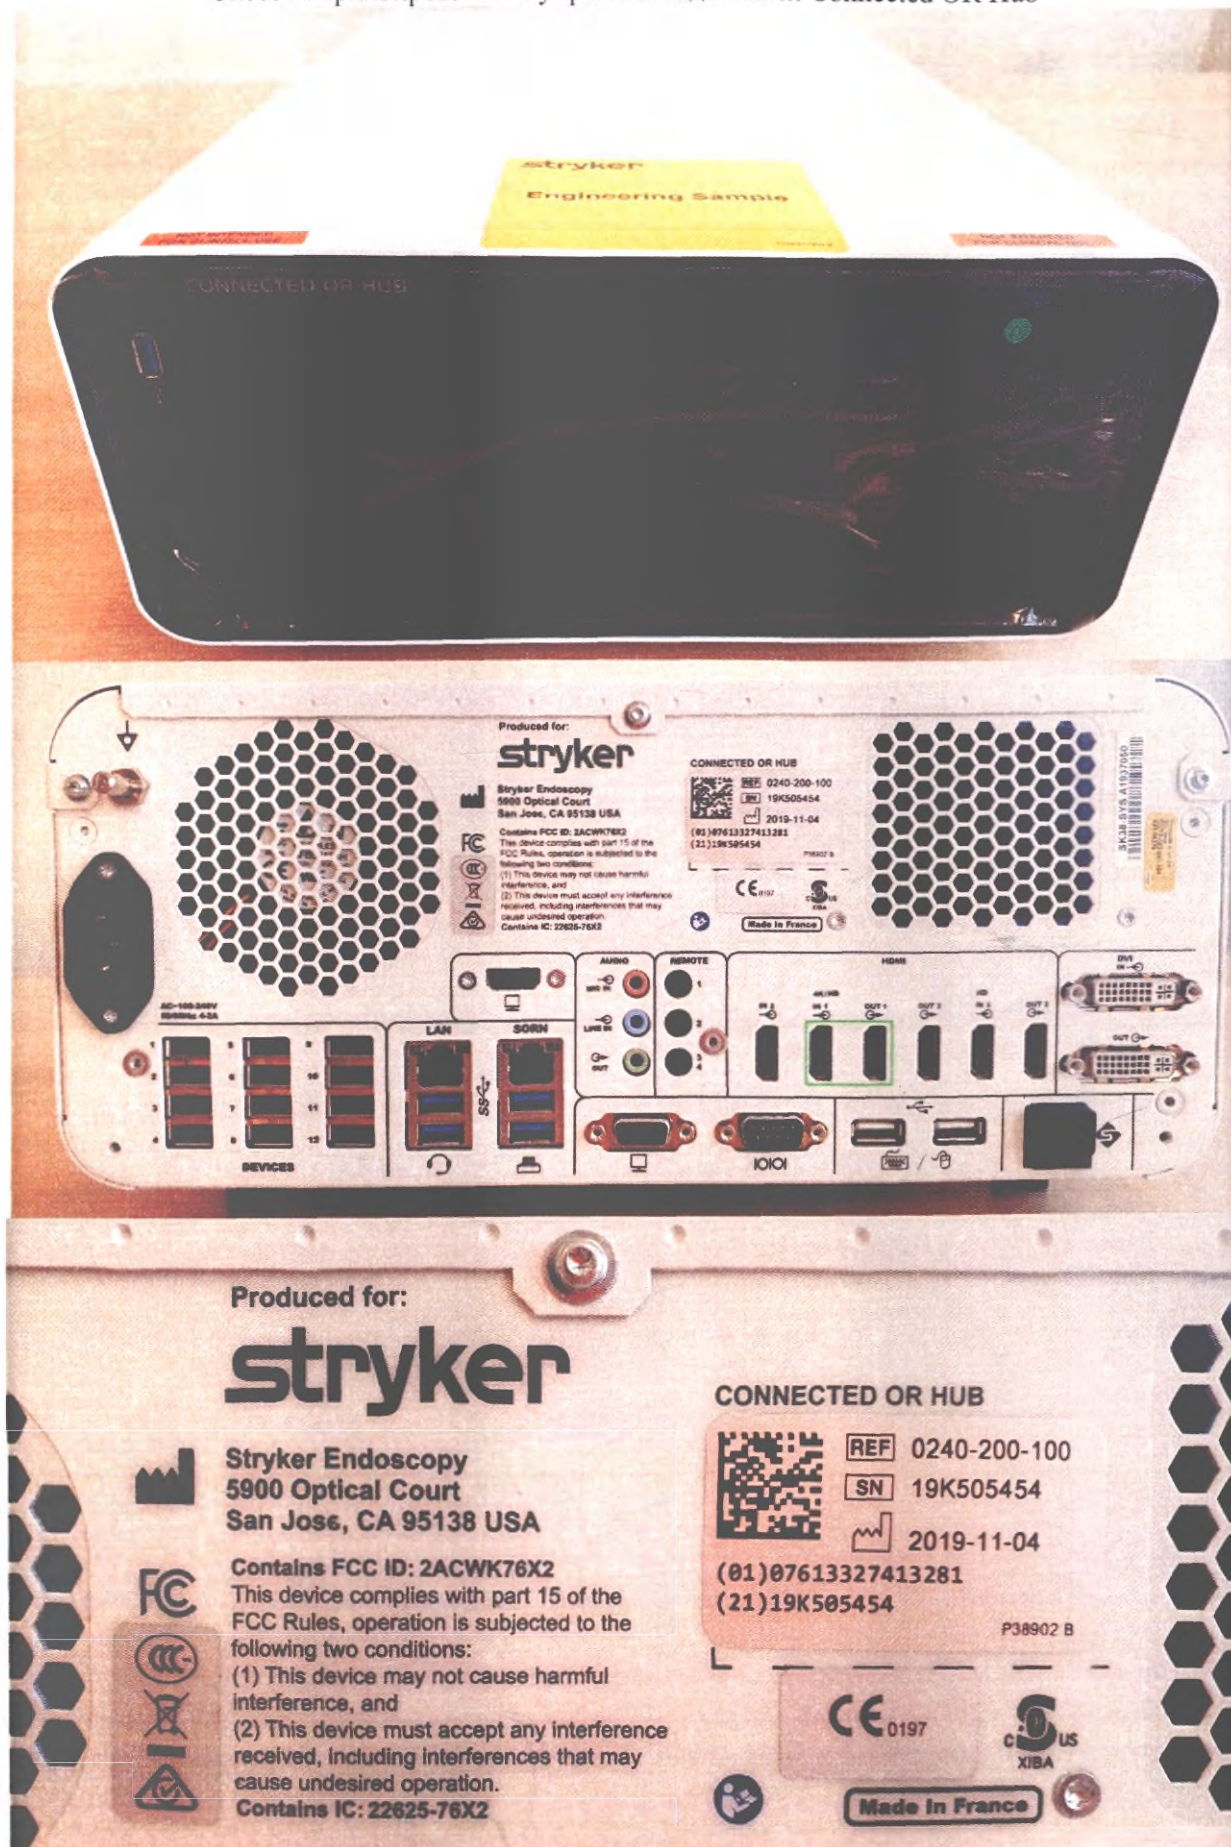

Windows® 10 IoT Ent
SAC Value
02219-083-841-164
X21-95375
Microsoft



SK38-SYS A1937050

stryker®



BREAKING THIS
SEAL VOIDS THE
MANUFACTURER'S
WARRANTY

1000-201-096

REV. G



C2G



C2G



C2G



C2G



stryker®

REF 0240-200-100

Catalogue number

Connected OR Hub

QTY 1

Quantity

R_x ONLY



Consult
instructions
for use



Caution see
instructions
for use

Made in
France



Produced for:

Stryker Endoscopy

5900 Optical Court

San Jose, CA 95138 USA

1-800-624-4422

REF 0240-200-100

Catalogue number

Connected OR Hub

QTY 1

Quantity



(01) 07613327413281

(21) 19K505454



Date of manufacture

2019-11-04

SN 19K505454

Serial number






(01)07613327413281(21)19K505454

U.S. Patents: www.stryker.com/patents

P35946 A

1. Консоль Connected OR Hub

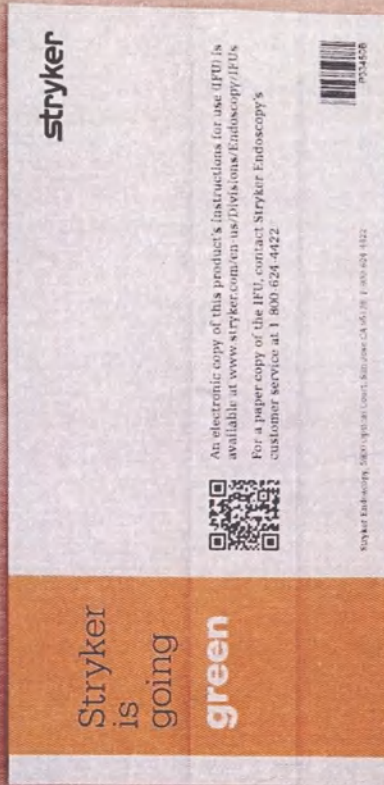

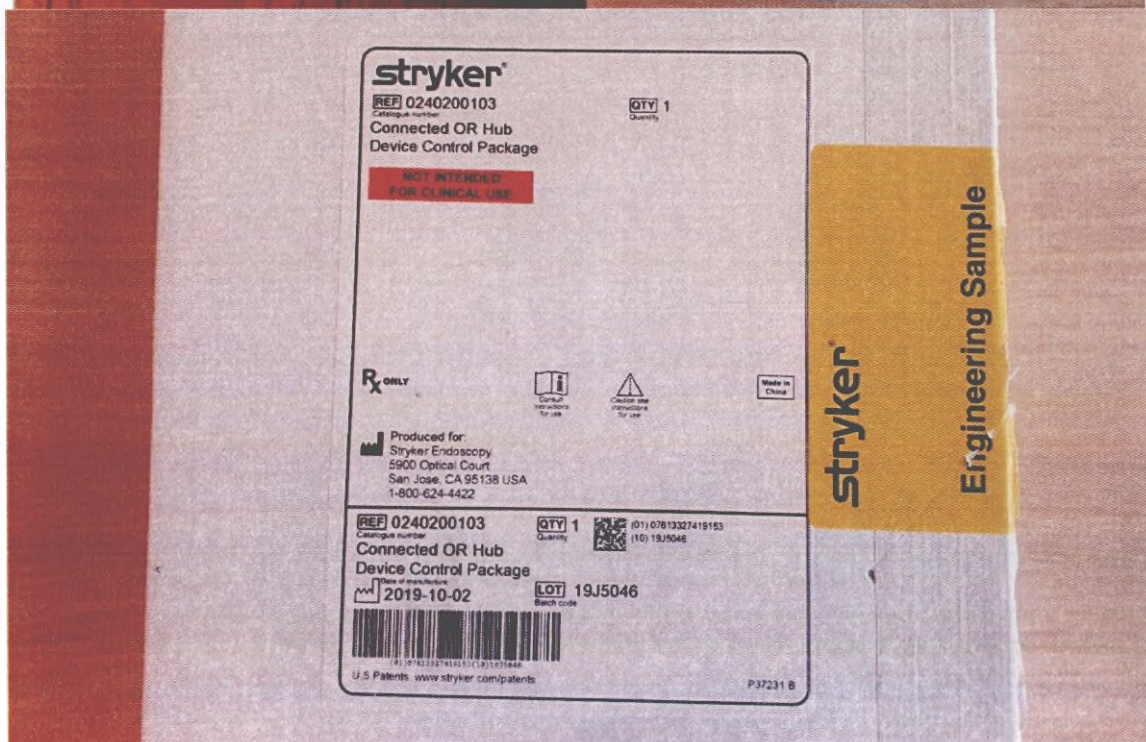

2. Пакет управления устройствами Connected OR Hub



Stryker
is
going
green

stryker



An electronic copy of this product's instructions for use (IFU) is available at www.stryker.com/en-us/Divisions/Endoscopy/IFUs
For a paper copy of the IFU, contact Stryker Endoscopy's customer service at 1-800-624-4422.



P33450B

Stryker Endoscopy, 5900 Optical Court, San Jose, CA 95138, 1-800-624-4422

stryker

**Warranty and
Return Policy**

REF 0240200102
Connected OR Hub
Voice Package
P37227 Rev. A

REF 0240200102



Connected OR Hub
Voice Package

P37227 Rev. A

USB 3.0





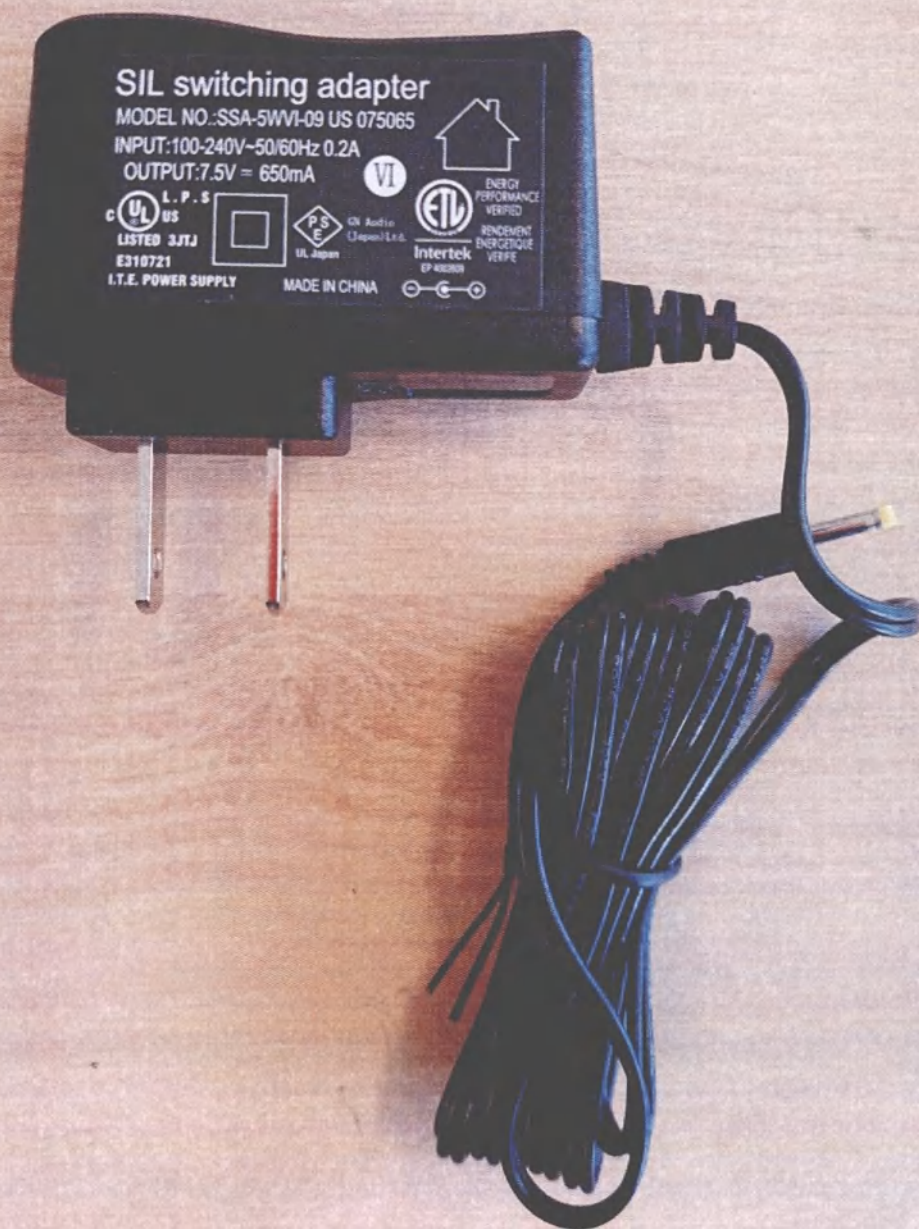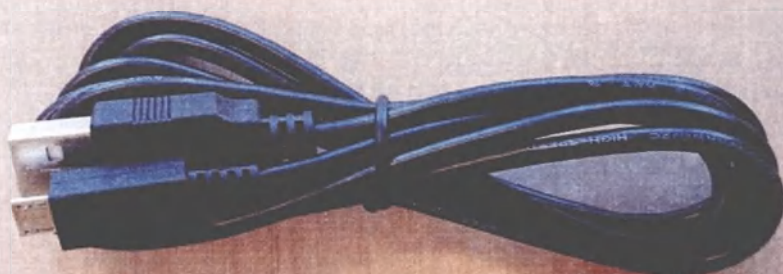

SIL switching adapter

MODEL NO.:SSA-5WVI-09 US 075065

INPUT:100-240V~50/60Hz 0.2A

OUTPUT:7.5V = 650mA



LISTED 3JTJ

E310721

I.T.E. POWER SUPPLY



UL Japan

GN Audio
(Japan) Ltd.

MADE IN CHINA




ENERGY
PERFORMANCE
VERIFIED

RENDIMENT
ENERGETIQUE
VERIFIE

Intertek

EP 400888



stryker

REF 0240200102

Catalogue number

Connected OR Hub
Voice Package

QTY 1

Quantity

NOT INTENDED
FOR CLINICAL USE

Rx ONLY



Consult
instructions
for use



Caution see
instructions
for use

Made in
China

Produced for:
Stryker Endoscopy
5900 Optical Court
San Jose, CA 95138 USA
1-800-624-4422

REF 0240200102

Catalogue number

Connected OR Hub
Voice Package

QTY 1

Quantity



(01) 07613327419146

(10) 19G5335

Date of manufacture
2019-07-22

LOT 19G5335

Batch code



(01)07613327419146(10)19G5335

U.S. Patents: www.stryker.com/patents

P37228 B

3. Пакет голосового управления Connected OR Hub

Stryker
is
going
green

stryker



An electronic copy of this product's instructions for use (IFU) is available at www.stryker.com/en-us/Divisions/Endoscopy/IFUs

For a paper copy of the IFU, contact Stryker Endoscopy's customer service at 1 800-624-4422.



P33450B

Stryker Endoscopy, 5900 Optical Court, San Jose CA 95138, 1-800-624-4422



stryker®

REF 0240200111

Catalogue number

Connected OR Hub
4K Recording Package

QTY 1

Quantity

**NOT INTENDED
FOR CLINICAL USE**

Rx ONLY



Consult
instructions
for use



Caution see
instructions
for use

USB - Made in Taiwan
Software Developed in the US



Produced for:
Stryker Endoscopy
5900 Optical Court
San Jose, CA 95138 USA
1-800-624-4422

REF 0240200111

Catalogue number

Connected OR Hub
4K Recording Package

QTY 1

Quantity



(01) 07613327460162

(10) 19J5646

(93) 1732719



Date of manufacture

2019-10-31

LOT 19J5646

Batch code



(01)07613327460162(10)19J5646

U.S. Patents: www.stryker.com/patents

P41046 C

Stryker
is
going
green

stryker



An electronic copy of this product's instructions for use (IFU) is available at www.stryker.com/en-us/Divisions/Endoscopy/IFUs

For a paper copy of the IFU, contact Stryker Endoscopy's customer service at 1-800-624-4422.

Stryker Endoscopy, 5900 Optical Court, San Jose CA 95138, 1-800-624-4422



P33450B



stryker®

REF 0240200106

Catalogue number

Connected OR Hub

DICOM Package

QTY 1

Quantity

**NOT INTENDED
FOR CLINICAL USE**

R_x ONLY



Consult
instructions
for use



Caution see
instructions
for use

USB - Made in Taiwan
Software Developed in the US



Produced for:

Stryker Endoscopy

5900 Optical Court

San Jose, CA 95138 USA

1-800-624-4422

REF 0240200106

Catalogue number

Connected OR Hub

DICOM Package

QTY 1

Quantity



(01) 07613327459593

(10) 19J5085

(93) 1725489



Date of manufacture:

2019-10-03

LOT 19J5085

Batch code



(01)07613327459593(10)19J5085

U.S. Patents: www.stryker.com/patents

P37240 C

5. Программное обеспечение DICOM для Connected OR Hub



6. Кабель VPI



7. Кабель HDMI




8. Кабель HDMI высокоскоростной



9. Кабель питания

10. Кабель USB A-B

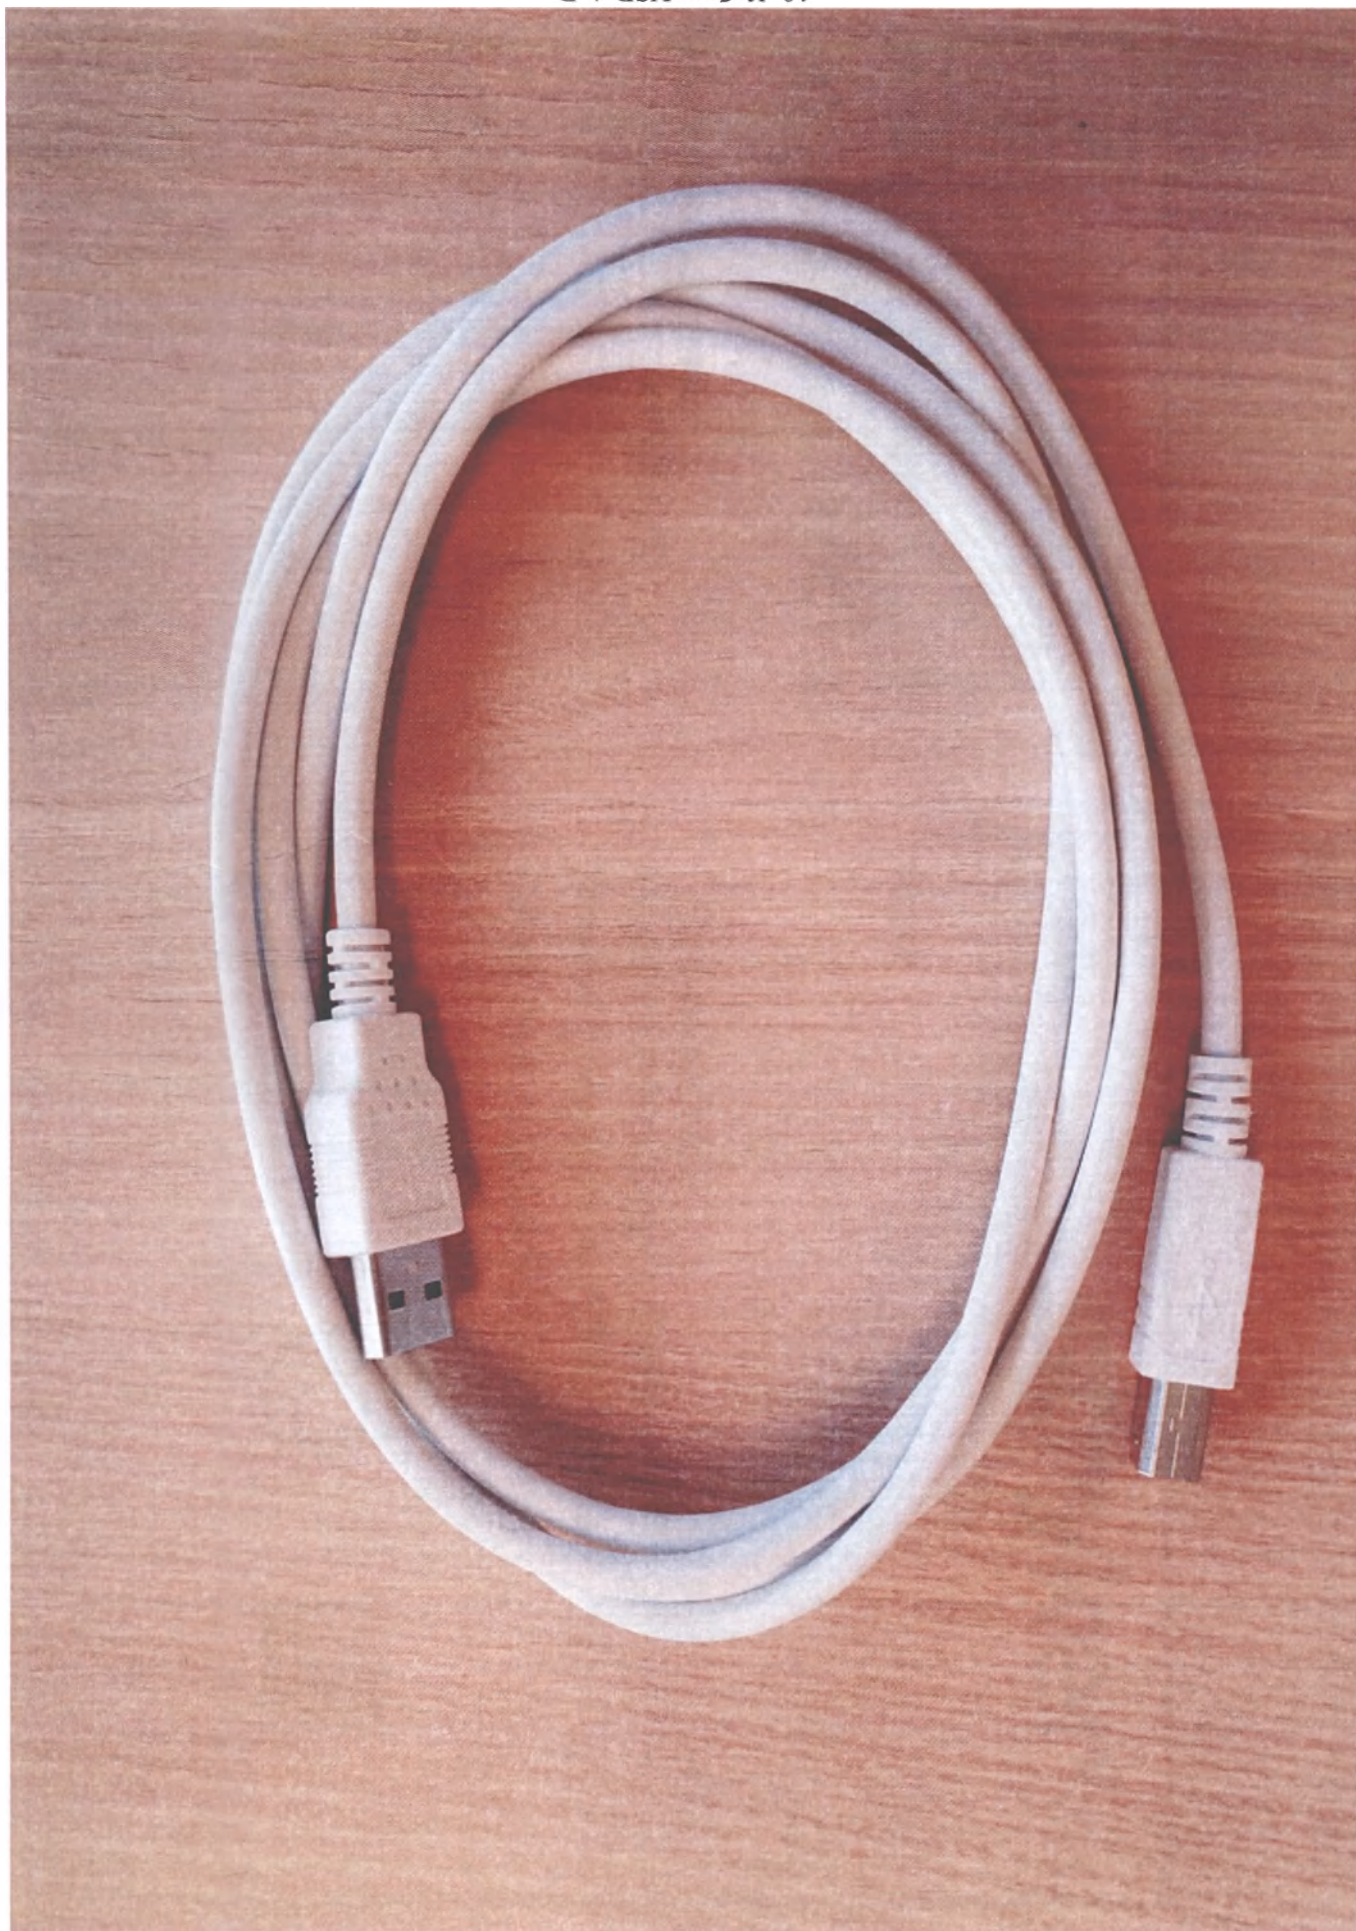

REF

240200100

LOT

№ PЗН

от

года

Консоль Connected OR Hub

Место производства:

XXXXXXX

Производитель:

Stryker Endoscopy, a Division of
Stryker Corporation, 5900 Optical
Court, San Jose CA 95138, USA


stryker[®]

Design





Пример упаковки Connected OR Hub

Прошнуровано, пронумеровано и
скреплено печатью 23 листа (ов)
Менеджер по регистрации и контролю
качества ООО «Страйкер»
 А.В. Моисеева
По доверенности б/н от 4.07.2019 г