

Генеральный директор

ООО "Адвamedics"

Сухарев И.В.



2020г.

Наборы для катетеризации центральных вен NOVOCENT(НОВОЦЕНТ)

Фотографические изображения медицинского изделия

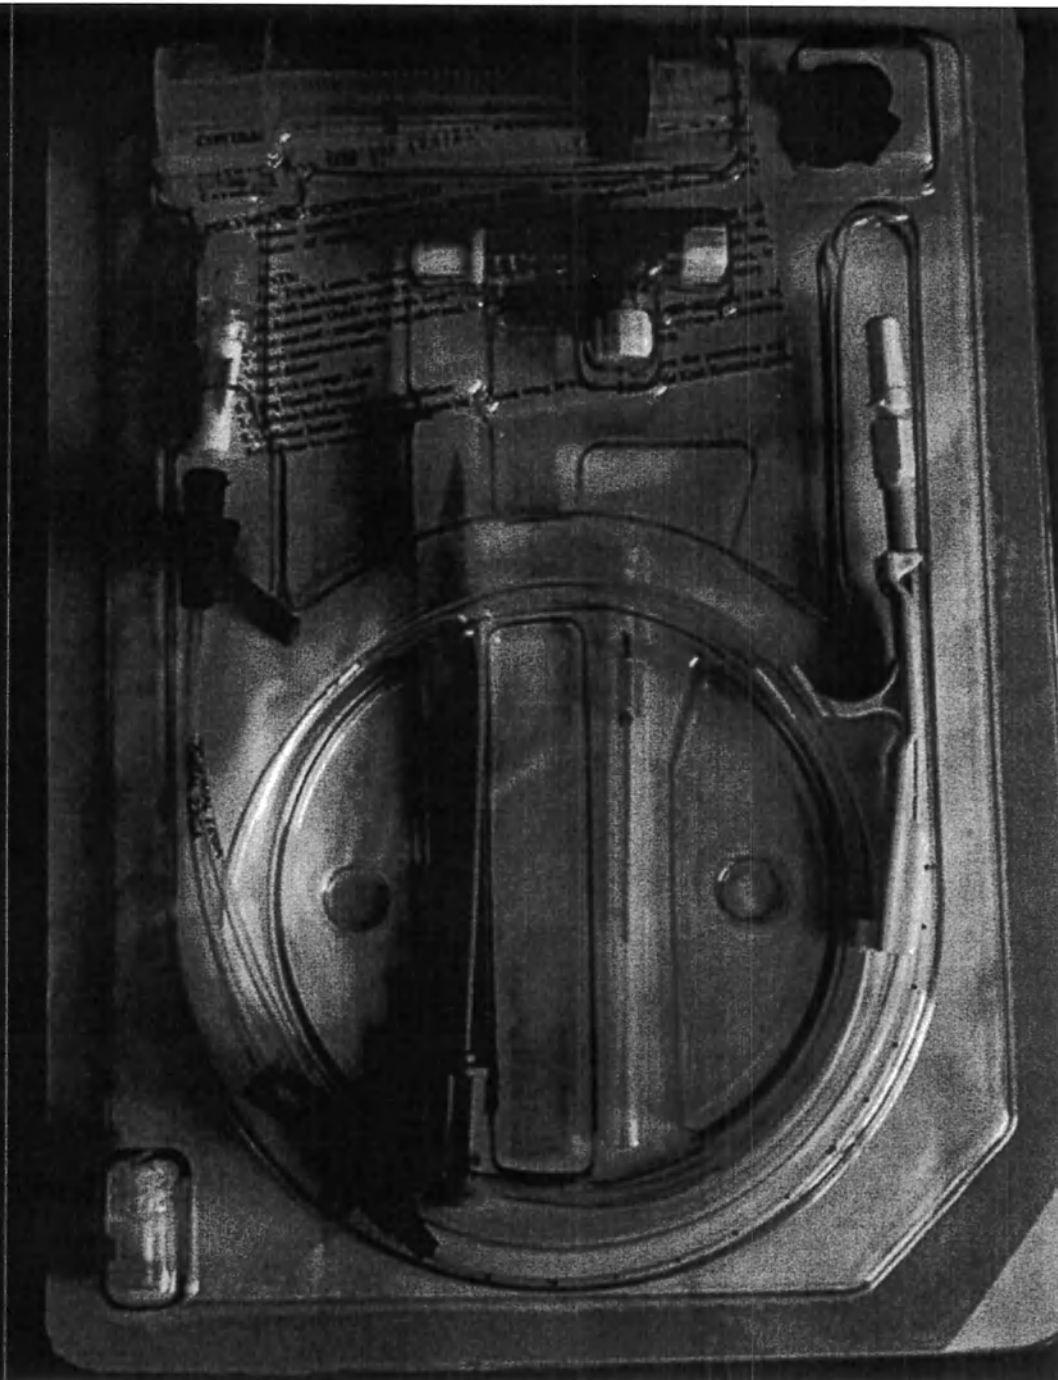
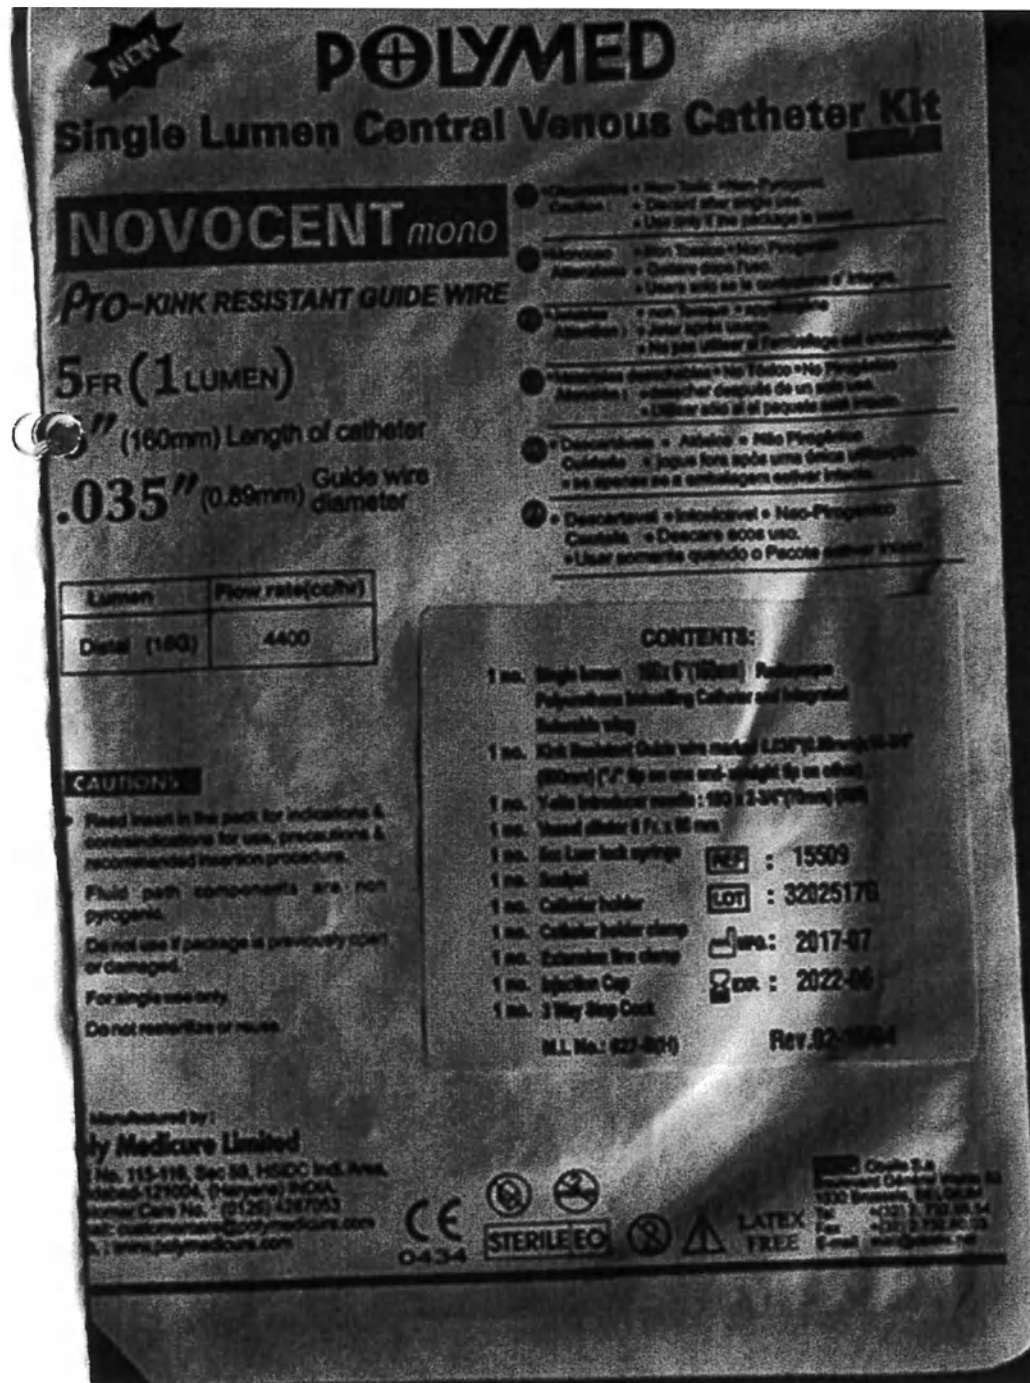


Фото 1- Набор для катетеризации центральных вен «Novocent Pro mono» (Новосецт про моно), однопросветный

CONTENTS

- 1 no. Single lumen Introducing Catheter
39 x 6" (100cm) Polyurethane
With Ball tip
- 1 no. No Needle Side arm set 6.5" (16.5cm) 18-24"
(50cm) ("J" tip on one and straight tip on other)
- 1 no. Introducer needle 20G x 1-1/2" (50cm) (114)
- 1 no. Vessel dilator 4 Fr x 90mm
- 1 no. Sea-Lock Syringe
- 1 no. Scalpel With long handle
- 1 no. Catheter holder
- 1 no. Catheter holder clamp
- 1 no. Extension line clamp
- 1 no. 200cc stopcock
- 1 no. Injection cap

Ref. No.: 15503

LOT: 8. NO: 33871

MFG: 2017-08

EXP: 2022-07

Manufactured by:

POLY MEDICURE LTD.
Plot No. 115-116 Sec-44, MIDC Ind. Estate,
Faridabad - 121004, (Haryana) INDIA
Customer Care No.: (0129) 4287093
M.L.NO.: 627-B(H)

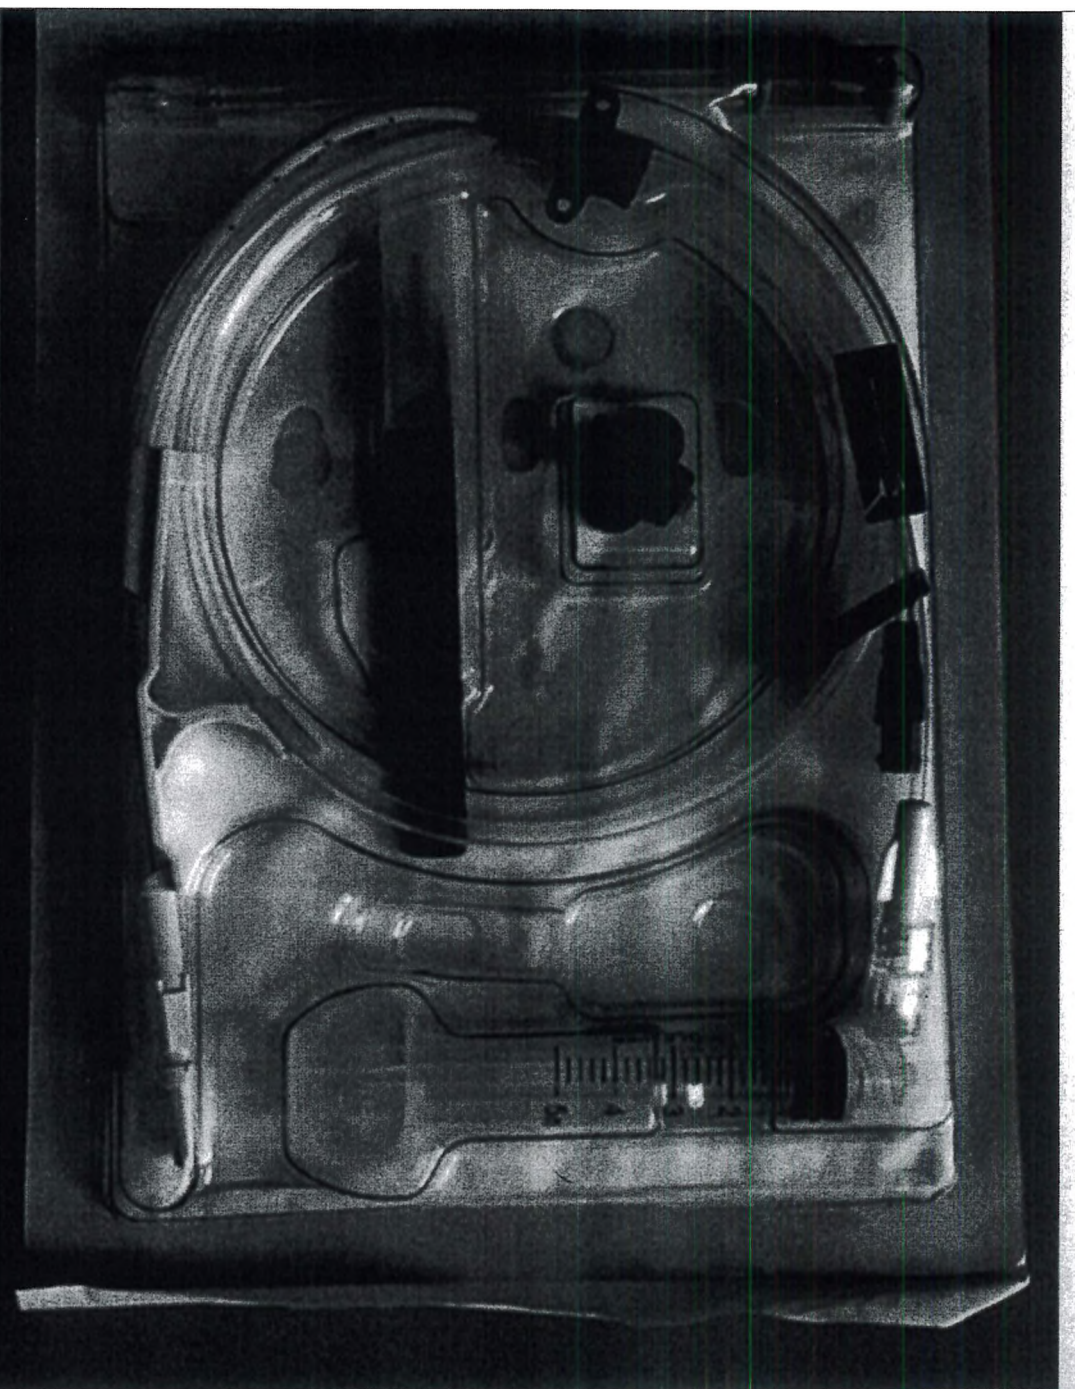


Фото 2- Набор для катетеризации центральных вен «Novocent mono» (Новосент моно) однопросветный

Double Lumen Central Venous Catheter Kit

NOVOCENT duo

PRO-KINK RESISTANT GUIDE WIRE

4 FR (2 LUMEN)

6" (160mm) Length of catheter

0.018" (0.46mm) Guide wire diameter



Lumen	Flow rate(cc/hr)
Distal (230)	1800
Proximal (230)	1800

CAUTIONS:

- Read insert in the pack for indications & contraindications for use, precautions & recommended insertion procedure.
- Fluid path components are not pyrogenic.
- Do not use if package is previously open or damaged.
- For single use only.
- Do not resterilize or reuse.

- **Dispositivo** - Non Toxic - Non-Pyrogenic
Caution - • Discard after single use
 • Use only if the package is intact.
- **Atenção** - Não Tóxico - Não Piropégeno
Atenção - • Descarte após uso único
 • Usar só se a embalagem estiver intacta.
- **Dispositivo** - Non Toxic - Non-Pyrogenic
Atenção - • Discard after single use
 • Use only if the package is intact.
- **Dispositivo** - Non Toxic - Non-Pyrogenic
Atenção - • Discard after single use
 • Use only if the package is intact.
- **Dispositivo** - Non Toxic - Non-Pyrogenic
Atenção - • Discard after single use
 • Use only if the package is intact.
- **Dispositivo** - Non Toxic - Non-Pyrogenic
Atenção - • Discard after single use
 • Use only if the package is intact.

CONTENTS

- 1 no. Two lumen Indwelling Catheter
 4Fr x 6" (160mm) Radiopaque polyurethane
 With Lock tip
- 1 no. Kink resistant Guide wire marked 5" (127.46mm) x 0.018"
 (500mm) ("V" tip on one end straight tip on other)
- 1 no. Introducer needle 20Gx1 1/2" (38mm) (P/V)
- 1 no. Vessel dilator 5 Fr x 70mm
- 1 no. 5cc Luer lock Syringe
- 1 no. Scalpel
- 1 no. Catheter holder
- 1 no. Catheter holder clamp
- 2 nos. Injection cap
- 2 nos. Extension line clamps
- 1 no. 3 Way Stop Cock

REF 15531

LOT 32025190

MFG. 2012

EXP. 2015

M.L. NO 627-B(H)

Rev.02-2004

Manufactured by:

Polymed Limited

Plot No. 115-116, Sec 59, HSIIDC Ind. Area,
 Industrial Estate, (Gurgaon) Haryana
 India
 Phone No. : (0129) 4297083
 Fax : (0129) 4297083
 E-mail : customerservice@polymed.com
 Website : www.polymed.com



Polymed Limited
 Plot No. 115-116, Sec 59, HSIIDC Ind. Area,
 Industrial Estate, (Gurgaon) Haryana
 India
 Phone No. : (0129) 4297083
 Fax : (0129) 4297083
 E-mail : customerservice@polymed.com
 Website : www.polymed.com

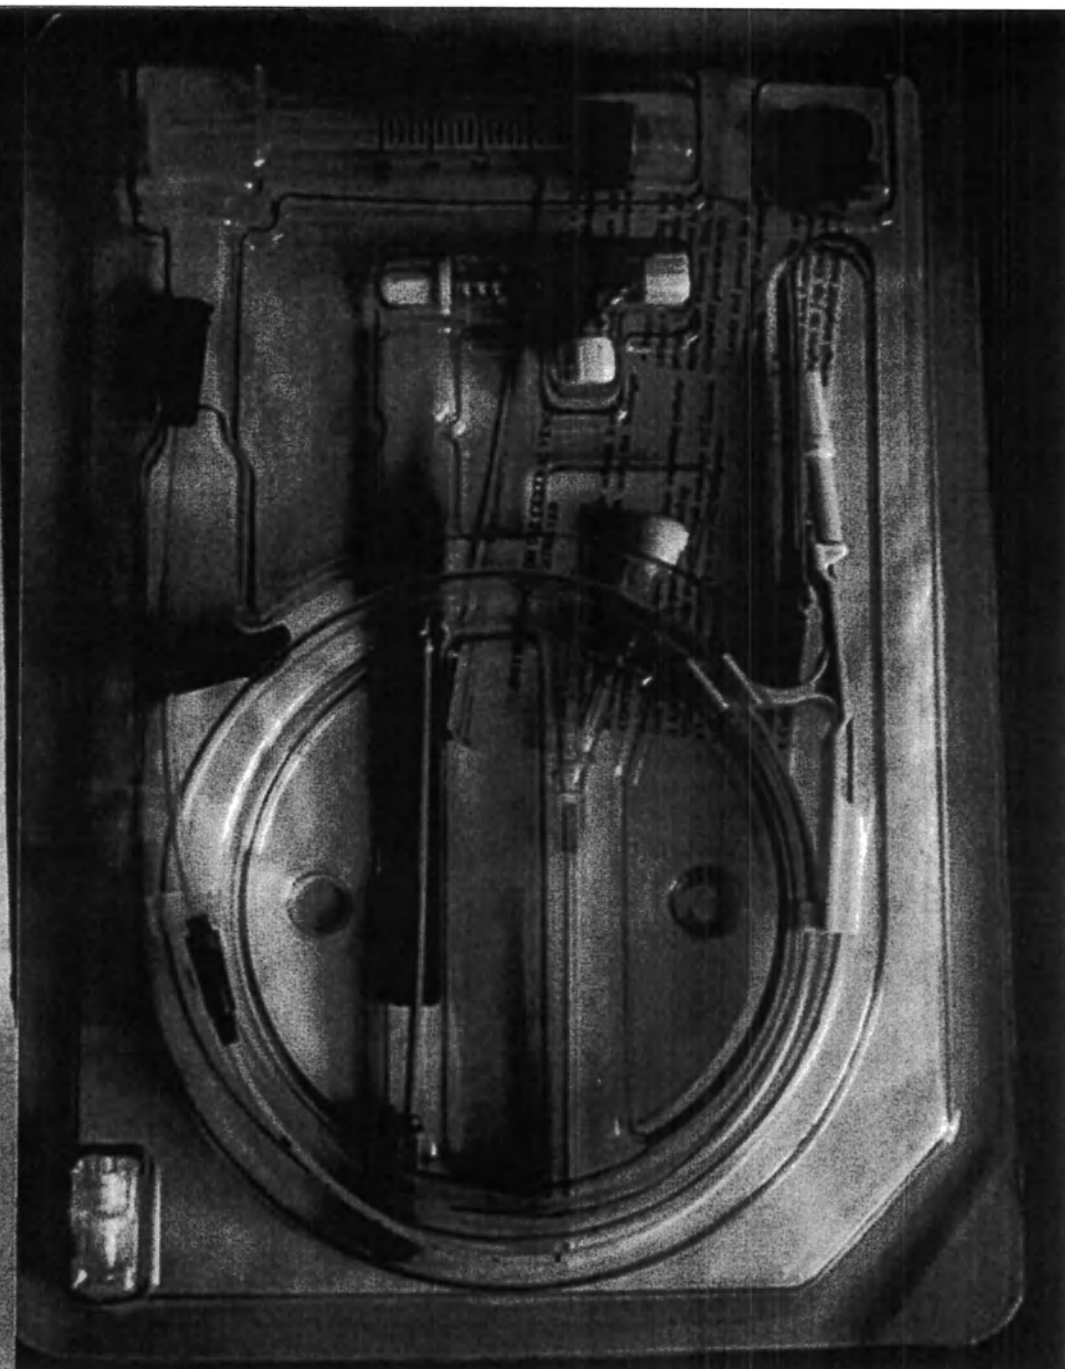


Фото 3- Набор для катетеризации центральных вен «Novocent Pro duo» (Новоцент про дуо) двухпросветный

POLYMED

Double Lumen Central Venous Catheter Kit

NOVOCENT duo

7FR 2 LUMEN 6 inches (160mm)
length of catheter

.035" (0.89mm) Guide
wire diameter

CAUTIONS

- Read insert in the pack for indications & contraindications for use, precautions & recommended insertion procedure.
- Fluid path components are non pyrogenic.
- Do not use if package is previously opened or damaged.
- For single use only.
- Do not resterilize or reuse.

COBALT S.r.l.
Boulevard Général Wauters 53
1030 Brussels, BELGIUM
Tel: +32(0)2 732.99.34
Fax: +32(0)2 732.99.03
E-mail: mail@cobalt.be

Manufactured by
Poly Medcare Limited

Plot No. 115-116, Sec. 38, MIDC Ind. Area,
Pune-411 004, (Maharashtra) INDIA
Customer Care No.: (020) 4281103
E-mail: customercare@polymedcare.com

- Contraindications: Non Thrombolytic, Non Painless, Non Pyrogenic, Non Sterile, Non Reusable, Non Disposable, Non Single Use, Non Single Patient Use, Non Single Room Use, Non Single Ward Use, Non Single Department Use, Non Single Hospital Use, Non Single Country Use, Non Single Continent Use, Non Single World Use.
- Warnings: Do not use if package is damaged or expired, Do not use if the catheter is kinked or bent, Do not use if the catheter is blocked or occluded, Do not use if the catheter is leaking or dripping, Do not use if the catheter is discolored or stained, Do not use if the catheter is contaminated or dirty, Do not use if the catheter is exposed to heat or cold, Do not use if the catheter is exposed to radiation or other sources of energy, Do not use if the catheter is exposed to chemicals or other substances, Do not use if the catheter is exposed to moisture or humidity, Do not use if the catheter is exposed to air or oxygen, Do not use if the catheter is exposed to light or UV radiation, Do not use if the catheter is exposed to magnetic fields or other electromagnetic interference, Do not use if the catheter is exposed to static electricity or other electrical fields, Do not use if the catheter is exposed to mechanical stress or strain, Do not use if the catheter is exposed to vibration or shock, Do not use if the catheter is exposed to pressure or vacuum, Do not use if the catheter is exposed to tension or compression, Do not use if the catheter is exposed to bending or twisting, Do not use if the catheter is exposed to stretching or pulling, Do not use if the catheter is exposed to crushing or squeezing, Do not use if the catheter is exposed to cutting or tearing, Do not use if the catheter is exposed to puncturing or piercing, Do not use if the catheter is exposed to crushing or squeezing, Do not use if the catheter is exposed to cutting or tearing, Do not use if the catheter is exposed to puncturing or piercing.



Lumen	Flow rate (cc/hr)
Distal (160)	4200
Proximal (160)	3100

CONTENTS:

- 1 no. Two lumen Intubating Catheter
7Fr x 6" (160mm) Radiopaque
Polyurethane with soft tip
- 1 no. Guide wire marked 0.035" (0.89mm) x 18-34"
(600mm) ("J" tip on one end, straight tip on other)
- 1 no. Y-Valve Introducer needle: 18G x 1-3/4" (76mm) (RW)
- 1 no. Vessel dilator 8 Fr x 100mm
- 1 no. Ice/Luar lock syringe **REF**: 15055
- 1 no. Scalpel **LOT**: 3234817H
- 1 no. Catheter holder **REF**: 2017-08
- 1 no. Catheter holder clamp **REF**: 2022-07
- 2105. Injection cap
- 2005. Extension line clamps

M.L. No.: 827-80(1)

Rev. 01-1992



Фото 4- Набор для катетеризации центральных вен «Novocent duo» (Новоцент дуо) двухпросветный

Triple Lumen Central Venous Catheter Kit

NOVOCENT trio

Pro-KINK RESISTANT GUIDE WIRE

5.5FR (3 LUMEN)

6" (160mm) Length of catheter

.018" (0.46mm) Guide wire diameter



Lumen	Flow rate(cc/hr)
Distal (20G)	1500
Medial (22G)	250
Proximal (22G)	200

CAUTIONS:

- Read insert in the pack for indications & contraindications for use, precautions & recommended insertion procedure.
- Fluid path components are non pyrogenic.
- Do not use if package is previously open or damaged.
- For single use only.
- Do not resterilize or reuse.

- Contraindications: Non-Tolerant, Non-Pyrogenic, Catheter:
 - Discontinue after single use.
 - Use only if the package is intact.
- Warnings:
 - Non-Tolerant, Non-Pyrogenic, Catheter:
 - Discontinue after single use.
 - Use only if the package is intact.
- Indications:
 - Non-Tolerant, Non-Pyrogenic, Catheter:
 - Discontinue after single use.
 - Use only if the package is intact.
- Material:
 - Non-Tolerant, Non-Pyrogenic, Catheter:
 - Discontinue after single use.
 - Use only if the package is intact.
- Disinfection:
 - Non-Tolerant, Non-Pyrogenic, Catheter:
 - Discontinue after single use.
 - Use only if the package is intact.
- Decontamination:
 - Non-Tolerant, Non-Pyrogenic, Catheter:
 - Discontinue after single use.
 - Use only if the package is intact.

CONTENTS

- 1 no. Triple Lumen Indwelling Catheter 5.5Fr x 6" (160mm) Polyurethane with Ball tip
- 1 no. Pre-sterilized Guide wire 0.018" (0.46mm) x 16" (406mm) (7" (17.8cm) in one end straight by an other)
- 1 no. Introducer needle 20G x 1/2" (12.7mm) (114)
- 1 no. Ventral Filter 6 Fr x 80mm
- 1 no. Sea-Lock Lock Syringe
- 1 no. Syringe
- 1 no. Catheter holder
- 1 no. Catheter holder clamp
- 2 nos. Injection cap
- 2 nos. Extension line clamps
- 1 no. J-Way Stop Cock

REF: 15561
LOT: 3244817H
MFG: 2817-08
EXP: 2822-07

Manufactured by:
POLY MEDICURE LTD.
Plot No. 115-116, Sec 59, HSIIDC Ind. Area,
Faridkot - 151004, (Punjab) INDIA
Customer Care No. (0151) 4267053

Manufactured by:
Poly Medisure Limited

Plot No. 115-116, Sec 59, HSIIDC Ind. Area,
Faridkot - 151004, (Punjab) INDIA
Customer Care No. (0151) 4267053
E-mail: customercare@polymedisure.com
Web: www.polymedisure.com

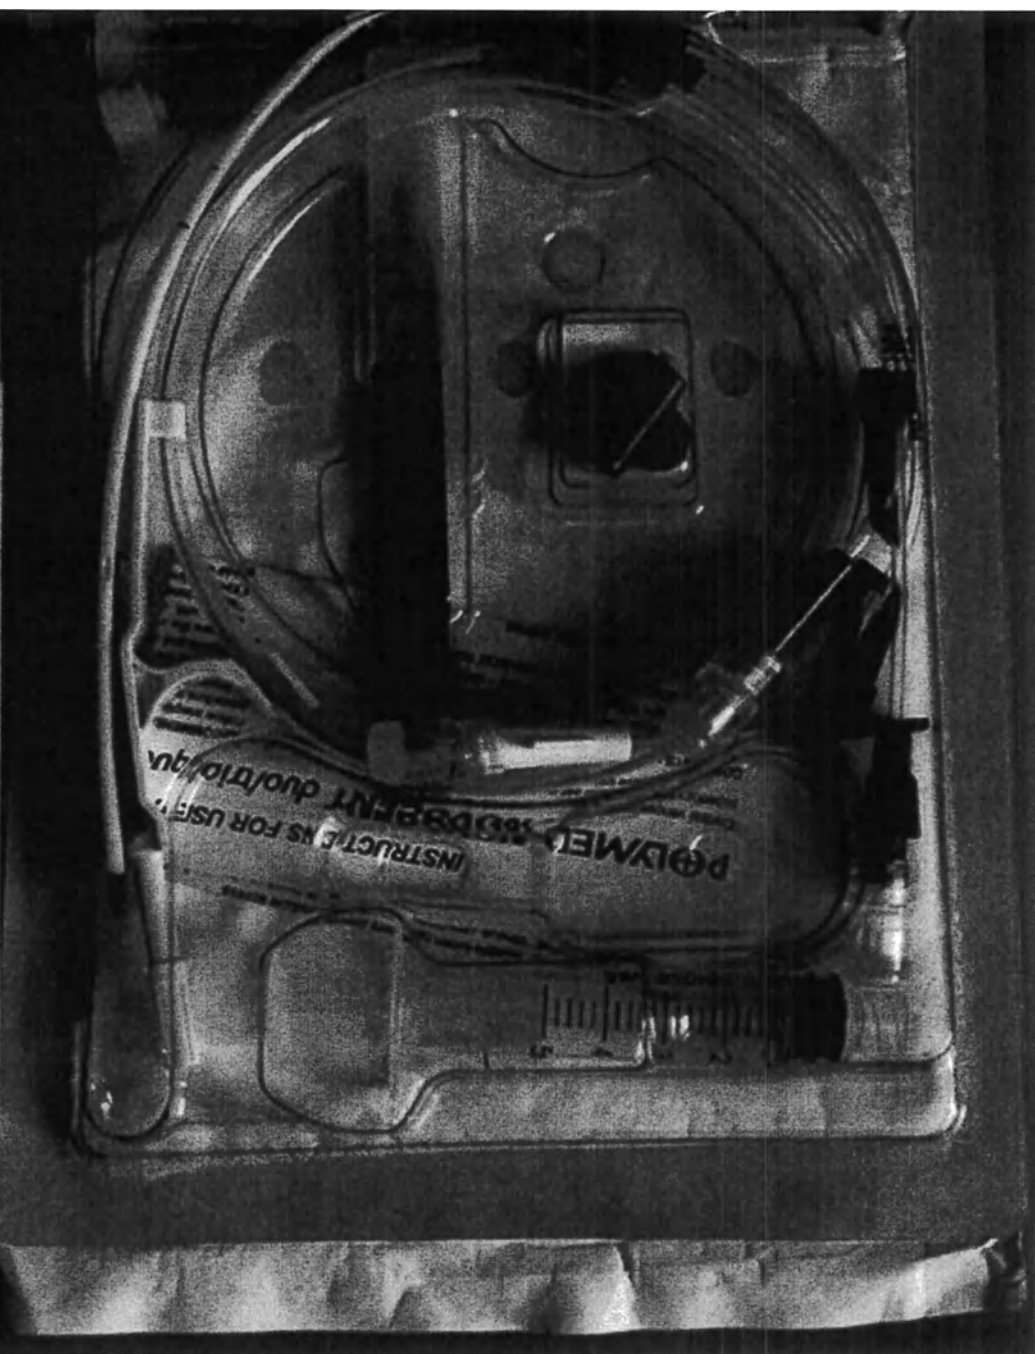


Фото 5 - Набор для катетеризации центральных вен «Novocent Pro trio» (Новоцент про трио) трехпросветный

POLYMED

Triple Lumen Central Venous Catheter Kit

NOVOCENT trio

5.5 FR 3 LUMEN 6 Inches (150mm)
Length of catheter

.018" (0.46mm) Guide
wire diameter

CAUTIONS:


- Read insert in the pack for indications & contraindications for use, precautions & recommended insertion procedure.
- Fluid path components are non pyrogenic.
- Do not use if package is previously open or damaged.
- For single use only.
- Do not reuse or reuse.

COBOL Obols S.A.
Boulevard Général Wavre 53
1030 Brussels, BELGIUM
Tel : +32(2) 2.732.88.54
Fax : +32(2) 2.732.80.03
E-mail : mail@obols.net

Manufactured by:
Poly Medcare Limited

Plot No. 115-116, Sec. 58, MIDC Ind. Area,
Fardesh, 421004, (Pune) INDIA
Customer Care No. : 01291 4387053
E-mail : sales@polymedcare.com
Web : www.polymedcare.com

- **Contraindications:** • Non Sterile • Non Pyrogenic
Cautions : • Observe shelf life only
• Use only if the package is intact
- **Warnings:** • Non Sterile • Non Pyrogenic
• Attention : • Catheter design : • Intended only for use in conjunction with a syringe
- **Indications:** • Non Sterile • Non Pyrogenic
• Attention : • Intended for use in conjunction with a syringe
- **Instructions:** • Non Sterile • Non Pyrogenic
• Attention : • Intended for use in conjunction with a syringe



Lumen	Flow rate (ml/min)
Distal (20G)	1800
Medial (22G)	250
Proximal (22G)	200

CONTENTS

- 1 no. Three lumen Indwelling Catheter
5.5 Fr x 6" (150mm) Radiopaque polyurethane
With Soft tip
- 1 no. Guide wire marked 0.018" (0.46mm) x 19-3/4"
(500mm) ("J" tip on one end and straight tip on other)
- 1 no. Introducer needle 20G x 1-1/2" (38mm) (RW)
- 1 no. Vessel dilator 5 Fr x 80mm
- 1 no. Sea Luer lock Syringe
- 1 no. Scalpel
- 1 no. Catheter holder
- 1 no. Catheter holder clamp
- 1 no. Injection cap
- 1 no. Extension line clamp

Ref. No.: 15101

LOT B.NO: 3218917H

MFG: 2017-08
EXP: 2022-07

M.L.NO.: 627-B(M)

Rev. 06/2016/04

STERILE EO




CE
0434

LATEX
FREE



Фото 6 - Набор для катетеризации центральных вен «Novocent trio» (Новоцент трио) трехпросветный

2

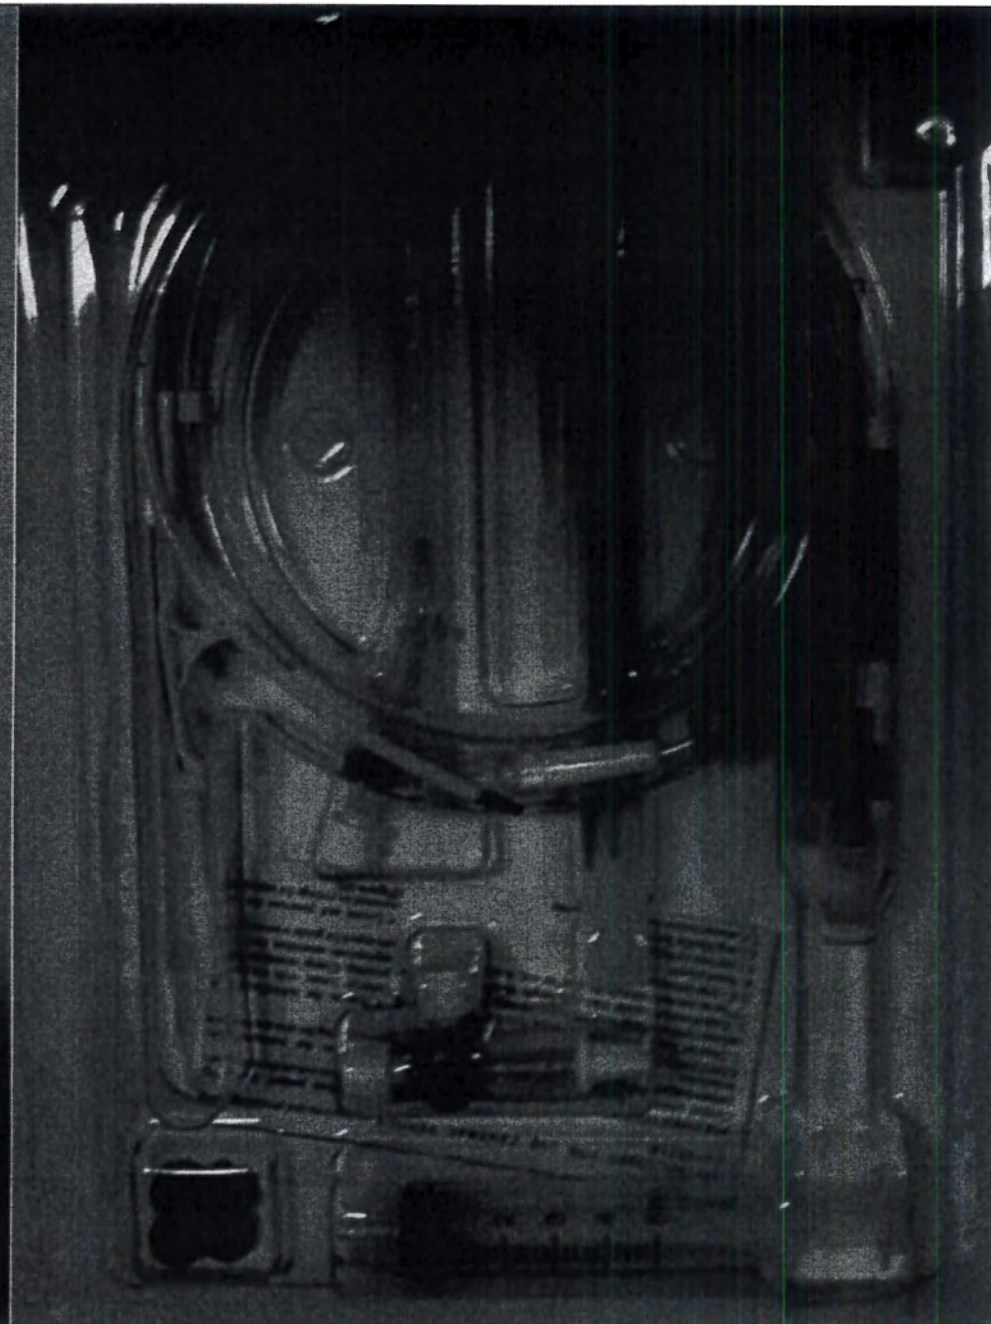

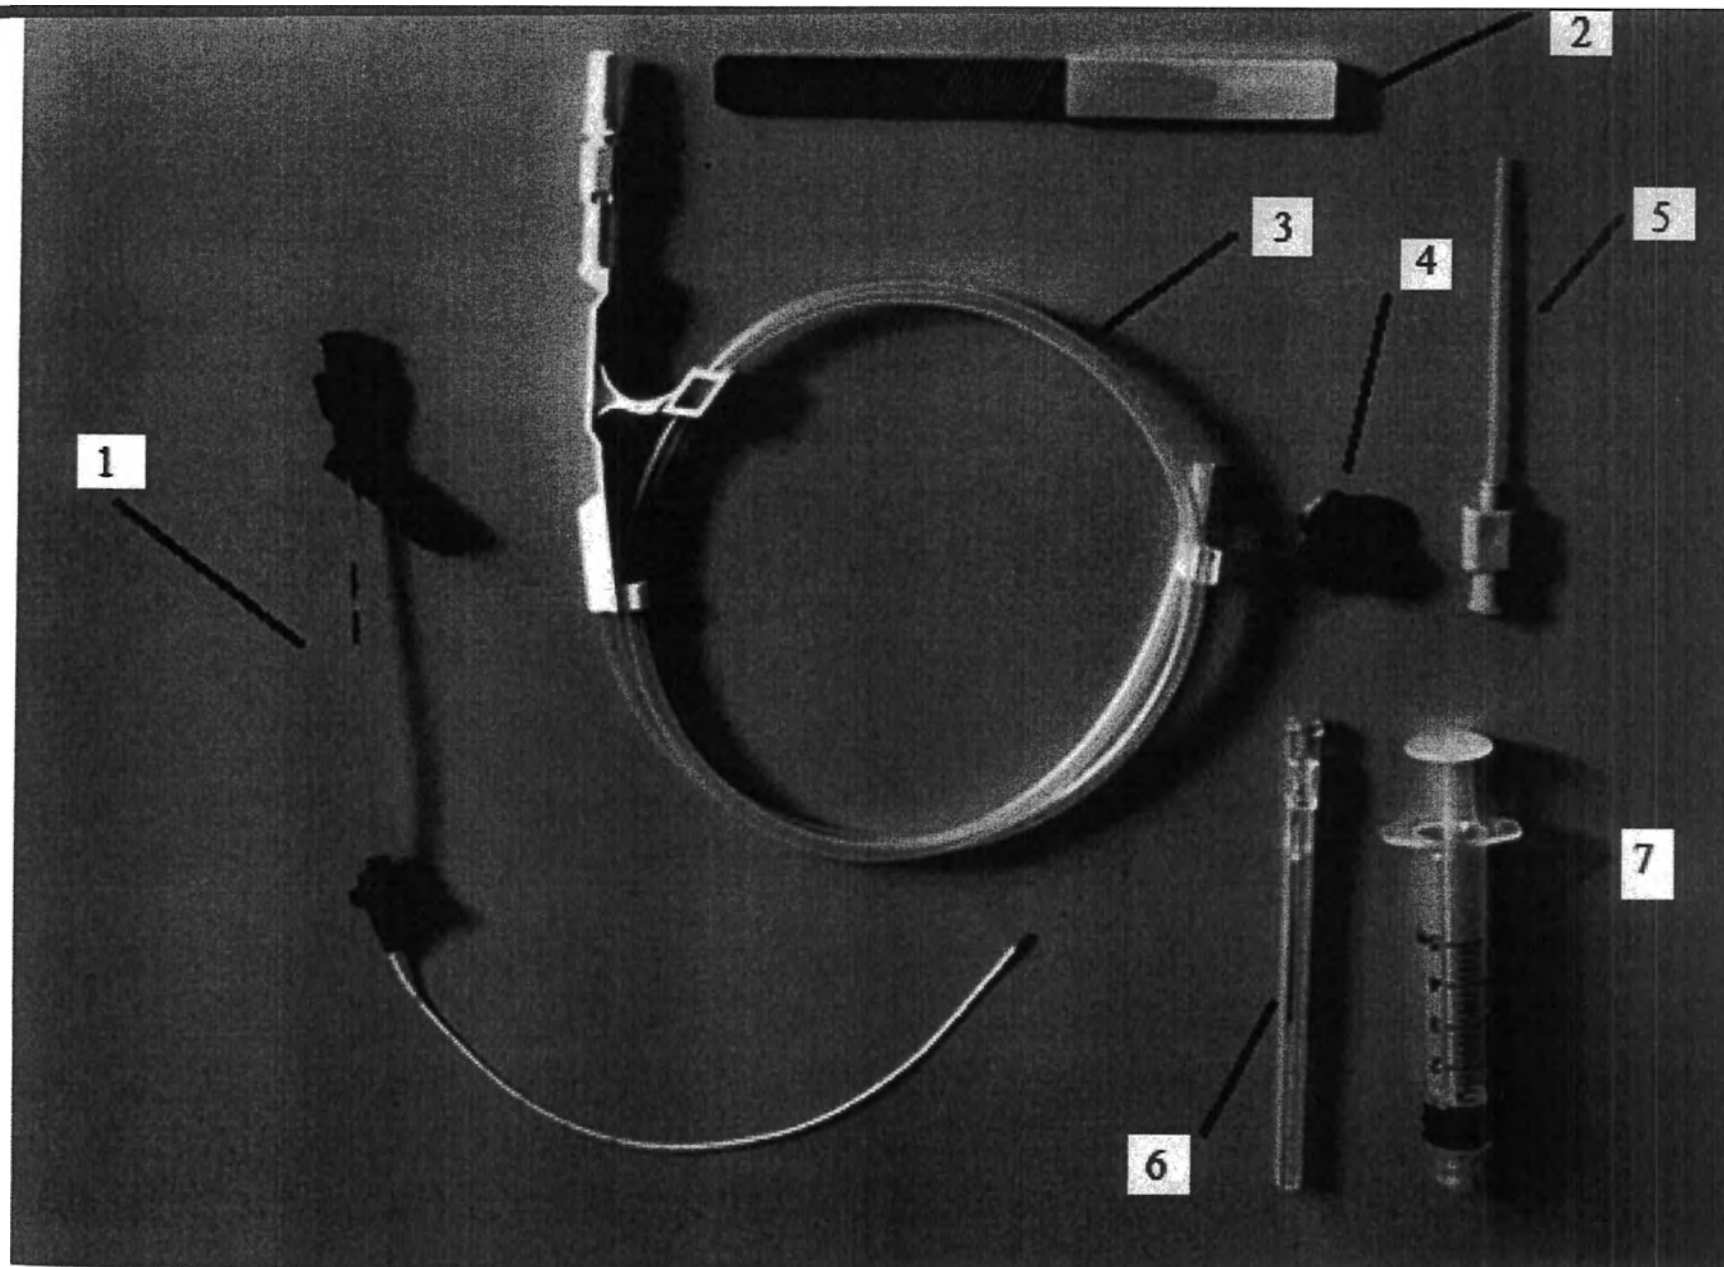


Фото 8 – Состав набора «Novocent mono» (Новоцент моно) однопросветный:

однопросветной катетер, проводочный проводник с J-образным кончиком на одном конце и прямым на другом с одним просветом; 2- скальпель; 3- толкатель проводочного проводника с держателем; 4- зажим катетера; 5- сосудистый дилататор; 6- проводниковая игла/проводниковая игла с Y-портом; 7- шприц с наконечником Люэра/проводниковый шприц.

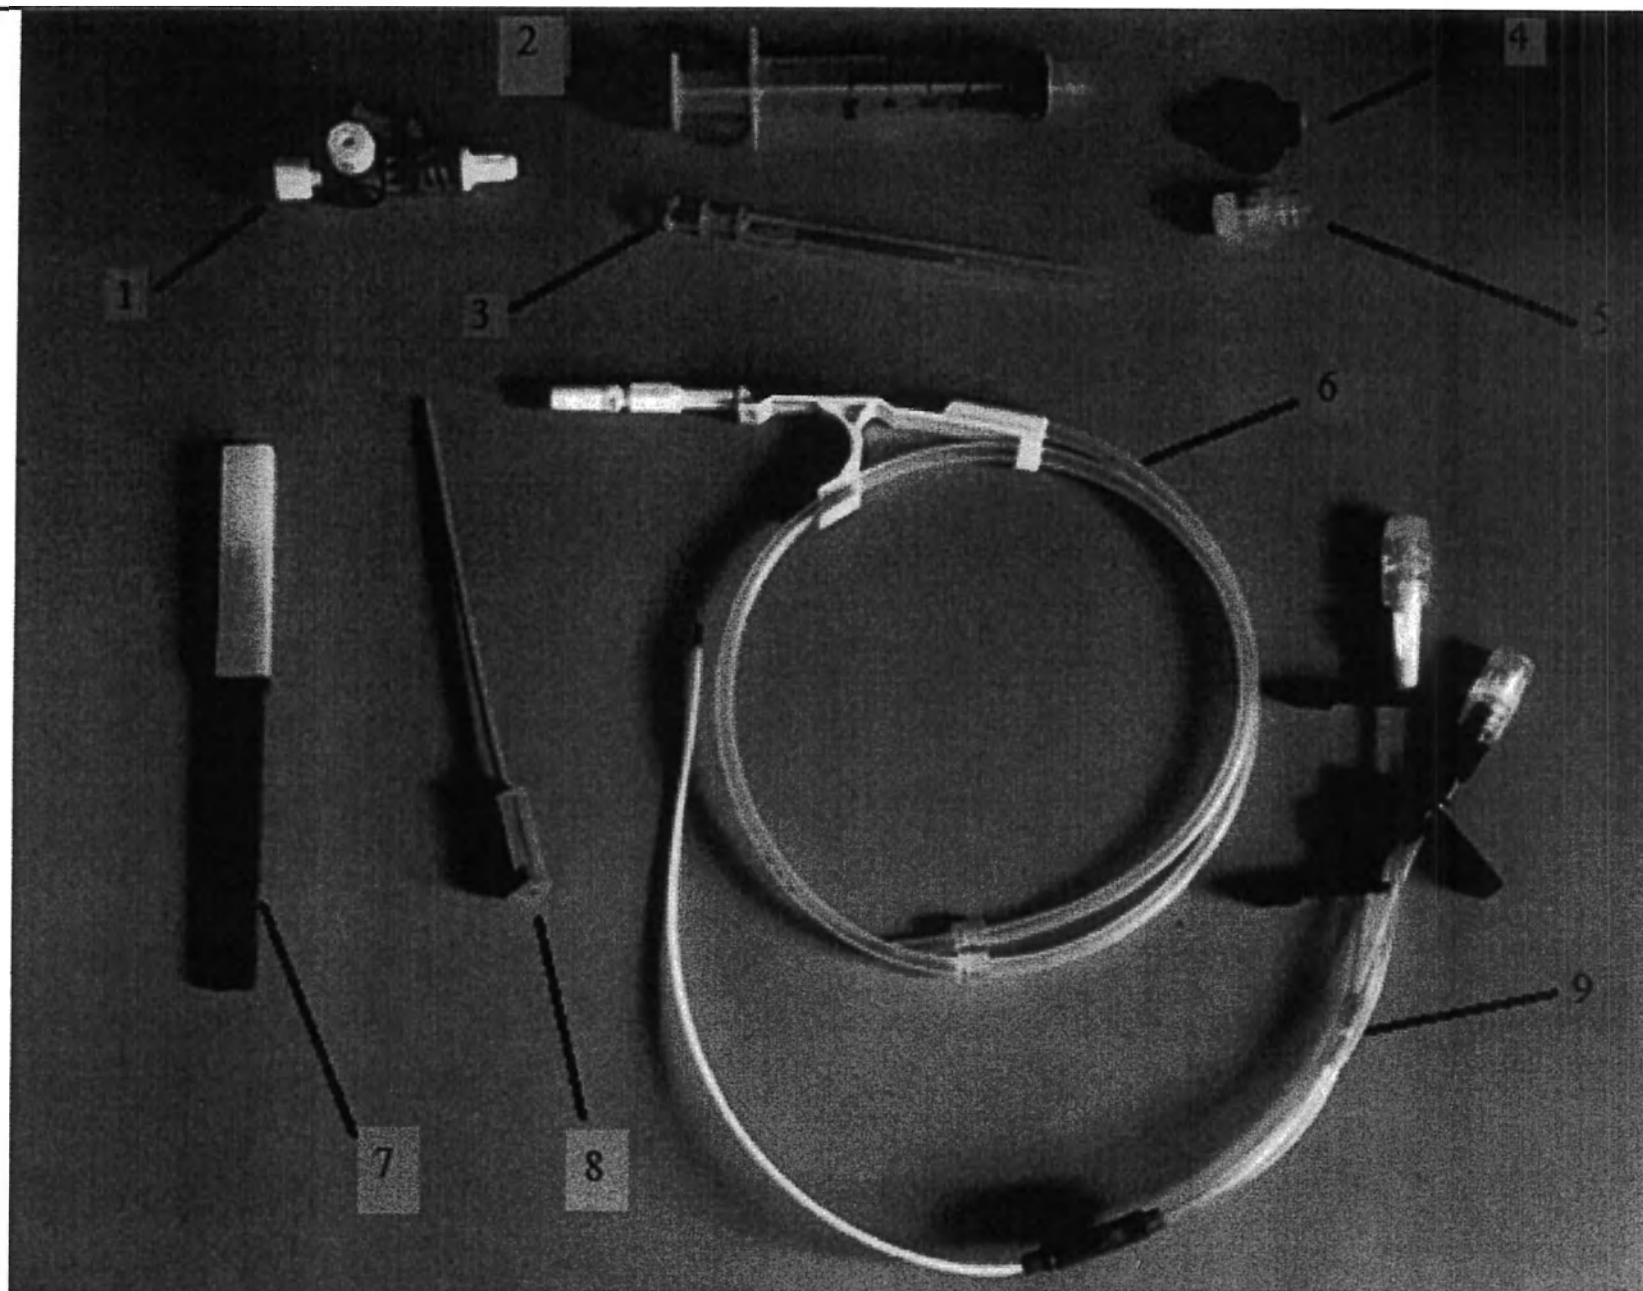


Фото 9 – Состав набора «Novocent pro trio» (Новоцент про трио) трехпросветный:

1- 3-х ходовой кран; 2- шприц с наконечником Люэра/проводниковый шприц; 3- проводниковая игла/проводниковая игла с Y портом; 4- зажим катетера; 5- зажим с портом люэр-лок; 6- толкатель проволочного проводника; 7- скальпель; 8- сосудистый дилататор; 9- полостной катетер, проволочный проводник с J-образным кончиком на одном конце и прямым на другом с тремя просветами.

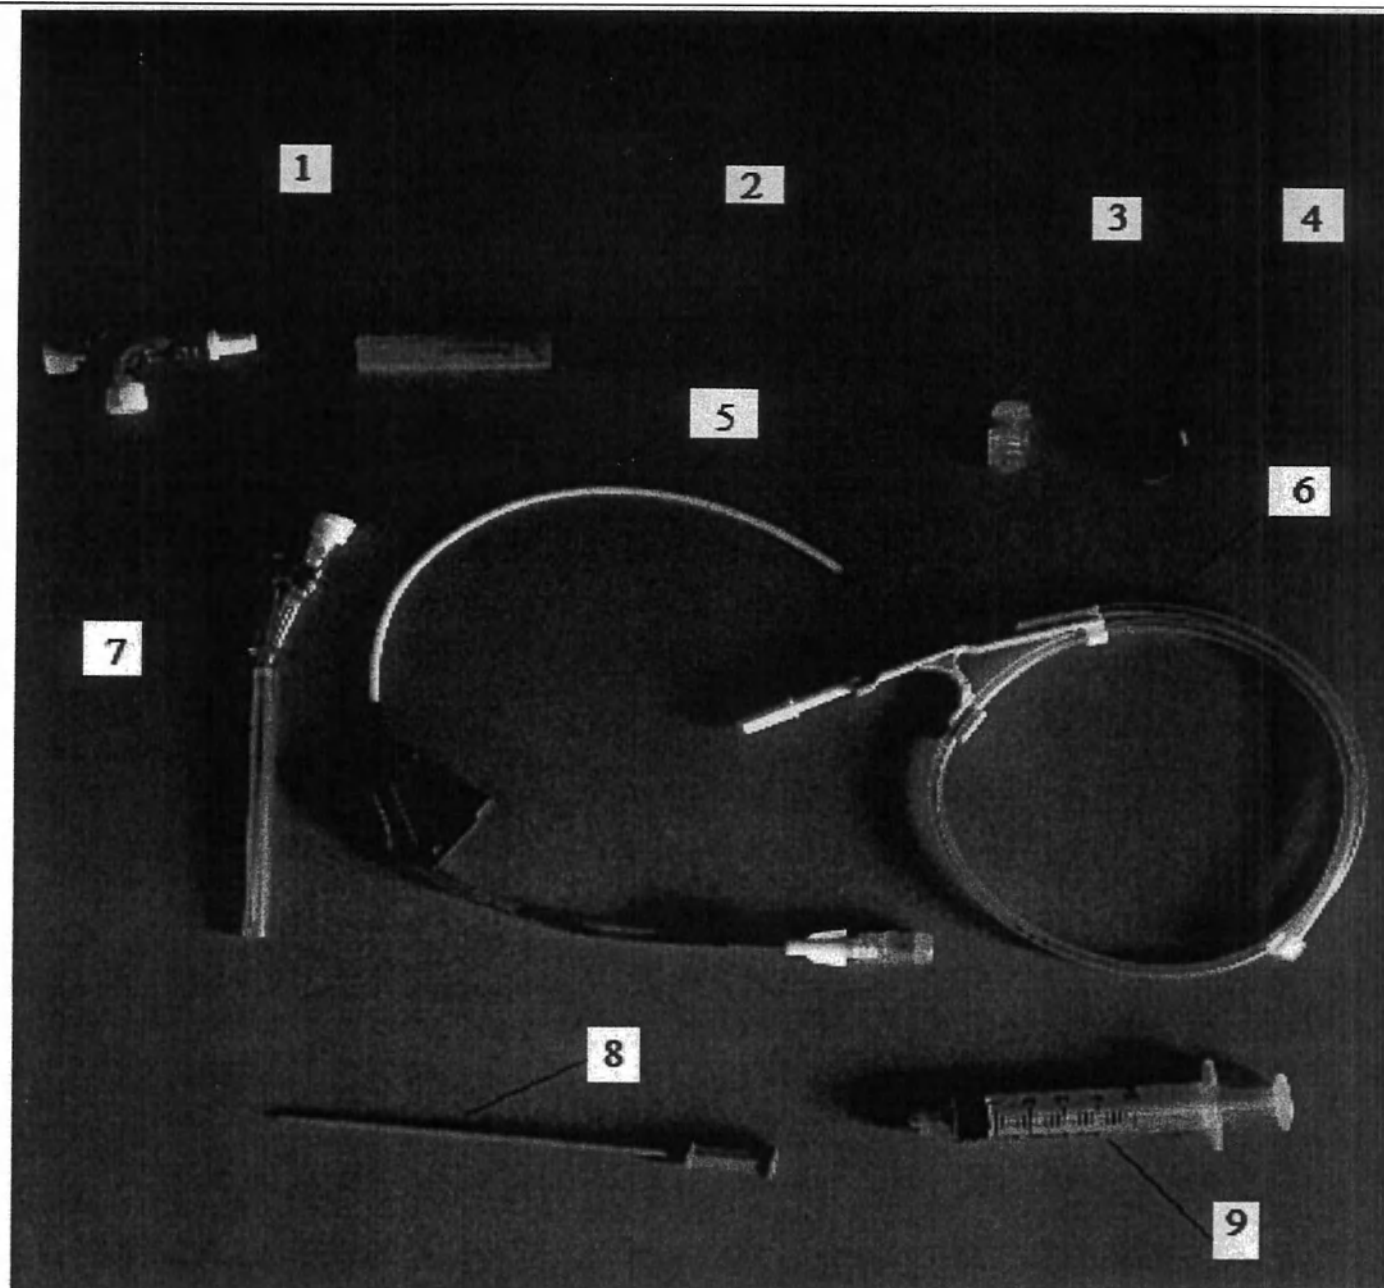


Фото 10 – Состав набора «Novocent pro duo» (Новоцент про дуо) двухпросветный:

1-3-ходовой кран; 2- скальпель; 3- зажим с портом люэр-лок; 4- зажим катетера; 5-полостной катетер, проводочный проводник с J-образным кончиком на одном конце и прямым на другом с двумя просветами; 6- толкатель проводочного проводника с держателем; 7- проводниковая игла/проводниковая игла с Y-портом; 8- сосудистый дилататор; 9- шприц с наконечником Люэра/проводниковый шприц.

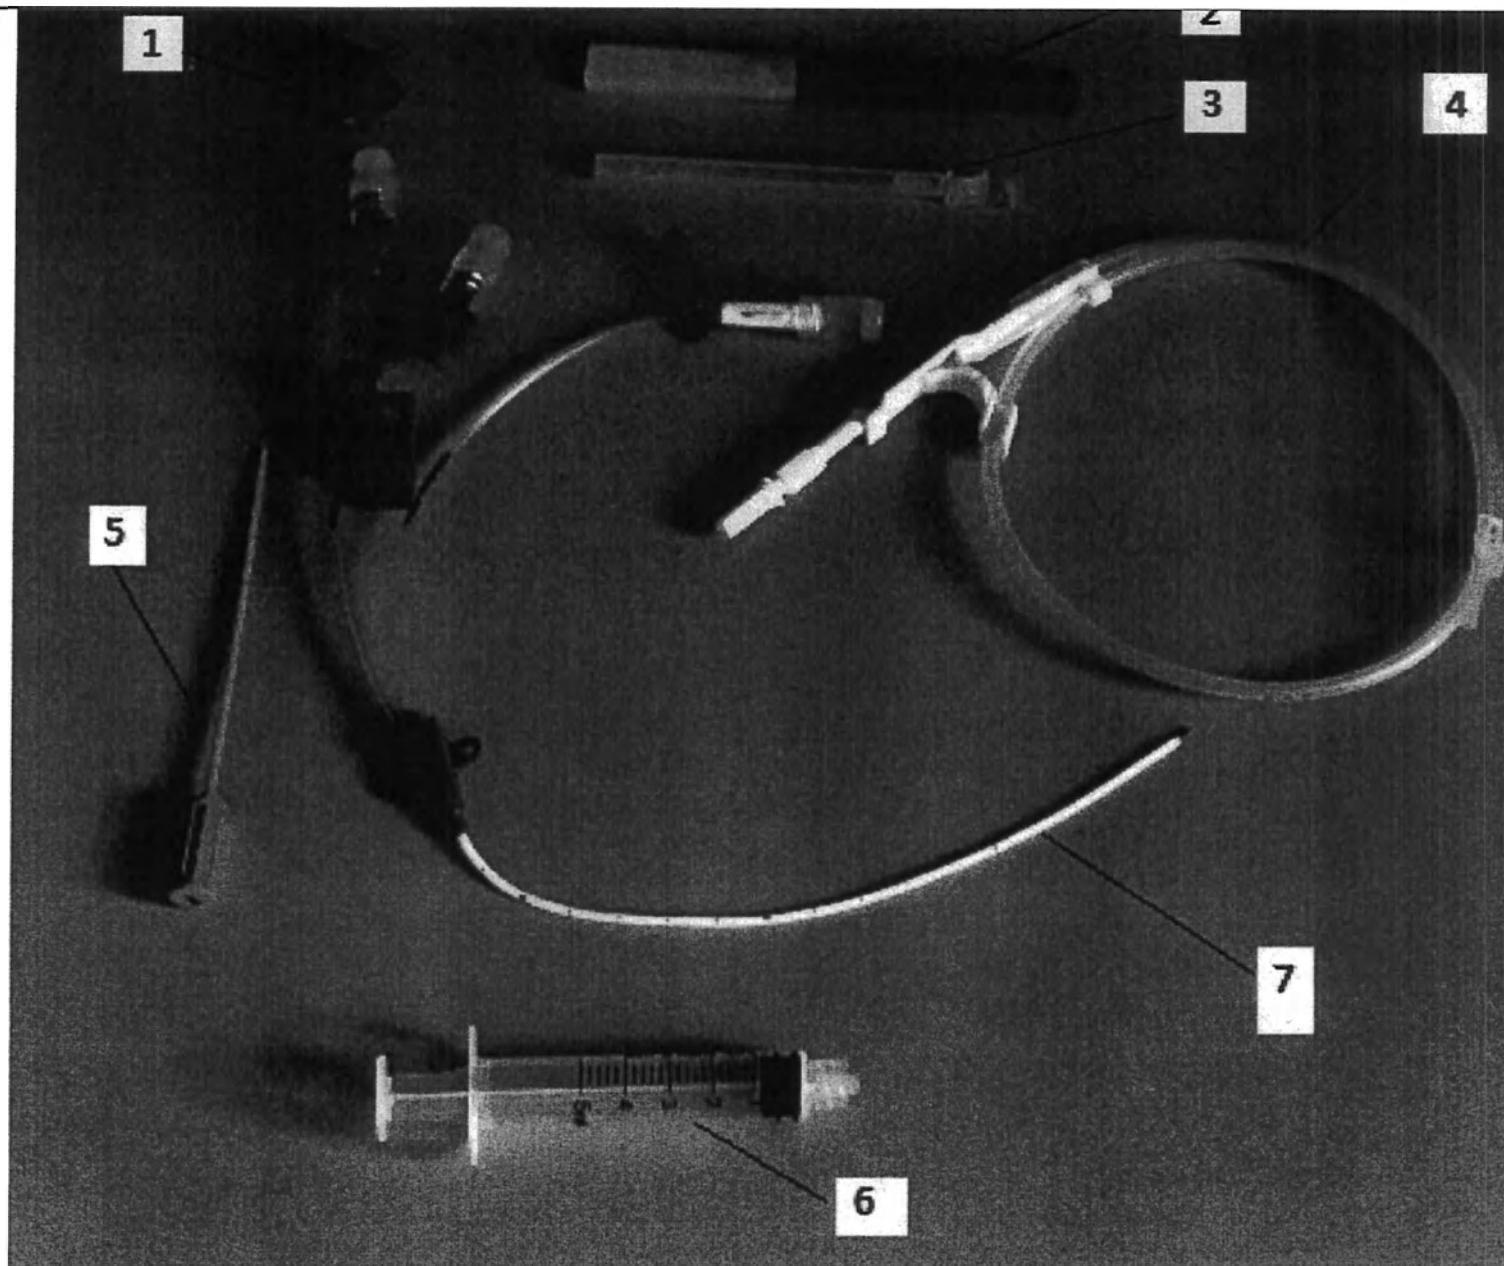


Фото 11- Состав набора «Novocent trio» (Новоцент трио) трехпросветный

полостной катетера; 2- скальпель; 3- проводниковая игла/проводниковая игла с Y портом; 4- толкатель проводочного проводника с держателем; 5- сосудистый дилататор; 6- шприц с наконечником Люэра/проводниковый шприц; 7- полостной катетер, проводочный проводник с J –образным кончиком на одном конце и прямым на другом с тремя просветами.

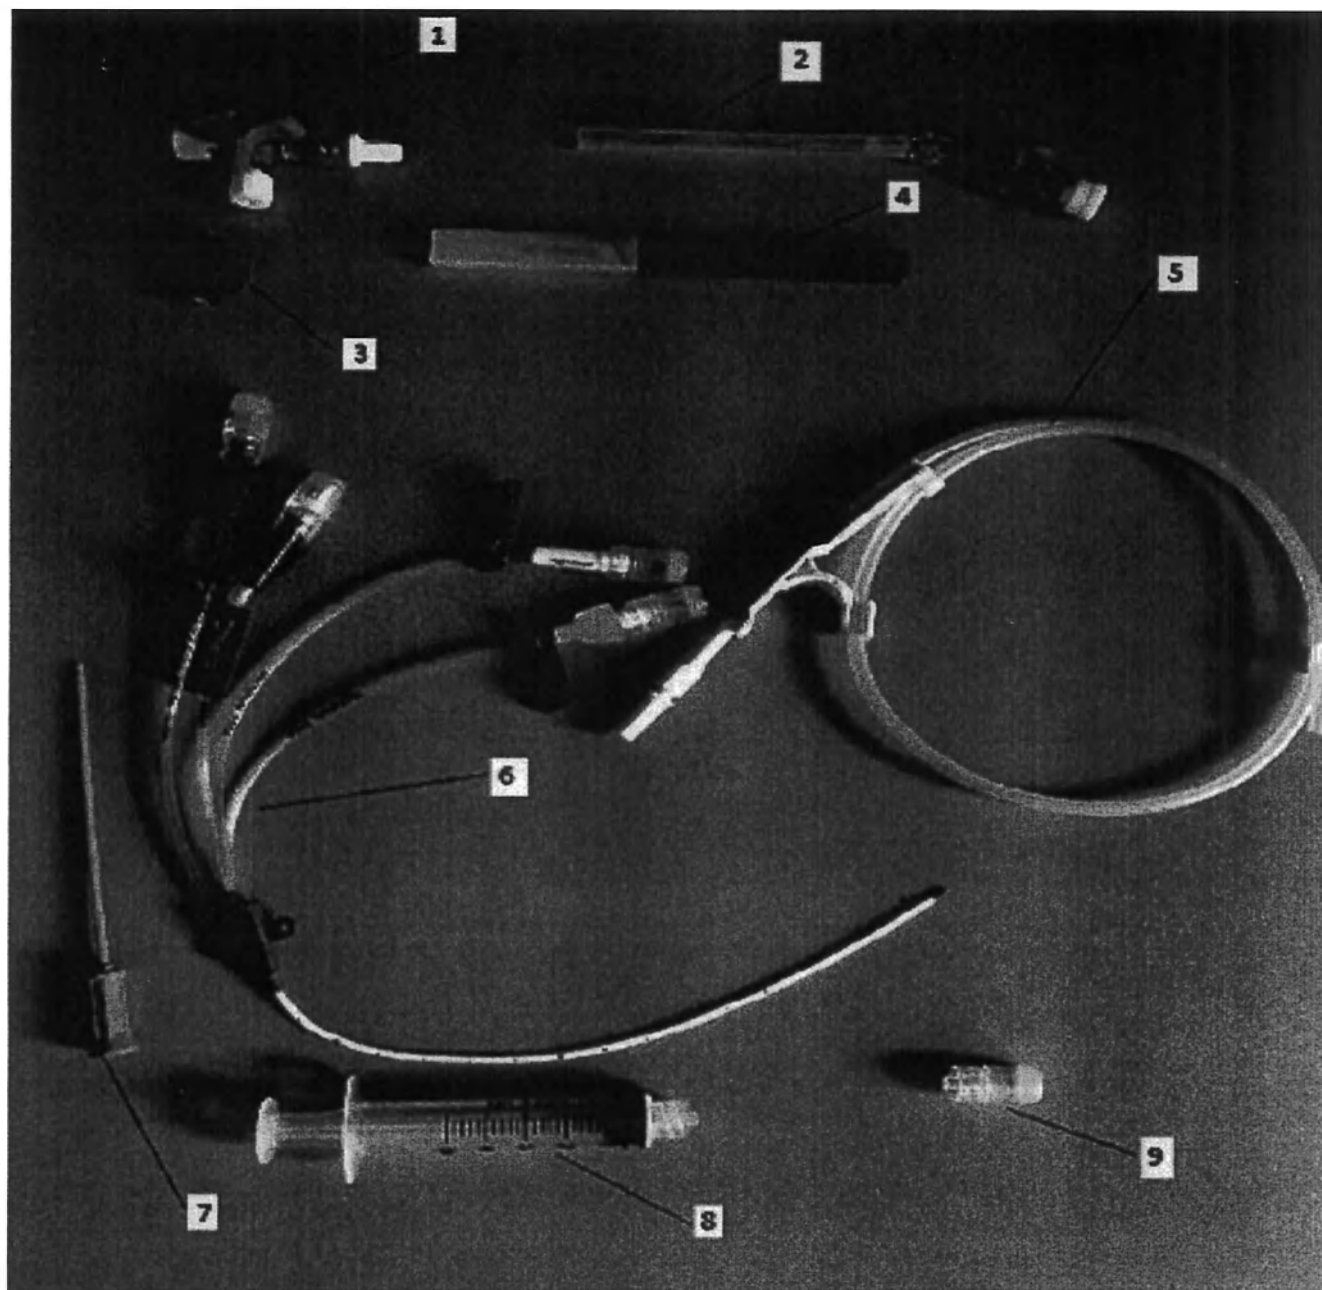


Фото 12- Состав набора «Novocent pro four » (Новоцент про фор) четырехпросветный:

1- кран; 2- проводниковая игла/проводниковая игла с Y-портом; 3- зажим катетера; 4- скальпель; 5- толкатель проводочного проводника с держателем; 6- полостной катетер, проводочный проводник с J-образным кончиком на одном конце и прямым на другом с четырьмя просветами; 7- сосудистый дилататор; 8- шприц с наконечником Люэра/проводниковый шприц; 9- зажим с портом Люэра-лок.

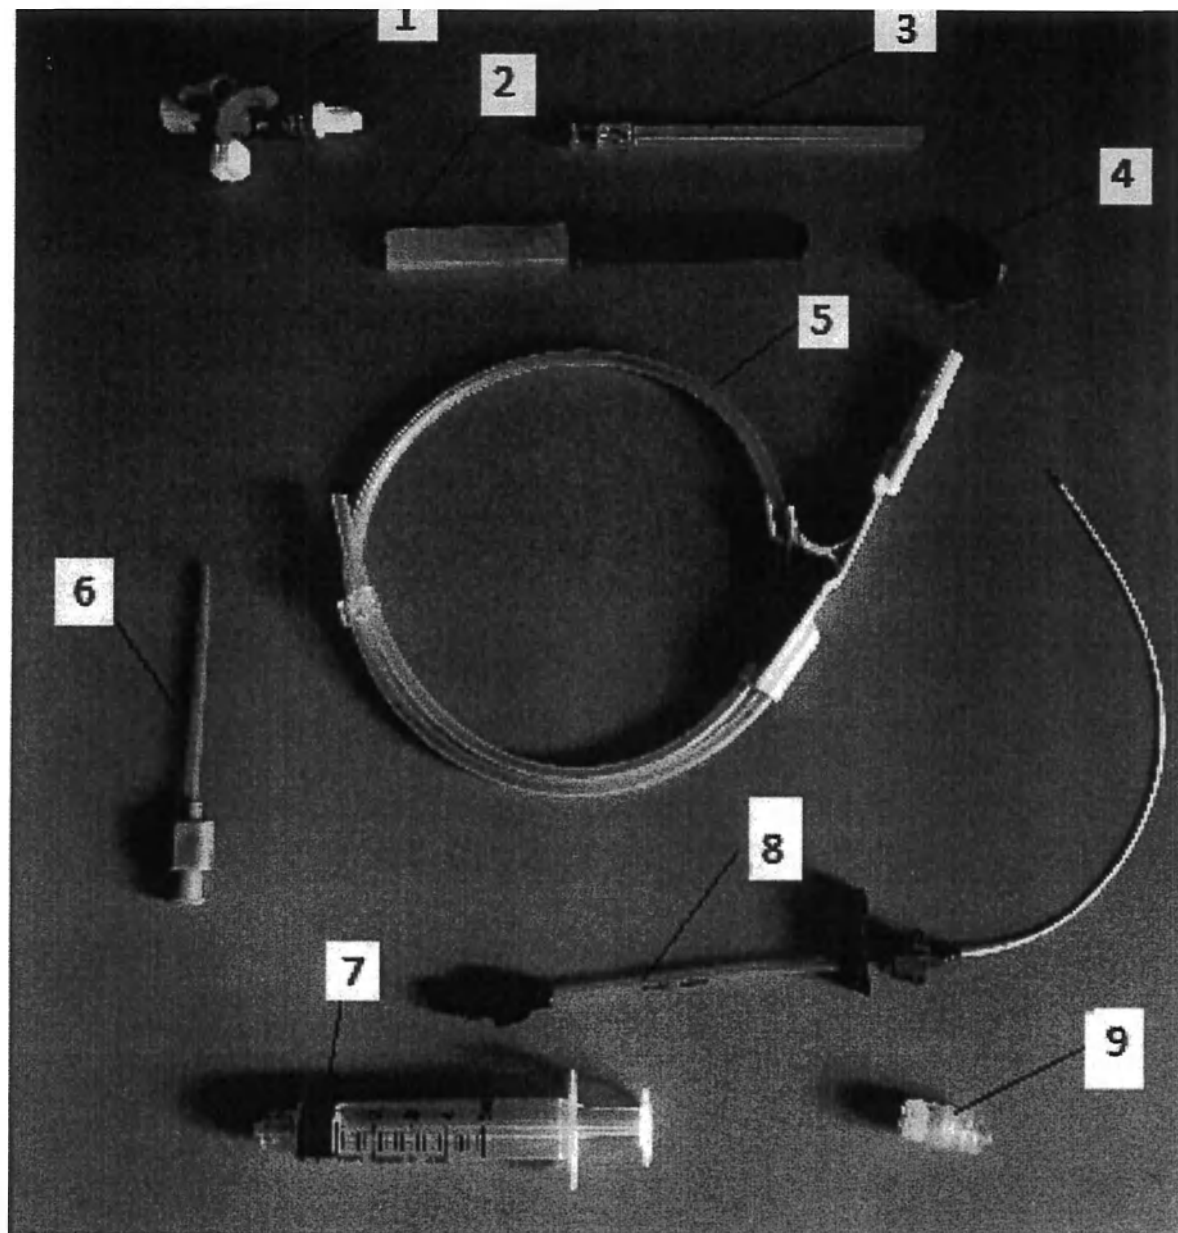


Фото 13- Состав набора «Novocent pro mono» (Новоцент про моно) однопросветный:

1- выходной кран; 2- скальпель; 3- проводниковая игла/проводниковая игла с Y-образным портом; 4- зажим катетера; 5- толкатель проволоочного проводника с держателем; 6- сосудистый дилататор; 7- шприц с наконечником Люэра/проводниковый шприц; 8- полостной катетер, проволоочный проводник с J-образным кончиком на одном конце и прямым на другом с одним просветом; 9- зажим с портом люэр-лок;

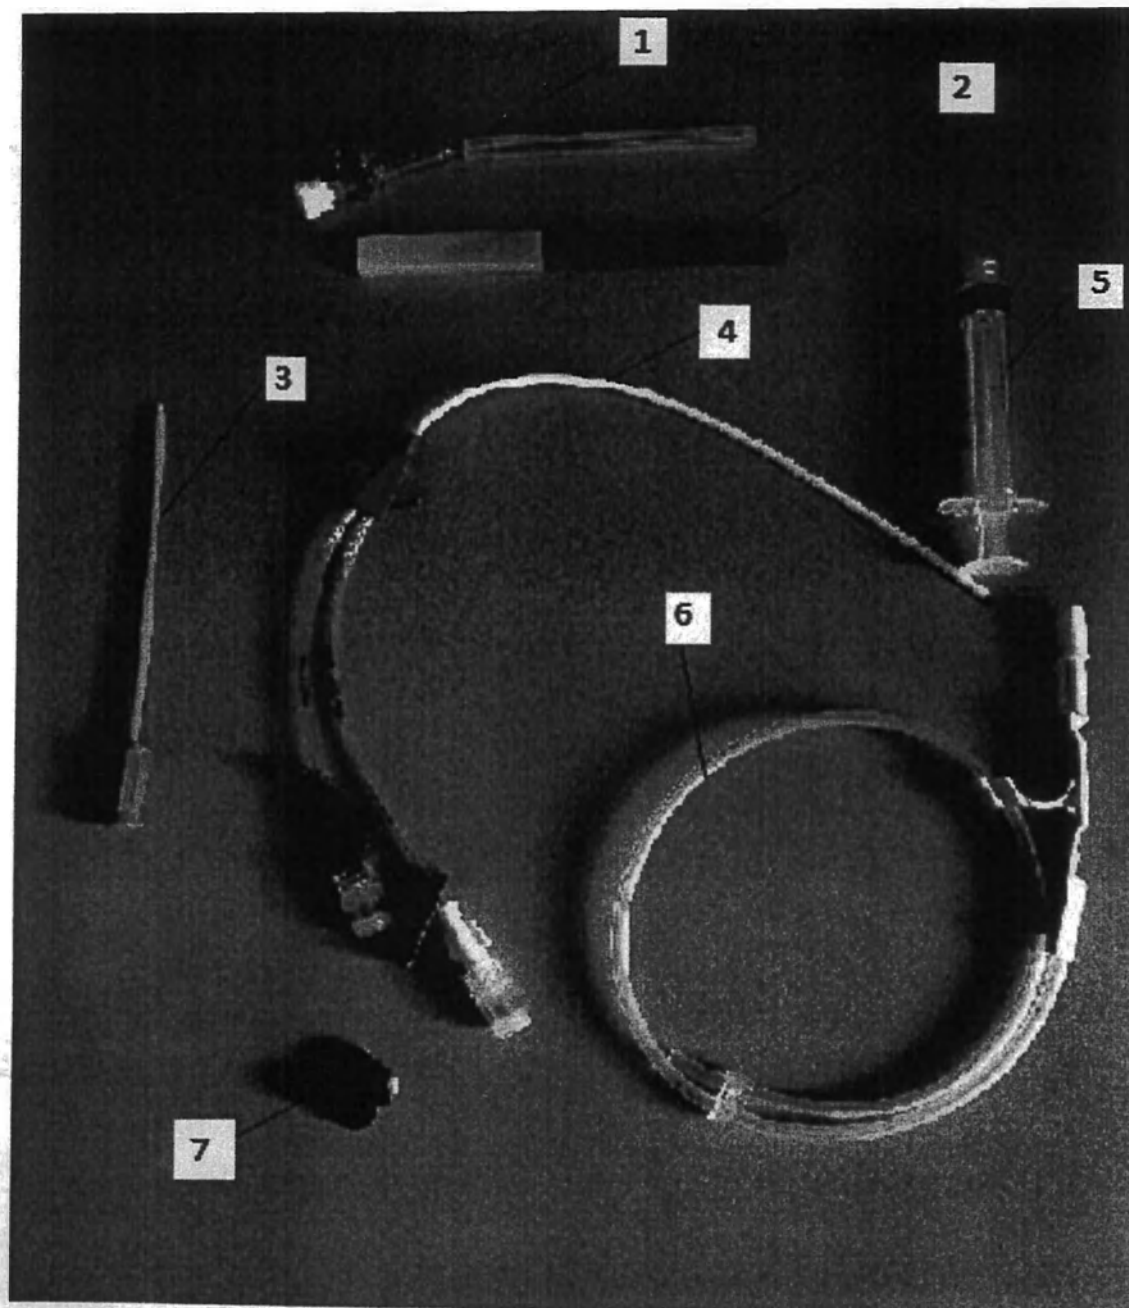


Фото 14- Состав набора «Novocent duo» (Новоцент дуо) двухпросветный:

1- проводниковая игла/проводниковая игла с Y-портом; 2- скальпель; 3- сосудистый дилататор; 4- полостной катетер, проволоочный проводник с J-образным кончиком на одном конце и прямым на другом с двумя просветами; 5- шприц с наконечником Люэра/проводниковый шприц; 6- толкатель проволоочного проводника с держателем; 7- зажим катетера.