



**Фотографическое изображение
общего вида медицинского изделия:**

Система автоматизированная ТСА для преаналитической и постаналитической обработки образцов



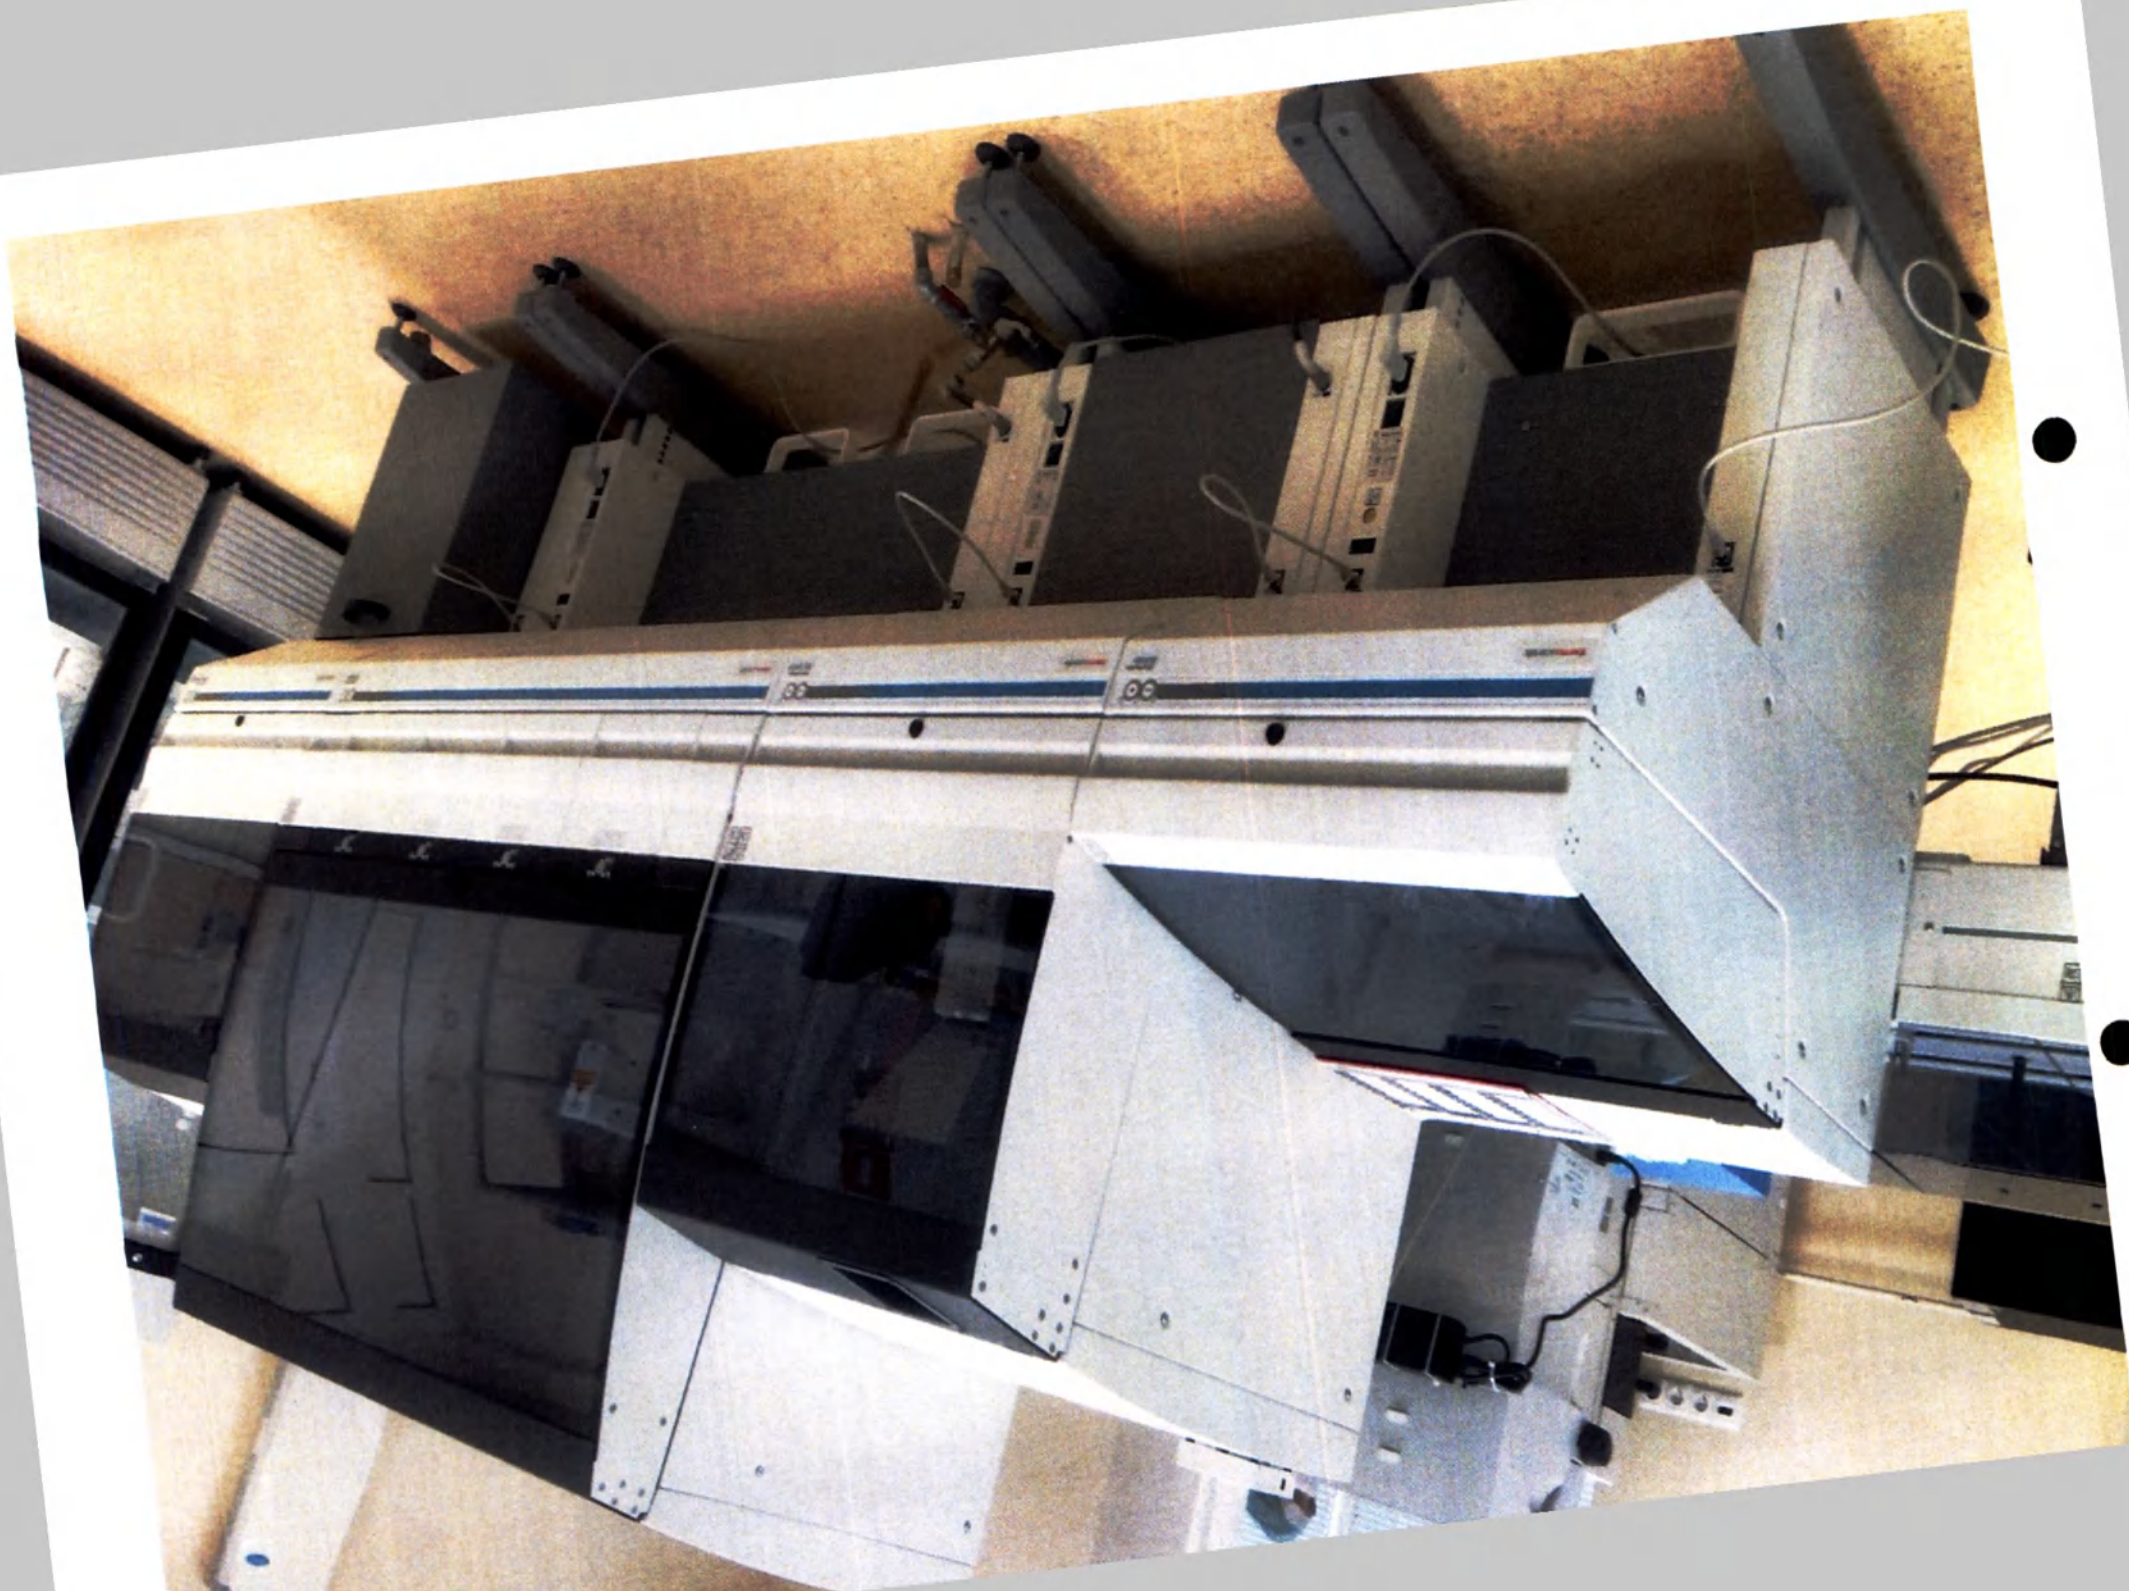

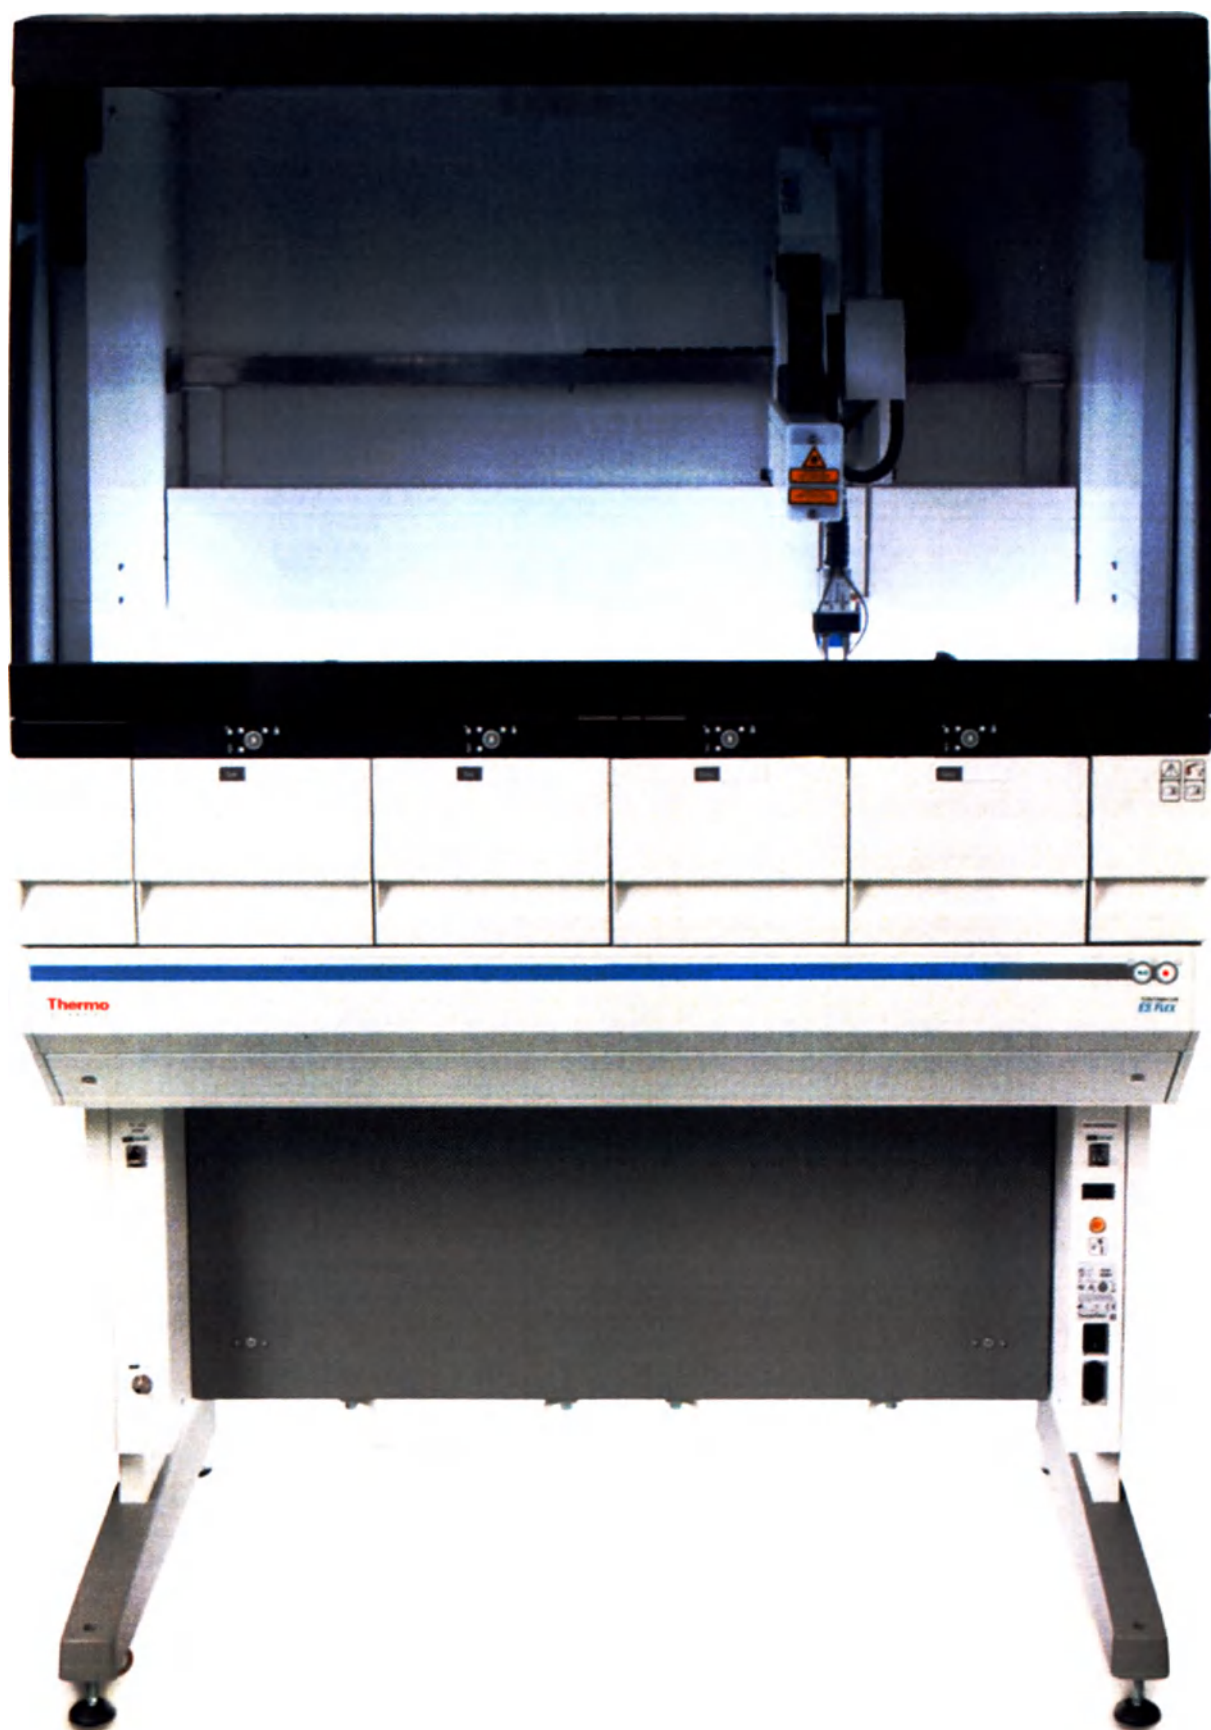

ES Flex, TCA

REF

952202



SN

58991



Type: 1038

Mains: 100-240Vac, 50-60Hz, 400W



710364



This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.

CAN ICES-3(B)/NMB-3(B)

Made in Finland



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

Thermo Fisher
SCIENTIFIC







Decapper Flex, TCA

REF

952039




SN

58990



Type: 1031

Mains: 100-240Vac, 50-60Hz, 300W




This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.
CAN ICES-3(B)/NMB-3(E)

Made in Finland



2019



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland



ThermoFisher
SCIENTIFIC







Recapper, 230V, TCA

REF

952036



SN

58989



Type:


1027

Mains:

220-230Vac, 50Hz, 300W



2019



Made in Finland



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

ThermoFisher
SCIENTIFIC







Buffer, TCA

REF

952013




SN

58988



Type: 1018

Mains: 100-240Vac, 50-60Hz, 300W



This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.

CAN ICES-3(B)/NMB-3(B)

Made in Finland




2019



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

ThermoFisher
SCIENTIFIC



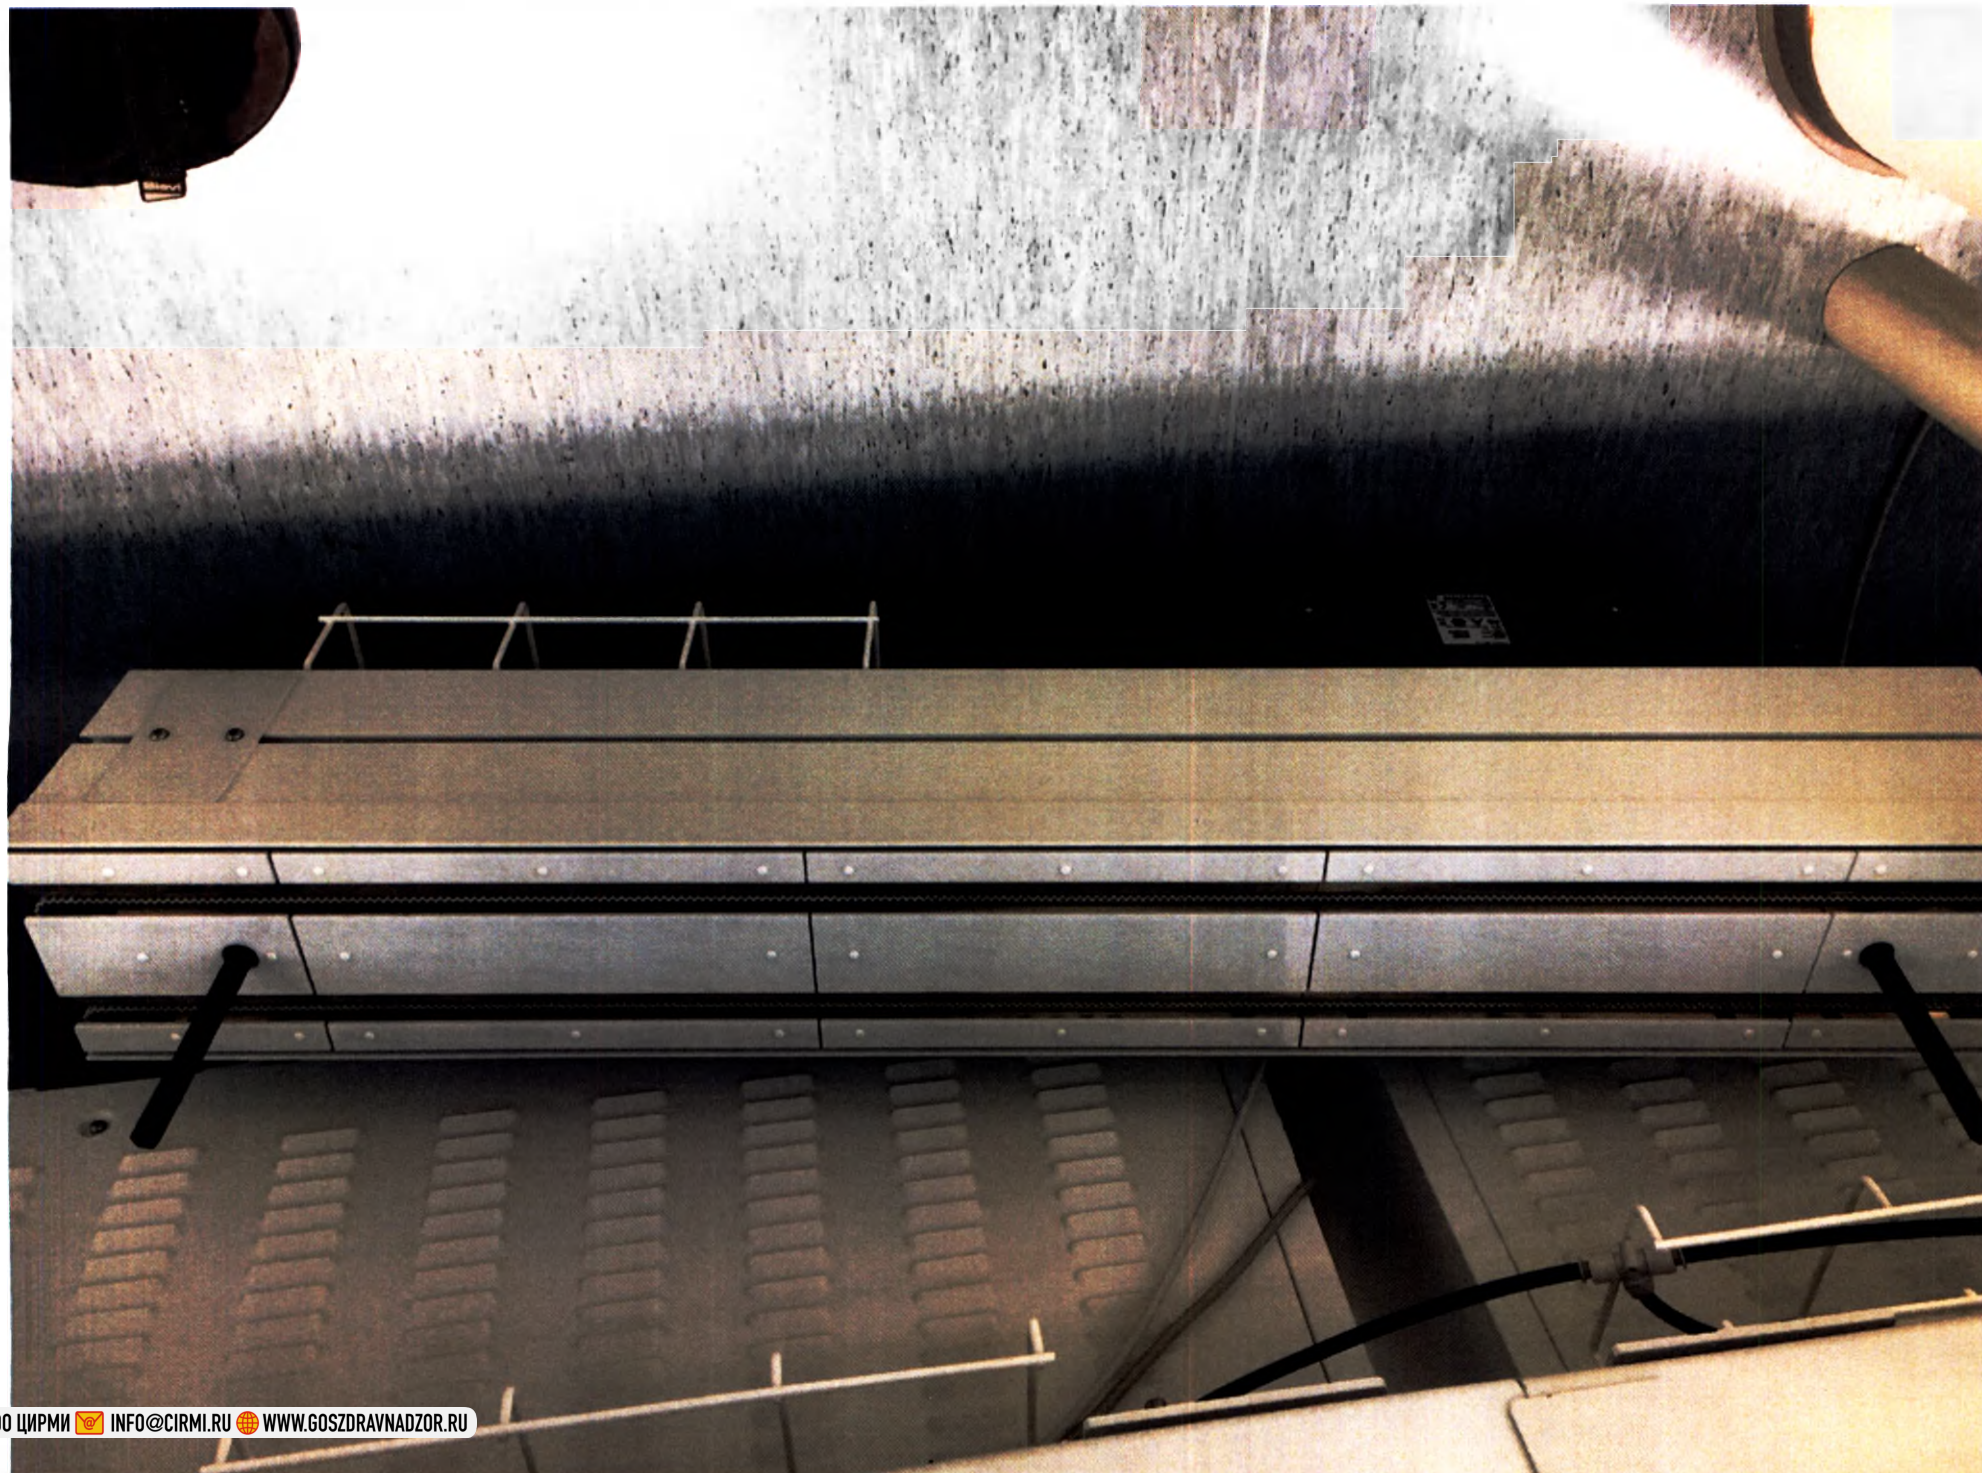

Conveyor 2400, TCA

REF

952025



SN

58980




Type: 1007

Mains: 100-240Vac, 50-60Hz, 50W




This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.
CAN ICES-3(B)/NMB-3(B) Made in Finland



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

ThermoFisher
SCIENTIFIC



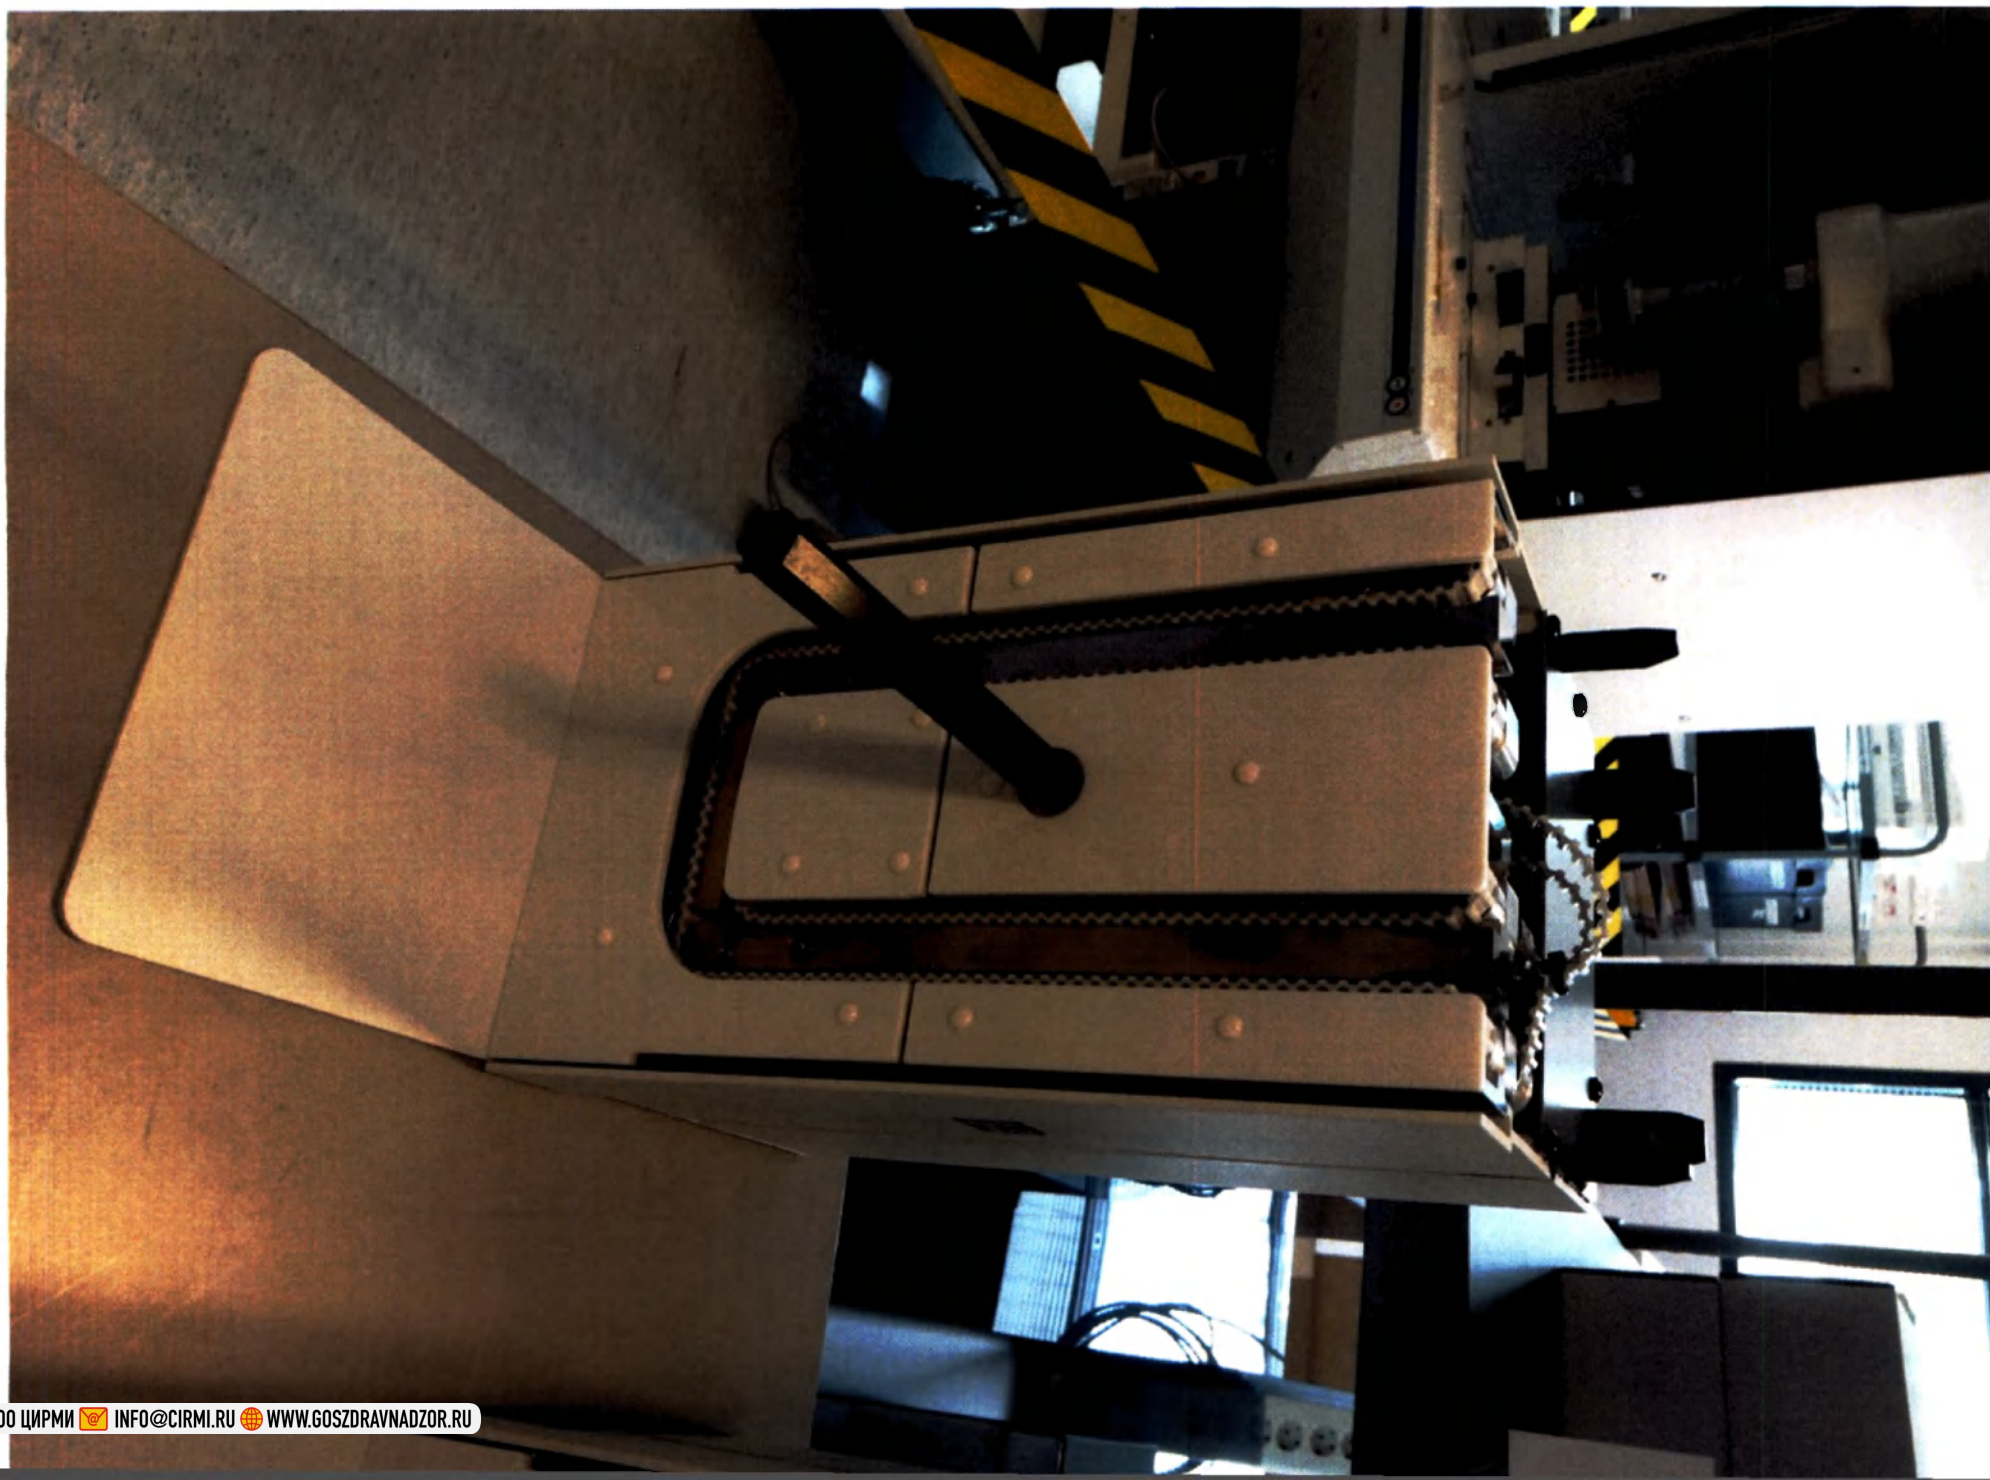

U-Turn Mek

REF

952226

SN

58984

Type:

1034

Mains:

-



2019

IVD

Made in Finland




Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

Thermo Fisher
SCIENTIFIC



6) U-образный транспортер – не более 8 шт. (при необходимости) (фотографические изображения маркировки производителя)

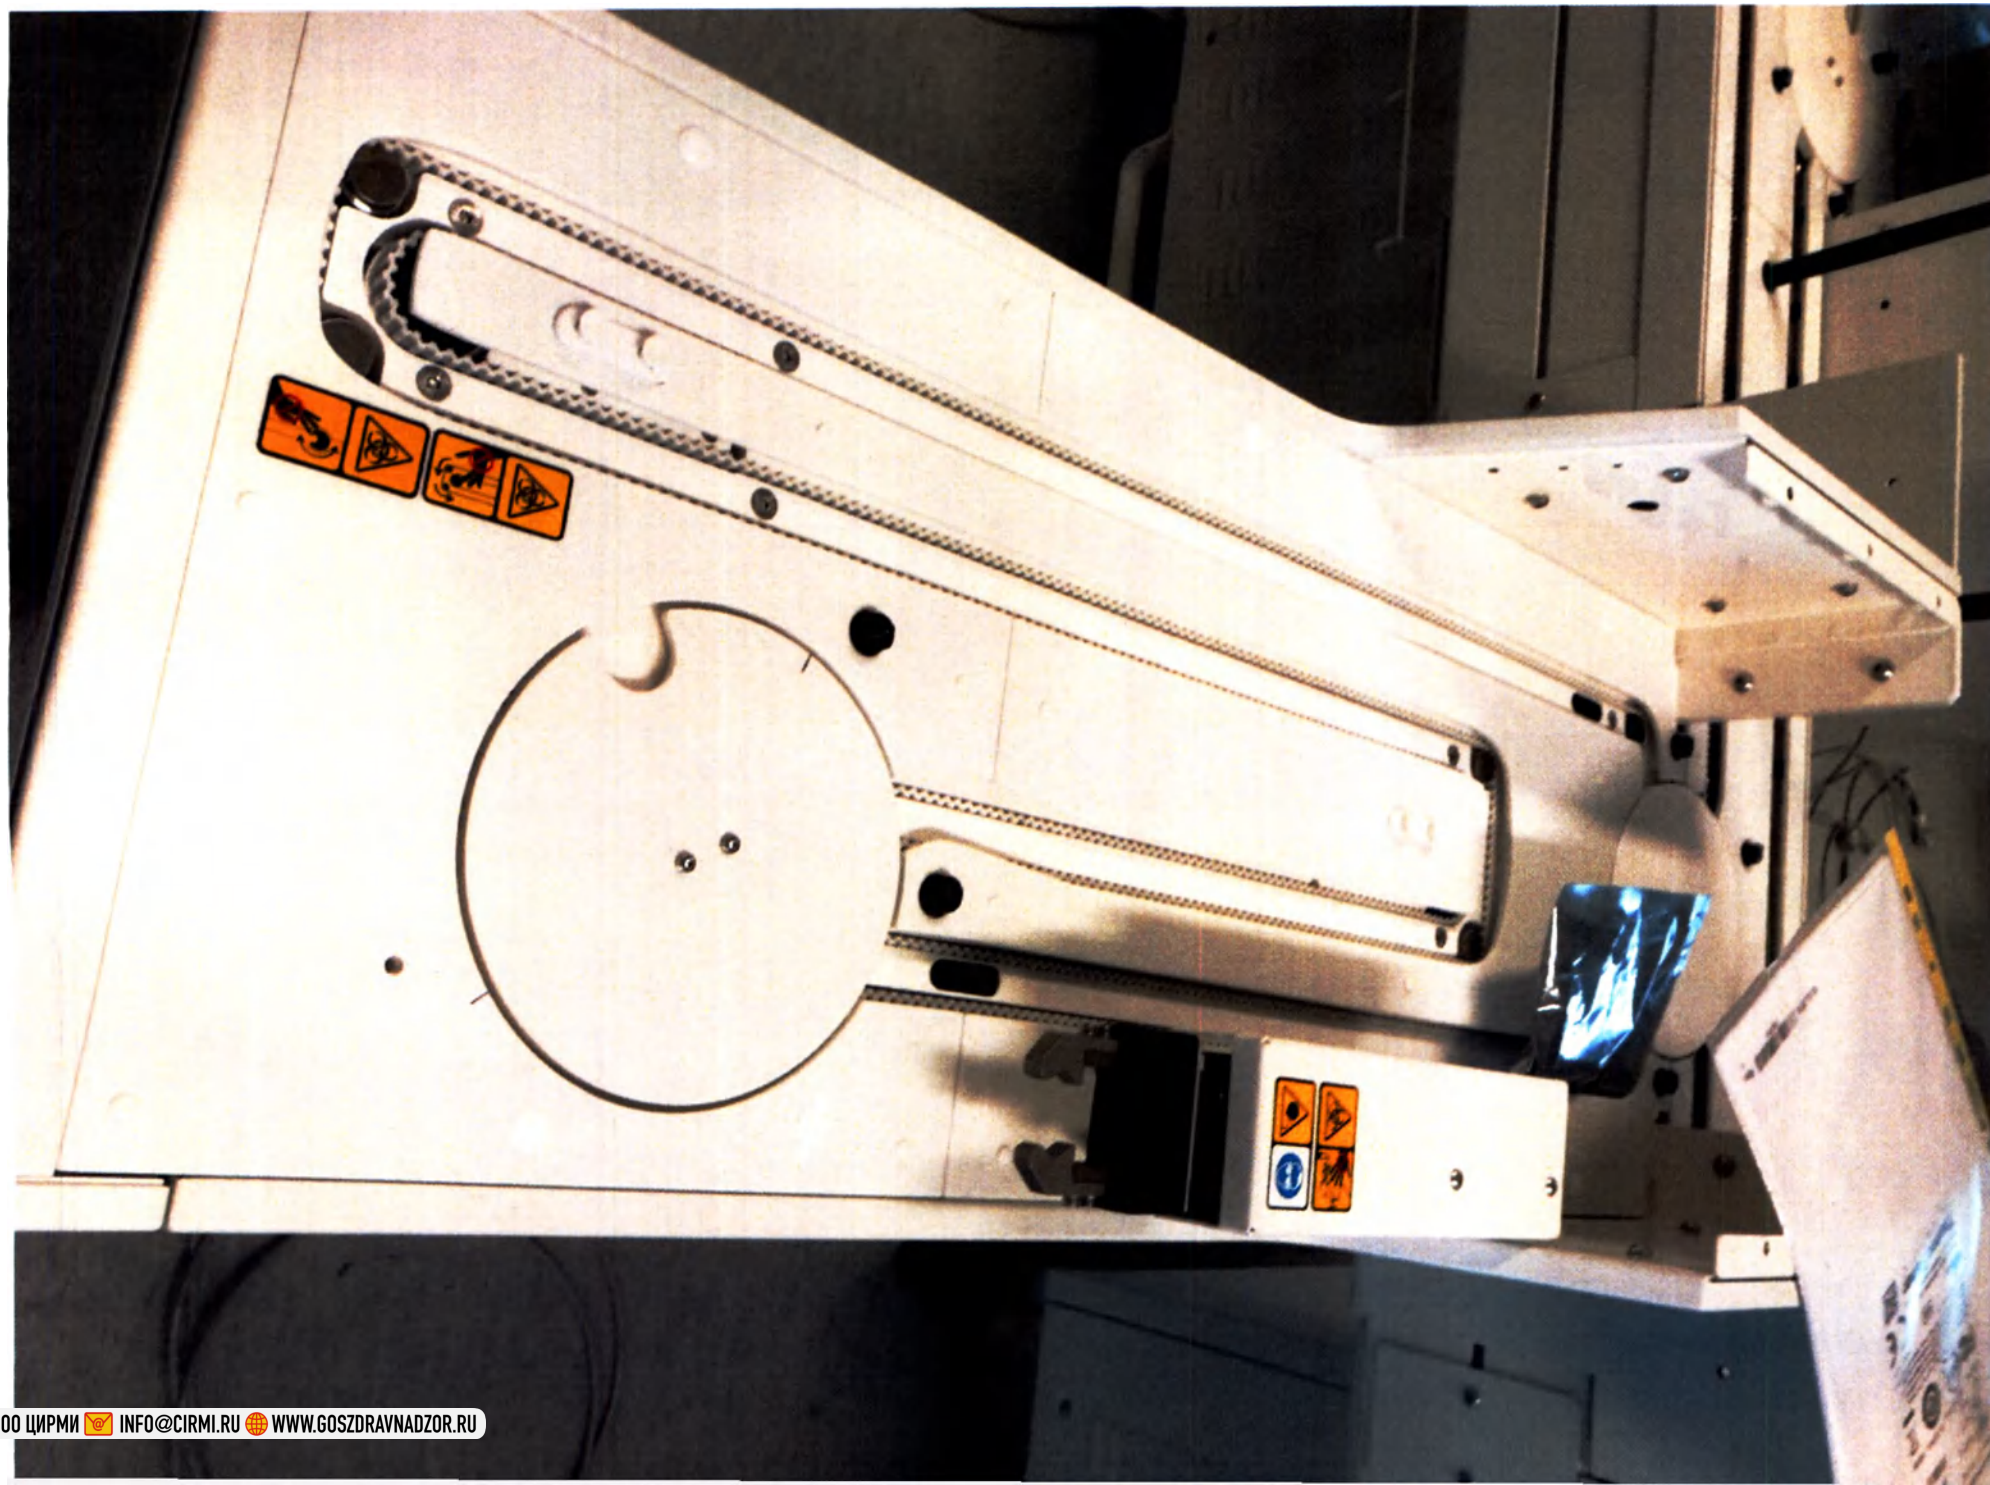

Internal U-Turn, TCA

REF

952046



SN

58982





Type: 1025

Mains: 100-240Vac, 50-60Hz, 150W



This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
1) This device may not cause harmful interference, and
2) This device must accept any interference received,
including interference that may cause undesired operation.
CAN ICES-3 (B) NMB-3 (B) Made in Finland



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

ThermoFisher
SCIENTIFIC





PIEM
Kivinkyläntie 221 A
02440 VILMELA
FINLAND
Tel. +358 (0)9 2524 4000
www.piem.fi

Модель:
PC 3-4 Makower
Сер. Номер: 133

PIEM
Kivinkyläntie 221 A
02440 VILMELA
FINLAND
Tel. +358 (0)9 2524 4000
www.piem.fi

Модель:
PC 3-4 Makower
Сер. Номер: 133

PIEM
Kivinkyläntie 221 A
02440 VILMELA
FINLAND
Tel. +358 (0)9 2524 4000
www.piem.fi

Модель:
PC 3-4 Makower
Сер. Номер: 133

PIEM
Kivinkyläntie 221 A
02440 VILMELA
FINLAND
Tel. +358 (0)9 2524 4000
www.piem.fi

Модель:
PC 3-4 Makower
Сер. Номер: 133

L-Turn, TCA

REF

952027



SN

58981



Type: 1009

Mains: 100-240Vac, 50-60Hz, 50W



This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.
CAN ICES 3(B)/NMB-3(B)

Made in Finland




2019



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

ThermoFisher
S C I E N T I F I C



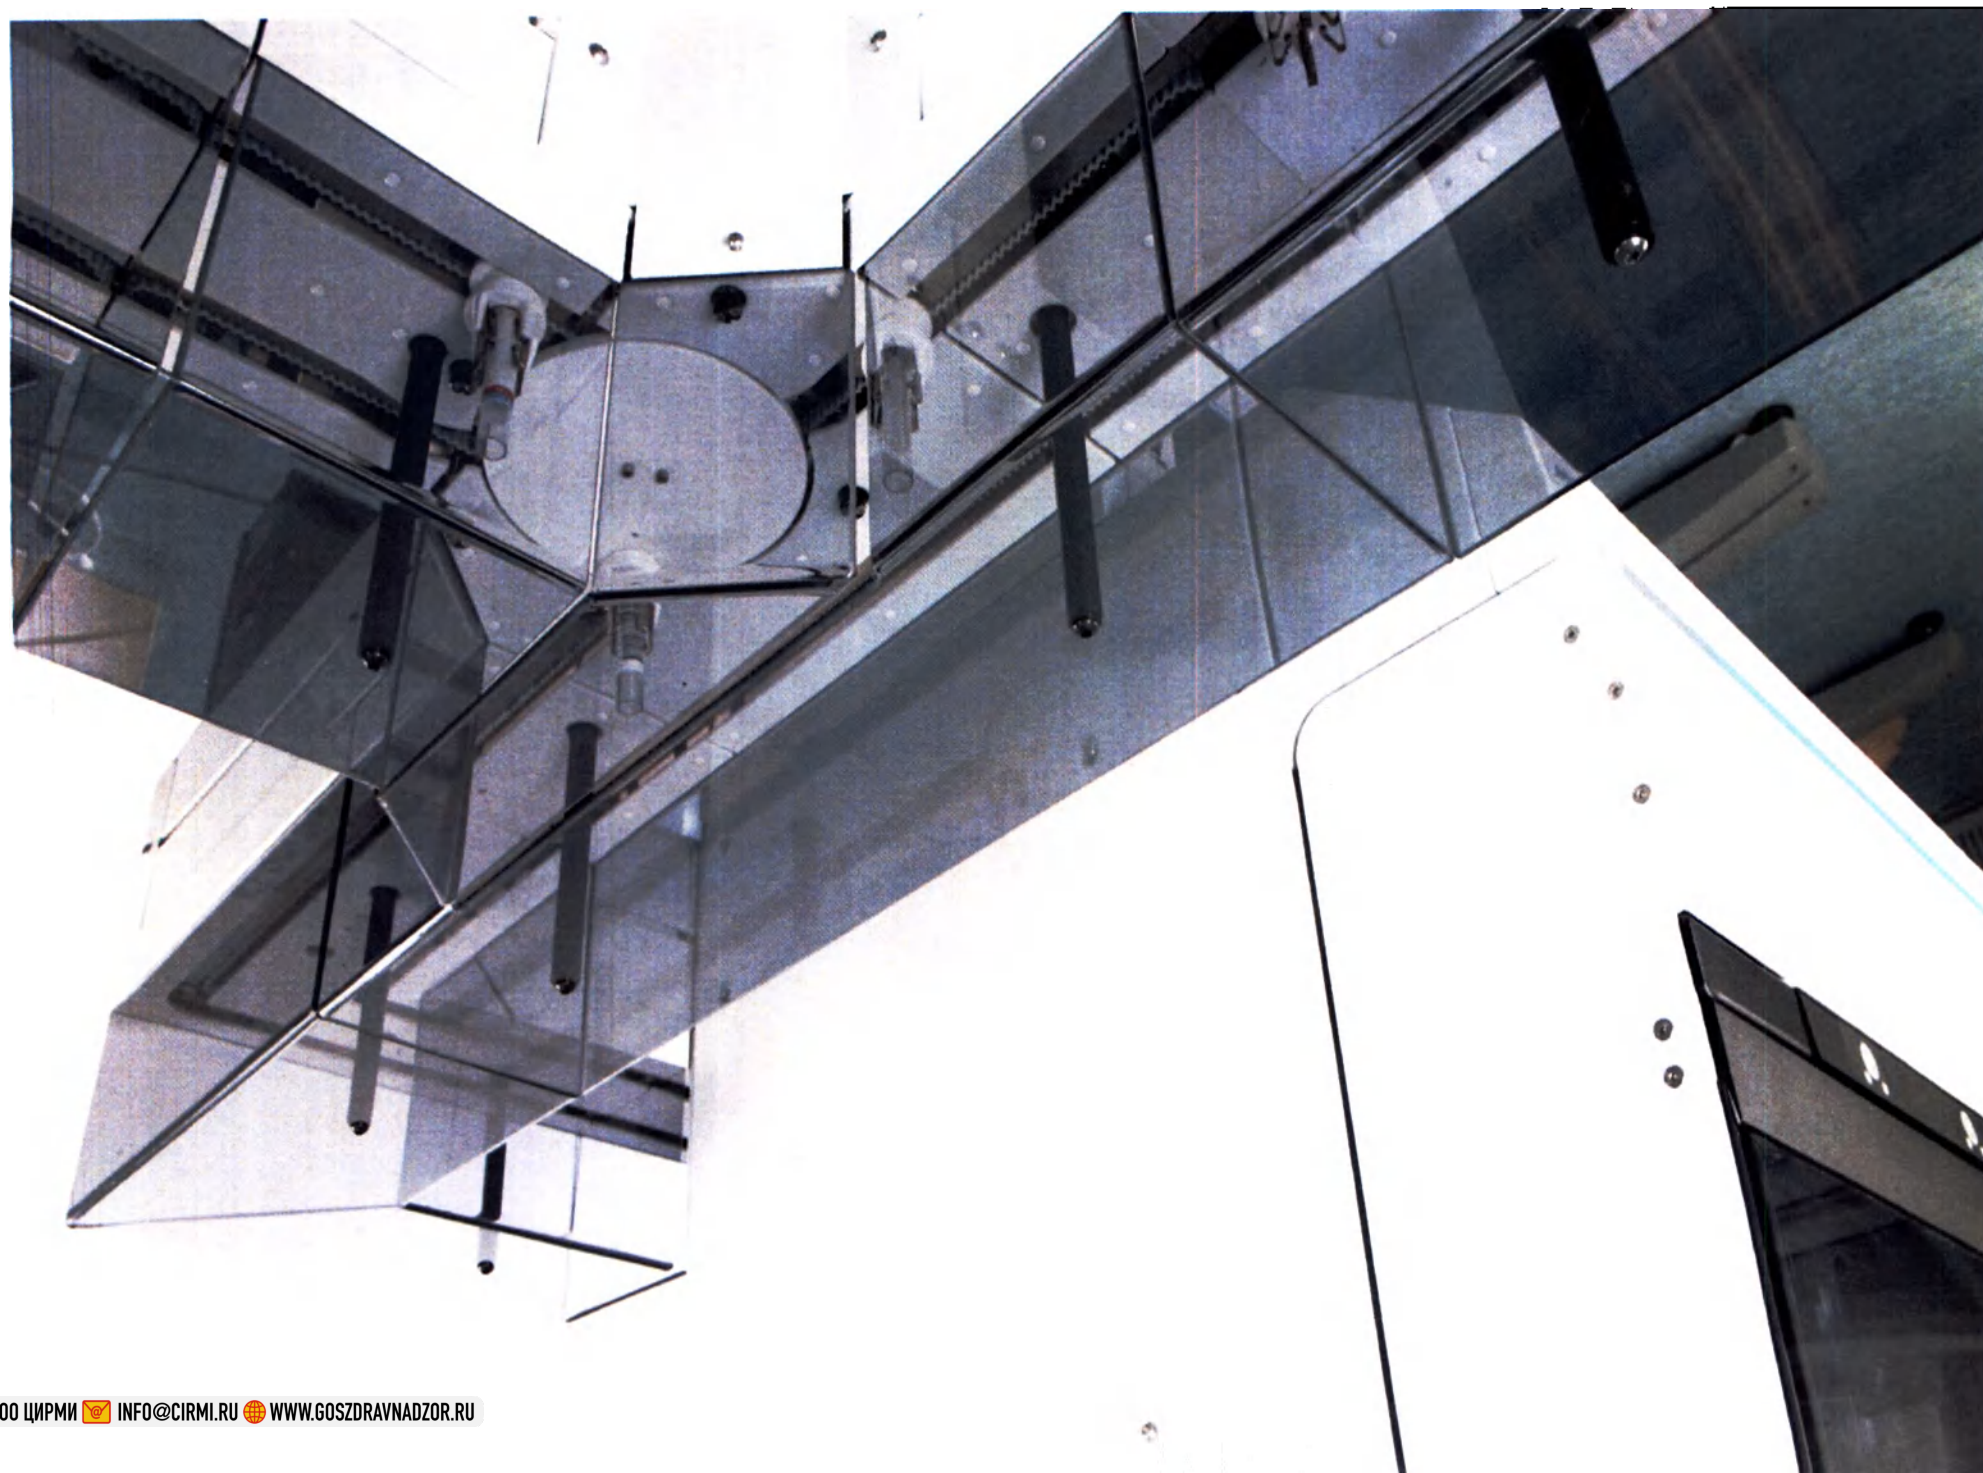

T-Tum, TCA

REF

952244



SN

90967



Type:

1044

Mains:

100-240 Vac, 50-60Hz, 100W



710004



**This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.**

0401 4100-3 (410000-300)

Made in Finland



1019



**Thermo Fisher Scientific Oy
Puhkatie 2, FI-01500 Vantaa, Finland**

**ThermoFisher
SCIENTIFIC**







Z-Turn, left, TCA

REF

952049



SN

58983



Type: 1029

Mains: 100-240Vac, 50-60Hz, 50W



713384

This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.

CAN ICES-3(B)/NMB-3(B)

Made in Finland




Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland


ThermoFisher
SCIENTIFIC



PC2 121



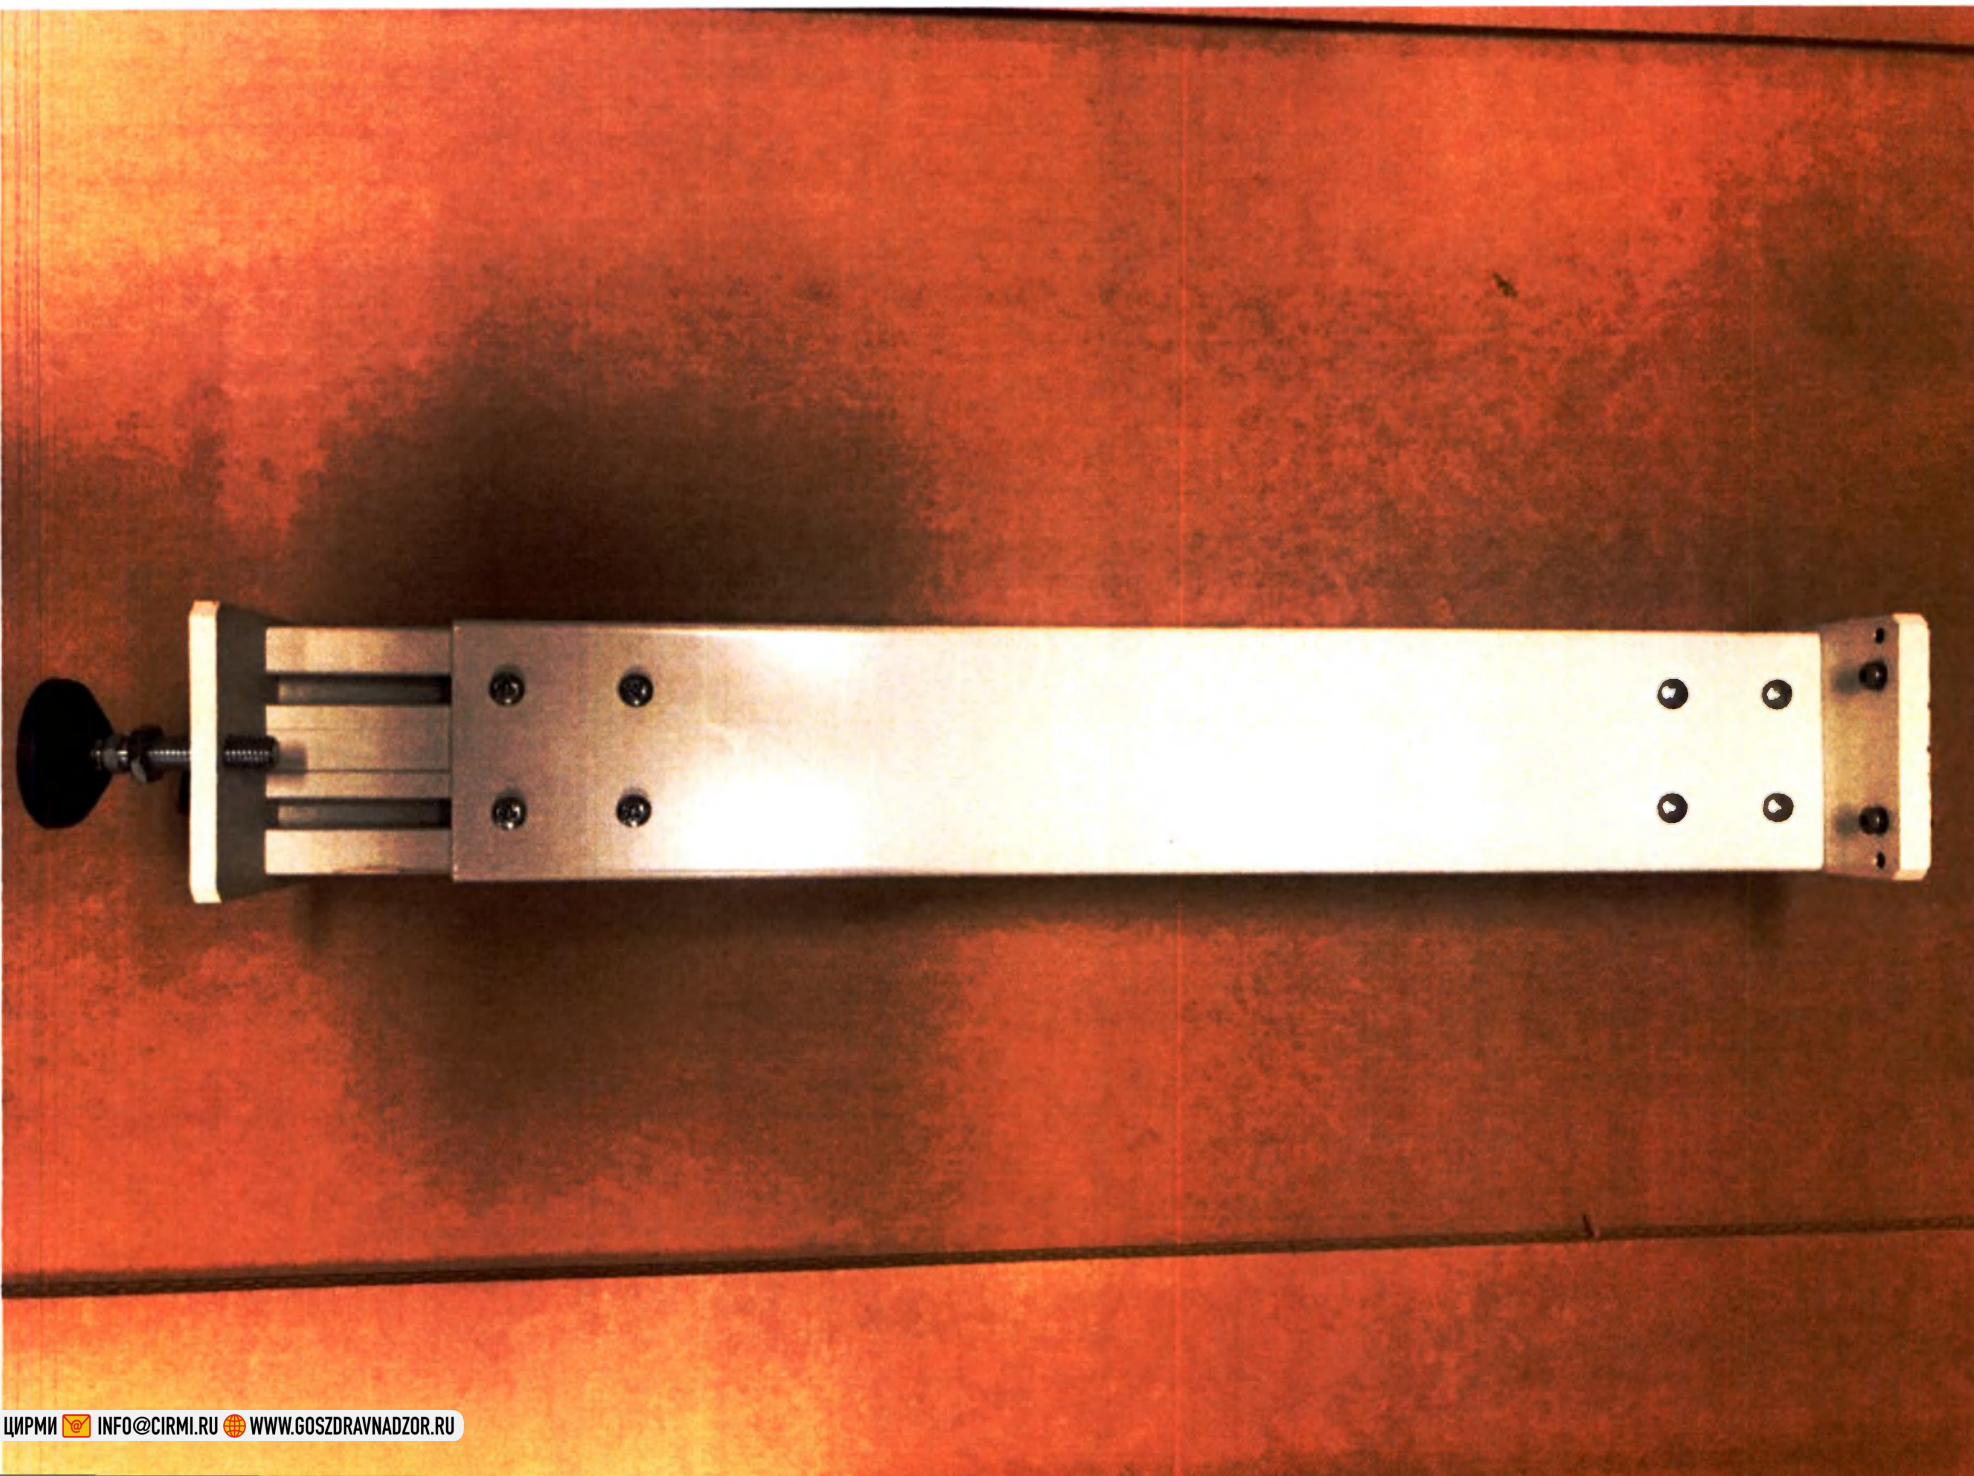

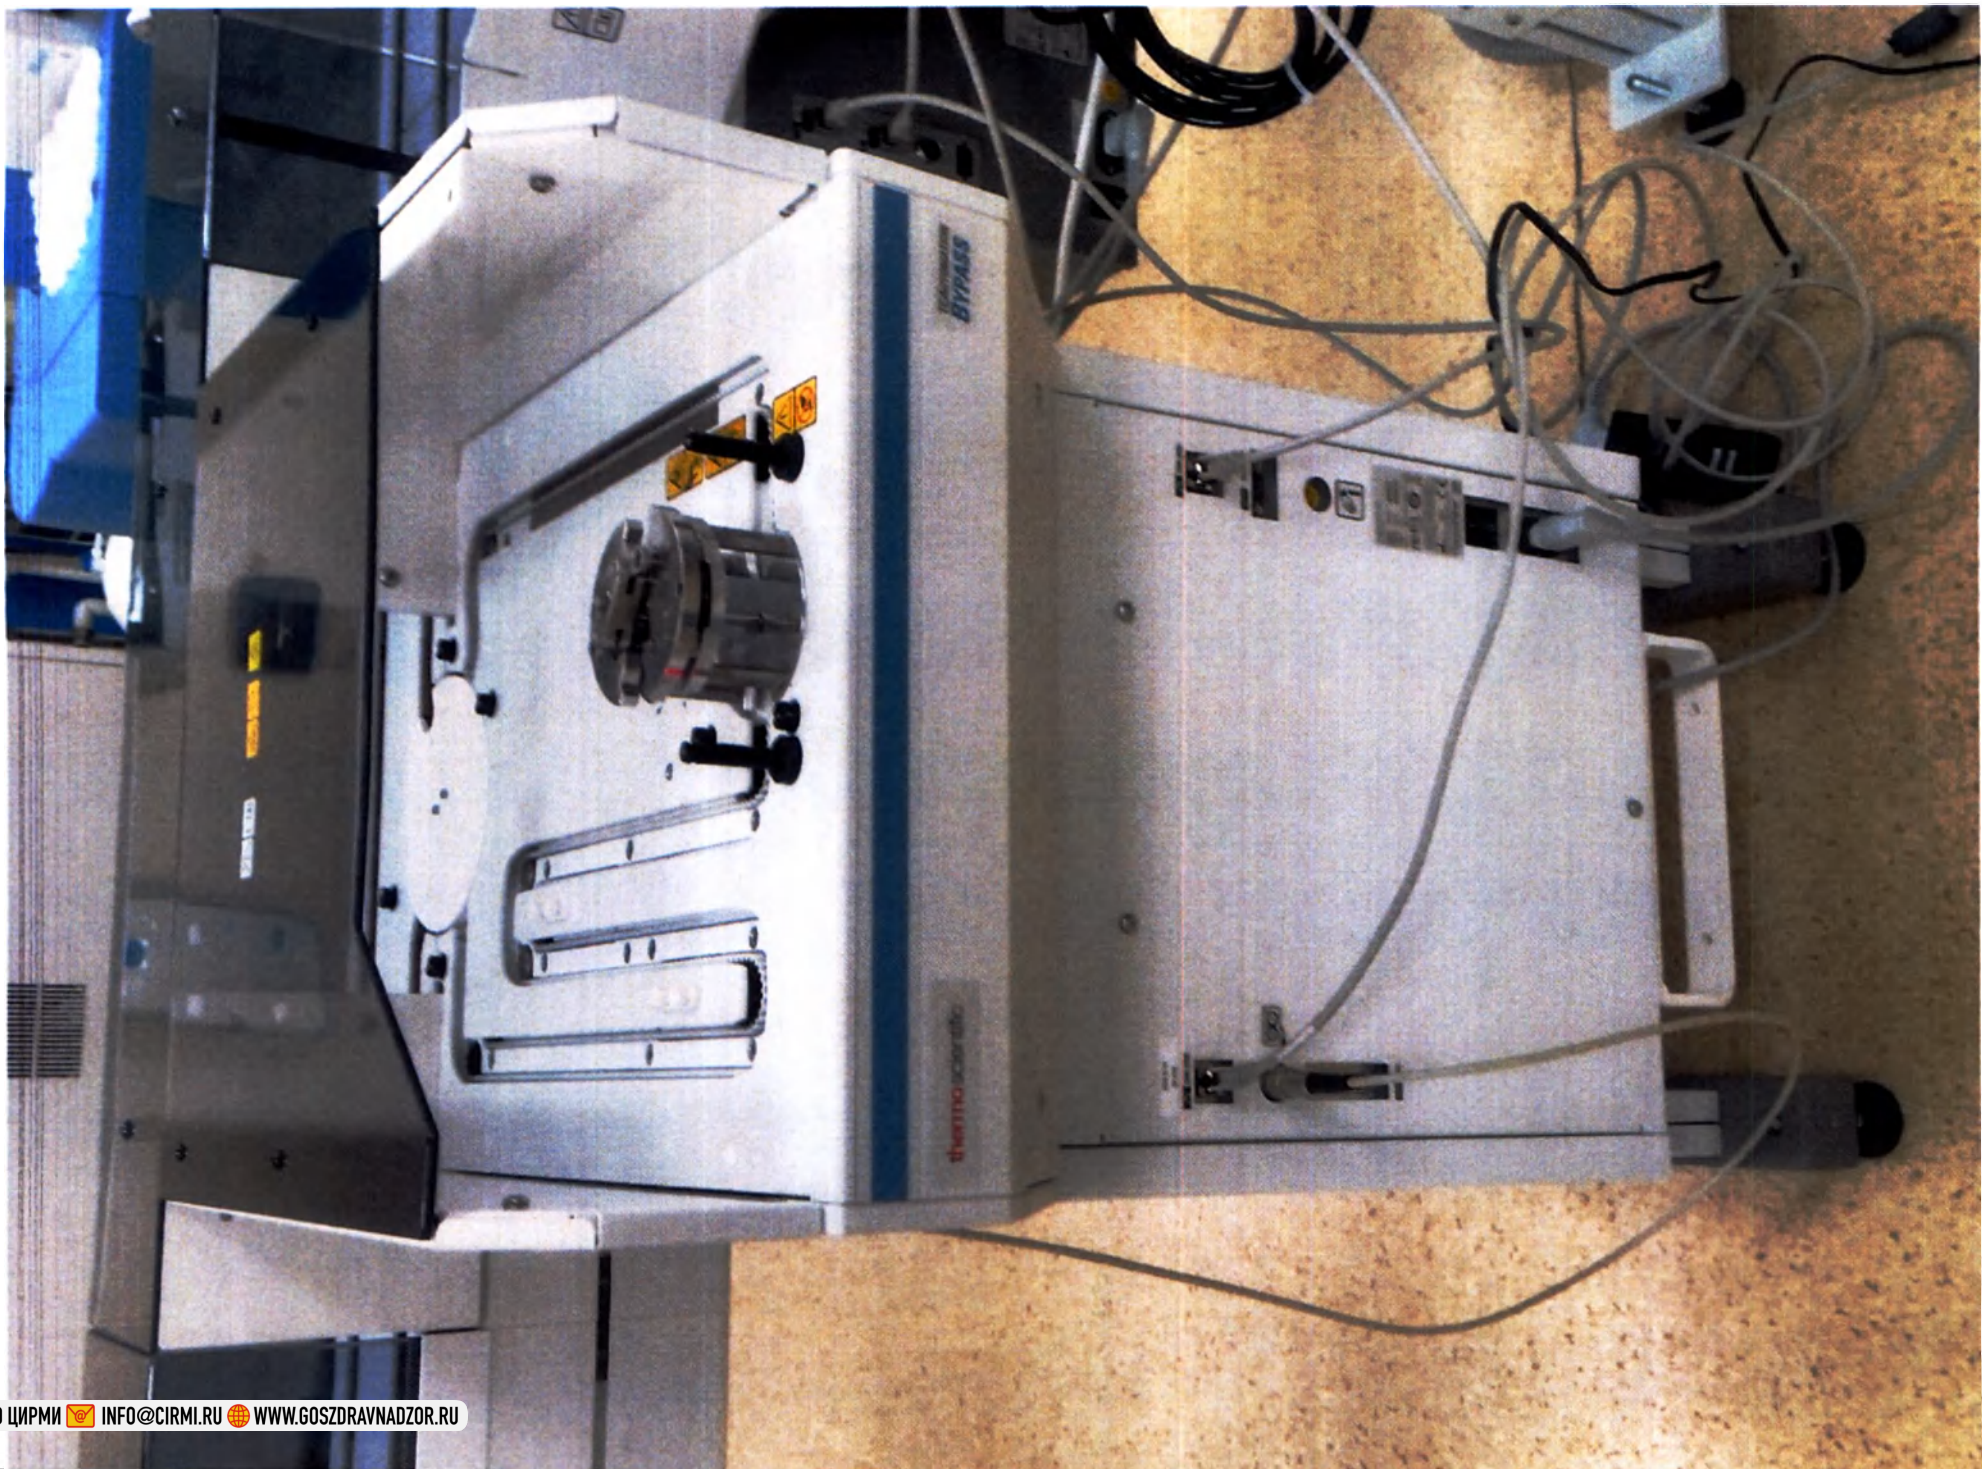

Parallel Bypass, TCA
IL ACL Top

REF

9522245



SN

58979



Type:

1041

Mains:

100-240Vac, 50-60Hz, 150W




710364



This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
1) This device may not cause harmful interference.
2) This device must accept any interference, including interference that may cause undesired operation, and can cause interference that may cause undesired operation.



2019




Made in Finland

ThermoFisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

ThermoFisher
SCIENTIFIC



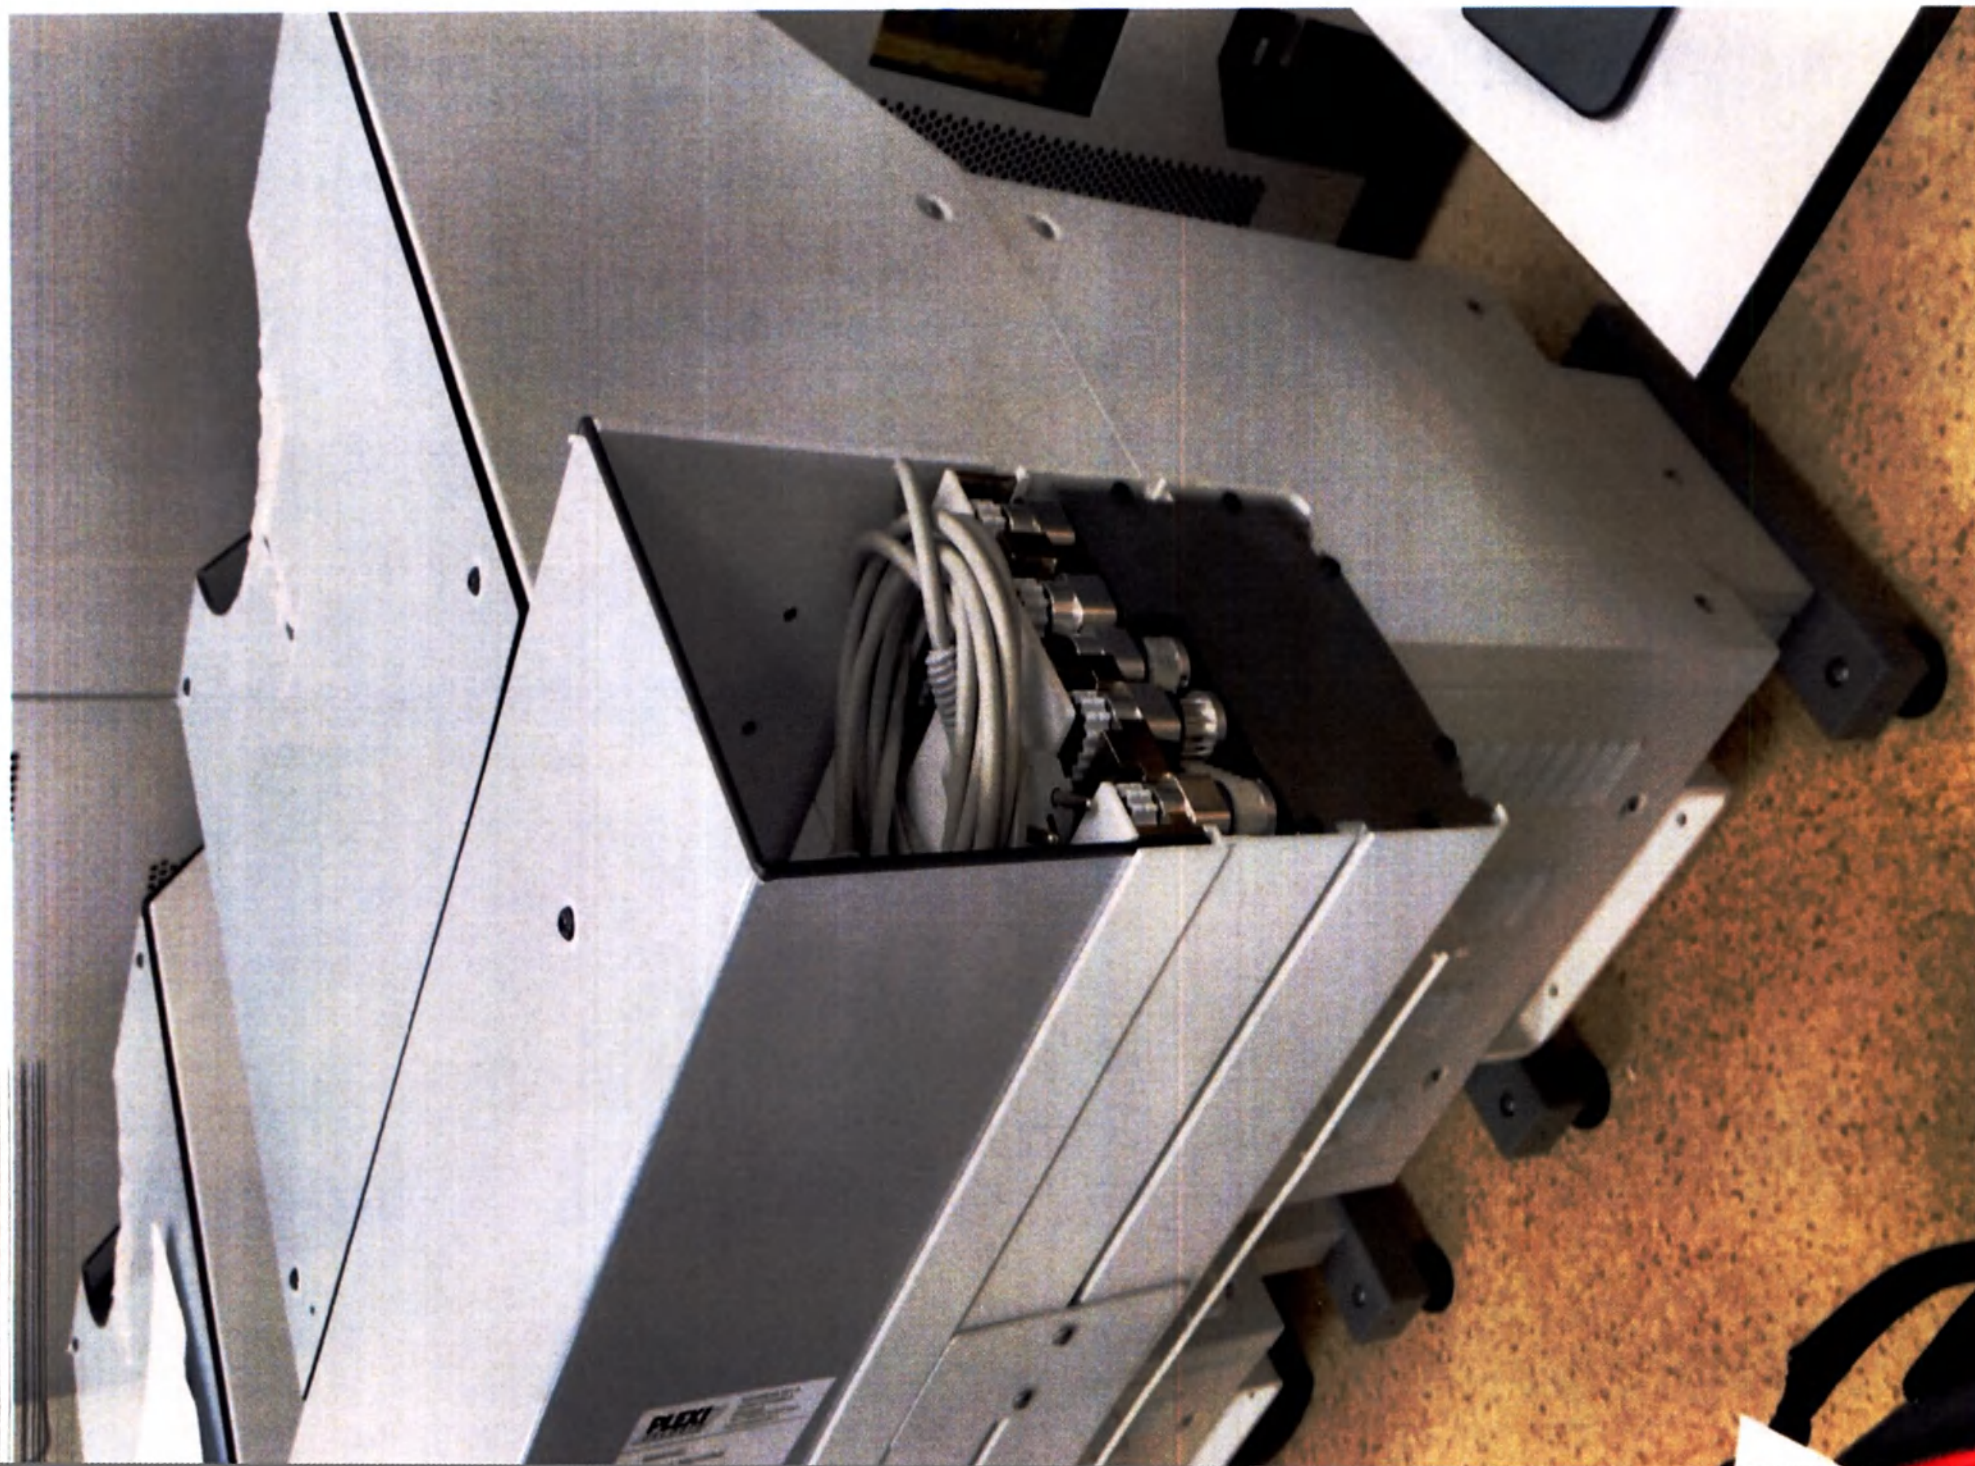

Parallel Bypass, TCA

Vitros 5.1 FS

REF

952131



SN

58978




Type:

1010

Mains:

100-240Vac, 50-60Hz, 150W



710364



This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.

CAN ICES-3(B)/NMB-3(B)

Made in Finland



2019

Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland



ThermoFisher
S C I E N T I F I C







Perpendicular Bypass, TCA
Vitros 5.1 FS AT

REF

952043



SN

58976




Type: 1011

Mains: 100-240Vac, 50-60Hz, 150W



This device complies with Part 15 of the FCC Rules.
Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) This device must accept any interference received,
including interference that may cause undesired operation.
CAN ICES-3(B)/NMB-3(B)

Made in Finland



Thermo Fisher Scientific Oy
Ratastie 2, FI-01620 Vantaa, Finland

ThermoFisher
SCIENTIFIC





WASTE DISPOSAL UNIT

REF 962085

Thermo Fisher Scientific Oy
Rautatie 2
FIN-01620 Vantaa
Finland

Thermo





DE: GEFÄHRLICHER BIOLOGISCHER ABFALL
FR: DÉCHETS PRÉSENTANT UN DANGER BIOLOGIQUE
EN: BIOHAZARDOUS WASTE
RU: ОПАСНЫЙ БИОЛОГИЧЕСКИЙ ОТХОД
PL: OPAKOWANIE ZAWIERAJĄCE WYKŁADZIKI BIOLOGICZNE
PT: RESÍDUO BIOLÓGICO PERIGOSO
NL: BIOLOGISCH GEVAARLIJKE AFVAL
IT: RIFIUTO BIOLOGICO DANGEROLO
ES: RESIDUO BIOLÓGICO PELIGROSO
FI: VAARALLINEN BIOLOGINEN JÄTTE

Date / Datum / Fecha

Sender / Absender / Expéditeur / Adressant / Ursender

Addressee / Empfänger / Destinataire / Destinatario / Bestemmings

Character / Inhalt / Contenu / Inhoud / Stoff



EN: BIOHAZARDOUS WASTE
DE: GEFÄHRLICHER BIOLOGISCHER ABFALL
FR: DÉCHETS PRÉSENTANT UN DANGER BIOLOGIQUE
RU: ОПАСНЫЙ БИОЛОГИЧЕСКИЙ ОТХОД
PL: OPAKOWANIE ZAWIERAJĄCE WYKŁADZIKI BIOLOGICZNE
PT: RESÍDUO BIOLÓGICO PERIGOSO
NL: BIOLOGISCH GEVAARLIJKE AFVAL
IT: RIFIUTO BIOLOGICO DANGEROLO
ES: RESIDUO BIOLÓGICO PELIGROSO
FI: VAARALLINEN BIOLOGINEN JÄTTE



EN: BIOHAZARDOUS WASTE
DE: GEFÄHRLICHER BIOLOGISCHER ABFALL
FR: DÉCHETS PRÉSENTANT UN DANGER BIOLOGIQUE
RU: ОПАСНЫЙ БИОЛОГИЧЕСКИЙ ОТХОД
PL: OPAKOWANIE ZAWIERAJĄCE WYKŁADZIKI BIOLOGICZNE
PT: RESÍDUO BIOLÓGICO PERIGOSO
NL: BIOLOGISCH GEVAARLIJKE AFVAL
IT: RIFIUTO BIOLOGICO DANGEROLO
ES: RESIDUO BIOLÓGICO PELIGROSO
FI: VAARALLINEN BIOLOGINEN JÄTTE


WASTE DISPOSAL UNIT

REF 952085

Thermo Fisher Scientific Oy
Ratastie 2
FIN-01620 Vantaa
Finland



Thermo

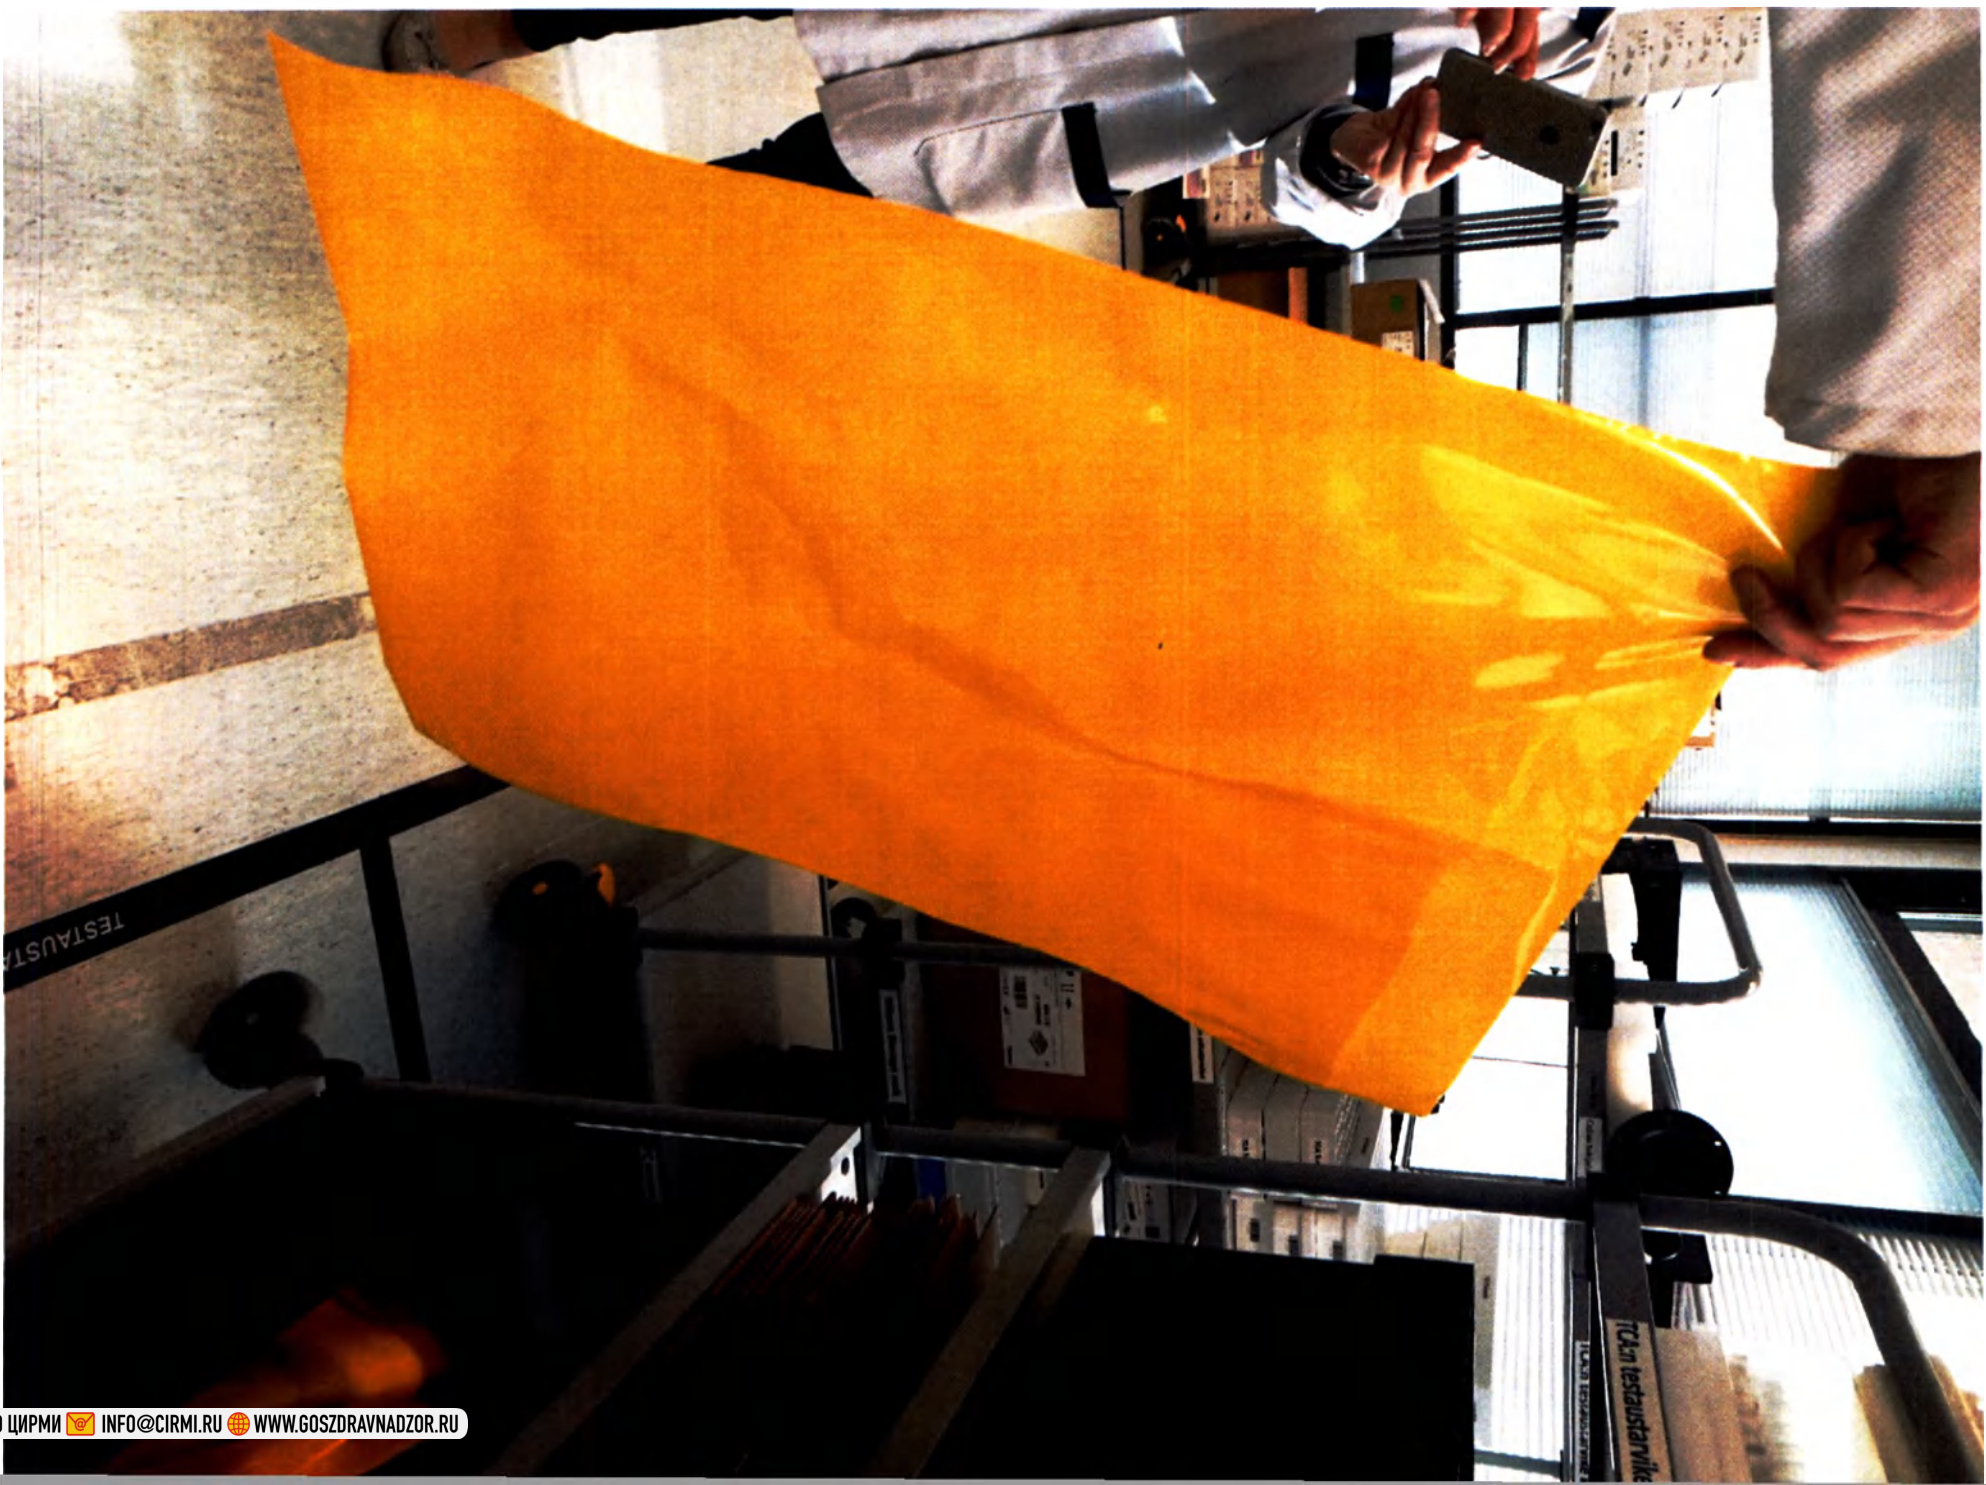





100% PE

Plastic Garbage Bag

(for Waste Disposal Unit)

REF 952086

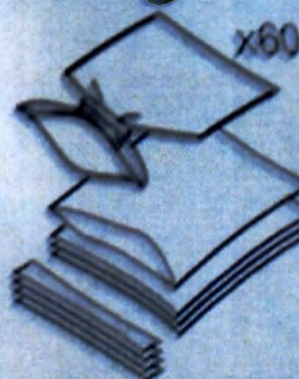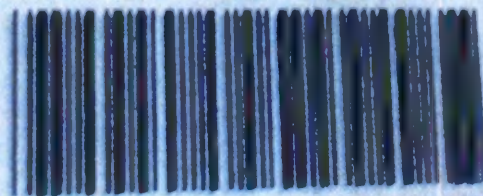

Thermo Fisher Scientific Oy
Ratatie 2
FI-01620 Vantaa
Finland

Part of Thermo Fisher Scientific

Thermo
SCIENTIFIC



NOTES

☔ ☹ ☯

TCA Storage Cap

REF 952314

GTIN 6 438153 004523

LOT 524489

4 bags of 1000 pcs.
(4000 pcs in total)



Country of origin: Netherlands

Thermo SCIENTIFIC

Thermo Scientific is a leader in laboratory equipment and reagents. For more information, please visit our website at www.thermo.com.





JUN-AIR®

www.jun-air.com

2xOF302-40M

SERIAL NO 0218801008

PS

12,2 bar

V

40 liter

T

0/40 C

ITEM NO: 1609207

VOLT: 230V~/50-60Hz

CURRENT

6,8 A

Year

02 2018



JUN-AIR®



Gast Manufacturing, Inc

A Unit of IDEX Corporation

2300 M-139, Benton Harbor, MI 49023

Tel: (269)926-6171 Fax: (800)331-3289

Made in USA using foreign and domestic components

Basic Kit: 2x5470400

Comp. Kit: 2x5470450

Controller USB Clear Case including
TCAutomation Software
TCA Operator Manual
LAS PC Win 10 Drive Image XE3 and
Controller PC Win 10 Drive Image XE3

H21130 Rev A
Image for Unit Optima XE3
TCA Controller (Win10)
SP01130

H21131 Rev A
Image for Unit Optima XE3
TCA LASPC (Win10)
SP01131

854110 TCAutomation
Software
Controller 4.5
LAS PC-4.5


TCAOM 5.03
TCAutomation
Operator Manuals

952276



TCA CONTROLLER INCLUDING SW (Win10)

1 pcs

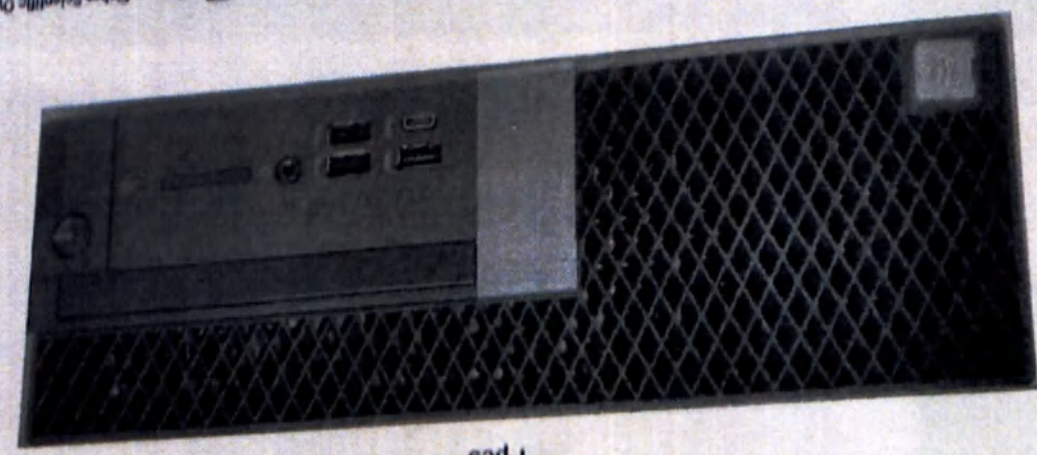

Thermo Fisher Scientific Oy
Ratatie 2,
FI-01620 Vantaa,
Finland

D19382-01



952277



LAS PC INCLUDING SW (Win10)


1 pcs



ThermoFisher Scientific Oy
Pohjois 2,
FI-01420 Vantaa,
Finland

ThermoFisher
SCIENTIFIC

010000-01

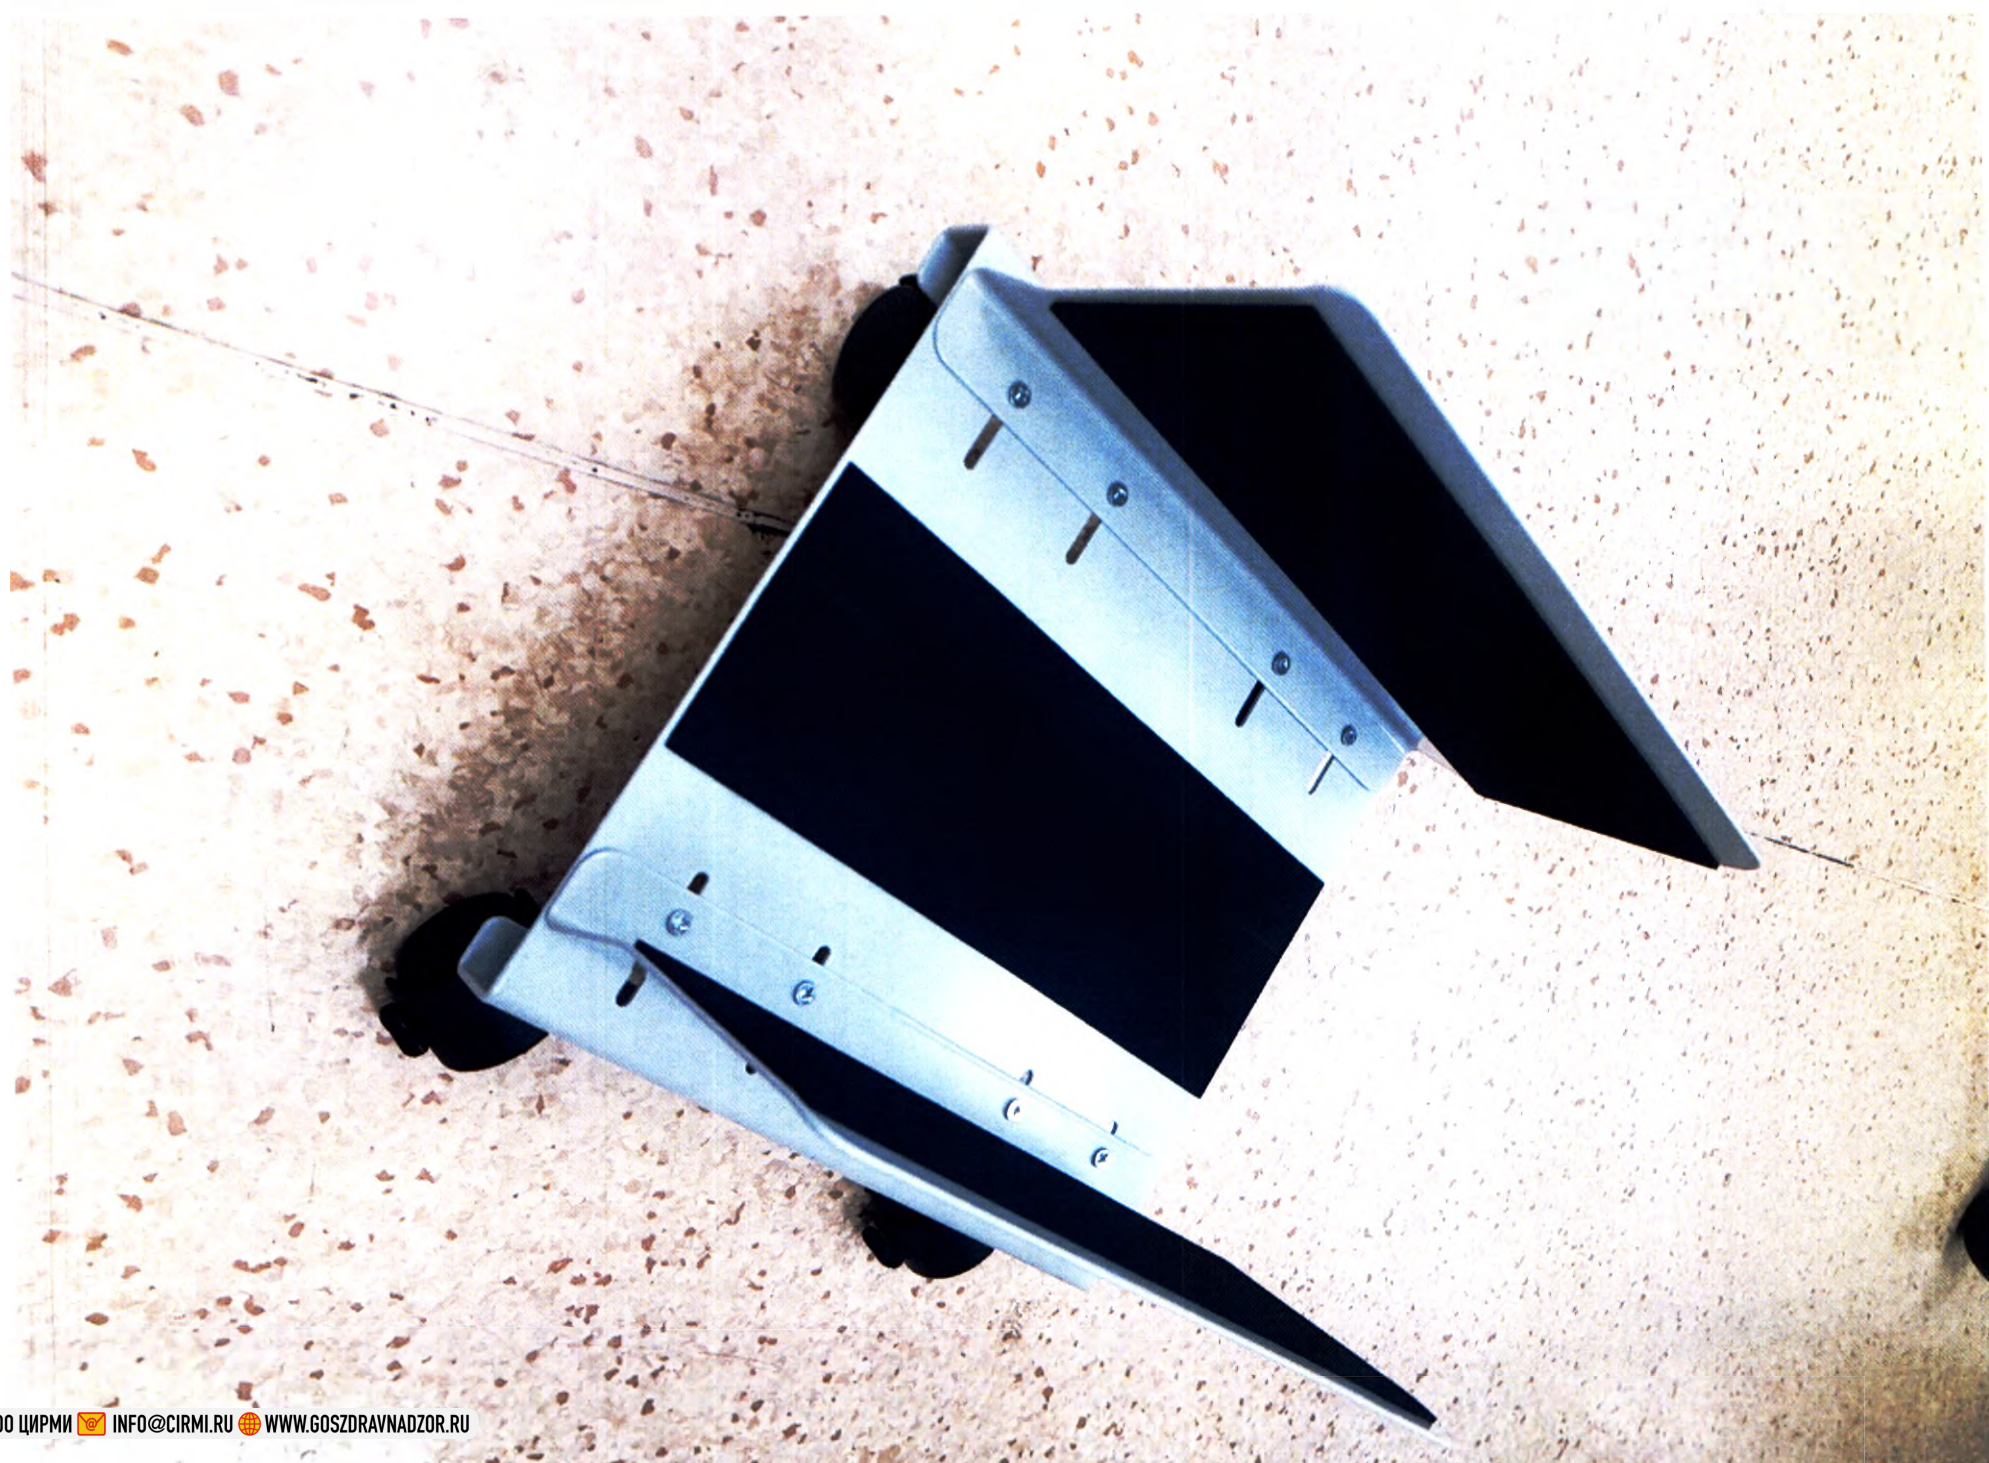





N13767

Tray for Multitube TCA Rack


REF 952237



GTIN




1 pcs

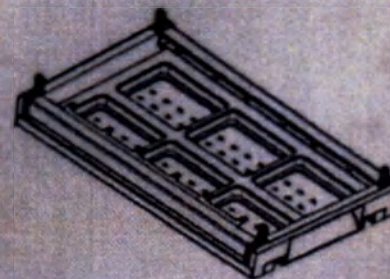

Thermo Fisher Scientific Oy
Ratastie 2,
FI-01620 Vantaa,
Finland

Thermo
SCIENTIFIC



Tray for 2xTCA MT Storage Slim rack

REF


952251



x1

Thomas Paster Scientific Oy
Rantaan 2
P.O. Box 1630 Vammala
Finland


Thomas Paster Scientific Oy



Tray for 2xTCA MT Storage Slim rack

REF

952251

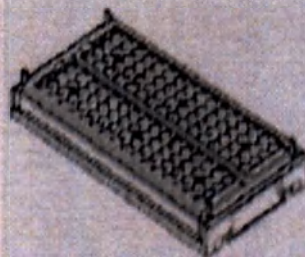


x 1



Thermo Fisher Scientific Oy
Ratastie 2
FIN-01620 Vantaa
Finland

www.thermo.com/tcautomation

Thermo
SCIENTIFIC

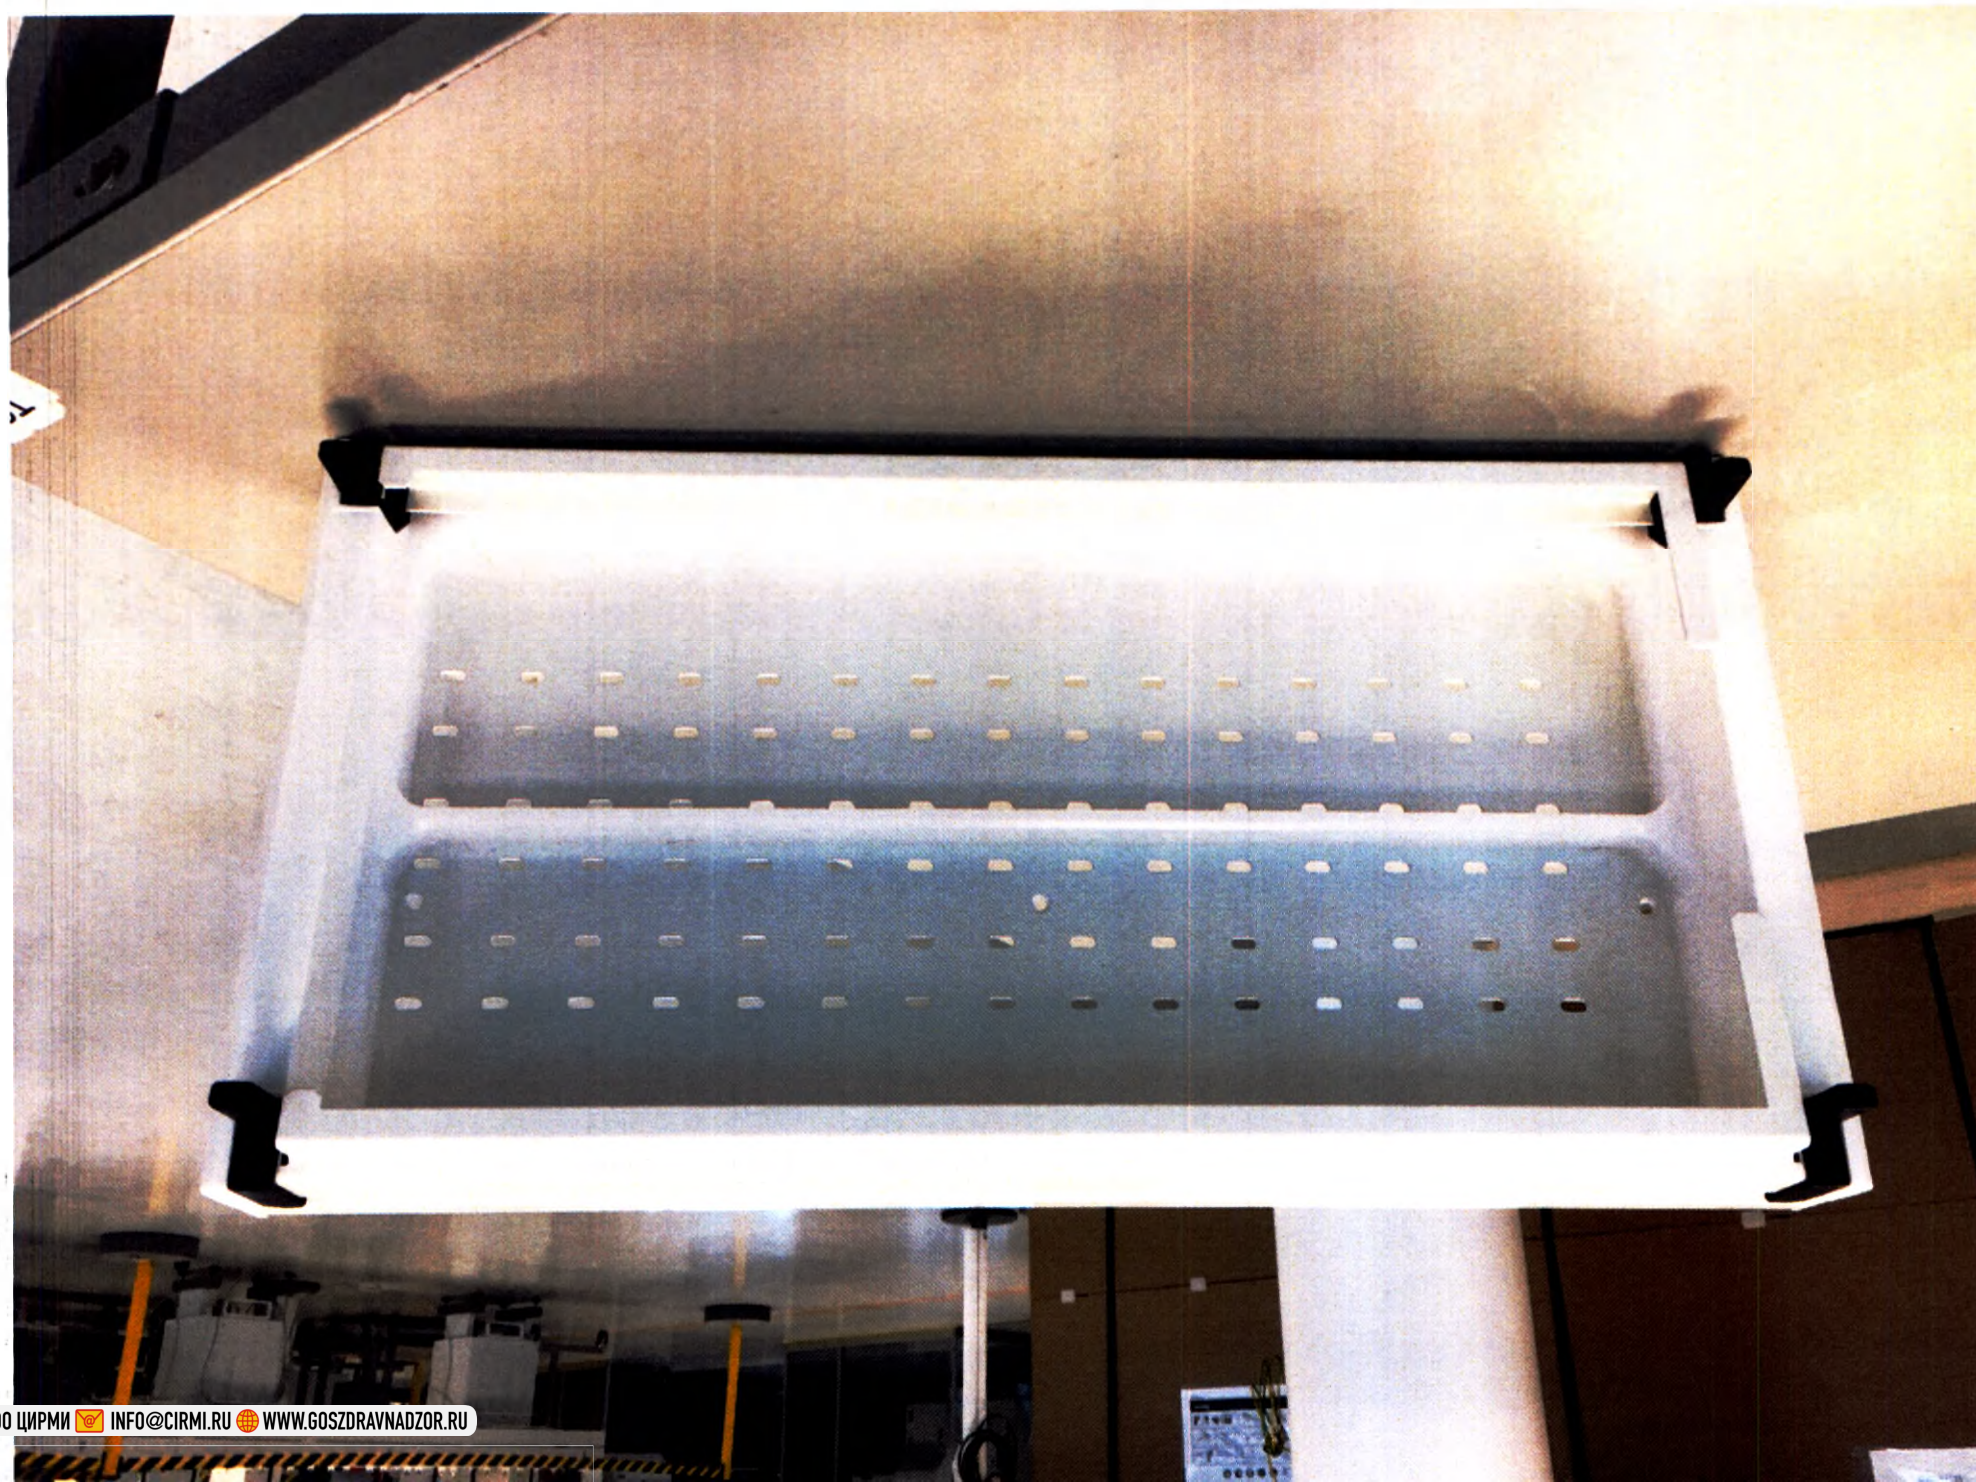



Tray for 2x Storage Rack Slim for 80 sample pos.

(13mm tubes) ES Flex


REF

952282




1 pcs

GTIN

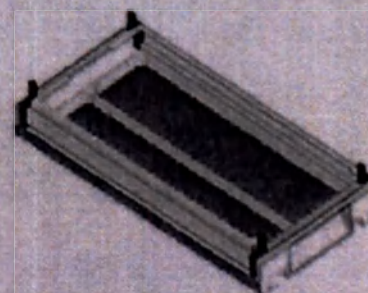

Thermo Fisher Scientific Oy
Ratastie 2,
FI-01620 Vantaa,
Finland

Thermo
SCIENTIFIC

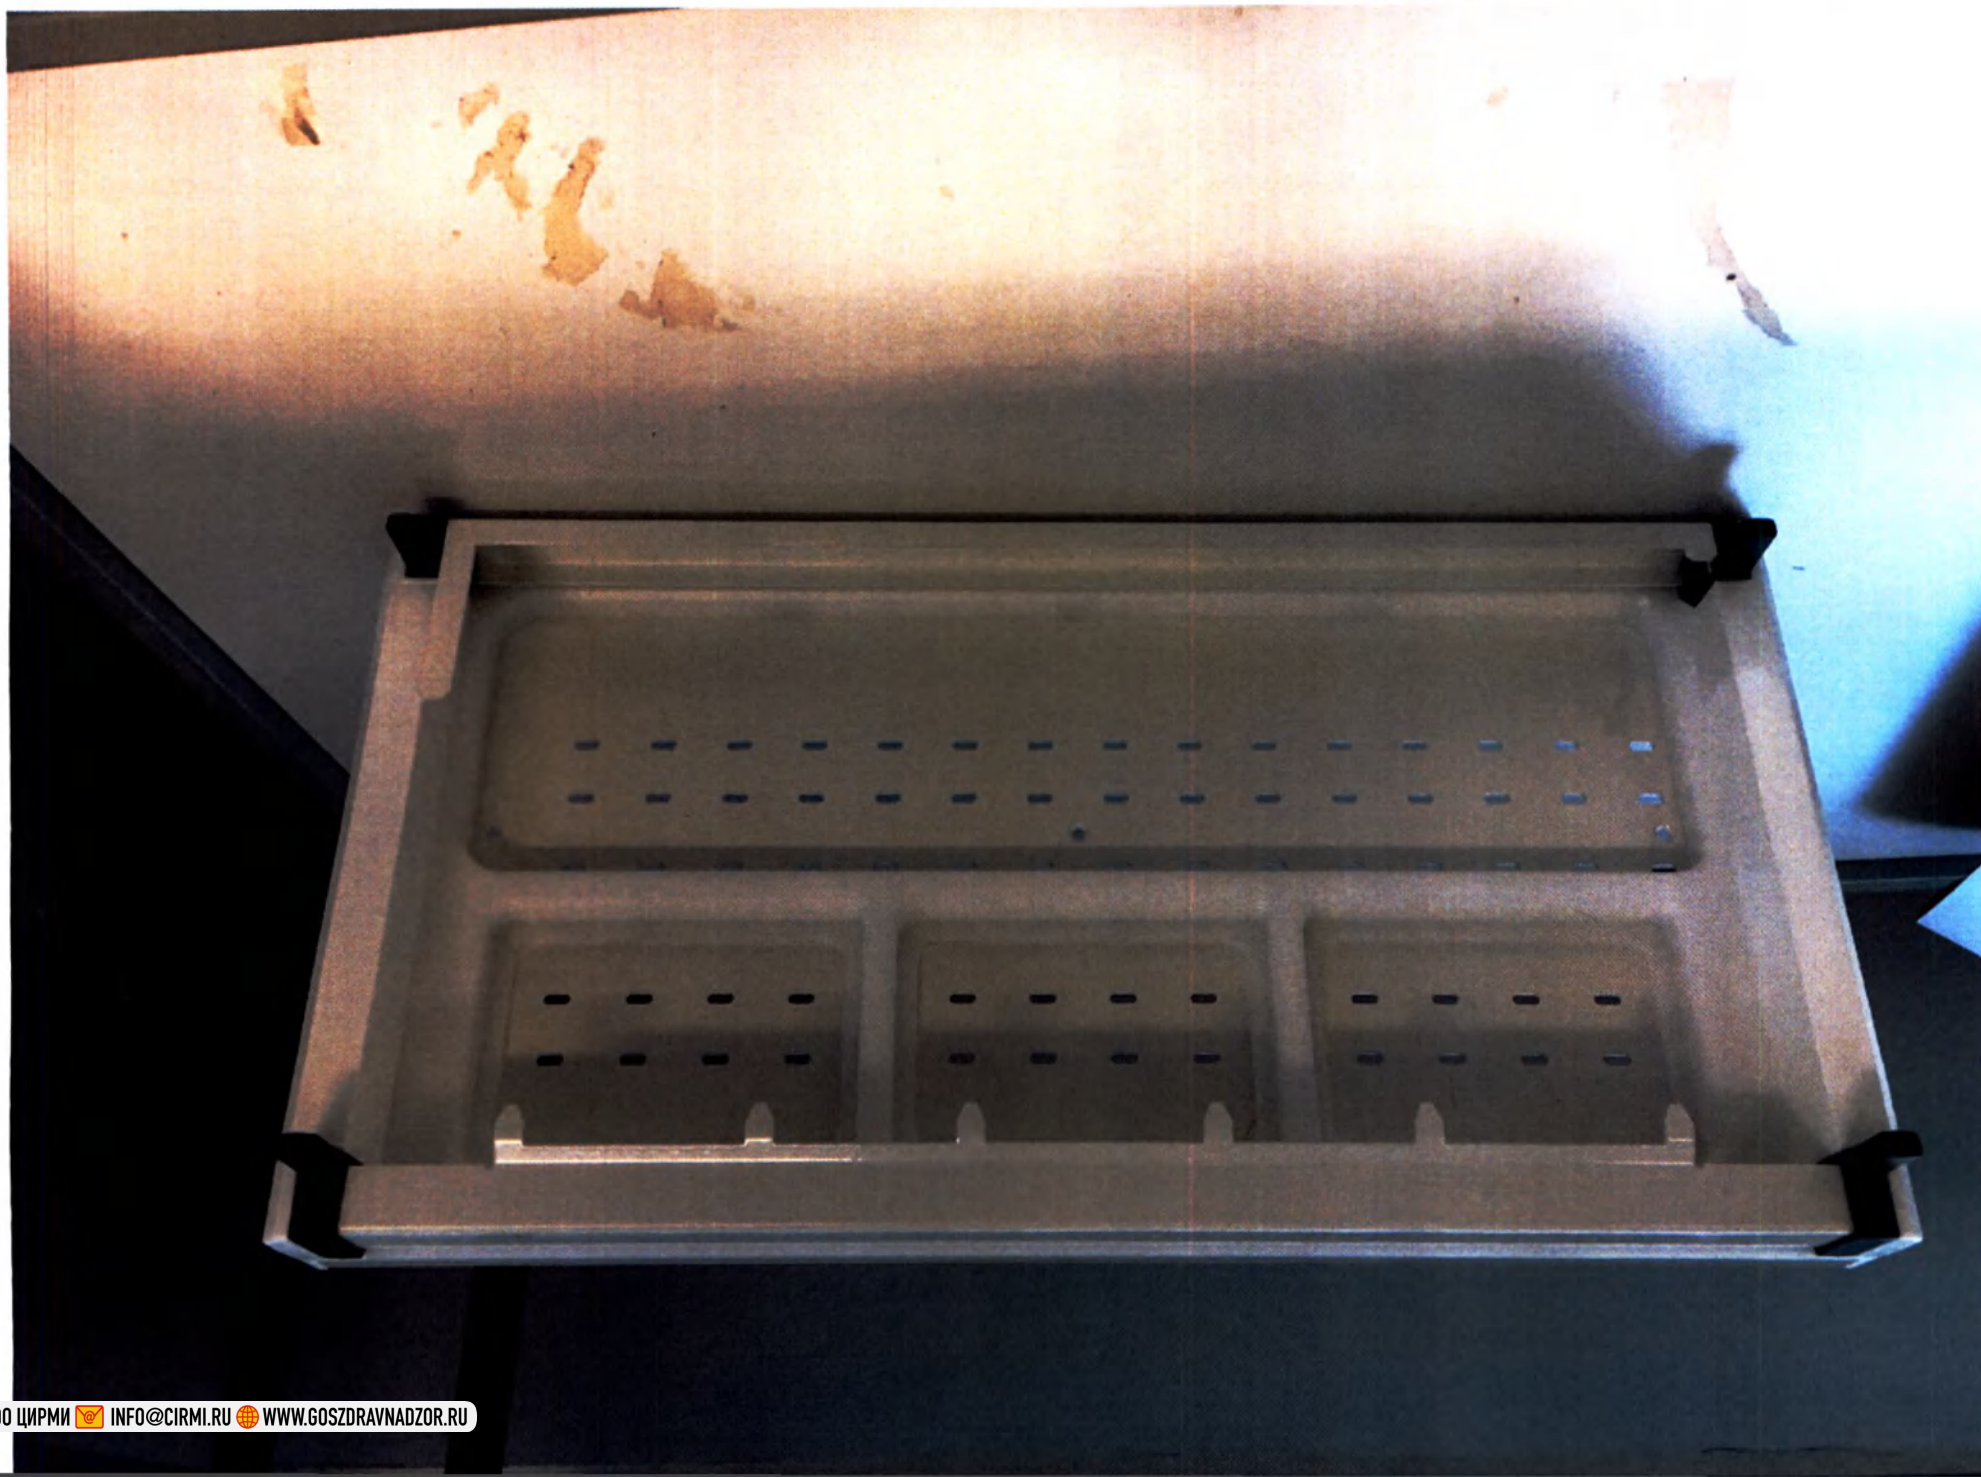



1 pcs




6 438163 002536



Thermo Fisher Scientific Co.
Scientific &
PLASMA Vectors
United

Thermo
SCIENTIFIC

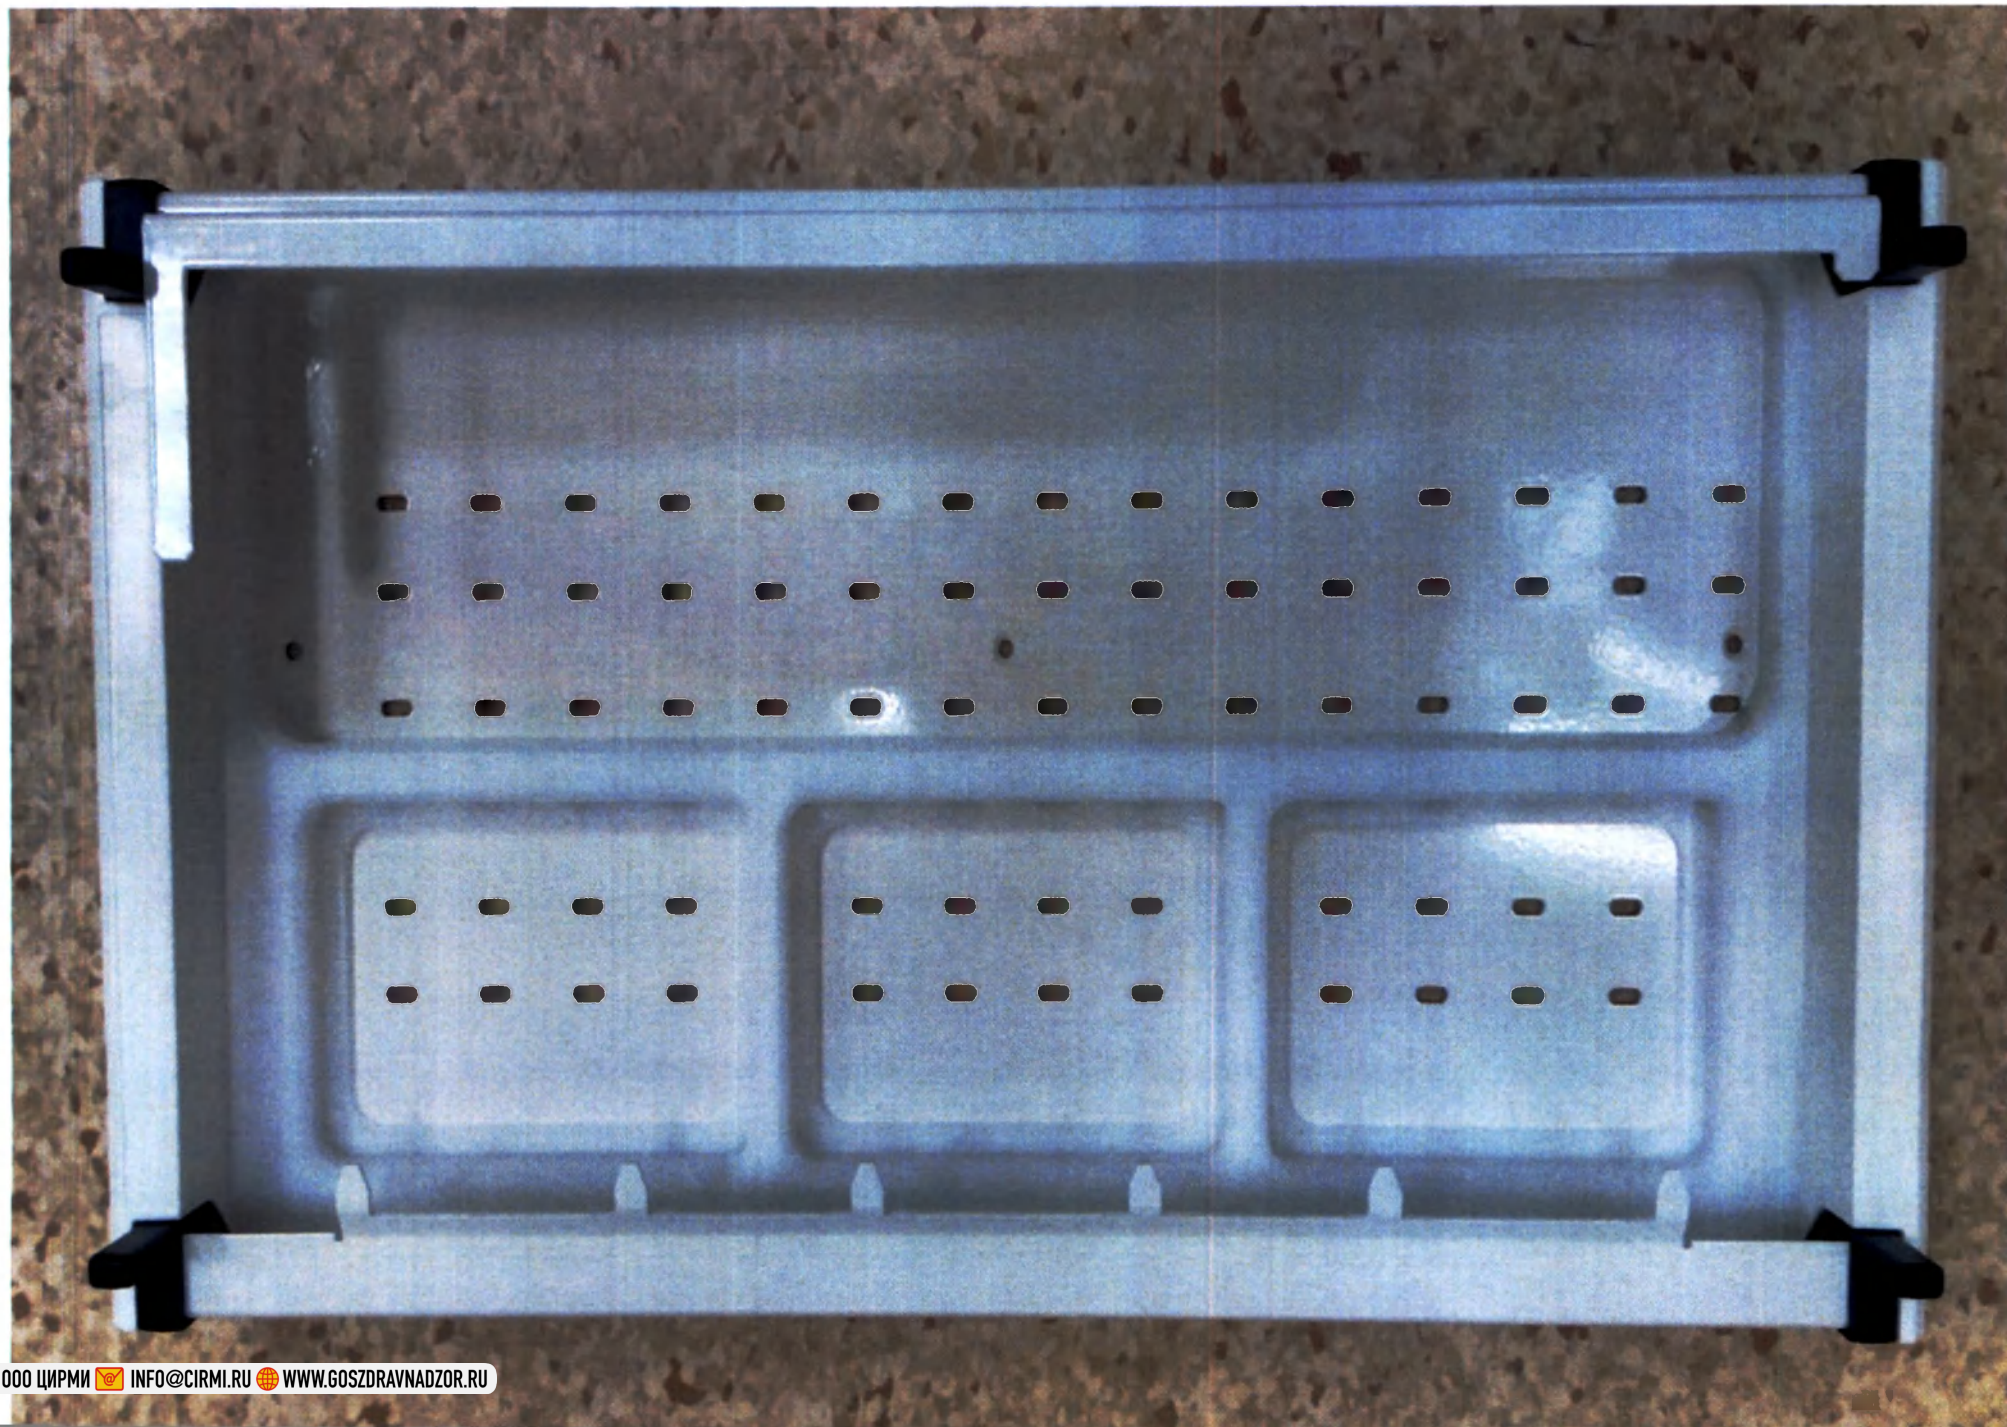



0N1873740

Tray for TCA Storage Rack Slim + 3 x Multitube TCA Rack


REF 952284



GTIN



6 438153 004721

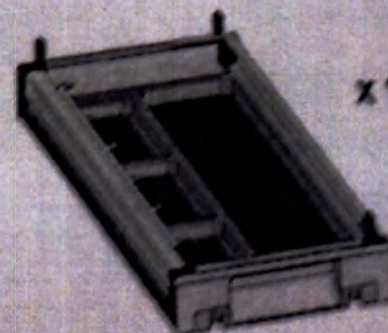



x1



ThermoFisher Scientific Oy
Pietari 2,
FI-01520 Vantaa,
Finland

Thermo
SCIENTIFIC

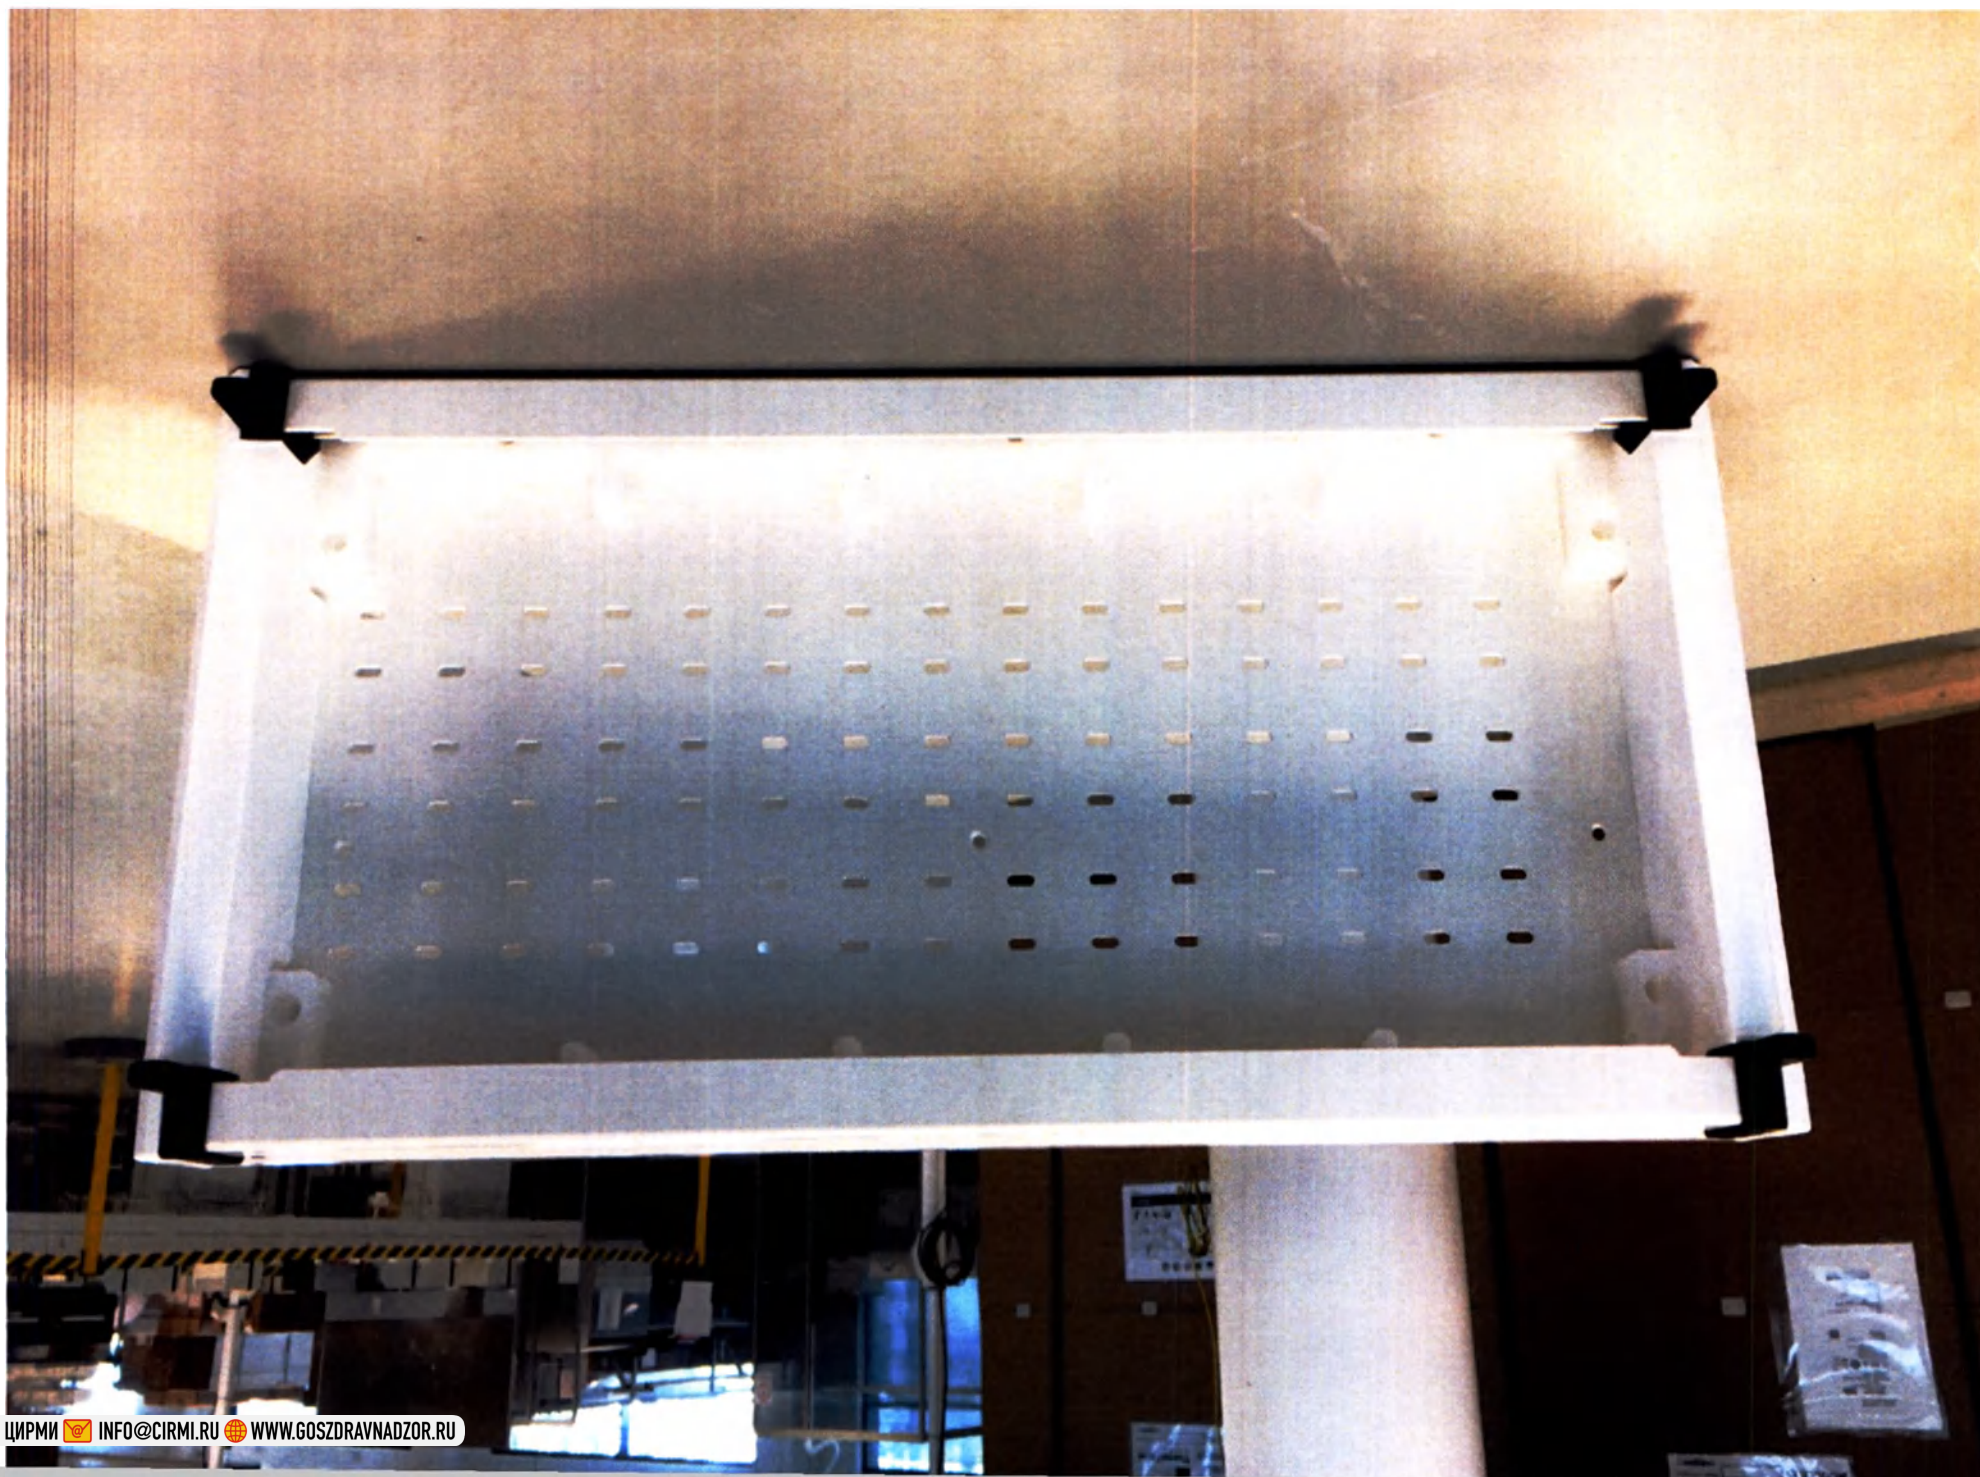




Tray for Transport Rack

REF

952253




x 1



Thermo Fisher Scientific Oy
Ratastie 2
FIN-01620 Vantaa
Finland

Thermo
SCIENTIFIC

www.thermo.com/tcautomation

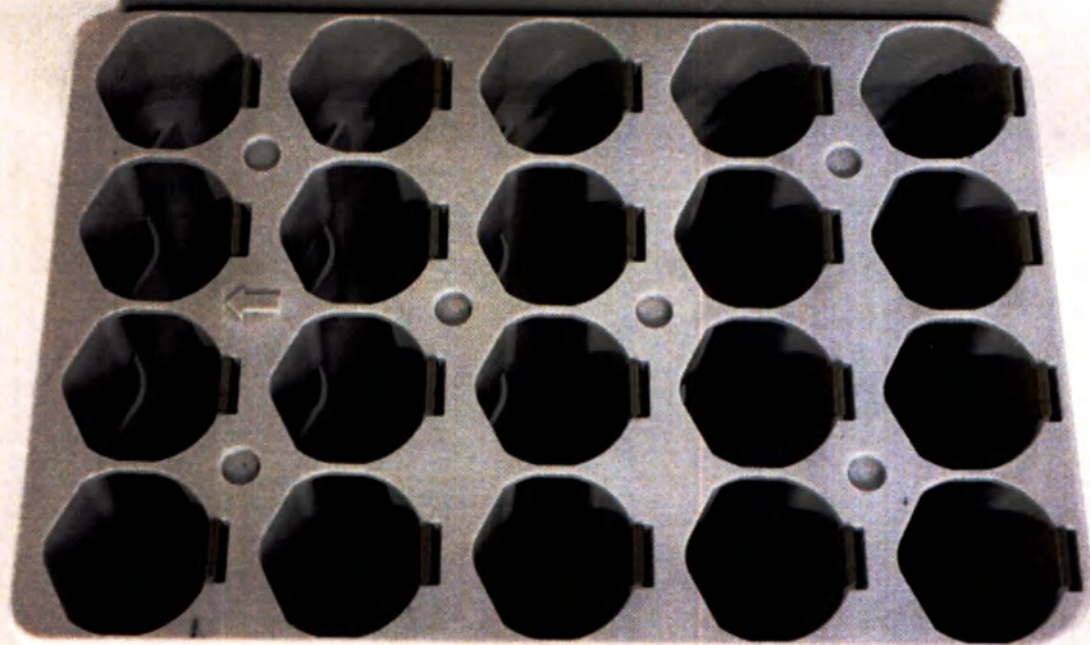



DN13756-0

Multitube TCA Rack - White

10 pcs

REF


952236



GTIN




6 438 153 002 550

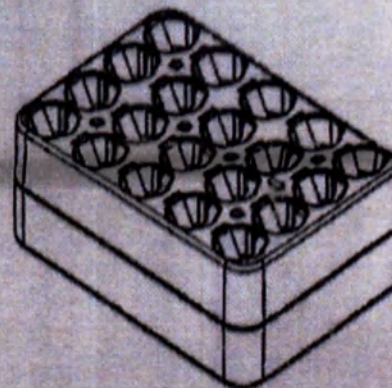



Thermo Fisher Scientific Oy
Ratastie 2,
FI-01620 Vantaa,
Finland


Thermo
SCIENTIFIC

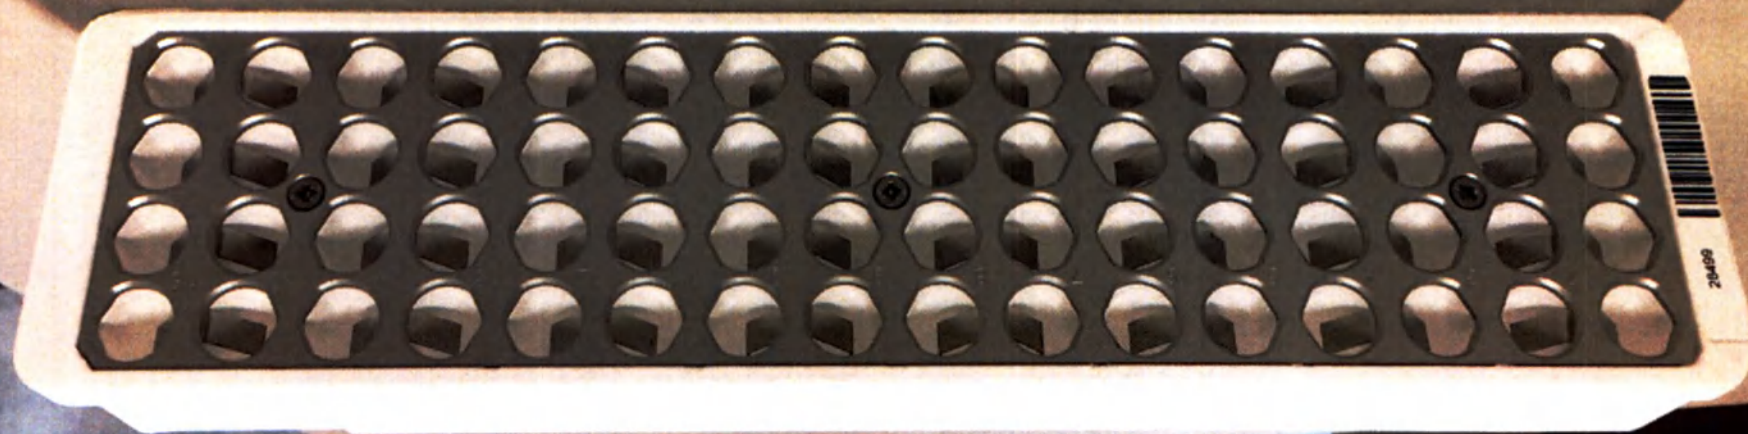

1 Box (1000)
www.thomsonrussia.ru
TCA MT Storage Slim Rack
x 10
952164
Thomson Russia Scientific Co.
Petrovskiy
x 10
952164
Petrovskiy
x 10
952164
Petrovskiy

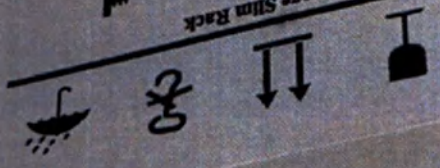

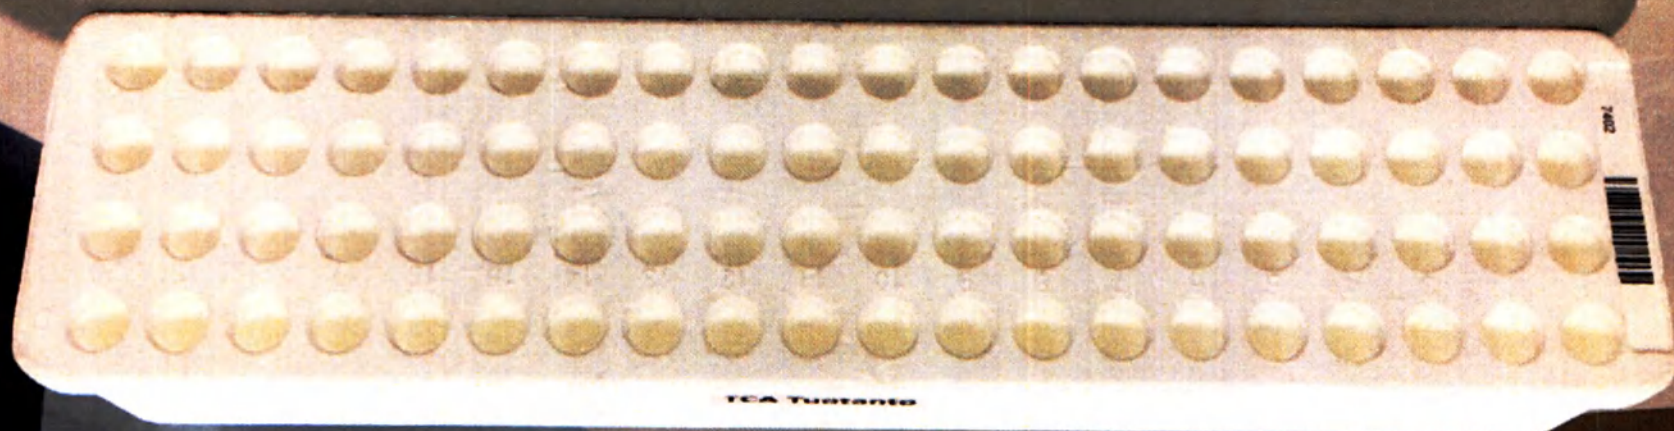




Storage Rack Slim for 80 Sample pos.
(13mm tubes) ES Flex

REF 952249

GTIN




10 pcs



Thermo Fisher Scientific Oy
Rusnarkki 2,
Pohjois-Vantaan,
Finland

Thermo
SCIENTIFIC

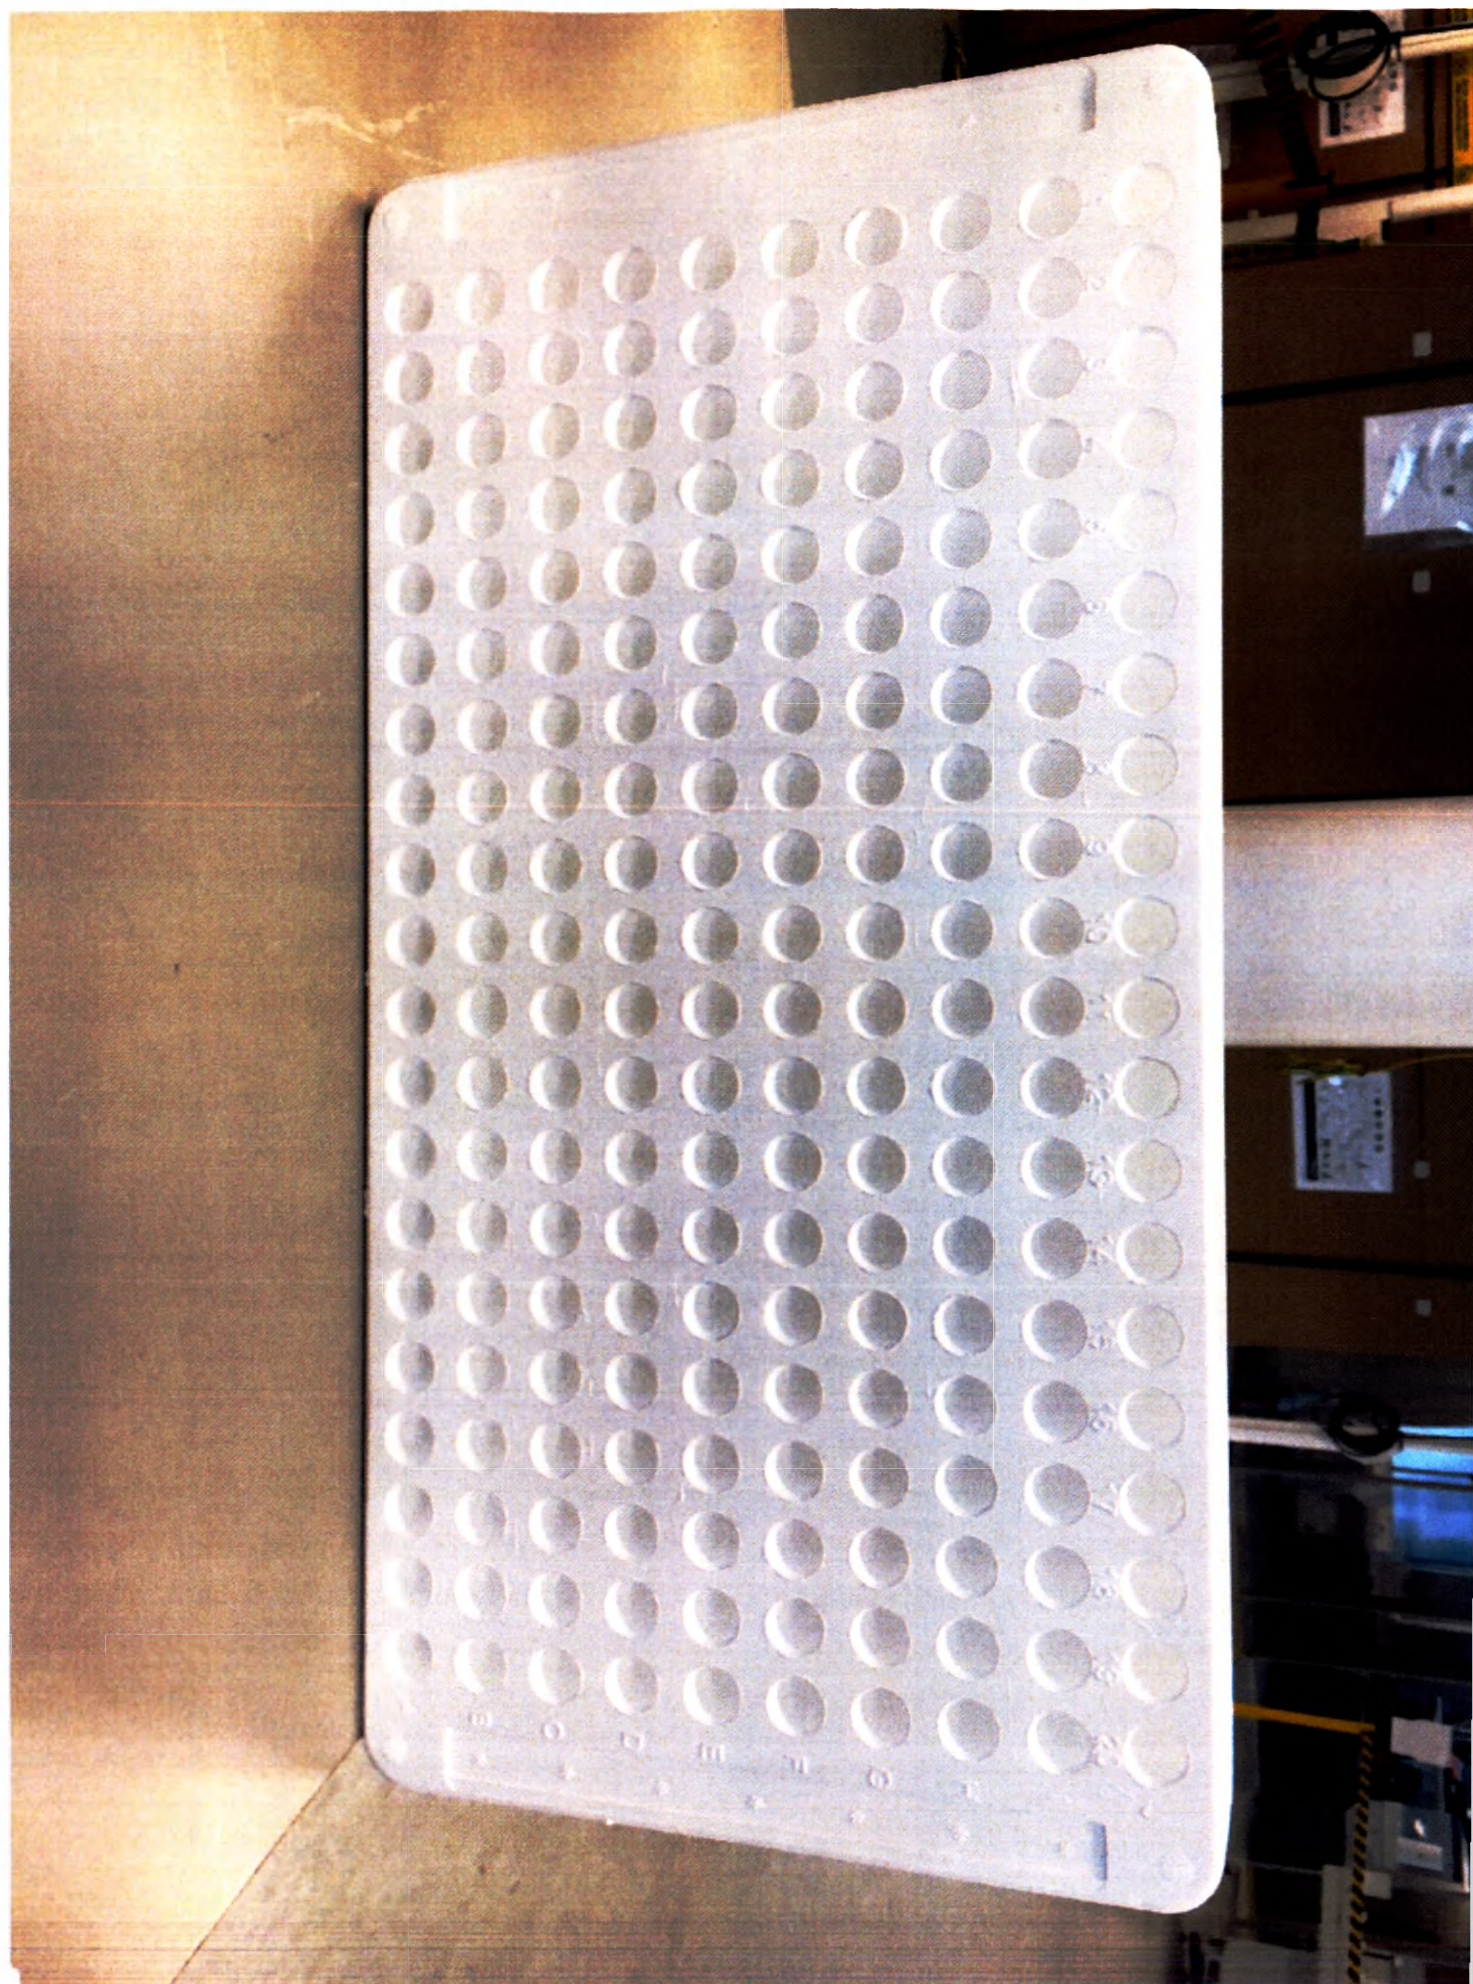



Storage rack for 200 sample pos.


(13mm tubes) ES Flex

REF 952280

GTIN





10 pcs



Thermo Fisher Scientific Oy
Russettinkatu 2
00050 Vantaa,
Finland

Thermo
SCIENTIFIC

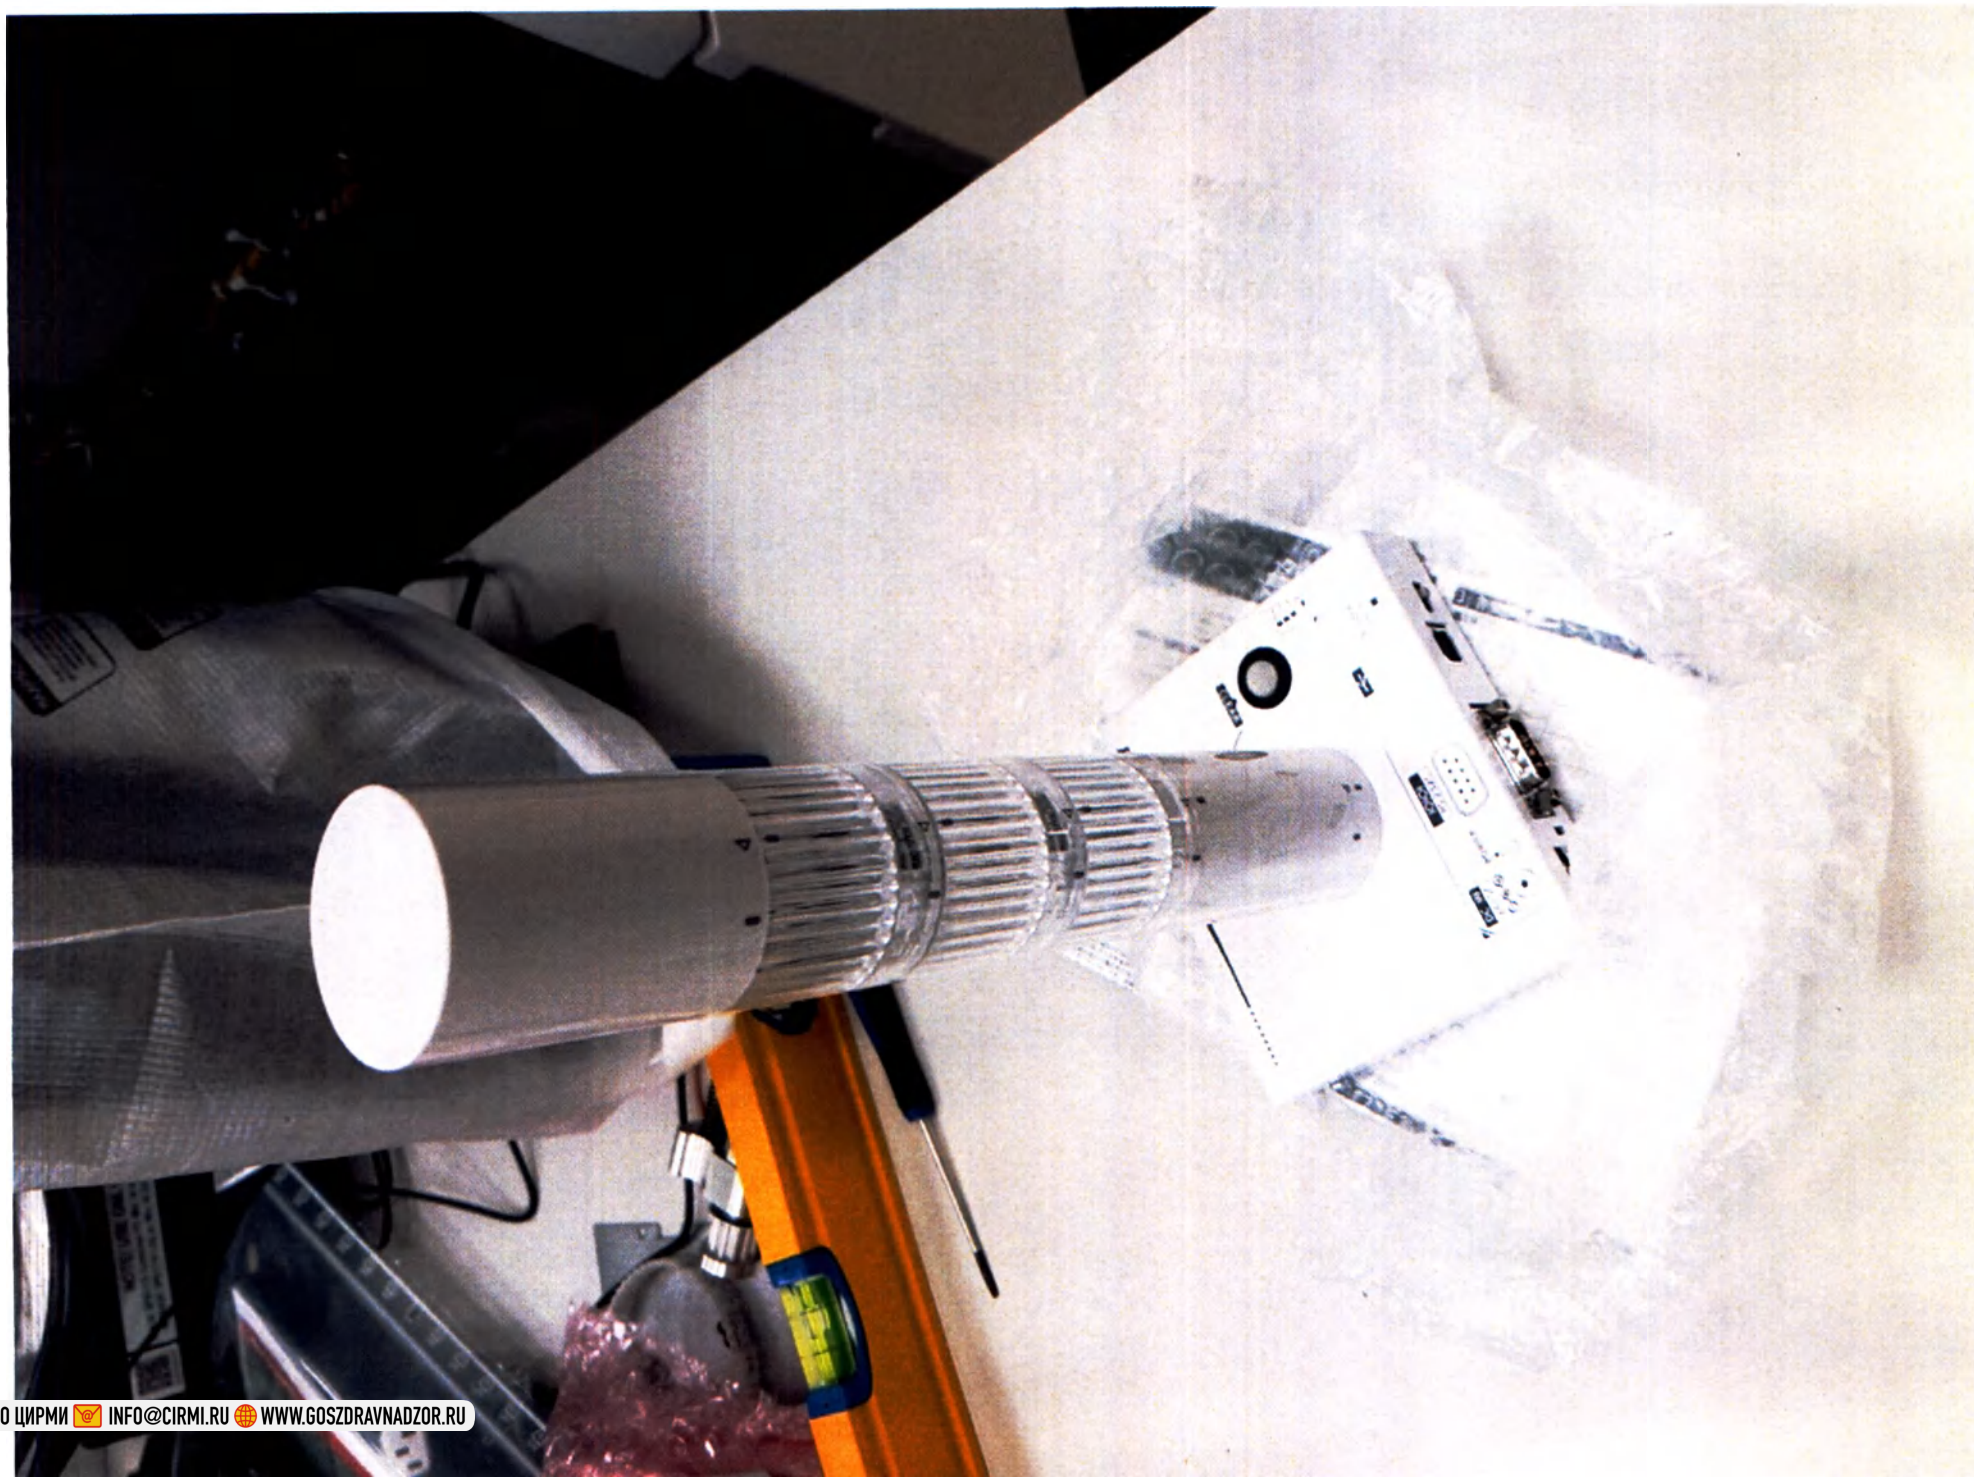

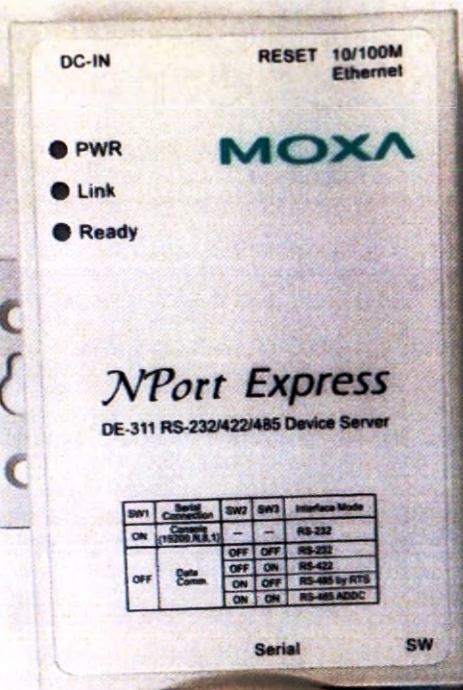








N15957
Power supply 24V





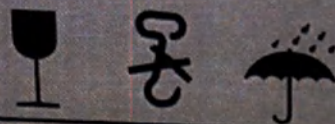


117490120

PC-Controlled Signal tower light with MOXA

REF 952271

GTIN

SN



1 pcs




Thermo Fisher Scientific Oy
Rataatie 2,
FI-01820 Vantaa,
Finland


Assembled in Finland

Thermo
SCIENTIFIC



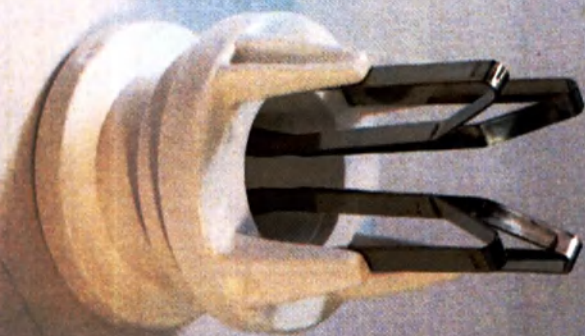



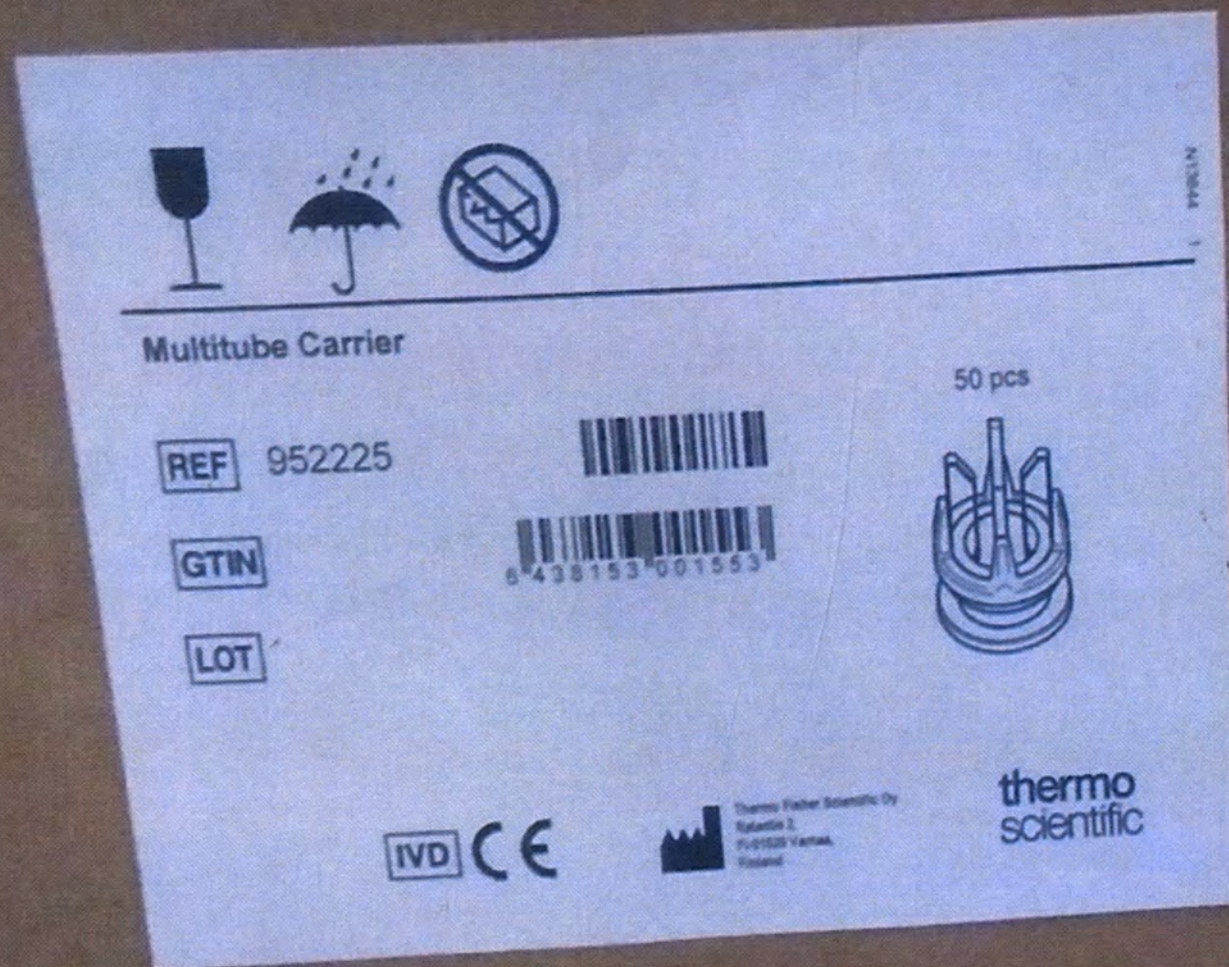

Прошито, скреплено печатью

ВСЕГО 78 листов

« 02 » 08 2021 г.

Генеральный Директор

ООО «Орто-Клиникал Диагностика»

Сергеенко В.К.

