

Boston
Scientific


Pt Cr

Promus PREMIER™ MONORAIL™

Everolimus-Eluting Platinum Chromium Coronary Stent System

Sistema de stent coronario de platino-cromo con liberación de everolimus. Système de stent coronaire en alliage platine-chrome à élution d'everolimus. Everolimus-abgebendes Platin-Chrom-Koronarstentsystem. Sistema de stent coronario de platino-cromo a rilascio di everolimus. Everolimus eluerend coronare stentsysteem van platina-chroom. エベロリムス放出型プラチナ・クロム冠動脈ステントシステム. Everolimus eluerende platina-krom koronarstentsysteem. Συστήμα στεφανιαίου stent (αγγειοπλαστική) εκκλυόν everolimus. Sistema de Stent Coronario de Crômio e Platina com Eluição de Everolimus. Everolimus-eluerende koronarstentsysteem i platina-krom. Everolimus-kibocsato platina-krom szívkoronár-szűzéstendizer. System stentu w wielocowym ze stopu platyny i chromu uwalnający everolimus. Everolimus-avgivanda koronarstentsystem av platnakrom. Everolimus Salarmibi Platin Krom Koroner Stent Sistem.

Controls (1)



ID 4.25mm

Minimum Bend Radius

GW ≤ 0.014in (0.35mm)

Maximum recommended

≥ 0.056in (1.42mm)

Recommended Guide Catheter

mm	MPa	Stent I O	Stent O O
8 - 854	3.24	3.43	
9 - 910	3.36	3.54	
10 - 1014	3.43	3.62	
11 - 1117	3.51	3.70	
12 - 1219	3.58	3.77	
13 - 1317	3.63	3.82	
14 - 1420	3.68	3.87	
15 - 1517	3.73	3.92	
16 - 1620	3.77	3.96	
17 - 1724	3.81	4.00	
18 - 1827	3.85	4.04	
19 - 1924	3.91	4.10	
20 - 2027	3.97	4.16	
21 - 2120			
22 - 2227			

Stent Body Pressure, DO NOT EXCEED

(2) Includes CLIP™

(2) Includes Hypoheal Clip

(1) Includes Flushing Nozzle

with Laser Etching

REF Catalog No.

39251-2035

Use By

2015-09

DO NOT

USE

Store at 25 °C (77 °F)

avoid exposure to moisture

15-30 °C (59-86 °F)

Protect from

Humidity

Protect from

Light

Do not open foil pouch

until ready for use

See foil pouch and carton

label for Use By date

Promus PREMIER™		MONORAIL™		3.50 20
 9024534-01		 9024534-01		Promus PREMIER™ MONORAIL™ 3.50mm x 20mm REF 39251-2035 LOT 16899596
 *44262835 2035-20*		 *44262835 2035-20*		Promus PREMIER™ MONORAIL™ 3.50mm x 20mm REF 39251-2035 LOT 16899596
Made in IRELAND Ballybrack Business Park Galway, IRELAND				
CE 0344		Product No UPN 47493925120350		
LOT 16899596		Sterilized using ethylene oxide		
STERILE EO				



Boston
Scientific



10 07980026

Pt
Gr

R ONLY


EC REP
EU Authorized Representative
Boston Scientific Corporation S.A.
55 Avenue des Champs Elysees
75008 PARIS
FRANCE


Legal

Manufacturer:
Boston Scientific Corporation
One Boston Scientific Place
Natick, MA 01913-1527
USA Customer Service 800-272-1001

- For single use only.
- Do not reuse.
- Do Not Sterilize
- Consult instructions for use.
- Do not use if package is damaged.

Стент коронарный Promus Premier с лекарственным покрытием предустановленный на системе доставки.

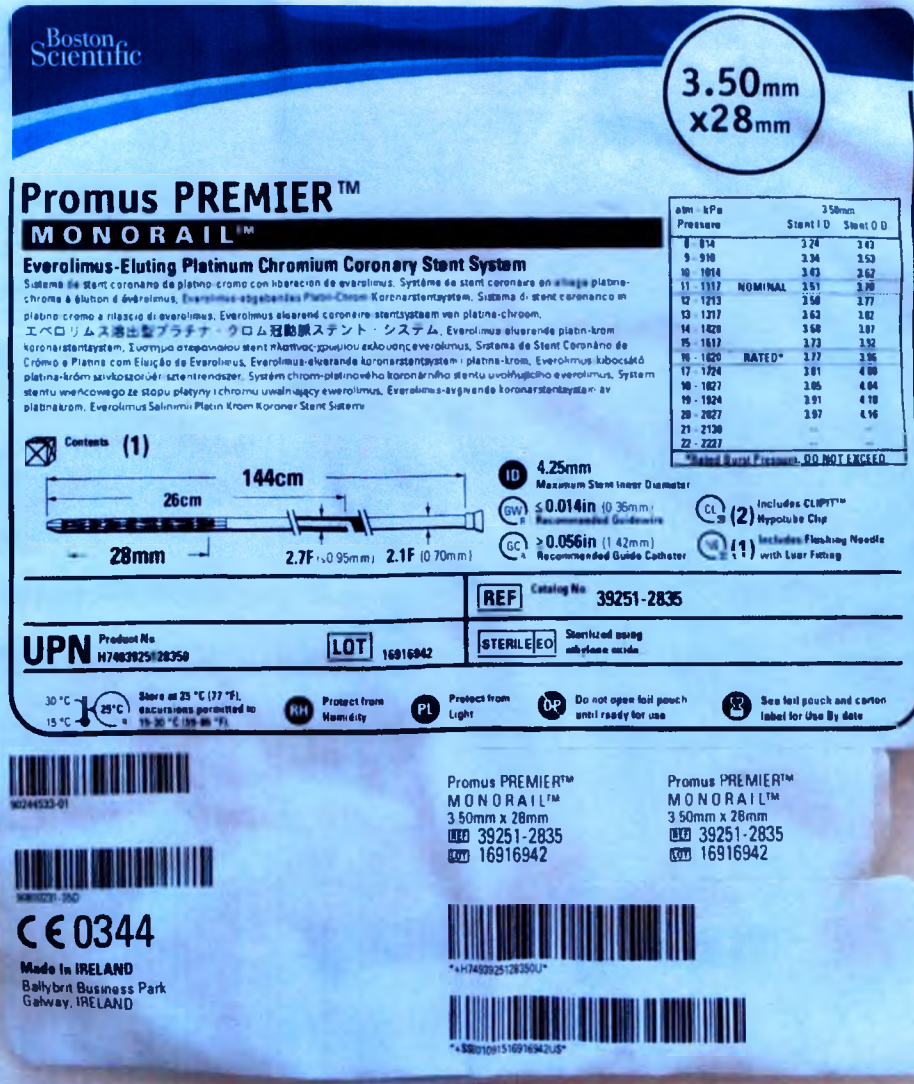

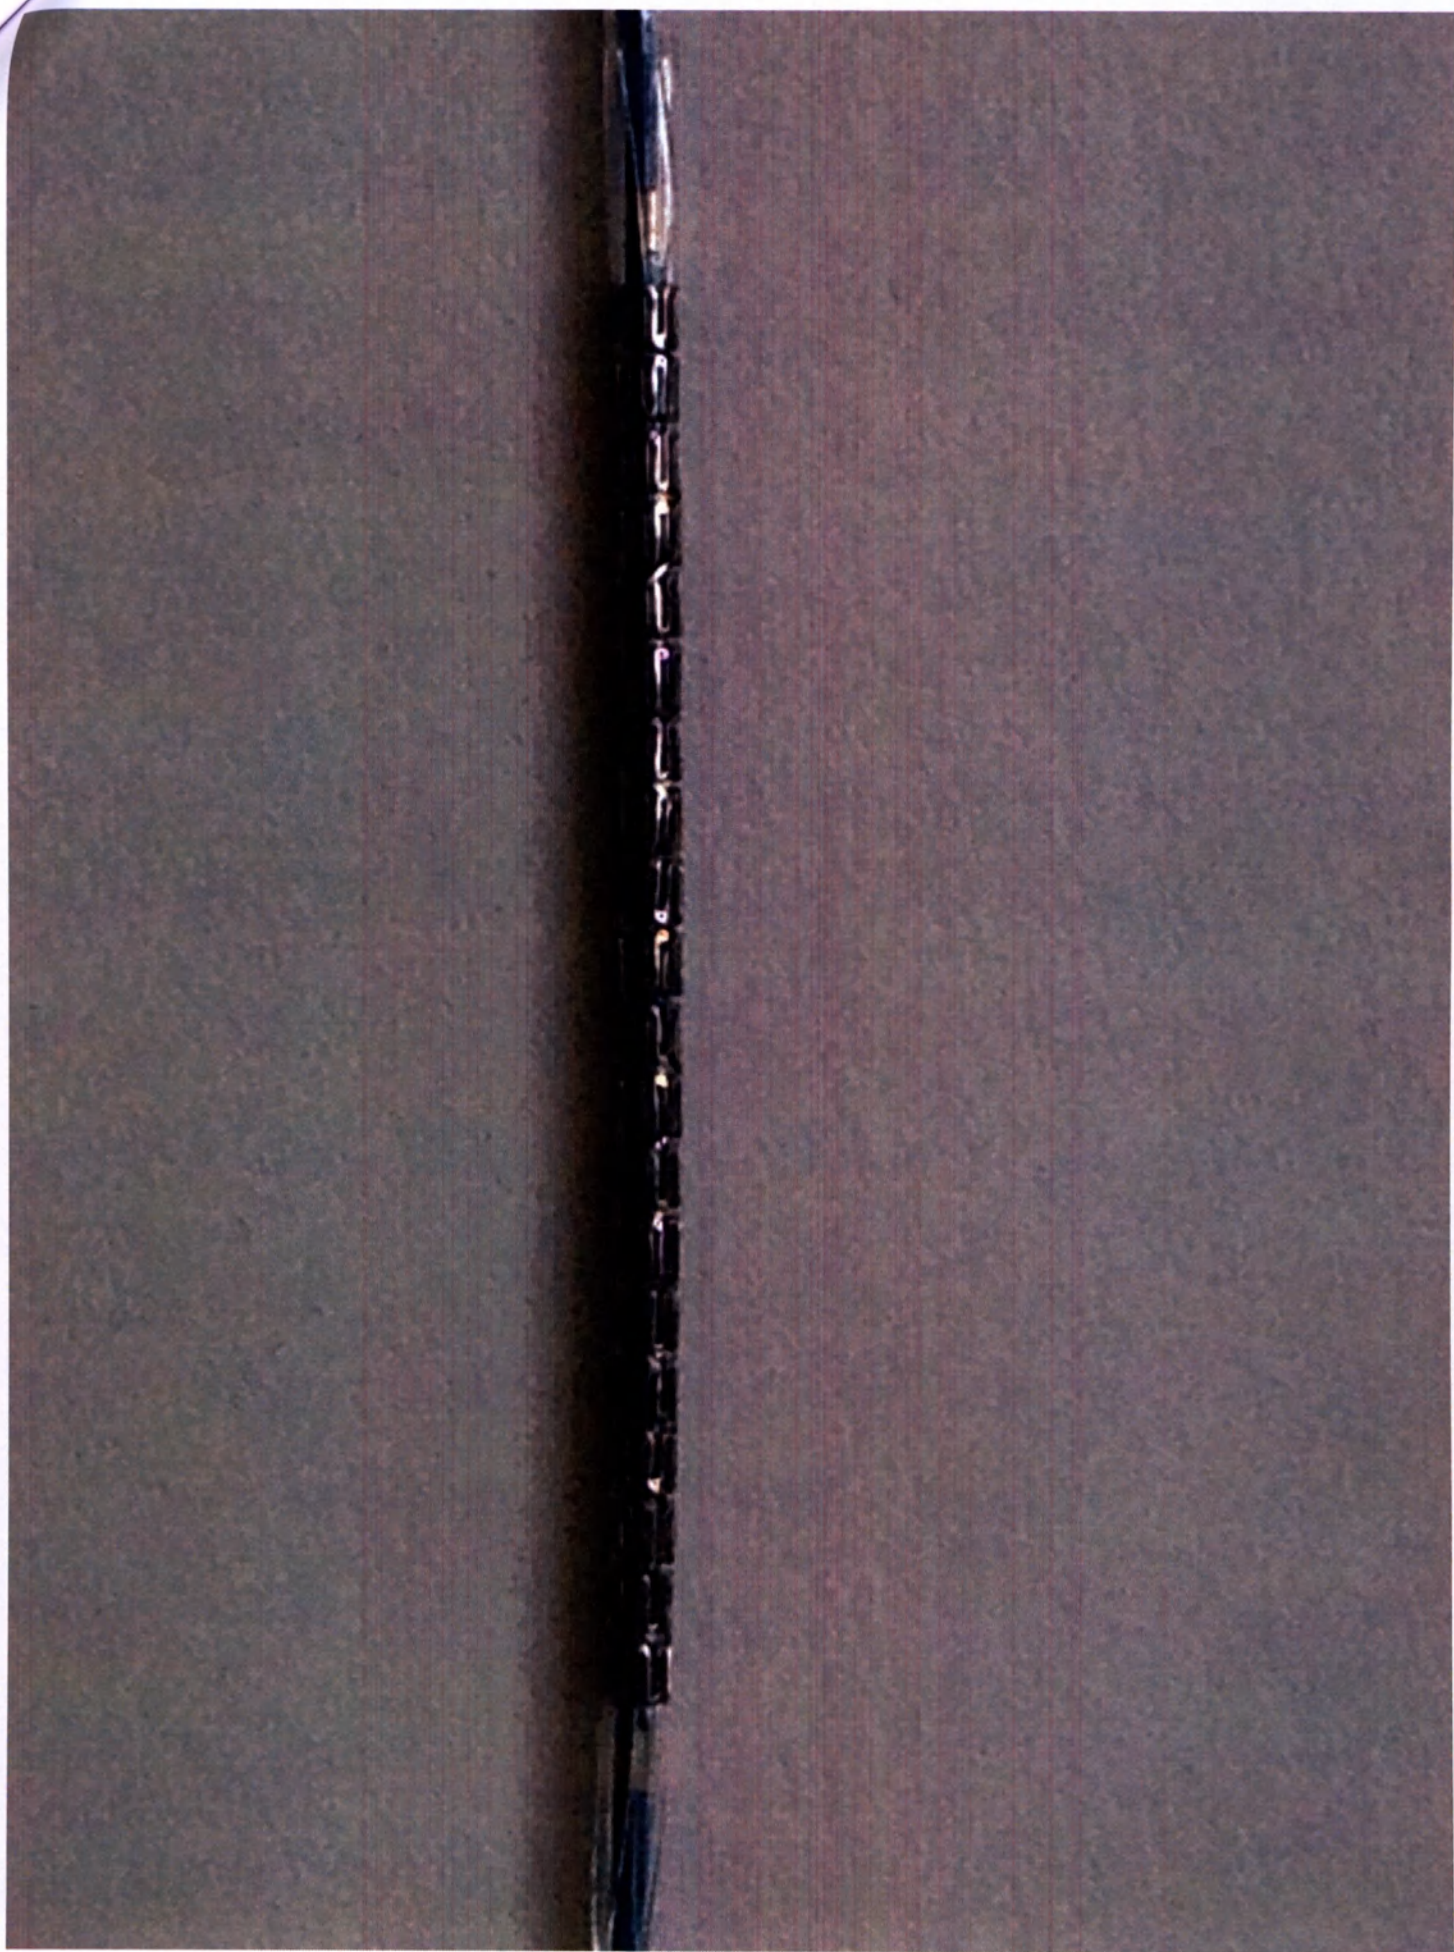

Стент коронарный Promus Premier с лекарственным покрытием предустановленный на системе доставки.

Всего прошнуровано,
пронумеровано и скреплено
печатью 4 листа (ов)



Генеральный директор
ООО «Кардиомедикс»

Меролаев А.А.