




INTRA Endo Kopf L80
(Ref.: 1.004.4456)

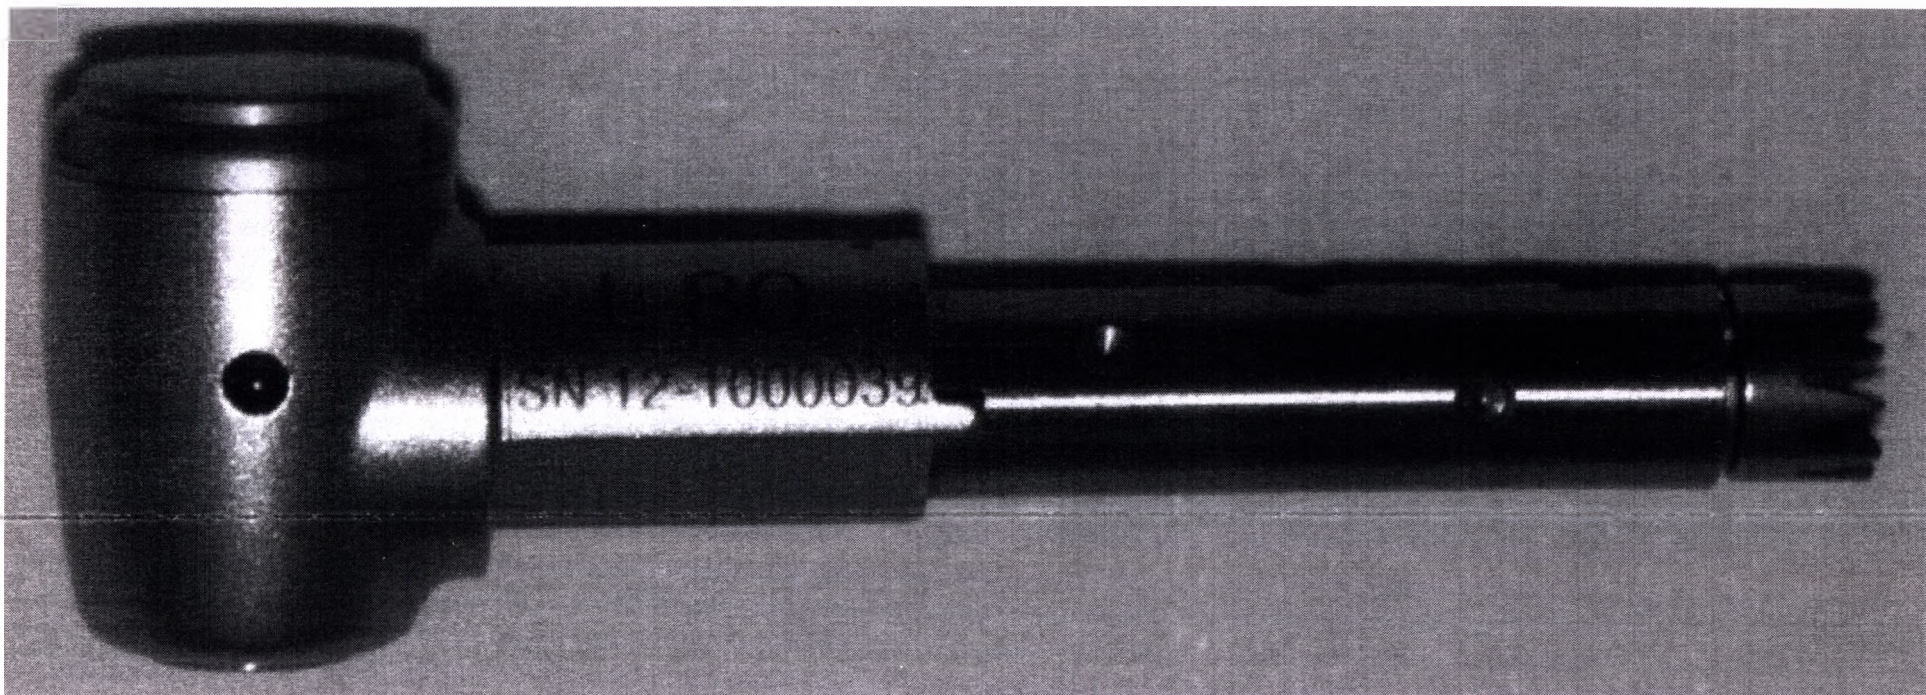



INTRA Endo Kopf L3
(Ref.: 1.008.1822)

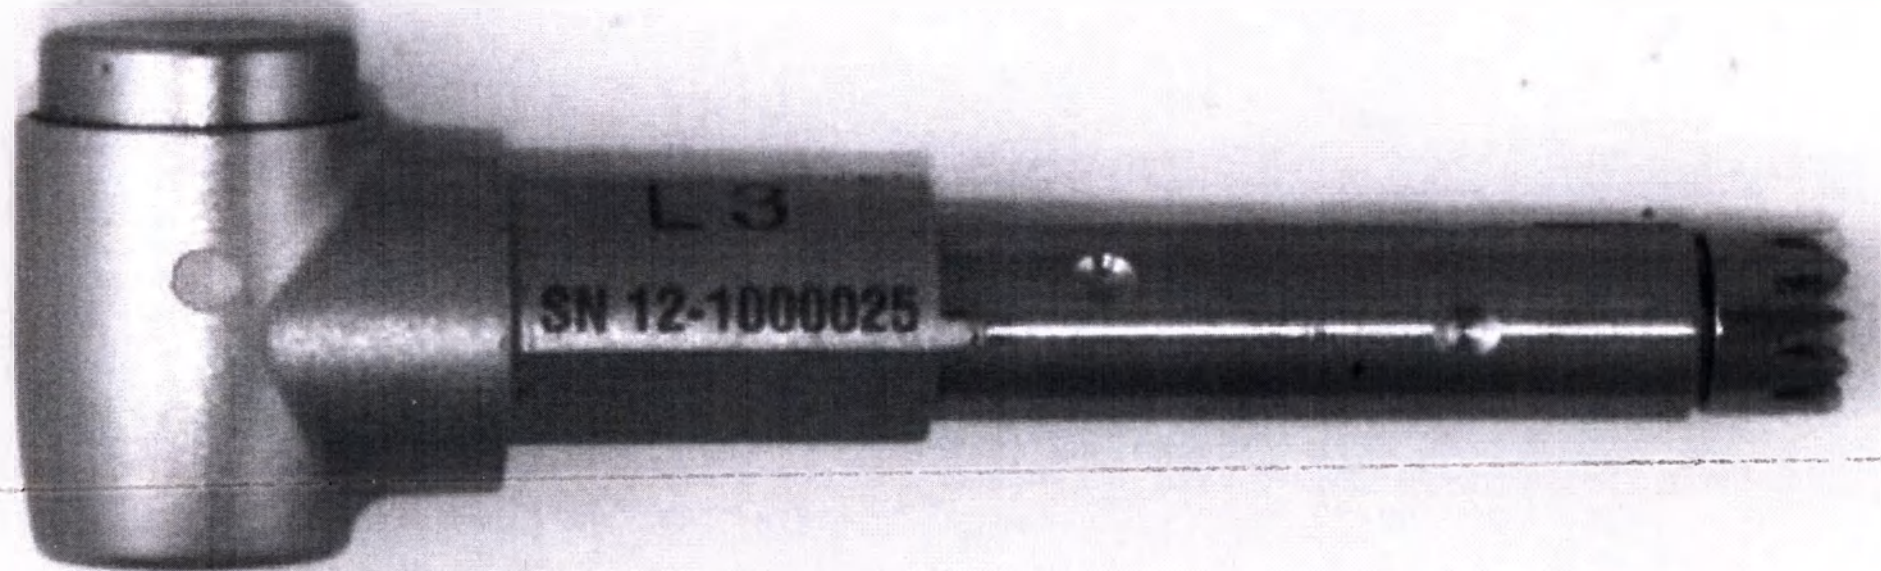


I INTRA Endo Kopf L3 Y
(Ref.: 1.008.1823)

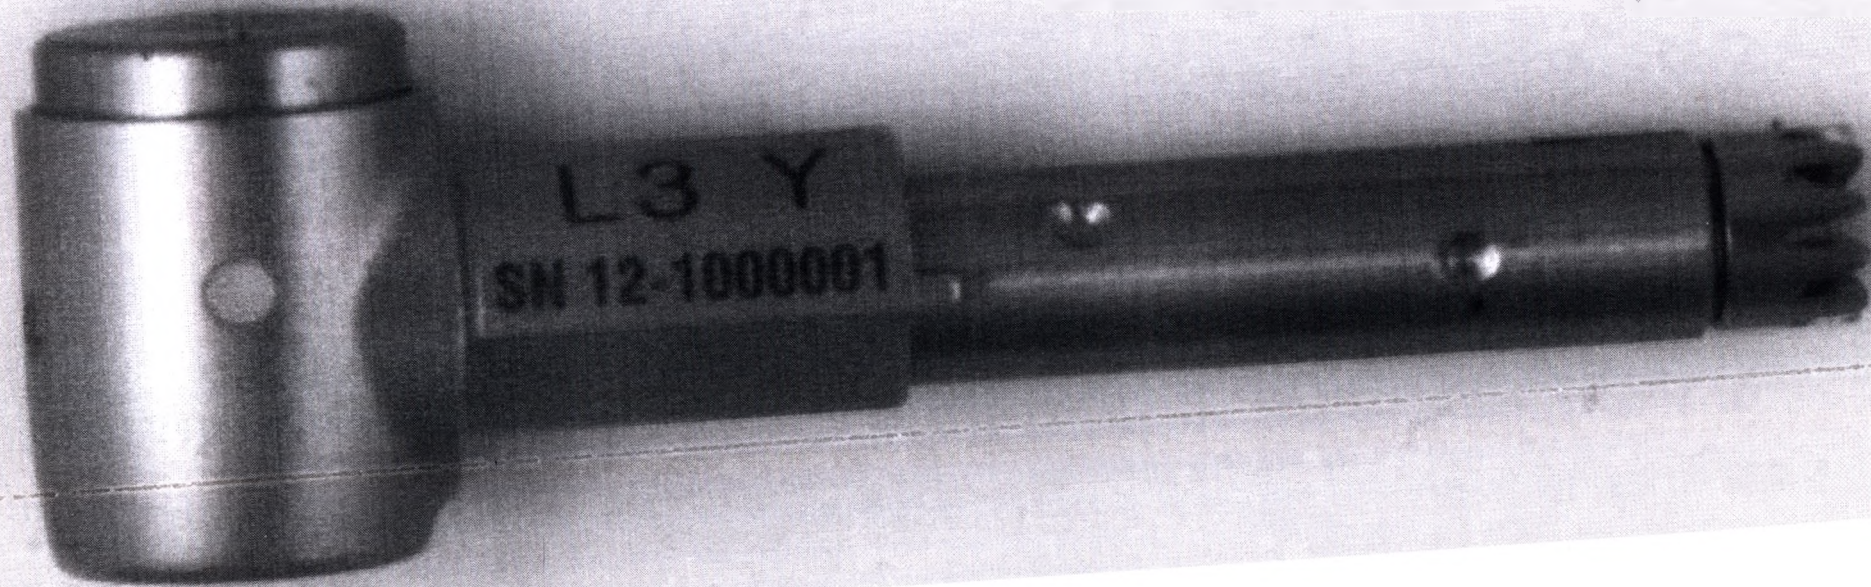


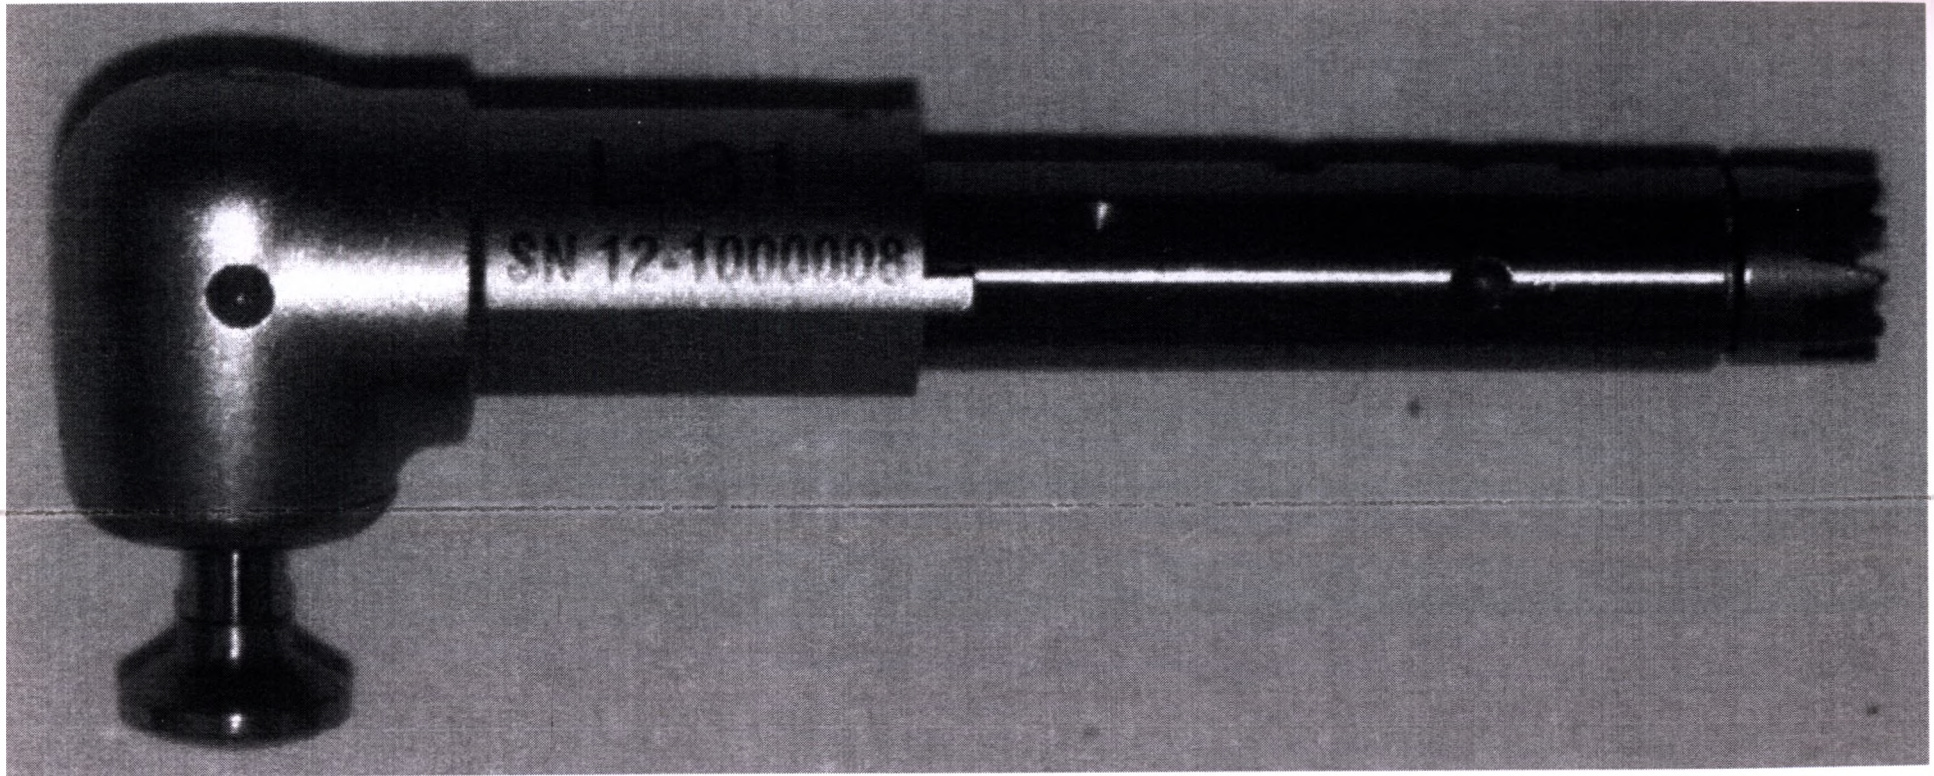

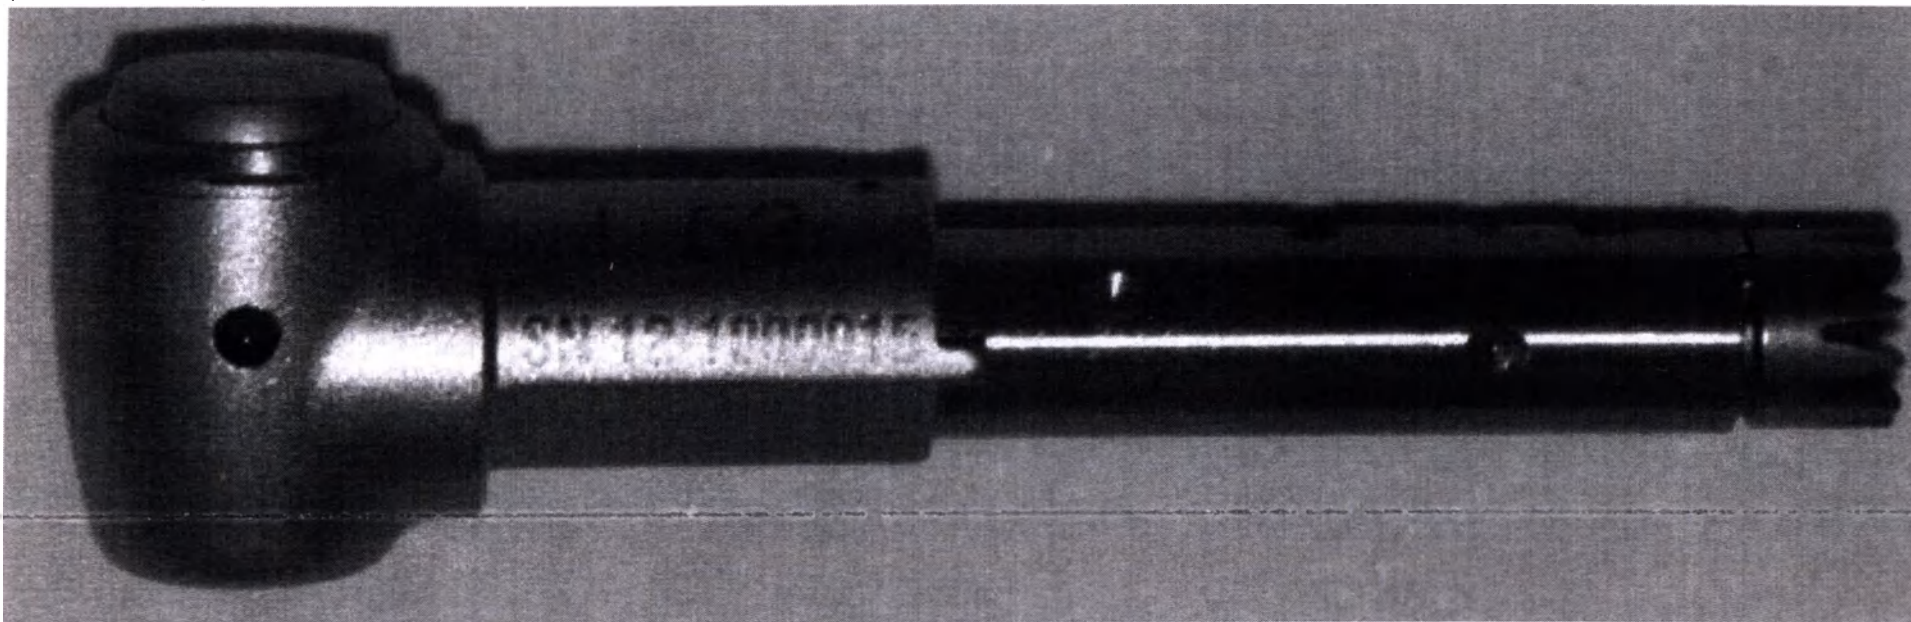



(Кей.: 1.000.1020)

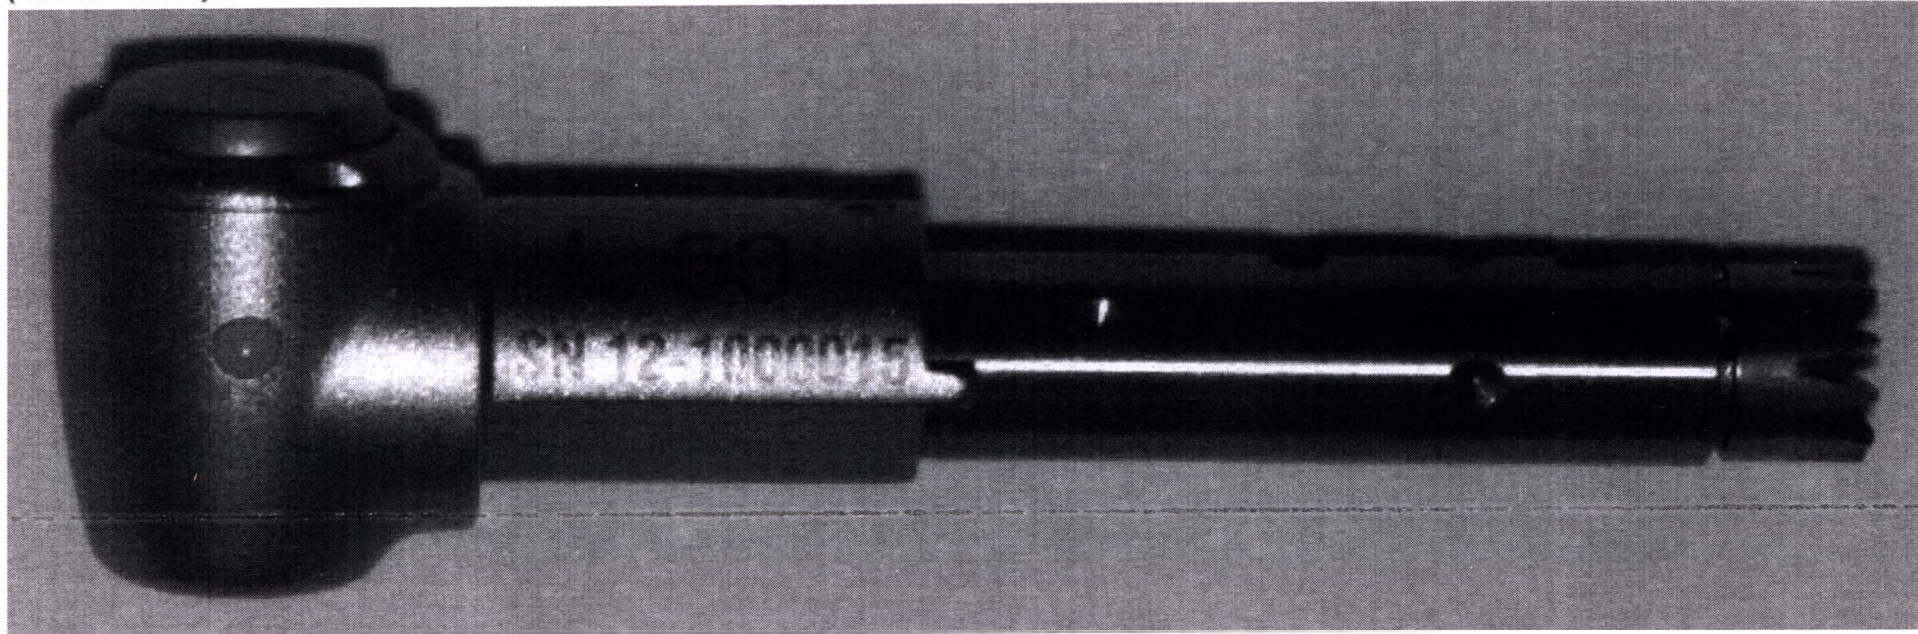


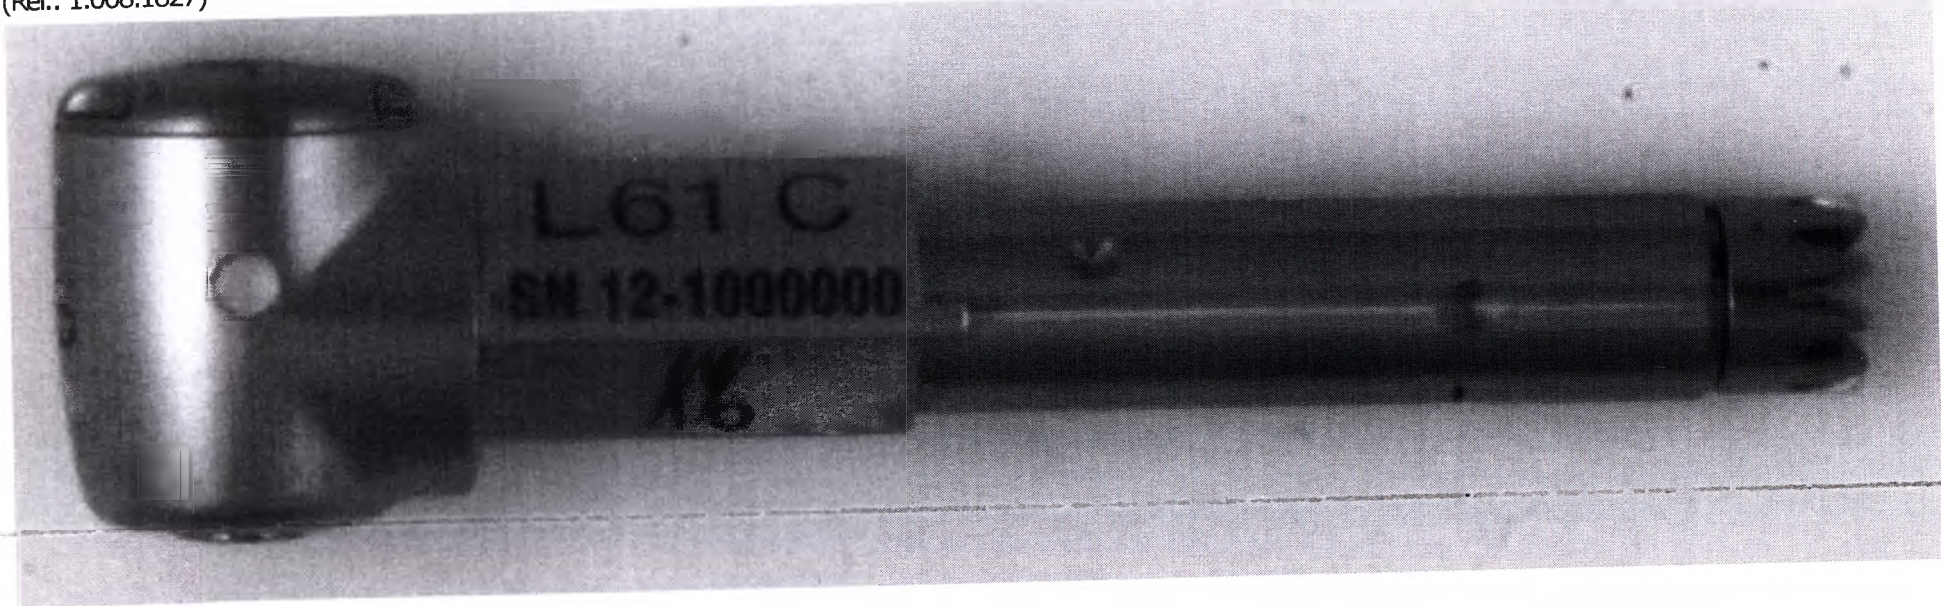


(Ref.: 1.008.1828)

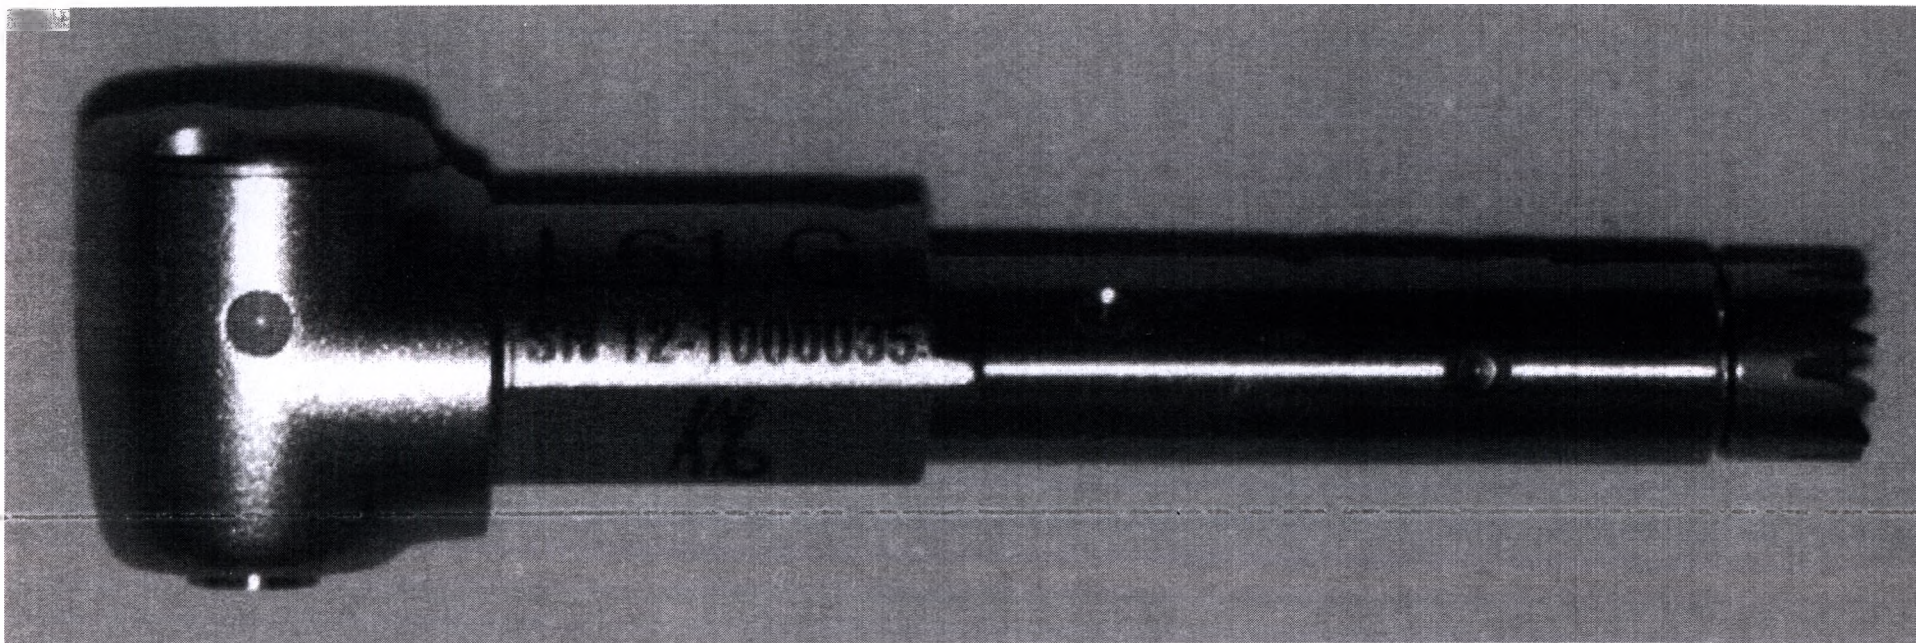


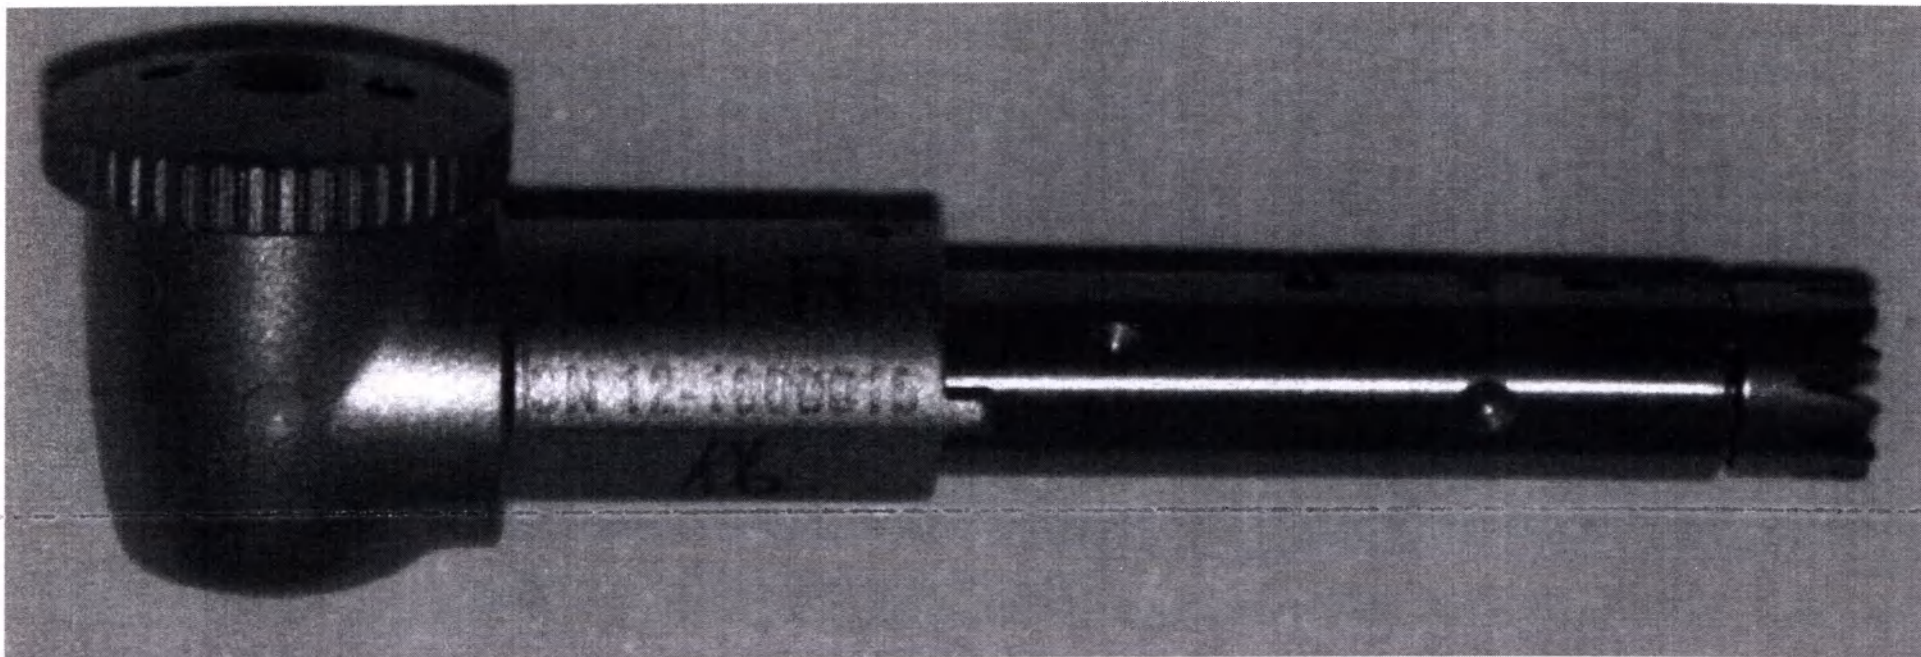

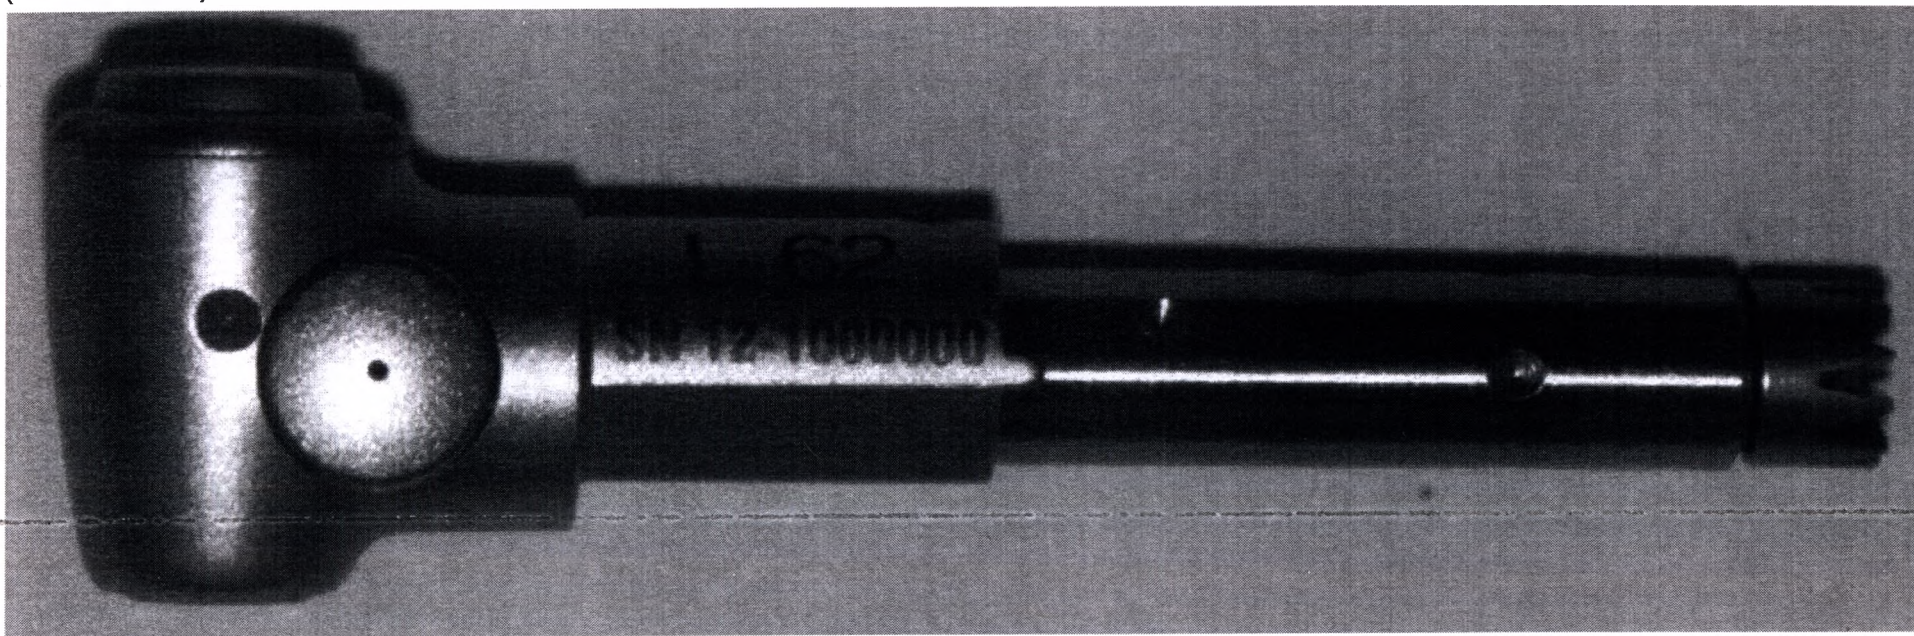


INTRA Kopf L66 B
(Ref.: 1.008.1831)

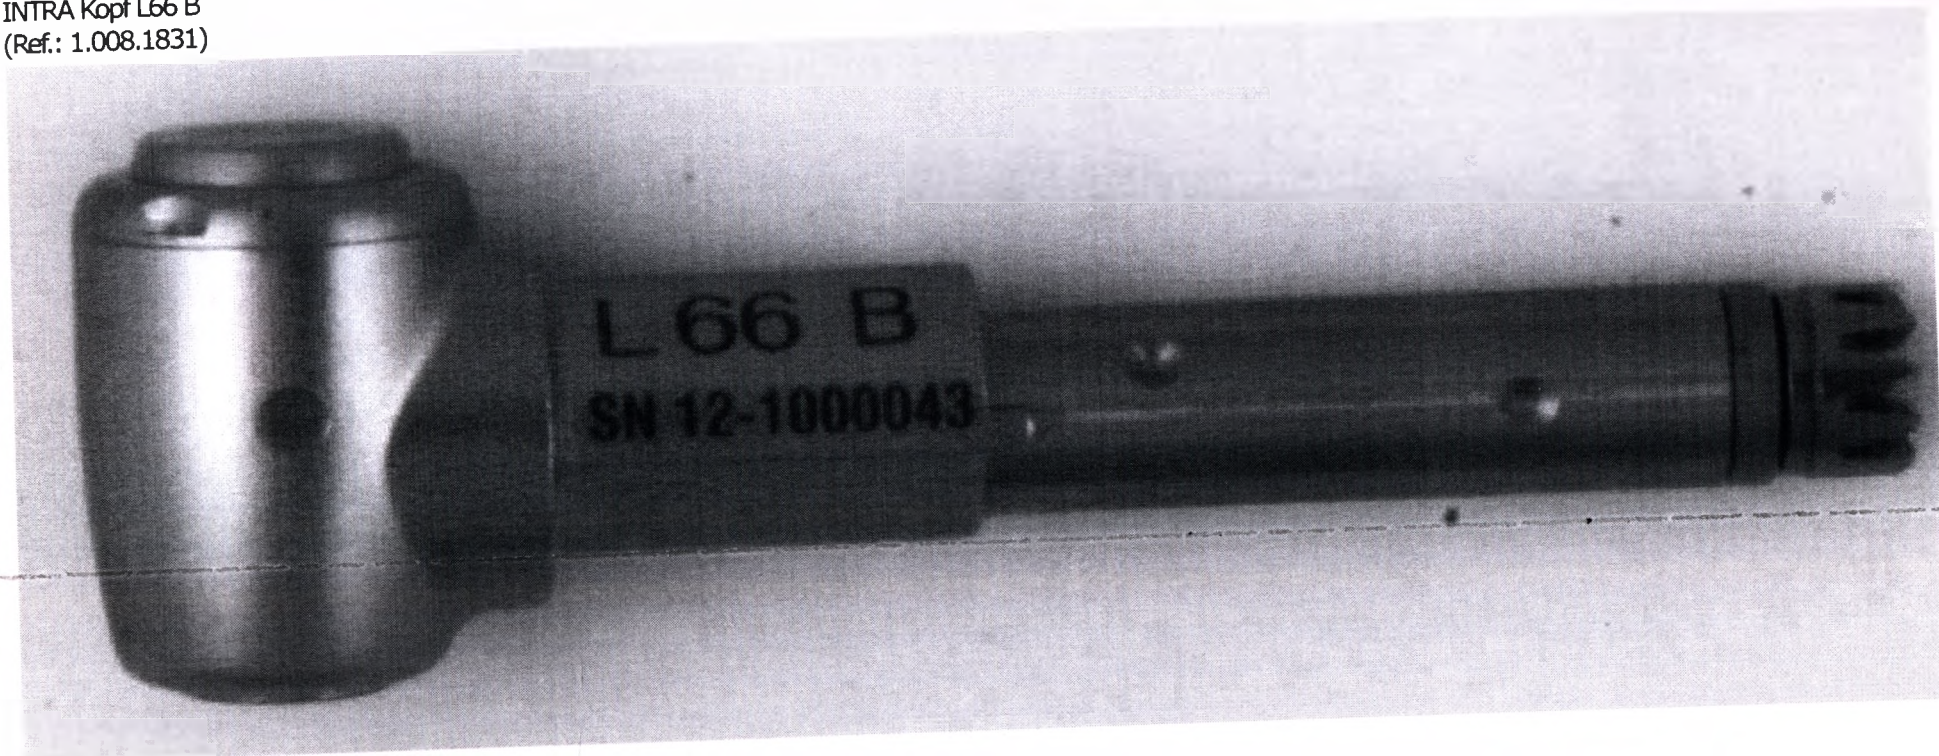

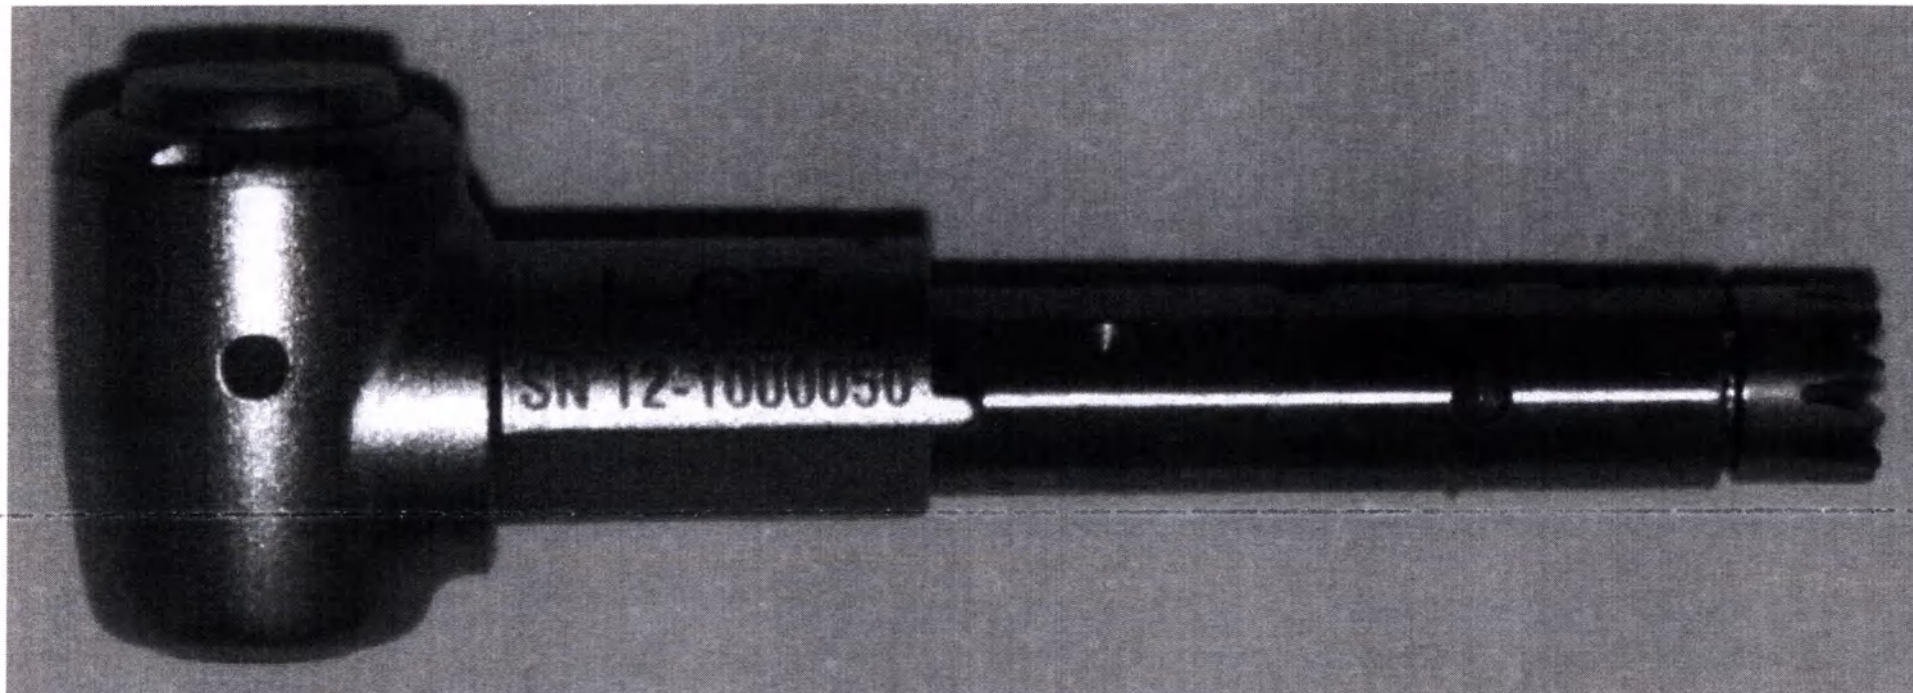



54

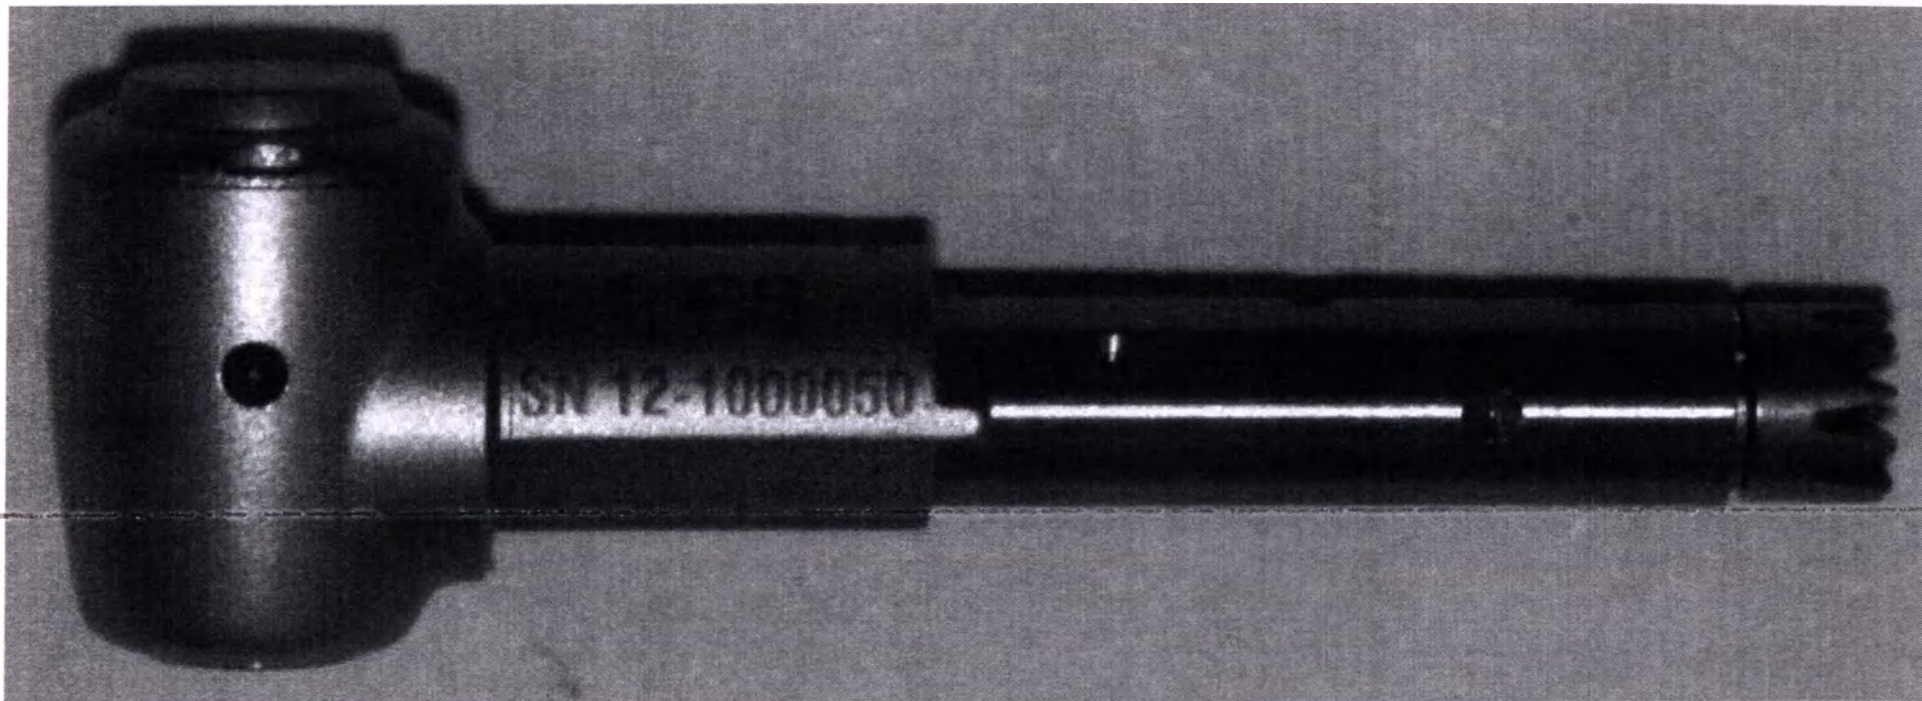


154


INTRA Kopf L68 B
(Ref.: 1.008.1834)

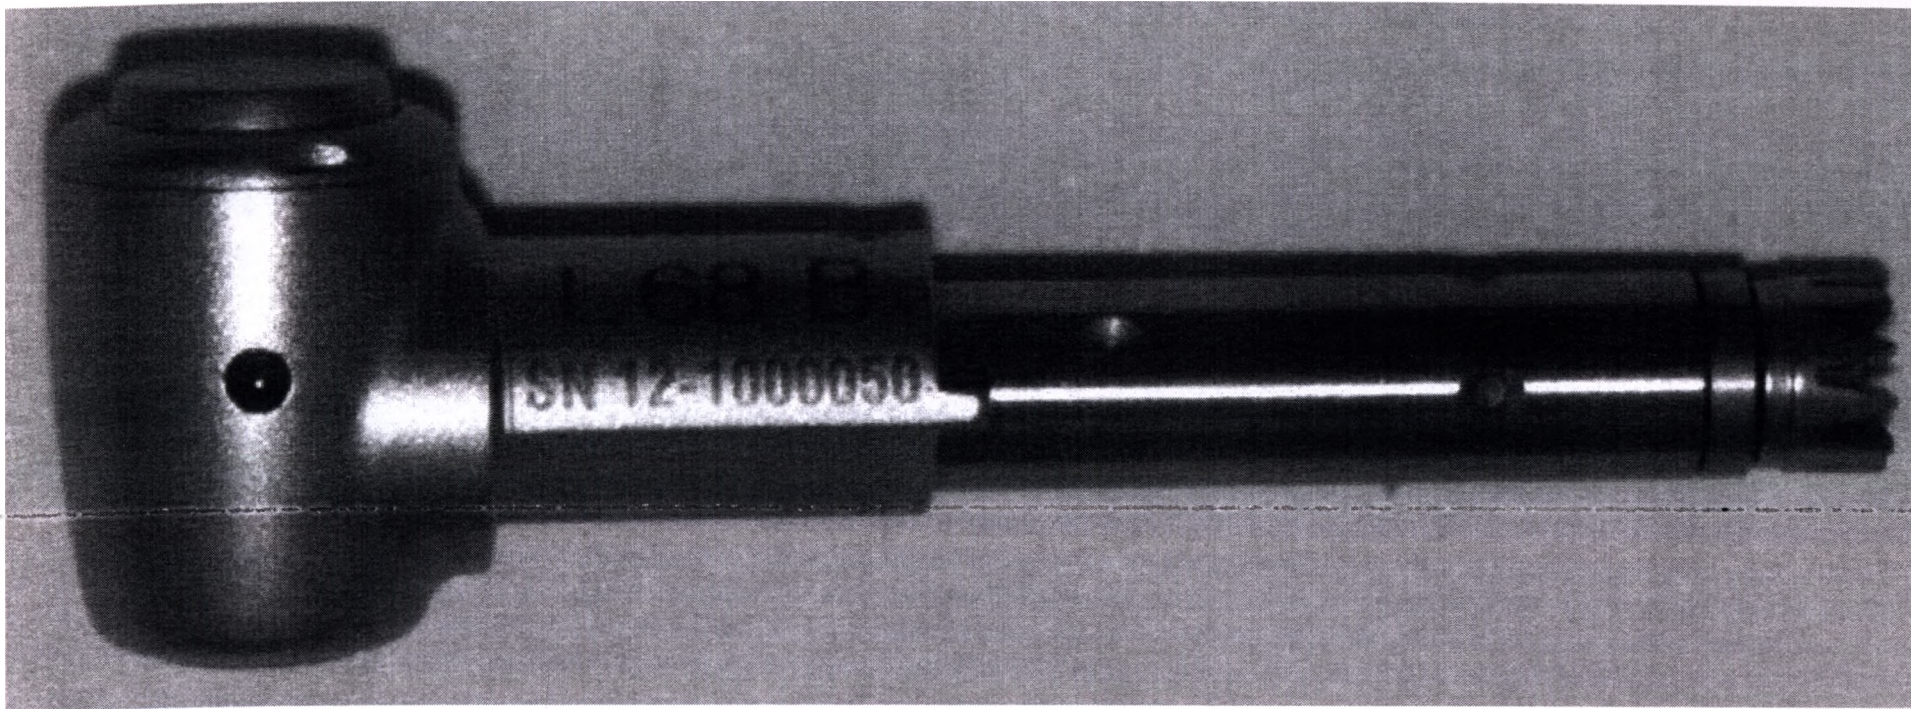


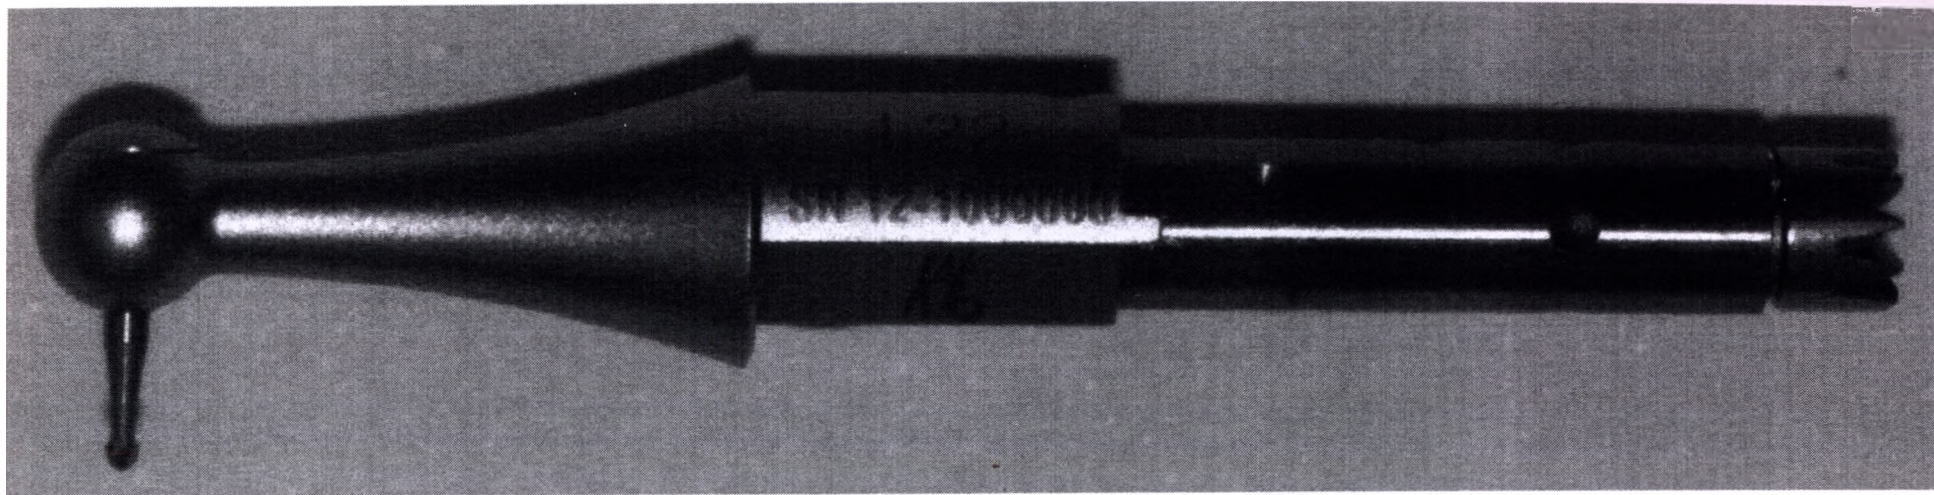

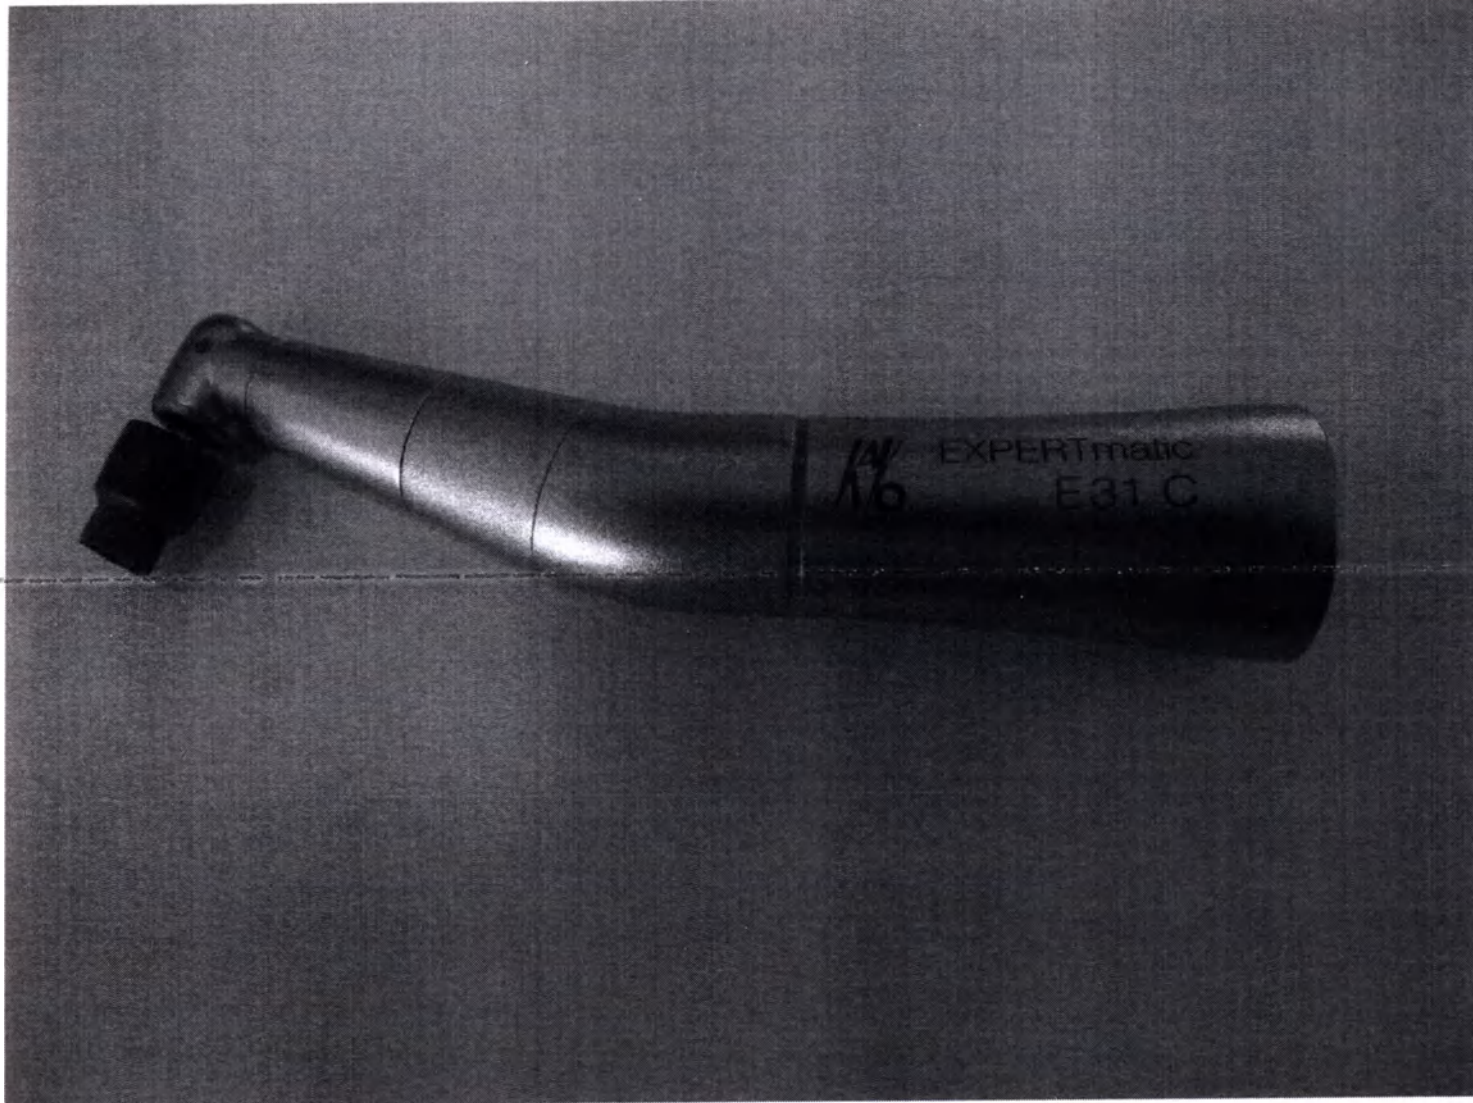

157

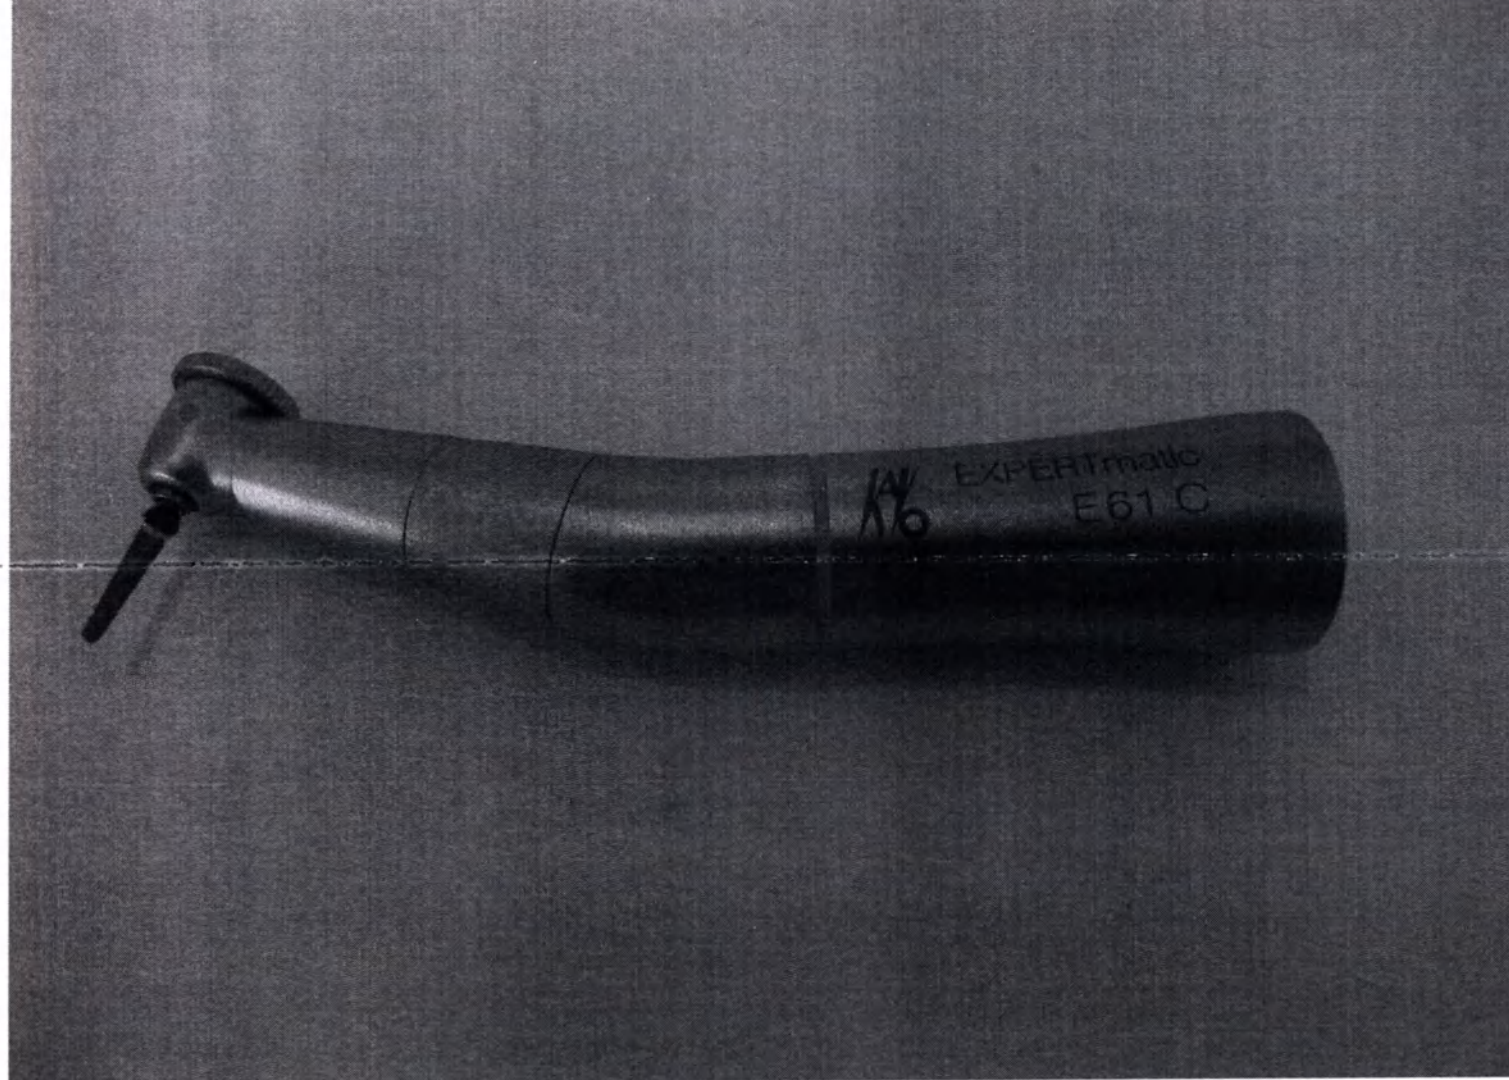

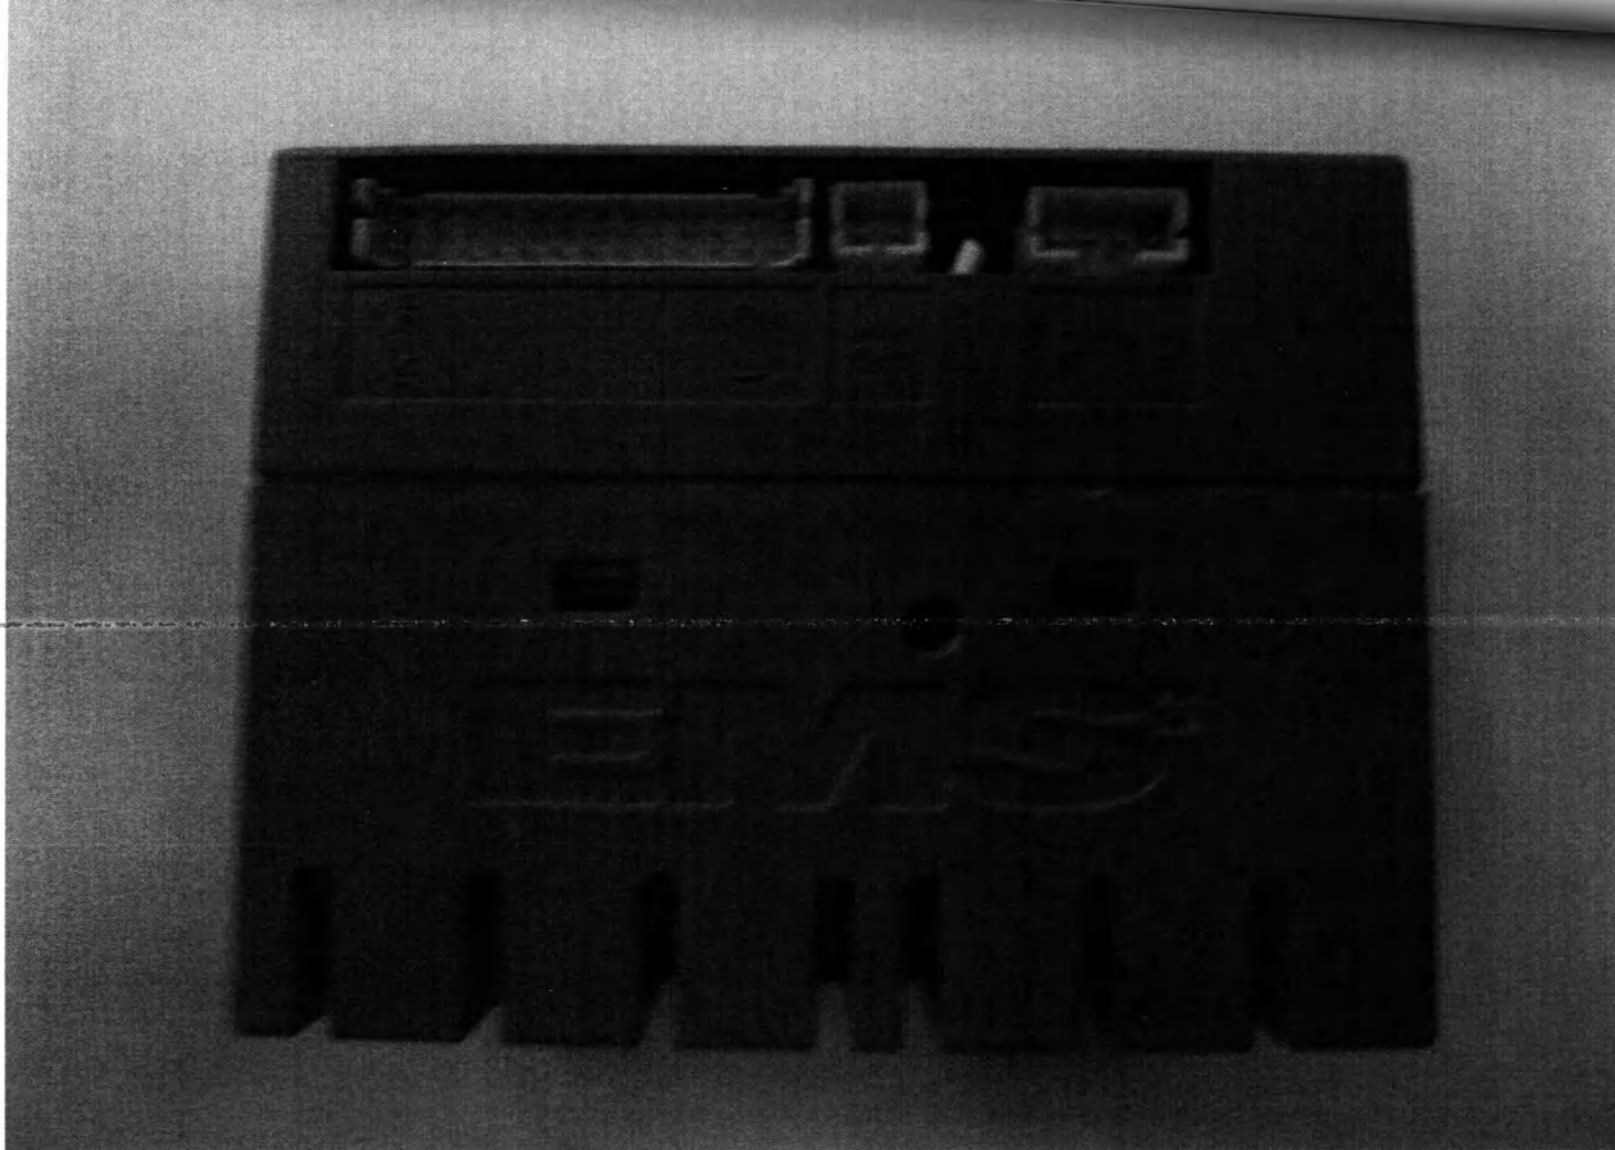

10073966_EMS PiezoLED Modul.JPG



10073995_PiezoLED Handstück.JPG



10074002_Piezo Scaler Schlauch.JPG




10074006_PiezoLED Paro 212.JPG



10074024_PiezoLED Scaler 201.JPG




10074026_PiezoLED Scaler 202.JPG



10074027_PiezoLED Cem 225.JPG




10074033_PiezoLED Paro 213.JPG

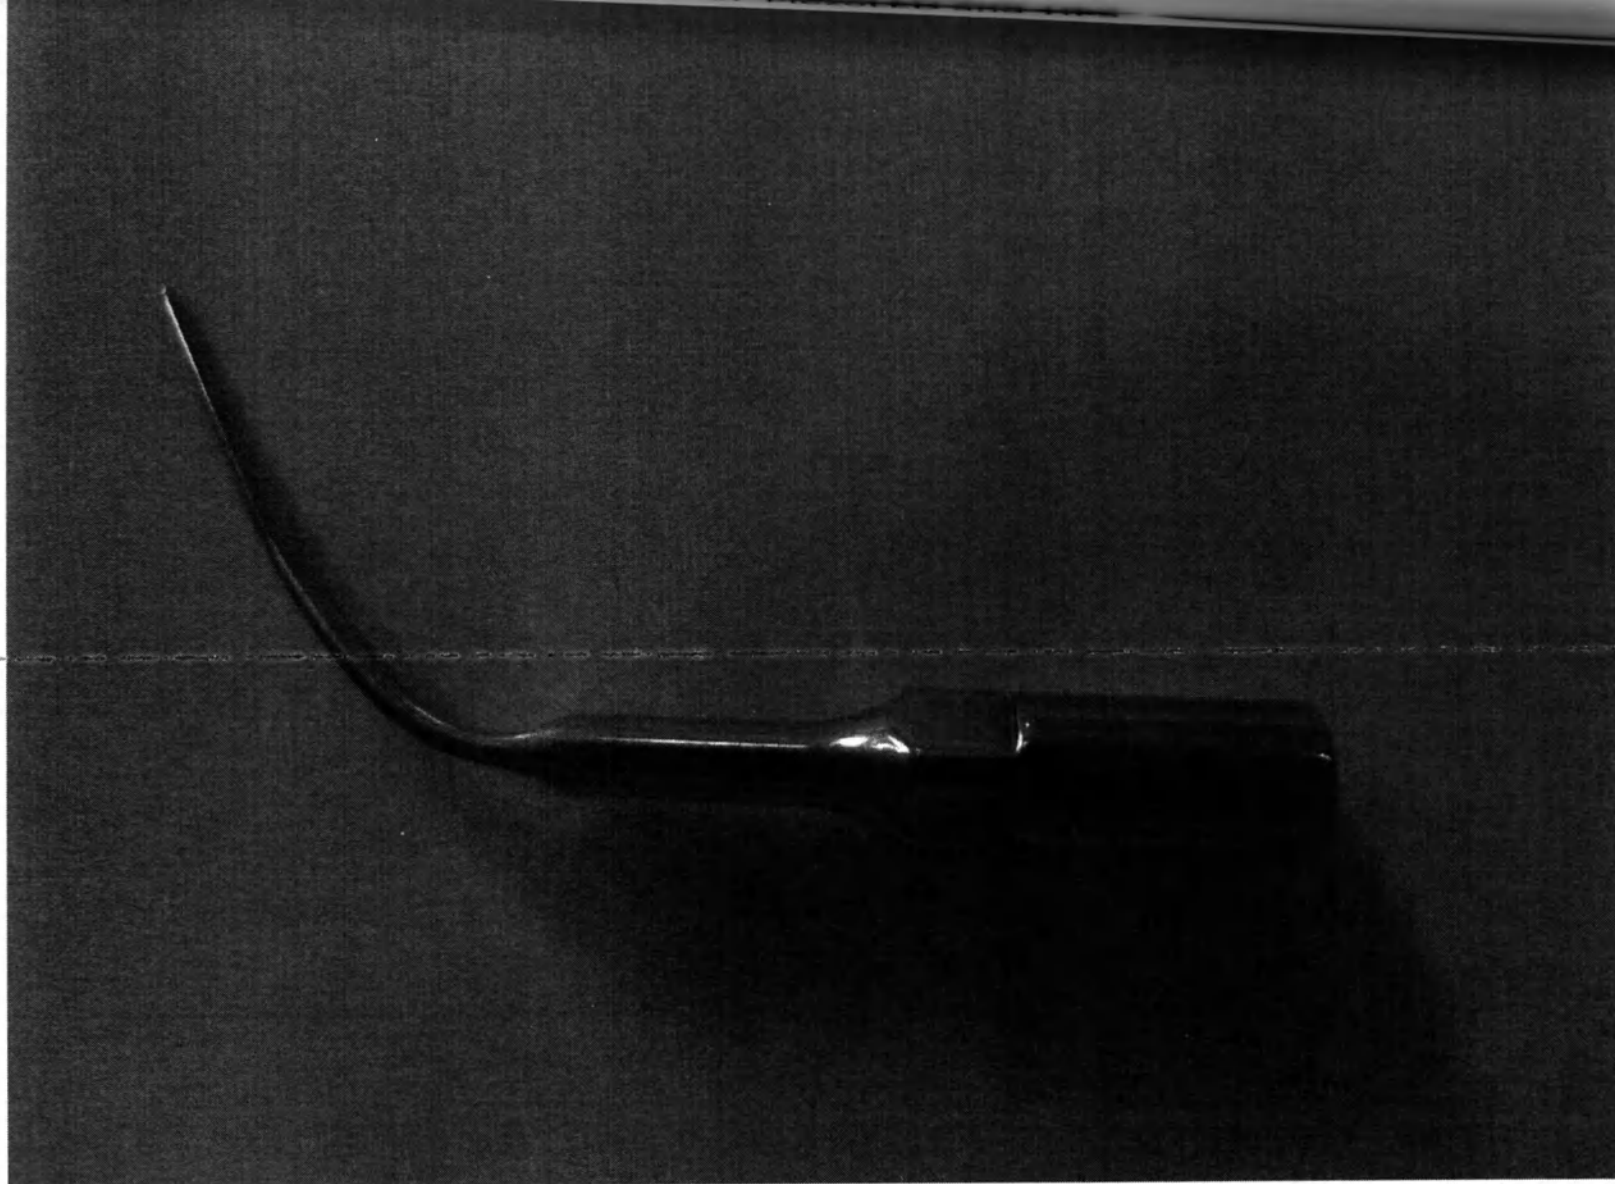

10074034_PiezoLED Paro 214.JPG

105

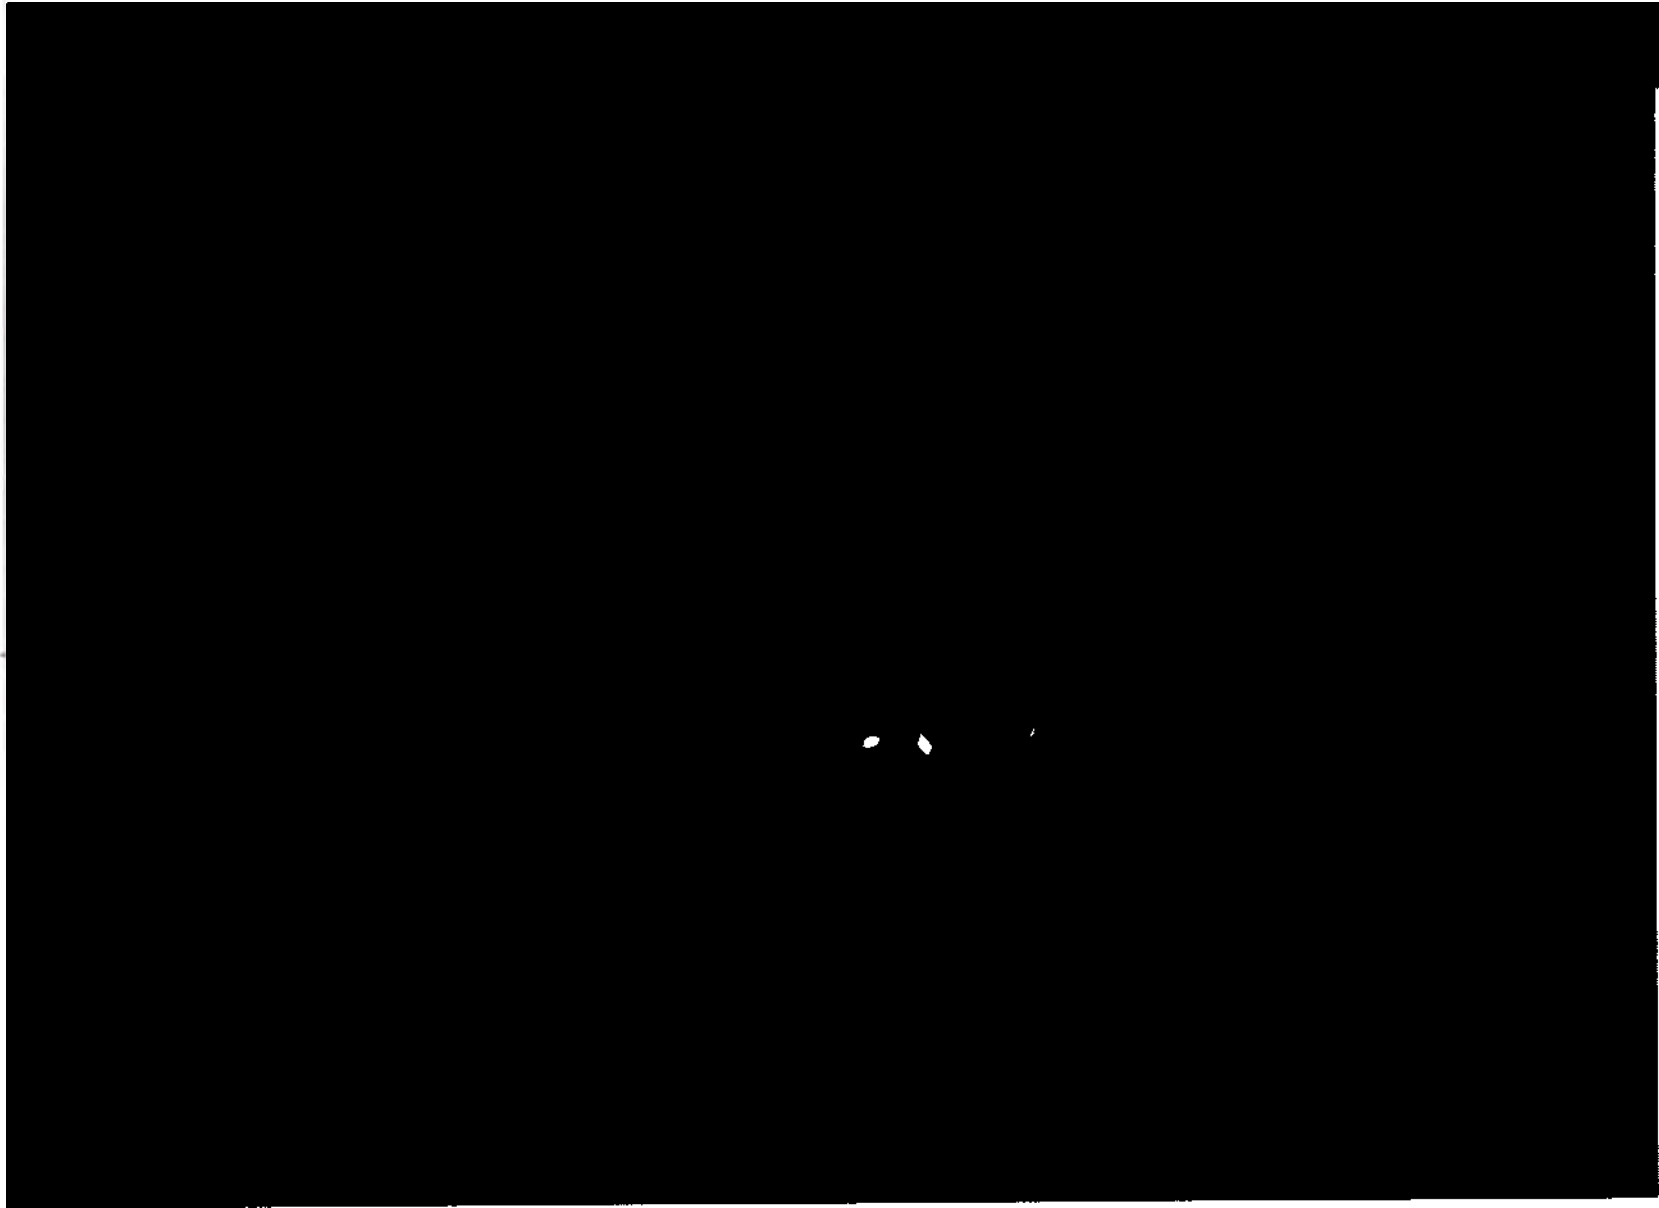

10074035__PiezoLED Prep 226.JPG


201



10074036_PiezoLED Prep 227.JPG




10074037_PiezoLED Prep 228.JPG

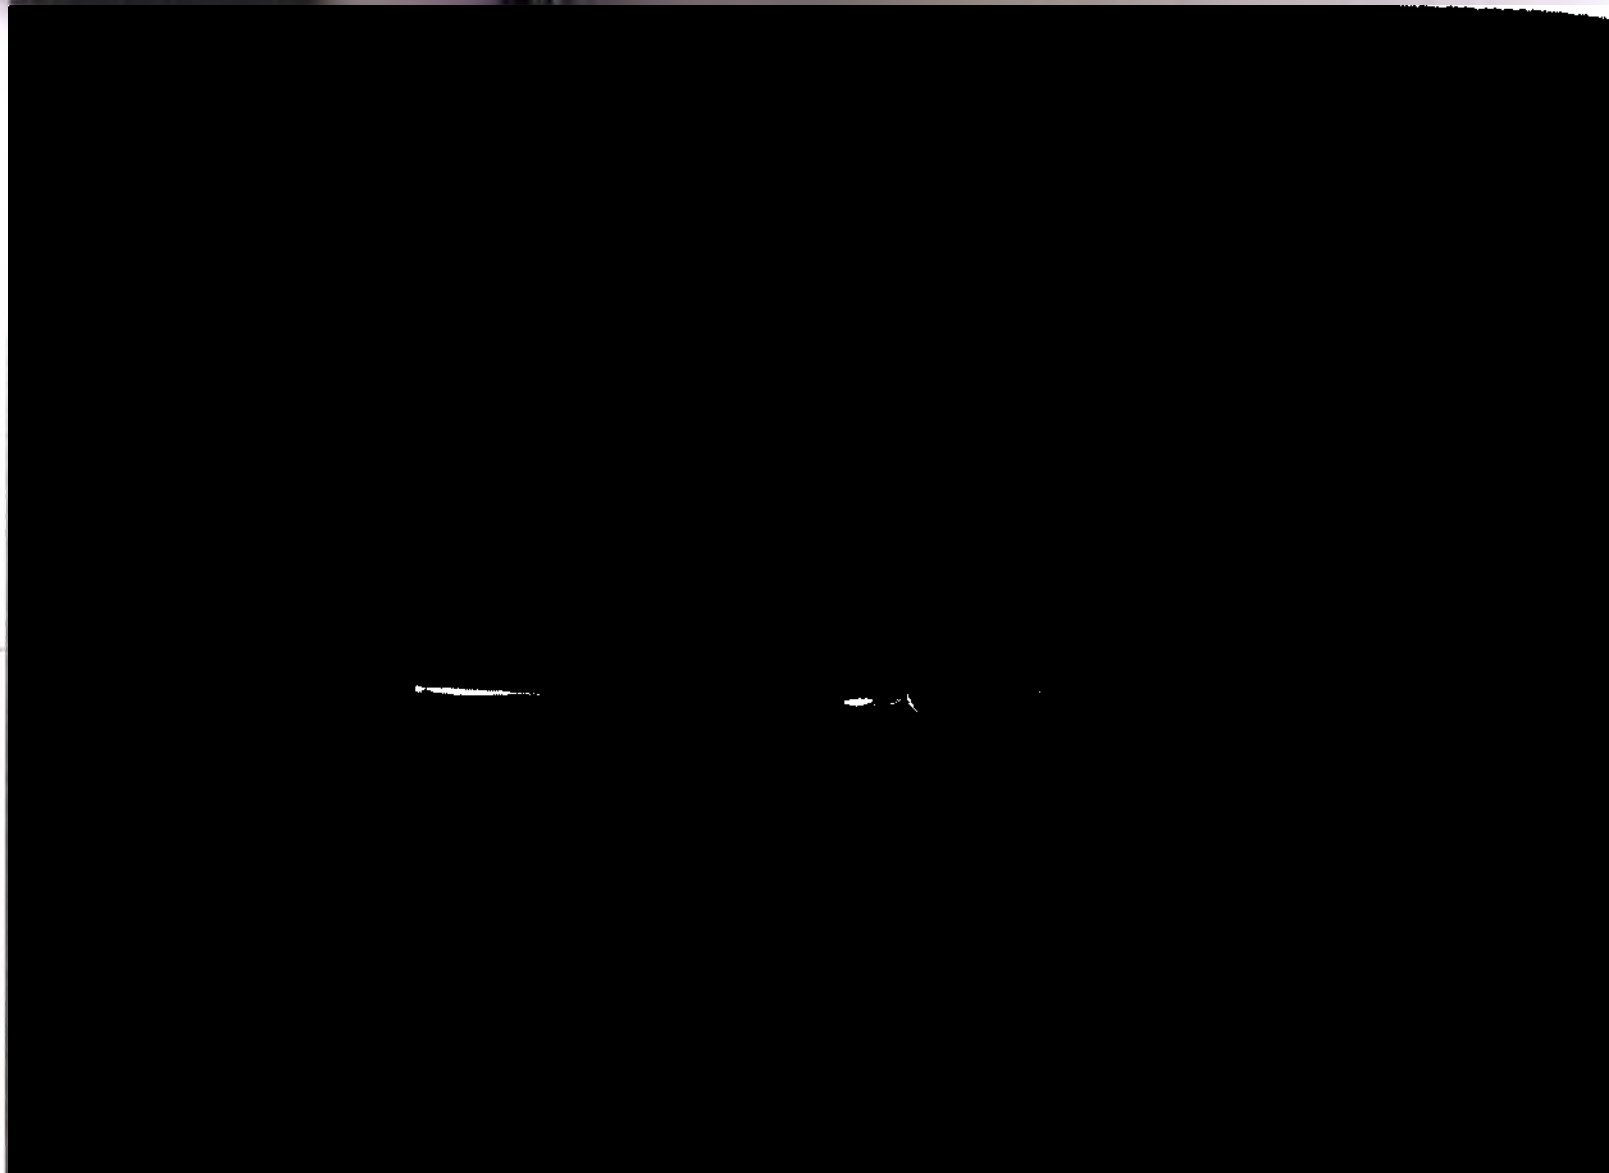

10074038_PiezoLED Prep 229.JPG



10074039_PiezoLED Paro 210.JPG

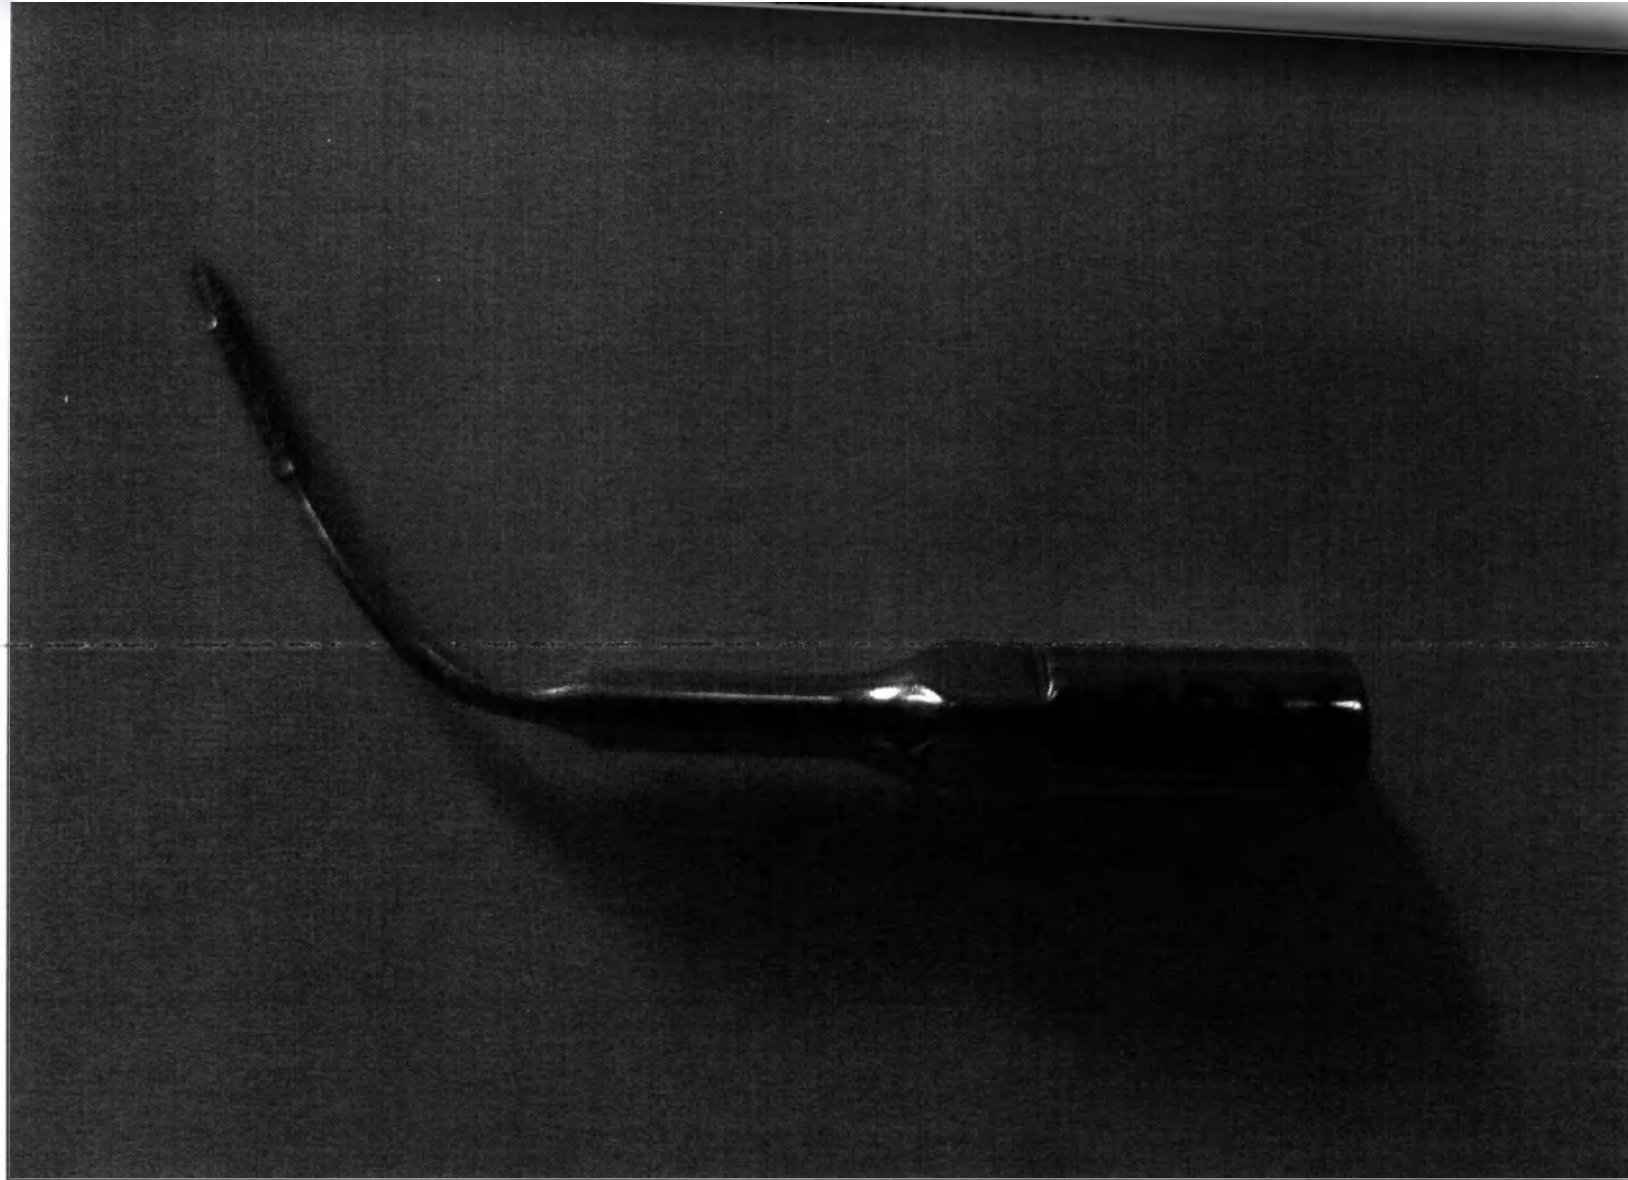


10074041_PiezoLED Endo 221.JPG



10074042_PiezoLED Paro 211.JPG




10074043_PiezoLED Endo 222.JPG

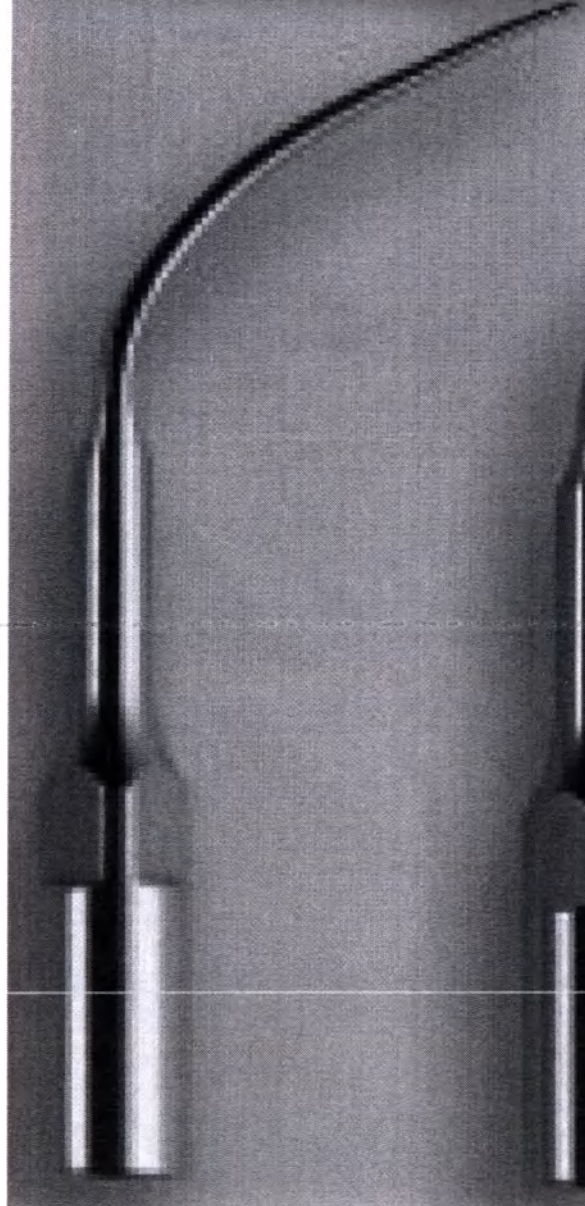

1.007.4028 – PiezoLED Scaler 203

177

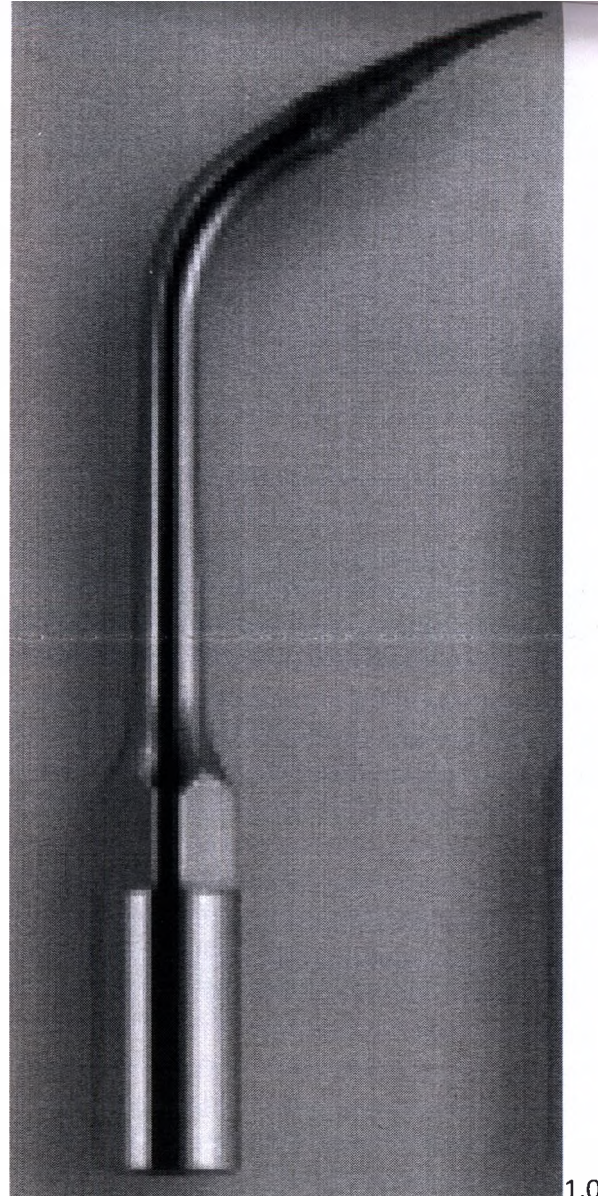

1.007.4040 – PiezoLED ENDO 220

Всего 36 стр.




ГЕНЕРАЛЬНЫЙ ДИРЕКТОР
Шумилов Е.С.