



ООО «МайДент24»
125124, РФ, г. Москва, 5-я ул. Ямского поля,
д.7, корп.2, ЭТ/ПОМ/КОМ 2/1/68
тел./факс: +7 (495) 665-79-32
ИНН 7714780239/ КПП 771401001

Фотографические изображения маркировки медицинского изделия:

Лампа полимеризационная, модели: X-Cure, B-Cure, iLed, LED.H

1. Лампа полимеризационная, модель: X-Cure. Маркировка на упаковке.



Дампа полимеризационная, модель: X-Cure. Маркировка на упаковке.

Warning:

The equipment should be handled with care and kept away from the epicenter.
Keep away from the articles which are combustible, poisonous, caustic or explosive.

All rights of modifying the product are reserved to the manufacturer without further notice. The pictures are only for reference. The final interpretation rights belong to GUILIN WOODPECKER MEDICAL INSTRUMENT CO., LTD. The industrial design, inner structure, etc. have claimed for several patents by WOODPECKER. Any copy or fake products must take legal responsibilities.



Input: ~100V-240V 50/60Hz 800mA

Output: DC15.0V $\approx$ 1.6A



Guilin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, Guilin National High-Tech
Zone, Guilin, Guangxi, 541004 P. R. China

Tel:

Europe Sales Dept.: +86-773-5873196, +86-773-2125222

North America, South America &


Oceania Sales Dept.: +86-773-5873198, +86-773-2125123

Asia & Africa Sales Dept.: +86-773-5855350, +86-773-2125896

Fax: +86-773-5822450

E-mail: woodpecker@glwoodpecker.com, sales@glwoodpecker.com

Website: <http://www.glwoodpecker.com>



MedNet GmbH
Borkstrasse 10 · 48163 Muenster · Germany

Лампа полимеризационная, модель: X-Cure. Основной блок из светодиодов. Маркировка.




Product Name: Curing Light

Model: X-Cure



Guilin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, Guilin National High-Tech
Zone, Guilin, Guangxi, 541004 P. R. China
Website: <http://www.glwoodpecker.com>



MedNet GmbH
Borkstrasse 10 · 48163 Muenster · Germany


Charge for battery: 7.4V (ICR18490)

Rated input: DC 15.0V/1.6A

Adapter Model: UE24WCP1-150160SPA

Use only with adapter provided by manufacturer

2019





II. Лампа полимеризационная, модель B-Cure. Маркировка на упаковке.

Model: B-Cure

SN

UDI

(01) 0 6944843 60270 7 (21) L1980616BC

SN

Ⓟ

L1980616BC

Model: B-Cure
Focused-light
Curing Light


B-Cure

CURING LIGHT

Warning:


The equipment should be handled with care and kept away from the epicenter. Keep away from the articles which are combustible, poisonous, caustic or explosive.

All rights of modifying the product are reserved to the manufacturer without further notice. The pictures are only for reference. The final interpretation rights belong to GUILIN WOODPECKER MEDICAL INSTRUMENT CO., LTD. The industrial design, inner structure, etc, have claimed for several patents by WOODPECKER, any copy or fake products must take legal responsibilities.



Basic Data

Battery	3.7V
Power Input	AC100V~240V
Dimensions	215X155X100mm

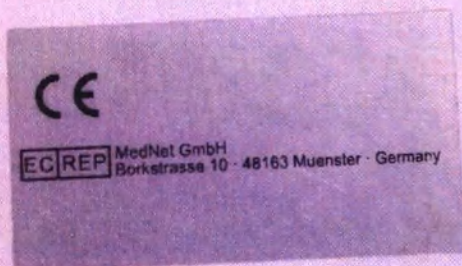

 Guilin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, Guilin National
High-Tech Zone, Guilin, Guangxi, 541004 P. R. China

Tel:

Europe Sales Dept.: +86-773-5873196, +86-773-2125222

North America, South America &

Oceania Sales Dep.: +86-773-5873198, +86-773-2125123

Asia & Africa Sales Dep.: +86-773-5855350, +86-773-2125896

Fax: +86-773-5822450

E-mail: woodpecker@glwoodpecker.com, sales@glwoodpecker.com

Website: <http://www.glwoodpecker.com>

ZMN/WI-10-742 V1.2


Scan and Login website
for more information



Лампа полимеризационная, модель B-Cure. Основной блок из светодиодов. Маркировка.



Лампа полимеризационная, модель B-Cure. Аккумуляторная батарея

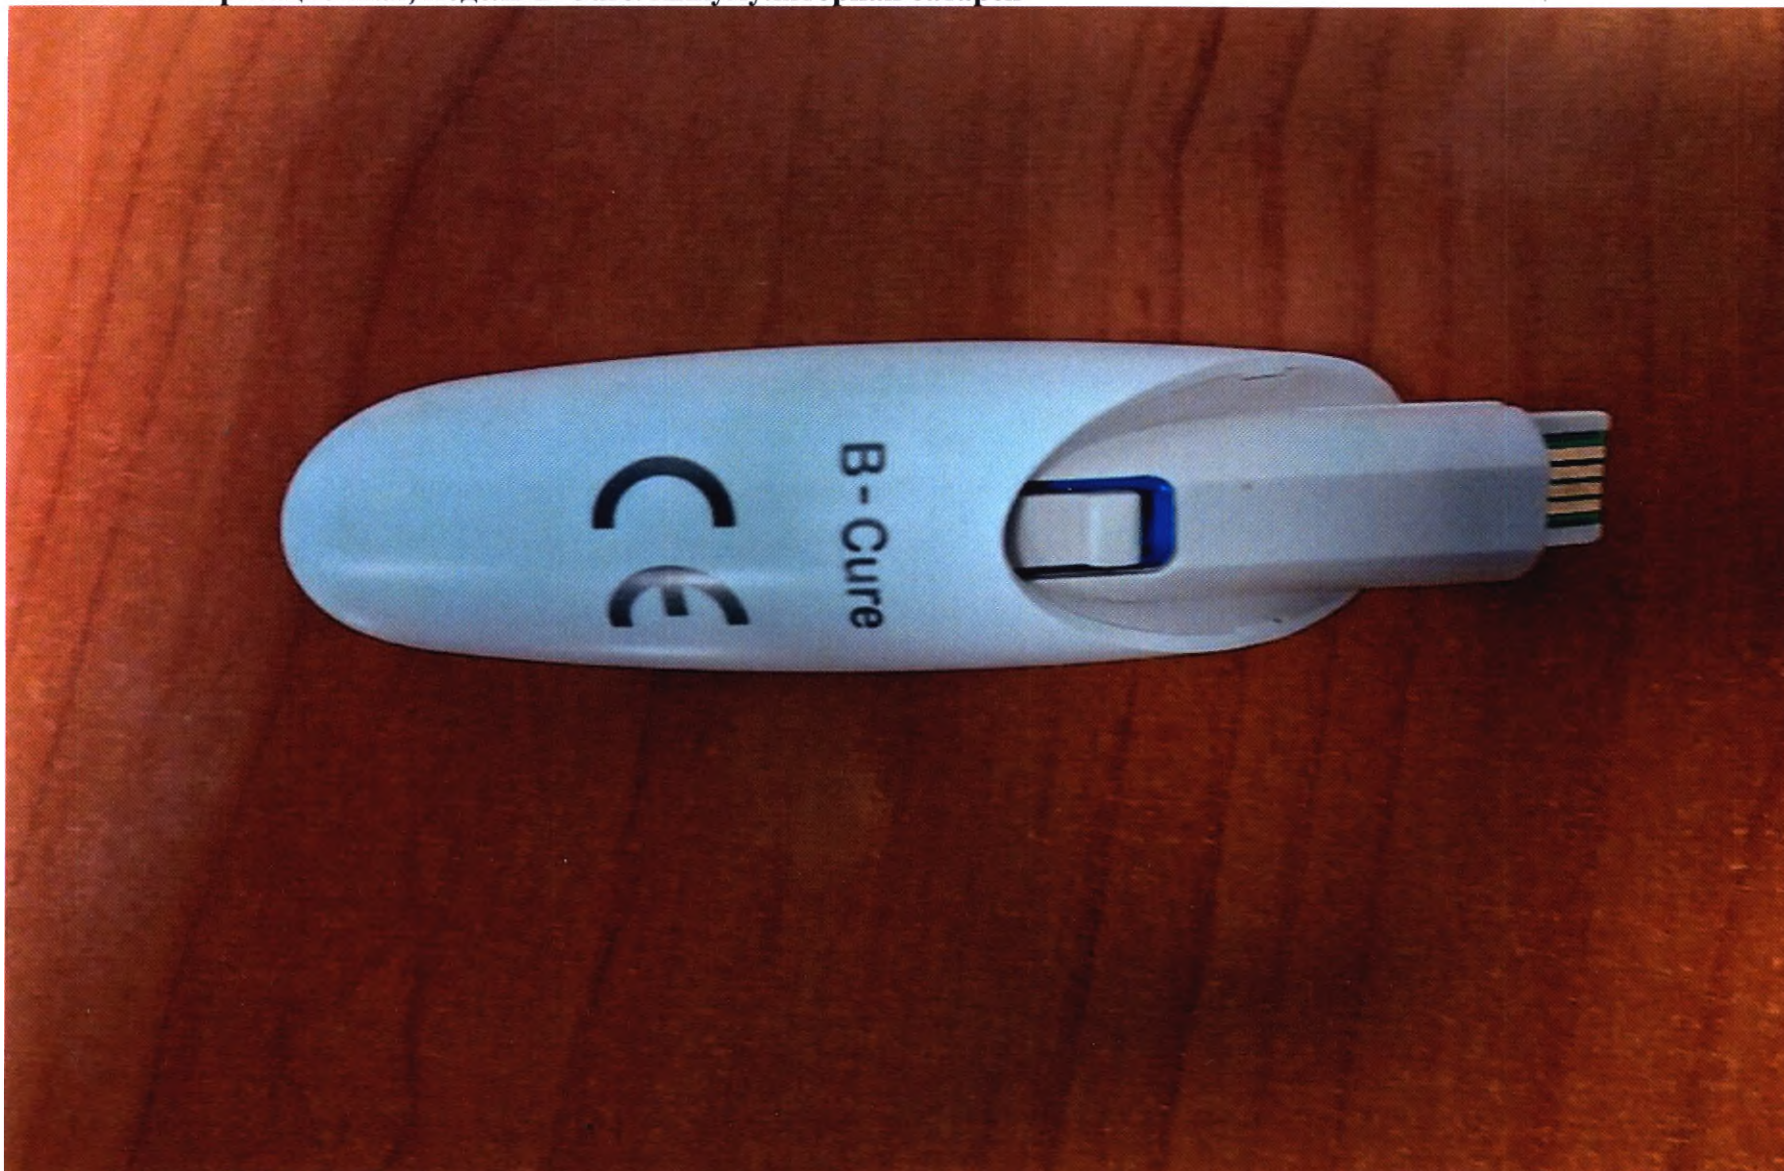

Лампа полимеризационная, модель B-Cure. Зарядное устройство. Маркировка.

Product Name: Curing Light **Model:** B-Cure
Guilin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, Gullin National High-Tech
Zone, Guilin, Guangxi, 541004 P. R. China
Website: <http://www.glwoodpecker.com>



EC REP MedNet GmbH
Borkstrasse 10 · 48163 Muenster · Germany

Charge for battery: 3.7V (DLG14500)

Rated input: DC 5.0V  1A

Adapter Model: DJ-0500100-A5

Duty Cycle: ≤400S on and ≥30s off

Use only with adapter provided by manufacturer

2019



Лампа полимеризационная, модель B-Cure. Адаптер. Маркировка.



III. Лампа полимеризационная, модель i Led. Маркировка на упаковке.

Model: i Led

UDI



(01) 0 6944843 60242 4 (21) L1991563i

SN



(a)

L1991563i

Model: i Led
Wide Spectrum
LED Curing Light



Лампа полимеризационная, модель i Led. Маркировка на упаковке.

Warning:

The equipment should be handled with care and kept away from the operator. Keep away from the articles which are combustible, poisonous, caustic or explosive.

All rights of modifying the product are reserved to the manufacturer without further notice. The pictures are only for reference. The final interpretation rights belong to GUILIN WOODPECKER MEDICAL INSTRUMENT CO., LTD. The industrial design, inner structure, etc., have claimed for several patents by WOODPECKER. Any copy or false products must take legal responsibility.



BASIC DATA:

Battery	3.7V
Power input	AC 100V-240V



Gulin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, Guilin National High-Tech
Zone, Guilin, Guangxi, 541004 P. R. China


Tel:

Europe Sales Dept.: +86-773-5873196, +86-773-2125222
North America, South America &
Oceania Sales Dept.: +86-773-5873198, +86-773-2125123
Asia & Africa Sales Dept.: +86-773-5855350, +86-773-2125896

Fax: +86-773-5822450

E-mail: woodpecker@glwoodpecker.com, sales@glwoodpecker.com

Website: <http://www.glwoodpecker.com>



MedNet GmbH


Borkstrasse 10 · 48163 Muenster · Germany

ZMN/WI-10-585 V1.1

Лампа полимеризационная, модель i Led. Основной блок из светодиодов. Маркировка.



Лампа полимеризационная, модель i Led. Основной блок из светодиодов. Маркировка.

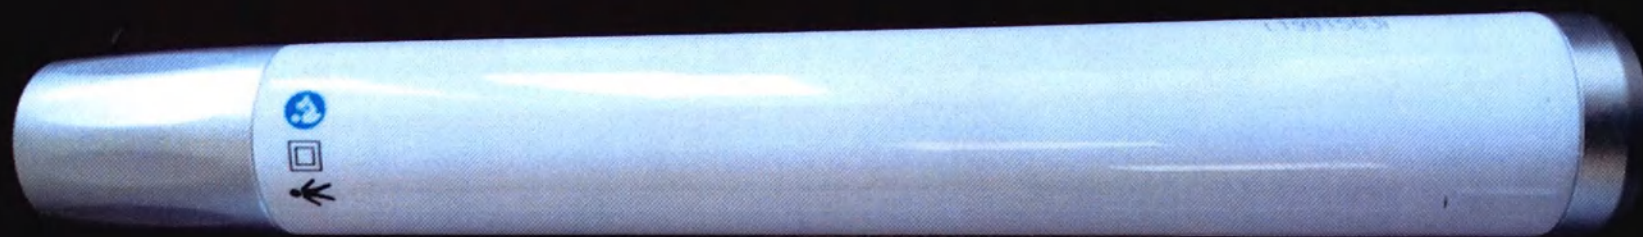

Product Name: Curing Light

Model: i Led



Guilin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, Guilin National High-Tech
Zone, Guilin, Guangxi, 541004 P. R. China
Website: <http://www.glwoodpecker.com>

EC REP

MedNet GmbH
Borkstrasse 10 · 48163 Muenster · Germany

Charge for battery: 3.7V (ICR18490)

Rated input: DC 5.0V/1A

Adapter Model: DJ-0500100-A5

Use only with adapter provided by manufacturer

2019



Лампа полимеризационная, модель i Led. Адаптер. Маркировка.



IV. Лампа полимеризационная, модель LED.H. Маркировка на упаковке.

Model: LED.H

UDI



(01) 0 6944843 60239 4 (21) L1990105H

SN



(a)

L1990105H

Model:
LED.H




Лампа полимеризационная, модель LED.H. Маркировка на упаковке.

Warning:

The equipment should be handled with care and kept away from the epicenter.
Keep away from the articles which are combustible, poisonous, caustic or explosive.

All rights of modifying the product are reserved to the manufacturer without further notice. The pictures are only for reference. The final interpretation rights belong to GUILIN WOODPECKER MEDICAL INSTRUMENT CO., LTD. The industrial design, inner structure, etc., have claimed for several patents by WOODPECKER. any copy or fake product must take legal responsibilities.
Industrial design patent No.: CN 201130176281.3



BASIC DATA:


Battery	3.7V
Power Input	AC110V~240V
Dimensions	272mm*191mm*94mm



Guilin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, Guilin National High-Tech
Zone, Guilin, Guangxi, 541004 P. R. China

Tel:

Europe Sales Dept.: +86-773-5873196, +86-773-2125222
North America, South America &
Oceania Sales Dept.: +86-773-5873198, +86-773-2125123
Asia & Africa Sales Dept.: +86-773-5855350, +86-773-2125896
Fax: +86-773-5822450
E-mail: woodpecker@glwoodpecker.com, sales@glwoodpecker.com
Website: <http://www.glwoodpecker.com>



MedNet GmbH
Borkstrasse 10 · 48163 Münster · Germany

ZM2010-088 V1.1

Лампа полимеризационная, модель LED.H. Основной блок из светодиодов. Маркировка.



Лампа полимеризационная, модель LED.H. Основной блок из светодиодов. Маркировка.





Лампа полимеризационная, модель LED.H. Адаптер. Маркировка.



Лампа полимеризационная, модель LED.H. Фотометр - яркомер. Маркировка.



Product Name : LED Light Meter

Model : LM-1

Tolerance: $\pm 10\%$

Input: 4.5V, 3pcs AAA batteries

Test wavelength range: 400 - 500nm

Guilin Woodpecker Medical Instrument Co., Ltd.
Information Industrial Park, National High-Tech
Zone, Guilin, Guangxi, 541004 P.R. China

В настоящем документе прошито
и скреплено оттиском печати

25 лист об

Генеральный директор управляющей
организации ООО «Корос Групп»

Н.В. Тишина






ООО «МайДент24»
125124, РФ, г. Москва, 5-я ул. Ямского поля,
д.7, корп.2, ЭТ/ПОМ/КОМ 2/1/68
тел./факс: +7 (495) 665-79-32
ИНН 7714780239/ КПП 771401001

Фотографические изображения медицинского изделия:


Лампа полимеризационная, модели: X-Cure, B-Cure, iLed, LED.H

1. Лампа полимеризационная, модель: X-Cure


Упаковка

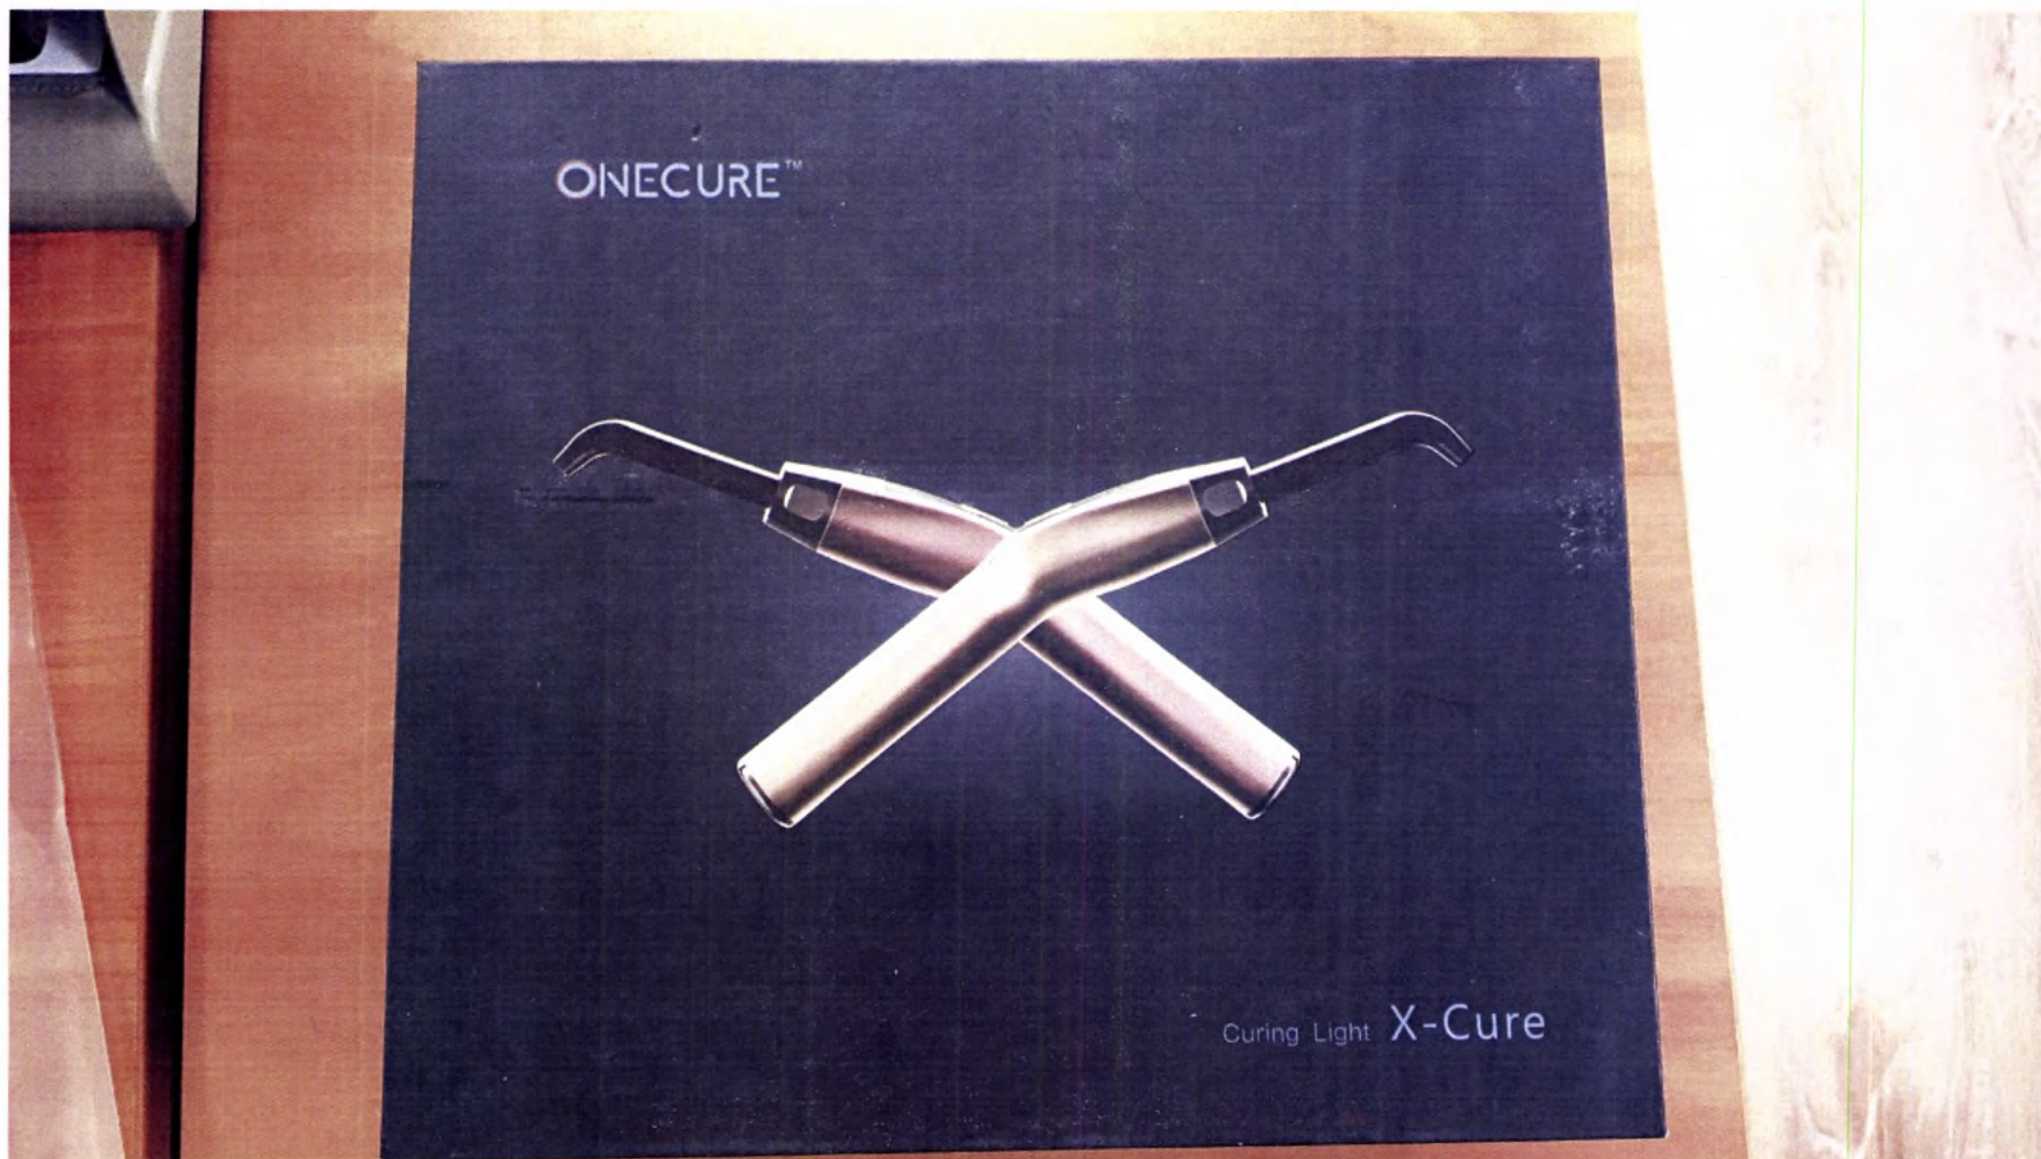


Вид в упаковке

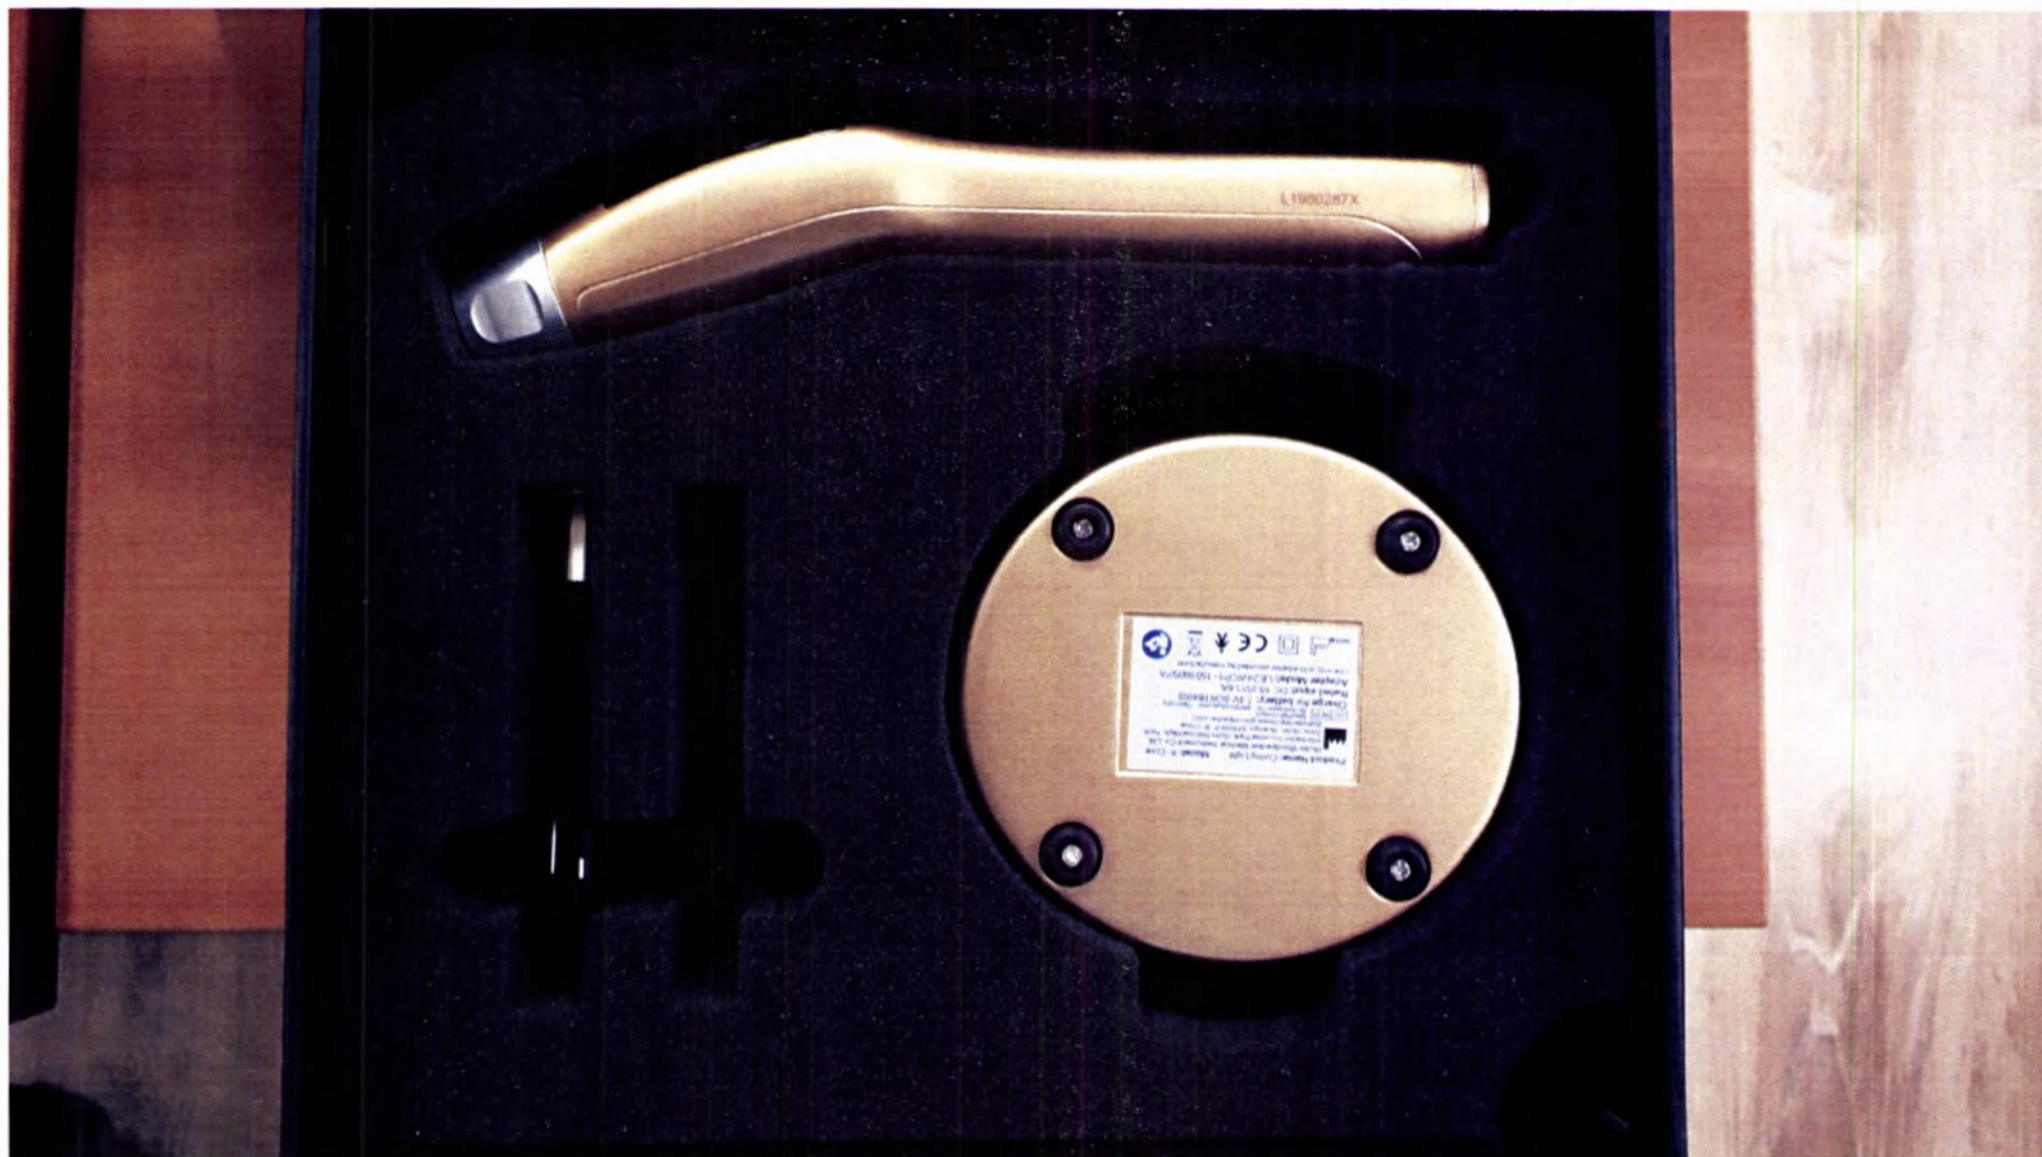


1. Основной блок из светодиодов.

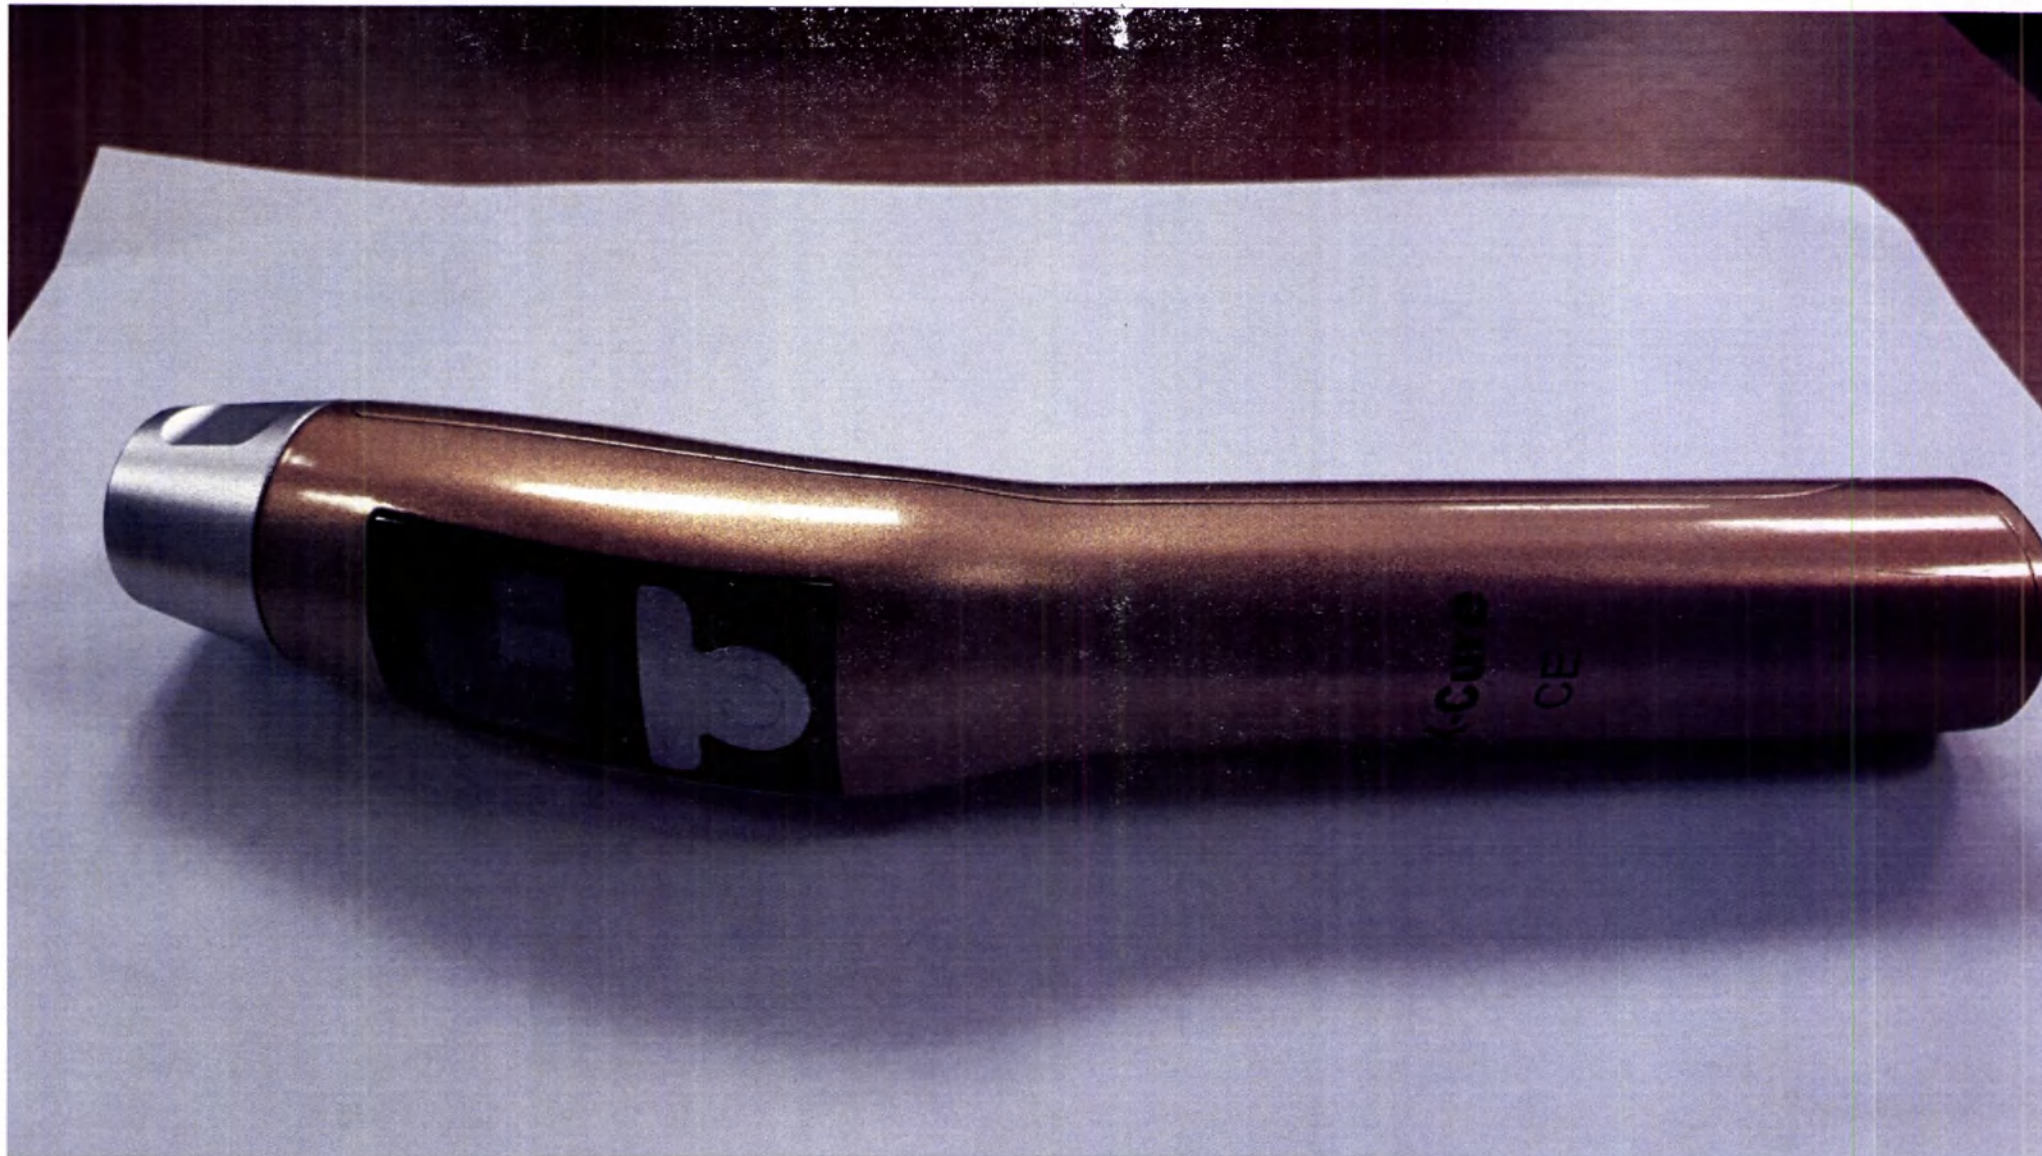


2. Наконечник оптоволоконный съемный.

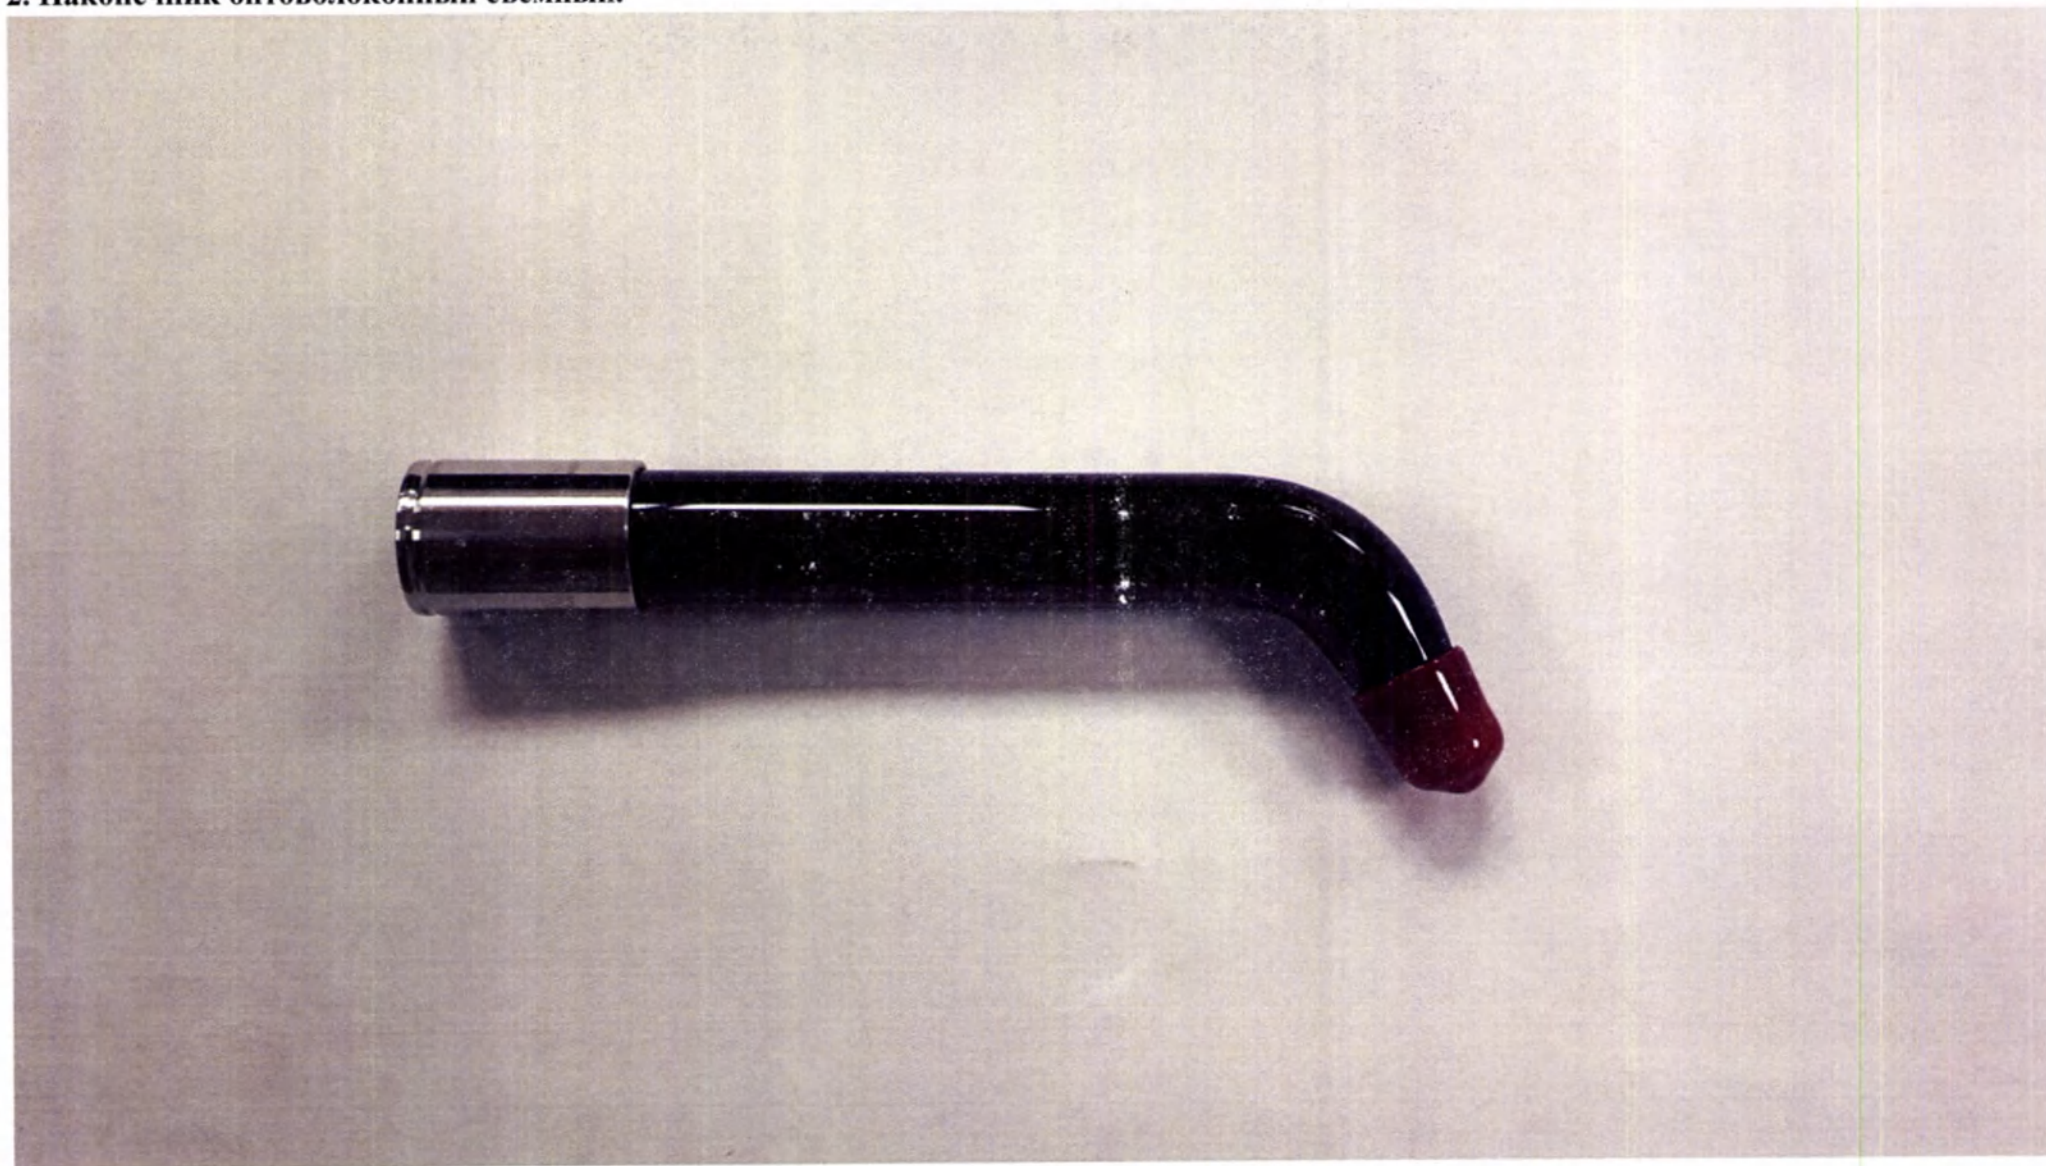


3. Световой фильтр.

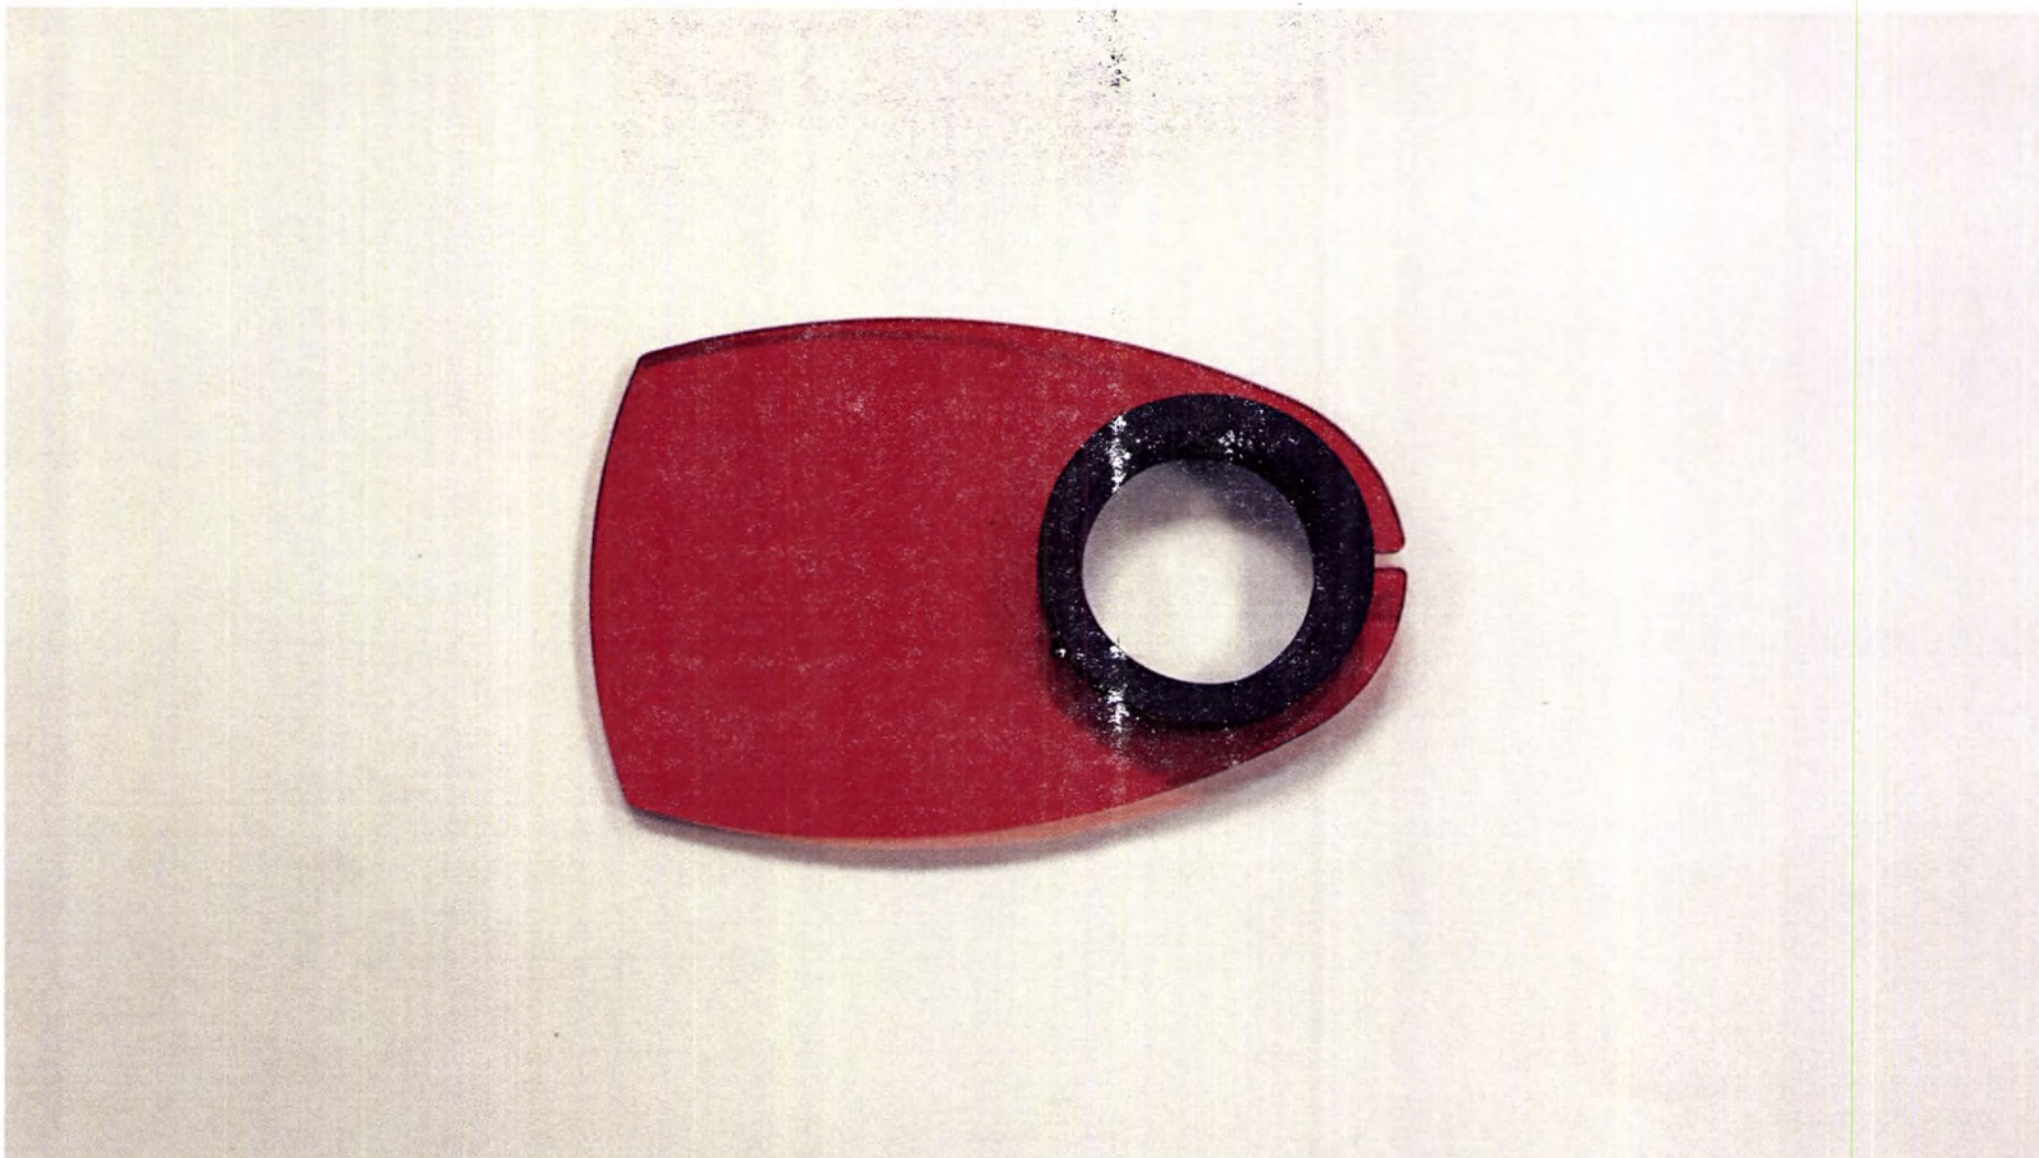

4. Зарядное устройство.

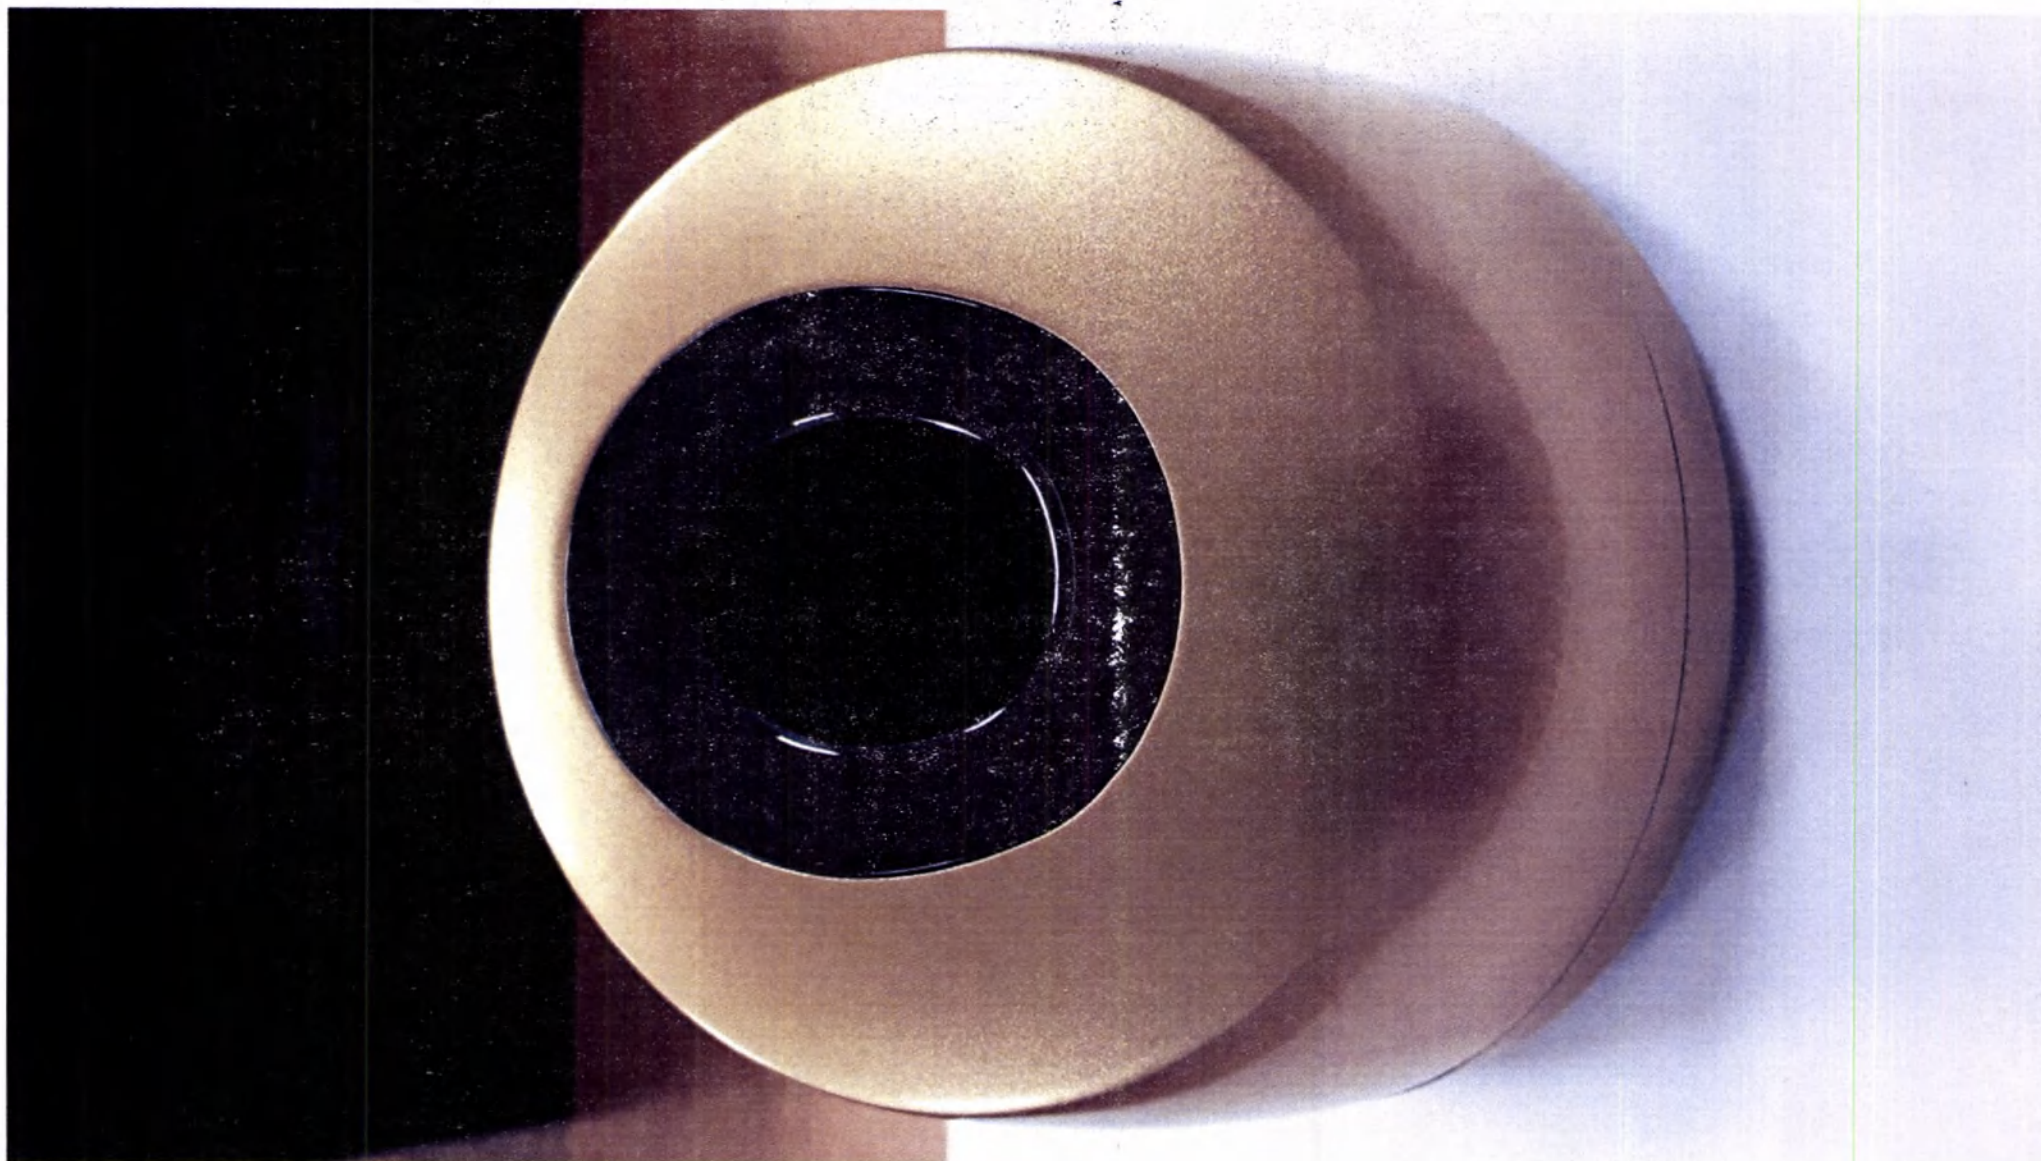

5. Адаптер.

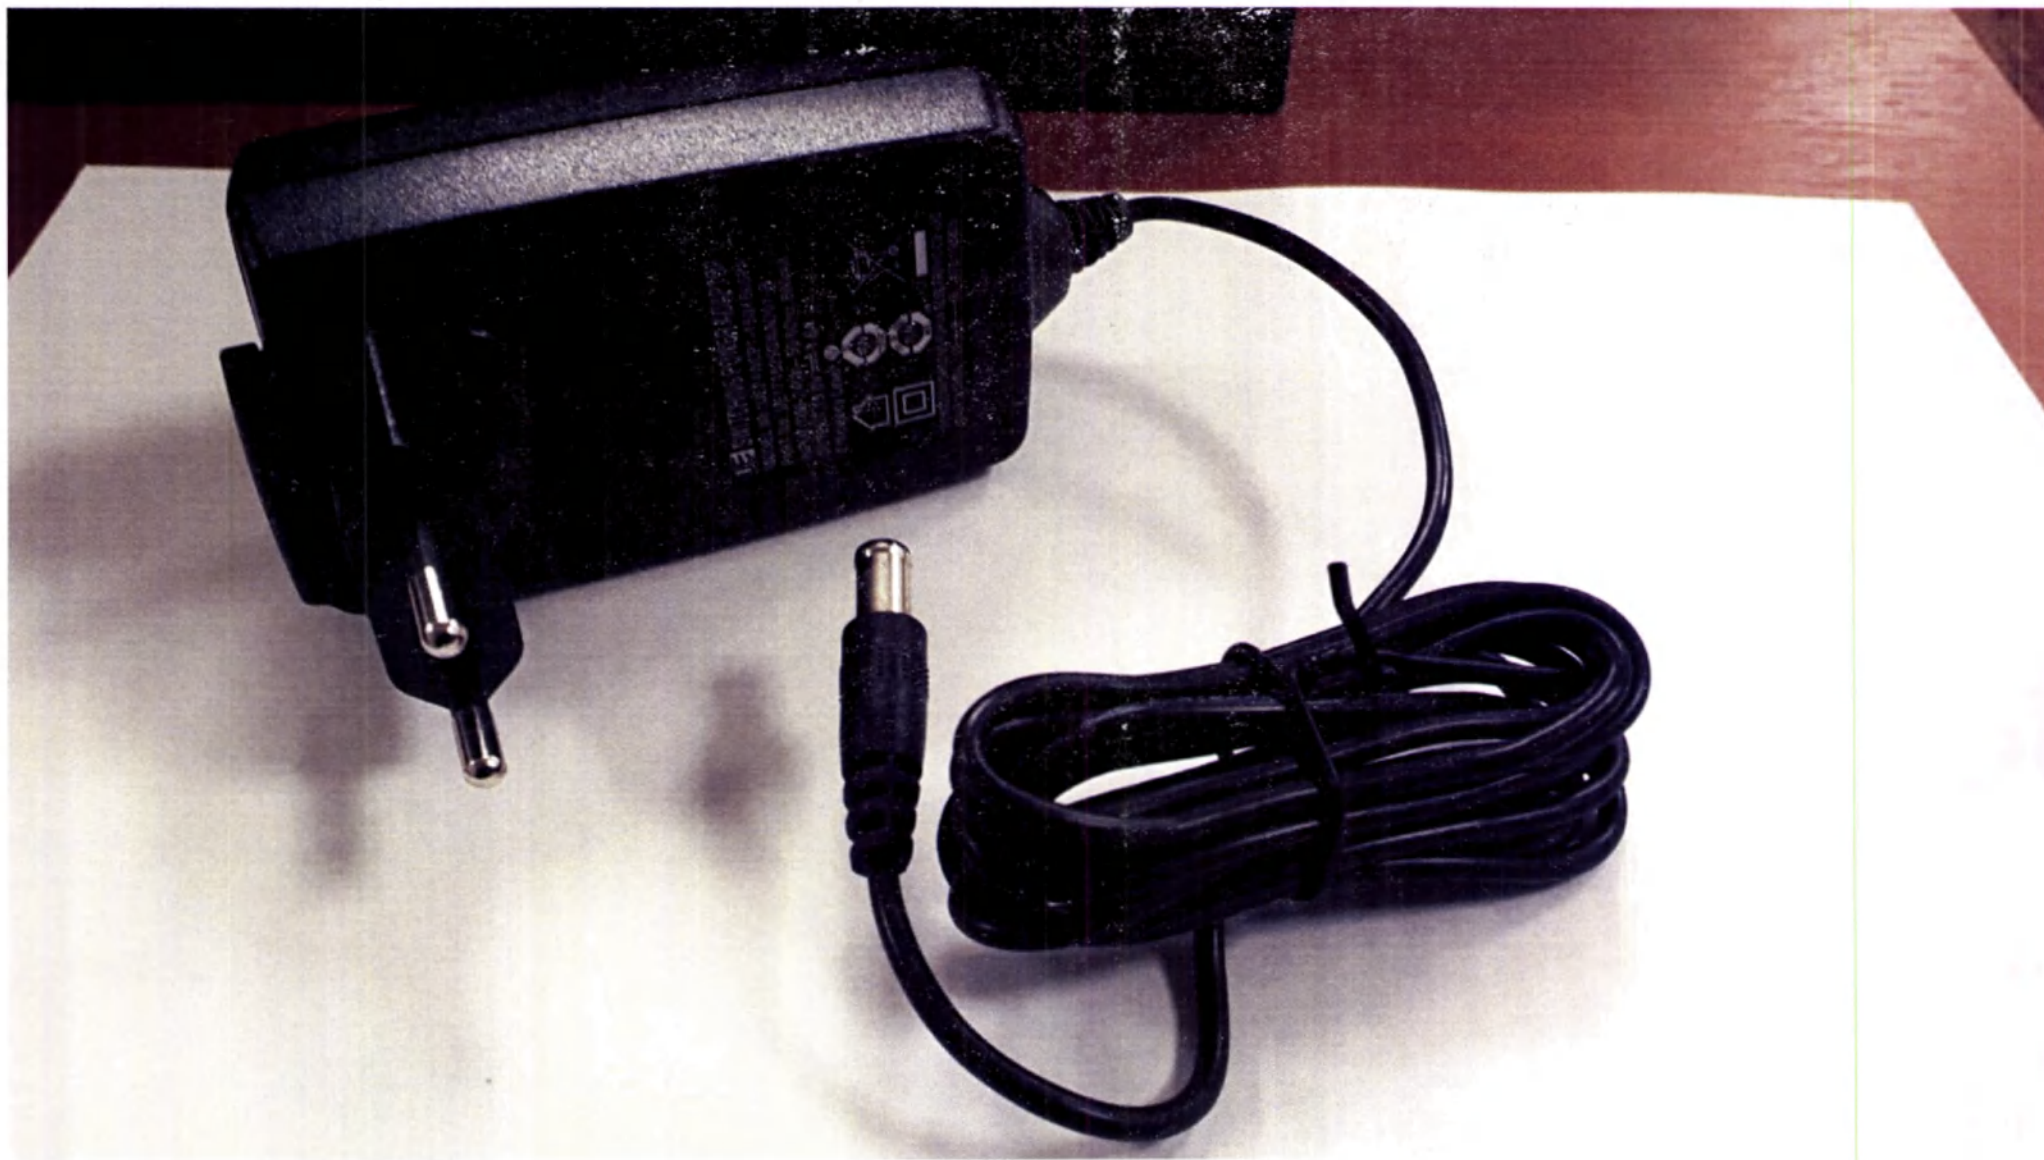


6. Батиметр.




7. Защитные очки.



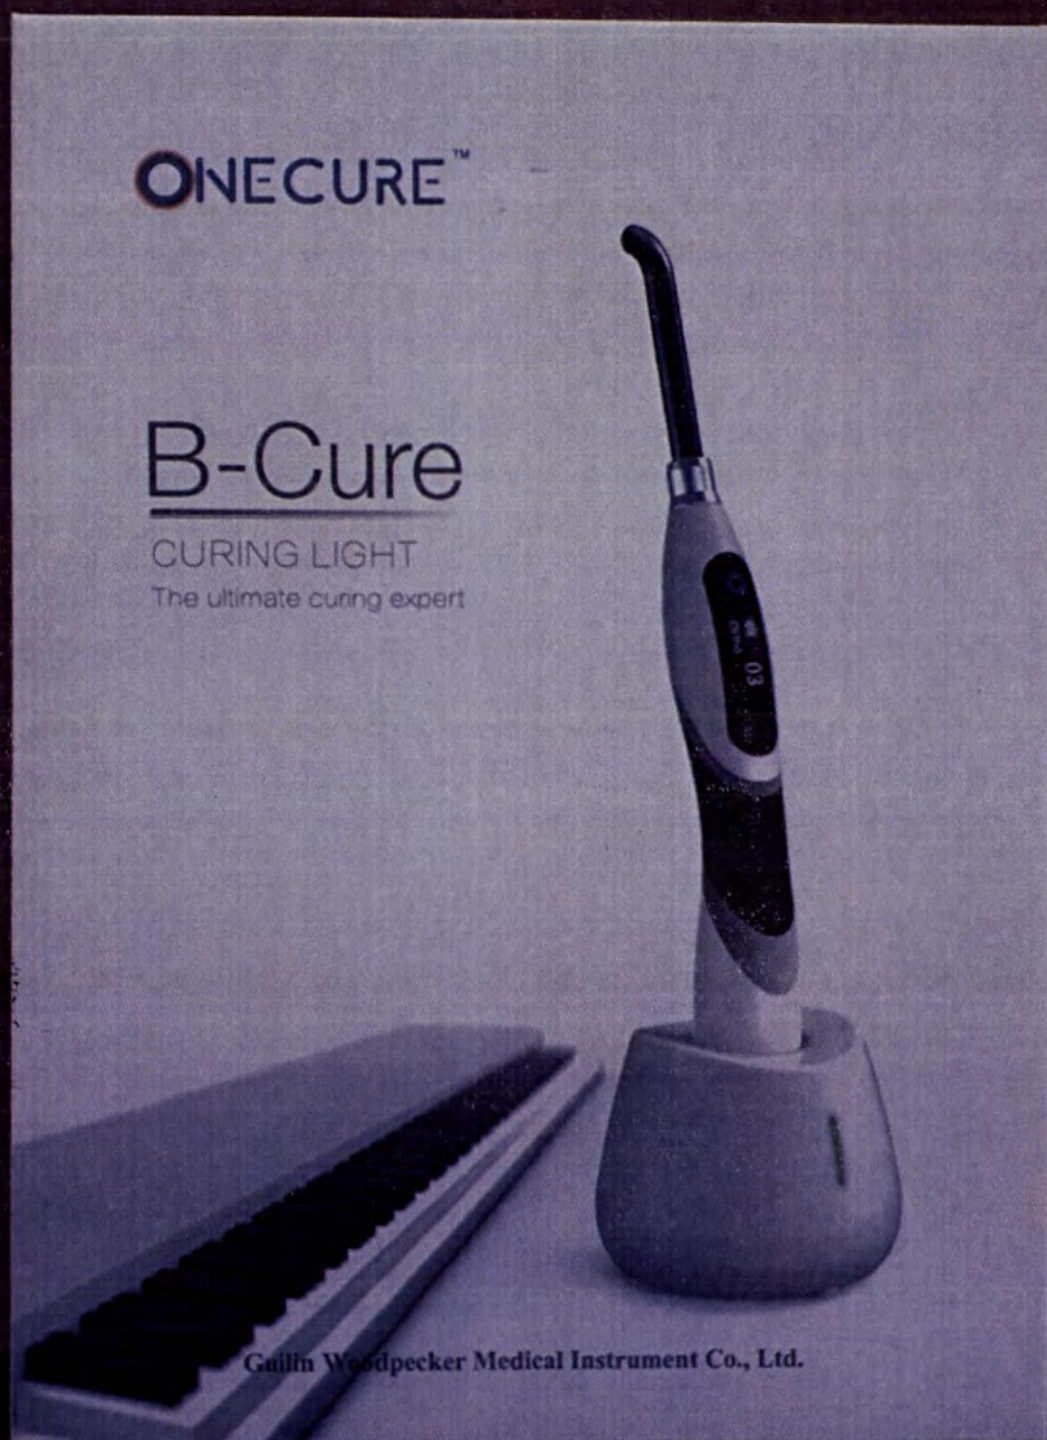


Guilin Woodpecker Medical Instrument Co., Ltd.


1. Основной блок из светодиодов.

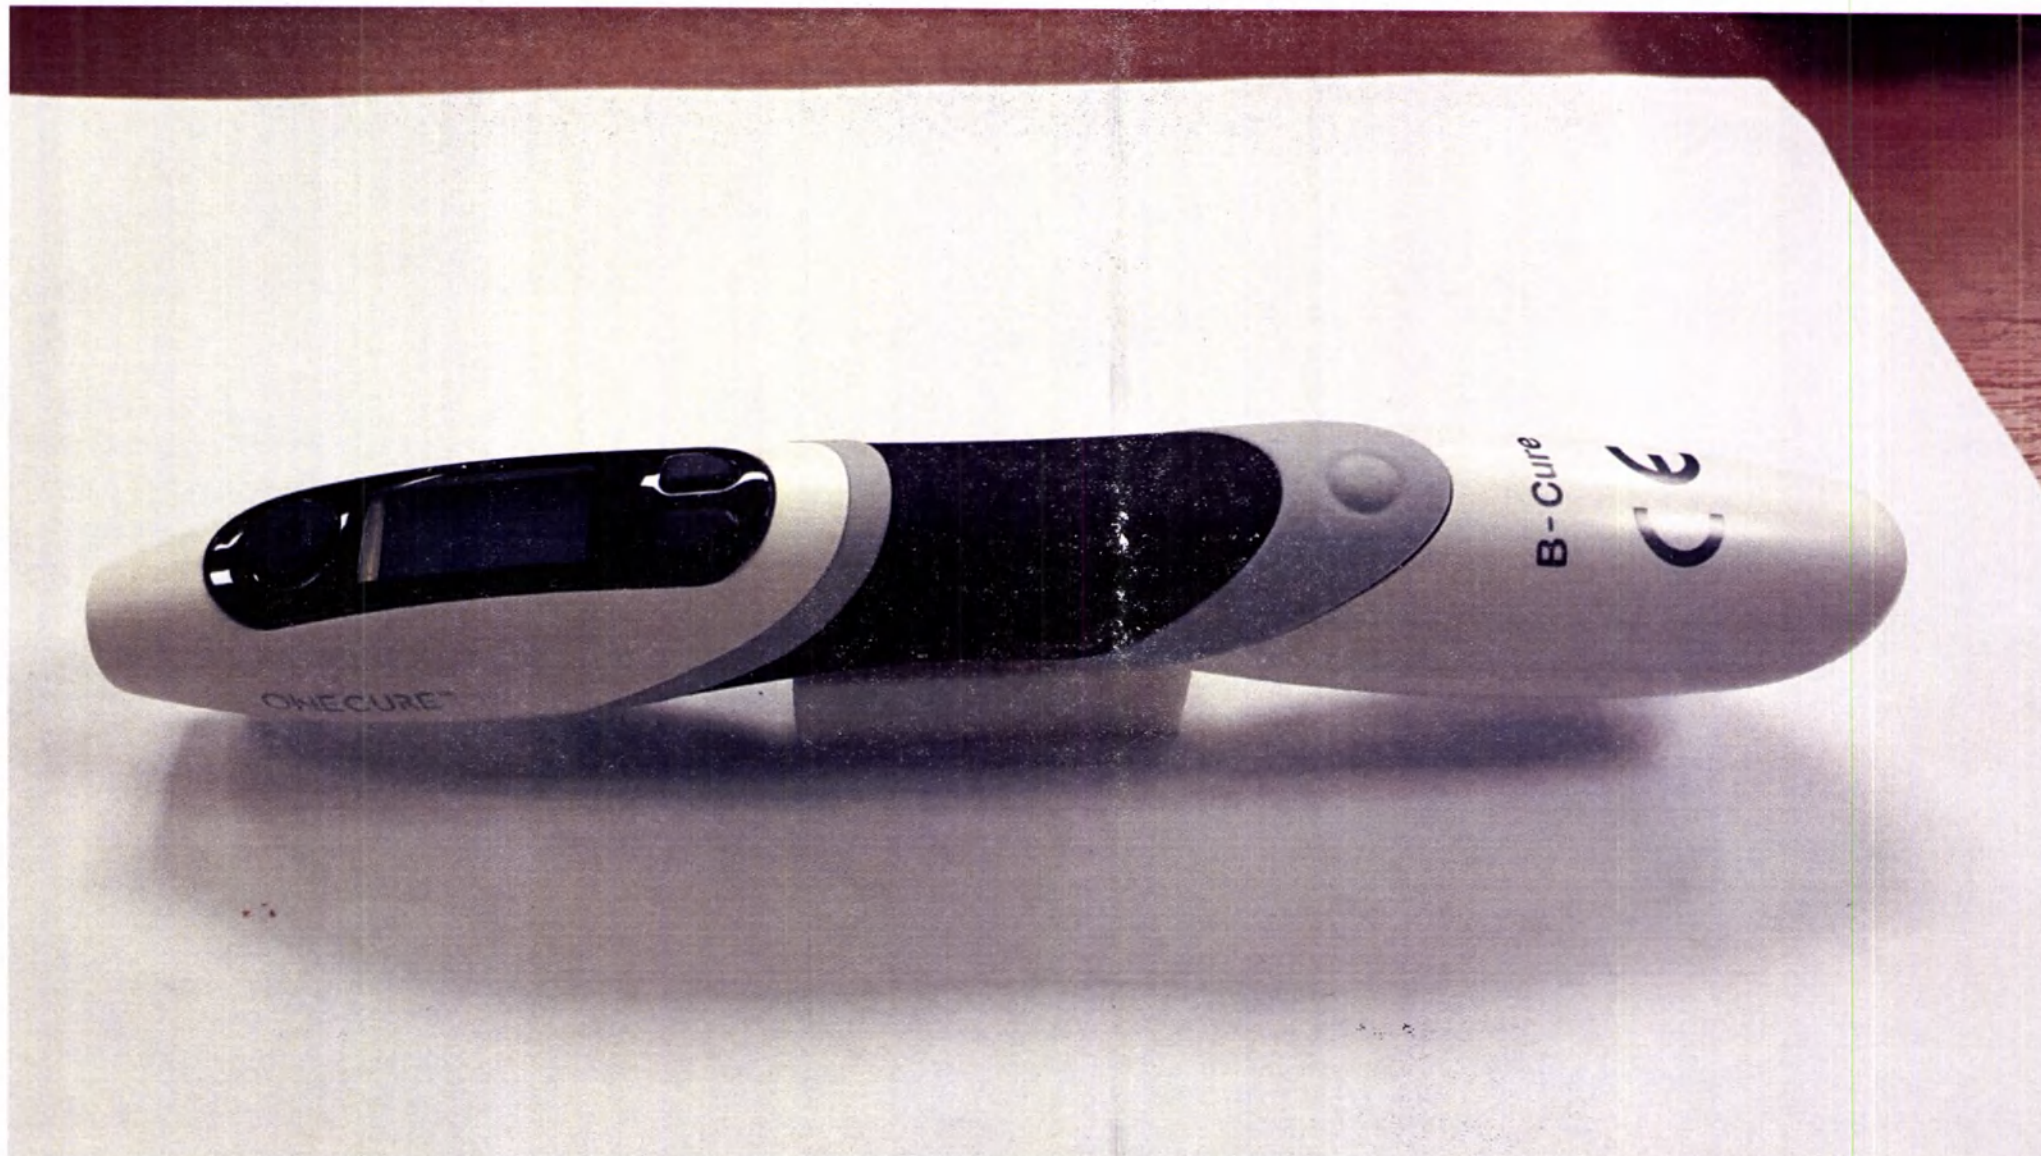


2. Наконечник оптоволоконный съемный.

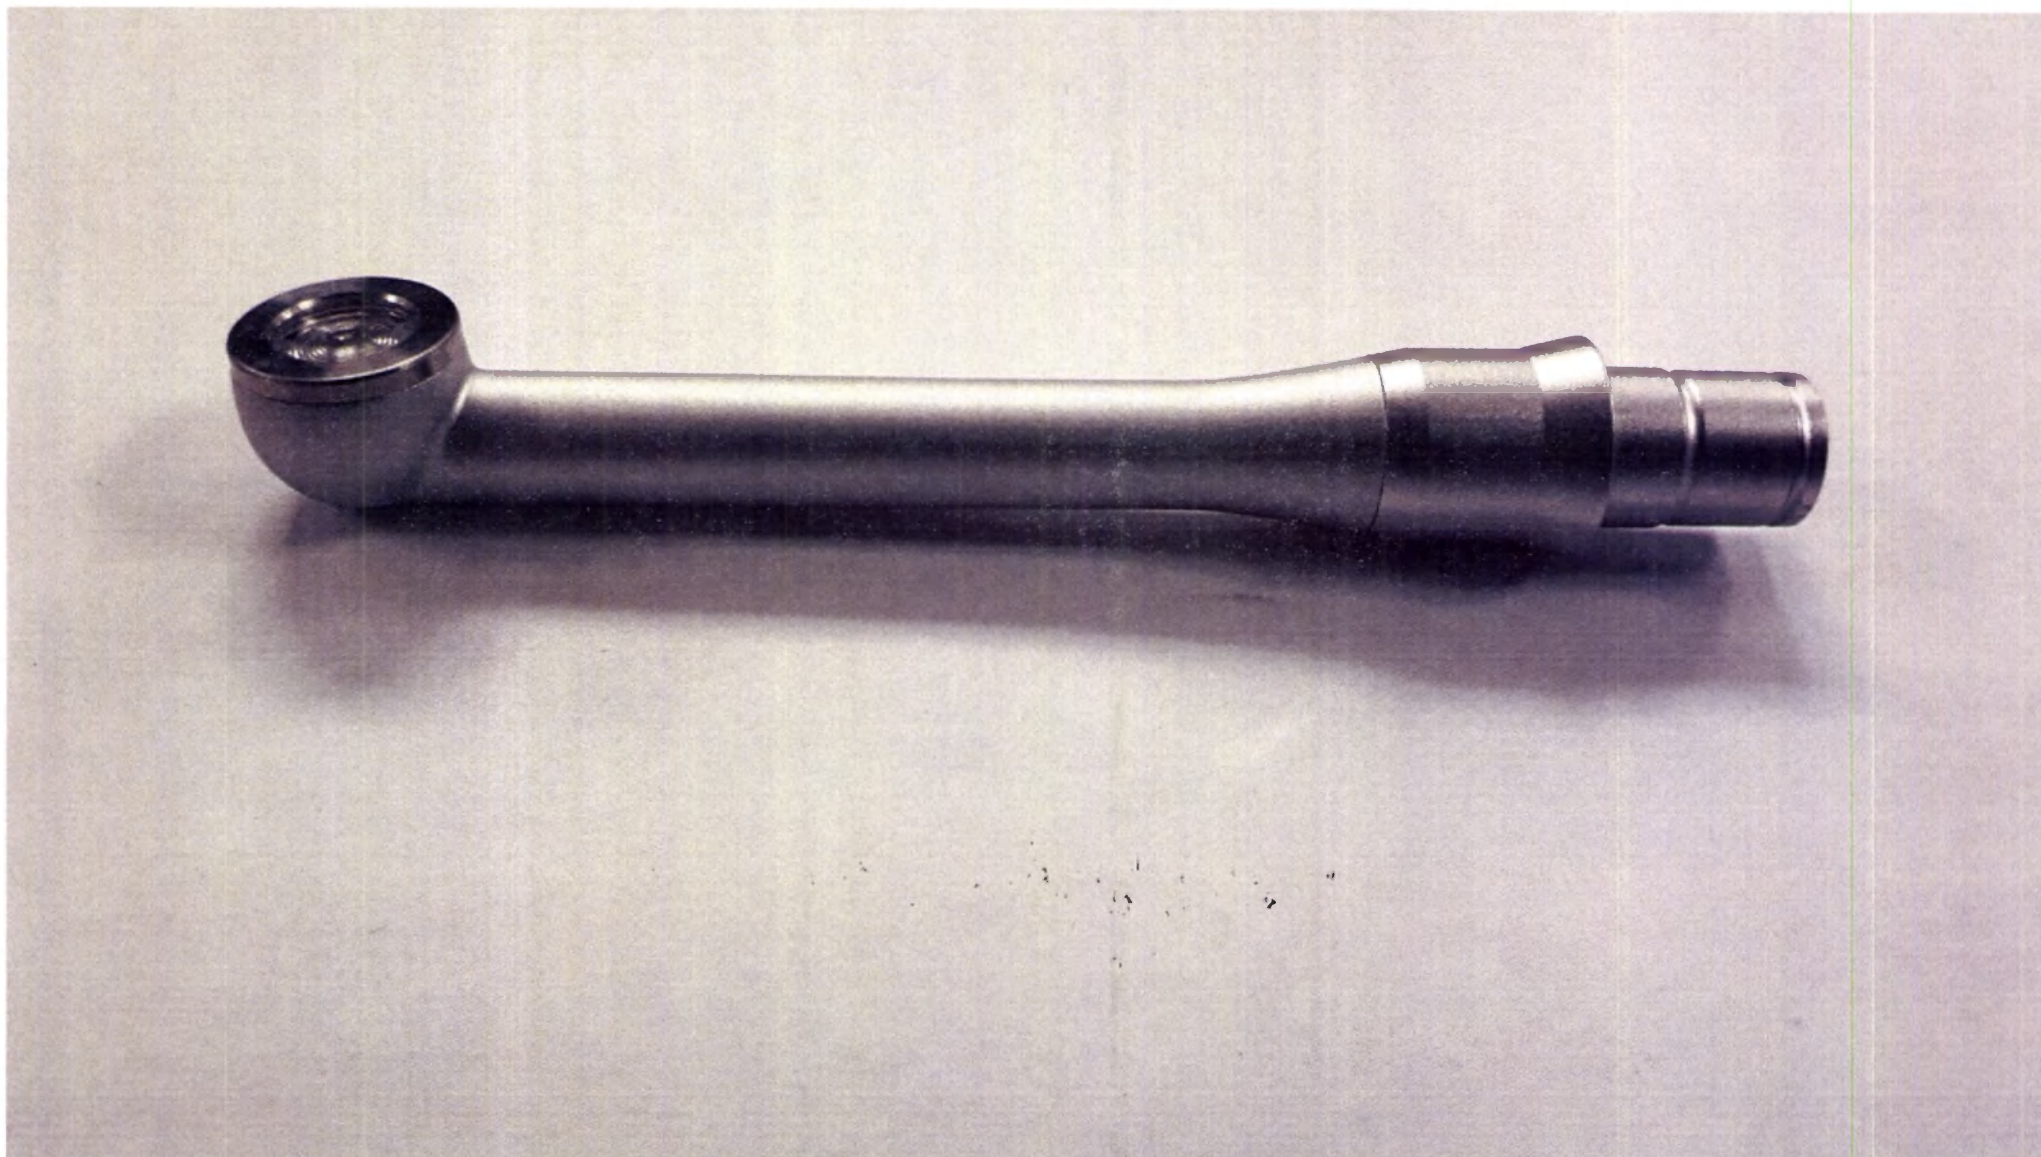

3. Световой фильтр.

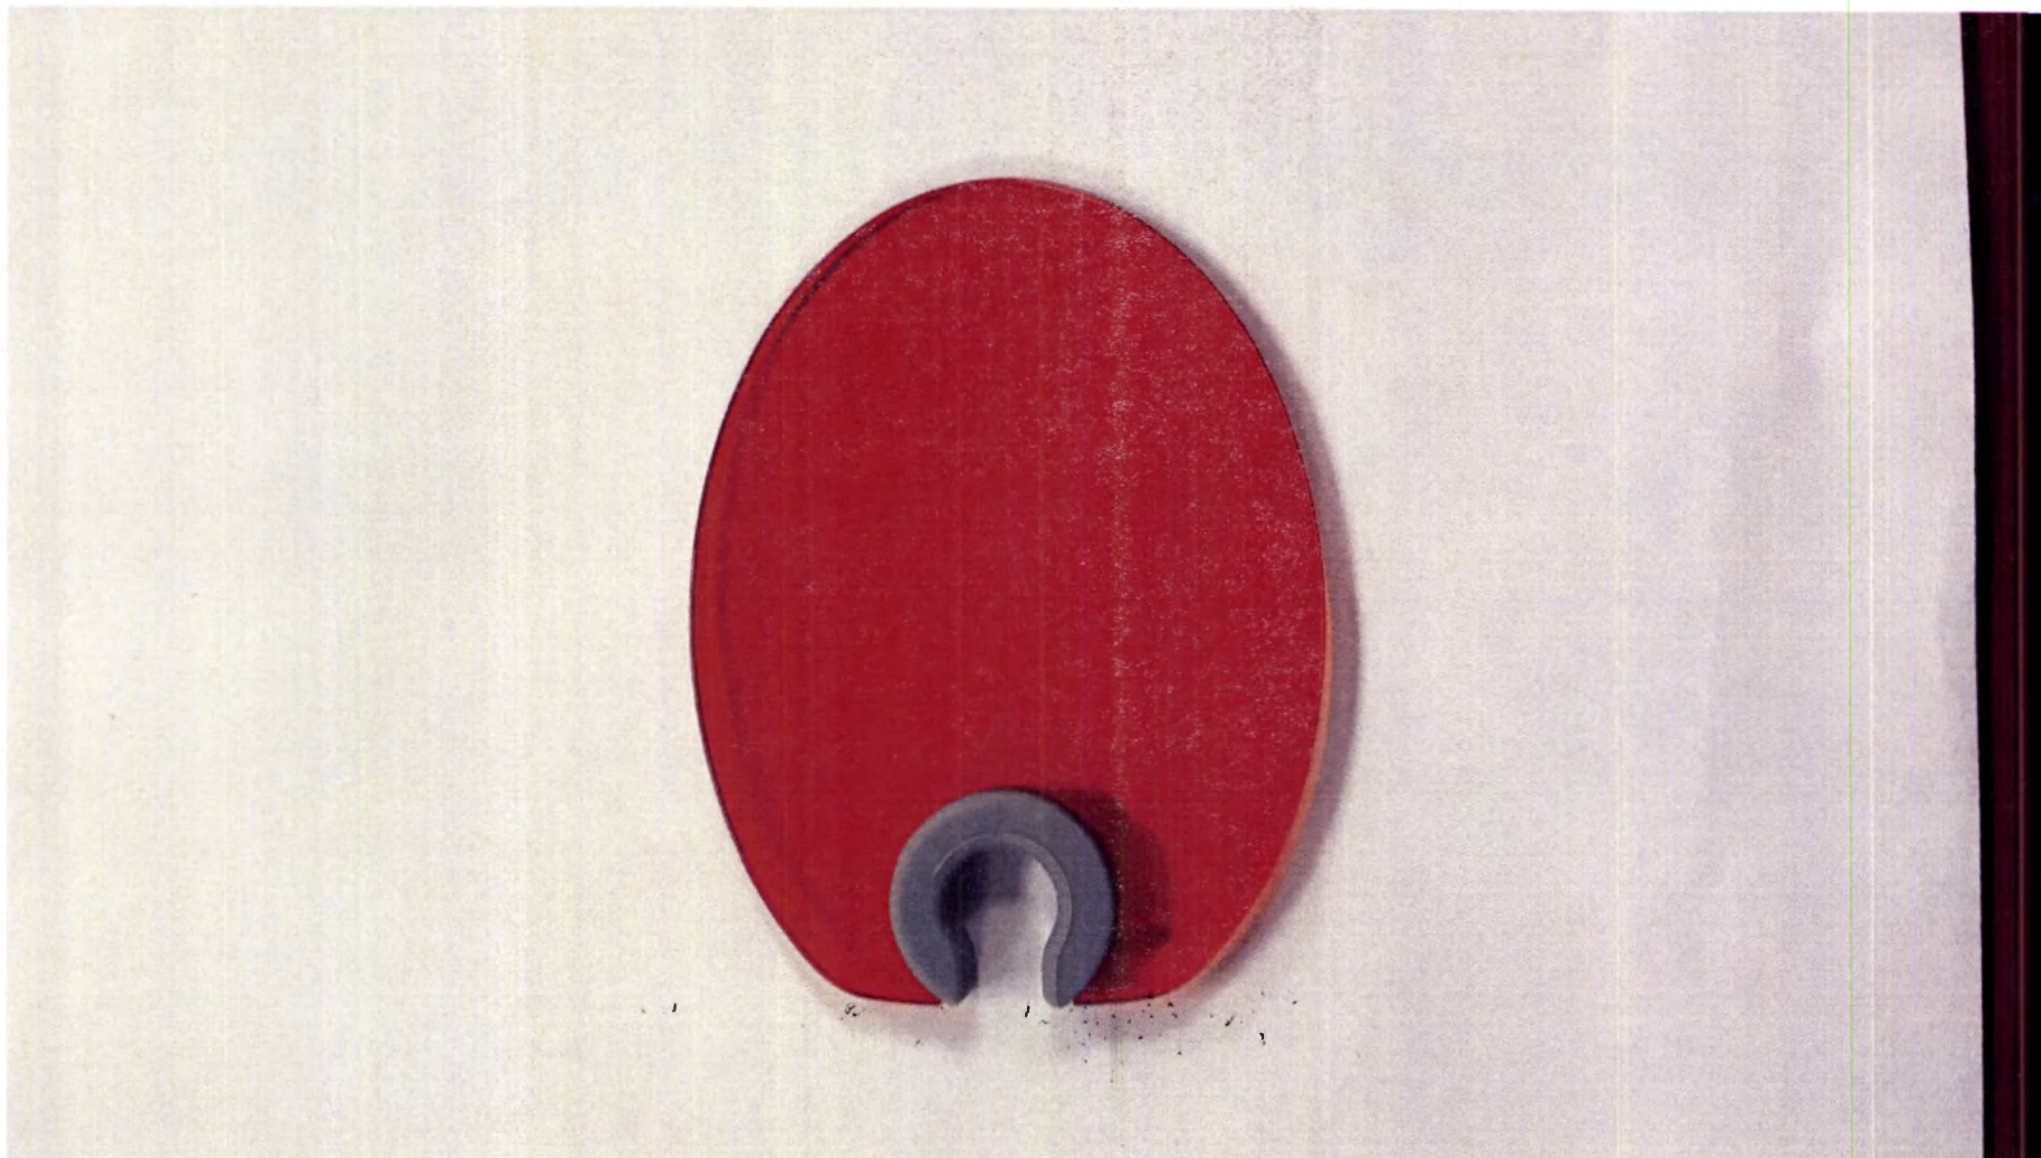


4. Зарядное устройство.

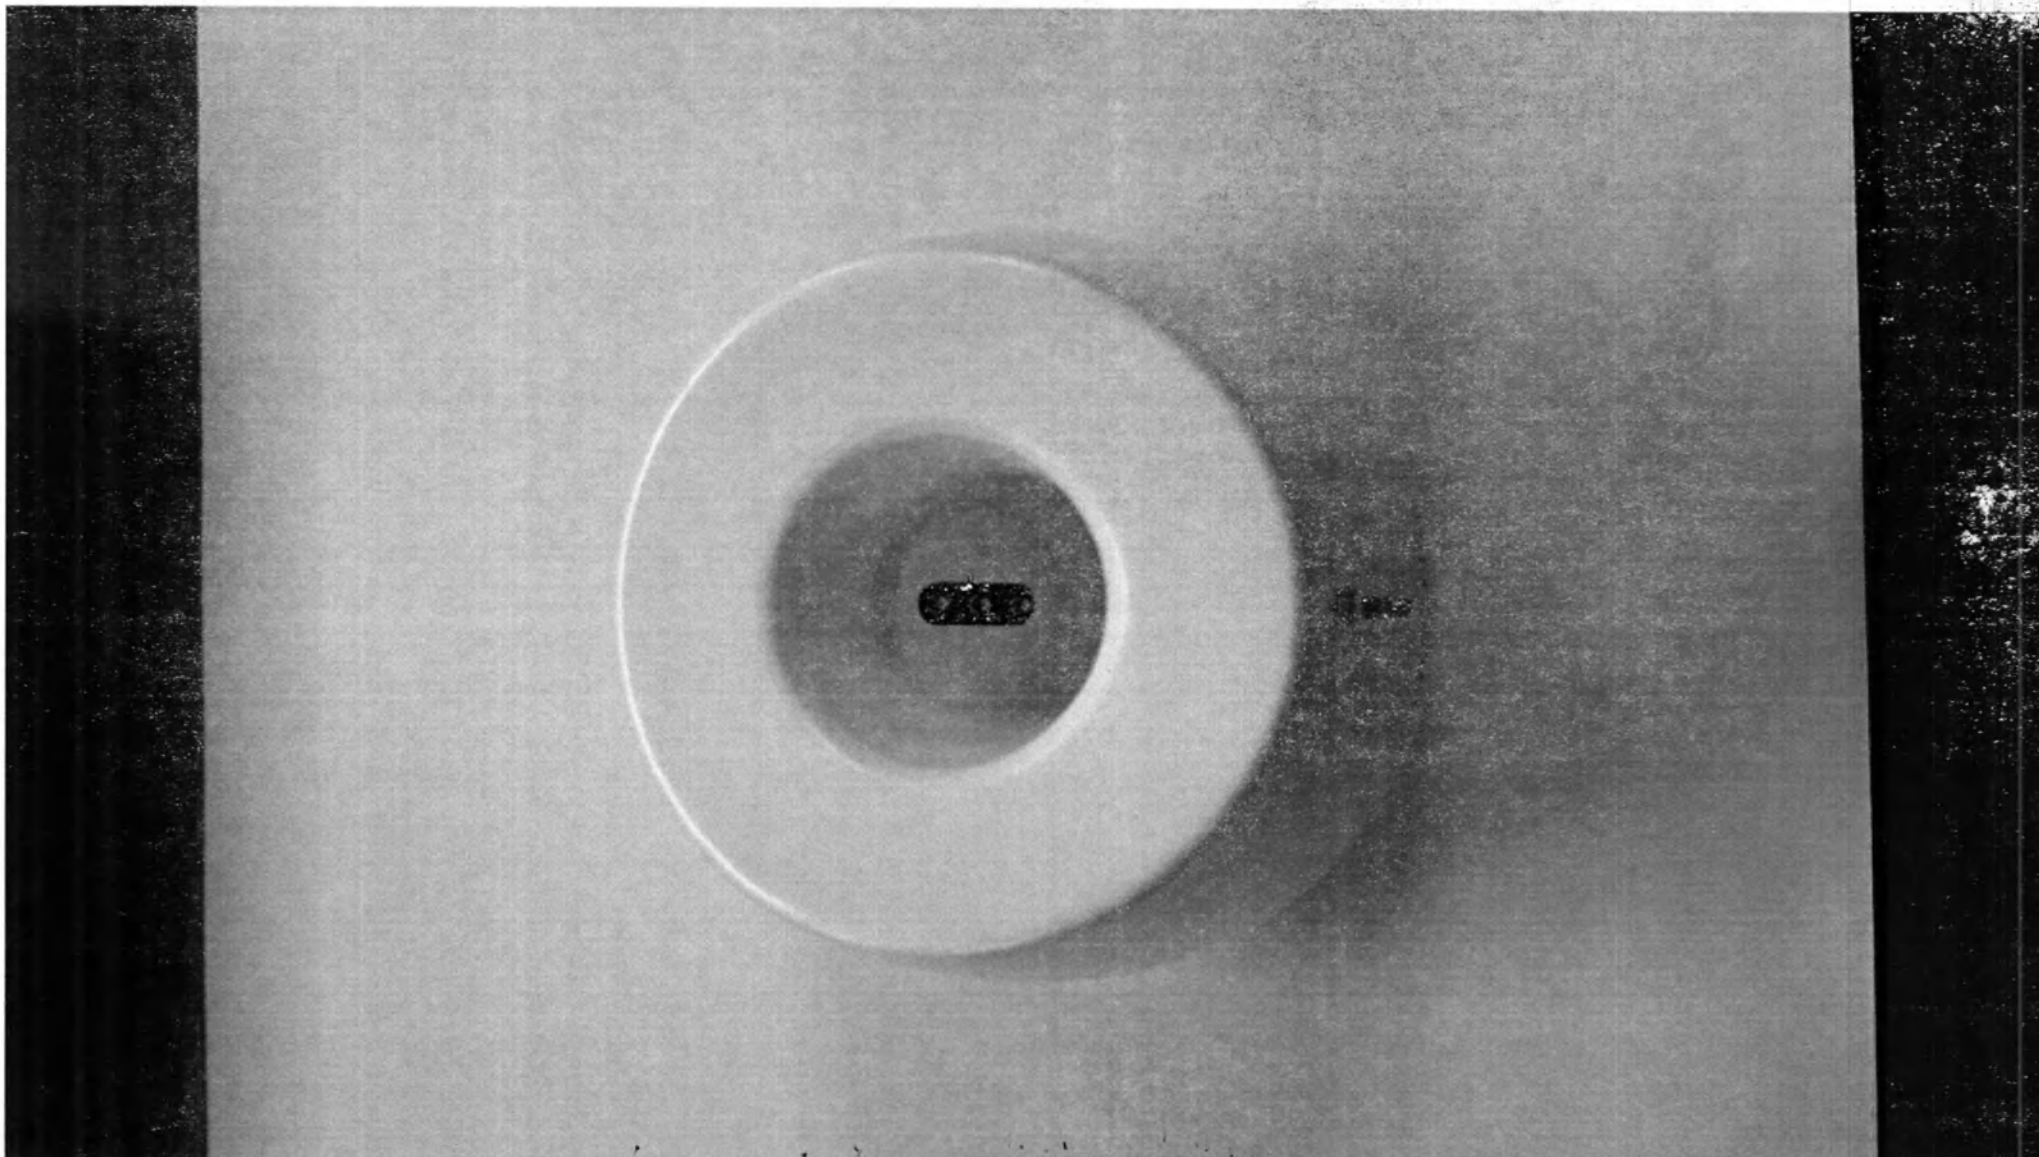

5. Адаптер.



6. Аккумуляторная батарея.

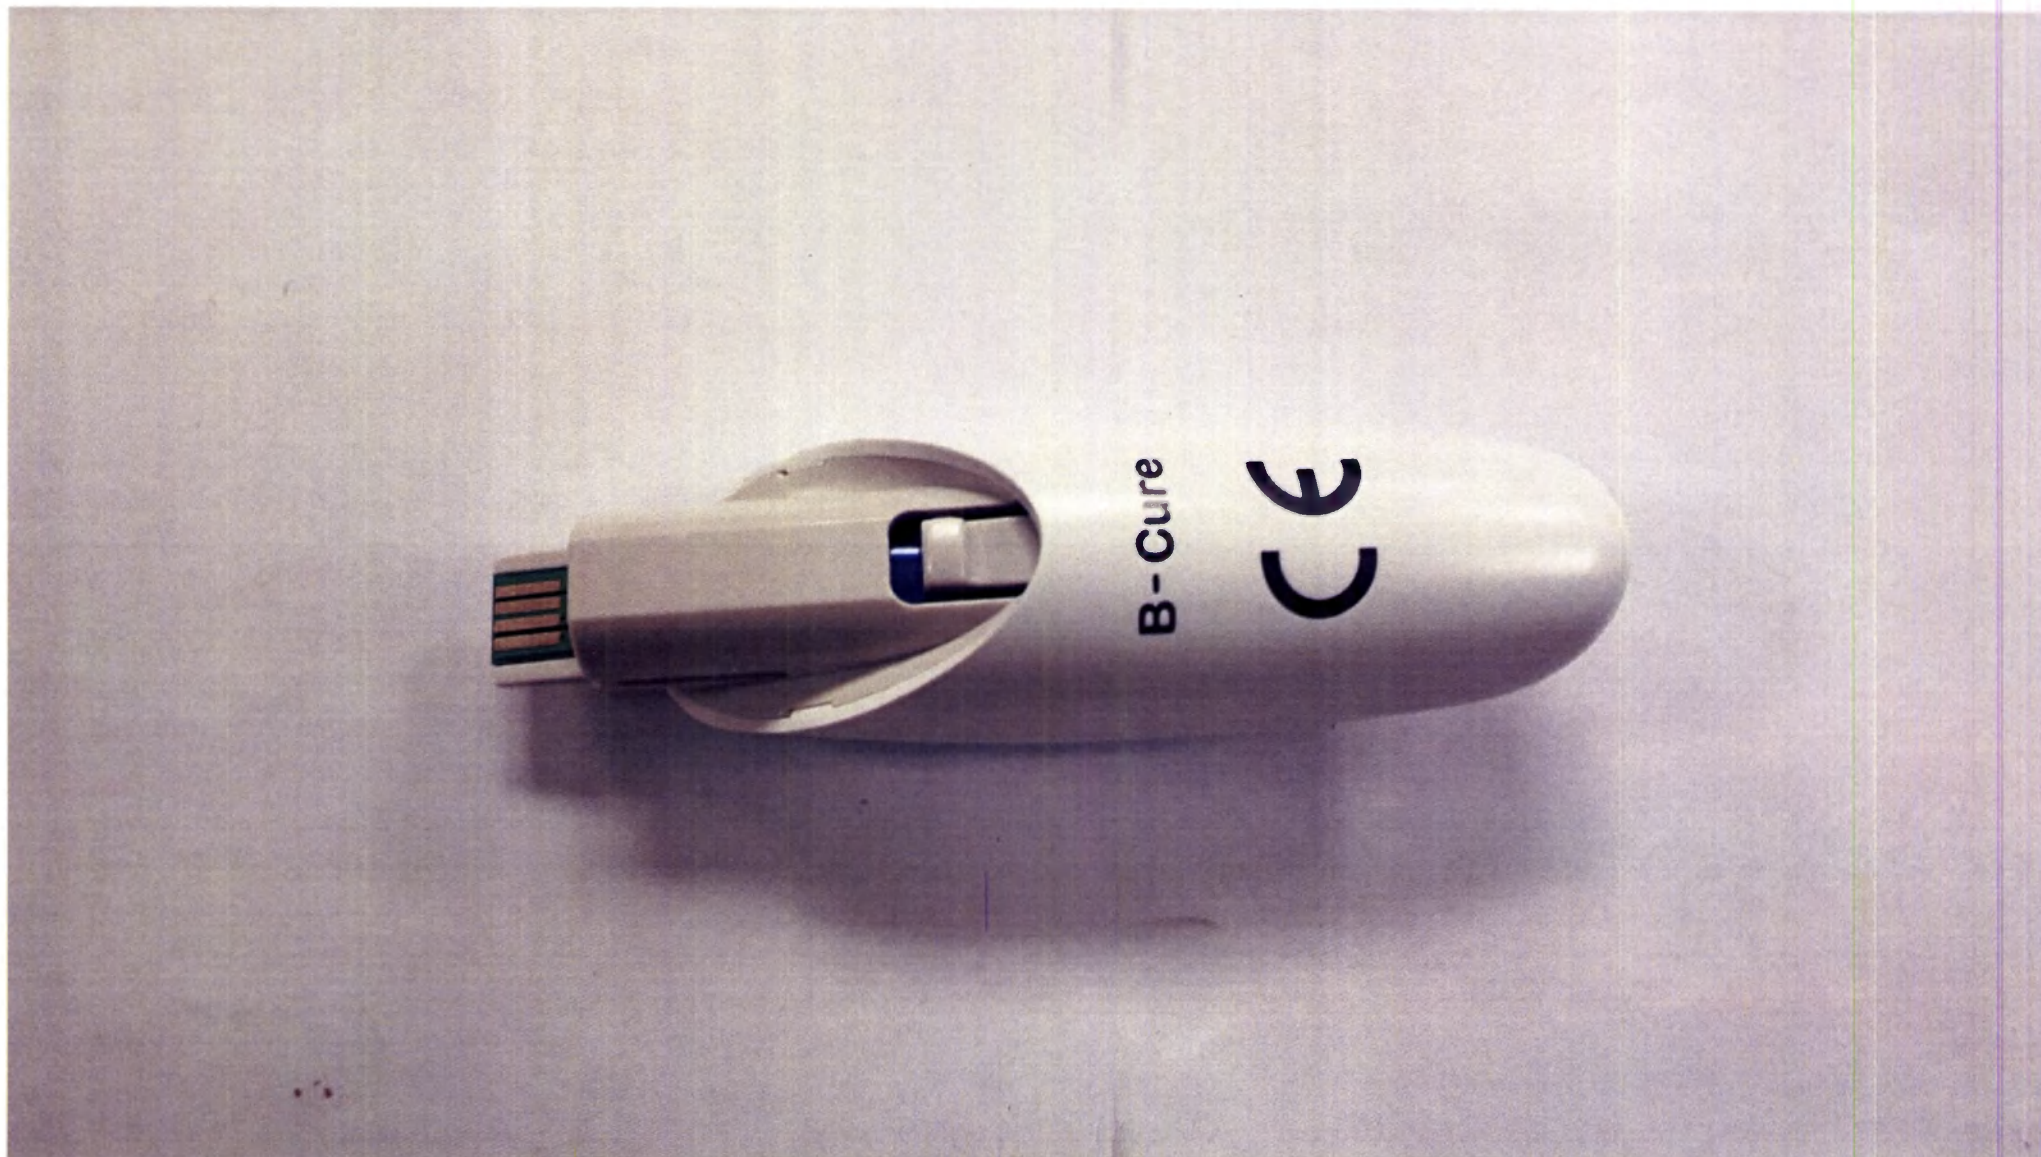



7. Батиметр.




III. Лампа полимеризационная, модель i Led

Упаковка

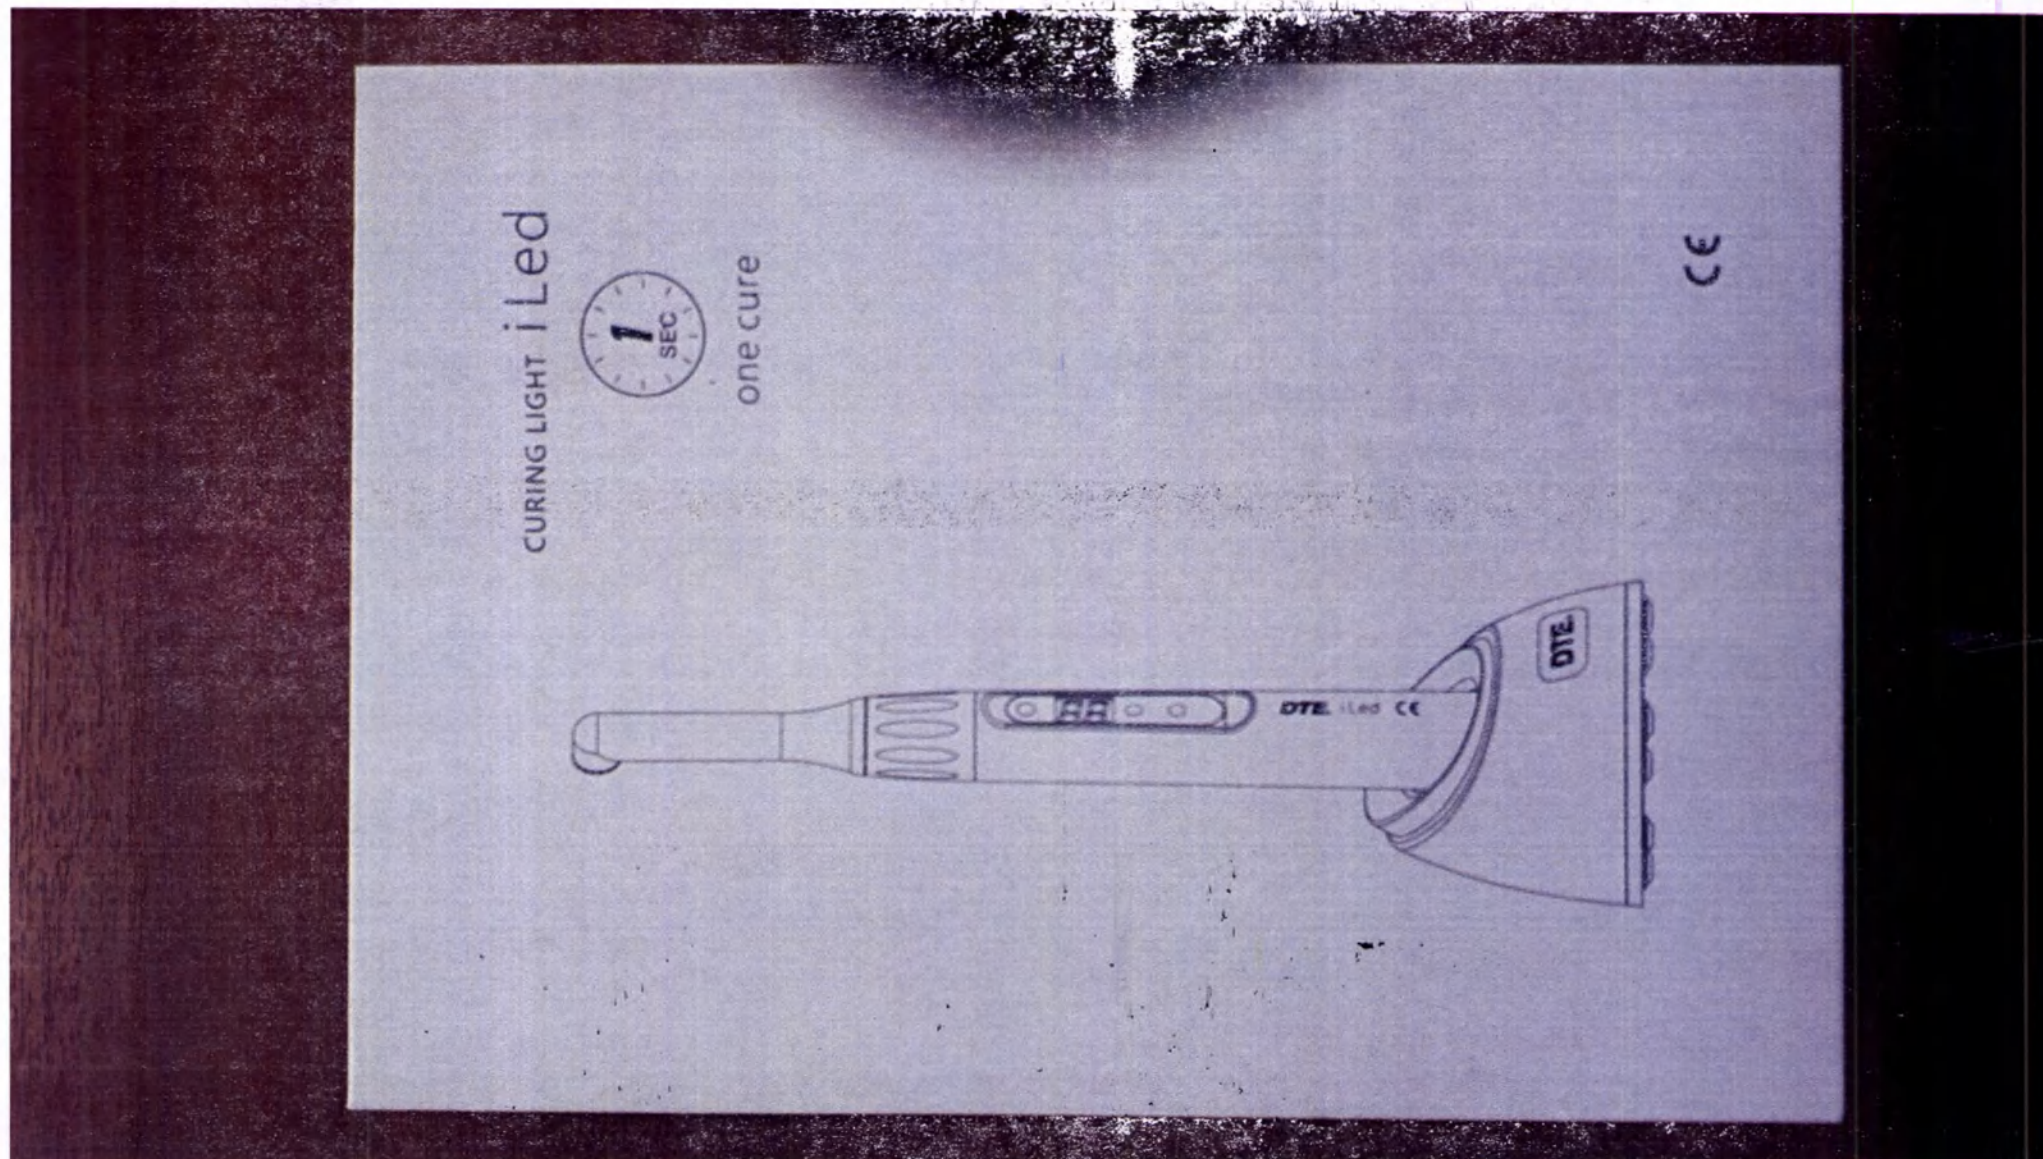


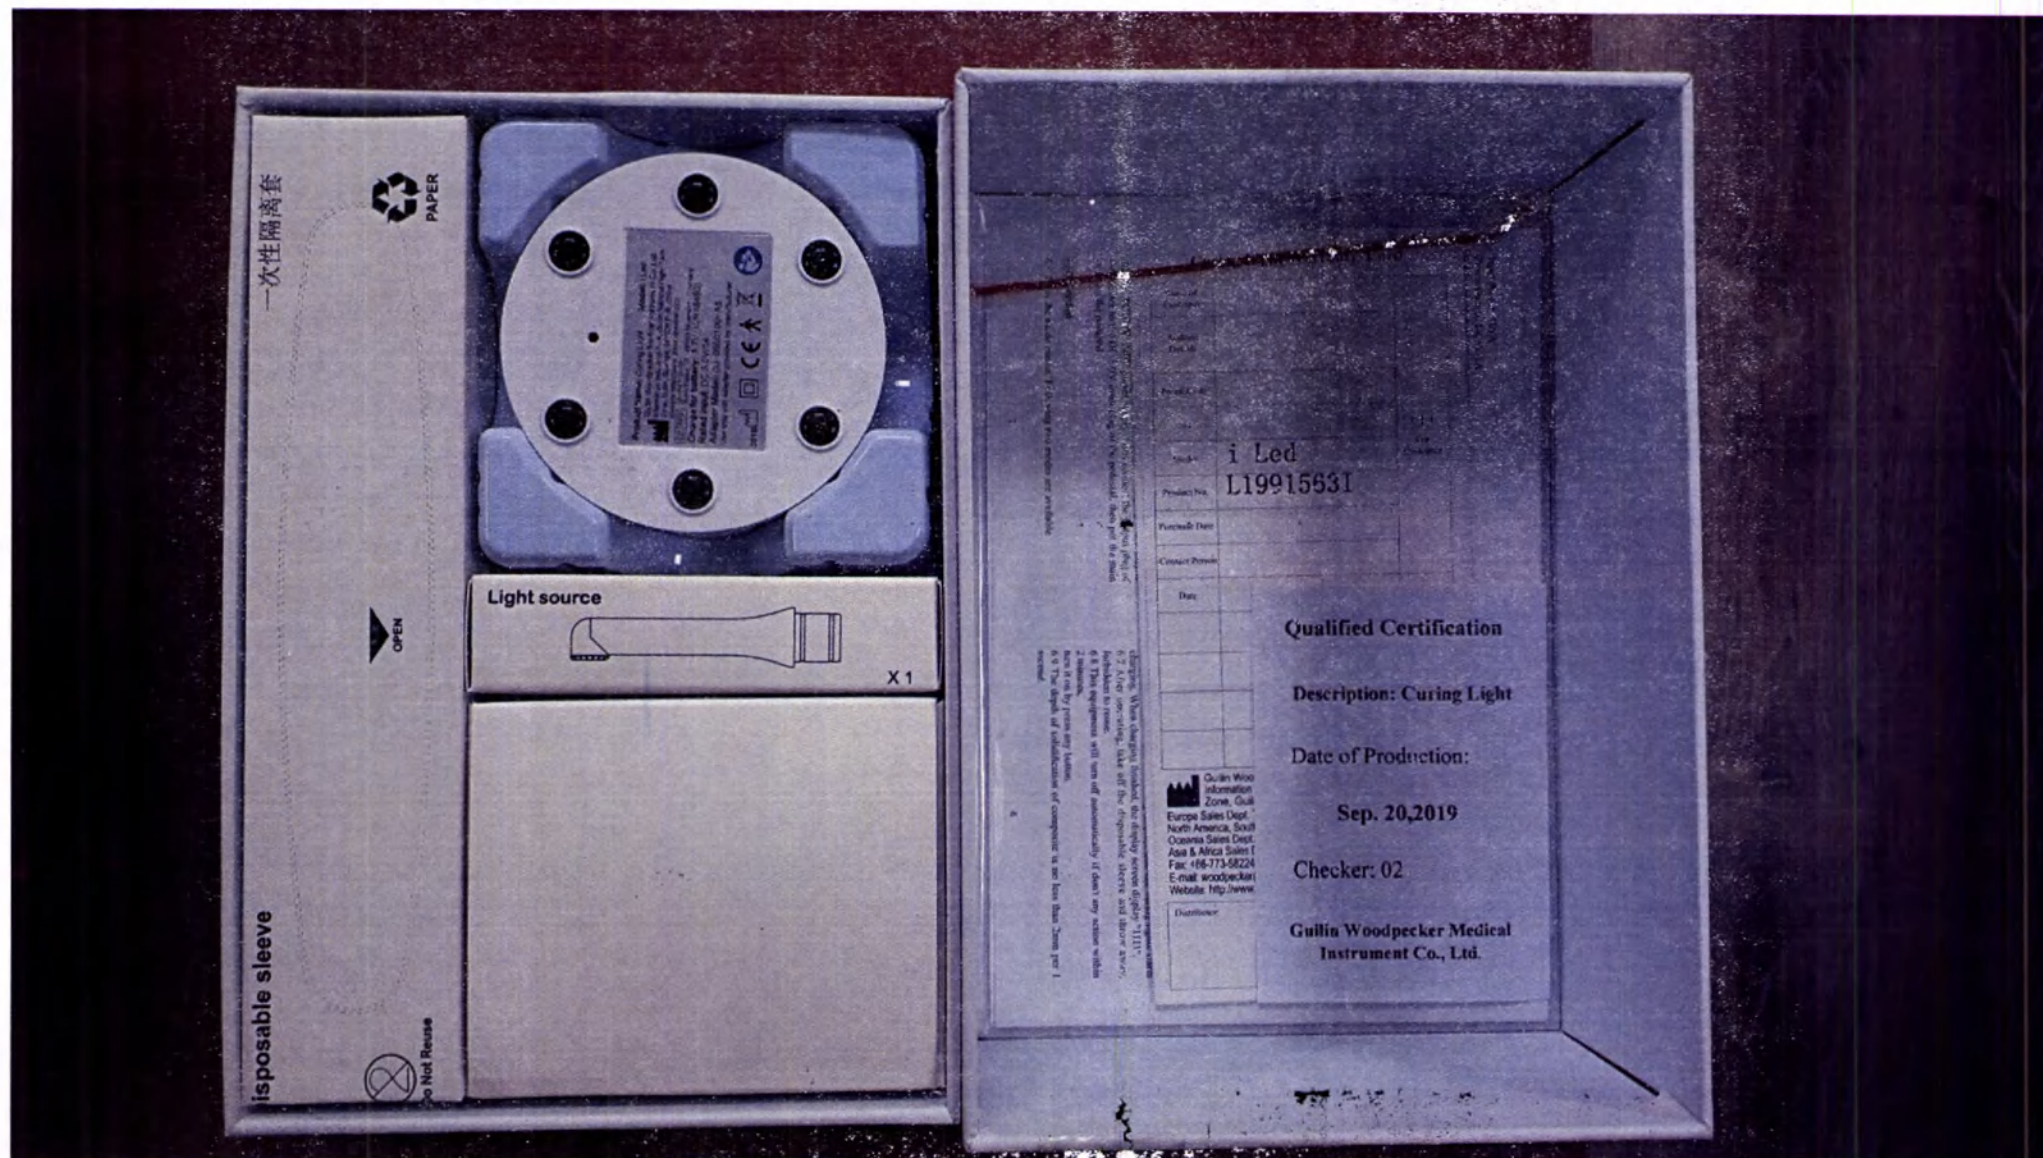


1. Основной блок из светодиодов.

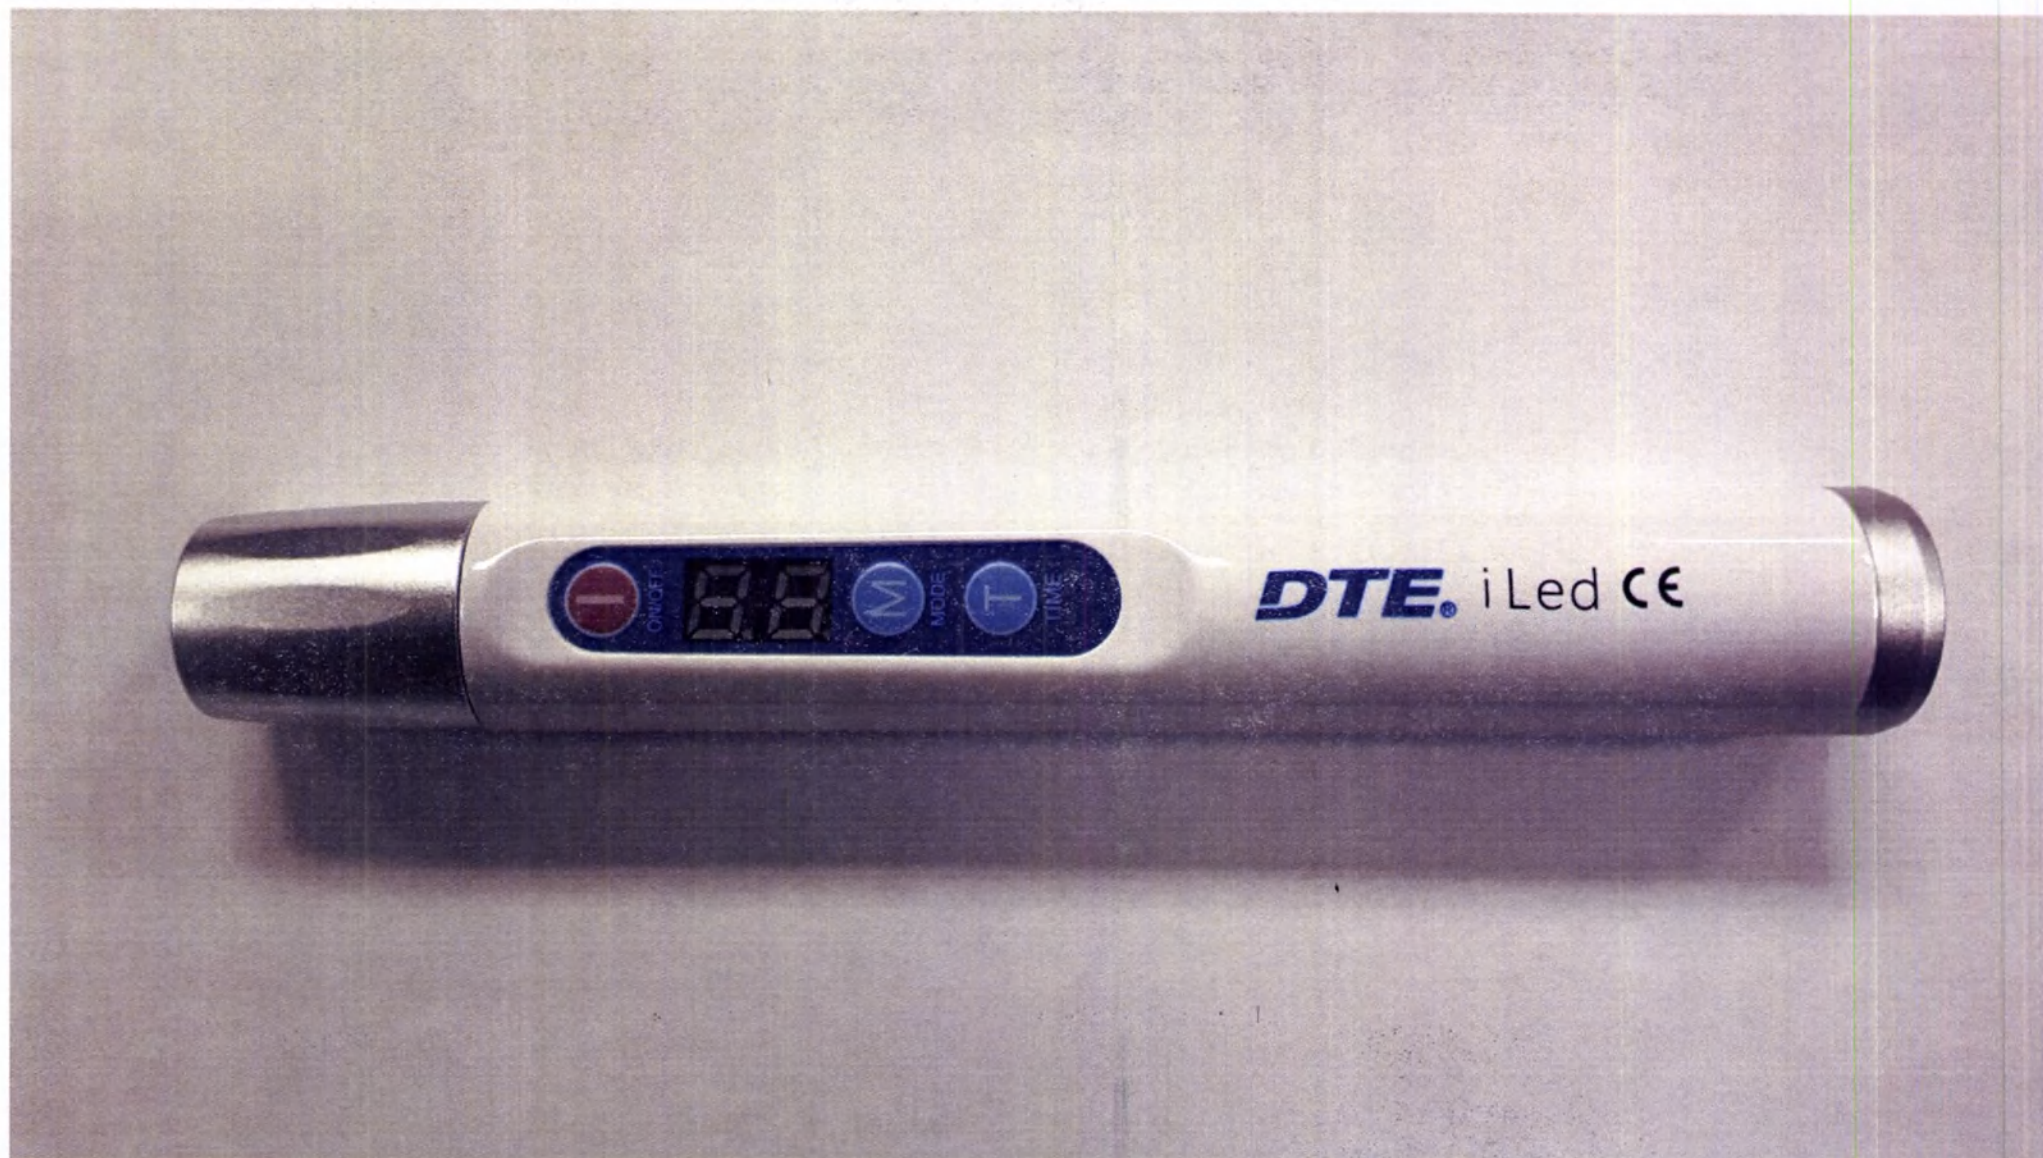


2. Наконечник оптоволоконный съемный.

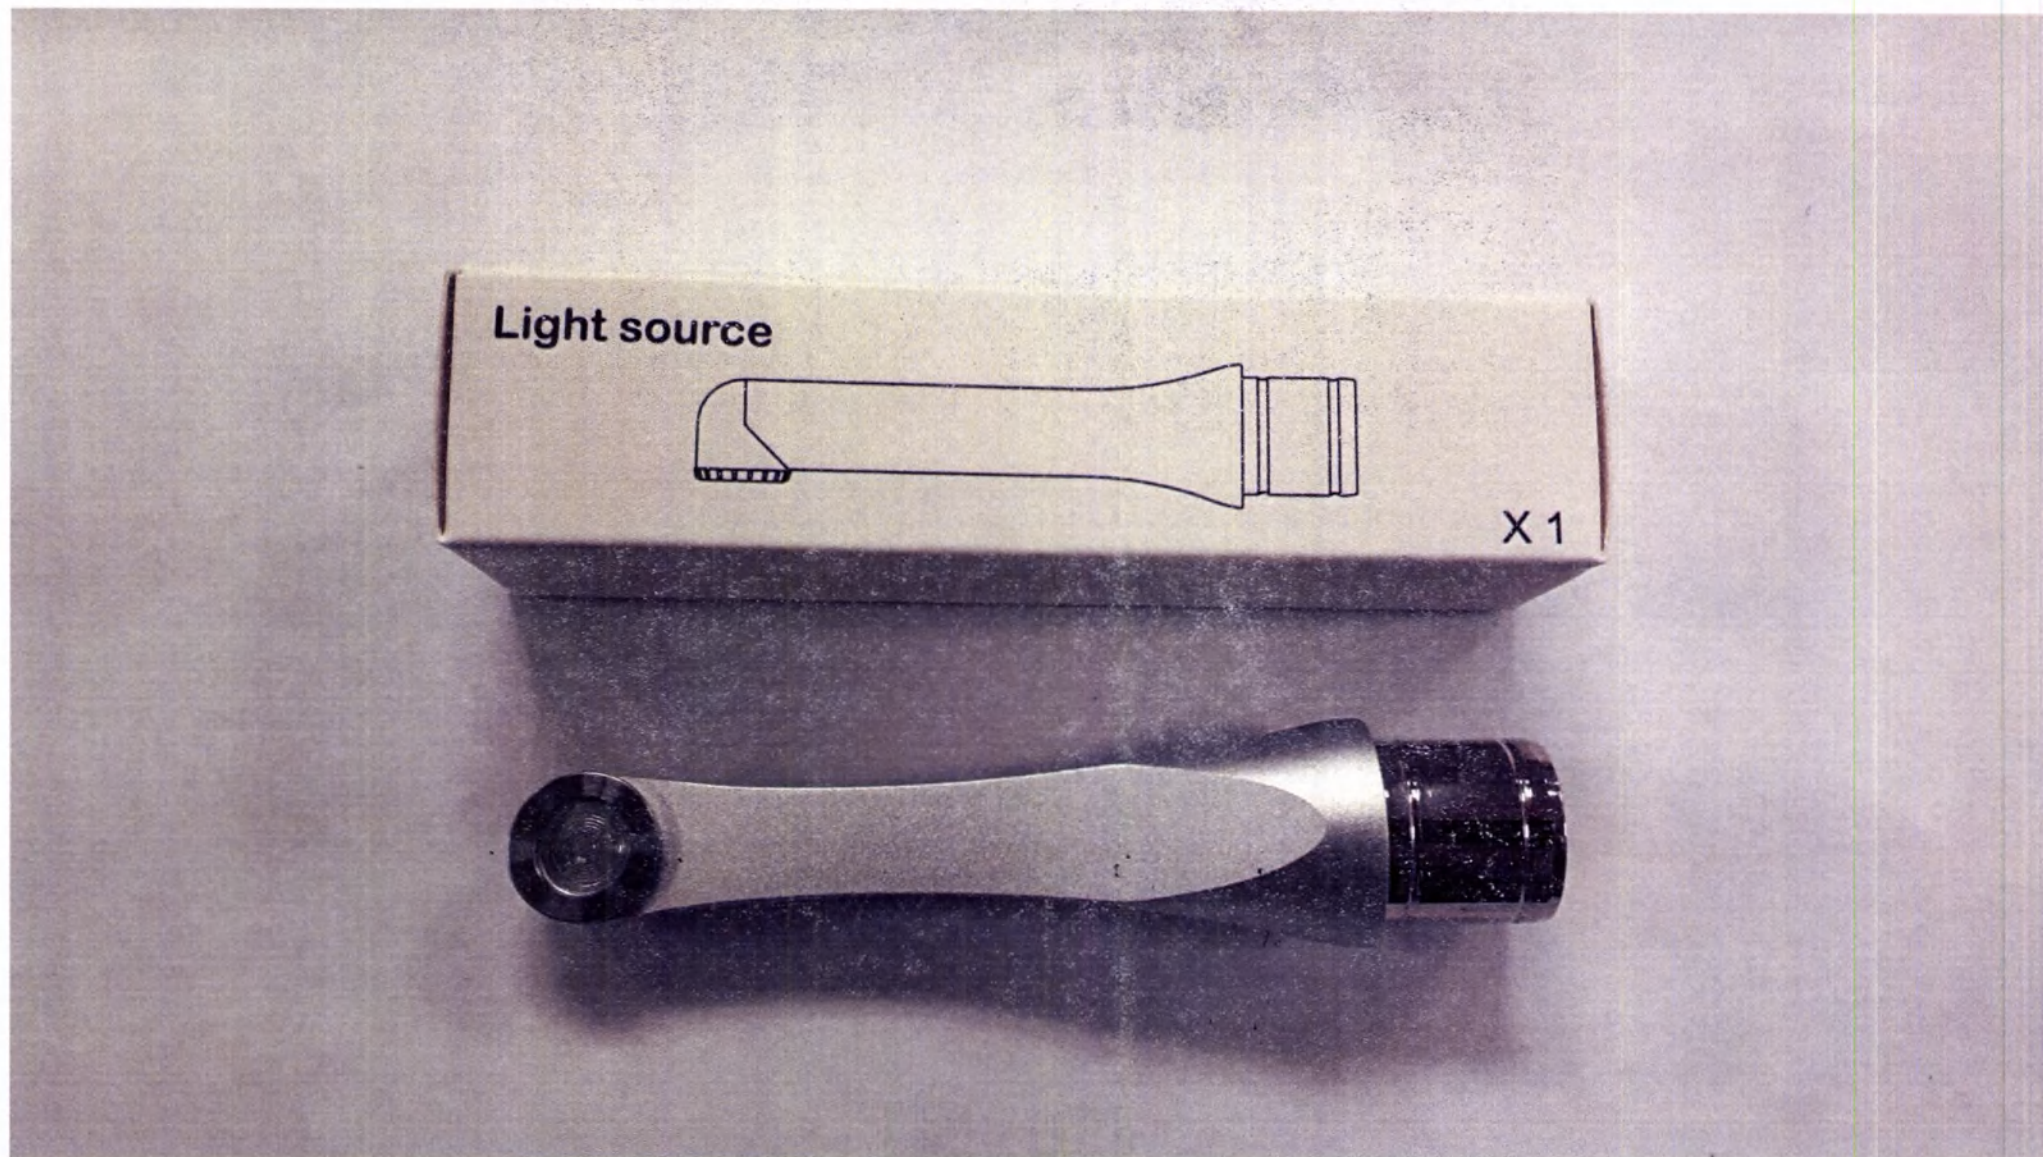


3. Световой фильтр.

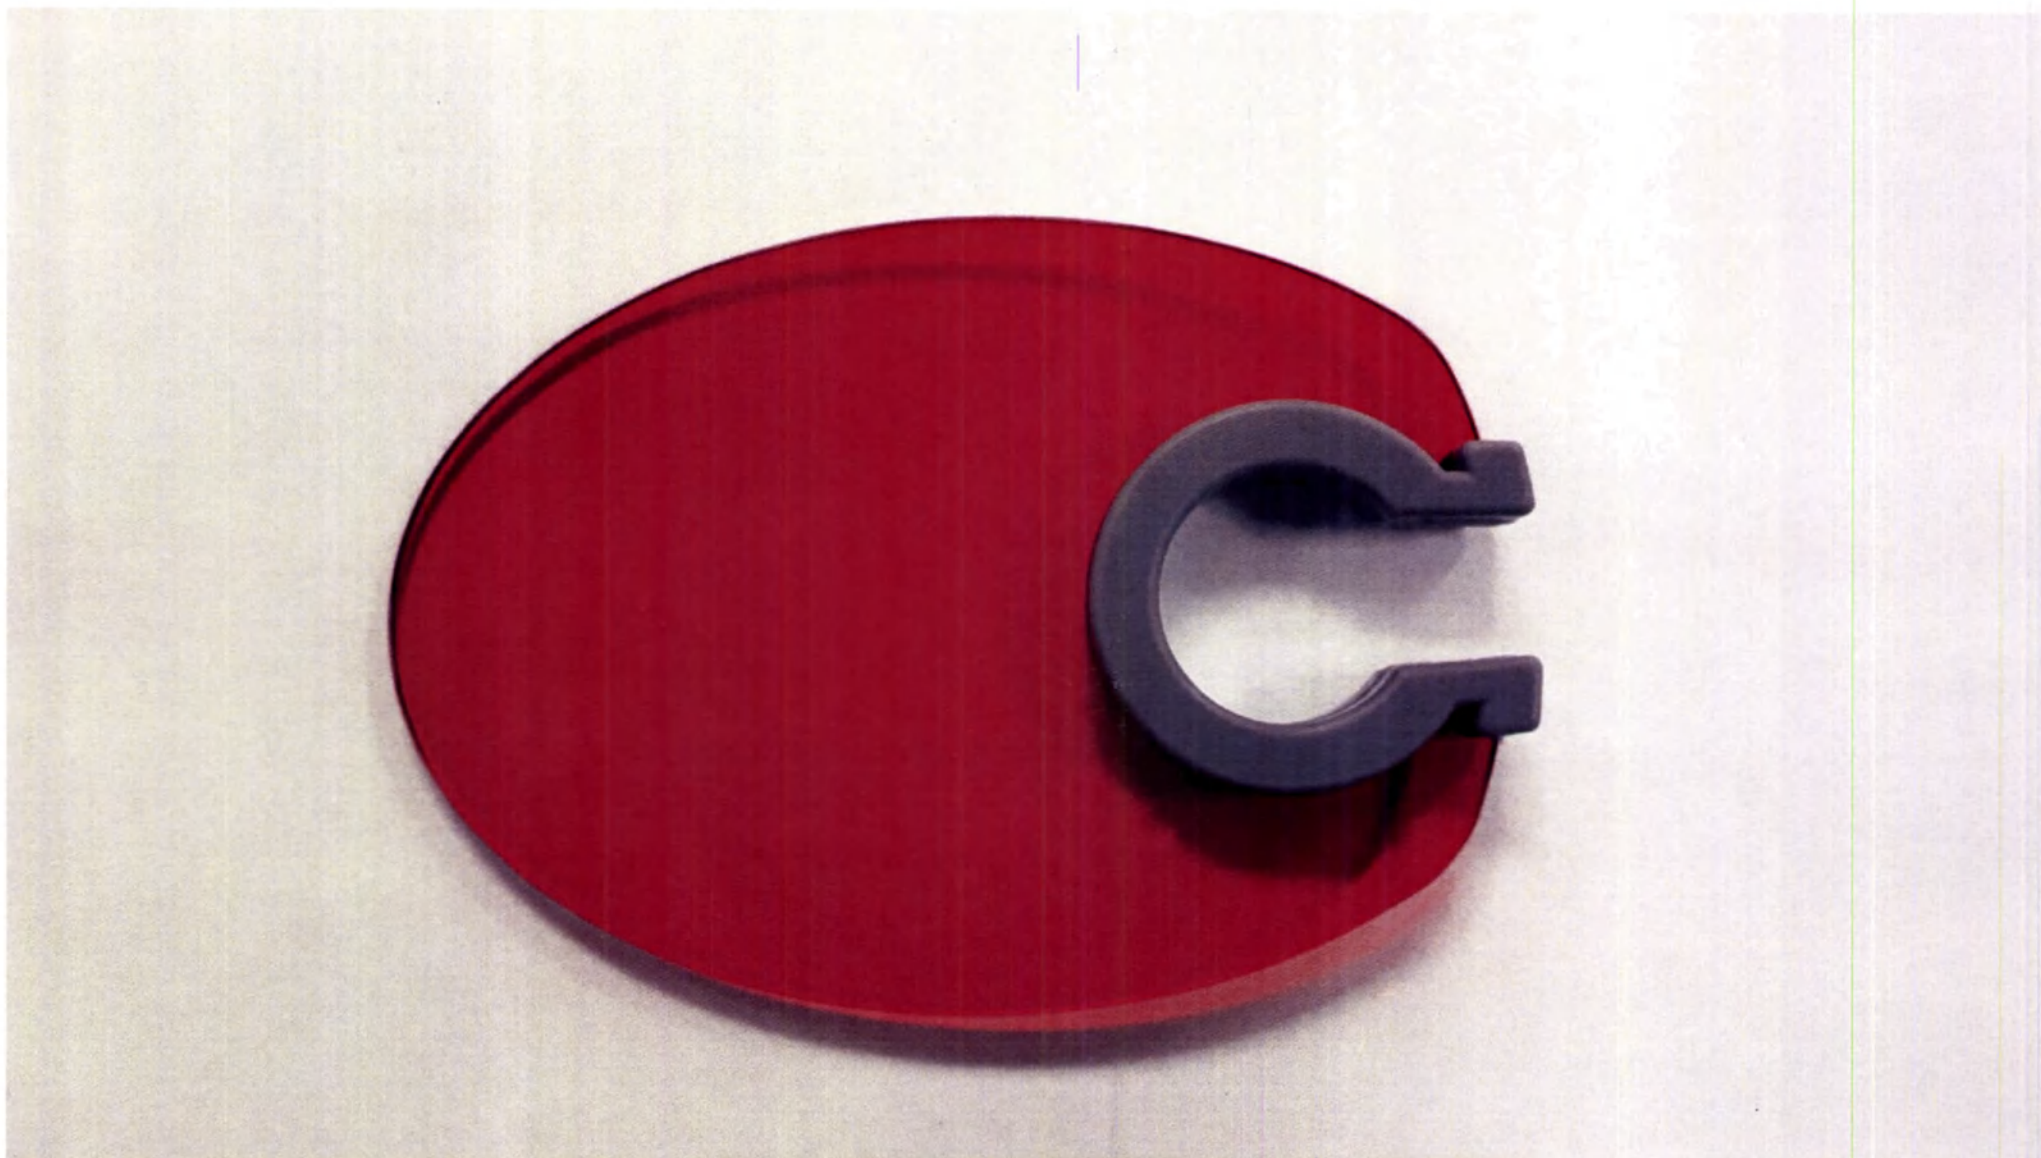


4. Зарядное устройство.

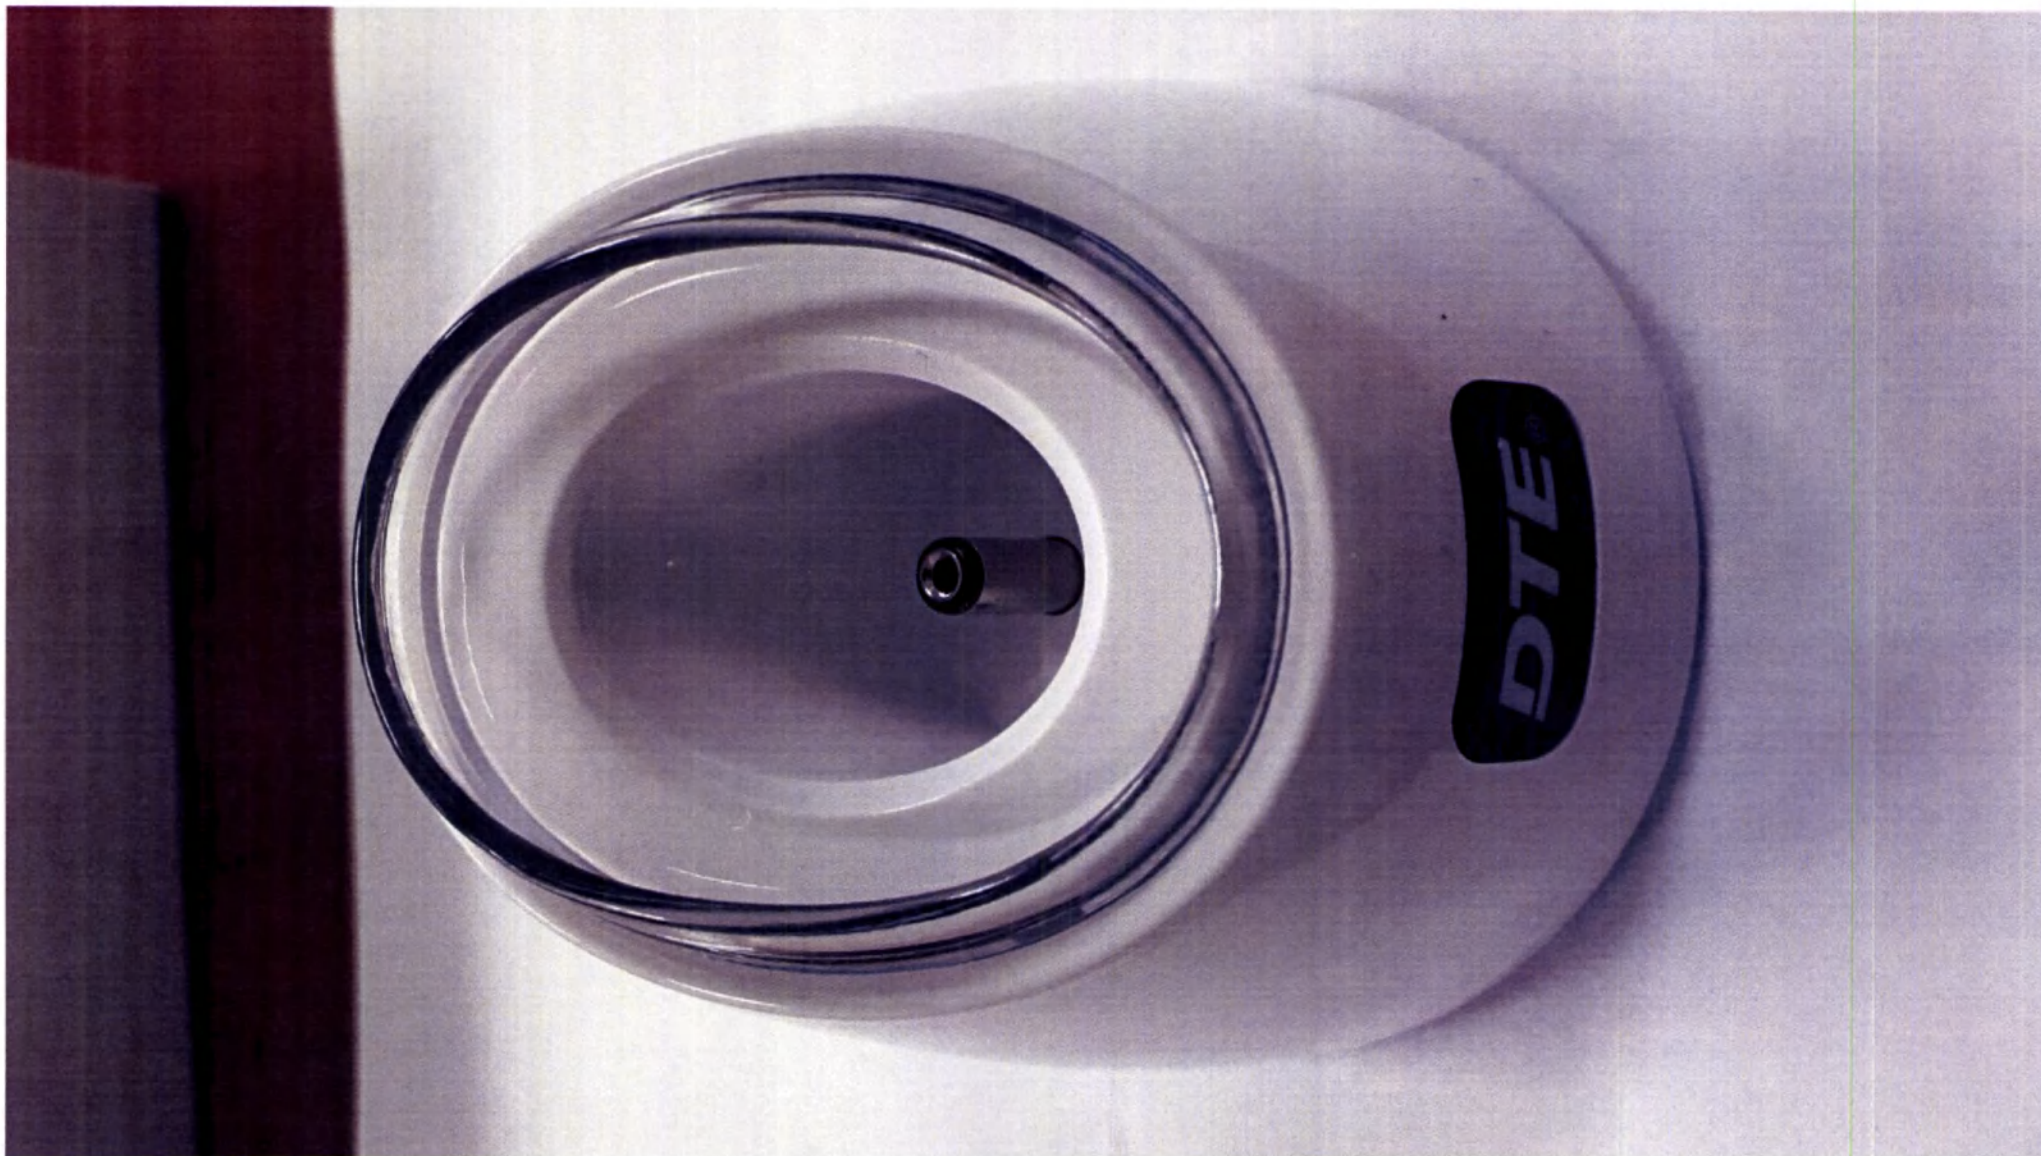


5. Адаптер.

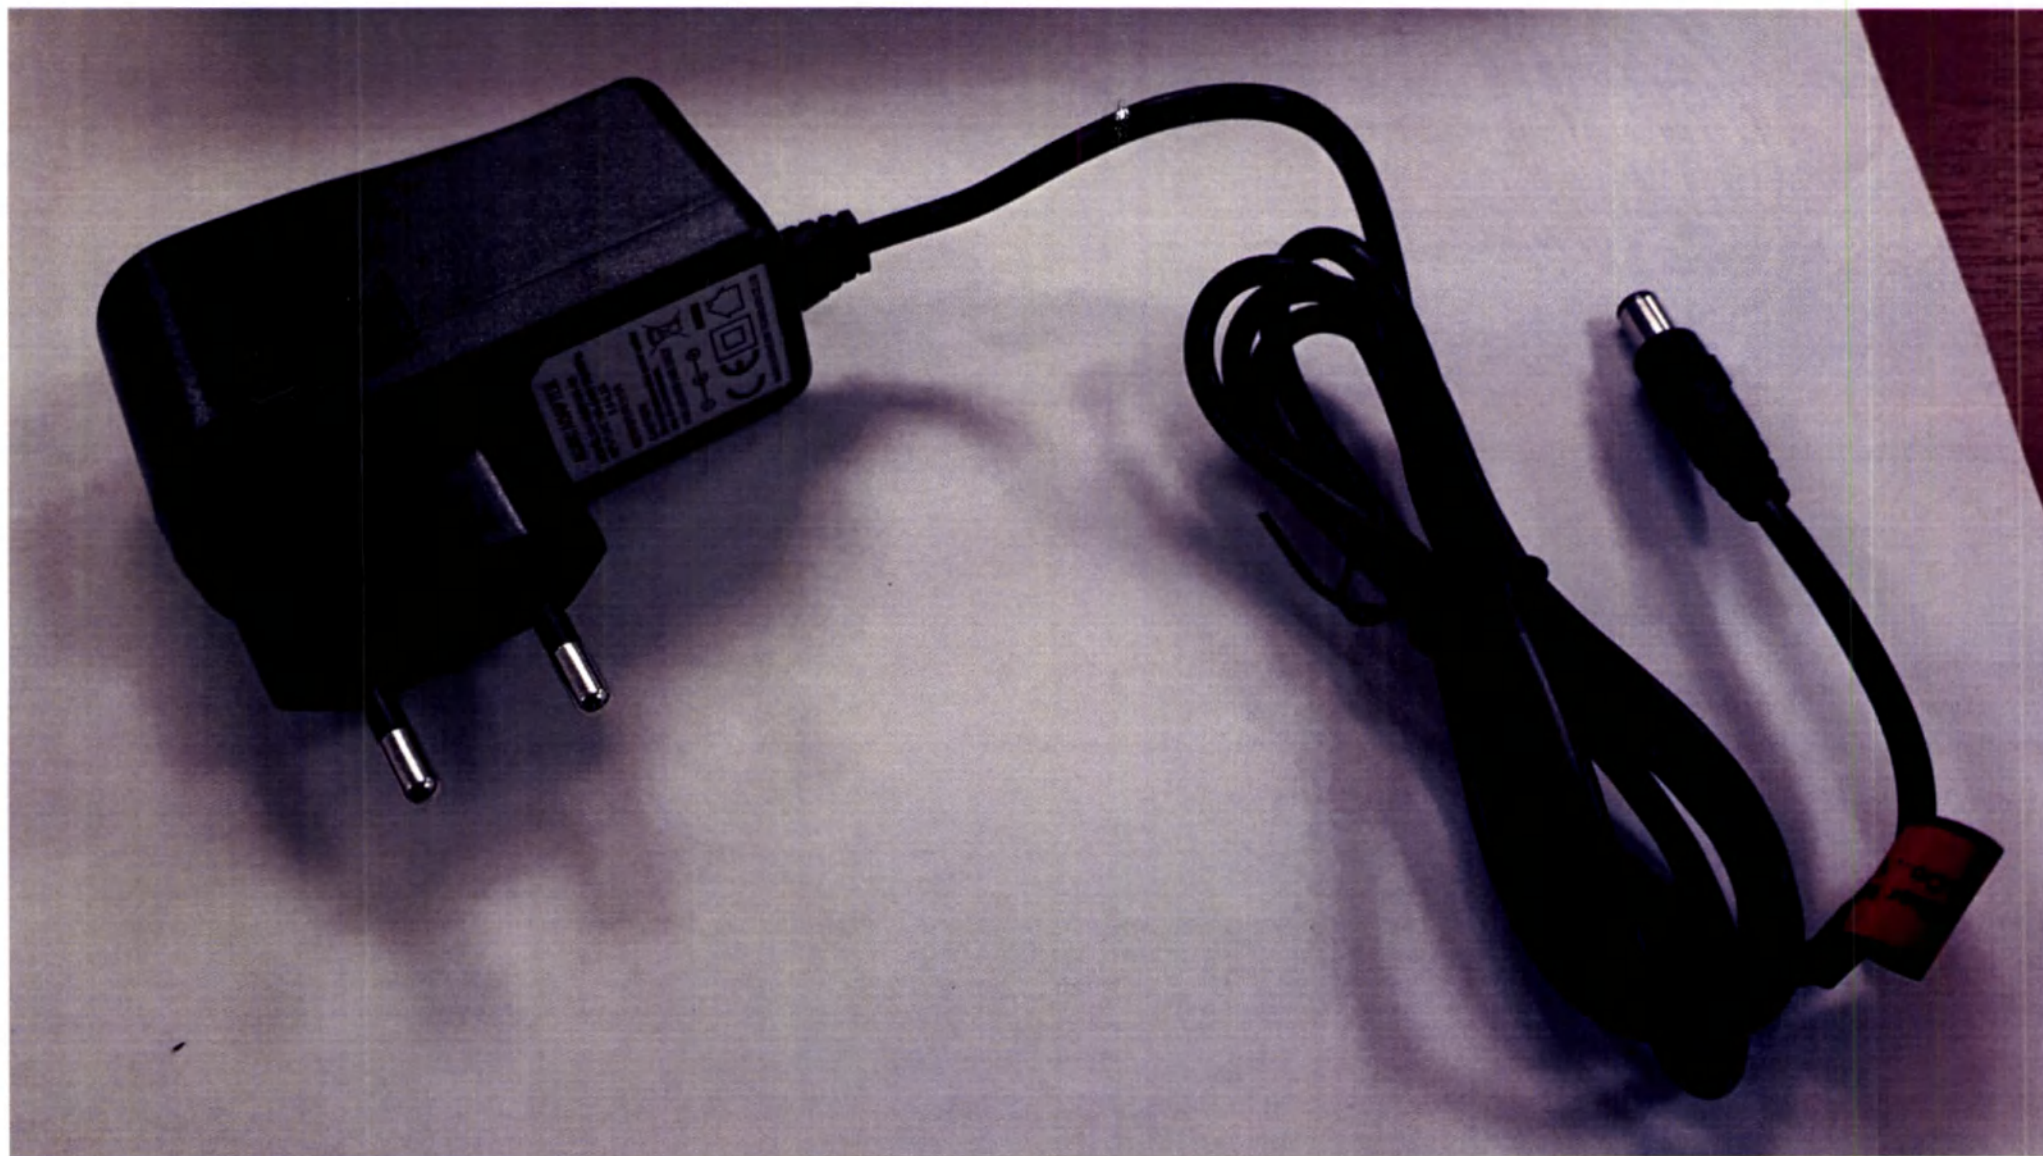

6. Батиметр.

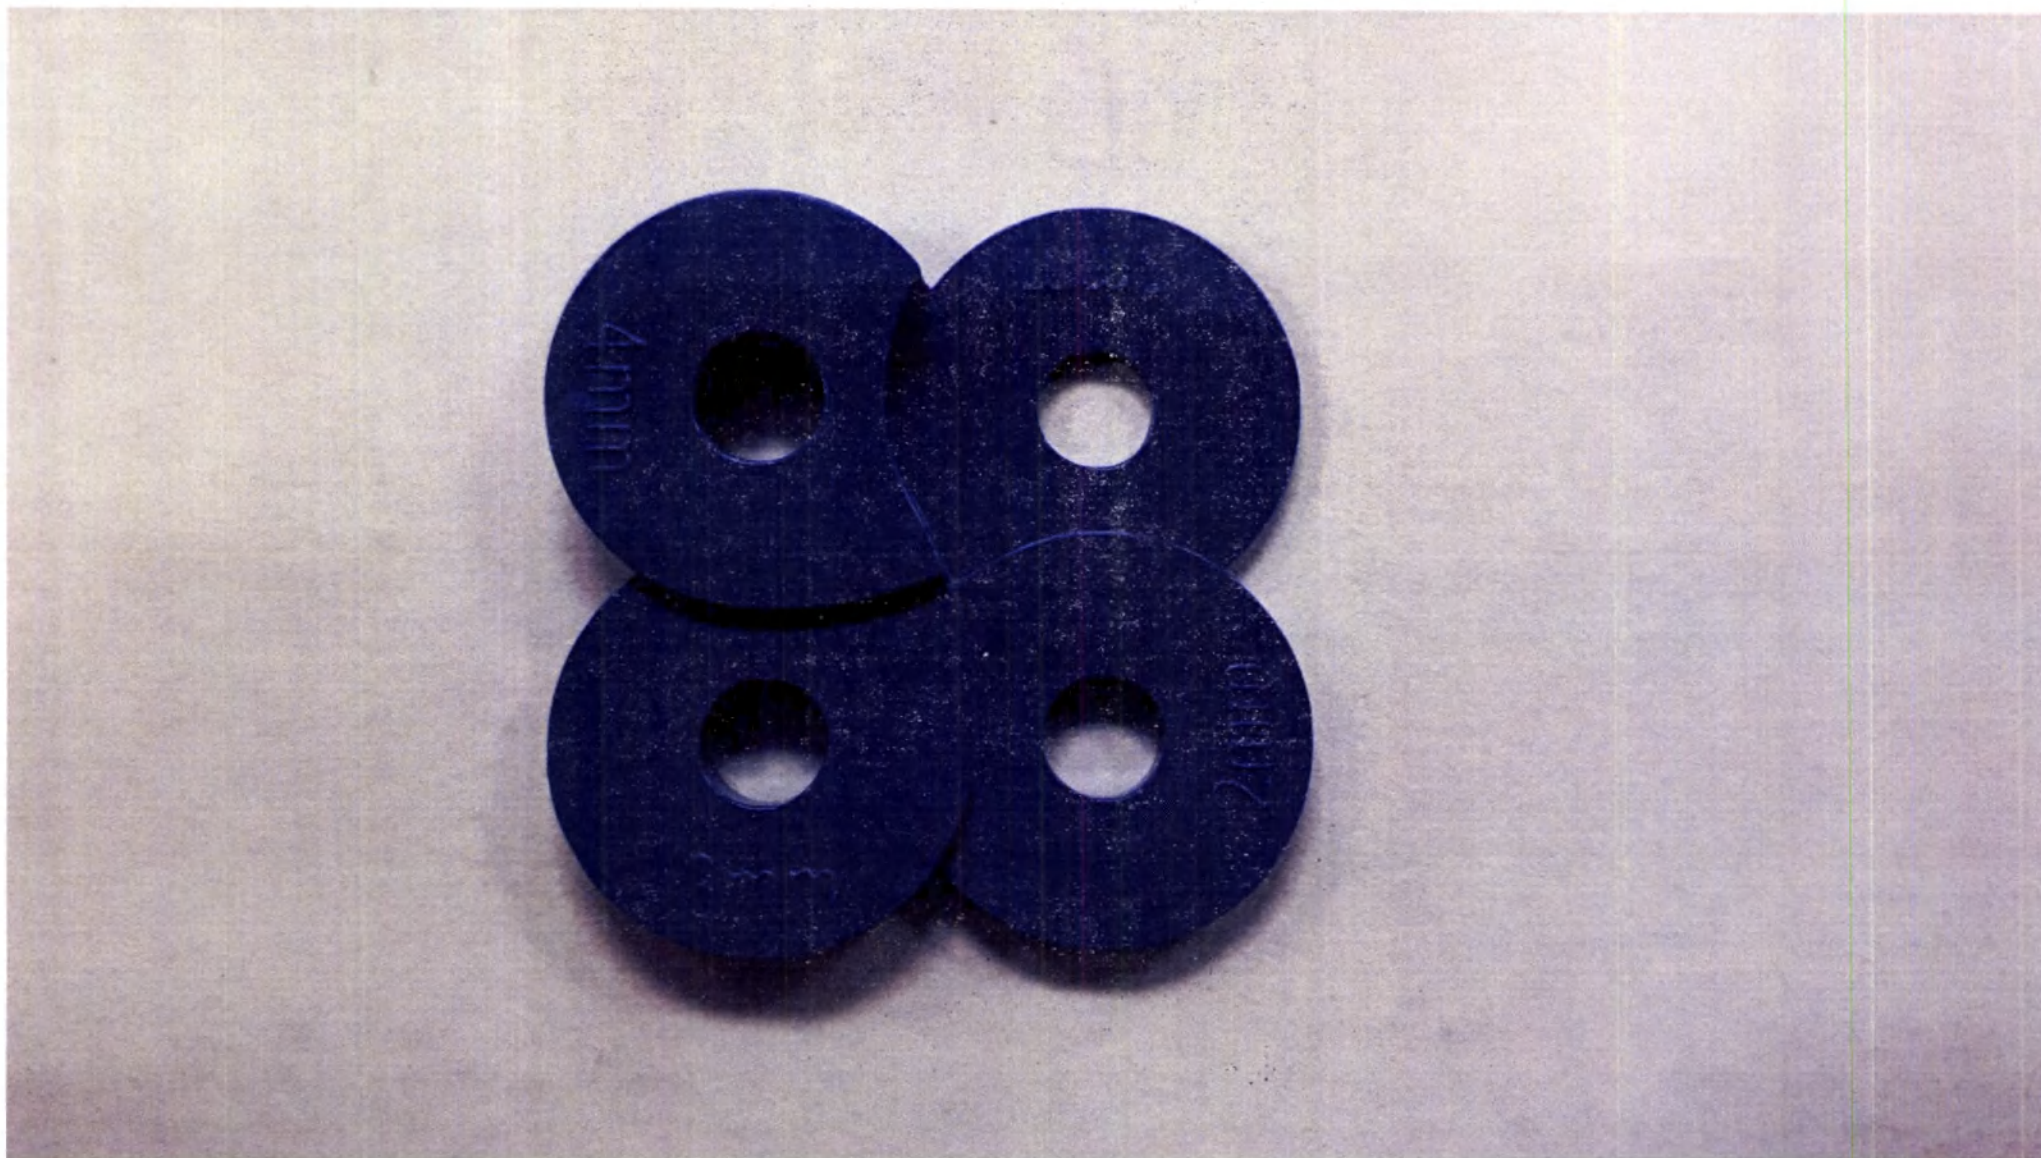

7. Насадка на основной блок сменная одноразовая – 100 шт.

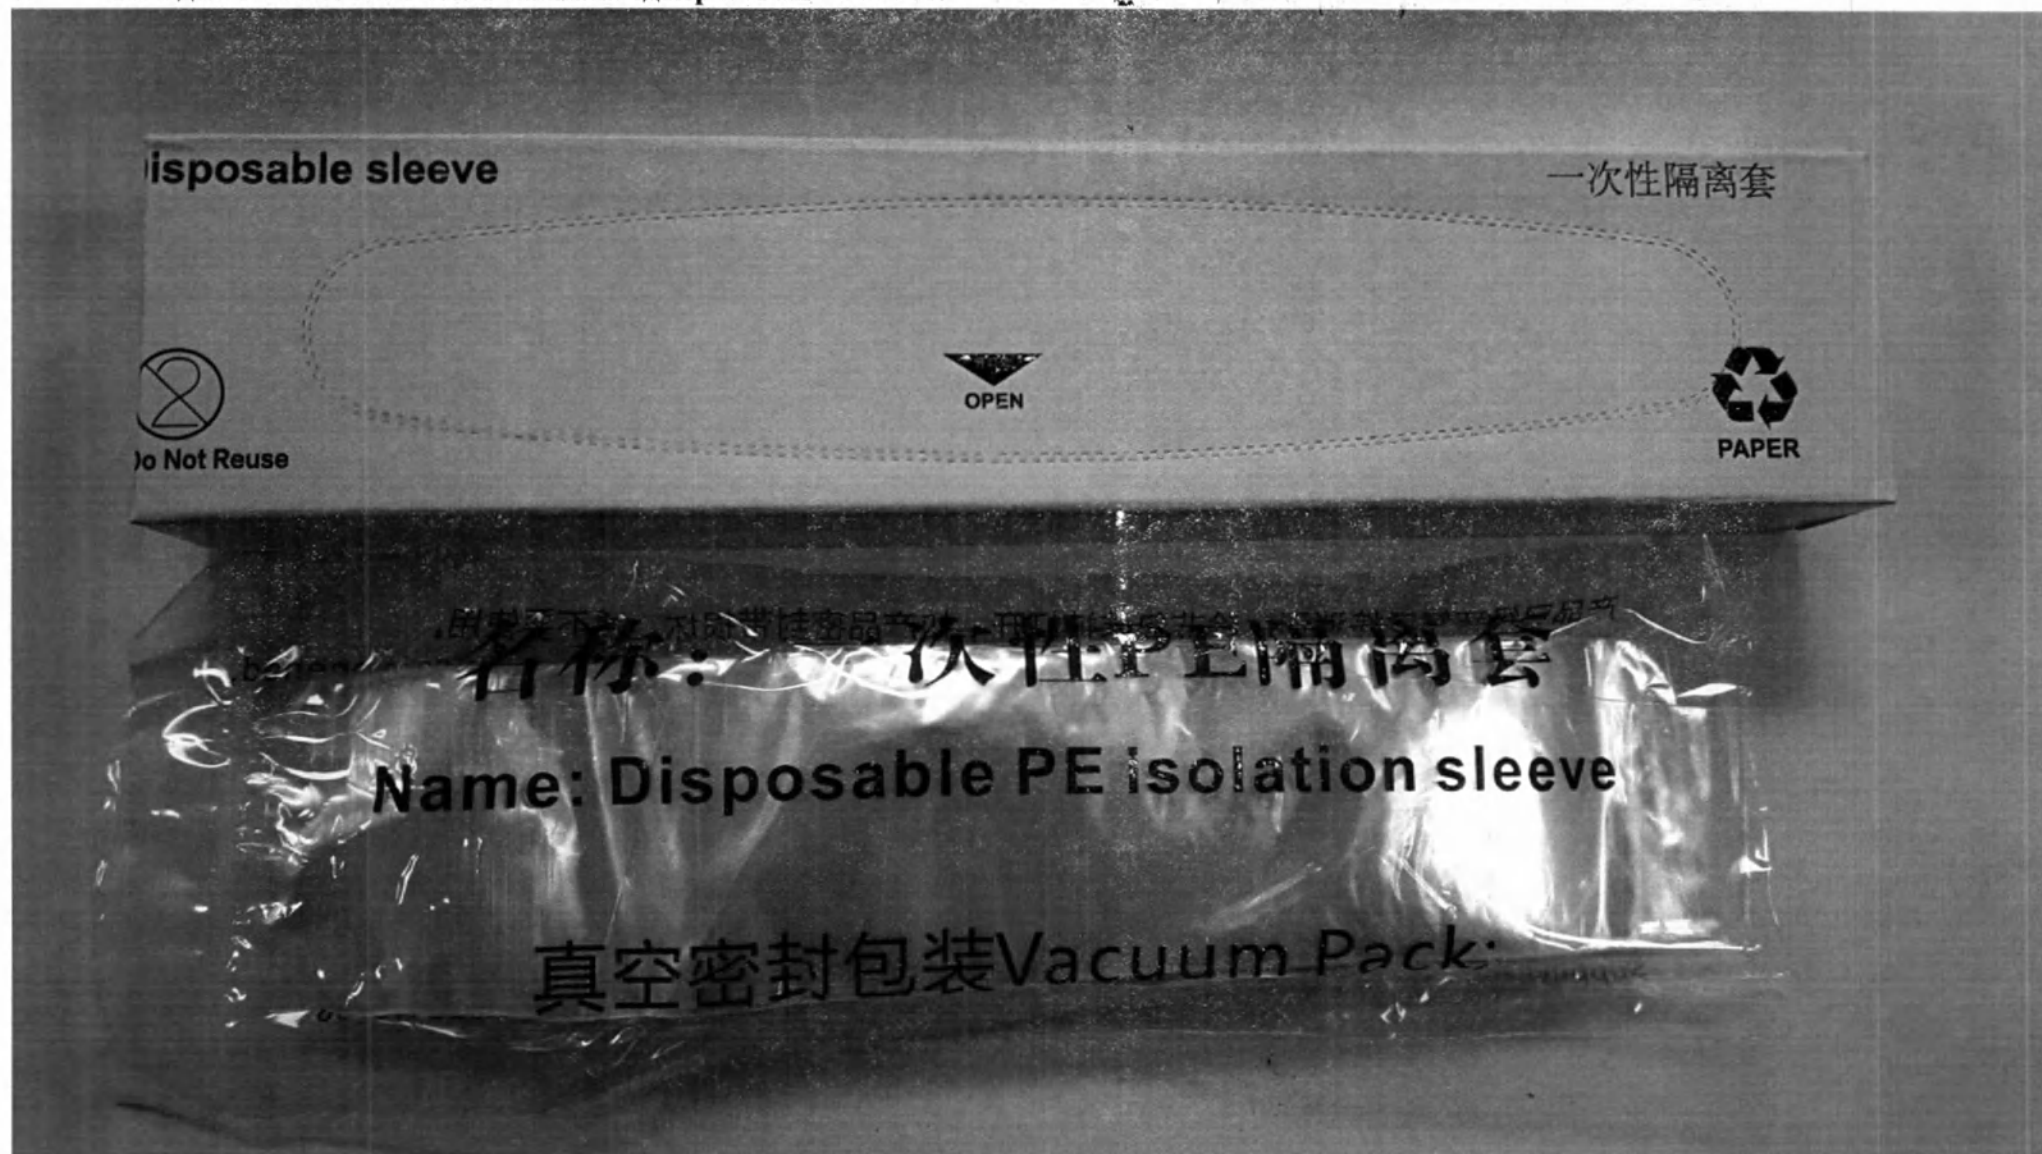


Насадка на основной блок сменная одноразовая – 100 шт.



IV. Лампа полимеризационная, модель LED.H

Упаковка

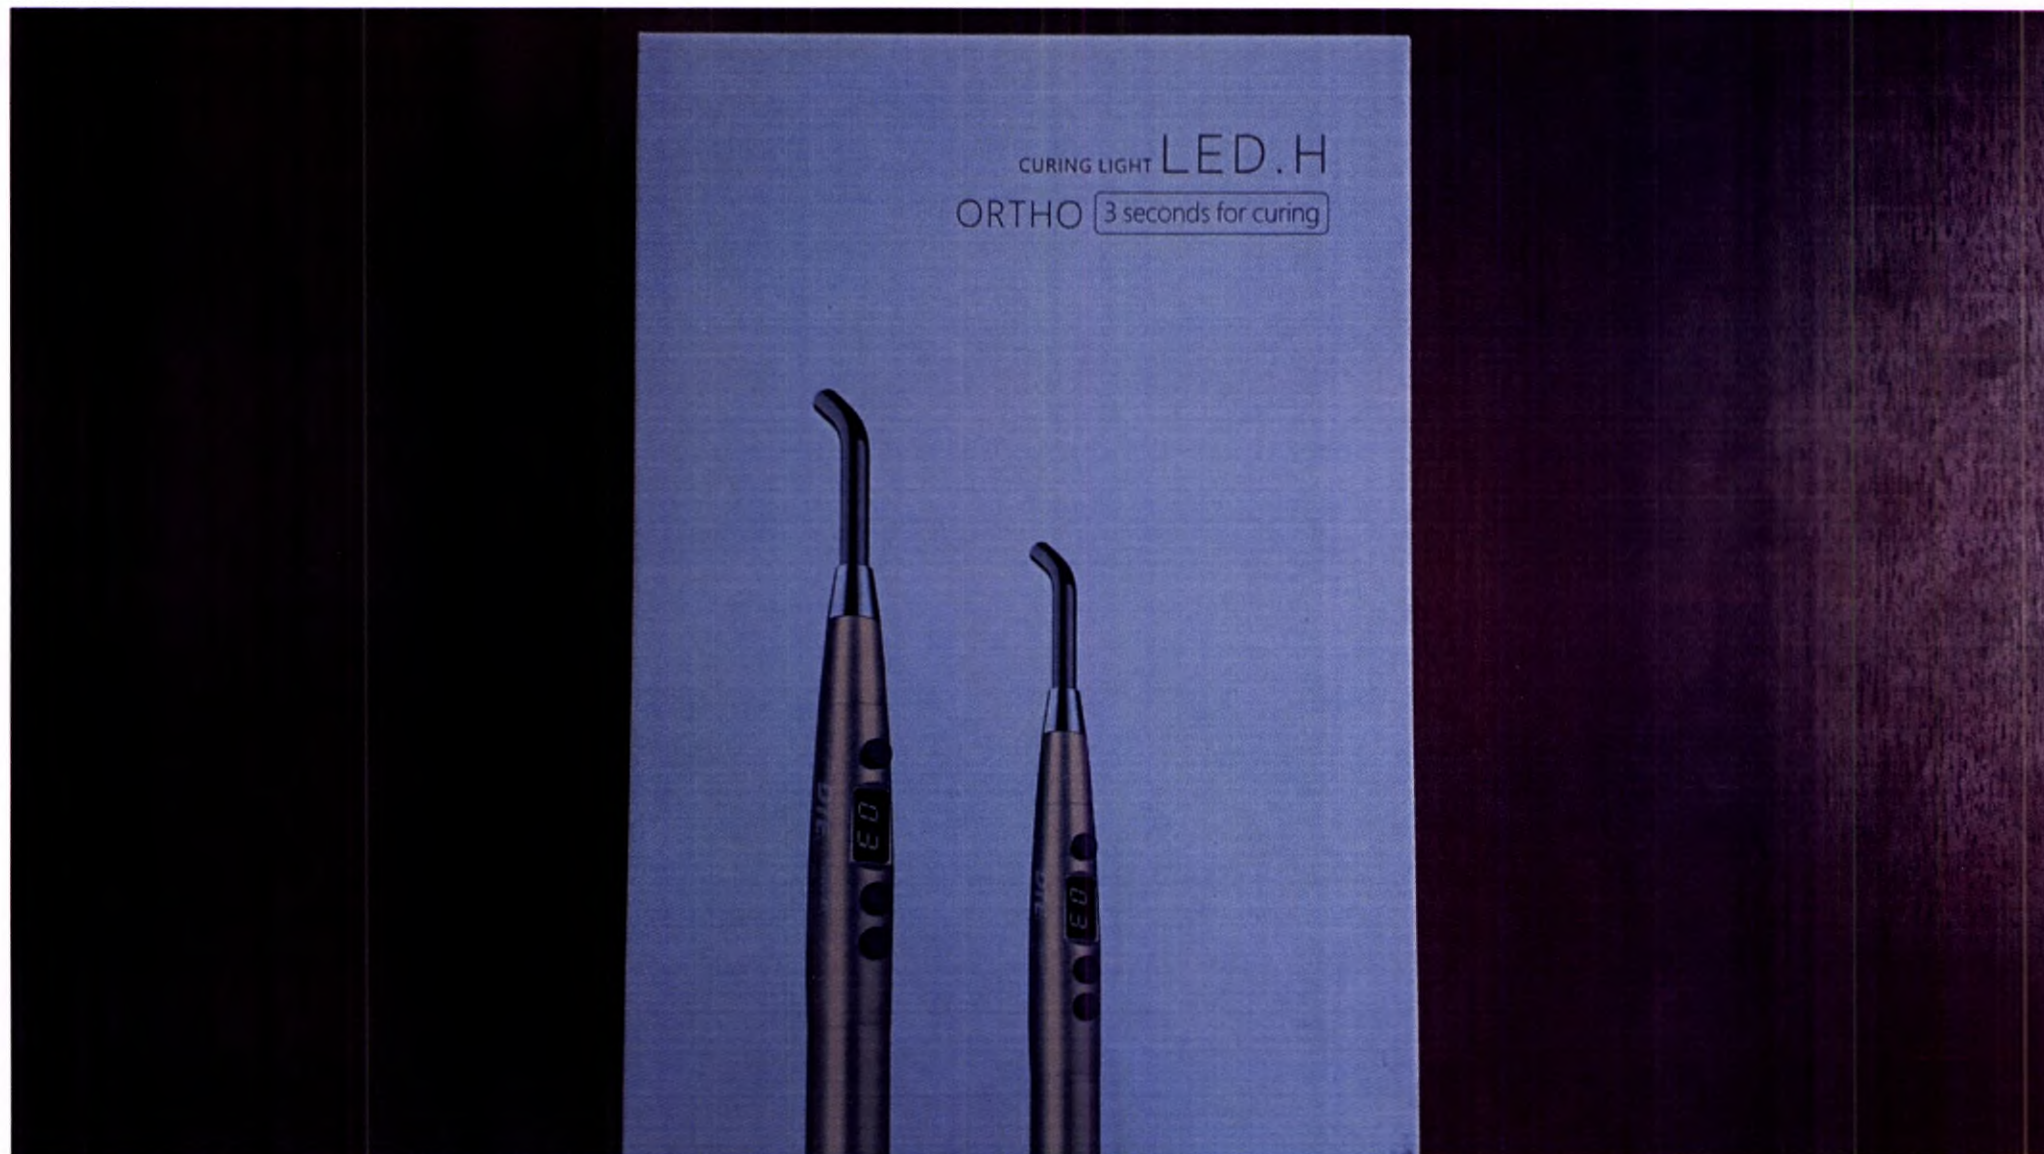


Вид в упаковке




1. Основной блок из светодиодов.



2. Наконечник оптоволоконный съемный (2 шт.).

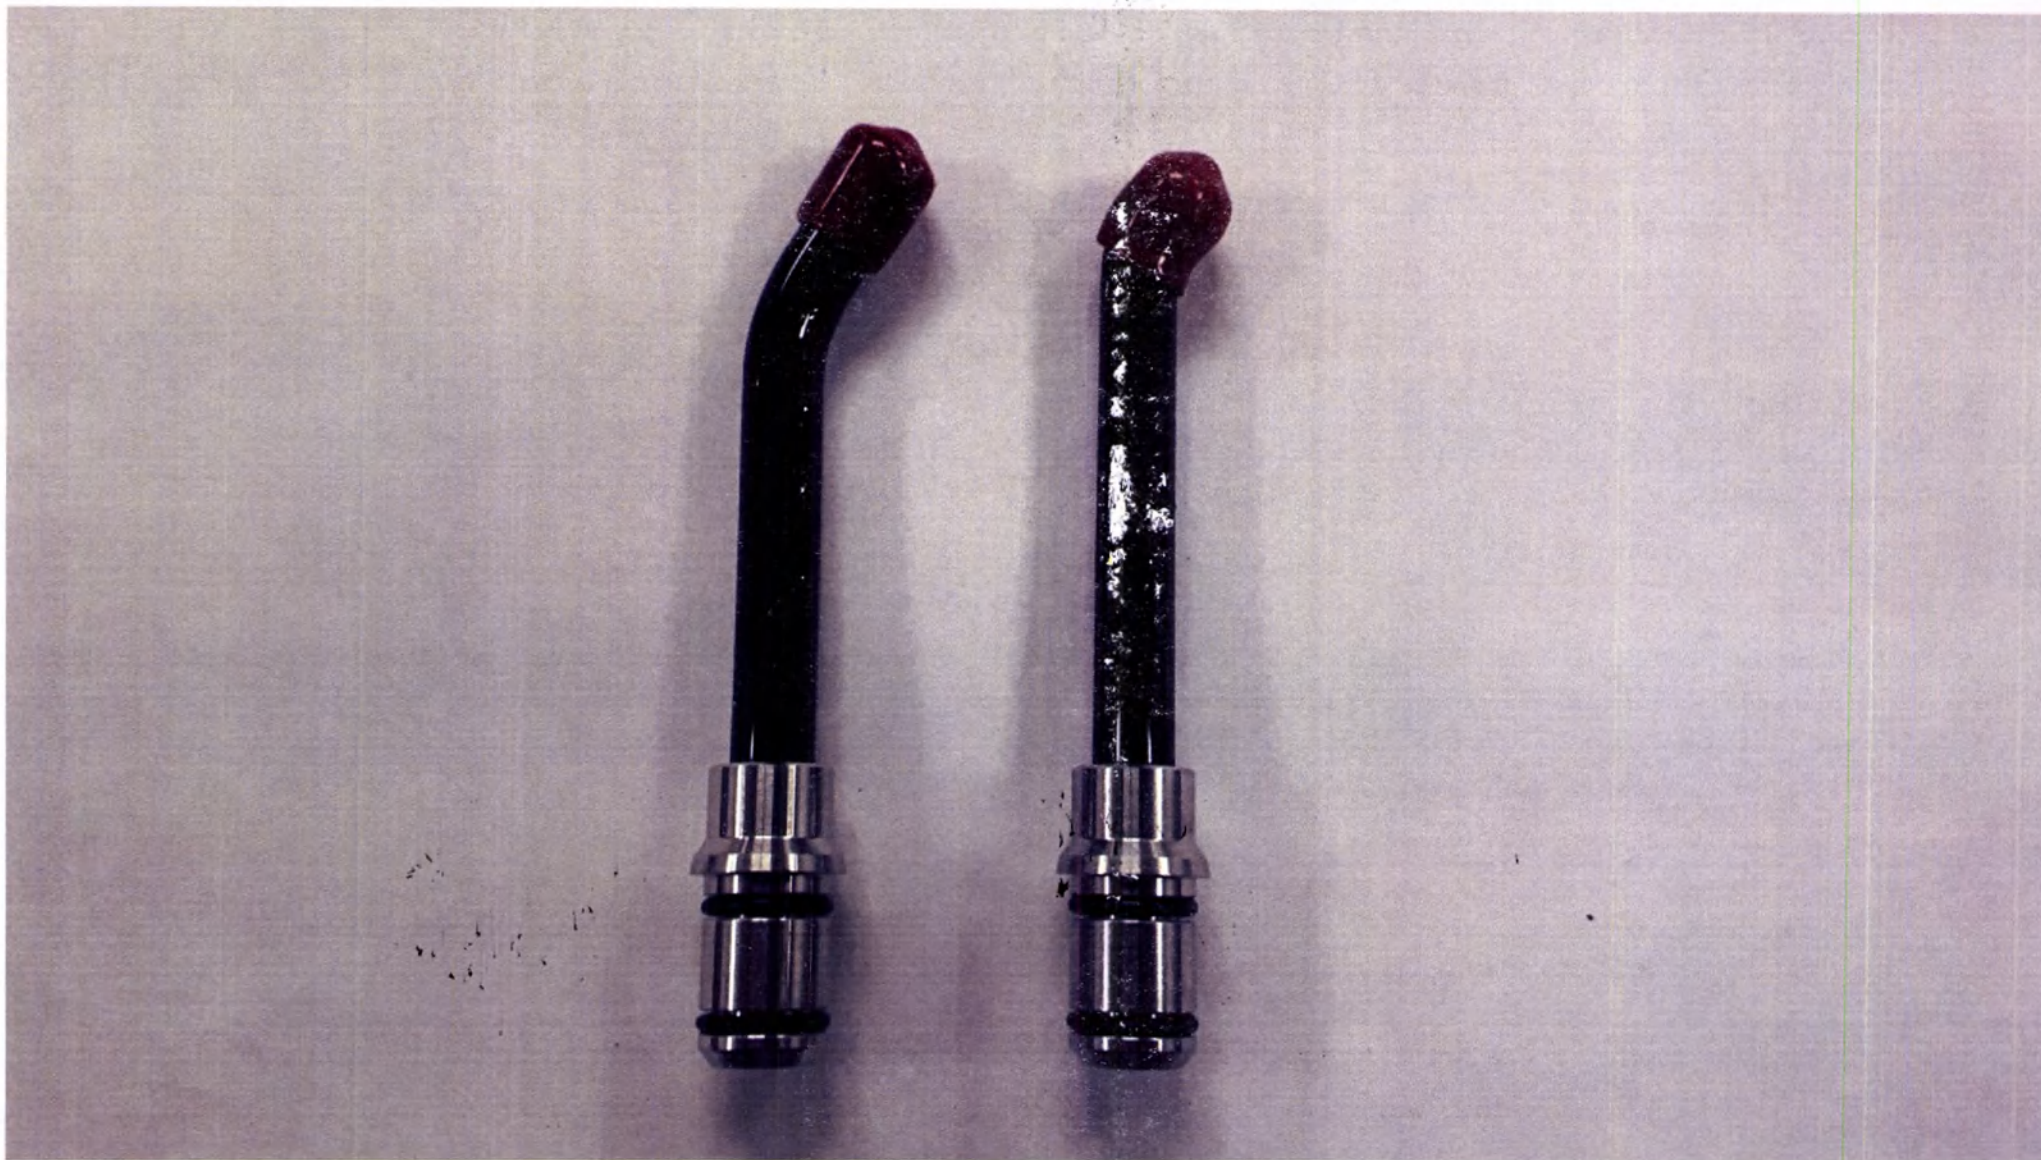


3. Световой фильтр.

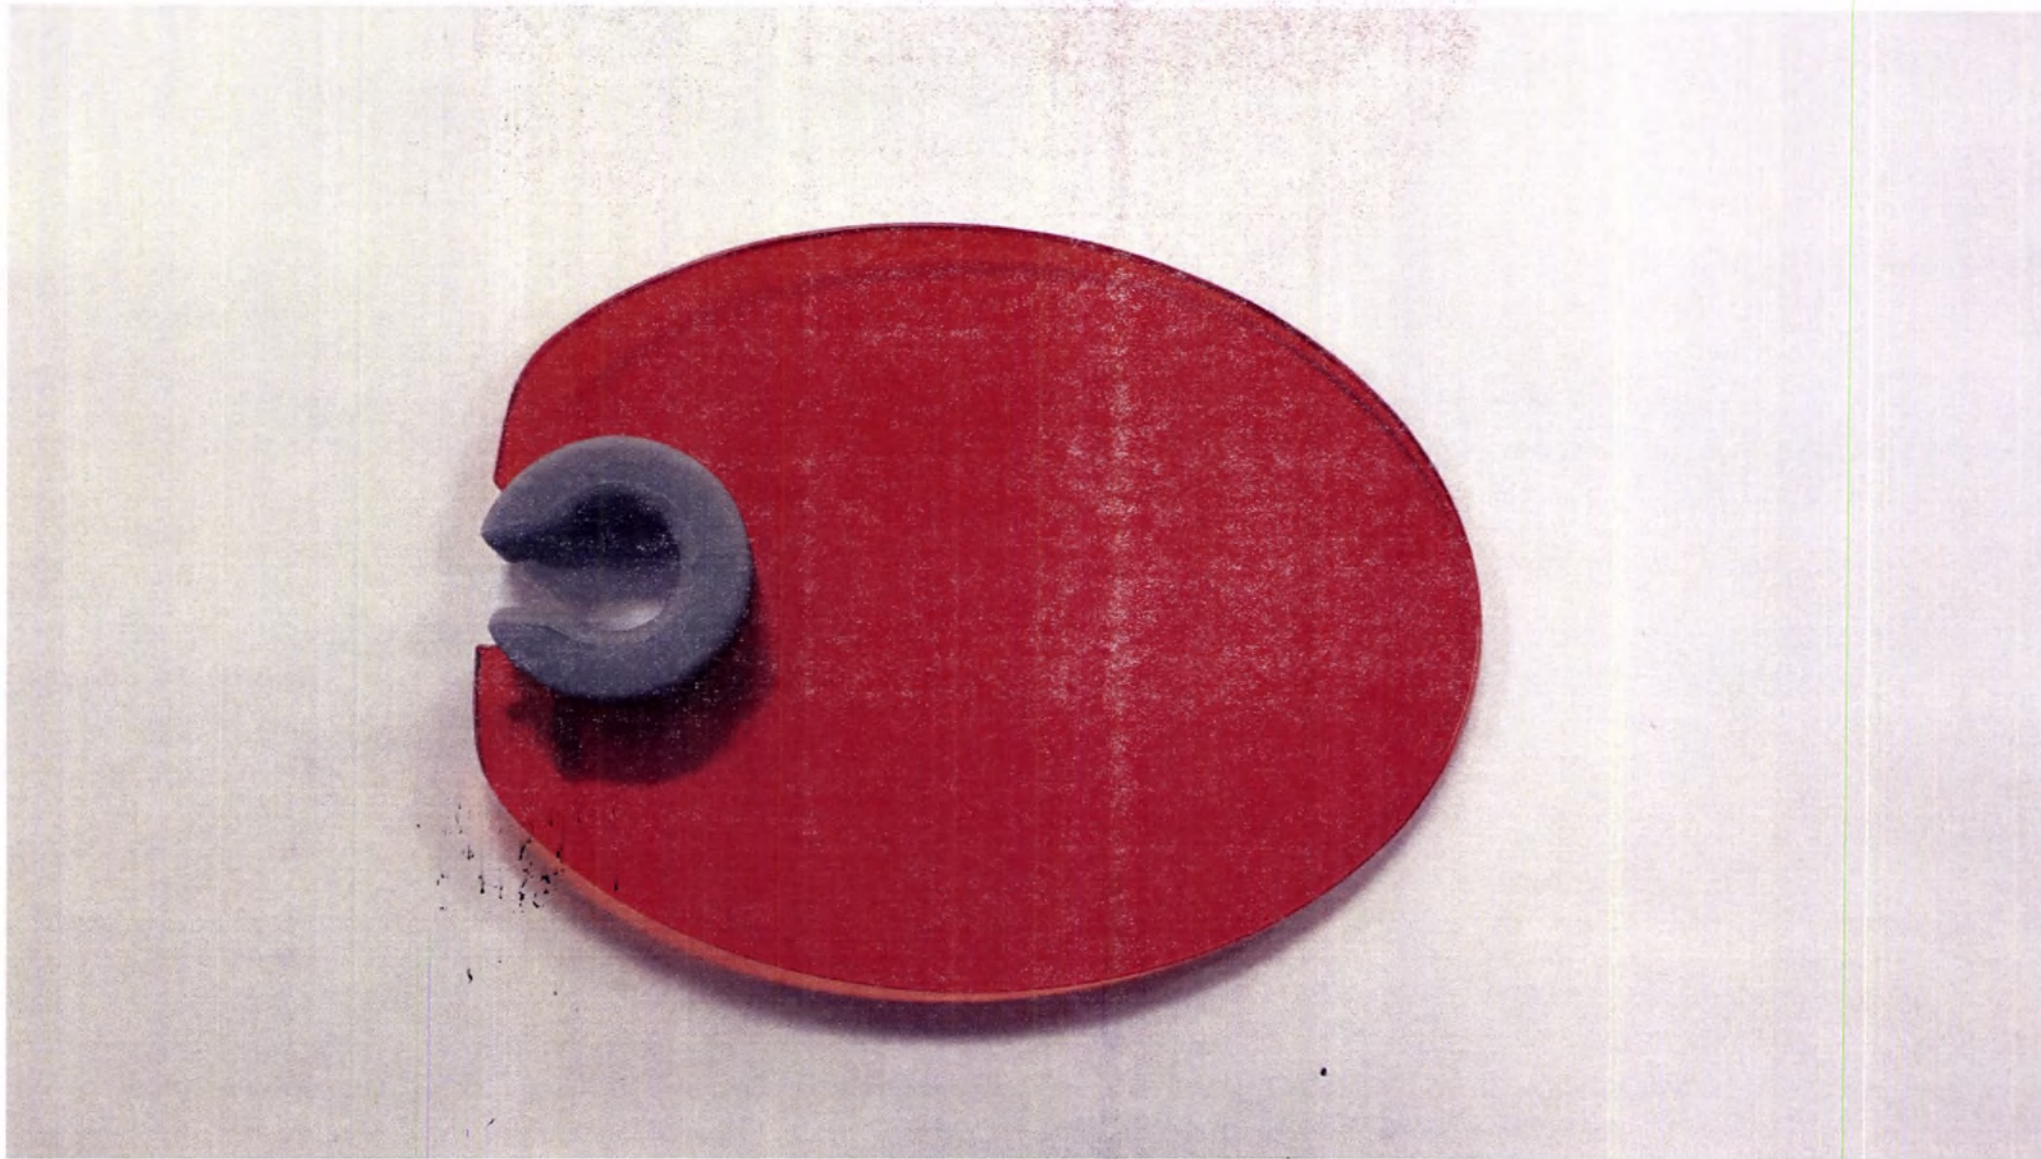


4. Зарядное устройство.



5. Адаптер.

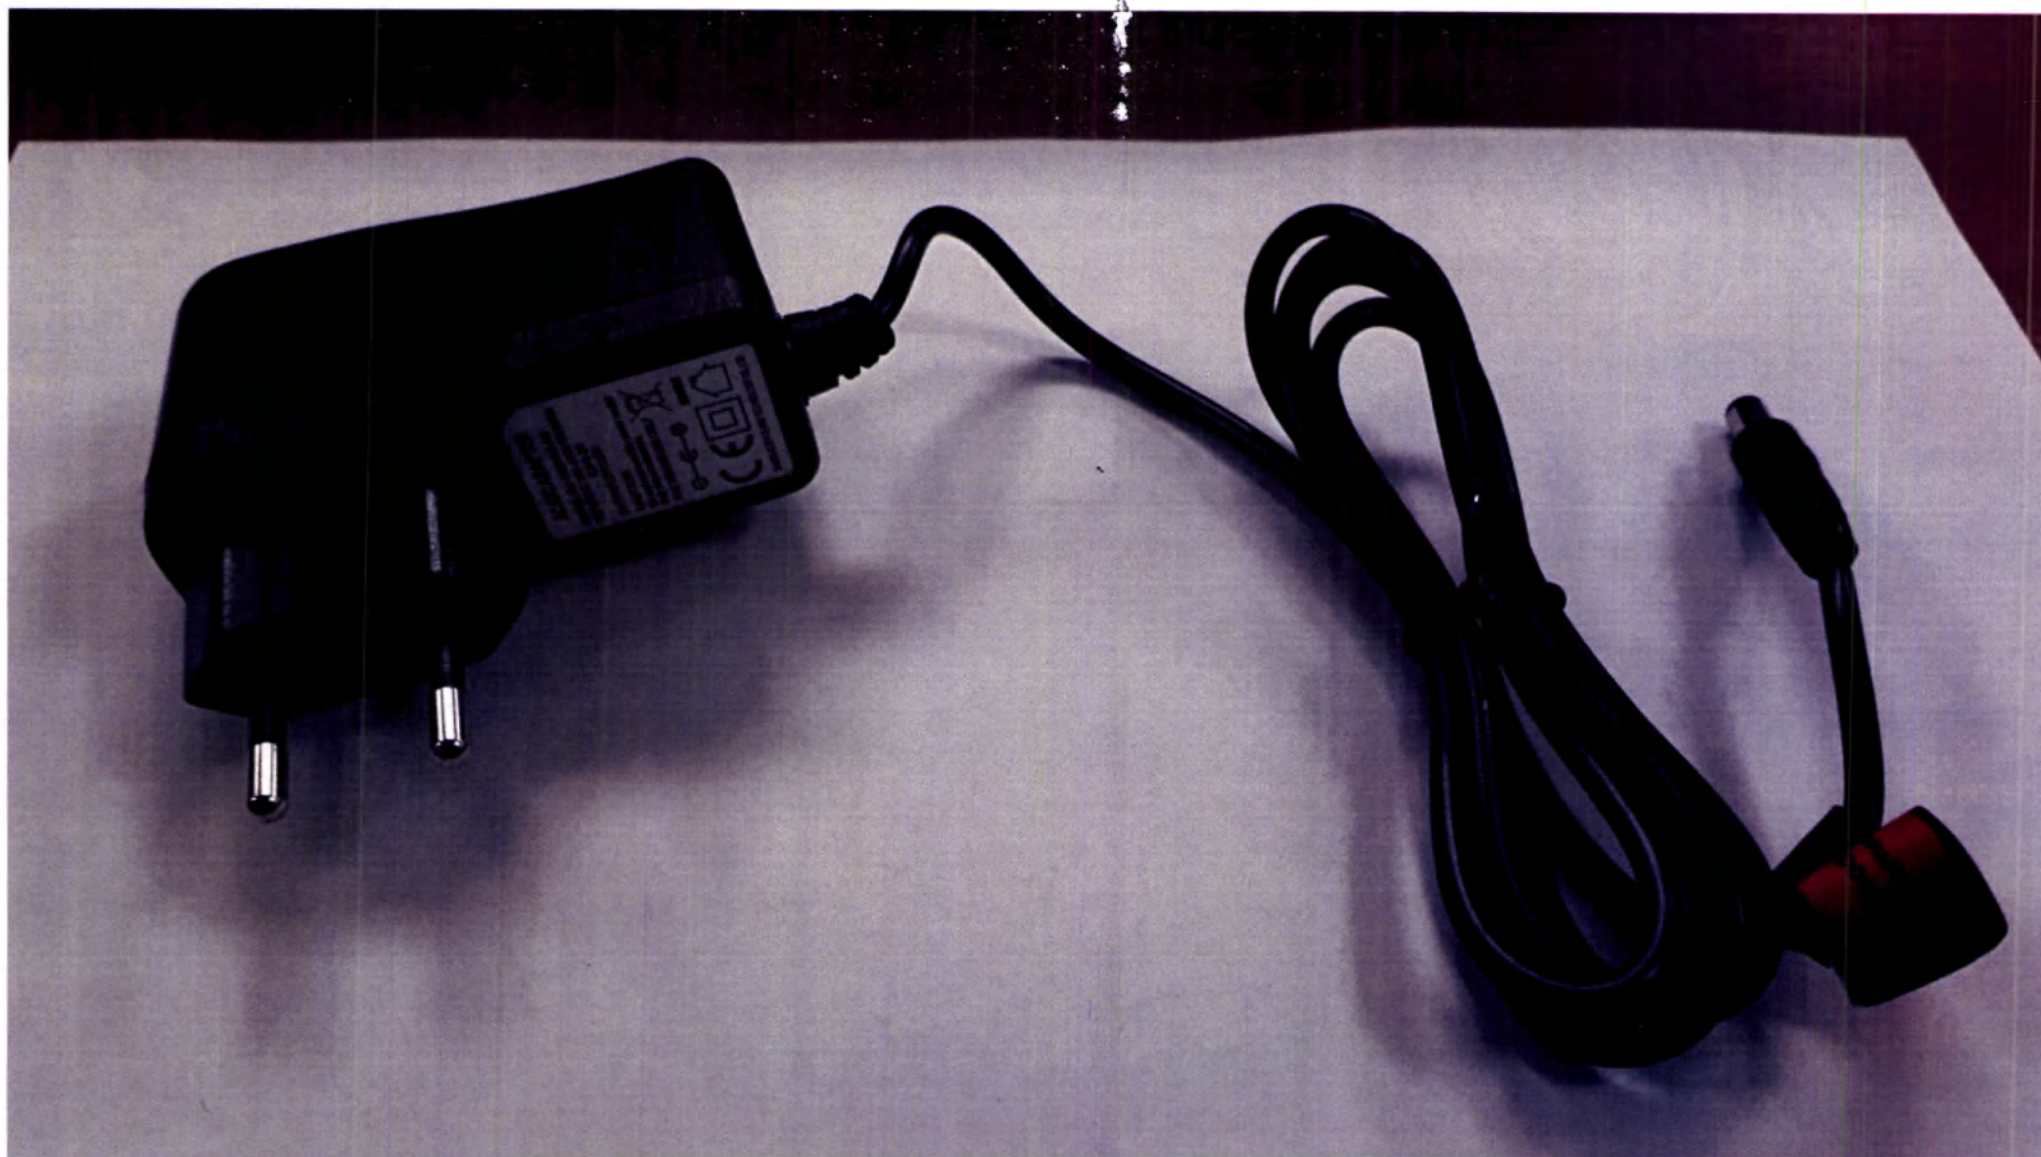


6. Батиметр.

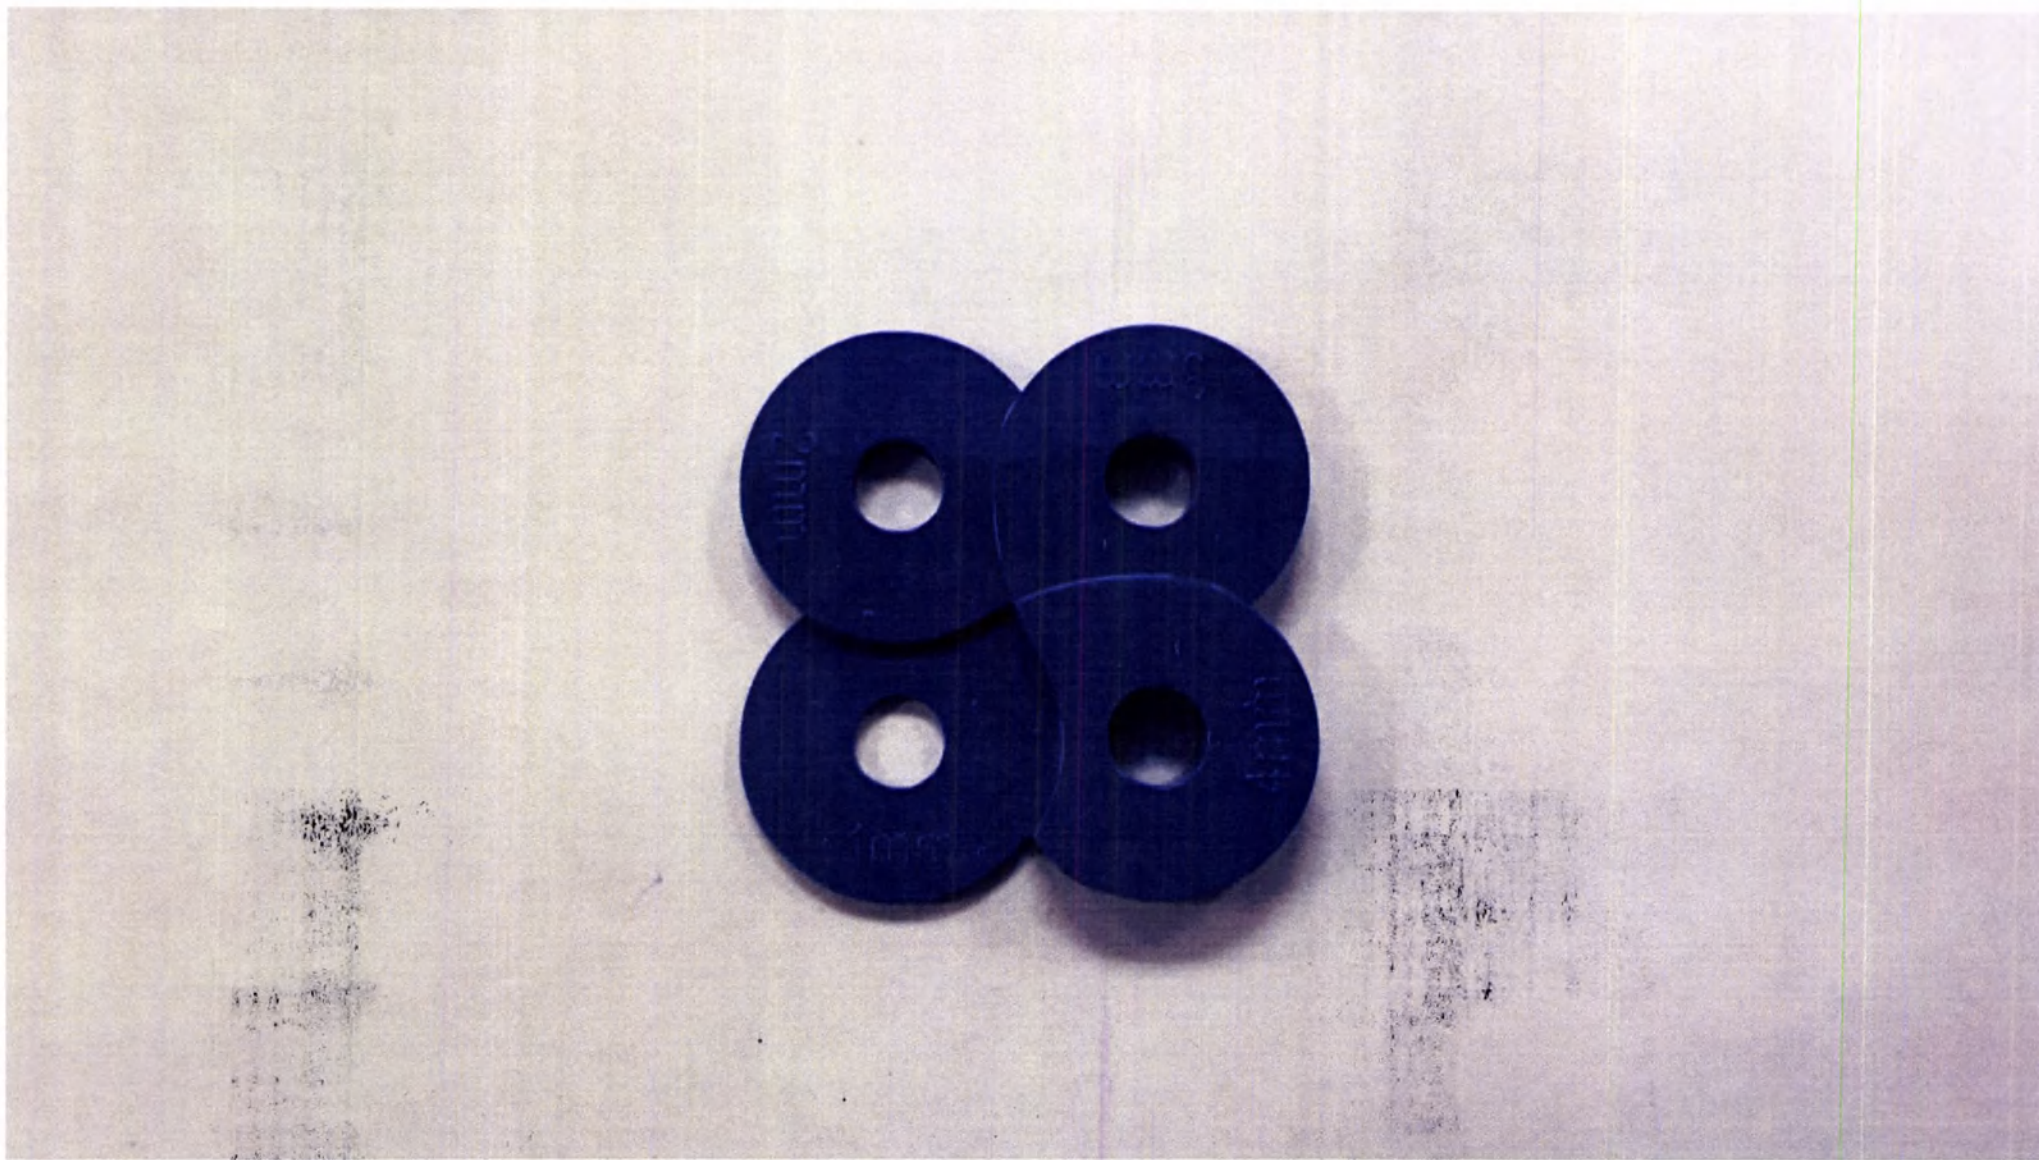

7. Фотометр-яркомер.



В настоящем документе прошито
и скреплено оттиском печати

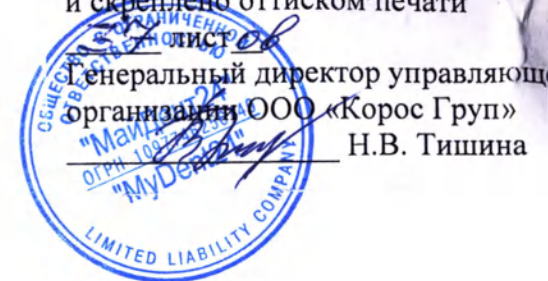

Генеральный директор управляющей
организации ООО «Корос Групп»
Н.В. Тишина