

УТВЕРЖДАЮ
Генеральный директор
ООО «БМТ»
Зимин А.В.



М.П.

«15» сентября 2021 г.

ФОТОГРАФИЧЕСКИЕ ИЗОБРАЖЕНИЯ МЕДИЦИНСКОГО ИЗДЕЛИЯ:

«Чашки лабораторные для вспомогательных репродуктивных технологий»

Culture Dish 40 mm

5 pcs

For in vitro fertilization.


STERILE R SAL 10⁻⁶. MEA (1-cell,
expanded blastocysts
within 96 hours) ≥ 80%. Endotoxin
≤ 0.25 EU/device. Rx only.

REF 16001

LOT 11735

 2020-06-29

 2023-06-29



For symbol glossary
see outer box.


 HertART ApS
Gustaf Werners gata 2
V. Frölunda, Sweden

Vitrolife 





(01)17350025914487(11)200629(17)230629(10)11735


Первичная упаковка

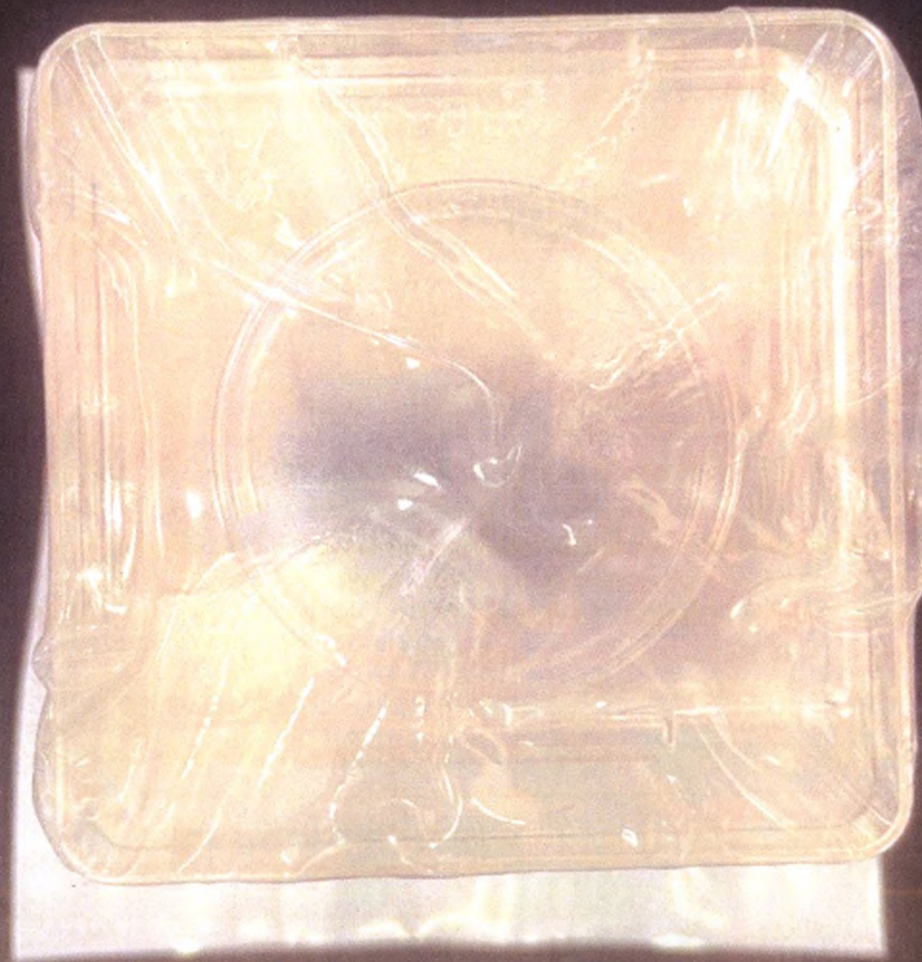

Первичная упаковка (с макетом маркировки на русском языке)

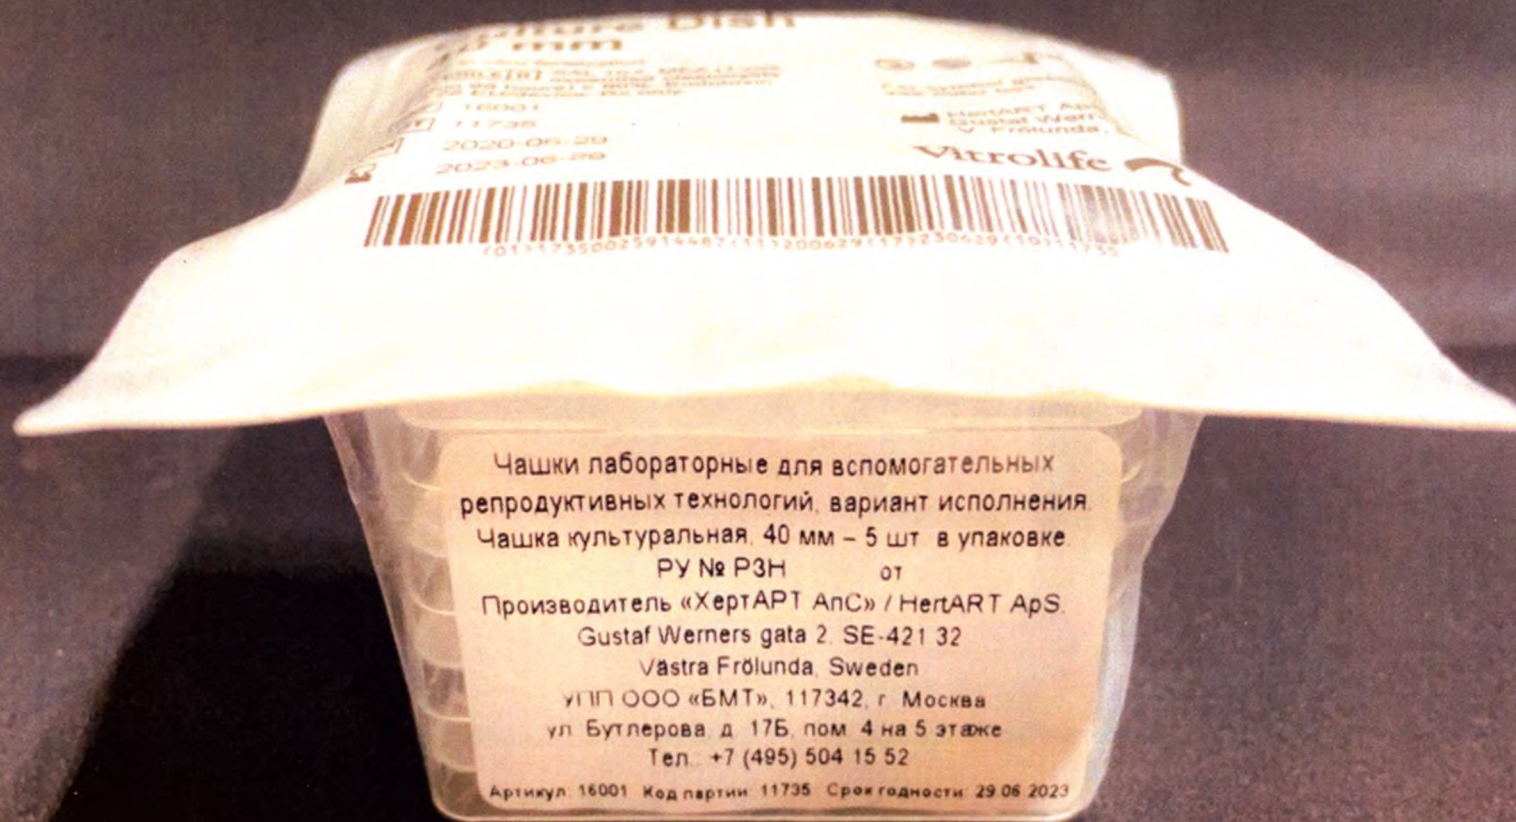


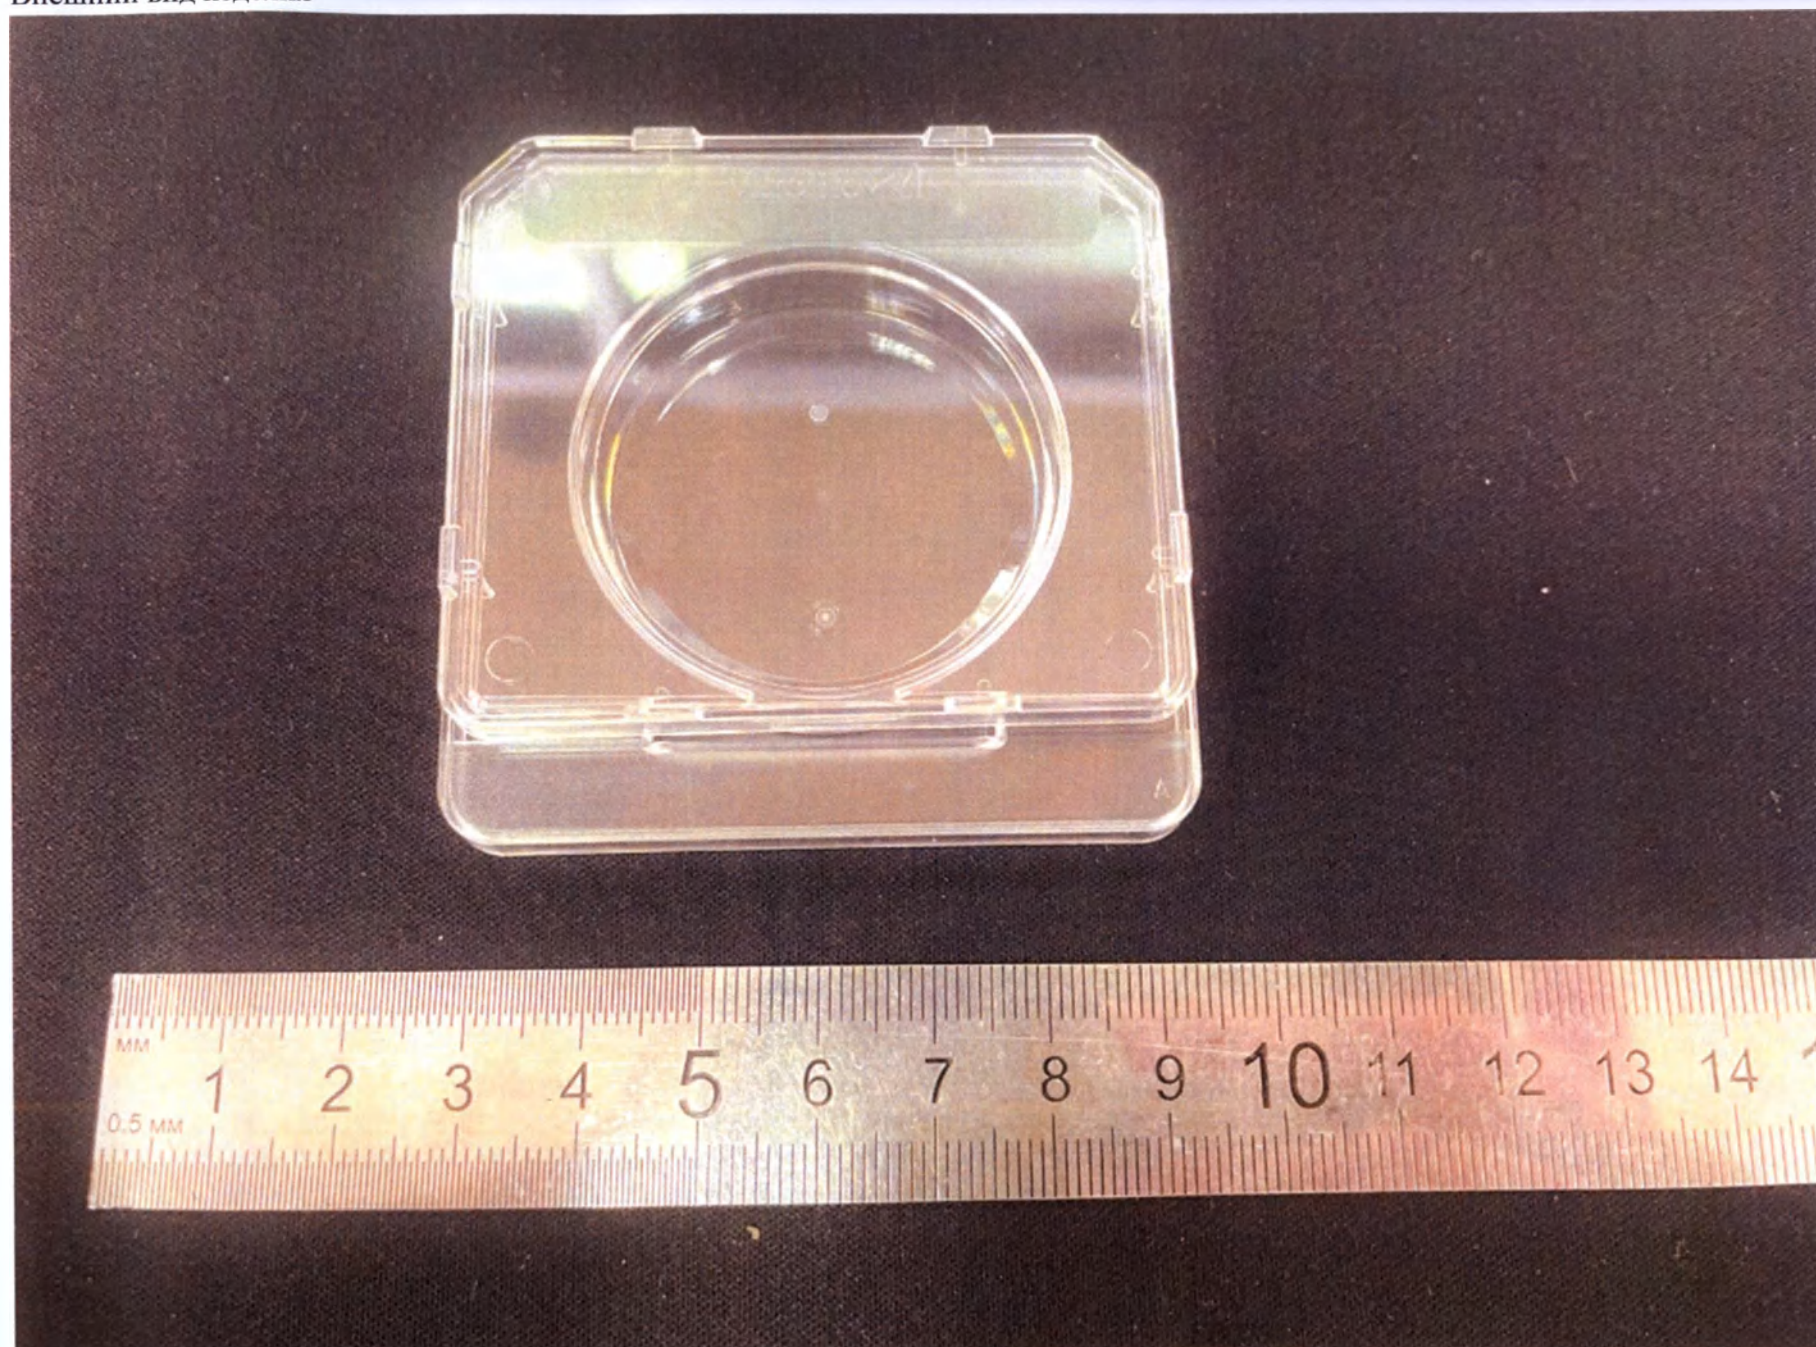

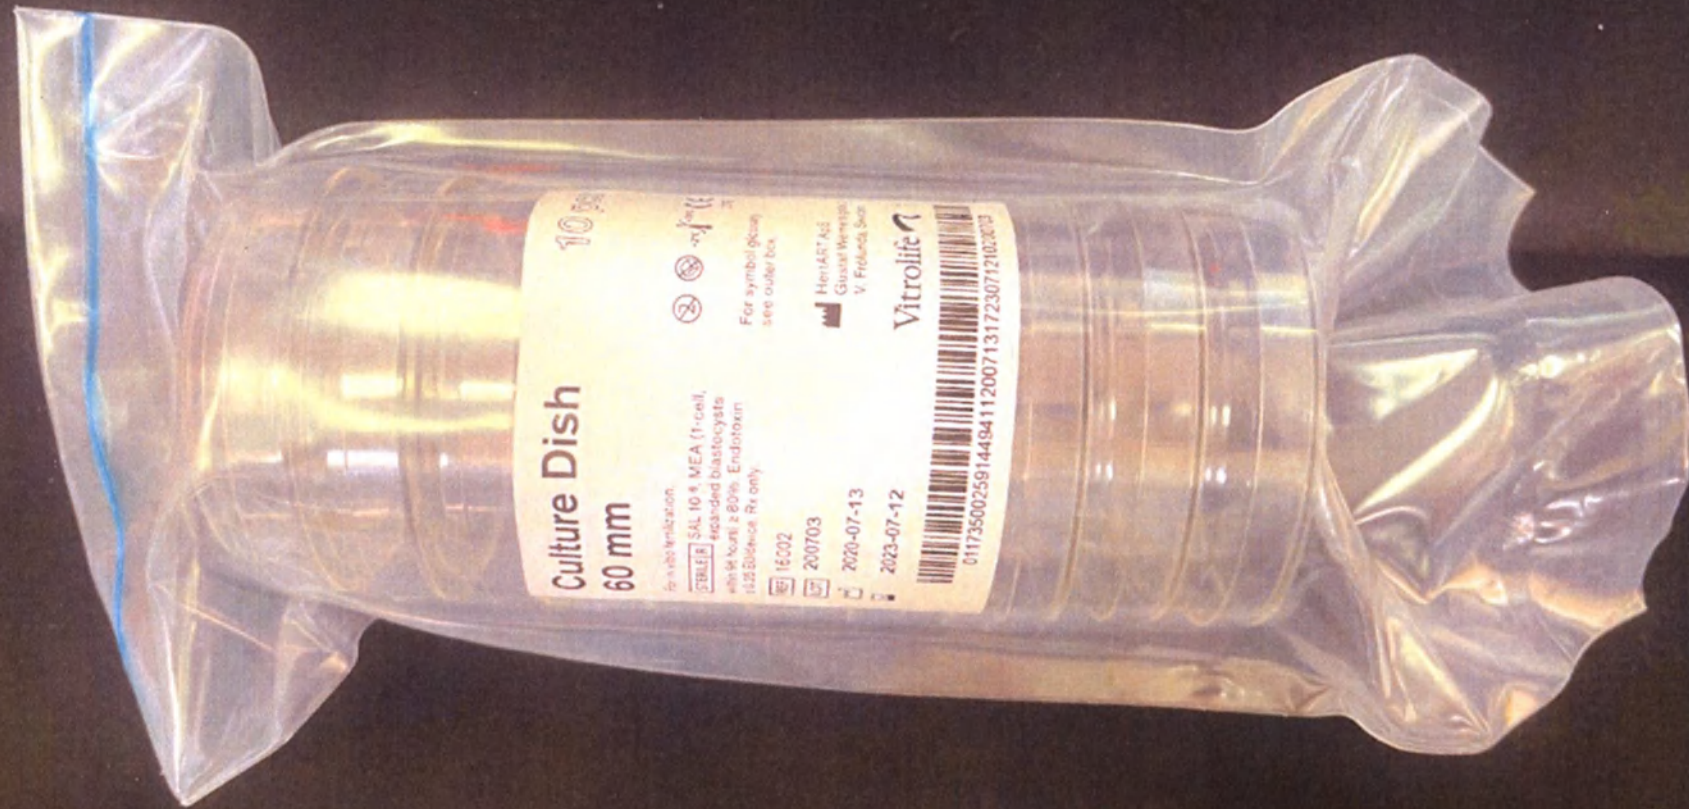

Первичная упаковка (с макетом маркировки на русском языке)



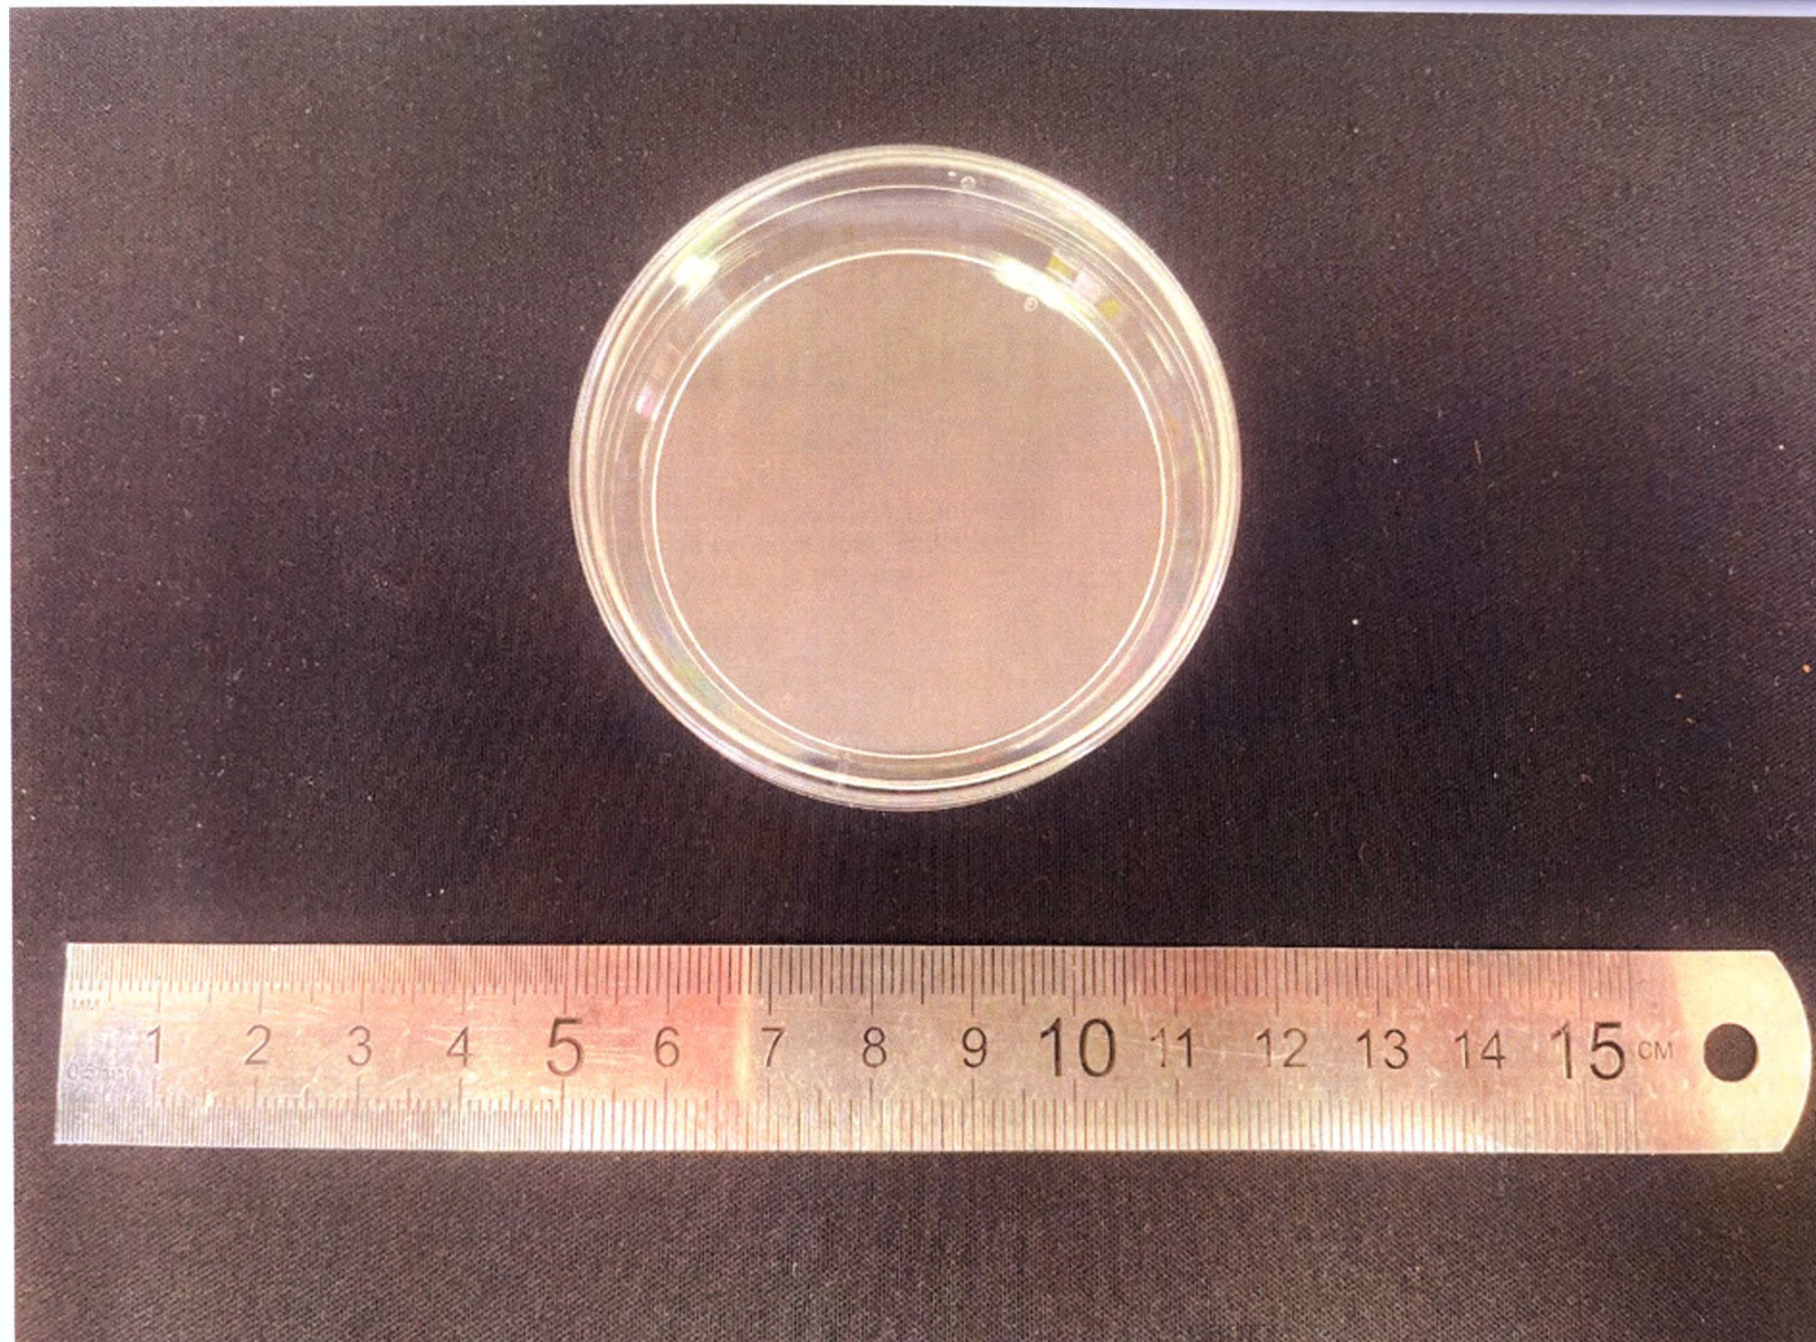

Micro-droplet Culture Dish

5 pcs

For in vitro fertilization.

STERILE R SAL 10⁻⁶. MEA (1-cell,
expanded blastocysts
within 96 hours) $\geq$ 80%. Endotoxin
 $\leq$ 0.25 EU/device. Rx only.

REF 16003

LOT 11762

 2020-08-28

 2023-08-28




For symbol glossary
see outer box.


 HertART ApS
Gustaf Werners gata 2
V. Frölunda, Sweden

Vitrolife  v.06



(01)17350025914500(11)200828(17)230828(10)11762

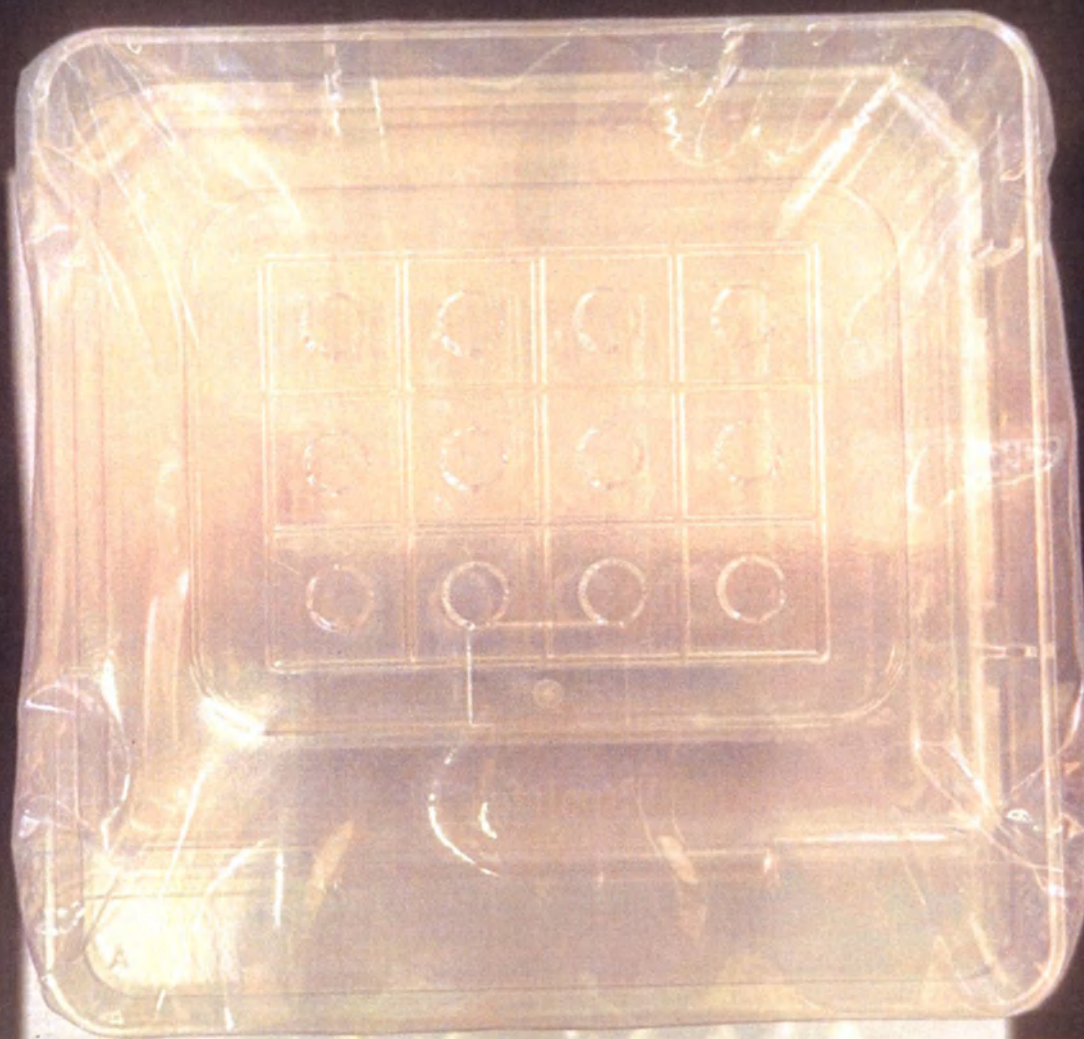

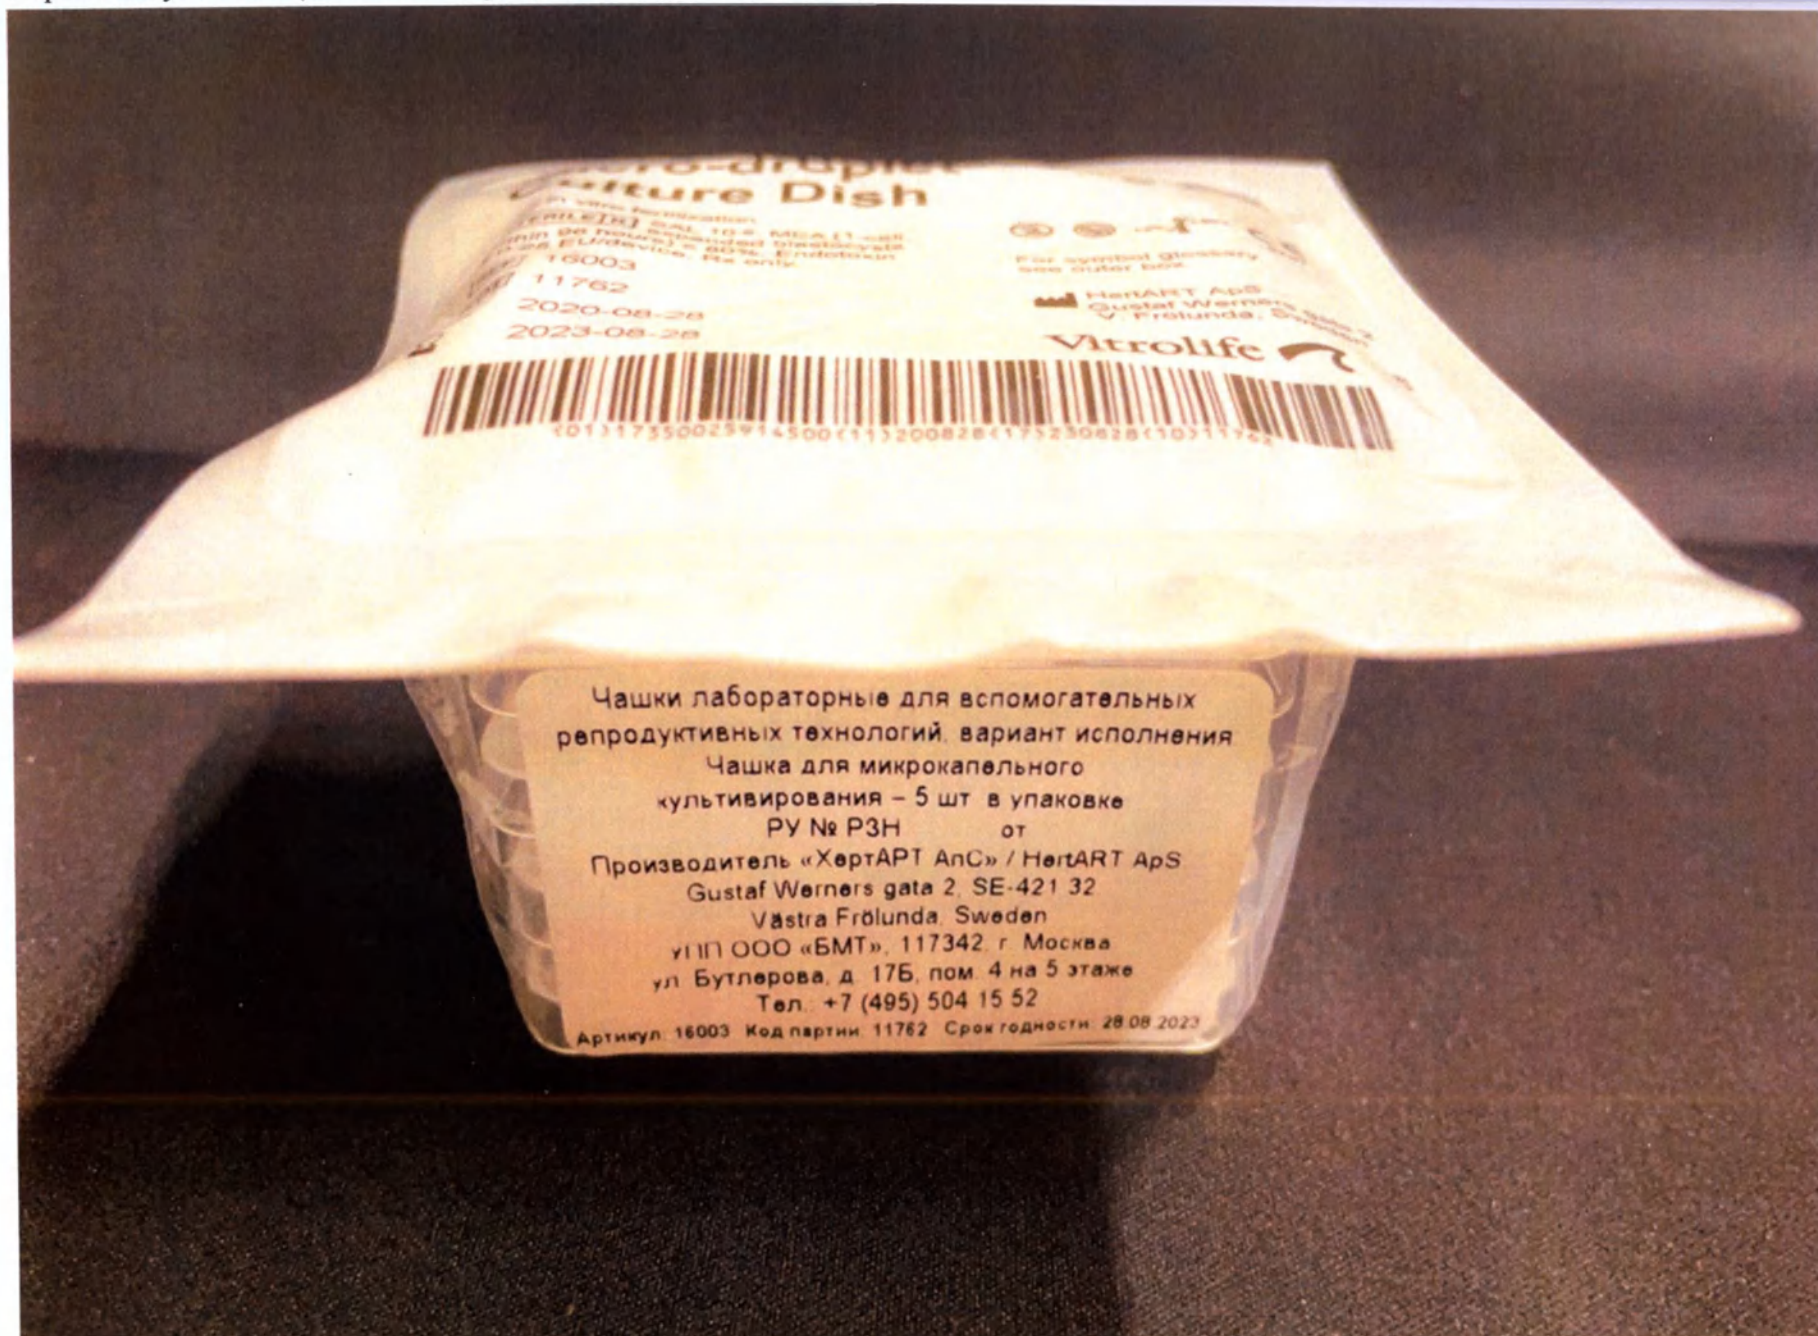



15.09.2021

5 Well Culture Dish

5 pcs

For in vitro fertilization.

STERILE **R** SAL 10⁻⁶. MEA (1-cell,
expanded blastocysts
within 96 hours) $\geq 80\%$. Endotoxin
 ≤ 0.25 EU/device. Rx only.

REF 16004

LOT 11720

 2020-06-22

 2023-06-22



For symbol glossary
see outer box.


 HertART ApS
Gustaf Werners gata 2
V. Frölunda, Sweden


Vitrolife 



(01)17350025914517(11)200622(17)230622(10)11720

Первичная упаковка

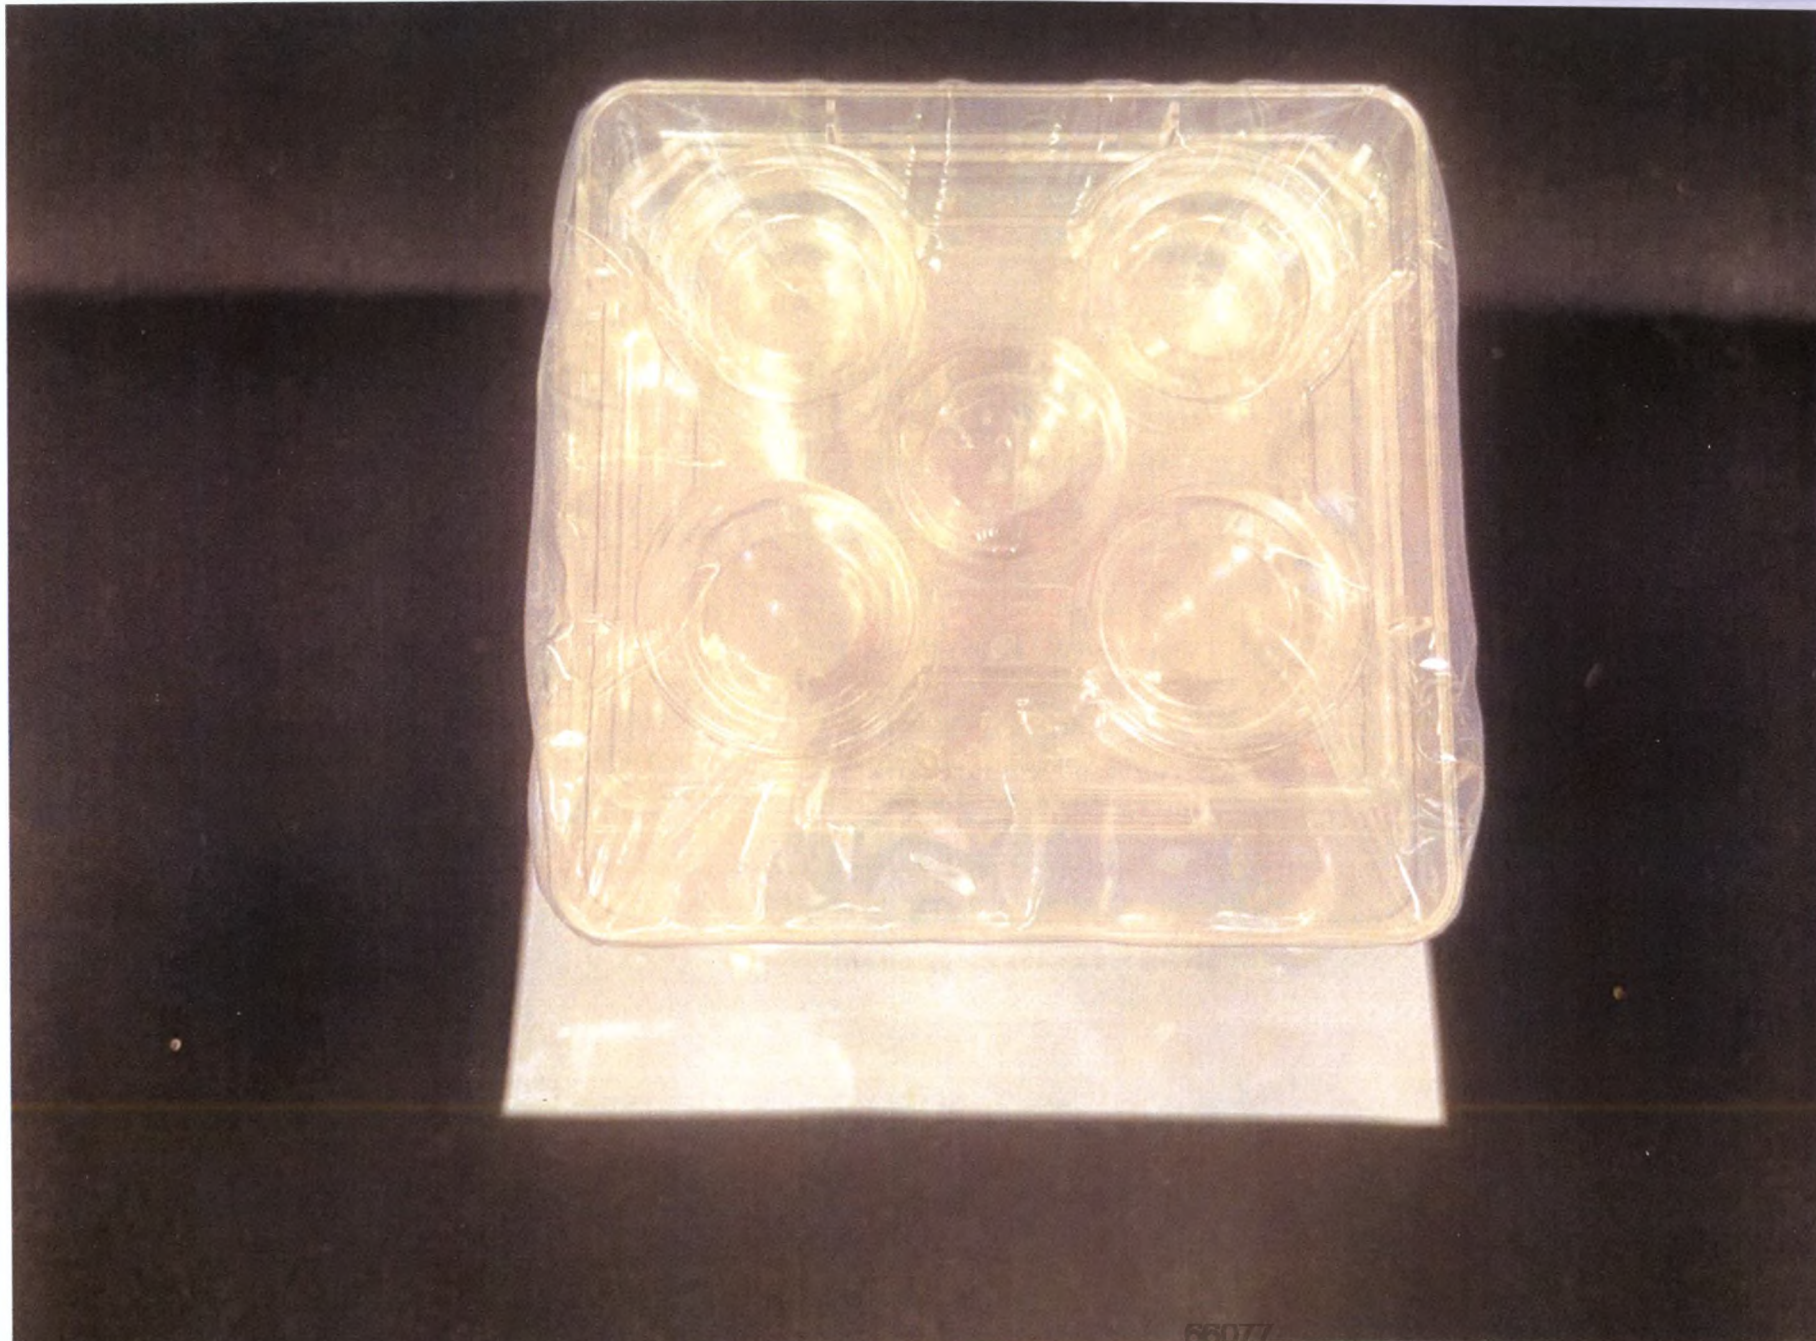

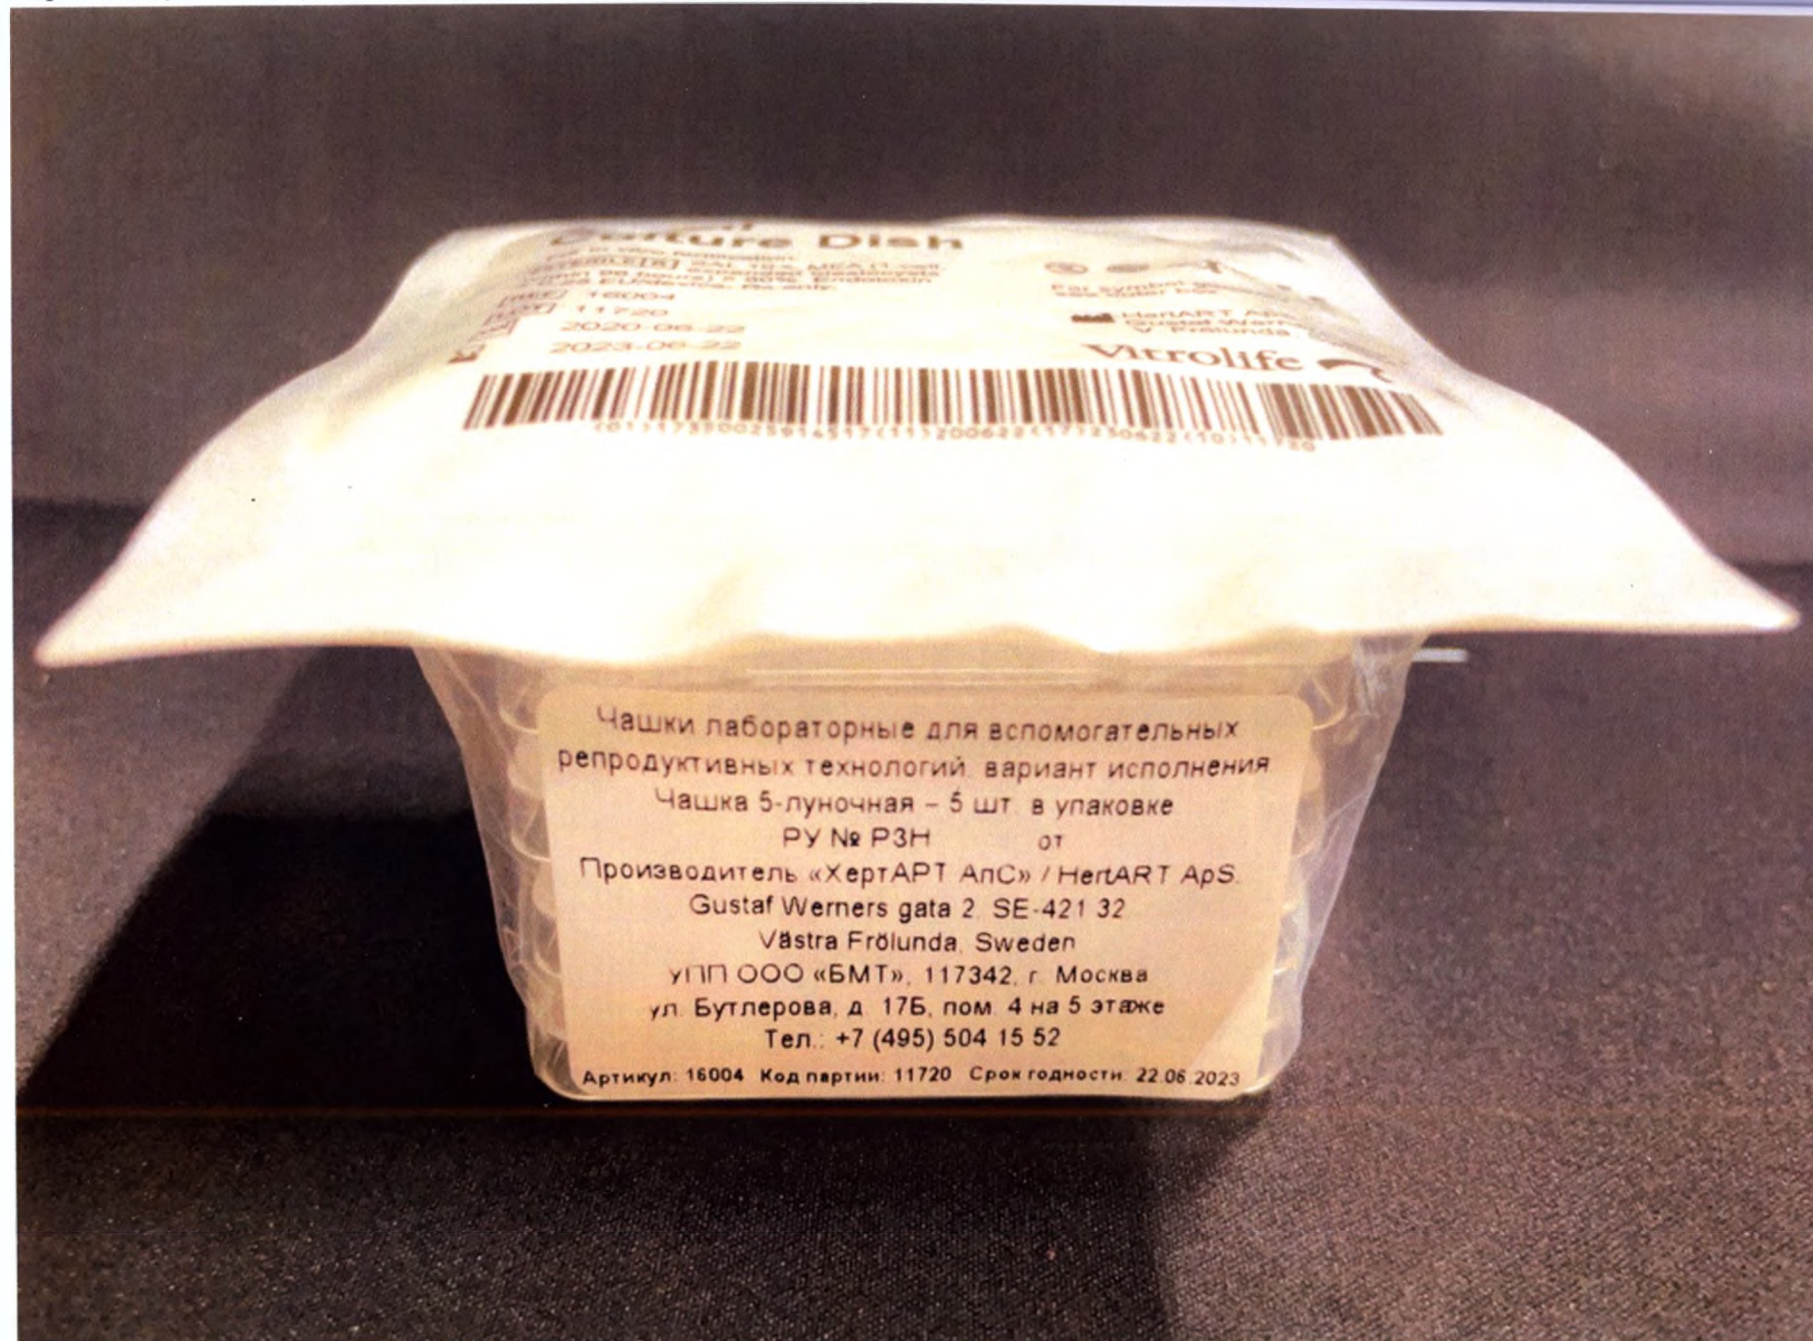



Centre Well Dish

5 pcs

For in vitro fertilization.


STERILE R SAL 10⁻⁶. MEA (1-cell,
expanded blastocysts
within 96 hours) $\geq 80\%$. Endotoxin
 ≤ 0.25 EU/device. Rx only.

REF 16005

LOT 11738

 2020-08-04

 2023-08-04




For symbol glossary
see outer box.

 HertART ApS
Gustaf Werners gata 2
V. Frölunda, Sweden


Vitrolife  v.06



(01)17350025914524(11)200804(17)230804(10)11738

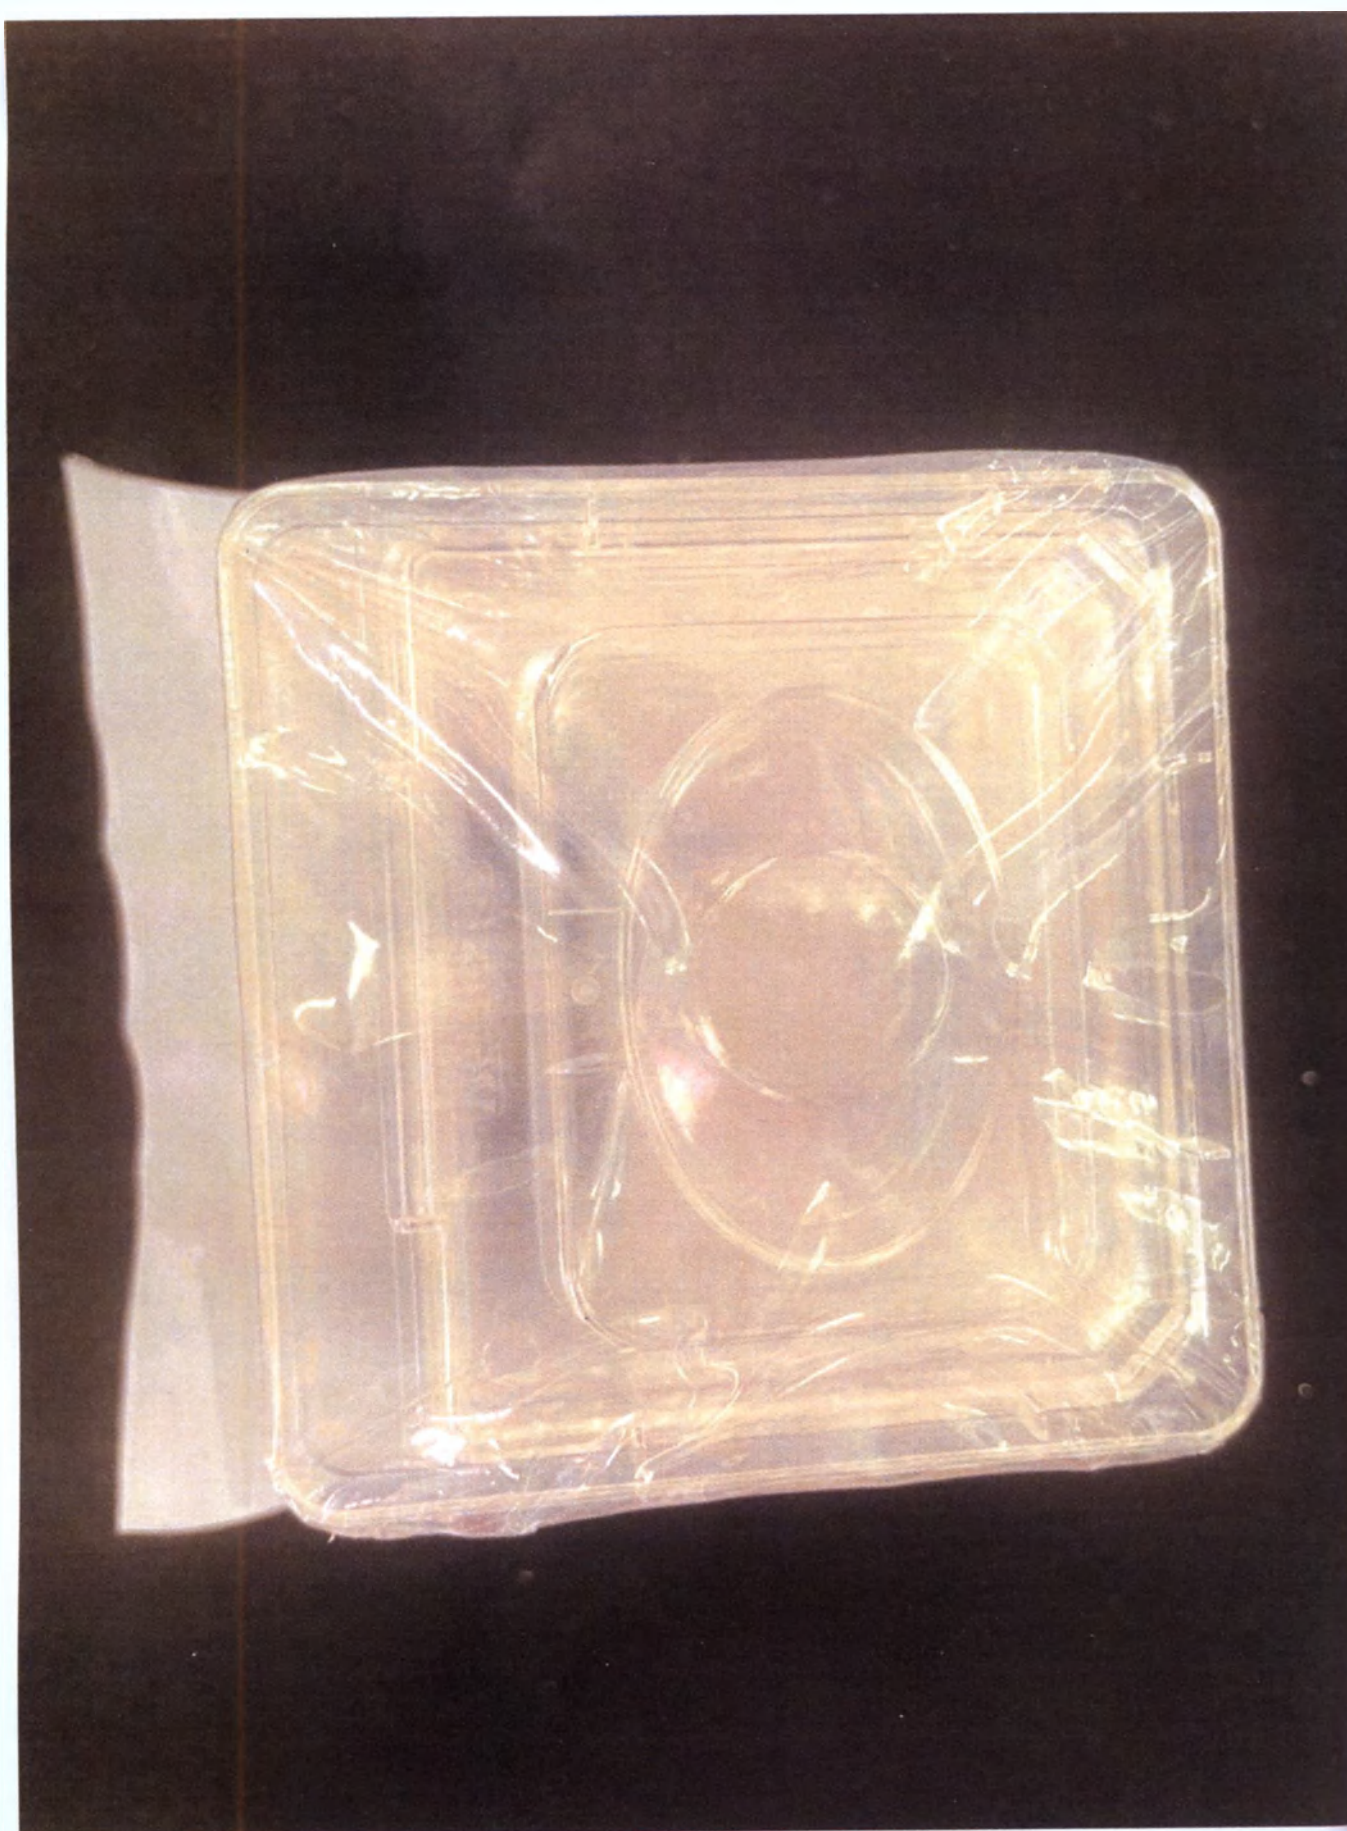

Внешний вид изделия

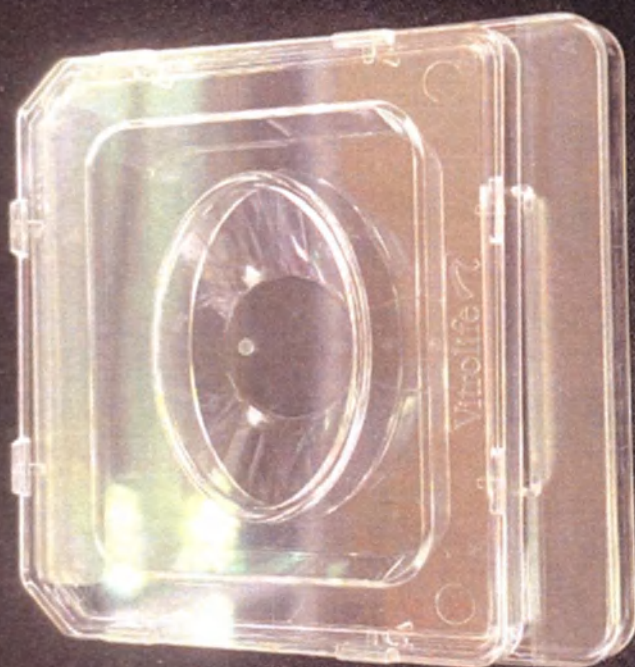

15.09.2021

ICSI Dish

5 pcs

For in vitro fertilization.


STERILE R SAL 10⁻⁶. MEA (1-cell,
expanded blastocysts
within 96 hours) ≥ 80%. Endotoxin
≤ 0.25 EU/device. Rx only.

REF 16006

LOT 11701

 2020-06-16

 2023-06-16



For symbol glossary
see outer box.


 HertART ApS
Gustaf Werners gata 2
V. Frölunda, Sweden

Vitrolife  v.05




(01)17350025914531(11)200616(17)230616(10)11701



Первичная упаковка

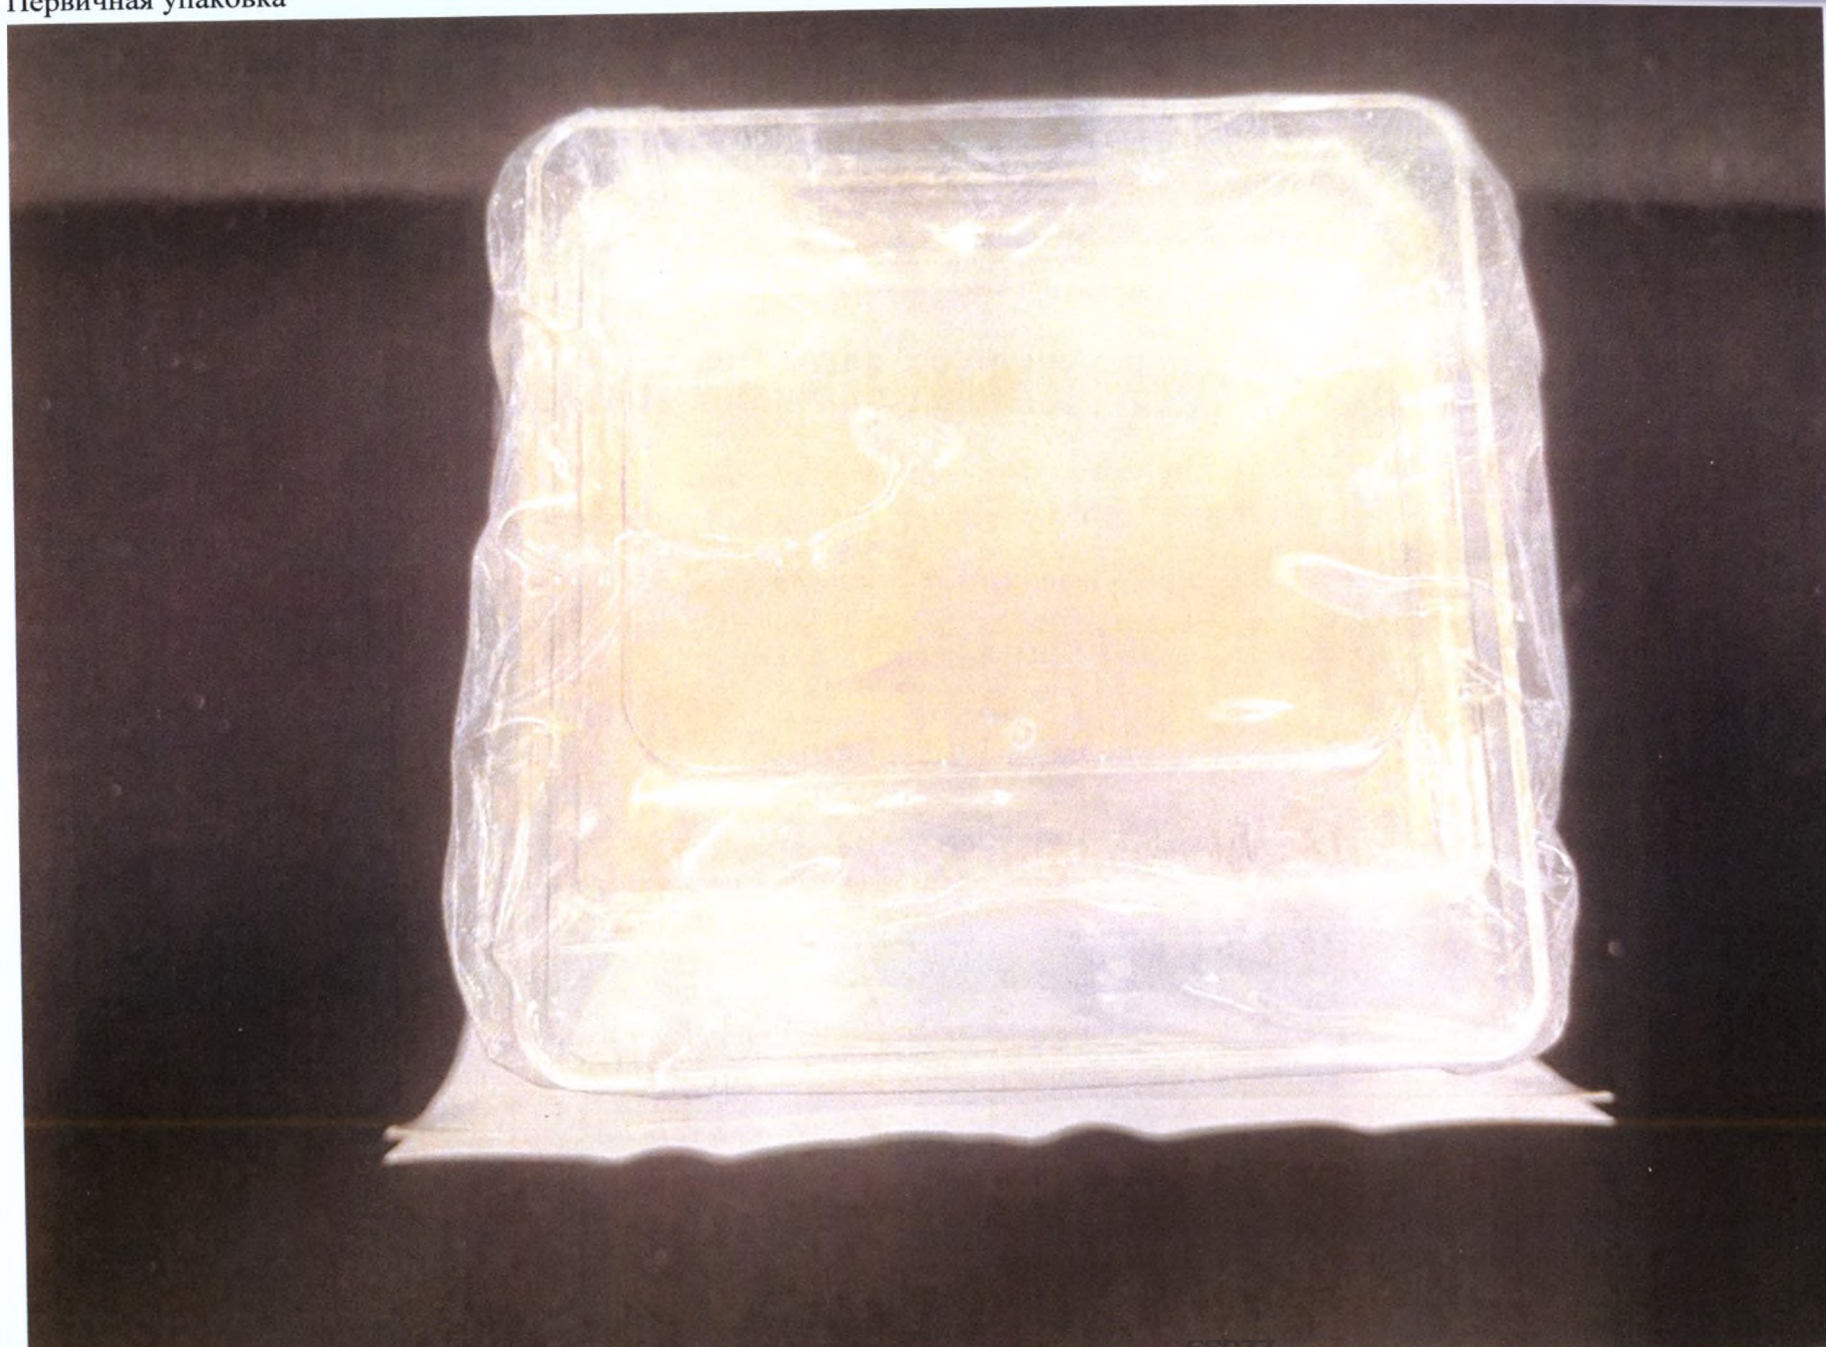


Первичная упаковка (с макетом маркировки на русском языке)

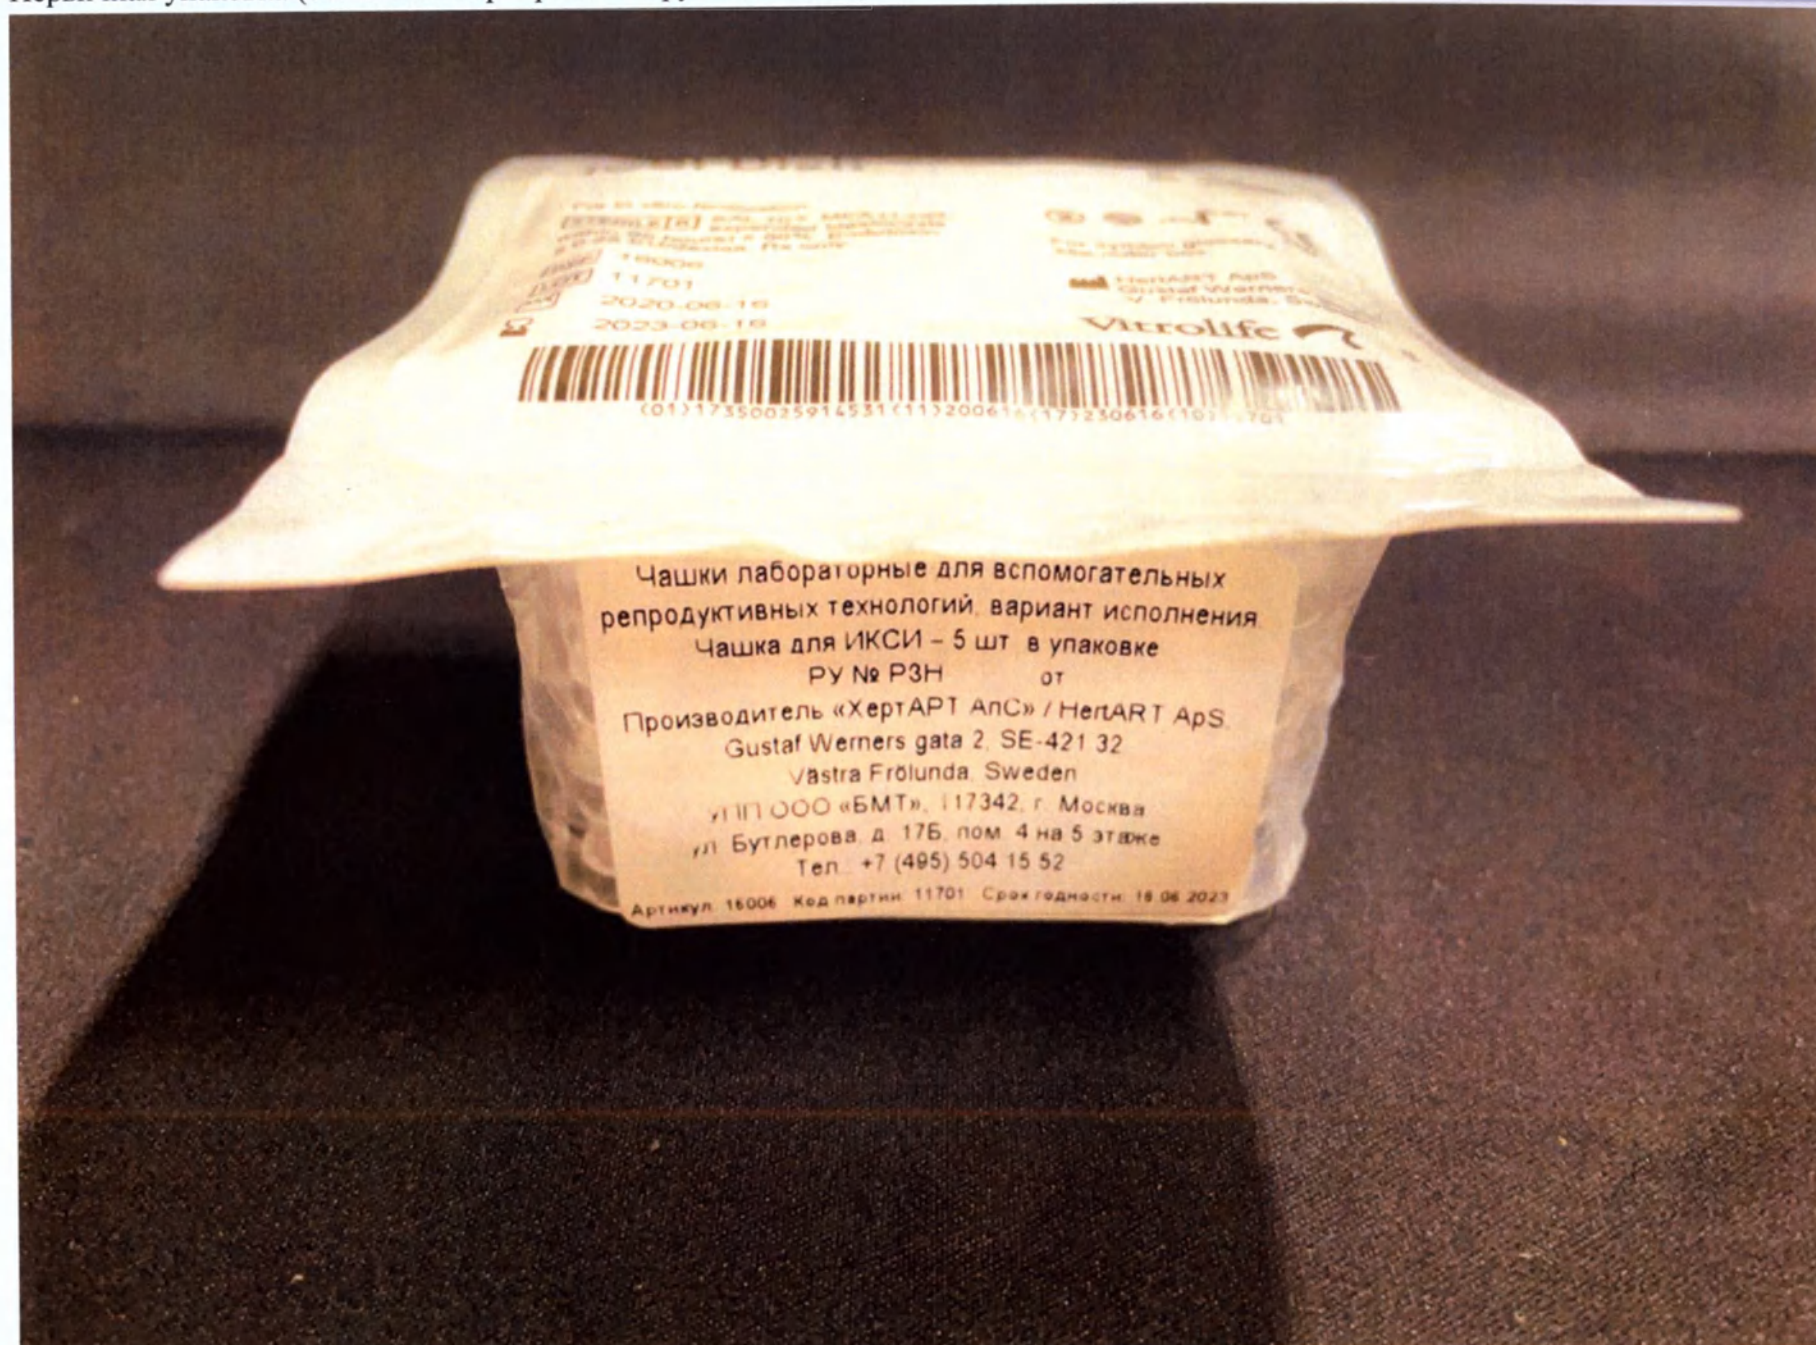


Внешний вид изделия

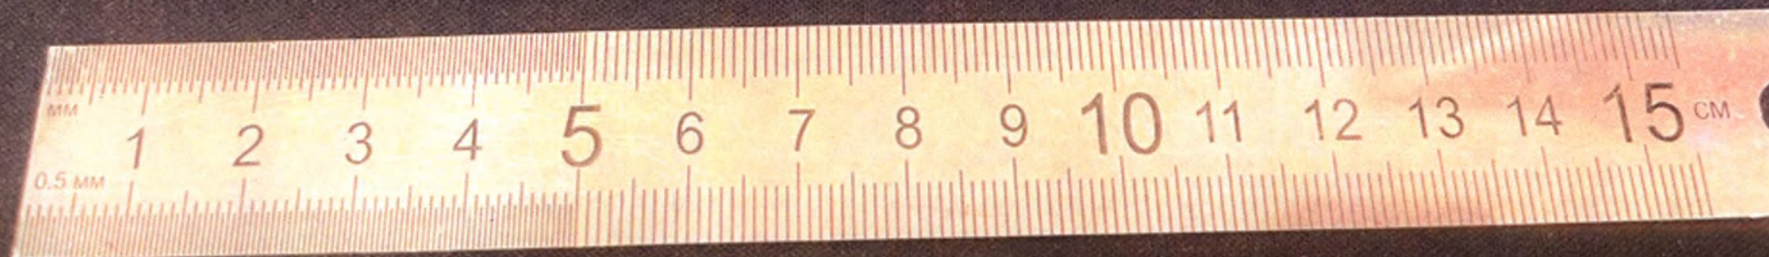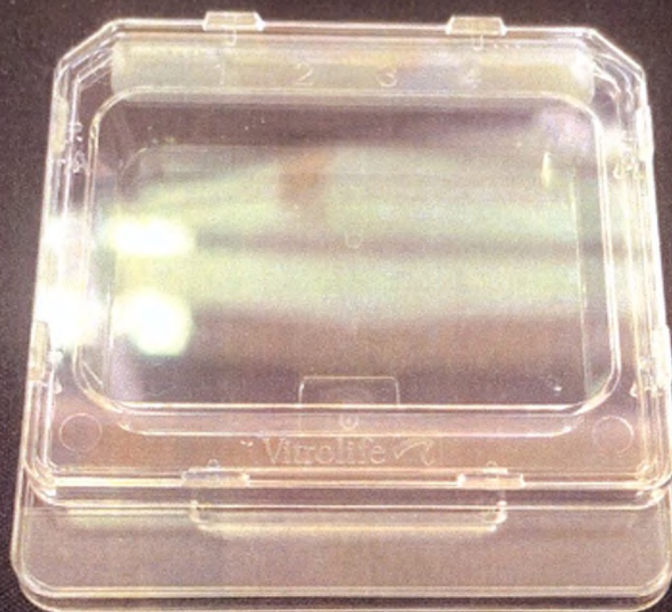

Первичная упаковка (с макетом маркировки на русском языке)

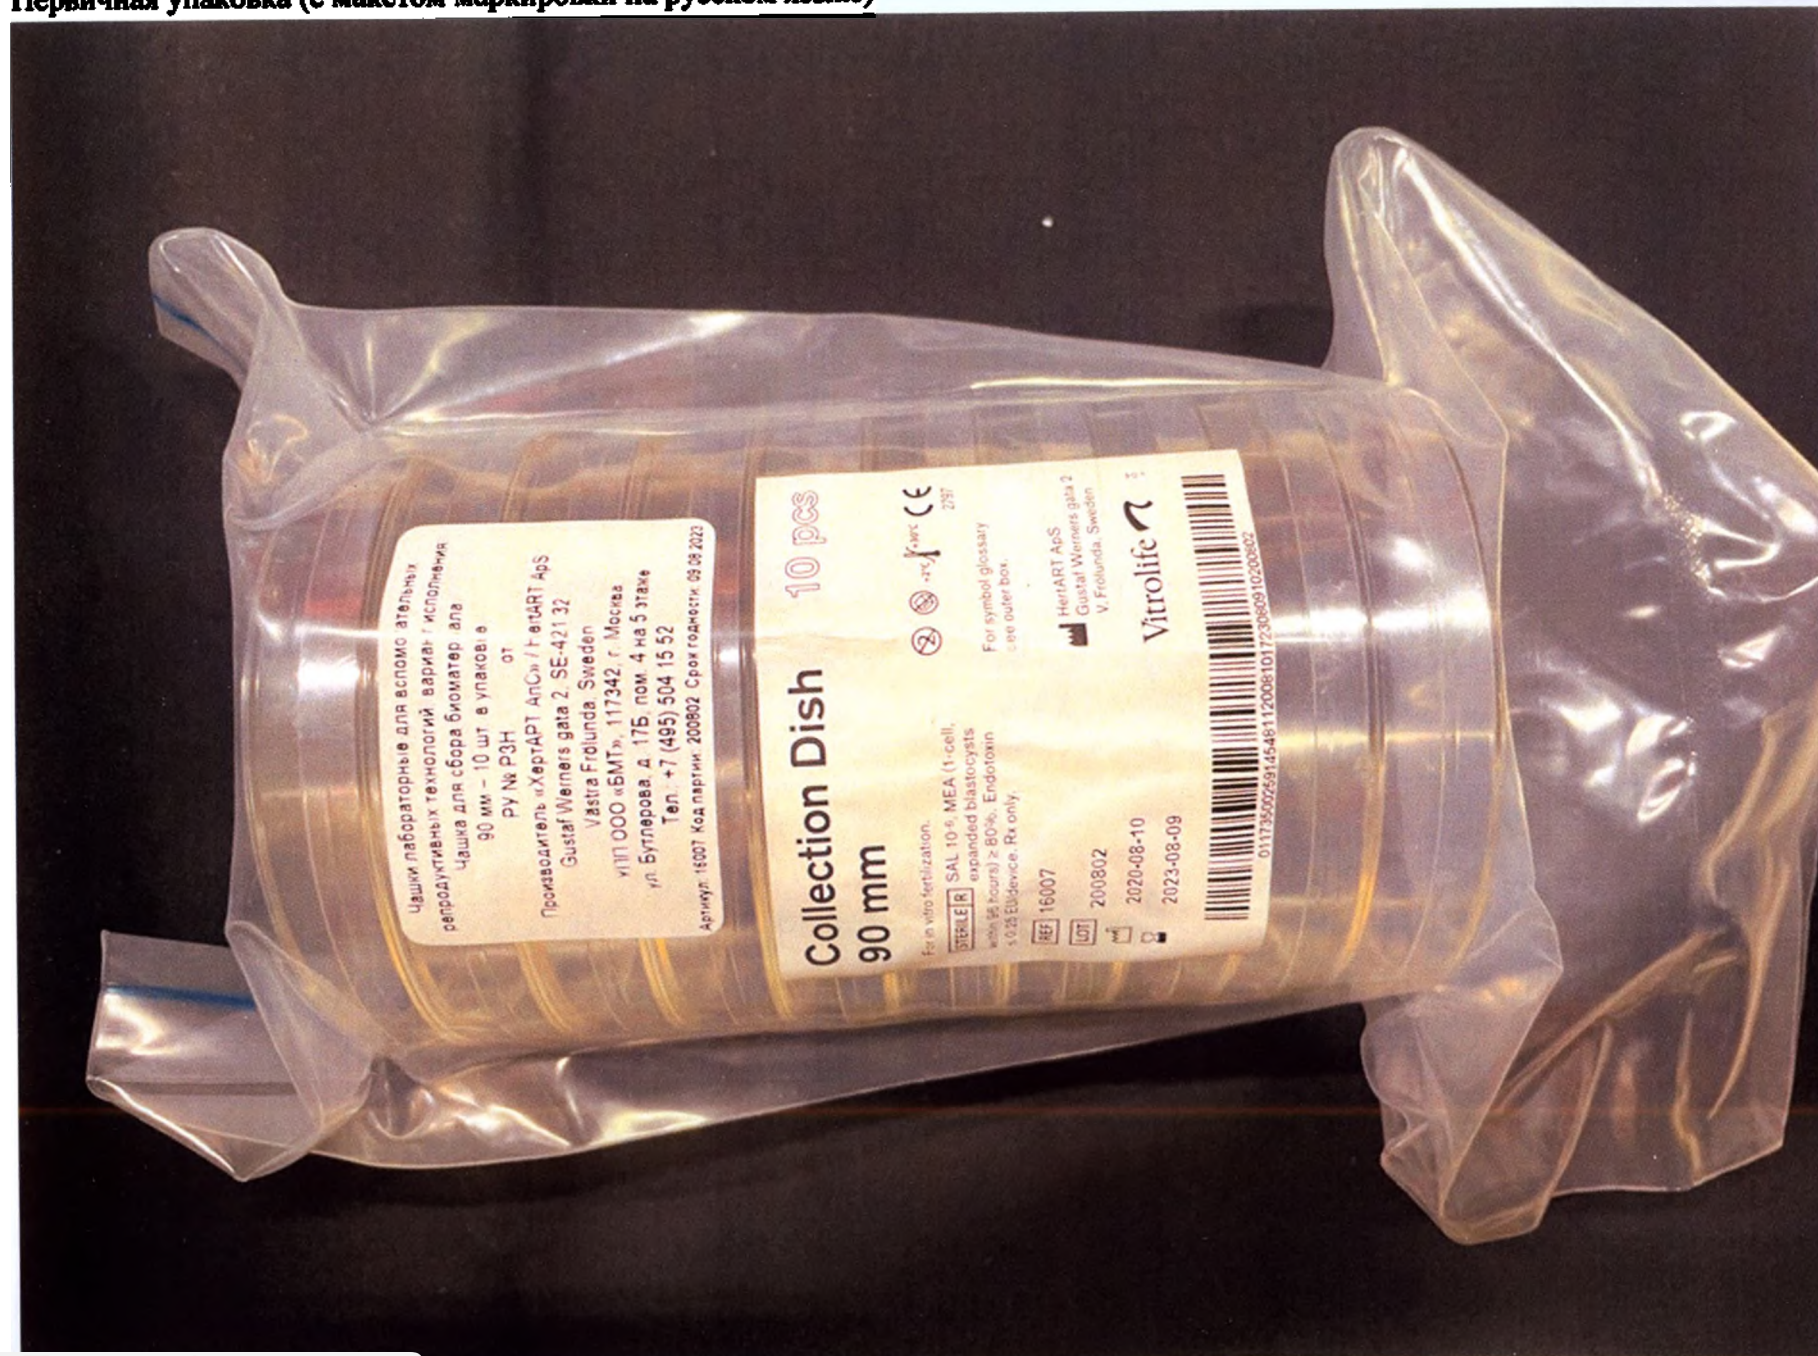

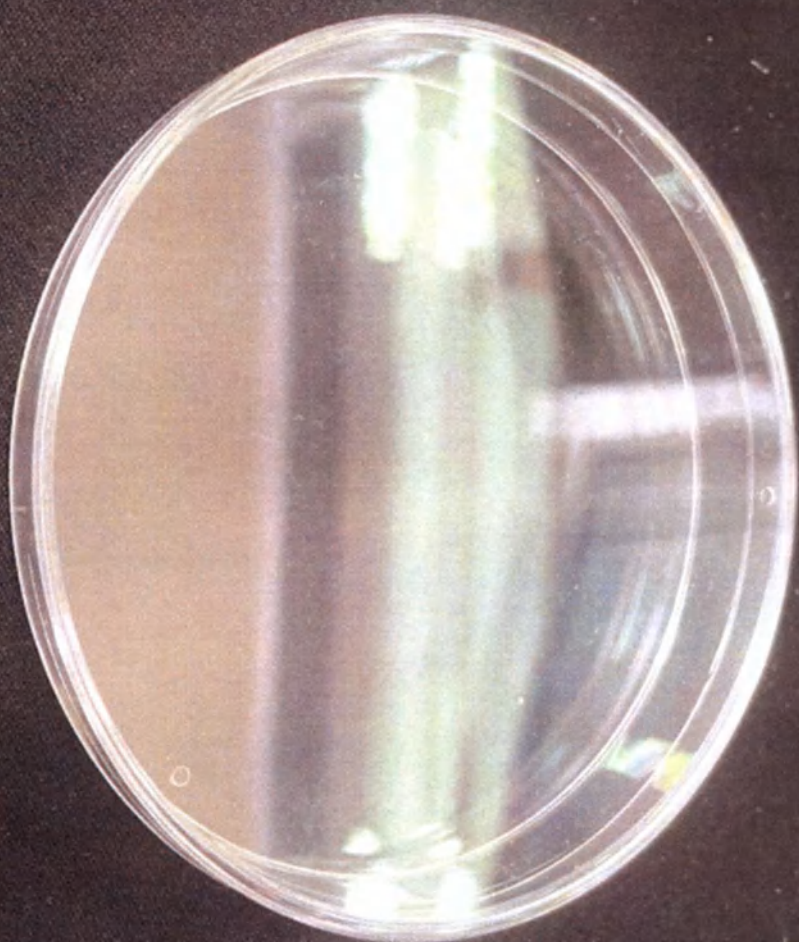

19.09.2021



Всего прошито, пронумеровано

И скреплено печатью 26 (двадцать шесть) лист 08

ГЕНЕРАЛЬНЫЙ ДИРЕКТОР
Зимин А.В.

