

ФОТОГРАФИЧЕСКОЕ ИЗОБРАЖЕНИЕ МЕДИЦИНСКОГО ИЗДЕЛИЯ
(ред. 1)

«Лезвия Leica микротомные одноразовые»,

производства

«Leica Biosystems Nussloch GmbH», Германия

июнь, 2021

СОДЕРЖАНИЕ

Изображение	Стр.
Раздел I. Изображения общего вида вариантов исполнения регистрируемого медицинского изделия:	3
1. Лезвия микротомные одноразовые низкого профиля Leica 819 (Leica 819 Low Profile Microtome Blades);	4
2. Лезвия микротомные одноразовые высокого профиля Leica 818 (Leica 818 High Profile Microtome Blades);	22
3. Лезвия микротомные одноразовые низкого профиля Leica DB80LS (Leica DB80LS Low Profile Microtome Blades);	35
4. Лезвия микротомные одноразовые низкого профиля Leica DB80LX (Leica DB80LX Low Profile Microtome Blades);	46
5. Лезвия микротомные одноразовые высокого профиля Leica DB80HS (Leica DB80HS High Profile Microtome Blades).	55
Раздел II. Изображения вариантов упаковки (фасовки), применяемых для каждого из вариантов исполнения регистрируемого медицинского изделия:	66
1. Общее изображение всех вариантов исполнения регистрируемого медицинского изделия с вариантом упаковки «1х50 (1 малая коробка по 50 изделий)»;	67
2. Общее изображение варианта упаковки «10х50 (1 большая коробка по 500 изделий)» на примере варианта исполнения «Лезвия микротомные одноразовые низкого профиля Leica DB80LX (Leica DB80LX Low Profile Microtome Blades)», кат. номер 14035843497.	71

Раздел I.
Изображения общего вида вариантов исполнения
регистрируемого медицинского изделия

**Лезвия микротомные одноразовые низкого профиля Leica 819
(Leica 819 Low Profile Microtome Blades)**

LEICA 819
Low Profile
Microtome Blades

Leica
SYSTEMS

819



REF 14035838925



14035838925



50 Blades



LOT

119381

33

In Case of Warranty Claims
Refer To Above Numbers

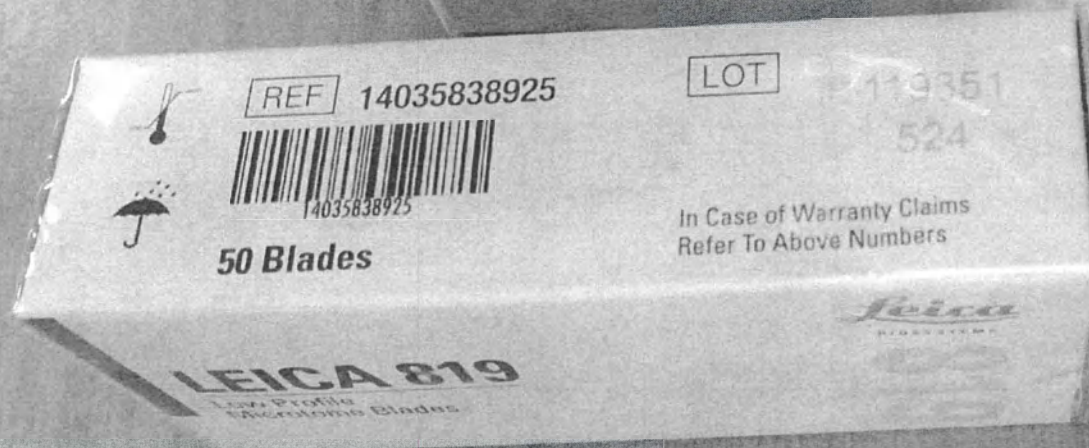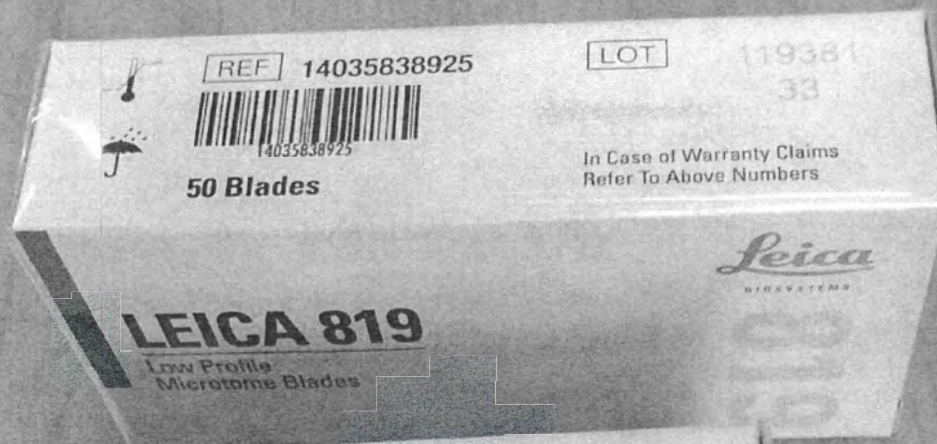

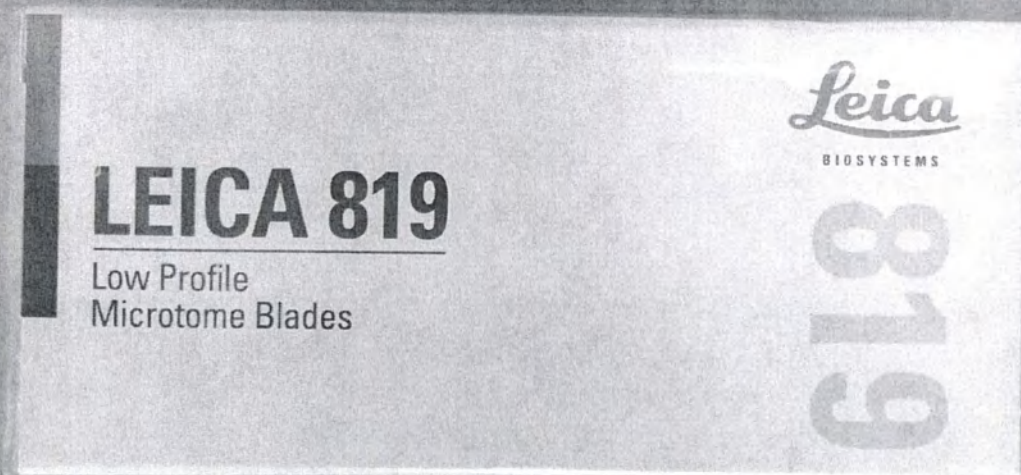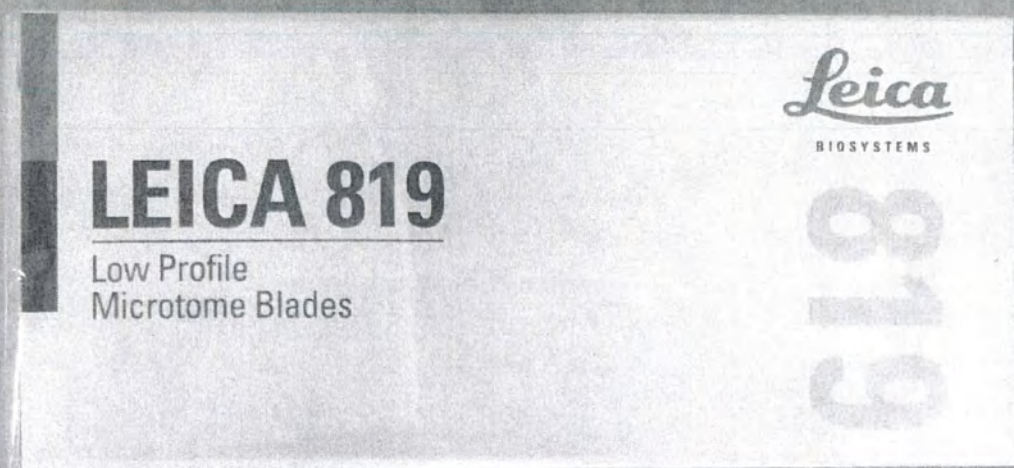

LEICA 819

Leica
BIO SYSTEM

LEICA 819

Low Profile
Microtome Blades

50 Blades



REF 14035838925



14035838925

50 Blades

LOT

119381


33

In Case of Warranty Claims
Refer To Above Numbers



Leica Biosystems Nussloch GmbH
D-59226 Nussloch (Germany)

Made in Germany




95.11495 Rev C



Use care when handling disposable
blades for microtomes.
Place used blades in used blade
compartment in the dispenser box.
Safely discard the dispenser box when
all blades have been used.



www.LeicaBiosystems.com

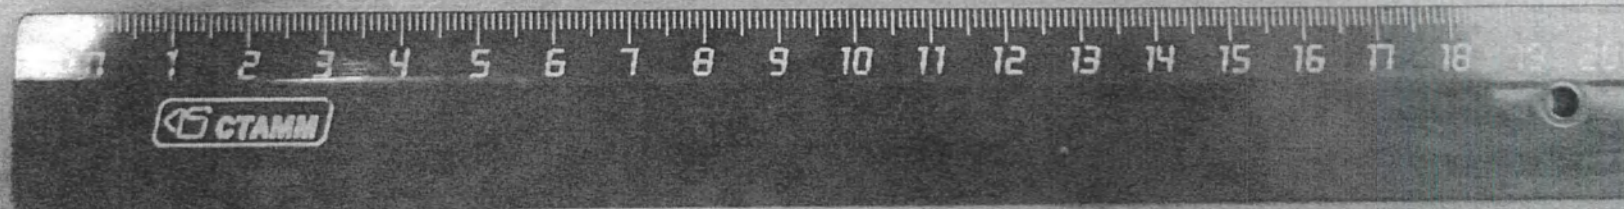



Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)

Made in Germany



95.11495 Rev C




Use care when handling disposable
blades for microtomes.

Place used blades in used blade
compartment in the dispenser box.

Safely discard the dispenser box when
all blades have been used.

www.LeicaBiosystems.com

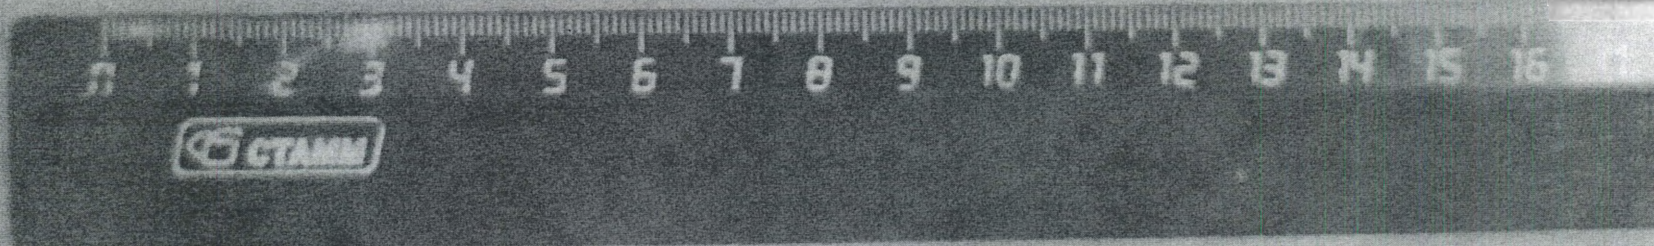



REF 14035838925



14035838925

50 Blades

LOT


119351
524

In Case of Warranty Claims
Refer To Above Numbers

LEICA 819

Low Profile
Microtome Blades

Leica
BIOSYSTEMS

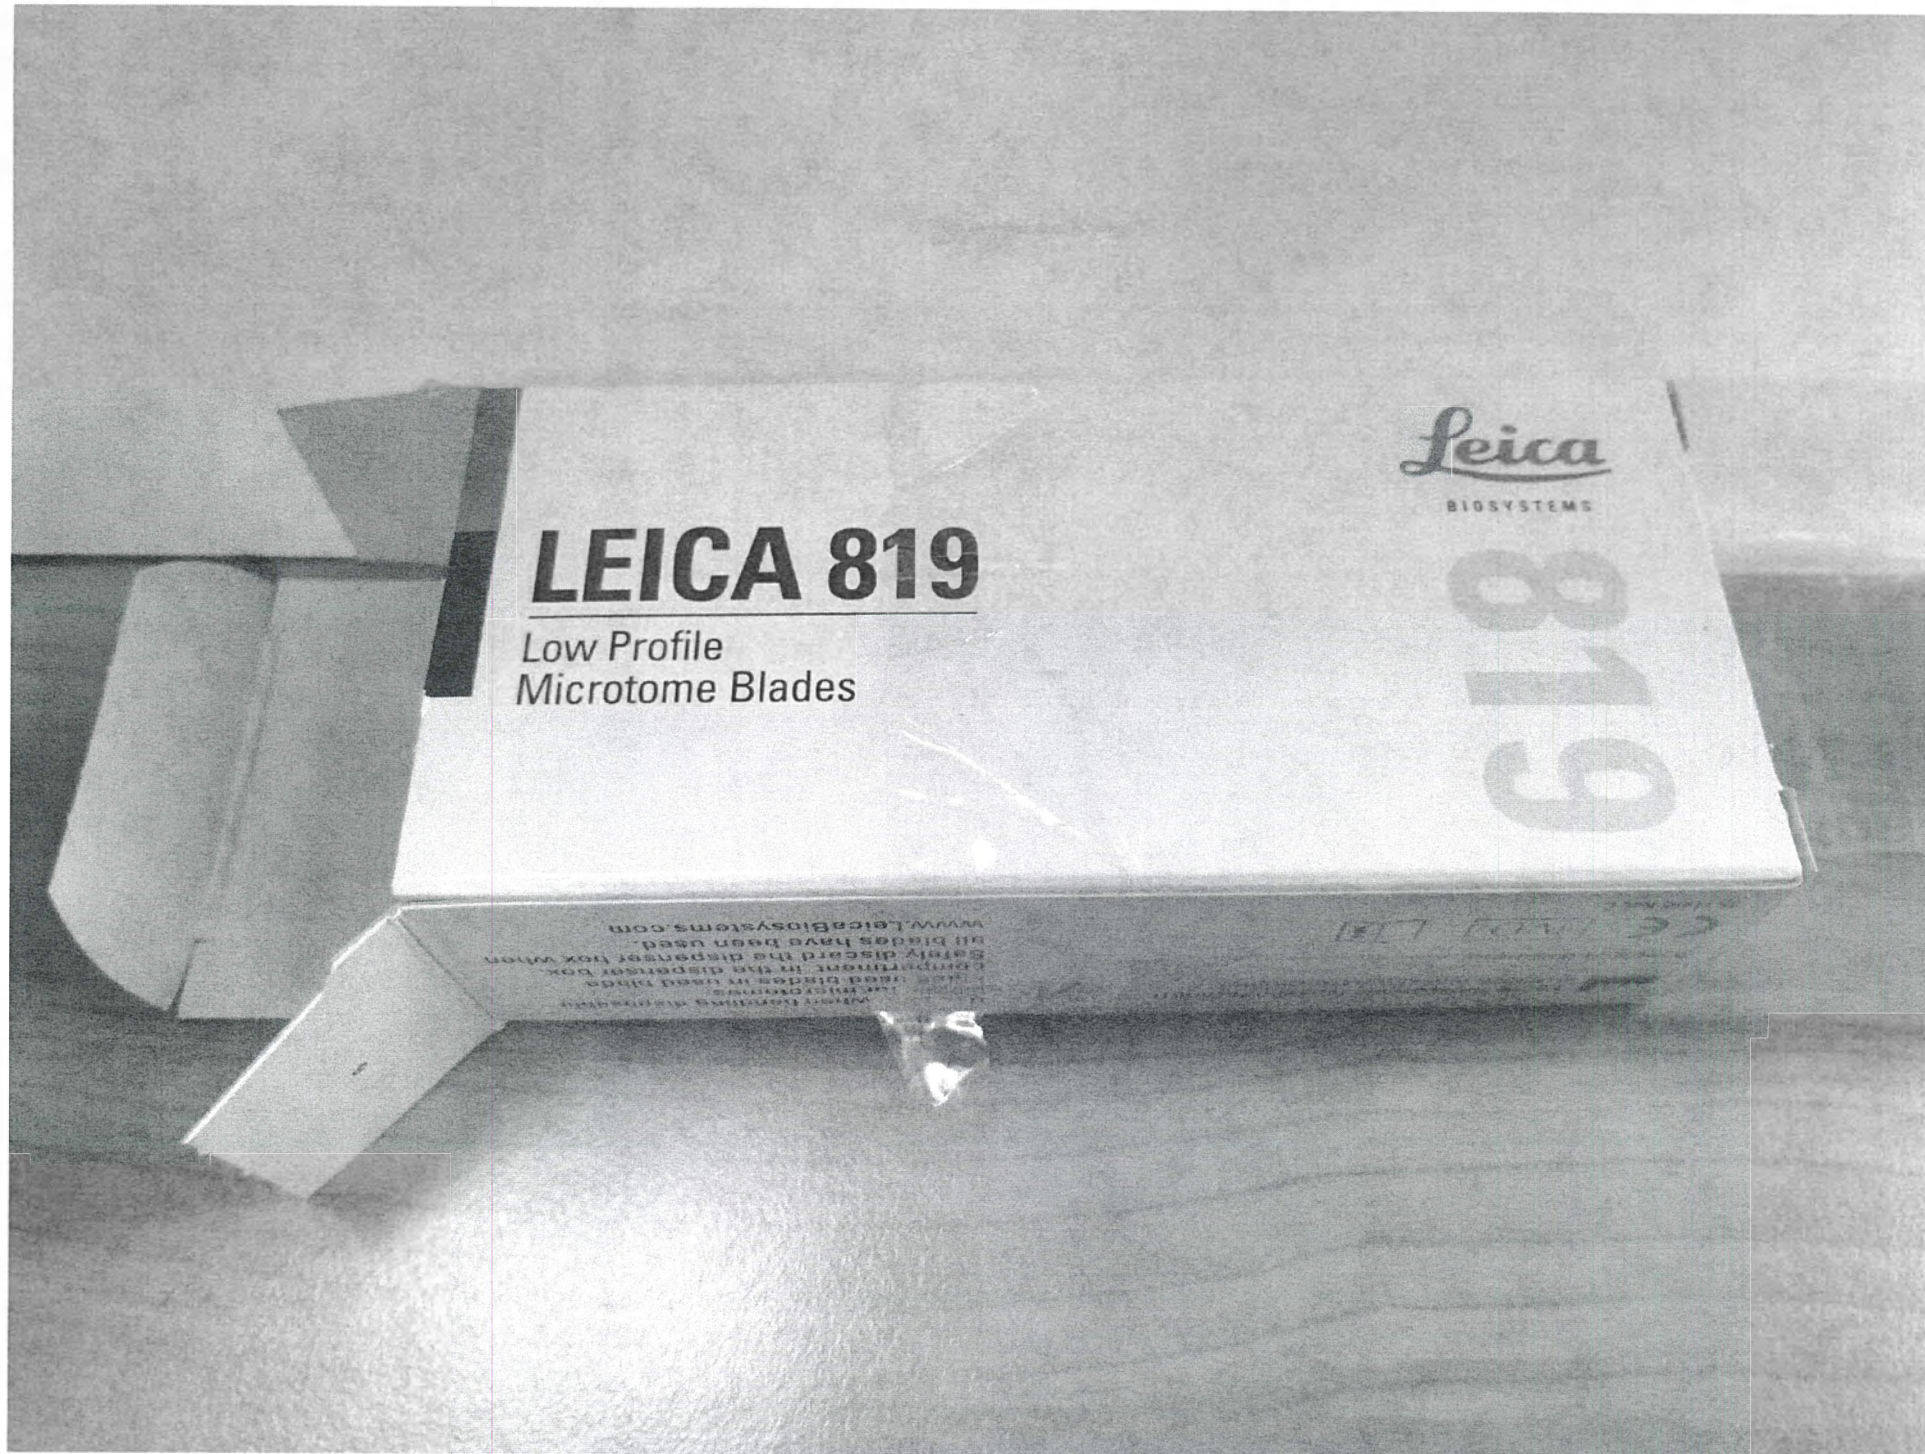


LEICA 819

Low Profile
Microtome Blades


Leica
BIOSYSTEMS


819


www.leicabiosystems.com
All blades have been used.
Safely discard the disposable box.
Leica Biosystems is not responsible for the use of blades in the disposable box.
When loading the blades, please use the provided instructions.

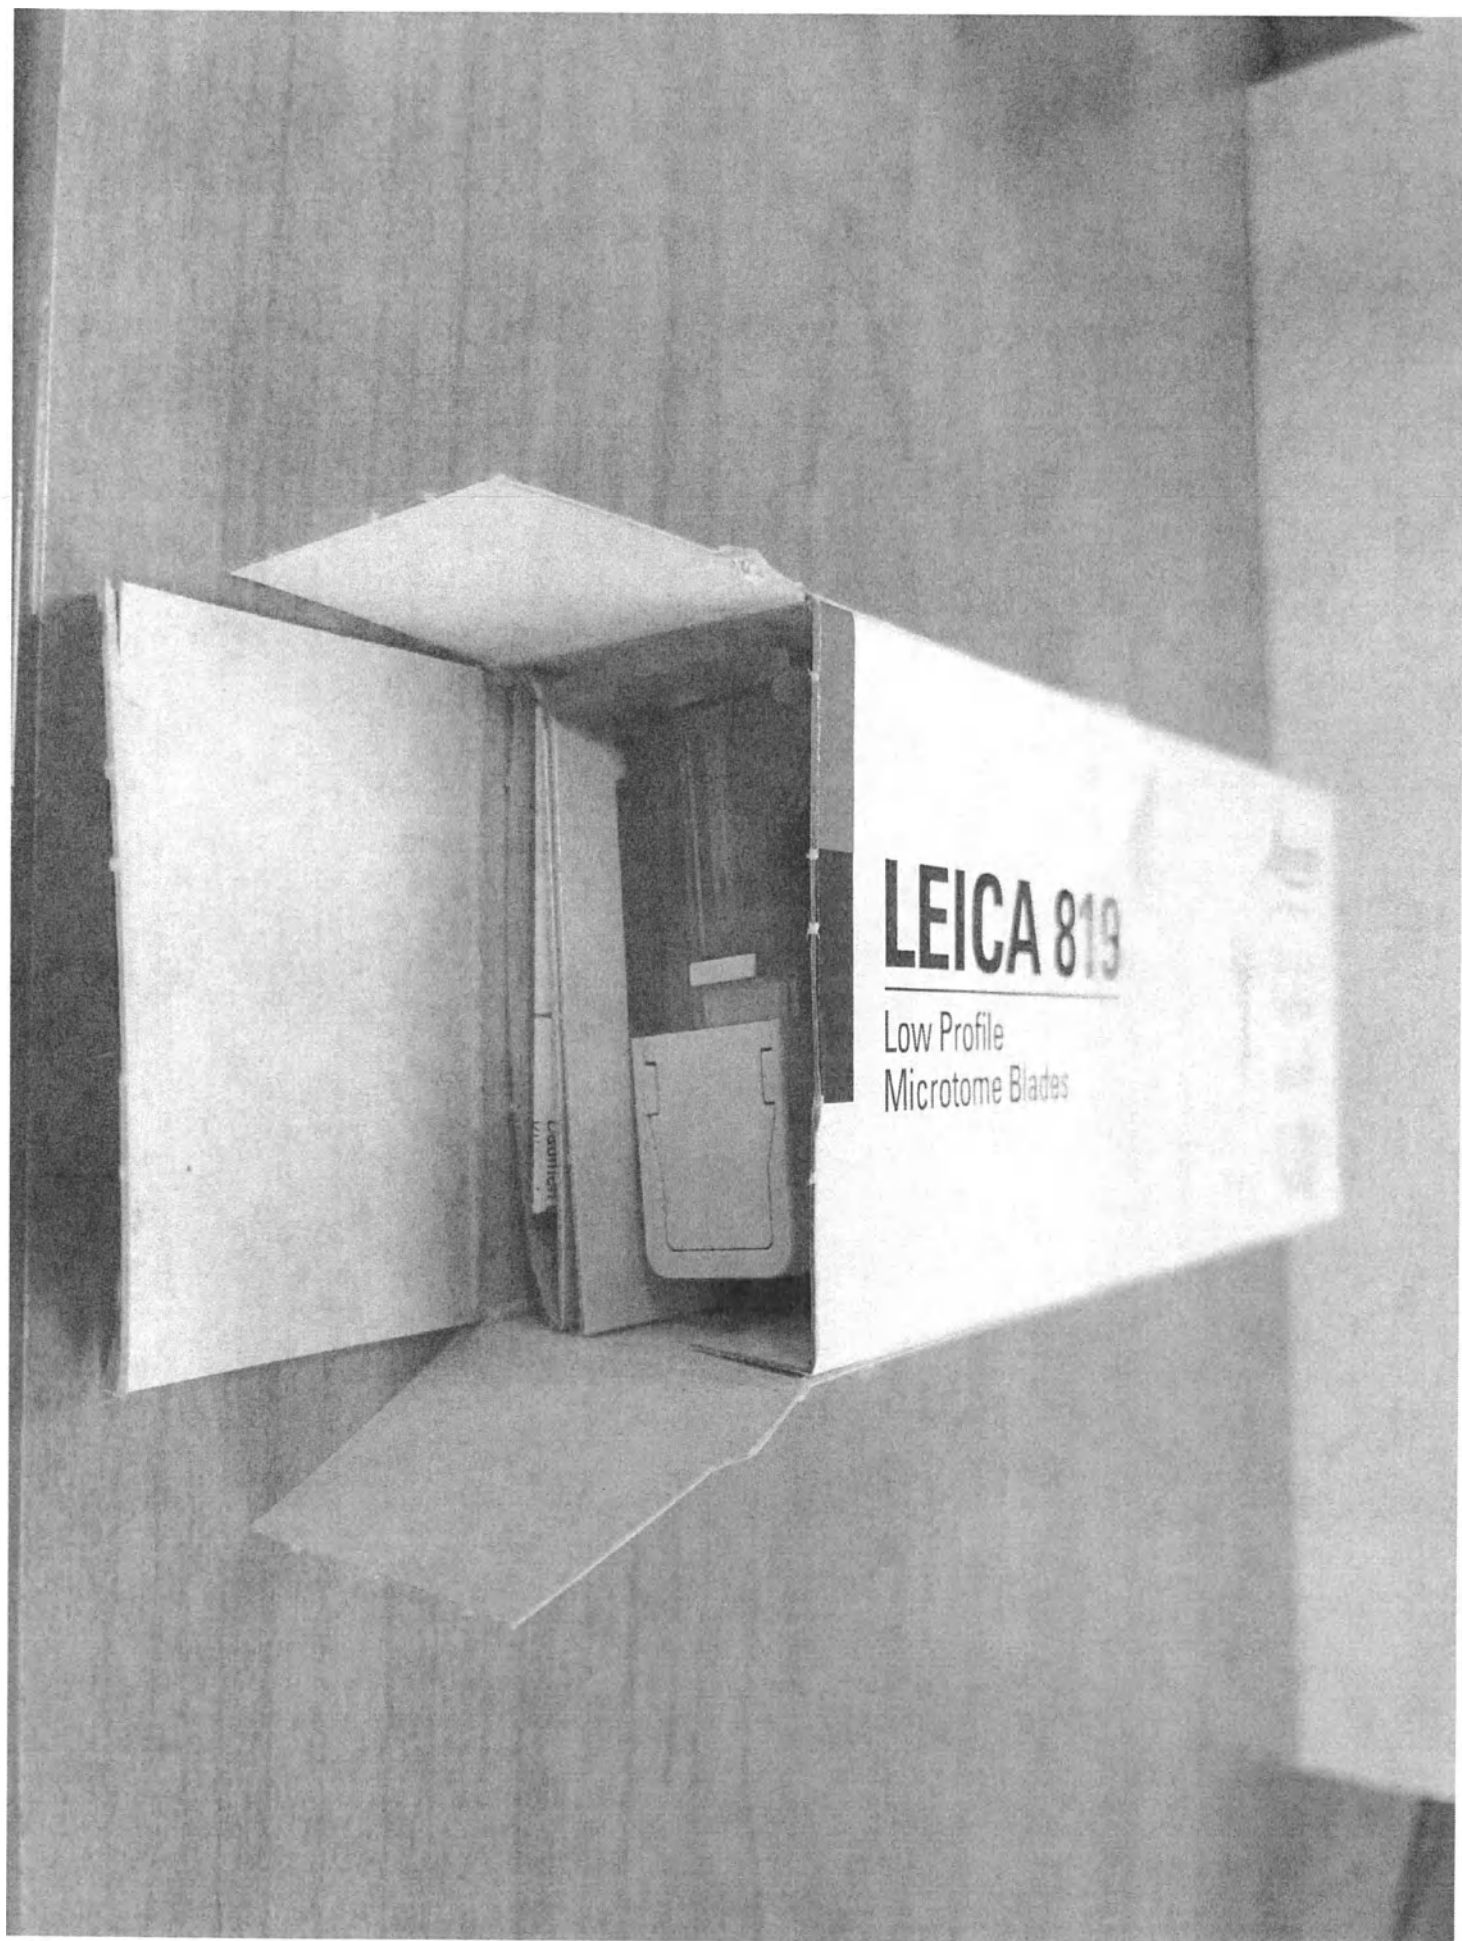





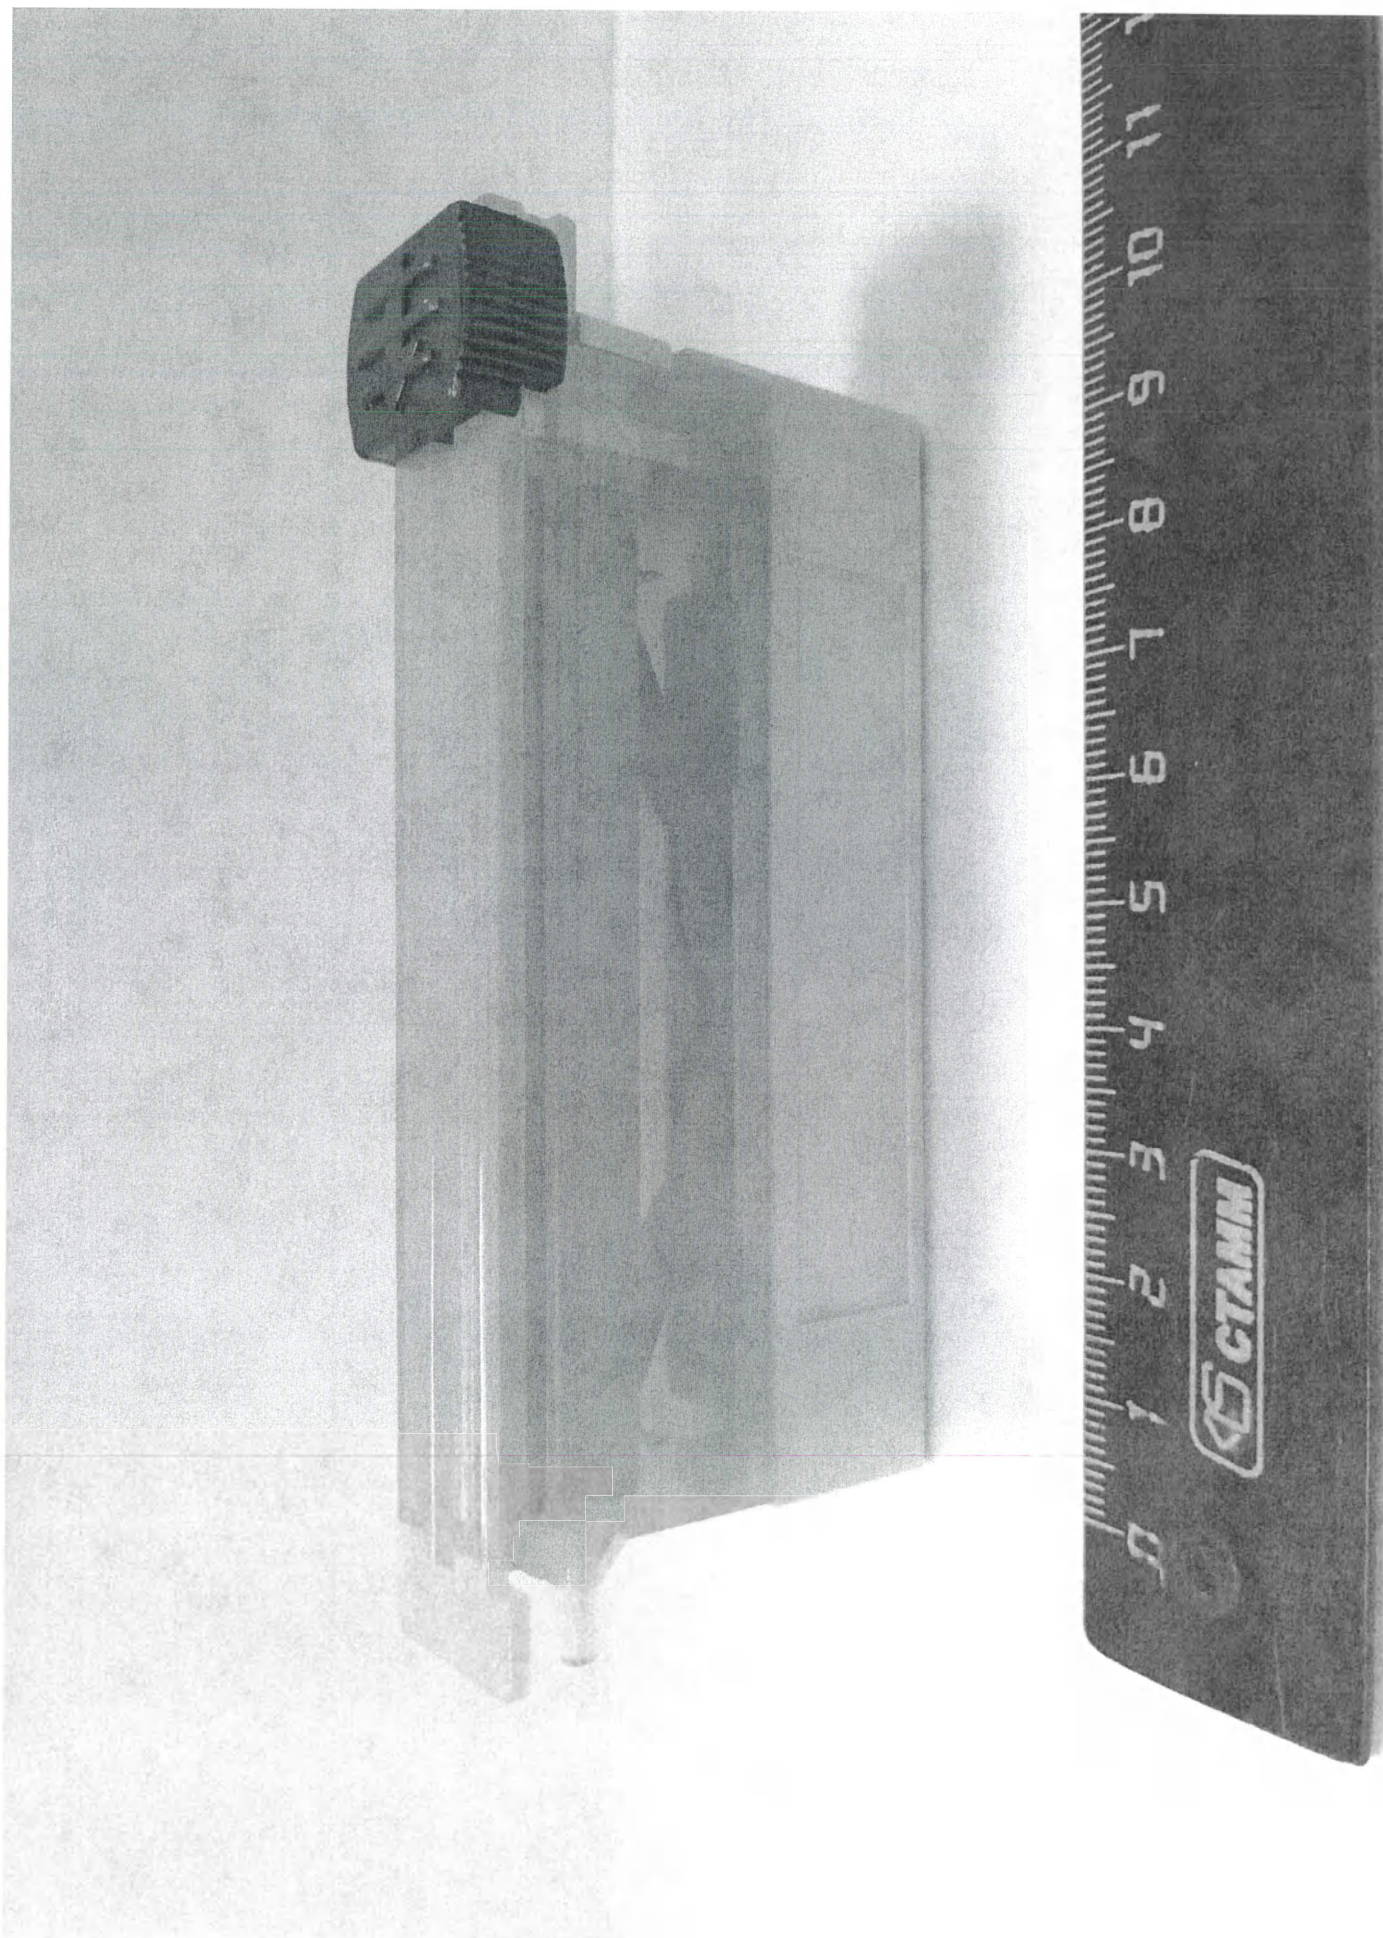


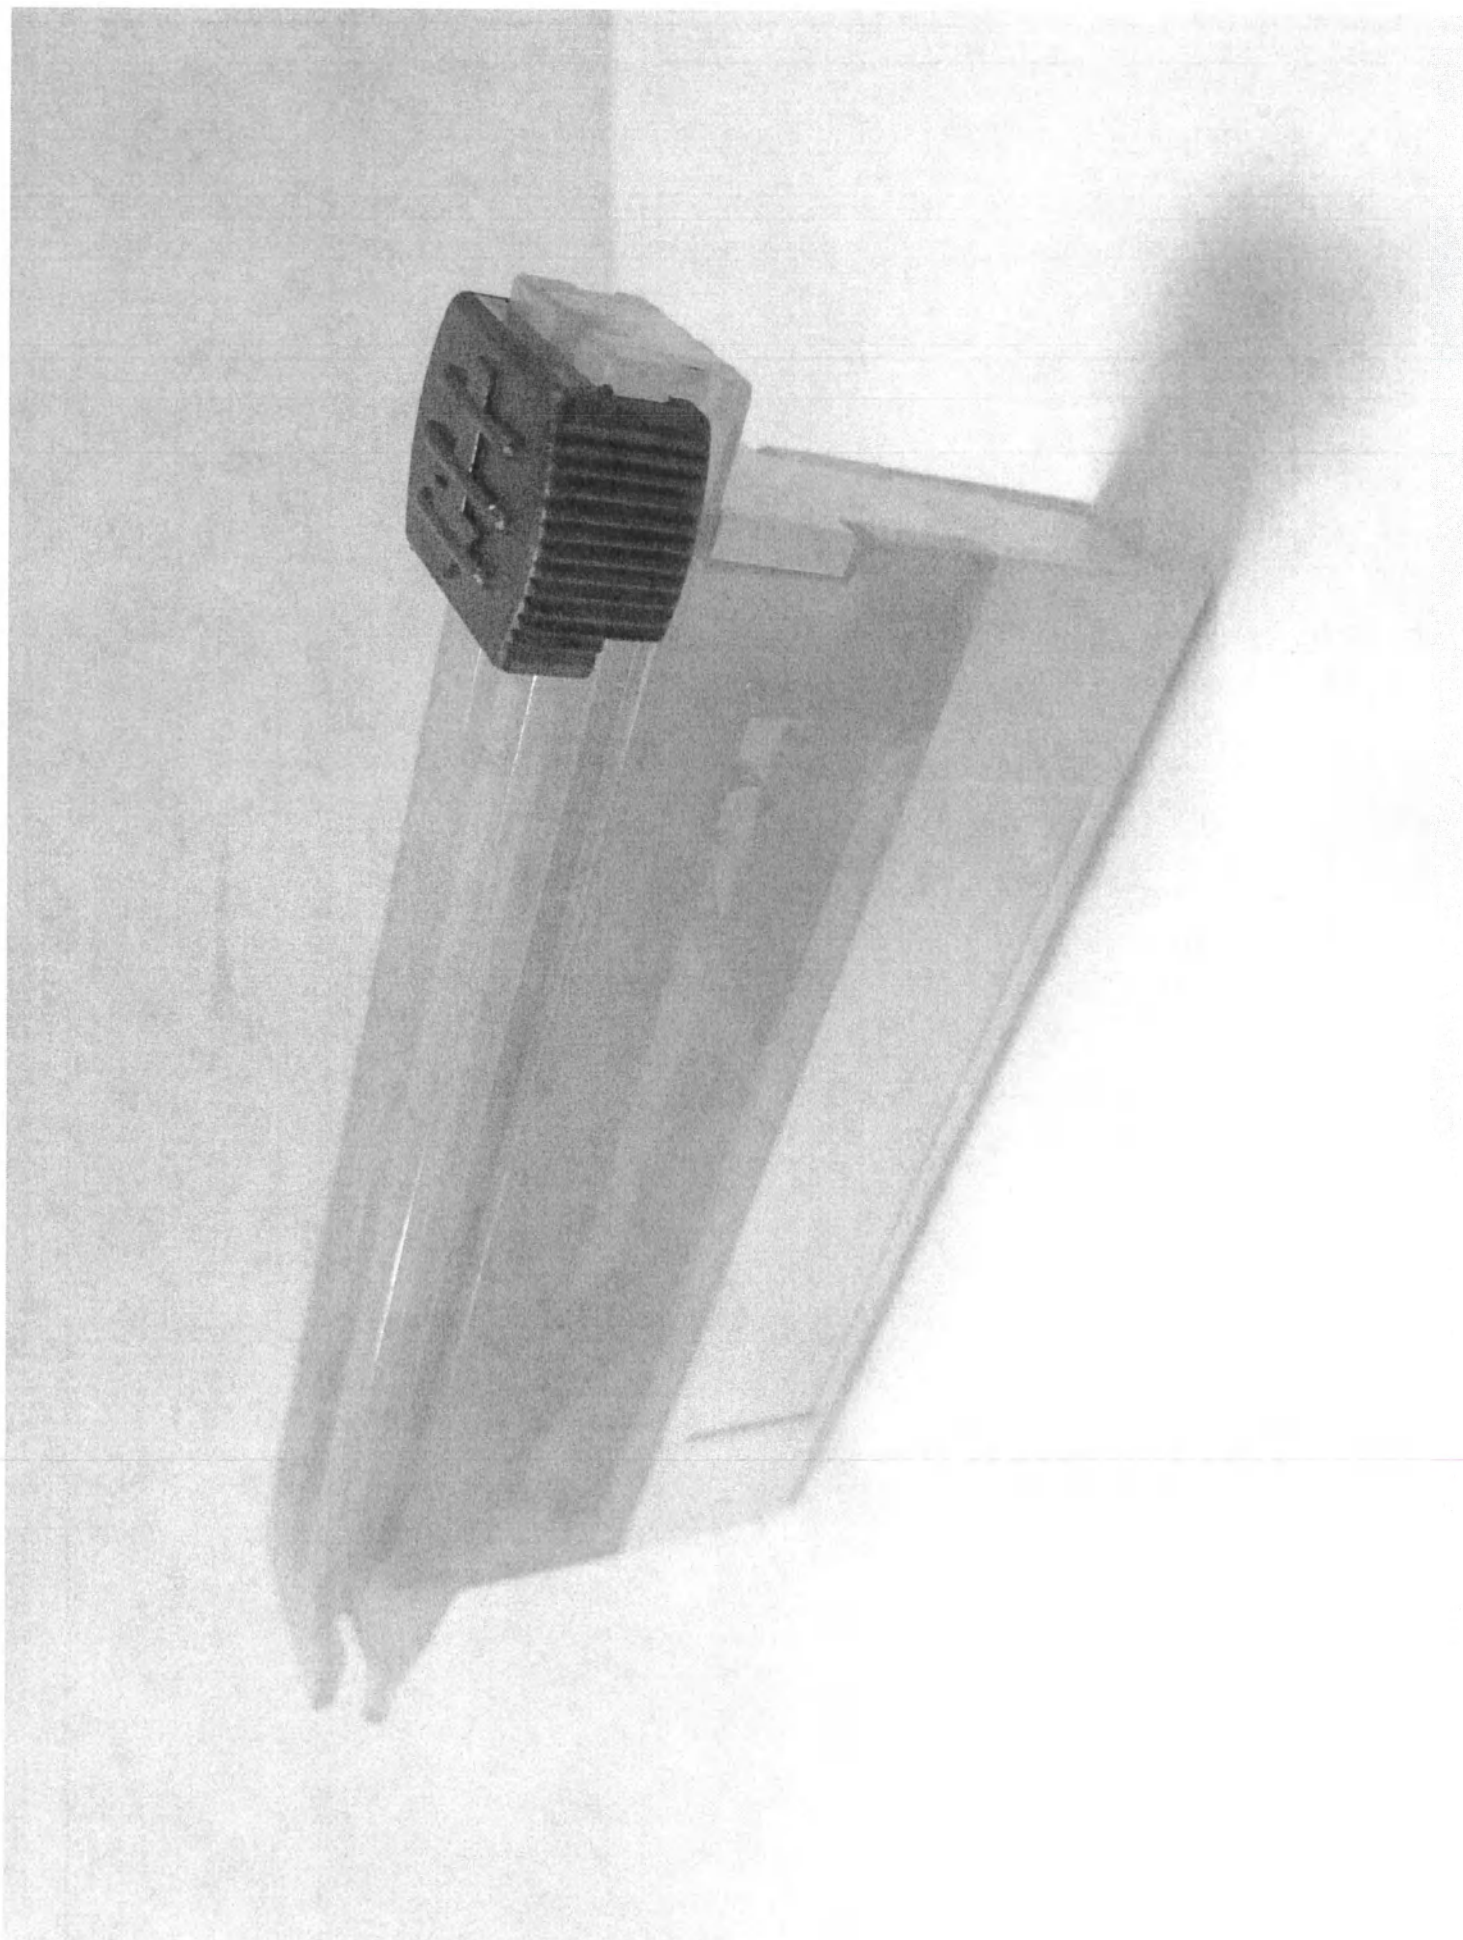


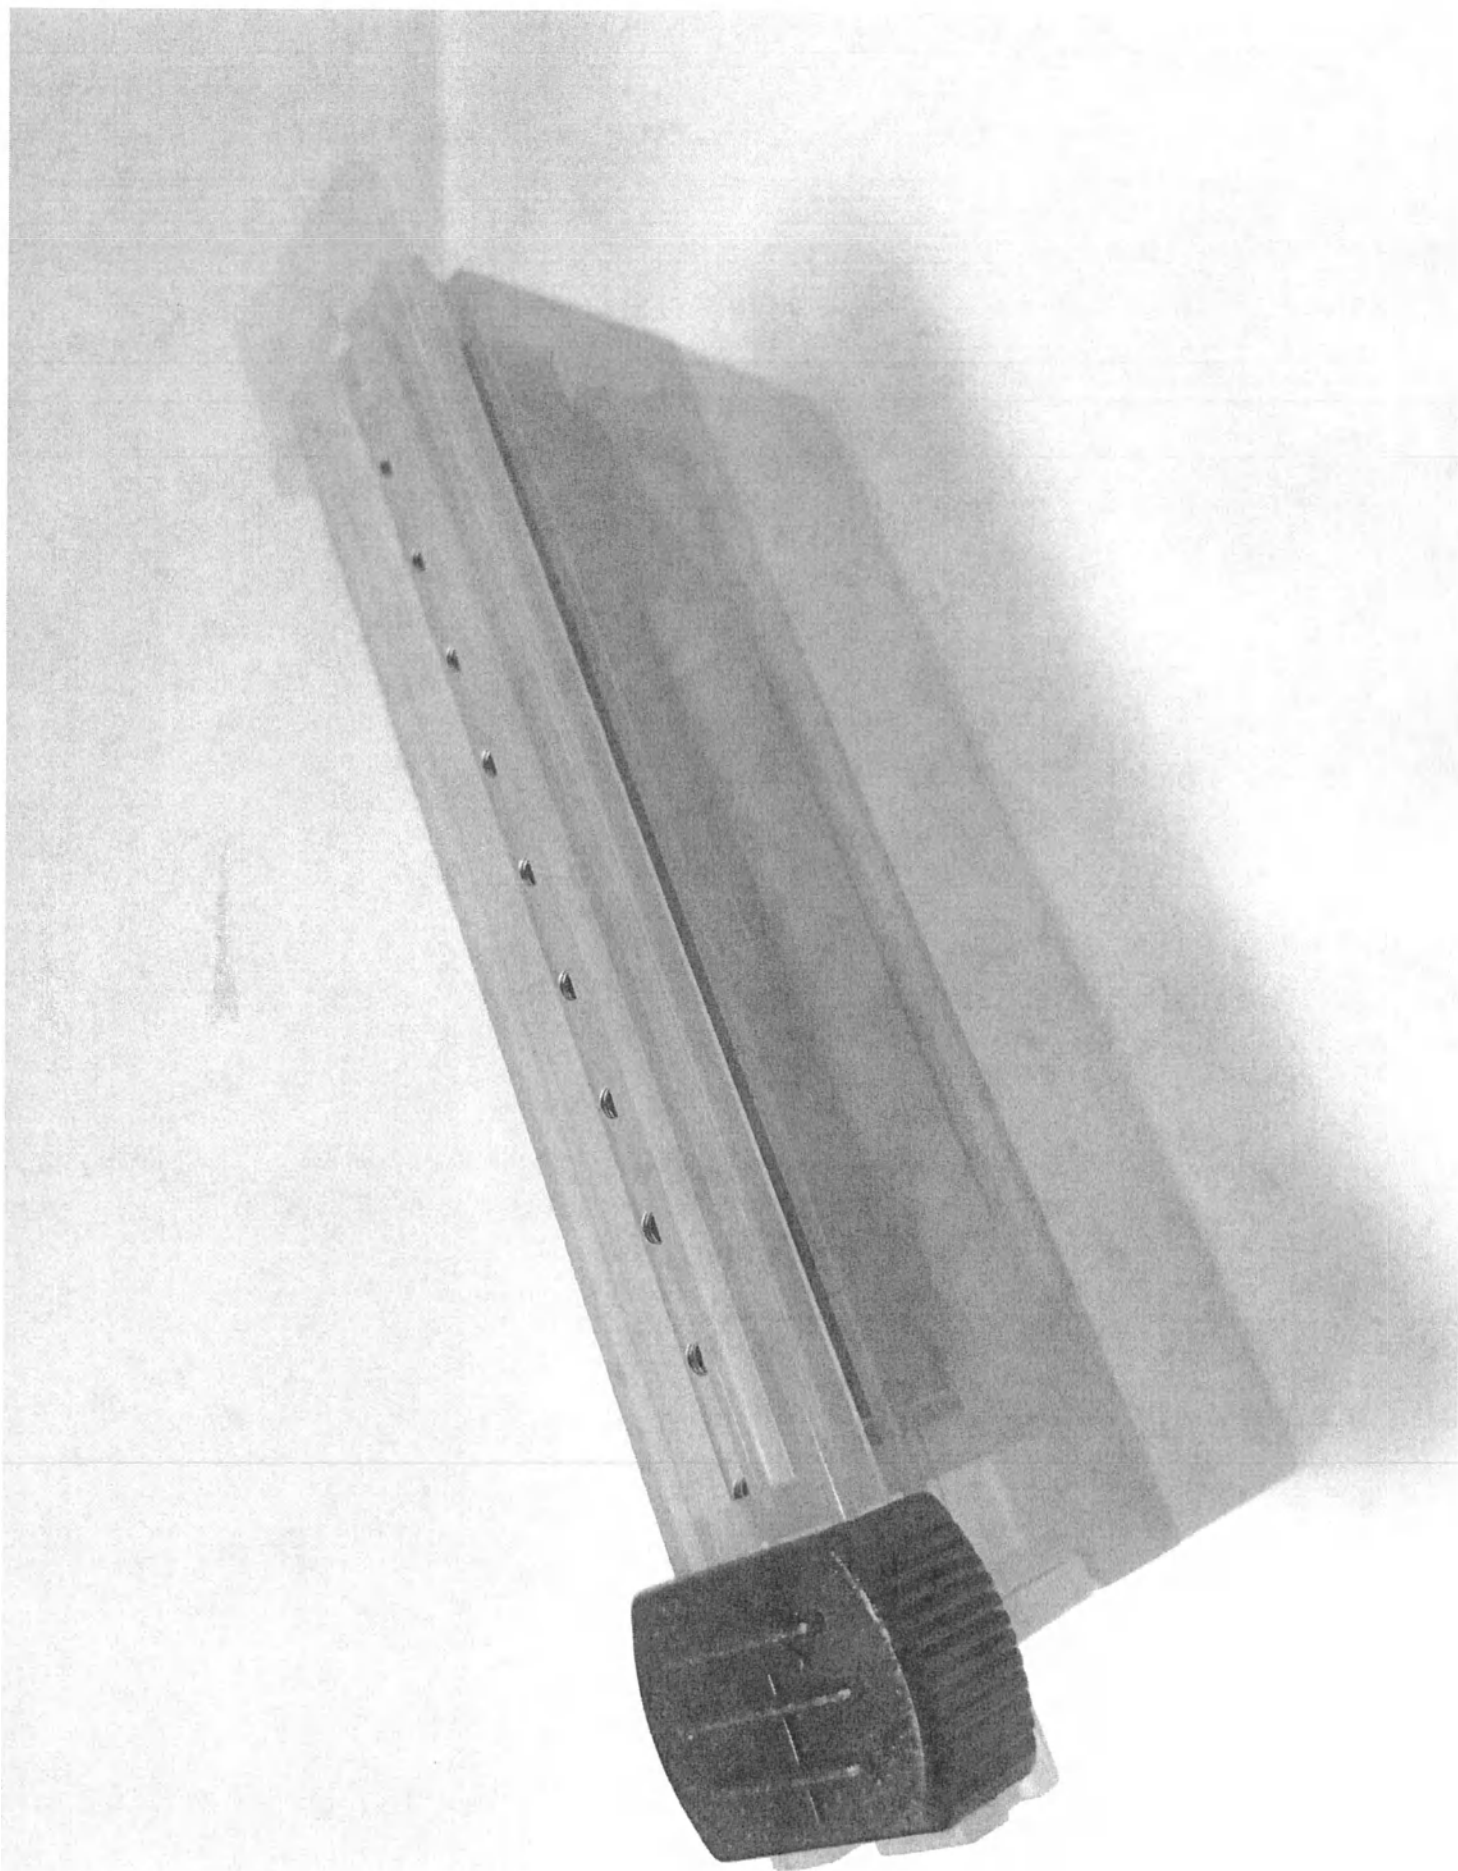



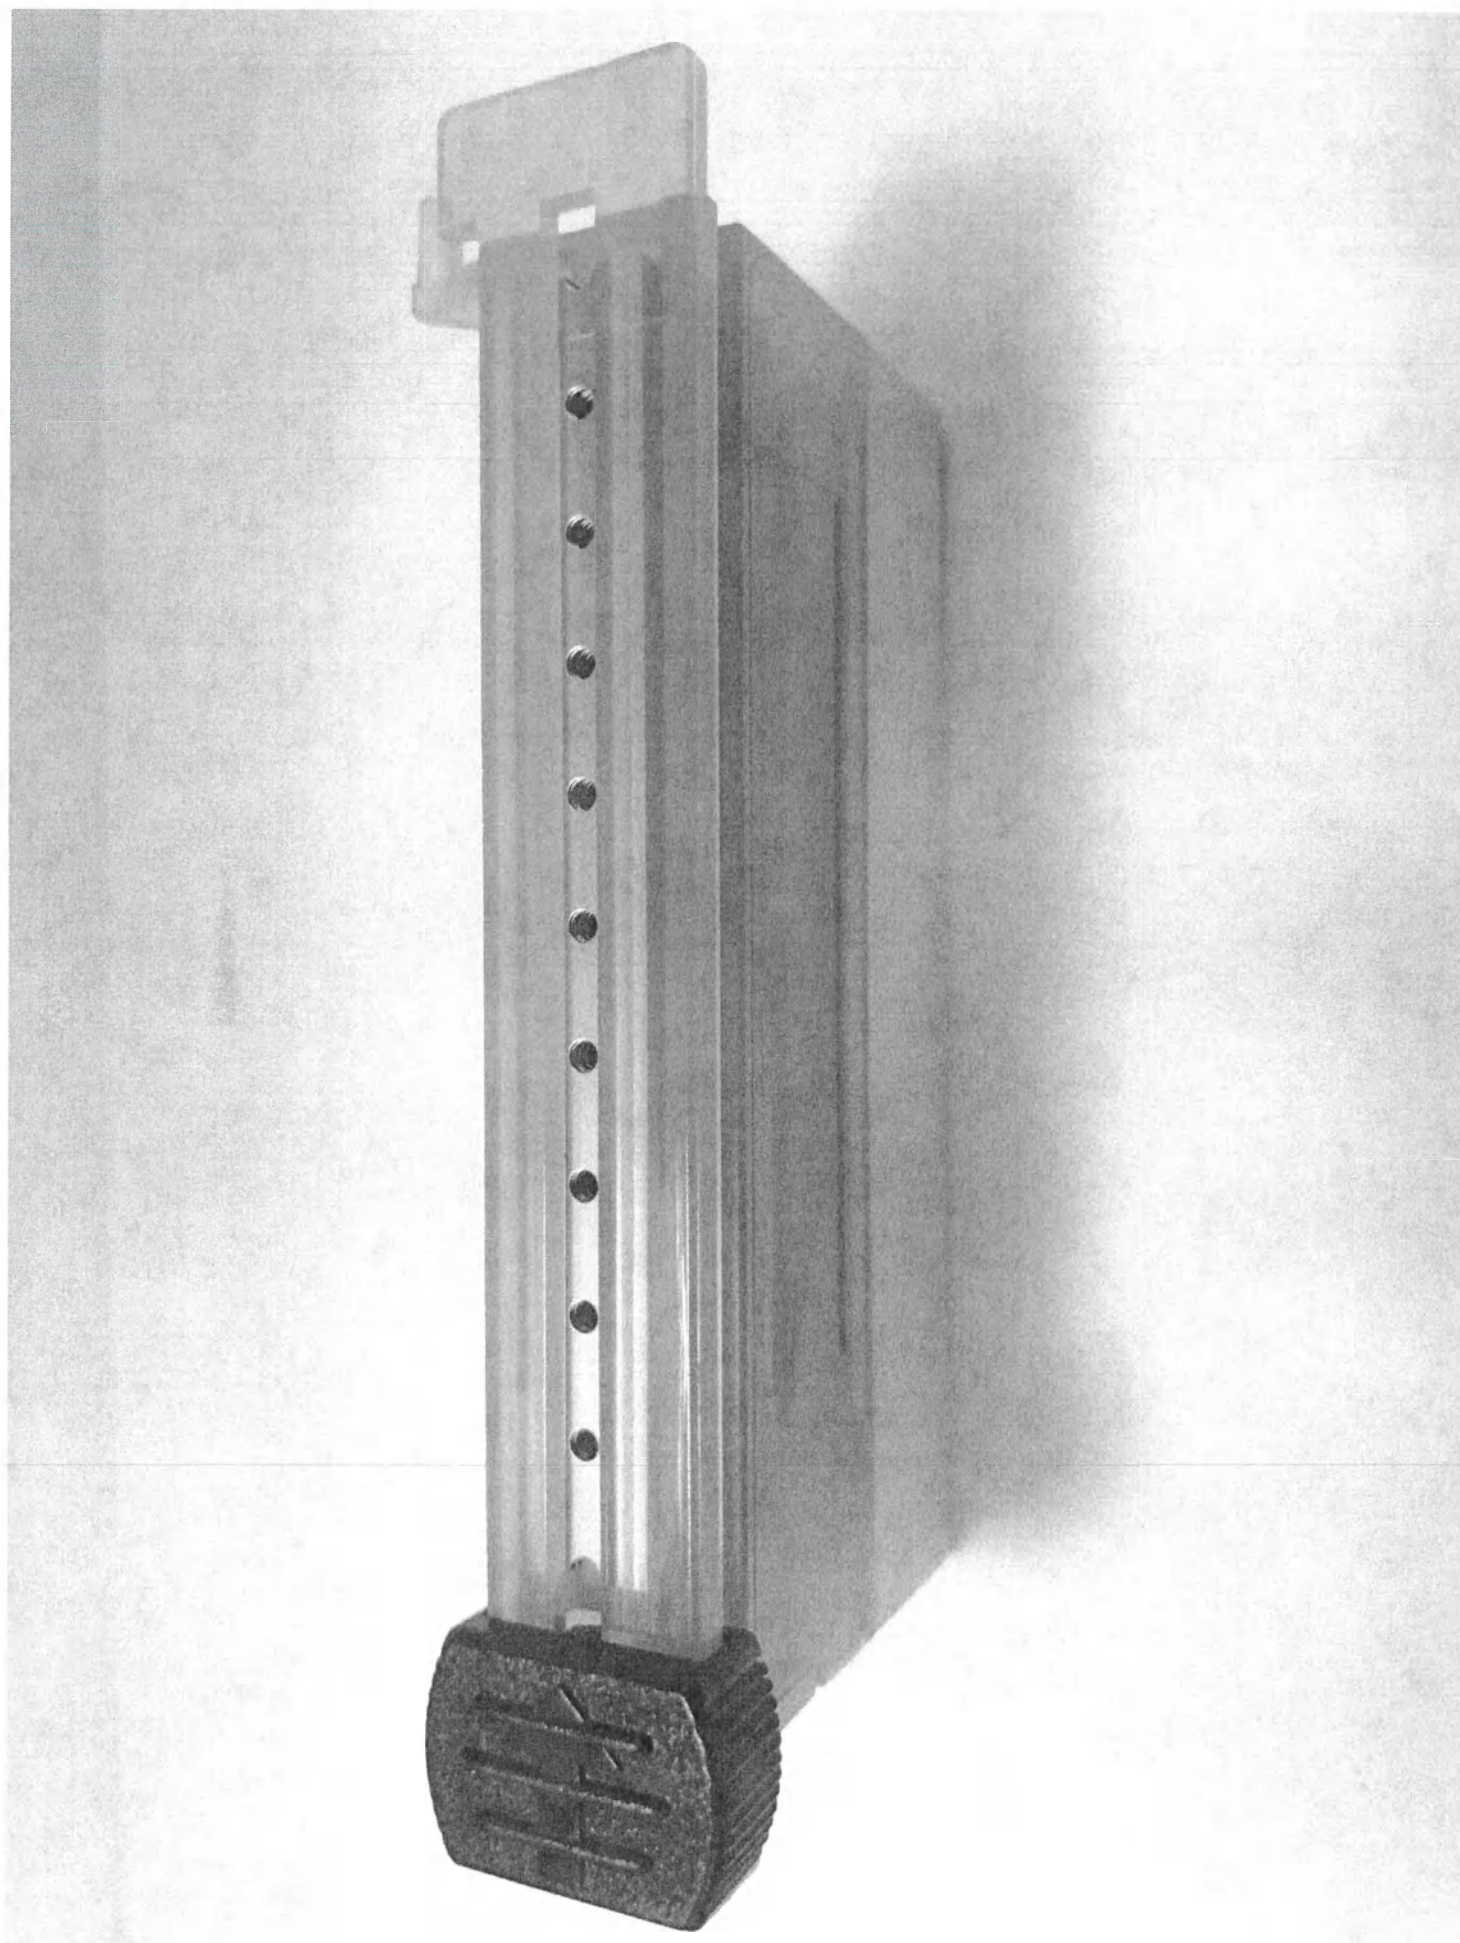


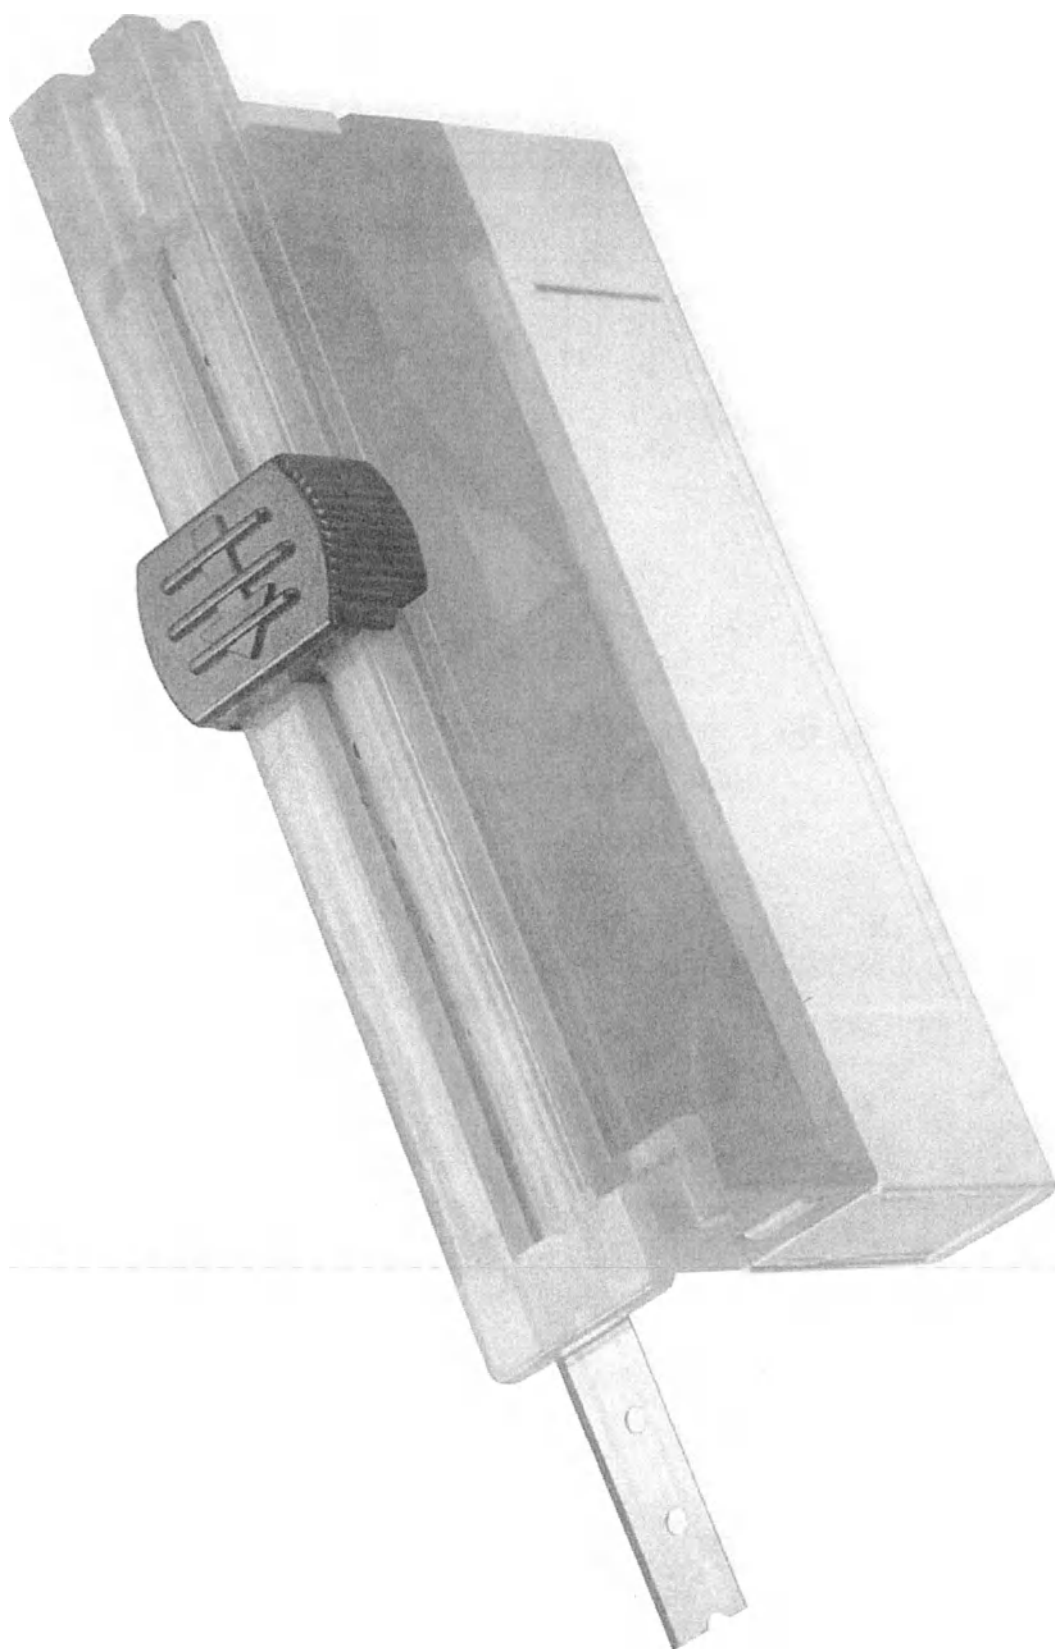

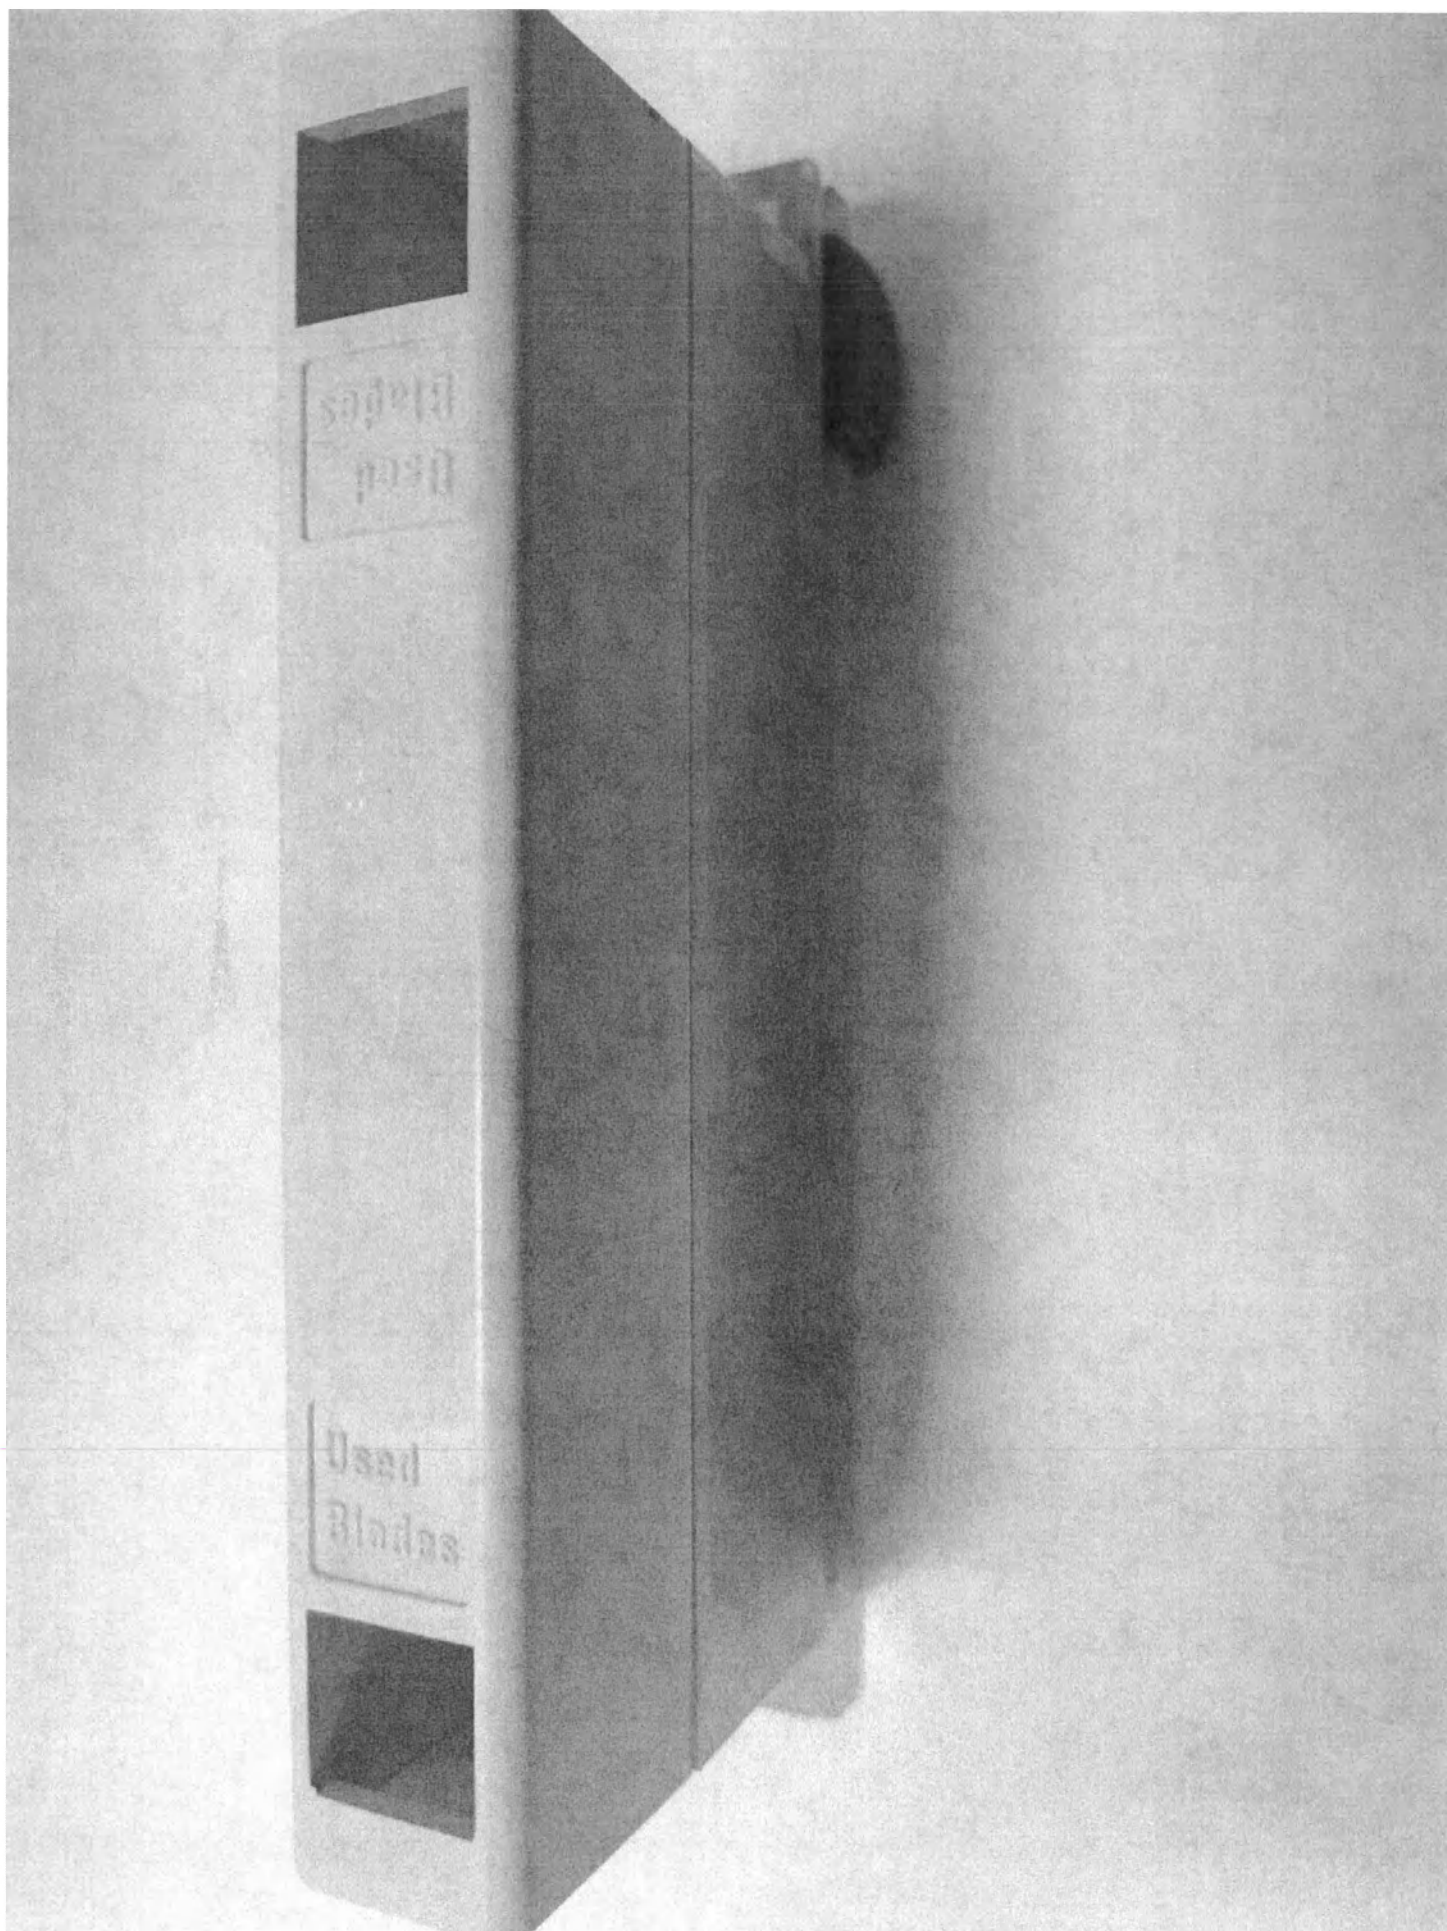


**Лезвия микротомные одноразовые высокого профиля Leica 818
(Leica 818 High Profile Microtome Blades)**

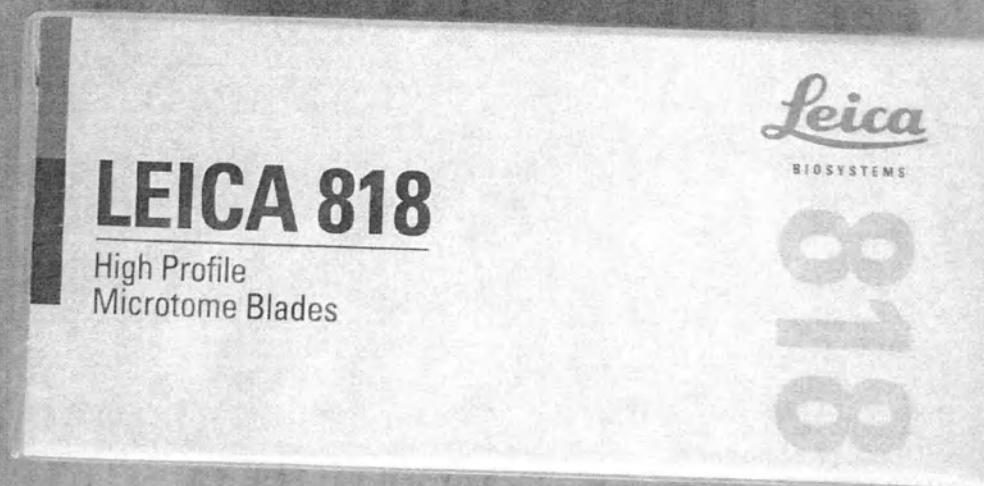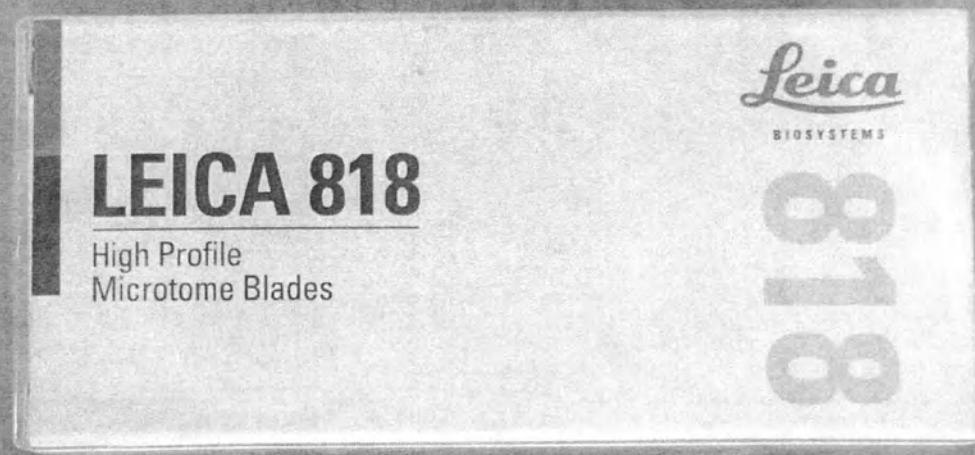

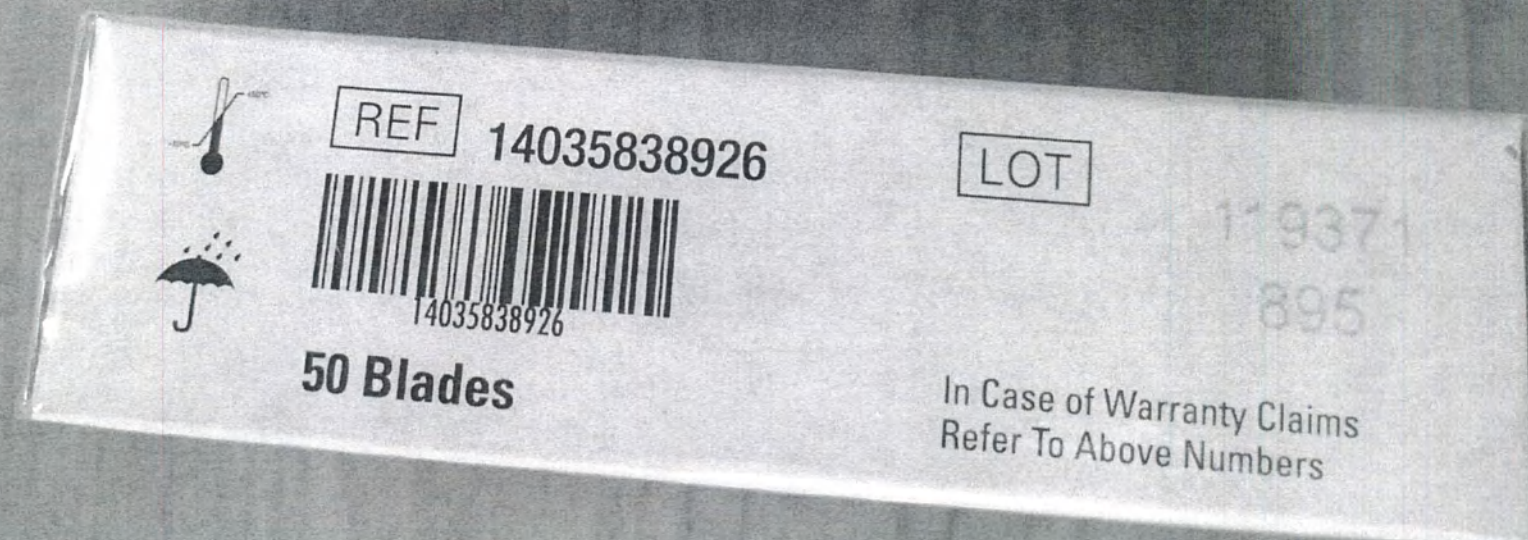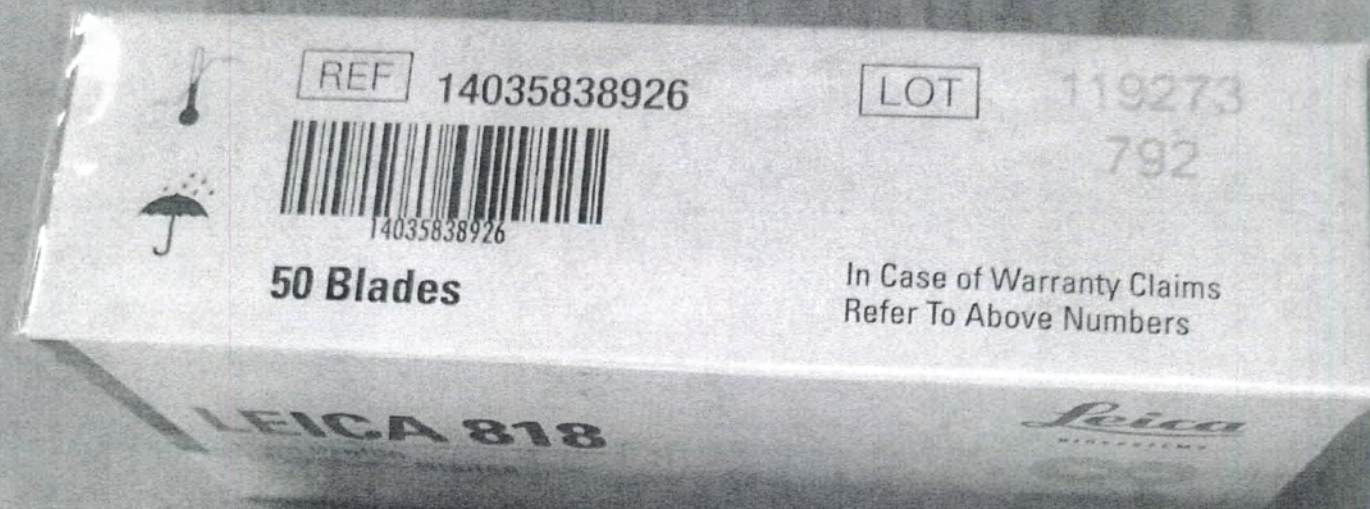



REF 14035838926



14035838926

50 Blades

LOT


119273
792


In Case of Warranty Claims
Refer To Above Numbers

LEICA 818

High Profile
Microtome Blades

Leica
BIO SYSTEMS

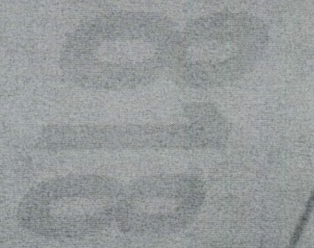


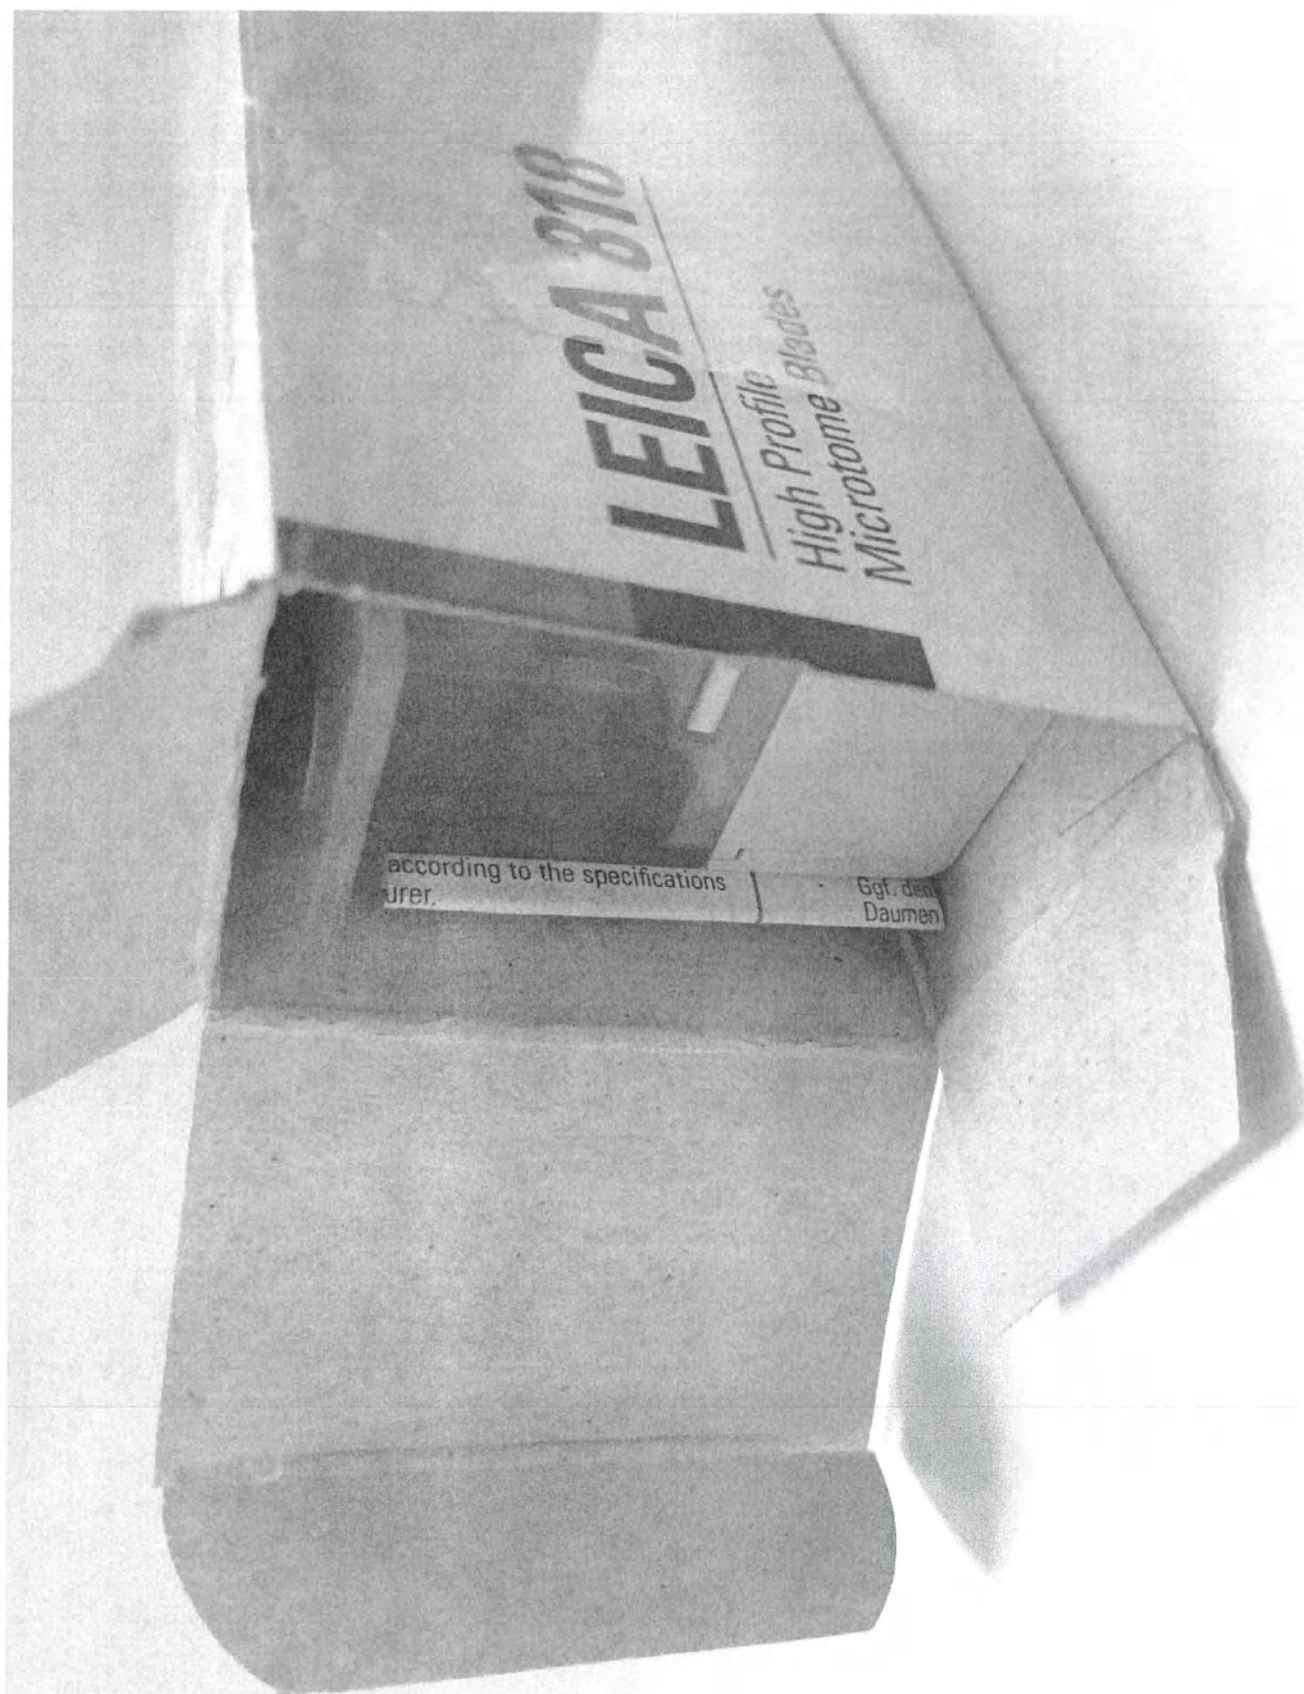






REF 14035838926
LOT 3273
792
In Case of Warranty Claims
Refer To Above Numbers
50 Blades


LEICA 818
High Profile
Microtome Blades
Leica
BIOSYSTEMS

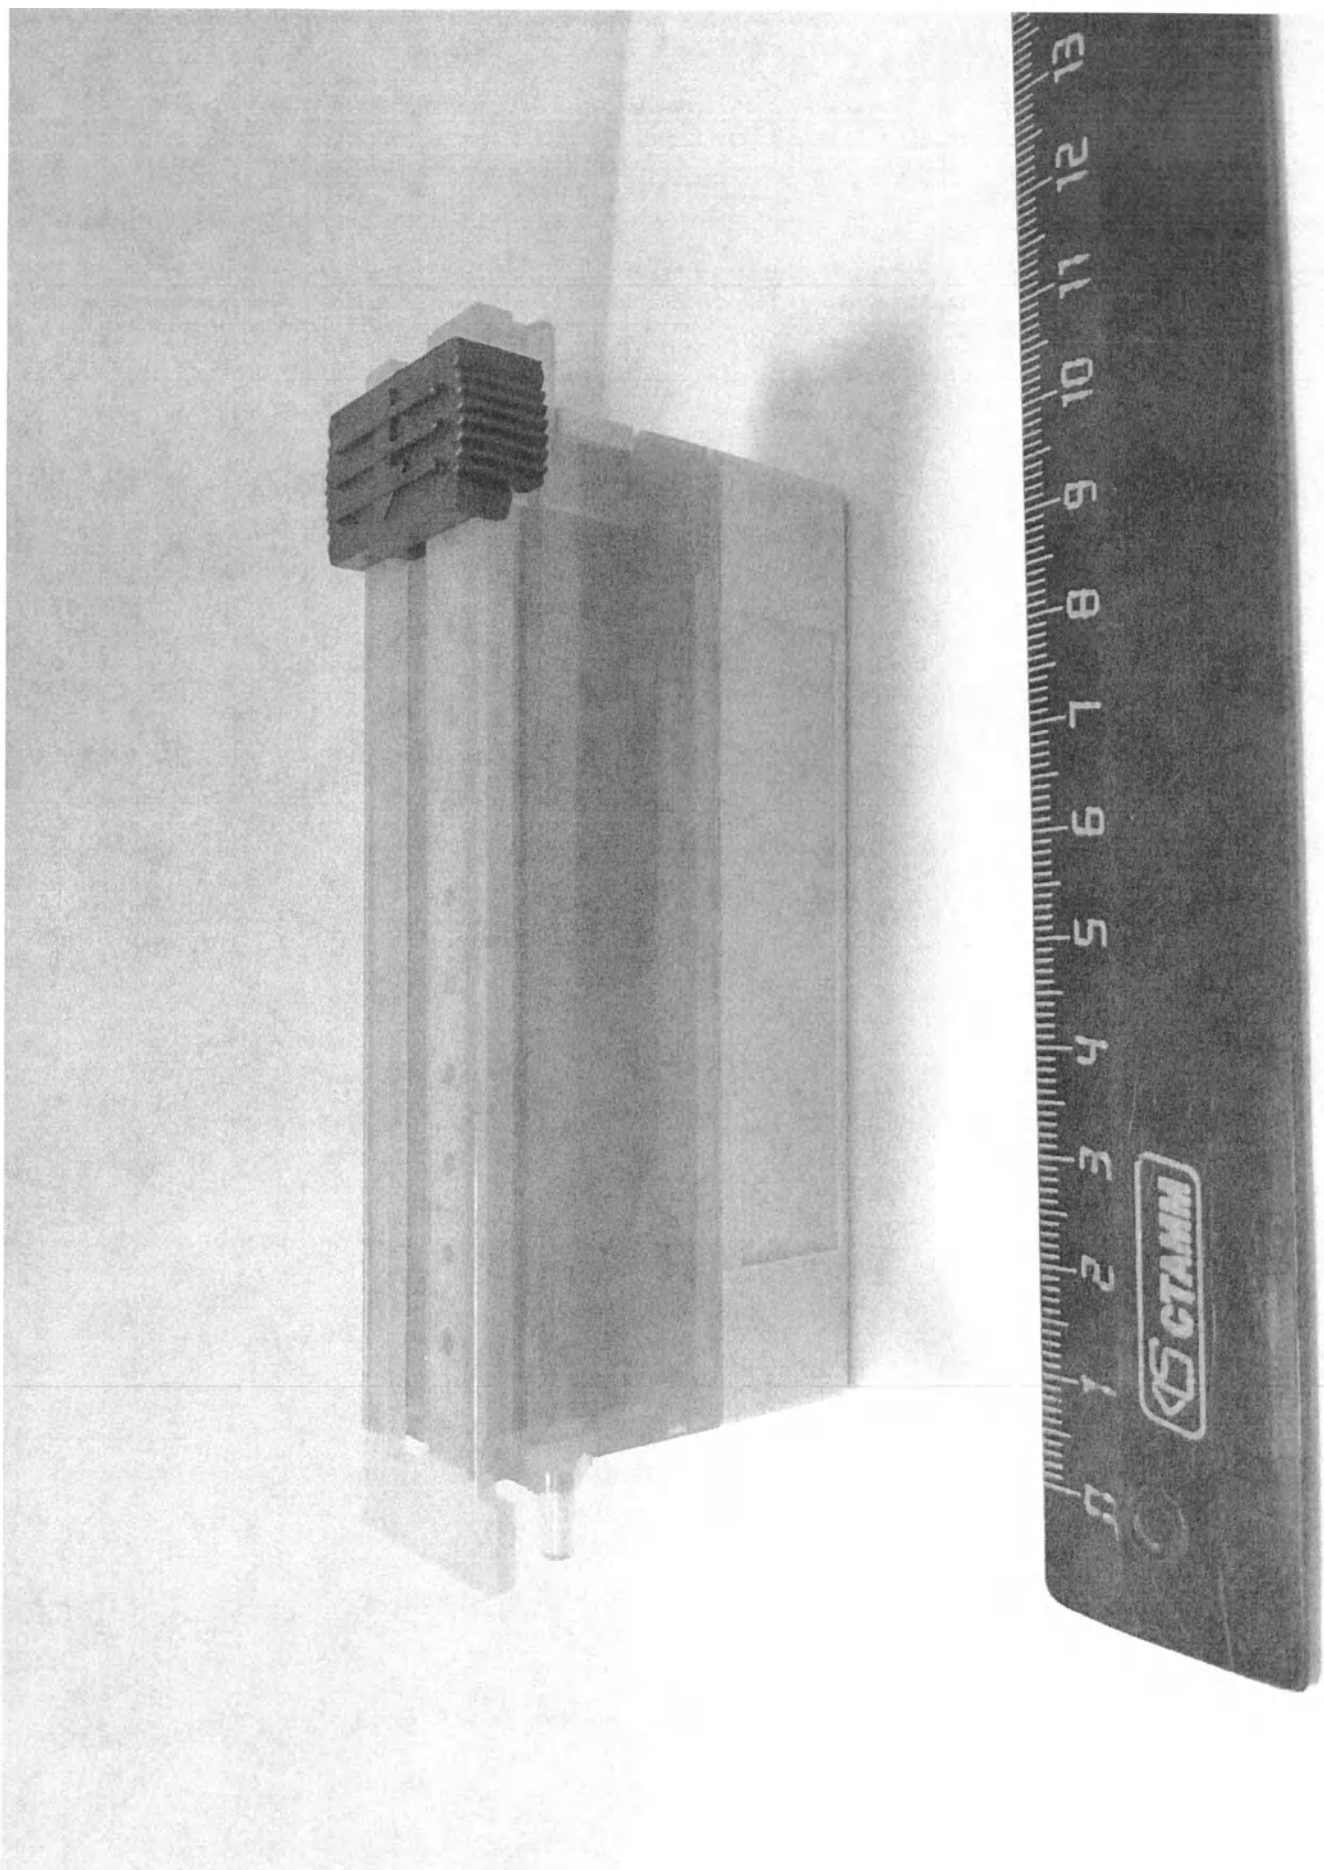


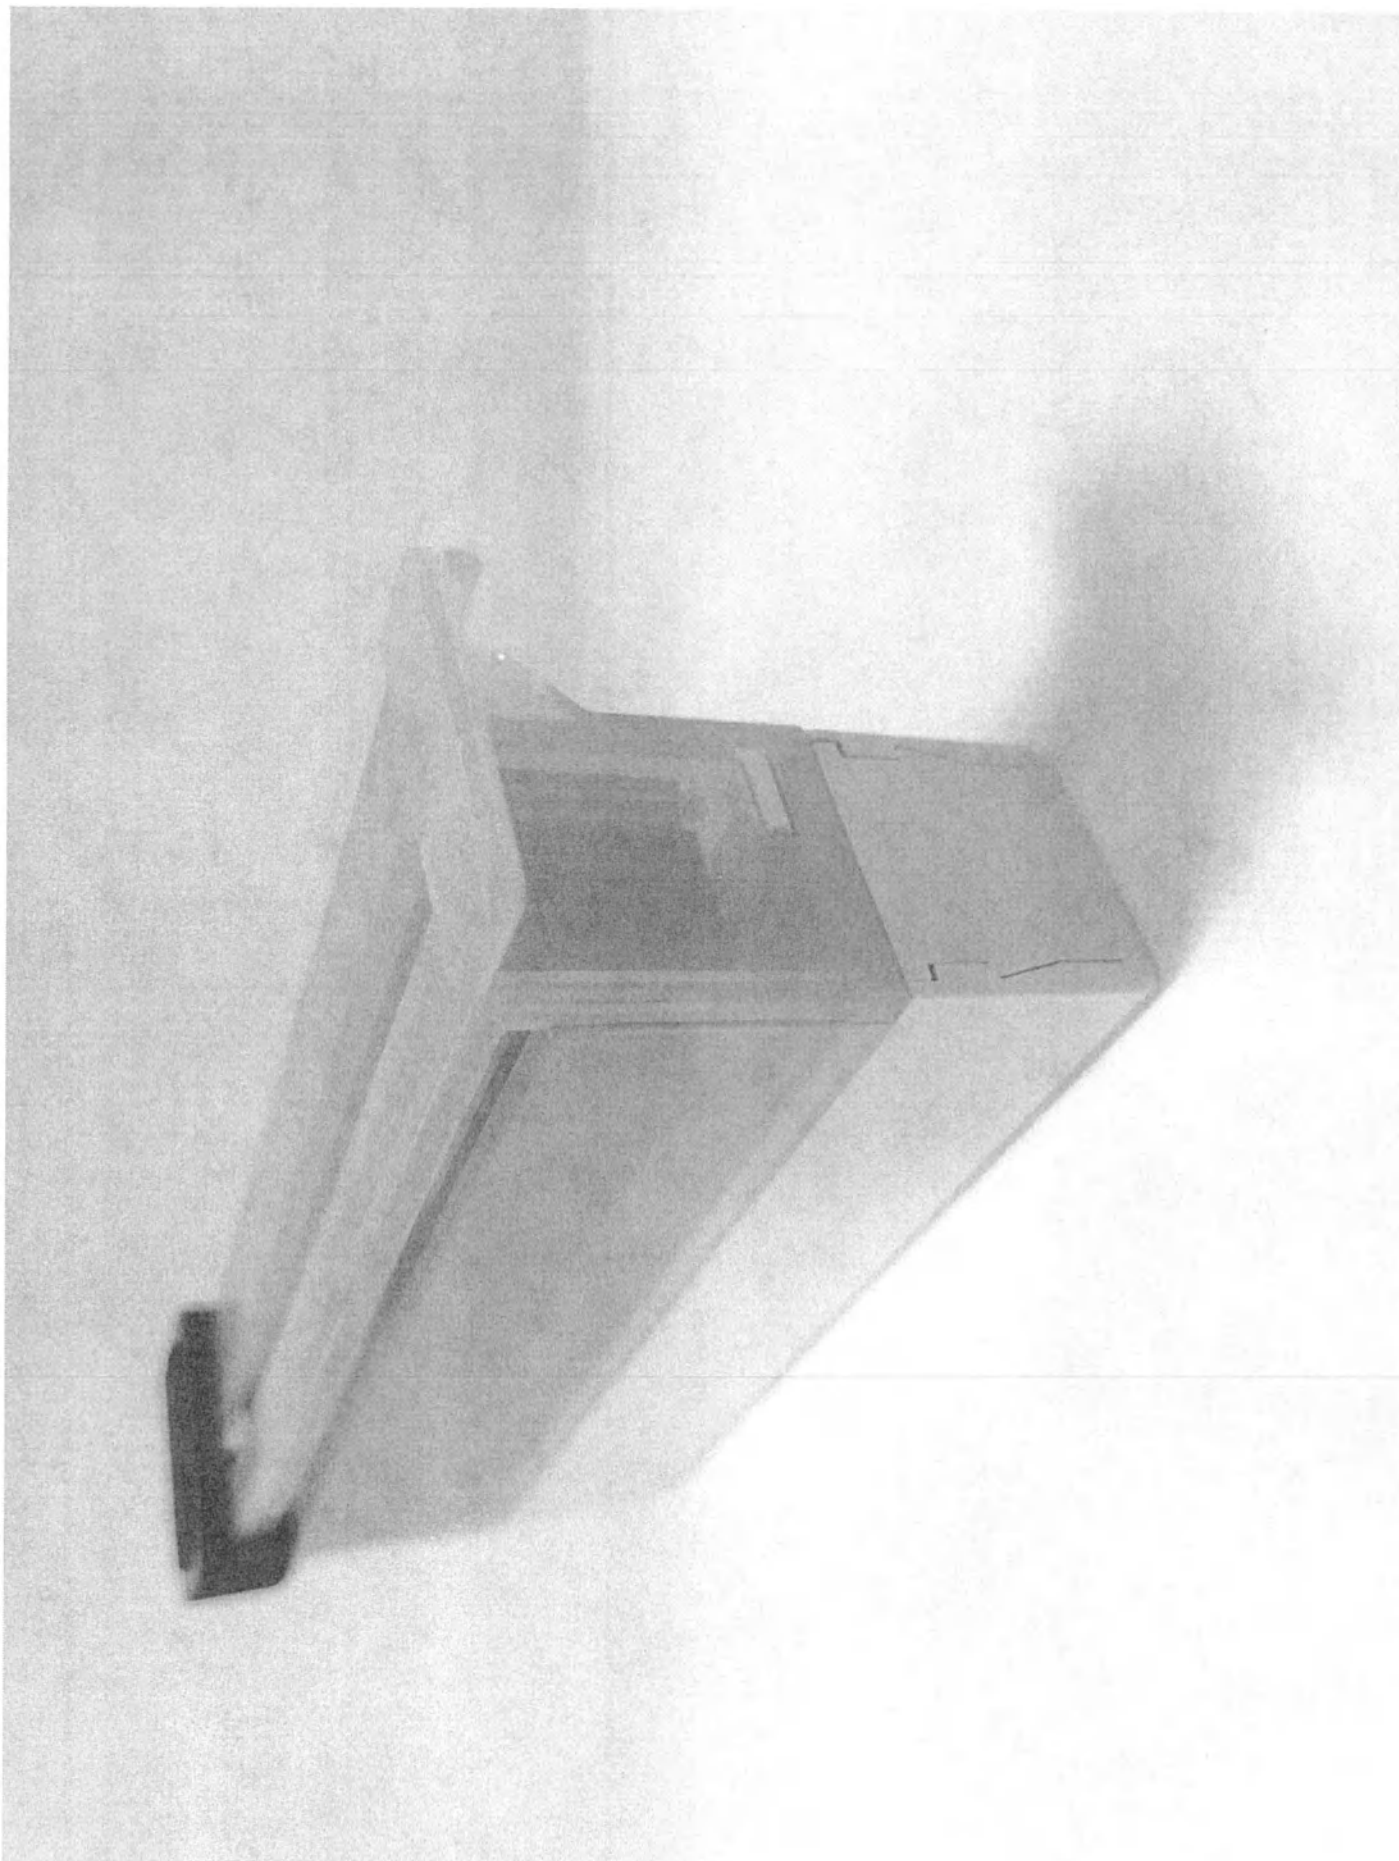


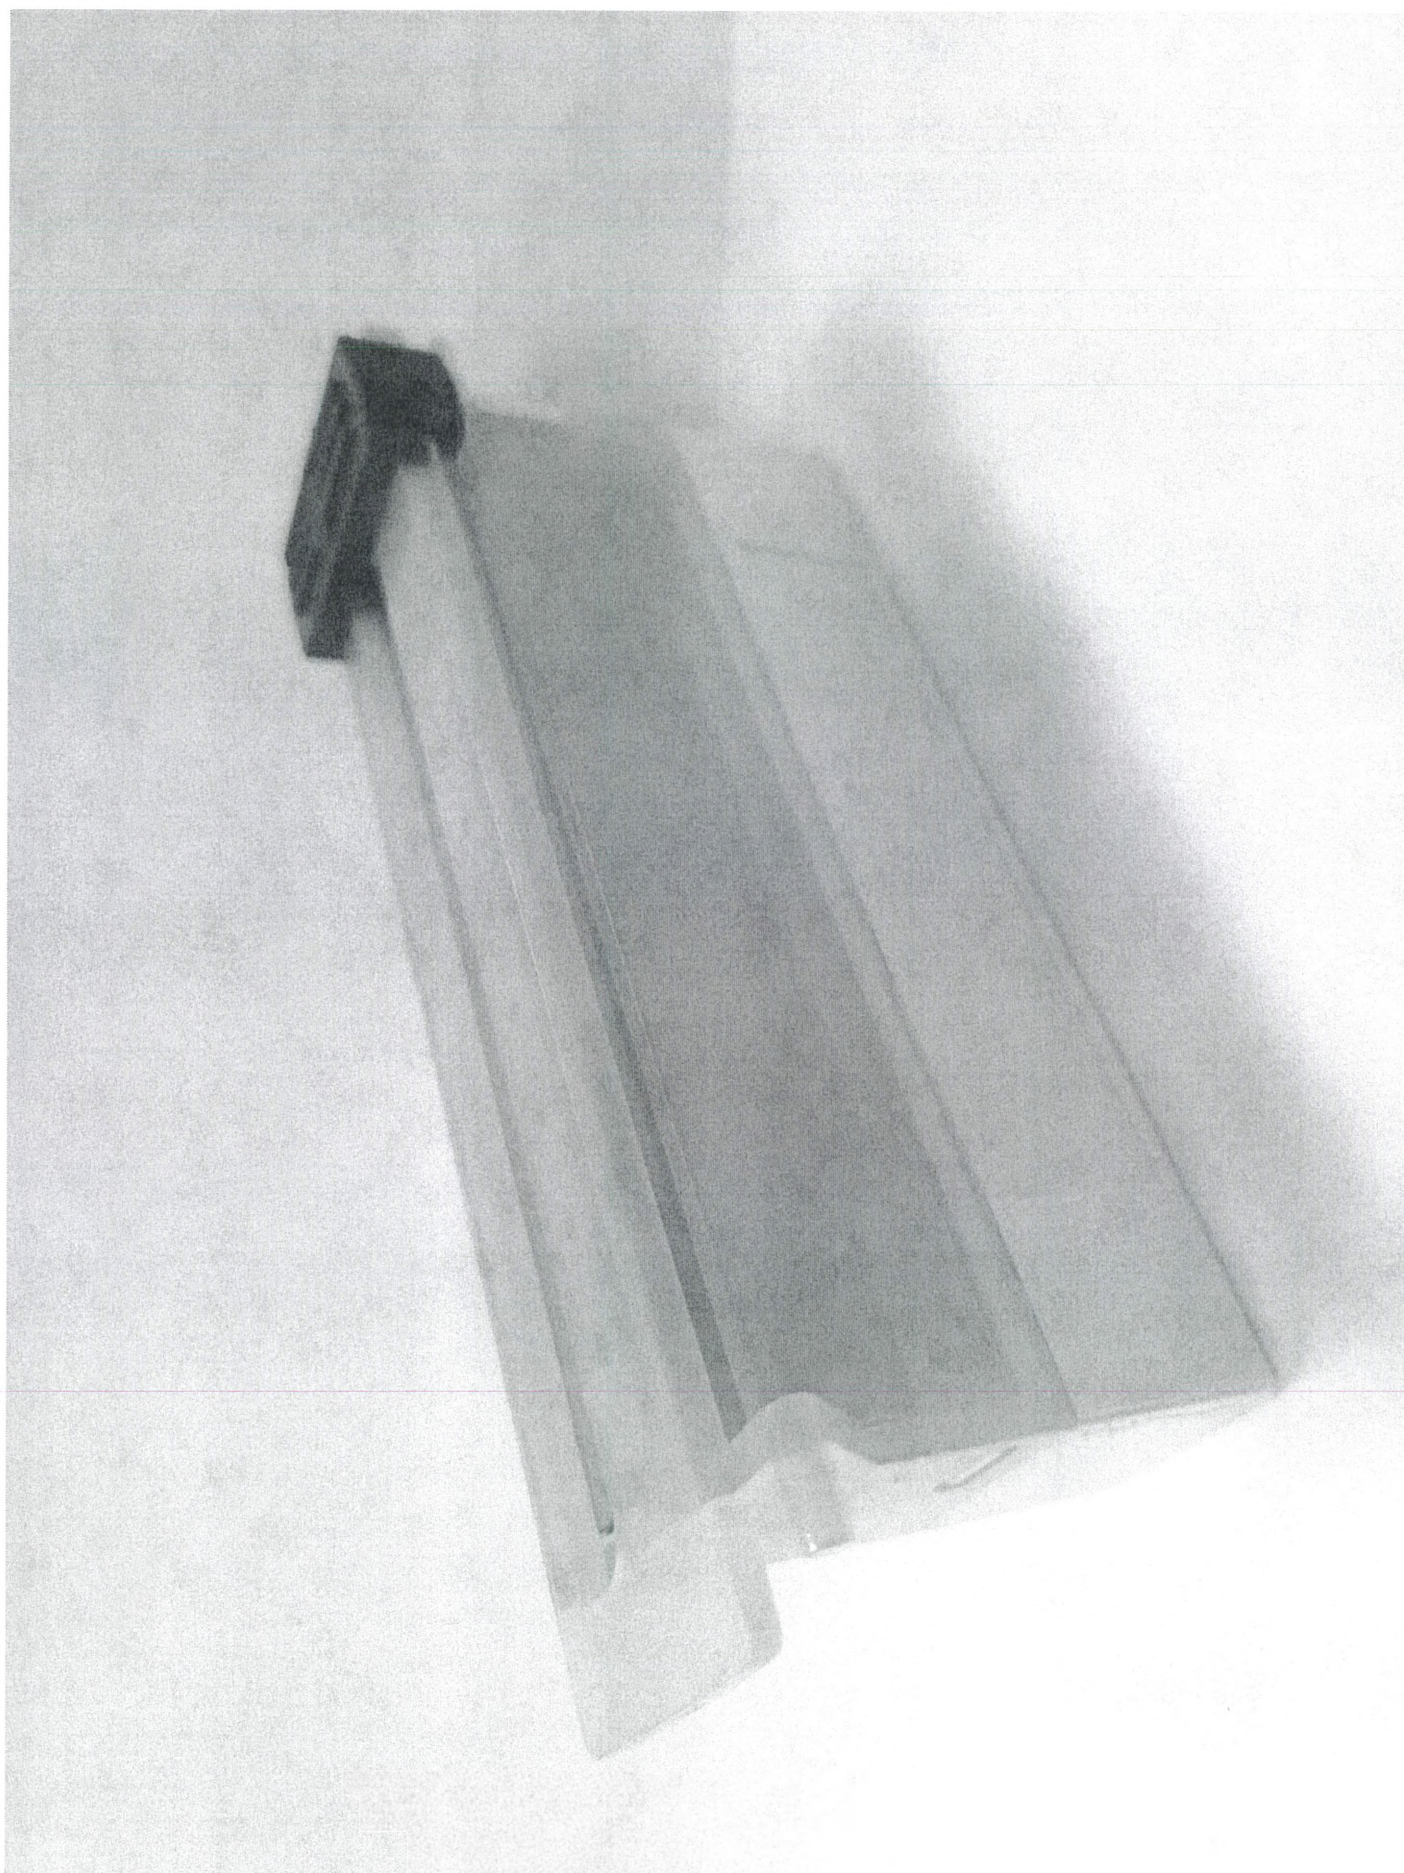



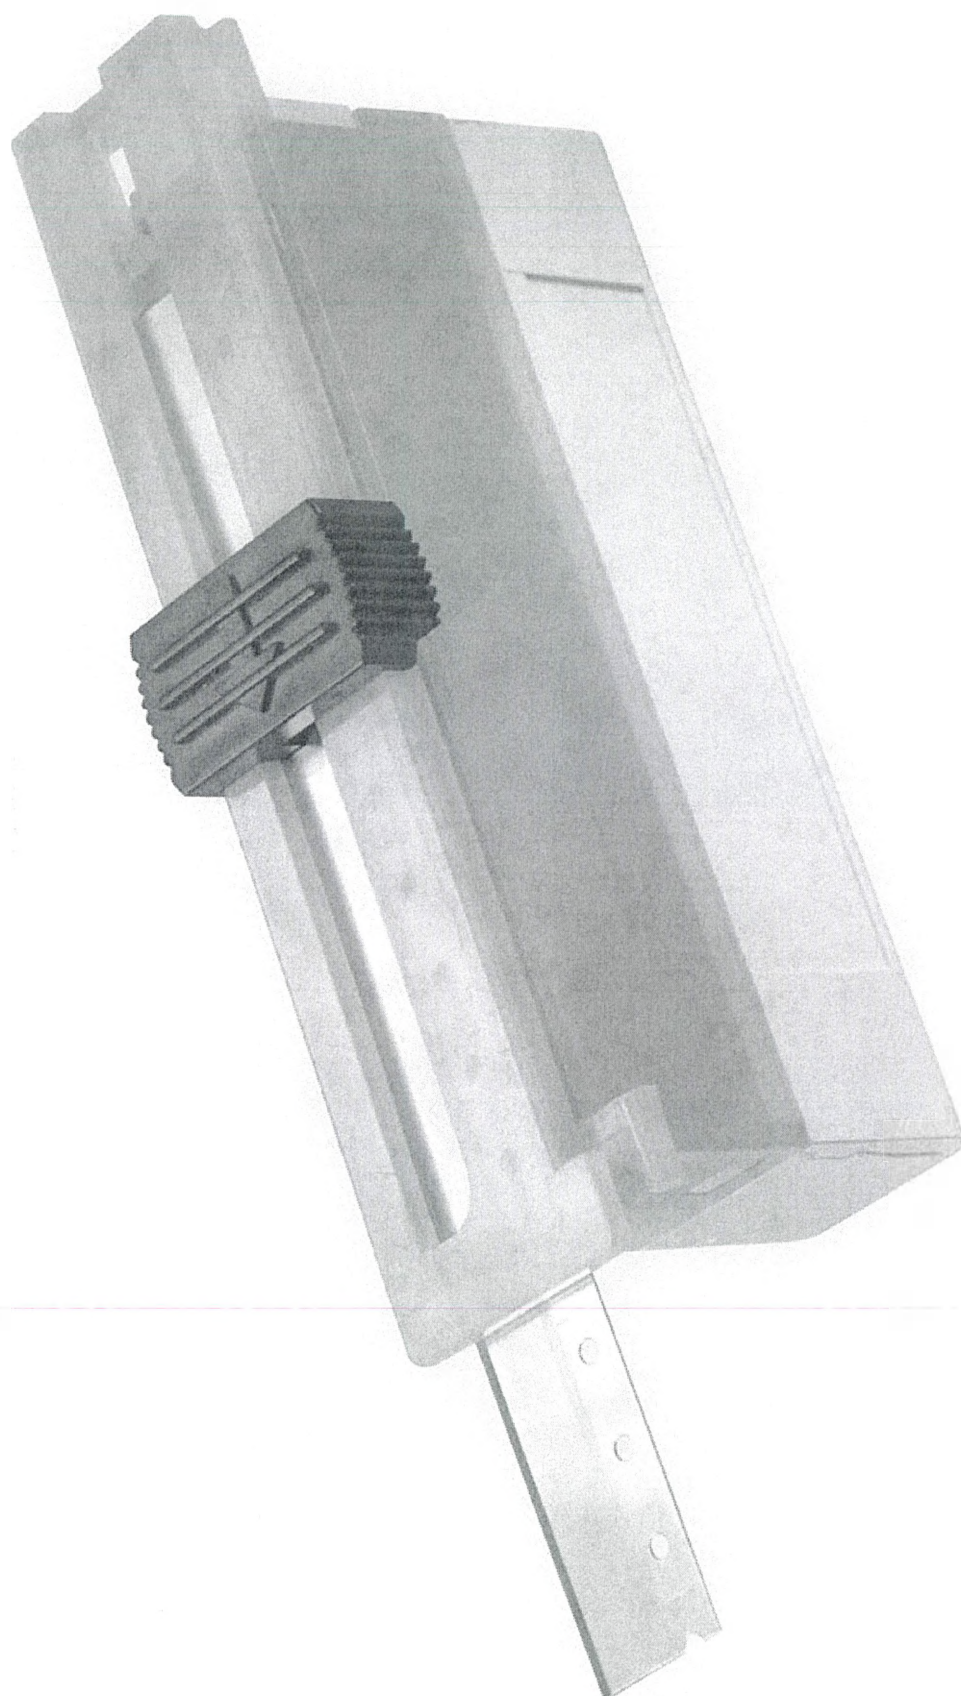


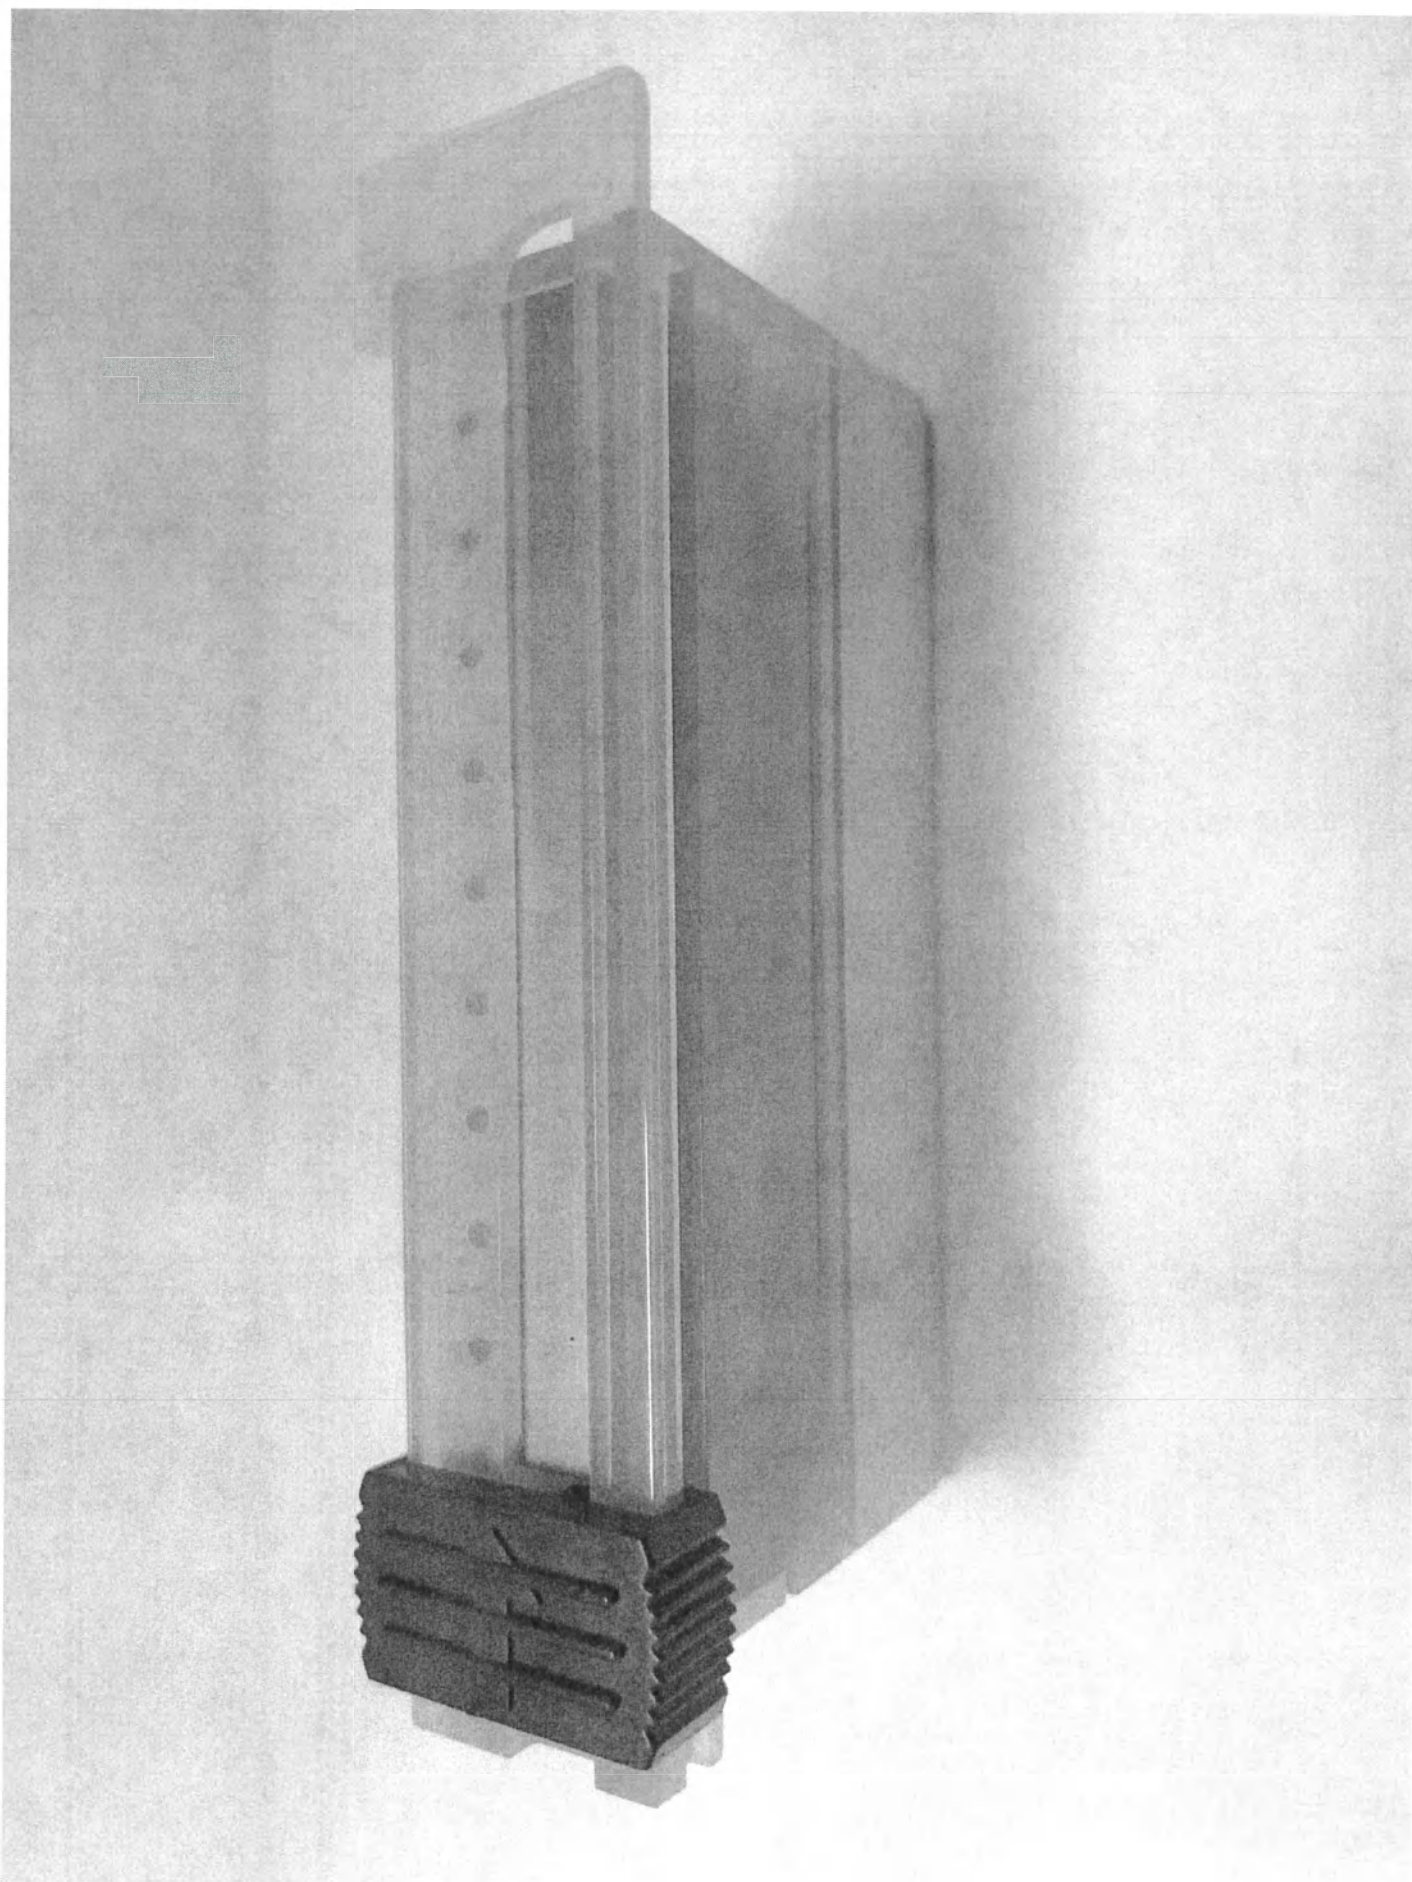

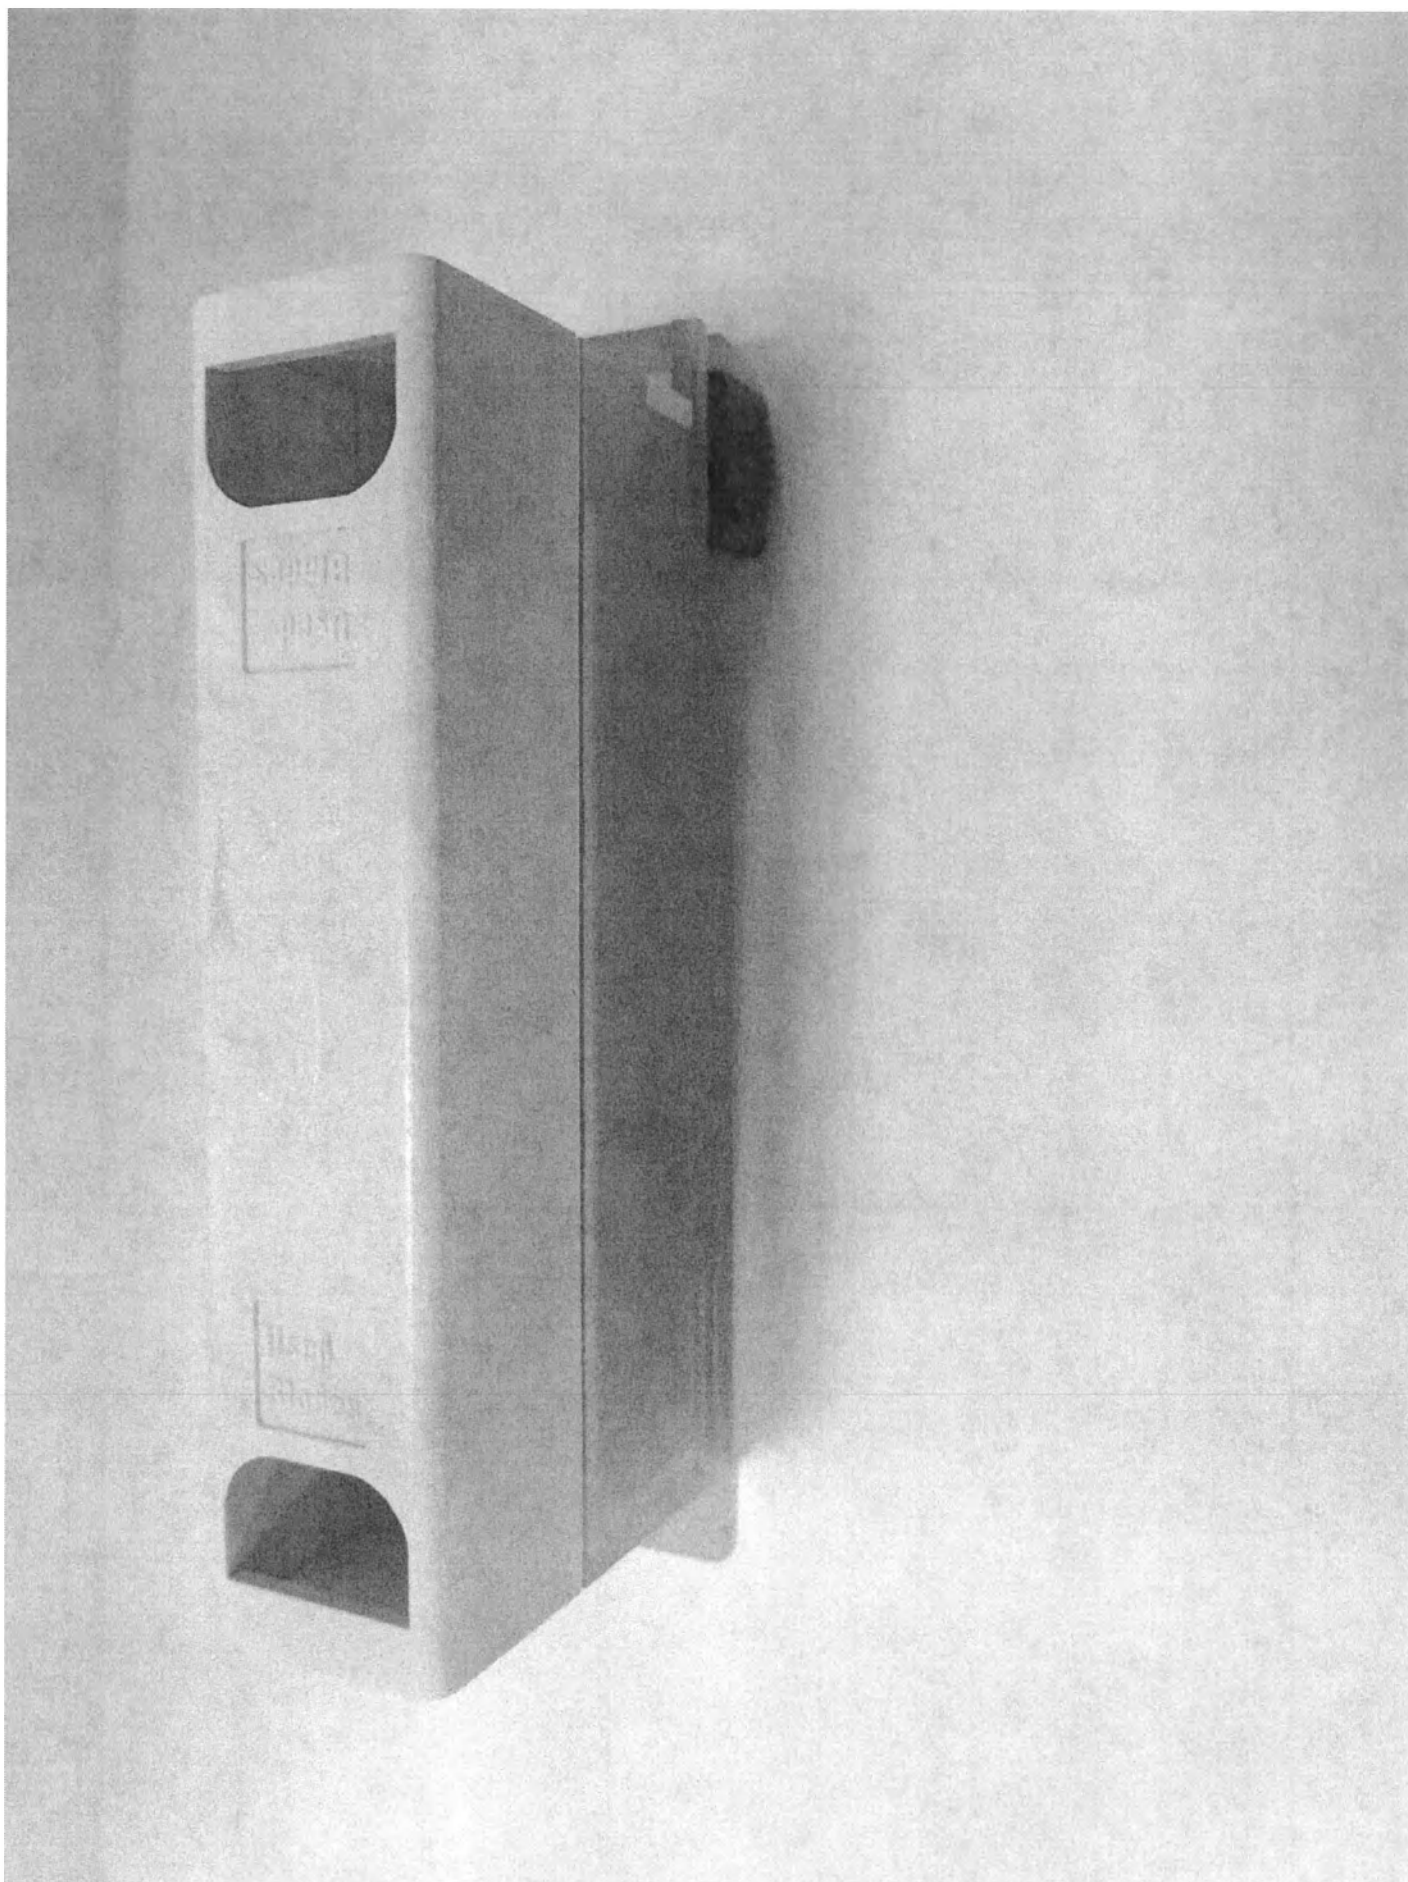

**Лезвия микротомные одноразовые низкого профиля Leica DB80LS
(Leica DB80LS Low Profile Microtome Blades)**

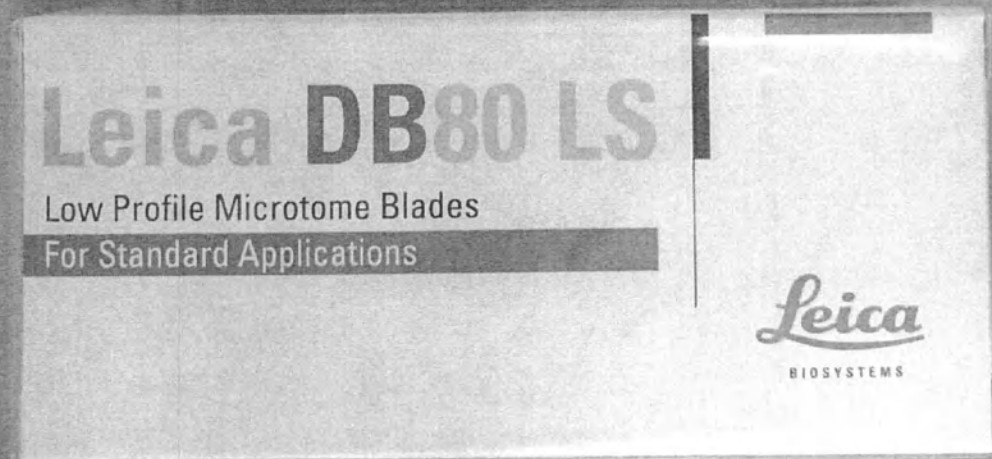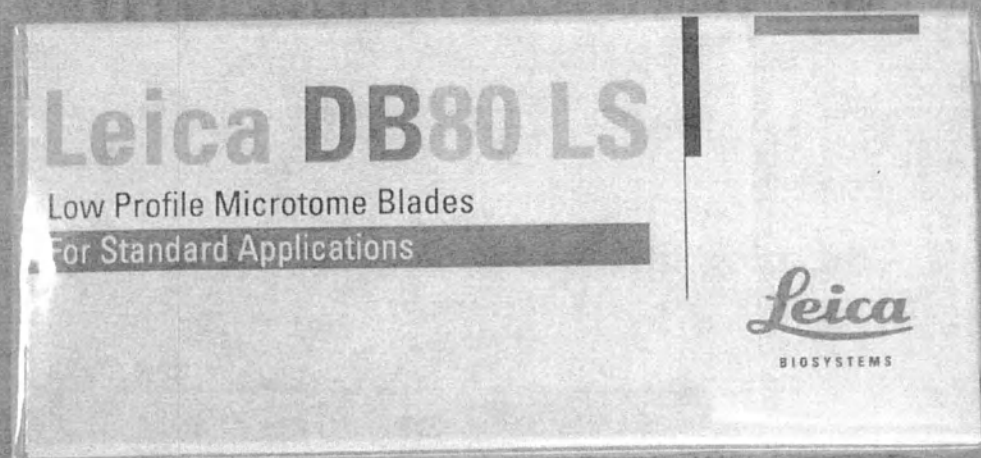

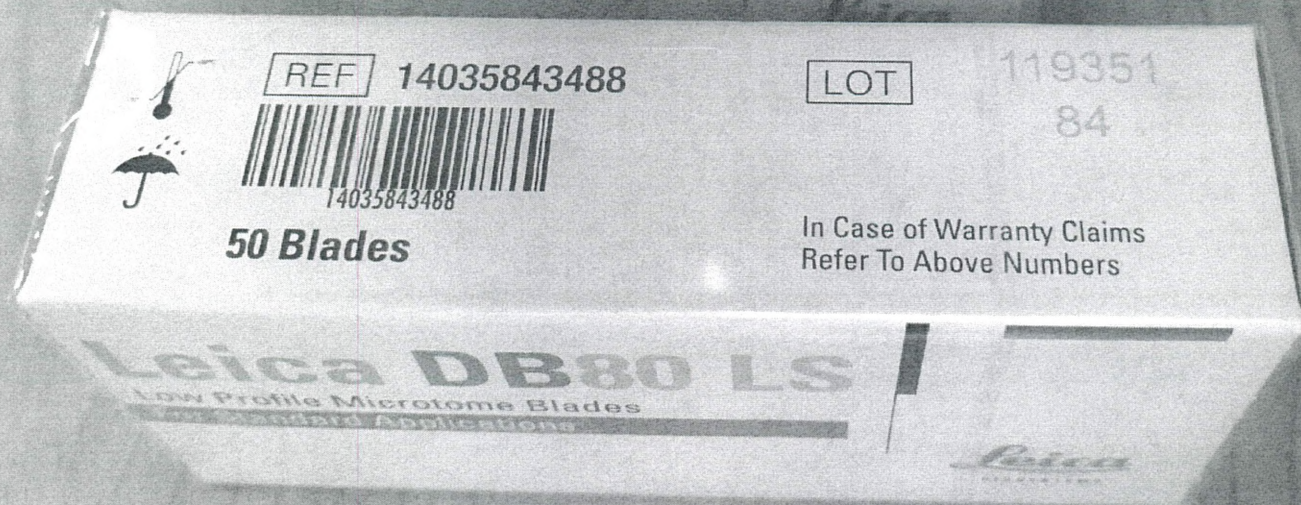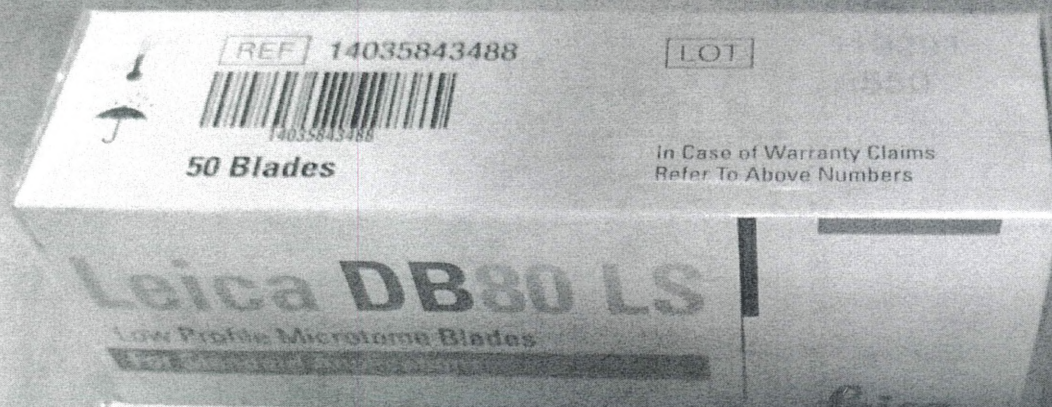



REF 14035843488



14035843488

50 Blades

LOT

119291
550


In Case of Warranty Claims
Refer To Above Numbers


Leica DB80 LS


Low Profile Microtome Blades


For Standard Applications


Leica
MICROSYSTEMS

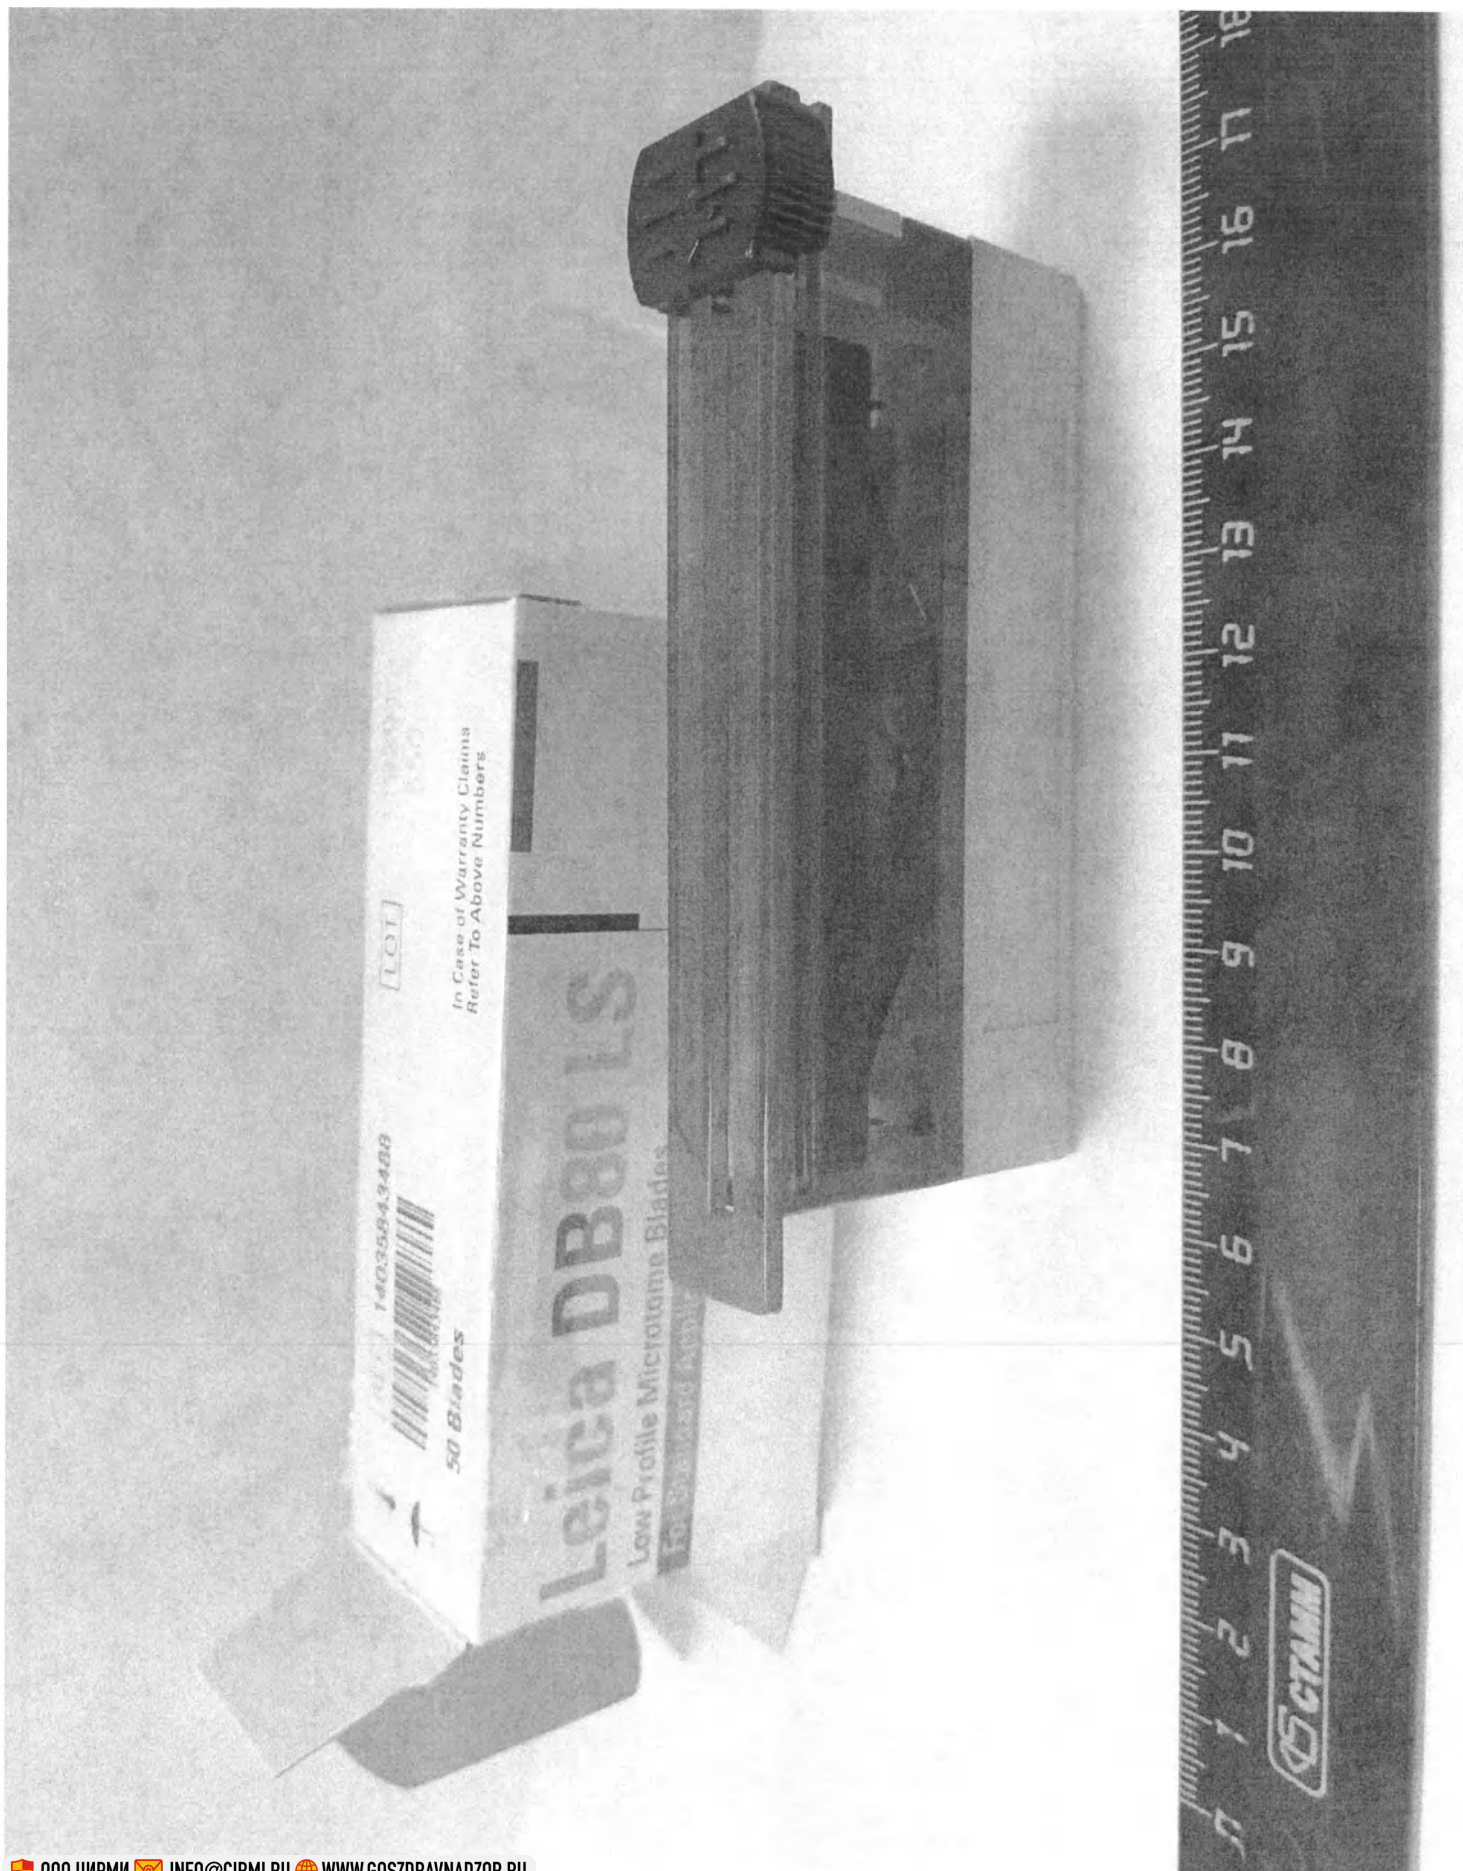


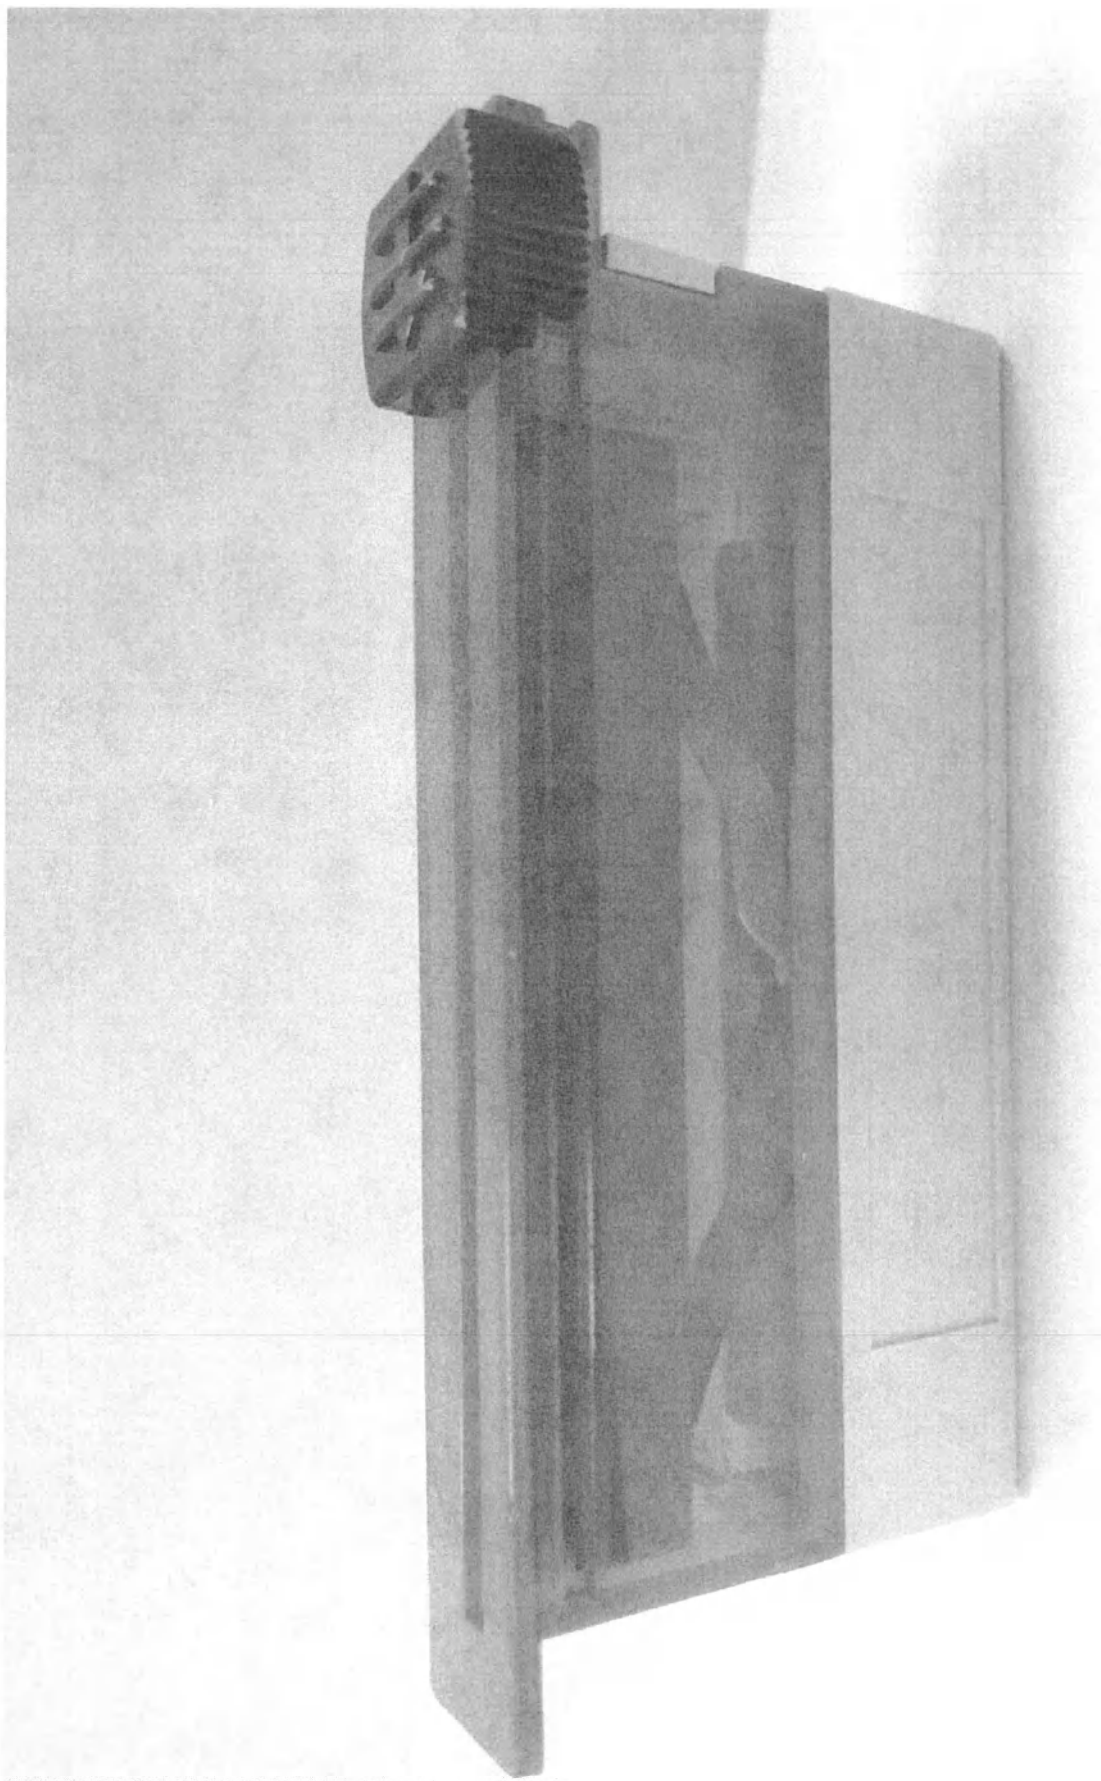


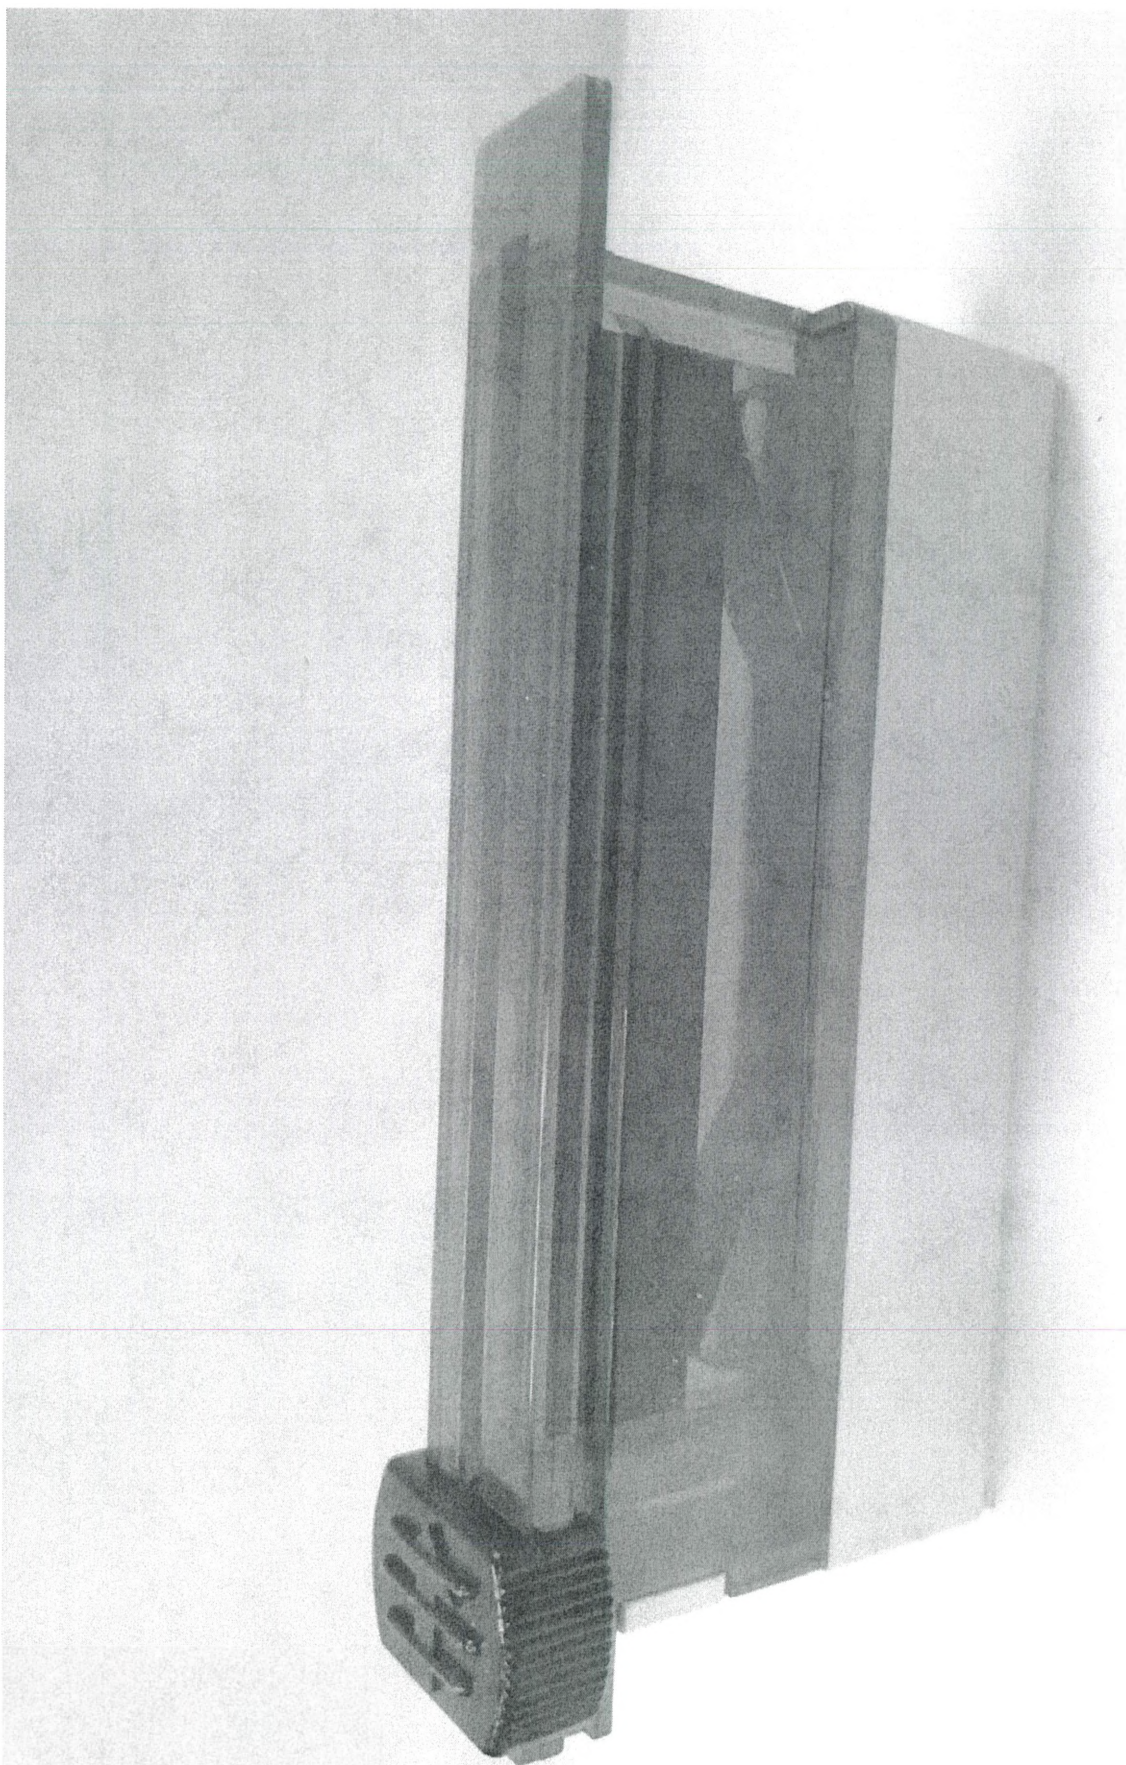

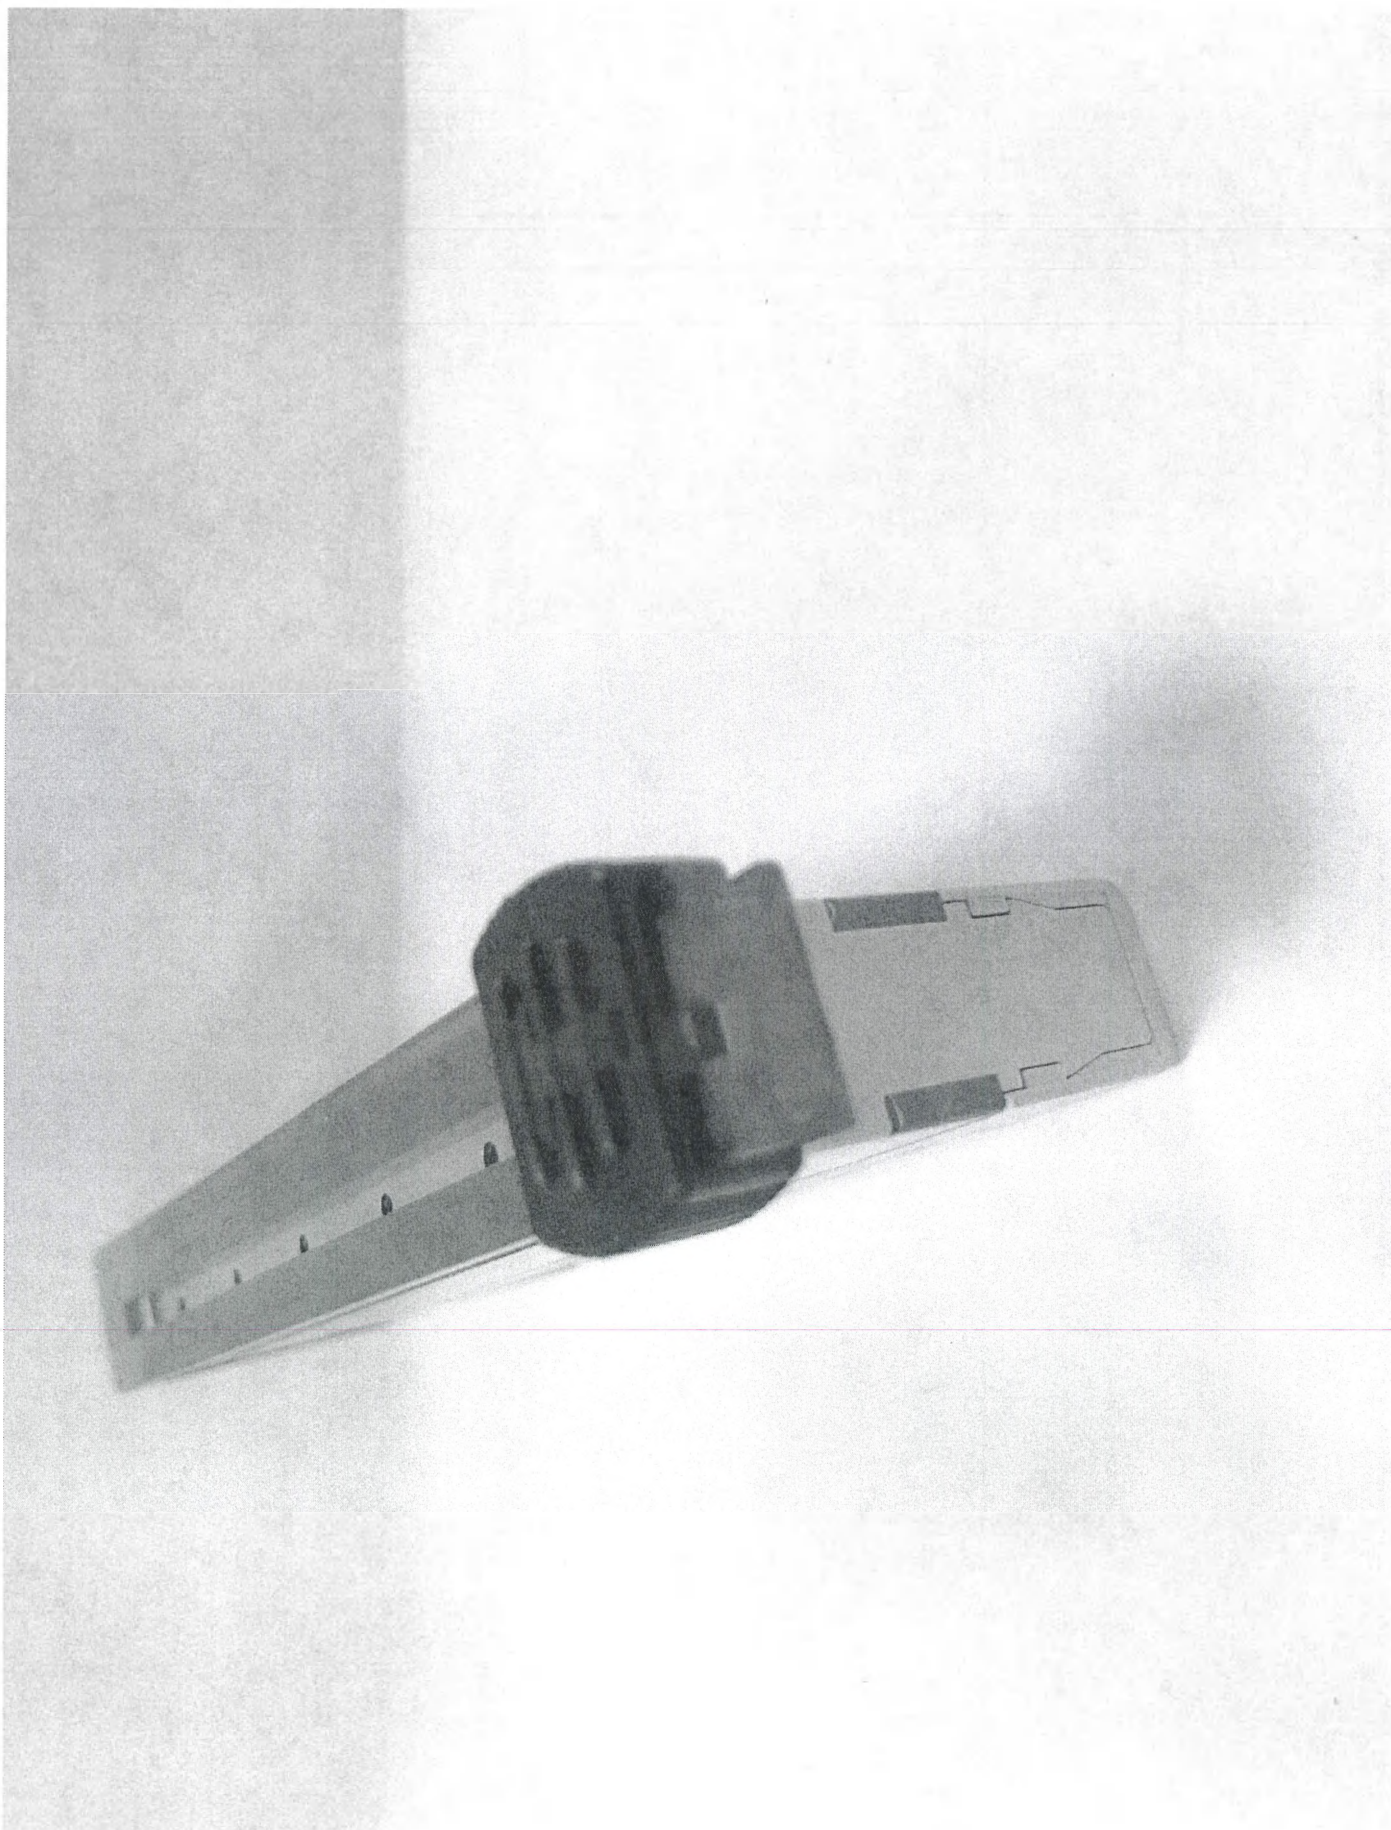

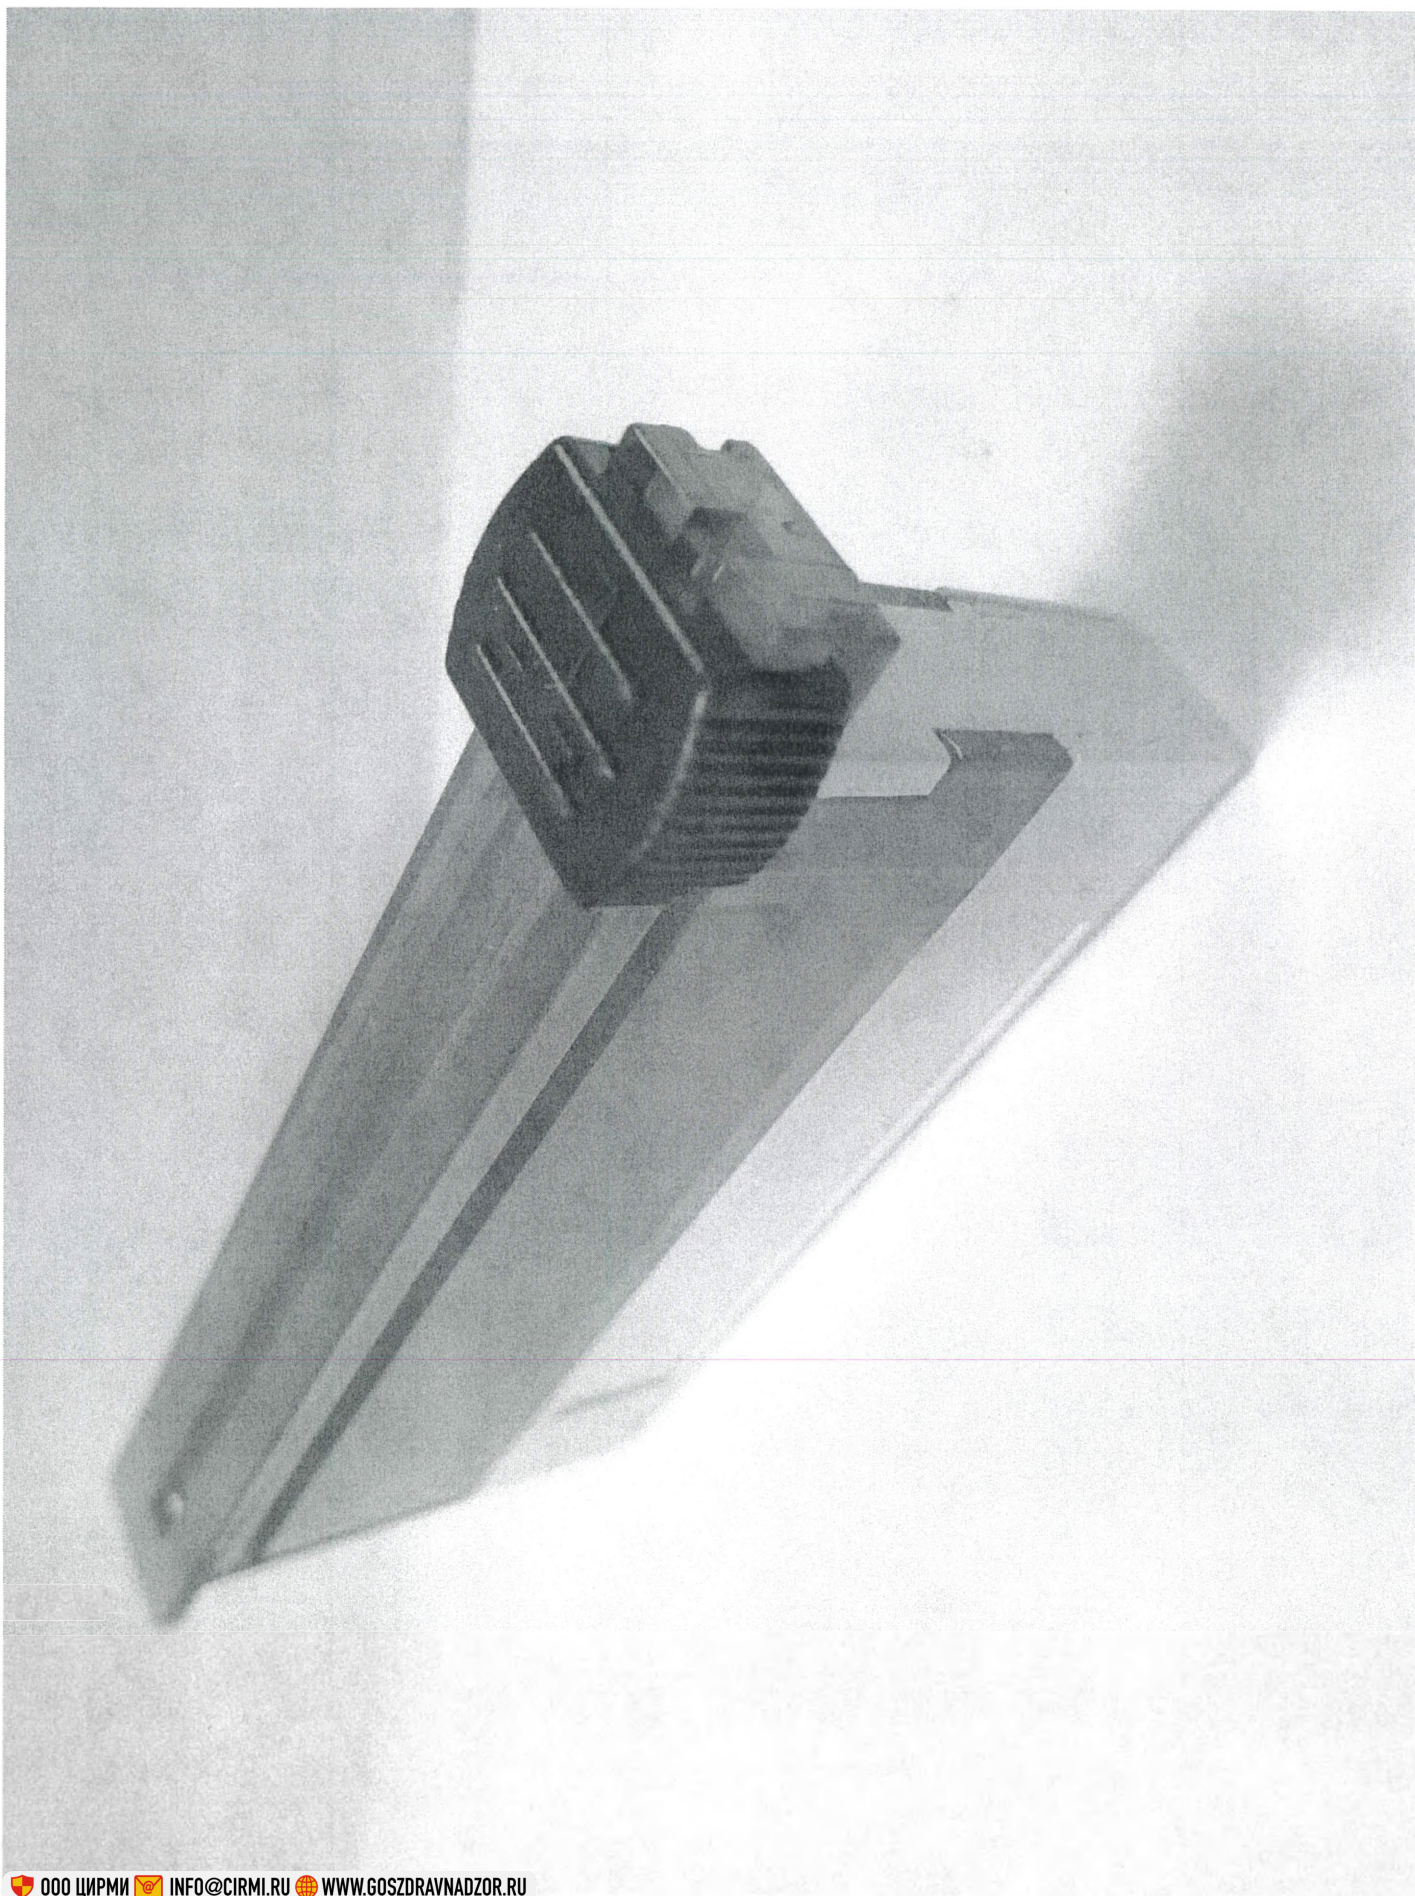

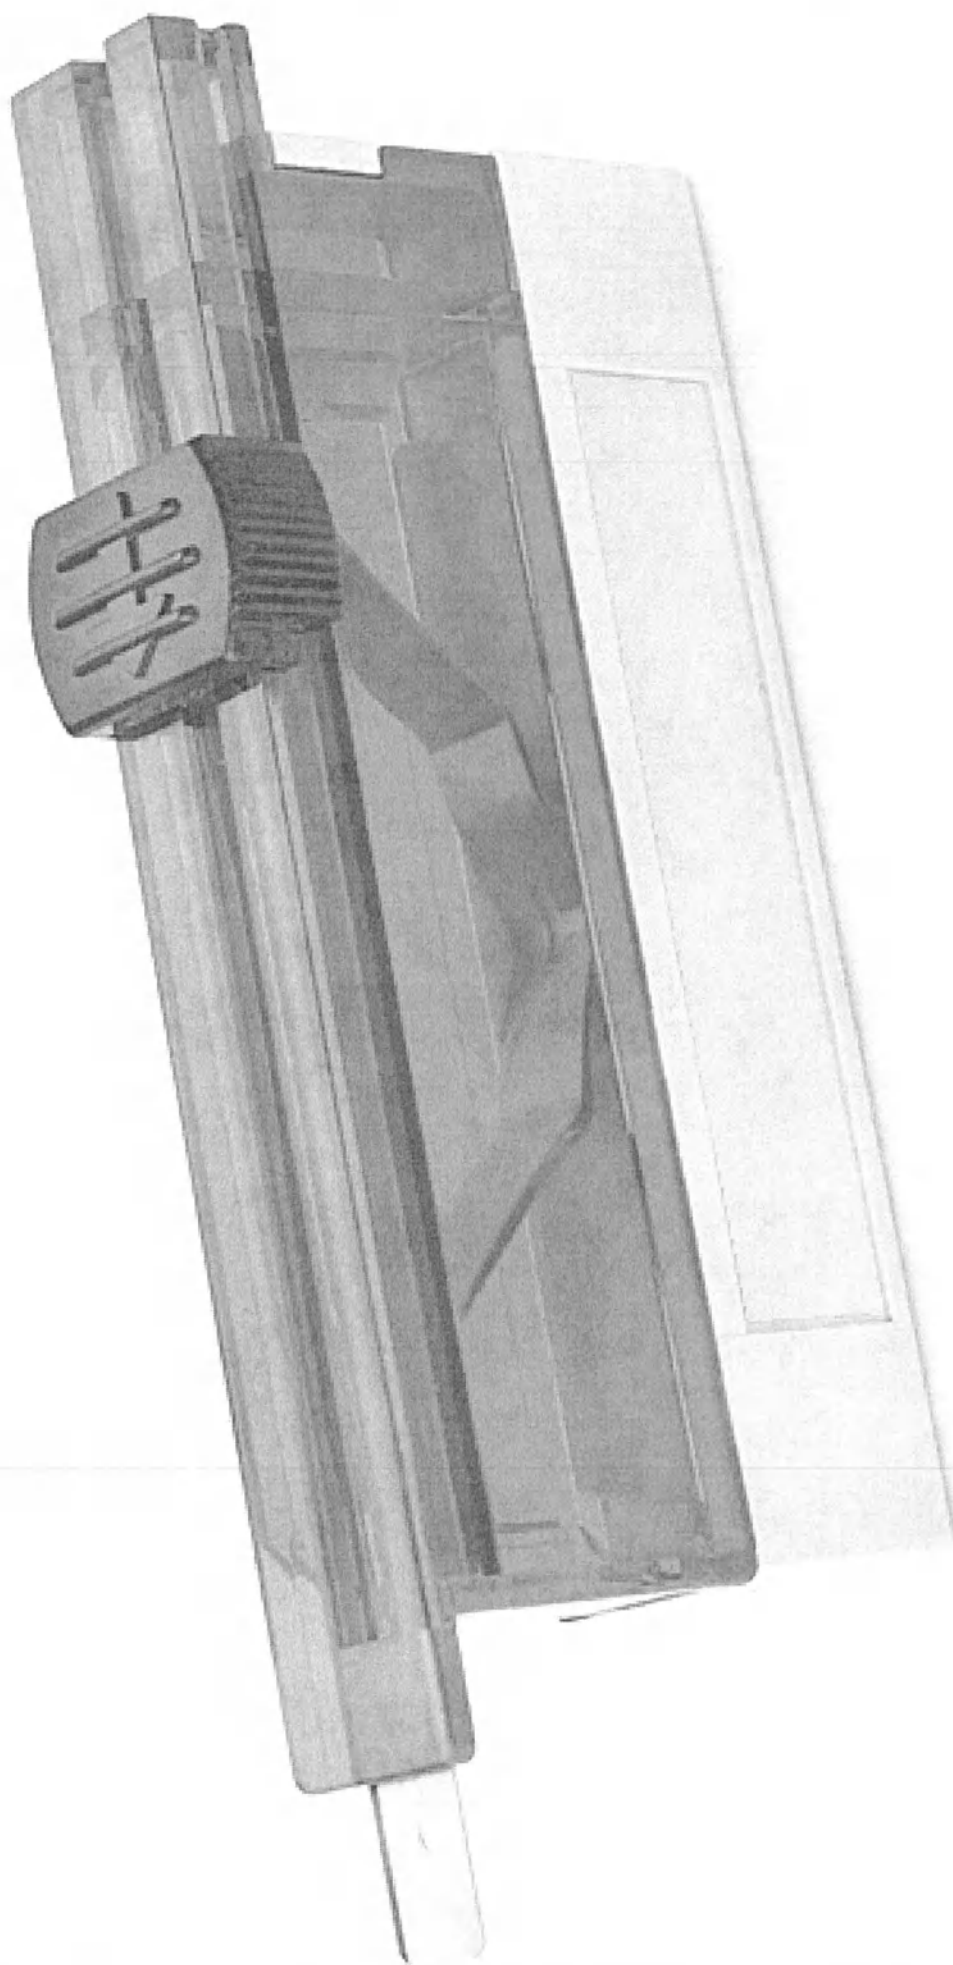

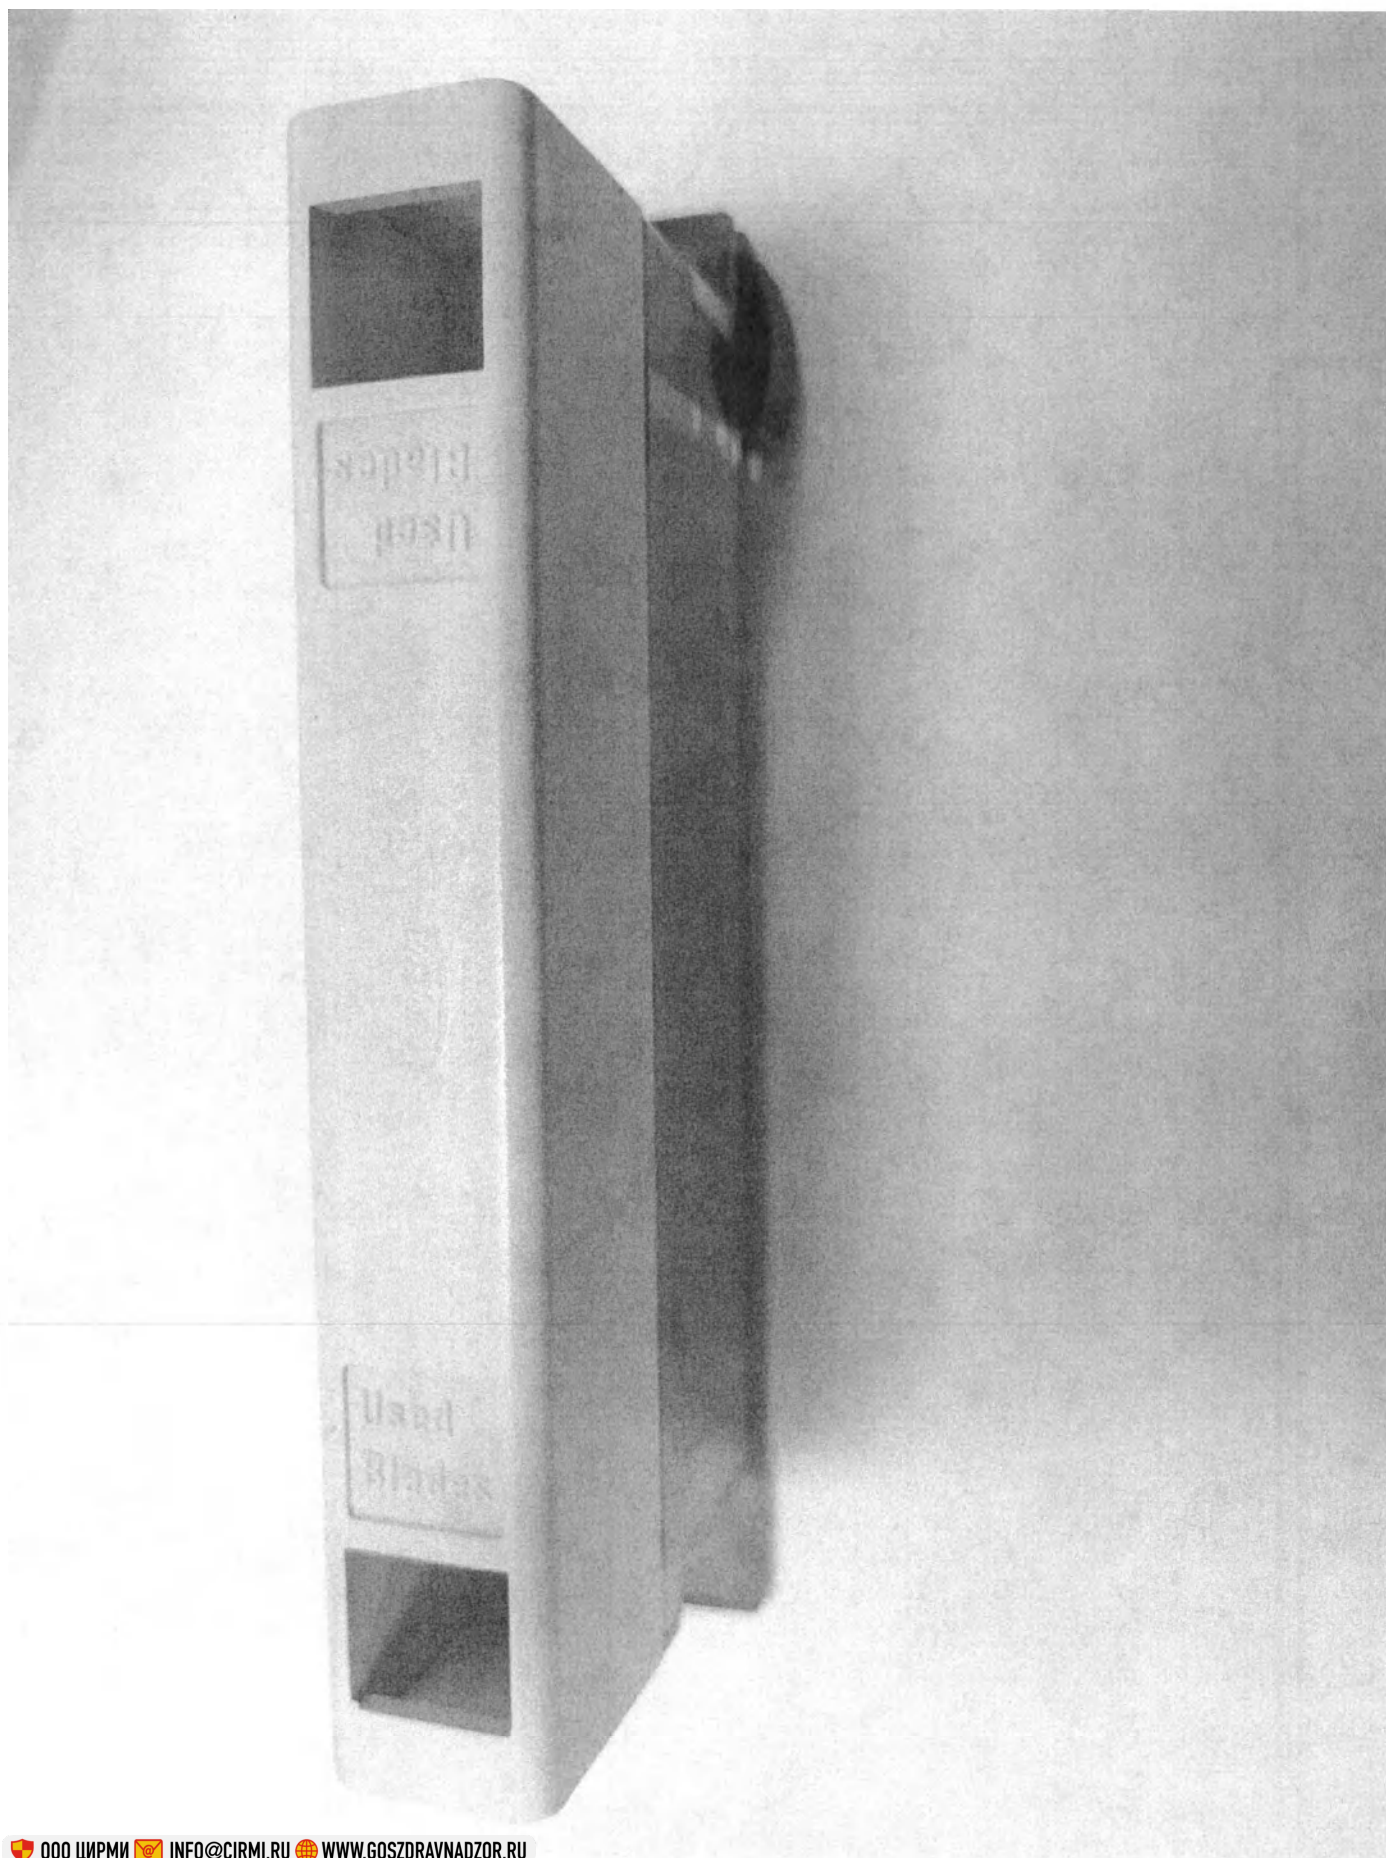

**Лезвия микротомные одноразовые низкого профиля Leica DB80LX
(Leica DB80LX Low Profile Microtome Blades)**

Leica DB80 LX

Low Profile Microtome Blades

For Standard Applications-Extra Durable

Leica
BIO SYSTEMS



REF 14035843496

LOT

119132

95




14035843496




50 Blades

In Case of Warranty Claims
Refer To Above Numbers

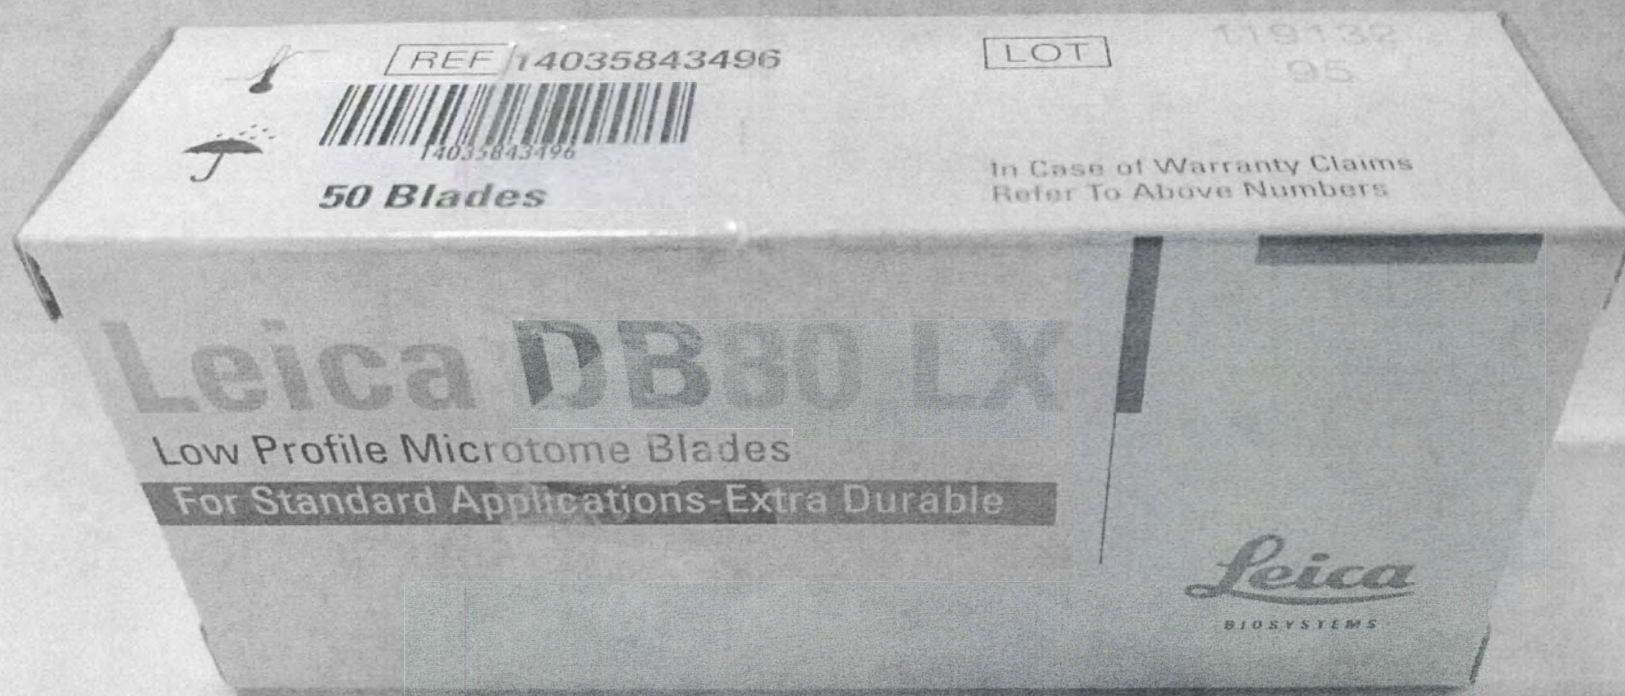



REF 14035843496



14035843496

50 Blades

LOT


110132
95


In Case of Warranty Claims
Refer To Above Numbers


Leica DB80 LX


Low Profile Microtome Blades

For Standard Applications-Extra Durable

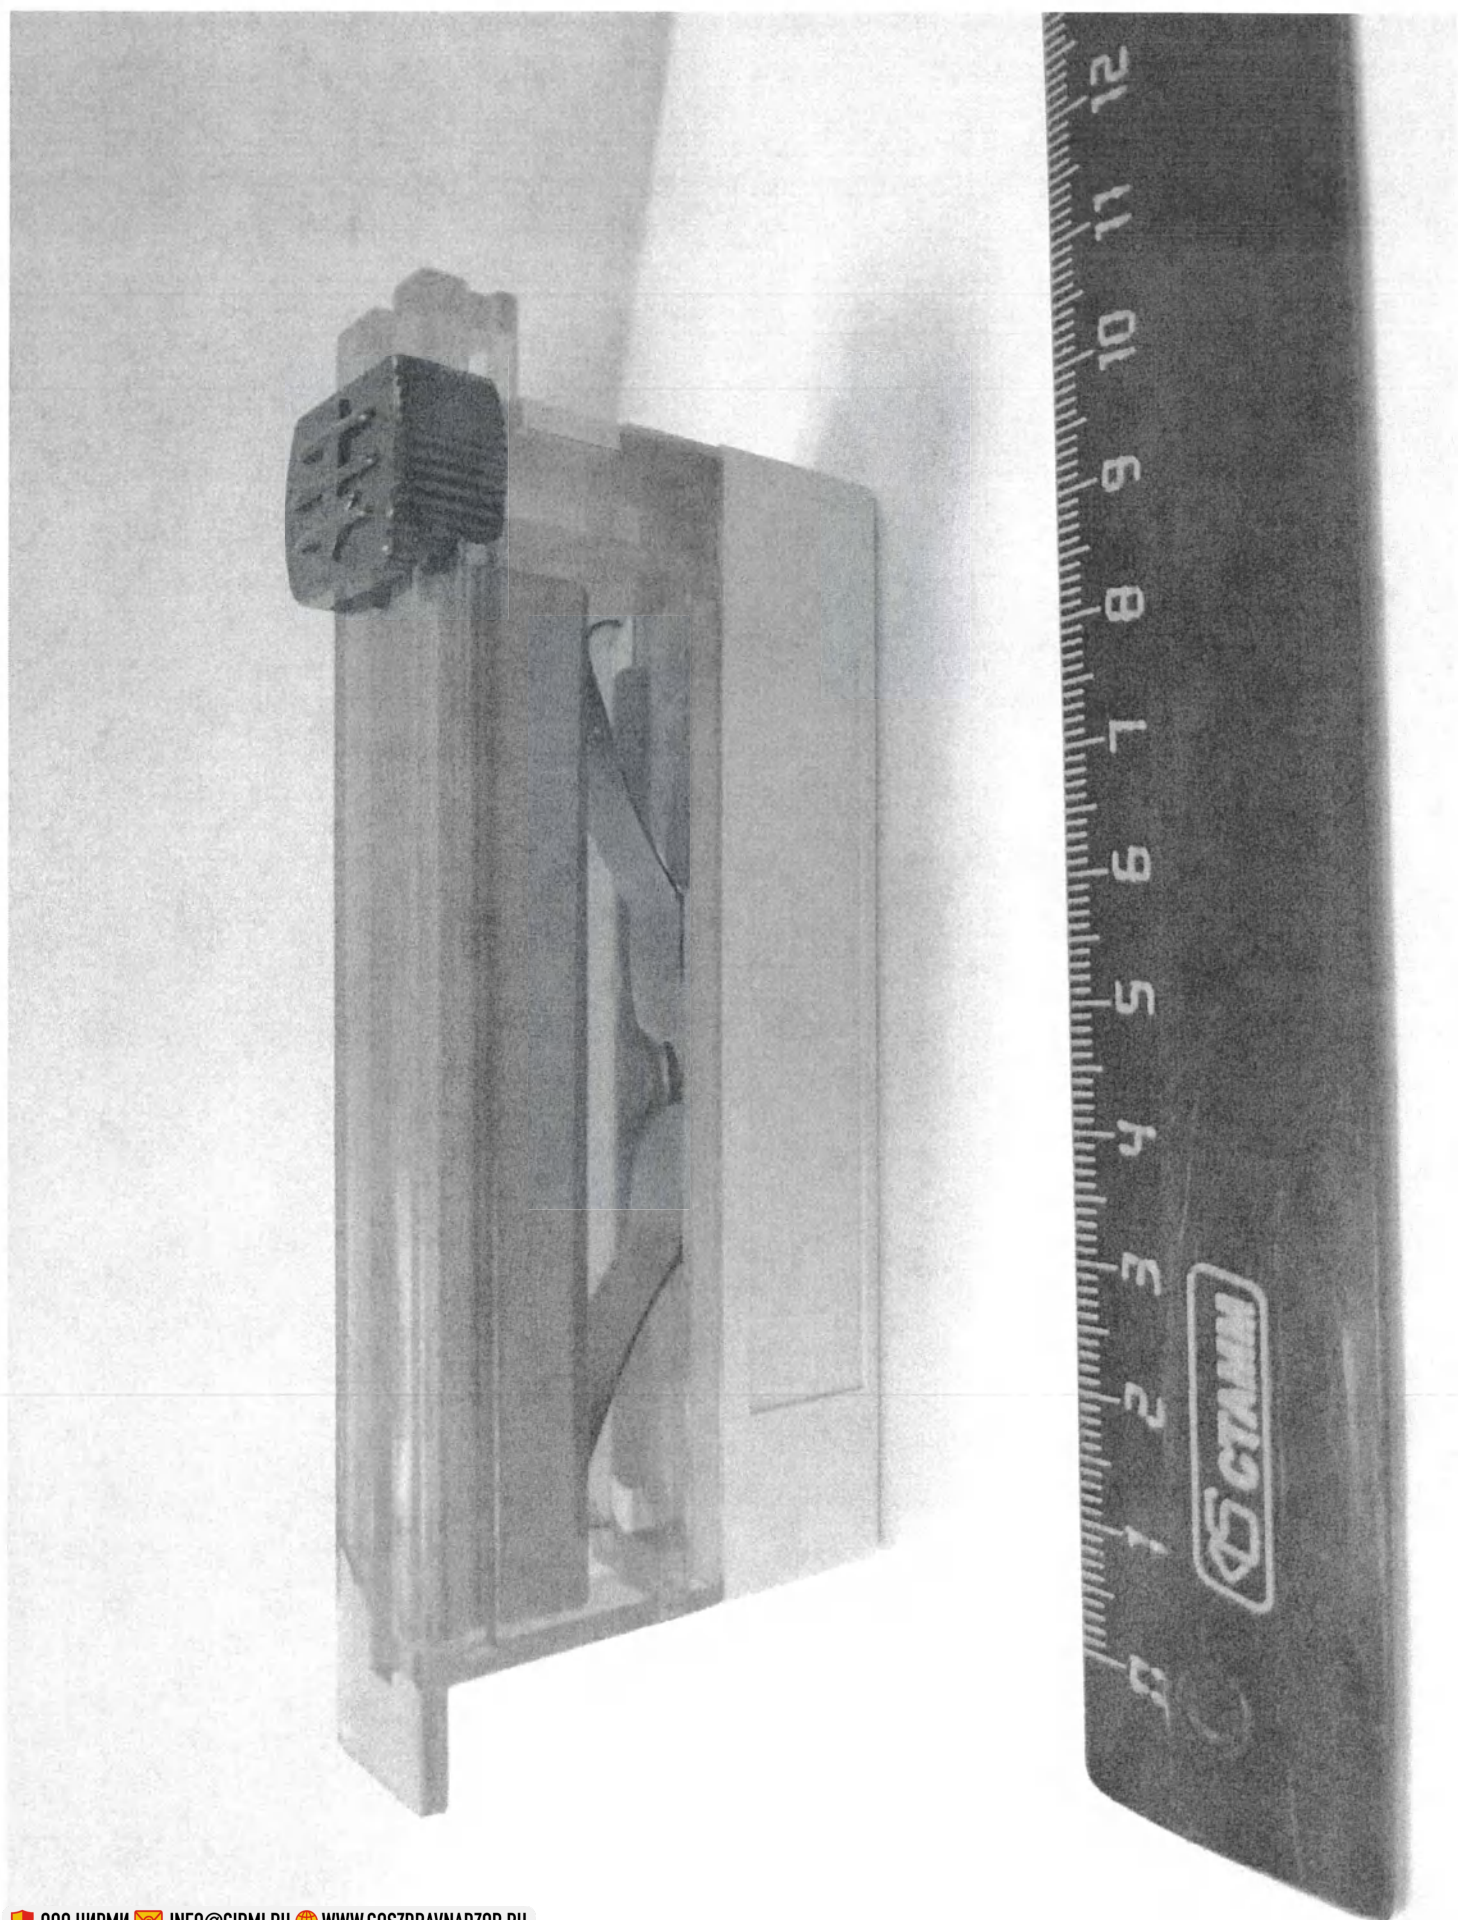

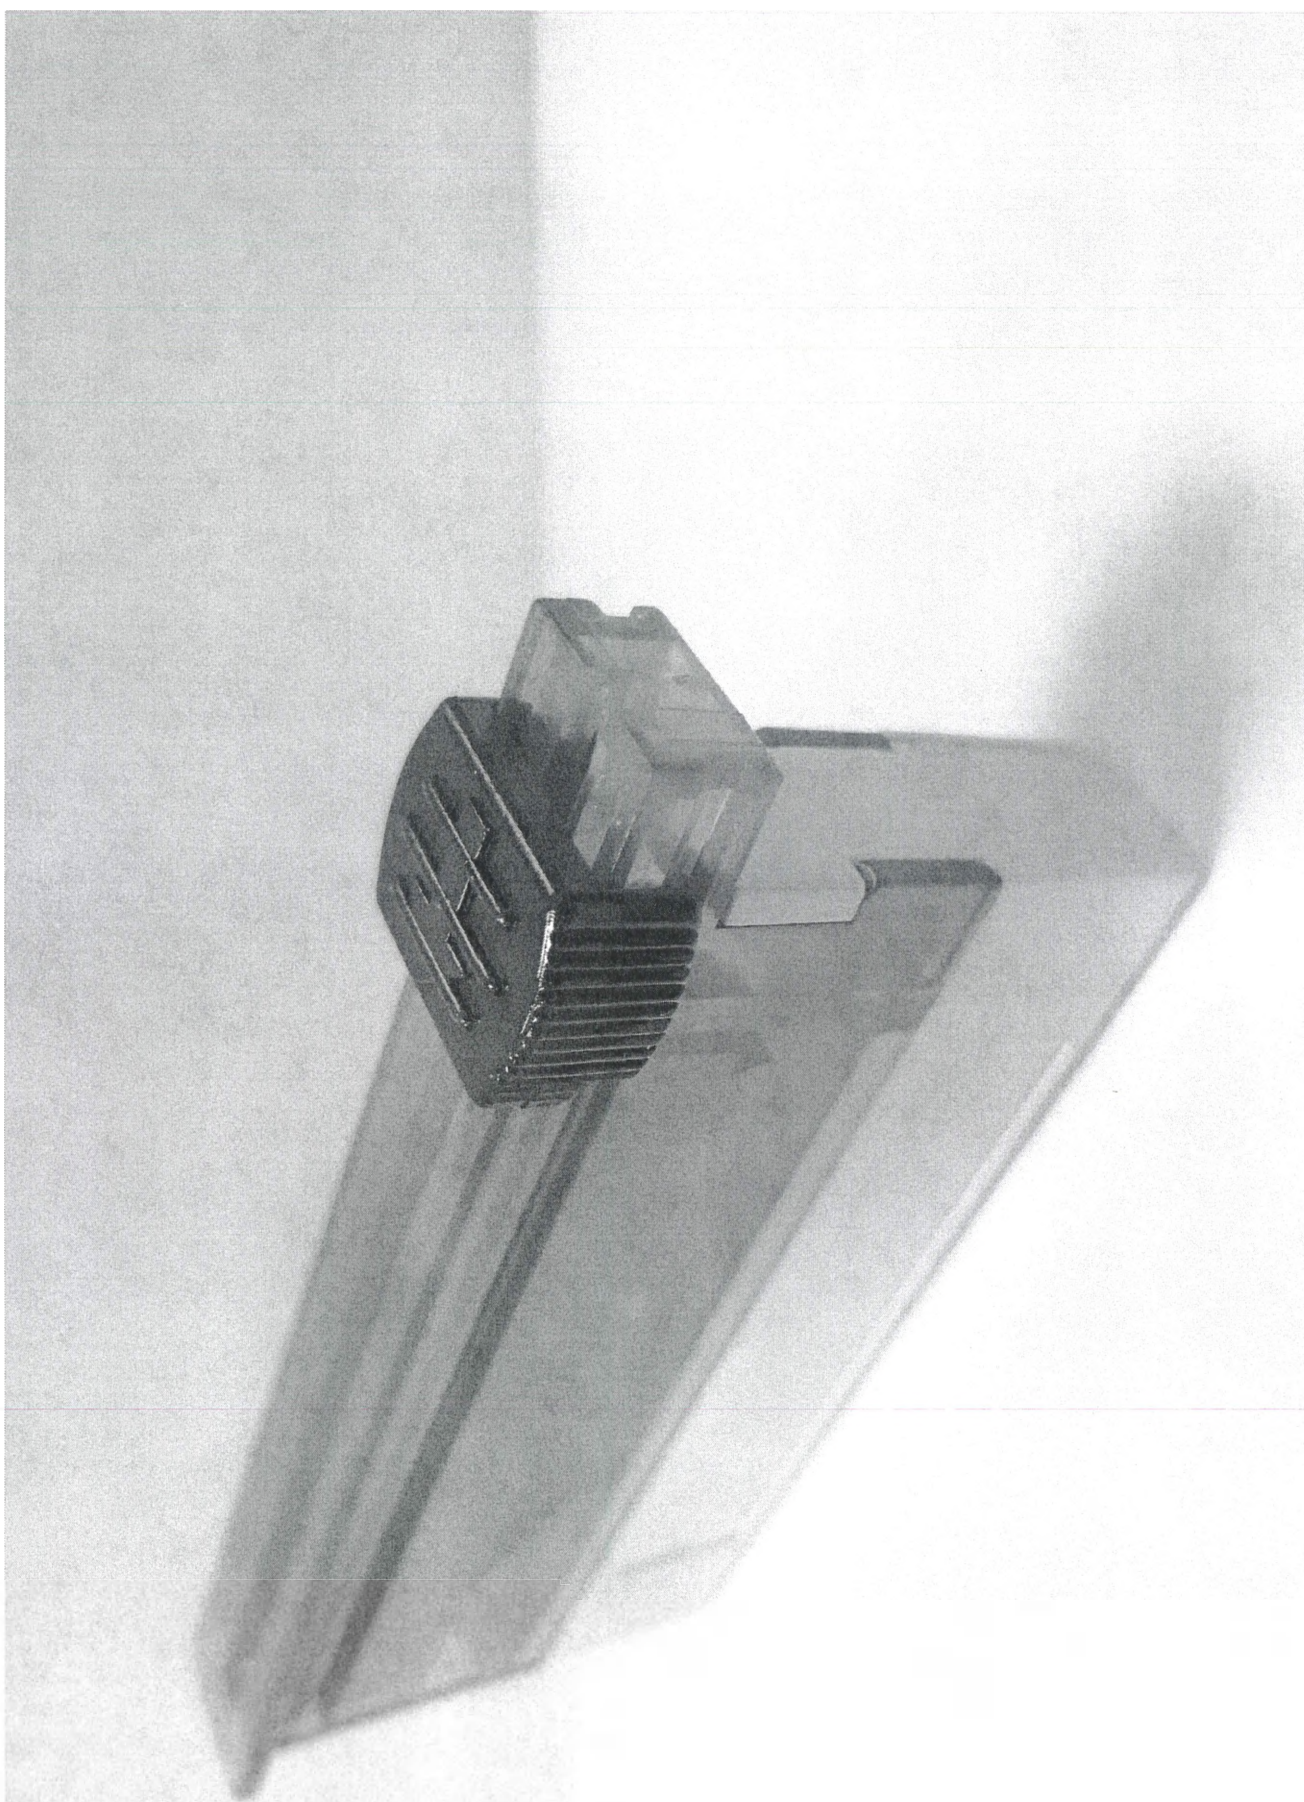

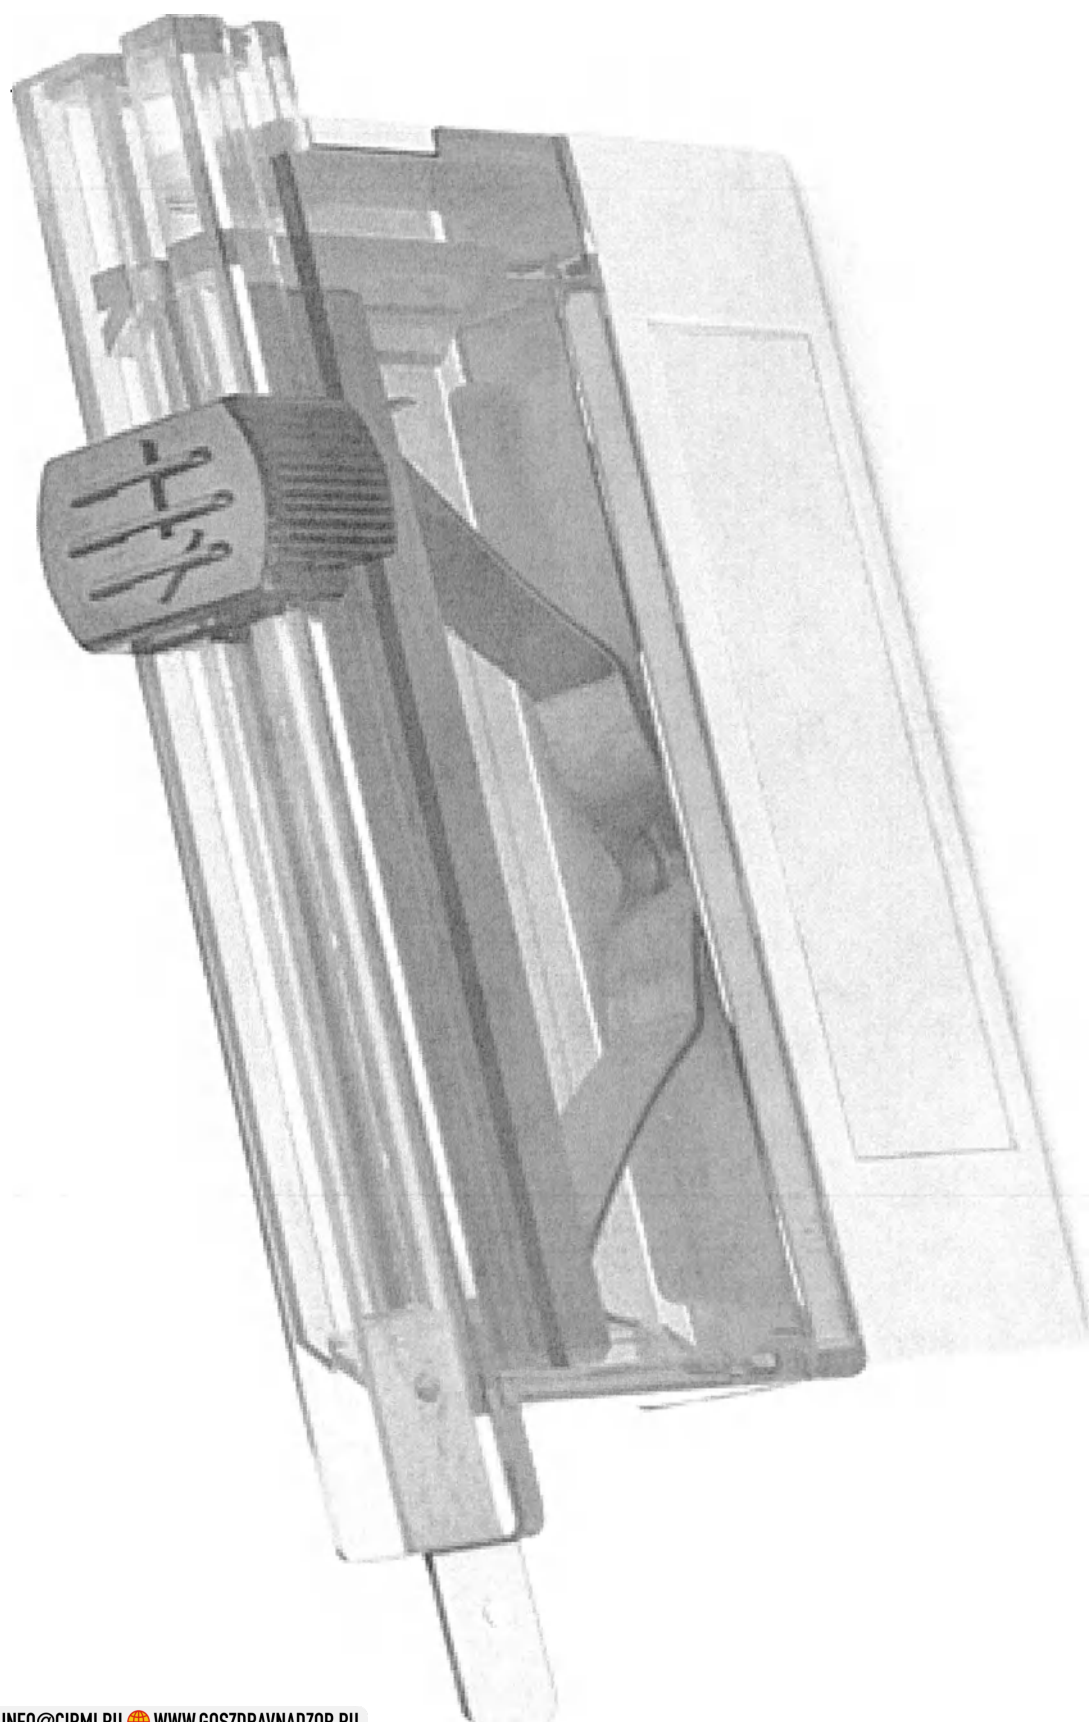

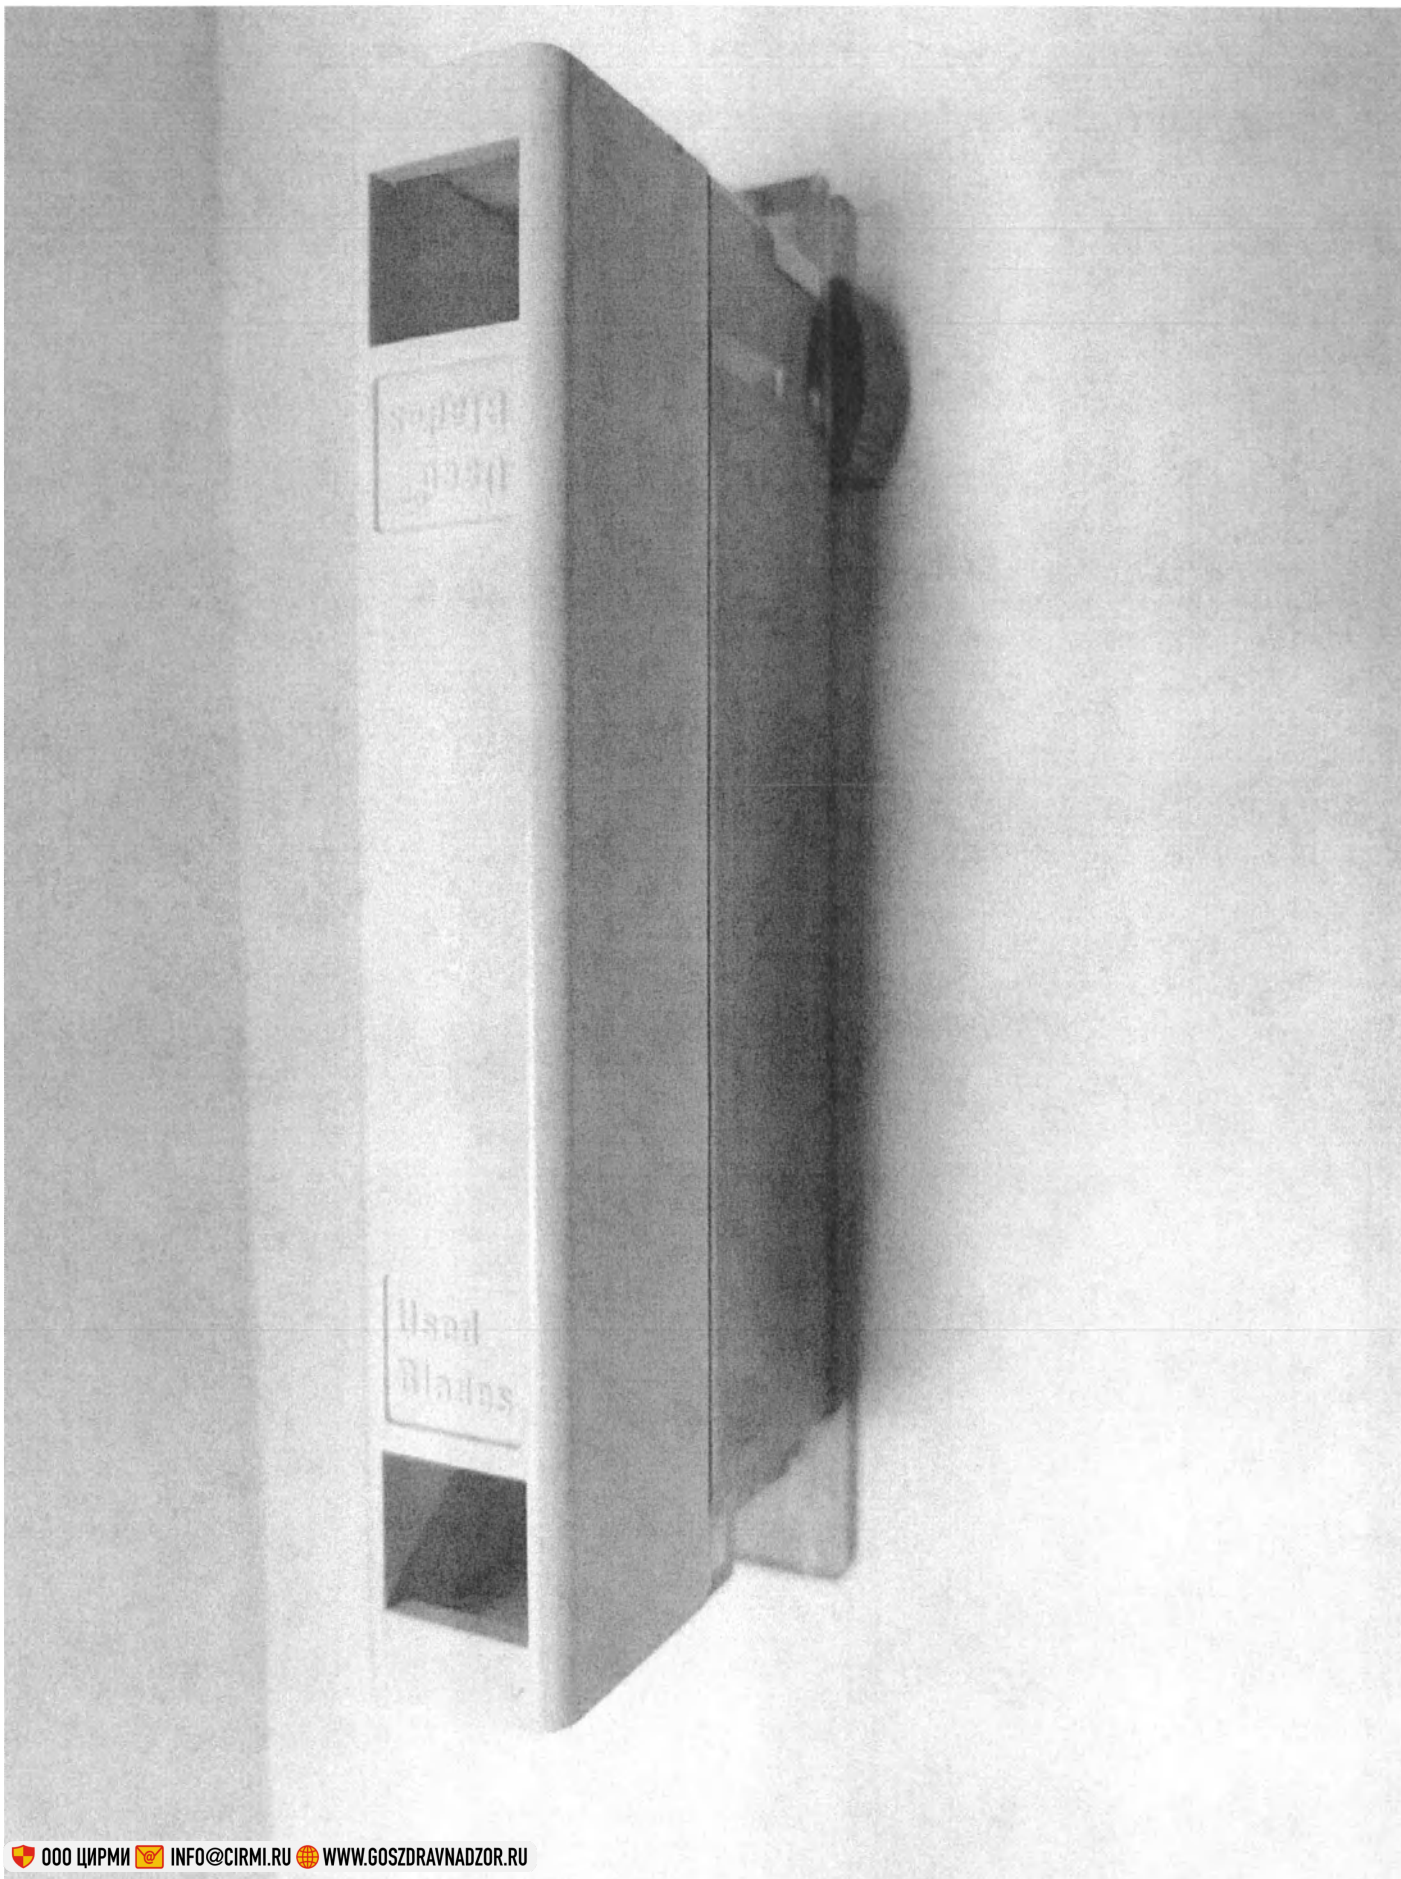

**Лезвия микротомные одноразовые высокого профиля Leica DB80HS
(Leica DB80HS High Profile Microtome Blades)**

Leica DB80 HS

High Profile Microtome Blades

For Standard Applications


Leica
BIOSYSTEMS

Leica DB80 HS

High Profile Microtome Blades

For Standard Applications

Leica
BIOSYSTEMS

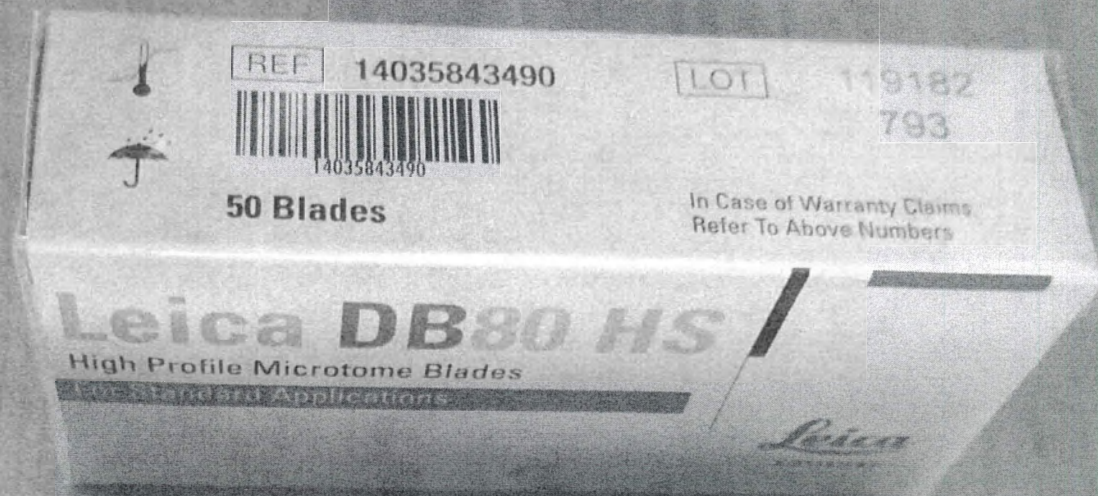



REF 14035843490



14035843490

LOT


119182
793

50 Blades


In Case of Warranty Claims
Refer To Above Numbers


Leica DB80 HS


High Profile Microtome Blades

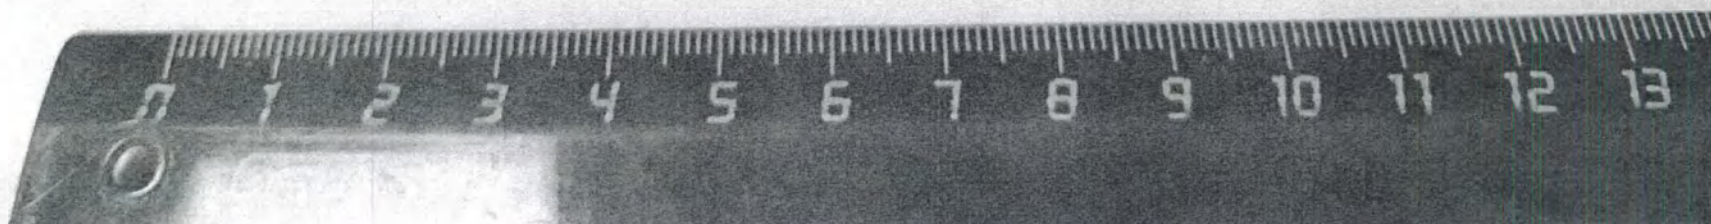





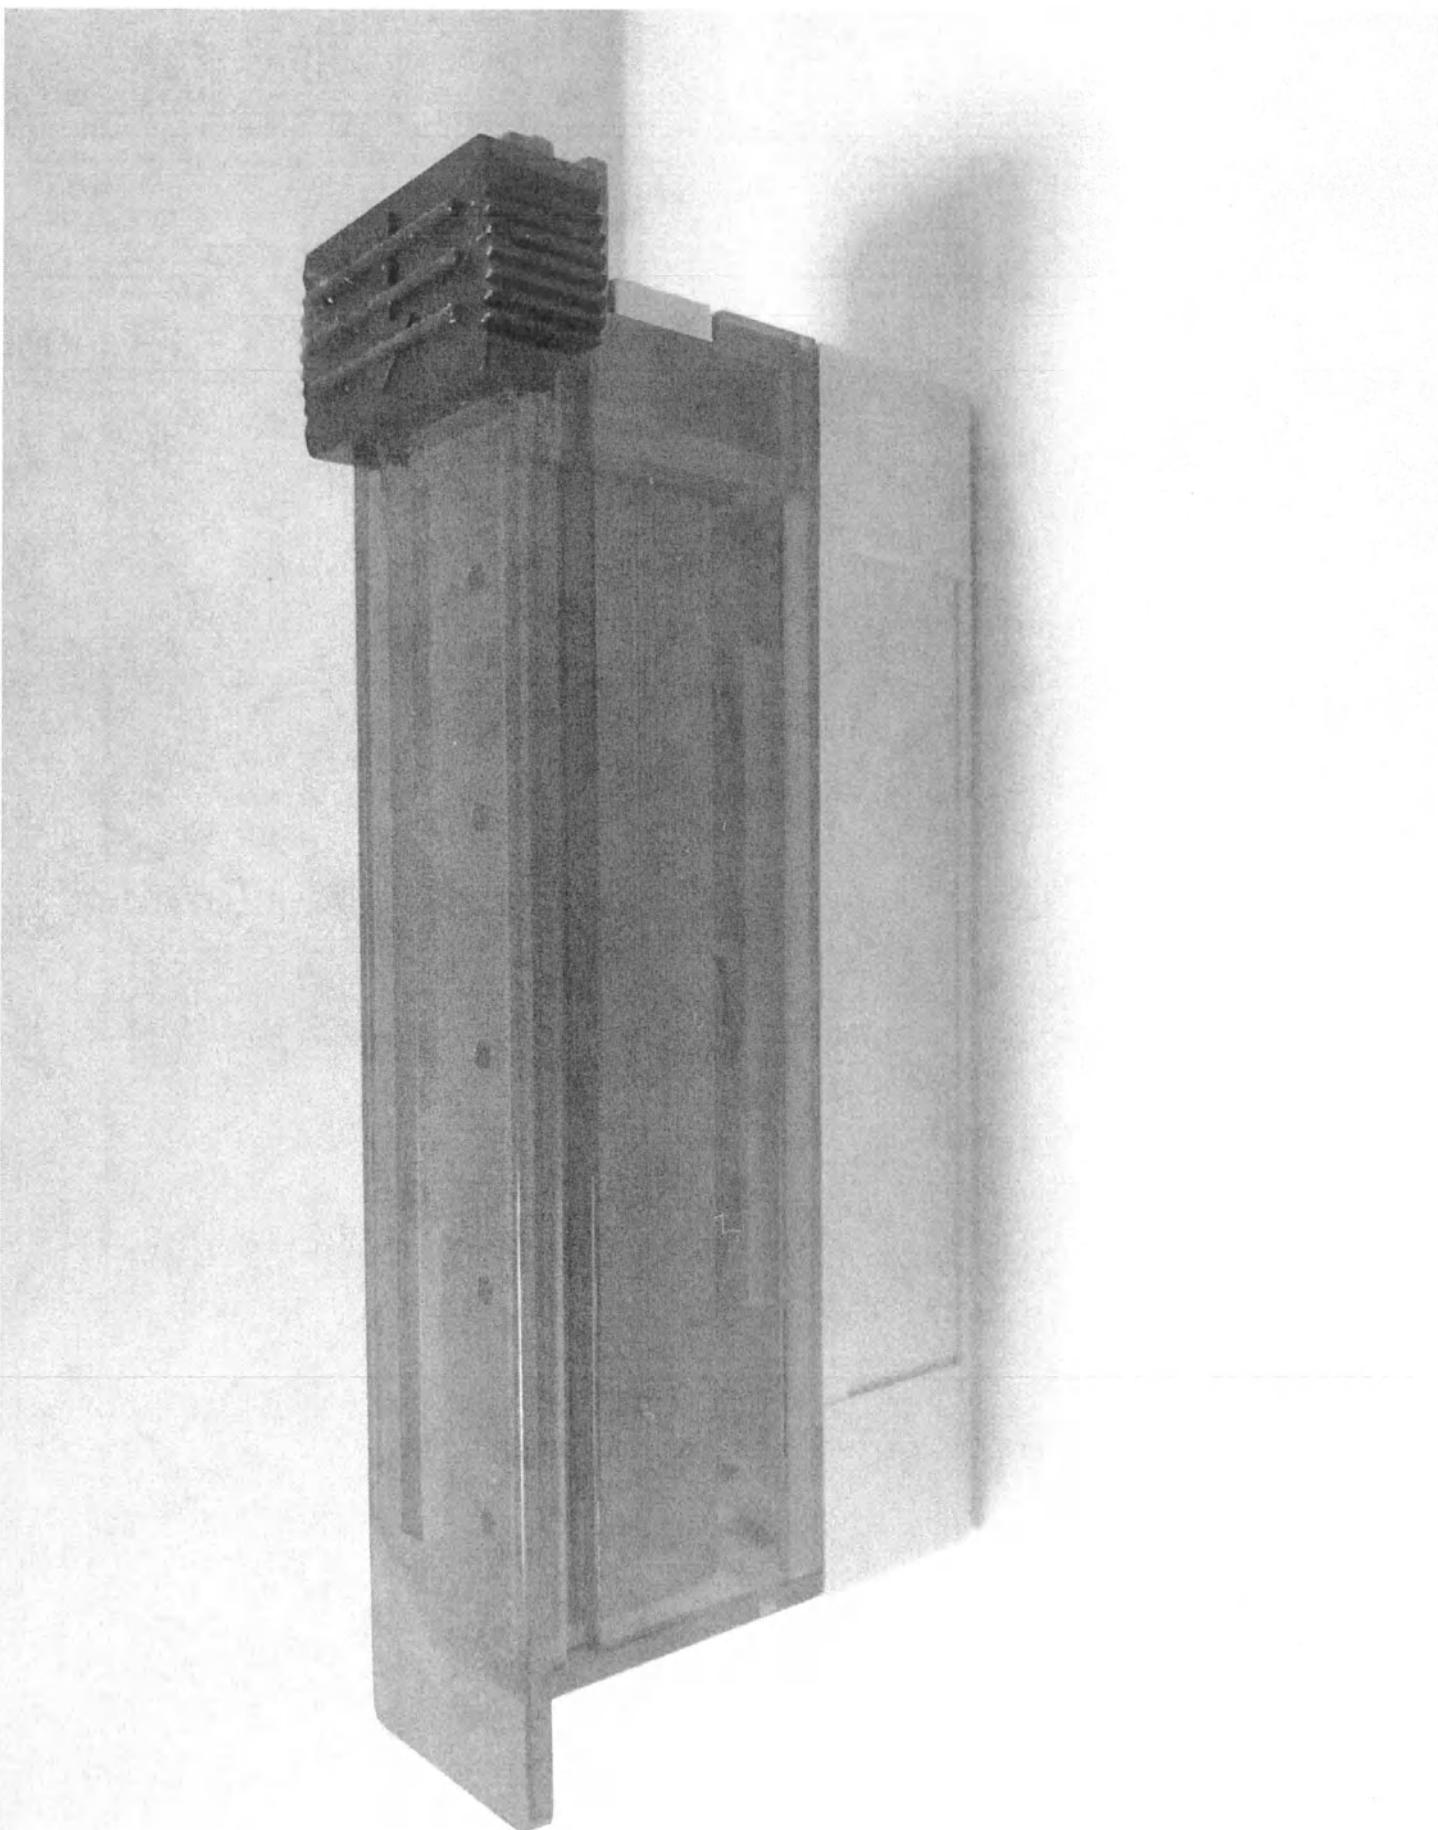


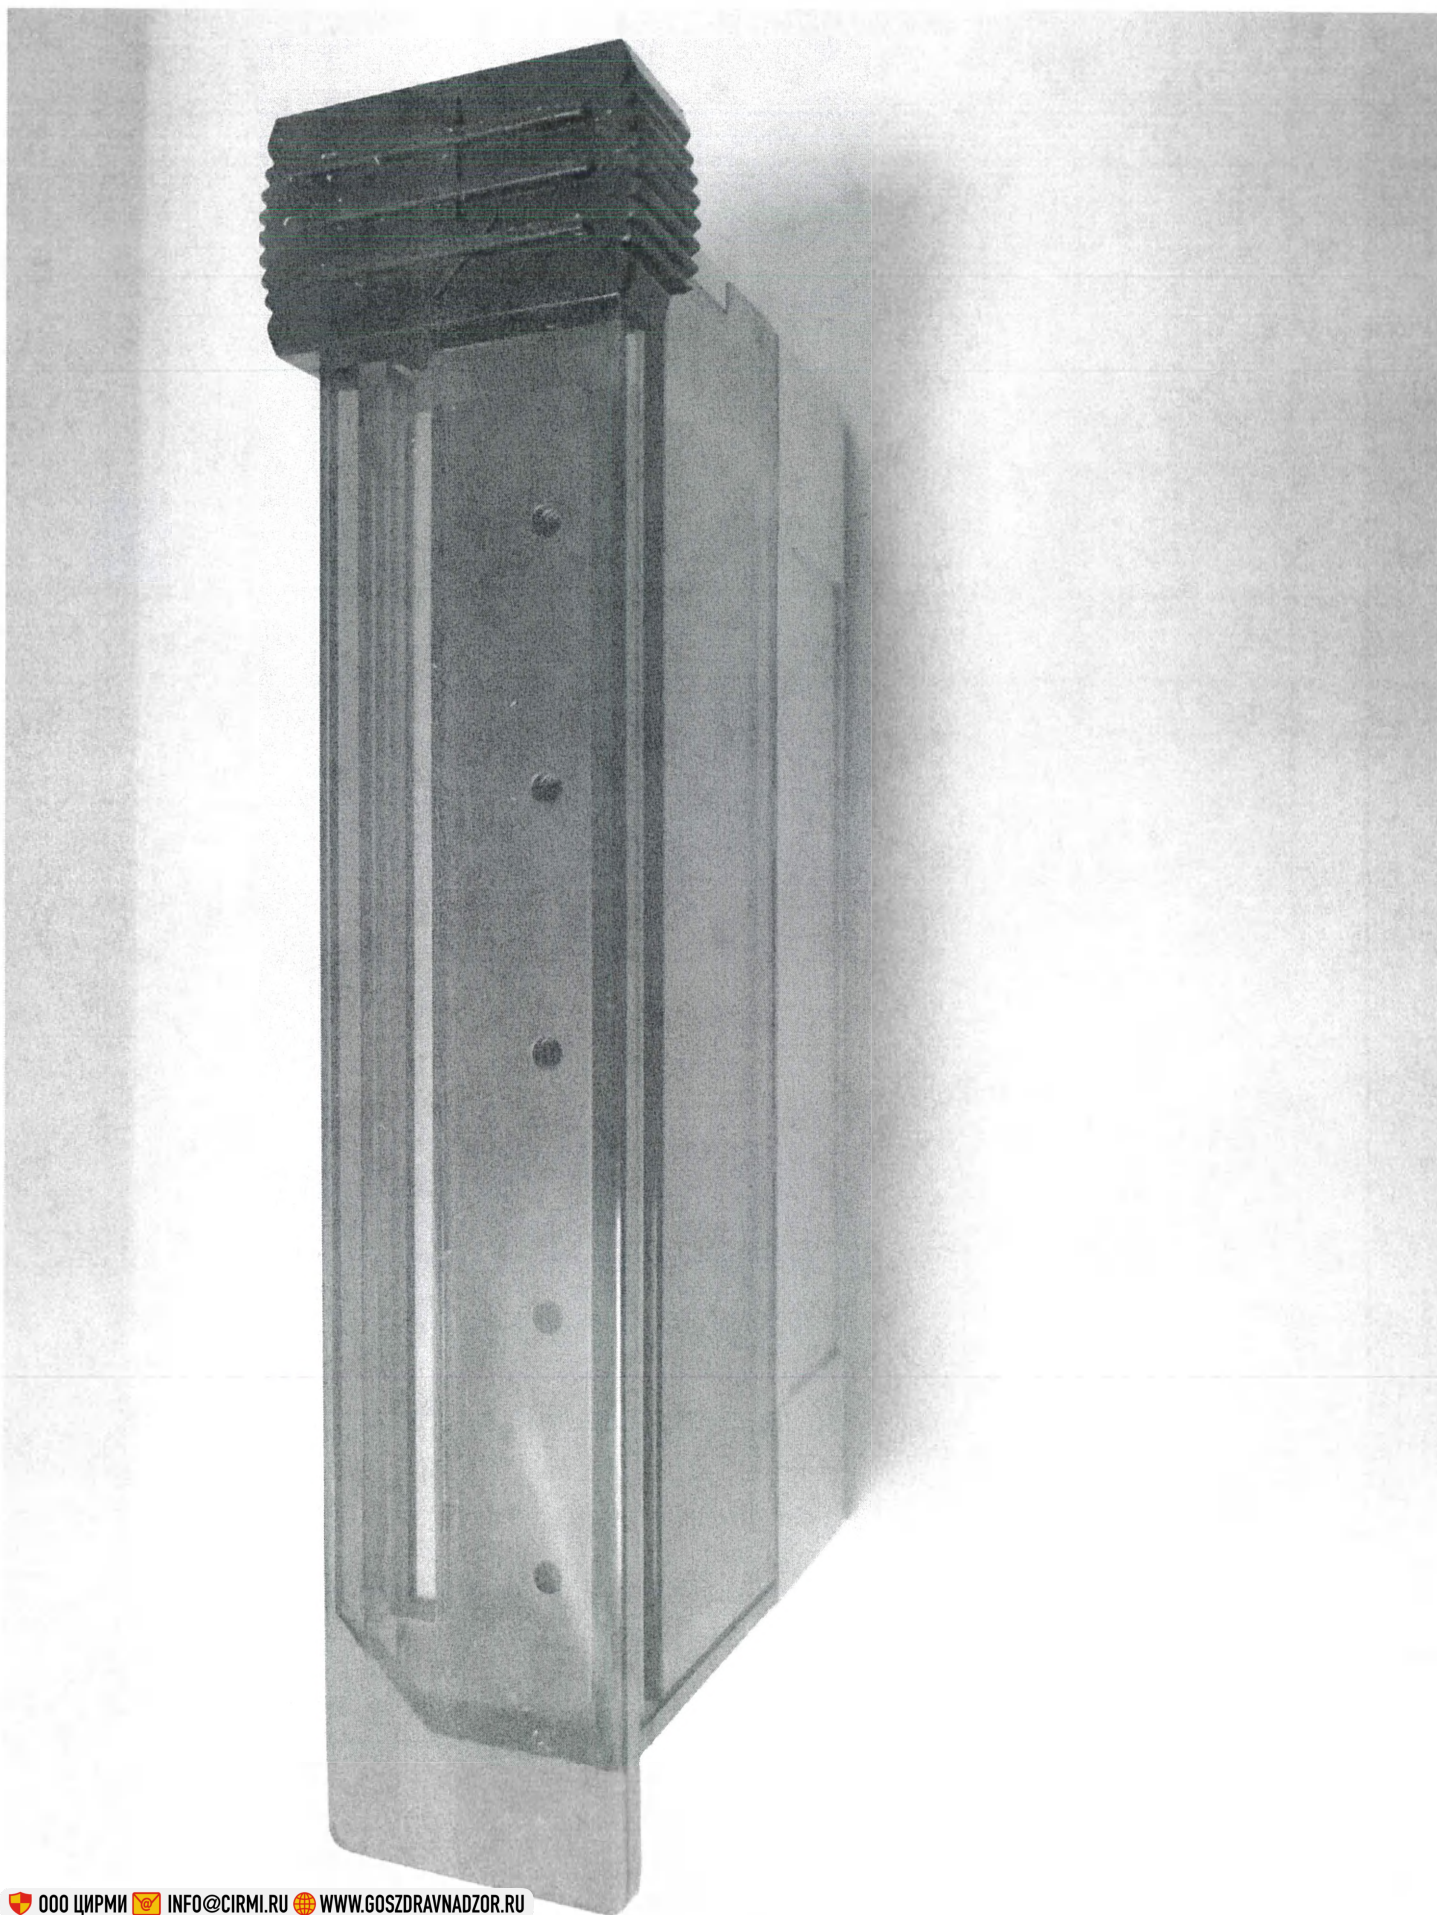

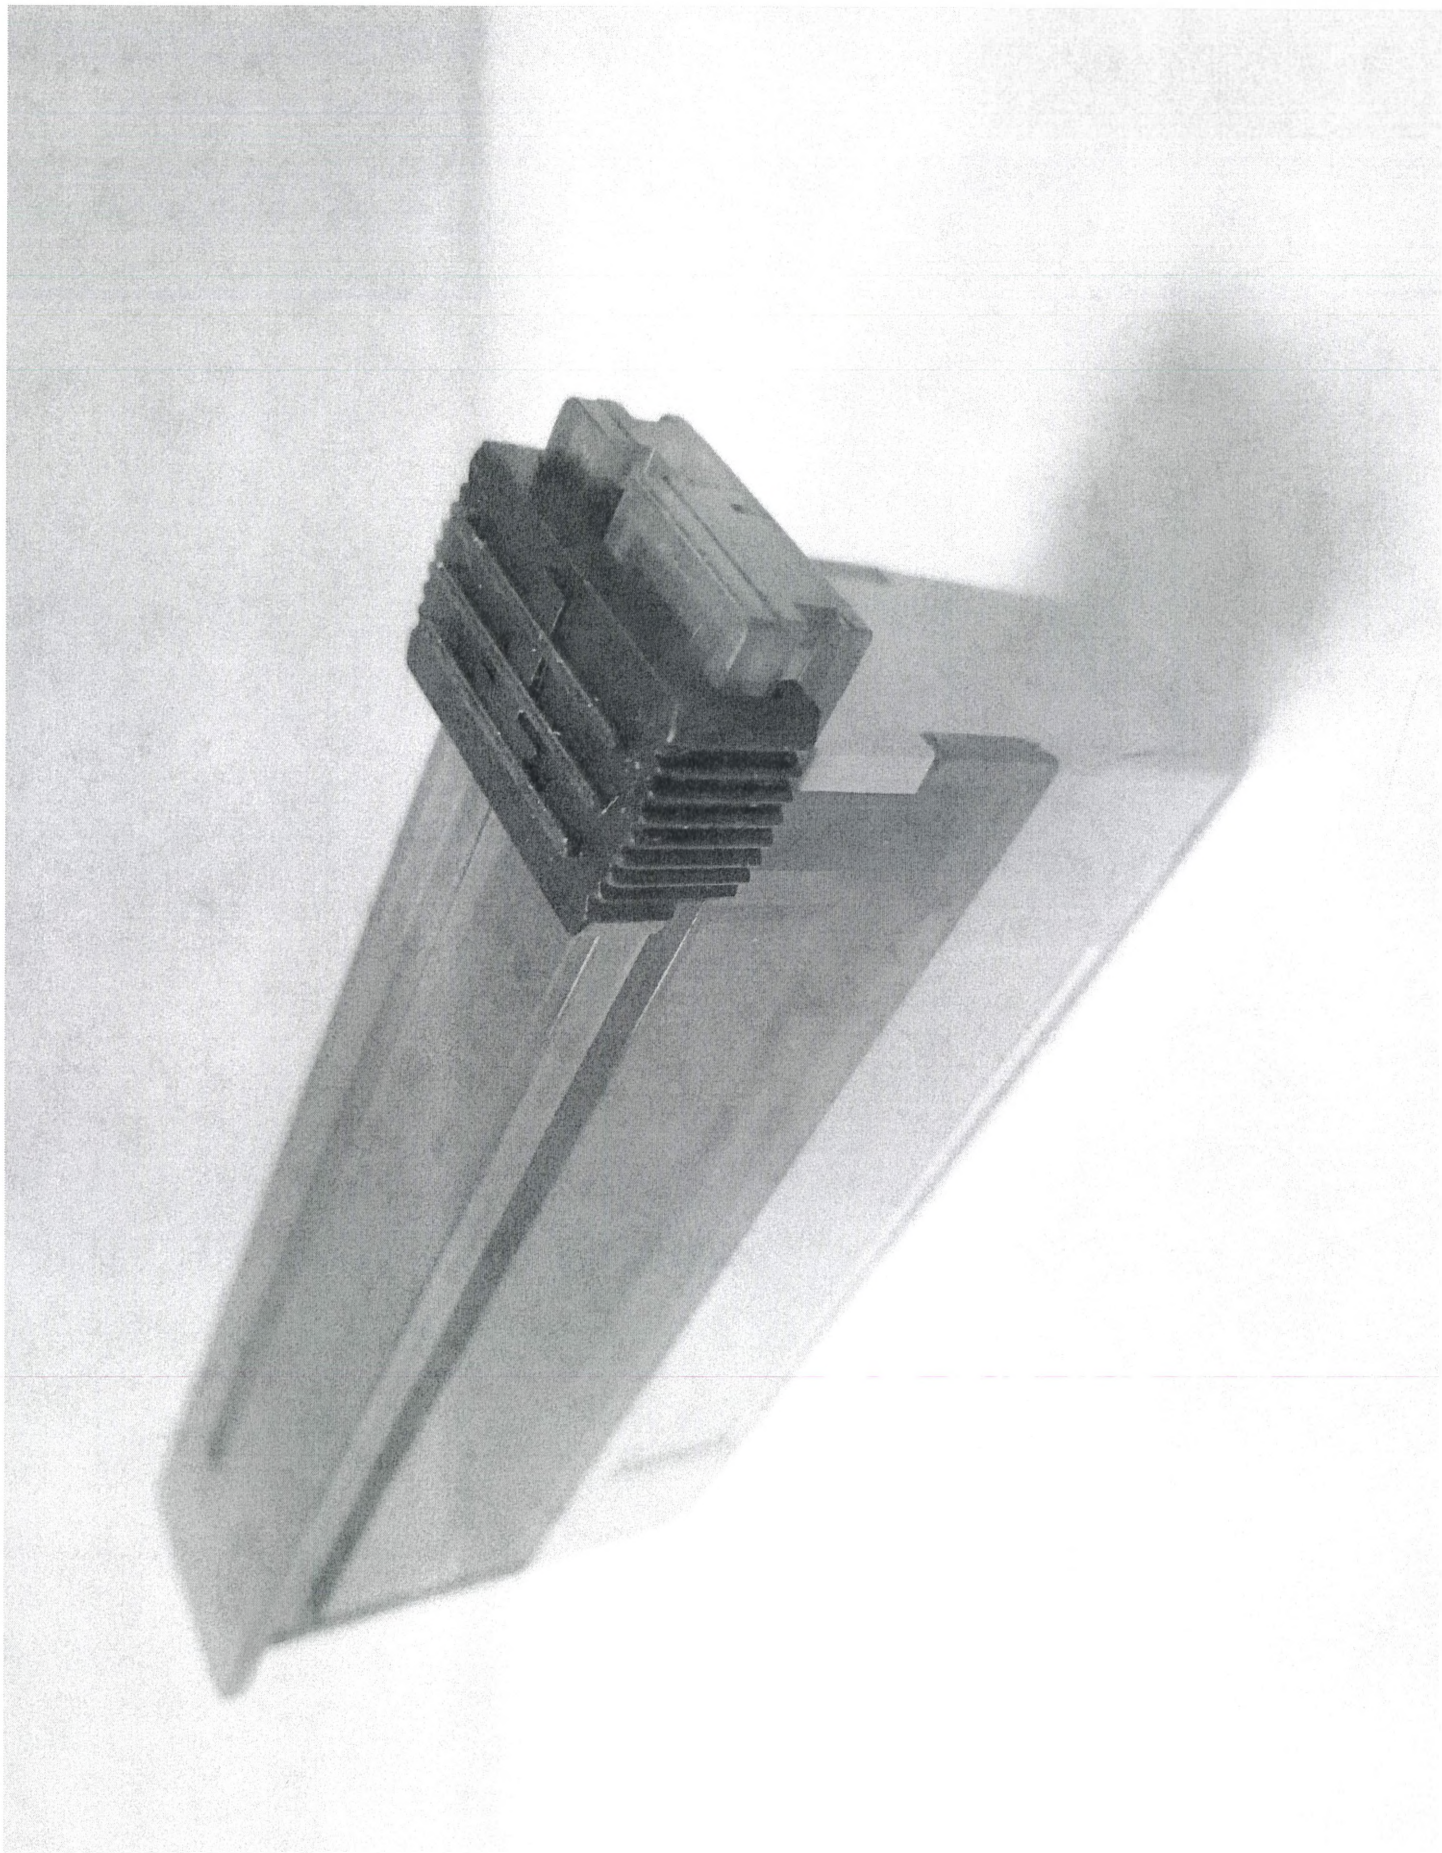

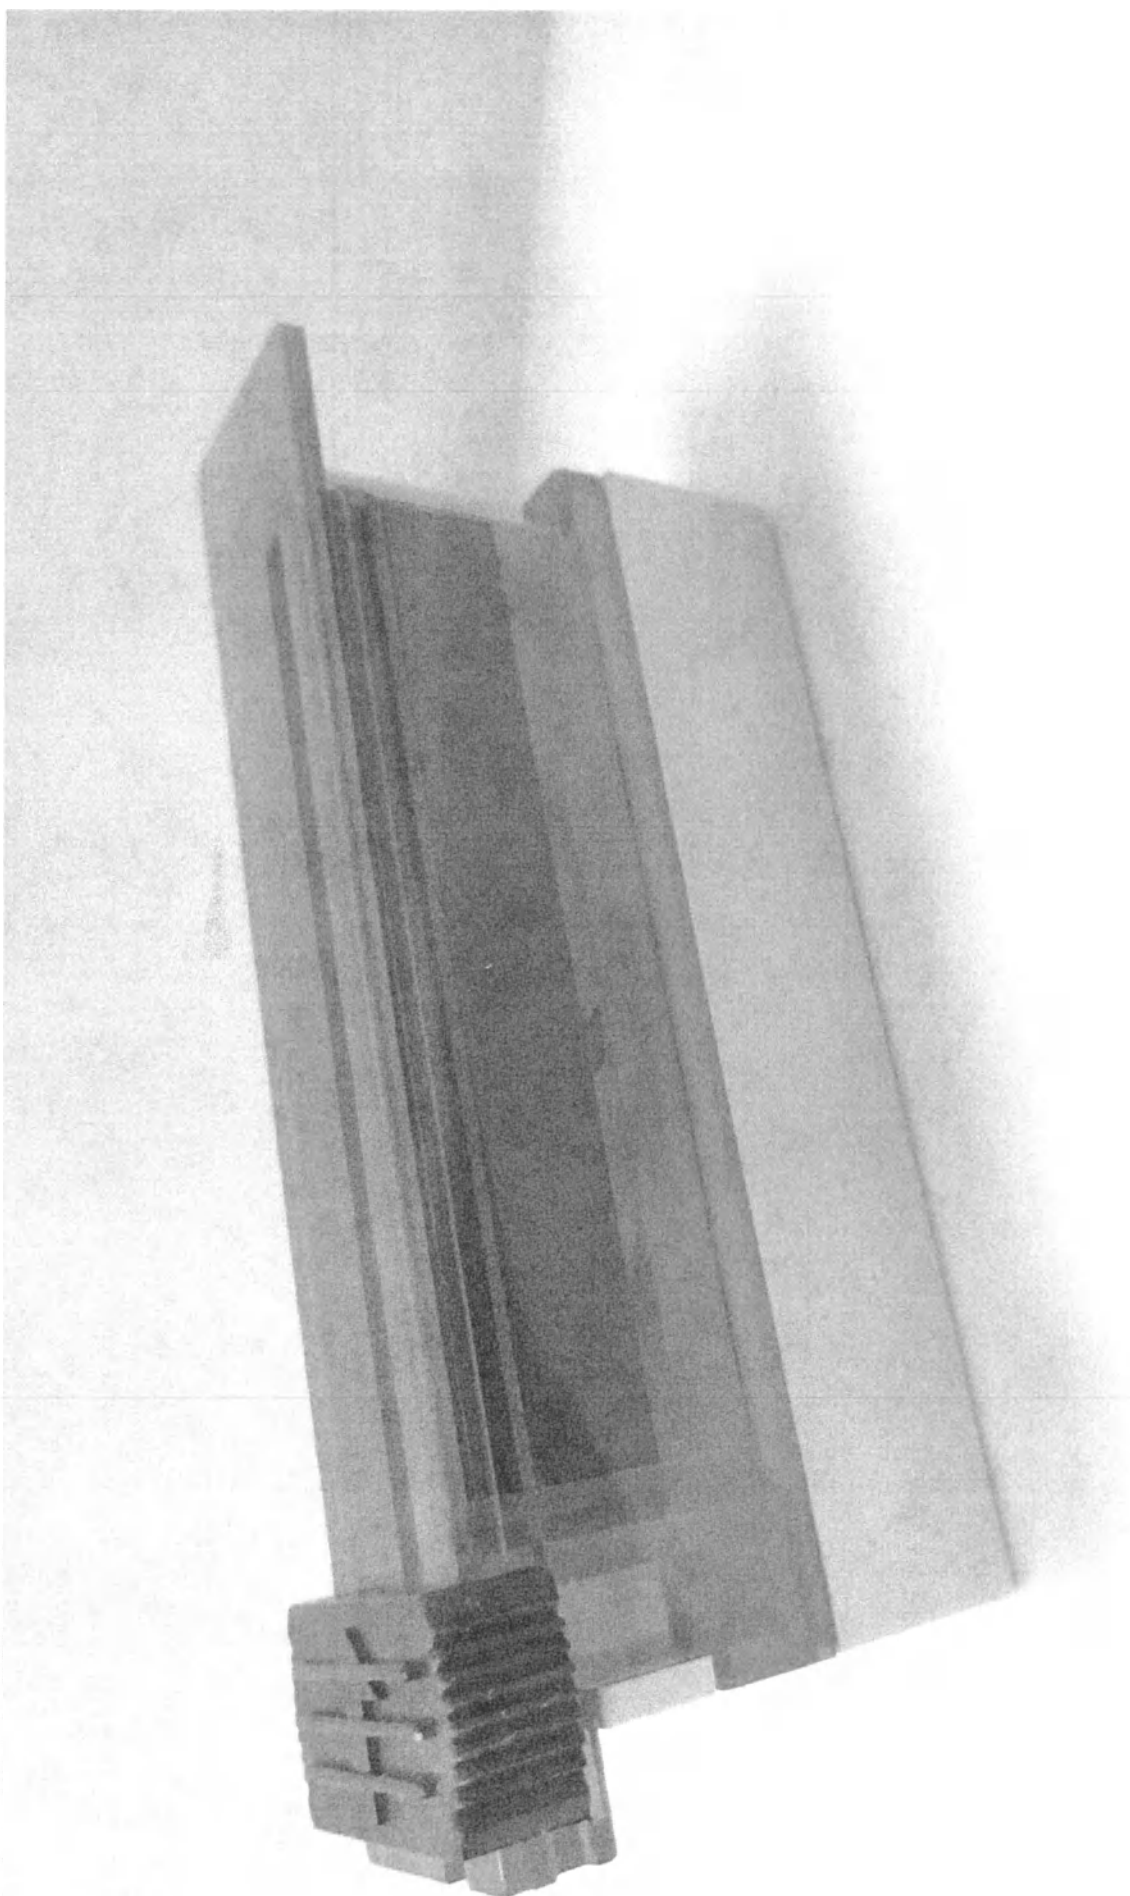

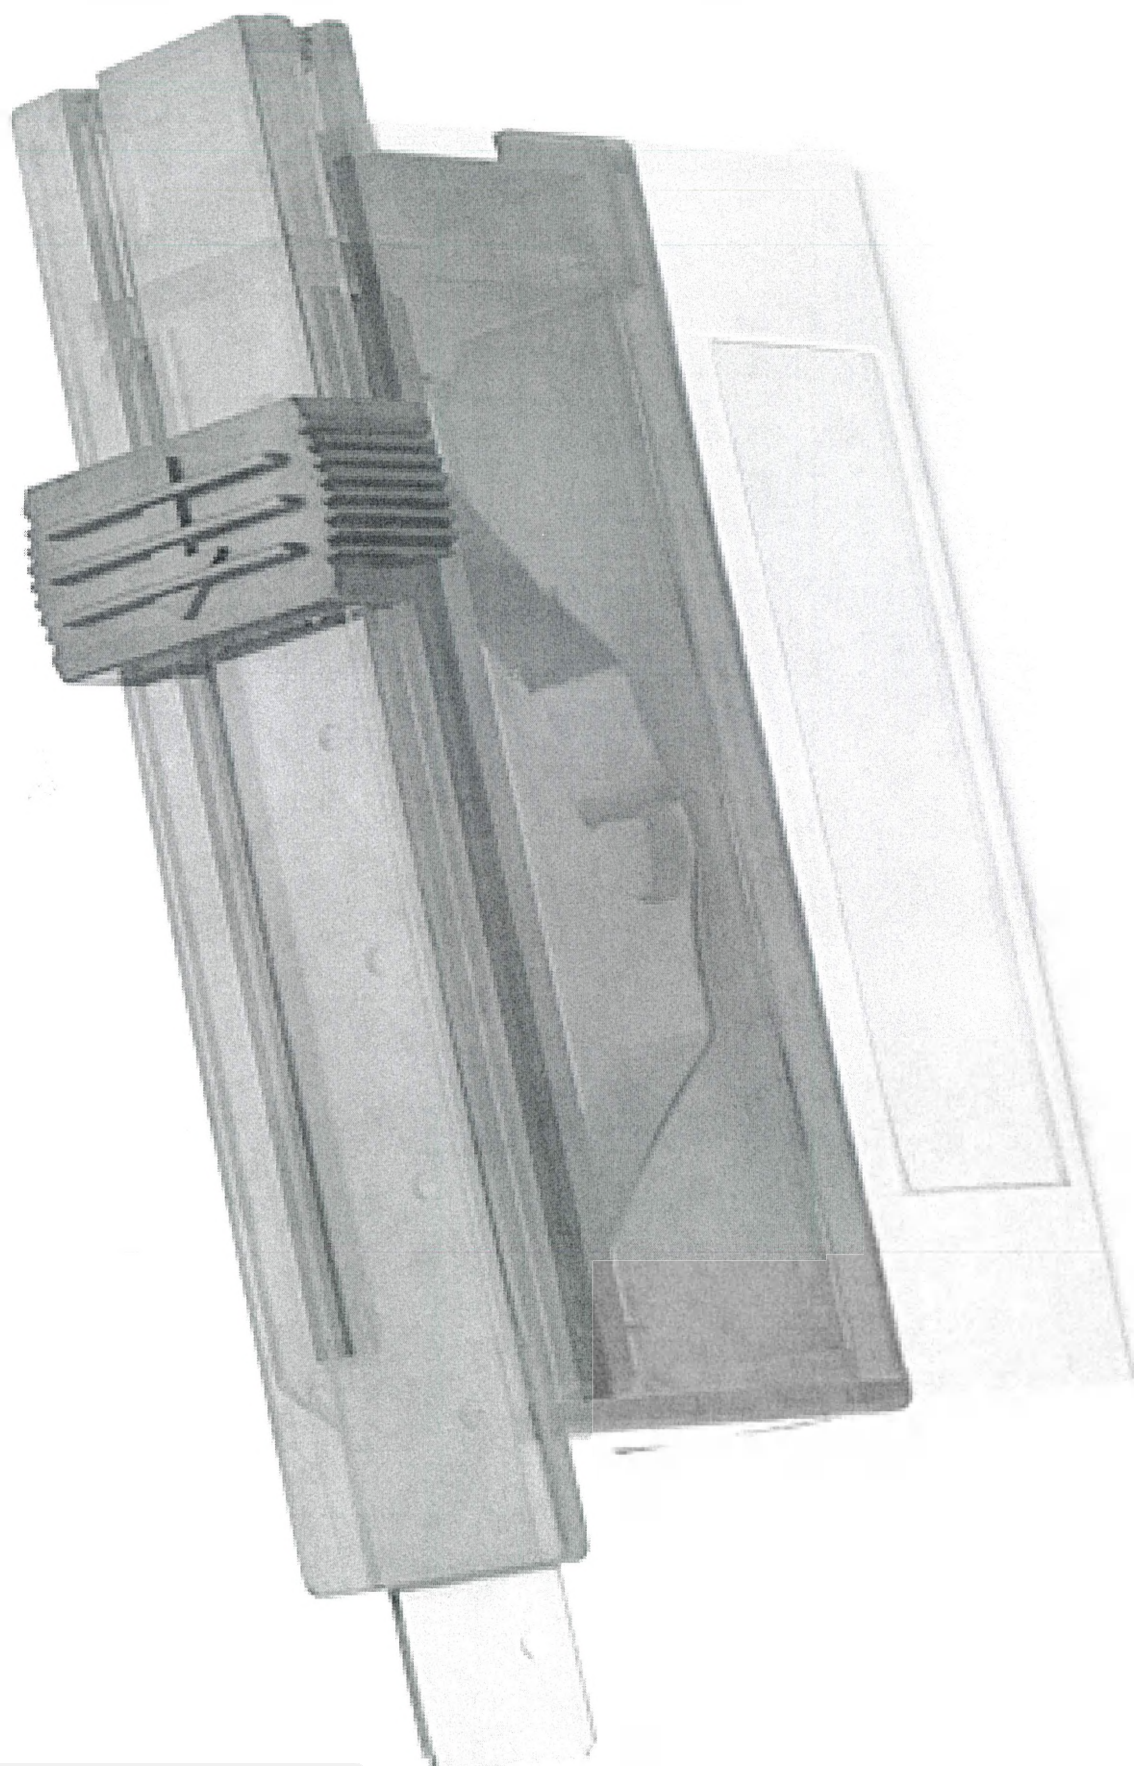

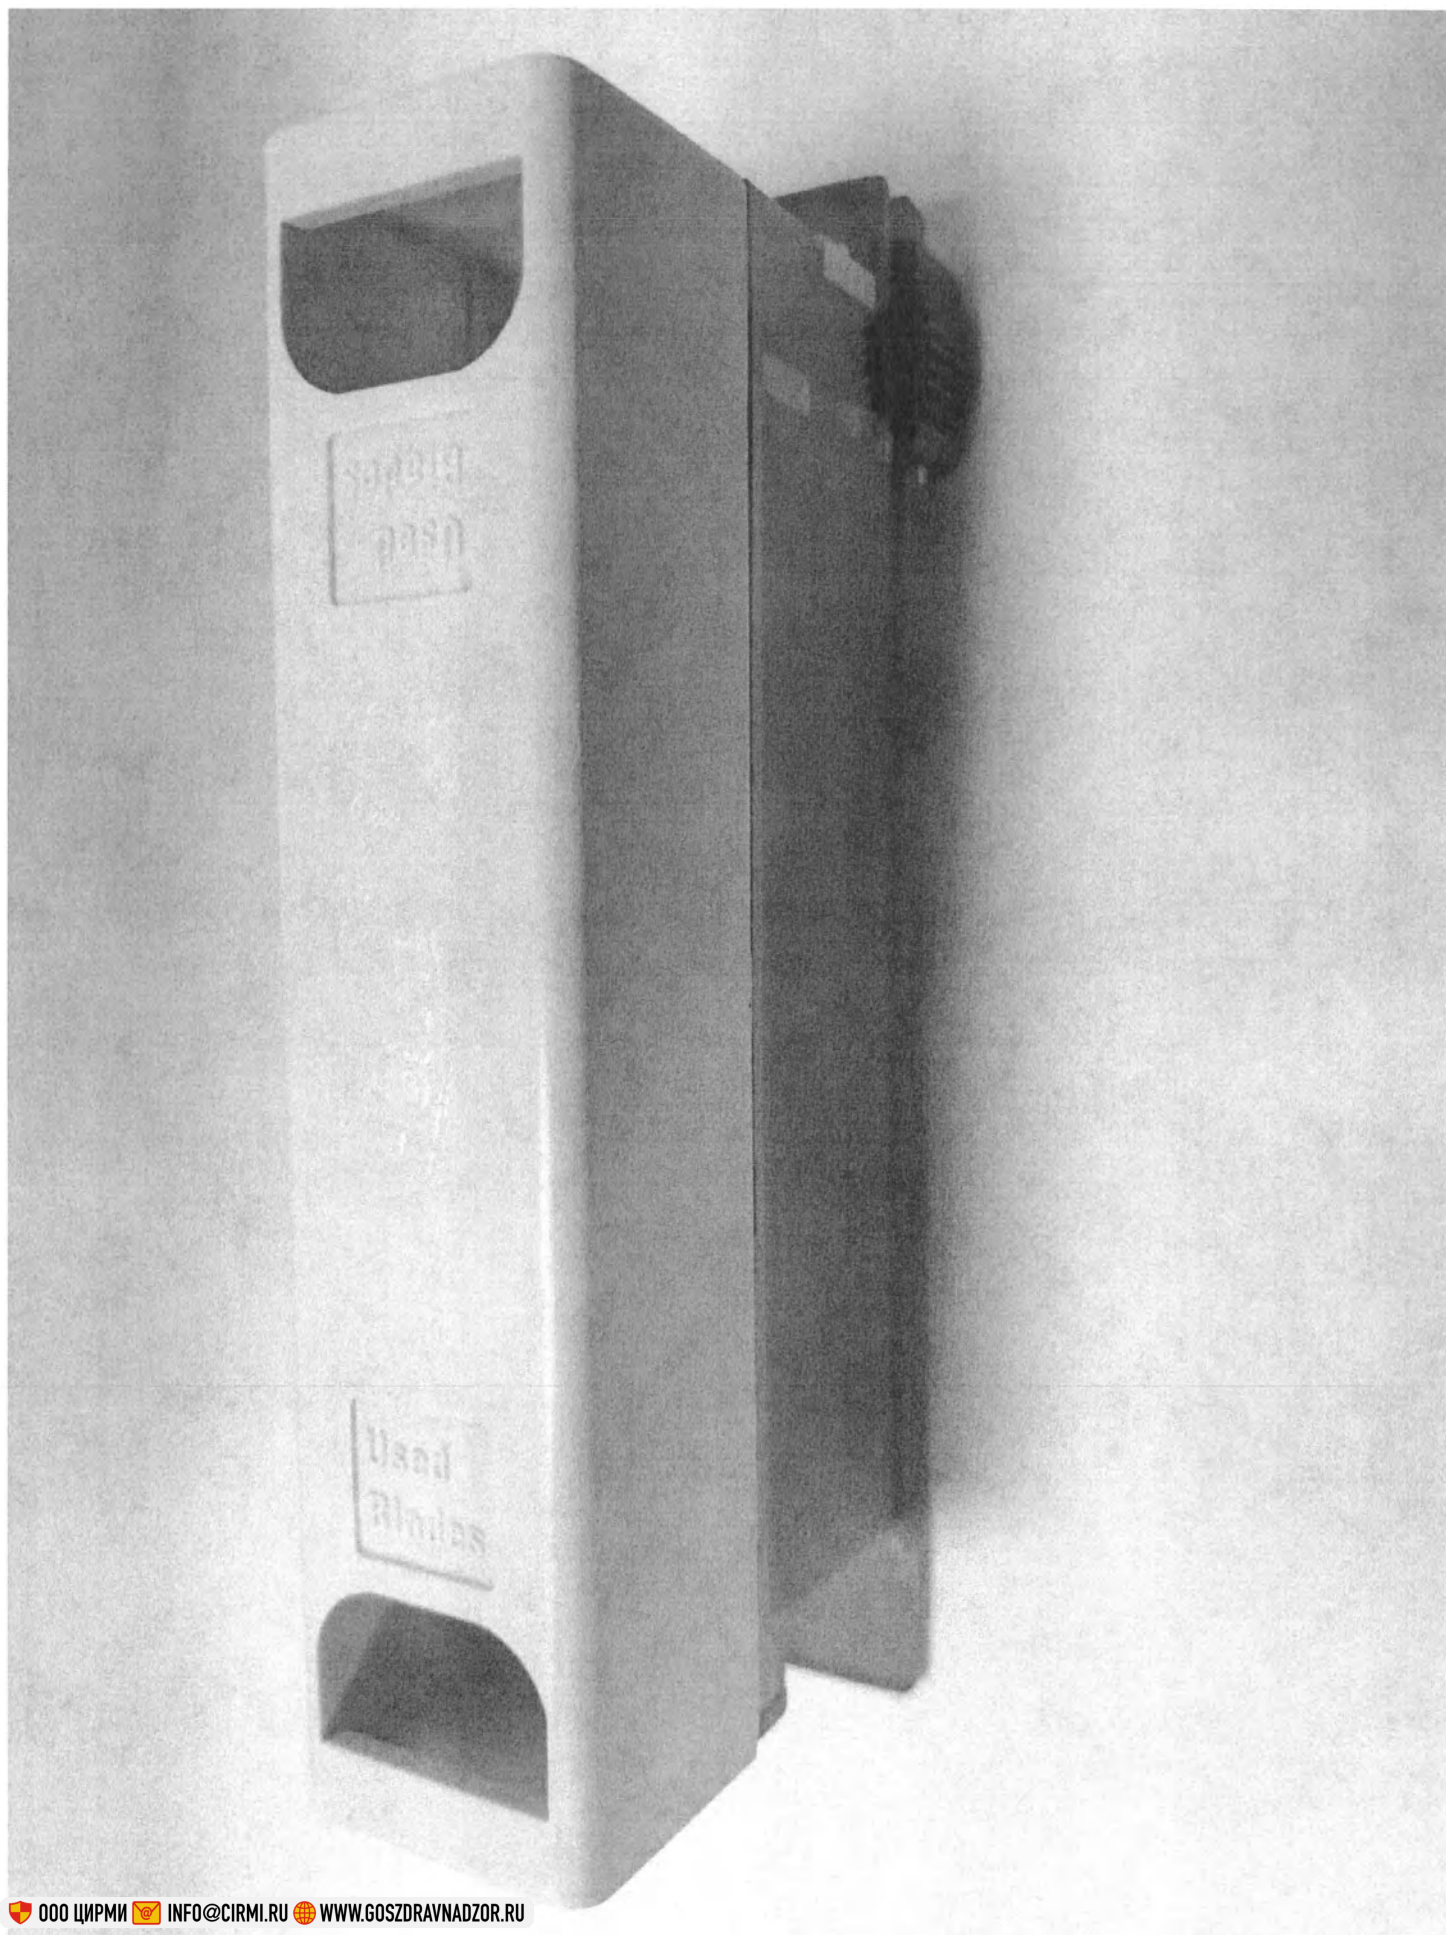

Раздел II.

**Изображения вариантов упаковки (фасовки), применяемых для каждого
из вариантов исполнения регистрируемого медицинского изделия**

Общее изображение всех вариантов исполнения регистрируемого медицинского изделия с вариантом упаковки «1х50 (1 малая коробка по 50 изделий)»

LEICA 819

Low Profile
Microtome Blades
50 Blades

LEICA 819

Low Profile
Microtome Blades
50 Blades

LEICA 818

High Profile
Microtome Blades
50 Blades

LEICA 818

High Profile
Microtome Blades
50 Blades

Leica DB80 LS

Low Profile Microtome Blades
For Standard Applications

Leica DB80 LS

Low Profile Microtome Blades
For Standard Applications

Leica DB80 LX

Low Profile Microtome Blades
For Standard Applications and Double

Leica DB80 HS

High Profile Microtome Blades
For Standard Applications


Leica DB80 HS

High Profile Microtome Blades
For Standard Applications



 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)

Made in Germany



95.11495 Rev C



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.
www.LeicaBiosystems.com

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)

Made in Germany




95.11495 Rev C



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.
www.LeicaBiosystems.com

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)

Made in Germany




95.11494 Rev C



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.
www.LeicaBiosystems.com

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)

Made in Germany




95.11494 Rev C



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.
www.LeicaBiosystems.com

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)


Made in Germany



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)


Made in Germany



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)


Made in Germany



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)


Made in Germany



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.

 Leica Biosystems Nussloch GmbH
D-69226 Nussloch (Germany)

Made in Germany



Use care when handling disposable blades for microtomes.
Place used blades in used blade compartment in the dispenser box.
Safely discard the dispenser box when all blades have been used.

Общее изображение варианта упаковки «10x50 (1 большая коробка по 500 изделий)» на примере варианта исполнения «Лезвия микротомные одноразовые низкого профиля Leica DB80LX (Leica DB80LX Low Profile Microtome Blades)», кат. номер 14035843497

Leica DB80 LX

Low Profile Microtome Blades

For Standard Applications-Extra Durable

Order No. 14035843407



CE

10 x 50 Blades

Leica
MICROSYSTEMS



Leica DB80 LX

Low Profile Microtome Blades

For Standard Applications-Extra Durable


Order No. 14035943497



CE

10 x 50 Blades

Leica
BIOSYSTEMS

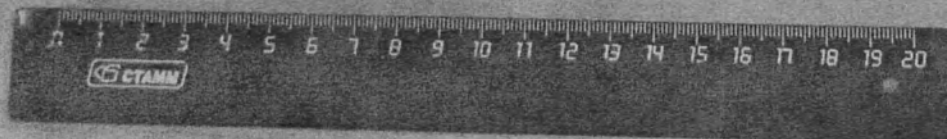

10 Dispenser

LOT

119343
10

35.11.05 Rev B

Leica DBM11

Low Profile Microplane Sensor

For Standard Applications



10 x 50 Standard

Leica

BIOSYSTEMS



Leica Biosystems Nussloch GmbH
Heidelberger Strasse 17-19
D-69226 Nussloch (Germany)
www.LeicaBiosystems.com
Made in Germany



CE





В настоящем документе прошито и
пронумеровано 1 лист
Генеральный директор
ООО «Биолайн»
Семенов А.В.

