

УТВЕРЖДАЮ

Генеральный директор
ООО «Синерджи Консалтинг»




Фотографические изображения

«Консоль системы ротационной атерэктомии ROTAPRO с принадлежностями»


Производитель: «Бостон Сайентифик Корпорейшн», США.

Boston Scientific Corporation, 300 Boston Scientific Way, Marlborough , MA 01752, USA

Фотографическое изображение общего вида: Консоль системы для ротационной атерэктомии ROTAPRO с принадлежностями.

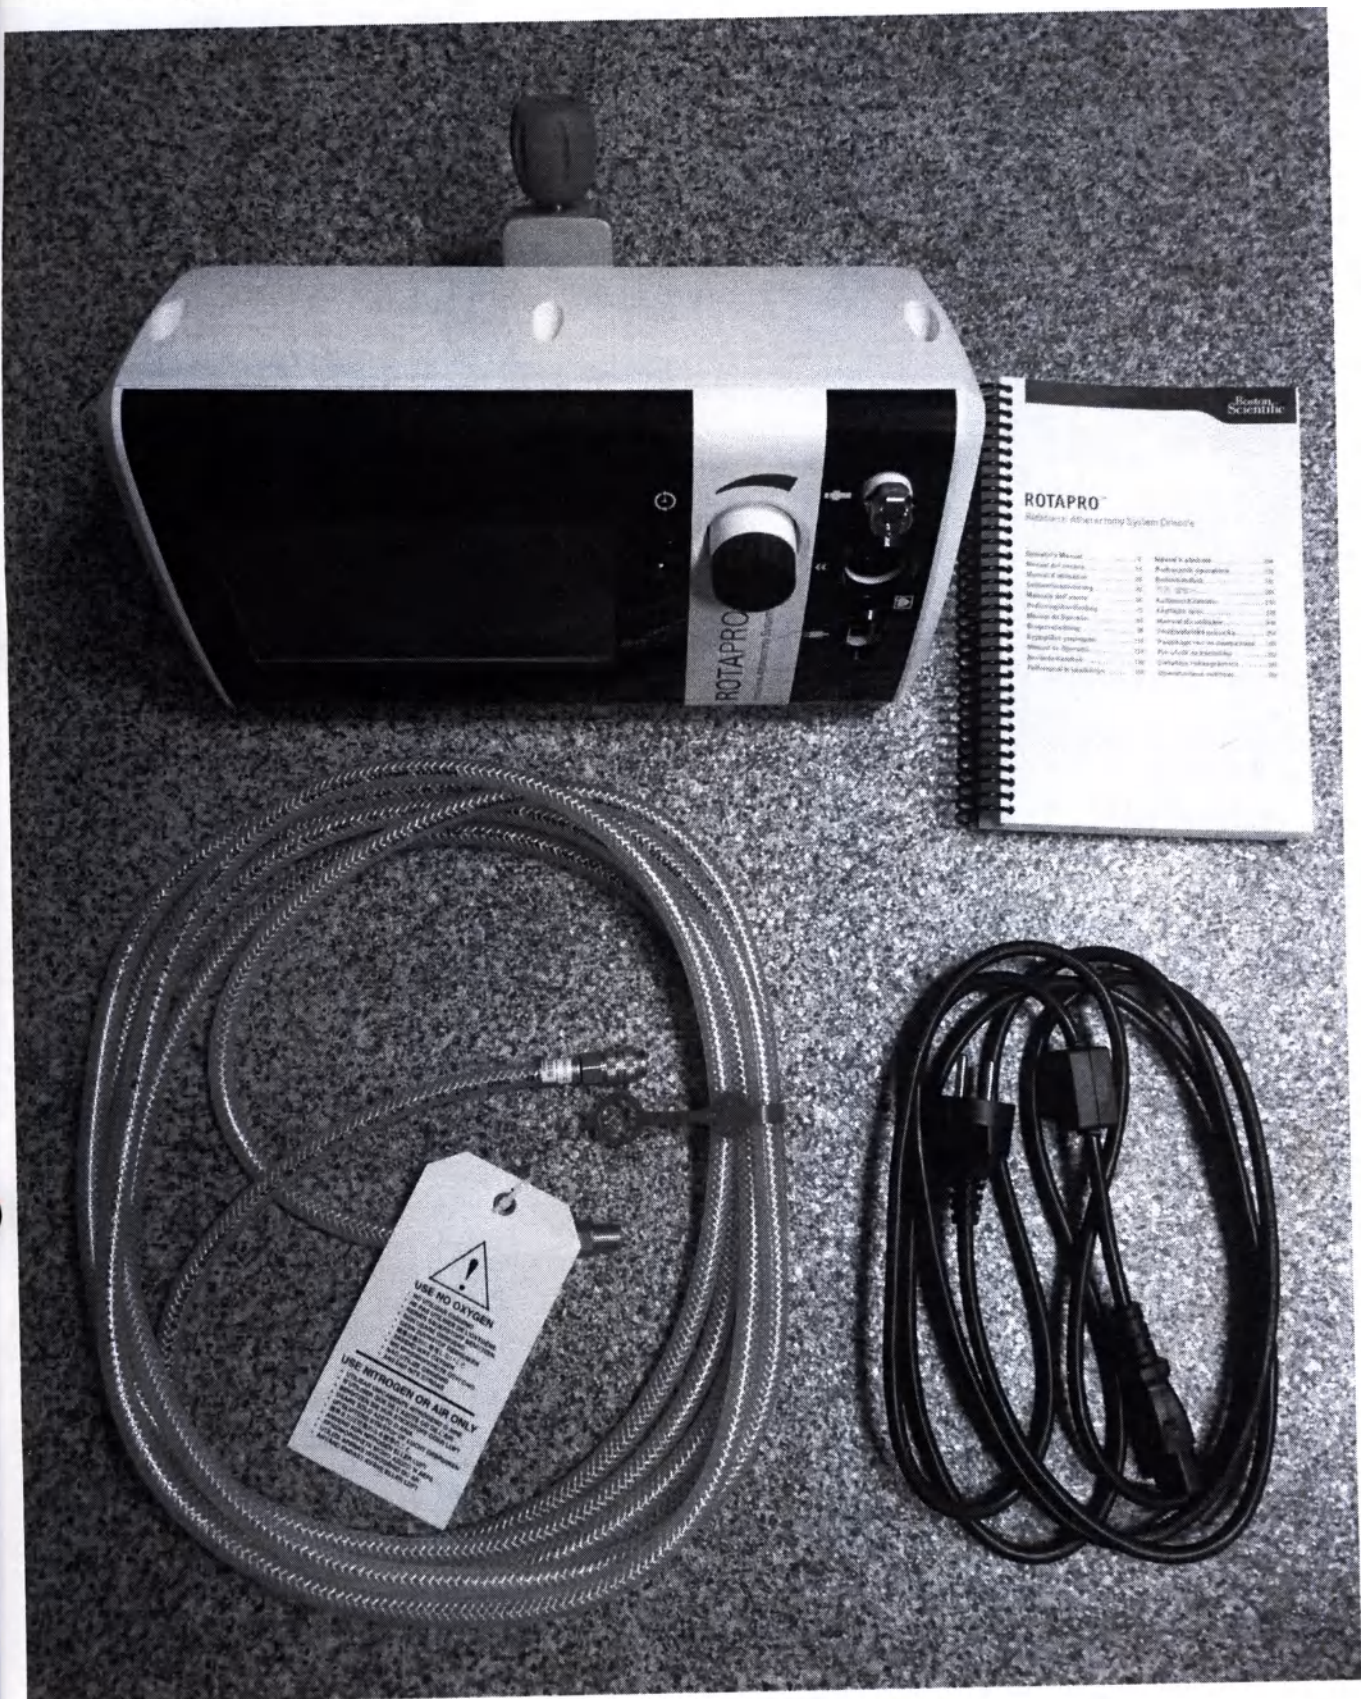

Фотографическое изображение общего вида: Консоль системы для ротационной атерэктомии ROTAPRO.

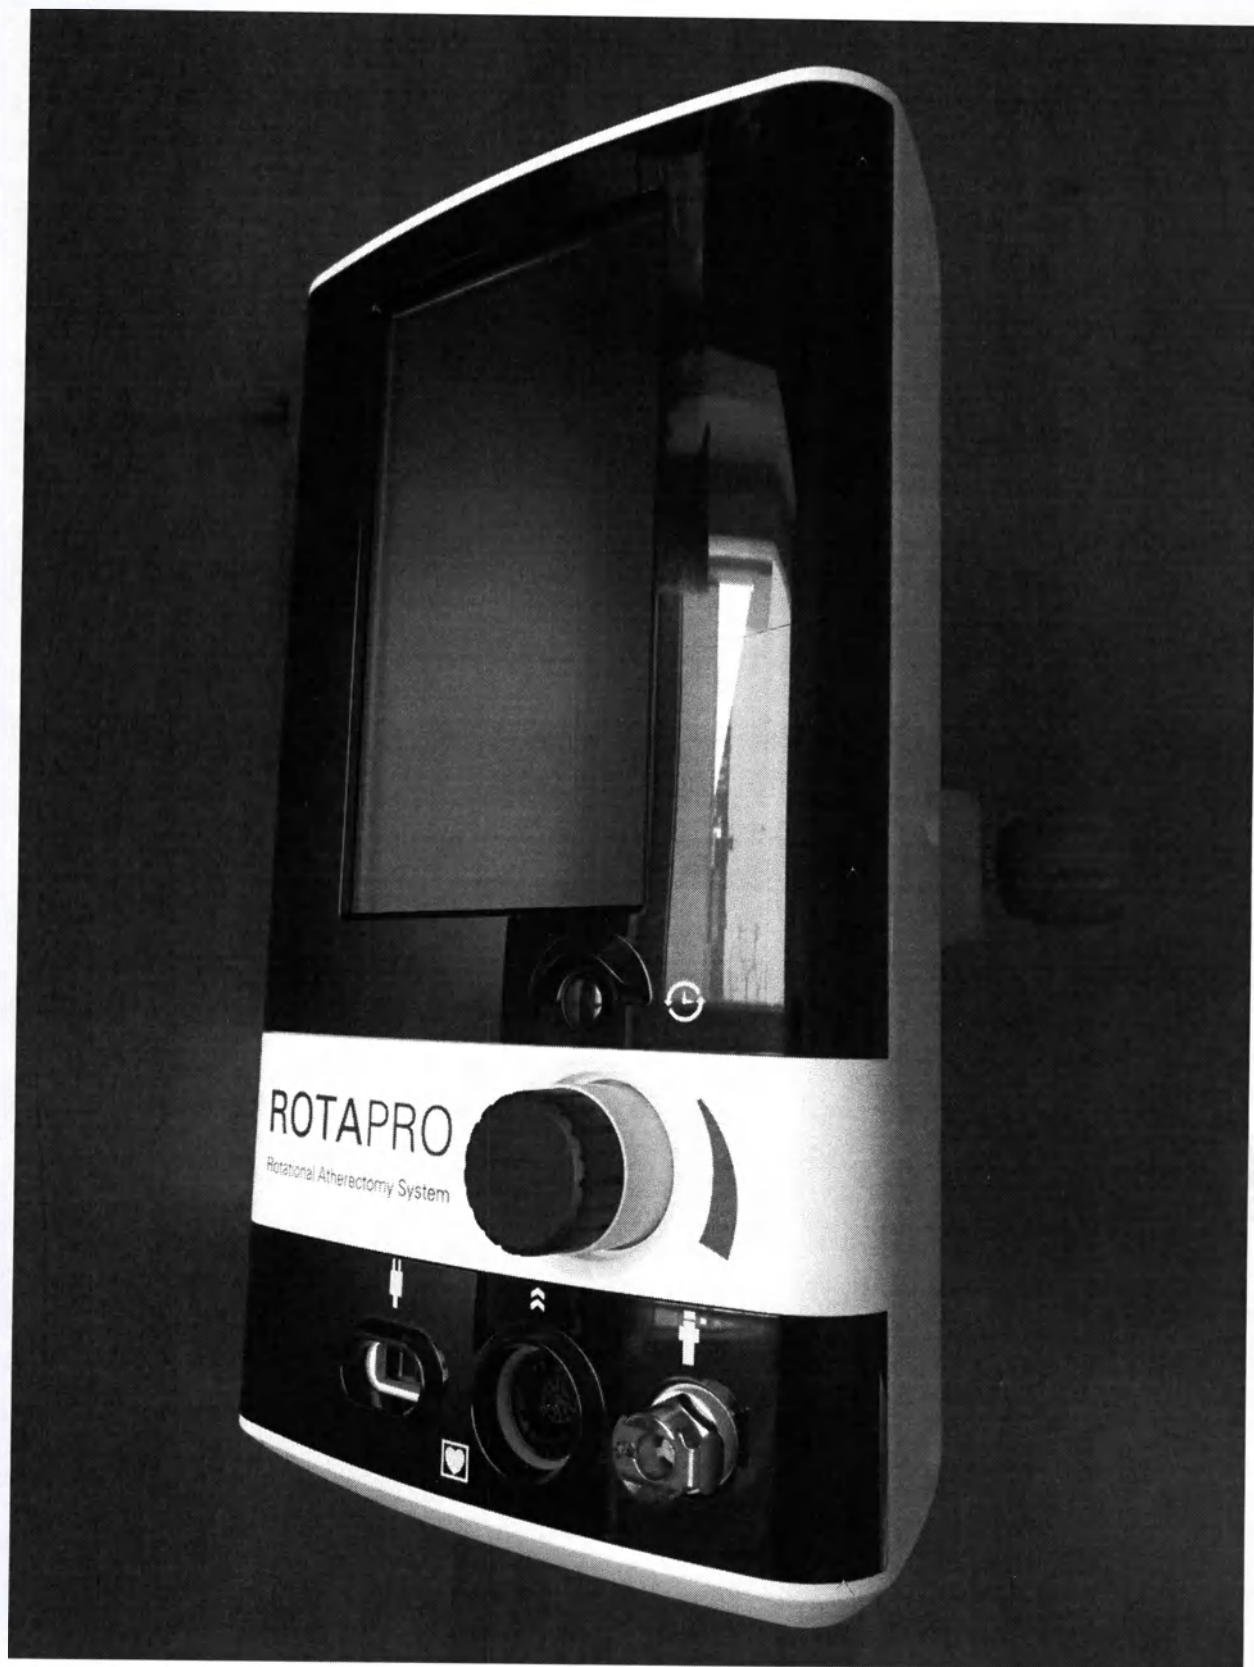

**Boston
Scientific**



50663104-01

REF Catalog No. H749 39309030
GTIN 08714729975151
LOT / SN Serial Number RP000655 
 Date of Manufacture 2019-05-29
92188690-09A

ROTAPRO™

Console

Consola, Console, Konsole, Console, console, Konsol, Κονσόλα, Consola, Konsol,
Konzol, Konzole, Konsola, Konsoll, Konsol, Konsoli, Consolă, Konzola, Консоль

Rx ONLY



**Follow Instructions
For Use**




**Separate
Collection**



CAUTION


**Attention: Consult
ACCOMPANYING DOCUMENTS.
AVERTISSEMENT.**

Attention : Lire les documents joints.



**Legal
Manufacturer**

Boston Scientific Corporation
300 Boston Scientific Way
Marlborough, MA 01752
USA
USA Customer Service 888-272-1001



**EU Authorized
Representative**


Boston Scientific Limited
Ballybrit Business Park
Galway
IRELAND

CE 0344

Made in USA:
150 Baytech Drive
San Jose, CA 95134
USA

This product may be protected by one or more patents. Patent information can be obtained at
<http://www.bostonscientific.com/patents>

Маркировка на изделии: Консоль системы для ротационной атерэктомии ROTAPRO.

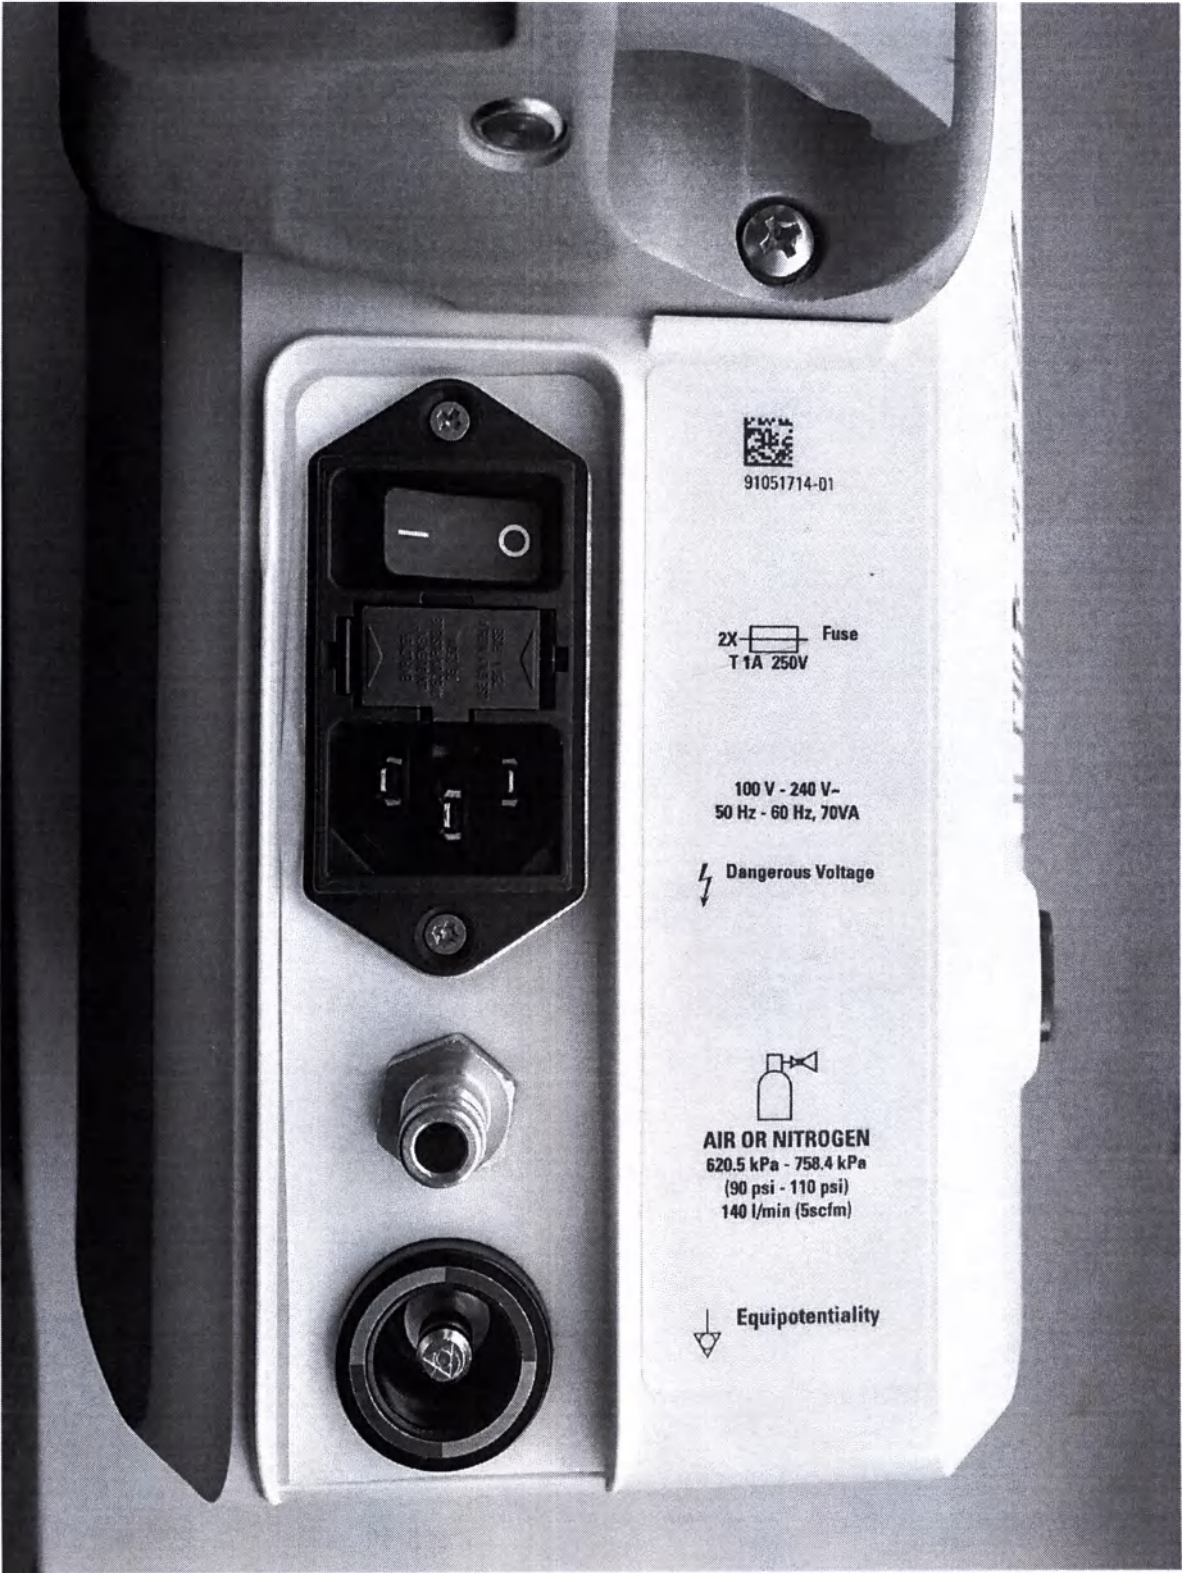

ROTAPRO™

Boston
Scientific

Rotational Atherectomy System

Sistema de aterectomia rotativa, Système d'athérectomie rotationnelle, Rotations-Atherectomiesystem, Sistema per aterectomia rotazionale, Roterbaar atherectomiesysteem, Roterende aterektomisystem, Σύστημα περιστροφικής αθηρεκτομής, Sistema de Aterectomia Rotacional, Roterande aterektomisystem, Rotációs aterektómia rendszer, Rotační aterektomický systém, System do aterektomii rotacyjnej, Roterande aterektomi-systeem, Rotasyonel Aterektomi Sistemi, Pyörivä aterektomiajärjestelmä, Sistem de aterectomie rotațională, Otočný aterektomický systém, Система ротационной атеректомии



Contents

- (1) Console, Console, Console, Konsola, Console, console, Konsol, Kονσόλα, Console, Konsol, Konzol, Konsole, Konsola, Konsoll, Konsol, Konsol, Konsol, Konsol, Kονσόλα
- (1) Accessories Set, Conjunto de accesorios, Ensemble d'accessoires, Zubehôr-Satz, Set of accessori, accessoireset, Tillbehôrset, Σet παρελκομένων, Conjunto de Accesorios, Tillbehôrssats, Tartozékkészlet, Sada príslušenství, Zestaw akcesoriów, Tillbehôrsett, Aksesuer Seti, Lisävarusteet, Set de accesorii, Súprava príslušenstva, Набор принадлежностей

Use only with ROTAPRO system

Utiliser uniquement avec le système ROTAPRO. Nur mit dem ROTAPRO System verwenden. Utilizzare solo con il sistema ROTAPRO. Alleen te gebruiken met het ROTAPRO-systeem. Kún til brug med ROTAPRO-systemet. Χρήση μόνο με το σύστημα ROTAPRO. Utilize apenas com o sistema ROTAPRO. Använd endast med ROTAPRO-systemet. Kiztrólag a ROTAPRO rendszerrel használja. Používať iba so systémom ROTAPRO. Używać wyłącznie z systemem ROTAPRO. Enk kan med ROTAPRO-systemet. Valinca ROTAPRO sistemni le kullatari. Käytä vain ROTAPRO-järjestelmän kanssa. Ase utilitas eksklusif cu sistemul ROTAPRO. Poizhivajte len so systémom ROTAPRO. Pôiznacevsa hupmo o sistemai ROTAPRO

GTIN 08714729975151

REF Catalog No.
H74939309030



9090527-01

Internal BSC Bar Code



91091721-008

CE 0344

Made in USA
150 Baytech Drive
San Jose, CA 95134 USA

Braided Air Hose Assembly Manufactured in Canada
Power Cord Manufactured in Taiwan



EU Authorized
Representative

Boston Scientific Limited
Ballybrit Business Park
Galway
IRELAND



Legal
Manufacturer

Boston Scientific Corporation
300 Boston Scientific Way
Marlborough, MA 01752
USA

USA Customer Service 888-272-1001

Rx ONLY



Separate
Collection



Do not use if package
is damaged.



Recyclable
Package



10% 95% Humidity
limitation.



CAUTION
Attention: Consult
ACCOMPANYING DOCUMENTS.
AVERTISSEMENT.
Attention : Lire les documents joints.

This product may be protected by one or more patents.
Patent information can be obtained at
<http://www.bostonscientific.com/patents>

60 °C Temperature limitation.



LOT RP000655

SN Serial Number
RP000655

Date of
Manufacture

2019-05-29



9090527-01

Internal BSC Bar Code

91091717-00A



(01)08714729975151 (11)190529 (10)RP000655 GS1




(21)RP000655

GS1


Фотографическое изображение общего вида: Набор принадлежностей, в составе:

- кабель питания, 3м (10ft).;**

- шланг для подводки газа прозрачный (ROTAPRO Gas Hose, Clear, 20')**

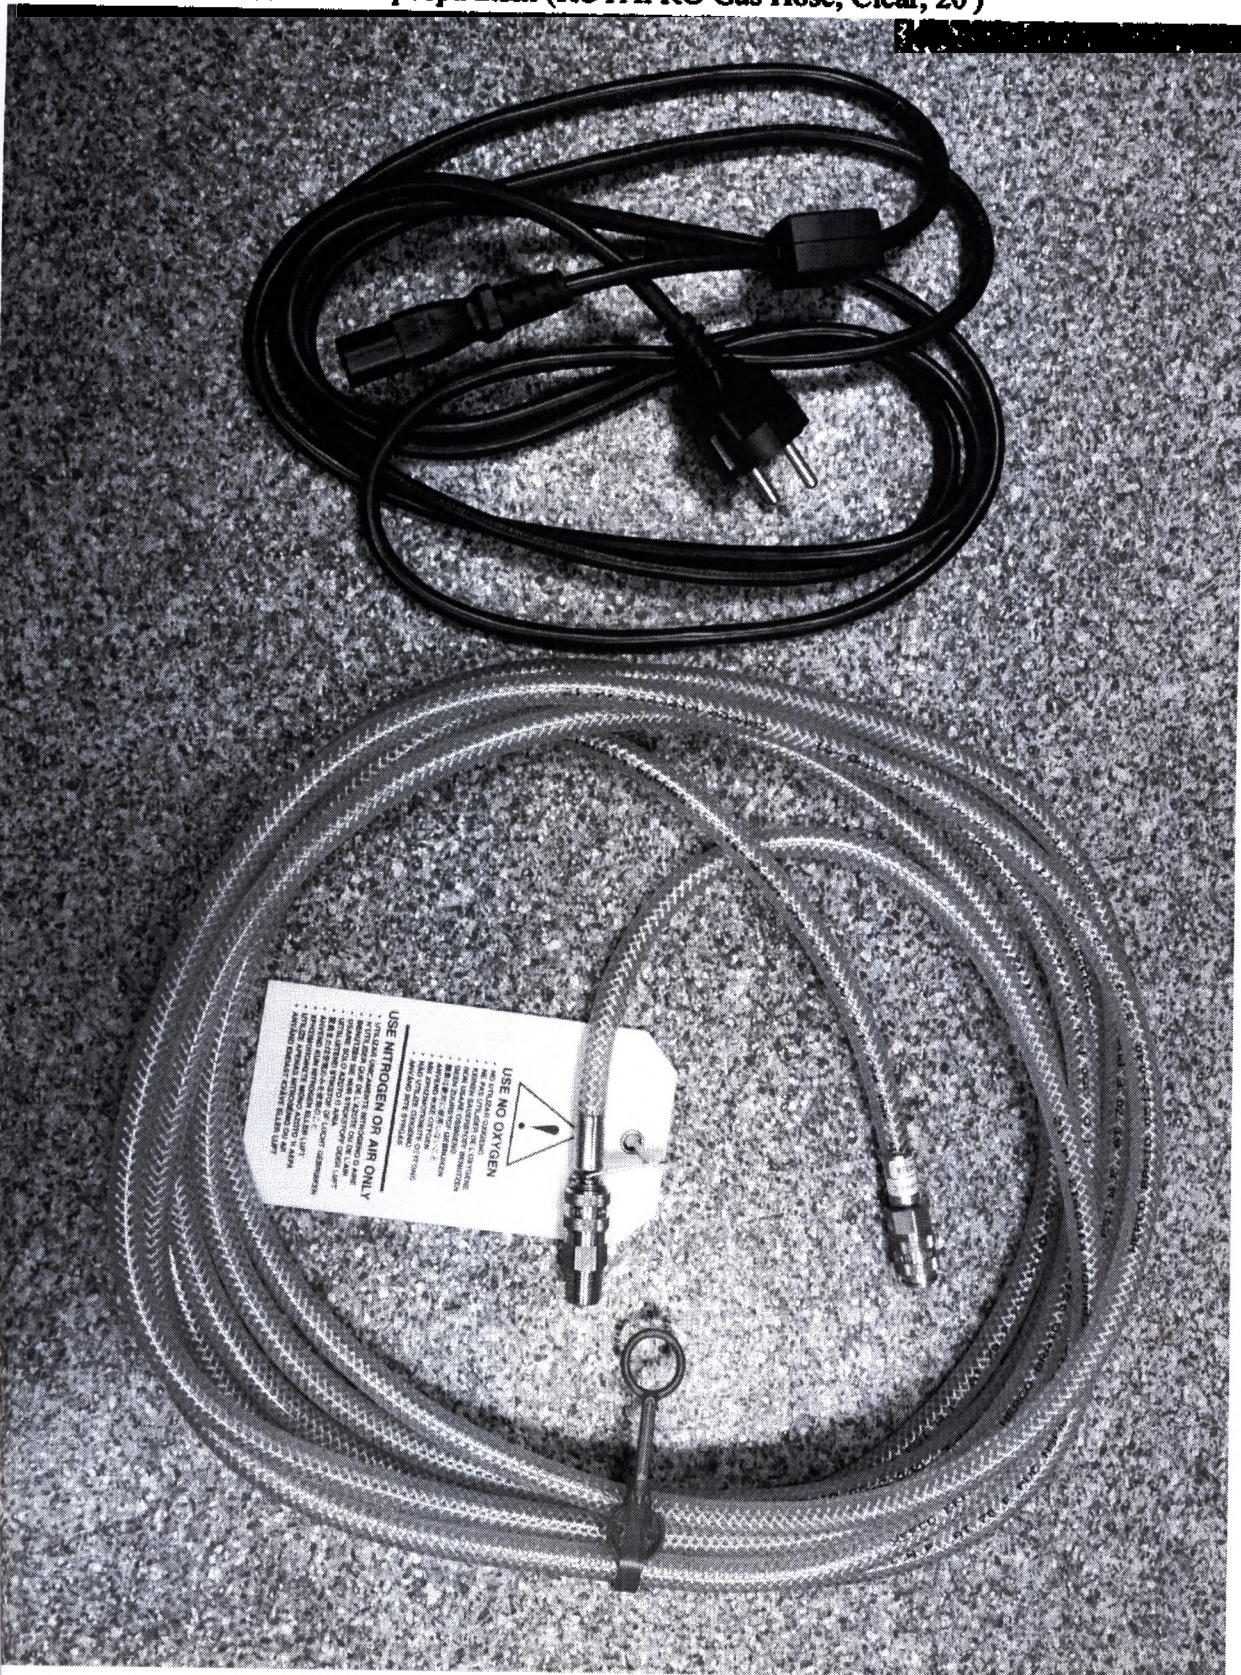

Ярлык на шланг для подводки газа прозрачный (ROTAPRO Gas Hose, Clear, 20')

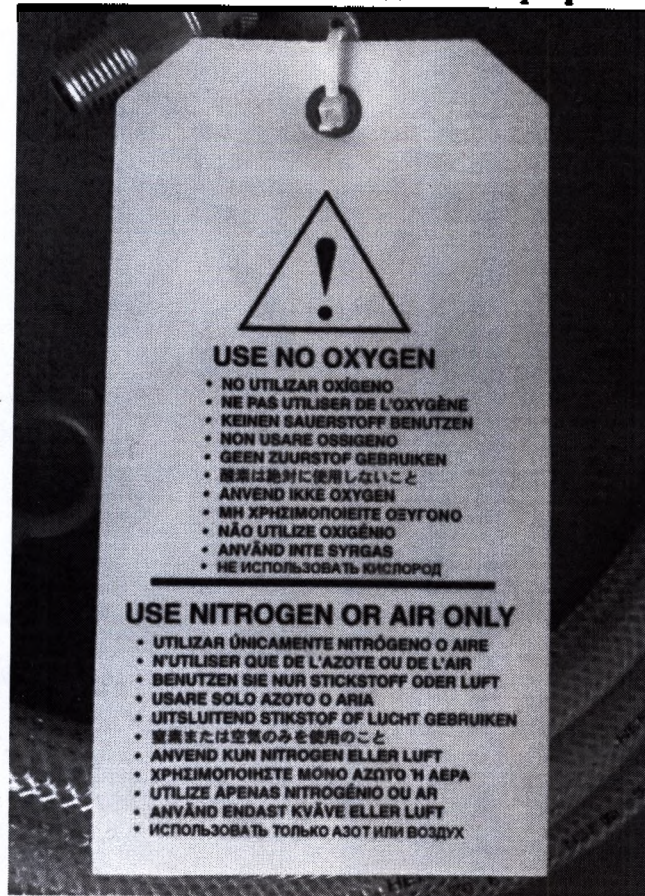

Прошито, пронумеровано
(8 лист(ов))
скреплено печатью

