

1 TEST
KIT

STANDARD Q

COVID-19 Ag Home Test

EN Nasal test | Result in 15 mins

ES Test nasal | Resultado en 15 mins

FR Test nasal | Résultat en 15 mins

PT Teste nasal | Resultado em 15 mins



Fix the solution tube.
Ponga el tubo en el paquete.
Fixer la tube de solution.
Coloque o tubo de solução.

LOT 5962571AC / Sub : 3


2021.04.30

2023.04.29



8 800111 705489

 SD BIOSENSOR

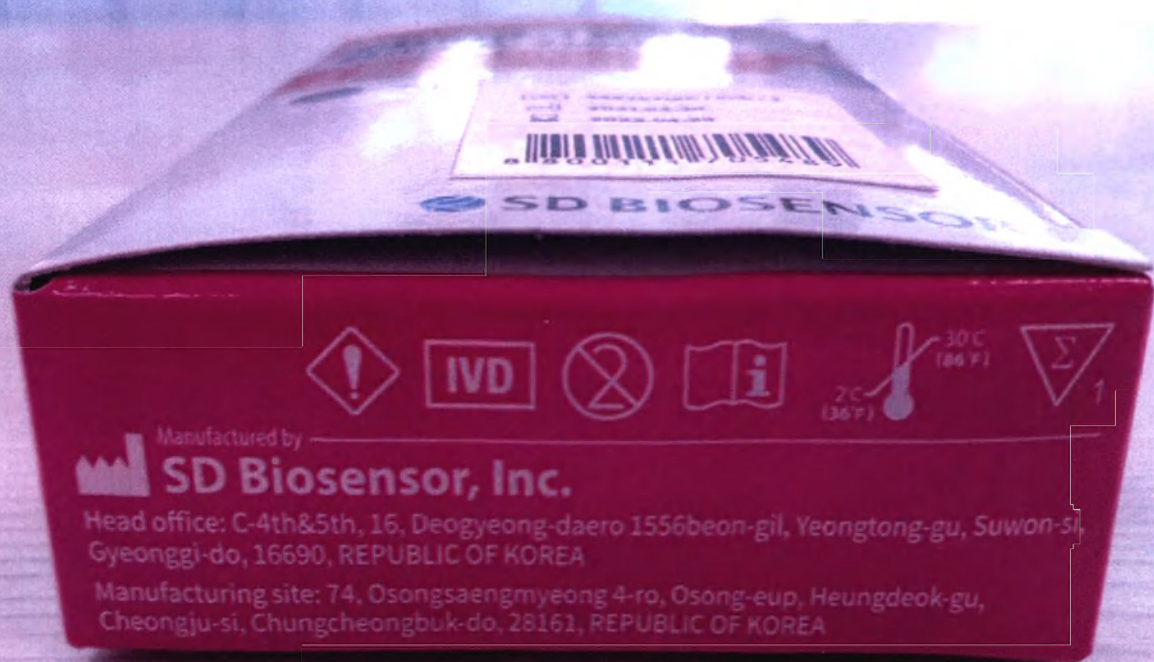

STANDARD Q
COVID-19 Ag Home Test



Video guide
Video de guía
Guide vidéo
Video de guía

www.sdbiosensor.com

 SD BIOSENSOR

EN

RU

INTERPRETATION OF TEST RESULTS

STANDARD Q

COVID-19 Ag Home Test

STANDARD™ Q COVID-19 Ag Home Test

SELF-DIAGNOSTIC TEST

Fast results in 15 minutes | Nasal Test

COVID-19 Antigen Test

Instructions for Use



Video Guide


 SD BIOSENSOR

Results	Example	Interpretation
Negative		Negative No test line appears result will be negative
Positive		Positive Test line appears result will be positive



STANDARD Q
COVID-19 Ag Test


iTest



STANDARDTM

/Item **STANDARD Q COVID-19 Ag Home Test**

REF /Ref **Q-NCOV-03G**

LOT /Lot **5962571AC / Sub : 3**

 /MFG DATE **2021.04.30**

 /EXP DATE **2023.04.29**

Manufactured by _____

MIL25RT15MLR0
Issue date : 2020.04



SD BIOSENSOR

에스디 바이오센서(주)
www.sdbiosensor.com

3



STANDARD™

STANDARD Q COVID-19 Ag Test

1 Test




COVID-19
Ag

C T
▲ ▲



Solution tube & Nozzle cap



www.sdbiosensor.com

SD BIOSENSOR

/ Item STANDARD Q COVID-19 Ag Home Test



/ LOT No.

STEB1021402



/ MFG DATE

2021.04.30.



/ EXP DATE

2023.04.29.

ML27COVIDENR1
Issue date: 2021.04

Manufactured by




SD BIOSENSOR

에스디 바이오센서(주)
www.sdbiosensor.com

40



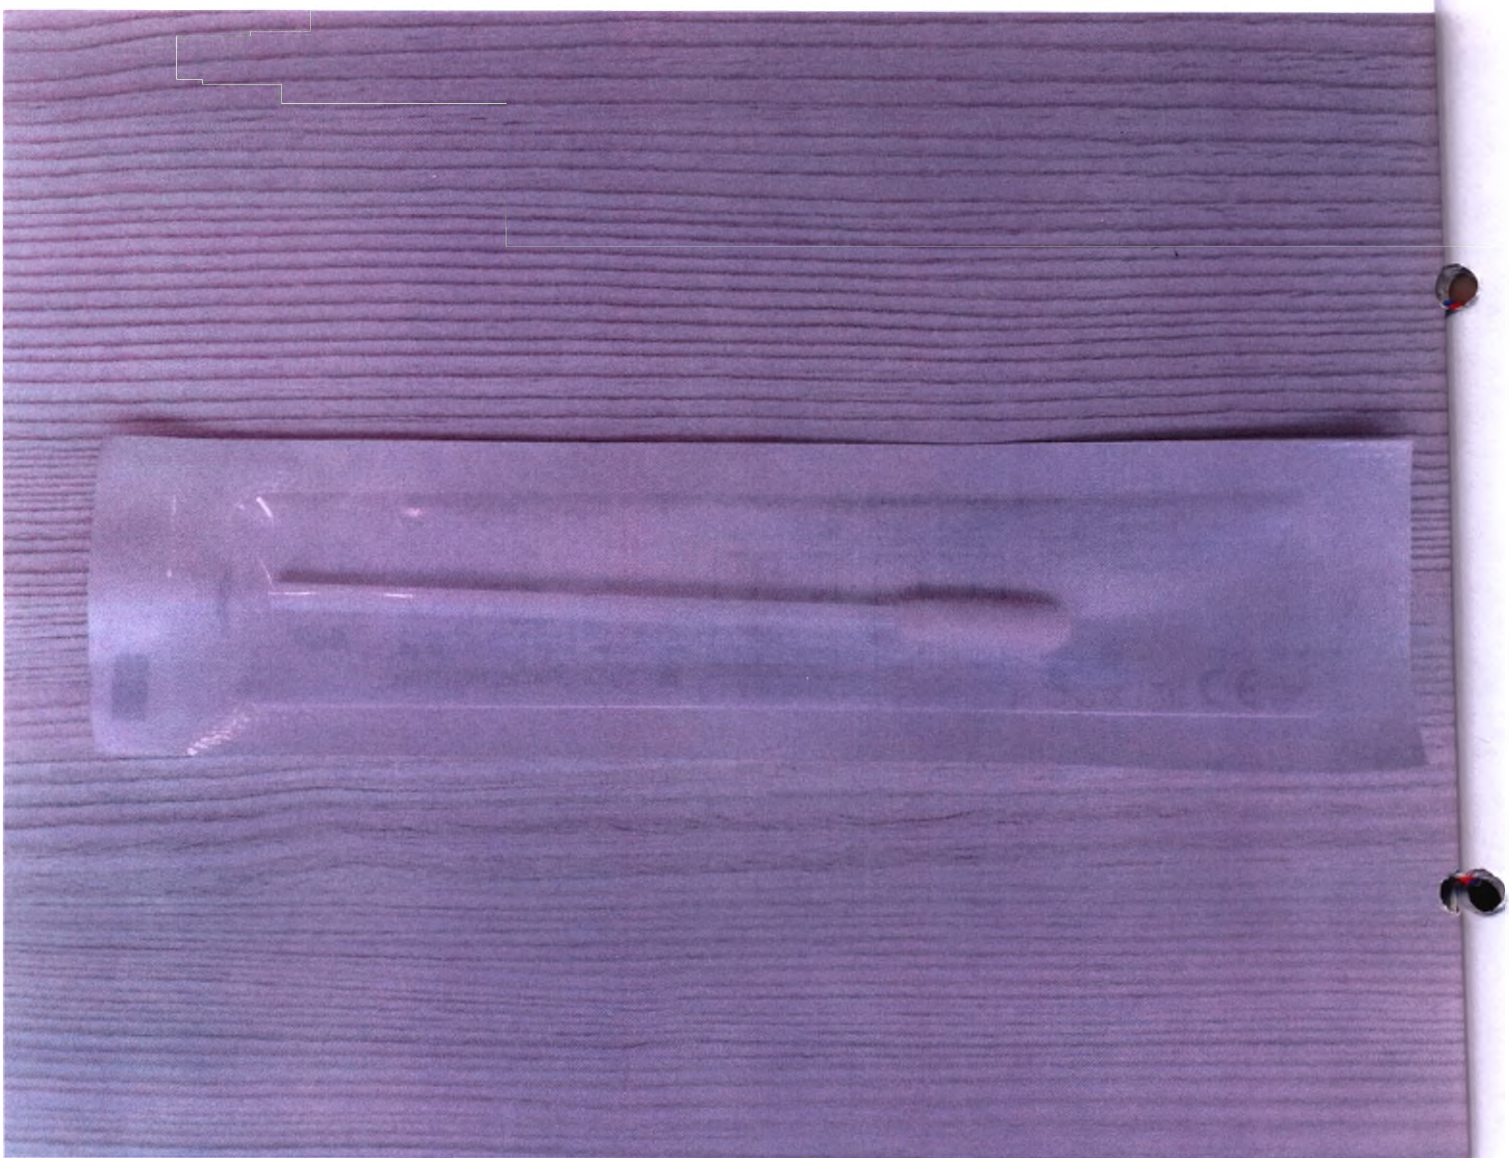



Miraclean Technology Co., Ltd.

Room 301, Building A, No. 18, Hongshata Industrial Zone, Tongxin Community, Baolong Street, Longgang District, Shenzhen, 518116, Guangdong, P.R. China

Tel: 86-755-89616772

Web: www.mantacc.com

P/N 96000G

LOT 2021040852

2021/04/16

2024/04/15

Disposable Sampling Swab 1pc



1. Peel apart the package



2. Remove the sterilized swab to collect samples



0197 FDA Registered



Share Info Consultant Service LLC
Repräsentanzbüro Heerdar
Lohweg 83, 40549 Düsseldorf

⚠ Use with caution if allergic to sponge and POM material.



Miraclean Technology Co., Ltd.

Room 301, Building A, No 18, Rongshu Industrial Zone, Tongxin Community, Baocong Street, Longgang District, Shenzhen, 518116, Guangdong, P.R. China

Tel: 86-755-89616772
Web: www.mantacc.com

P/N 96000G
LOT 2021040852
2021/04/16
2024/04/15

Disposable Sampling Swab 1 pc



1. Peel apart the package



2. Remove the sterilized swab to collect samples


⚠ Use with caution if allergic to sponge and POM material.



0197 FDA Registered



Share Info Consultant Service LLC
Repräsentanzbüro Heerdier
Lothweg 83, 40549 Düsseldorf

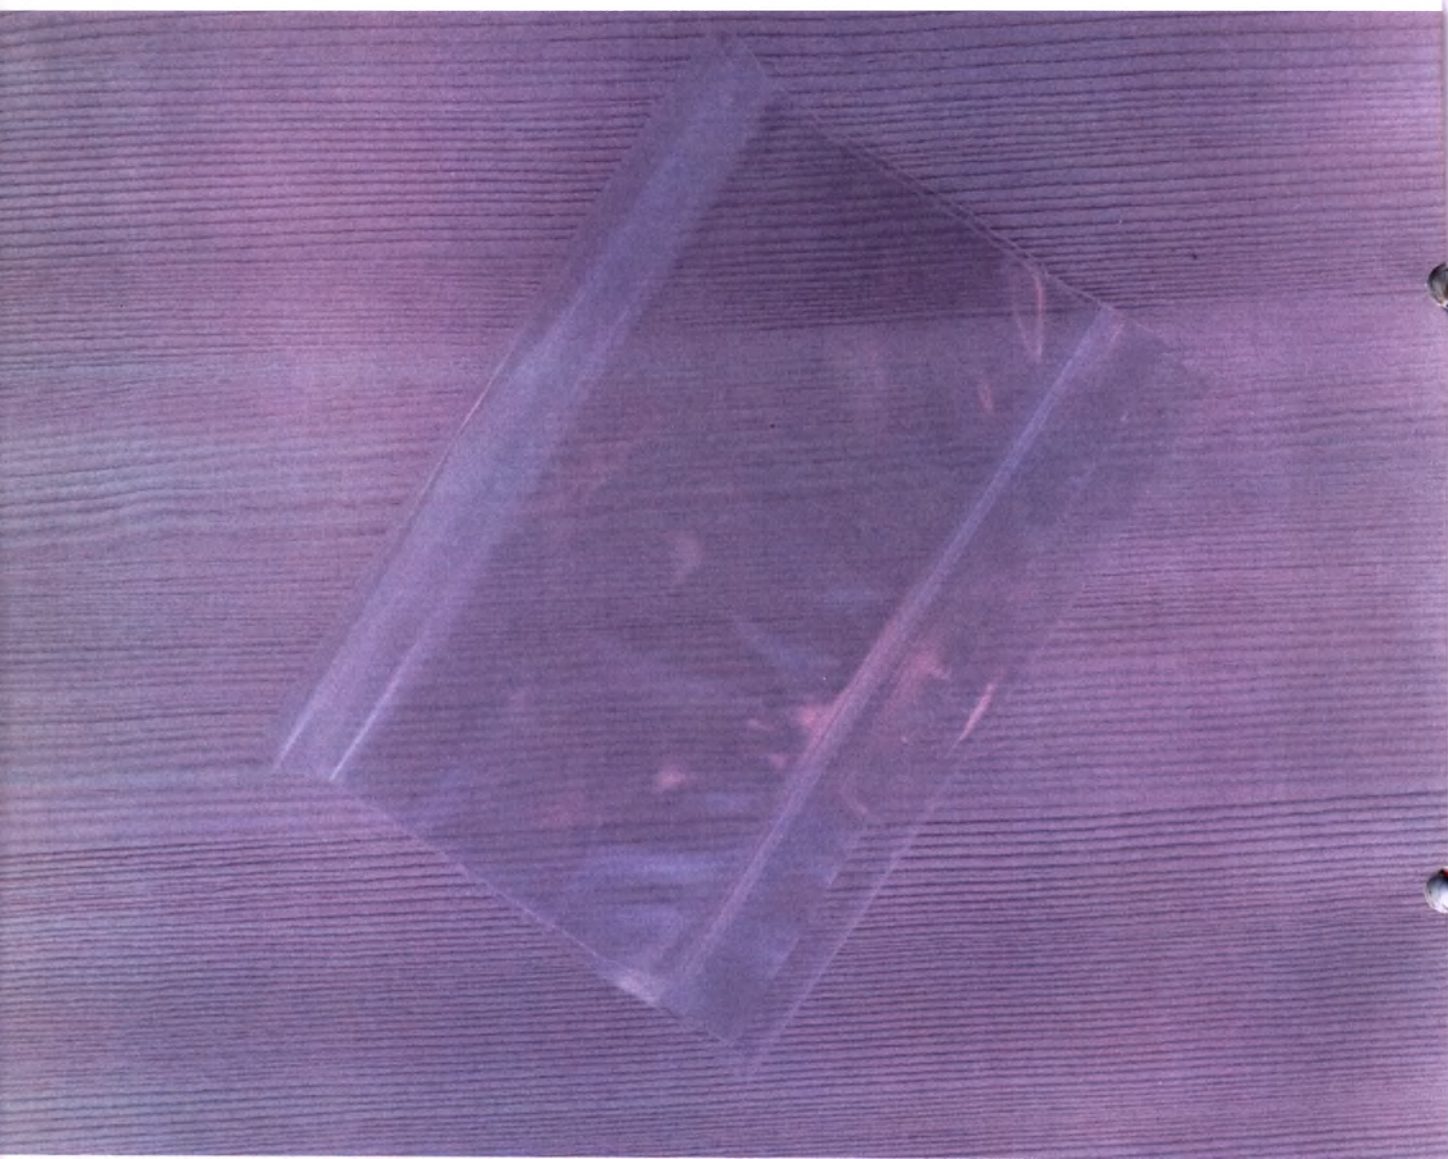



Прошито, пронумеровано и
скреплено печатью 16 листов.

Генеральный директор
ООО «Уайт Продакт»

Немцов В.Б.



**ФГБОУ ВО Московский государственный медико-стоматологический университет
имени А.И. Евдокимова Минздрава России**

127473, Москва, ул. Делегатская, д.20, стр.1

«СОГЛАСОВАНО»

ООО «Уайт Продакт»

Генеральный директор



«___» _____ Немцов В.Б.
2021 года



«УТВЕРЖДАЮ»

ФГБОУ ВО МГМСУ им. А.И. Евдокимова

Минздрава России

Проректор по научной работе



«___» _____ Крихели Н.И.
2021 года



ПРОГРАММА КЛИНИКО-ЛАБОРАТОРНЫХ ИСПЫТАНИЙ

Медицинского изделия для диагностики in vitro

Набор реагентов для иммунохроматографического выявления антигена SARS-CoV-2 в мазке из носа человека (STANDARD Q COVID-19 Ag Home Test). Lot 5962571AC/ Sub: 3.

№06-09/21-ИФА/1 от 06.09.2021