



Фотографические изображения медицинского изделия «Стент с системой доставки», производства
«Тазвоонг Медикал Ко., Лтд», Республика Корея
«Taewoong Medical Co., Ltd.», 14 Gojeong-ro, Wolgot-myeon, Gimpo-si, Gyeonggi-do, Korea.



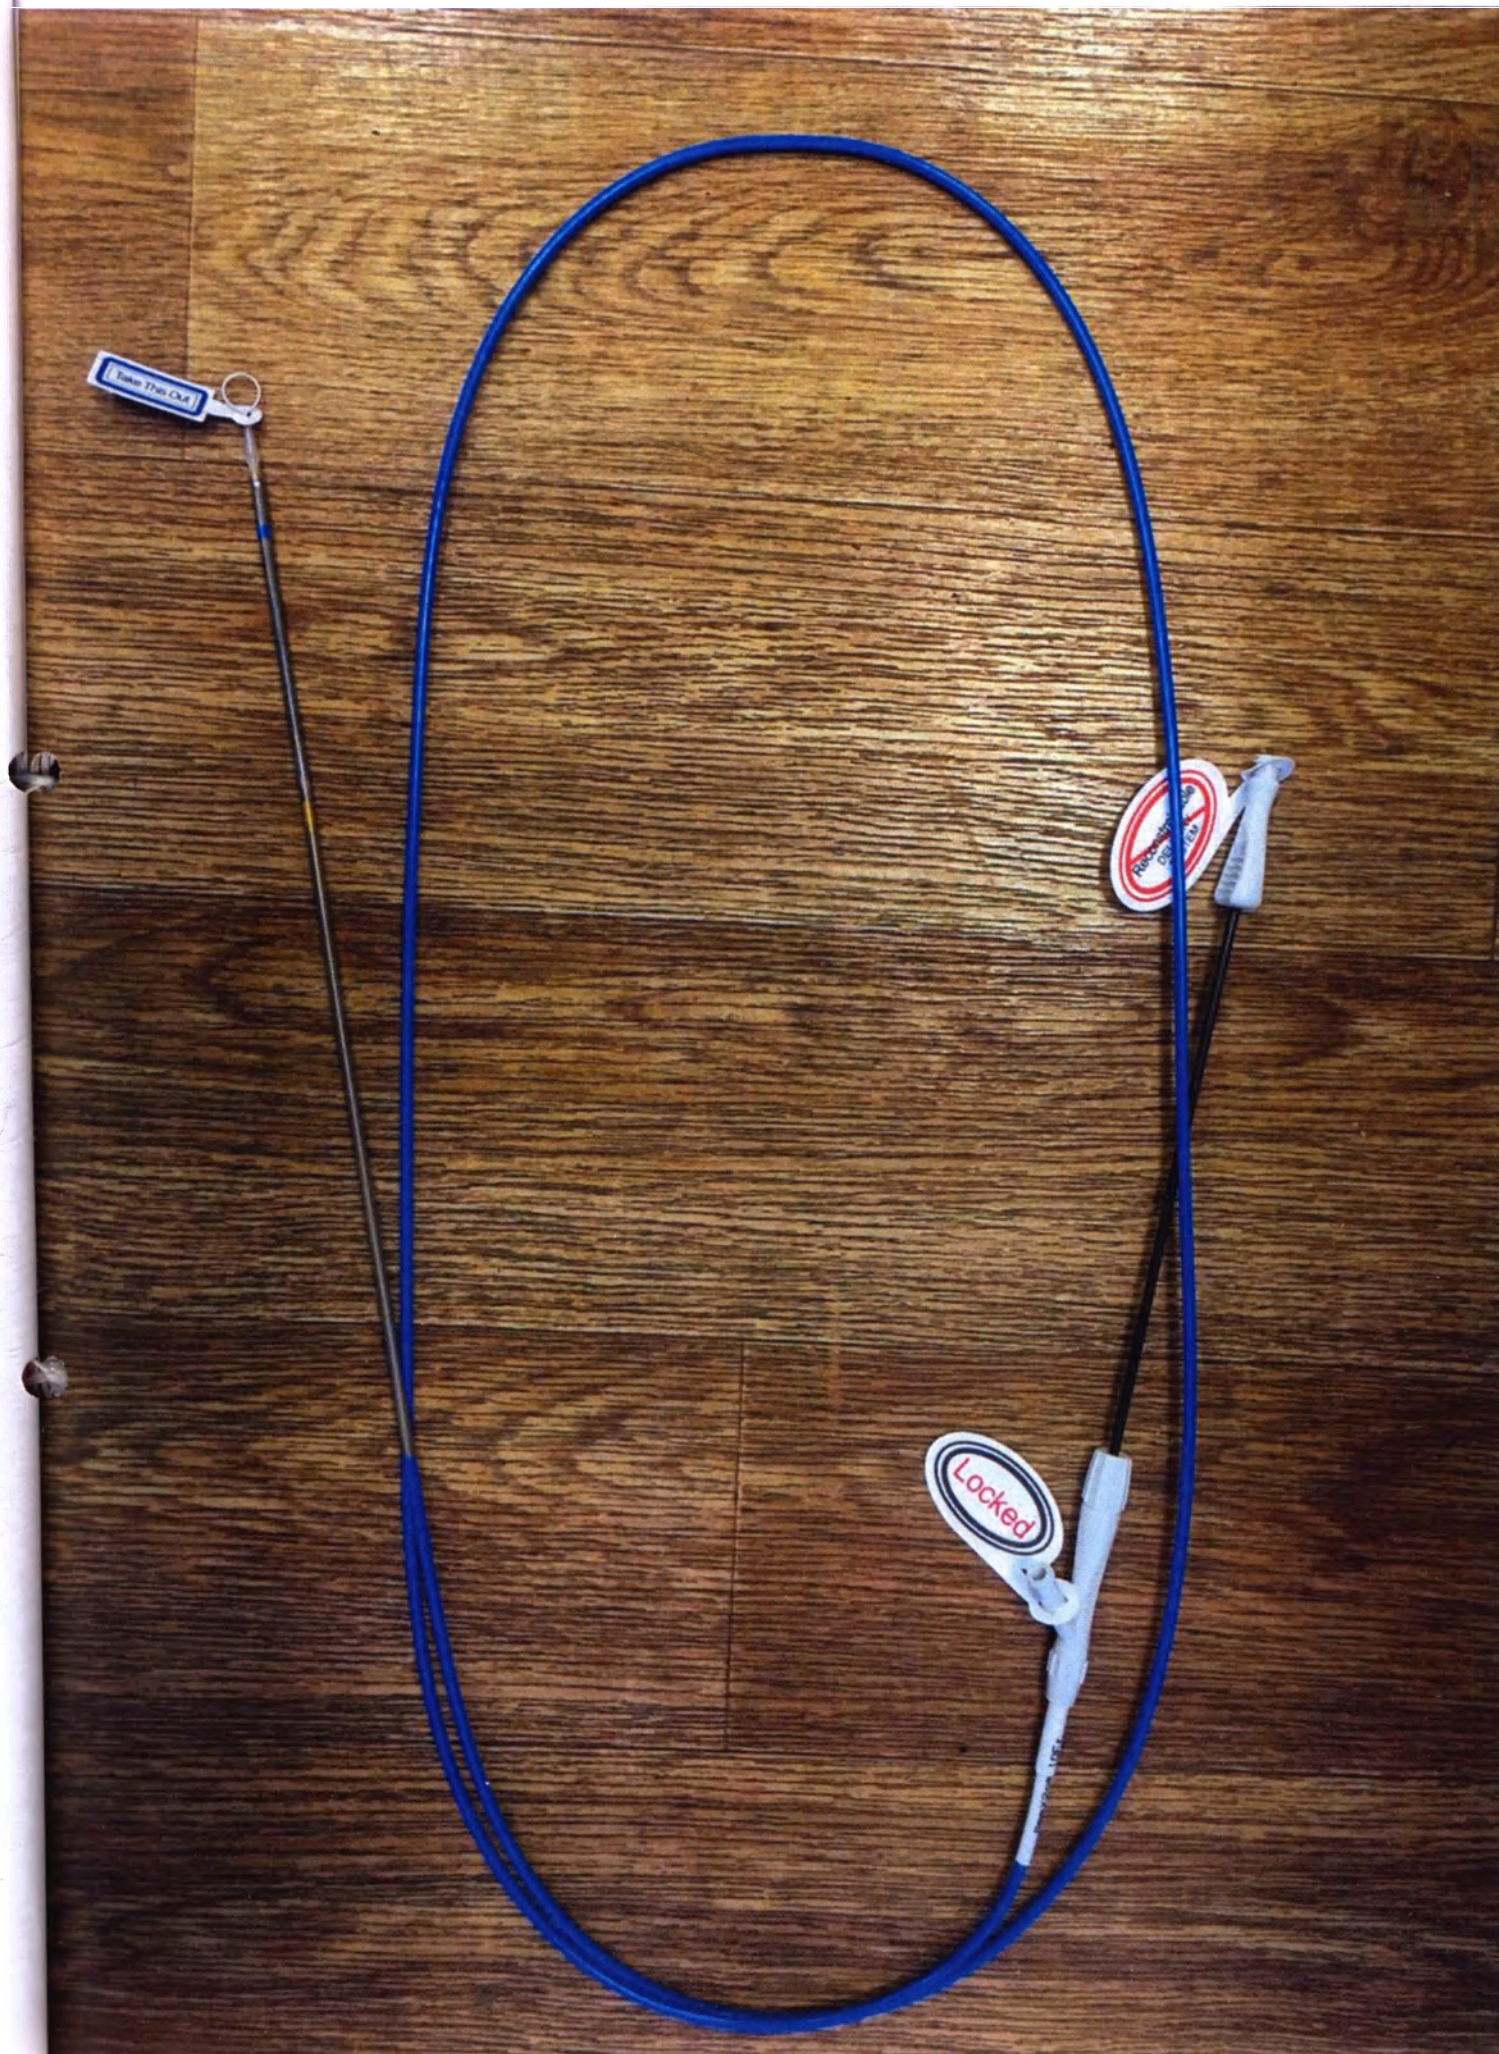

Система доставки

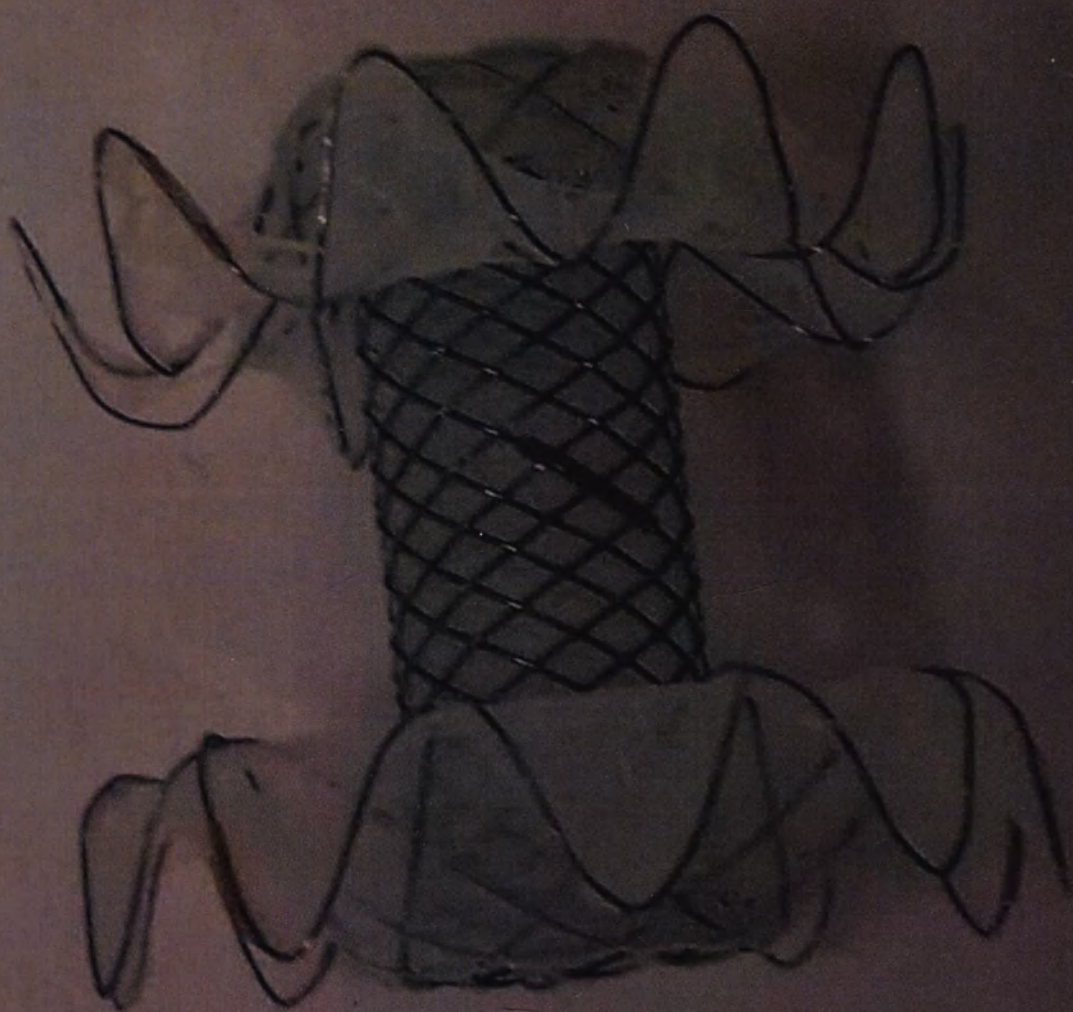



Niti-S SPAXUS™ Stent

8 mm X 20 mm



2020-04-15 2022-04-15

Use after unfolding

2020-04-15 2022-04-15

REF SS0802FW

SN 20E01300008751

CE 1539

ISO 13485

ISO 14971

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

ISO 10993

GSI-128 (UCC / EAN-128)




Niti-S SPAXUS™ Stent

8 mm X 20 mm


GS1-128 (UCC / EAN-128)




(01)06804482273436(11)200416(17)220415(21)20E0130I0DB751

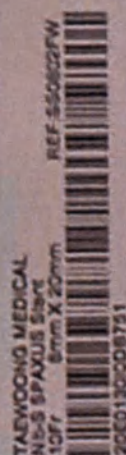

REF:SS0802FW

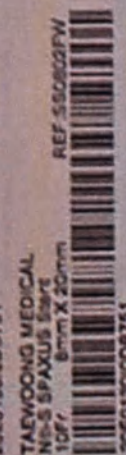

REF:SS0802FW


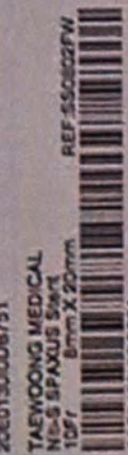


REF:SS0802FW



8 809482 273436

Length Unit : mm

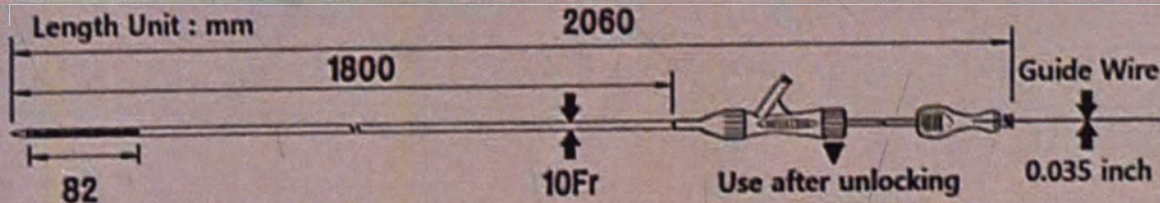

2020-04-16
Date of Manufacture

2022-04-15
Use by

REF SS0802FW

SN 20E0130I0DB751



CE 1639



TaeWoong medical Co., Ltd. :

14 Gajeong-ro, Wolgot-myeon, Gimpo-si, Gyeonggi-do, Korea 10022
TEL. +82-31-996-0641 FAX. +82-31-996-0645





EMERGO EUROPE
Prinsessegracht 20 2514 AP The Hague The Netherlands

LBN 00-01(Rev.02)
MADE IN KOREA



2021/10/25 14:3

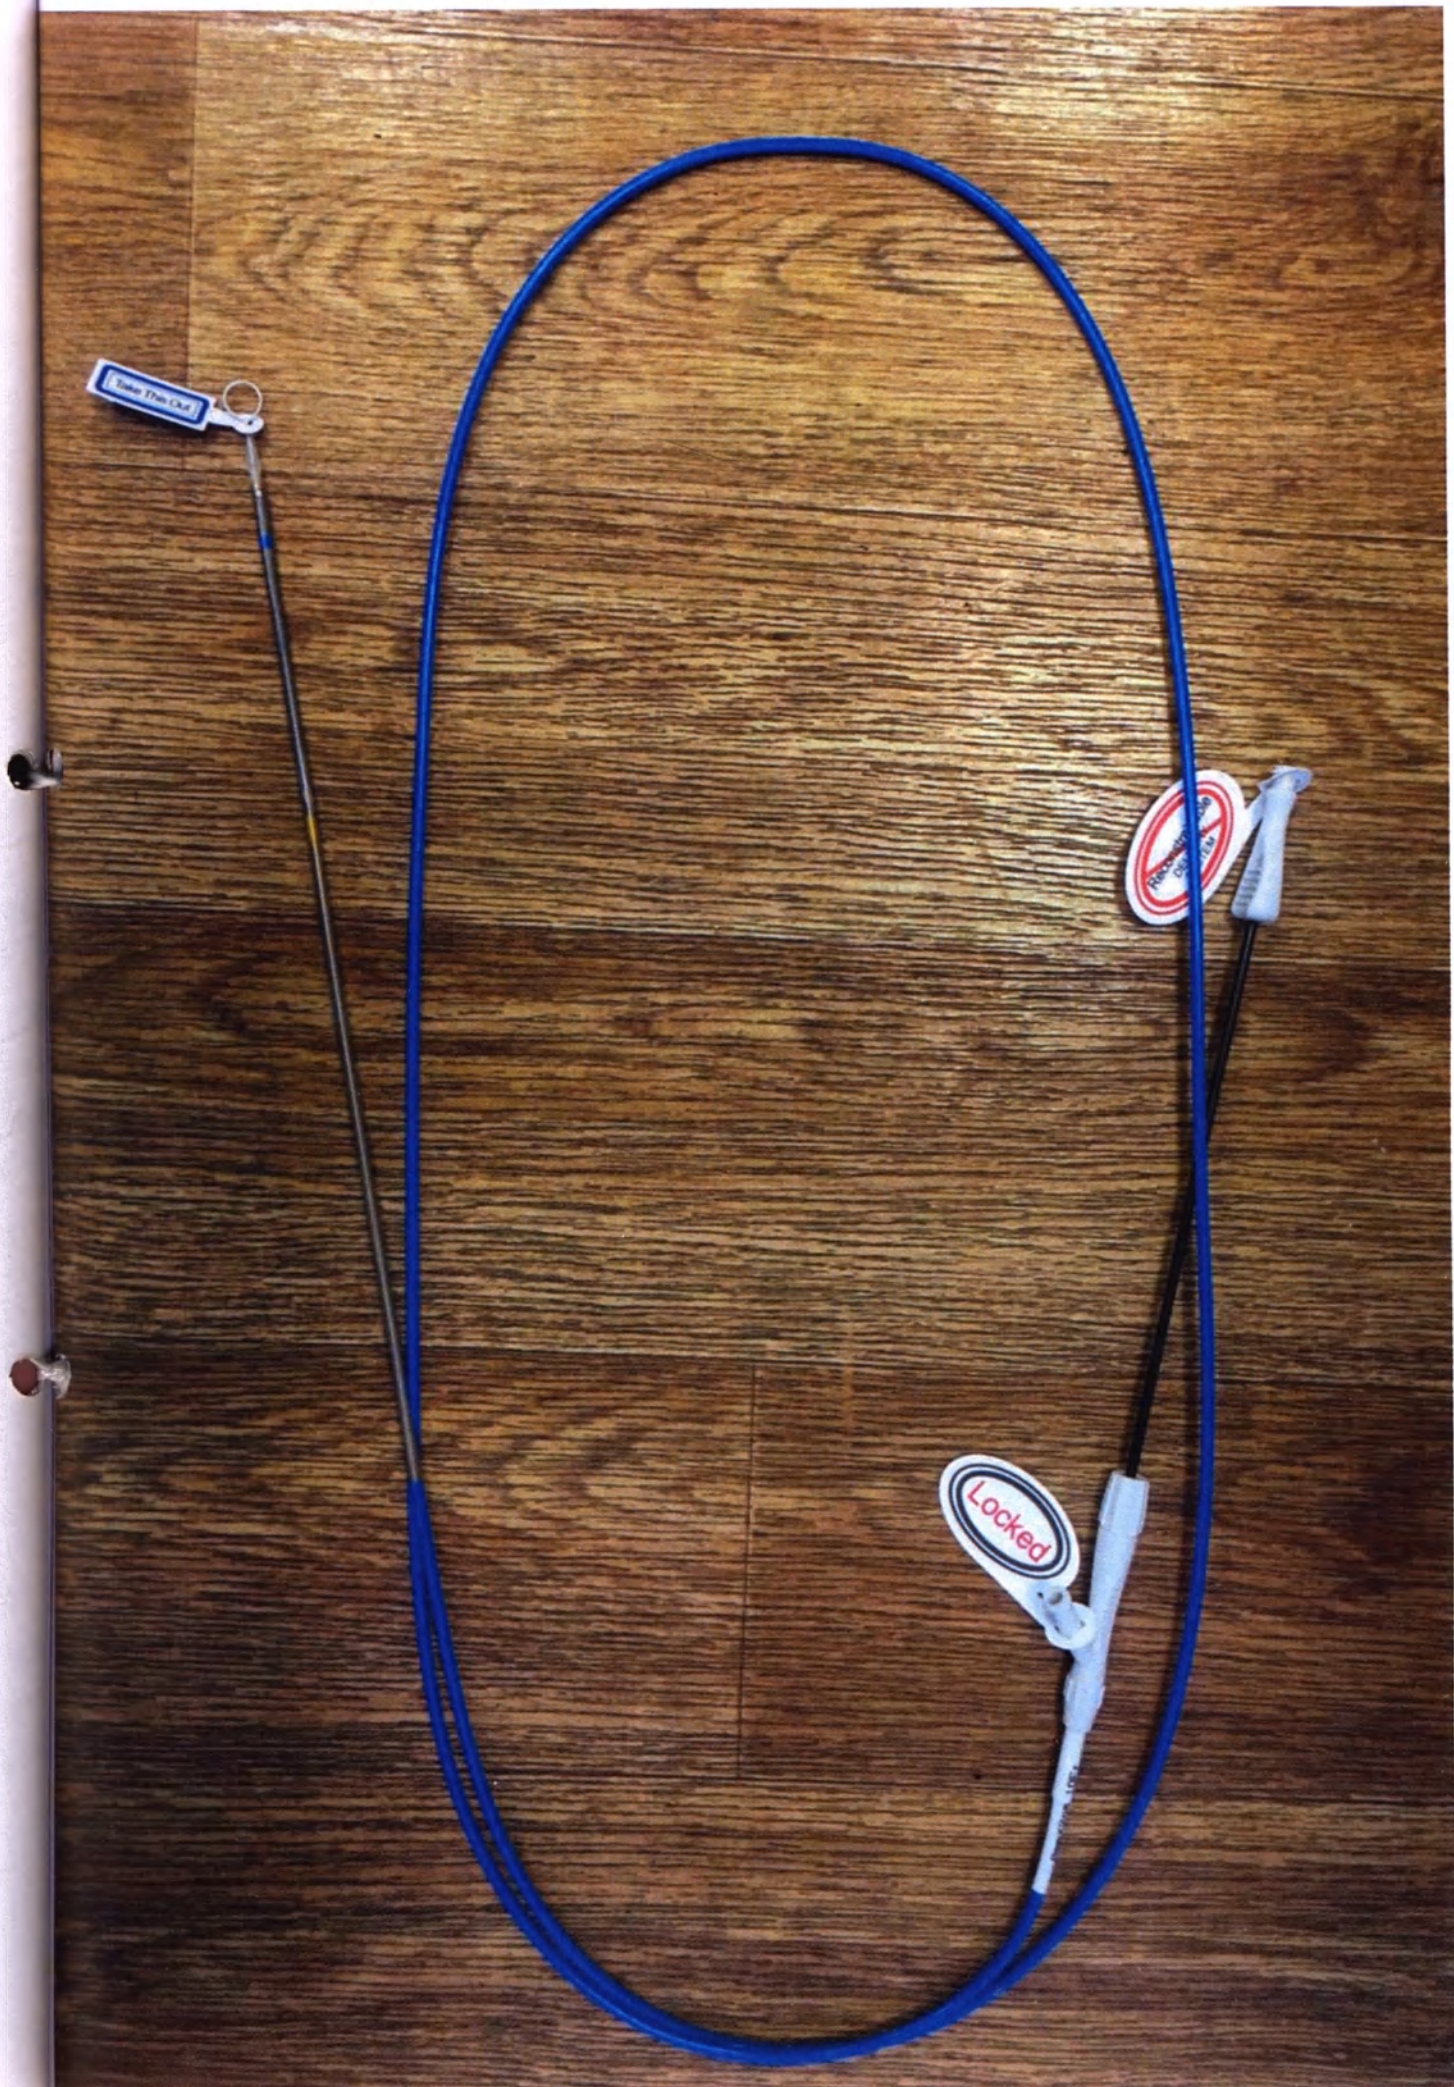

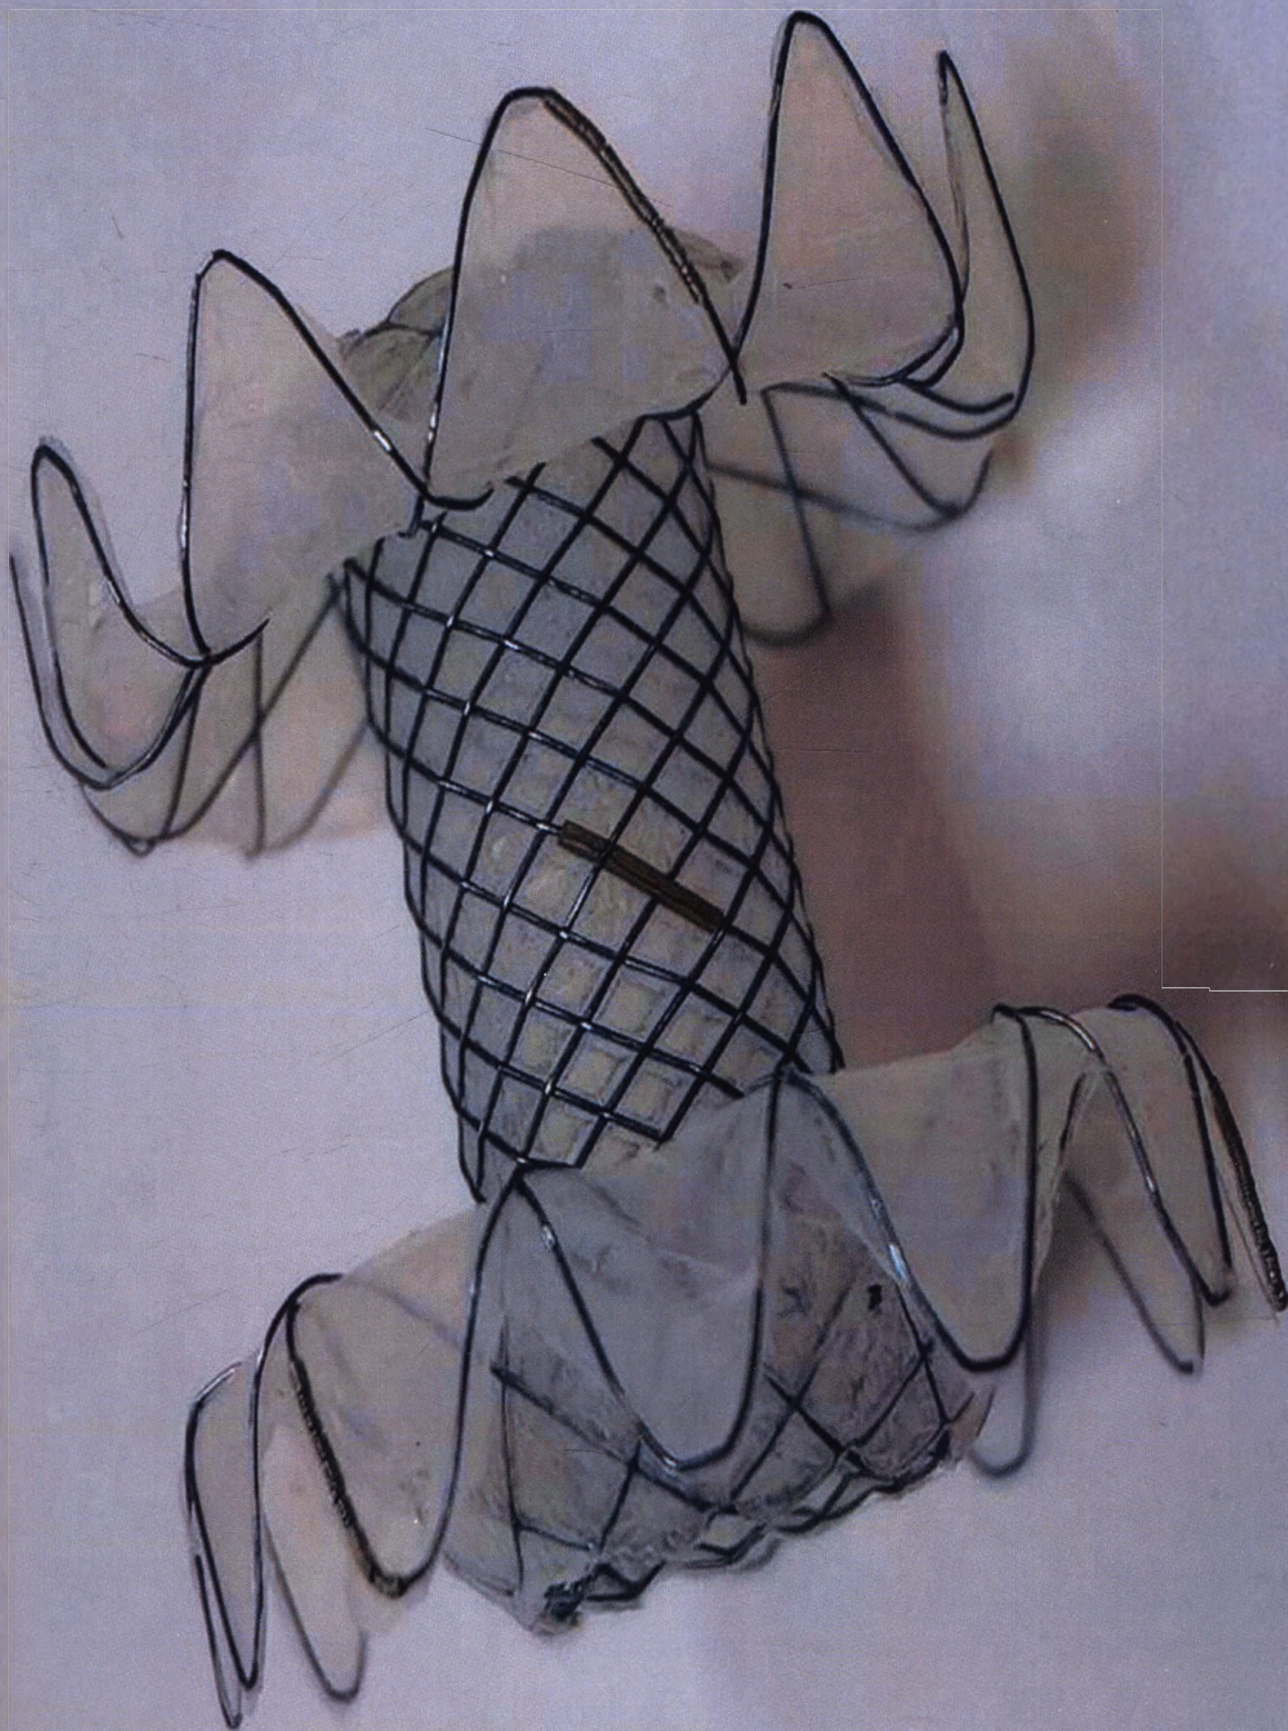

Стент в развернутом виде

검

Niti-S SPAXUS™ Stent

10 mm X 20 mm

Length Unit : mm



2022-04-15
2022-04-15
2022-04-15

Use after unpacking
0.033 inch

REF SS1002FW

SN 20C1032008752

CE 1639

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485

ISO 13485


ISO 13485

031-128 (UCC / EAN-128)

Taewoong
MEDICAL

Niti-S SPAXUS™ Stent

10 mm X 20 mm

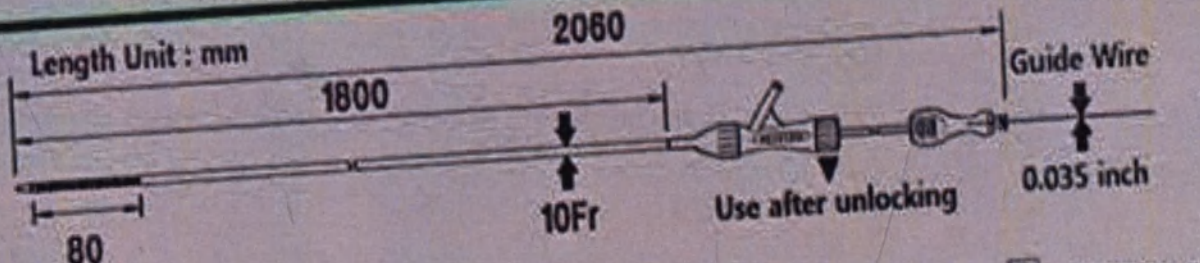

2020-04-16
Date of Manufacture

2022-04-15
Use by

REF SS1002FW

SN 20C103210DB752



CE 1639



STERILE



TheWoong medical Co., Ltd.

14 Gajeong-ro, Wajong-myeon, Gimpo-si, Gyeonggi-do, Korea 10022
TEL. +82-31-996-0641 FAX. +82-31-996-0643




EMERGO EUROPE
Prinsesengracht 20 2514 AP The Hague The Netherlands

LBN 00-01 (Rev.02)
MADE IN KOREA

GS1-128 (UCC / EAN-128)




TAEWOONG MEDICAL
Niti-S SPAXUS Stent
10mm X 20mm
10Fr
REF SS1002FW



20C103210DB752

TAEWOONG MEDICAL
Niti-S SPAXUS Stent
10mm X 20mm
10Fr
REF SS1002FW



20C103210DB752


TAEWOONG MEDICAL
Niti-S SPAXUS Stent
10mm X 20mm
10Fr
REF SS1002FW



20C103210DB752



8 809482 273375









LEWIS CO. (936) 201-0111
MADE IN KOREA

GS1-128 (UCC / EAN-128)

16



2021/10/

REF: HDS-10
 SN: Refer to Label
 Refer to Label

(Operating Condition)
 • Temperature: 15 °C to 40 °C
 • Humidity: 10 % to 75 %
 • Air Pressure: 70 kPa to 106 kPa
(Storage & Transportation Condition)
 • Temperature: -10 °C to 40 °C
 • Humidity: 10 % to 90 %
 • Air Pressure: 70 kPa to 106 kPa

TaeWoong Medical Co., Ltd.
 14 Gopong-ro, Bundang-myeon, Gyeonggi-do, Korea
 Tel: +82(31)896-0647 Fax: +82(31)896-0648
 Homepage: www.taeWoongmedical.com

EMERGO EUROPE
 Pinnerweg 20
 2114 AP The Hague
 The Netherlands

GB1-128 (UCC / EAN-128)

Niti-S Hot SPAXUS™ Stent & Electrocautery Stent Delivery System
 16 mm X 20 mm

Length Unit: mm

104 1800 2080

10Fr

Use after unlocking

Guide Wire

0.035 inch

2020-04-16 (Date of Manufacture)

2022-04-15 (Exp. Dt.)

REF: HSS1602FW

SN: 20C9352100B756

CE 1639

EMERGO EUROPE
 Pinnerweg 20 2114 AP The Hague The Netherlands

TaeWoong
 MEDICAL



GS1-128 (UCC / EAN-128)



(01)20C93210DB756 (11)300418 (17)220415 (21)20C93210DB756

TAEWOONG MEDICAL
Niti-S Hot SPAXUS Stent
10Fr 16mm X 20mm

REF HSS1602FW

TAEWOONG MEDICAL
Niti-S Hot SPAXUS Stent
10Fr 16mm X 20mm

REF HSS1602FW

TAEWOONG MEDICAL
Niti-S Hot SPAXUS Stent
10Fr 16mm X 20mm


REF HSS1602FW



8 809482 278103

Niti-S Hot SPAXUS™ Stent & Electrocautery Stent Delivery System

16 mm X 20 mm

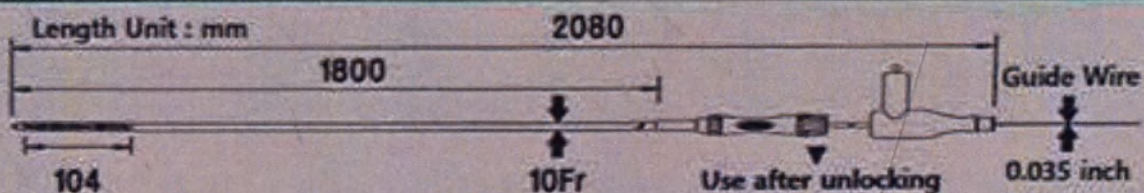

2020-04-16

Date of Manufacture



2022-04-15

Use by



HSS1602FW



20C935210DB756



CE 1639



TaeWoong Medical Co., Ltd.


14 Gajeong-ro, Wolgot-myeon, Gimpo-si, Gyeonggi-do, Korea 10022
TEL: +82-31-996-0641 FAX: +82-31-996-0645


EMERGO EUROPE

Prinsengracht 20 2514 AP The Hague The Netherlands


LHS 00-02(Rev.01)

MADE IN KOREA

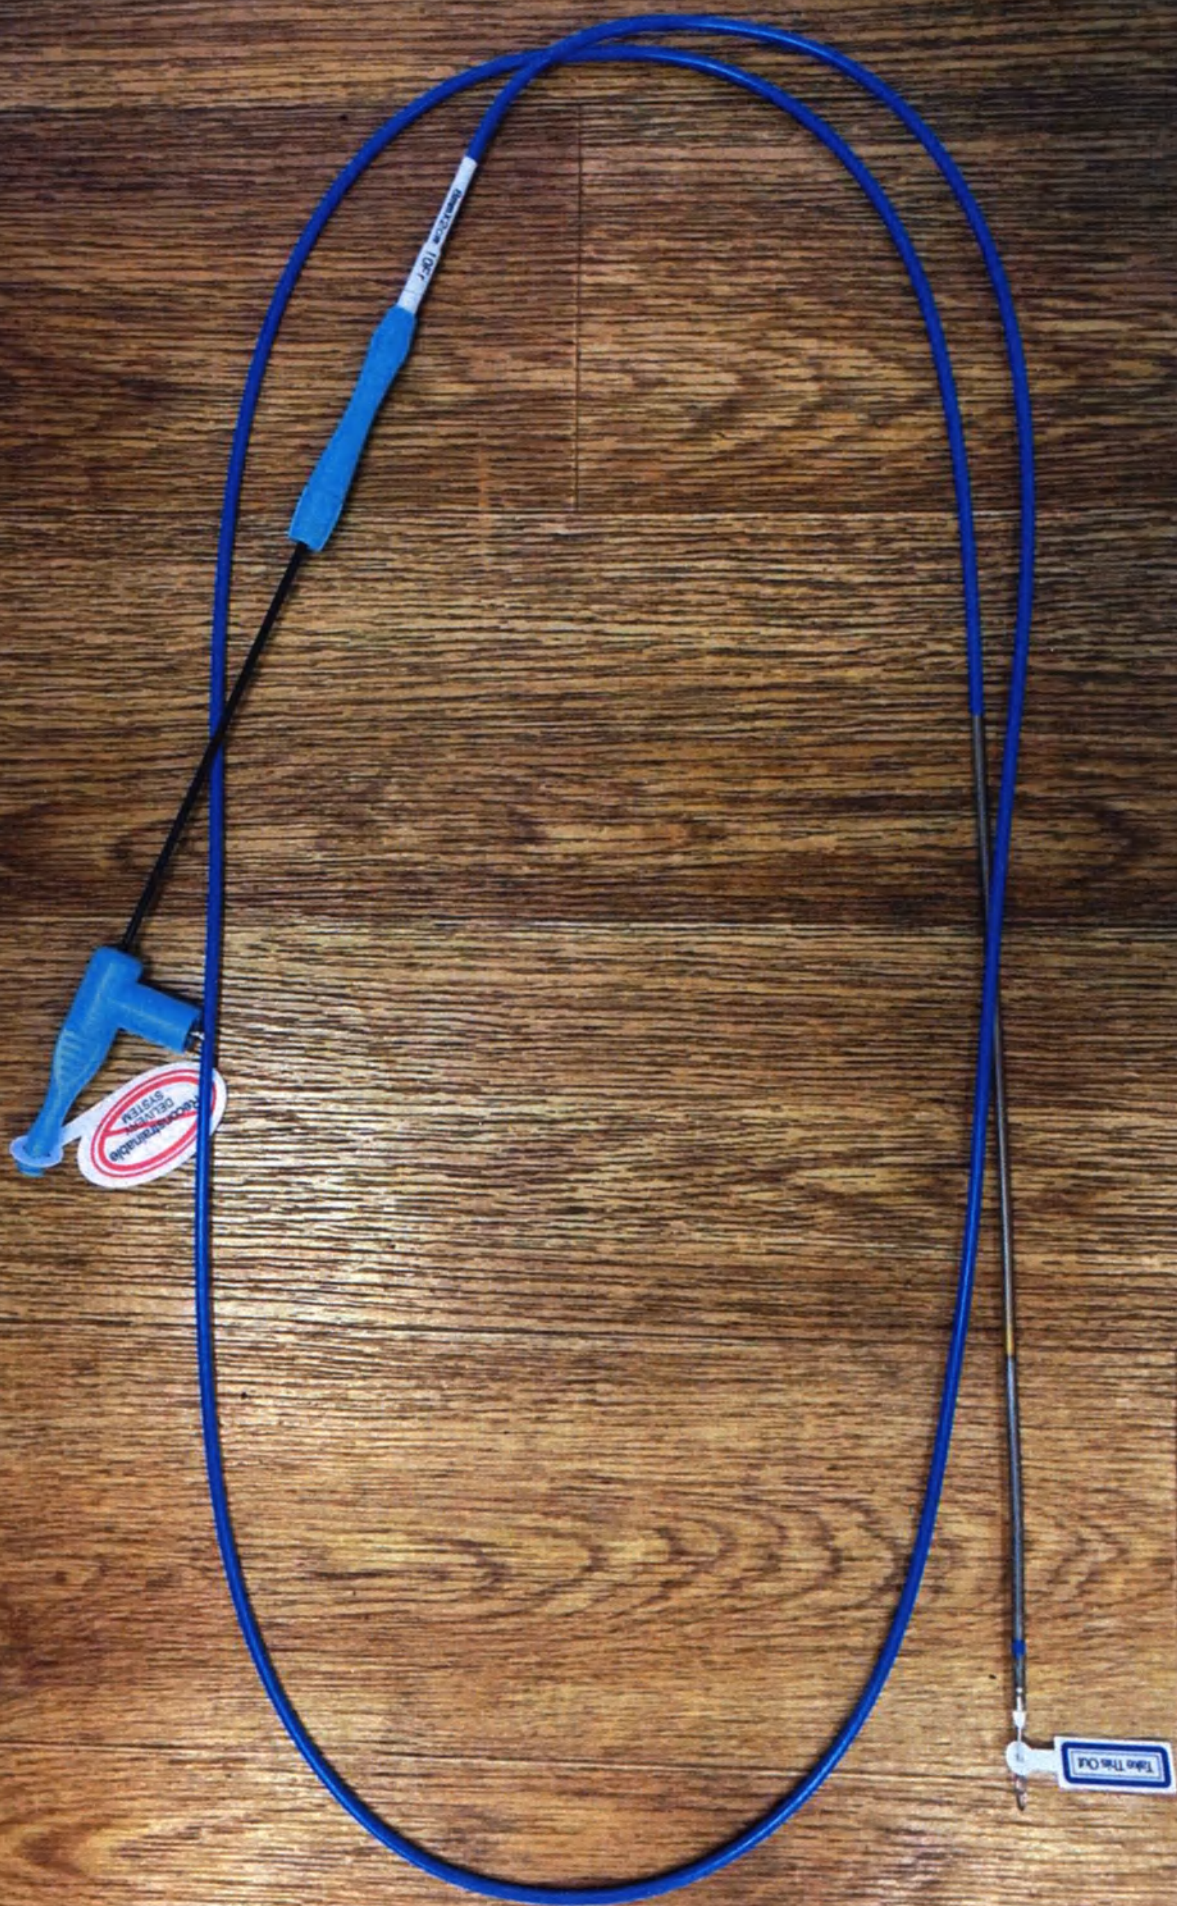

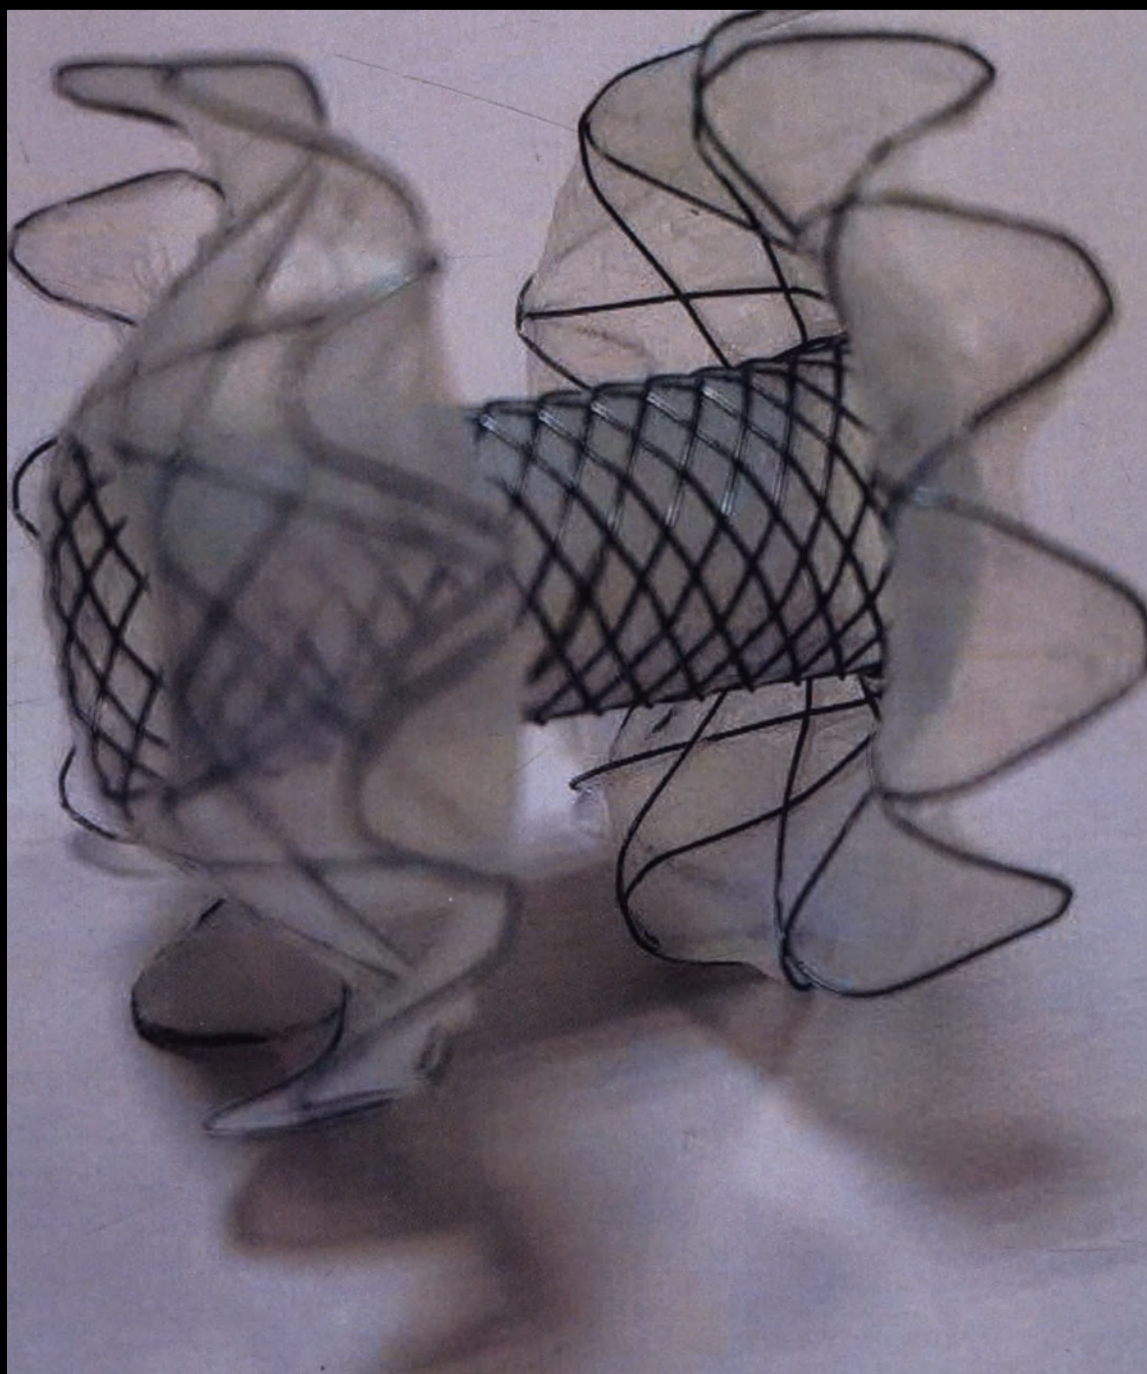

Стент в развернутом виде

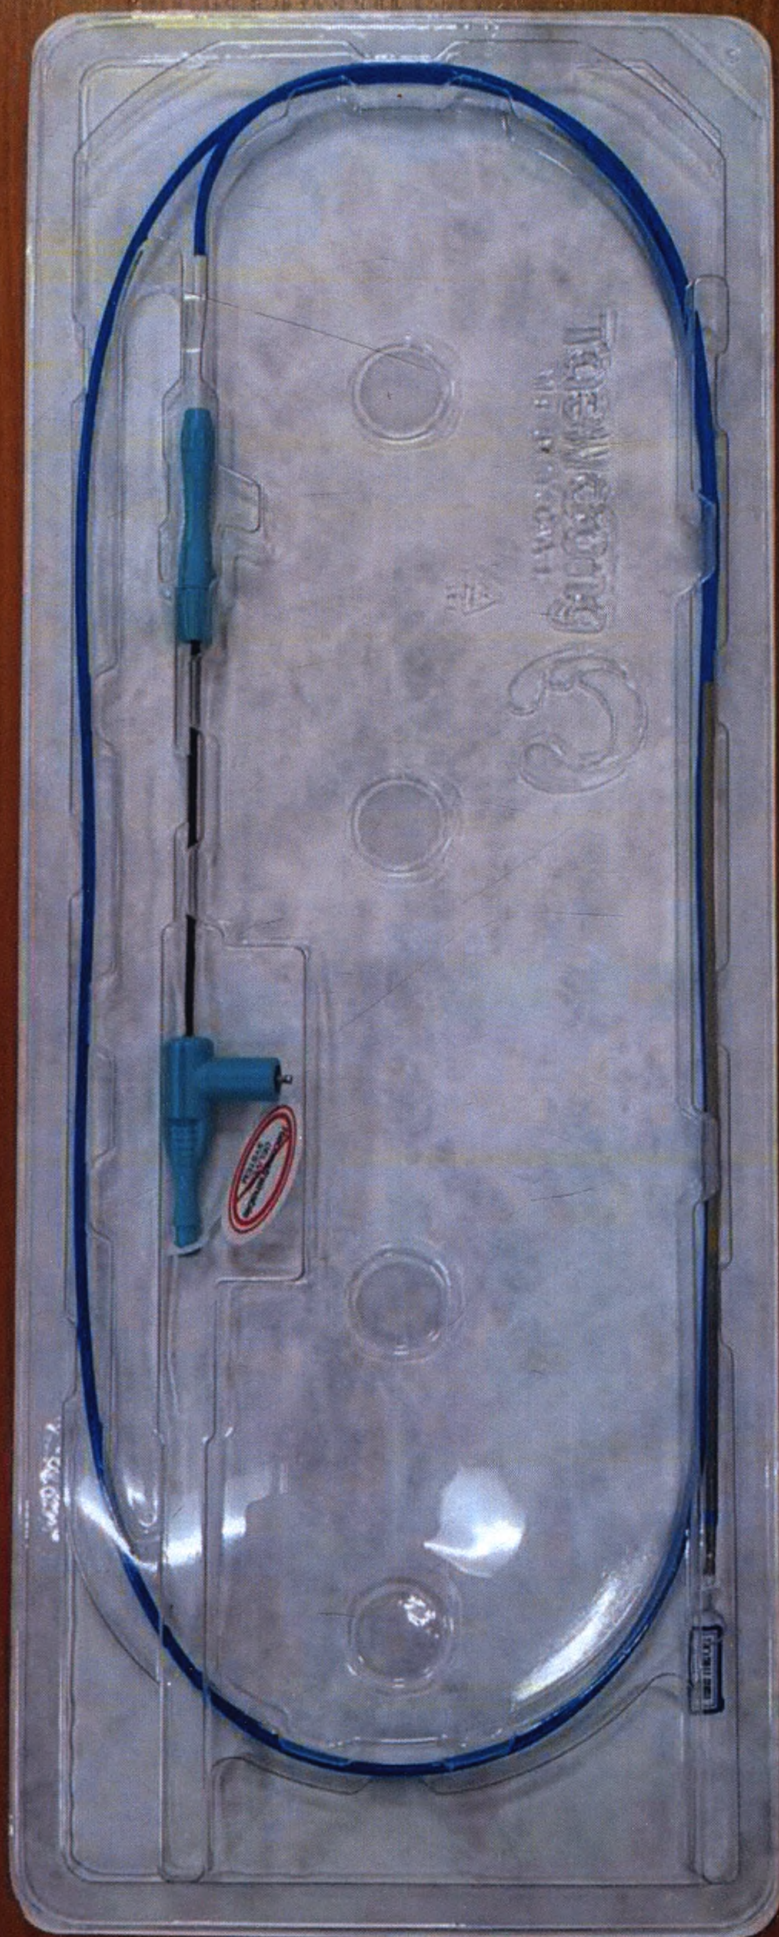

Niti-S Hot SPAXUS™ Stent & Electrocautery Stent Delivery System

8 mm X 20 mm


GS1-128 (UCC / EAN-128)
 (01)08809643750356(11)200413(17)220412(21)20E011710DB353

TAEWOONG MEDICAL
 Niti-S Hot SPAXUS Stent
 10Fr 8mm X 20mm REF:HSS0802FW
 20E011710DB353

TAEWOONG MEDICAL
 Niti-S Hot SPAXUS Stent
 10Fr 8mm X 20mm REF:HSS0802FW
 20E011710DB353

TAEWOONG MEDICAL
 Niti-S Hot SPAXUS Stent
 10Fr 8mm X 20mm REF:HSS0802FW
 20E011710DB353

8 809643 750356

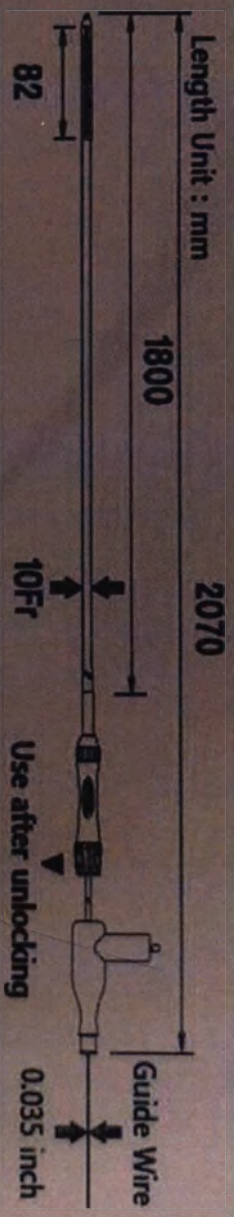



TaeWoong Medical Co., Ltd.
 14 Gogyeong-ro, Wolgot-myeon, Gimpo-si, Gyeonggi-do, Korea 10022
 TEL: +82-31-996-0641 FAX: +82-31-996-0645

CE 1639
 EMERGO EUROPE
 Prinsesengracht 20 2514 AP The Hague The Netherlands
 LHS 00-02(Rrv.01)
 MADE IN KOREA

REF HSS0802FW
 SN 20E011710DB353

2020-04-13
 Date of Manufacture
 2022-04-12
 Use by

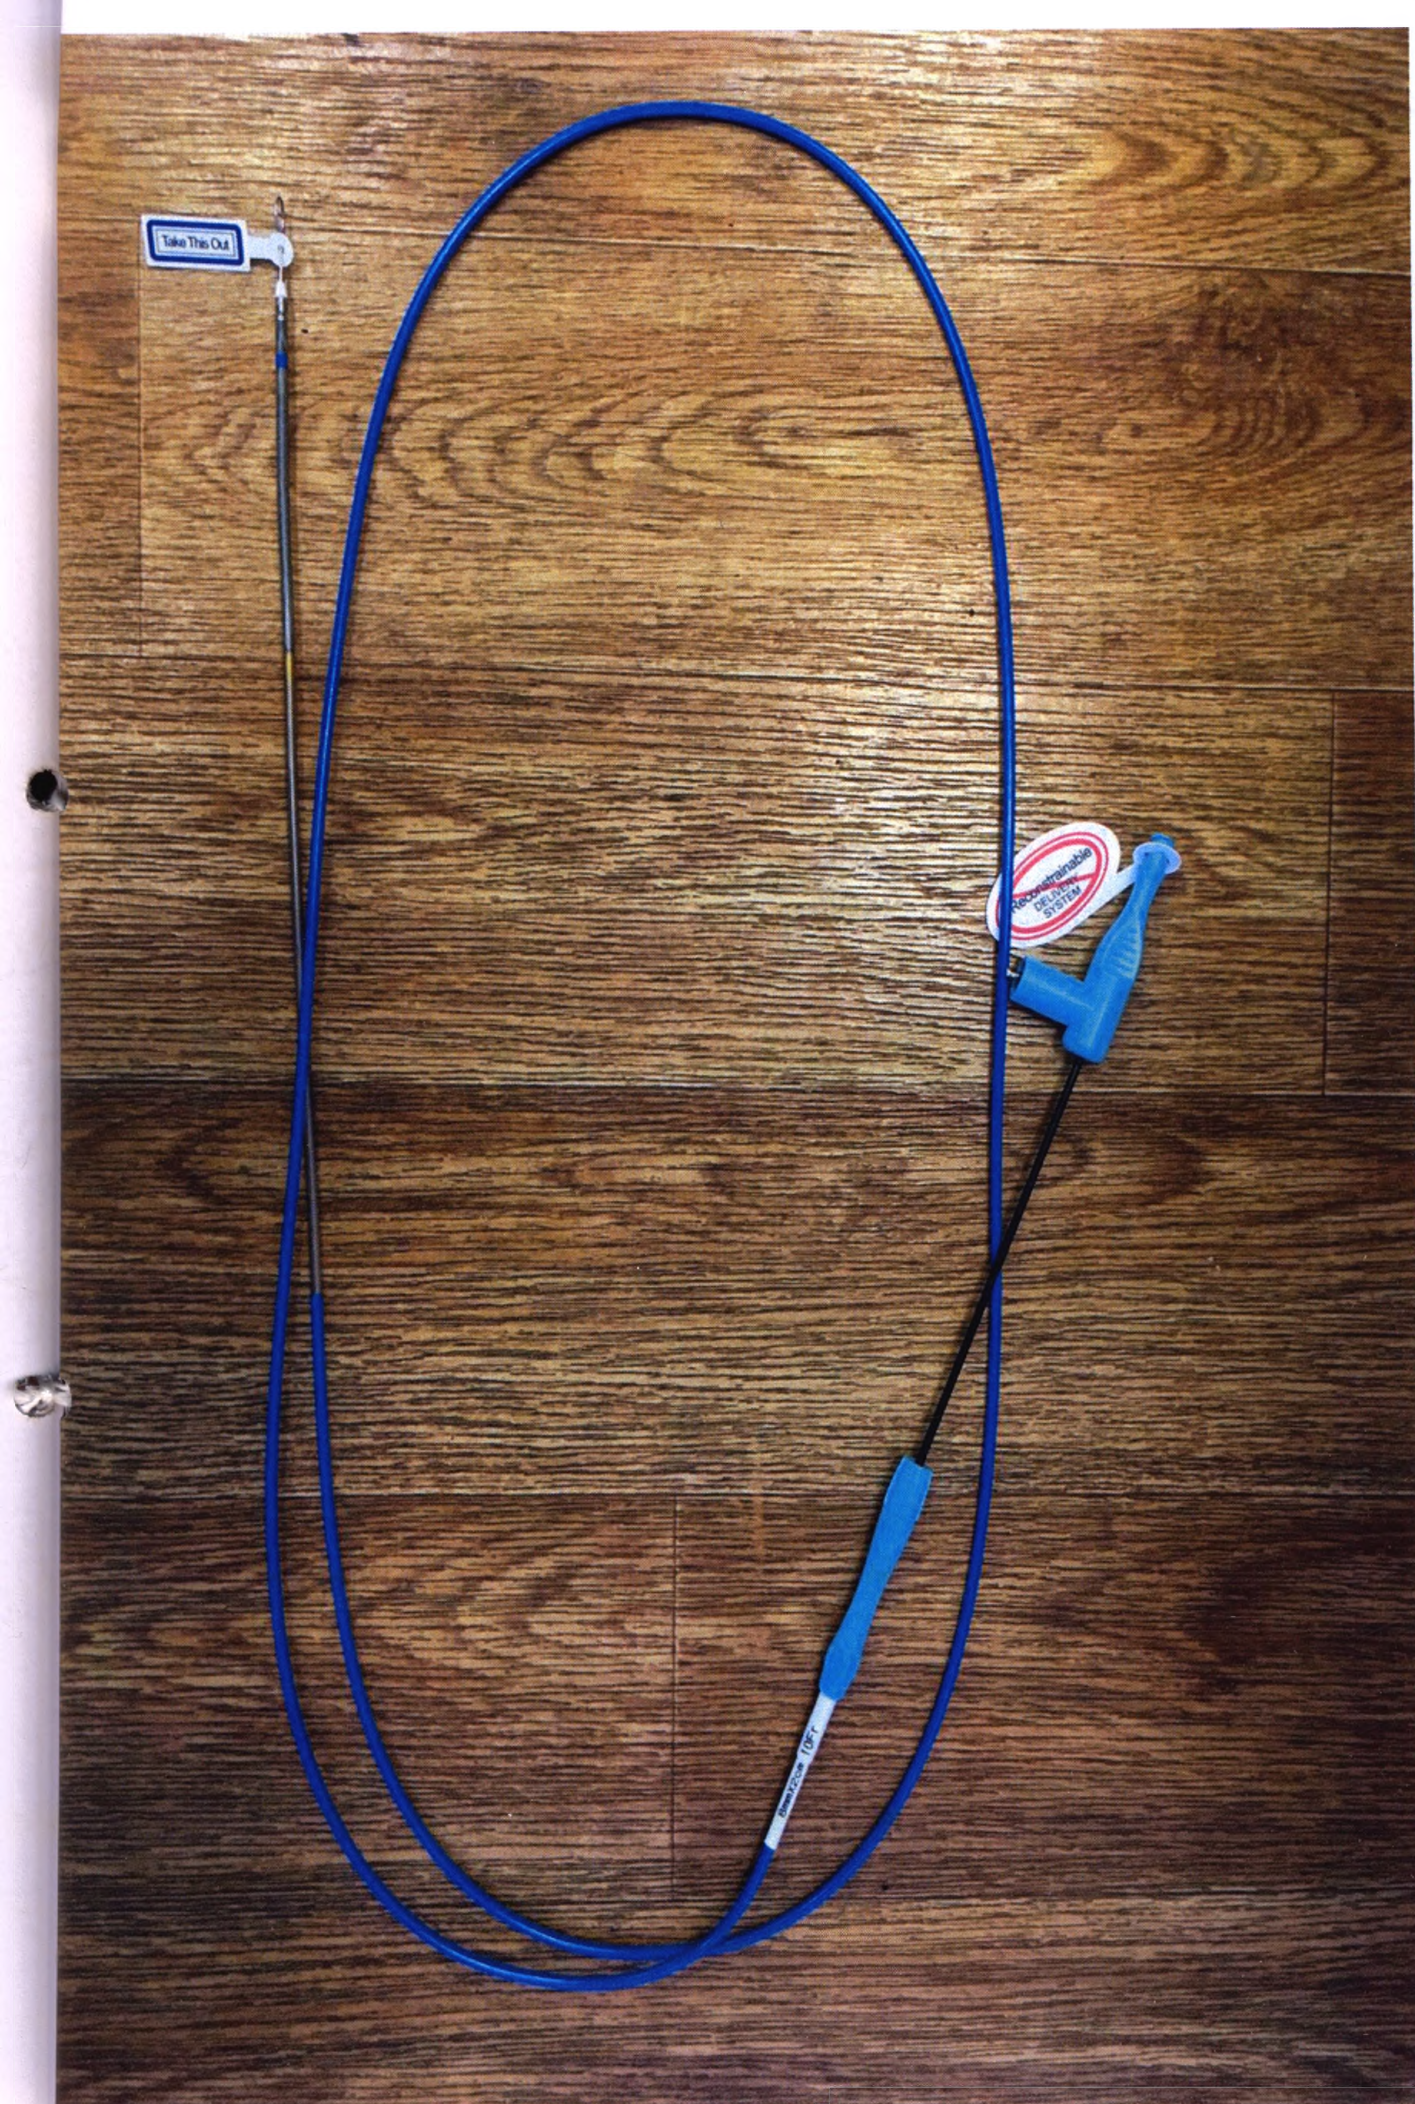


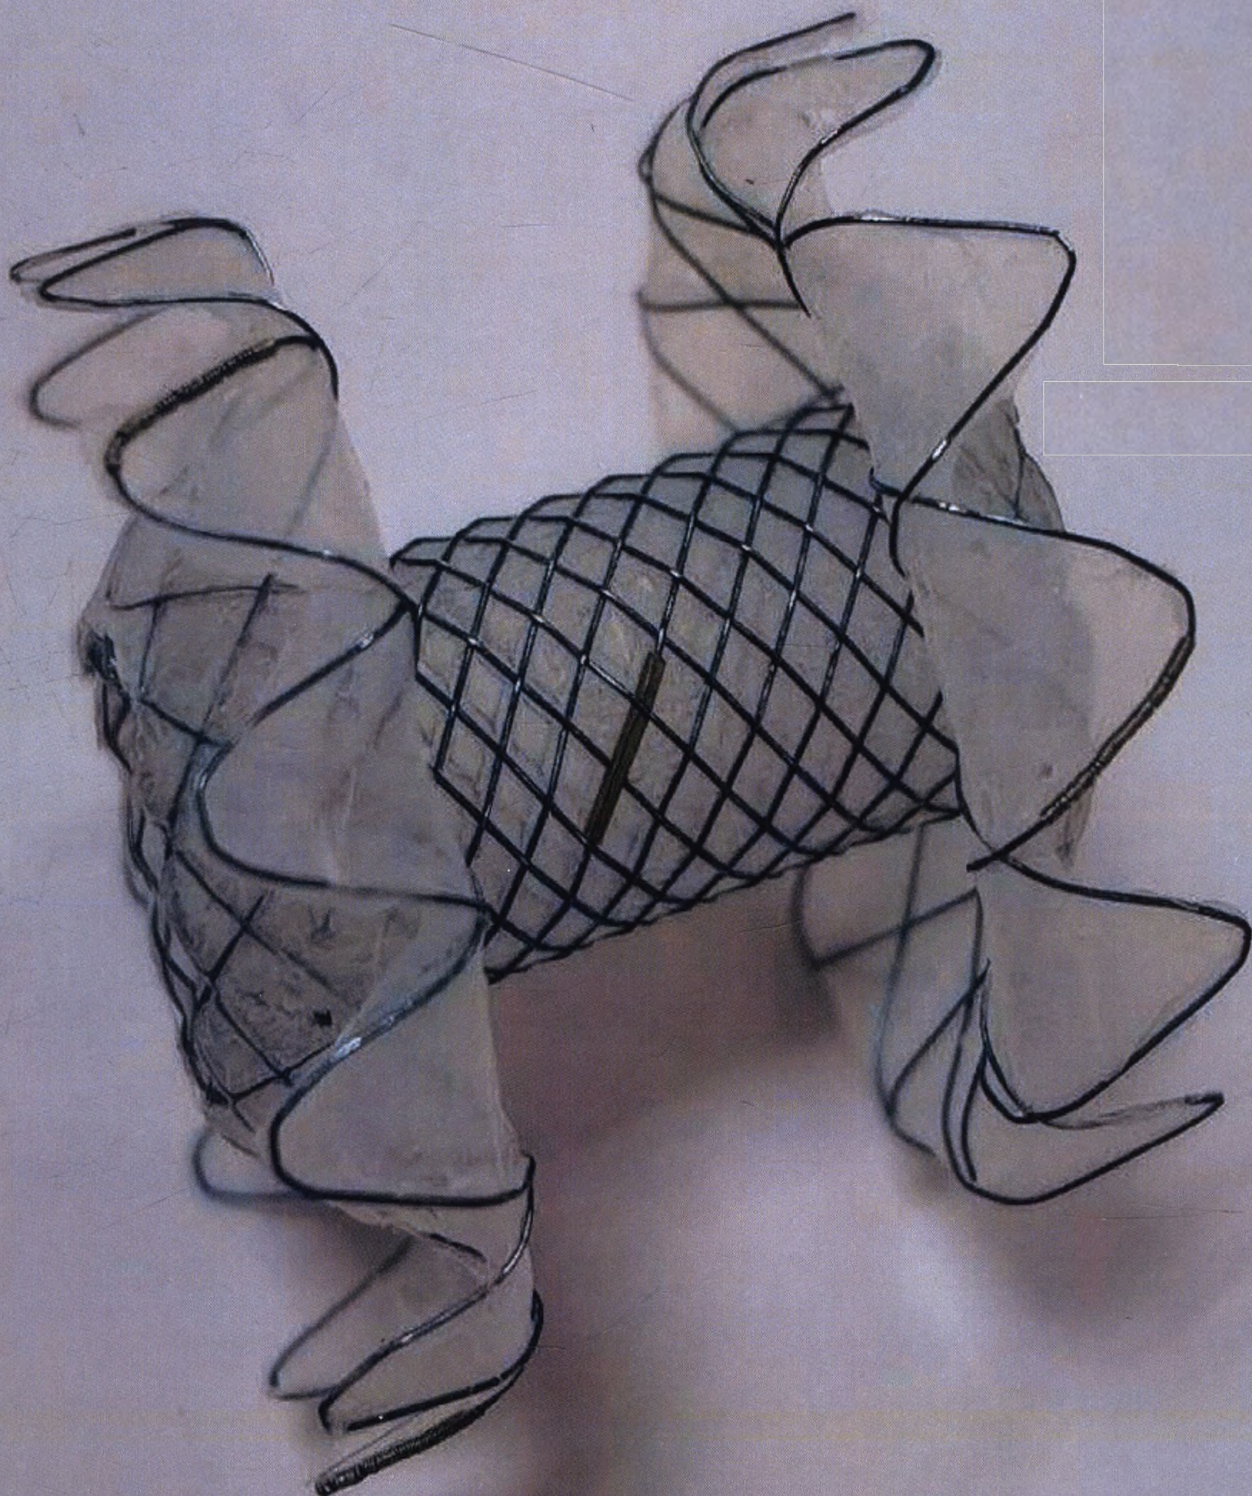


Стент в развернутом виде

GS1-128 (UCC / EAN-128)

Niti-S Hot SPAXUS™ Stent & Electrocatheter Stent Delivery System

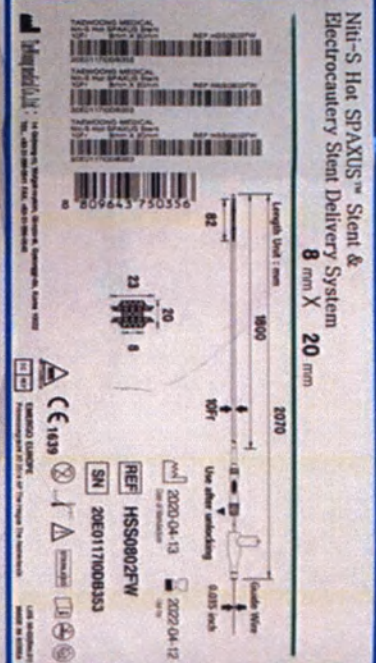

Taewoong
MEDICAL

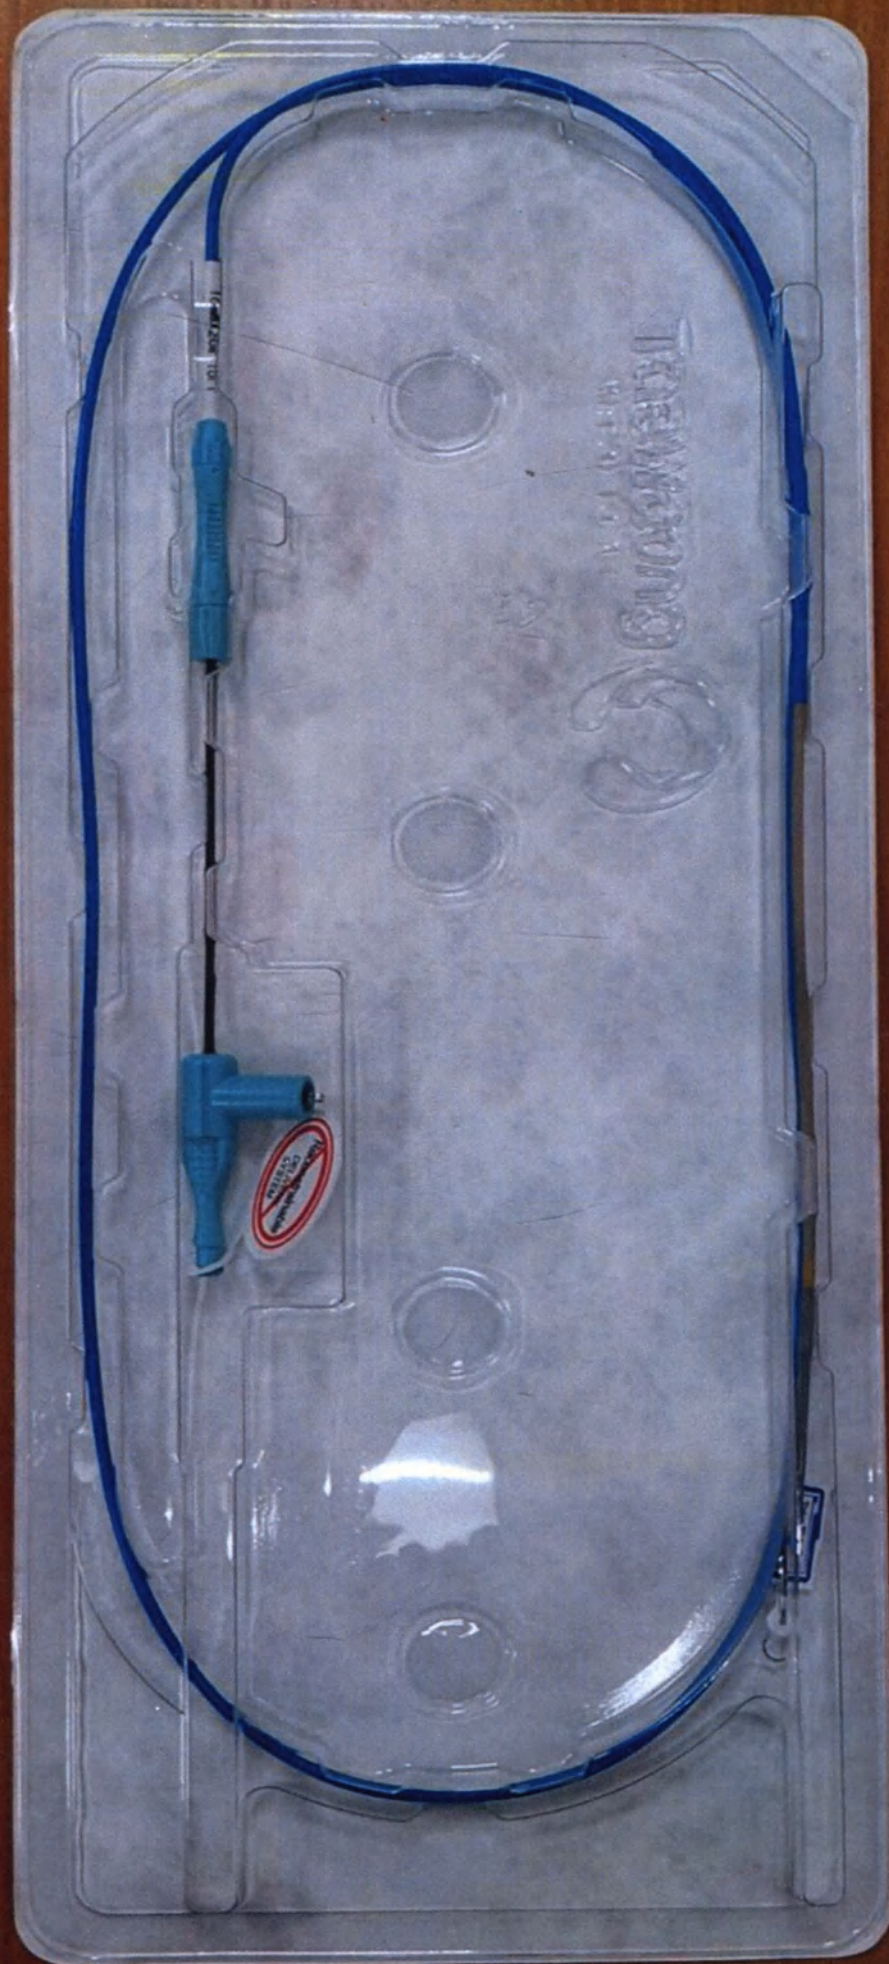



ISO 13485
2016

TaeWoong
MEDICAL

CE 1639

Electrocautery Stent Delivery System

REF: HDS-10

SN: Refer to Label

Refer to Label

Operating Condition

- Temperature: -10 °C to 40 °C
- Humidity: 10 % to 75 %
- Air Pressure: 70 kPa to 106 kPa

Storage & Transportation Condition

- Temperature: -10 °C to 40 °C
- Humidity: 10 % to 90 %
- Air Pressure: 70 kPa to 106 kPa

TaeWoong Medical Co., Ltd.
14, Gwangmyeong-ro, Gwangmyeong, Gyeonggi-do, Korea
Tel: +82(0)10-8996-0643 Fax: +82(0)10-8996-0646
Homepage: www.taeWoongmedical.co.kr

EMERGO EUROPE
Postbus 3433
2514 AP The Hague
The Netherlands

051-128 (UCC / EAN-128)

Niti-S Hot SPAXUS™ Stent & Electrocautery Stent Delivery System
10 mm X 20 mm

Length Unit : mm

80 1800 2070

10Fr

Use after unlocking

0.035 inch

Guide Wire

2020-04-13
Date of Manufacture

2022-04-12
Exp. Date

REF: HSS1002FW

SN: 20C6556100B359

CE 1639

EMERGO EUROPE
Postbus 3433
2514 AP The Hague The Netherlands


LOT: 20-03090171
Model: 20-03090171

TaeWoong
MEDICAL

Niti-S Hot SPAXUS™ Stent & Electrocautery Stent Delivery System

10 mm X 20 mm

Length Unit : mm

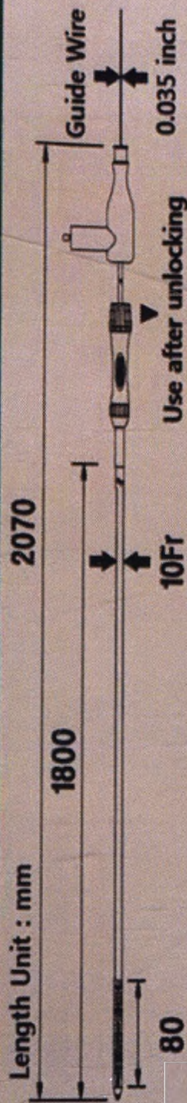


GS1-128 (UCC / EAN-128)



TAEWOONG MEDICAL
Niti-S Hot SPAXUS Stent
10Fr
10mm X 20mm
20C655610DB359
REF:HSS1002FW

TAEWOONG MEDICAL
Niti-S Hot SPAXUS Stent
10Fr
10mm X 20mm
20C655610DB359
REF:HSS1002FW

TAEWOONG MEDICAL
Niti-S Hot SPAXUS Stent
10Fr
10mm X 20mm
20C655610DB359
REF:HSS1002FW




2020-04-13
Date of Manufacture

2022-04-12
Use by

REF HSS1002FW


SN 20C655610DB359




TaeWoong medical Co., Ltd. : 14 Gajong-ro, Wolgot-myeon, Gimpo-si, Gyeonggi-do, Korea 10022
TEL +82-31-996-0641 FAX +82-31-996-0645

EMERGO EUROPE
Prinsessegracht 20 2514 AP The Hague The Netherlands

LHS 00-02(Rav.01)
MADE IN KOREA

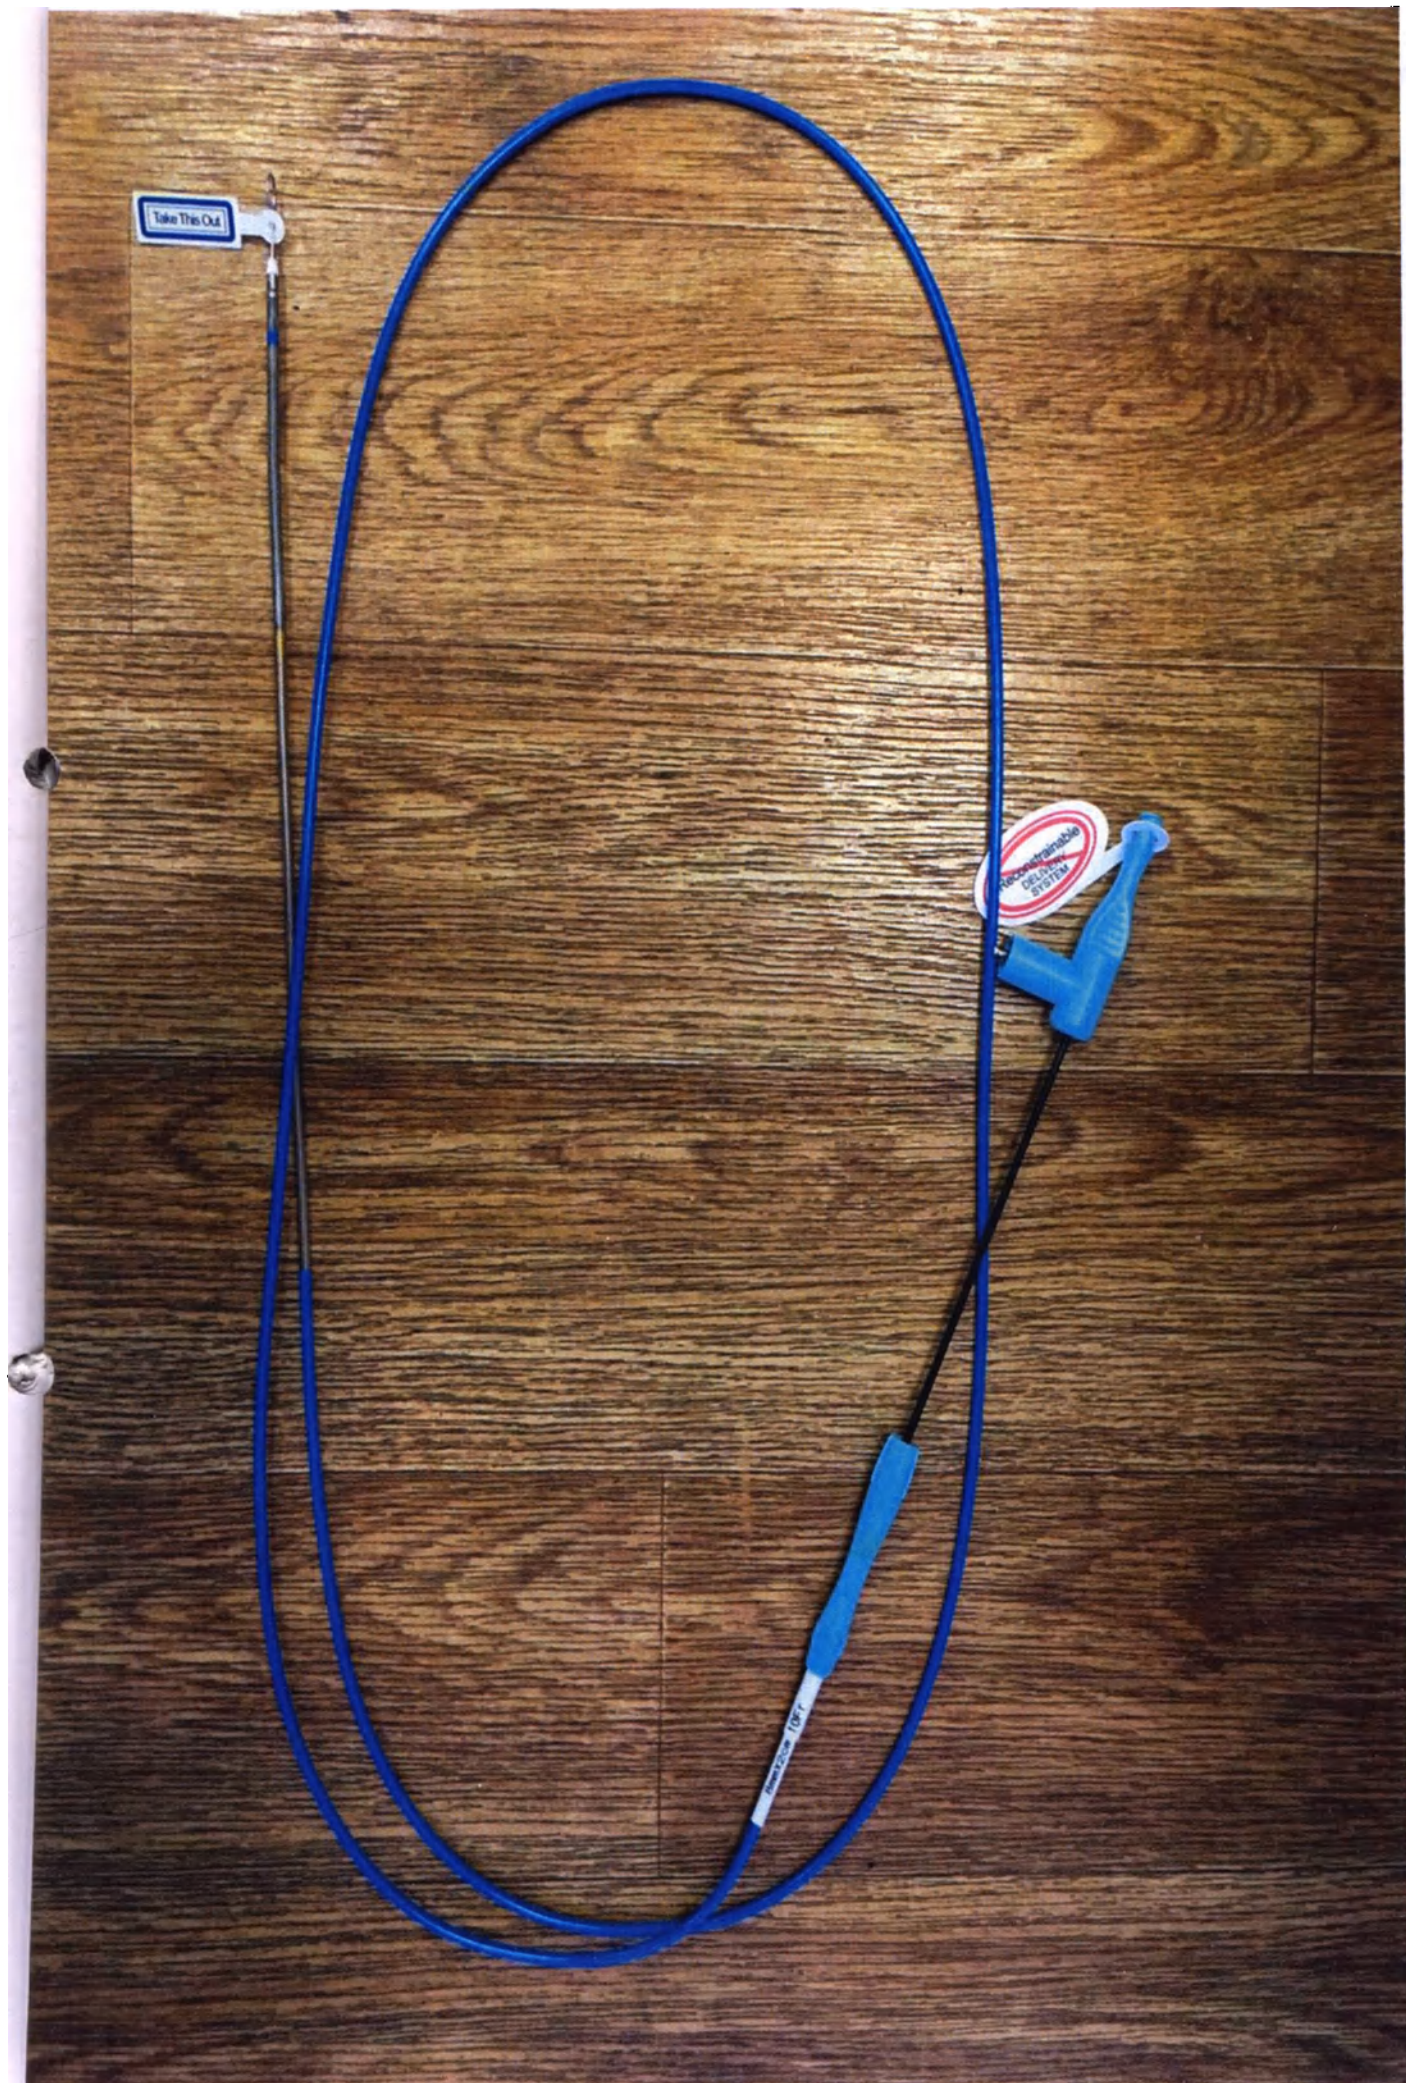

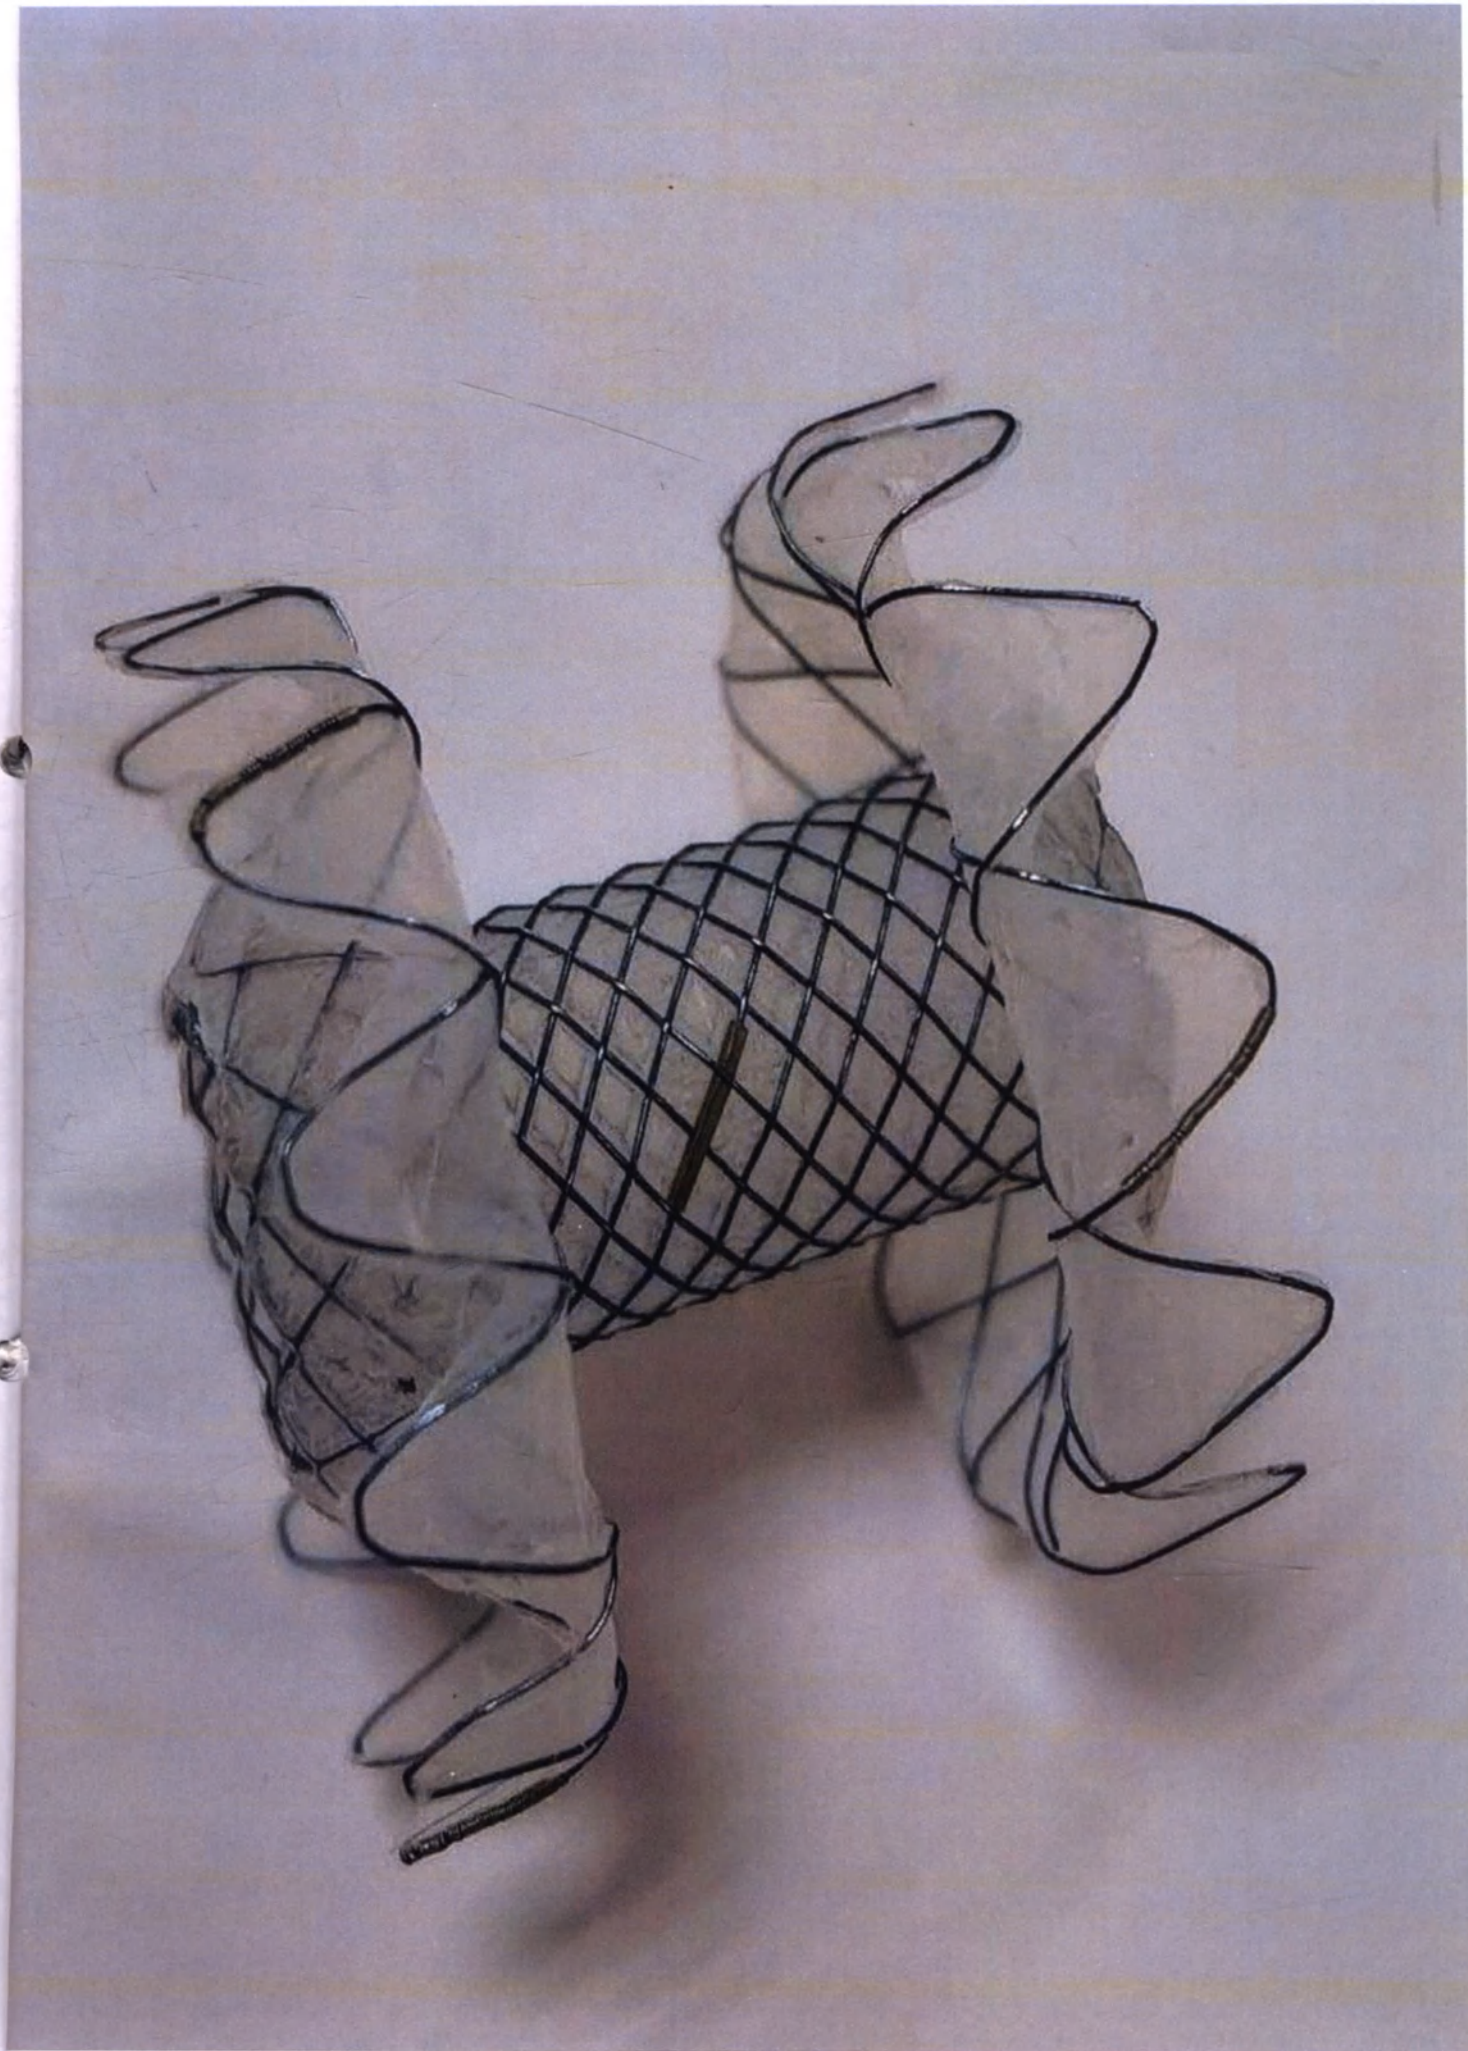

Стент в развернутом виде

Генеральный директор
ООО «Надмед»



Глебов Д.А.

Прошито и пронумеровано

39

лист 2