

Фотографические изображения медицинского изделия:

Бронховидеоскоп Olympus варианты исполнения BF-Q170, BF-1TQ170 с принадлежностями



Бронховидеоскоп Olympus варианты исполнения BF-Q170, BF-1TQ170



12/12/2014

Загубник МА-651



Колпачок для стерилизации MAJ-1538

12/12/2014



Адаптер для аспирационной очистки MAJ-222

12/12/2014




Одноразовый клапан для биопсии MAJ-210

12/12/2014



Одноразовый клапан для аспирации MAJ-209

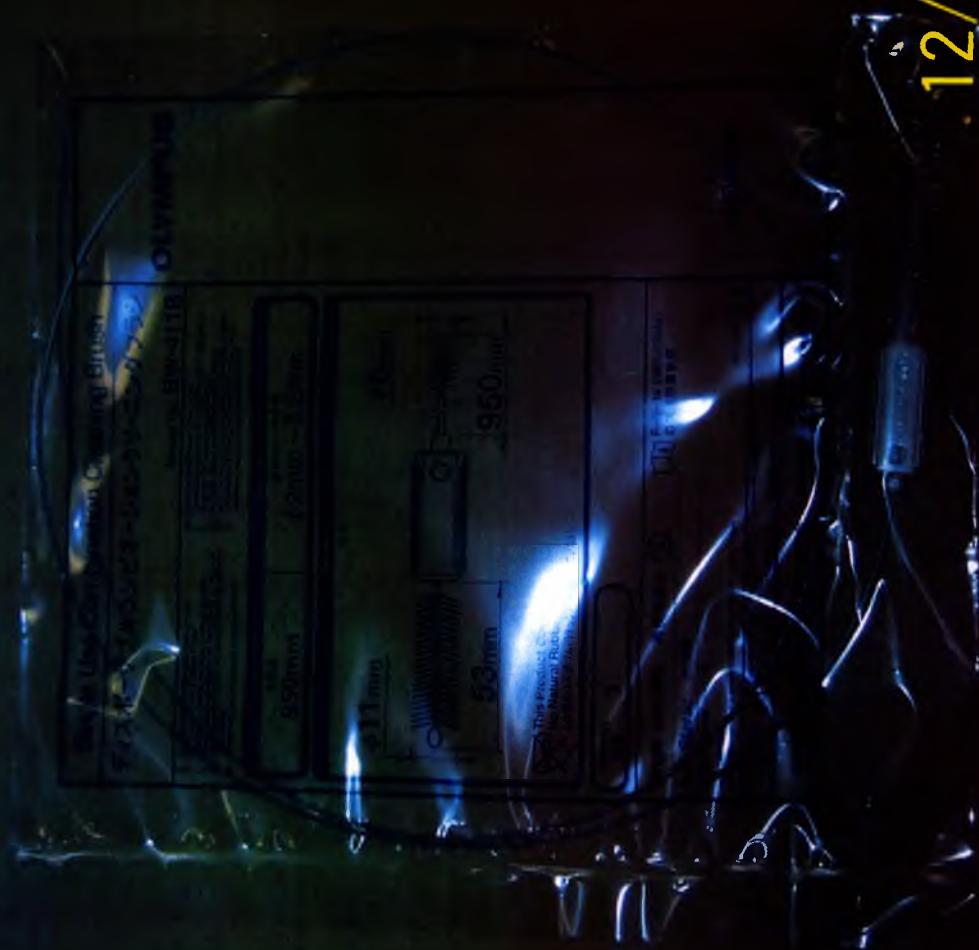

12/12/2014

Одноразовая комбинированная щетка BW-411B

OLYMPUS


INSTRUCTIONS

BRONCHOVIDEOSCOPE

OLYMPUS BF-Q170
OLYMPUS BF-1TQ170

OPERATION MANUAL

Symbols	1
Important Information — Please Read Before Use	2
Chapter 1 Checking the Package Contents	13
Chapter 2 Instrument Nomenclature and Specifications	17
Chapter 3 Preparation and Inspection	25
Chapter 4 Operation	49
Chapter 5 Troubleshooting	71
Appendix	79

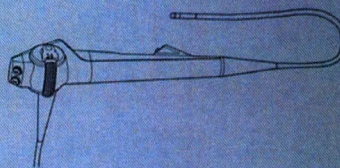

Refer to the endoscope's companion manual, the "REPROCESSING MANUAL" with your endoscope model listed on the cover for reprocessing information.
USA: CAUTION: Federal law restricts this device to sale by or on the order of a physician.

CE
0177

12/12/2014

OLYMPUS

INSTRUCTIONS

ENDOSCOPES


OLYMPUS BF-Q170
OLYMPUS BF-1TQ170

REPROCESSING MANUAL


Chapter 1. General Policy	1
Chapter 2. Functions and Inspection of the Accessories for Reprocessing	9
Chapter 3. Compatible Reprocessing Methods and Chemical Agents	19
Chapter 4. Reprocessing Workflow for Endoscopes and Accessories	31
Chapter 5. Reprocessing the Endoscope (and Related Reprocessing Accessories)	39
Chapter 6. Reprocessing the Accessories	73
Chapter 7. Reprocessing Endoscopes and Accessories Using an Automated Endoscope Reprocessor/Washer-Disinfector	85
Chapter 8. Storage and Disposal	88

Accessories:

- Sterilization cap (MAJ-1534)
 - Channel cleaning brush (BW-156)
 - Channel opening cleaning brush (JH-507)
 - Suction valve (MAJ-207^{*)}
- * These products may not be available in some areas.



- Suction cleaning adapter (MAJ-222)
- Single use configuration cleaning brush (BBI-4193)
- Empty valve (MO-405[†])
- Mouthpiece (MA-451)



Refer to the endoscope's companion manual, the "OPERATION MANUAL," with your endoscope model listed on the cover, for operation information.

USA: CAUTION: Federal law prohibits this device to be sold by or on the order of a physician.

12/12/2014

Всего пронумеровано,
прошнуровано и
скреплено печатью
10 (десять) листа (ов)

