

ООО «Смит энд Нефью»
Юр.адрес: 105120 г. Москва,
2-й Сыромятнический пер, 1
эт.9, пом.1, комн.1

Почт.адрес: 105120 г. Москва,
2-й Сыромятнический пер, 1

Т: + 7 495 755 55 03
www.smith-nephew.com
info.russia@smith-nephew.com

SmithNephew

«УТВЕРЖДАЮ»

Руководитель отдела
регистрации и нормативно-
правовой документации
ООО «Смит энд Нефью»

Хайруллина А.А.



(Доверенность: б/н, № бланка 77-АД 0948378 от 03.08.2022 г.
Зарегистрировано в реестре: № 77/216-н/77-2022-3-1888)

«07» сентября 2022 г.

Фотографические изображения


«Компоненты ревизионного протеза тазобедренного сустава REDAPT»

Производства

Smith & Nephew Inc. (Смит энд Нефью Инк.), USA (США).

2022

Маркировка вторичной упаковки (картонной коробки) медицинского изделия на примере варианта исполнения: Ножка ревизионная монокитная REDAPT, латерализованная, L 240 мм, размер 17

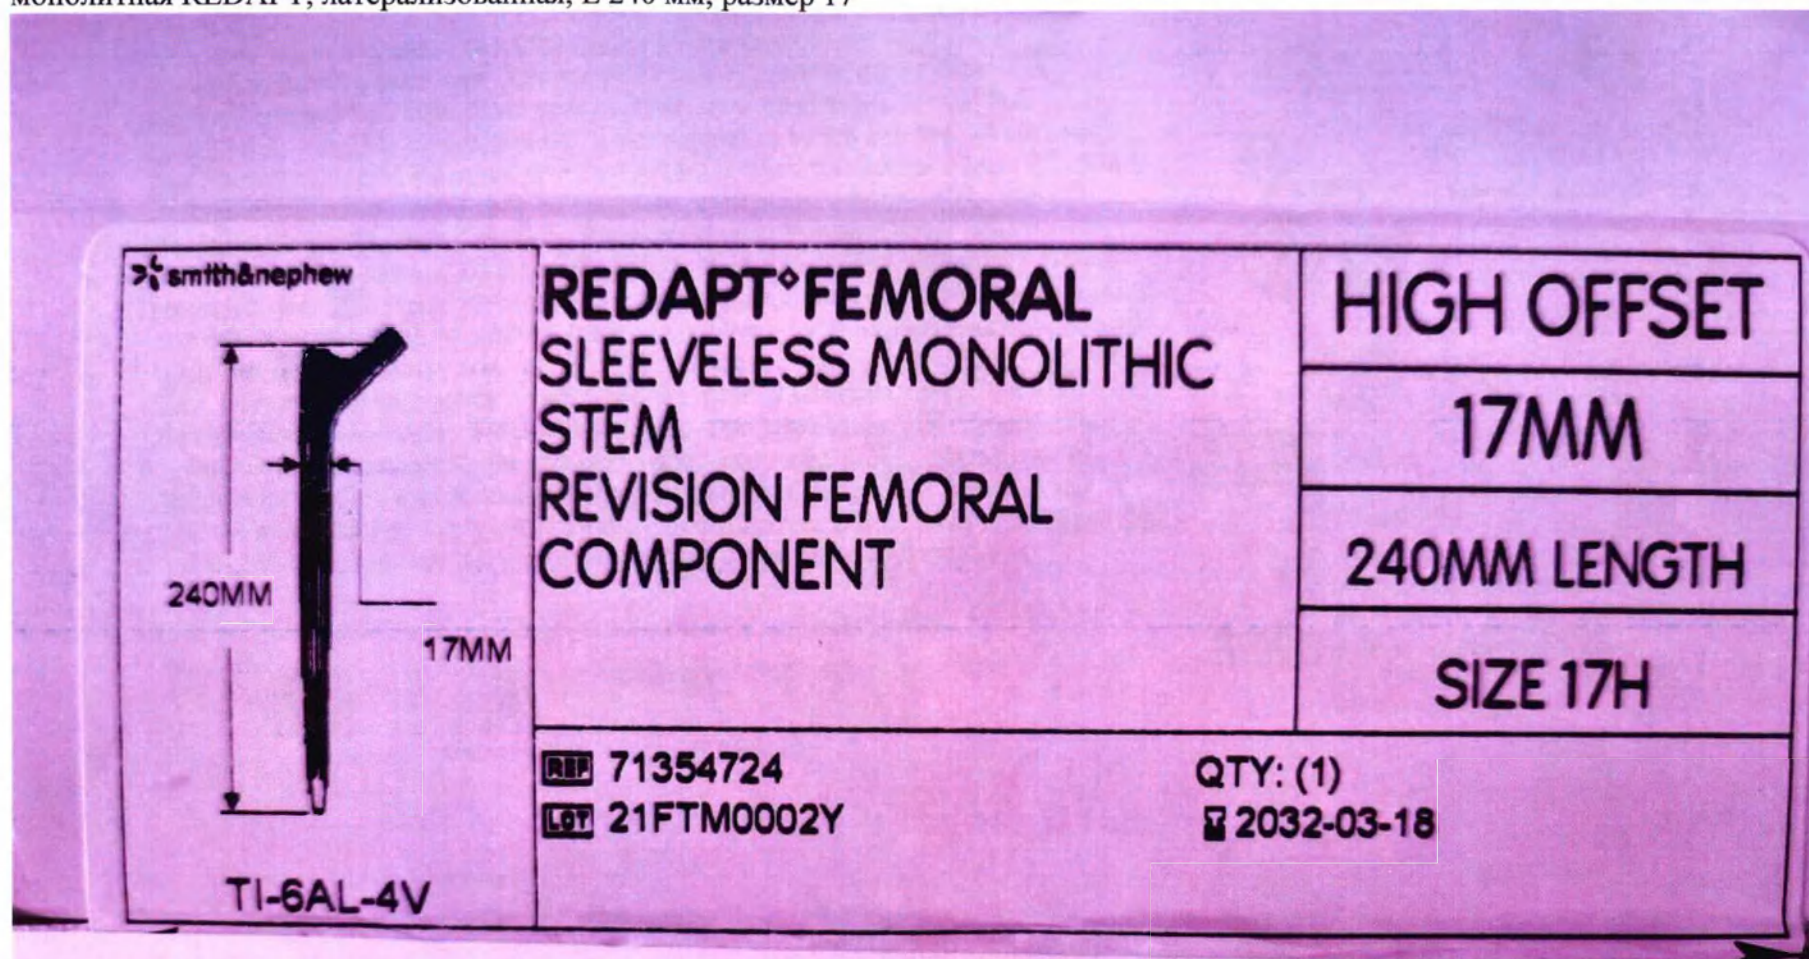

EN Sleeveless Monolithic Stem Revision Femoral Component High Offset **DE**
 Monoblock-Schaft ohne Hülse, Revisions-Femurkomponente, hoher Offset **NL**
 Femurcomponent met hoge offset voor monolithische steelrevisie zonder huls **IT**
 Componente femorale di revisione con stele monolitico senza camicia, offset alto **FR**
 Tige monolithique sans manchon pour composant fémoral de reprise, déport élevé **ES**
 Vástago monolítico sin vaina para componente femoral de revisión, offset alto **PT**
 Mansõesuz Monolitik Stem Revizyonu Femoral Bileşeni Yüksek Offsetli **PL**
 Monolityczny trzon bez tulei do elementu kości udowej do operacji rewizyjnej z dużym
 przesunięciem **PT** Haste monolítica sem manga para revisão do componente femoral
 com desvio elevado **NO** Monolitisk stamme uten hylse for revisjonsfemurkomponent,
 høy offset **SV** Monolitiskt skaft utan muff revision femoral komponent hög förskjutning
DA Femurrevisionskomponent med monolitisk skaft uden krave, højt offset **FI**
 Holkiton monolittinen varsi, revision reisiiluosa, suuri polkkeama **CS** Vysoký offset
 revizní femorální komponenty monolitického dílku bez pouzdra **RO** Componentă
 femorală de revizie tipă monolitică fără manșon cu decalaj mare **EL** Μονολιθικός
 στυλός αναθεώρησης χωρίς χιτώνιο για μηριαίο εξάρτημα, υψηλή πλάγια μετάθεση **HU**
 Hüvely nélküli, monolitikus törzsrevisziós femorális komponens, erős eltolással

This product may be covered by one or more U.S. patents. See smith-nephew.com/patents for details.

UDI



(01) 00665556578466 (17) 320318 (10) 21FTM0002Y



(11) 220321

* Trademark(s) of Smith & Nephew.

STERILE R

CE 2797

Rx only



COUNTRY OF ORIGIN

USA

2022-03-21

Smith & Nephew, Inc. 1450
 Brooks Road, Memphis, TN
 38116 USA

EC REP

Smith & Nephew Operations
 B.V., Bloemlaan 2, 2132 NP
 Hoofddorp, Netherlands



Internal Use Only
 825H19C4AA; 11



Internet Use Only
EIS-19000a-1



Fraserburgh, of Smith & Nephew



 smith&nephew

R_x only

REF 71354464
LGT 21CTM0019S
REDAPT FEMORAL
STANDARD OFFSET, 15MM, 190MM, SIZE 15
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-6AL-4V

UDI

17132038
R0121CTM0019S
101 00865556560565

QTY: (1)
2032-03-18

2022-03-21
Smith & Nephew, Inc.
1450 Brooks Road,
Memphis, TN 38116 USA

smith&nephew

STERILE R

PEEL



CHART LABEL

REF 71354464

LOT 21CTM0019S

REDAPT FEMORAL
STANDARD OFFSET, 15MM, 190MM, SIZE 15
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-6AL-4V

STERILE R

smith & nephew

2032-03-18



(01) 00885556580585 (17) 320318 (10) 21CTM0019S

(11) 220321

G90H0000AA; 6

CHART LABEL

REF 71354464

LOT 21CTM0019S

REDAPT FEMORAL
STANDARD OFFSET, 15MM, 190MM, SIZE 15
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-6AL-4V

STERILE R

smith & nephew

2032-03-18



(01) 00885556580585 (17) 320318 (10) 21CTM0019S

(11) 220321

G90H0000AA; 6

Implant Card

REDAPT FEMORAL
STANDARD OFFSET, 15MM, 190MM, SIZE 15
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT

REF 71354464

LOT 21CTM0019S

UDI-DI: (01)00885556580585

UDI



(01) 00885556580585
(17) 320318
(10) 21CTM0019S



ifu.smith-nephew.com

EN Hip Implant **DE** Hüftimplantat **NL** Heupimplantaat
IT Impianto per anca **FR** Implant de hanche **ES** Implante de cadera **TR** Kalça Implantı **PL** Implant stawu biodrowego
PT Implante da anca **NO** Hofteimplantat **SV** Höftimplantat
DA Hofteimplantat **FI** Lonkkaimplantti **CS** Kýčelní implantát **RO** Implant de sold **EL** Εμφύτευση ισχίου **HU** Csípőimplantátum **LT** Klubo implantas **ET** Puusä implantaat **LV** Gūžas implants **BG** Имплант за тазобедрена става **SL** Kolčni vsadek **HR** Implantat za kuk **SK** Bedrový implantát

Smith & Nephew, Inc. 1450 Brooks Road, Memphis, TN 38116 USA

В настоящем документе приведены вносимые изменения, для тех вариантов исполнения, которые они затрагивают: изменения маркировки для всех размеров и вариантов исполнения следующего компонента: Ножка ревизионная монолитная REDAPT. Для остальных вариантов исполнения и компонентов актуальными являются данные, предоставленные в регистрационном досье ранее.

ПРОШТО И
ПРОНУМЕРОВАНО
9 ЛИСТОВ



ООО «Смит энд Нефью»
Юр.адрес: 105120 г. Москва,
2-й Сыромятнический пер, 1
эт.9, пом.1, комн.1

Почт.адрес: 105120 г. Москва,
2-й Сыромятнический пер, 1

Smith+Nephew

Т: + 7 495 755 55 03
www.smith-nephew.com
info.russia@smith-nephew.com

«УТВЕРЖДАЮ»
Руководитель отдела
регистрации и нормативно-правовой
документации
ООО «Смит энд Нефью»
Хайруллина А.А.



(Доверенность: б/н, № бланка 77 АД 0948378 от 03.08.2022 г.
Зарегистрировано в реестре: № 77/216-н/77-2022-3-1888)

«10» января 2022 г.

Фотографические изображения


«Компоненты ревизионного протеза тазобедренного сустава REDAPT»

Производства

Smith & Nephew Inc. (Смит энд Нефью Инк.), USA (США).

2022

I. Ножки ревизионные монолитные REDAPT, на примере вариантов исполнения
Ножка ревизионная монолитная REDAPT, стандартная, L 190 мм, размер 15

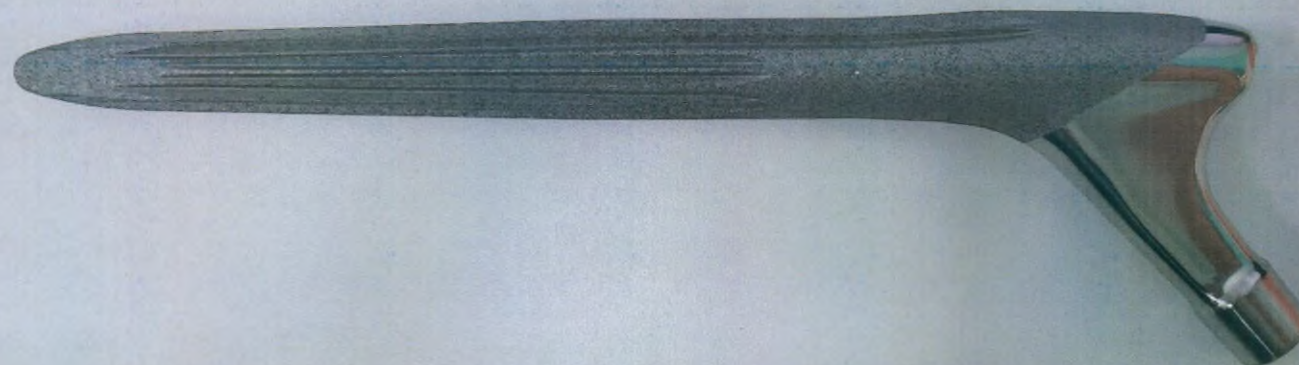

Индивидуальная упаковка: изделие во внутреннем лотке

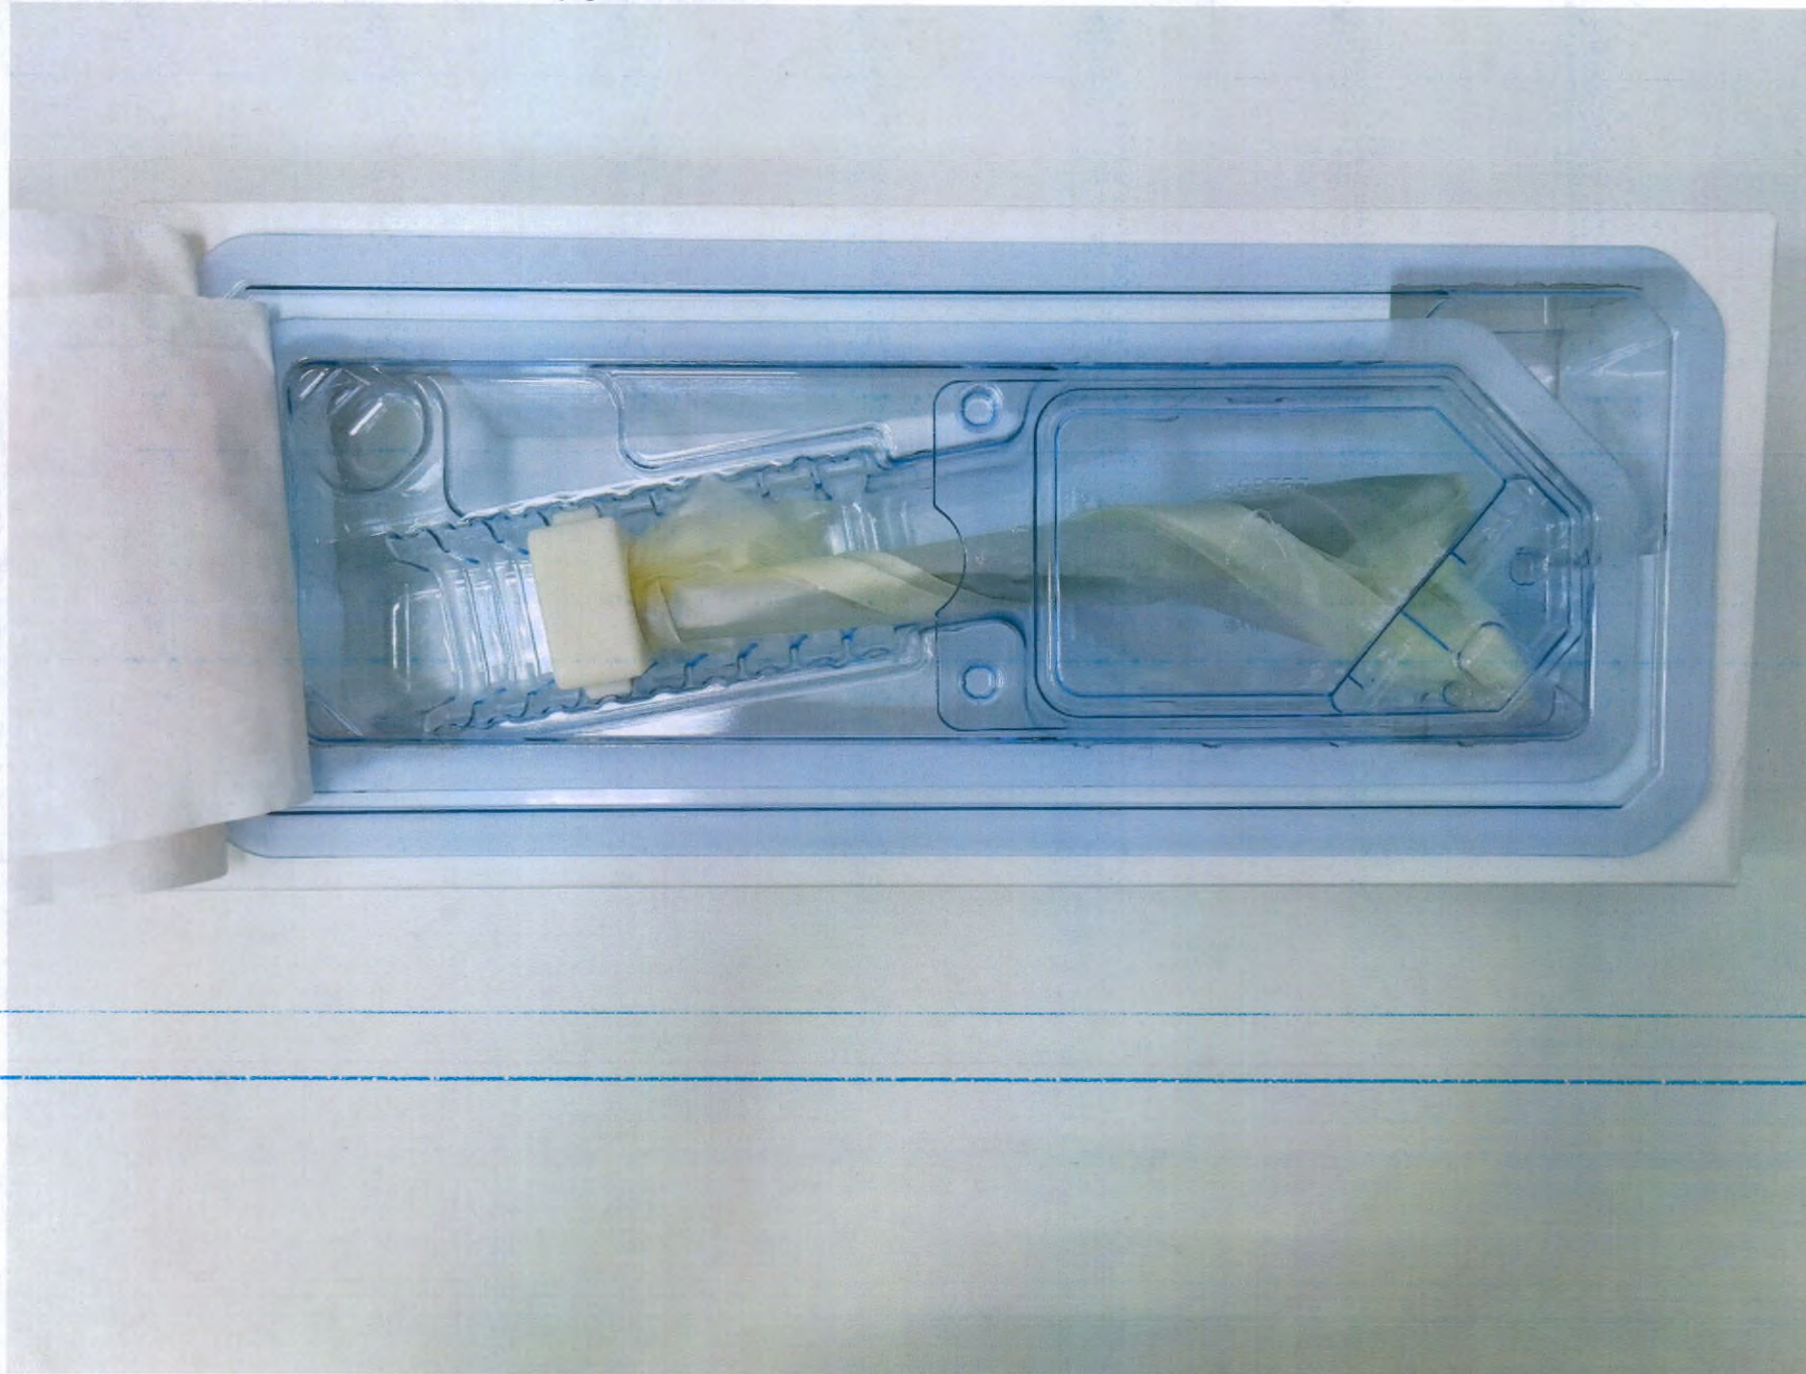




CHART LABEL

REF 71354464

LOT 21CTM0019S

REDAPT FEMORAL
STANDARD OFFSET, 15MM, 190MM, SIZE 15
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-6AL-4V

smith&nephew

2032-03-18

STERILE R



(01) 00885556580585 (17) 320318 (10) 21CTM0019S



(11) 220321

G90H0000AA, 6

CHART LABEL

REF 71354464

LOT 21CTM0019S

REDAPT FEMORAL
STANDARD OFFSET, 15MM, 190MM, SIZE 15
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-6AL-4V

smith&nephew

2032-03-18

STERILE R



(01) 00885556580585 (17) 320318 (10) 21CTM0019S



(11) 220321

G90H0000AA, 6

Implant Card



REDAPT FEMORAL

STANDARD OFFSET, 15MM, 190MM, SIZE 15
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT

REF 71354464

LOT 21CTM0019S

UDI-DI: (01)00885556580585

UDI



(01) 00885556580585
(17) 320318
(10) 21CTM0019S



rfu.smith-nephew.com

EN Hip Implant DE Hüftimplantat NL Heupimplantaat
IT Impianto per anca FR Implant de hanche ES Implante
de cadera TR Kalça Implantı PL Implant stawu biodrowego
PT Implante da anca NO Høfteimplantat SV Höftimplantat
DA Høfteimplantat FI Lonkkaimplantti CS Kýčelní
implantát RO Implant de șold EL Εμφύτεμα ισχίου HU
Csípőimplantátum LT Klubo implantas ET Puusaimplantaat
LV Gūžas implants BG Имплант за
тазобедрена става SL Kolčni vsadek HR Implantat za kuk
SK Bedrový implantát

Smith & Nephew, Inc. 1450 Brooks Road, Memphis, TN 38116 USA

Instructions for Use

English

Gebrauchsanweisung

Total Hip Systems

CAUTION: Federal law (FDA) restricts the sale of total hip arthroplasty devices to sale by or on the order of a physician.

Device Descriptions

Total Hip Systems

The Total Hip Systems consist of femoral components, modular necks, proximal sleeves, taper sleeves, acetabular components, fixation screws and pegs, hole covers, contrails, and femoral heads. Components may be grit blasted, porous coated, hydroxyapatite (HA) coated, or HA porous coated. All implantable devices are for single use only.

Materials

Femoral components are manufactured from cobalt chromium alloy, titanium 6Al-4V alloy, or stainless steel (SS). Femoral heads are manufactured from cobalt chromium alloy (CoCr), 316L stainless steel, BIOLOX forte alumina ceramic, BIOLOX delta alumina/zirconia ceramic, zirconia ceramic, or stainless steel. Acetabular liners are manufactured from ultra-high molecular weight polyethylene (UHMWPE), BIOLOX forte alumina ceramic, or BIOLOX delta alumina/zirconia ceramic. In the U.S., refer to the separate package insert provided with the ceramic acetabular liners. All poly acetabular components are manufactured from UHMWPE. Acetabular shells are manufactured from titanium 6Al-4V alloy or cobalt chromium (CoCr) alloy. BIOLOX delta HPA acetabular cups are cobalt chromium (CoCr) alloy. The component material is provided on the particle carton label. Note: BIOLOX delta ceramic liners are not available for use in the U.S.

Some of the alloys needed to produce orthopedic implants contain metallic components that may be carcinogenic in tissue cultures as in an intact organism under very unique circumstances. Questions have been raised in the scientific literature as to whether or not these alloys may be carcinogenic in implant recipients. Studies conducted to evaluate this issue have not identified conclusive evidence of such phenomenon, in spite of the millions of implants in use.

Femoral Components

Femoral components are available in a variety of sizes. Porous coated components are coated for biological ingrowth and are intended for use without cement. Modular femoral components are available with an oval taper to accept Smith & Nephew CoCr modular necks and/or a Morse type taper to accept proximal sleeves. Non-porous femoral components can feature polyethylene (PE) acetabular components that help produce a uniform cement thickness. Femoral components, available with 12/14, 12/16, and 14/16 tapers, mate and lock directly with Smith & Nephew femoral heads having the same size taper. Certain femoral heads may require laser sleeves for attachment to the femoral stem taper. Refer to the label on the taper sleeve section for details.

Taper Sleeves

A taper sleeve may be required when mating femoral stems with specific types of femoral heads. Refer to the sleeve compatibility table for the appropriate combinations. Failure to utilize the proper sleeve to head combination may lead to implant failure and may result in revision surgery. Never place more than one taper sleeve on a femoral component; this combination will increase stresses on the implant and may lead to failure and may result in revision surgery.

Modular Necks

Modular necks are made from CoCr alloy and are available in a variety of configurations. The modular neck mates and locks with the oval taper of a modular femoral component on one end and the taper of a 12/14 femoral head on the other end.

Compatible Sleeve Combinations

Femoral Stem	40, 44 mm Modular CoCr Heads	40, 44 mm Modular CoCr Heads	BH Modular CoCr Heads	14/16 OXNUM and CoCr Heads	14/16 OXNUM and CoCr Heads
12/14	A	A	B	B	C
14/16	-	-	-	D	No sleeve required
12/12	-	-	-	E	F

* Modular CoCr heads are made from CoCr alloy and are intended for hemiarthroplasty use in the U.S. Refer to the separate package insert provided with the components.

** BH Modular heads are not available for use in the U.S. These heads can only be used with cemented BIODUC® femoral stems.

Sleeve	Material	Description/Part Numbers
A	Ti-6Al-4V	12/14 Modular Sleeve - 71344231, +0: 71344232, +8: 71344233, +16: 71344234
B	CoCr	12/14 Modular Sleeve - 71322700, +0: 71322701, +8: 71322702, +16: 71322703
C	Ti-6Al-4V	14/16 12/14 Modular Sleeve - 71326603, +0: 71326604, +8: 71326605, +16: 71326606
D	Ti-6Al-4V	14/16 12/14 Modular Sleeve - 71326603, +0: 71326604, +8: 71326605, +16: 71326606
E	Ti-6Al-4V	12/12 12/14 Modular Sleeve - 71326603, +0: 71326604, +8: 71326605, +16: 71326606
F	Ti-6Al-4V	12/12 12/14 Modular Sleeve - 71326603, +0: 71326604, +8: 71326605, +16: 71326606

Femoral Heads

For proper anatomic and mechanical fit, cobalt chromium, stainless steel, oxidized titanium, and ceramic heads are available in multiple neck lengths. Heads are available in 12/12, 12/14, and 14/16 tapers. Certain modular heads and unipolar heads may require taper sleeves for attachment to the femoral stem taper. Refer to the Compatible Sleeve Combinations table in the Taper Sleeve section for details. Heads are highly polished for reduced friction and wear. Femoral components and femoral heads are designed for use with any Smith & Nephew cemented acetabular component or cementless BIODUC® cemented acetabular component. Cemented acetabular components are not available for use in the U.S.

Hüfttotalsysteme

VORSICHT: Gemäß der US-amerikanischen Bundesgesetzgebung ist der Verkauf von Hüftgelenkprothesen nur an einen Arzt oder auf dessen Rezept zulässig.

Produktbeschreibungen

Hüfttotalsysteme

Die Hüfttotalsysteme bestehen aus Femoral- und Acetabularkomponenten, modulare Halsen, proximale Ärmeln, Taper-Ärmeln, Acetabularschalen, Fixationschrauben und -Nägeln, Lochabdeckungen, Kontrails und Femurköpfe. Die Komponenten können sandgestrahtet, porös beschichtet, mit Hydroxyapatit (HA) beschichtet oder mit HA-poröser Beschichtung versehen sein. Alle implantierbaren Geräte sind nur zum einmaligen Gebrauch vorgesehen.

Materialien

Femorale Komponenten werden aus Kobalt-Chrom-Legierung, Titan 6Al-4V-Legierung oder Edelstahl (SS) gefertigt. Die Hüftköpfe sind aus Kobalt-Chrom-Legierung, Titan 316L, BIOLOX forte Aluminiumoxid-Keramik, BIOLOX delta Aluminiumoxid-Zirkonoxid-Keramik oder Edelstahl gefertigt. Die Acetabularschalen werden aus ultrahochmolekularem Polyethylen (UHMWPE), BIOLOX forte Aluminiumoxid-Keramik oder BIOLOX delta Aluminiumoxid-Zirkonoxid-Keramik gefertigt. In den USA: Bitte auf das separate Packungsbeilage für die Acetabularschalen mit Keramikacetabularschalen achten. Alle polyacetabularen Komponenten werden aus UHMWPE gefertigt. Acetabulare Schalen werden aus Titan 6Al-4V-Legierung oder Kobalt-Chrom-Legierung (CoCr) gefertigt. BIOLOX delta HPA Acetabulare Schalen sind aus Kobalt-Chrom-Legierung (CoCr). Das Komponente-Material ist auf dem Partikelkarton angegeben. Hinweis: BIOLOX delta Keramikacetabularschalen sind nicht für den Einsatz in den USA verfügbar. Einige Legierungen, die zur Herstellung von orthopädischen Implantaten verwendet werden, enthalten metallische Komponenten, die in Zellkulturen als potenziell karzinogen unter sehr speziellen Umständen identifiziert wurden. In der wissenschaftlichen Literatur wurde diskutiert, ob diese Legierungen in Implantatempfängern karzinogen sein könnten. Durchgeführte Studien zur Bewertung dieses Phänomens haben keine schlüssigen Ergebnisse geliefert.

Femorale Komponenten

Femorale Komponenten sind in verschiedenen Größen erhältlich. Porös beschichtete Komponenten sind für den Einsatz ohne Zement vorgesehen. Modulare femorale Komponenten sind mit einem Ovaltaper, der mit Smith & Nephew CoCr-Modularen Halsen und/oder Morse-Taper, der mit proximalen Ärmeln, kompatibel ist. Nicht-poröse femorale Komponenten können mit einer Polyethylen-Acetabularkomponente ausgestattet sein, die zu einer gleichmäßigen Zementstärke beiträgt. Femorale Komponenten, die mit 12/14, 12/16 und 14/16 Tapers, passen direkt mit Smith & Nephew Femurköpfen, die den gleichen Taper haben. Bestimmte Femurköpfe erfordern Laser-Ärmel für die Montage am Femurstamm-Taper. Bitte auf das Etikett der Taper-Ärmel-Sektion für Details achten.

Kugelhülsen

Ein Taper-Sleeve kann erforderlich sein, wenn femorale Stämme mit bestimmten Arten von Femurköpfen zusammengebracht werden. Bitte auf die Kompatibilitätstabelle für die richtigen Kombinationen achten. Ein falsches Taper-Sleeve-Kombination kann zu einer Lockerung des Implantats und damit zu einer Revisionsoperation führen. Setzen Sie nie mehr als einen Kugelhülse auf ein Implantat. Diese Kombination erhöht die Belastung des Implantats und kann zu einem Versagen führen.

Modulare Hälse

Modulare Hälse werden aus CoCr-Legierung gefertigt und sind in verschiedenen Konfigurationen erhältlich. Der modulare Hals passt zu einem Ovaltaper einer modulare femoralen Komponente auf einer Seite und zu einem 12/14 Femurkopf auf der anderen Seite.

Femoraler Schaft	40, 44 mm Modulare CoCr Köpfe	40, 44 mm Modulare CoCr Köpfe	BH Modulare CoCr Köpfe	14/16 OXNUM und CoCr Köpfe	14/16 OXNUM und CoCr Köpfe
12/14	A	A	B	B	C
14/16	-	-	-	D	Kein Sleeve erforderlich
12/12	-	-	-	E	F

* Modulare CoCr-Köpfe sind aus CoCr-Legierung gefertigt und sind für die Hemiarthroplastie in den USA vorgesehen. Bitte auf das separate Packungsbeilage für die Komponenten achten.


** BH-Modulköpfe sind in den USA nicht verfügbar. Diese Köpfe können nur mit zementierten BIODUC® Femoralstäben verwendet werden.

Ärmel	Material	Beschreibung/Teilenummern
A	Ti-6Al-4V	12/14 Modularer Ärmel - 71344231, +0: 71344232, +8: 71344233, +16: 71344234
B	CoCr	12/14 Modularer Ärmel - 71322700, +0: 71322701, +8: 71322702, +16: 71322703
C	Ti-6Al-4V	14/16 12/14 Modularer Ärmel - 71326603, +0: 71326604, +8: 71326605, +16: 71326606
D	Ti-6Al-4V	14/16 12/14 Modularer Ärmel - 71326603, +0: 71326604, +8: 71326605, +16: 71326606
E	Ti-6Al-4V	12/12 12/14 Modularer Ärmel - 71326603, +0: 71326604, +8: 71326605, +16: 71326606
F	Ti-6Al-4V	12/12 12/14 Modularer Ärmel - 71326603, +0: 71326604, +8: 71326605, +16: 71326606

Femurköpfe

Für eine korrekte anatomische und mechanische Passform sind verschiedene Halslängen verfügbar. Die Köpfe sind in 12/12, 12/14 und 14/16 Tapers erhältlich. Bestimmte modulare Köpfe und unipolare Köpfe erfordern Taper-Ärmel für die Montage am Femurstamm-Taper. Bitte auf die Kompatibilitätstabelle in der Taper-Ärmel-Sektion für Details achten. Die Köpfe sind hochpoliert, um die Reibung zu reduzieren und den Verschleiß zu verringern. Femoral-Komponenten und Femurköpfe sind für den Einsatz mit jedem zementierten Acetabular-Komponente oder zementlosem BIODUC® zementiertem Acetabular-Komponente geeignet. Zementierte Acetabular-Komponenten sind in den USA nicht verfügbar.

smith&nephew

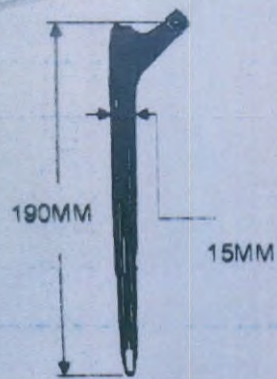

TI-6AL-4V

REDAPT° FEMORAL
SLEEVELESS MONOLITHIC
STEM
REVISION FEMORAL
COMPONENT

STANDARD OFFSET

15MM

190MM LENGTH


SIZE 15

REF 71354464
LOT 21CTM0019S


QTY: (1)
2032-03-18




Ножка ревизионная монолитная REDAPT, латерализованная, L 240 мм, размер 17

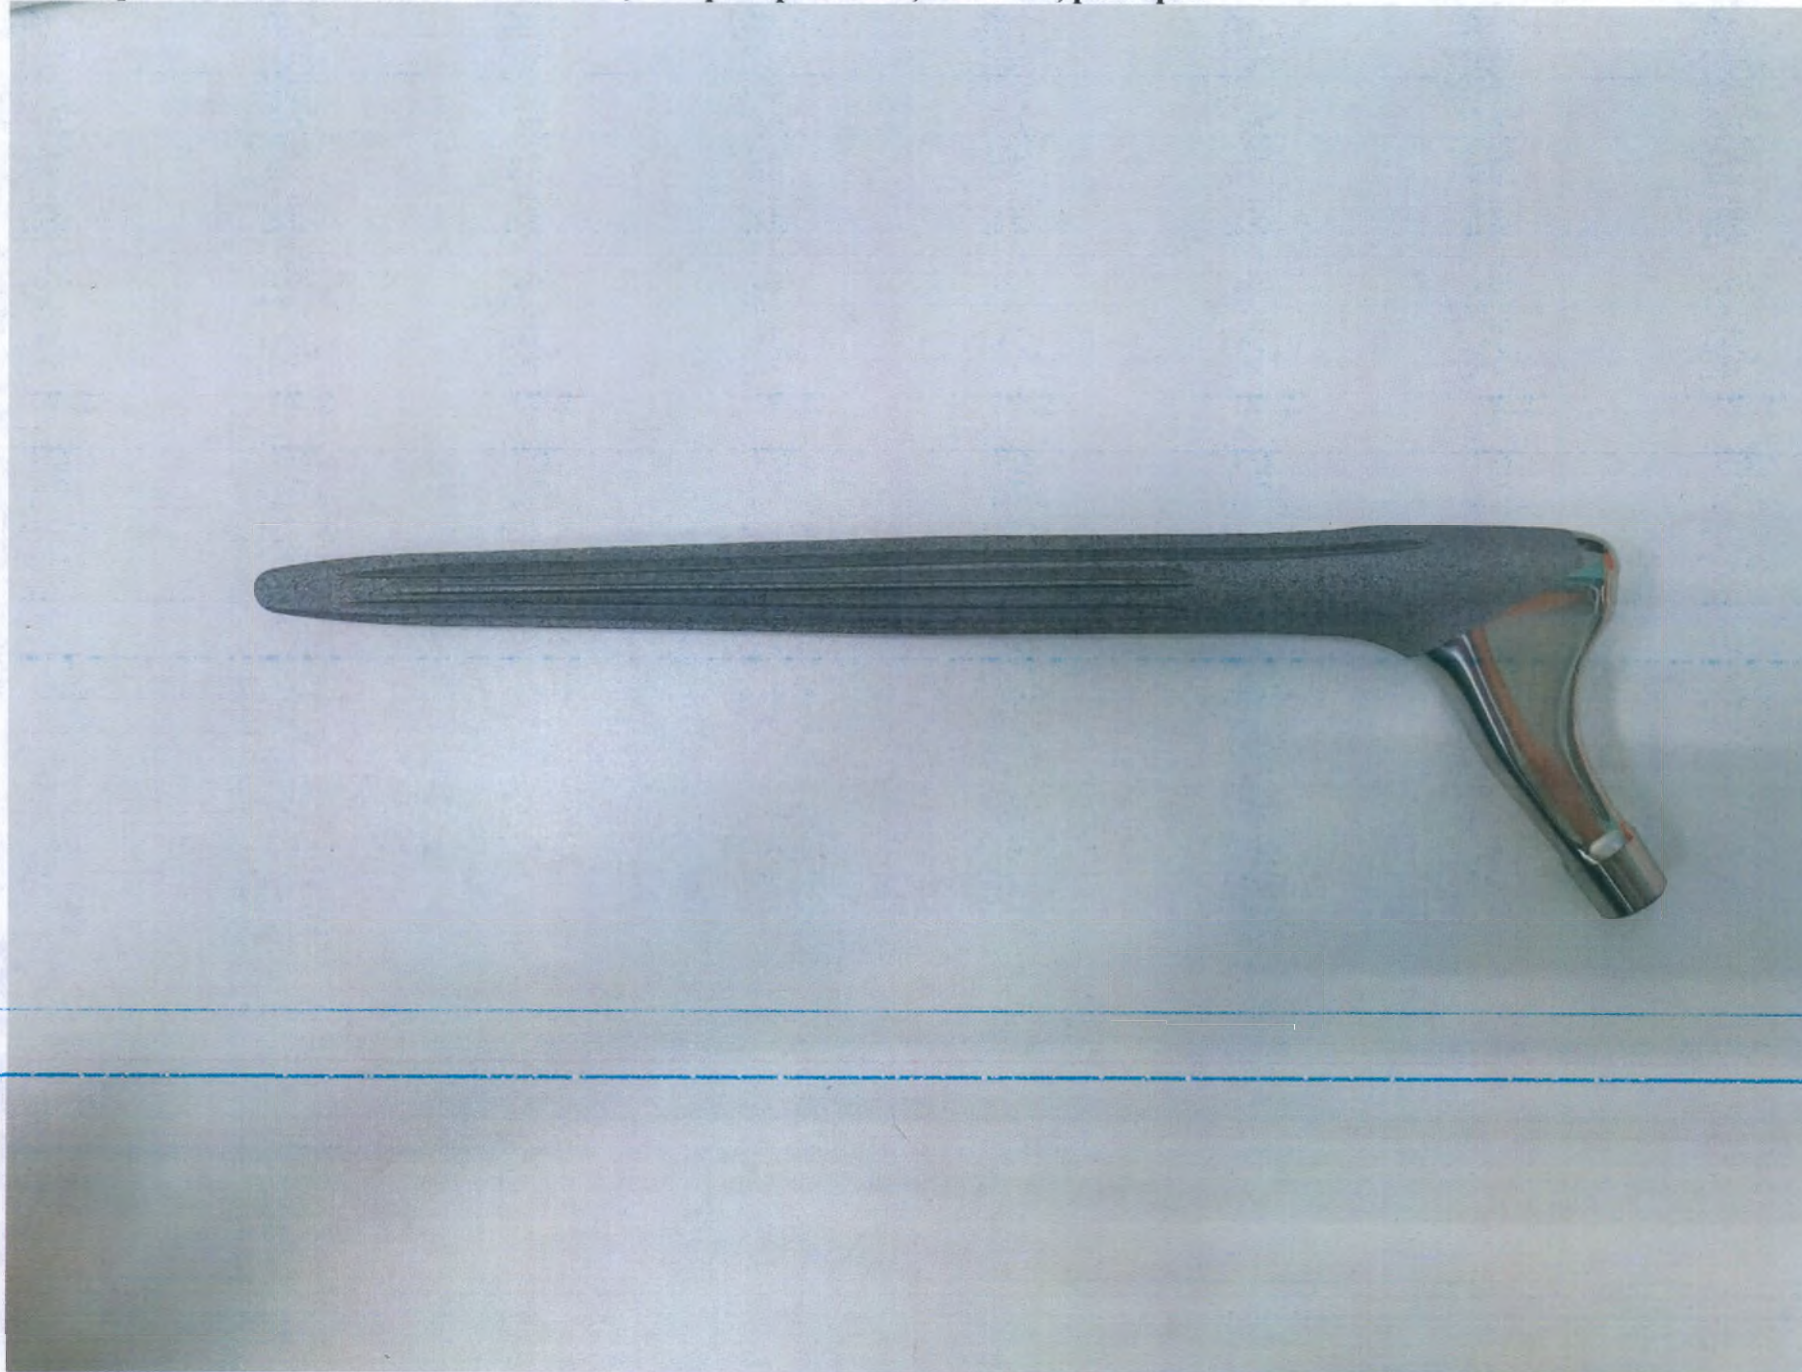

Индивидуальная упаковка: изделие во внутреннем лотке

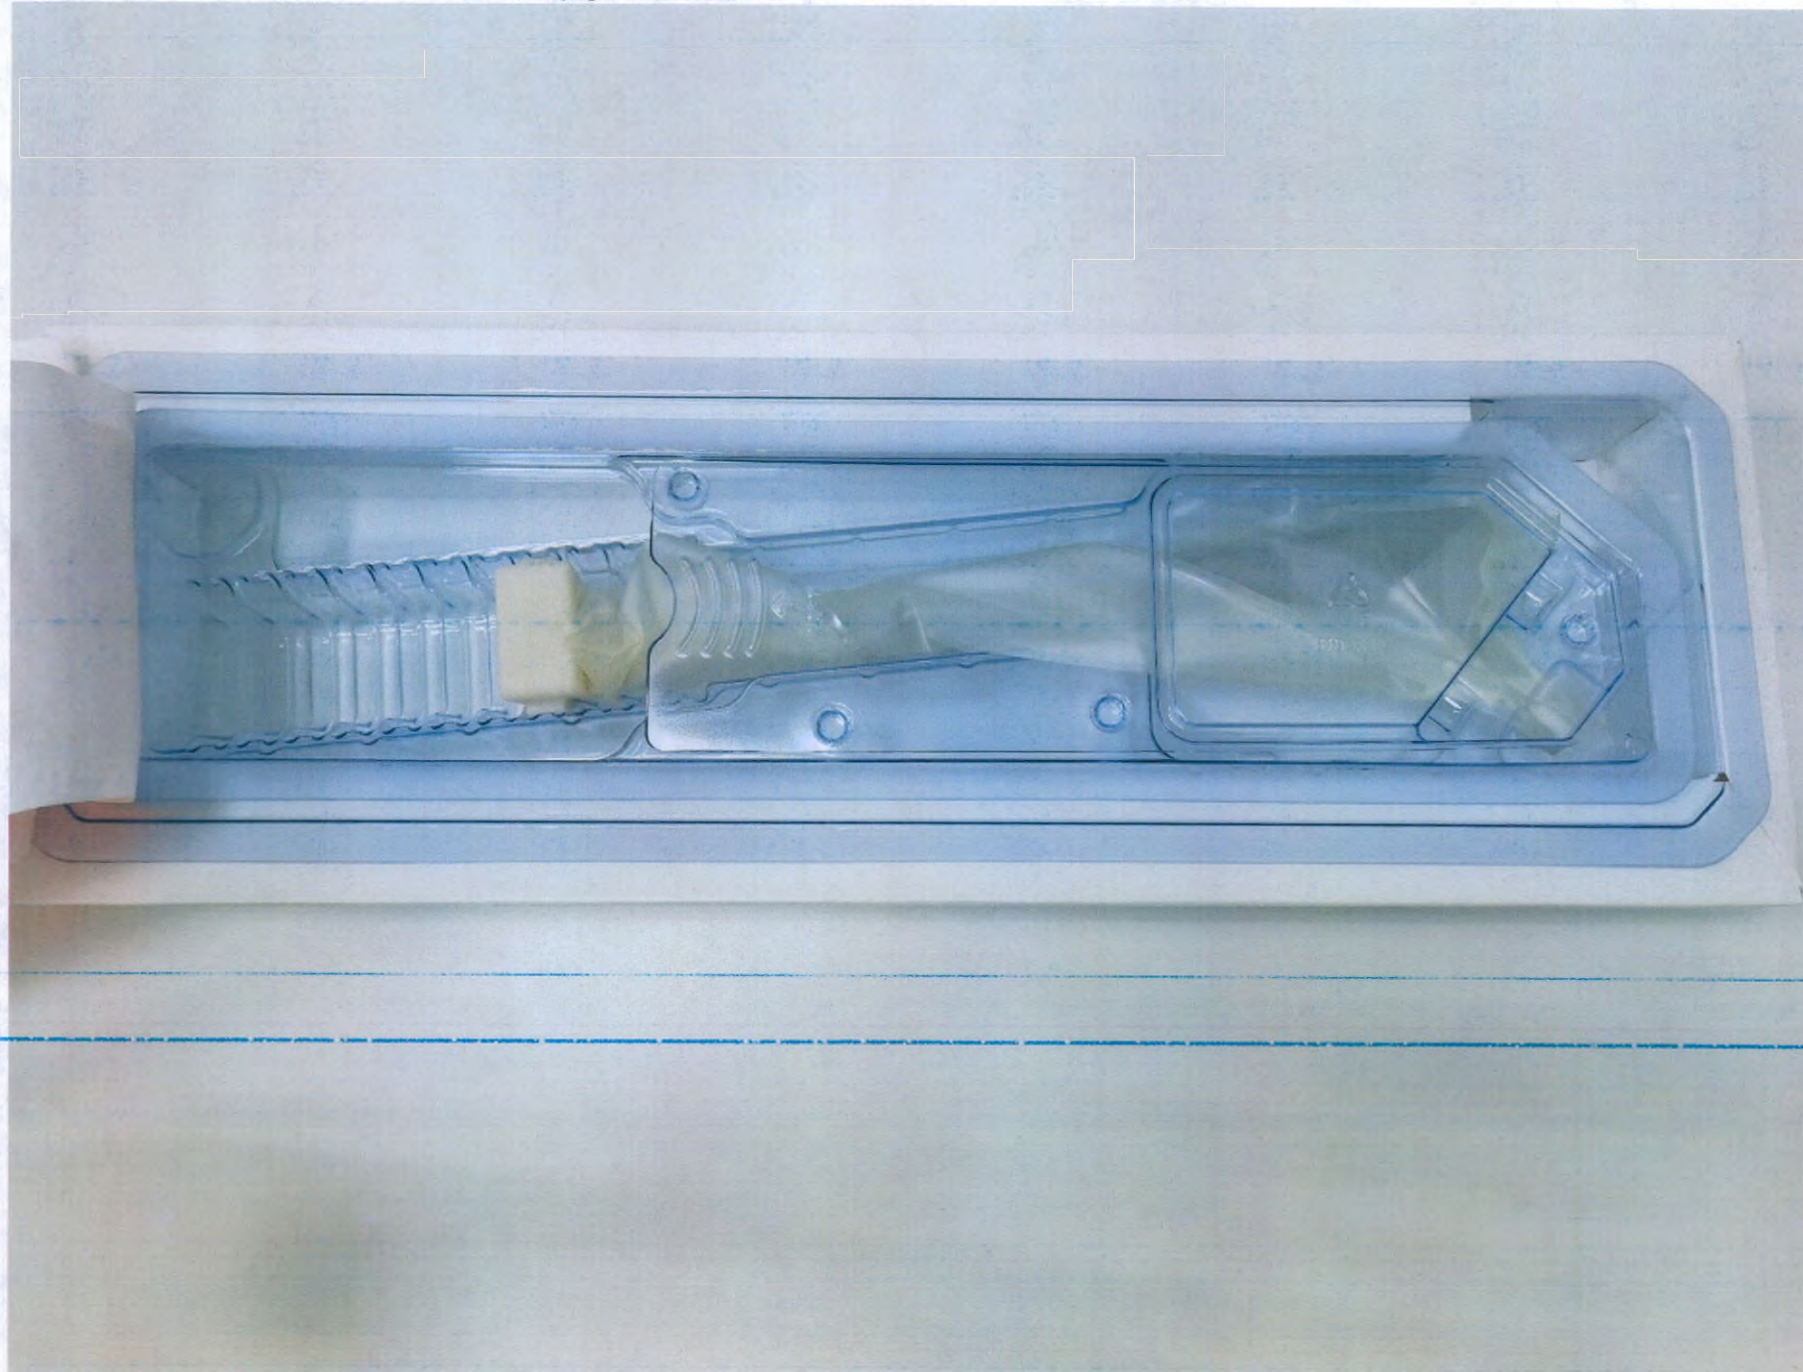

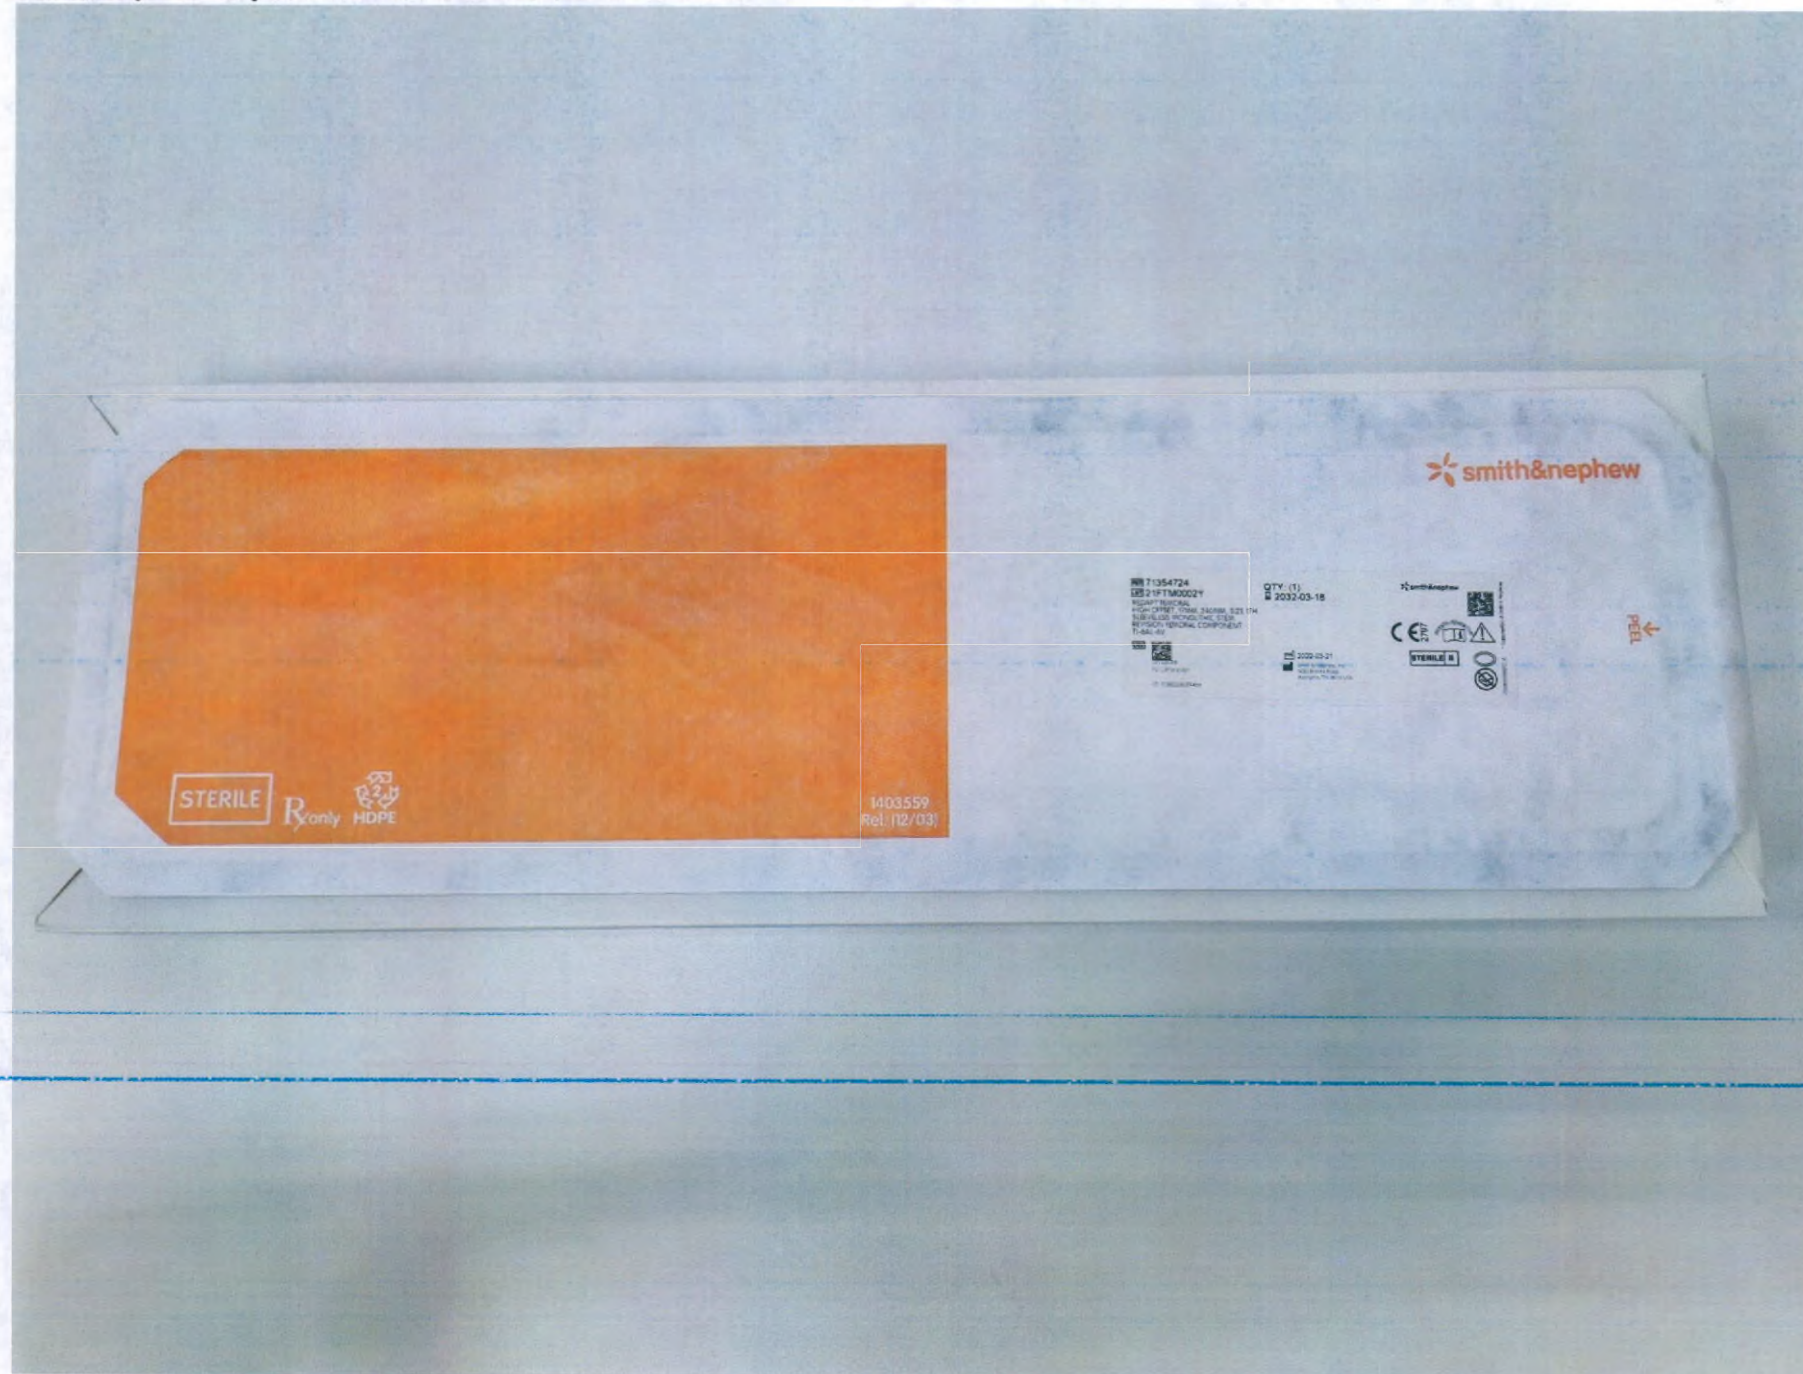

(11) 220321

GRH0000AA, 6

CHART LABEL

RED 71354724

RED 21FTM0002Y STERILE R 2032-03-18

REDAPT FEMORAL
HIGH OFFSET, 17MM, 240MM, SIZE 17H
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-SAL-4V

(01) 00885558579466 (17) 320318 (10) 21FTM0002Y
(11) 220321

GRH0000AA, 6

CHART LABEL

RED 71354724

RED 21FTM0002Y STERILE R 2032-03-18

REDAPT FEMORAL
HIGH OFFSET, 17MM, 240MM, SIZE 17H
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-SAL-4V

(01) 00885558579466 (17) 320318 (10) 21FTM0002Y
(11) 220321

GRH0000AA, 6

CHART LABEL

RED 71354724

RED 21FTM0002Y STERILE R 2032-03-18

REDAPT FEMORAL
HIGH OFFSET, 17MM, 240MM, SIZE 17H
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
TI-SAL-4V

(01) 00885558579466 (17) 320318 (10) 21FTM0002Y
(11) 220321

GRH0000AA, 6

Implant Card

REDAPT FEMORAL

HIGH OFFSET, 17MM, 240MM, SIZE 17H

SLEEVELESS MONOLITHIC STEM

REVISION FEMORAL COMPONENT

RED 71354724 **RED 21FTM0002Y**

UDI-DI: (01)00885558579466

MD

(01) 00885558579466
CN 320318
(10) 21FTM0002Y

ifu.smith-nephew.com

EN Hip Implant **DE** Hüftimplantat **NL** Heup implantaat
IT Impianto per anca **FR** implant de hanche **ES** Implante
 de cadera **RU** Кольца импланти **PL** Implant stawu biodrowego
PT Implante da anca **NO** Høfteimplantat **SV** Höftimplantat
DA Høfteimplantat **FI** Lonkkaimplantti **CZ** Kyčelní
 implantát **RO** Implant de sold **EL** Εμφύτεμα ισχίου **HU**
 Csípőimplantátum **LT** Klubo implantas **ET**
 Puusai implantaat **LV** Gūžas implants **BG** Имплант за
 тазобедрена става **SL** Kolčni vsadek **HR** Implantat za kuk
SK Bedrový implantát

Smith & Nephew, Inc. 1450 Brooks Road, Memphis, TN 38116 USA

Instructions for Use

Total Hip Systems

R

Device Description

The Total Hip System is a modular, cementless, total hip replacement system. It consists of a femoral component, a tibial component, and a tibial head. The femoral component is made of titanium alloy and is cementless. The tibial component is made of titanium alloy and is cementless. The tibial head is made of titanium alloy and is cementless. The system is designed for use in patients with end-stage hip disease.

Indications

The Total Hip System is indicated for use in patients with end-stage hip disease, including osteoarthritis, rheumatoid arthritis, and trauma. It is also indicated for use in patients with hip dysplasia and hip fracture.

Contraindications

The Total Hip System is contraindicated for use in patients with severe osteoporosis, severe joint infection, and severe soft tissue disease. It is also contraindicated for use in patients with severe hip dysplasia and hip fracture.

Warnings

The Total Hip System should be used in accordance with the instructions for use. It should not be used in patients with severe osteoporosis, severe joint infection, and severe soft tissue disease. It should also not be used in patients with severe hip dysplasia and hip fracture.

Precautions

The Total Hip System should be used in accordance with the instructions for use. It should not be used in patients with severe osteoporosis, severe joint infection, and severe soft tissue disease. It should also not be used in patients with severe hip dysplasia and hip fracture.

Adverse Effects

The Total Hip System may cause adverse effects, including pain, swelling, and redness. It may also cause infection and joint loosening. Patients should be monitored for these effects.

Storage

The Total Hip System should be stored in a dry, clean, and cool place. It should not be exposed to moisture or extreme temperatures.

Disposal

The Total Hip System should be disposed of in accordance with local regulations. It should not be incinerated or disposed of in the environment.

Gebrauchsanweisung

Hüfttotalsystem

R

Gerätebeschreibung

Das Hüfttotalsystem ist ein modulares, zementloses, totalprothetisches Hüftgelenk. Es besteht aus einem Femurkomponente, einem Tibiakomponente und einem Tibiakopf. Das Femurkomponente ist aus Titanlegierung gefertigt und zementlos. Das Tibiakomponente ist aus Titanlegierung gefertigt und zementlos. Der Tibiakopf ist aus Titanlegierung gefertigt und zementlos. Das System ist für Patienten mit Endstadium der Hüftgelenkkrankheit konzipiert.

Indikationen

Das Hüfttotalsystem ist für Patienten mit Endstadium der Hüftgelenkkrankheit, einschließlich Osteoarthritis, Rheumatoide Arthritis und Trauma, indiziert. Es ist auch für Patienten mit Hüftgelenkdisplasie und Hüftfraktur indiziert.

Kontraindikationen

Das Hüfttotalsystem ist kontraindiziert für Patienten mit schwerer Osteoporose, schwerer Gelenkinfektion und schwerer Weichteilkrankheit. Es ist auch kontraindiziert für Patienten mit schwerer Hüftgelenkdisplasie und Hüftfraktur.

Warnungen

Das Hüfttotalsystem sollte gemäß den Gebrauchsanweisungen verwendet werden. Es sollte nicht bei Patienten mit schwerer Osteoporose, schwerer Gelenkinfektion und schwerer Weichteilkrankheit verwendet werden. Es sollte auch nicht bei Patienten mit schwerer Hüftgelenkdisplasie und Hüftfraktur verwendet werden.

Vorsichtsmaßnahmen

Das Hüfttotalsystem sollte gemäß den Gebrauchsanweisungen verwendet werden. Es sollte nicht bei Patienten mit schwerer Osteoporose, schwerer Gelenkinfektion und schwerer Weichteilkrankheit verwendet werden. Es sollte auch nicht bei Patienten mit schwerer Hüftgelenkdisplasie und Hüftfraktur verwendet werden.

Nebenwirkungen

Das Hüfttotalsystem kann Nebenwirkungen verursachen, einschließlich Schmerzen, Schwellung und Rötung. Es kann auch Infektionen und Gelenklockerungen verursachen. Patienten sollten auf diese Nebenwirkungen überwacht werden.


Lagerung

Das Hüfttotalsystem sollte in einem trockenen, sauberen und kühlen Ort gelagert werden. Es sollte nicht Feuchtigkeit oder extremen Temperaturen ausgesetzt werden.


Entsorgung

Das Hüfttotalsystem sollte gemäß den örtlichen Vorschriften entsorgt werden. Es sollte nicht verbrannt oder in die Umwelt entsorgt werden.




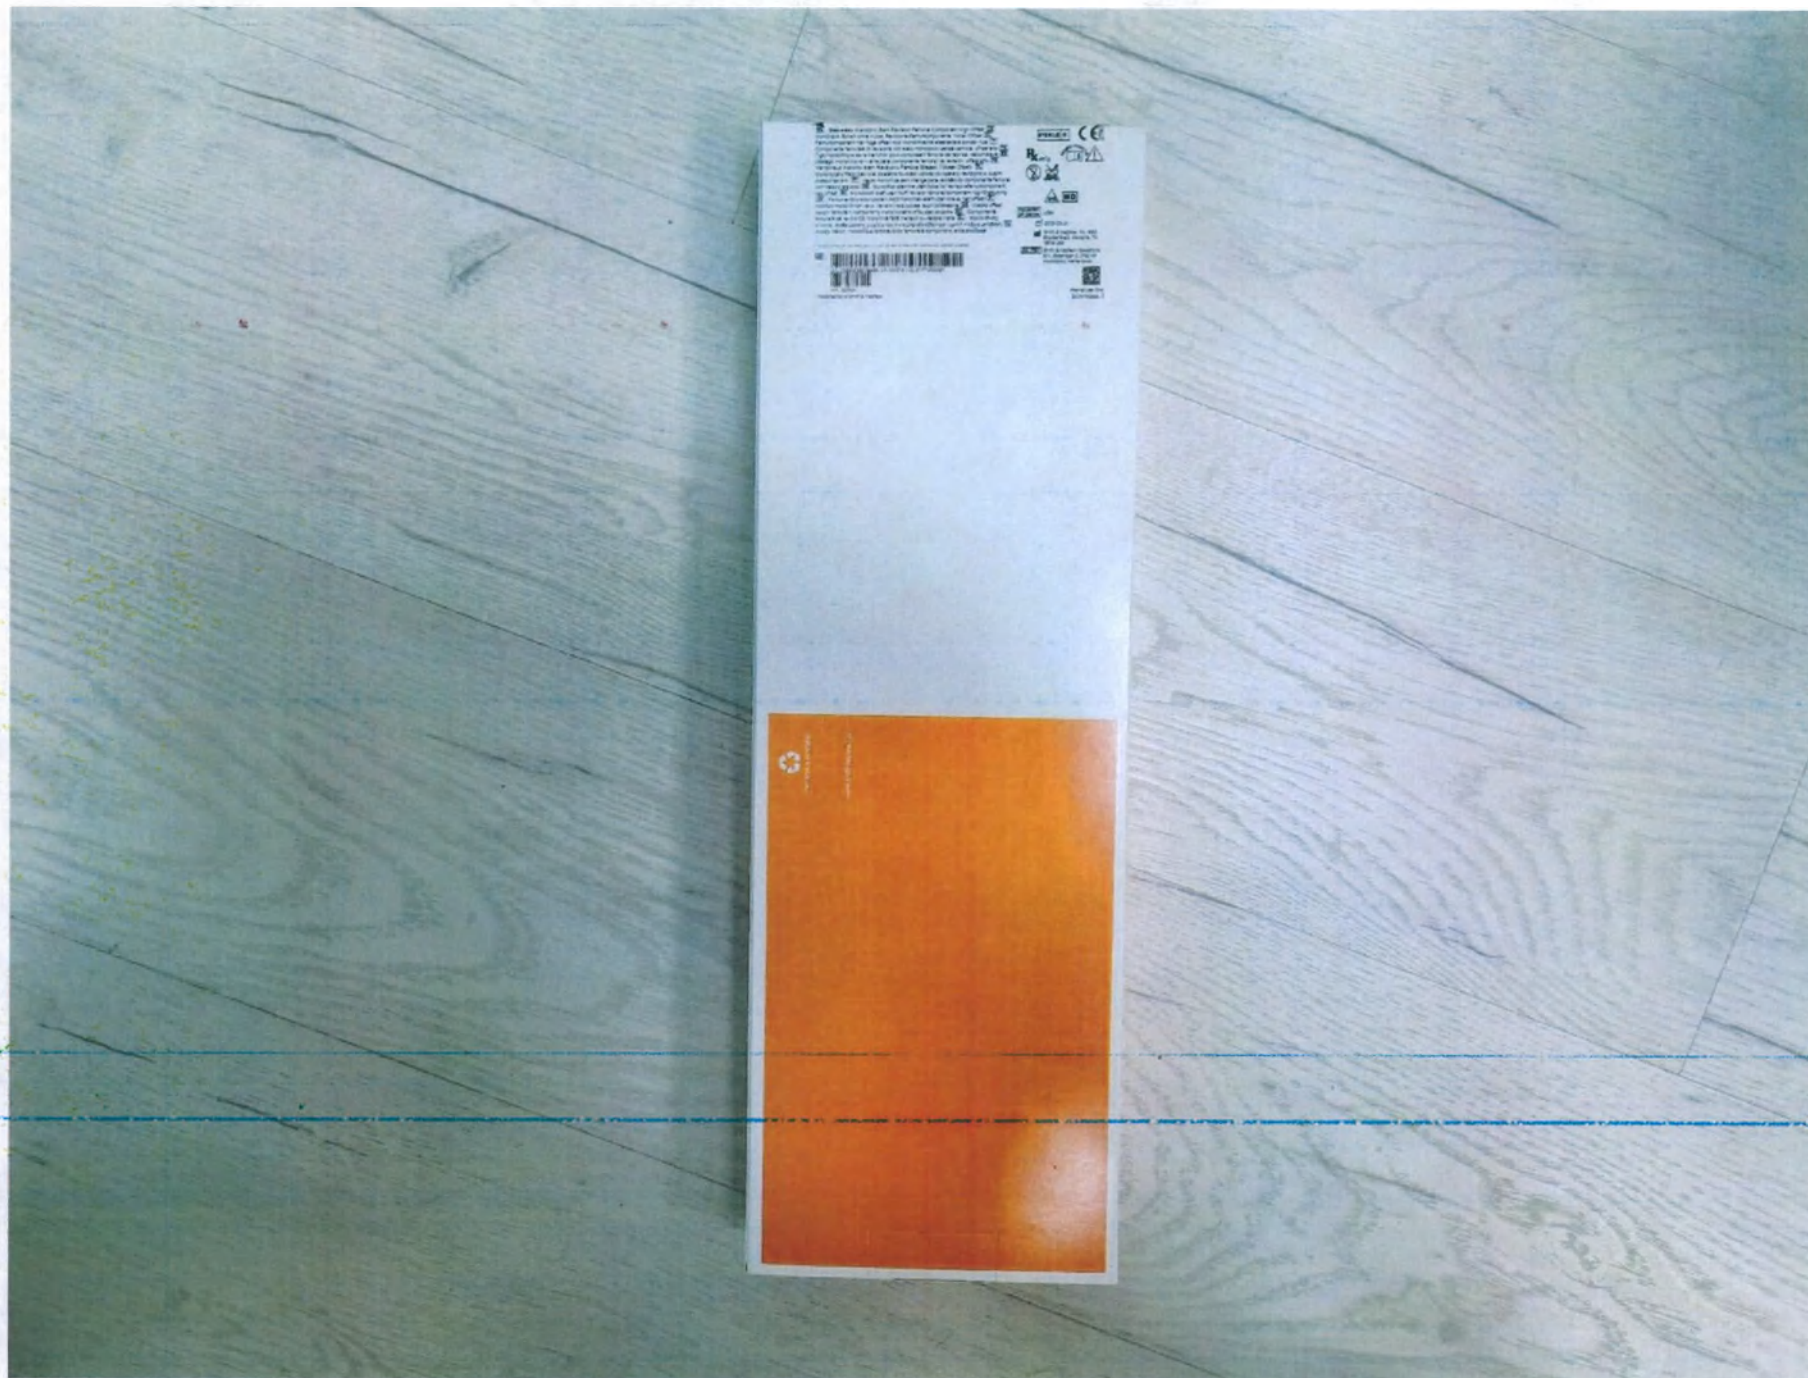

Ножка ревизионная монолитная REDAPT, стандартная, L 300 мм, размер 18

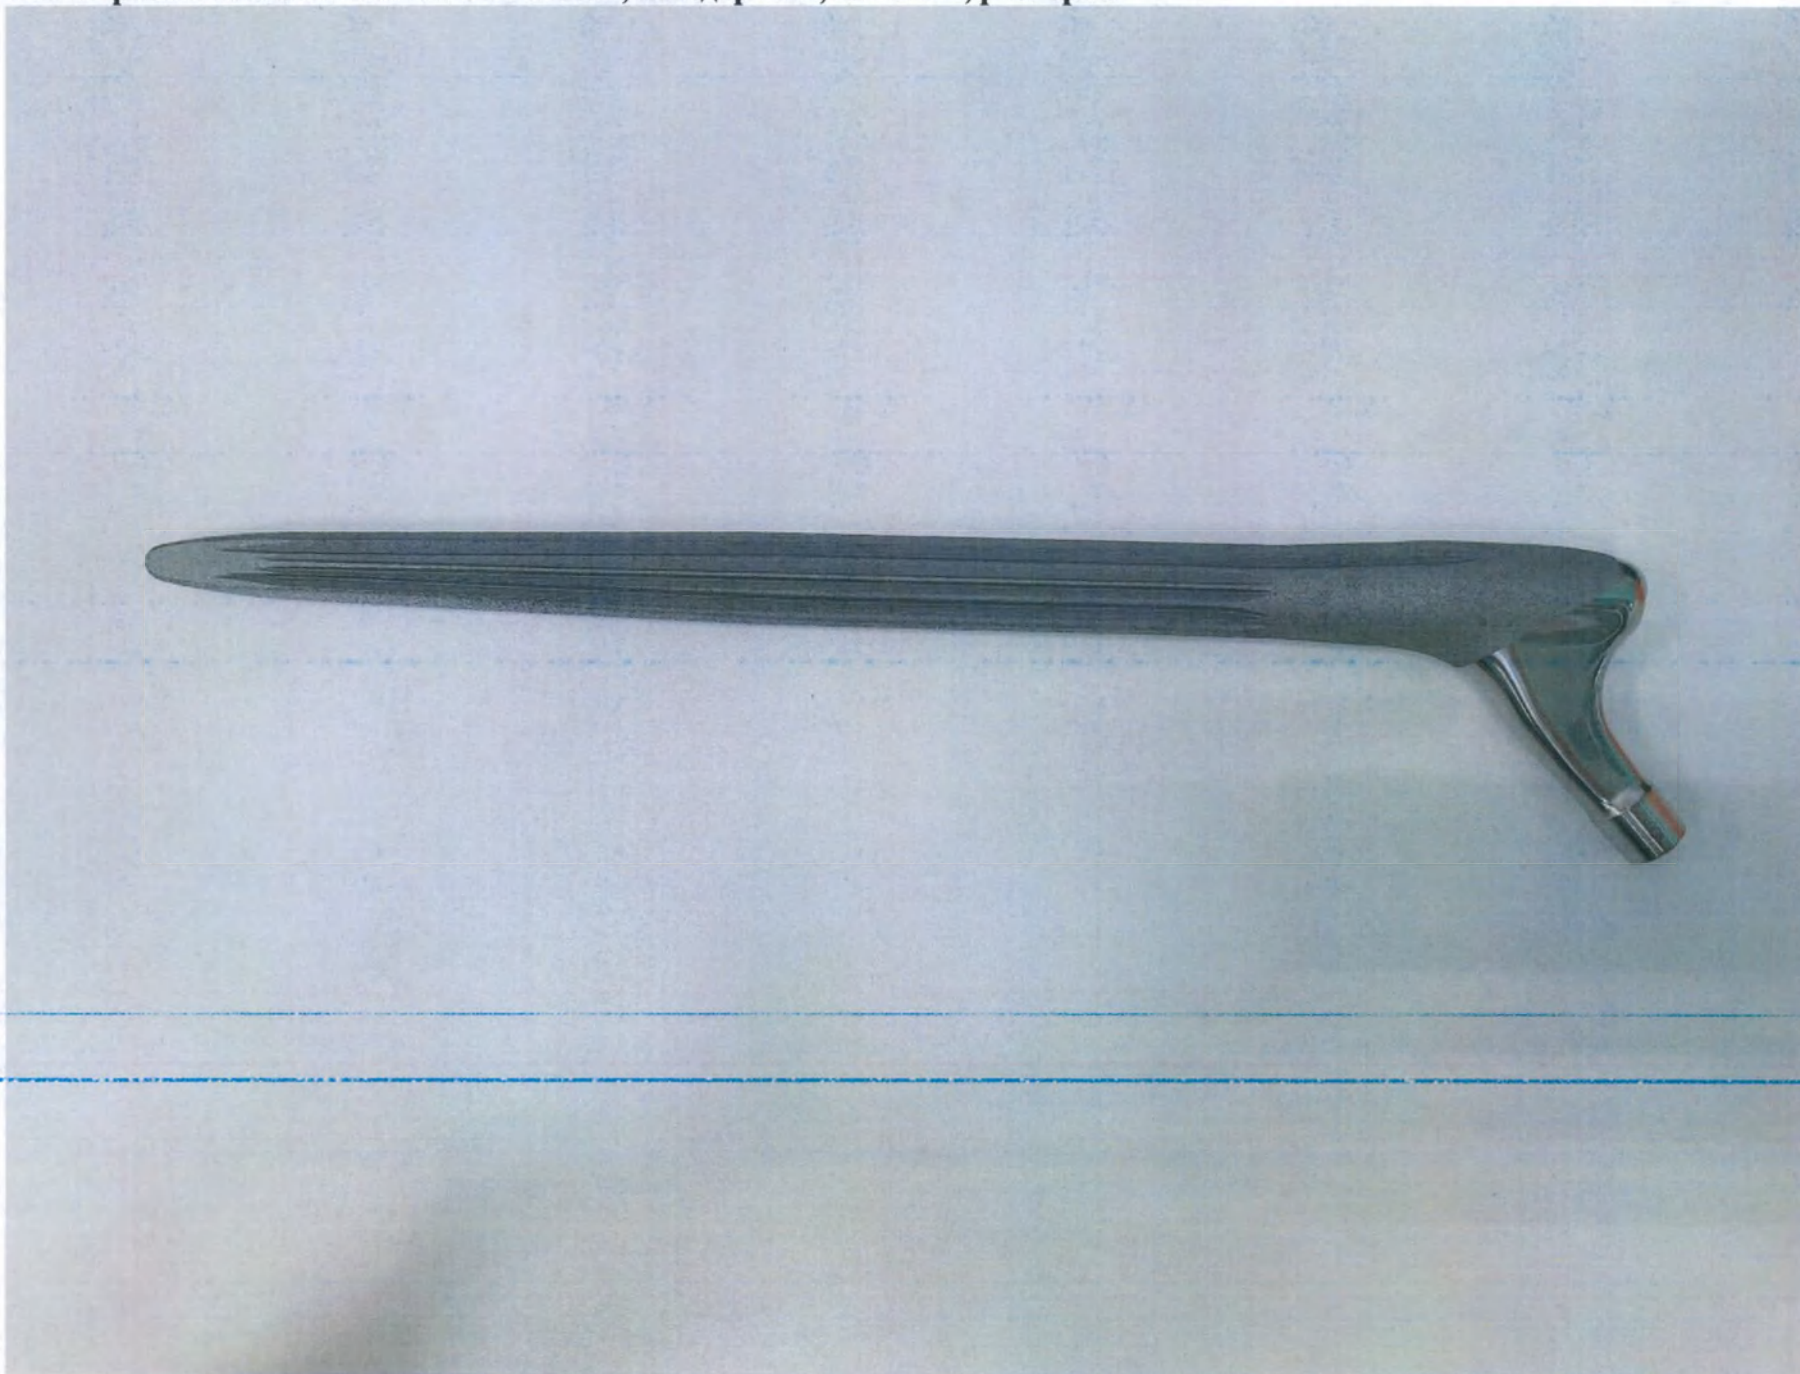

Индивидуальная упаковка: изделие во внутреннем лотке

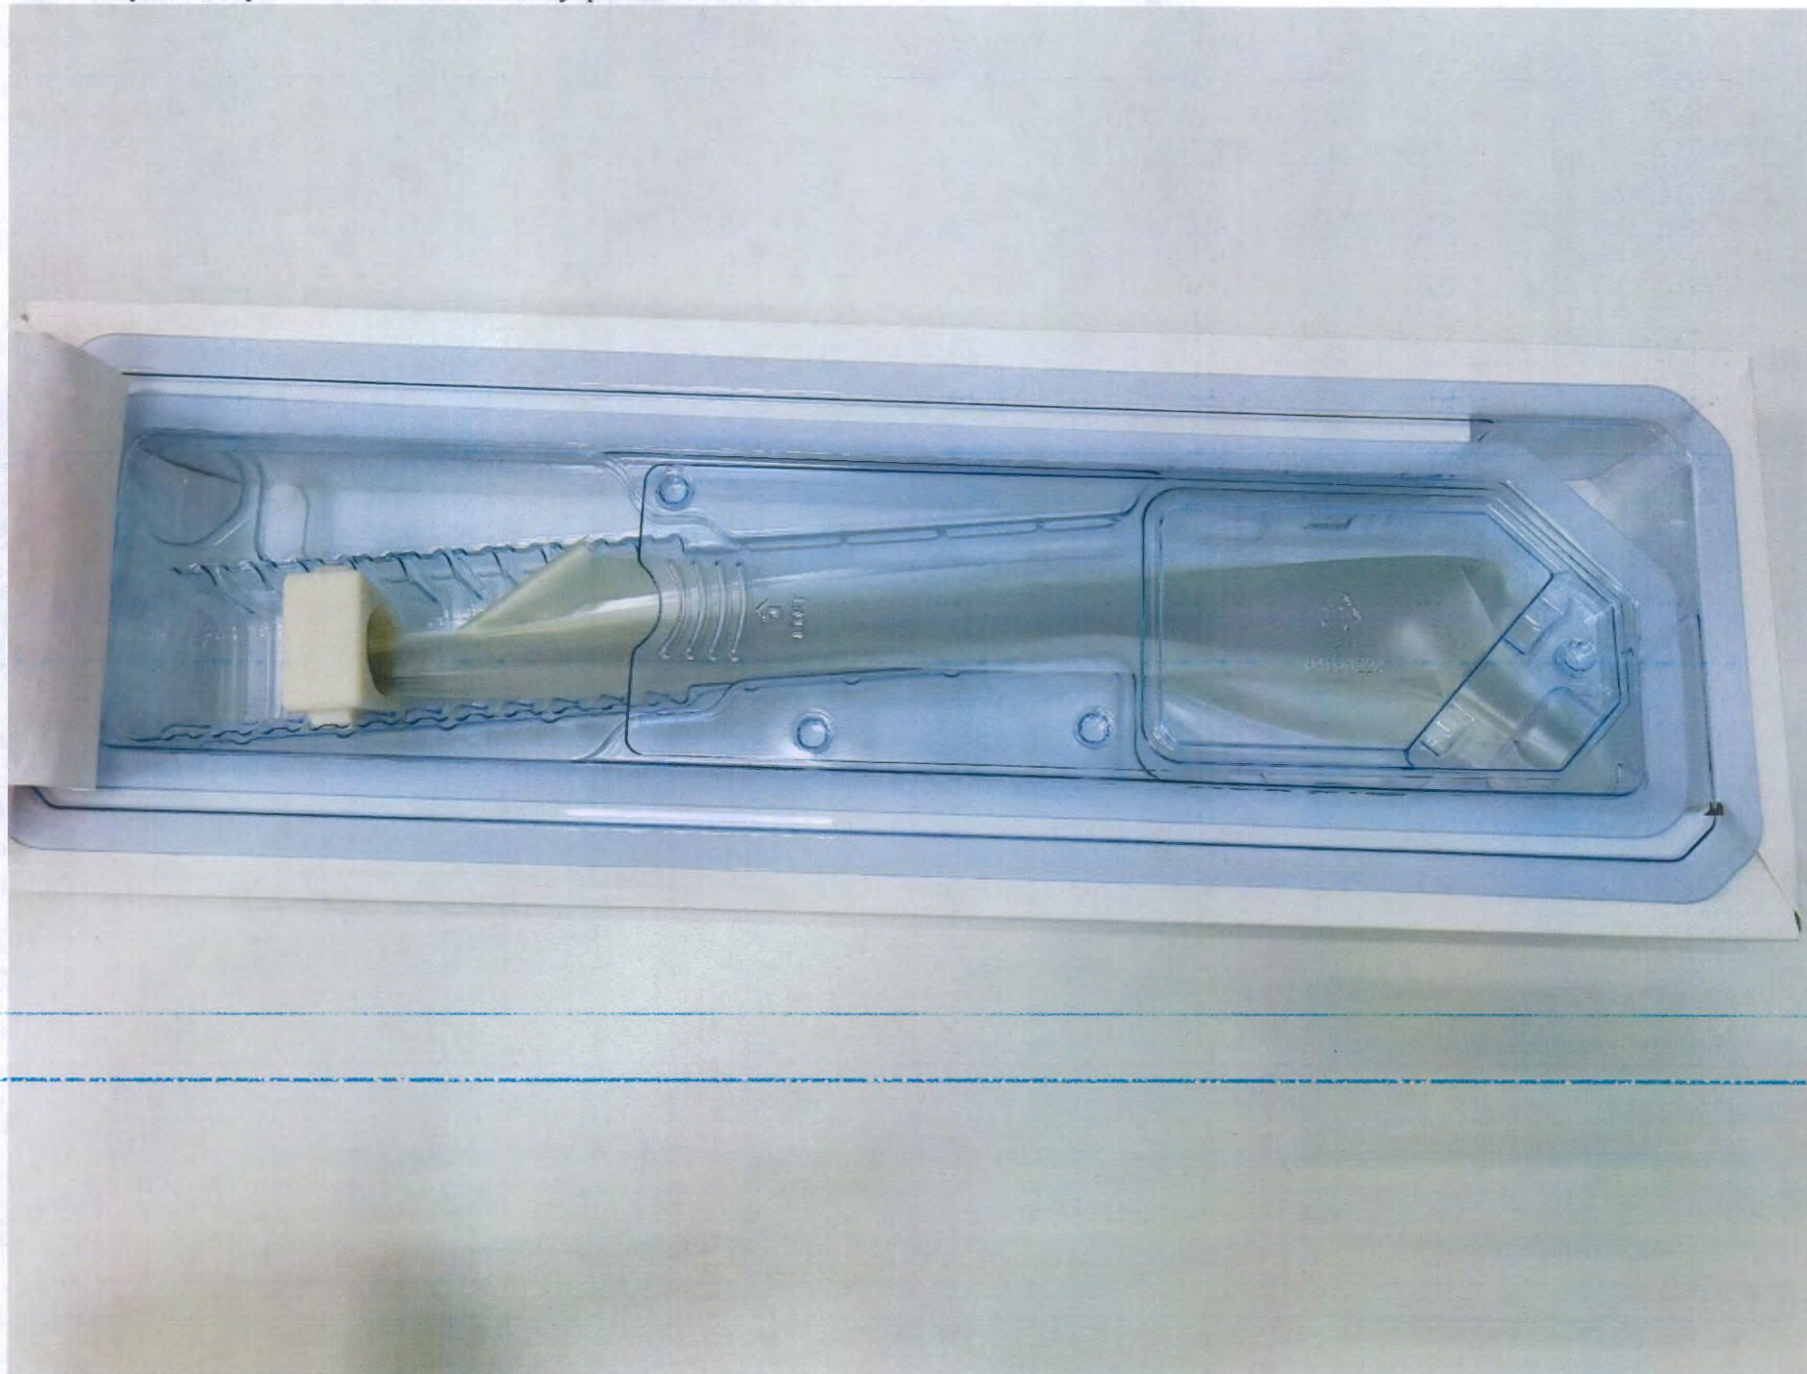

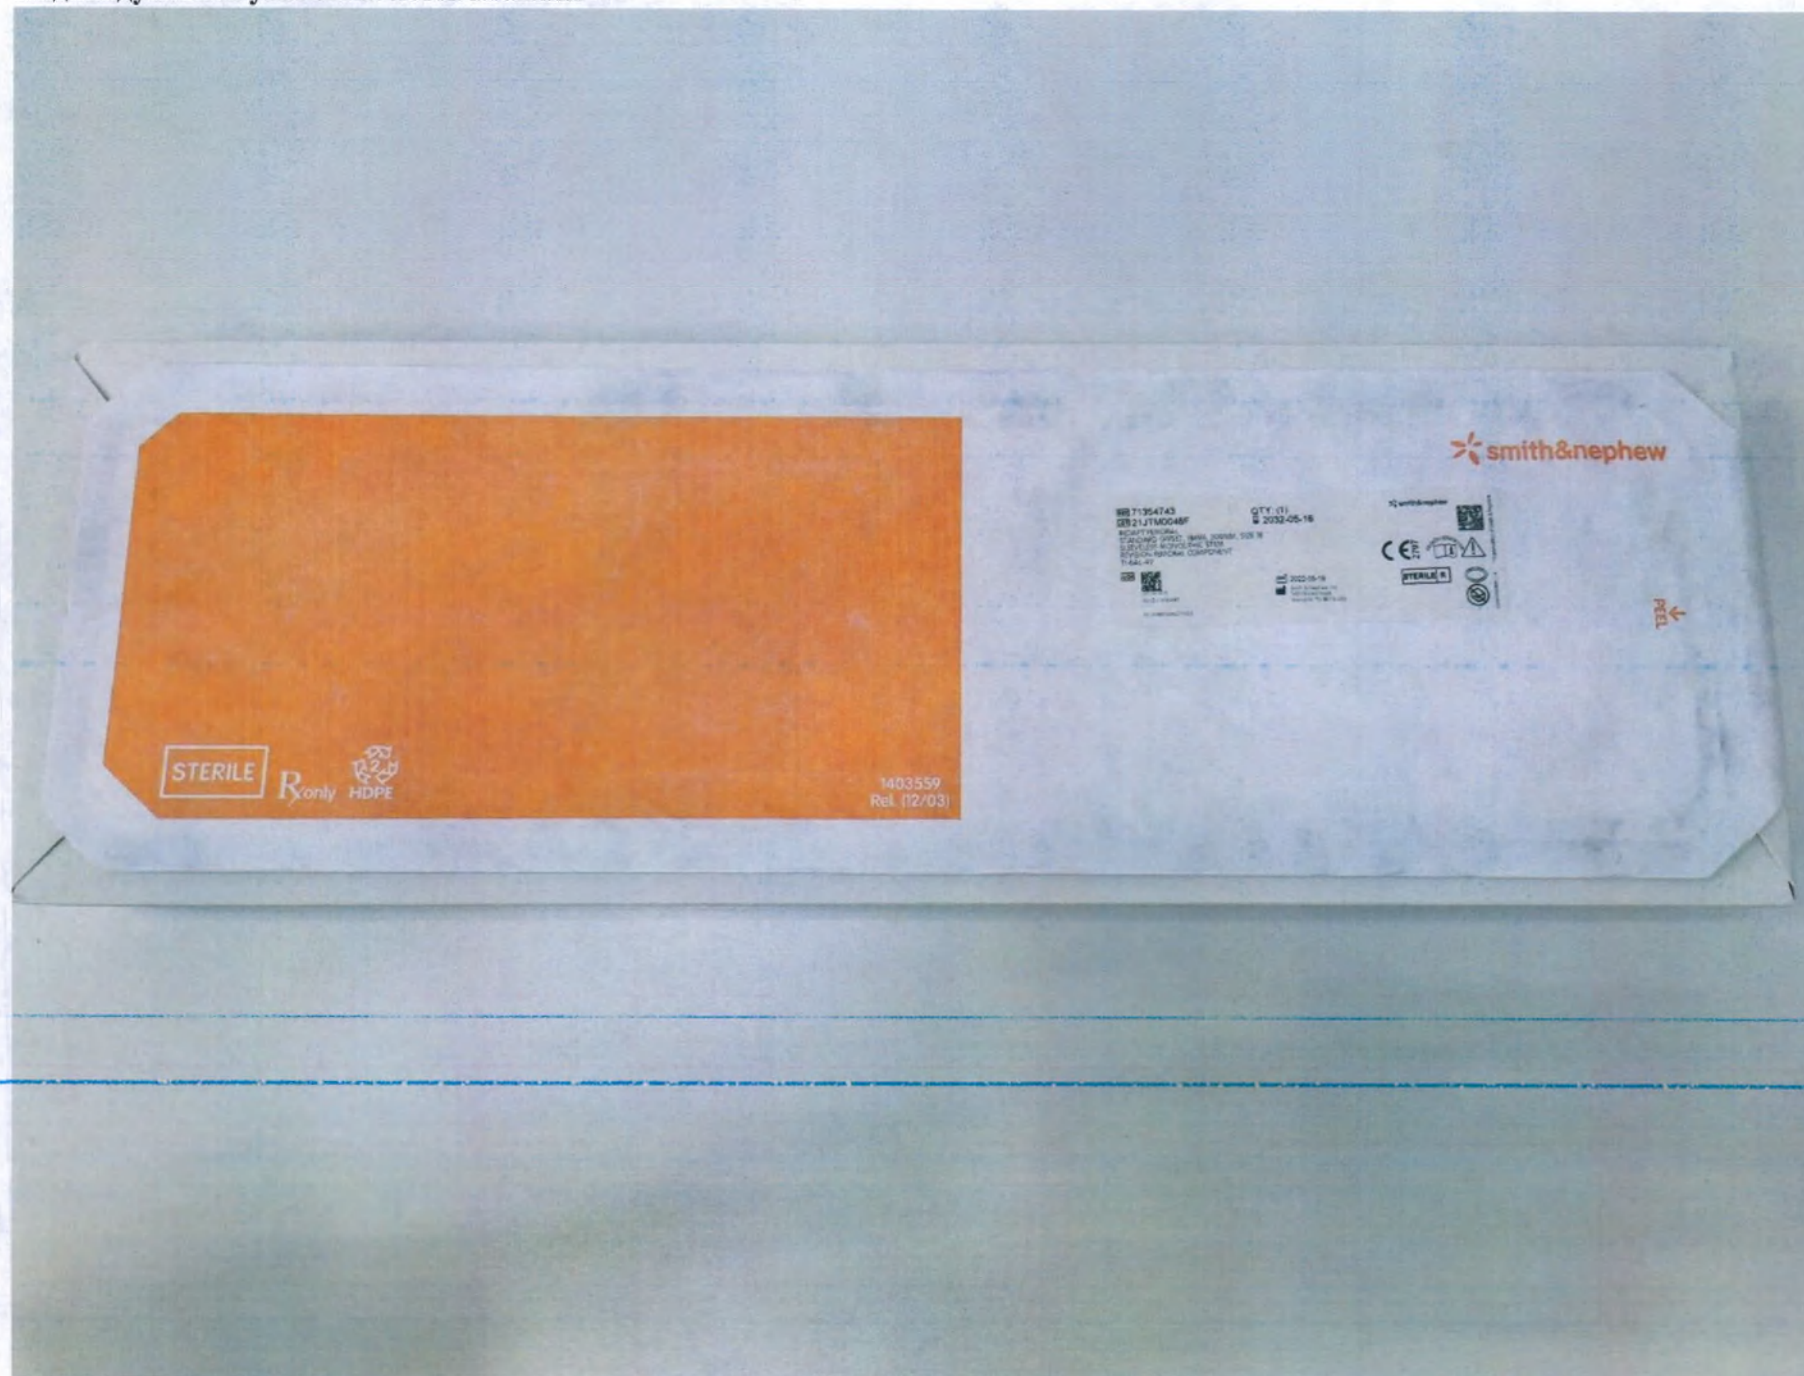


CHART LABEL

REF 71354743
LOT 21JTM0048F

STERILE R

2032-05-16

REDAPT FEMORAL
STANDARD OFFSET, 18MM, 300MM, SIZE 18
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
T-64L-4V

UDI-DI: (01)00885556579633

Smith & Nephew

www.smith-nephew.com

CHART LABEL

REF 71354743
LOT 21JTM0048F

STERILE R

2032-05-16

REDAPT FEMORAL
STANDARD OFFSET, 18MM, 300MM, SIZE 18
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
T-64L-4V

UDI-DI: (01)00885556579633

Smith & Nephew

www.smith-nephew.com

CHART LABEL

REF 71354743
LOT 21JTM0048F

STERILE R

2032-05-16

REDAPT FEMORAL
STANDARD OFFSET, 18MM, 300MM, SIZE 18
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT
T-64L-4V

UDI-DI: (01)00885556579633

Smith & Nephew

www.smith-nephew.com

Implant Card

REDAPT FEMORAL
STANDARD OFFSET, 18MM, 300MM, SIZE 18
SLEEVELESS MONOLITHIC STEM
REVISION FEMORAL COMPONENT

REF 71354743 LOT 21JTM0048F
UDI-DI: (01)00885556579633

UPD 10/12/2016 10:27:19 AM

MR 10/12/2016 10:27:19 AM

www.smith-nephew.com

Smith & Nephew

www.smith-nephew.com


EN Hip implant **DE** Hüftimplantat **NL** Heuplantaat
IT Impianto per anca **FR** Implant de hanche **ES** Implante
de cadera **TR** Kalça implantı **PL** Implant stawu biodrowego
PT Implante de anca **HU** Hofteimplantát **SV** Höftimplantát
DA Hofteimplantát **FI** Lonkkaimplanti **CS** Kůčelní
implantát **RO** Implant de sold **EL** Εμφύτευση ισχίου **HU**
Csípőimplantátum **LT** Klubo implantas **ET**
Puusaimplantaat **LV** Gūžas implants **BG** Имплант за
тазобедрена става **SL** Kolčni vsadek **HR** Implantat za kuk
SK Bedrový implantát


Smith & Nephew

www.smith-nephew.com

Smith & Nephew, Inc. 1450 Brooks Road, Memphis, TN 38198 USA



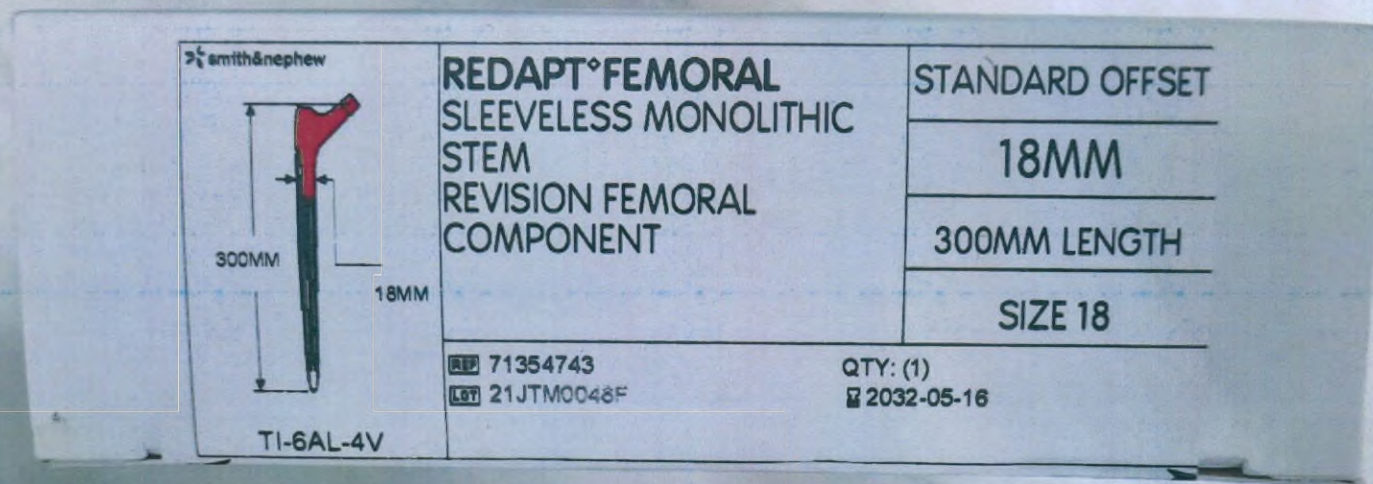


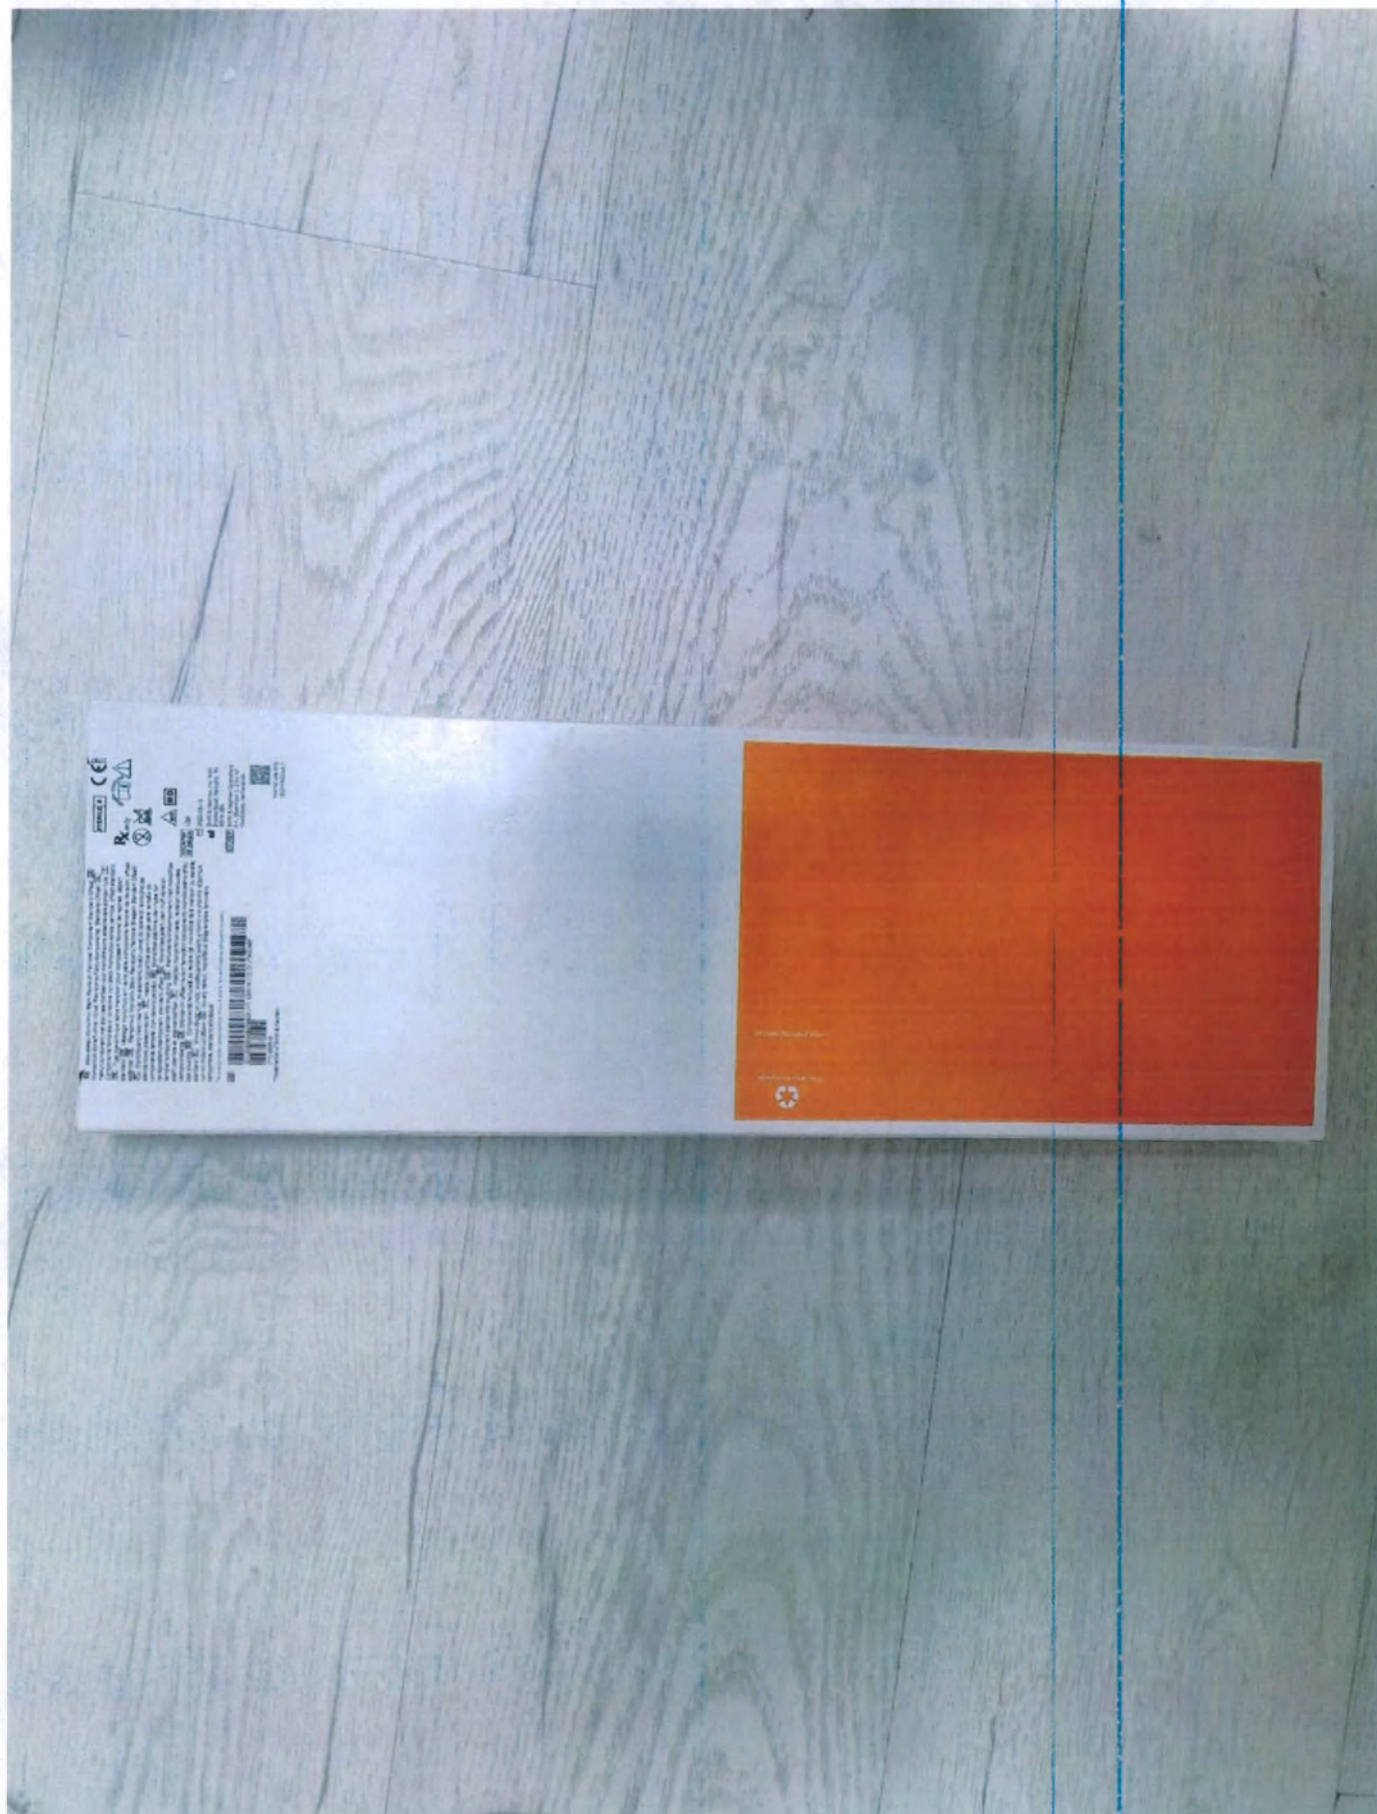

II. Чашки пористые REDAPT, на примере вариантов исполнения
Чашка пористая REDAPT, 52 мм. (для размерного ряда с 48 по 58 мм)



Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

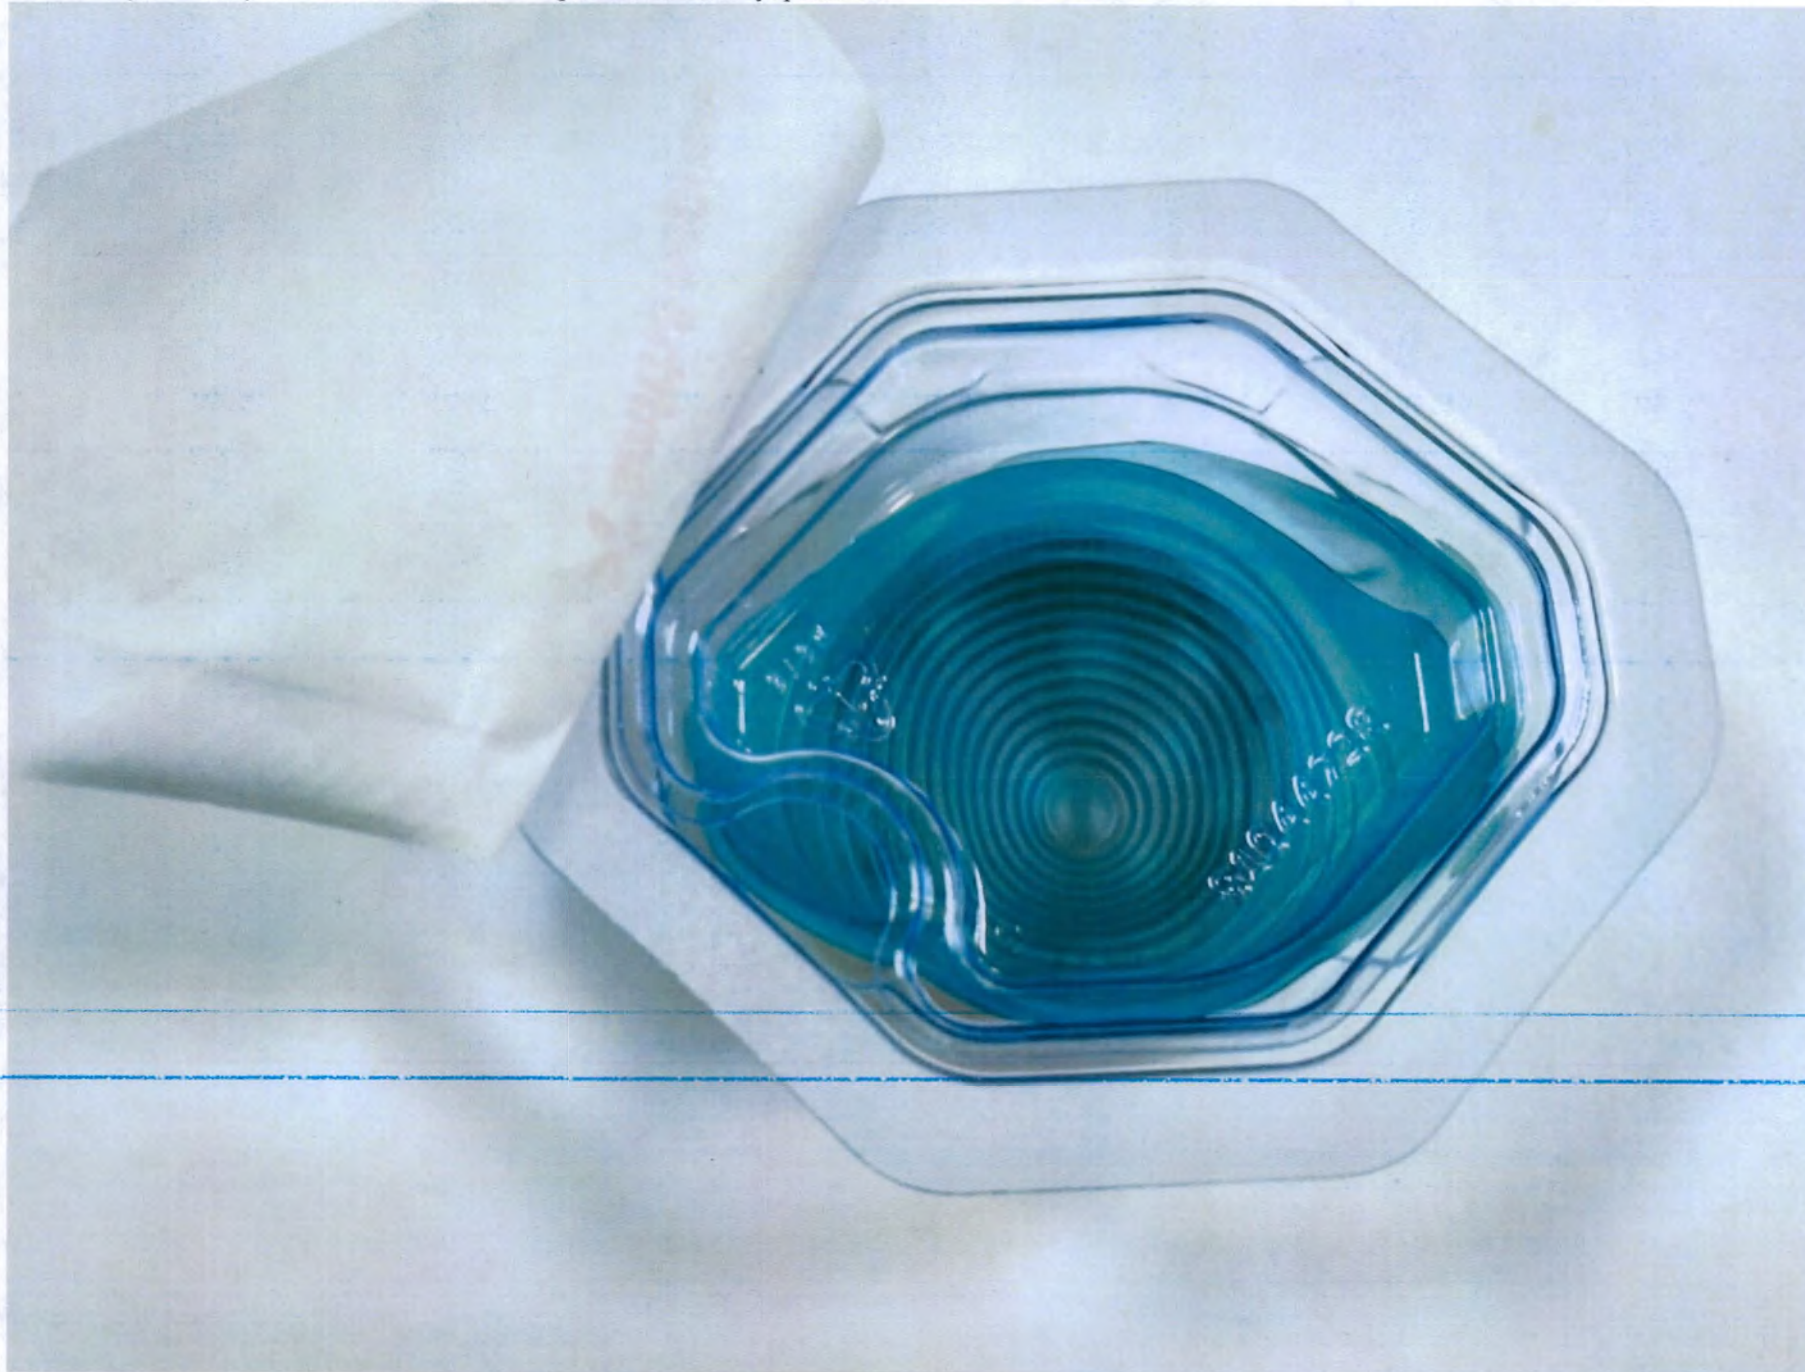

Индивидуальная упаковка: лоток внутренний.







52 MM OD
USE WITH SIZE 52 MM OD LINER
REDAPT®
FULLY POROUS SHELL
TI-6AL-4V



(01) 00885556321294 (17) 270110 (10) 17AM07941



(11) 170112

T94HSTIK; 4

ATTACH TO PATIENT'S

CHART-STIK® LABEL

71354231

LOT BATCH 17AM07941

52 MM OD
USE WITH SIZE 52 MM OD LINER
REDAPT®
FULLY POROUS SHELL
TI-6AL-4V



(01) 00885556321294 (17) 270110 (10) 17AM07941



(11) 170112

STERILE R

IRRADIATION STERILIZED

smith&nephew

EXP 2027-01-10

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

71354231

LOT BATCH 17AM07941

52 MM OD
USE WITH SIZE 52 MM OD LINER
REDAPT®
FULLY POROUS SHELL
TI-6AL-4V



(01) 00885556321294 (17) 270110 (10) 17AM07941



(11) 170112

STERILE R

IRRADIATION STERILIZED

smith&nephew

EXP 2027-01-10

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

71354231

LOT BATCH 17AM07941

52 MM OD
USE WITH SIZE 52 MM OD LINER
REDAPT®
FULLY POROUS SHELL
TI-6AL-4V



(01) 00885556321294 (17) 270110 (10) 17AM07941



(11) 170112

STERILE R

IRRADIATION STERILIZED


smith&nephew

EXP 2027-01-10

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD



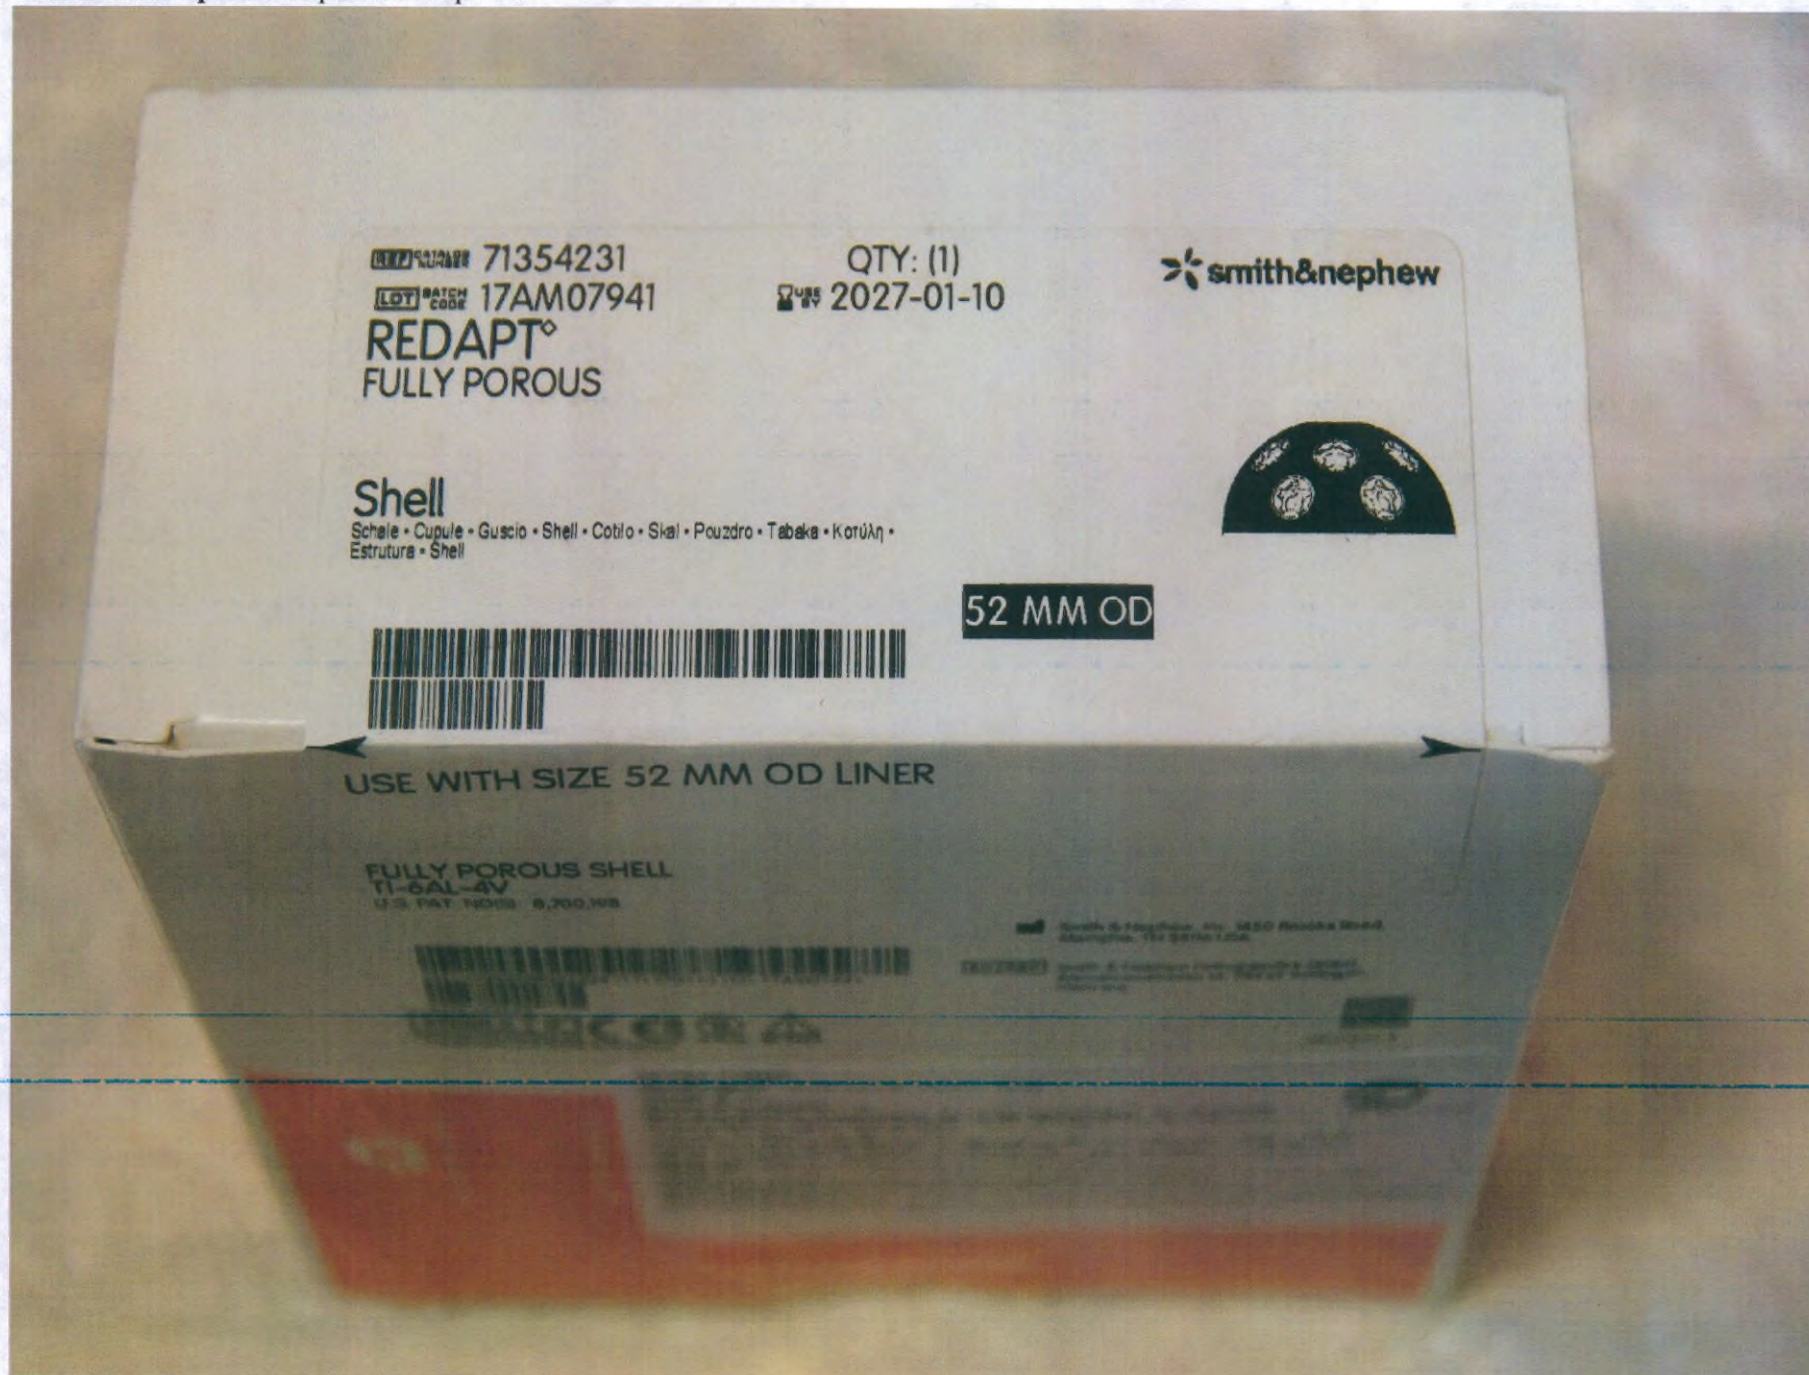

USE WITH SIZE 52 MM OD LINER

FULLY POROUS SHELL
TI-6AL-4V
U.S. PAT. NO(S): 8,700,198

Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA



(01) 00865556321294 (17) 270110 (10) 17AM07941




(11) 170112

STERILE R

IRRADIATION STERILIZED

*Trademark(s) of Smith & Nephew.



EC REP

Smith & Nephew Orthopaedics GmbH,
Alemannenstrasse 14, 78532 Tuttlingen,
Germany



T49H18AT; 2

Артикул: 71364231

Наименование: Чашка пористая REDAPT, 52 мм

Размер: 52 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: «Смит энд Непью Инк» (Smith & Nephew, Inc.), 1450 Brooks Road,
Memphis, Tennessee (TN), 38116, USA

Уполномоченный представитель на территории РФ: ООО «Смит энд Непью», 105120, Россия, г.
Москва, 2-й Сыромятнический пер., д. 1, 9 этаж, пом. 1, ком. 1 тел./факс: +7 495 755 55 03

Метод стерилизации: Радиационная стерилизация Стерильно Апиогенно Натоксично

Номер РУ:

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: в сухом, защищенном от света месте, при температуре от -20°C до +35°C

Меры предосторожности:


Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/usa/ru/>




This carton is recyclable.

www.smith-nephew.com

Чашка пористая REDAPT, 80 мм (для размерного ряда с 60 по 80 мм)

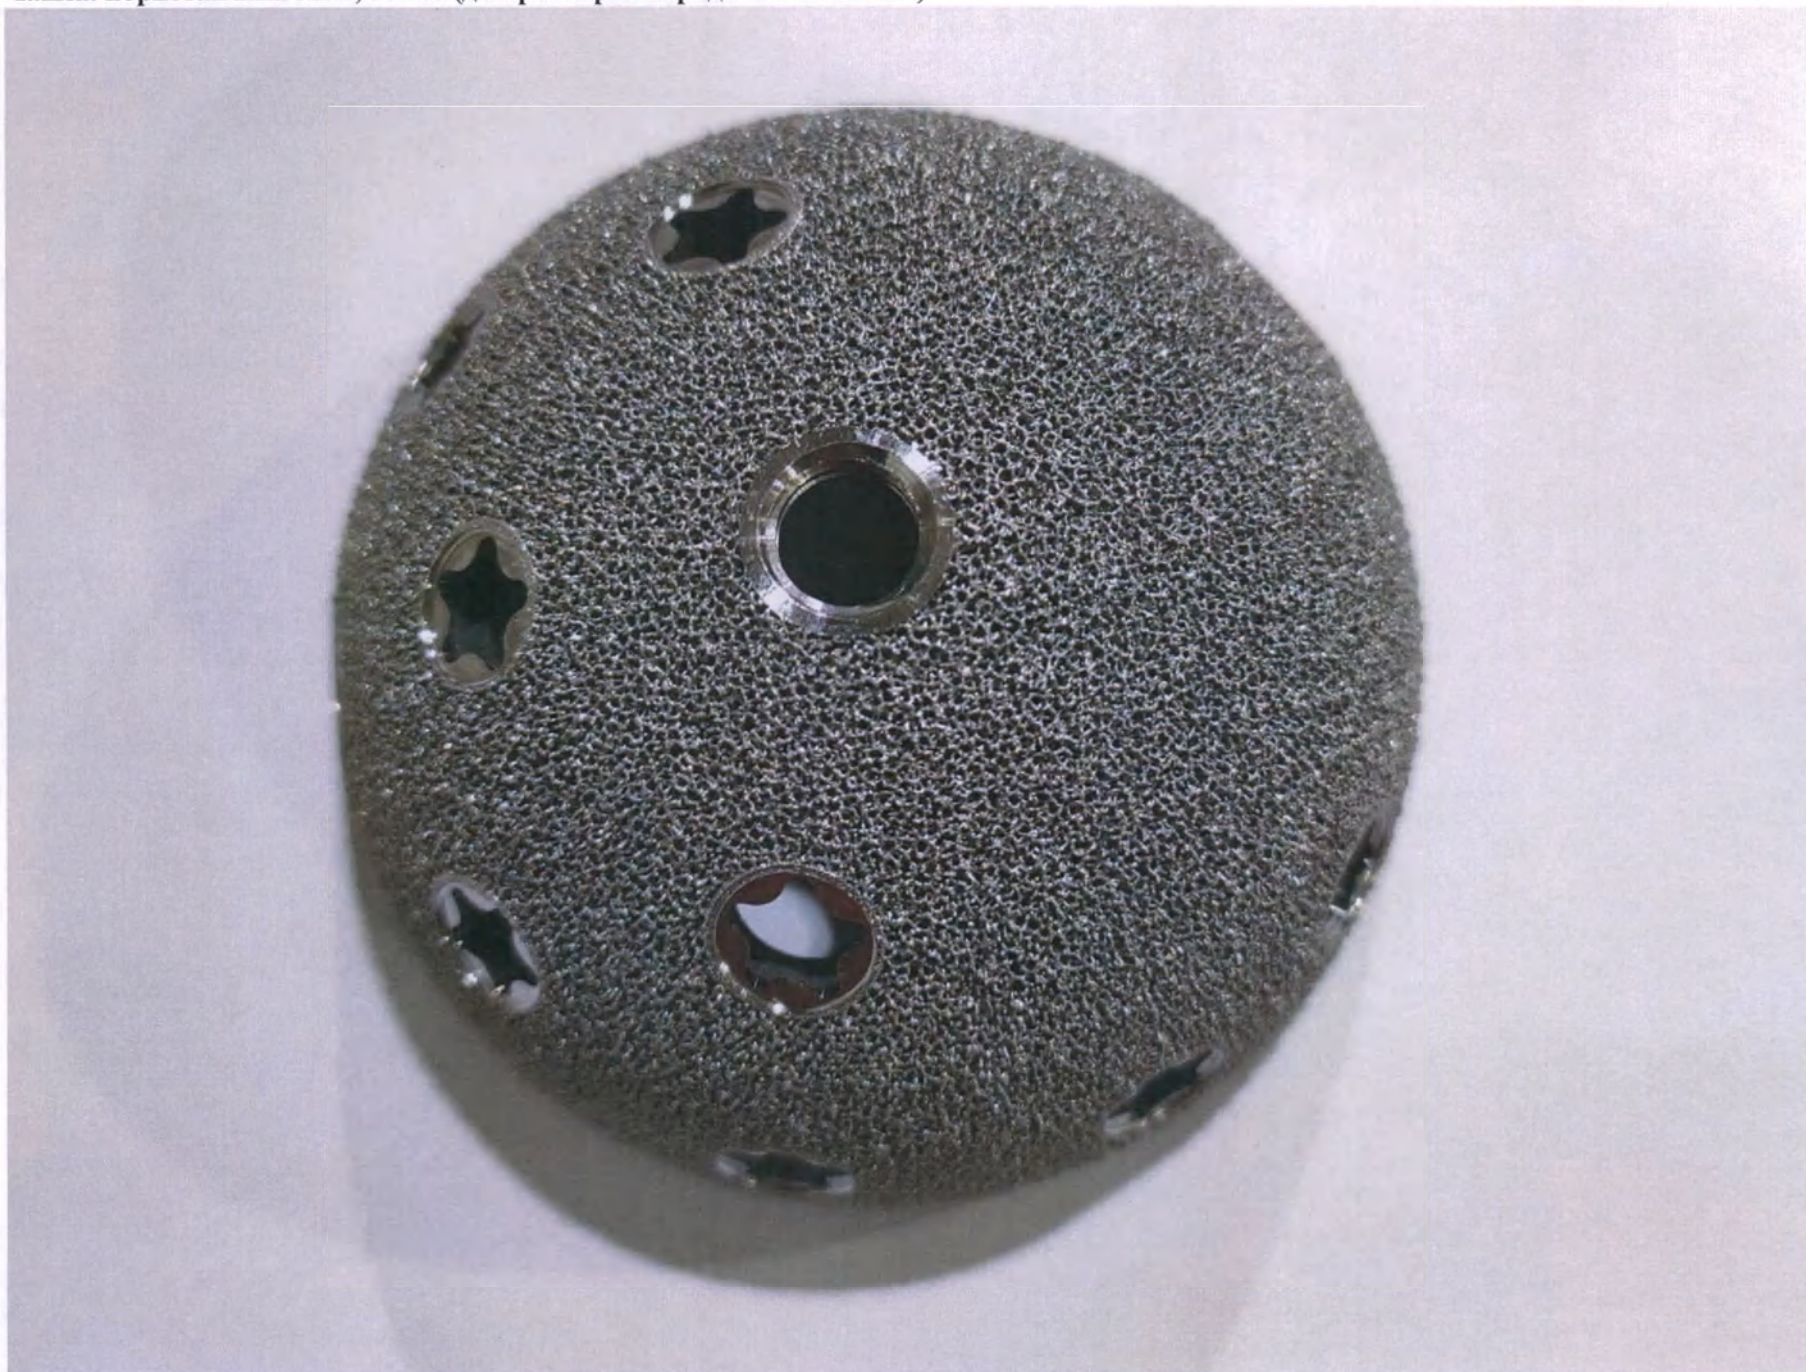

Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

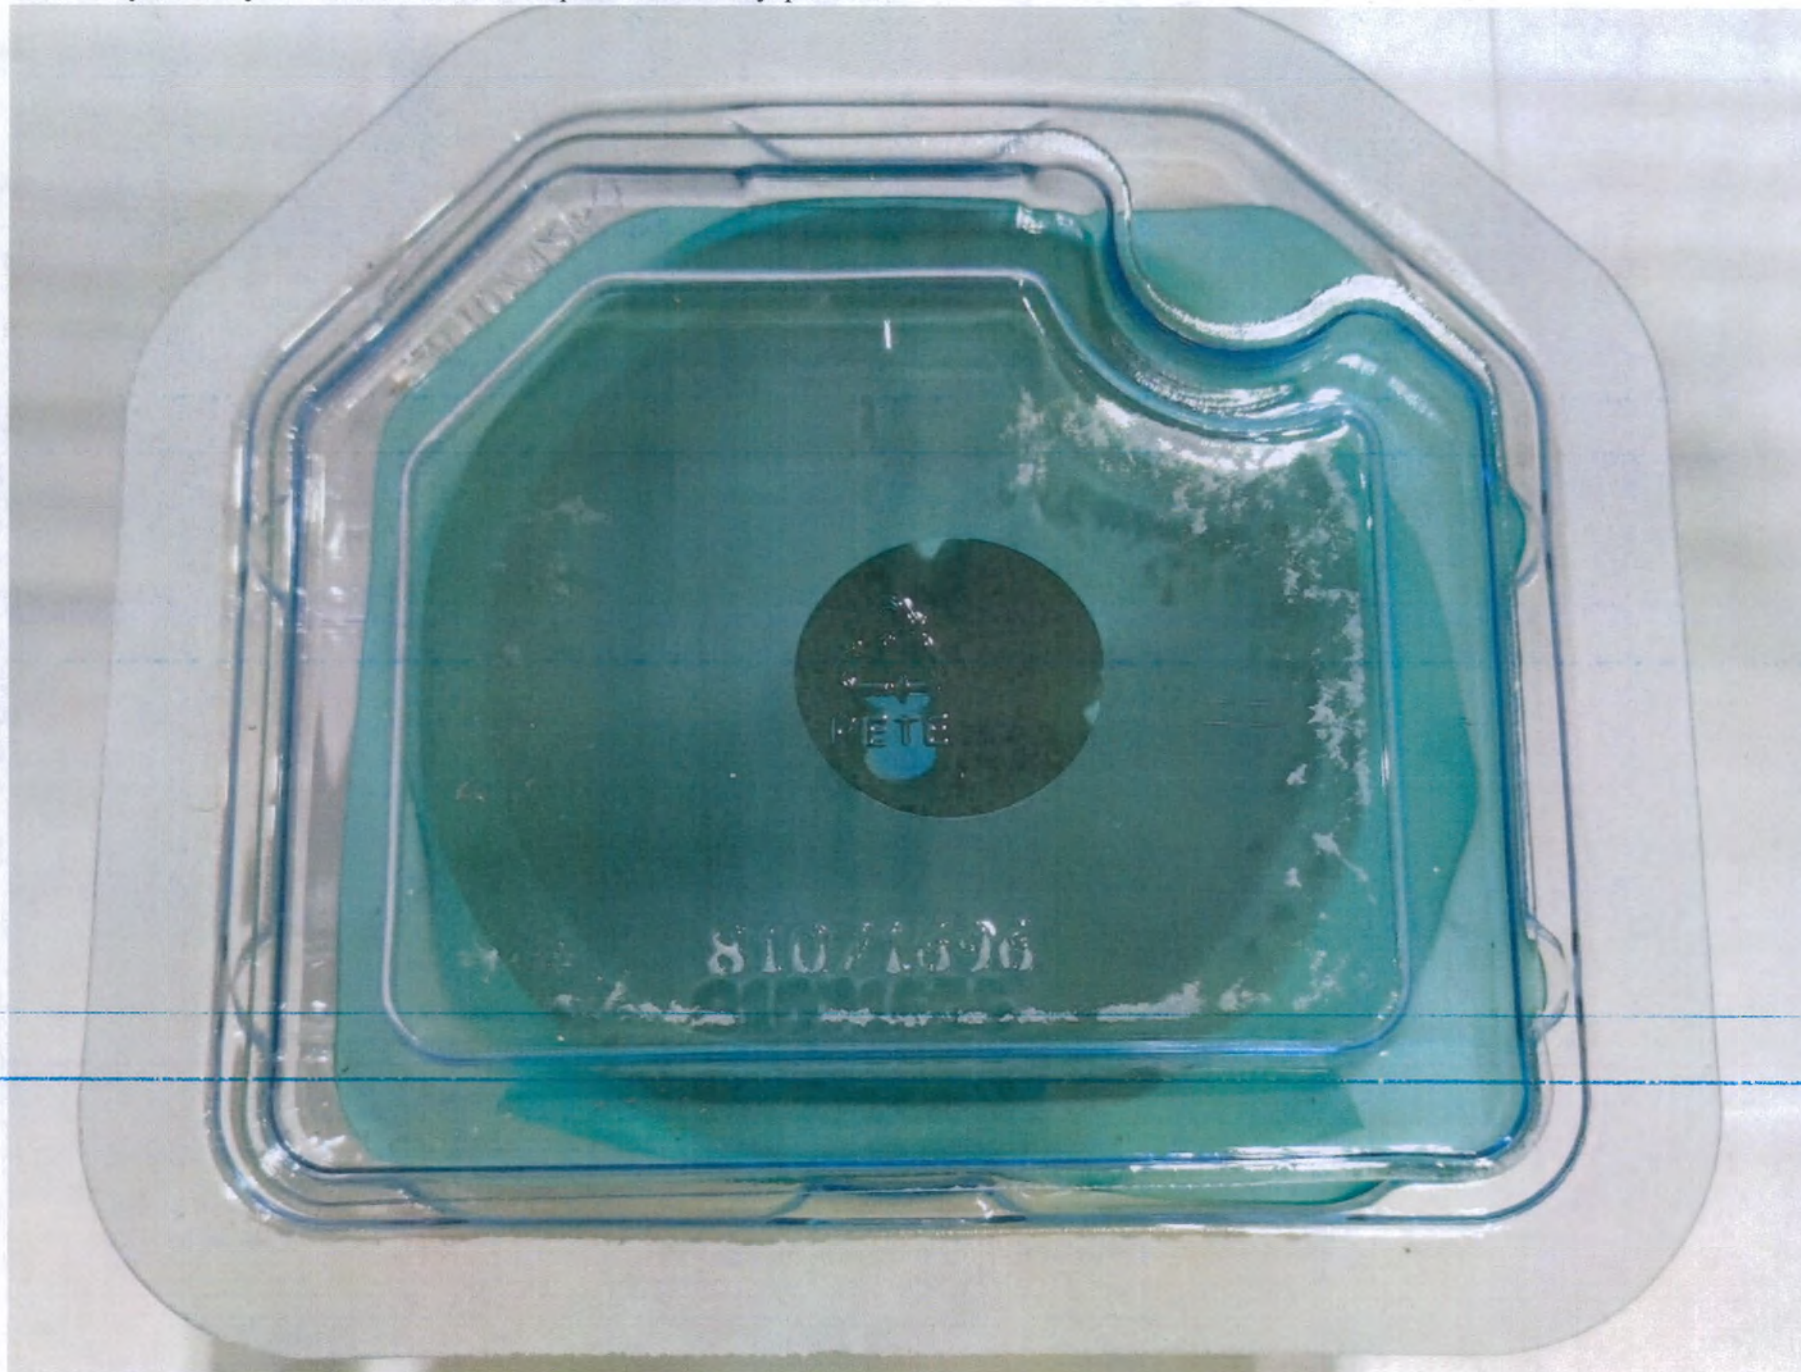

Индивидуальная упаковка: лоток внутренний.







(11) 170919 T94HSTIK, 4 AT

CHART-STIK® LABEL

REF NUMBER 71354246

LOT BATCH CODE 17JM13406

80 MM OD
USE WITH SIZE 80 MM OD LINER
REDAPT®
FULLY POROUS SHELL
TI-6AL-4V

STERILE R **EXP** 2027-09-17
IRRADIATION STERILIZED

smith&nephew

(01) 00885556321997 (17) 270917 (10) 17JM13406

(11) 170919 T94HSTIK, 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF NUMBER 71354246

LOT BATCH CODE 17JM13406

80 MM OD
USE WITH SIZE 80 MM OD LINER
REDAPT®
FULLY POROUS SHELL
TI-6AL-4V

STERILE R **EXP** 2027-09-17
IRRADIATION STERILIZED

smith&nephew

(01) 00885556321997 (17) 270917 (10) 17JM13406

(11) 170919 T94HSTIK, 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF NUMBER 71354246

LOT BATCH CODE 17JM13406

80 MM OD
USE WITH SIZE 80 MM OD LINER
REDAPT®
FULLY POROUS SHELL
TI-6AL-4V


STERILE R **EXP** 2027-09-17
IRRADIATION STERILIZED

smith&nephew

(01) 00885556321997 (17) 270917 (10) 17JM13406

(11) 170919 T94HSTIK, 4

ATTACH TO PATIENT'S RECORD

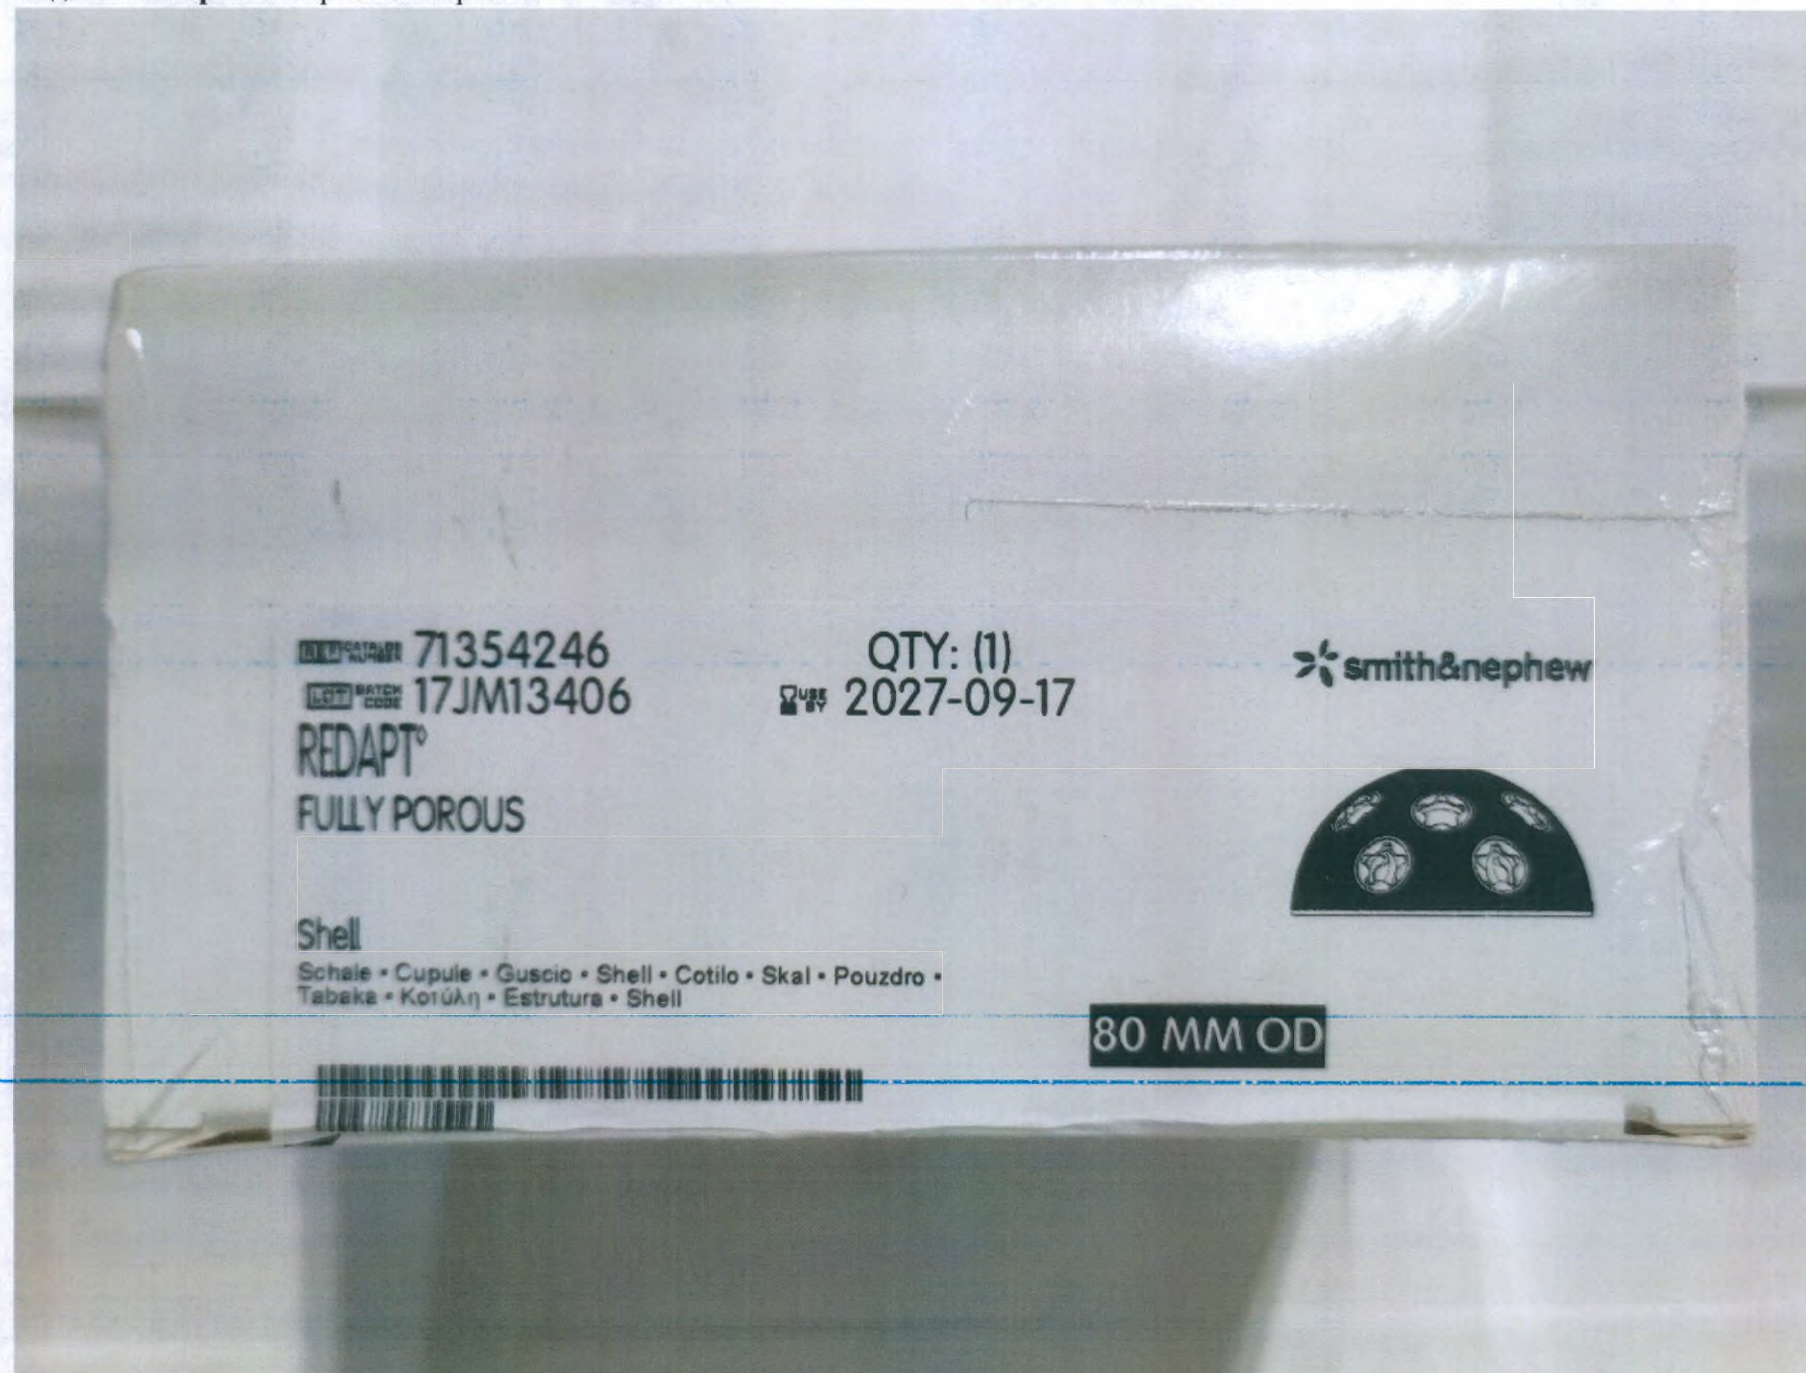

USE WITH SIZE 80 MM OD LINER


FULLY POROUS SHELL
TI-6AL-4V
U.S. PAT. NOISI: 8,700,198

Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA

EGIMED
Smith & Nephew Orthopaedics GmbH,
Altenmünstersweg 14, 79532 Tuttlingen,
Germany



(11) 170919



TZSH18AK.4



This carton is recyclable

Артикул: 7136424E
Наименование: Компонент радионуклеонного протеза тазобедренного сустава REDART чашка пористая
REDART, 80 мм
Размер: 80 мм
Кольцо ш. в упаковке: 1 шт
Дата изготовления, использовать до: номер партии/серии. См на упаковке
Наименование и адрес изготовителя: Смит энд Непью, Инк. США Smith & Nephew, Inc. 1450,
Brooks Road, Memphis, Tennessee 38116, USA
Исполнительный представитель на территории РФ: ООО "Смит энд Непью" 105120, Россия
Восста, 2-й Сыромятнинский пер., д. 1, этаж 9, пом. 1, комн.
Место стерилизации: Радиационная стерилизация
Номер Рз: РЗН 20209750 от 16.06.2022
Назначение, способ применения, противопоказания: См инструкцию
Условия хранения: при температуре от -20 - 35°С, влажности от 40 - 90%, атмосферном давлении от
366 - 1067 гПа
Марка радиостерилизации:
Инструкция по применению: [http://www.smith-nephew.com/about-us/members-orthopaedics/usa/ru/](http://www.smith-nephew.com/about-us/members-orthopaedics/usa/ru)

**III. Вкладыши цементируемые REDAPT, на примере вариантов исполнения:
Вкладыш цементируемый REDAPT, XLPE, 0°, 36/54 мм.**







CHART-STIK® LABEL

71354522
16HM10839

0"
36MM X 54MM
REDAPT®
CEMENTED LINER
XLPE

STERILE EO 2026-08-14



(01) 00885556413197 (17) 260814 (10) 16HM10839

(11) 160816

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

71354522
16HM10839

0"
36MM X 54MM
REDAPT®
CEMENTED LINER
XLPE

STERILE EO 2026-08-14



(01) 00885556413197 (17) 260814 (10) 16HM10839

(11) 160816

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

71354522
16HM10839

0"
36MM X 54MM
REDAPT®
CEMENTED LINER
XLPE

STERILE EO 2026-08-14



(01) 00885556413197 (17) 260814 (10) 16HM10839

(11) 160816

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

71354522
16HM10839

0"
36MM X 54MM
REDAPT®
CEMENTED LINER
XLPE

STERILE EO 2026-08-14



(01) 00885556413197 (17) 260814 (10) 16HM10839

(11) 160816

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

71354522
16HM10839

0"
36MM X 54MM
REDAPT®
CEMENTED LINER
XLPE

STERILE EO 2026-08-14



(01) 00885556413197 (17) 260814 (10) 16HM10839

(11) 160816

T94HSTK 4


ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

71354522
16HM10839

0"
36MM X 54MM
REDAPT®
CEMENTED LINER
XLPE

STERILE EO 2026-08-14



(01) 00885556413197 (17) 260814 (10) 16HM10839

(11) 160816

T94HSTK 4

ATTACH TO PATIENT'S RECORD

Instructions for Use

English

Gebrauchsanweisung

Total Hip Systems

CAUTION: Federal law (21CFR) restricts the subject total hip arthroplasty devices to sale by or on the order of a physician.

Device Descriptions

Total Hip Systems

The Total Hip Systems consist of femoral components, modular necks, proximal sleeves, taper sleeves, acetabular components, fixation screws and pegs, hole covers, cementizers, and femoral heads. Components may be grit blasted, porous coated, hydroxyapatite (HA) coated, or HA porous coated. All implantable devices are for single use only.

Materials

Femoral components are manufactured from cobalt chromium alloy, titanium alloy, or stainless steel (SS). Femoral heads are manufactured from cobalt chromium alloy (COXNUM), oxidized zirconium, BIOLOX forte alumina ceramic, BIOLOX delta alumina/zirconia ceramic, zirconia ceramic, or stainless steel. Acetabular liners are manufactured from ultra-high-molecular weight polyethylene (UHMWPE), BIOLOX forte alumina ceramic, or BIOLOX delta alumina/zirconia ceramic. In the U.S., refer to the separate package insert provided with the ceramic acetabular liners. All poly acetabular components are manufactured from UHMWPE. Acetabular shells are manufactured from titanium (Ti-6Al-4V alloy) or cobalt chromium (CoCr) alloy. BIRMINGHAM HIP acetabular cups are cobalt chromium (CoCr) alloy. The component material is provided on the outside canon label. **NOTE:** BIOLOX delta ceramic liners are not available for use in the U.S.

Some of the alloys needed to produce orthopedic implants contain metallic components that may be carcinogenic in tissue cultures or in an intact organism under very unique circumstances. Questions have been raised in the scientific literature as to whether or not these alloys may be carcinogenic in implant recipients. Studies conducted to evaluate this issue have not identified conclusive evidence of such phenomenon, in spite of the millions of implants in use.

Femoral Components

Femoral components are available in a variety of sizes. Porous coated components are coated for biological growth and are intended for use without cement. Modular femoral components are available with an oval taper to accept Smith & Nephew CoCr modular necks and/or a Morse taper to accept proximal sleeves. Non porous femoral components can feature polyethylene/methacrylate (PMMA) cementation that help produce a uniform cement thickness.

Femoral components, available with 10/12, 12/14, and 14/16 tapers, mate and lock directly with Smith & Nephew femoral heads having the same size taper. Certain femoral heads may require taper sleeves for attachment to the femoral stem taper. Refer to the table in the taper sleeves section for details.

Taper Sleeves

A taper sleeve may be required when mating femoral stems with specific types of femoral heads. Refer to the sleeve compatibility table for the appropriate combinations. Failure to utilize the proper sleeve in head combination may lead to implant failure and may result in revision surgery. Never place more than one taper sleeve on a femoral component; this combination will increase stresses on the implant and may lead to failure and may result in revision surgery.

Modular Neck

Modular necks are made from CoCr alloy and are available in a variety of configurations. The modular neck mates and locks with the oval taper of a modular femoral component on one end and the taper of a 12/14 femoral head on the other end.

Compatible Sleeve Combinations

Femoral Stem Taper	40, 44 mm Modular COXNUM Heads	40, 44 mm Modular COCr Heads	BH Modular CoCr Heads*	TANDEM* CoCr & COXNUM Unipolar Heads	14/16 COXNUM and CoCr Heads
12/14	A	A	B	C	-
14/16	-	-	-	D	-
10/12	-	-	-	E	F

* Modular CoCr heads are made from CoCr alloy and are intended for hemiarthroplasty use in the U.S. Refer to the separate package insert provided with the components.

** BH Modular heads are not available for use in the U.S. These heads can only be used with cemented and CoCr femoral stems.

Sleeve	Material	Description/Part Numbers
A	Ti-6Al-4V	12/14 Modular Sleeve +A: 7034241; +B: 7034242; +C: 70344248; +D: 70344230
B	CoCr	CoCr 12/14 Modular Sleeve +B: 70222700; +D: 70222700; +E: 70222700; +F: 70222490
C	Ti-6Al-4V	14/16 TANDEM Unipolar Sleeve +C: 70326013; +D: 70326000; +E: 70326004; +F: 70326008
D	Ti-6Al-4V	14/16 TANDEM Unipolar Sleeve +D: 70326000; +E: 70326004; +F: 70326008
E	Ti-6Al-4V	10/12 TANDEM Unipolar Sleeve +E: 70326000; +F: 70326004; +G: 70326008
F	Ti-6Al-4V	10/12 to 14/16 Taper Conversion Sleeve +F: 70326000; +G: 70326004

Femoral Heads

For proper anatomy, and modularity fit, cobalt chromium, stainless steel, oxidized zirconium, and ceramic heads are available in multiple neck lengths. Heads are available in 10/12, 12/14, and 14/16 tapers. Certain modular heads and certain heads may require taper sleeves for attachment to the femoral stem taper. Refer to the Compatible Sleeve Combinations table in the taper sleeves section for details. Heads are highly polished for maximum friction, and wear. Femoral components and femoral heads are designed for use with any Smith & Nephew unipolar acetabular component or polyethylene liner, metal backed acetabular component, or cemented acetabular component.

Hüfttotalsysteme

YORCON: Gesetzlich ist die Verwendung dieser Hüftprothesen nur auf Anweisung eines Arztes zulässig.

Produktbeschreibungen

Hüfttotalsysteme

Die Hüfttotalsysteme bestehen aus folgenden Komponenten: Femoral-Komponente, modulare Halsstücke, proximale Hüftschläuche, Taper-Hüftschläuche, Acetabularkomponenten, Fixationschrauben und -kegel, Lochabdeckungen, Zement, Zementersatz und Zementersatzpulver. Alle implantierbaren Komponenten sind für den Einmalgebrauch bestimmt.

Materialien

Femorale Komponenten werden aus Kobalt-Chrom-Legierung, Titan-Legierung oder Edelstahl gefertigt. Die Hüftköpfe sind aus Kobalt-Chrom-Legierung, oxidisiertem Zirkon, BIOLOX forte Aluminiumoxid/Zirkonoxid, Zirkonoxid oder Edelstahl gefertigt. Acetabularkomponenten werden aus ultrahochmolekularem Polyethylen (UHMWPE), BIOLOX forte Aluminiumoxid/Zirkonoxid oder BIOLOX delta Aluminiumoxid/Zirkonoxid gefertigt. In den USA, siehe das separate Packungsbeilage der Acetabularkomponenten für Details. Alle polyacetabularen Komponenten werden aus UHMWPE gefertigt. Acetabularkomponenten werden aus Titan (Ti-6Al-4V-Legierung) oder Kobalt-Chrom-Legierung gefertigt. Die Komponente ist auf dem äußeren Kanon-Label angegeben. **HINWEIS:** BIOLOX delta Keramik-Linien sind in den USA nicht verfügbar.

Femorale Komponenten

Femorale Komponenten sind in verschiedenen Größen erhältlich. Porös beschichtete Komponenten sind für biologisches Wachstum vorgesehen und sind für den Einsatz ohne Zement vorgesehen. Modulare femorale Komponenten verfügen über ein ovales Taper, um Smith & Nephew CoCr-Modulhalsstücke und/oder ein Morse-Taper, um proximale Hüftschläuche zu akzeptieren. Nichtporöse femorale Komponenten können mit PMMA-Zementierung versehen sein, die zu einer gleichmäßigen Zementstärke führt.

Taper-Hüftschläuche

Ein Taper-Hüftschlauch kann erforderlich sein, wenn femorale Stämme mit bestimmten Hüftköpfen mated werden. Siehe die Kompatibilitätstabelle für die geeigneten Kombinationen. Falsche Hüftschläuche zu verwenden kann zu Implantatversagen und zu einer Revisionsoperation führen. Setzen Sie nie mehr als einen Hüftschlauch auf ein Implantat. Diese Kombination erhöht die Belastung des Implantats und kann zu Versagen und Revisionsoperationen führen.

Modulare Halsstücke

Modulare Halsstücke sind aus CoCr-Legierung gefertigt und sind in verschiedenen Konfigurationen erhältlich. Das modulare Halsstück mated und verriegelt mit dem ovalen Taper einer modulare femoralen Komponente auf der einen Seite und dem Taper eines 12/14-Hüftkopfes auf der anderen Seite.

Kompatible Hüftschläuche-Kombinationen

Femorale Halsstücke-Taper	40, 44 mm modulare COXNUM Köpfe	40, 44 mm modulare COCr Köpfe	BH modulare CoCr Köpfe*	TANDEM* CoCr & COXNUM unipolare Köpfe	14/16 COXNUM und CoCr Köpfe
12/14	A	A	B	C	-
14/16	-	-	-	D	-
10/12	-	-	-	E	F

* Modulare CoCr-Köpfe sind in den USA für Hemiarthroplastik vorgesehen.

** BH-Modulköpfe sind in den USA nicht verfügbar. Diese Köpfe können nur mit zementierten und CoCr-Femorstämmen verwendet werden.

Hüftschlauch	Material	Beschreibung/Teilenummern
A	Ti-6Al-4V	12/14 modulare Hüftschlauch +A: 7034241; +B: 7034242; +C: 70344248; +D: 70344230
B	CoCr	CoCr 12/14 modulare Hüftschlauch +B: 70222700; +D: 70222700; +E: 70222700; +F: 70222490
C	Ti-6Al-4V	14/16 TANDEM unipolarer Hüftschlauch +C: 70326013; +D: 70326000; +E: 70326004; +F: 70326008
D	Ti-6Al-4V	14/16 TANDEM unipolarer Hüftschlauch +D: 70326000; +E: 70326004; +F: 70326008
E	Ti-6Al-4V	10/12 TANDEM unipolarer Hüftschlauch +E: 70326000; +F: 70326004; +G: 70326008
F	Ti-6Al-4V	10/12 zu 14/16 Taper Umwandlungshüftschlauch +F: 70326000; +G: 70326004

Hüftköpfe

Für die richtige Anatomie und die Modularität passen Hüftköpfe in verschiedenen Halslängen. Hüftköpfe sind in 10/12, 12/14 und 14/16 Taper erhältlich. Bestimmte modulare Hüftköpfe und bestimmte Hüftköpfe benötigen Hüftschläuche für die Verbindung zum Femorstamm-Taper. Siehe die Kompatibilitätstabelle in der Taper-Hüftschläuche-Sektion für Details. Hüftköpfe sind hochpoliert, um die maximale Reibung und den Verschleiß zu gewährleisten. Femorale Komponenten und Hüftköpfe sind für den Einsatz mit jedem Smith & Nephew unipolaren Acetabularkomponenten oder Polyethylen- oder Metallrückstütze-Acetabularkomponenten oder zementierten Acetabularkomponenten ausgelegt.

REF CATALOG 71354522
LOT BATCH CODE 16HM10839
REDAPT°
0° CEMENTED

QTY: (1)
USE 2026-08-14

 **smith&nephew**

Liner

Einsatz • Insert • Inserto • Liner • Inserto • Mellanlägg • Vložka • Aster • Ένθετο •
Revestimento • Liner




54 MM OD
36 MM ID



REDAPT[®]
0°
CEMENTED LINER
XLPE



Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA

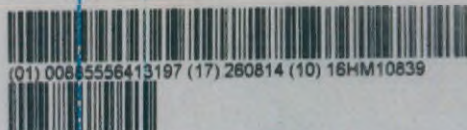

(01) 00865556413197 (17) 260814 (10) 16HM10839

(11) 160816

STERILE EO

ETO STERILIZED
* Trademark(s) of Smith & Nephew.



NO REUSE



SEE INSERT

EC REP

Smith & Nephew Orthopaedics GmbH,
Alemannenstrasse 14, 78532 Tuttlingen,
Germany




T49H18AB; 2



This carton is recyclable.

www.smith-nephew.com



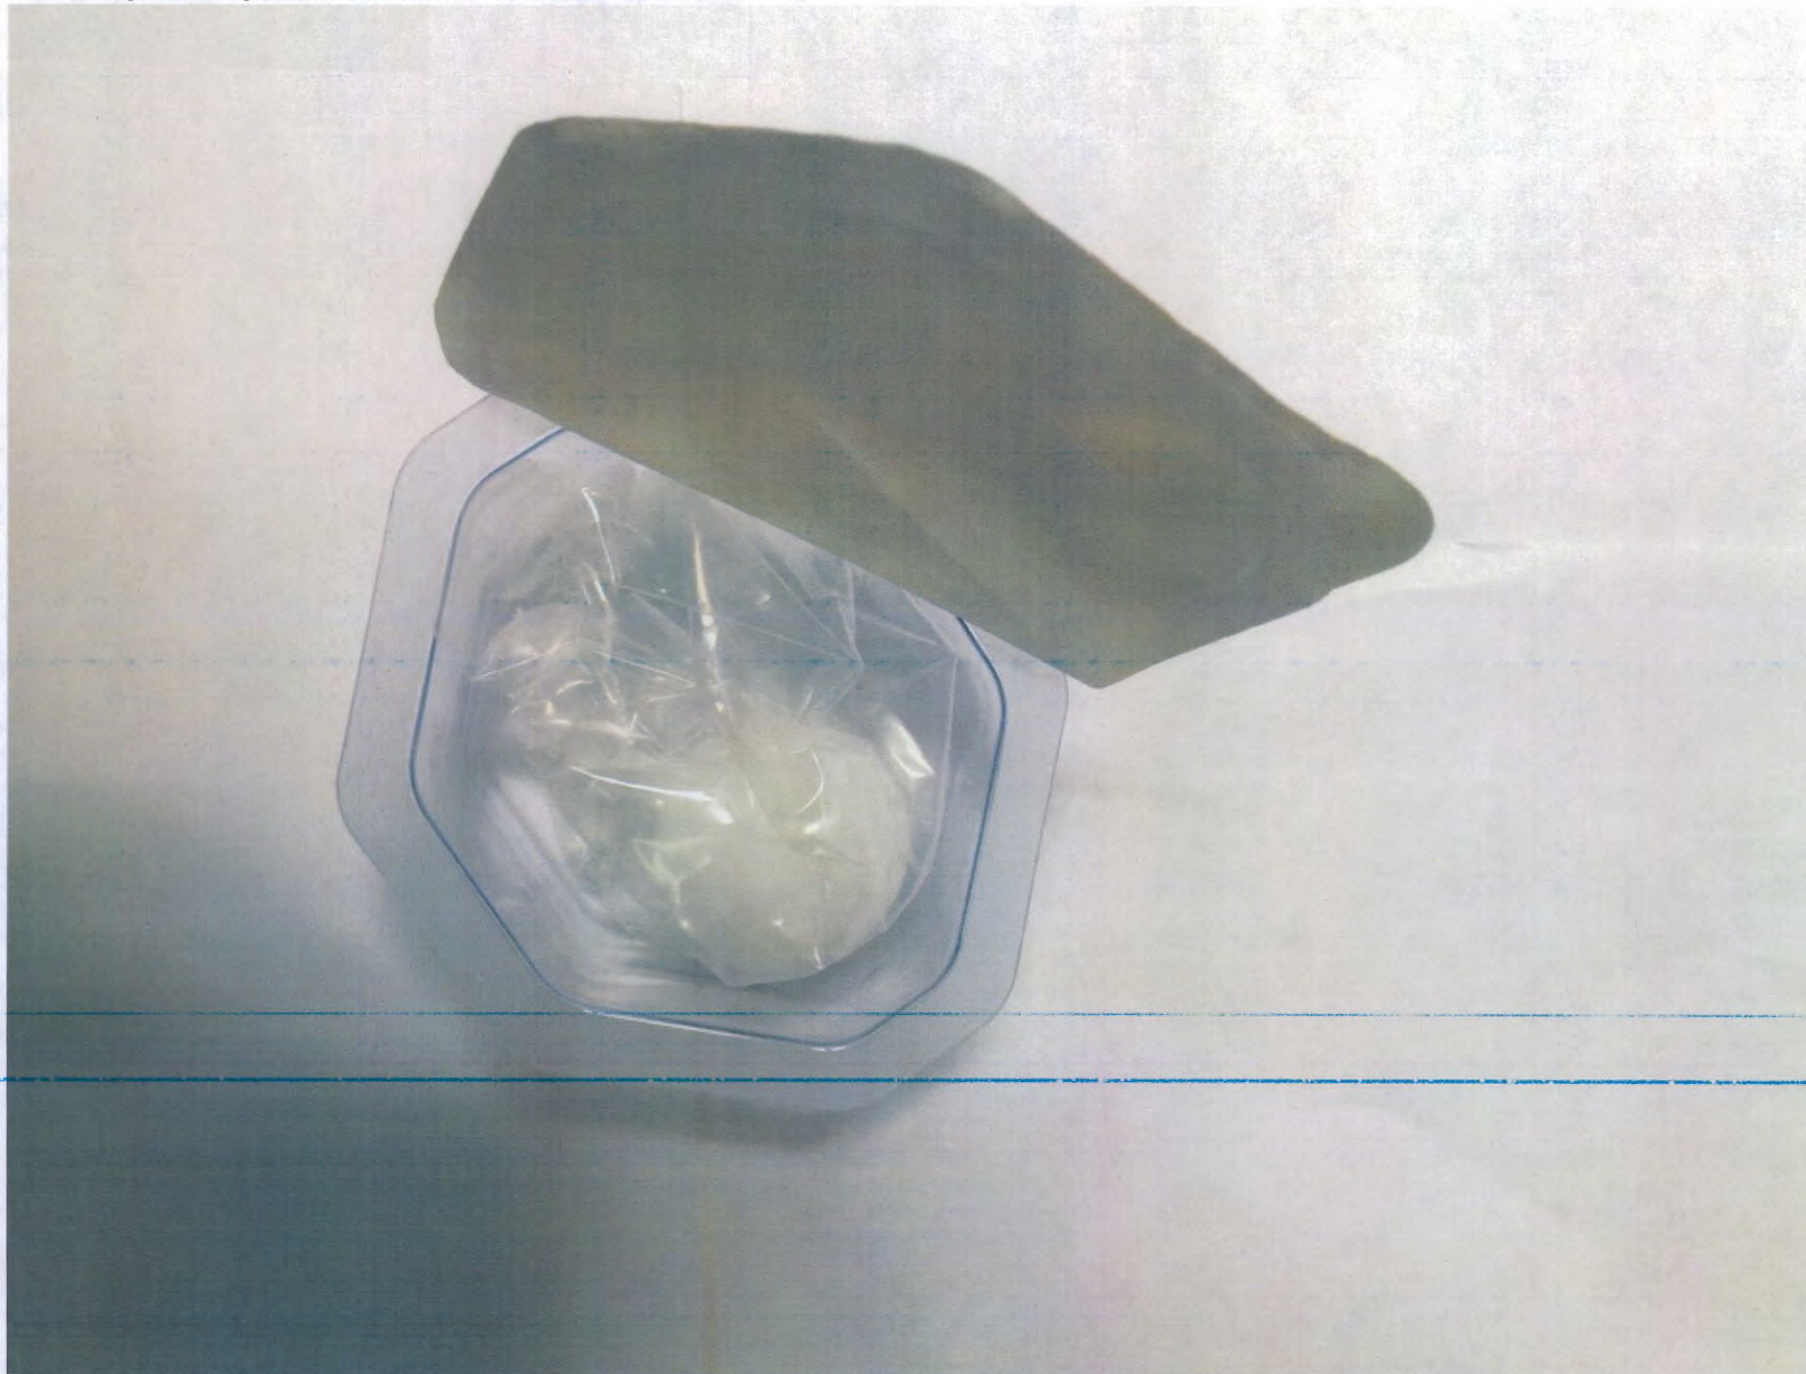





TO4HCTIK 4
ATTACH

CHART-STIK® LABEL

7354249
16GM10824

STERILE EO 2026-07-15

ANTEVERTED
28 MM X 50 MM
REDAPT
CEMENTED LINER
XLPE



TO4HCTIK 4
ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

7354249
16GM10824

STERILE EO 2026-07-15

ANTEVERTED
28 MM X 50 MM
REDAPT
CEMENTED LINER
XLPE



TO4HCTIK 4
ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

7354249
16GM10824

STERILE EO 2026-07-15

ANTEVERTED
28 MM X 50 MM
REDAPT
CEMENTED LINER
XLPE



TO4HCTIK 4
ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

smith&nephew

Instructions for Use

English

Gebrauchsanweisung

Total Hip Systems

R The total hip system is a modular system for total hip replacement. It consists of a femoral component, an acetabular component, and a liner. The system is designed for use in patients with a primary hip joint disease.

Device Description

The total hip system consists of a femoral component, an acetabular component, and a liner. The femoral component is made of titanium alloy and is designed to be cemented into the femoral canal. The acetabular component is made of titanium alloy and is designed to be cemented into the acetabulum. The liner is made of ultra-high molecular weight polyethylene and is designed to be inserted into the acetabular component.

Assembly

The femoral component is assembled by inserting the femoral neck into the femoral canal. The acetabular component is assembled by inserting the acetabular cup into the acetabulum. The liner is assembled by inserting it into the acetabular cup. The system is then tested for stability and range of motion.

Functional Components

The functional components of the total hip system are the femoral component, the acetabular component, and the liner. The femoral component is made of titanium alloy and is designed to be cemented into the femoral canal. The acetabular component is made of titanium alloy and is designed to be cemented into the acetabulum. The liner is made of ultra-high molecular weight polyethylene and is designed to be inserted into the acetabular cup.

Taper Sleeve

The taper sleeve is a component of the total hip system that is used to secure the femoral component into the femoral canal. It is made of titanium alloy and is designed to be cemented into the femoral canal.

Model	Component	Material	Weight	Length	Width
Model 1	Femoral Head	Titanium Alloy	100g	40mm	40mm
Model 2	Acetabular Cup	Titanium Alloy	150g	60mm	60mm
Model 3	Liner	Ultra-High Molecular Weight Polyethylene	50g	40mm	40mm
Model 4	Taper Sleeve	Titanium Alloy	80g	30mm	30mm

Model	Component	Material	Weight	Length	Width
Model 1	Femoral Head	Titanium Alloy	100g	40mm	40mm
Model 2	Acetabular Cup	Titanium Alloy	150g	60mm	60mm
Model 3	Liner	Ultra-High Molecular Weight Polyethylene	50g	40mm	40mm
Model 4	Taper Sleeve	Titanium Alloy	80g	30mm	30mm

Model	Component	Material	Weight	Length	Width
Model 1	Femoral Head	Titanium Alloy	100g	40mm	40mm
Model 2	Acetabular Cup	Titanium Alloy	150g	60mm	60mm
Model 3	Liner	Ultra-High Molecular Weight Polyethylene	50g	40mm	40mm
Model 4	Taper Sleeve	Titanium Alloy	80g	30mm	30mm

Model	Component	Material	Weight	Length	Width
Model 1	Femoral Head	Titanium Alloy	100g	40mm	40mm
Model 2	Acetabular Cup	Titanium Alloy	150g	60mm	60mm
Model 3	Liner	Ultra-High Molecular Weight Polyethylene	50g	40mm	40mm
Model 4	Taper Sleeve	Titanium Alloy	80g	30mm	30mm

Model	Component	Material	Weight	Length	Width
Model 1	Femoral Head	Titanium Alloy	100g	40mm	40mm
Model 2	Acetabular Cup	Titanium Alloy	150g	60mm	60mm
Model 3	Liner	Ultra-High Molecular Weight Polyethylene	50g	40mm	40mm
Model 4	Taper Sleeve	Titanium Alloy	80g	30mm	30mm

Hüfttotalsystem

R Das Hüfttotalsystem ist ein modulares System für die totale Hüftgelenkprothese. Es besteht aus einem Femurkomponente, einer Acetabulumkomponente und einer Linie. Das System ist für Patienten mit einer primären Hüftgelenkerkrankung konzipiert.

Produktbeschreibung

Das Hüfttotalsystem besteht aus einer Femurkomponente, einer Acetabulumkomponente und einer Linie. Die Femurkomponente ist aus Titanlegierung gefertigt und ist dazu vorgesehen, in den Femurkanal zementiert zu werden. Die Acetabulumkomponente ist aus Titanlegierung gefertigt und ist dazu vorgesehen, in das Acetabulum zementiert zu werden. Die Linie ist aus ultrahochmolekularem Polyethylen gefertigt und ist dazu vorgesehen, in die Acetabulumkomponente eingesetzt zu werden.

Montage

Die Femurkomponente wird montiert, indem der Femurhals in den Femurkanal eingesetzt wird. Die Acetabulumkomponente wird montiert, indem die Acetabulumschale in das Acetabulum eingesetzt wird. Die Linie wird montiert, indem sie in die Acetabulumschale eingesetzt wird. Das System wird dann auf Stabilität und Bewegungsbereich getestet.

Funktionale Komponenten

Die funktionellen Komponenten des Hüfttotalsystems sind die Femurkomponente, die Acetabulumkomponente und die Linie. Die Femurkomponente ist aus Titanlegierung gefertigt und ist dazu vorgesehen, in den Femurkanal zementiert zu werden. Die Acetabulumkomponente ist aus Titanlegierung gefertigt und ist dazu vorgesehen, in das Acetabulum zementiert zu werden. Die Linie ist aus ultrahochmolekularem Polyethylen gefertigt und ist dazu vorgesehen, in die Acetabulumschale eingesetzt zu werden.

Keilring

Der Keilring ist ein Bestandteil des Hüfttotalsystems, der verwendet wird, um die Femurkomponente in den Femurkanal zu sichern. Er ist aus Titanlegierung gefertigt und ist dazu vorgesehen, in den Femurkanal zementiert zu werden.


Modell	Komponente	Material	Gewicht	Länge	Breite
Modell 1	Femurkopf	Titaniumlegierung	100g	40mm	40mm
Modell 2	Acetabulumschale	Titaniumlegierung	150g	60mm	60mm
Modell 3	Linie	Ultrahochmolekulares Polyethylen	50g	40mm	40mm
Modell 4	Keilring	Titaniumlegierung	80g	30mm	30mm

Modell	Komponente	Material	Gewicht	Länge	Breite
Modell 1	Femurkopf	Titaniumlegierung	100g	40mm	40mm
Modell 2	Acetabulumschale	Titaniumlegierung	150g	60mm	60mm
Modell 3	Linie	Ultrahochmolekulares Polyethylen	50g	40mm	40mm
Modell 4	Keilring	Titaniumlegierung	80g	30mm	30mm

Modell	Komponente	Material	Gewicht	Länge	Breite
Modell 1	Femurkopf	Titaniumlegierung	100g	40mm	40mm
Modell 2	Acetabulumschale	Titaniumlegierung	150g	60mm	60mm
Modell 3	Linie	Ultrahochmolekulares Polyethylen	50g	40mm	40mm
Modell 4	Keilring	Titaniumlegierung	80g	30mm	30mm

Modell	Komponente	Material	Gewicht	Länge	Breite
Modell 1	Femurkopf	Titaniumlegierung	100g	40mm	40mm
Modell 2	Acetabulumschale	Titaniumlegierung	150g	60mm	60mm
Modell 3	Linie	Ultrahochmolekulares Polyethylen	50g	40mm	40mm
Modell 4	Keilring	Titaniumlegierung	80g	30mm	30mm

Modell	Komponente	Material	Gewicht	Länge	Breite
Modell 1	Femurkopf	Titaniumlegierung	100g	40mm	40mm
Modell 2	Acetabulumschale	Titaniumlegierung	150g	60mm	60mm
Modell 3	Linie	Ultrahochmolekulares Polyethylen	50g	40mm	40mm
Modell 4	Keilring	Titaniumlegierung	80g	30mm	30mm

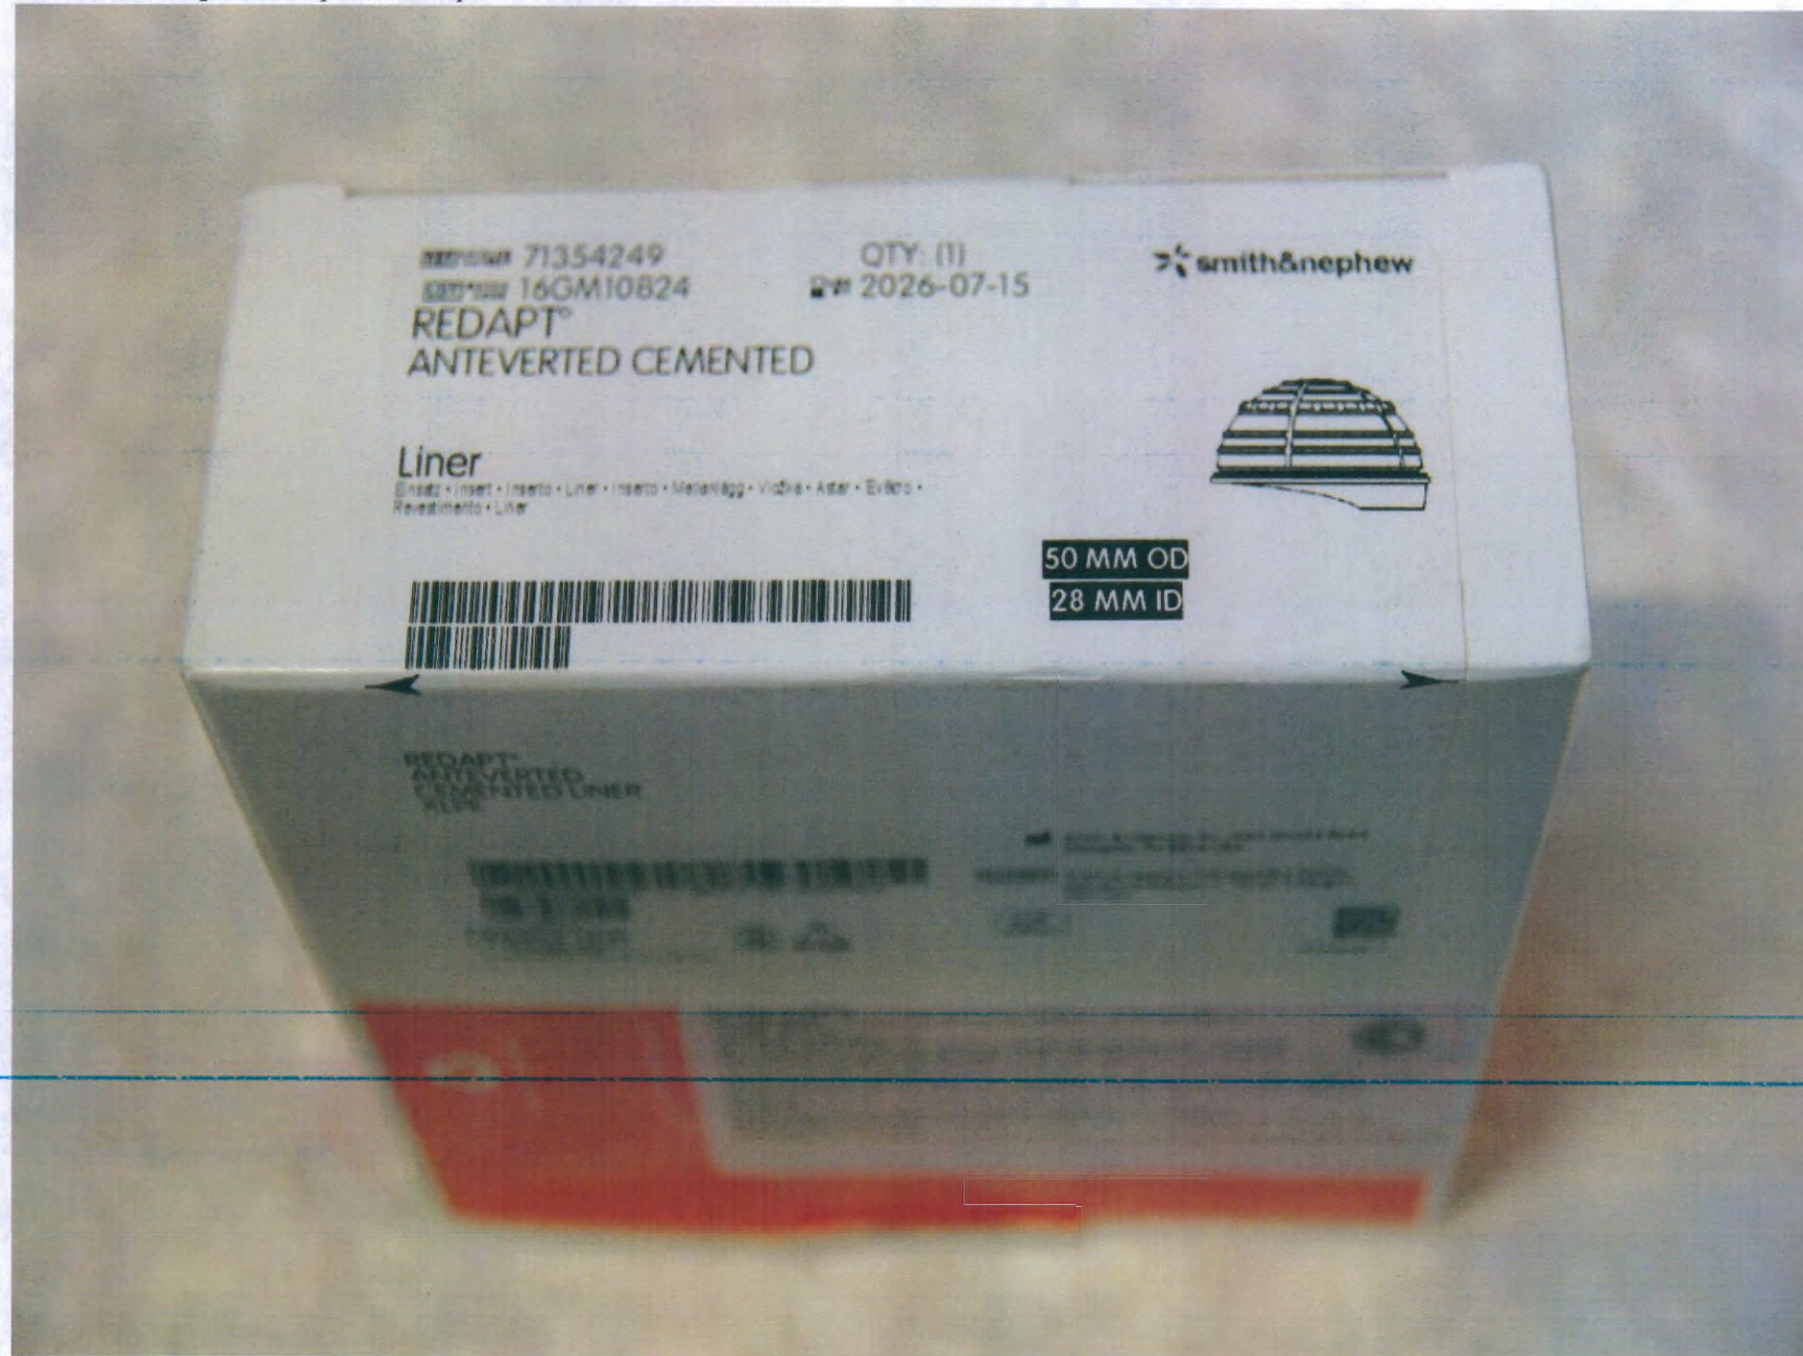

REDAPT®
ANTEVERTED
CEMENTED LINER
XLPE

Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA



(01) 00885556320297 (17) 280715 (10) 16GM10824



(11) 160717

STERILE EO

ETO STERILIZED
Trademarks of Smith & Nephew.



EC REP

Smith & Nephew Orthopaedics GmbH,
Altmannstrasse 14, 76532 Tuttlingen,
Germany



T49H18AB; 2



This carton is recyclable.

www.smith-nephew.com

Артикул: 71354249

Наименование: Вкладыш цементируемый REDAPT, XLPE, 20°, 28/50 мм

Размер: 28/50 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: «Смит энд Непью Инк» (Smith & Nephew, Inc.), 1450 Brooks Road,
Memphis, Tennessee (TN), 38116, USA

Уполномоченный представитель на территории РФ: ООО «Смит энд Непью», 105120, Россия, г.
Москва, 2-й Сыромятнический пер., д. 1, 9 этаж, пом. 1, ком. 1 тел./факс: +7 495 756 55 03

Метод стерилизации: Стерилизация оксидом этилена. Стерильно. Алергенно. Нетоксично.

Номер RU:

Назначение, способ применения, противопоказания: См. инструкцию


Условия хранения: в сухом, защищенном от света месте, при температуре от -20°C до +35°C


Меры предосторожности: -


Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-sell-it/europe/russia/ru/>



**IV. Винты блокирующие REDAPT, на примере варианта исполнения:
Винт блокирующий REDAPT, 35 мм**

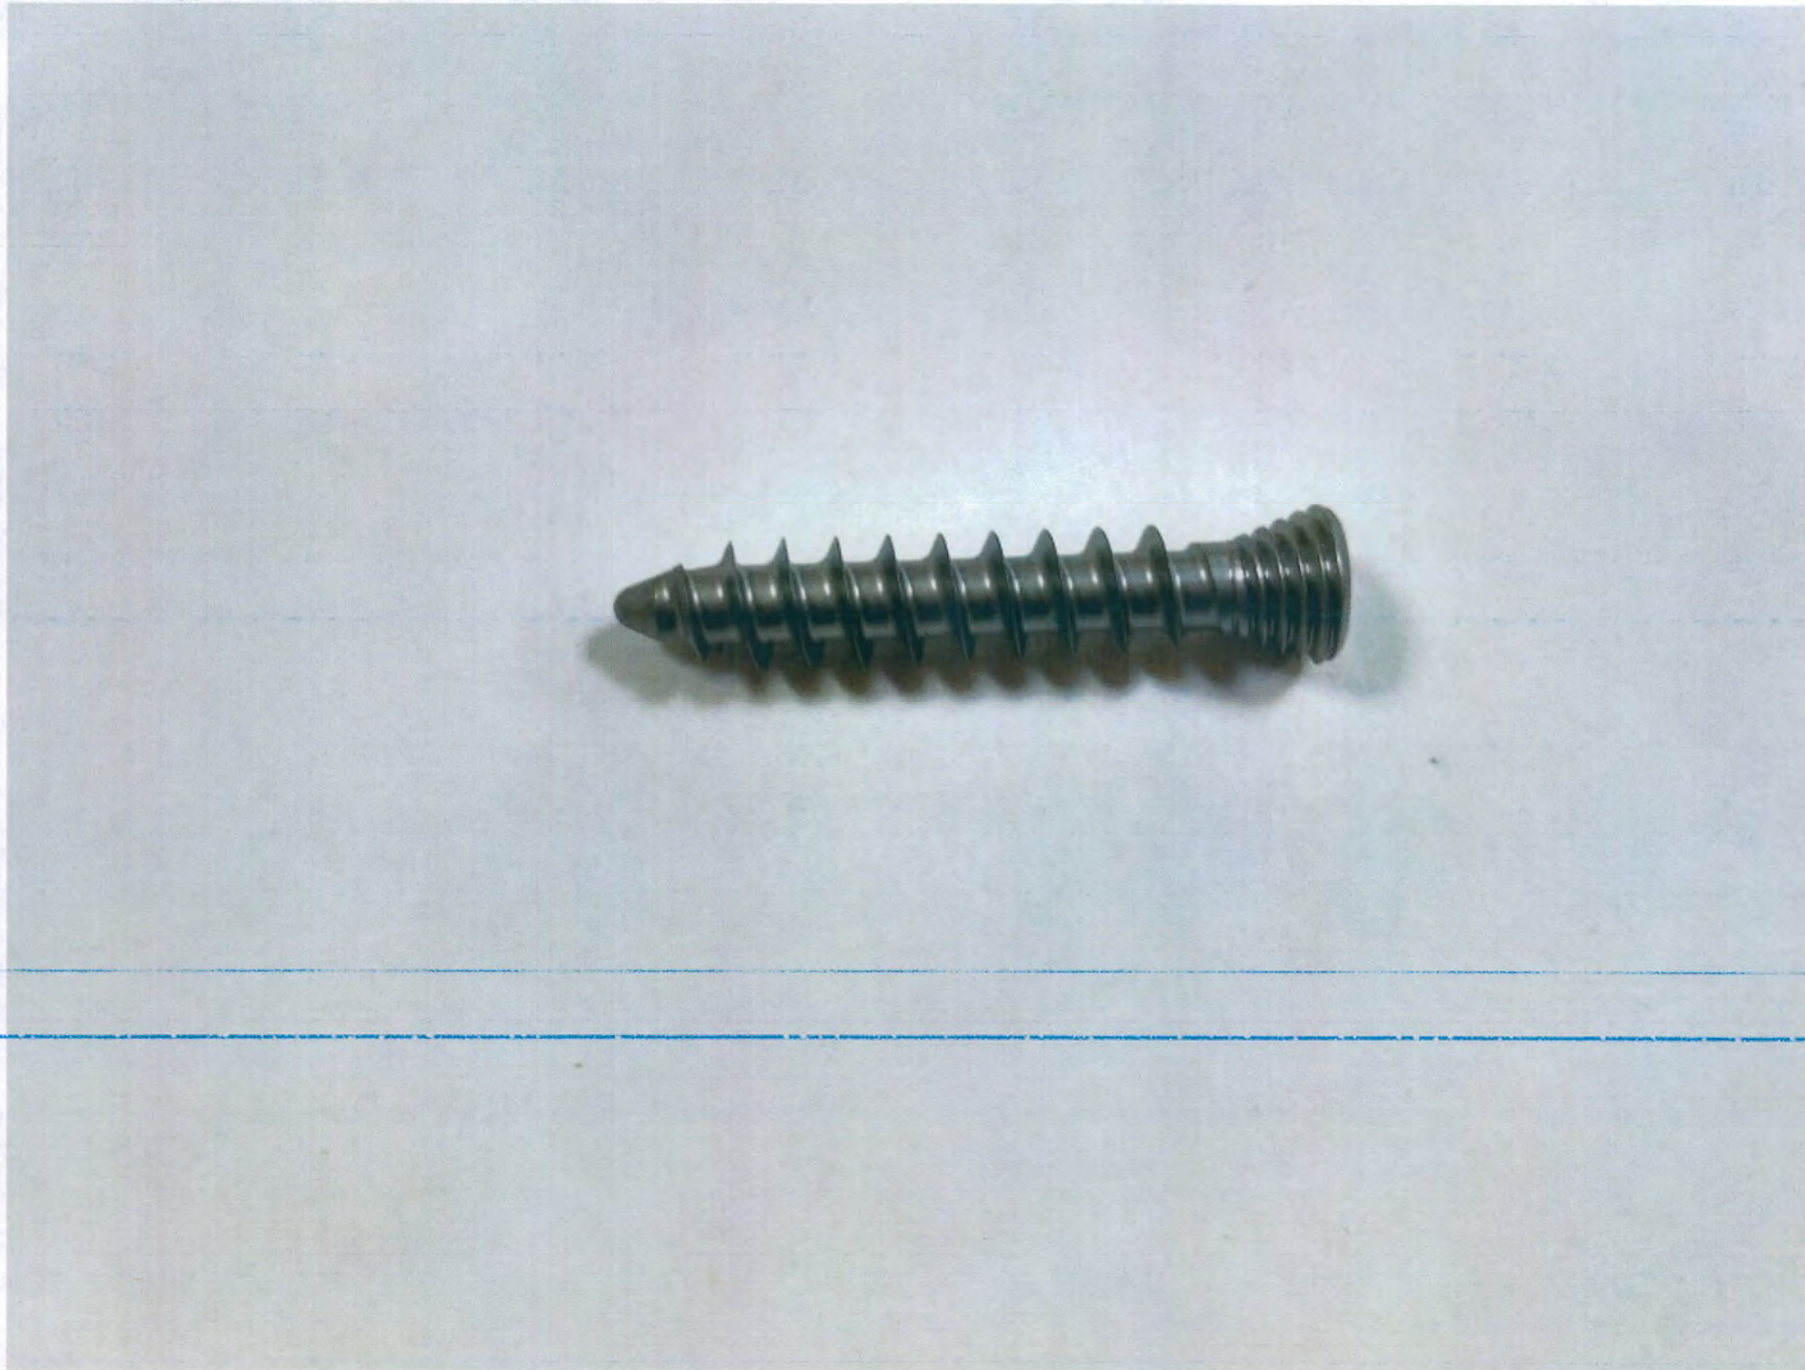

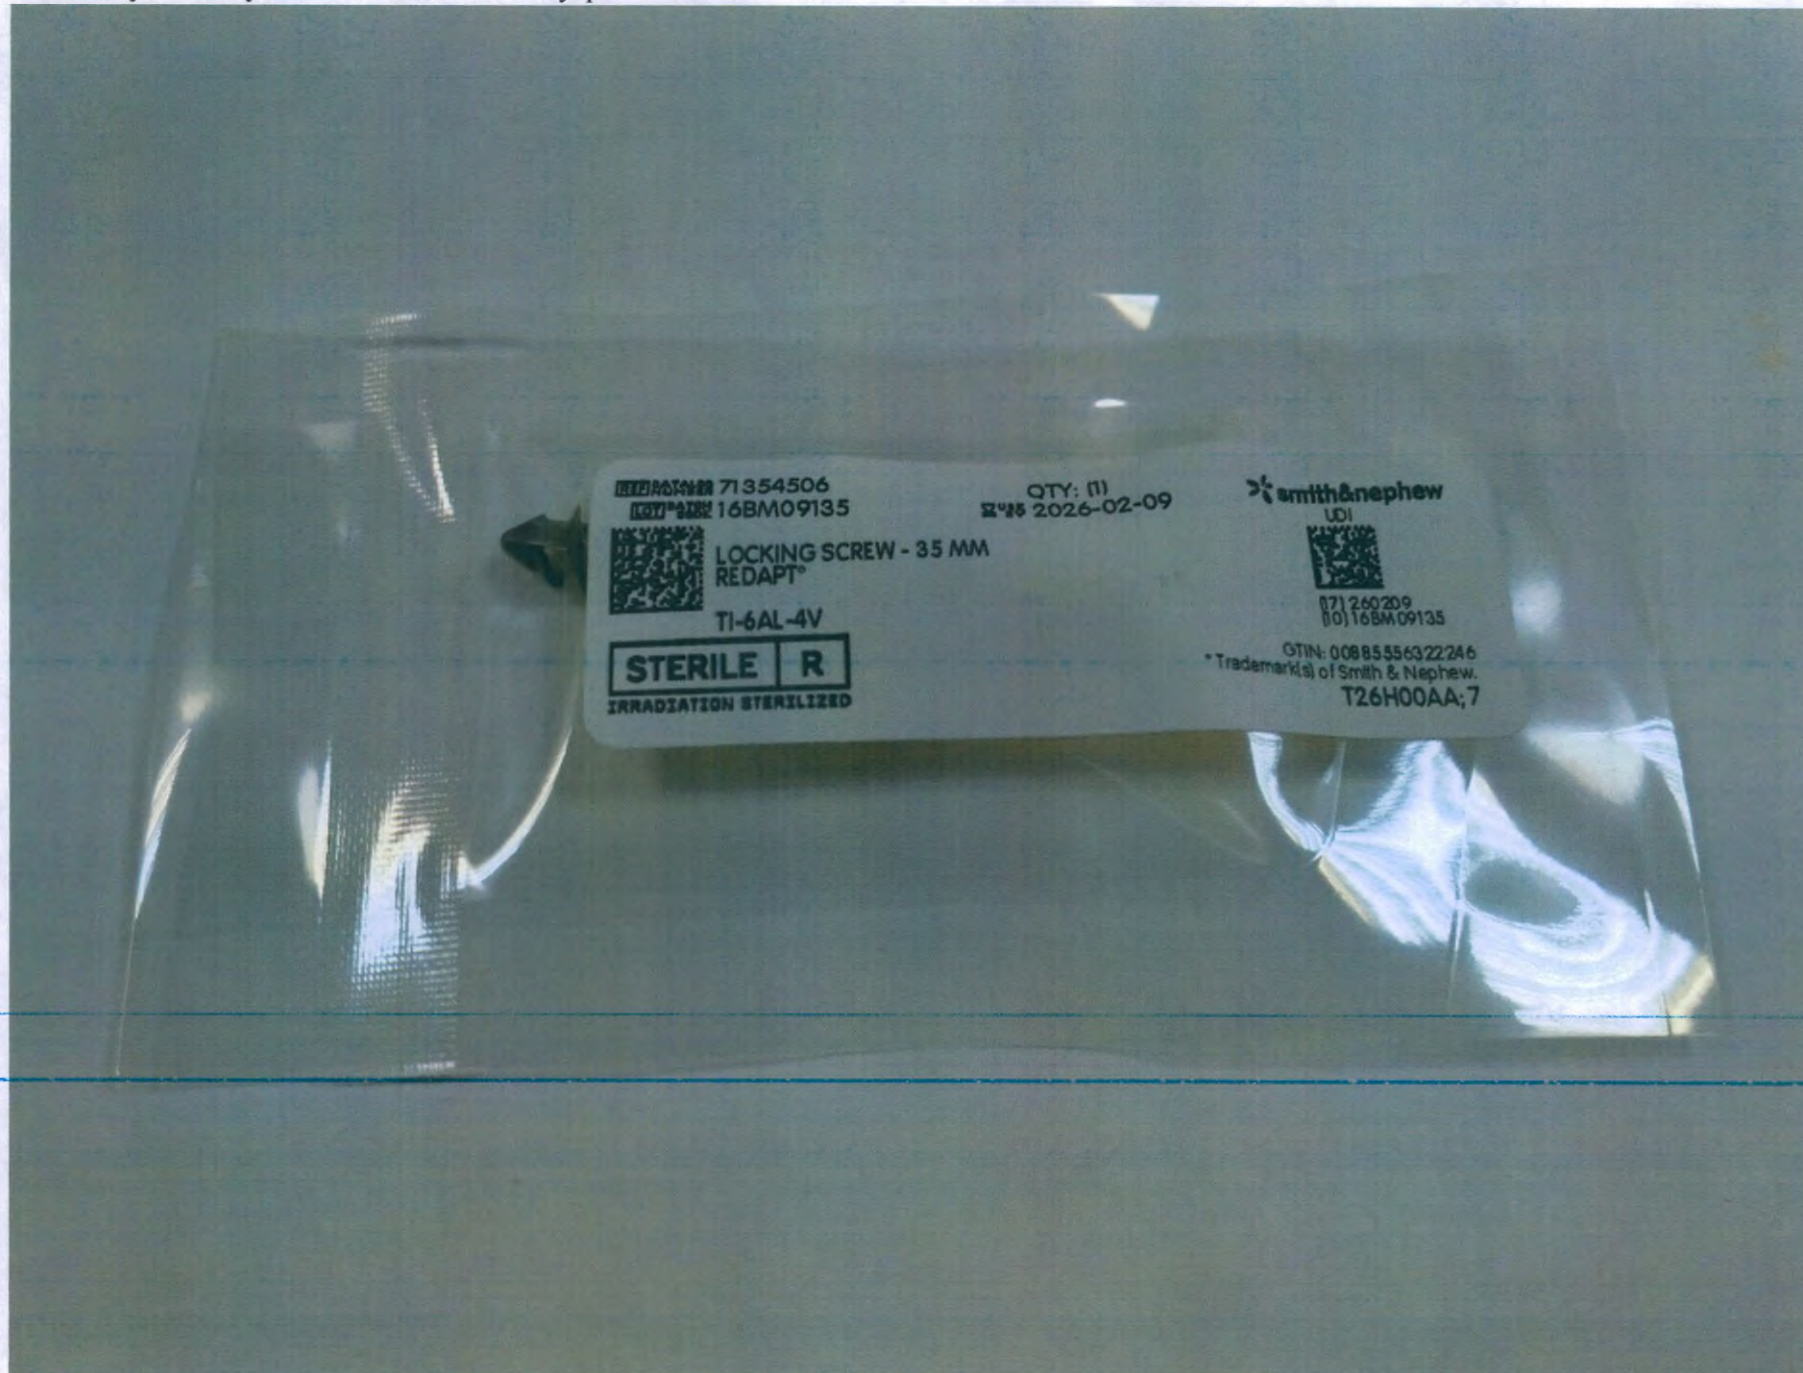

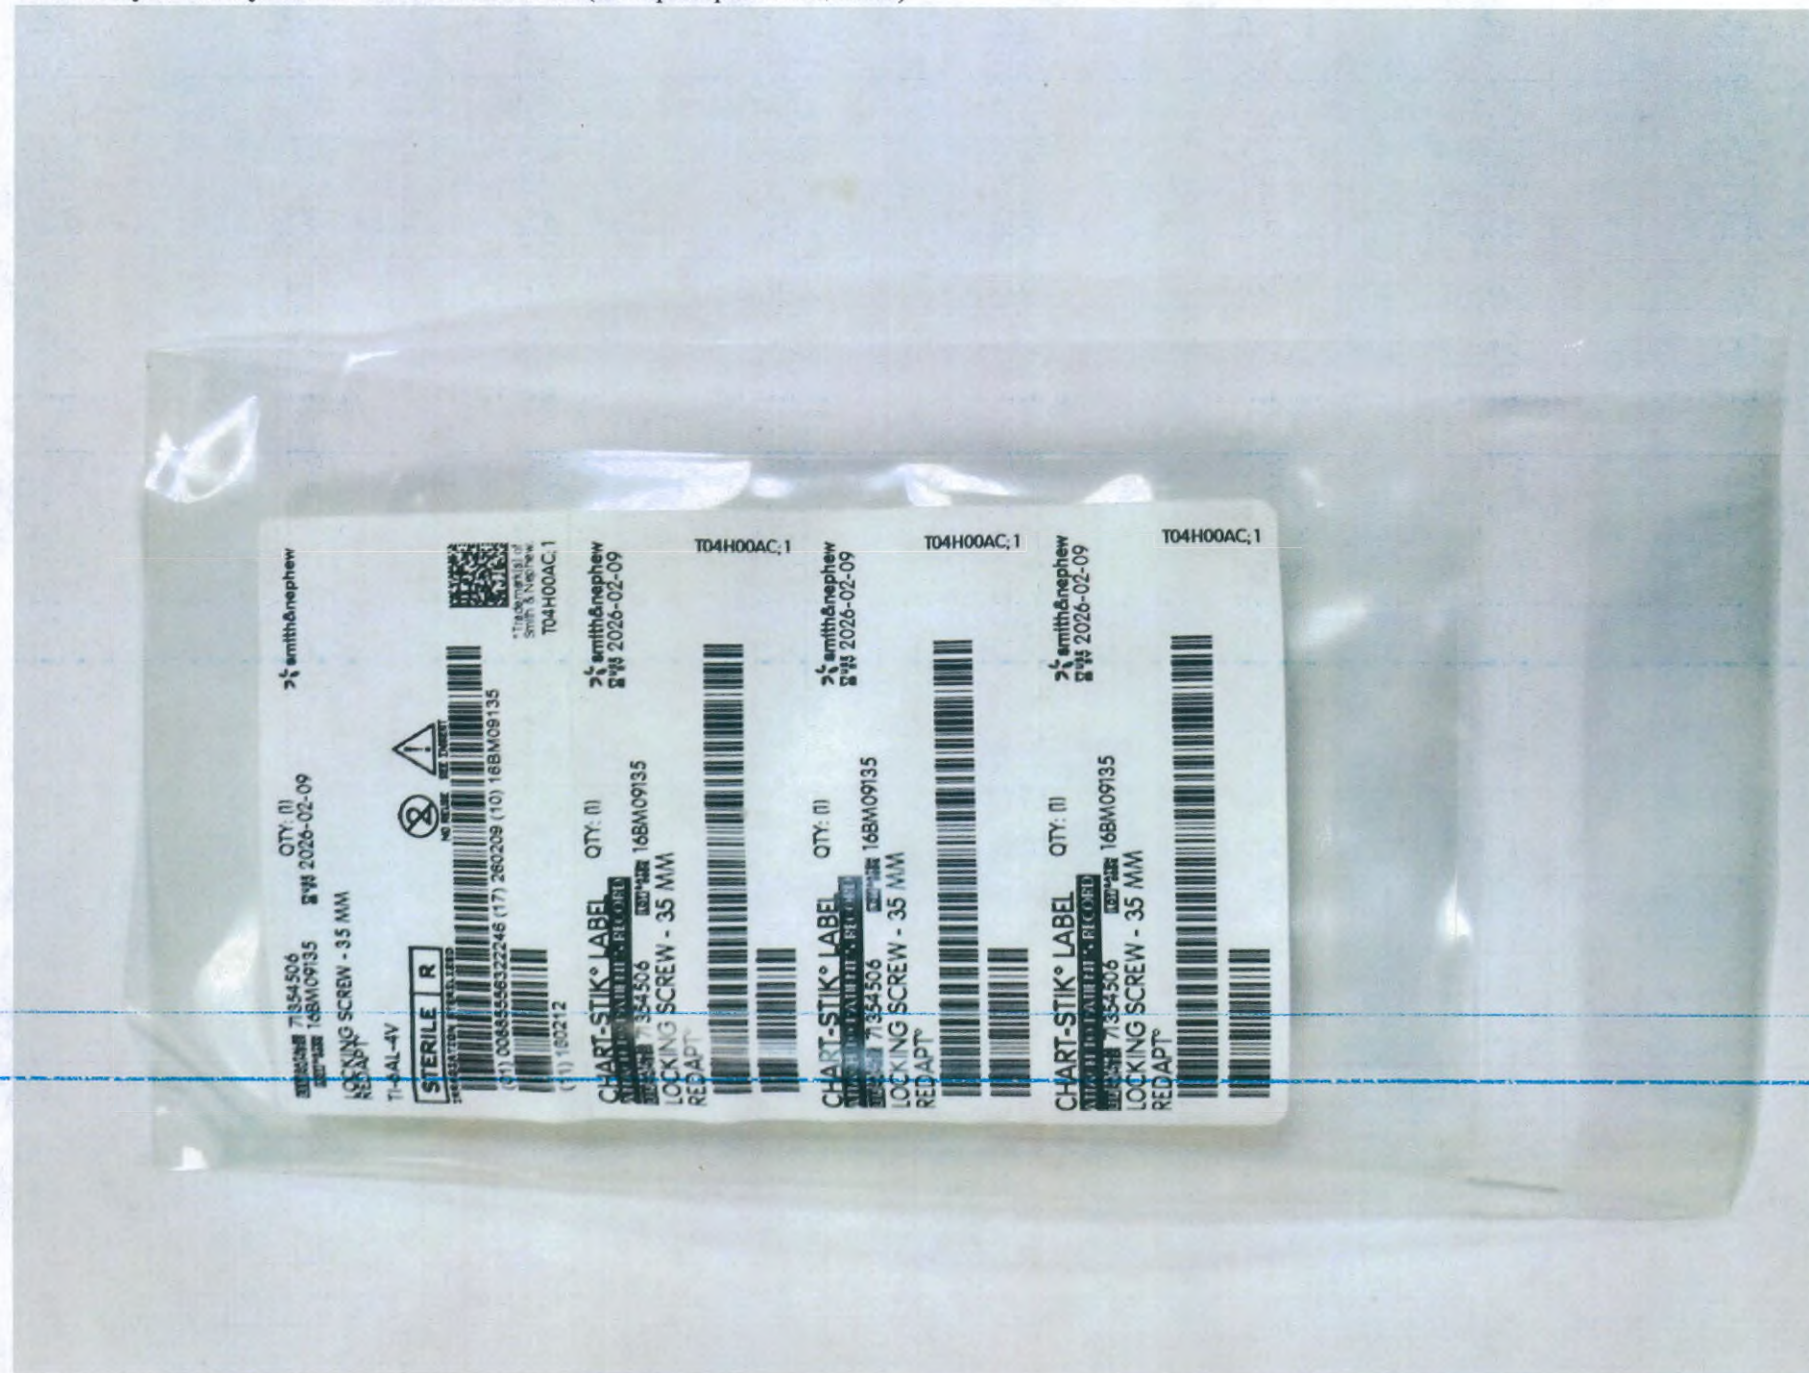

Instructions for Use

Total Hip Systems

R Orthopaedic Joint Prostheses (Endoprosthesis) Hip Joint

Device Description
The Total Hip System consists of a femoral component, a acetabular component, and a femoral head. The femoral component is made of titanium alloy and the acetabular component is made of ultra-high molecular weight polyethylene (UHMWPE). The femoral head is made of cobalt-chromium alloy.

Indications
The Total Hip System is indicated for the treatment of degenerative joint disease of the hip, traumatic joint injury, and congenital hip dysplasia. It is also indicated for the treatment of hip pain and disability due to osteoarthritis, rheumatoid arthritis, and ankylosing spondylitis.

Contraindications
The Total Hip System is contraindicated in patients with severe osteoporosis, active infection of the hip joint, and severe medical conditions that may increase the risk of complications. It is also contraindicated in patients with a known hypersensitivity to the components of the prosthesis.

Preoperative Preparation
The patient should be evaluated preoperatively for medical conditions that may increase the risk of complications. The patient should also be evaluated for the presence of infection and for the presence of a known hypersensitivity to the components of the prosthesis.

Implantation
The Total Hip System is implanted using a minimally invasive surgical approach. The femoral component is implanted into the femoral canal and the acetabular component is implanted into the acetabulum.

Component	Material	Size	Weight
Femoral Head	Cobalt-Chromium Alloy	28 mm	100 g
Femoral Neck	Titanium Alloy	125 mm	200 g
Acetabular Cup	UHMWPE	48 mm	150 g

Postoperative Care
The patient should be monitored for signs of infection, bleeding, and pain. The patient should also be monitored for the presence of a known hypersensitivity to the components of the prosthesis.

Long-term Follow-up
The patient should be followed up for the long-term results of the surgery. The patient should also be followed up for the presence of a known hypersensitivity to the components of the prosthesis.

Warranty
The Total Hip System is covered by a 10-year warranty. The warranty is void if the patient has not followed the instructions for use.

References
The Total Hip System is described in the following references:

Appendix A: Component Specifications

Appendix B: Component Dimensions

Appendix C: Component Weights

Appendix D: Component Materials

Appendix E: Component Images

Appendix F: Component Diagrams

Appendix G: Component Tables

Appendix H: Component Lists

Appendix I: Component Index

Appendix J: Component Glossary

Appendix K: Component Bibliography

Appendix L: Component Index

English

Gebrauchsanweisung

Hüfttotalprothesen

R

Prothetische Gelenkprothesen

Hüftgelenk

Gerätebeschreibung

Das Total-Hip-System besteht aus einem Femurkomponente, einer Acetabulumkomponente und einem Femurkopf. Das Femurkomponente ist aus Titanlegierung gefertigt und die Acetabulumkomponente ist aus ultrahochmolekularem Polyethylen (UHMWPE) gefertigt. Der Femurkopf ist aus Kobalt-Chrom-Legierung gefertigt.

Indikationen
Das Total-Hip-System ist indiziert zur Behandlung von degenerativen Gelenkerkrankungen des Hüftgelenks, traumatischen Gelenkverletzungen und angeborenen Hüftgelenkfehlern. Es ist auch indiziert zur Behandlung von Hüftschmerzen und -funktionsstörungen bei Osteoarthritis, Rheumatoidea Arthritis und Ankylosierung des Hüftgelenks.

Gegenanzeigen
Das Total-Hip-System ist kontraindiziert bei Patienten mit schwerer Osteoporose, aktiver Infektion des Hüftgelenks und schweren Vorerkrankungen, die das Risiko von Komplikationen erhöhen. Es ist auch kontraindiziert bei Patienten mit einer bekannten Überempfindlichkeit gegen die Komponenten der Prothese.

Vorbereitung der Operation
Der Patient sollte präoperativ auf medizinische Vorerkrankungen, die das Risiko von Komplikationen erhöhen, untersucht werden. Der Patient sollte auch auf das Vorhandensein einer Infektion und auf das Vorhandensein einer bekannten Überempfindlichkeit gegen die Komponenten der Prothese untersucht werden.

Implantation
Das Total-Hip-System wird über einen minimal-invasiven chirurgischen Zugang implantiert. Das Femurkomponente wird in den Femurkanal und die Acetabulumkomponente wird in das Acetabulum implantiert.

Komponente	Material	Größe	Gewicht
Femurkopf	Kobalt-Chrom-Legierung	28 mm	100 g
Femurhals	Titanlegierung	125 mm	200 g
Acetabulumschale	UHMWPE	48 mm	150 g

Postoperative Pflege
Der Patient sollte auf Anzeichen von Infektion, Blutung und Schmerzen überwacht werden. Der Patient sollte auch auf das Vorhandensein einer bekannten Überempfindlichkeit gegen die Komponenten der Prothese überwacht werden.

Langfristige Nachsorge
Der Patient sollte langfristig auf das Ergebnis der Operation überwacht werden. Der Patient sollte auch langfristig auf das Vorhandensein einer bekannten Überempfindlichkeit gegen die Komponenten der Prothese überwacht werden.

Garantie
Das Total-Hip-System ist durch eine 10-jährige Garantie geschützt. Die Garantie ist ungültig, wenn der Patient die Gebrauchsanweisung nicht befolgt.

Referenzen
Das Total-Hip-System ist in den folgenden Referenzen beschrieben:

Anhang A: Komponentenspezifikationen

Anhang B: Komponentendimensionen

Anhang C: Komponentengewichte

Anhang D: Komponentematerialien

Anhang E: Komponente Abbildungen

Anhang F: Komponentendiagramme

Anhang G: Komponententabellen

Anhang H: Komponentelisten

Anhang I: Komponente Index

Anhang J: Komponente Glossar

Anhang K: Komponente Bibliographie

Anhang L: Komponente Index

Артикул: 71364506
Наименование: Винт блокирующий REDAPT, 35 мм
Размер: 35 мм
Кол-во шт. в упаковке: 1 шт
Дата изготовления, использовать до, номер партии/серии: См. на упаковке
Наименование и адрес изготовителя: «Смит энд Нефью Инк» (Smith & Nephew, Inc.), 1450 Brooks Road, Memphis, Tennessee (TN), 38116, USA
Уполномоченный представитель на территории РФ: ООО «Смит энд Нефью», 105120, Россия, г. Москва, 2-й Сыромятнинский пер., д. 1, 9 этаж, пом. 1, ком. 1 тел./факс: +7 495 755 55 03
Метод стерилизации: Радиационная стерилизация Стерильно Асепрично Нетоксично
Номер РУ:
Назначение, способ применения, противопоказания: См. инструкцию
Условия хранения: в сухом, защищенном от света месте, при температуре от -20°C до +35°C
Меры предосторожности:
Инструкция по применению: <http://www.smith-nephew.com/about-us/more-we-operate/eurotel.russia/us/>



tion is recyclable.

smith-nephew.com

REF CATALOG NUMBER 71354506
LOT BATCH CODE 16BM09135

QTY: (1)
EXP. DATE 2026-02-09

smith&nephew

LOCKING SCREW - 35 MM
REDAPT®

TI-6AL-4V

Locking Screw • Verriegelungsschraube • Vis de Blocage • Vite bloccante • Afsluitschroef • Tornillo de bloqueo • Låsskruv • Uzamykací šroub • Kilitleme Vidası • Βίδα κλειδώματος • Parafuso de bloqueio • Låseskrue



STERILE R

IRRADIATION STERILIZED



Smith & Nephew, Inc. 1450 Brooks Road
 Memphis, TN 38116 USA

EC REP Smith & Nephew Orthopaedics GmbH,
 Altmannstrasse 14, 78532 Tuttlingen,
 Germany



(01) 00885556322246 (17) 260209 (10) 16BM09135



(11) 160212


*Trademarks of Smith & Nephew.

T36H04AA: 1


**V. Набор заглушек REDAPT, в составе:
Заглушка отверстия**






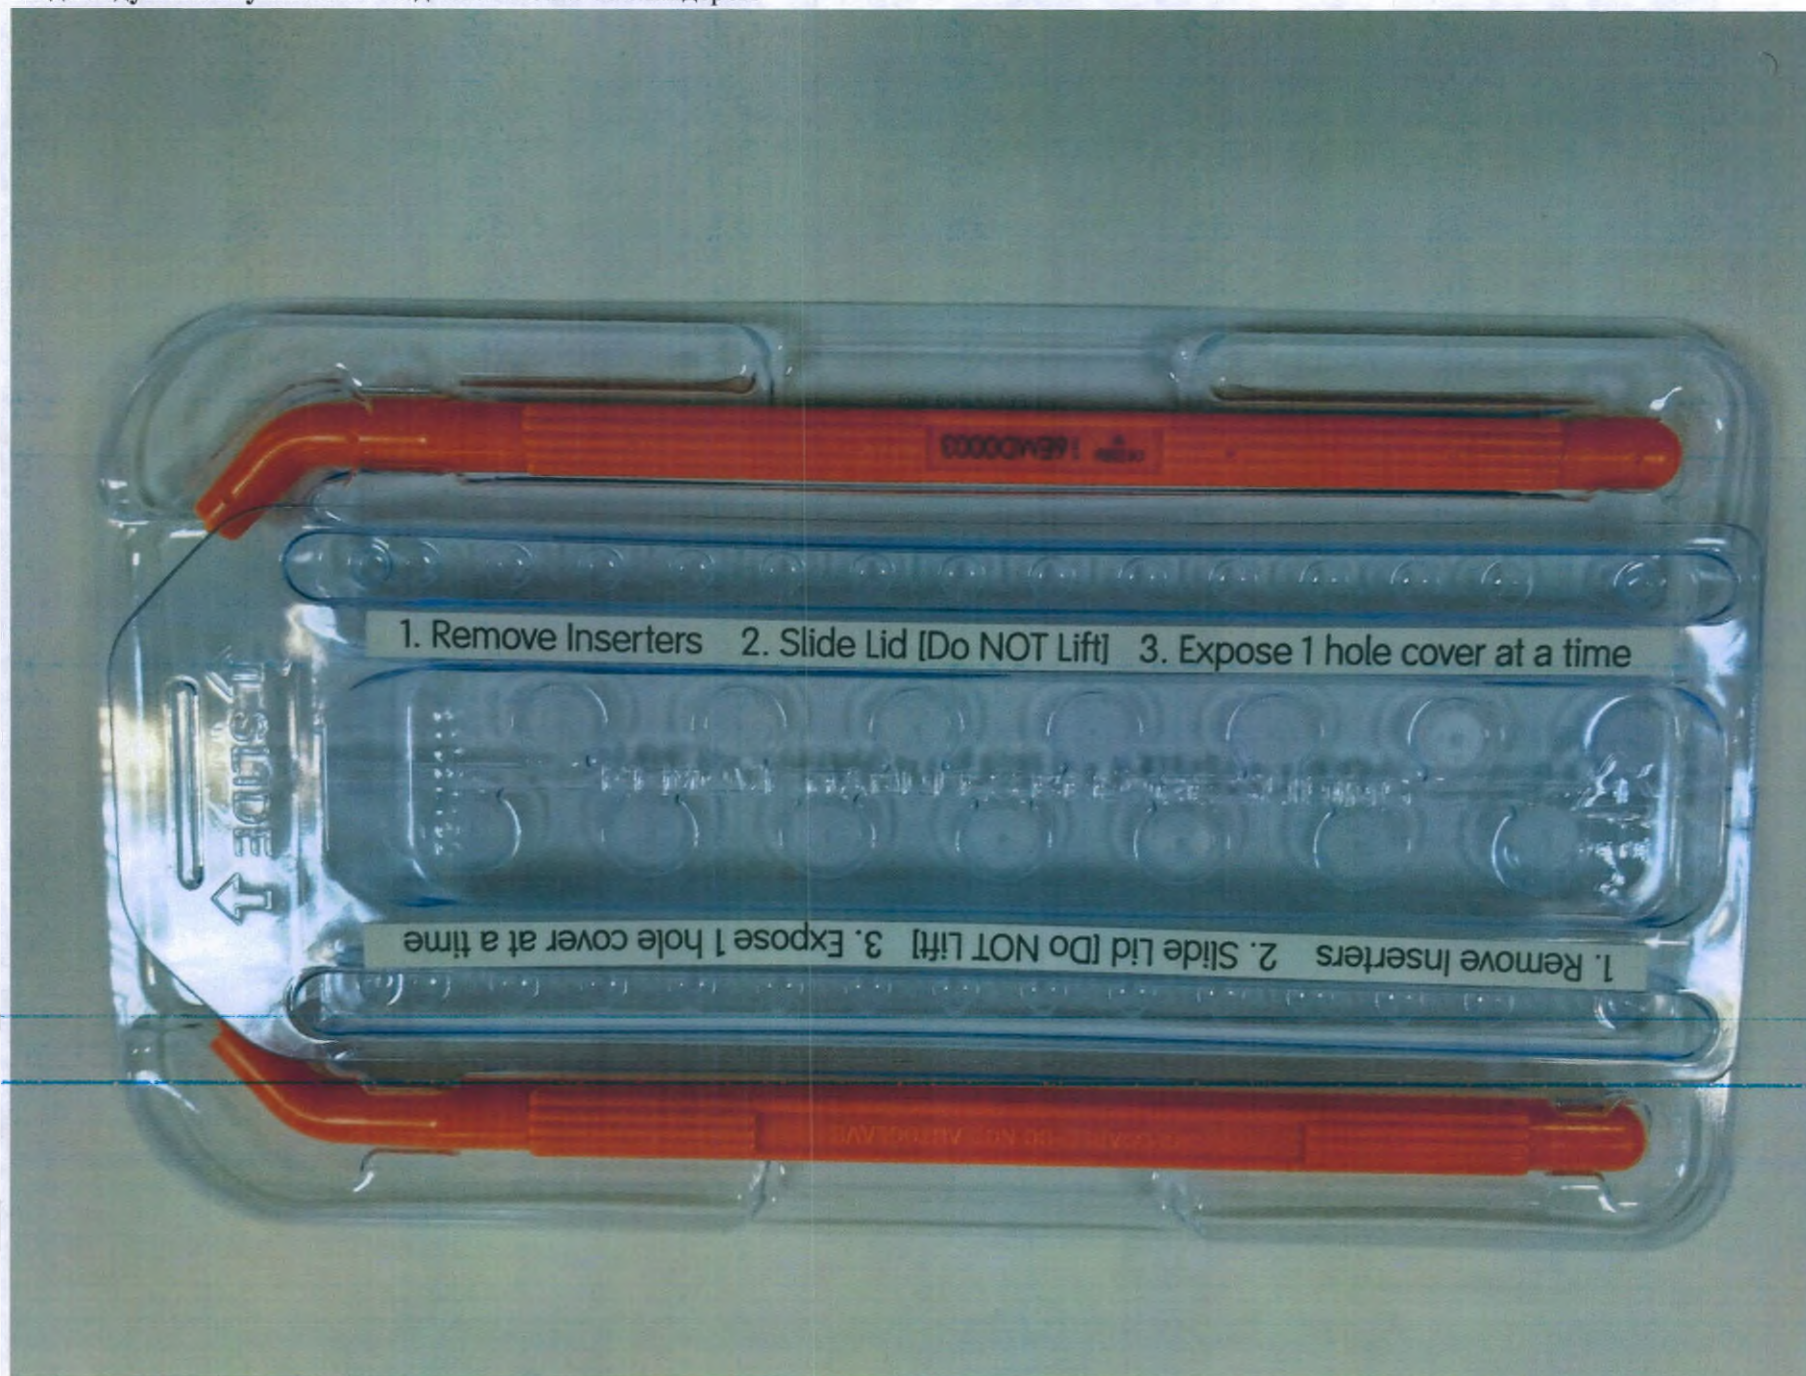



Индивидуальная упаковка: изделие во внутреннем пакете

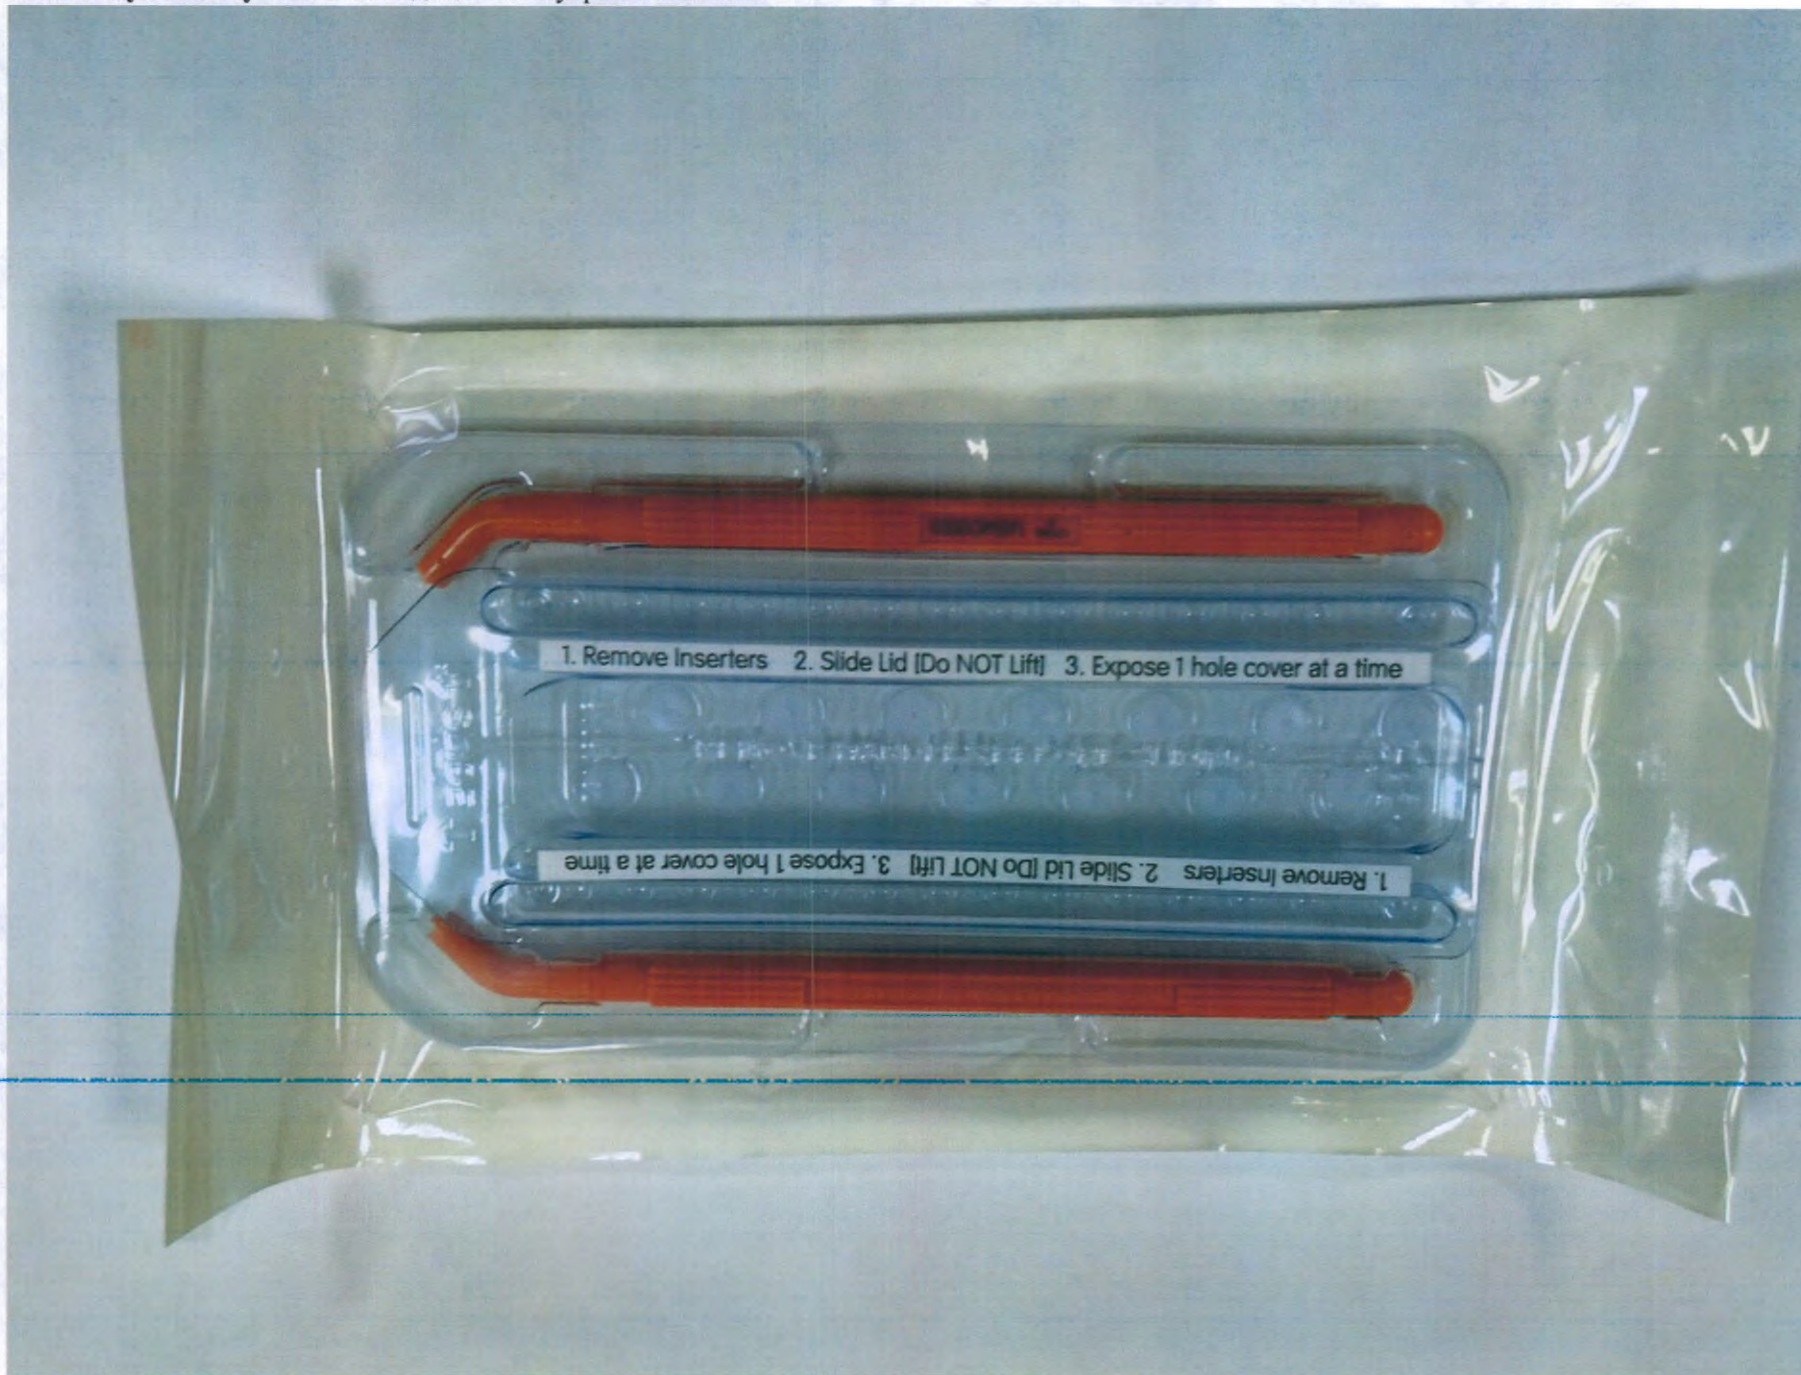

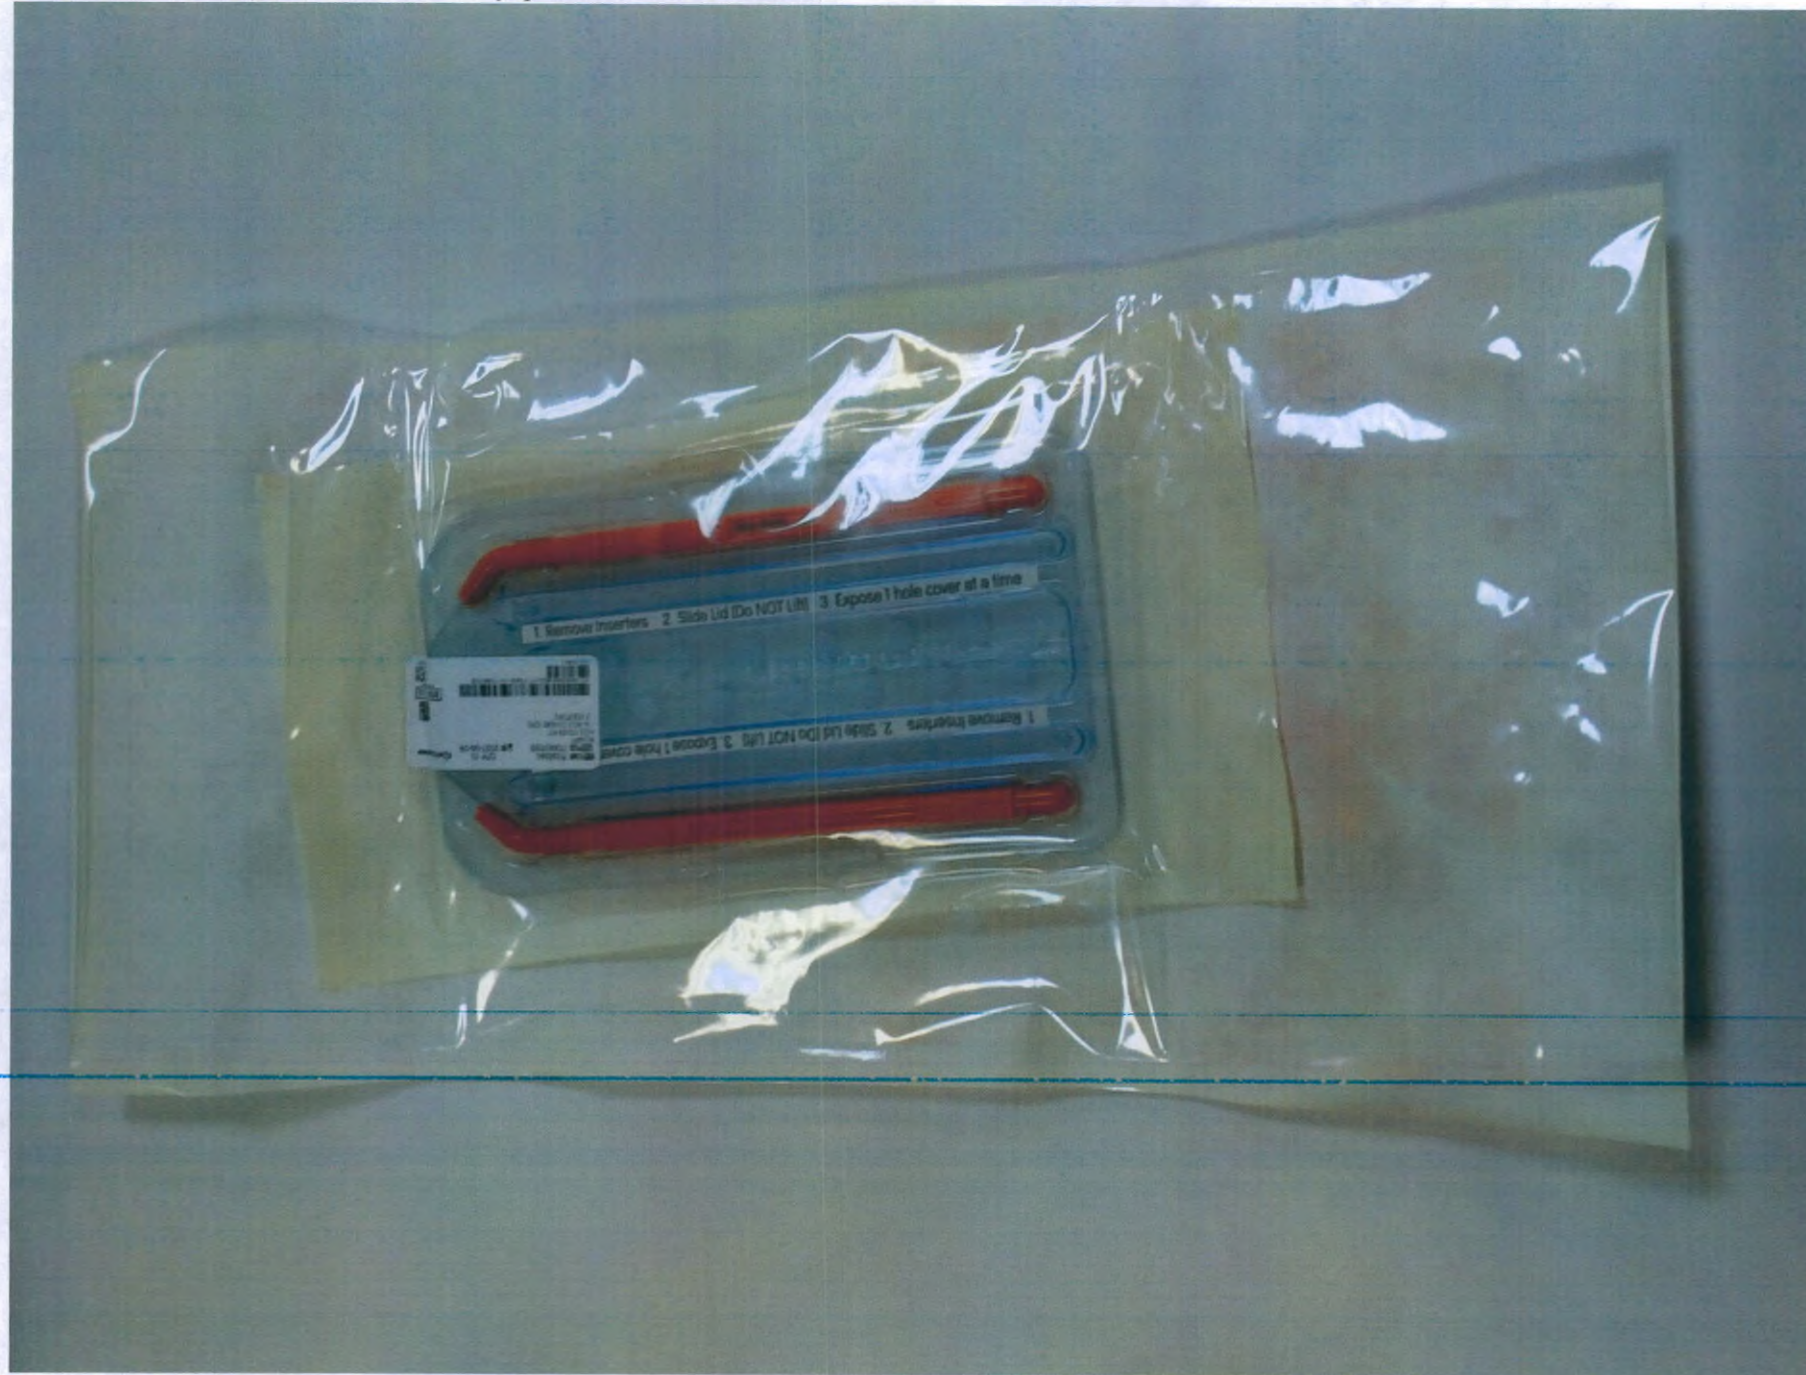

Индивидуальная упаковка: пакет внешний.

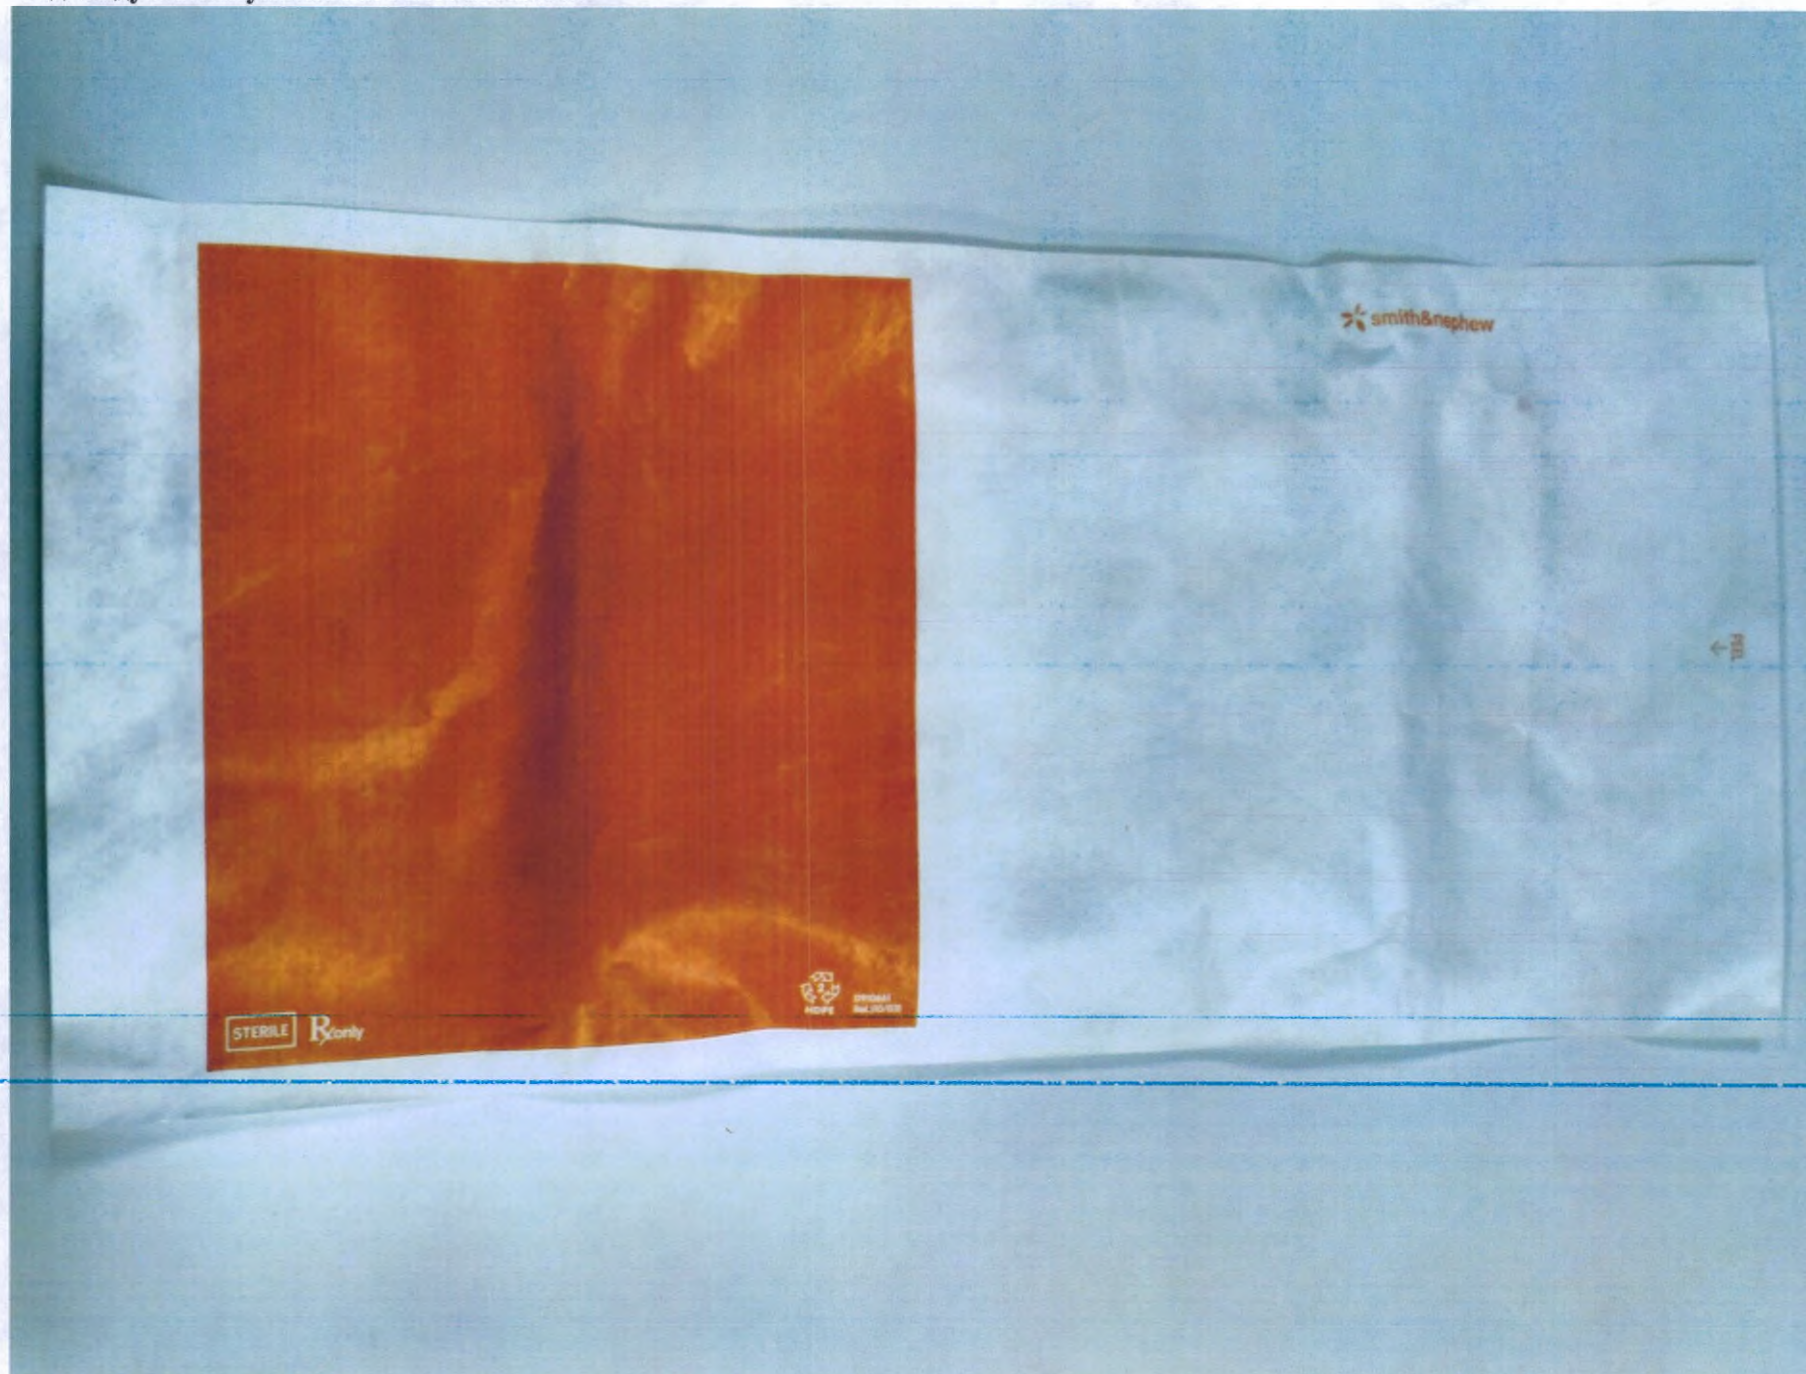

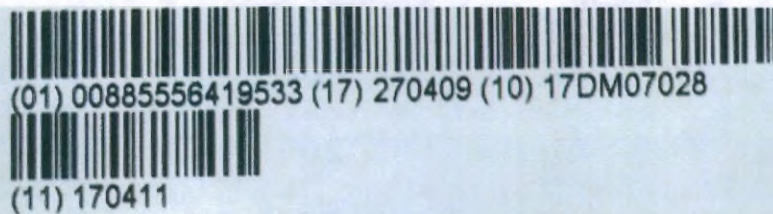

T94HSTIK; 4

ATTACH TO

CHART-STIK® LABEL

REF ID: A71354240


LOT BATCH CODE 17DM07028

REDAPT®
HOLE COVER KIT
- 14 HOLE COVERS (CPE)
- 2 INSERTERS

STERILE EO
ETO STERILIZED

smith&nephew

USE BY 2027-04-09

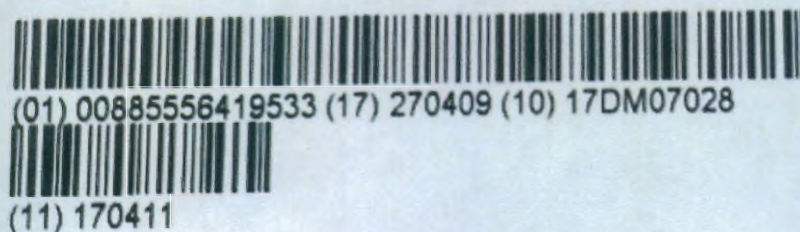

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF ID: A71354240

LOT BATCH CODE 17DM07028


REDAPT®
HOLE COVER KIT
- 14 HOLE COVERS (CPE)

STERILE EO
ETO STERILIZED

smith&nephew

USE BY 2027-04-09


NT'S RECORD

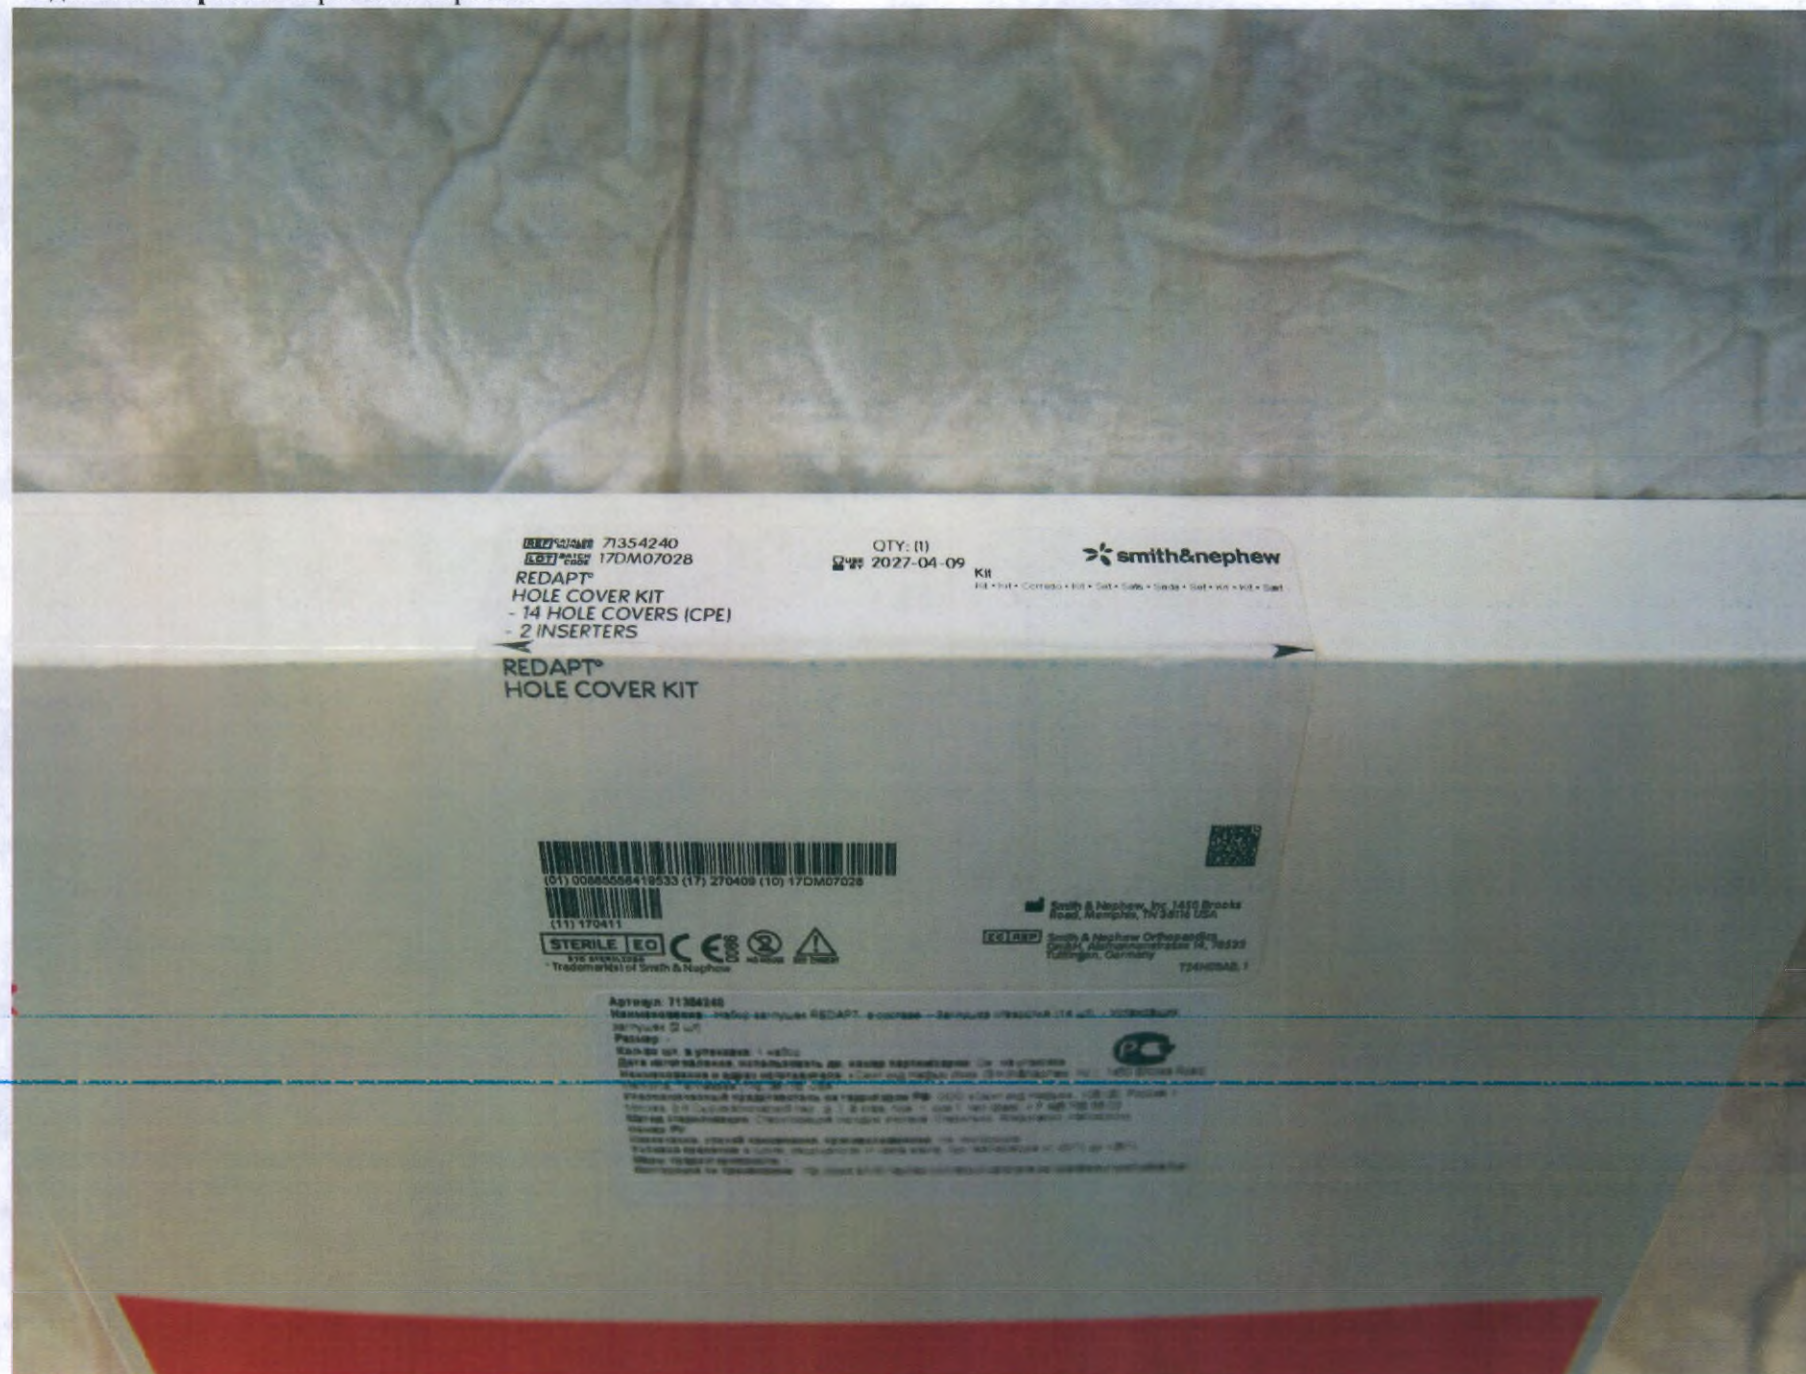






VI. Заглушки центрального отверстия чашки REFLECTION.



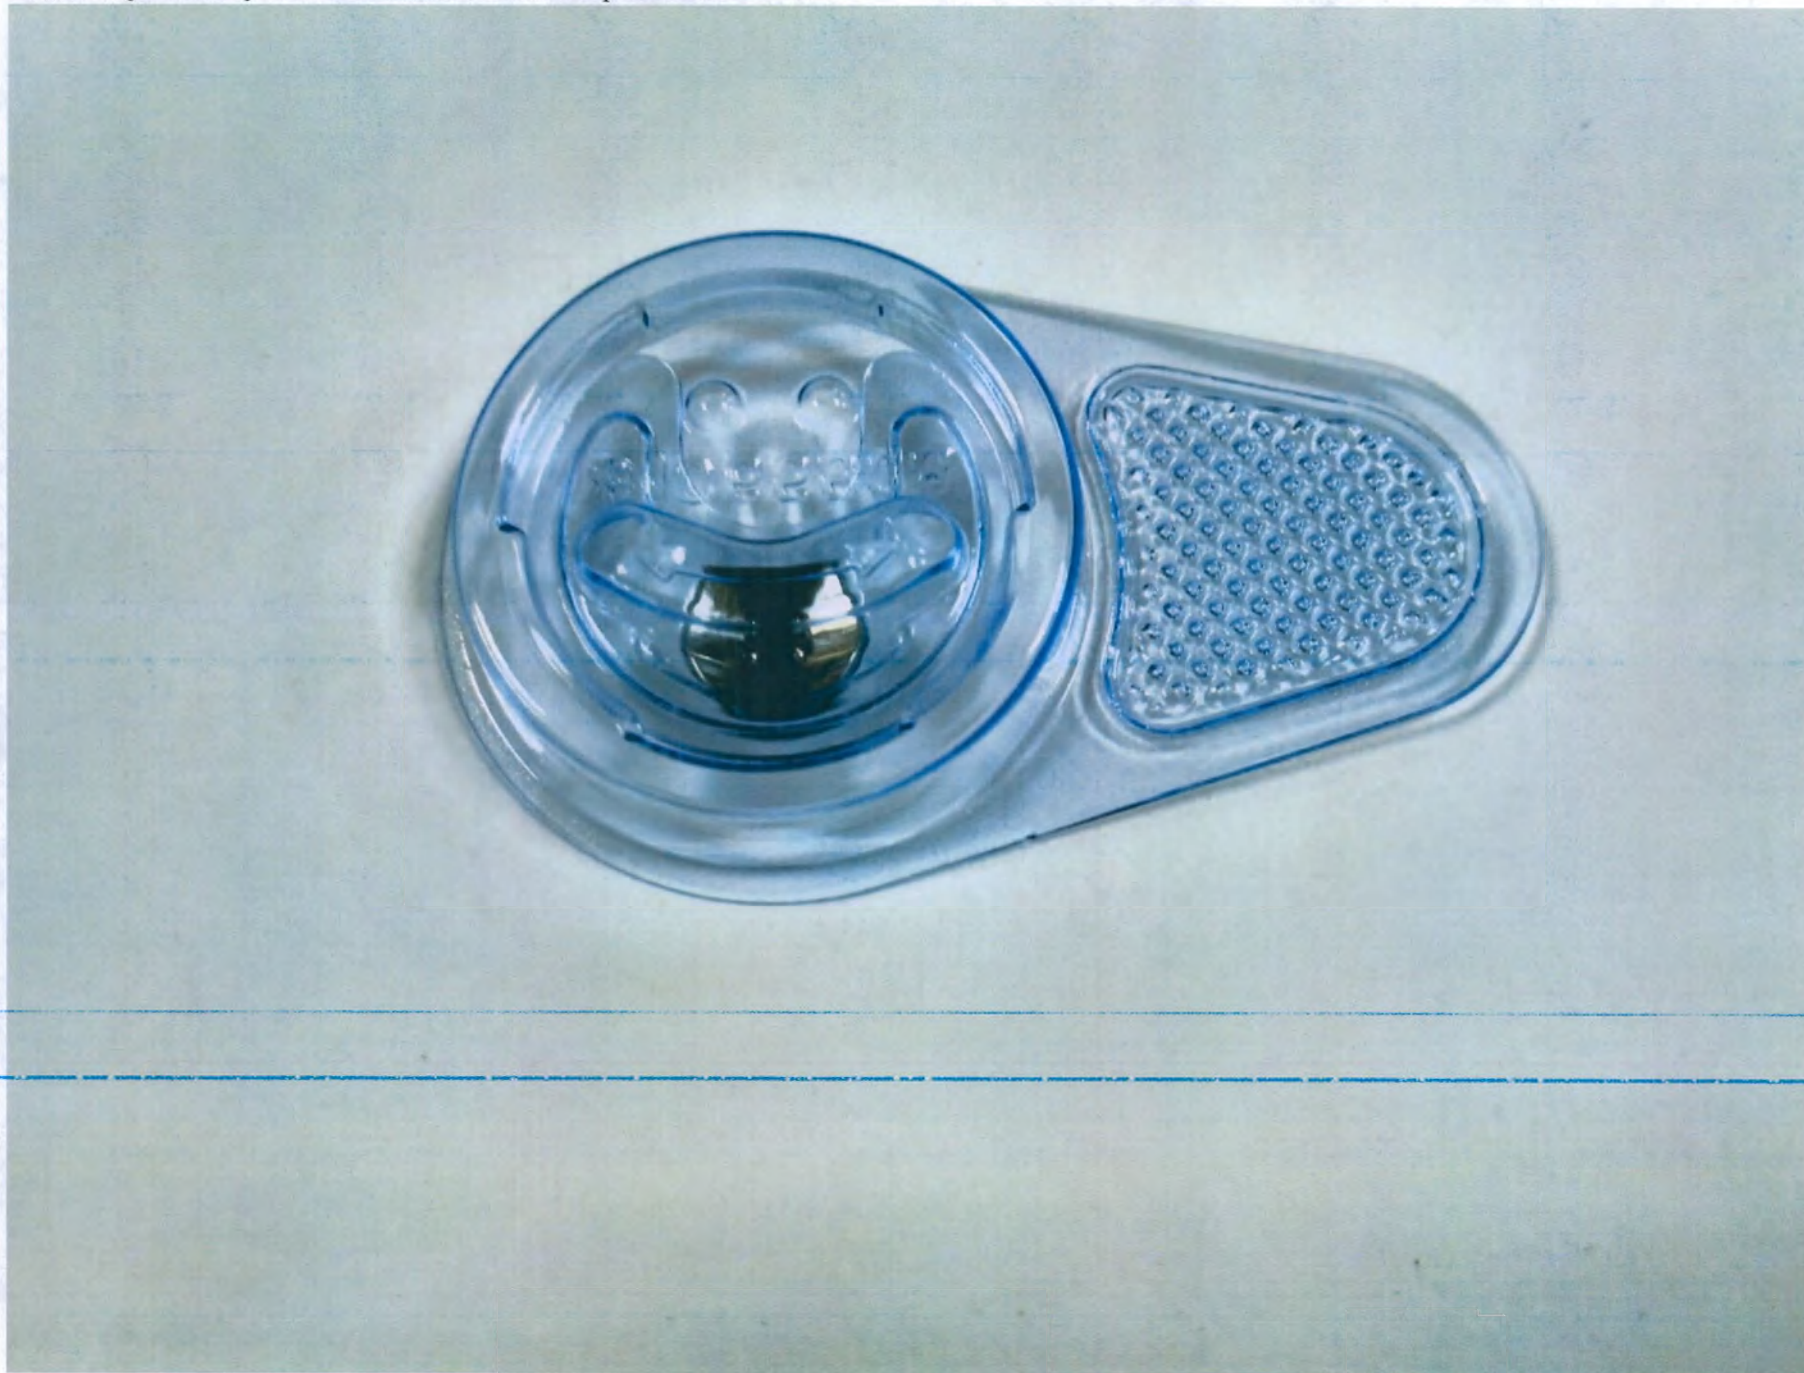

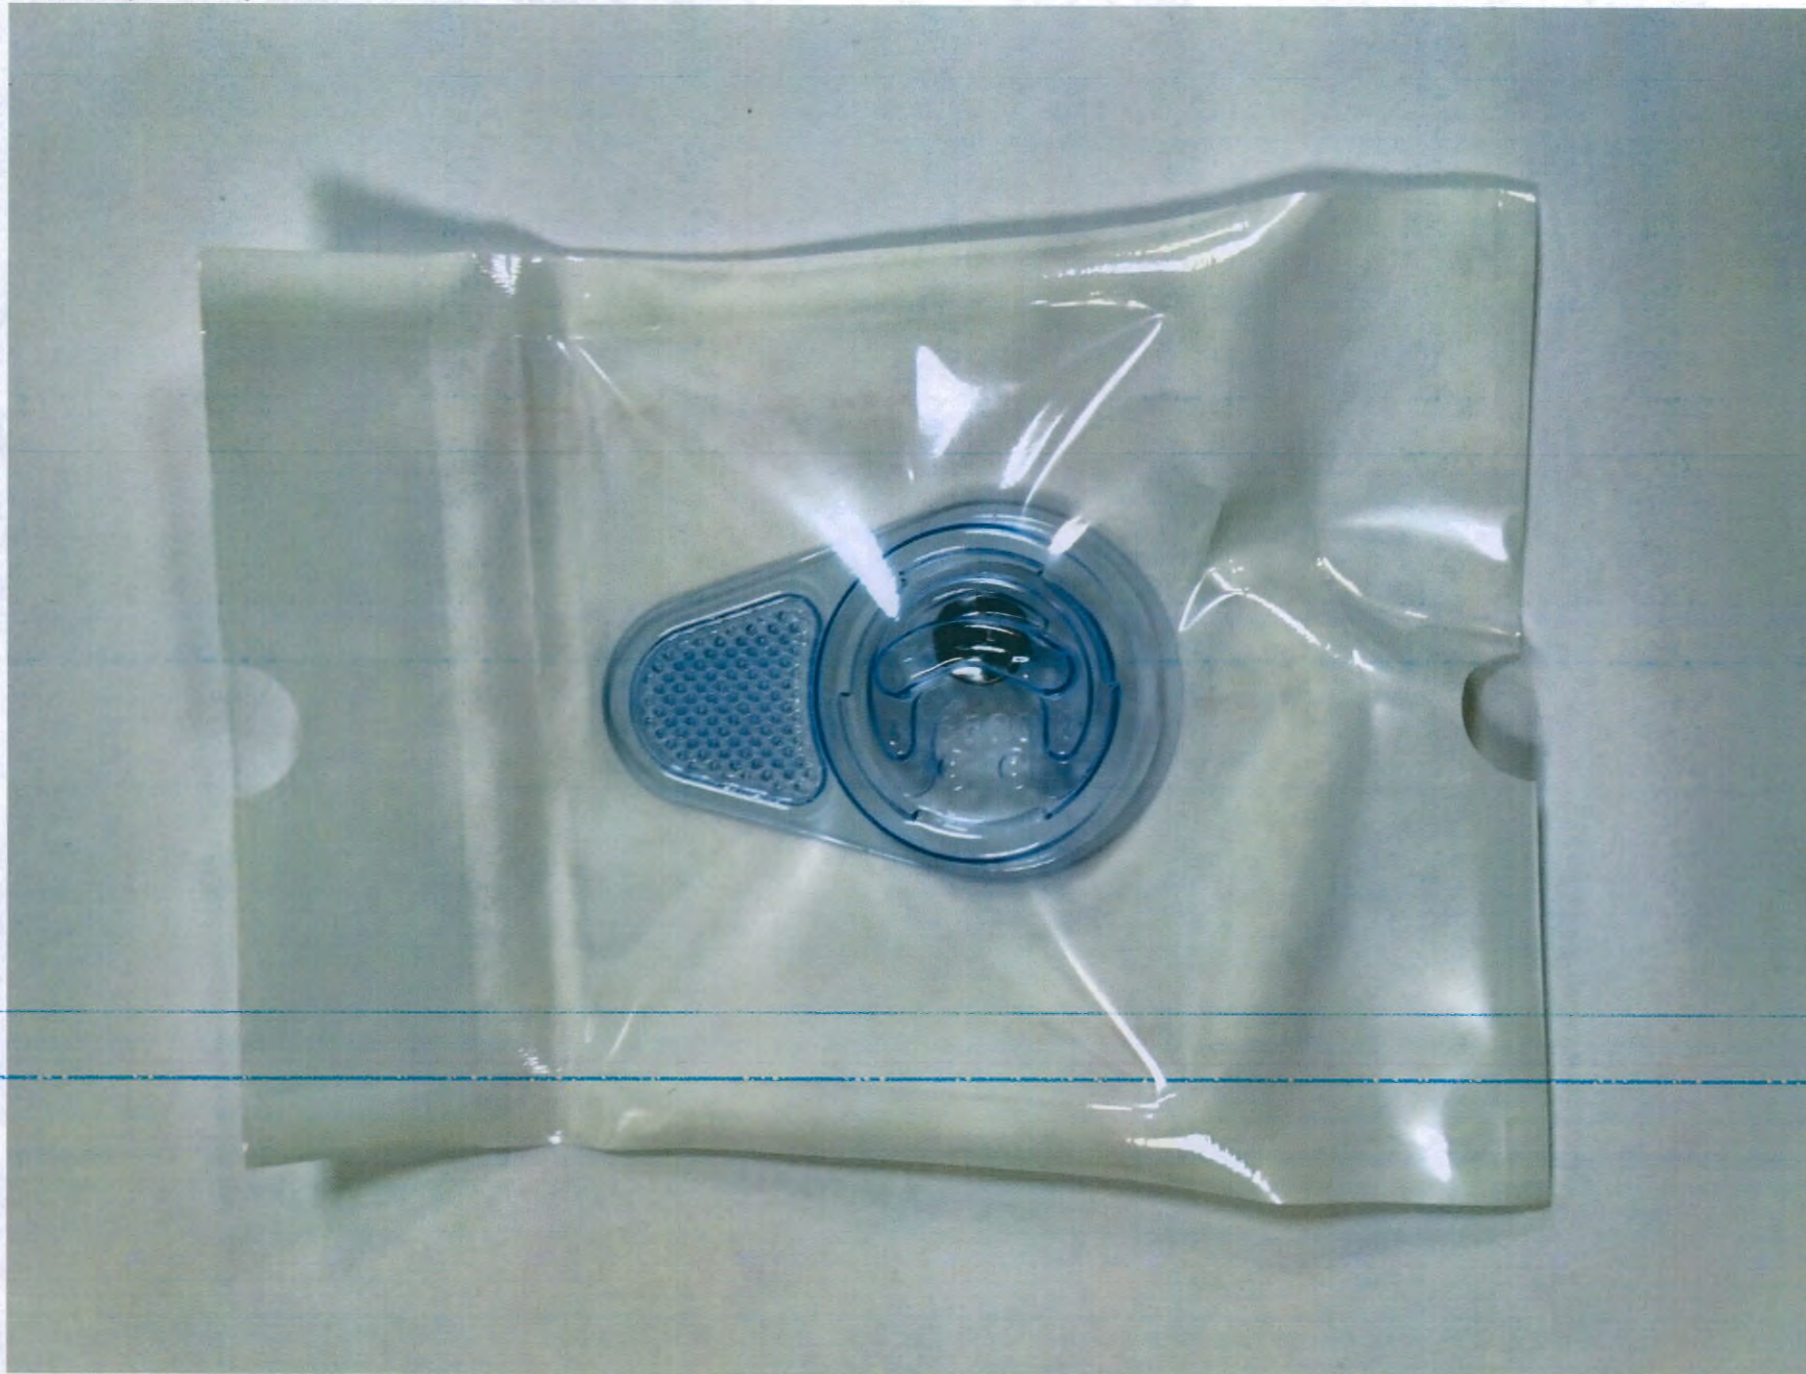


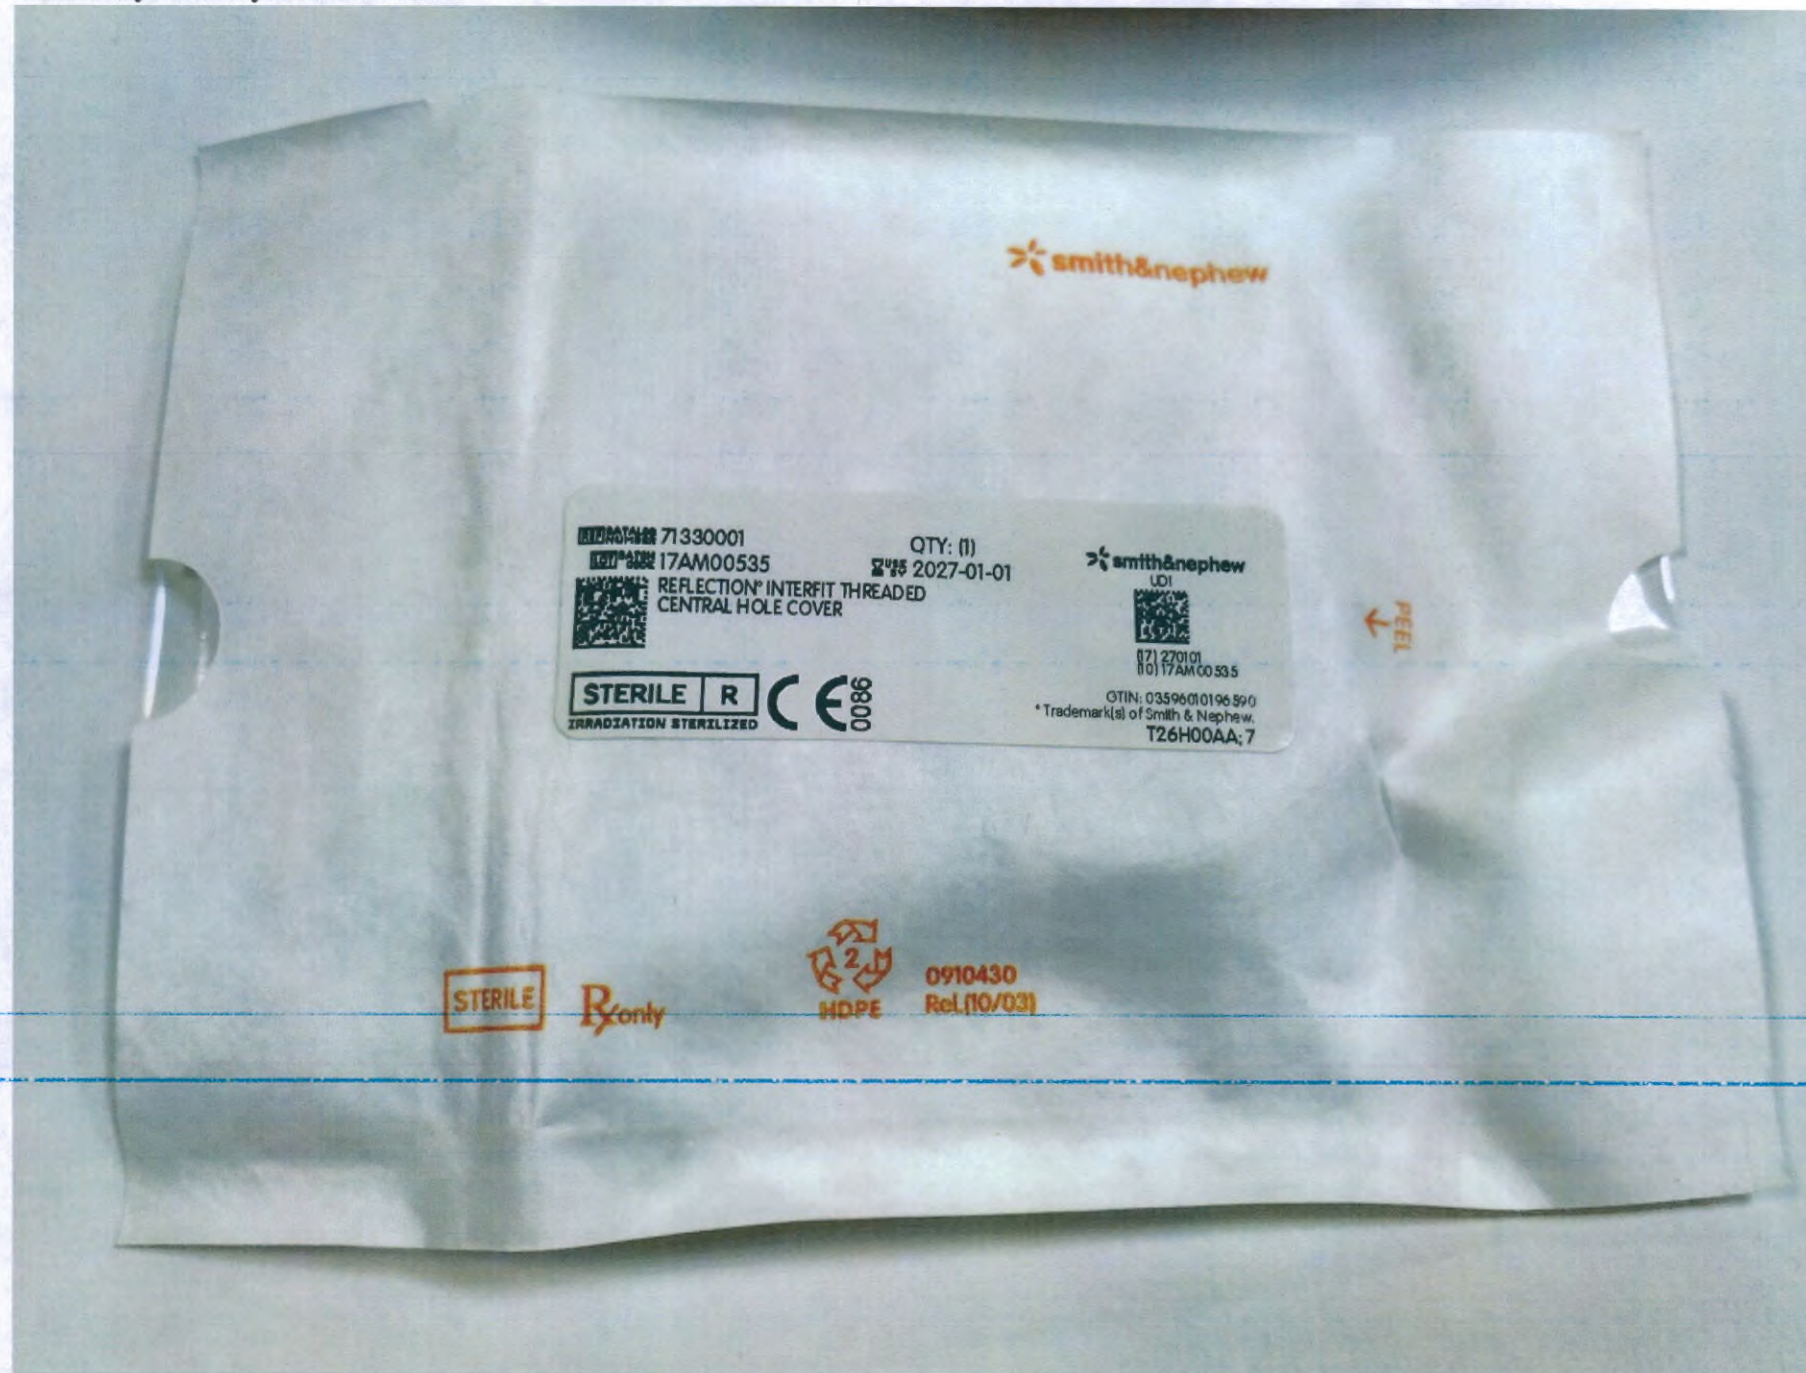

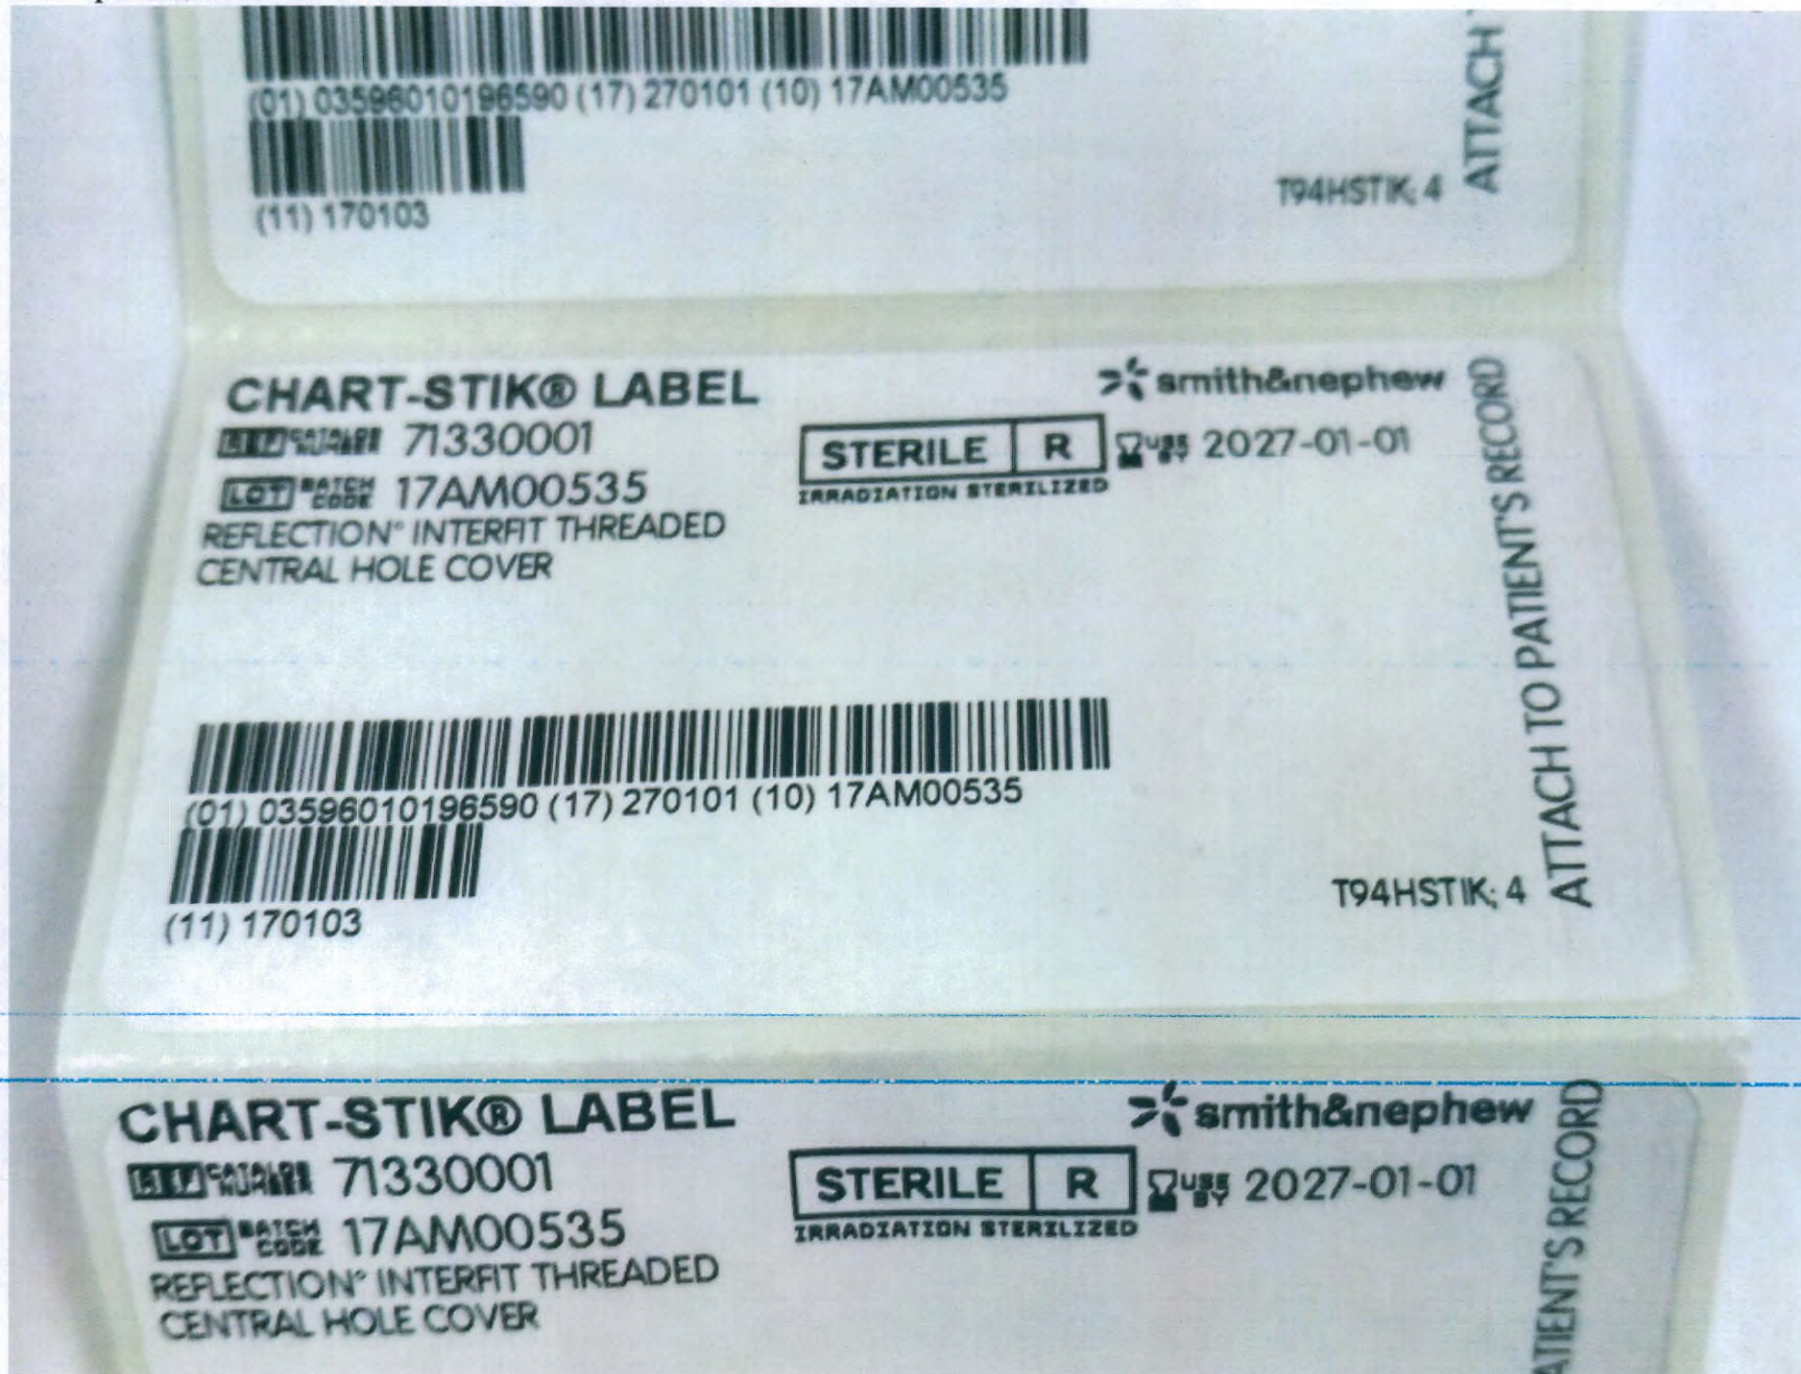




VII. Блоки замещающие REDAPT, на примере вариантов исполнения:
Блок замещающий REDAPT сегментарный, 56 x 12 мм

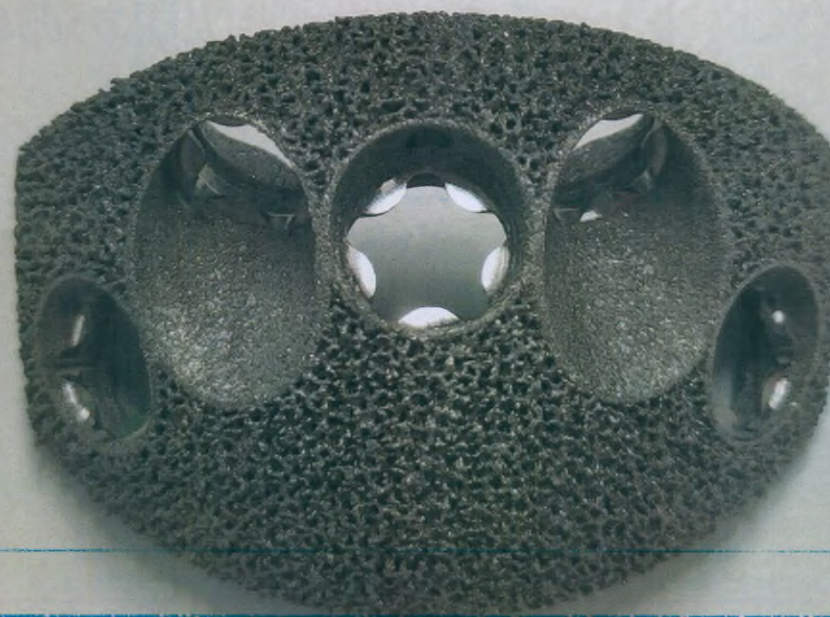


Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

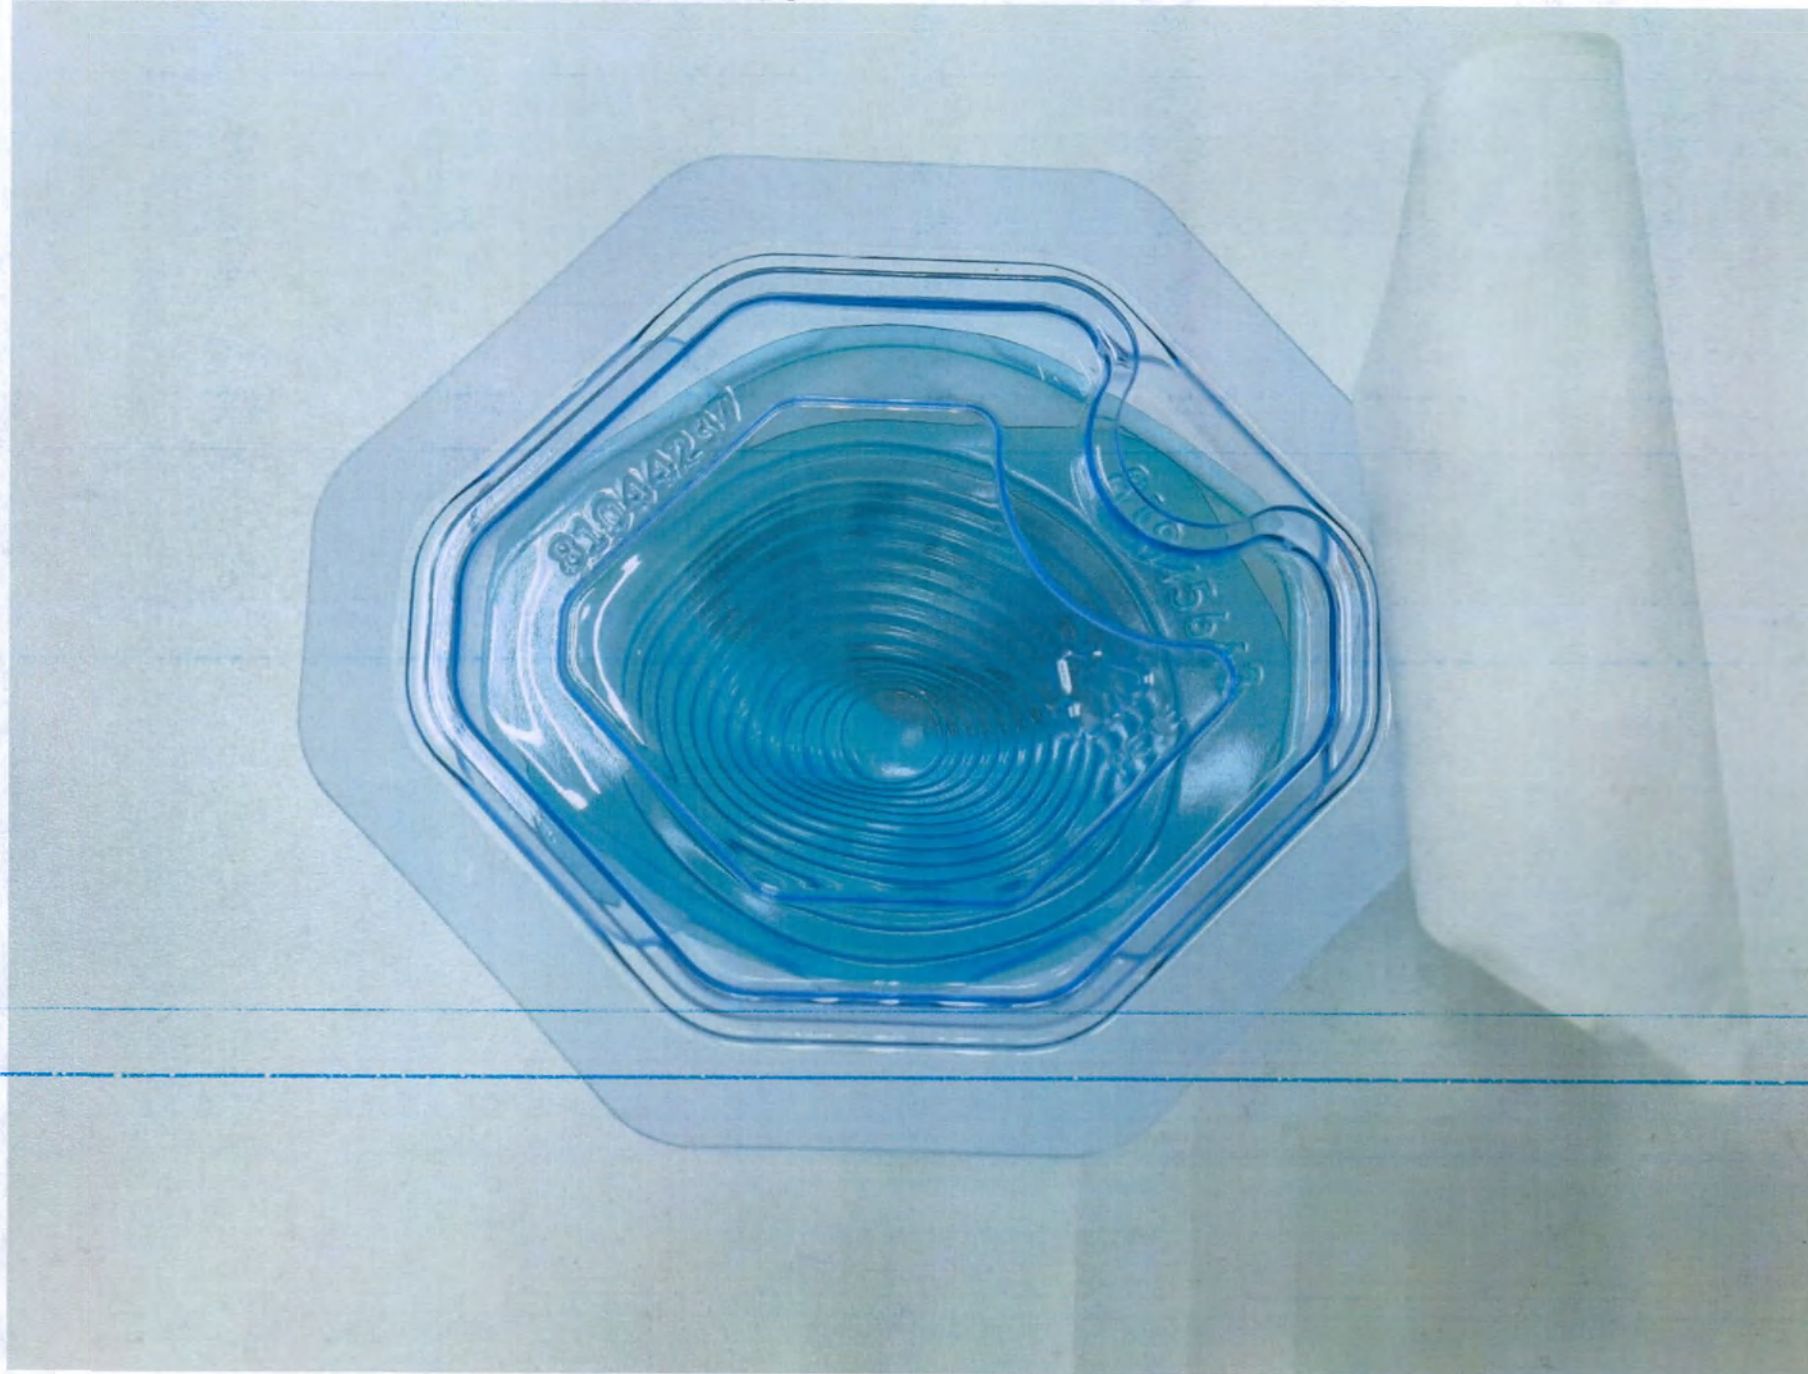

Индивидуальная упаковка: лоток внутренний.



Индивидуальная упаковка: лоток внутренний в лотке внешнем

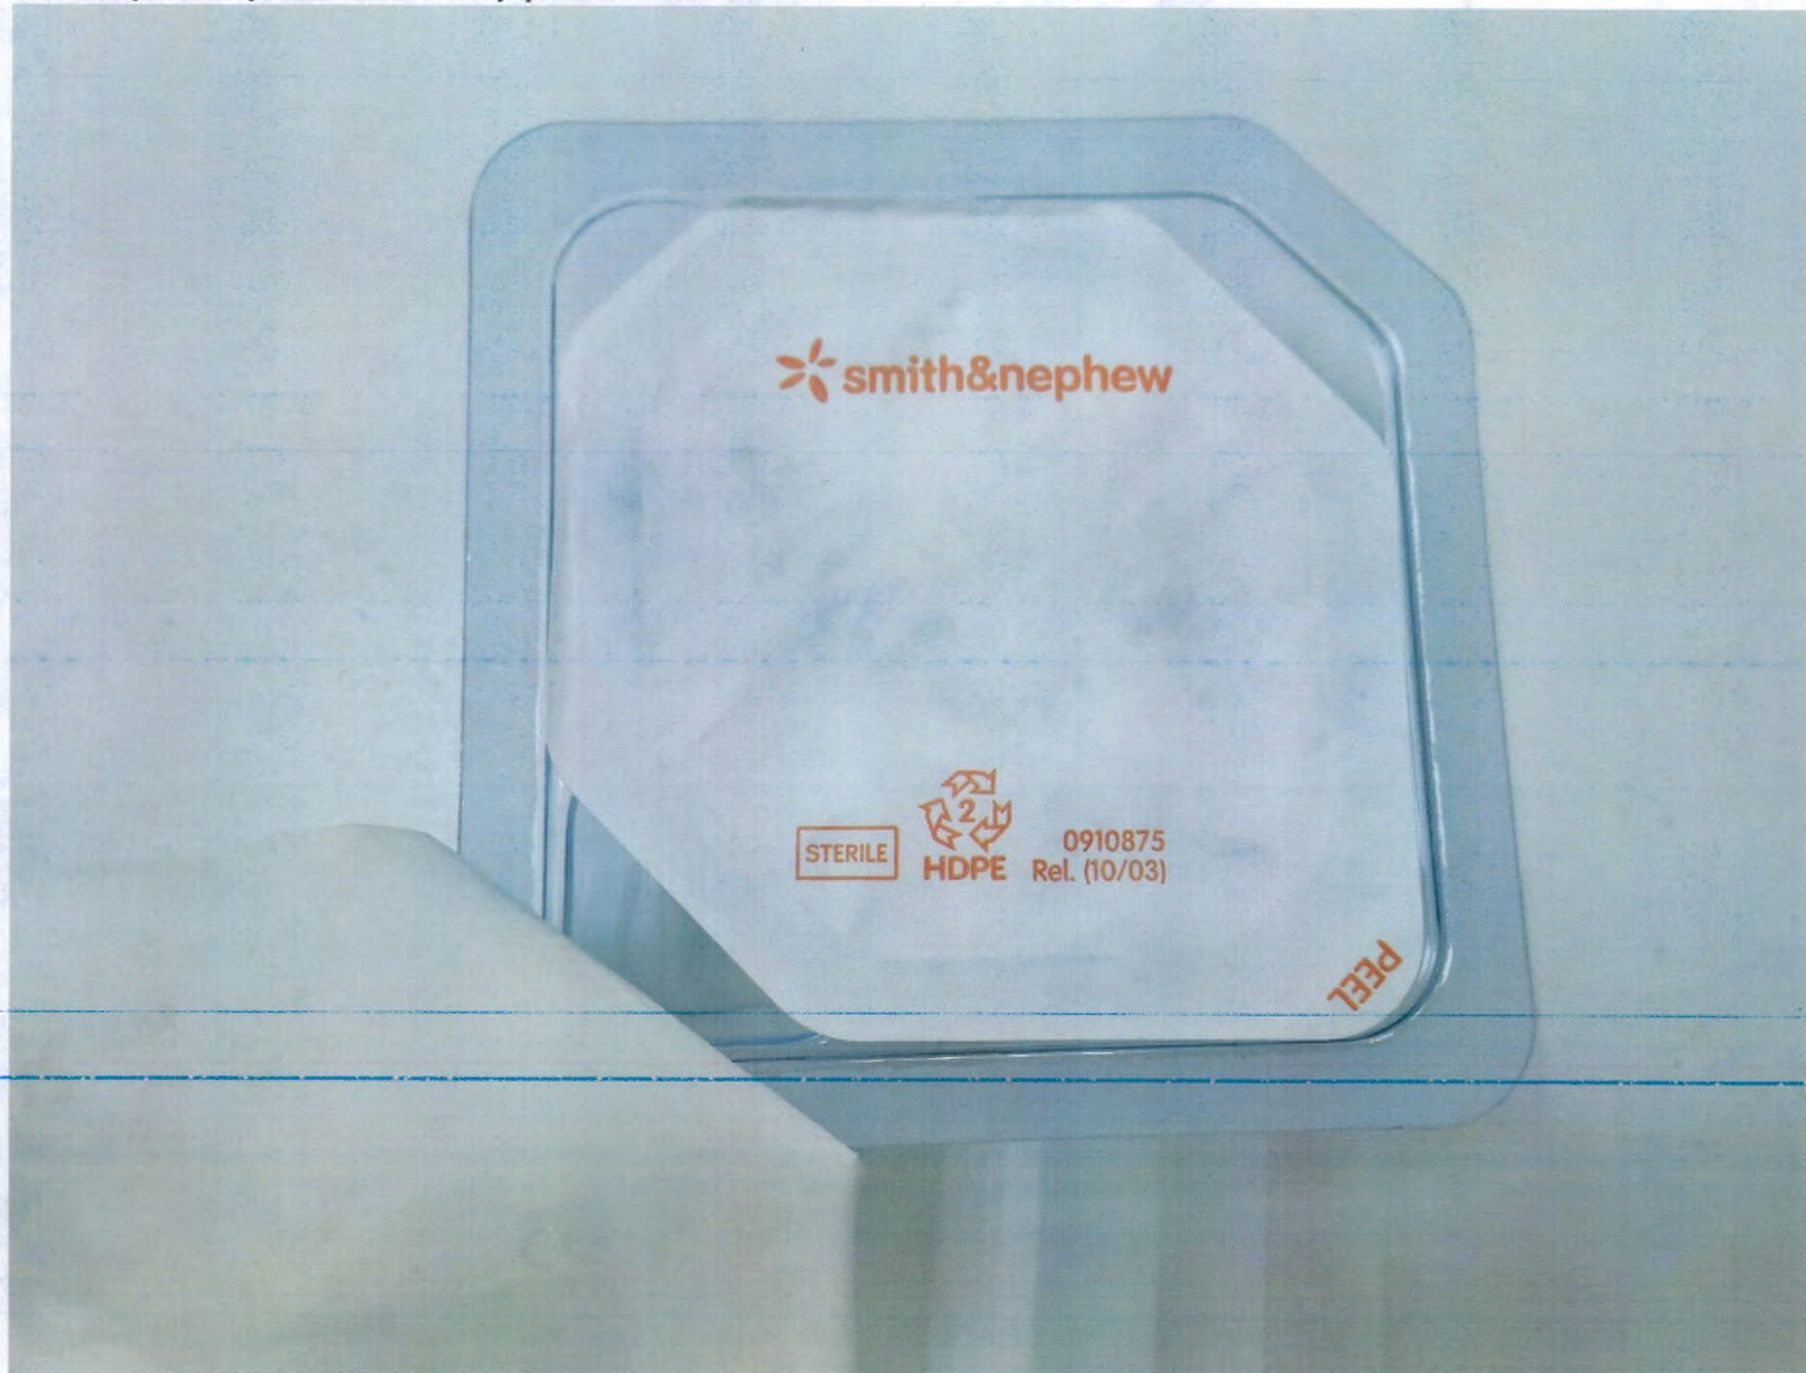

↓
PEEL


 smith&nephew

REF: 71354412
LOT: 18EM12599

QTY: (1)
EXP: 2028-05-13

 smith&nephew

REDAPT[®] SLICE AUGMENT
56 MM X 12 MM
Ti-6AL-4V


(01) 00885556685831 (17) 280513 (10) 18EM12599

(11) 180516



STERILE R
IRRADIATION STERILIZED

 0086
T94H00AL;1

STERILE

R_xonly



0910876
Rel. (10/03)

CHART-STIK® LABEL
 DEVIDUM 71354412
 LOT# 18EM12599
 REDAPT SLICE AUGMENT
 56 MM X 12 MM
 TI-4AL-4V
 (01) 0086556995931 (17) 280513 (10) 18EM12599
 (11) 180518

 TRANSTK 4
 ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL
 DEVIDUM 71354412
 LOT# 18EM12599
 REDAPT SLICE AUGMENT
 56 MM X 12 MM
 TI-4AL-4V
 (01) 0086556995931 (17) 280513 (10) 18EM12599
 (11) 180518

 TRANSTK 4
 ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL
 DEVIDUM 71354412
 LOT# 18EM12599
 REDAPT SLICE AUGMENT
 56 MM X 12 MM
 TI-4AL-4V
 (01) 0086556995931 (17) 280513 (10) 18EM12599
 (11) 180518

 TRANSTK 4
 ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL
 DEVIDUM 71354412
 LOT# 18EM12599
 REDAPT SLICE AUGMENT
 56 MM X 12 MM
 TI-4AL-4V
 (01) 0086556995931 (17) 280513 (10) 18EM12599
 (11) 180518

 TRANSTK 4
 ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL
 DEVIDUM 71354412
 LOT# 18EM12599
 REDAPT SLICE AUGMENT
 56 MM X 12 MM
 TI-4AL-4V
 (01) 0086556995931 (17) 280513 (10) 18EM12599
 (11) 180518

 TRANSTK 4
 ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL
 DEVIDUM 71354412
 LOT# 18EM12599
 REDAPT SLICE AUGMENT
 56 MM X 12 MM
 TI-4AL-4V
 (01) 0086556995931 (17) 280513 (10) 18EM12599
 (11) 180518

 TRANSTK 4
 ATTACH TO PATIENT'S RECORD

Instructions for Use

English

Gebrauchsanweisung

Total Hip Systems

CAUTION: Federal law (FDA) restricts the subject total hip orthopedic devices to sale by or on the order of a physician.

Device Descriptions

Total Hip Systems

The Total Hip Systems consist of femoral components, modular necks, proximal sleeves, taper sleeves, acetabular components, fixation screws and pegs, hole covers, contrainers, and femoral heads. Components may be grit blasted, porous coated, hydroxyapatite (HA) coated, or HA porous coated. All implantable devices are for single use only.

Materials

Femoral components are manufactured from cobalt chromium alloy, titanium 6Al-4V alloy, or stainless steel 316L. Femoral heads are manufactured from cobalt chromium alloy, COXINUM oxidized zirconium, BIOLOX forte alumina ceramic, BIOLOX delta alumina/zirconia ceramic, zirconia ceramic, or stainless steel. Acetabular liners are manufactured from ultra-high molecular weight polyethylene (UHMWPE), BIOLOX forte alumina ceramic, or BIOLOX delta alumina/zirconia ceramic. In the U.S., refer to the separate package insert provided with the ceramic acetabular liners. All poly acetabular components are manufactured from UHMWPE. Acetabular shells are manufactured from titanium 6Al-4V alloy or cobalt chromium (CoCr) alloy. BIONICGRAM HA® acetabular cups are cobalt chromium (CoCr) alloy. The components material is provided on the outside carton label. Note: BIOLOX delta ceramic liners are not available for use in the U.S.

Some of the alloys needed to produce orthopedic implants contain metallic components that may be carcinogenic in tissue cultures or in an intact organism under very unique circumstances. Questions have been raised in the scientific literature as to whether or not these alloys may be carcinogenic in implant recipients. Studies conducted to evaluate this issue have not identified conclusive evidence of such phenomenon, in spite of the millions of implants in use.

Femoral Components

Femoral components are available in a variety of sizes. Porous coated components are coated for biological ingrowth and are intended for use without cement. Modular femoral components are available with an oval taper to accept Smith & Nephew CoCr modular necks and/or a Morse-type taper to accept proximal sleeves. Non-porous femoral components can feature polyethylene/methylene (PMMA) cementations that help produce a uniform cement thickness.

Femoral components, available with 12/14, 12/14, and 14/16 tapers, mate and lock directly with Smith & Nephew femoral heads having the same size taper. Certain femoral heads may require taper sleeves for attachment to the femoral stem taper. Refer to the table in the taper sleeves section for details.

Taper Sleeves

A taper sleeve may be required when mating femoral stems with specific types of femoral heads. Refer to the sleeve compatibility table for the appropriate combinations. Failure to utilize the proper sleeve to head combination may lead to implant failure and may result in revision surgery. Never place more than one taper sleeve on a femoral component. This combination will increase stresses on the implant and may lead to failure and may result in revision surgery.

Modular Necks

Modular necks are made from CoCr alloy and are available in a variety of configurations. The modular neck mates and locks with the oval taper of a modular femoral component on one end and the taper of a 12/14 femoral head on the other end.

Compatible Sleeve Combinations

Femoral Stem Taper	40, 44 mm COXINUM Modular Heads	40, 44 mm COCr Modular Heads	BH Modular CoCr Heads	DANDEL® CoCr & COXINUM Unipolar Heads	14/16 COXINUM and CoCr Heads
12/14	A	A	B	B	C
14/16	-	-	-	D	No sleeve required
12/12	-	-	-	E	F

* Modular CoCr heads are made from CoCr alloy and are intended for noncemented use in the U.S. Refer to the separate package insert provided with the components.

** In the U.S., modular heads are not available for use in the U.S. These heads can only be used with cemented acetabular components.

Sleeve	Material	Description/Part Numbers
A	Ti-6Al-4V	12/14 Modular Sleeve + 7324414, + 7324415, + 7324416, + 7324417, + 7324418, + 7324419, + 7324420, + 7324421, + 7324422, + 7324423, + 7324424, + 7324425, + 7324426, + 7324427, + 7324428, + 7324429, + 7324430, + 7324431, + 7324432, + 7324433, + 7324434, + 7324435, + 7324436, + 7324437, + 7324438, + 7324439, + 7324440, + 7324441, + 7324442, + 7324443, + 7324444, + 7324445, + 7324446, + 7324447, + 7324448, + 7324449, + 7324450, + 7324451, + 7324452, + 7324453, + 7324454, + 7324455, + 7324456, + 7324457, + 7324458, + 7324459, + 7324460, + 7324461, + 7324462, + 7324463, + 7324464, + 7324465, + 7324466, + 7324467, + 7324468, + 7324469, + 7324470, + 7324471, + 7324472, + 7324473, + 7324474, + 7324475, + 7324476, + 7324477, + 7324478, + 7324479, + 7324480, + 7324481, + 7324482, + 7324483, + 7324484, + 7324485, + 7324486, + 7324487, + 7324488, + 7324489, + 7324490, + 7324491, + 7324492, + 7324493, + 7324494, + 7324495, + 7324496, + 7324497, + 7324498, + 7324499, + 7324500, + 7324501, + 7324502, + 7324503, + 7324504, + 7324505, + 7324506, + 7324507, + 7324508, + 7324509, + 7324510, + 7324511, + 7324512, + 7324513, + 7324514, + 7324515, + 7324516, + 7324517, + 7324518, + 7324519, + 7324520, + 7324521, + 7324522, + 7324523, + 7324524, + 7324525, + 7324526, + 7324527, + 7324528, + 7324529, + 7324530, + 7324531, + 7324532, + 7324533, + 7324534, + 7324535, + 7324536, + 7324537, + 7324538, + 7324539, + 7324540, + 7324541, + 7324542, + 7324543, + 7324544, + 7324545, + 7324546, + 7324547, + 7324548, + 7324549, + 7324550, + 7324551, + 7324552, + 7324553, + 7324554, + 7324555, + 7324556, + 7324557, + 7324558, + 7324559, + 7324560, + 7324561, + 7324562, + 7324563, + 7324564, + 7324565, + 7324566, + 7324567, + 7324568, + 7324569, + 7324570, + 7324571, + 7324572, + 7324573, + 7324574, + 7324575, + 7324576, + 7324577, + 7324578, + 7324579, + 7324580, + 7324581, + 7324582, + 7324583, + 7324584, + 7324585, + 7324586, + 7324587, + 7324588, + 7324589, + 7324590, + 7324591, + 7324592, + 7324593, + 7324594, + 7324595, + 7324596, + 7324597, + 7324598, + 7324599, + 7324600, + 7324601, + 7324602, + 7324603, + 7324604, + 7324605, + 7324606, + 7324607, + 7324608, + 7324609, + 7324610, + 7324611, + 7324612, + 7324613, + 7324614, + 7324615, + 7324616, + 7324617, + 7324618, + 7324619, + 7324620, + 7324621, + 7324622, + 7324623, + 7324624, + 7324625, + 7324626, + 7324627, + 7324628, + 7324629, + 7324630, + 7324631, + 7324632, + 7324633, + 7324634, + 7324635, + 7324636, + 7324637, + 7324638, + 7324639, + 7324640, + 7324641, + 7324642, + 7324643, + 7324644, + 7324645, + 7324646, + 7324647, + 7324648, + 7324649, + 7324650, + 7324651, + 7324652, + 7324653, + 7324654, + 7324655, + 7324656, + 7324657, + 7324658, + 7324659, + 7324660, + 7324661, + 7324662, + 7324663, + 7324664, + 7324665, + 7324666, + 7324667, + 7324668, + 7324669, + 7324670, + 7324671, + 7324672, + 7324673, + 7324674, + 7324675, + 7324676, + 7324677, + 7324678, + 7324679, + 7324680, + 7324681, + 7324682, + 7324683, + 7324684, + 7324685, + 7324686, + 7324687, + 7324688, + 7324689, + 7324690, + 7324691, + 7324692, + 7324693, + 7324694, + 7324695, + 7324696, + 7324697, + 7324698, + 7324699, + 7324700, + 7324701, + 7324702, + 7324703, + 7324704, + 7324705, + 7324706, + 7324707, + 7324708, + 7324709, + 7324710, + 7324711, + 7324712, + 7324713, + 7324714, + 7324715, + 7324716, + 7324717, + 7324718, + 7324719, + 7324720, + 7324721, + 7324722, + 7324723, + 7324724, + 7324725, + 7324726, + 7324727, + 7324728, + 7324729, + 7324730, + 7324731, + 7324732, + 7324733, + 7324734, + 7324735, + 7324736, + 7324737, + 7324738, + 7324739, + 7324740, + 7324741, + 7324742, + 7324743, + 7324744, + 7324745, + 7324746, + 7324747, + 7324748, + 7324749, + 7324750, + 7324751, + 7324752, + 7324753, + 7324754, + 7324755, + 7324756, + 7324757, + 7324758, + 7324759, + 7324760, + 7324761, + 7324762, + 7324763, + 7324764, + 7324765, + 7324766, + 7324767, + 7324768, + 7324769, + 7324770, + 7324771, + 7324772, + 7324773, + 7324774, + 7324775, + 7324776, + 7324777, + 7324778, + 7324779, + 7324780, + 7324781, + 7324782, + 7324783, + 7324784, + 7324785, + 7324786, + 7324787, + 7324788, + 7324789, + 7324790, + 7324791, + 7324792, + 7324793, + 7324794, + 7324795, + 7324796, + 7324797, + 7324798, + 7324799, + 7324800, + 7324801, + 7324802, + 7324803, + 7324804, + 7324805, + 7324806, + 7324807, + 7324808, + 7324809, + 7324810, + 7324811, + 7324812, + 7324813, + 7324814, + 7324815, + 7324816, + 7324817, + 7324818, + 7324819, + 7324820, + 7324821, + 7324822, + 7324823, + 7324824, + 7324825, + 7324826, + 7324827, + 7324828, + 7324829, + 7324830, + 7324831, + 7324832, + 7324833, + 7324834, + 7324835, + 7324836, + 7324837, + 7324838, + 7324839, + 7324840, + 7324841, + 7324842, + 7324843, + 7324844, + 7324845, + 7324846, + 7324847, + 7324848, + 7324849, + 7324850, + 7324851, + 7324852, + 7324853, + 7324854, + 7324855, + 7324856, + 7324857, + 7324858, + 7324859, + 7324860, + 7324861, + 7324862, + 7324863, + 7324864, + 7324865, + 7324866, + 7324867, + 7324868, + 7324869, + 7324870, + 7324871, + 7324872, + 7324873, + 7324874, + 7324875, + 7324876, + 7324877, + 7324878, + 7324879, + 7324880, + 7324881, + 7324882, + 7324883, + 7324884, + 7324885, + 7324886, + 7324887, + 7324888, + 7324889, + 7324890, + 7324891, + 7324892, + 7324893, + 7324894, + 7324895, + 7324896, + 7324897, + 7324898, + 7324899, + 7324900, + 7324901, + 7324902, + 7324903, + 7324904, + 7324905, + 7324906, + 7324907, + 7324908, + 7324909, + 7324910, + 7324911, + 7324912, + 7324913, + 7324914, + 7324915, + 7324916, + 7324917, + 7324918, + 7324919, + 7324920, + 7324921, + 7324922, + 7324923, + 7324924, + 7324925, + 7324926, + 7324927, + 7324928, + 7324929, + 7324930, + 7324931, + 7324932, + 7324933, + 7324934, + 7324935, + 7324936, + 7324937, + 7324938, + 7324939, + 7324940, + 7324941, + 7324942, + 7324943, + 7324944, + 7324945, + 7324946, + 7324947, + 7324948, + 7324949, + 7324950, + 7324951, + 7324952, + 7324953, + 7324954, + 7324955, + 7324956, + 7324957, + 7324958, + 7324959, + 7324960, + 7324961, + 7324962, + 7324963, + 7324964, + 7324965, + 7324966, + 7324967, + 7324968, + 7324969, + 7324970, + 7324971, + 7324972, + 7324973, + 7324974, + 7324975, + 7324976, + 7324977, + 7324978, + 7324979, + 7324980, + 7324981, + 7324982, + 7324983, + 7324984, + 7324985, + 7324986, + 7324987, + 7324988, + 7324989, + 7324990, + 7324991, + 7324992, + 7324993, + 7324994, + 7324995, + 7324996, + 7324997, + 7324998, + 7324999, + 7325000, + 7325001, + 7325002, + 7325003, + 7325004, + 7325005, + 7325006, + 7325007, + 7325008, + 7325009, + 7325010, + 7325011, + 7325012, + 7325013, + 7325014, + 7325015, + 7325016, + 7325017, + 7325018, + 7325019, + 7325020, + 7325021, + 7325022, + 7325023, + 7325024, + 7325025, + 7325026, + 7325027, + 7325028, + 7325029, + 7325030, + 7325031, + 7325032, + 7325033, + 7325034, + 7325035, + 7325036, + 7325037, + 7325038, + 7325039, + 7325040, + 7325041, + 7325042, + 7325043, + 7325044, + 7325045, + 7325046, + 7325047, + 7325048, + 7325049, + 7325050, + 7325051, + 7325052, + 7325053, + 7325054, + 7325055, + 7325056, + 7325057, + 7325058, + 7325059, + 7325060, + 7325061, + 7325062, + 7325063, + 7325064, + 7325065, + 7325066, + 7325067, + 7325068, + 7325069, + 7325070, + 7325071, + 7325072, + 7325073, + 7325074, + 7325075, + 7325076, + 7325077, + 7325078, + 7325079, + 7325080, + 7325081, + 7325082, + 7325083, + 7325084, + 7325085, + 7325086, + 7325087, + 7325088, + 7325089, + 7325090, + 7325091, + 7325092, + 7325093, + 7325094, + 7325095, + 7325096, + 7325097, + 7325098, + 7325099, + 7325100, + 7325101, + 7325102, + 7325103, + 7325104, + 7325105, + 7325106, + 7325107, + 7325108, + 7325109, + 7325110, + 7325111, + 7325112, + 7325113, + 7325114, + 7325115, + 7325116, + 7325117, + 7325118, + 7325119, + 7325120, + 7325121, + 7325122, + 7325123, + 7325124, + 7325125, + 7325126, + 7325127, + 7325128, + 7325129, + 7325130, + 7325131, + 7325132, + 7325133, + 7325134, + 7325135, + 7325136, + 7325137, + 7325138, + 7325139, + 7325140, + 7325141, + 7325142, + 7325143, + 7325144, + 7325145, + 7325146, + 7325147, + 7325148, + 7325149, + 7325150, + 7325151, + 7325152, + 7325153, + 7325154, + 7325155, + 7325156, + 7325157, + 7325158, + 7325159, + 7325160, + 7325161, + 7325162, + 7325163, + 7325164, + 7325165, + 7325166, + 7325167, + 7325168, + 7325169, + 7325170, + 7325171, + 7325172, + 7325173, + 7325174, + 7325175, + 7325176, + 7325177, + 7325178, + 7325179, + 7325180, + 7325181, + 7325182, + 7325183, + 7325184, + 7325185, + 7325186, + 7325187, + 7325188, + 7325189, + 7325190, + 7325191, + 7325192, + 7325193, + 7325194, + 7325195, + 7325196, + 7325197, + 7325198, + 7325199, + 7325200, + 7325201, + 7325202, + 7325203, + 7325204, + 7325205, + 7325206, + 7325207, + 7325208, + 7325209, + 7325210, + 7325211, + 7325212, + 7325213, + 7325214, + 7325215, + 7325216, + 7325217, + 7325218, + 7325219, + 7325220, + 7325221, + 7325222, + 7325223, + 7325224, + 7325225, + 7325226, + 7325227, + 7325228, + 7325229, + 7325230, + 7325231, + 7325232, + 7325233, + 7325234, + 7325235, + 7325236, + 7325237, + 7325238, + 7325239, + 7325240, + 7325241, + 7325242, + 7325243, + 7325244, + 7325245, + 7325246, + 7325247, + 7325248, + 7325249, + 7325250, + 7325251, + 7325252, + 7325253, + 7325254, + 7325255, + 7325256, + 7325257, + 7325258, + 7325259, + 7325260, + 7325261, + 7325262, + 7325263, + 7325264, + 7325265, + 7325266, + 7325267, + 7325268, + 7325269, + 7325270, + 7325271, + 7325272, + 7325273, + 7325274, + 7325275, + 7325276, + 7325277, + 7325278, + 7325279, + 7325280, + 7325281, + 7325282, + 7325283, + 7325284, + 7325285, + 7325286, + 7325287, + 7325288, + 7325289, + 7325290, + 7325291, + 7325292, + 7325293, + 7325294, + 7325295, + 7325296, + 7325297, + 7325298, + 7325299, + 7325300, + 7325301, + 7325302, + 7325303, + 7325304, + 7325305, + 7325306, + 7325307, + 7325308, + 7325309, + 7325310, + 7325311, + 7325312, + 7325313, + 7325314, + 7325315, + 7325316, + 7325317, + 7325318, + 7325319, + 7325320, + 7325321, + 7325322, + 7325323, + 7325324, + 7325325, + 7325326, + 7325327, + 7325328, + 7325329, + 7325330, + 7325331, + 7325332, + 7325333, + 7325334, + 7325335, + 7325336, + 7325337, + 7325338, + 7325339, + 7325340, + 7325341, + 7325342, + 7325343, + 7325344, + 7325345, + 7325346, + 7325347, + 7325348, + 7325349, + 7325350, + 7325351, + 7325352, + 7325353, + 7325354, + 7325355, + 7325356, + 7325357, + 7325358, + 7325359, + 7325360, + 7325361, + 7325362, + 7325363, + 7325364, + 7325365, + 7325366, + 7325367, + 7325368, + 7325369, + 7325370, + 7325371, + 7325372, + 7325373, + 7325374, + 7325375, + 7325376, + 7325377, + 7325378, + 7325379, + 7325380, + 7325381, + 7325382, + 7325383, + 7325384, + 7325385, + 7325386, + 7325387, + 7325388, + 7325389, + 7325390, + 7325391, + 7325392, + 7325393, + 7325394, + 7325395, + 7325396, + 7325397, + 7325398, + 7325399, + 7325400, + 7325401, + 7325402, + 7325403, + 7325404, + 7325405, + 7325406, + 7325407, + 7325408, + 7325409, + 7325410, + 7325411, + 7325412, + 7325413, + 7325414, + 7325415, + 7325416, + 7325417, + 7325418, + 7325419, + 7325420, + 7325421, + 7325422, + 7325423, + 7325424, + 7325425, + 7325426, + 7325427, + 7325428, + 7325429, + 7325430, + 7325431, + 7325432, + 7325433, + 7325434, + 7325435, + 7325436, + 7325437, + 7325438, + 7325439, + 7325440, + 7325441, + 7325442, + 7325443, + 7325444, + 7325445, + 7325446, + 7325447, + 7325448, + 7325449, + 7325450, + 7325451, + 7325452, + 7325453, + 7325454, + 7325455, + 7325456, + 7325457, + 7325458, + 7325459, + 7

LOT 71354412

LOT 18EM12599


REDAPT° SLICE
56 MM X 12 MM

Augment

Augment • Pièce • Spessore • Verlengstuk •
Aumento • Förstärkning • Påbygning • Augment •
Ενίσχυση • Aumento • Augment • 보강물

QTY: (1)
2028-05-13

 **smith&nephew**



TI-6AL-4V



(11) 180516

STERILE R CE 9800
 ISO 13485:2003 CERTIFIED
 Trademark of Smith & Nephew.

Smith & Nephew, Inc. 1450 Brooks Road,
 Memphis, TN 38116 USA

EC REP
 Smith & Nephew Orthopaedics GmbH,
 Altmannstrasse 14, 78532 Tuttlingen,
 Germany



T49H16AD, 2




This carton is recyclable.

www.smith-nephew.com

Блок замещающий REDAPT "скоба", 56 x 12 мм



Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

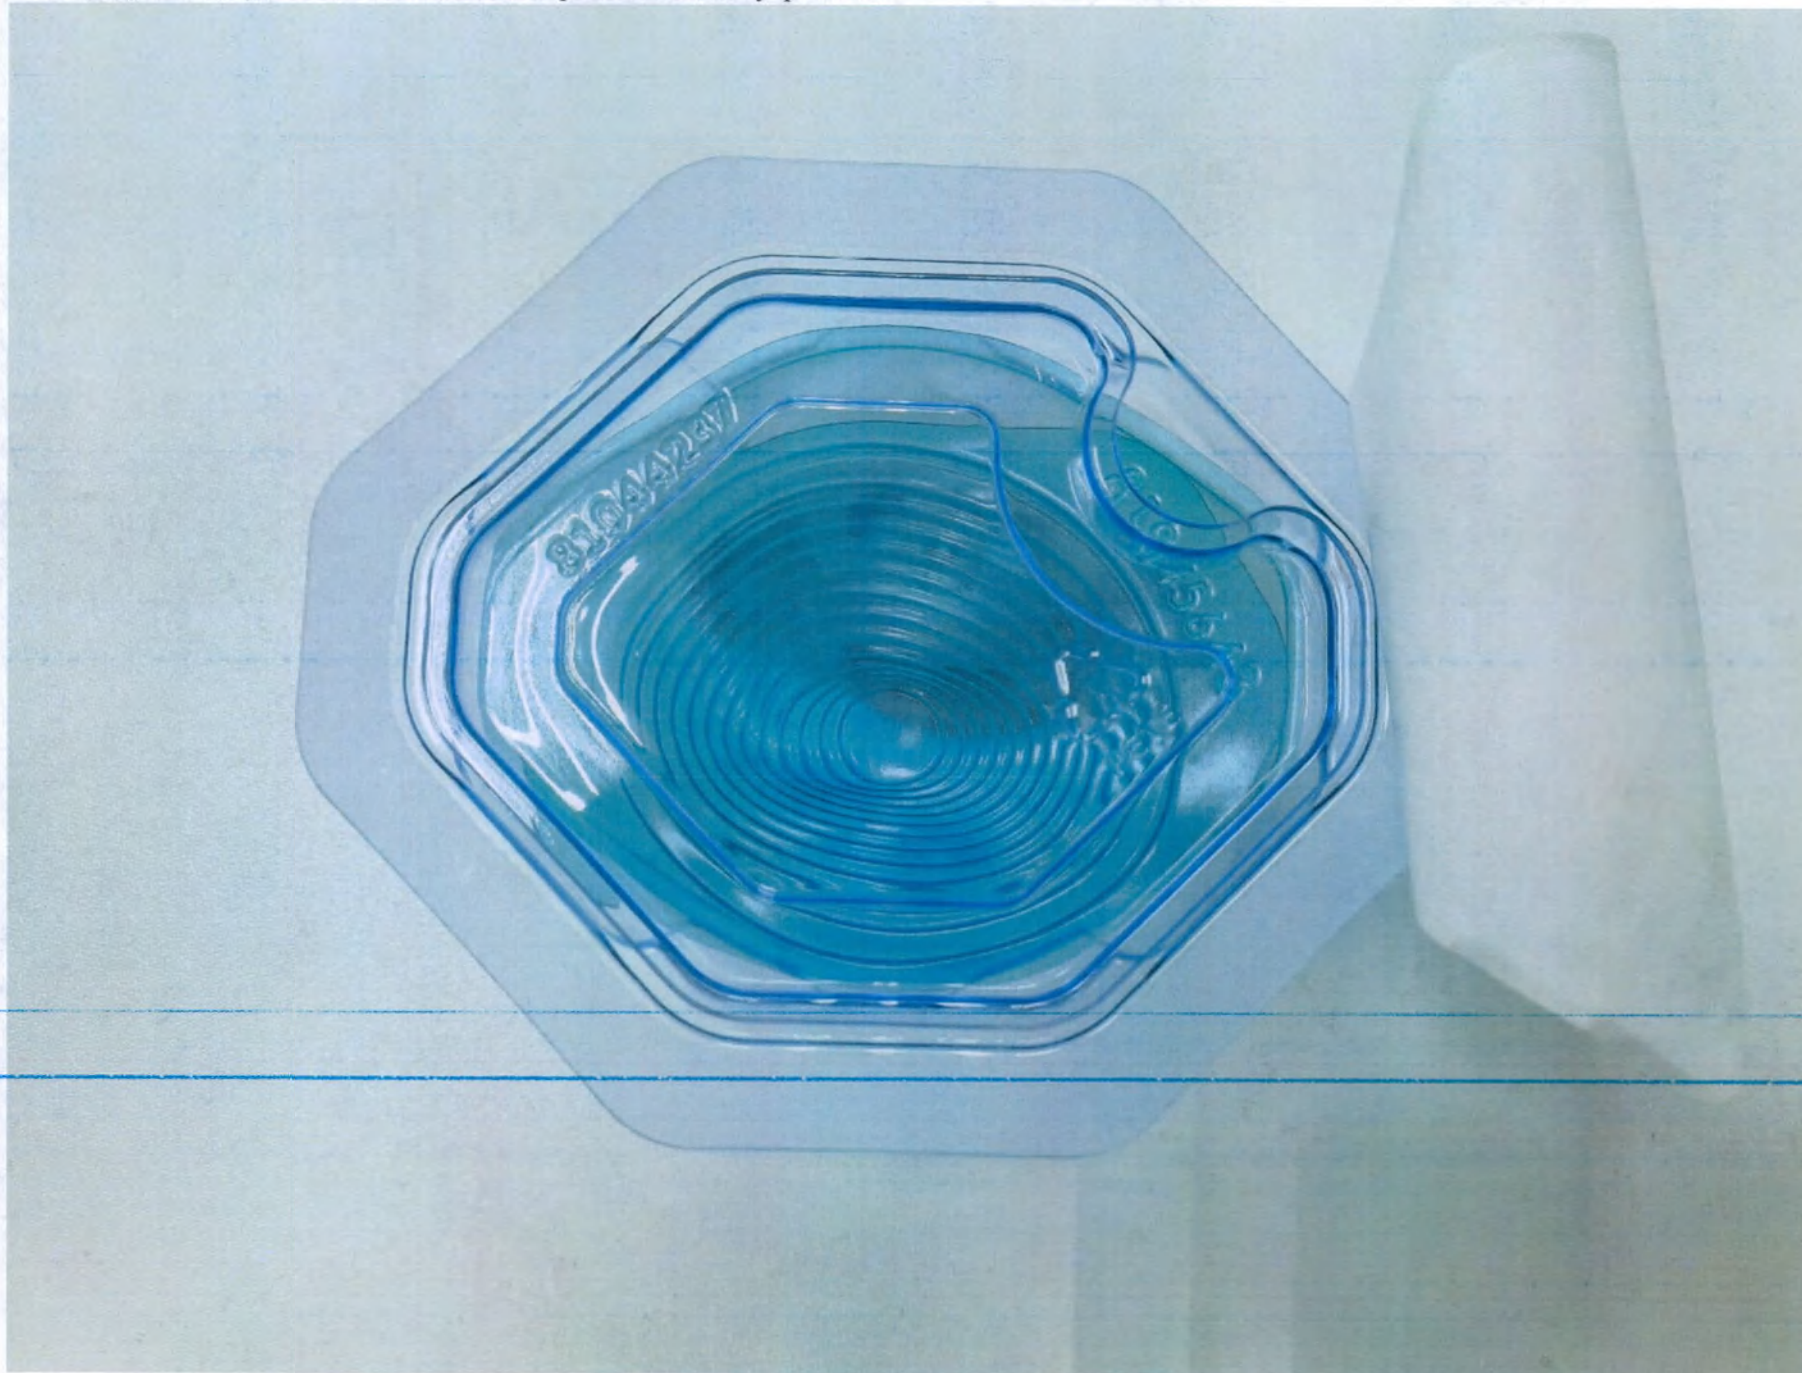

Индивидуальная упаковка: лоток внутренний.



Индивидуальная упаковка: лоток внутренний в лотке внешнем

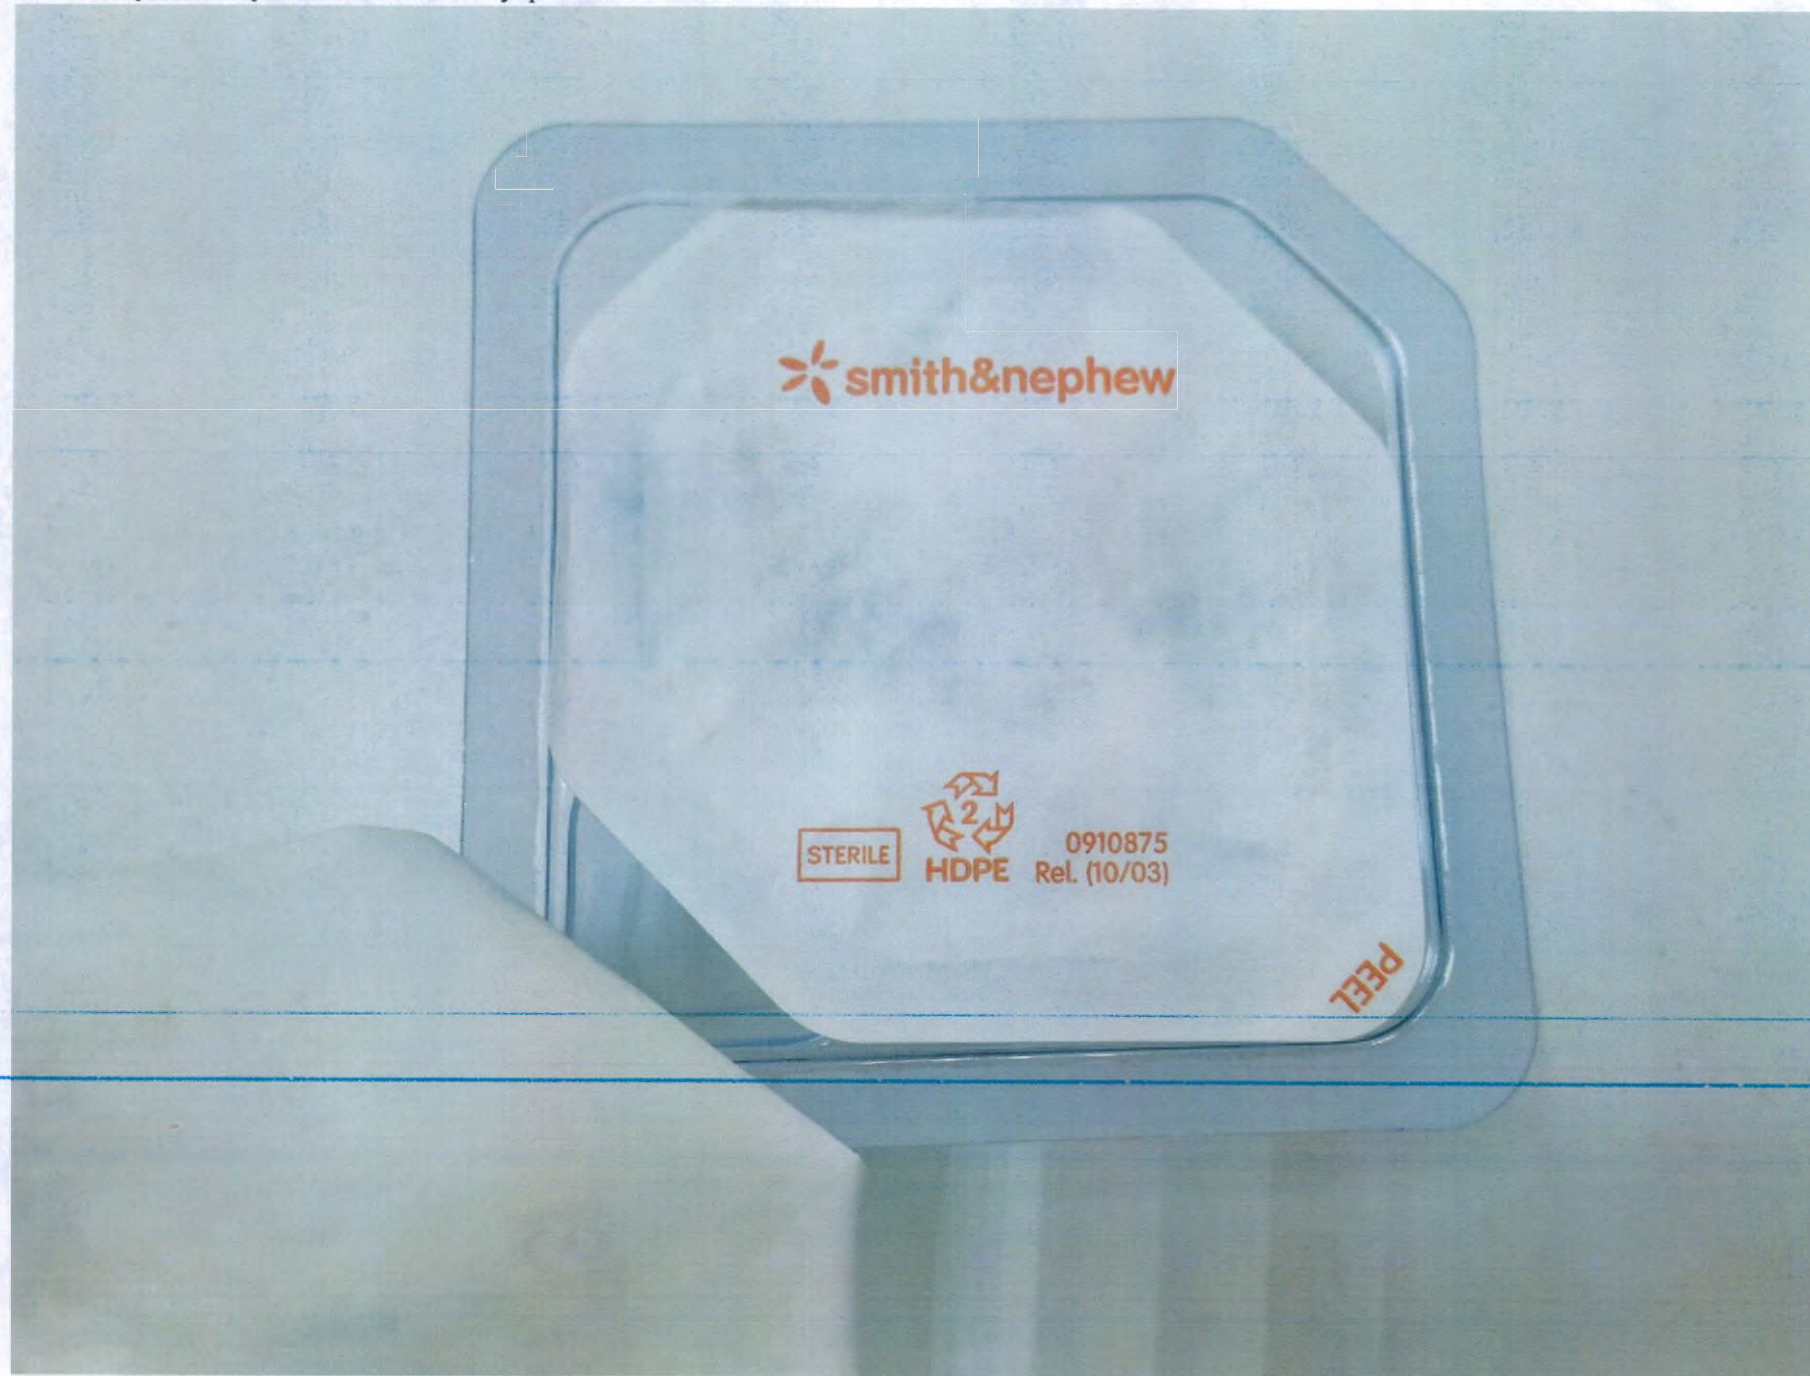




CHART-STIK® LABEL


REF ID: A11111 71354442
LOT: 17LM08444

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-11-11

REDAPT® STAPLE AUGMENT
56 MM X 12 MM
TI-6AL-4V



(01) 00885556316443 (17) 271111 (10) 17LM08444
(11) 171113

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL


REF ID: A11111 71354442
LOT: 17LM08444

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-11-11

REDAPT® STAPLE AUGMENT
56 MM X 12 MM
TI-6AL-4V



(01) 00885556316443 (17) 271111 (10) 17LM08444
(11) 171113

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL


REF ID: A11111 71354442
LOT: 17LM08444

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-11-11

REDAPT® STAPLE AUGMENT
56 MM X 12 MM
TI-6AL-4V



(01) 00885556316443 (17) 271111 (10) 17LM08444
(11) 171113

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF ID: A11111 71354442
LOT: 17LM08444

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-11-11

REDAPT® STAPLE AUGMENT
56 MM X 12 MM
TI-6AL-4V



(01) 00885556316443 (17) 271111 (10) 17LM08444
(11) 171113

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF ID: A11111 71354442
LOT: 17LM08444

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-11-11

REDAPT® STAPLE AUGMENT
56 MM X 12 MM
TI-6AL-4V



(01) 00885556316443 (17) 271111 (10) 17LM08444
(11) 171113

T94HSTK 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF ID: A11111 71354442
LOT: 17LM08444

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-11-11


REDAPT® STAPLE AUGMENT
56 MM X 12 MM
TI-6AL-4V



(01) 00885556316443 (17) 271111 (10) 17LM08444
(11) 171113

T94HSTK 4

ATTACH TO PATIENT'S RECORD

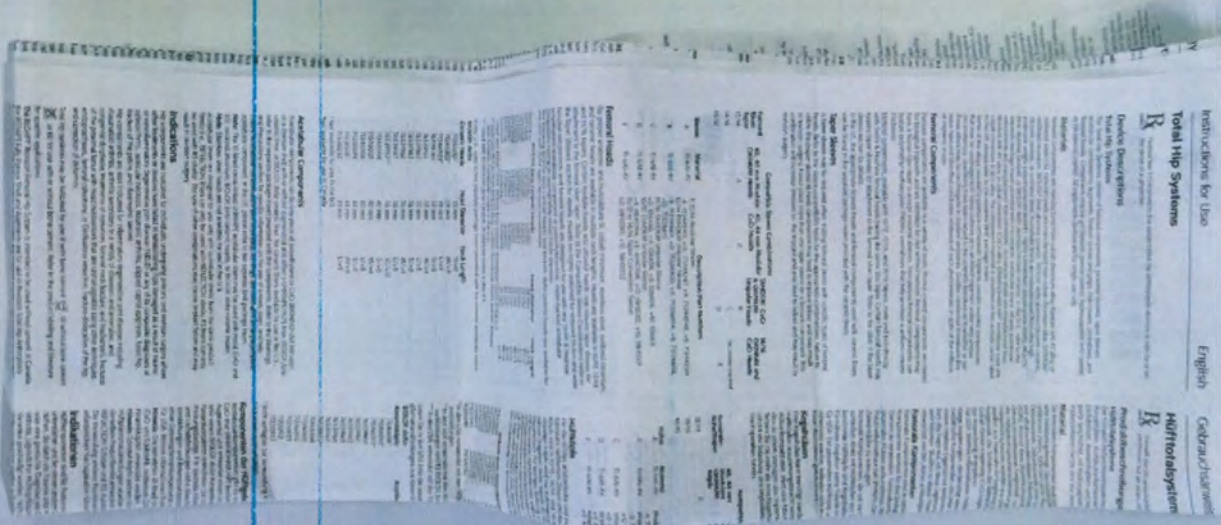

REF CAT# 71354442
LOT BATCH 17LM08444
REDAPT STAPLE
56 MM X 12 MM


Augment

Augment • Pièce • Spessore • Verlengstuk •
Aumento • Förstärkning • Påbygning • Augment •
Επαύξηση • Aumento • Augment • 보강물


QTY: (1)

USE 2027-11-11

 **smith&nephew**



TI-6AL-4V



STERILE R
IRRADIATION STERILIZED
* Trademark(s) of Smith & Nephew.



Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA

EC REP Smith & Nephew Orthopaedics GmbH,
Alemannenstrasse 14, 78532 Tuttlingen,
Germany



T49H16AD, 2




This carton is recyclable.

www.smith-nephew.com

Блок замещающий REDAPT клинковый – основание, размер 68 мм.



Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

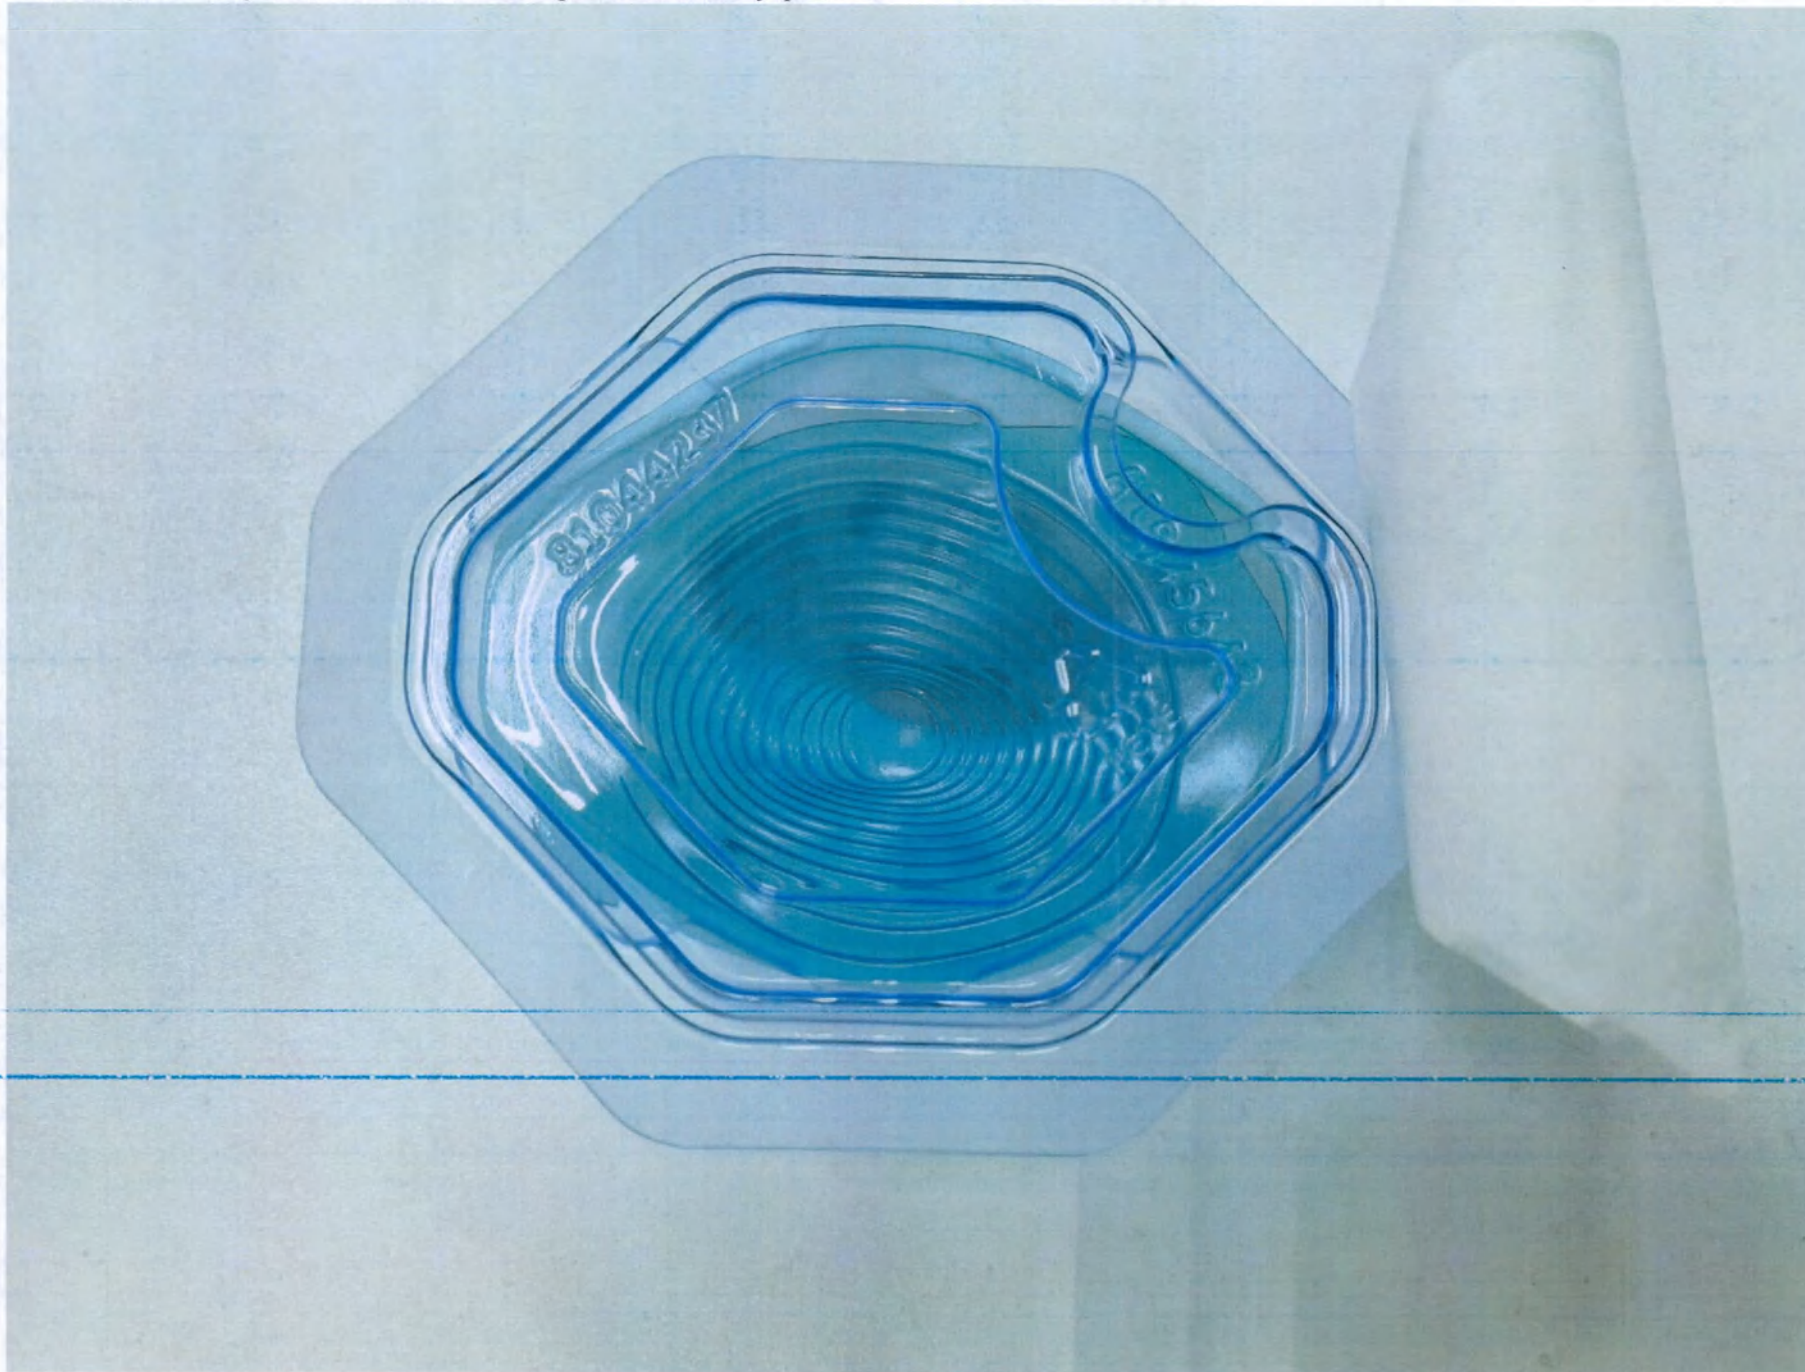

Индивидуальная упаковка: лоток внутренний.



Индивидуальная упаковка: лоток внутренний в лотке внешнем

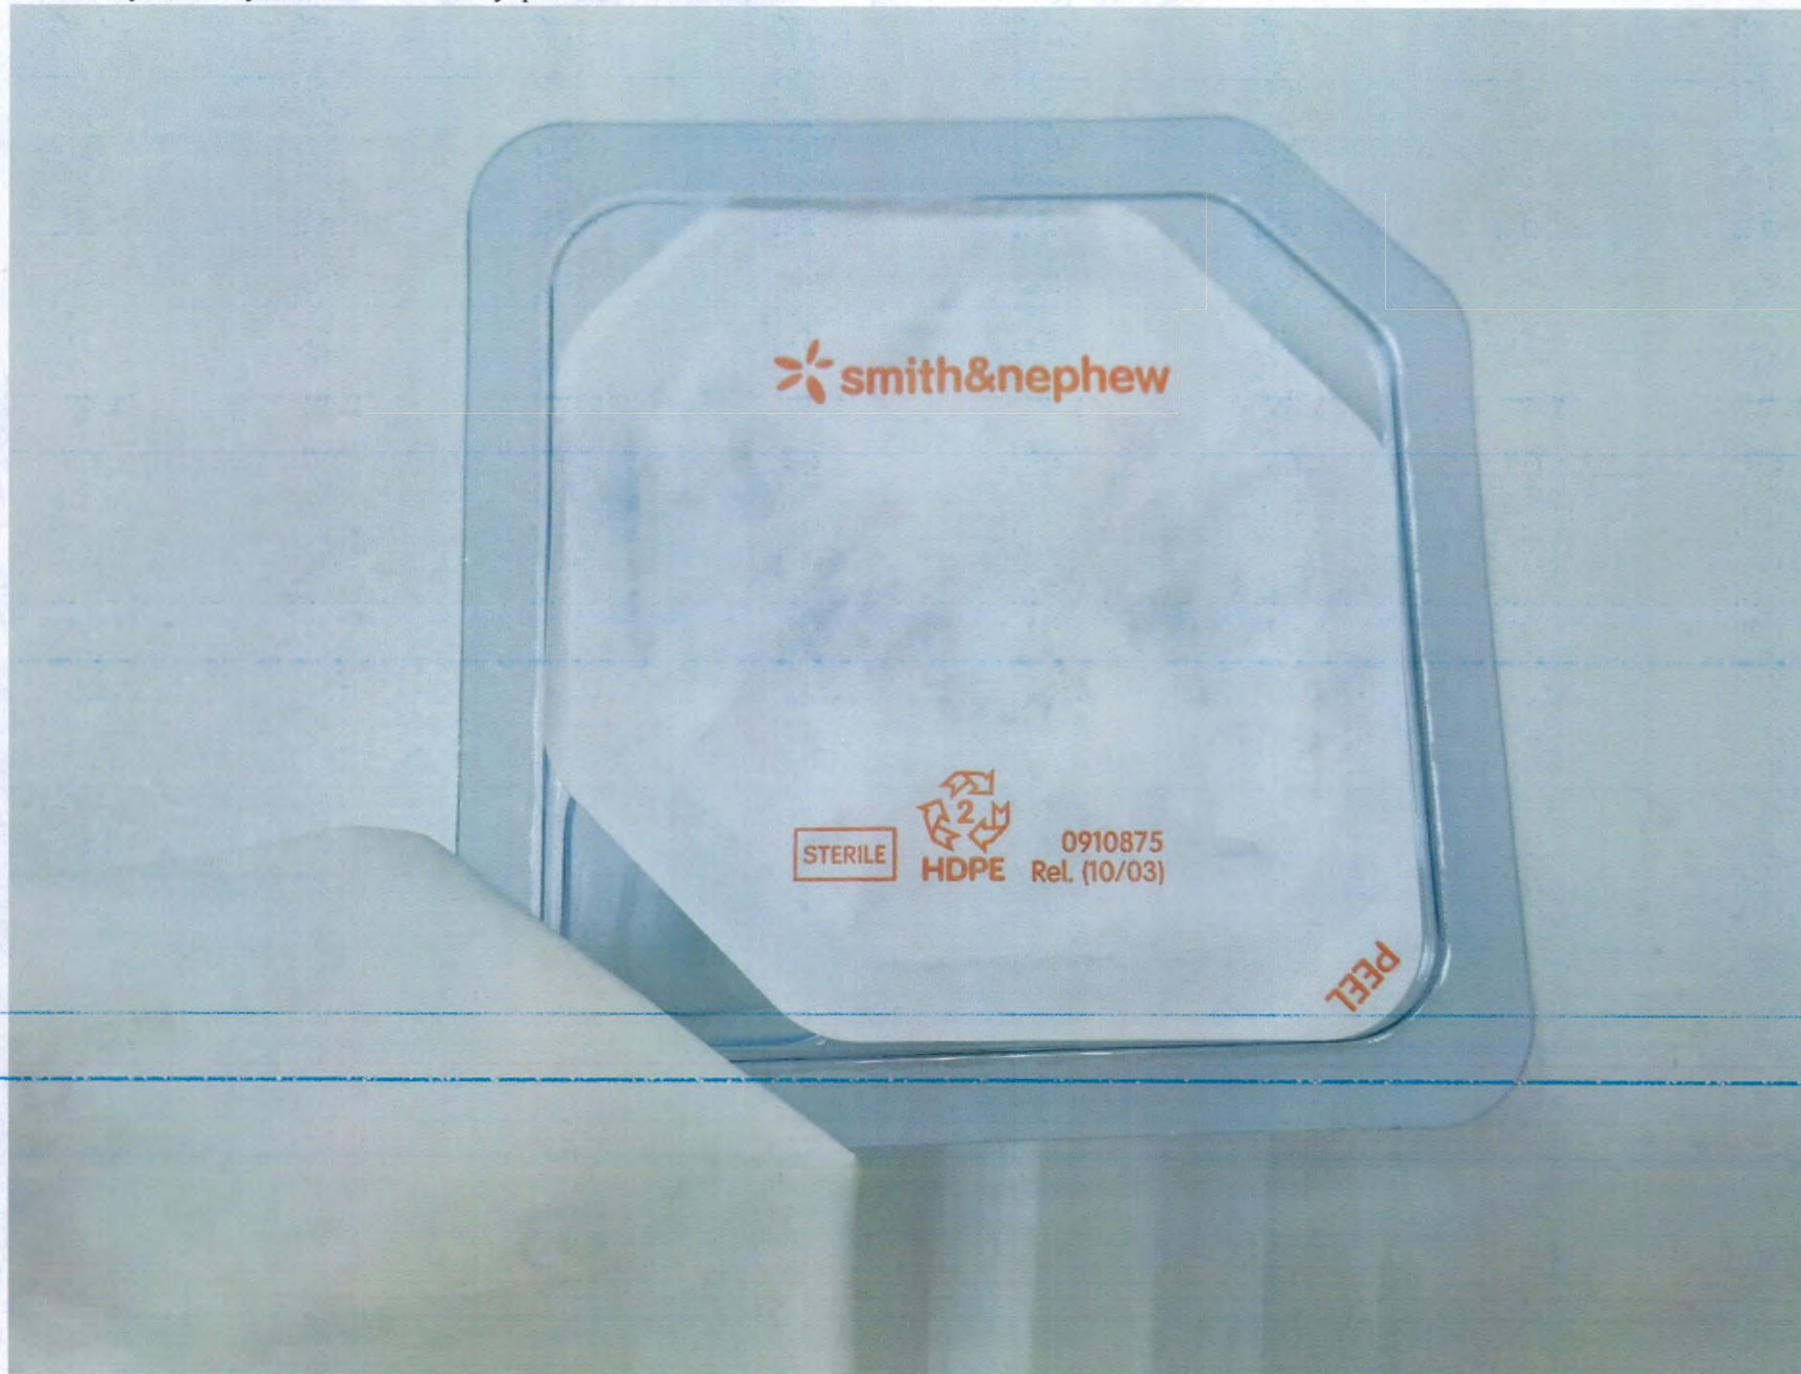




CHART-STIK® LABEL

REF 71354429

LOT BATCH CODE 20CM15096

smith&nephew

STERILE R
IRRADIATION STERILIZED

USE BY 2030-03-16

REDAPT® BLADE AUGMENT BASE
68 MM
TI-6AL-4V



(01) 00885556315842 (17) 300316 (10) 20CM15096



(11) 200316

T94HSTIK, 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF 71354429

LOT BATCH CODE 20CM15096

smith&nephew

STERILE R
IRRADIATION STERILIZED

USE BY 2030-03-16

REDAPT® BLADE AUGMENT BASE
68 MM
TI-6AL-4V




(01) 00885556315842 (17) 300316 (10) 20CM15096



(11) 200316

T94HSTIK, 4

ATTACH TO PATIENT'S RECORD

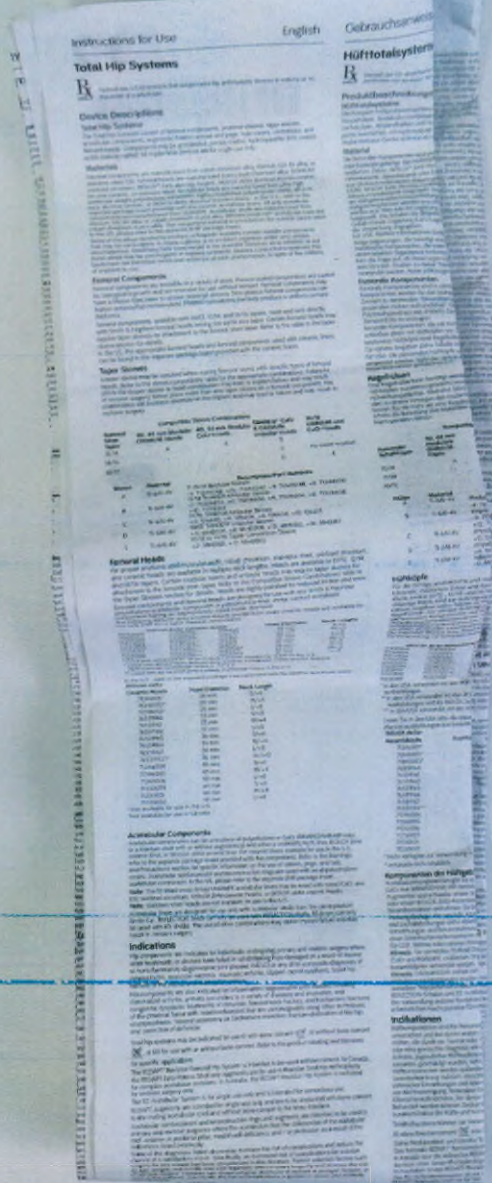

LOT NUMBER 71354429
LOT CODE 20CM15096
REDAPT° BLADE
68 MM

QTY: (1)

USE 2030-03-16

 smith&nephew

Augment Base

Augmentobasis • Augmenter base • Base di innalzamento • Basis
verlengstuk • Base de aumento • Förstärkingsbas •
Päbygningsbase • Ek Tabanı • Βάση αναύλησης • Base de
aumento • Forsterkningens base • 증대 베이스



TI-6AL-4V



(01) 00885556315842 (17) 300316 (10) 20CM15096



(11) 200318

STERILE R

IRRADIATION STERILIZED

* Trademarks of Smith & Nephew.



NO REUSE



CONSULT INSTRUCTIONS

EC REP

Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA

Smith & Nephew Orthopaedics GmbH,
Alemannenstrasse 14, 78532 Tuttlingen,
Germany



CAUTION



T49H16AD: 3




This carton is recyclable.

www.smith-nephew.com




Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

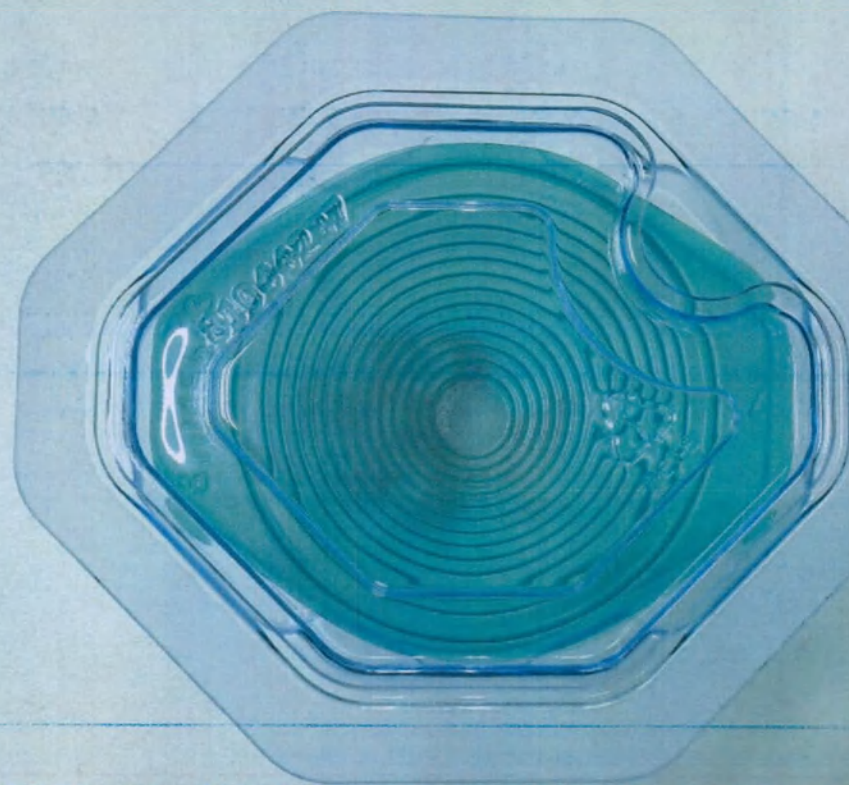

Индивидуальная упаковка: лоток внутренний.



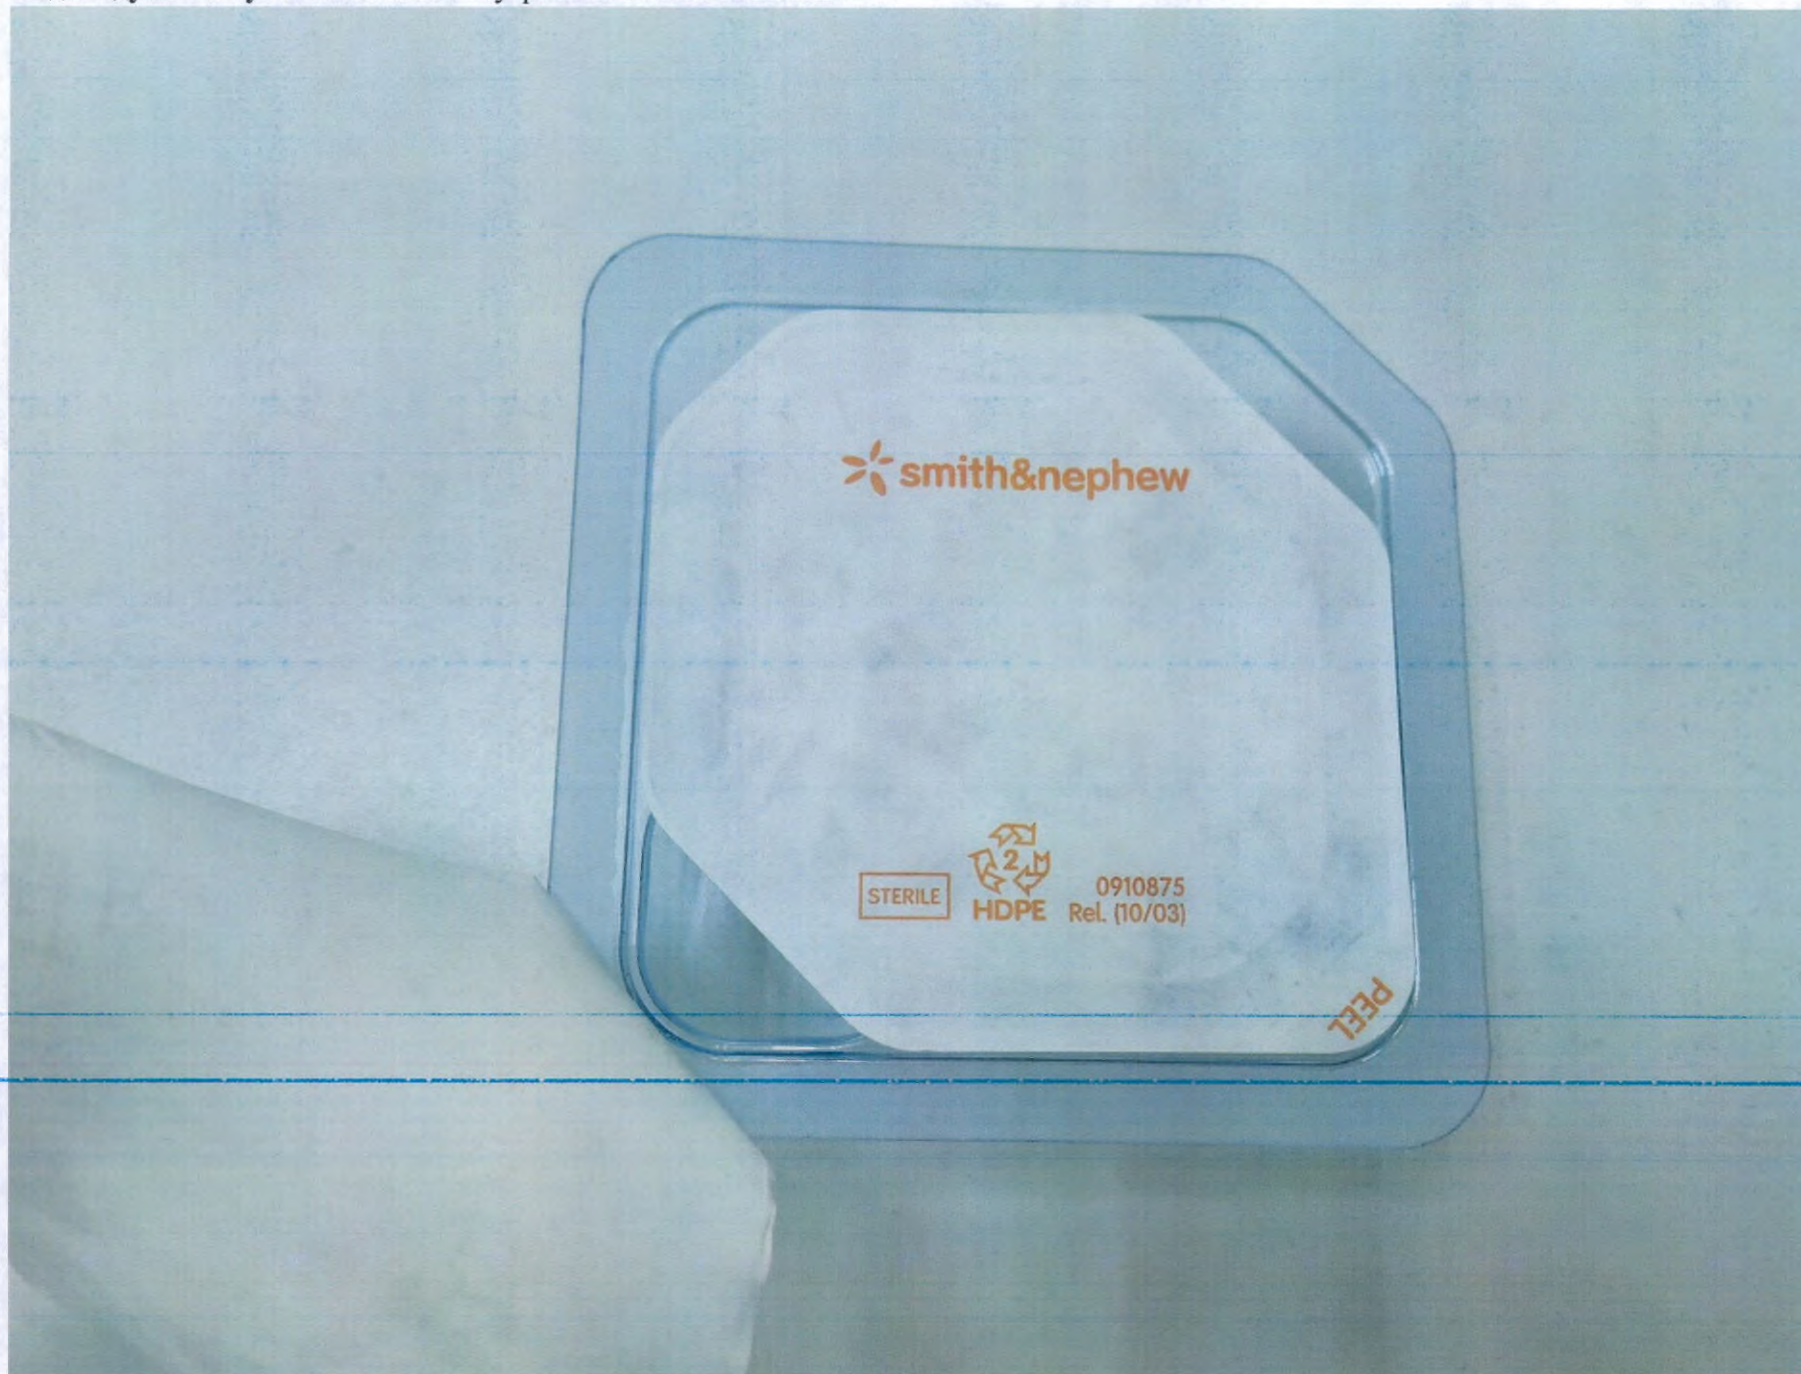







ITEM CATALOG 71354431
LOT BATCH CODE 19JM24567
REDAPT° BLADE

QTY: (1)
USE 2029-09-27

 smith&nephew

Augment Wing

AugmentWingel • Augmenter elle • Aletta di innalzamento • Vleugel
verhogingsluk • Ale de aumento • Forstærkningsvinge •
Pæbygningevinge • Ek Kienadi • Πτερόνιο αναύλησης • Suporte de
aumento • Forstærknings vinge • 증대 윙



TI-6AL-4V



(01) 00865558315941 (17) 290927 (10) 19JM24567



(11) 190930

STERILE R

IRRADIATION STERILIZED

*Trademarks of Smith & Nephew.



Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA



Smith & Nephew Orthopaedics GmbH,
Alemannenstrasse 14, 78532 Tuttlingen,
Germany



CAUTION



T49H16AD, 3




This carton is recyclable.

www.smith-nephew.com


VIII. Чашки модульные REDAPT, на примере вариантов исполнения
Чашка модульная REDAPT, 48 мм.




Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

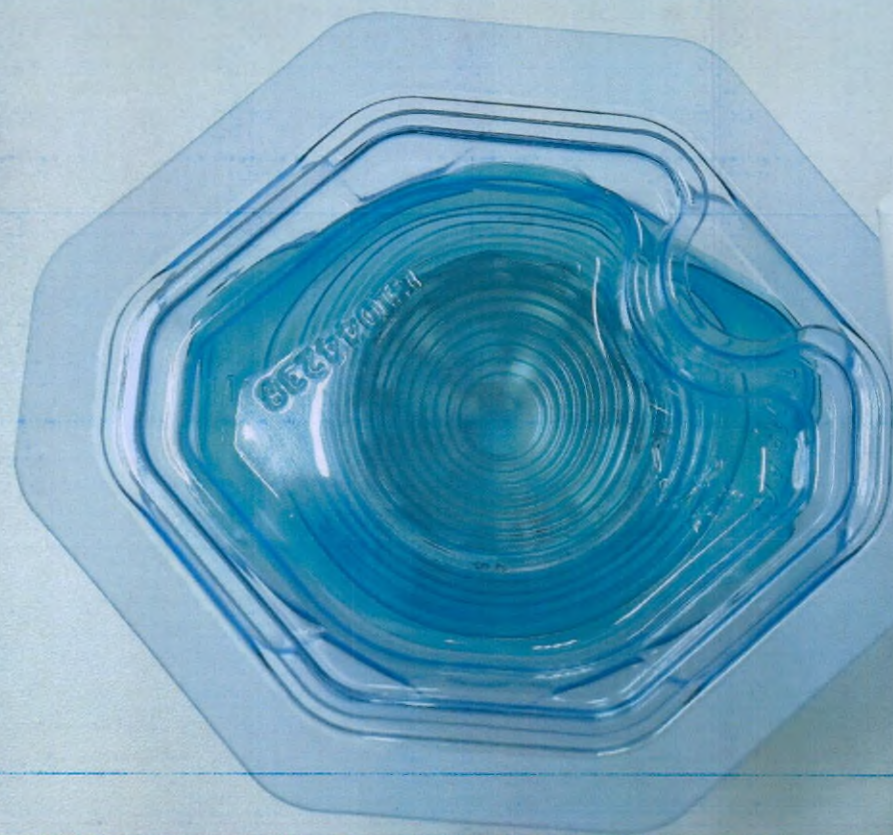

Индивидуальная упаковка: лоток внутренний.

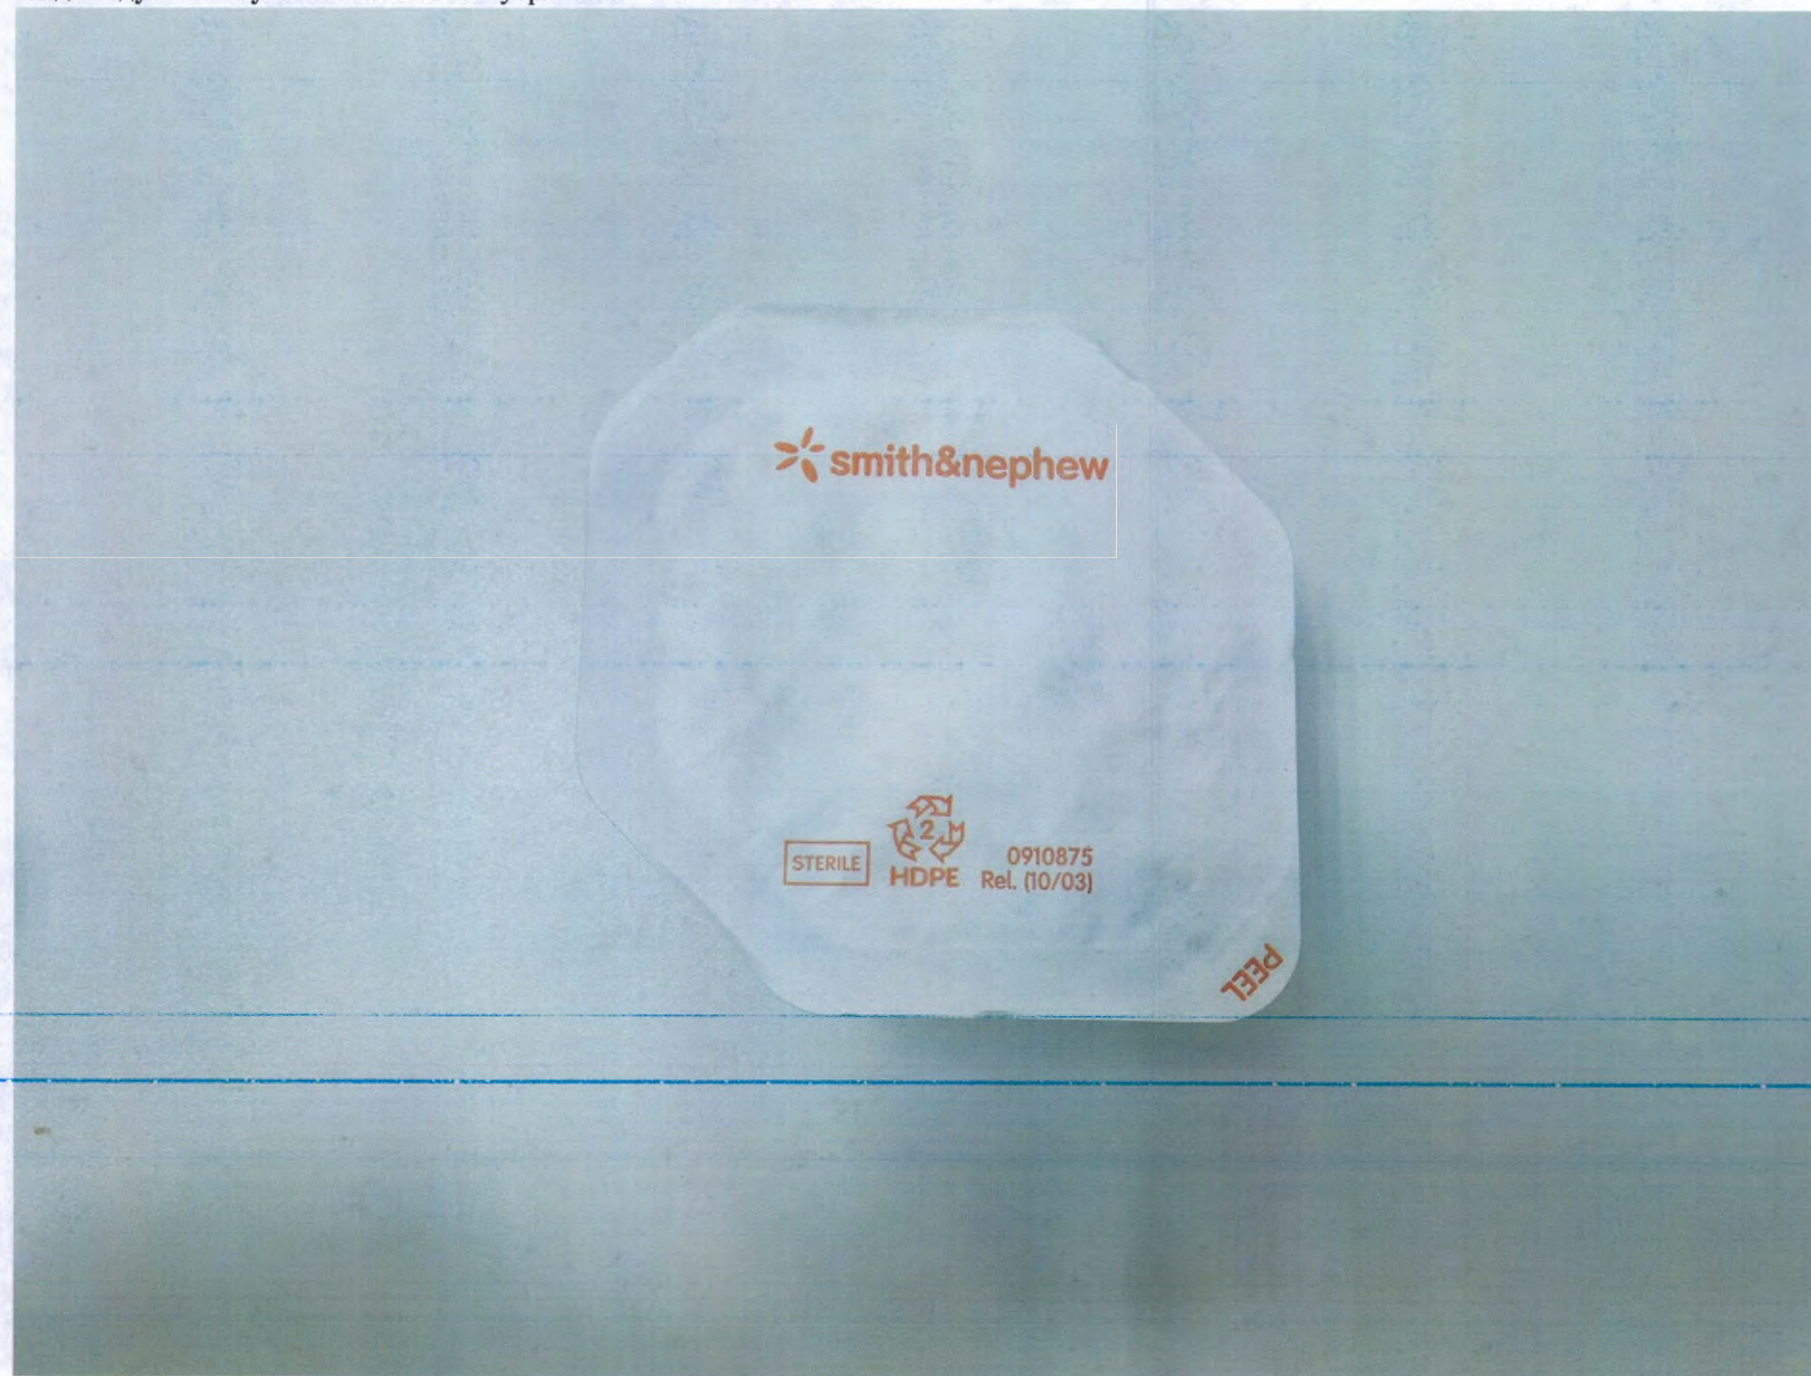

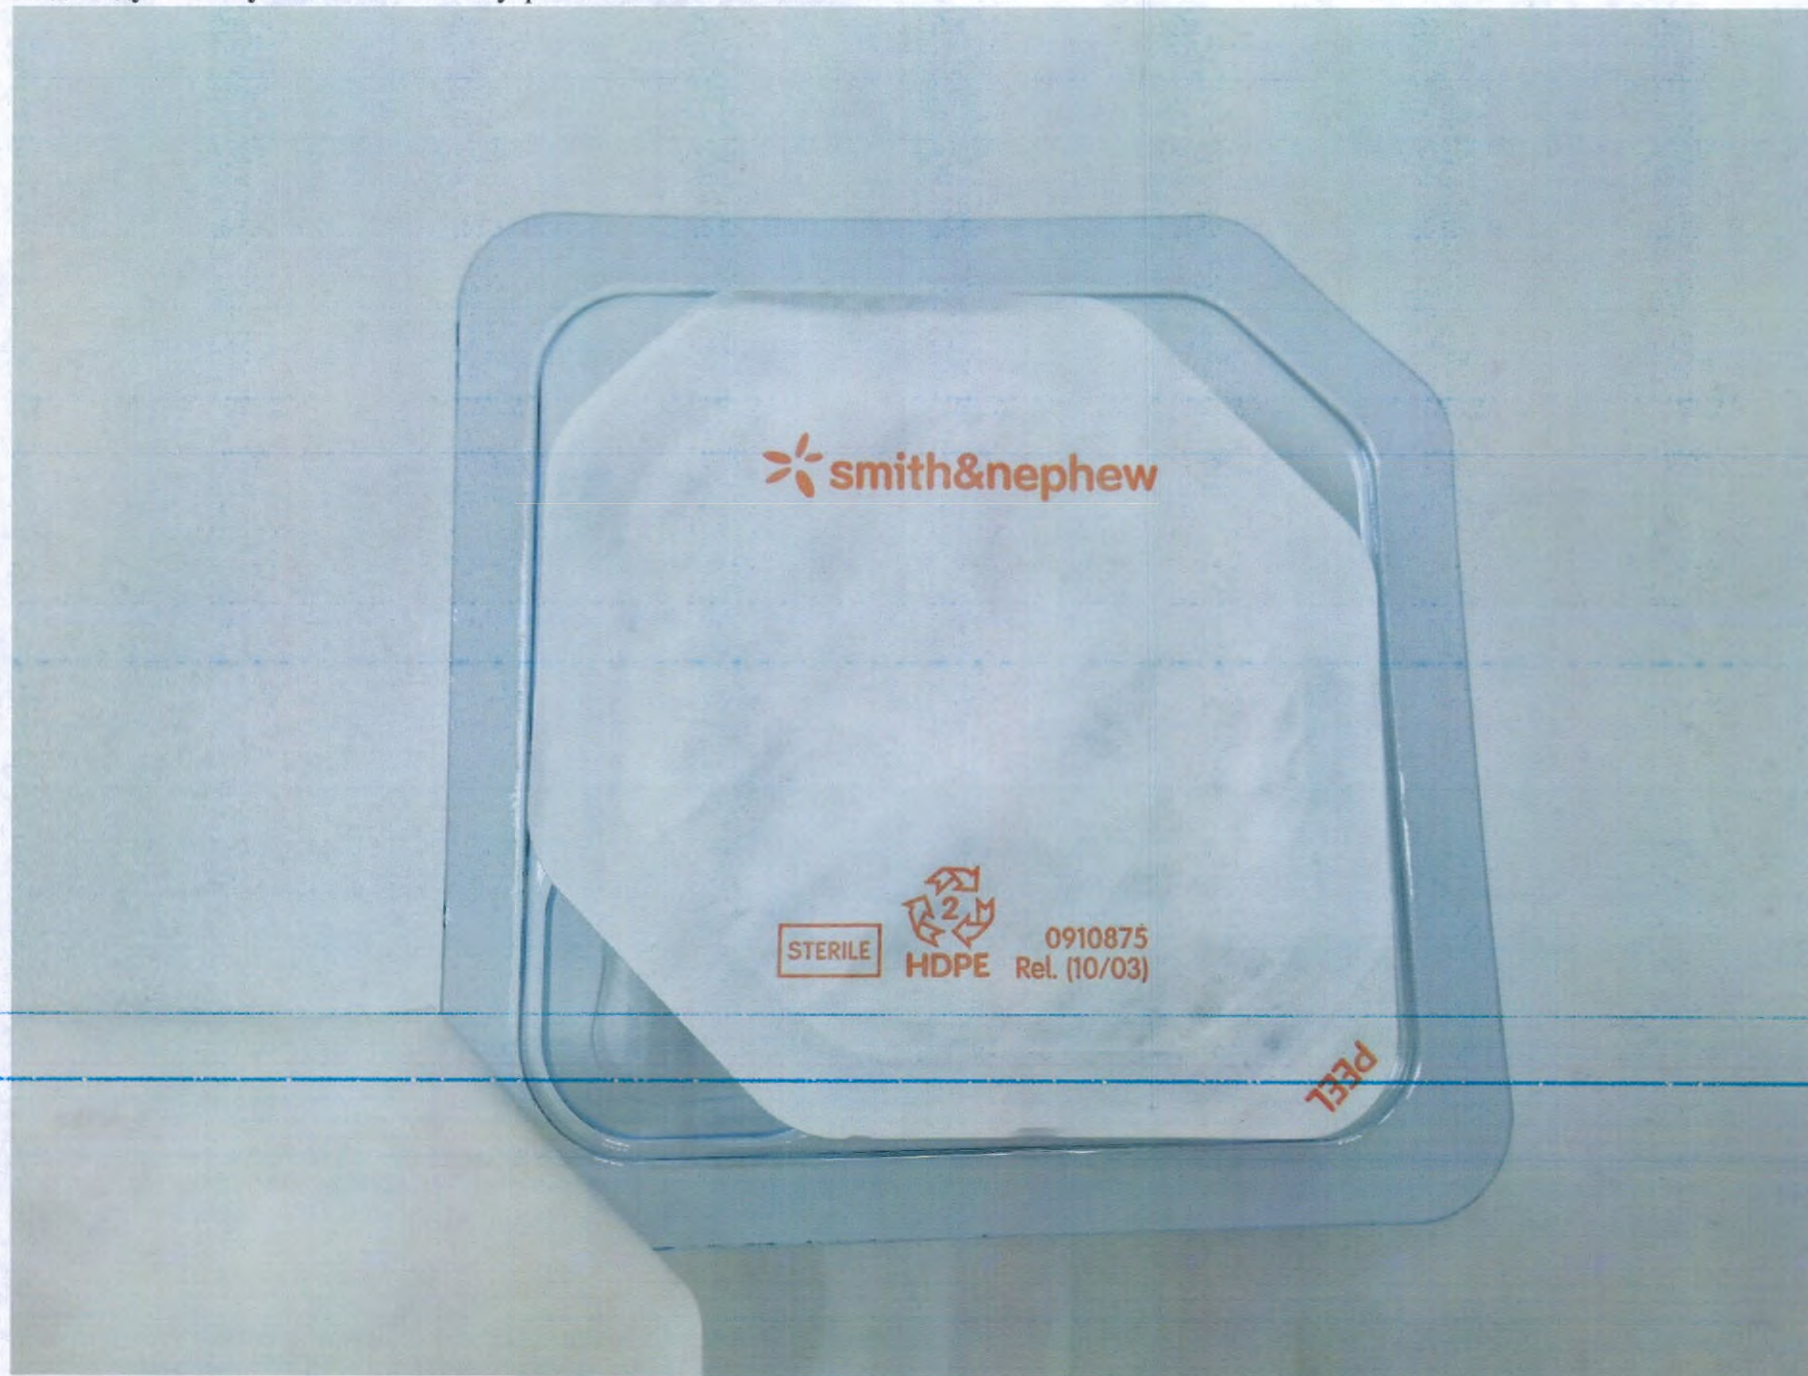

Индивидуальная упаковка: лоток внешний.







REF: 71352348
LOT: 20FM04543
REDAPT[®]
MODULAR


QTY: (1)
USE BY 2030-06-03

 smith&nephew

Shell
Schale • Cupule • Guscio • Shell • Cotilo • Skal • Pouzdro • Tabaka • Κοτούλη •
Estrutura • Shell



48 MM OD



USE WITH R3° SIZE 48 MM OD LINER

MODULAR SHELL
TI-6AL-4V



(01) 00885556657799 (17) 300603 (10) 20FM04543



(11) 200605

STERILE **R**

IRRADIATION STERILIZED

* Trademark(s) of Smith & Nephew.



NO REUSE



CONSULT
INSTRUCTIONS

EC REP

Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA

Smith & Nephew Orthopaedics GmbH,
Alemannenstrasse 14, 78532 Tuttlingen,
Germany



CEMENTLESS



CAUTION




T49H18AT, 2




This carton is recyclable.

www.smith-nephew.com

Чашка модульная REDAPT, 66 мм.

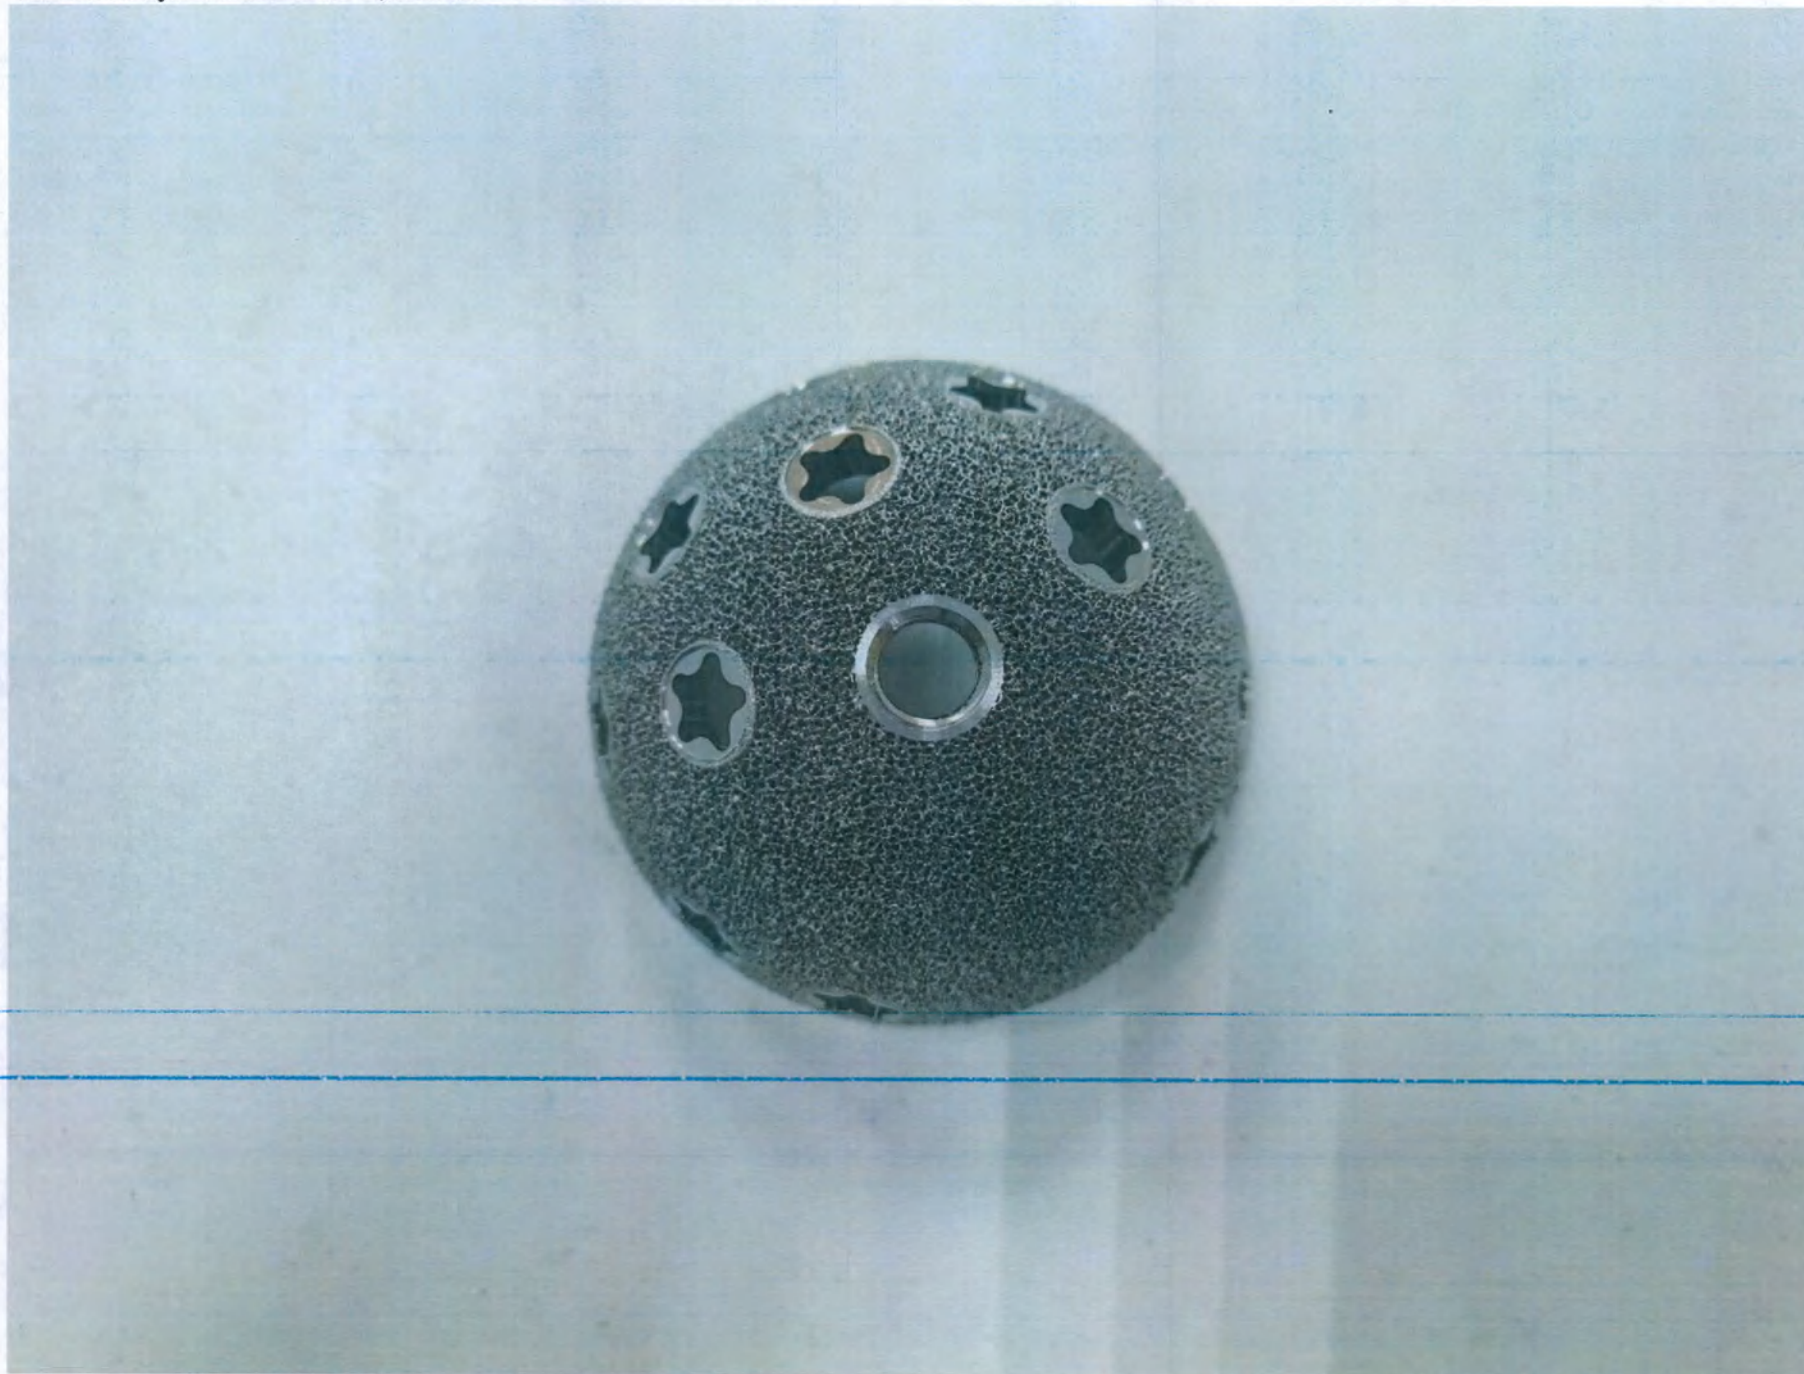

Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

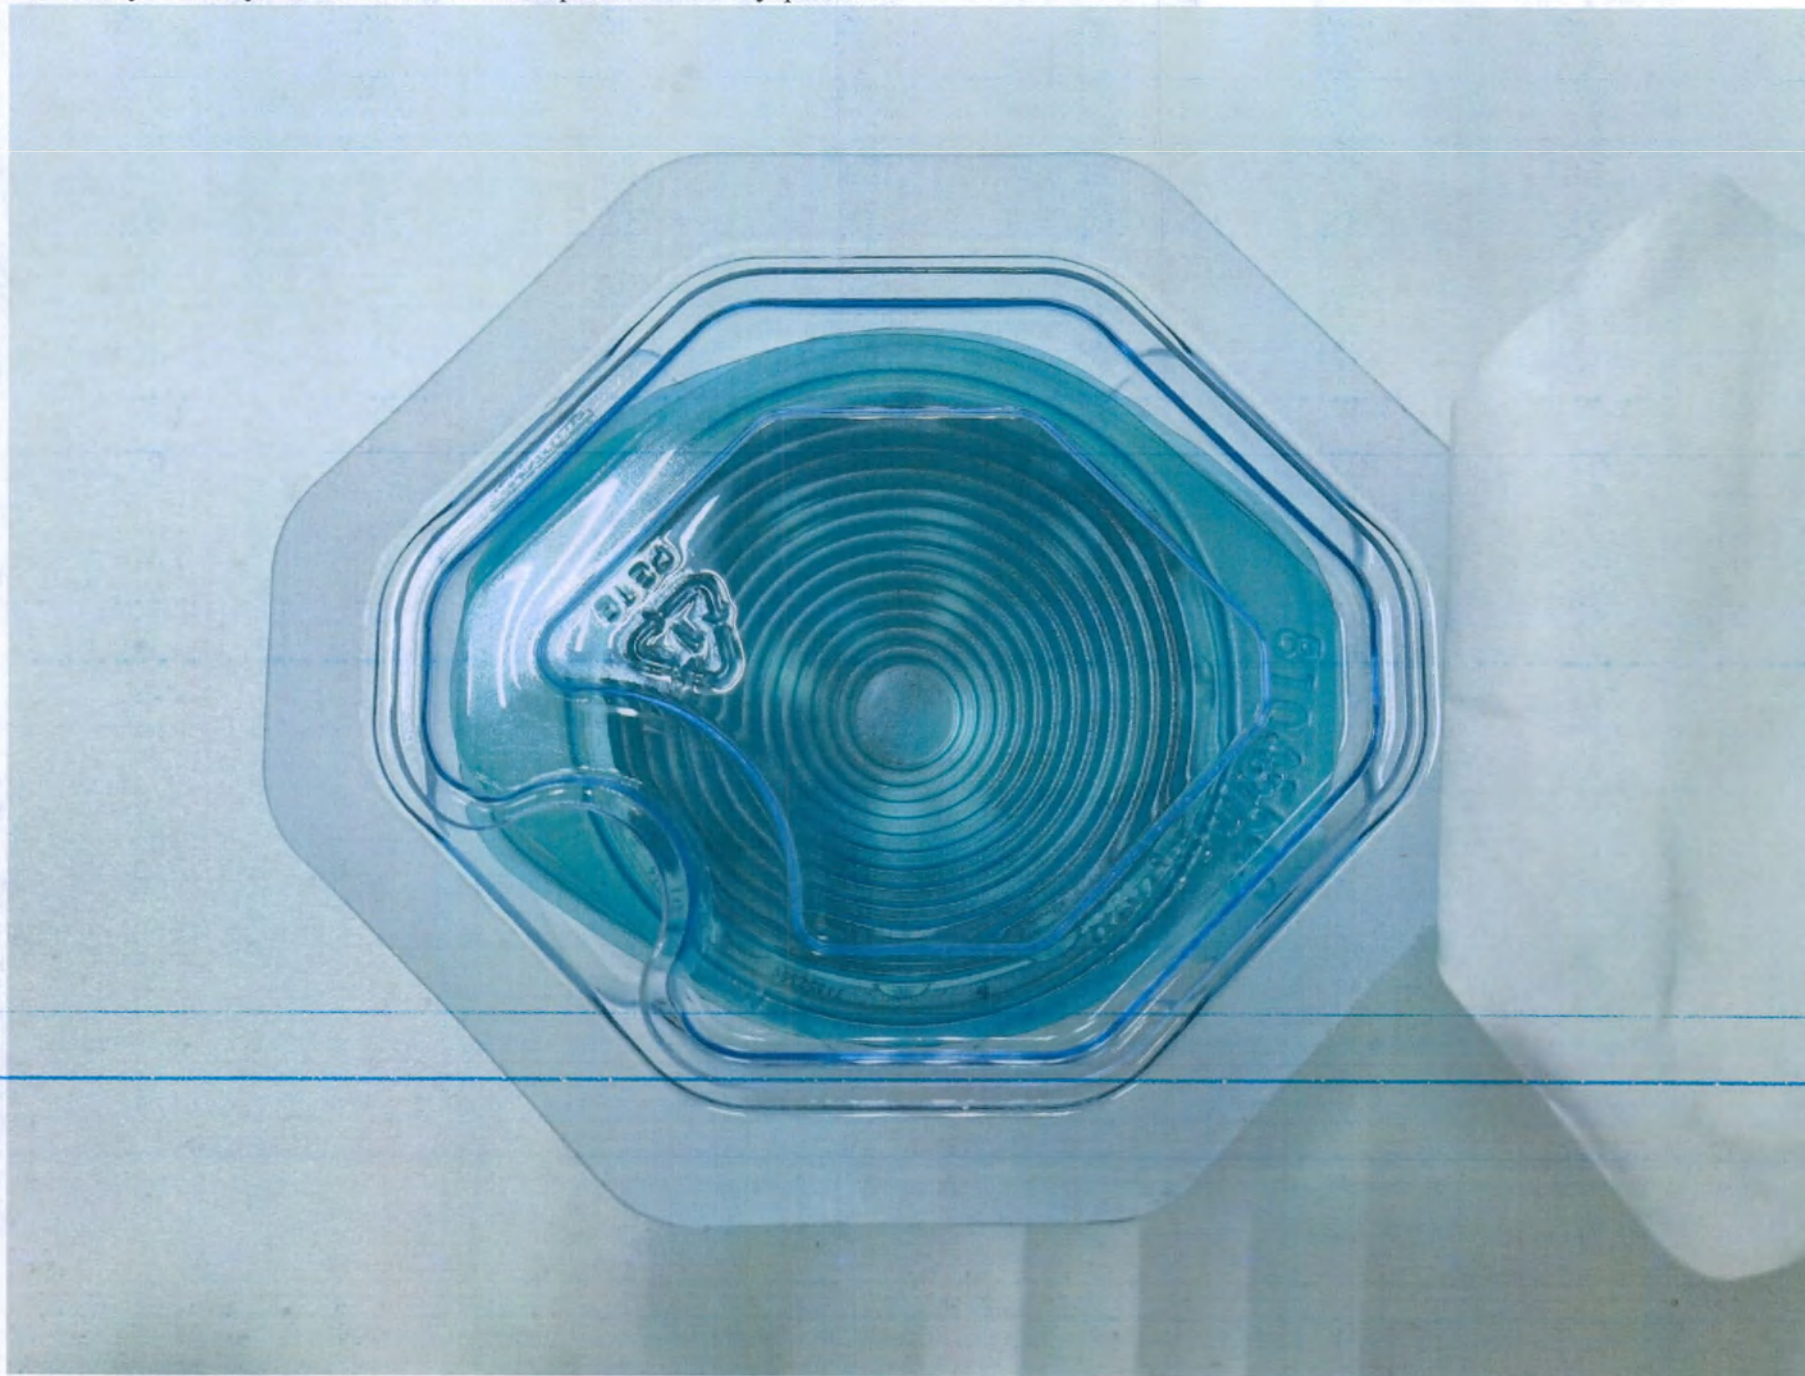

Индивидуальная упаковка: лоток внутренний.



Индивидуальная упаковка: лоток внутренний в лотке внешнем





CHART-STIK® LABEL

smith&nephew

REF ID: 71352366
LOT: 19HM12856

STERILE R
IRRADIATION STERILIZED

EXP 2029-08-12

66 MM OD
USE WITH R3° SIZE 66-70 MM OD LINER
REDAPT®
MODULAR SHELL
TI-6AL-4V



(01) 00885556657898 (17) 290812 (10) 19HM12856

(11) 190815

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

smith&nephew

REF ID: 71352366
LOT: 19HM12856

STERILE R
IRRADIATION STERILIZED

EXP 2029-08-12

66 MM OD
USE WITH R3° SIZE 66-70 MM OD LINER
REDAPT®
MODULAR SHELL
TI-6AL-4V



(01) 00885556657898 (17) 290812 (10) 19HM12856

(11) 190815

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

smith&nephew

REF ID: 71352366
LOT: 19HM12856

STERILE R
IRRADIATION STERILIZED

EXP 2029-08-12

66 MM OD
USE WITH R3° SIZE 66-70 MM OD LINER

S RECORD

Instructions for Use

English

Gebrauchsanweisung

Total Hip Systems

CAUTION: Federal law (USA) restricts the subject total hip orthopedic devices to sale by or on the order of a physician.

Device Descriptions

Total Hip Systems

The Total Hip Systems consist of femoral components, modular necks, proximal sleeves, taper sleeves, acetabular components, fixation sleeves and pegs, liner covers, caps, liners, and femoral heads. Components may be grit blasted, porous coated, hydroxyapatite (HA) coated, or HA porous coated. All implantable devices are for single use only.

Materials

Femoral components are manufactured from cobalt chromium alloy, titanium 6Al-4V alloy, or stainless steel (SS). Femoral heads are manufactured from cobalt chromium alloy, ORION[®] oxidized zirconium, BIOLOX[®] forte alumina ceramic, BIOLOX[®] delta alumina/zirconia ceramic, zirconia ceramic, or stainless steel. Acetabular liners are manufactured from ultra-high molecular weight polyethylene (UHMWPE), BIOLOX[®] forte alumina ceramic, or BIOLOX[®] delta alumina/zirconia ceramic. In the U.S., refer to the separate package insert provided with the ceramic acetabular liners. All poly acetabular components are manufactured from UHMWPE. Acetabular shells are manufactured from titanium 6Al-4V alloy or cobalt chromium (CoCr) alloy. BIRMINGHAM[®] HP[®] acetabular cups are cobalt chromium (CoCr) alloy. The component material is provided on the outside carton label. **NOTE:** BIOLOX[®] delta ceramic liners are not available for use in the U.S.

Some of the alloys needed to produce orthopedic implants contain metallic components that may be carcinogenic in tissue cultures or in an intact organism under very unique circumstances. Questions have been raised in the scientific literature as to whether or not these alloys may be carcinogenic in implant recipients. Studies conducted to evaluate this issue have not identified conclusive evidence of such phenomenon, in spite of the millions of implants in use.

Femoral Components

Femoral components are available in a variety of sizes. Porous coated components are coated for biological ingrowth and are intended for use without cement. Modular femoral components are available with an oval taper to accept Smith & Nephew CoCr modular necks and/or a Morse-type taper to accept proximal sleeves. Non-porous femoral components can tolerate polyethylene methacrylate (PMMA) cementations that help produce a uniform cement thickness.

Femoral components, available with 10/12, 12/14, and 14/16 tapers, mate and lock directly with Smith & Nephew femoral heads having the same size taper. Certain femoral heads may require taper sleeves for attachment to the femoral stem taper. Refer to the table in the Taper Sleeves section for details.

Taper Sleeves

A taper sleeve may be required when mating femoral stems with specific types of femoral heads. Refer to the sleeve compatibility table for the appropriate combinations. Failure to utilize the proper sleeve to head combination may lead to implant failure and may result in revision surgery. Never place more than one taper sleeve on a femoral component; this combination will increase stresses on the implant and may lead to failure and may result in revision surgery.

Modular Necks

Modular necks are made from CoCr alloy and are available in a variety of configurations. The modular neck mates and locks with the oval taper of a modular femoral component on one end and the taper of a 12/14 femoral head on the other end.

Compatible Sleeve Combinations

Femoral Stem Taper	40, 44 mm Modular CoCr Heads	40, 44 mm Modular CoCr Heads	BH Modular CoCr Heads	BANDEM [®] CoCr and CoCr Heads	14/16 ORION [®] and CoCr Heads
12/14	A	A	B	C	
14/16				D	No sleeve required
10/12				E	F

* Modular CoCr heads are made from CoCr alloy and are intended for cementless use in the U.S. Refer to the separate package insert provided with the components.

** The Modular Head is not available for use in the U.S. These heads can only be used with cemented (polyethylene) femoral stems.

Sleeve	Material	Description/Part Numbers
A	Ti-6Al-4V	Ti-6Al-4V Modular Stem
B	CoCr	4: 70344241, +0: 70344247, +8: 70344248, +8: 70344330
C	CoCr	4: 70222101, +0: 70222200, +8: 70222300, +8: 70222400
D	Ti-6Al-4V	3: 70226603, +0: 70226600, +8: 70226604, +8: 70226608
E	Ti-6Al-4V	14/16 12/14/12/14 Angular Sleeve
F	Ti-6Al-4V	10/12 12/14/14/14 Linear Sleeve
G	Ti-6Al-4V	4: 80000004, +8: 80000008, +0: 80000008, +8: 80000012
H	Ti-6Al-4V	10/12 to 14/16 Taper Conversion Sleeve
I	Ti-6Al-4V	+0: 80000008, +0: 80000012

Femoral Heads

For proper aseptic and modular fit, cobalt chromium, stainless steel, oxidized zirconium, and ceramic heads are available in multiple neck lengths. Heads are available in 10/12, 12/14, and 14/16 tapers. Certain modular heads and angular heads may require taper sleeves for attachment to the femoral stem taper. Refer to the Compatible Sleeve Combinations table in the Taper Sleeves section for details. Heads are highly polished for reduced friction and wear. Femoral components and femoral heads are designed for use with any Smith & Nephew cementless acetabular component or polyethylene liner, metal backed acetabular component, or cemented acetabular component, except heads designed for use with the cemented acetabular component.

Hüfttotalsysteme

VORSICHT: Gemäß der US-Regulation ist das Produkt nur an einen Arzt oder auf dessen Anweisung zu verkaufen.

Produktbeschreibungen

Hüfttotalsysteme

Die Hüfttotalsysteme bestehen aus Femoral-Komponenten, modulare Halsen, proximale Ärmeln, Taper-Ärmeln, Acetabulum-Komponenten, Fixations-Ärmeln und -Nägeln, Linien, Linien, Linien und Femoral-Köpfe. Komponenten können sandgestrahtet, porös beschichtet, Hydroxyapatit (HA) beschichtet oder HA-porös beschichtet sein. Alle implantierbaren Geräte sind für den einmaligen Gebrauch vorgesehen.

Materialien

Femoral-Komponenten sind aus Kobalt-Chrom-Legierung, Titan 6Al-4V-Legierung oder Edelstahl (SS) gefertigt. Die Hüftköpfe sind aus Kobalt-Chrom-Legierung, ORION[®] oxidiertes Zirkon, BIOLOX[®] forte Aluminiumoxid, BIOLOX[®] delta Aluminium/Zirkonoxid, Zirkonoxid oder Edelstahl gefertigt. Acetabulum-Ärmel sind aus hochmolekularem Polyethylen (UHMWPE), BIOLOX[®] forte Aluminiumoxid oder BIOLOX[®] delta Aluminium/Zirkonoxid gefertigt. In den USA: Bitte auf das separate Packungsbeilage für die Keramik-Acetabulum-Ärmel. Alle Polyacetabulum-Komponenten sind aus UHMWPE gefertigt. Acetabulum-Schalen sind aus Titan 6Al-4V-Legierung oder Kobalt-Chrom-Legierung (CoCr) gefertigt. BIRMINGHAM[®] HP[®] Acetabulum-Schalen sind aus Kobalt-Chrom-Legierung (CoCr) gefertigt. Das Komponente-Material ist auf dem äußeren Kartonschild angegeben. **HINWEIS:** BIOLOX[®] delta Keramik-Ärmel sind in den USA nicht verfügbar.

Einige der Legierungen, die zur Herstellung von orthopädischen Implantaten benötigt werden, können in Zellkulturen oder in einem intakten Organismus unter sehr speziellen Umständen als krebserregend wirken. In der wissenschaftlichen Literatur wurden Fragen darüber aufgeworfen, ob diese Legierungen in Implantatempfängern krebserregend wirken könnten. Durchgeführte Studien zur Bewertung dieses Problems haben keine schlüssigen Ergebnisse erbracht, obwohl Millionen von Implantaten im Einsatz sind.

Femorale Komponenten

Femorale Komponenten sind in verschiedenen Größen erhältlich. Porös beschichtete Komponenten sind für den biologischen Einbau vorgesehen. Modulare femorale Komponenten sind mit einem ovalen Taper zur Aufnahme von Smith & Nephew CoCr-Modulhalsen und/oder mit einem Morse-Taper zur Aufnahme von proximalen Ärmeln erhältlich. Nicht-poröse femorale Komponenten können mit Polyäthylenglycolmethacrylat (PMMA)-Zementierungen versehen werden, die zu einer gleichmäßigen Zementstärke beitragen.

Femorale Komponenten, die mit 10/12-, 12/14- und 14/16-Taperen erhältlich sind, passen direkt mit Smith & Nephew Femoral-Köpfen, die den gleichen Taper haben, zusammen. Bestimmte Femoral-Köpfe können Tapersleeves für die Verbindung zum Femoral-Stamm-Taper benötigen. Bitte auf die Tabelle in der Tapersleeves-Sektion für Details.

Kegelsleeves

Ein Tapersleeve kann erforderlich sein, wenn Femoral-Stämme mit bestimmten Typen von Femoral-Köpfen zusammengebracht werden sollen. Bitte auf die Tabelle der Tapersleeves-Kompatibilität für die entsprechenden Kombinationen. Ein falsches Tapersleeve-Verhältnis kann zu Implantatversagen und Revisionen führen. Setzen Sie nie mehr als einen Kegelsleeve auf ein Femoral-Komponente; dies erhöht die Belastung des Implantats und kann zu Versagen und Revisionen führen.

Modulare Halsen

Modulare Halsen bestehen aus CoCr-Legierung und sind in verschiedenen Konfigurationen erhältlich. Der modulare Hals passt zu einem ovalen Taper eines modulare femoralen Komponente auf einer Seite und zu einem 12/14-Femoral-Kopf auf der anderen Seite.

Kompatible Sleeve-Kombinationen

Femoraler Stamm-Taper	40, 44 mm Modulare CoCr Köpfe	40, 44 mm Modulare CoCr Köpfe	BH Modulare CoCr Köpfe	BANDEM [®] CoCr und CoCr Köpfe	14/16 ORION [®] und CoCr Köpfe
12/14	A	A	B	C	
14/16				D	Kein Sleeve erforderlich
10/12				E	F

* Modulare CoCr Köpfe sind aus CoCr-Legierung gefertigt und sind für den zementlosen Einsatz in den USA vorgesehen. Bitte auf das separate Packungsbeilage für die Komponenten.

** Der Modulare Kopf ist in den USA nicht verfügbar. Diese Köpfe können nur mit zementierten (Polyäthylenglycol) Femoral-Stämmen verwendet werden.

Sleeve	Material	Beschreibung/Teilnummern
A	Ti-6Al-4V	Ti-6Al-4V Modulhals
B	CoCr	4: 70344241, +0: 70344247, +8: 70344248, +8: 70344330
C	CoCr	4: 70222101, +0: 70222200, +8: 70222300, +8: 70222400
D	Ti-6Al-4V	3: 70226603, +0: 70226600, +8: 70226604, +8: 70226608
E	Ti-6Al-4V	14/16 12/14/12/14 Winkelhals
F	Ti-6Al-4V	10/12 12/14/14/14 Linearhals
G	Ti-6Al-4V	4: 80000004, +8: 80000008, +0: 80000008, +8: 80000012
H	Ti-6Al-4V	10/12 zu 14/16 Taper-Umwandlungshals
I	Ti-6Al-4V	+0: 80000008, +0: 80000012

Femoral-Köpfe

Für einen korrekten modulen und modulen Sitz, Kobalt-Chrom, Edelstahl, oxidiertes Zirkon und Keramik Köpfe sind in mehreren Halslängen erhältlich. Köpfe sind in 10/12-, 12/14- und 14/16-Taperen erhältlich. Bestimmte modulare Köpfe und Winkelköpfe können Tapersleeves zur Verbindung zum Femoral-Stamm-Taper benötigen. Bitte auf die Tabelle der Tapersleeves-Kompatibilität für die entsprechenden Kombinationen. Köpfe sind hochpoliert, um Reibung und Verschleiß zu reduzieren. Femoral-Komponenten und Femoral-Köpfe sind für den Einsatz mit jedem zementlosen Acetabulum-Komponente oder Polyäthylenglycol-Ärmel, Metall-Unterstützung-Acetabulum-Komponente oder zementiertes Acetabulum-Komponente, mit Ausnahme von Köpfen, die für den Einsatz mit zementierten Acetabulum-Komponenten vorgesehen sind.

REF ID: A1111 71352366
LOT BATCH CODE 19HM12856
REDAPT[®]
MODULAR

QTY: (1)
USE 2029-08-12

 smith&nephew

Shell

Schale • Cupule • Guscio • Shell • Cotilo • Skal • Pouzdro • Tabaka • Κορύλη •
Estrutura • Shell



66 MM OD



USE WITH R3° SIZE 66-70 MM OD LINER

MODULAR SHELL
TI-6AL-4V



(01) 00585556857898 (17) 290812 (10) 19HM12856



(11) 190815

STERILE R

STERILIZATION: ETHERILIZED

*Trademarks of Smith & Nephew.



2797

NO REUSE

CONSULT
INSTRUCTIONS



Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA



Smith & Nephew Orthopaedics GmbH,
Altmannstrasse 14, 78532 Tuttlingen,
Germany



CEMENTLESS

CAUTION




T49H18A7, 2




This carton is recyclable.

www.smith-nephew.com

**IX. Муфты модульные REDAPT, на примере вариантов исполнения:
Муфта модульная REDAPT, для ножек 12-13, размер XS**

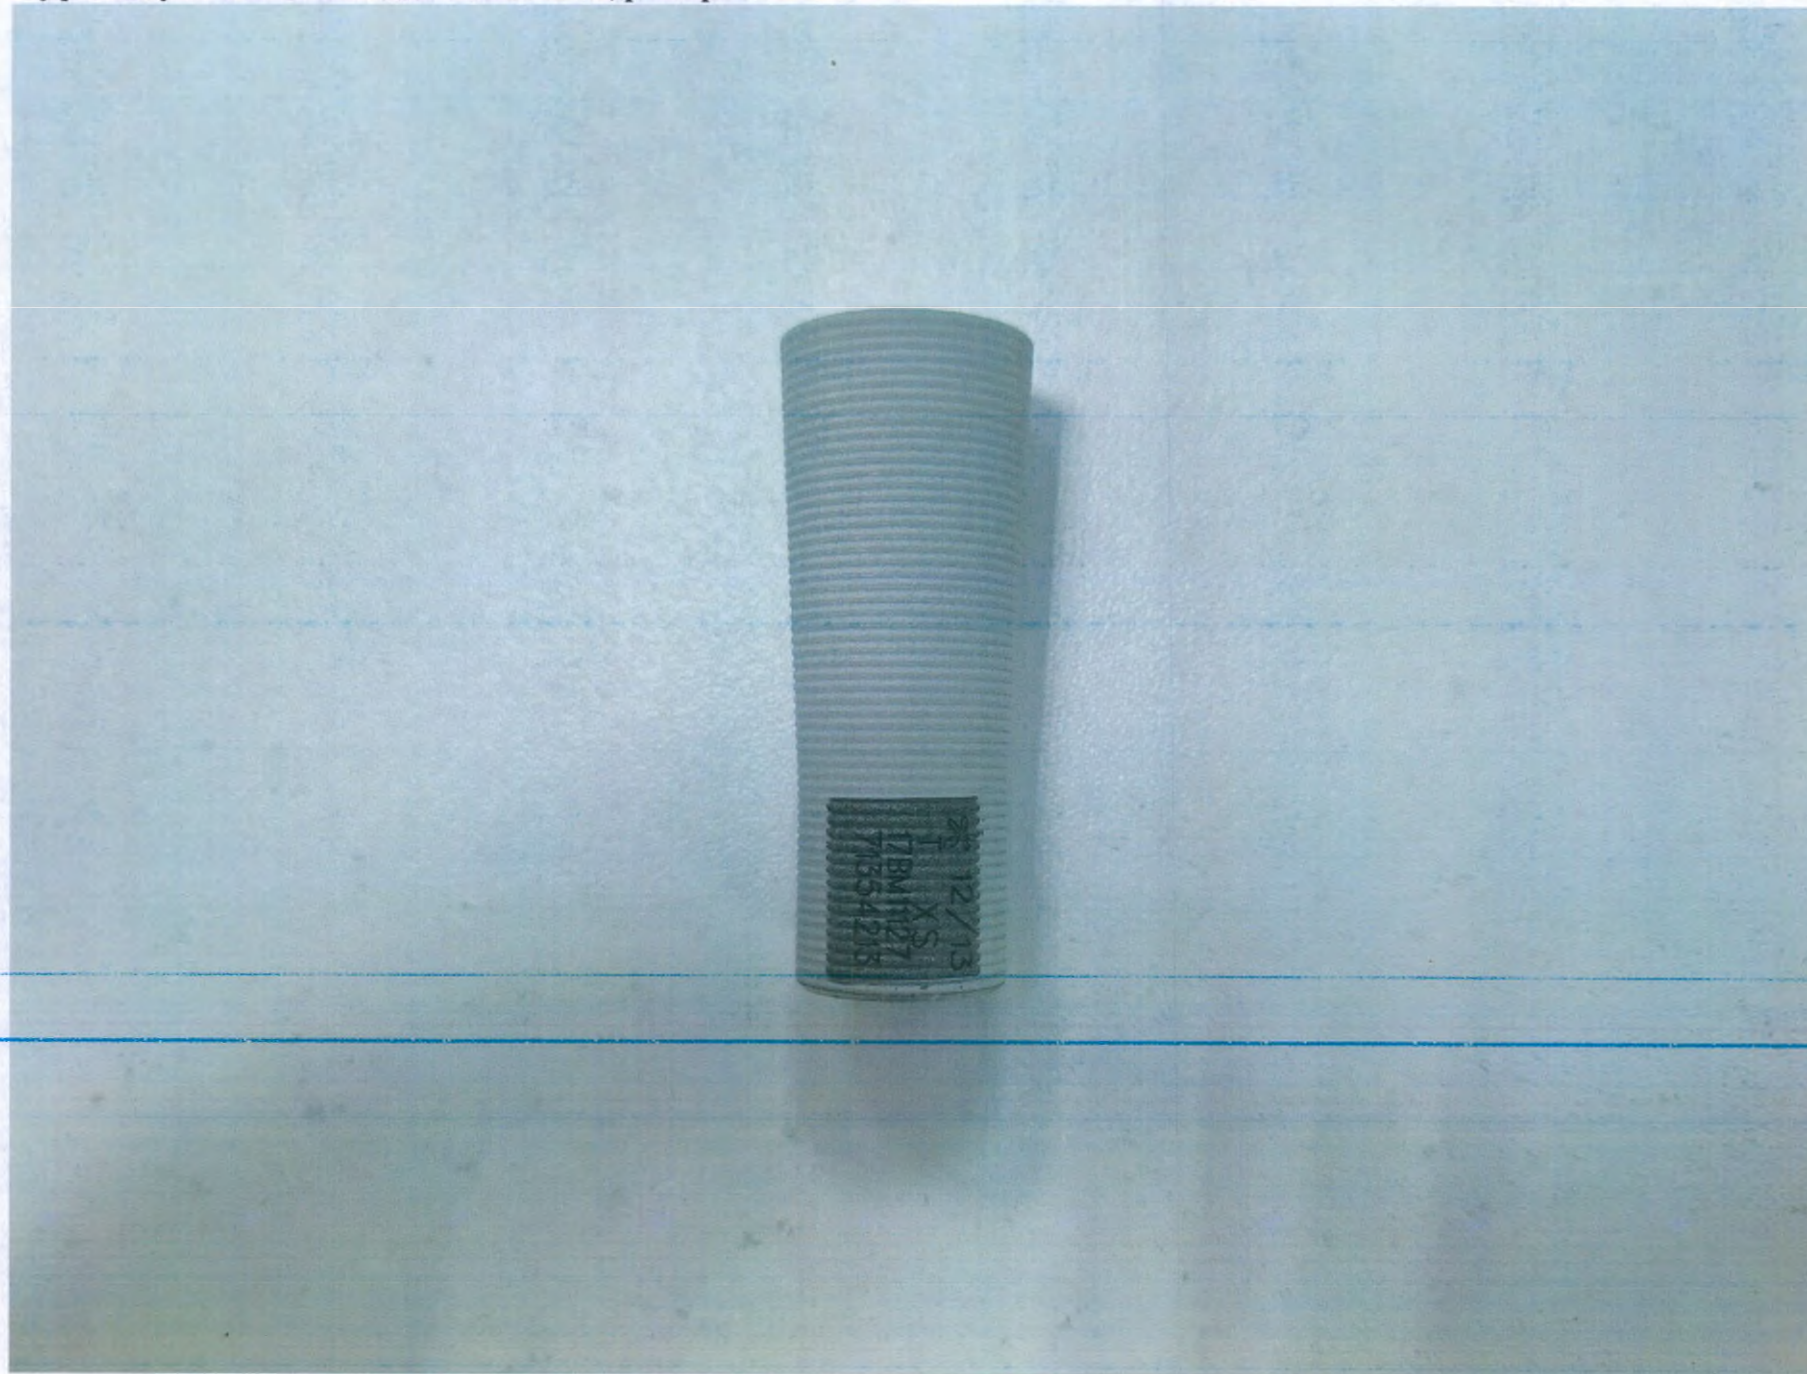

Индивидуальная упаковка: вкладыши и крышка лотка внутреннего

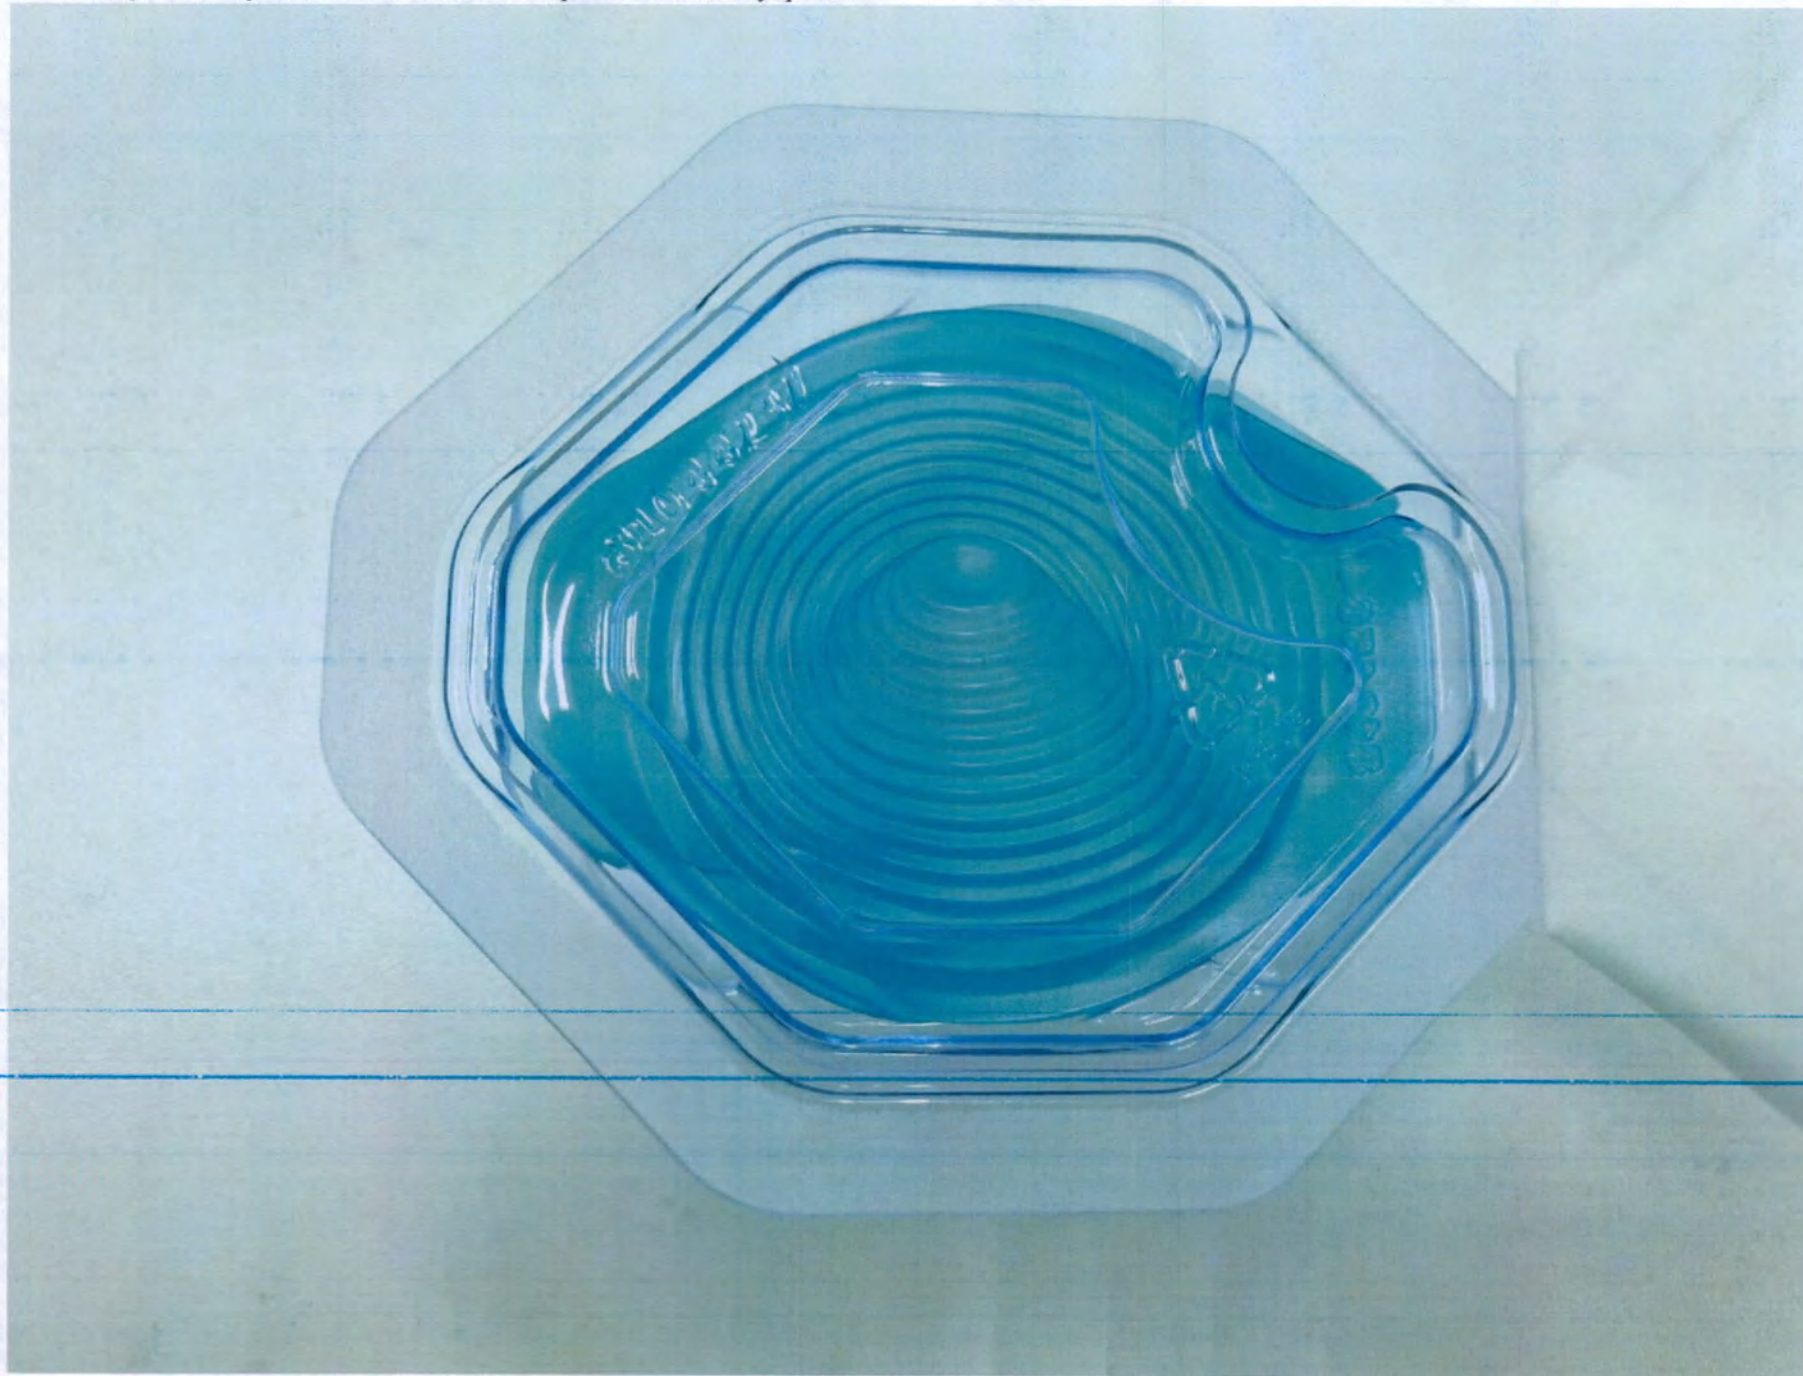

Индивидуальная упаковка: лоток внутренний.



Индивидуальная упаковка: лоток внутренний в лотке внешнем





CHART-STIK® LABEL

REF CATALOG 71354213

LOT BATCH CODE 17BM11127B

REDAPT® FEMORAL
SIZE 12-13 MODULAR SLEEVE
EXTRA SMALL
GRIT-BLASTED
TI-6AL-4V

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-06-11



(01) 00885556254219 (17) 270611 (10) 17BM11127B



(11) 170613

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF CATALOG 71354213

LOT BATCH CODE 17BM11127B

REDAPT® FEMORAL
SIZE 12-13 MODULAR SLEEVE
EXTRA SMALL
GRIT-BLASTED
TI-6AL-4V

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-06-11



(01) 00885556254219 (17) 270611 (10) 17BM11127B



(11) 170613

T94HSTIK; 4


ATTACH TO PATIENT'S RECORD

REF CATALOG NUMBER 71354213

LOT BATCH CODE 17BM11127B


REDAPT® FEMORAL
GRIT-BLASTED
Sleeve

Hüls • Manchon • Manicotto • Hülis • Manguito • Hüsa • Objímka • Kovan
• Типичный • Manga • Sleeve



USE BY 2027-06-11

QTY: (1)



12 - 13

Size

Größe • Taille • Misura • maat • Talla •
Storlek • Velikost • Boyut • Mărețoe •
Tamanho • Størrelse

smith&nephew

X-SMALL

USE ONLY WITH SMITH & NEPHEW STEMS

MODULAR SLEEVE
TI-6AL-4V



(01) 00885556254219 (17) 270811 (10) 17BM11127B



(11) 170813

STERILE R

RADIATION STERILIZED

Trademarks of Smith & Nephew.



Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA

EC REP

Smith & Nephew Orthopaedics GmbH,
Altmannstrasse 14, 78532 Tuttlingen,
Germany





C49H16AC, 5




This carton is recyclable.

www.smith-nephew.com

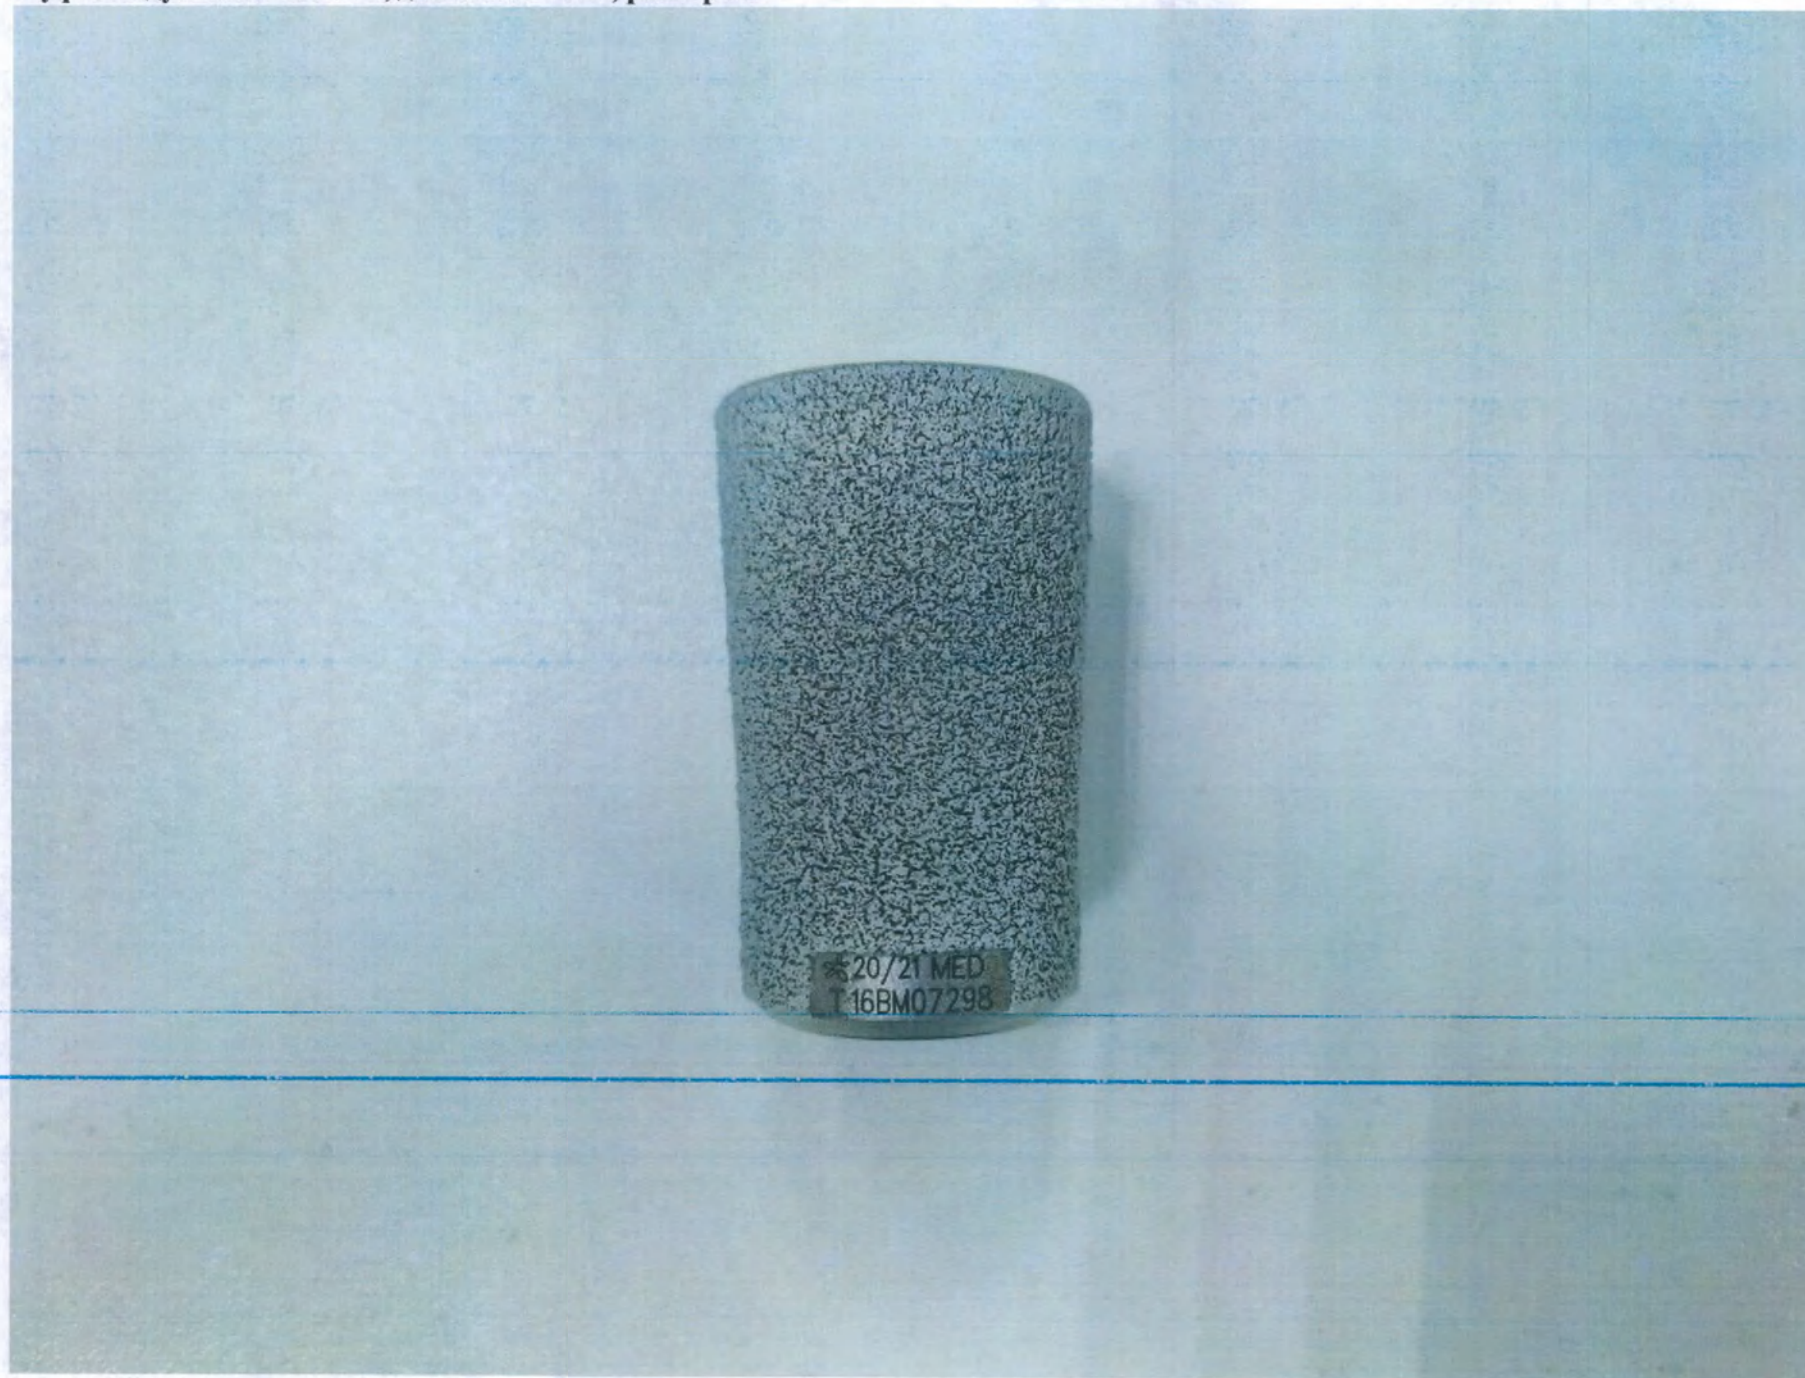

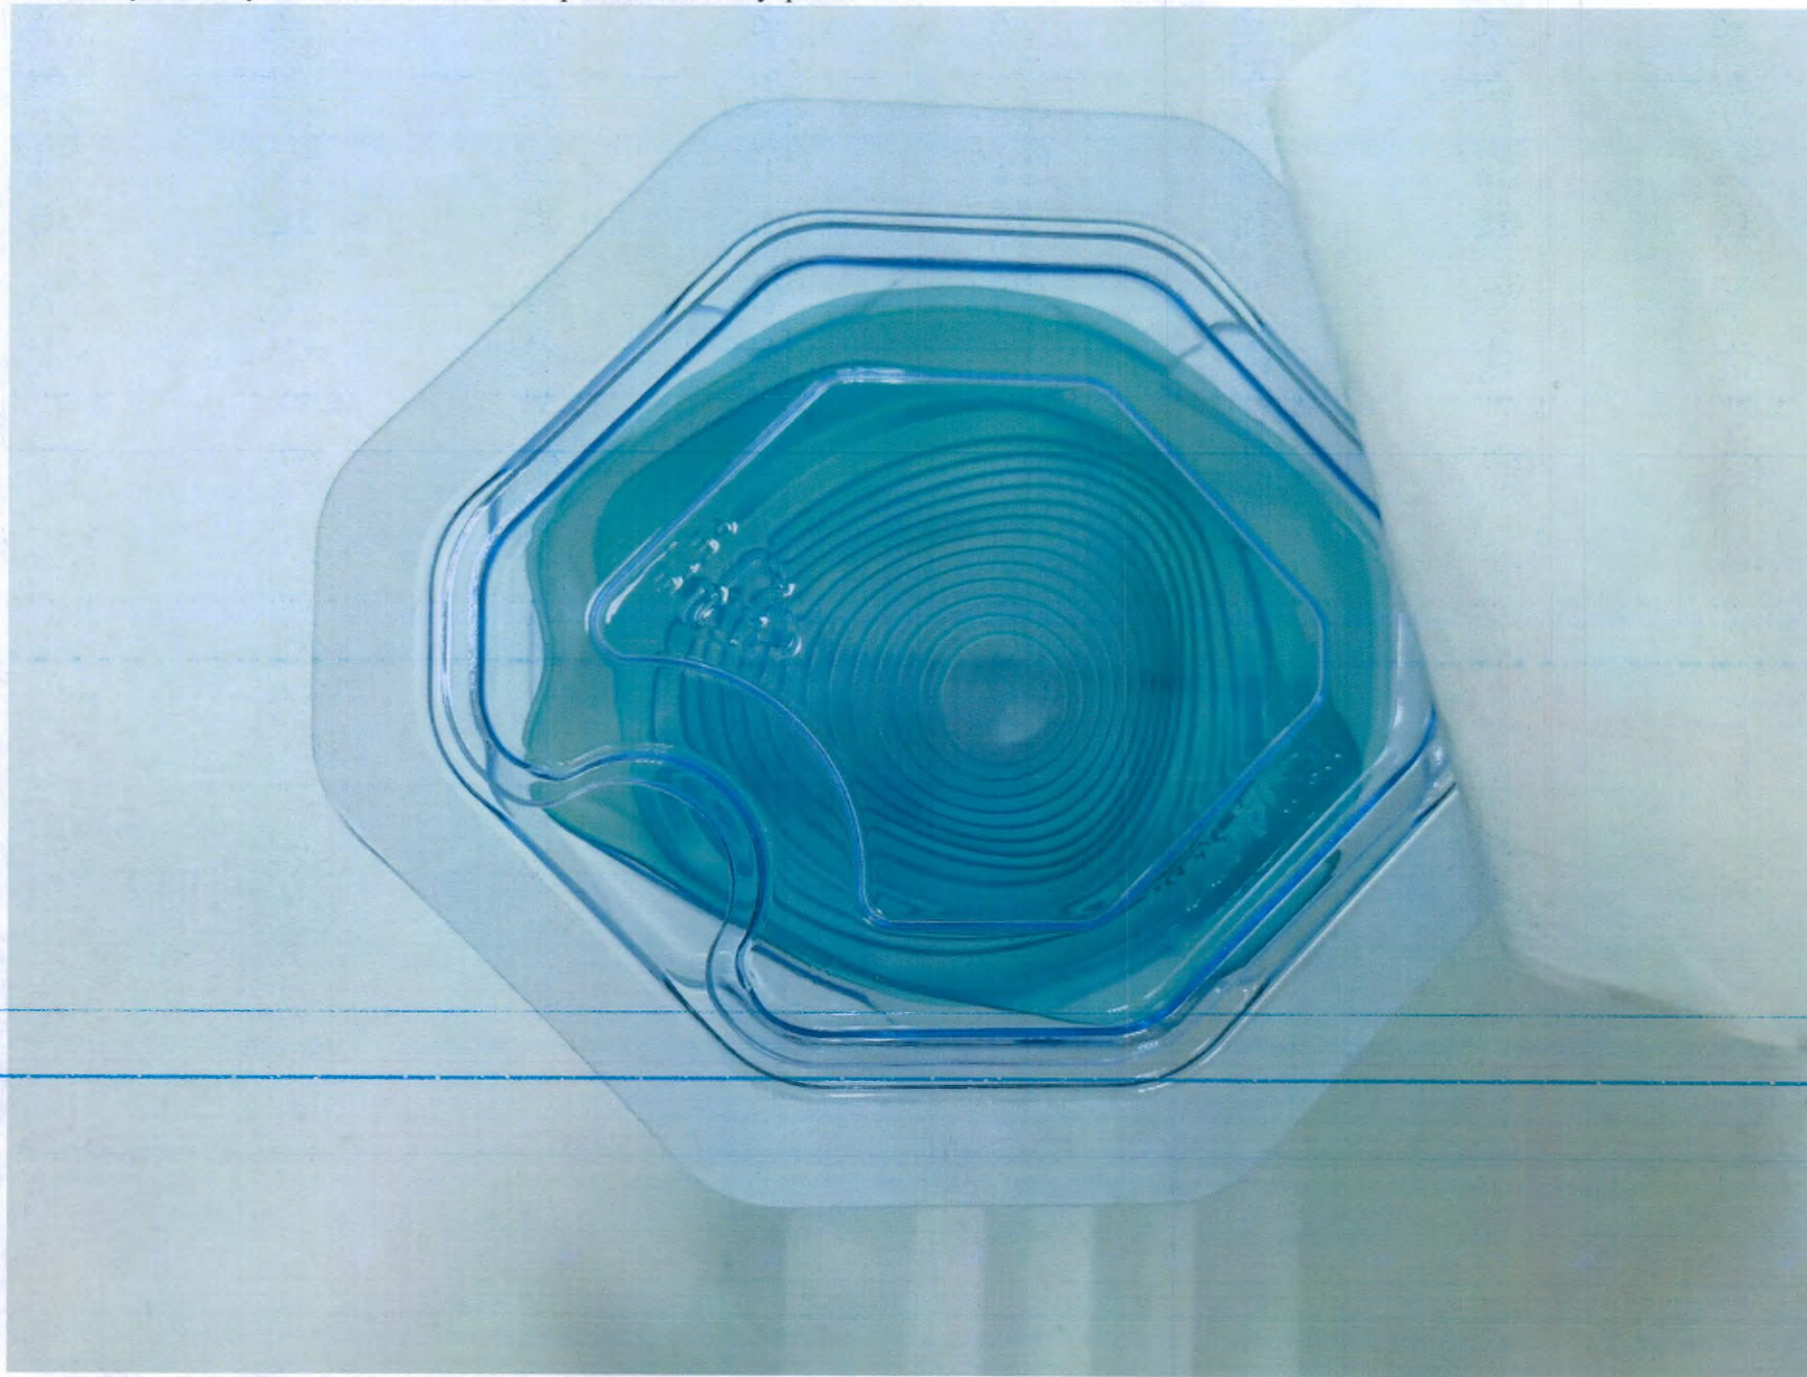

Индивидуальная упаковка: лоток внутренний.

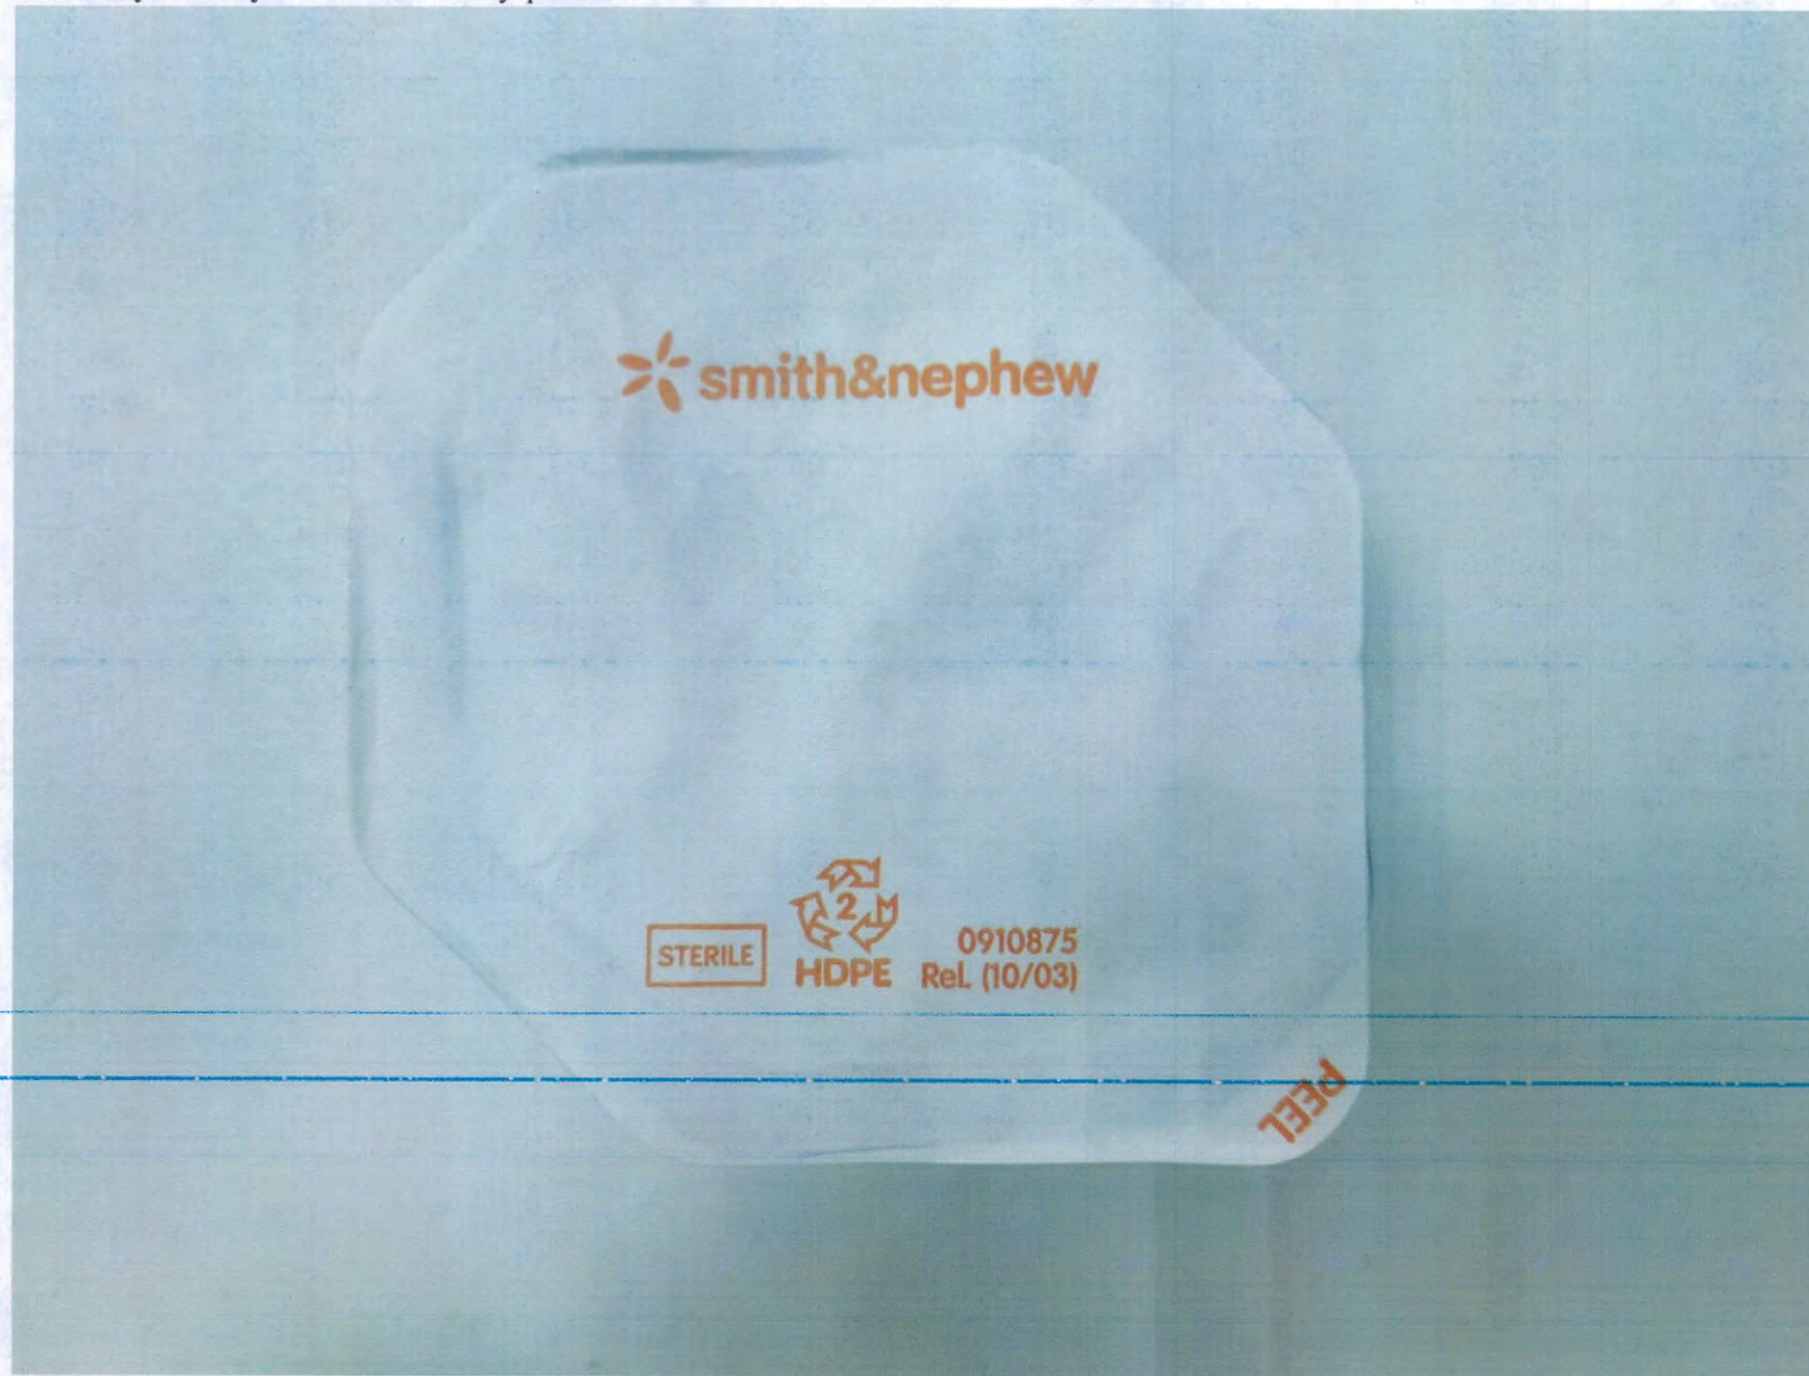

Индивидуальная упаковка: лоток внутренний в лотке внешнем





CHART-STIK® LABEL

REF CATALOG 71354045

LOT BATCH CODE 16BM07298A

REDAPT® FEMORAL
SIZE 20-21 MODULAR SLEEVE
MEDIUM
STIKTITE® COATED W/ HA
TI-6AL-4V

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2026-06-27



(01) 00885556023136 (17) 260627 (10) 16BM07298A



(11) 160629

T94HSTK, 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF CATALOG 71354045

LOT BATCH CODE 16BM07298A

REDAPT® FEMORAL
SIZE 20-21 MODULAR SLEEVE
MEDIUM
STIKTITE® COATED W/ HA
TI-6AL-4V

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2026-06-27



(01) 00885556023136 (17) 260627 (10) 16BM07298A



(11) 160629

T94HSTK, 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL

REF CATALOG 71354045

LOT BATCH CODE 16BM07298A


REDAPT® FEMORAL

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2026-06-27

ATTACH TO PATIENT'S RECORD

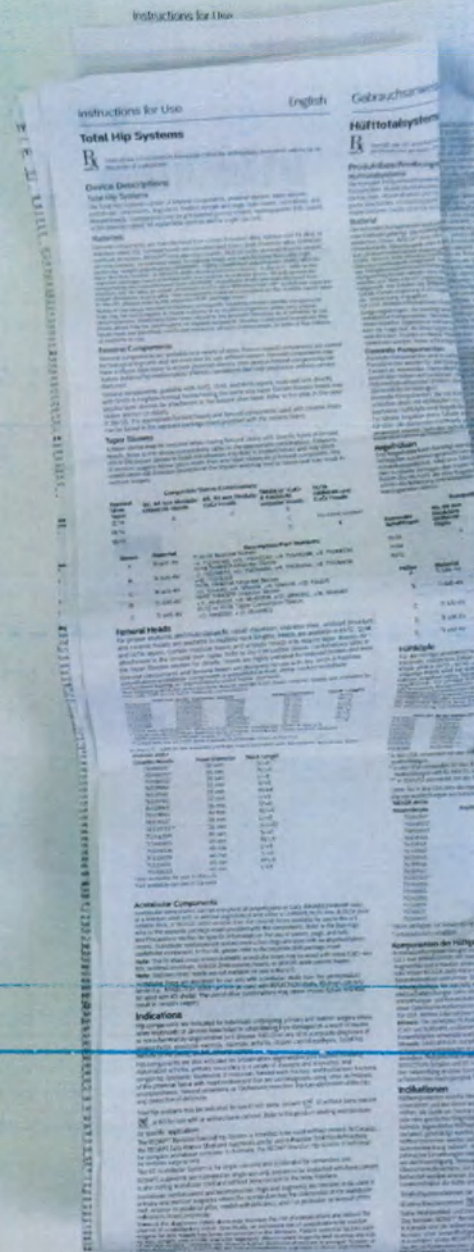



USE ONLY WITH SMITH & NEPHEW STEMS

MODULAR SLEEVE
TI-6AL-4V



(01) 00885558023136 (17) 260627 (10) 16BM07298A



(11) 160629

STERILE R

IRRADIATION STERILIZED

Trademarks of Smith & Nephew.



Smith & Nephew, Inc. 1450 Brooks Road,
Memphis, TN 38116 USA

EC REP

Smith & Nephew Orthopaedics GmbH,
Altmannstrasse 14, 78532 Tuttlingen,
Germany



C49H16AC, 5




www.smith-nephew.com

**Х. Ножки ревизионные REDAPT (под муфту), на примере вариантов исполнения:
Ножка ревизионная REDAPT (под муфту), стандартная, L 240 мм, размер 12.**




Индивидуальная упаковка: Изделие во внутреннем лотке

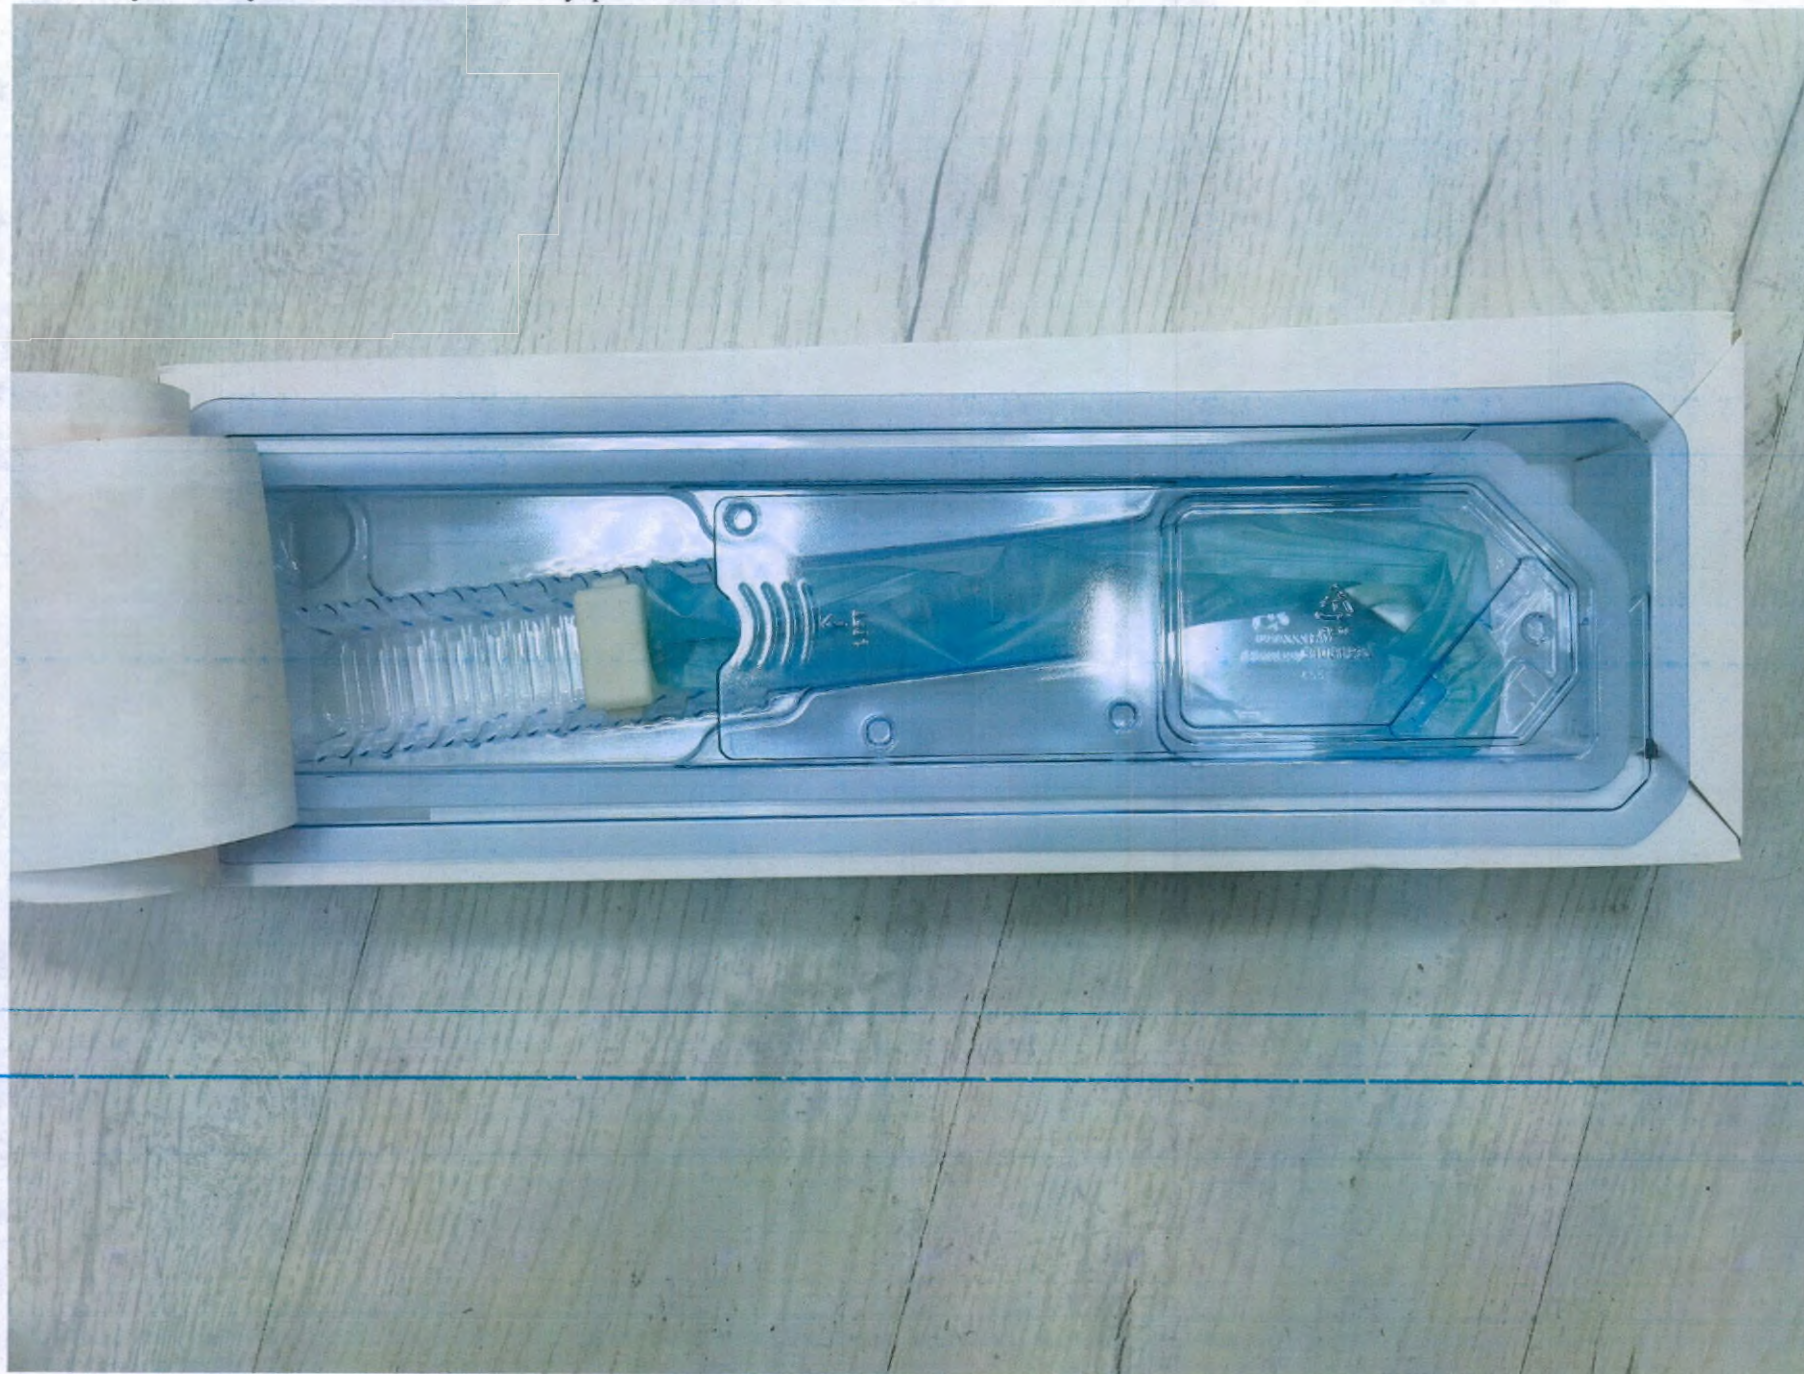

Индивидуальная упаковка: лоток внешний.



CHART-STIK® LABEL



REF CATALOG 71354801

LOT BATCH CODE 17CTM0101S

STERILE R

USE BY 2027-10-10

IRRADIATION STERILIZED

REDAPT® FEMORAL STANDARD OFFSET
SIZE 12, 240 MM LENGTH
SLEEVED STEM
REVISION FEMORAL COMPONENT
TI-6AL-4V



(01) 00885556579909 (17) 271010 (10) 17CTM0101S




(11) 171012

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL



REF CATALOG 71354801

LOT BATCH CODE 17CTM0101S

STERILE R

USE BY 2027-10-10

IRRADIATION STERILIZED

REDAPT® FEMORAL STANDARD OFFSET
SIZE 12, 240 MM LENGTH
SLEEVED STEM
REVISION FEMORAL COMPONENT
TI-6AL-4V



(01) 00885556579909 (17) 271010 (10) 17CTM0101S



(11) 171012

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

CHART-STIK® LABEL



REF CATALOG 71354801

LOT BATCH CODE 17CTM0101S


STERILE R


USE BY 2027-10-10

IRRADIATION STERILIZED

REDAPT® FEMORAL STANDARD OFFSET

S RECORD

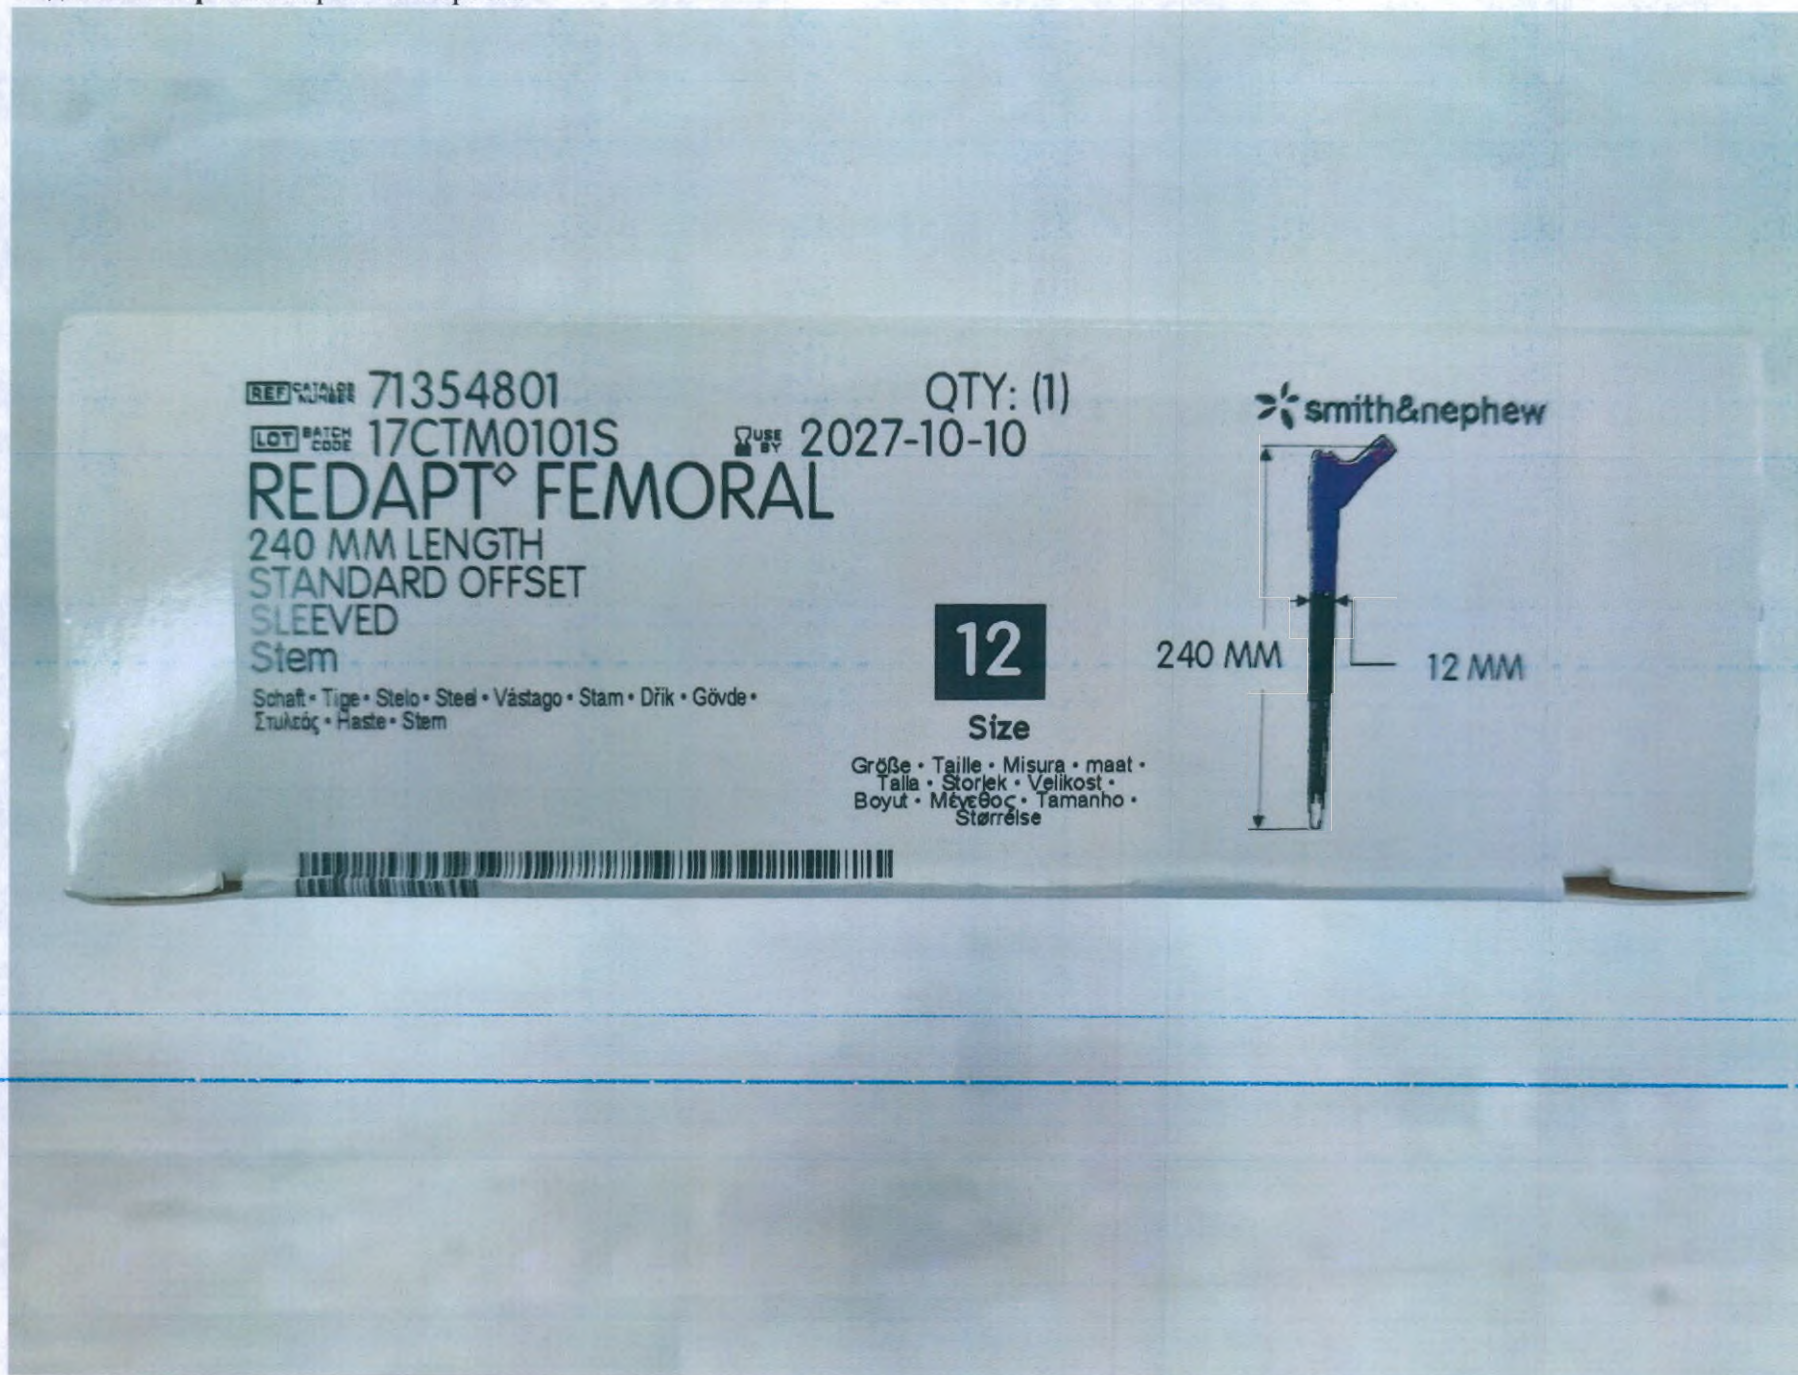


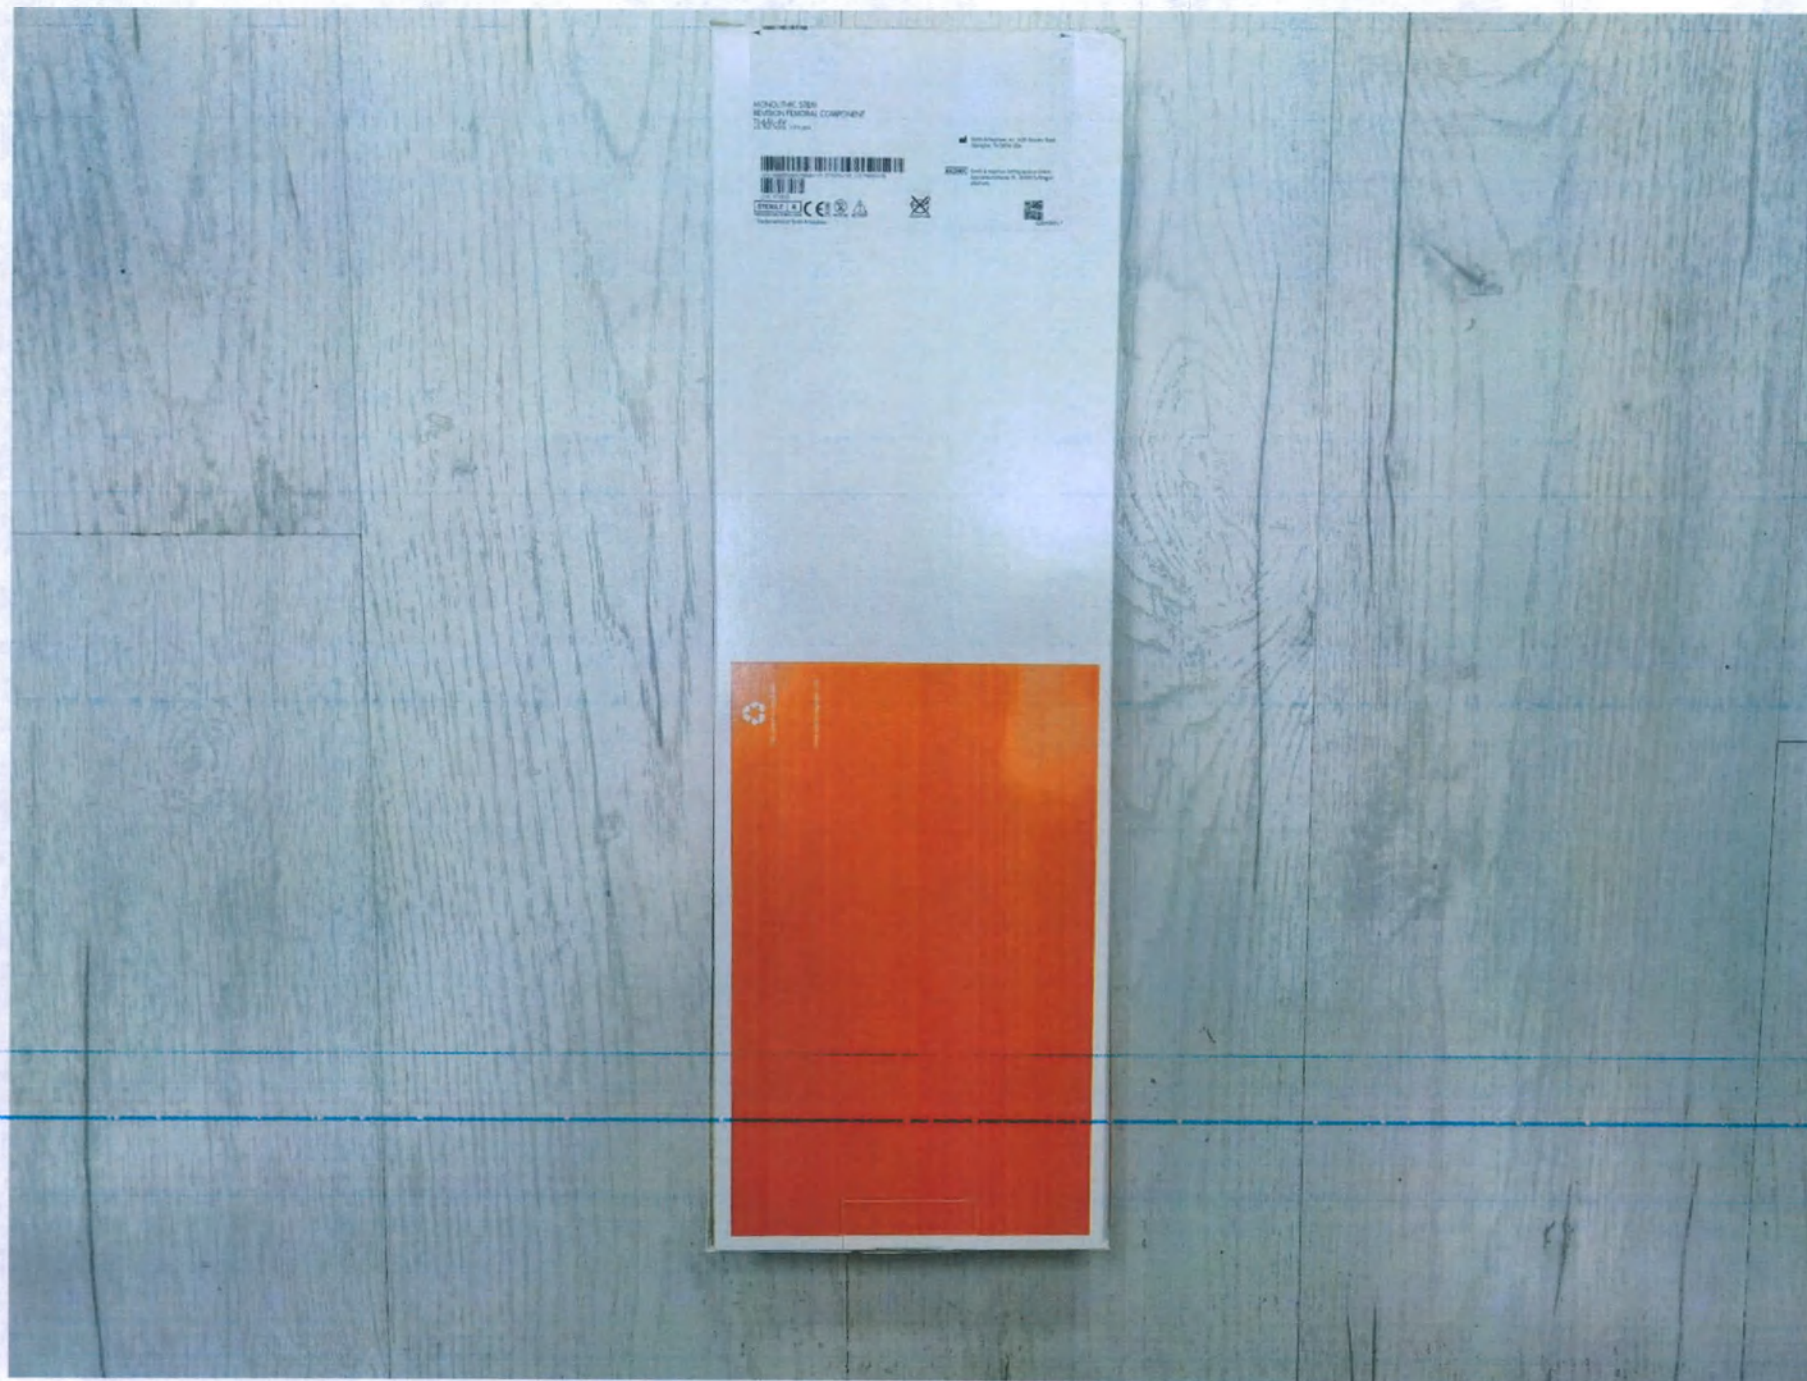

Ножка ревизионная REDAPT (под муфту), латерализованная, L 300 мм, размер 20.



Индивидуальная упаковка: изделие во внутреннем лотке

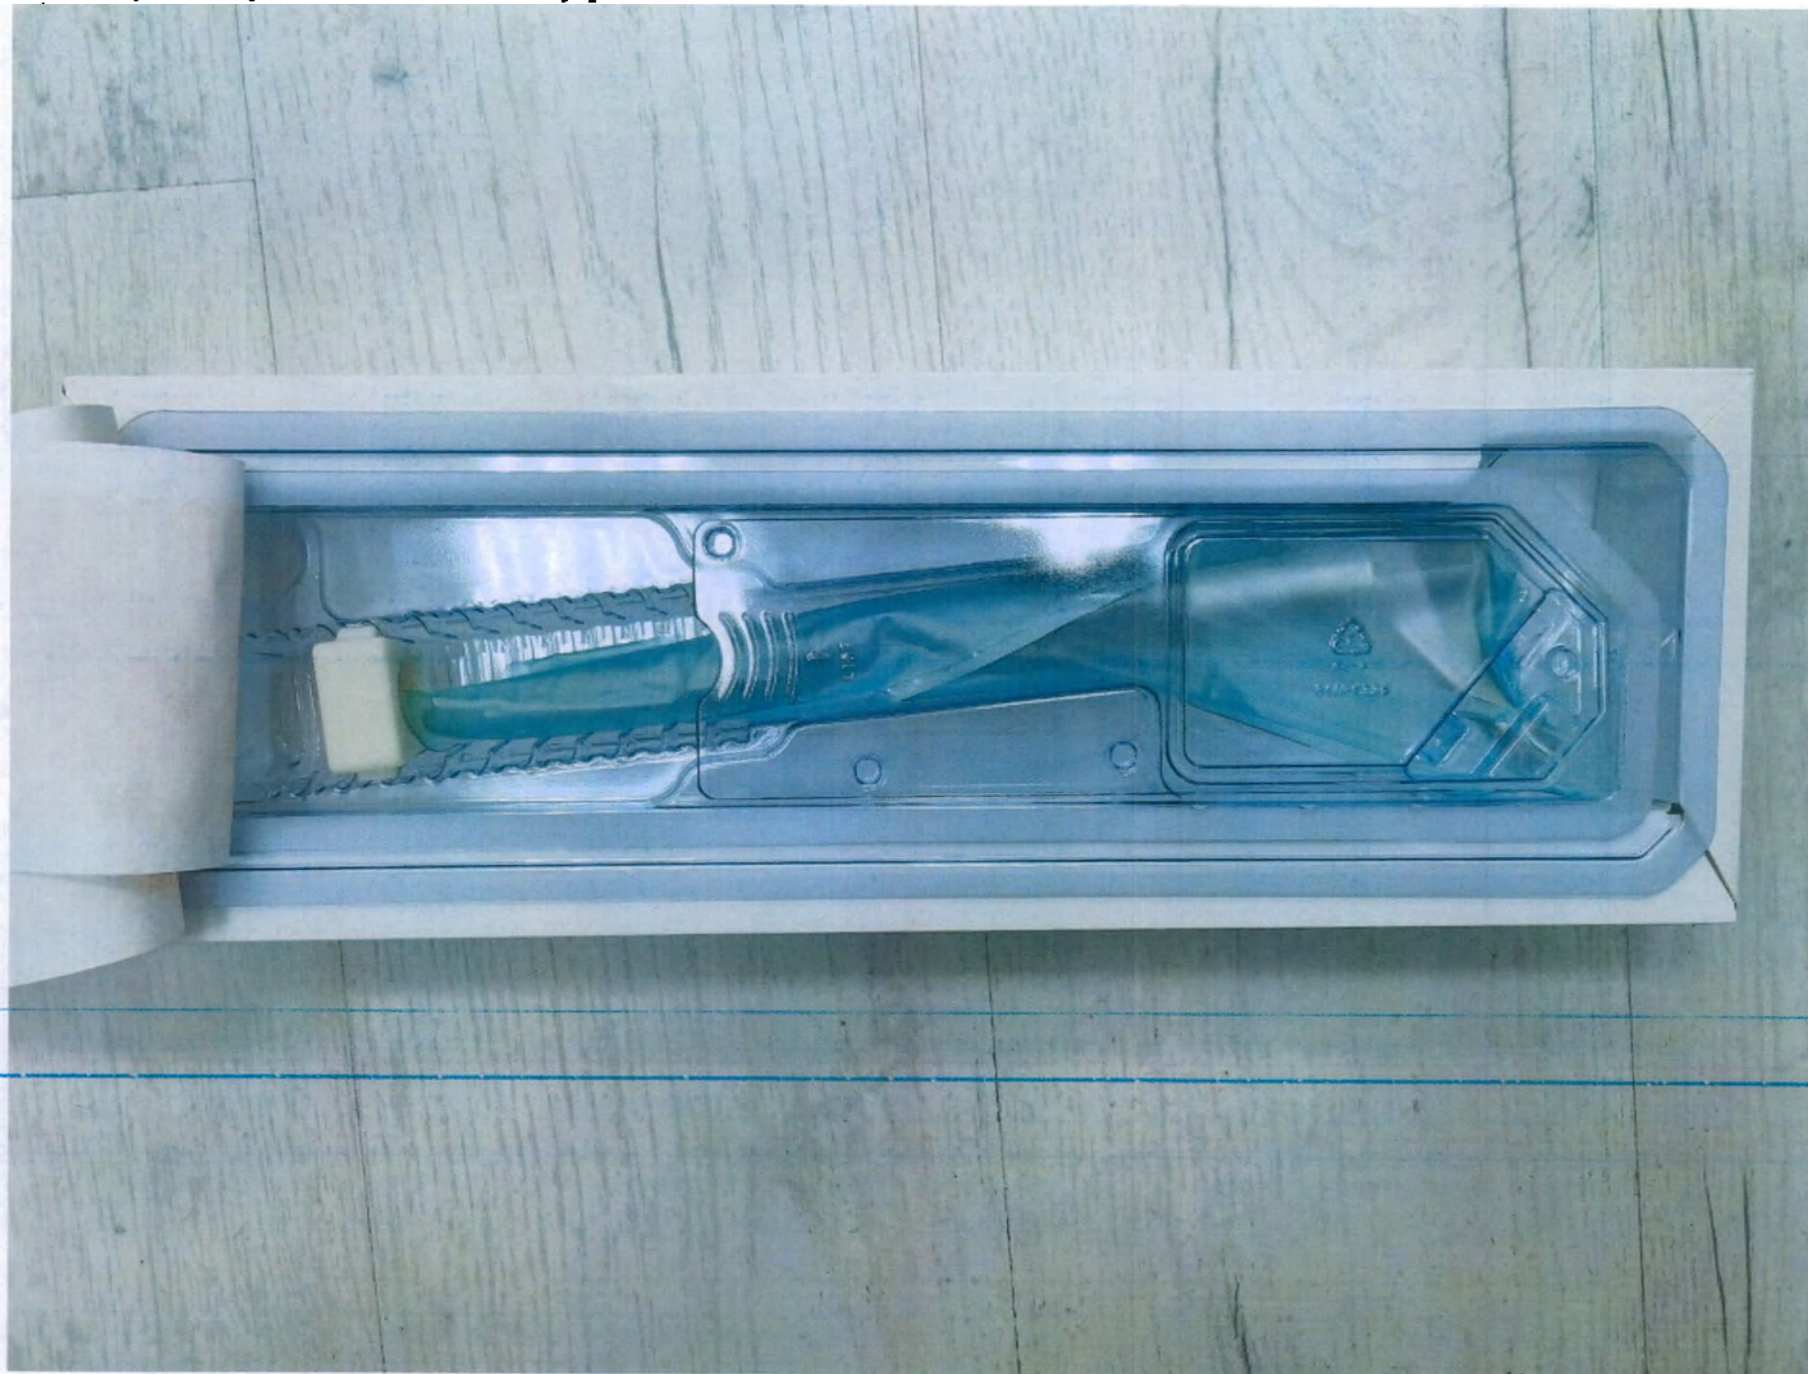

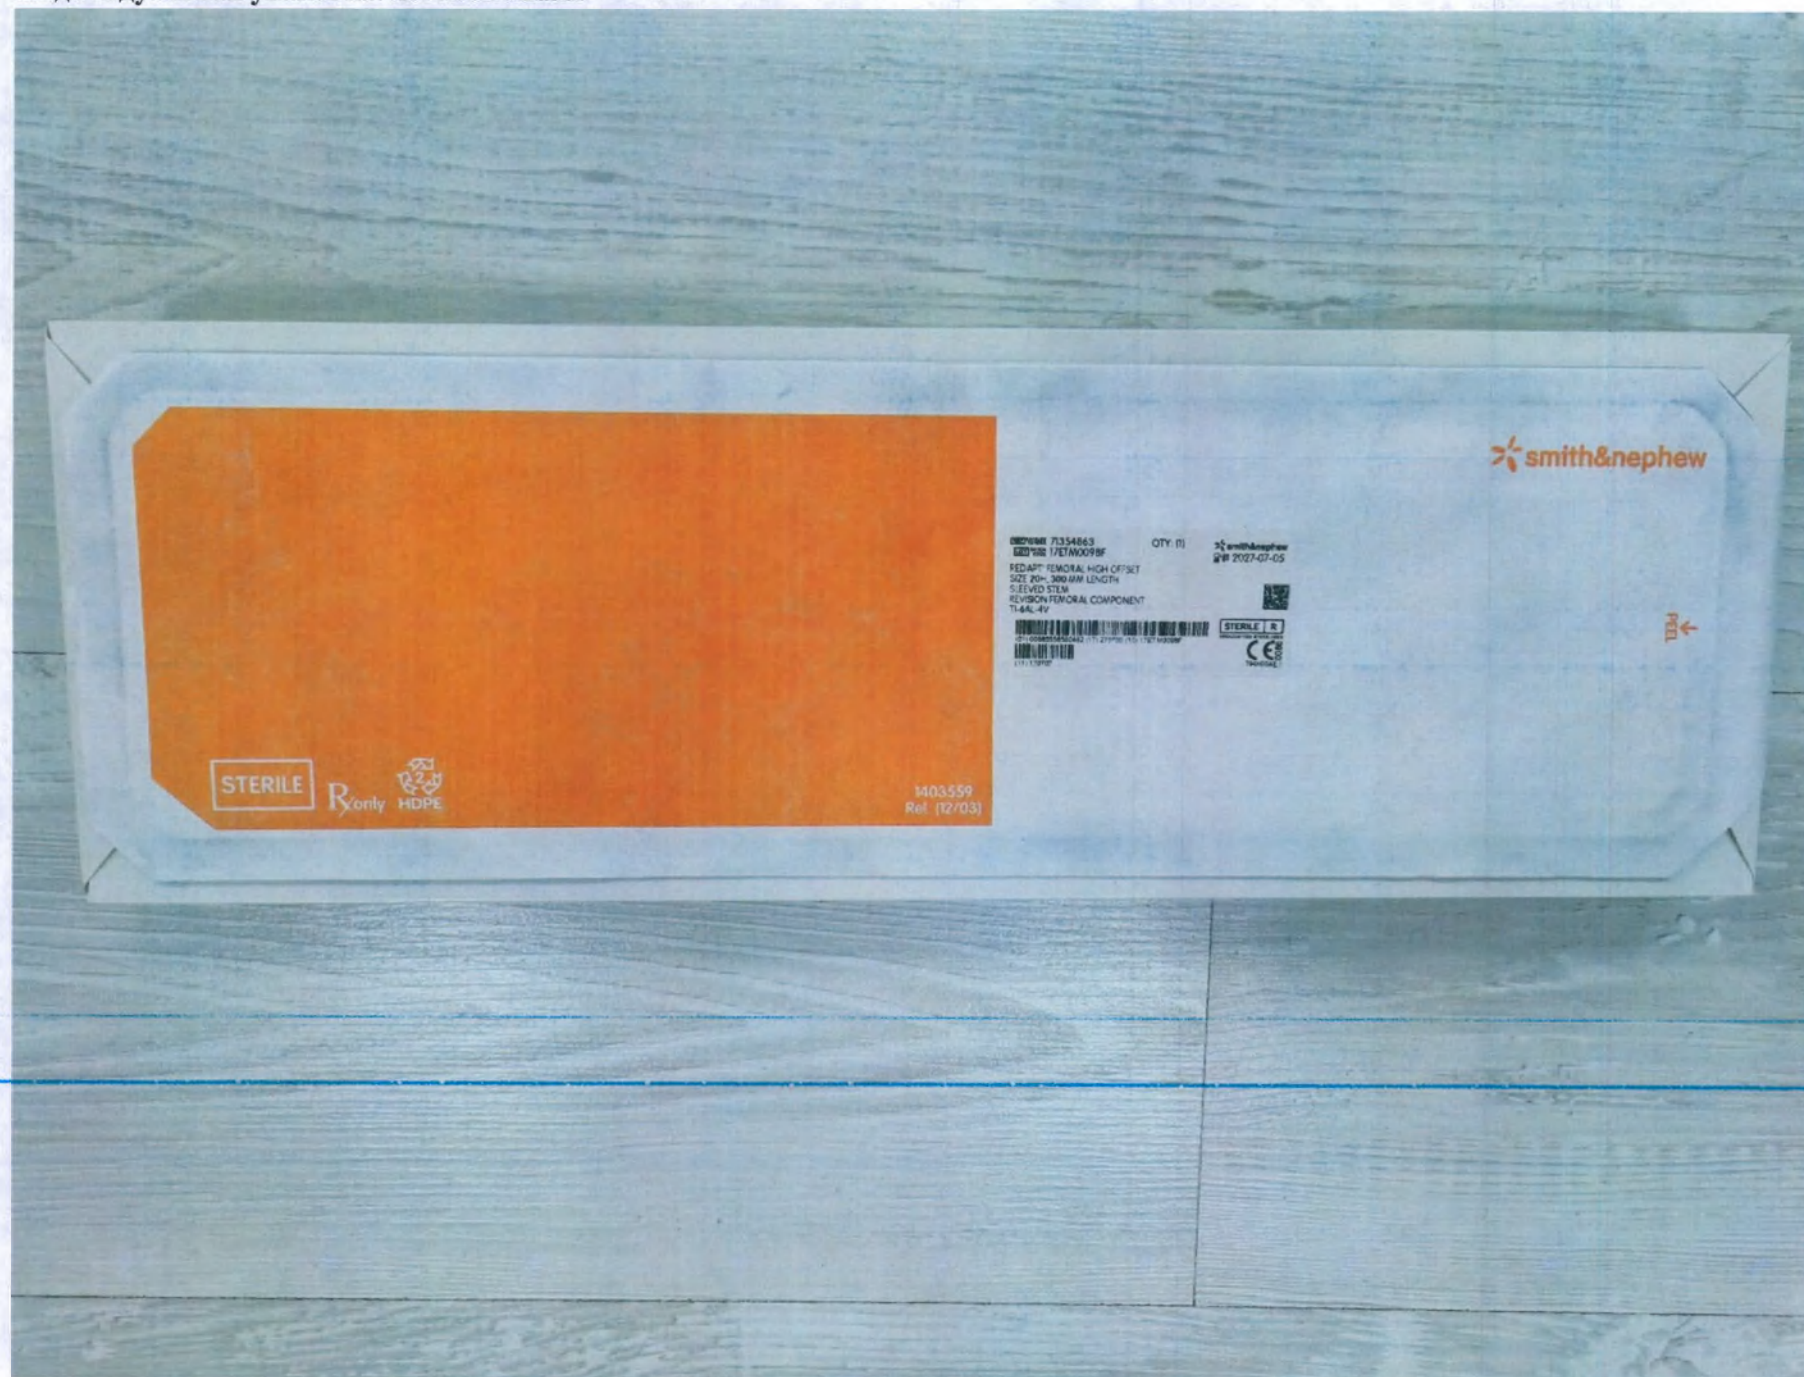


CHART-STIK® LABEL

REF NUMBER 71354863

LOT BATCH CODE 17ETM0098F

REDAPT® FEMORAL HIGH OFFSET

SIZE 20H, 300 MM LENGTH

SLEEVED STEM

REVISION FEMORAL COMPONENT

TI-6AL-4V

STERILE R
IRRADIATION STERILIZED

smith&nephew

EXP 2027-07-05



(01) 00865556580462 (17) 270705 (10) 17ETM0098F



(11) 170707

T94HSTIK; 4

ATTACH TO PATIENT'S RECORD

Instructions for Use

English

Gebrauchsanweisung

Total Hip Systems

R The total hip system is the most widely used hip prosthesis in the world. It consists of a femoral component, a acetabular component, and a femoral head.

Device Description

Total Hip System

The total hip system consists of a femoral component, a acetabular component, and a femoral head. The femoral component is made of titanium alloy and the acetabular component is made of ultra-high molecular weight polyethylene (UHMWPE).

Indications
The total hip system is indicated for the treatment of degenerative joint disease of the hip, trauma, and congenital hip dysplasia. It is also indicated for revision hip surgery.

Contraindications
The total hip system is contraindicated in patients with severe osteoporosis, active infection, or severe medical conditions that may affect the outcome of surgery.

Preoperative Preparation
The patient should be informed of the risks and benefits of the total hip system. Preoperative preparation includes blood work, chest X-ray, and physical therapy.

Postoperative Care
The patient should be monitored for pain, swelling, and redness. Physical therapy should be initiated as soon as possible. The patient should avoid high-impact activities for several months.

Complications
Complications of the total hip system include infection, dislocation, and wear. The risk of complications is higher in revision surgery.

Follow-up
The patient should be followed up regularly for the first two years after surgery. After two years, follow-up should be done every five years.

Storage
The total hip system should be stored in a clean, dry environment. It should not be exposed to moisture or extreme temperatures.

Warranty
The total hip system is warranted for a period of ten years. The warranty is void if the patient is not followed up regularly.

References
The following references provide additional information on the total hip system:

1. American Academy of Orthopaedic Surgeons. *Joint Replacement Surgery*. 2000.

2. British Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2001.

3. European Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2002.

4. International Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2003.

5. Japanese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2004.

6. Korean Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2005.

7. Russian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2006.

8. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2007.

9. Swedish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2008.

10. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2009.

11. Taiwanese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2010.

12. Thai Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2011.

13. Turkish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2012.

14. Vietnamese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2013.

15. Chinese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2014.

16. Indian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2015.

17. Pakistani Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2016.

18. Bangladeshi Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2017.

19. Nepalese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2018.

20. Sri Lankan Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2019.

21. Maldivian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2020.

22. Bhutanese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2021.

23. Mongolian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2022.

24. Kazakh Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2023.

25. Kyrgyz Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2024.

26. Tajik Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2025.

27. Turkmen Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2026.

28. Uzbek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2027.

29. Belarusian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2028.

30. Russian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2029.

31. Ukrainian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2030.

32. Polish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2031.

33. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2032.

34. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2033.

35. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2034.

36. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2035.

37. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2036.

38. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2037.

39. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2038.

40. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2039.

41. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2040.

42. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2041.

43. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2042.

44. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2043.

45. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2044.

46. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2045.

47. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2046.

48. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2047.

49. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2048.

50. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2049.

51. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2050.

52. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2051.

53. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2052.

54. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2053.

55. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2054.

56. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2055.

57. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2056.

58. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2057.

59. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2058.

60. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2059.

61. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2060.

62. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2061.

63. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2062.

64. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2063.

65. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2064.

66. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2065.

67. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2066.

68. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2067.

69. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2068.

70. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2069.

71. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2070.

72. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2071.

73. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2072.

74. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2073.

75. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2074.

76. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2075.

77. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2076.

78. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2077.

79. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2078.

80. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2079.

81. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2080.

82. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2081.

83. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2082.

84. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2083.

85. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2084.

86. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2085.

87. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2086.

88. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2087.

89. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2088.

90. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2089.

91. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2090.

92. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2091.

93. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2092.

94. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2093.

95. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2094.

96. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2095.

97. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2096.

98. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2097.

99. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2098.

100. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2099.

101. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2100.

102. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2101.

103. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2102.

104. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2103.

105. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2104.

106. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2105.

107. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2106.

108. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2107.

109. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2108.

110. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2109.

111. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2110.

112. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2111.

113. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2112.

114. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2113.

115. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2114.

116. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2115.

117. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2116.

118. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2117.

119. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2118.

120. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2119.

121. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2120.

122. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2121.

123. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2122.

124. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2123.

125. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2124.

126. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2125.

127. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2126.

128. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2127.

129. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2128.

130. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2129.

131. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2130.

132. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2131.

133. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2132.

134. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2133.

135. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2134.

136. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2135.

137. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2136.

138. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2137.

139. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2138.

140. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2139.

141. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2140.

142. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2141.

143. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2142.

144. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2143.

145. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2144.

146. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2145.

147. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2146.

148. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2147.

149. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2148.

150. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2149.

151. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2150.

152. Austrian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2151.

153. Czech Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2152.

154. Slovak Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2153.

155. Hungarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2154.

156. Romanian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2155.

157. Bulgarian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2156.

158. Greek Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2157.

159. Italian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2158.

160. French Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2159.

161. German Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2160.

162. Spanish Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2161.

163. Portuguese Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2162.

164. Dutch Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2163.

165. Belgian Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2164.

166. Swiss Society of Hip and Knee Surgeons. *Guidelines for Hip Replacement Surgery*. 2165.

REF CATALOG NUMBER 71354863

LOT BATCH CODE 17ETM0098F



USE BY 2027-07-05

QTY: (1)

REDAPT[®] FEMORAL

300 MM LENGTH

HIGH OFFSET

SLEEVED

Stem


Schaft • Tige • Stelo • Steel • Västago • Stam • Dřik • Gövde •
Stem • Haste • Stem

20H

Size

Größe • Taille • Misura • maat •
Talla • Storlek • Velikost • Boyut
• Μέγεθος • Tamanho •
Størrelse


 smith&nephew

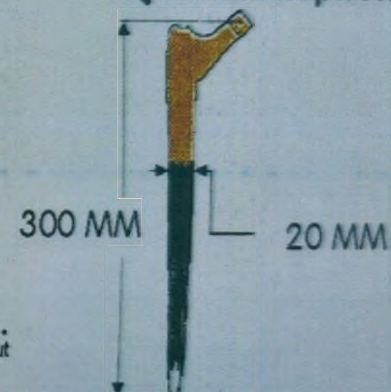





ПРОШТО И
ПРОНУМЕРОВАНО
162 ЛИСТОВ

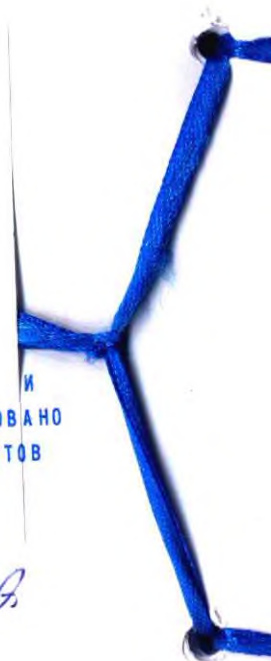


ООО «Смит энд Нефью»
Юр.адрес: 105120 г. Москва,
2-й Сыромятнический пер, 1
эт.9, пом.1, комн.1

Почт.адрес: 105120 г. Москва,
2-й Сыромятнический пер, 1

Т: + 7 495 755 55 03
www.smith-nephew.com
info.russia@smith-nephew.com

SmithNephew

«УТВЕРЖДАЮ»
Руководитель отдела
регистрации и нормативно-правовой
документации
ООО "Смит энд Нефью"
Хайруллина А.А.

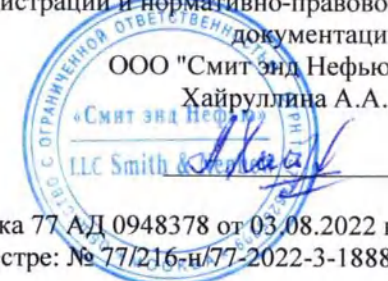

(Доверенность: б/н, № бланка 77 АД 0948378 от 03.08.2022 г.
Зарегистрировано в реестре: № 77/216-н/77-2022-3-1888)

«10» августа 2022 г.

Макеты русскоязычной маркировки

«Компоненты ревизионного протеза тазобедренного сустава REDAPT»

Производства

Smith & Nephew Inc. (Смит энд Нефью Инк.), USA (США).

2022

Ножки монолитные REDAPT, на примере варианта исполнения: Ножка ревизионная REDAPT монолитная, стандартная, L 190 мм, размер 19

Артикул: 71354468

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Ножка ревизионная REDAPT монолитная, стандартная, L 190 мм, размер 19

Размер: L 190 мм, размер 19

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул, длина и размер изделия

Ножки монолитные REDAPT, на примере варианта исполнения: Ножка ревизионная REDAPT монолитная, латерализованная, L 190 мм, размер 15

Артикул: 71354482

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Ножка ревизионная REDAPT монолитная, латерализованная, L 190 мм, размер 15

Размер: L 190 мм, размер 15

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул, длина и размер изделия

Чашки пористые REDAPT, на примере варианта исполнения: Чашка пористая REDAPT, 52 мм

Артикул: 71354231

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Чашка пористая REDAPT, 52 мм

Размер: 52 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifu/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Вкладыши цементируемые REDAPT, на примере варианта исполнения: Вкладыш цементируемый REDAPT, XLPE, 0°, 36/54 мм

Артикул: 71354522

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Вкладыш цементируемый REDAPT, XLPE, 0°, 36/54 мм

Размер: 0°, 36/54 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Стерилизация этиленоксидом

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Вкладыши цементируемые REDAPT, на примере варианта исполнения: Вкладыш цементируемый REDAPT, XLPE, 20°, 40/58 мм

Артикул: 71354226

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Вкладыш цементируемый REDAPT, XLPE, 20°, 40/58 мм

Размер: 20°, 40/58 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Стерилизация этиленоксидом

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Винты блокирующие REDAPT, на примере варианта исполнения: Винт блокирующий REDAPT, 25 мм

Артикул: 71354504

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Винт блокирующий REDAPT, 25 мм

Размер: 25 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifu/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Набор заглушек REDAPT

Артикул: 71354240

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Набор заглушек REDAPT, в составе: 1) заглушка отверстия - 14 шт, 2) установщик заглушек - 2 шт

Размер: -

Кол-во шт. в упаковке: 14 шт и 2 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Стерилизация этиленоксидом

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Блоки замещающие REDAPT, на примере варианта исполнения: Блок замещающий REDAPT, сегментарный, 56 x 12 мм

Артикул: 71354412

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Блок замещающий REDAPT сегментарный, 56 x 12 мм

Размер: 56 x 12 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifu/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Блоки замещающие REDAPT, на примере варианта исполнения: Блок замещающий REDAPT, "скоба", 56 x 12 мм

Артикул: 71354442

Наименование: Компоненты ревизионного протеза тазобедренного сустава REDAPT: Блок замещающий REDAPT "скоба", 56 x 12 мм

Размер: 56 x 12 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Блоки замещающие REDAPT, на примере варианта исполнения: Блок замещающий REDAPT, клинковый – основание, 62 мм

Артикул: 71354428

Наименование: Компоненты протеза тазобедренного сустава REDAPT: Блок замещающий REDAPT клинковый - основание, размер 62 мм

Размер: 62 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifu/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Блоки замещающие REDAPT, на примере варианта исполнения: Блок замещающий REDAPT, клинковый - крыло

Артикул: 71354431

Наименование: Компоненты протеза тазобедренного сустава REDAPT: Блок замещающий REDAPT клинковый - крыло

Размер: -

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Чашки модульные REDAPT, на примере варианта исполнения: Чашка модульная REDAPT, 60 мм

Артикул: 71352360

Наименование: Компоненты протеза тазобедренного сустава REDAPT: Чашка модульная REDAPT, 60 мм

Размер: 60 мм

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Муфты модульные REDAPT, на примере варианта исполнения: Муфта модульная REDAPT, для ножек 18-19 мм, размер М

Артикул: 71354044

Наименование: Компоненты протеза тазобедренного сустава REDAPT:Муфта модульная REDAPT, для ножек 18-19, размер М

Размер: М

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул и размер изделия

Ножки ревизионные REDAPT (под муфту), на примере варианта исполнения: Ножка ревизионная REDAPT, стандартная, L 240 мм, размер 15

Артикул: 71354804

Наименование: Компоненты протеза тазобедренного сустава REDAPT: Ножка ревизионная REDAPT (под муфту), стандартная, L 240 мм, размер 15

Размер: 15

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifu/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул, длина и размер изделия

Ножки ревизионные REDAPT (под муфту), на примере варианта исполнения: Ножка ревизионная REDAPT, латерализованная, L 240 мм, размер 15

Артикул: 71354833

Наименование: Компоненты протеза тазобедренного сустава REDAPT: Ножка ревизионная REDAPT (под муфту), латерализованная, L 240 мм, размер 25

Размер: 25

Кол-во шт. в упаковке: 1 шт

Дата изготовления, использовать до, номер партии/серии: См. на упаковке

Наименование и адрес изготовителя: "Смит энд Нефью, Инк.", США, Smith & Nephew, Inc., 1450 Brooks Road, Memphis, Tennessee 38116, USA

Уполномоченный представитель на территории РФ: ООО "Смит энд Нефью", 105120, Россия, Москва, 2-й Сыромятнический пер., д. 1, этаж 9, пом. 1, комн. 1

Метод стерилизации: Радиационная стерилизация

Номер РУ: РЗН 2020/9750

Назначение, способ применения, противопоказания: См. инструкцию

Условия хранения: при температуре от -20...35°C, влажности от 40...90%, атмосферном давлении от 86.6...106.7кПа

Меры предосторожности: -

Инструкция по применению: <http://www.smith-nephew.com/about-us/where-we-operate/europe/russia/ifus/>

Примечание: в зависимости от варианта исполнения на маркировке может изменяться артикул, длина и размер изделия



ПРОШТО И
ПРОНУМЕРОВАНО
16 ЛИСТОВ

Лагутина Р.А.