


Фотографические изображения медицинского изделия

Контрольные материалы для контроля характеристик системы анализа качественного определения антител класса IgG к вирусу SARS-CoV-2 в сыворотке и плазме крови человека, иммунохемилюминесцентным методом для диагностики *in vitro* на анализаторах иммунохимических серии ACCESS system (ACCESS SARS-CoV-2 IgG QC) (LOT 124874)

2021 г.



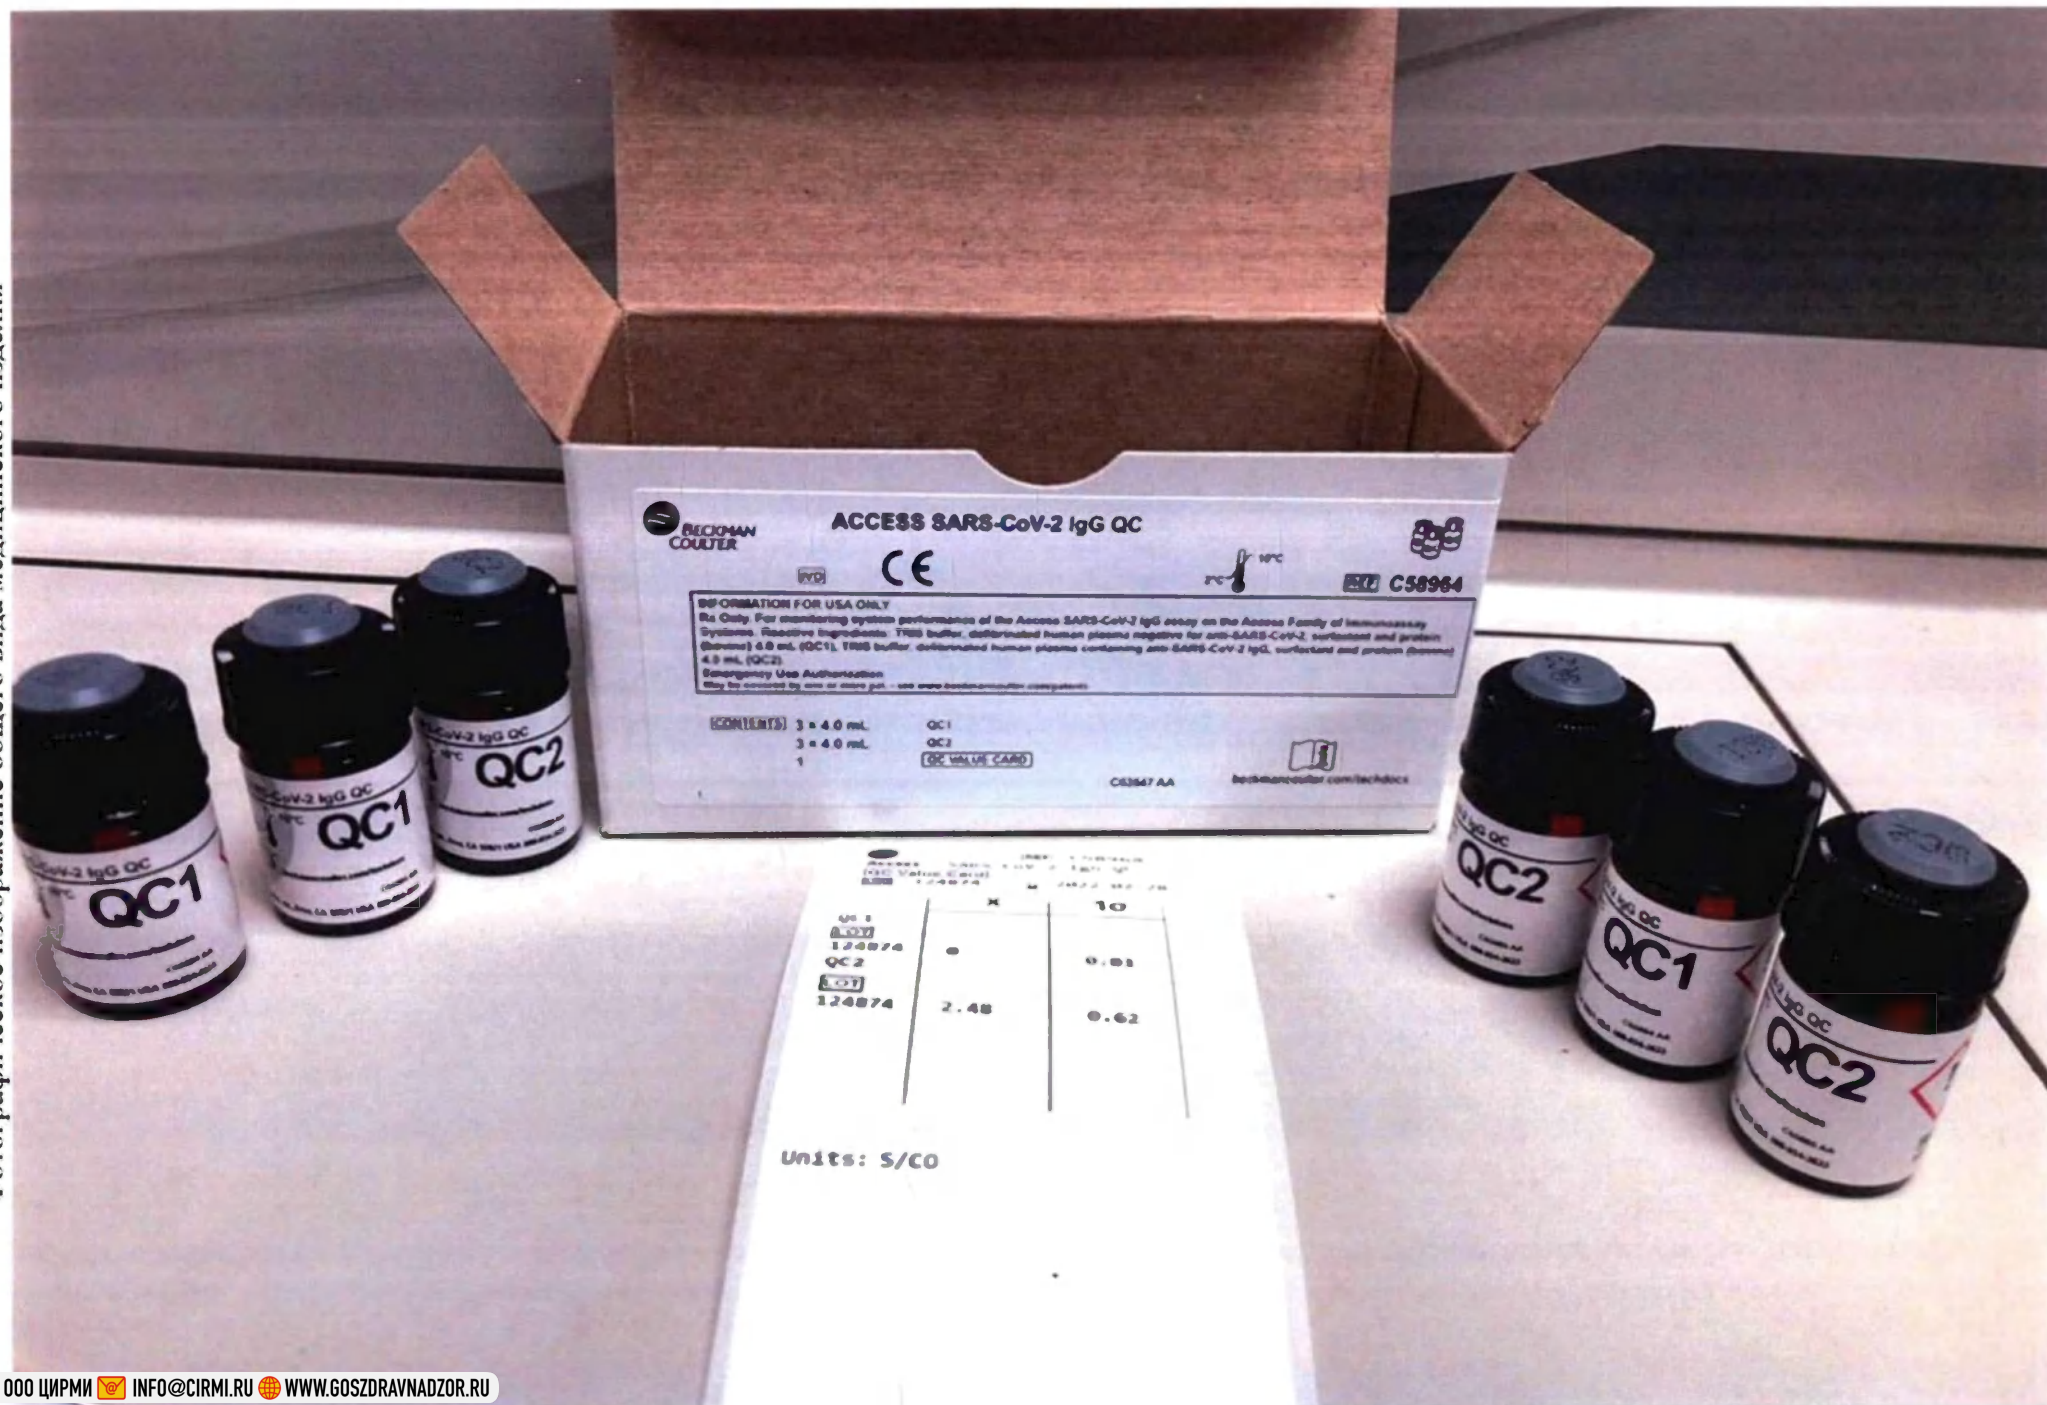



ACCESS SARS-CoV-2 IgG QC

IVD



2°C 10°C



REF C58964

INFORMATION FOR USA ONLY

Rx Only. For monitoring system performance of the Access SARS-CoV-2 IgG assay on the Access Family of Immunoassay Systems. Reactive Ingredients: TRIS buffer, defibrinated human plasma negative for anti-SARS-CoV-2, surfactant and protein (bovine) 4.0 mL (QC1), TRIS buffer, defibrinated human plasma containing anti-SARS-CoV-2 IgG, surfactant and protein (bovine) 4.0 mL (QC2).

Emergency Use Authorization

May be covered by one or more pat. - see www.beckmancoulter.com/patents

CONTENTS 3 x 4.0 mL
3 x 4.0 mL
1

QC1
QC2

QC VALUE CARD

C63547 AA



beckmancoulter.com/techdocs



REF C58964

Access SARS-CoV-2 IgG QC

QC Value Card

LOT 124874

 2022-02-28

	$\bar{x}$	1σ
QC1		
LOT		
124874	0	0.03
QC2		
LOT		
124874	2.48	0.62

Units: S/CO

A54420A

ПРОШТО, ПРОНУМЕРАВАНО
И СКРЕПЛЕНО ПЕЧАТЈУ

5 ЛИСТОВ

