




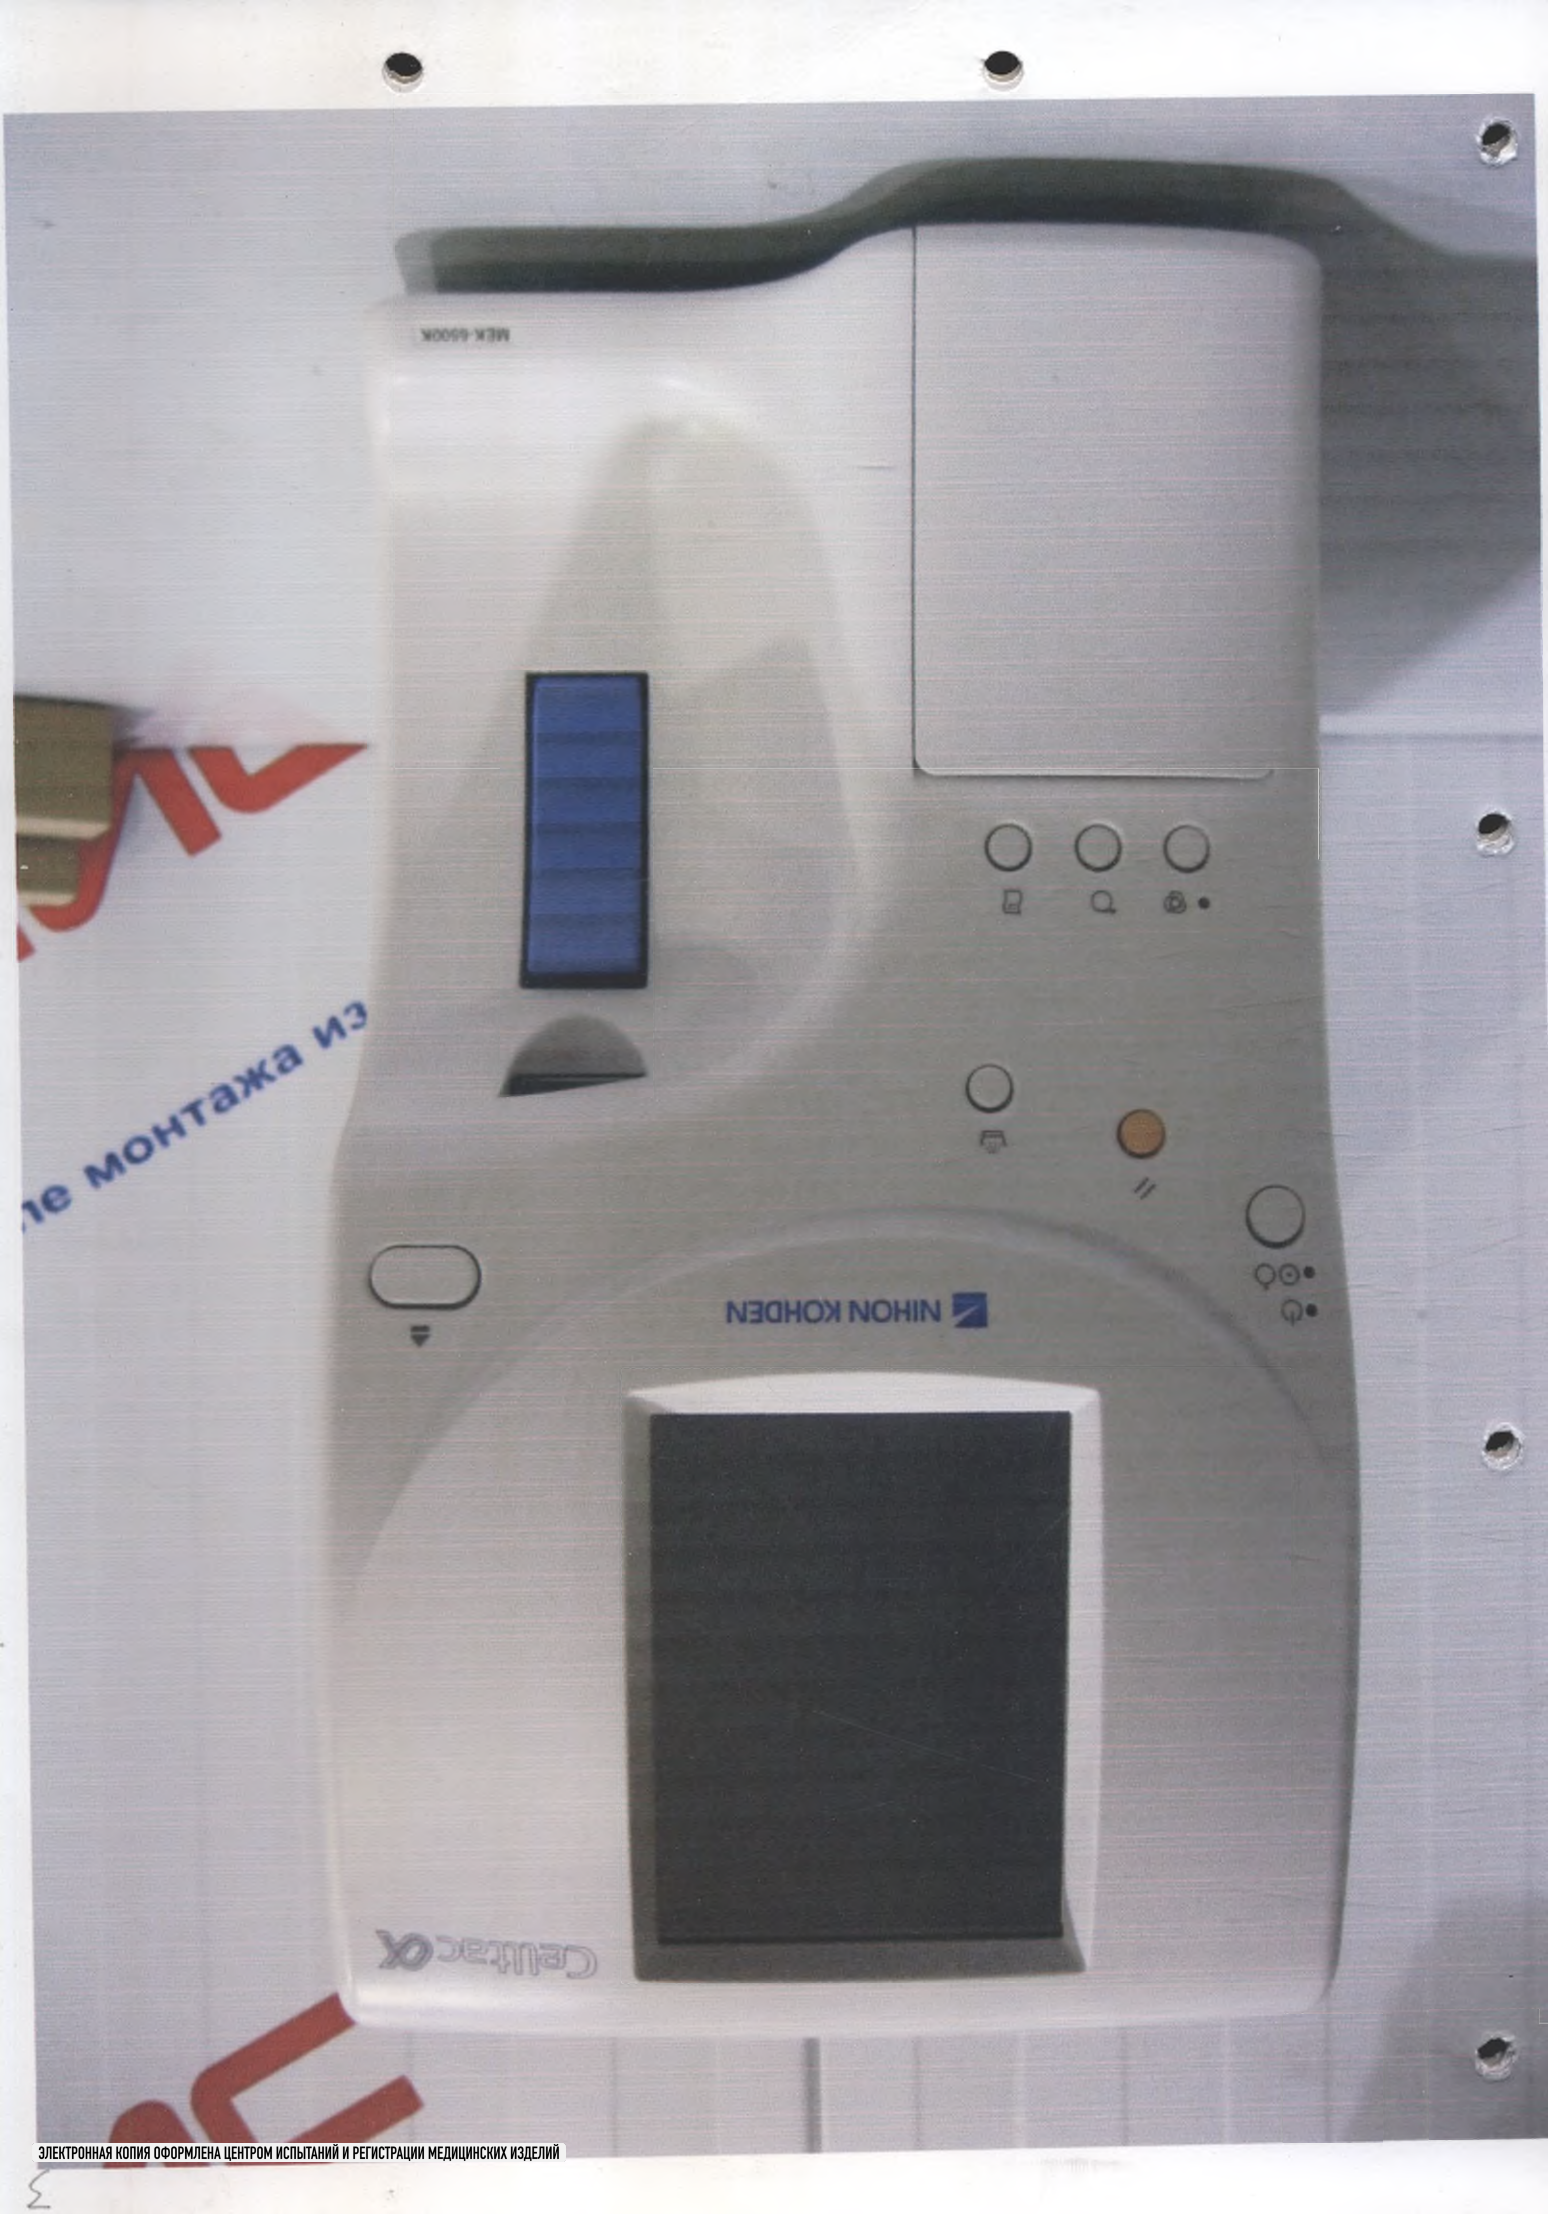


MEK-6500K



NIHON KOHDEN



Celltac α

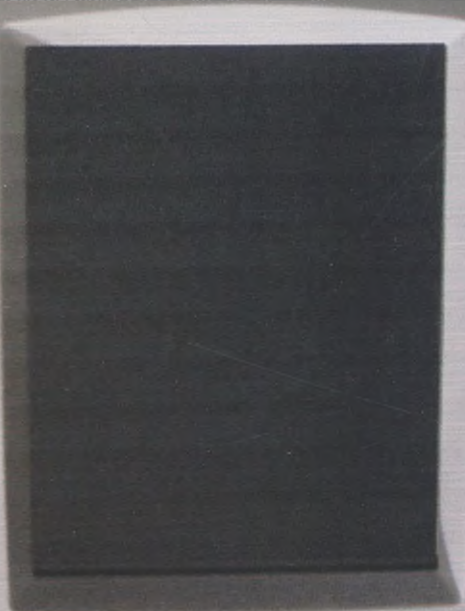

ON
OFF



220-240V
50/60Hz



FUSE



T 1.0A/250V



AC SOURCE



CE NIHON KOHDEN CORPORATION
1-31-4 Nishiotsu, Shinjuku-ku
Tokyo, Japan
EC NIHON KOHDEN EUROPE GmbH
Raffelstrasse 10
D-61191 Rostbach, Germany

IVD

MEK-6500K
VER. 01-03



MEK-6500K
00018 AA



AUTOMATED
HEMATOLOGY ANALYZER
MODEL MEK-6500K
POWER INPUT 120VA

SN 00018

2013

Made in Japan
NIHON KOHDEN CORPORATION
21-4 Nishiotsu, Shinjuku-ku, Tokyo, Japan

For the member states of the European Union only



Contact your NIHON KOHDEN
representative for disposal at the
end of its working life



Celltac α

NIHON KOHDEN

MEK-6510K

ON
OFF



220-240V
50/60Hz



FUSE 
T 1.0A/250V



AC SOURCE



CE NIHON KOHDEN CORPORATION
1-31-4 Nishichoai, Shinjuku-ku
Tokyo, Japan
EC REP NIHON KOHDEN EUROPE GmbH
Raffelstrasse 10
D-51191 Rostock, Germany

IVD

MEK-6510K
VER. 01-03



MEK-6510K
00081 AA



AUTOMATED
HEMATOLOGY ANALYZER
MODEL MEK-6510K
POWER INPUT 120VA

SN 00081

2013

Made in
Japan

NIHON KOHDEN CORPORATION
31-4 Nishichoai 1-chome, Shinjuku-ku, Tokyo, Japan

For the member states of the European Union only



Contact your NIHON KOHDEN
representative for disposal at the
end of its working life.




























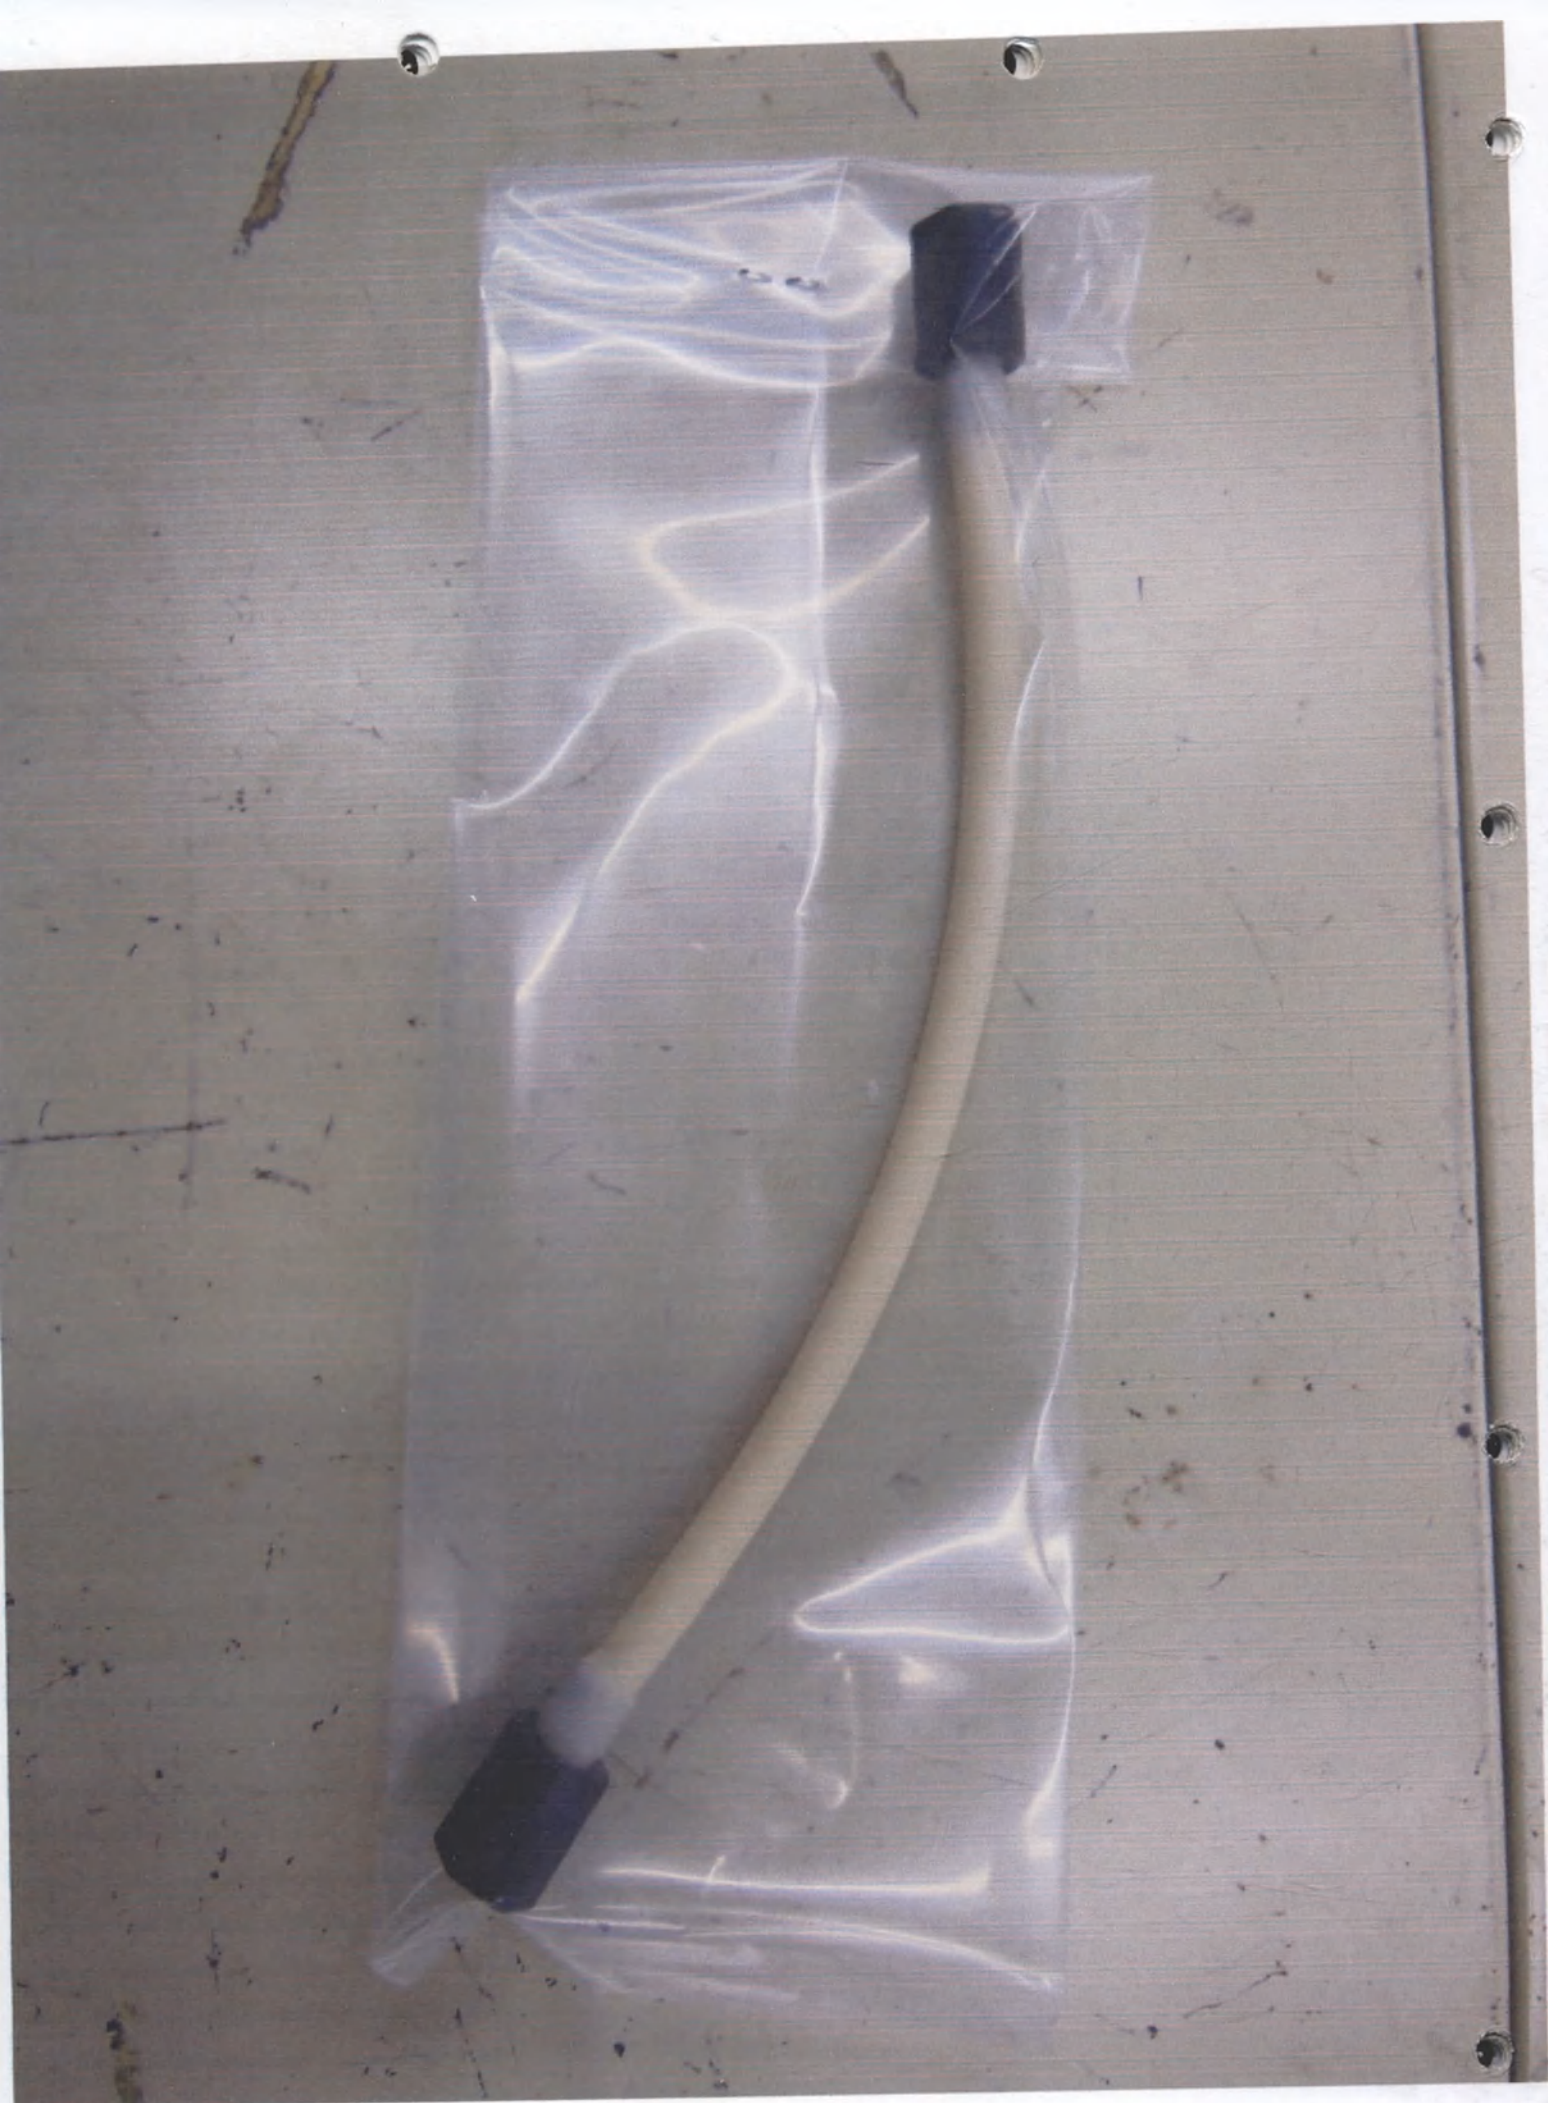






持出禁止!







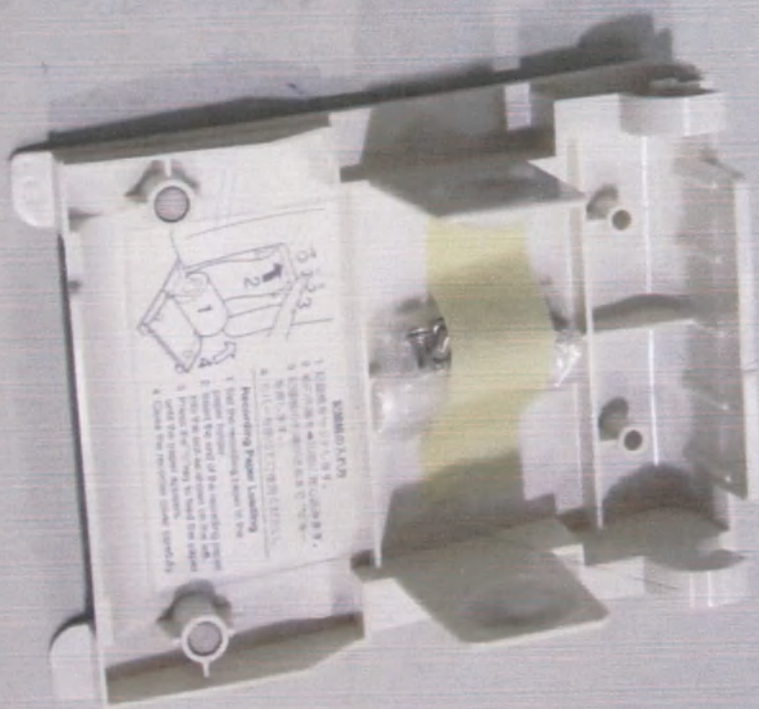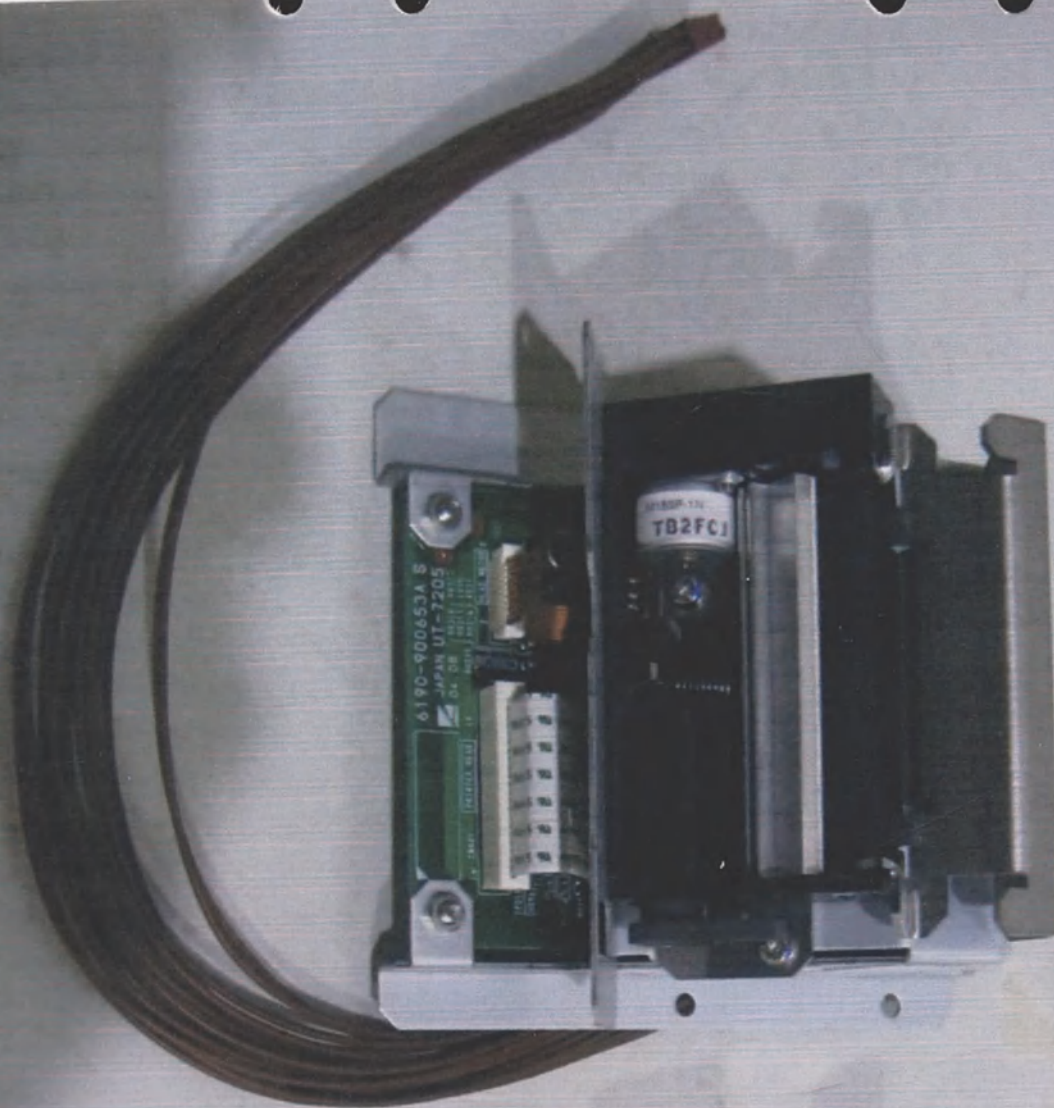

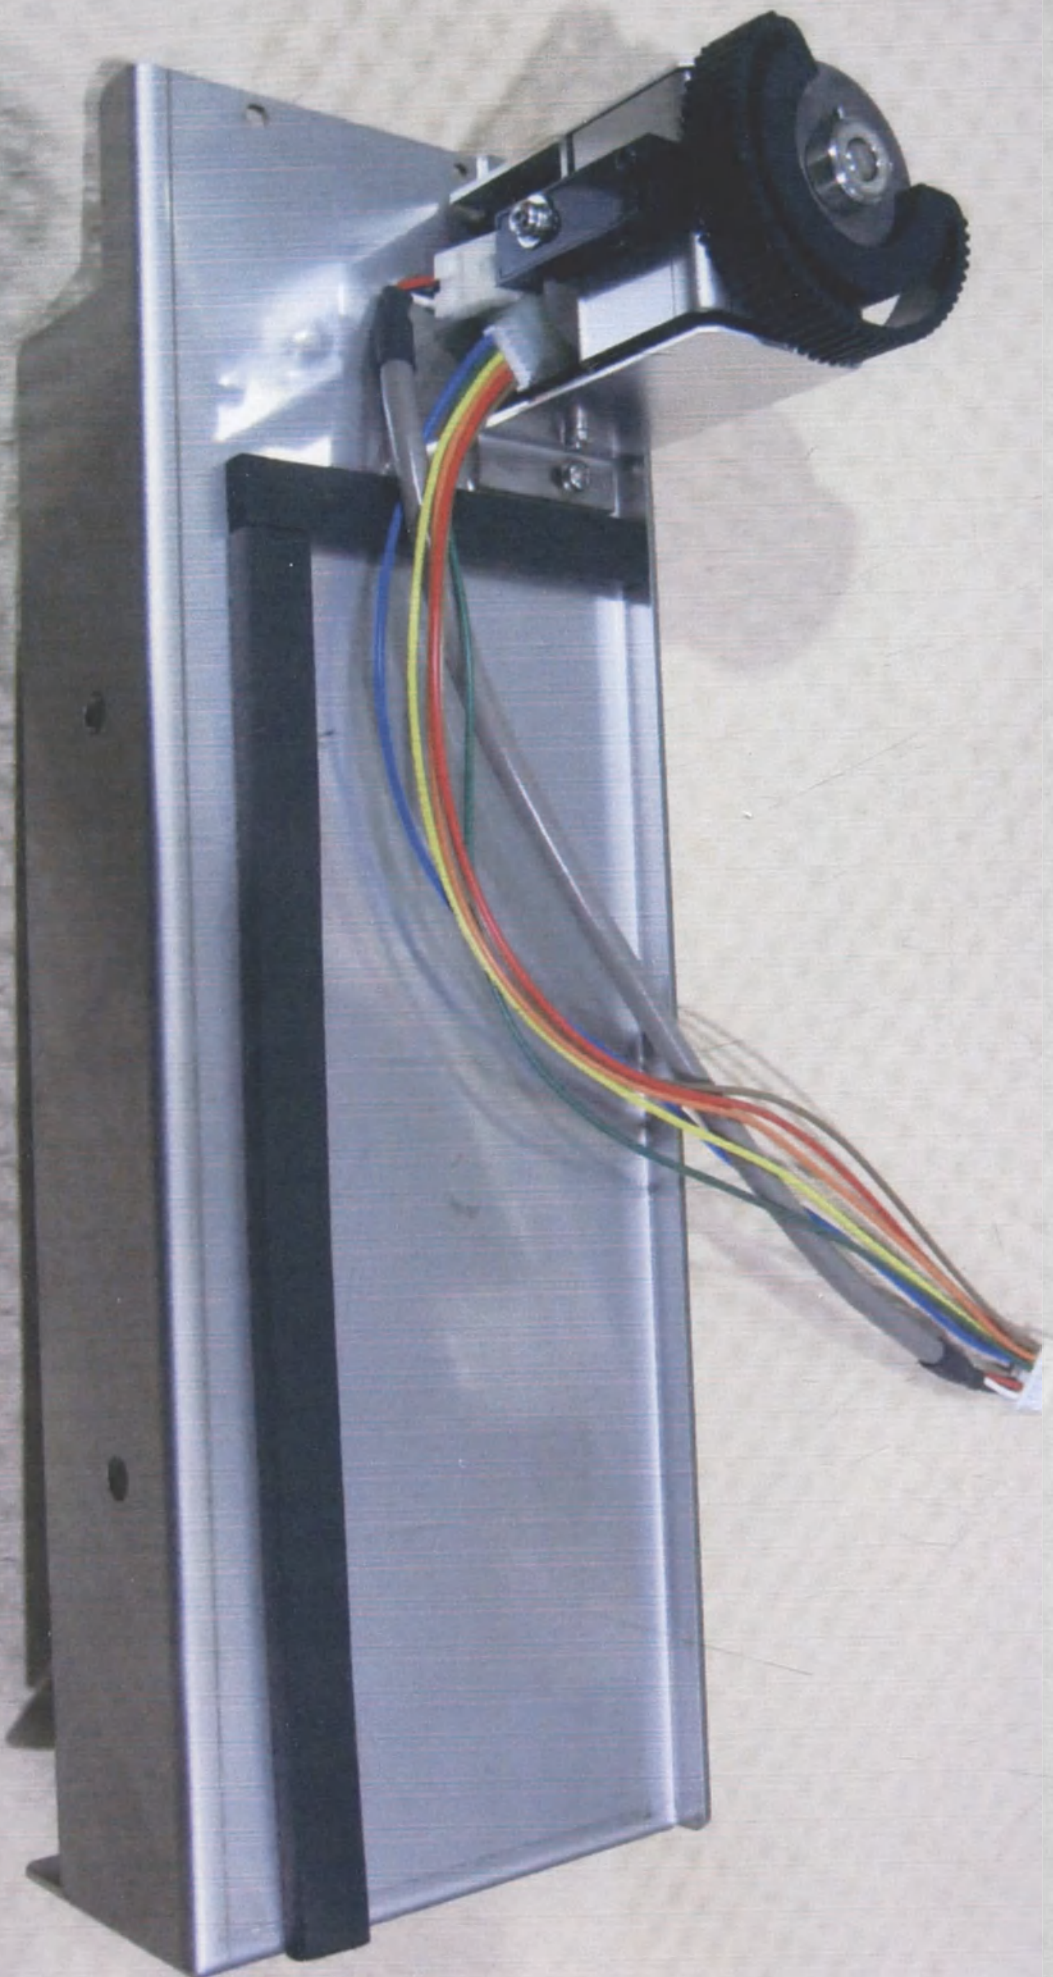

27

OPERATOR'S MANUAL

Celltac α

Automated Hematology Analyzer

MEK-6500

MEK-6500J
MEK-6500K

First Edition: 22 Oct 2012

0614-906126

Printed: 2013/04/09

 NIHON KOHDEN