


ФОТОГРАФИЧЕСКИЕ ИЗОБРАЖЕНИЯ МЕДИЦИНСКОГО ИЗДЕЛИЯ

**«Катетеры абляционные
с принадлежностями, варианты
исполнения»**






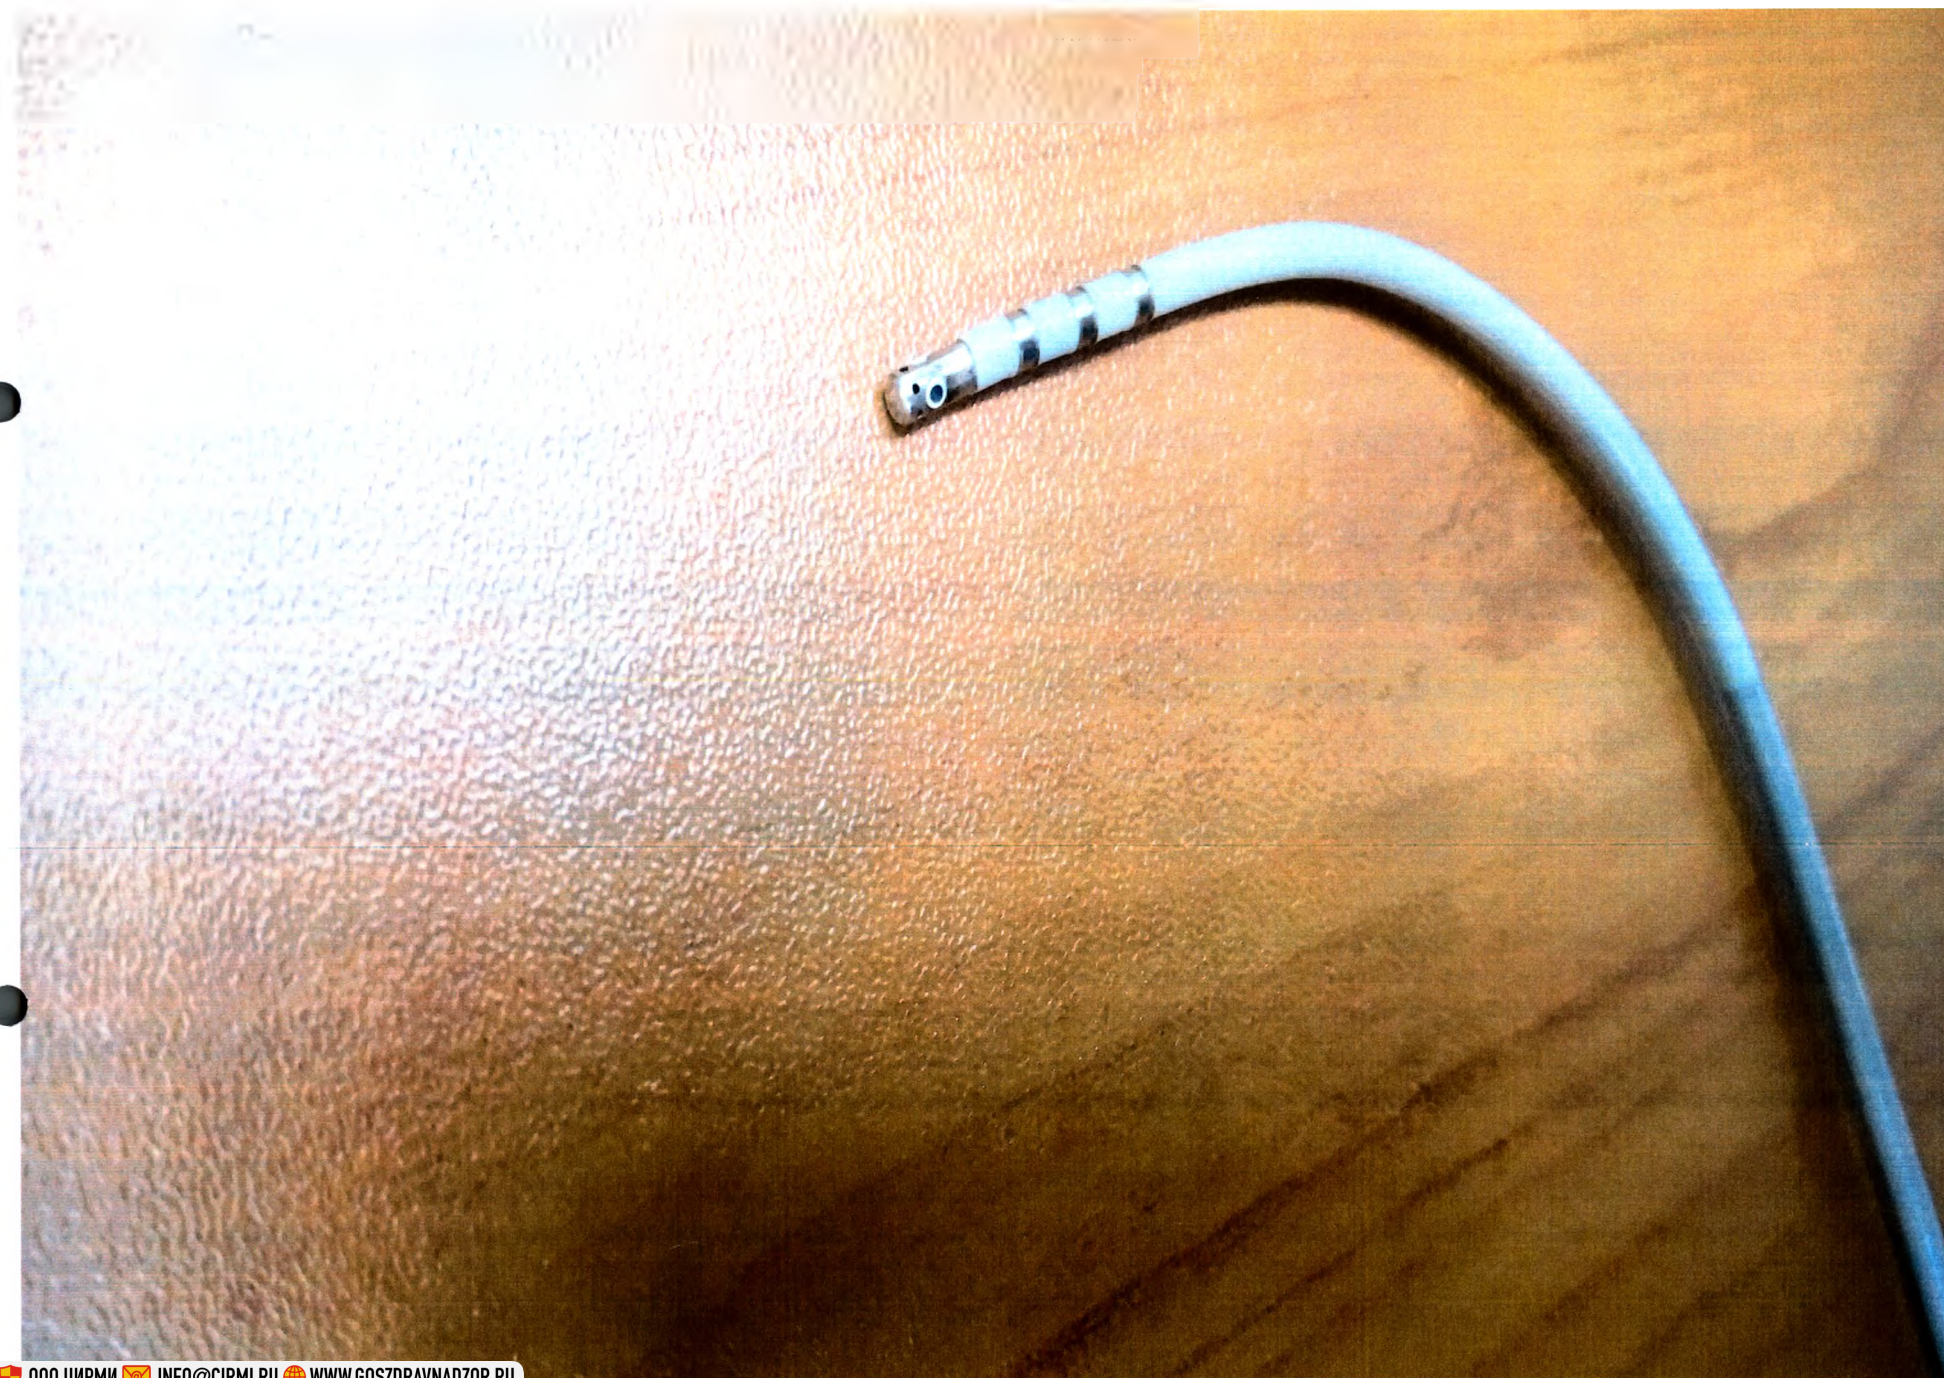



Рукоятка. Ручка управления. Ручка регуляции натяжения. Удлинительная трубка охлаждения (для катетеров IntellaTip MiFi OI, IntellaNav OI)






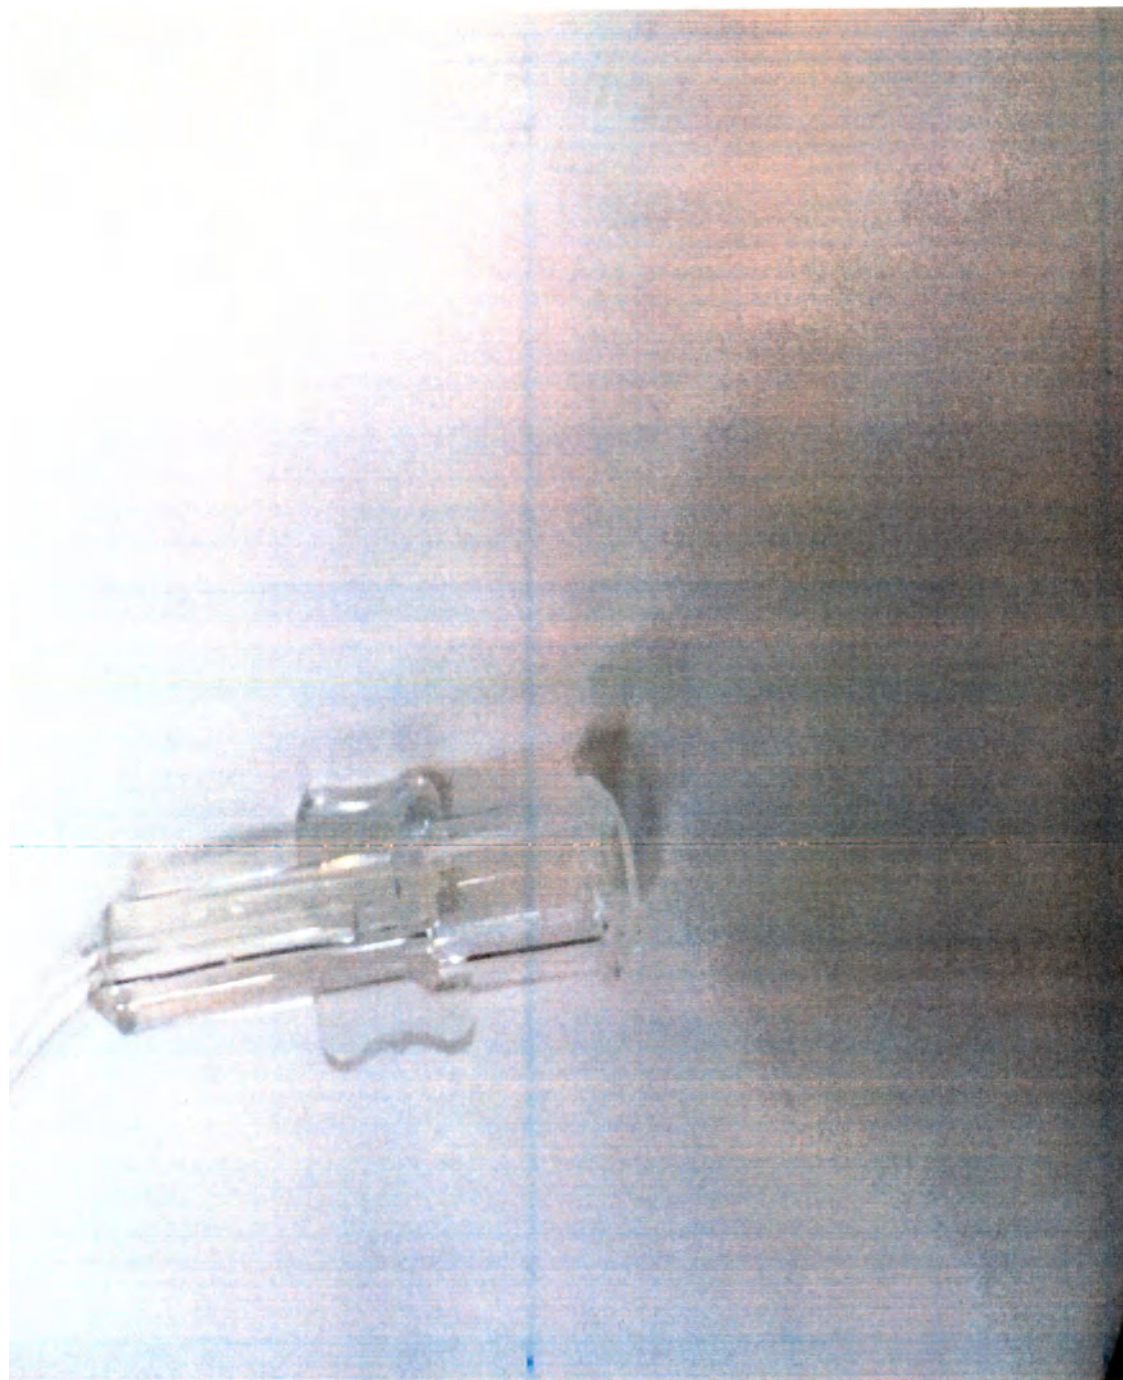

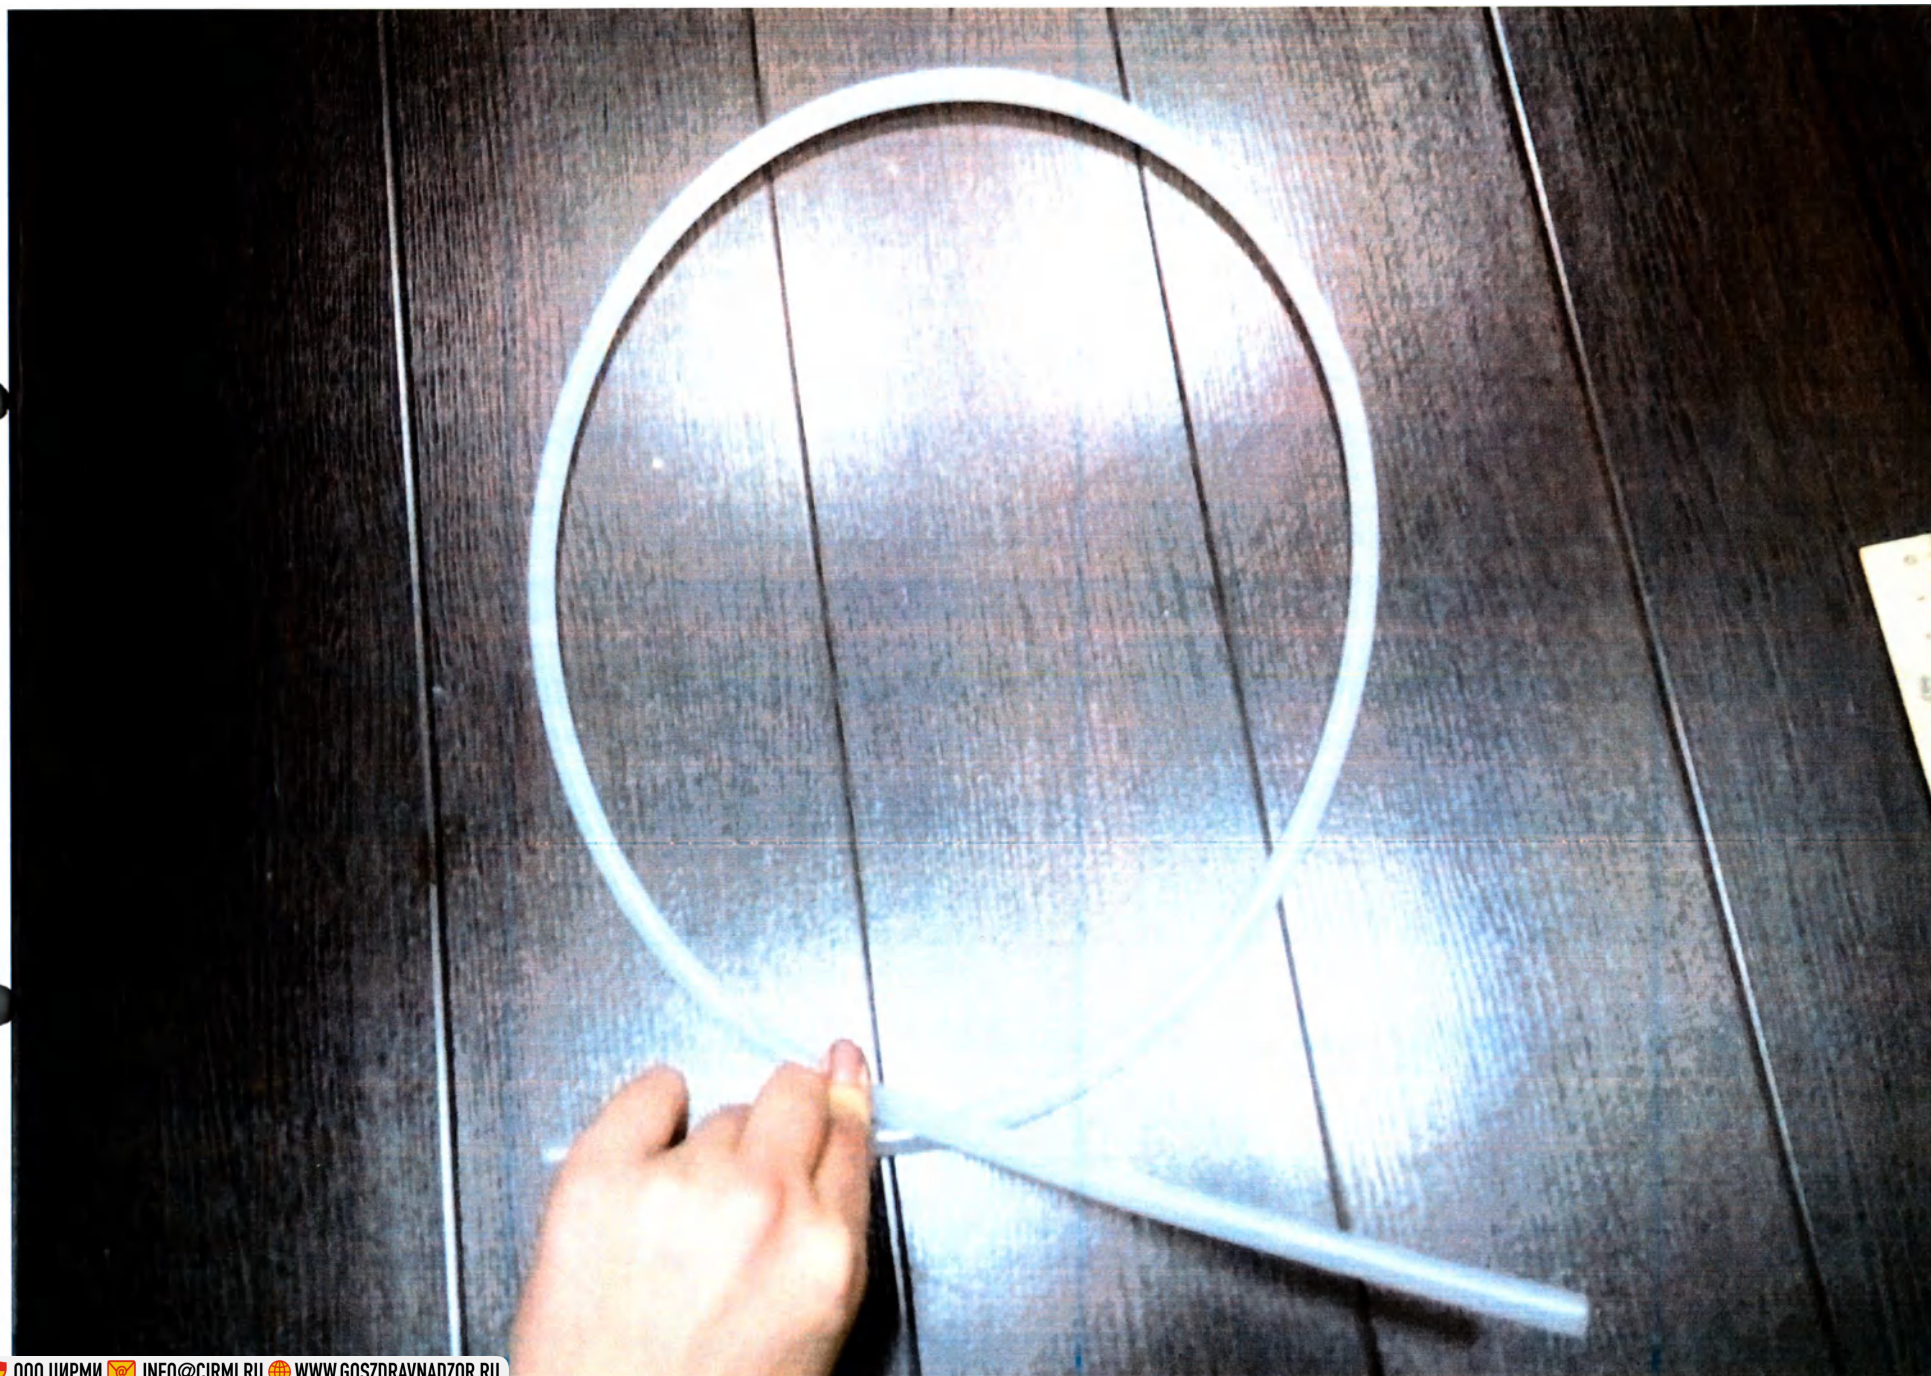


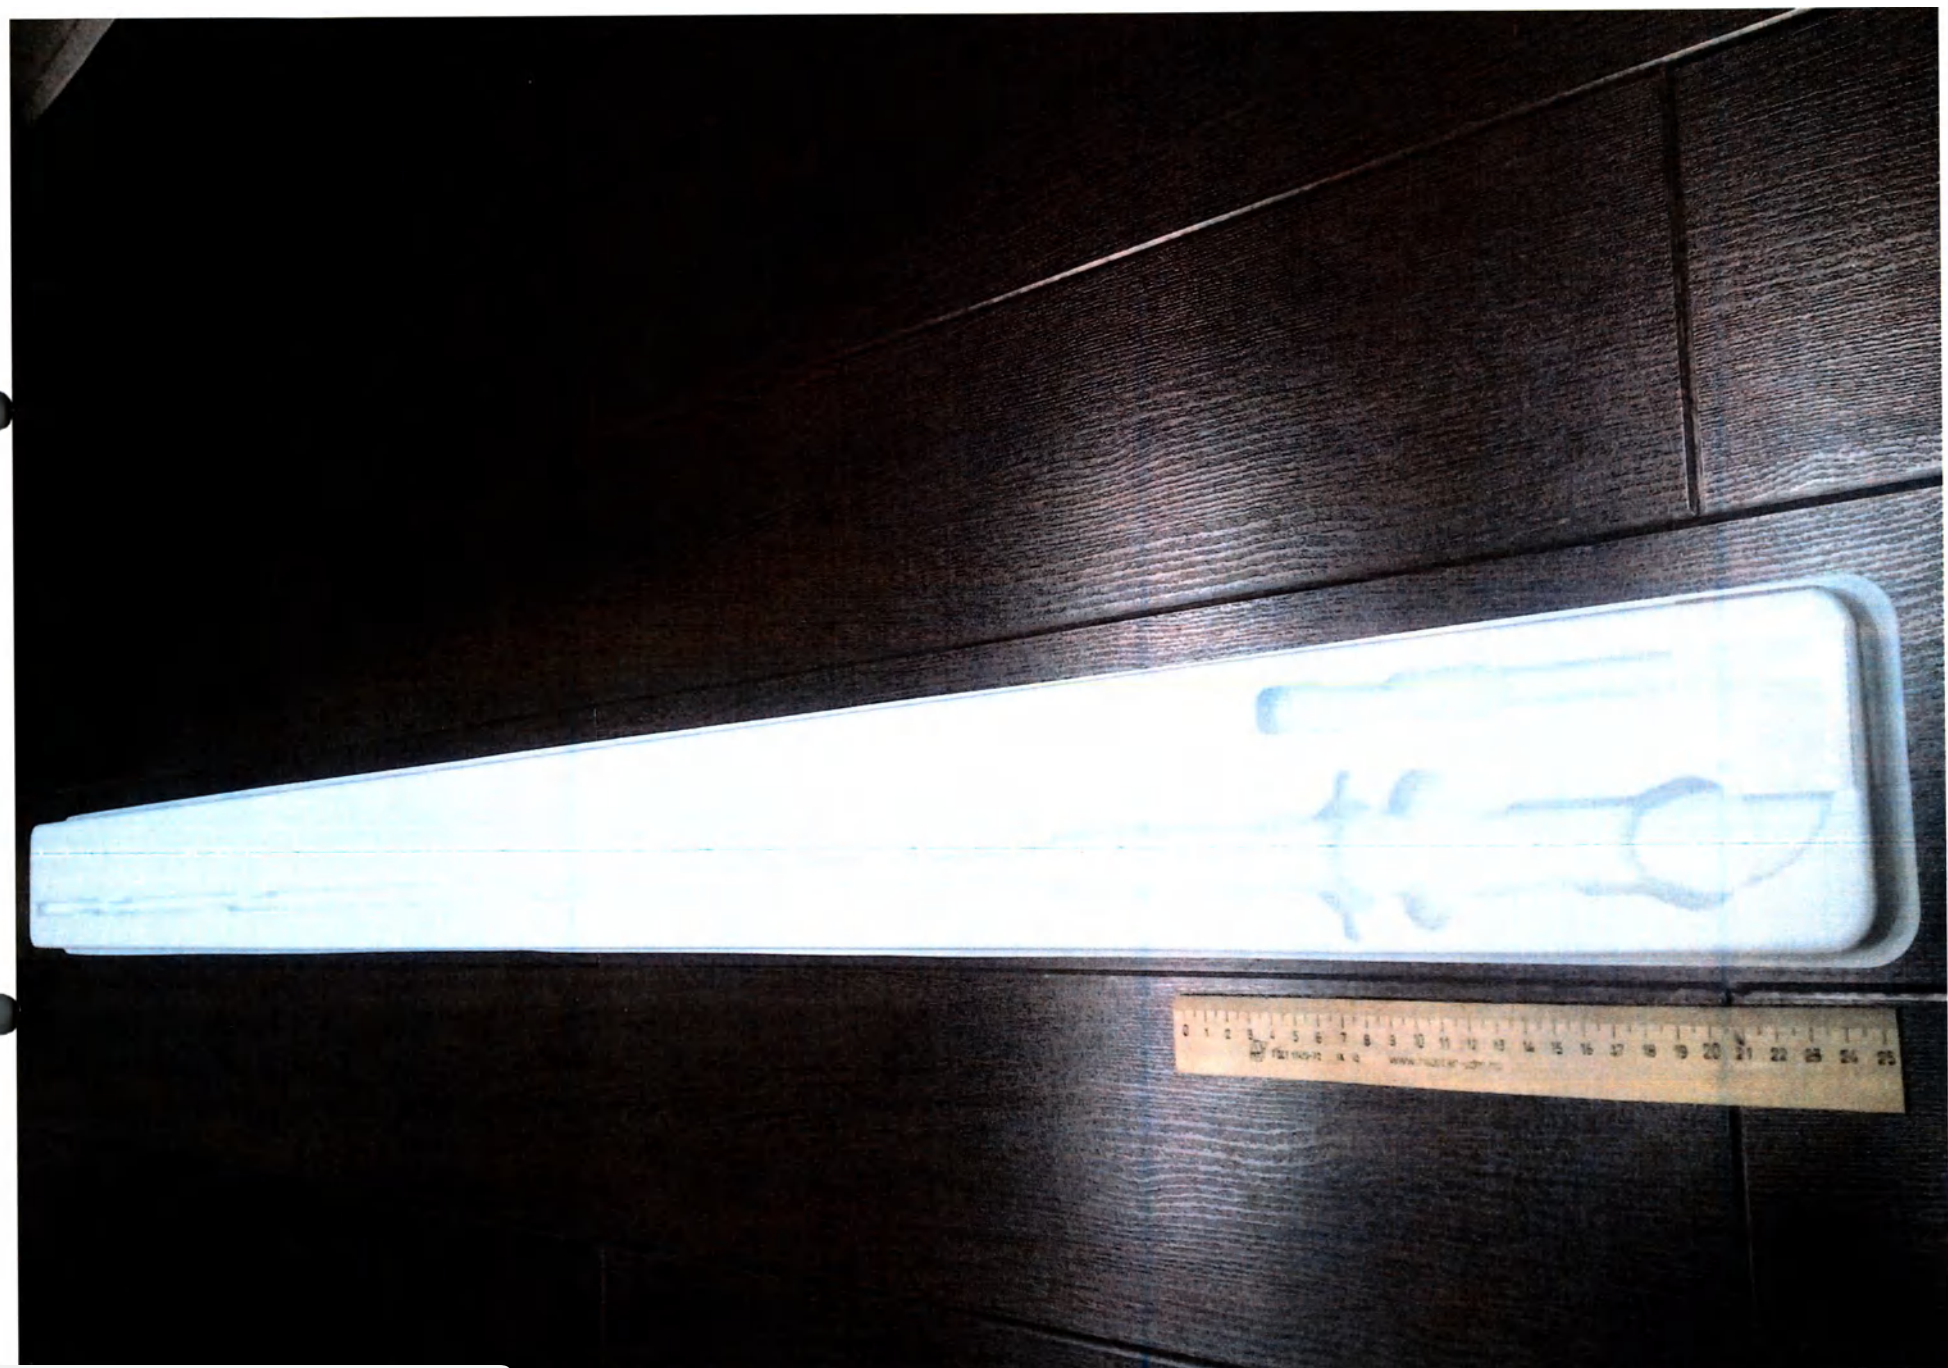

Катетер абляционный навигационный орошаемый по открытому контуру IntellaNav OI, размер электрода кончика 7F (2.33 мм) x 4мм, диаметр катетера 7.5F (2.50 мм), кривизна: стандартная, большая, ассиметричная: общий вид

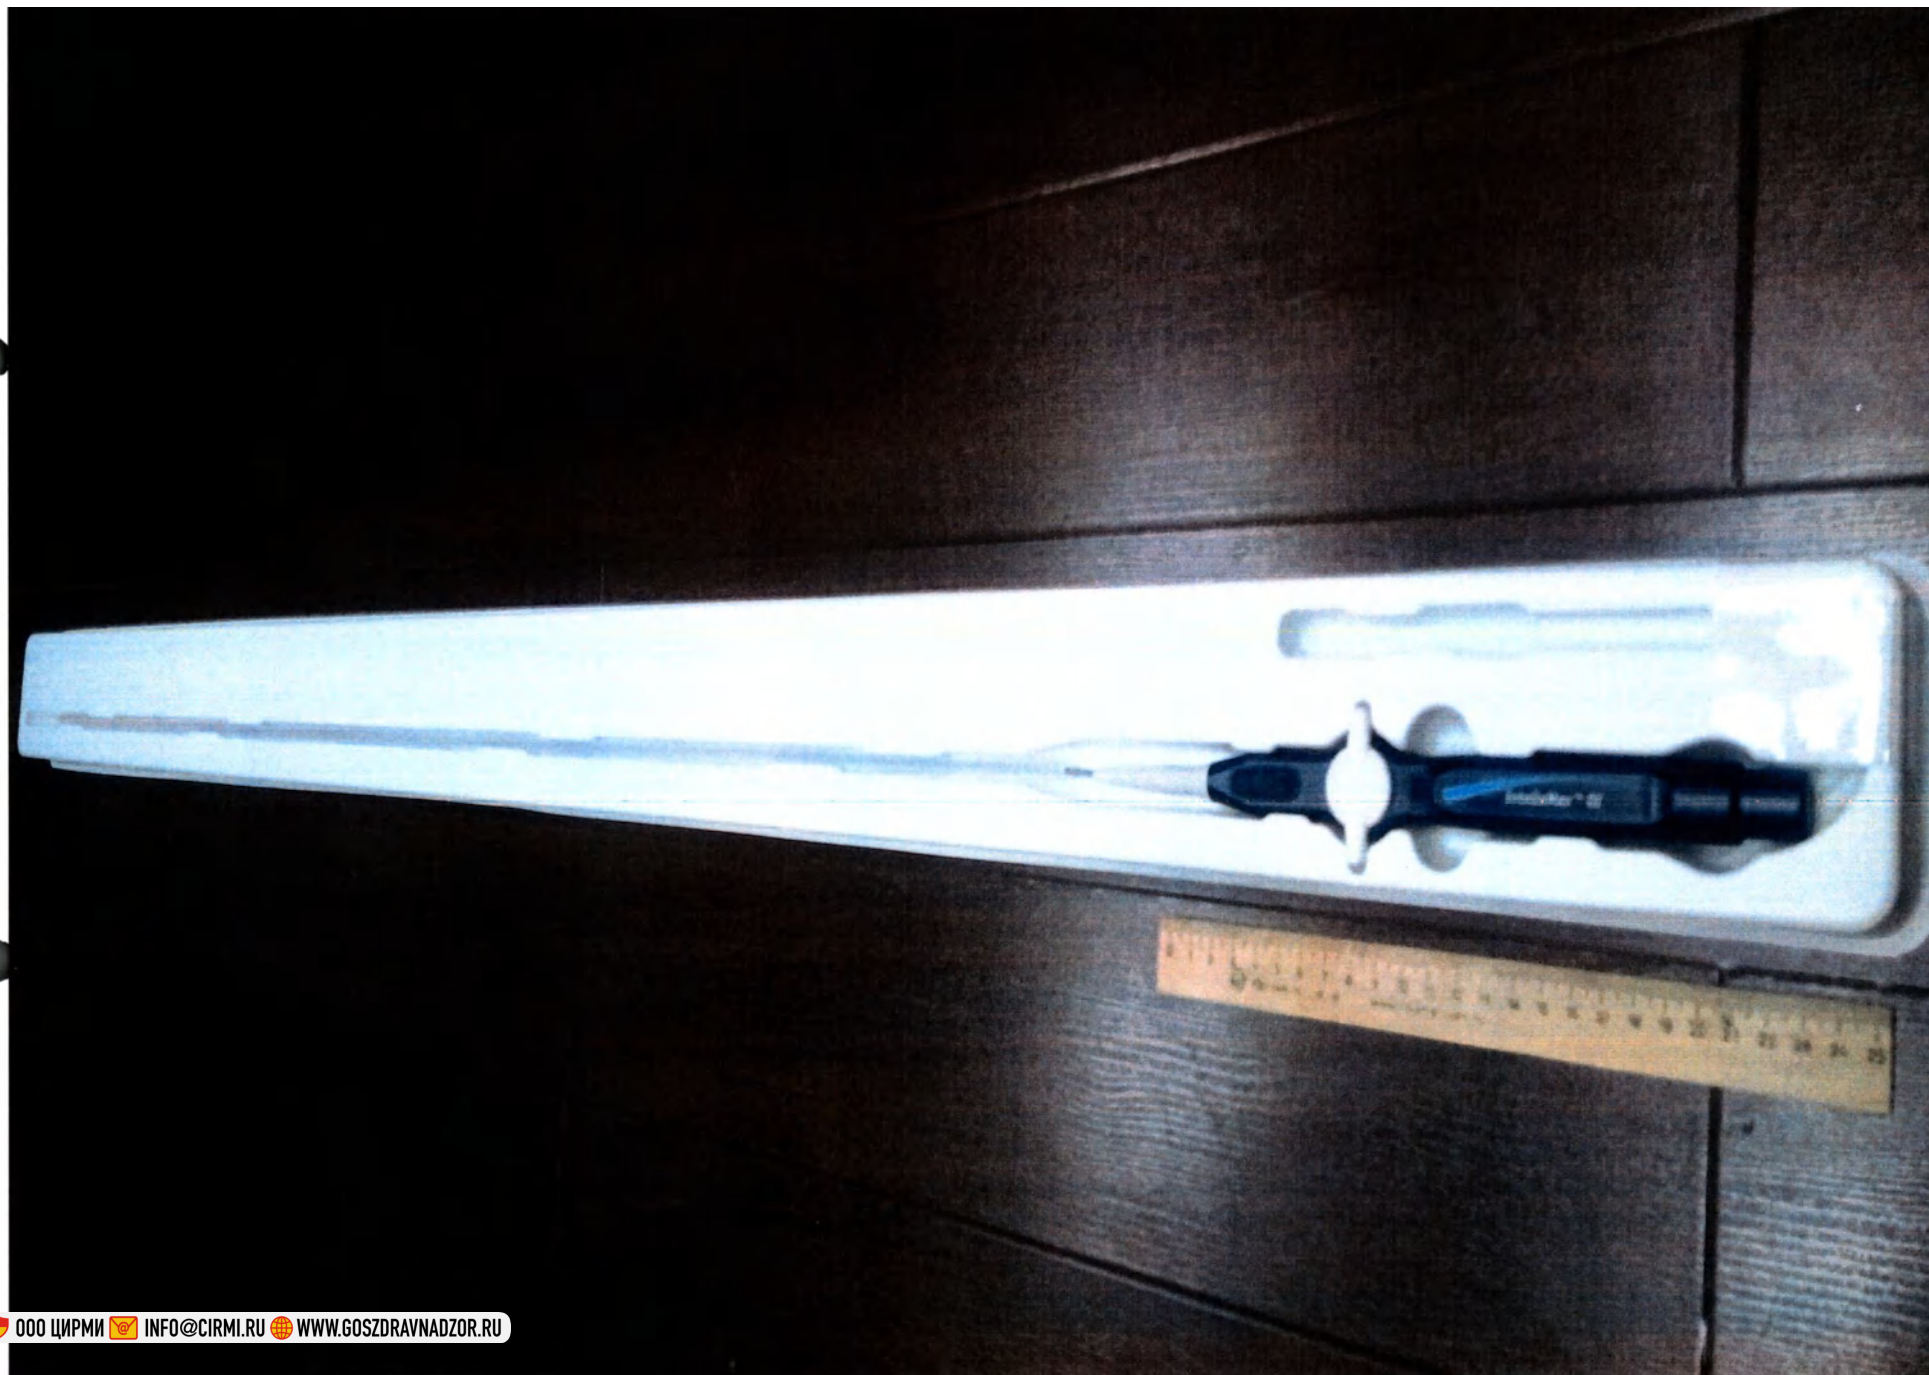


Катетер абляционный навигационный орошаемый по открытому контуру IntellaNav OI, размер электрода кончика 7F (2.33 мм) x 4мм, диаметр катетера 7.5F (2.50 мм), кривизна: стандартная, большая, ассиметричная: запечатываемый пакет

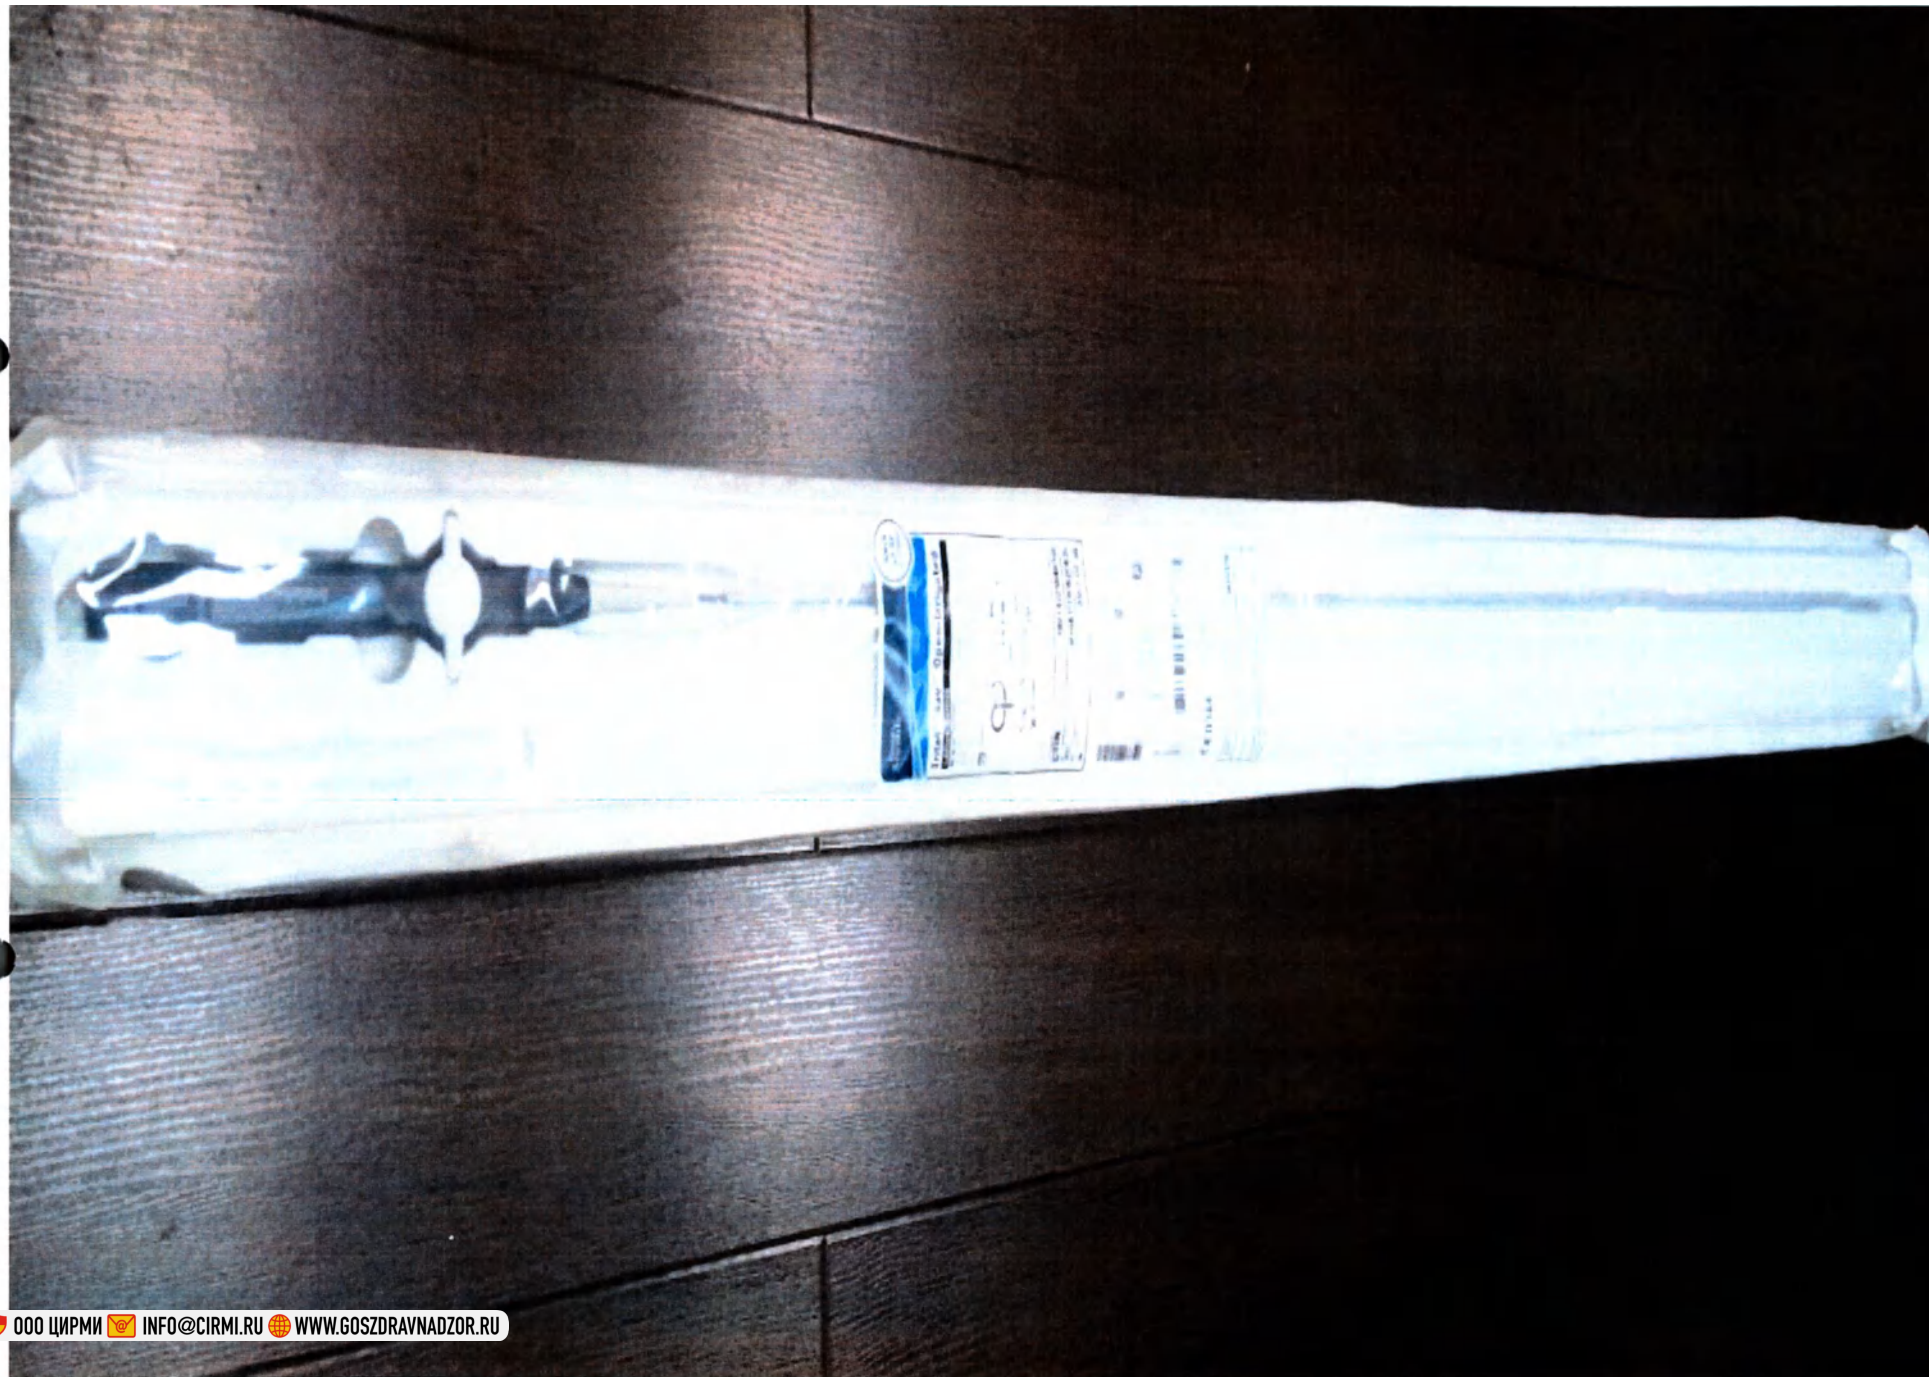


Катетер абляционный навигационный орошаемый по открытому контуру IntellaNav OI, размер электрода кончика 7F (2.33 мм) x 4мм, диаметр катетера 7.5F (2.50 мм), кривизна: стандартная, большая, ассиметричная: картонная коробка



Катетер абляционный орошаемый по открытому контуру IntellaTip MiFi OI, размер электрода кончика 7F (2.33 мм) x 4.5мм, диаметр катетера 7.5F (2.50 мм), кривизна: стандартная, большая, ассиметричная: общий вид

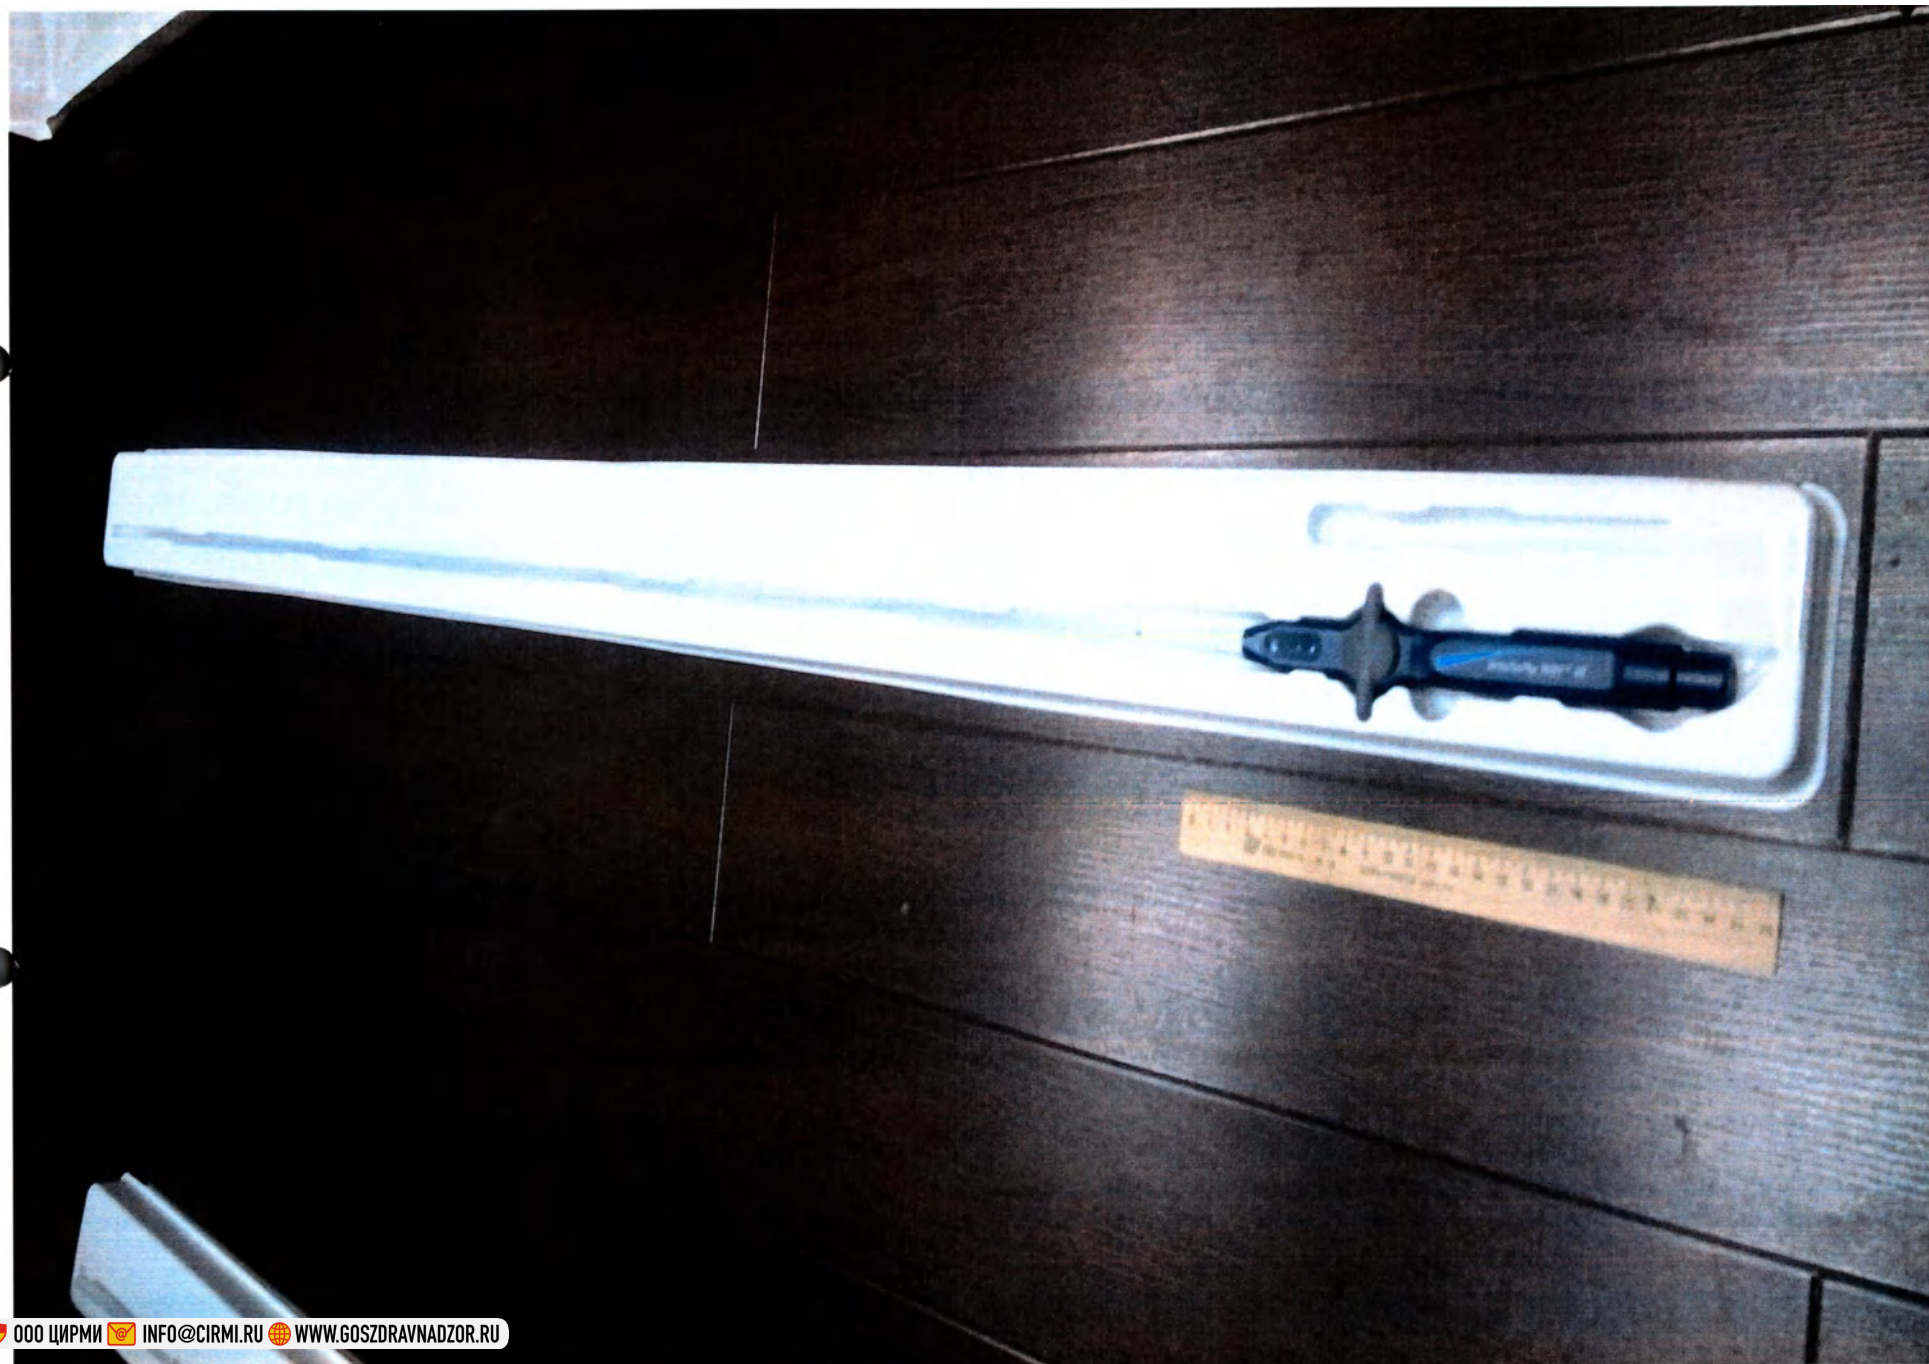

Катетер абляционный орошаемый по открытому контуру IntellaTip MIFI OT, размер электрода кончика 7F (2.35 мм) x 4.5мм, диаметр катетера 7.5F (2.50 мм), кривизна: стандартная, большая, ассиметричная: запечатываемый пакет

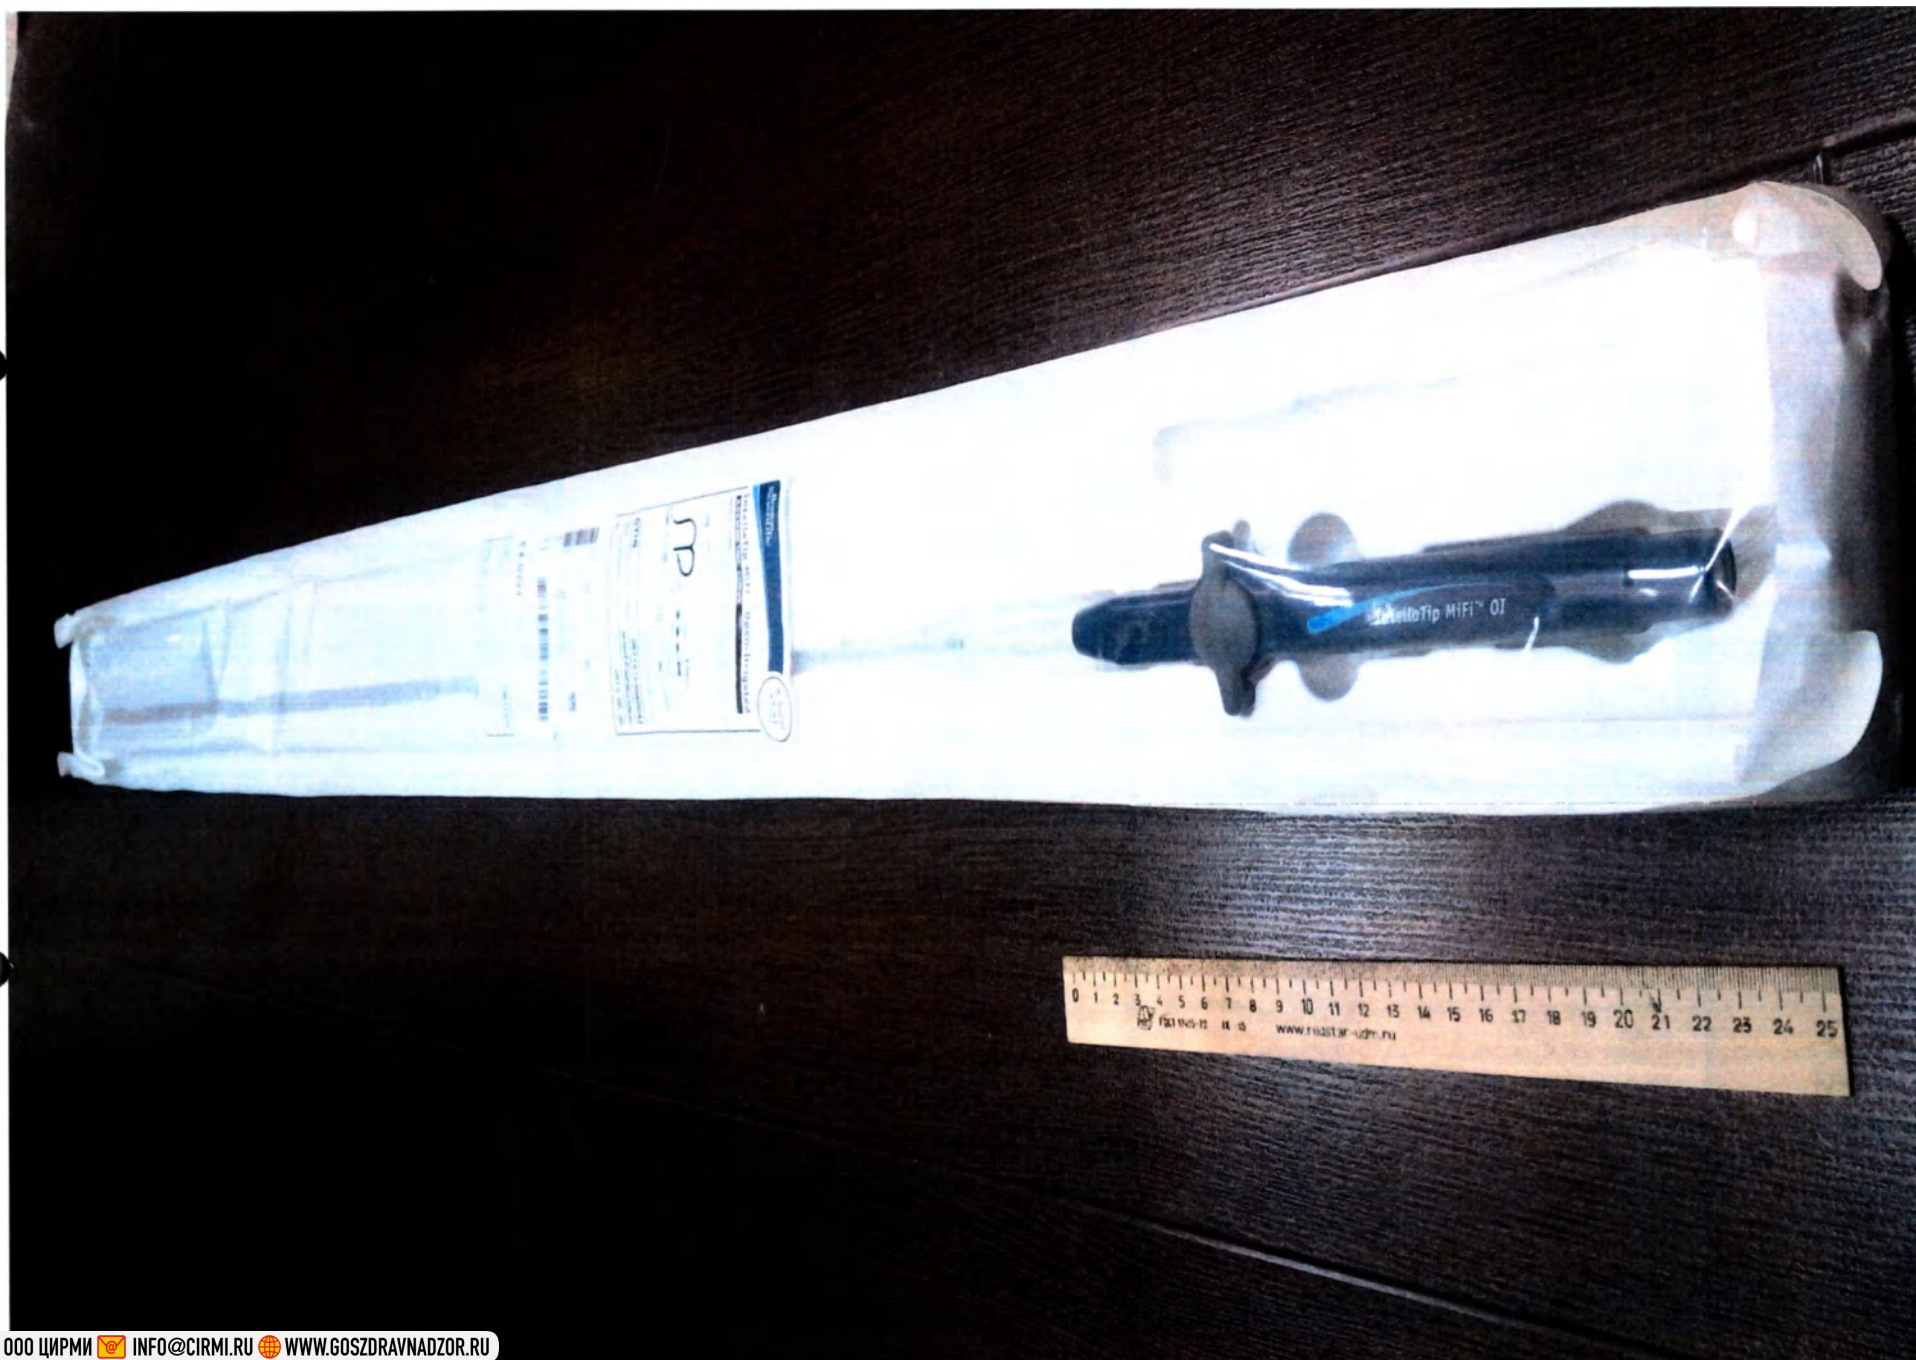

Катетер абляционный орошаемый по открытому контуру IntellaTip MiFi OI, размер электрода кончика 1F (2.55 мм) x 4.5мм, диаметр катетера 7.5F (2.50 мм), кривизна: стандартная, большая, ассиметричная: картонная коробка

Boston Scientific

IntellaTip MiFi™ Open-Irrigated
ASYMMETRIC CURVE
Ablation Catheter

Катетер для абляции. Cathéter d'ablation. Ablationskatheter. Catetera per ablación. Ablationskatheter. アブレーション・カテーテル. Ablationskatheter. Катетер для абляции. Cateter para Ablação. Ablationskatheter. Ablációs katéter. Ablaci katéter. Ceonik ablačný. Ablationskatheter. Ablasyon Katheteri.

Contents (1)

GTIN **08714729940043**

REF **M004EPM9620N40**

Catalog No

PNF **DEHP** **Box (2 ethylene glycol phthalate)**

Boston Scientific
 IntellaTip MiFi™ Open-Irrigated
 4.5mm x 7.5F (2.50mm)
GTIN 08714729940043
REF M004EPM9620N40
LOT 19671979

Boston Scientific
 IntellaTip MiFi™ Open-Irrigated
 4.5mm x 7.5F (2.50mm)
GTIN 08714729940043
REF M004EPM9620N40
LOT 19671979



08714729940043



90246075 01

C € 0344


Made in COSTA RICA
 200 Parkway
 One of Park Halls
 COSTA RICA

IntellaTip MiFi™

90246075 01

LOT	19671979	Exp By	2019-09-05
STERILE			
Sterilized using ethylene oxide			

Катетер абляционный с температурным датчиком IntellaTip MiFi XP, размер электрода кончика: 8F (2.67 мм) x 8мм, 8F (2.67 мм) x 10мм, диаметр катетера 7F (2.33 мм), кривизна: стандартная, большая: общий вид

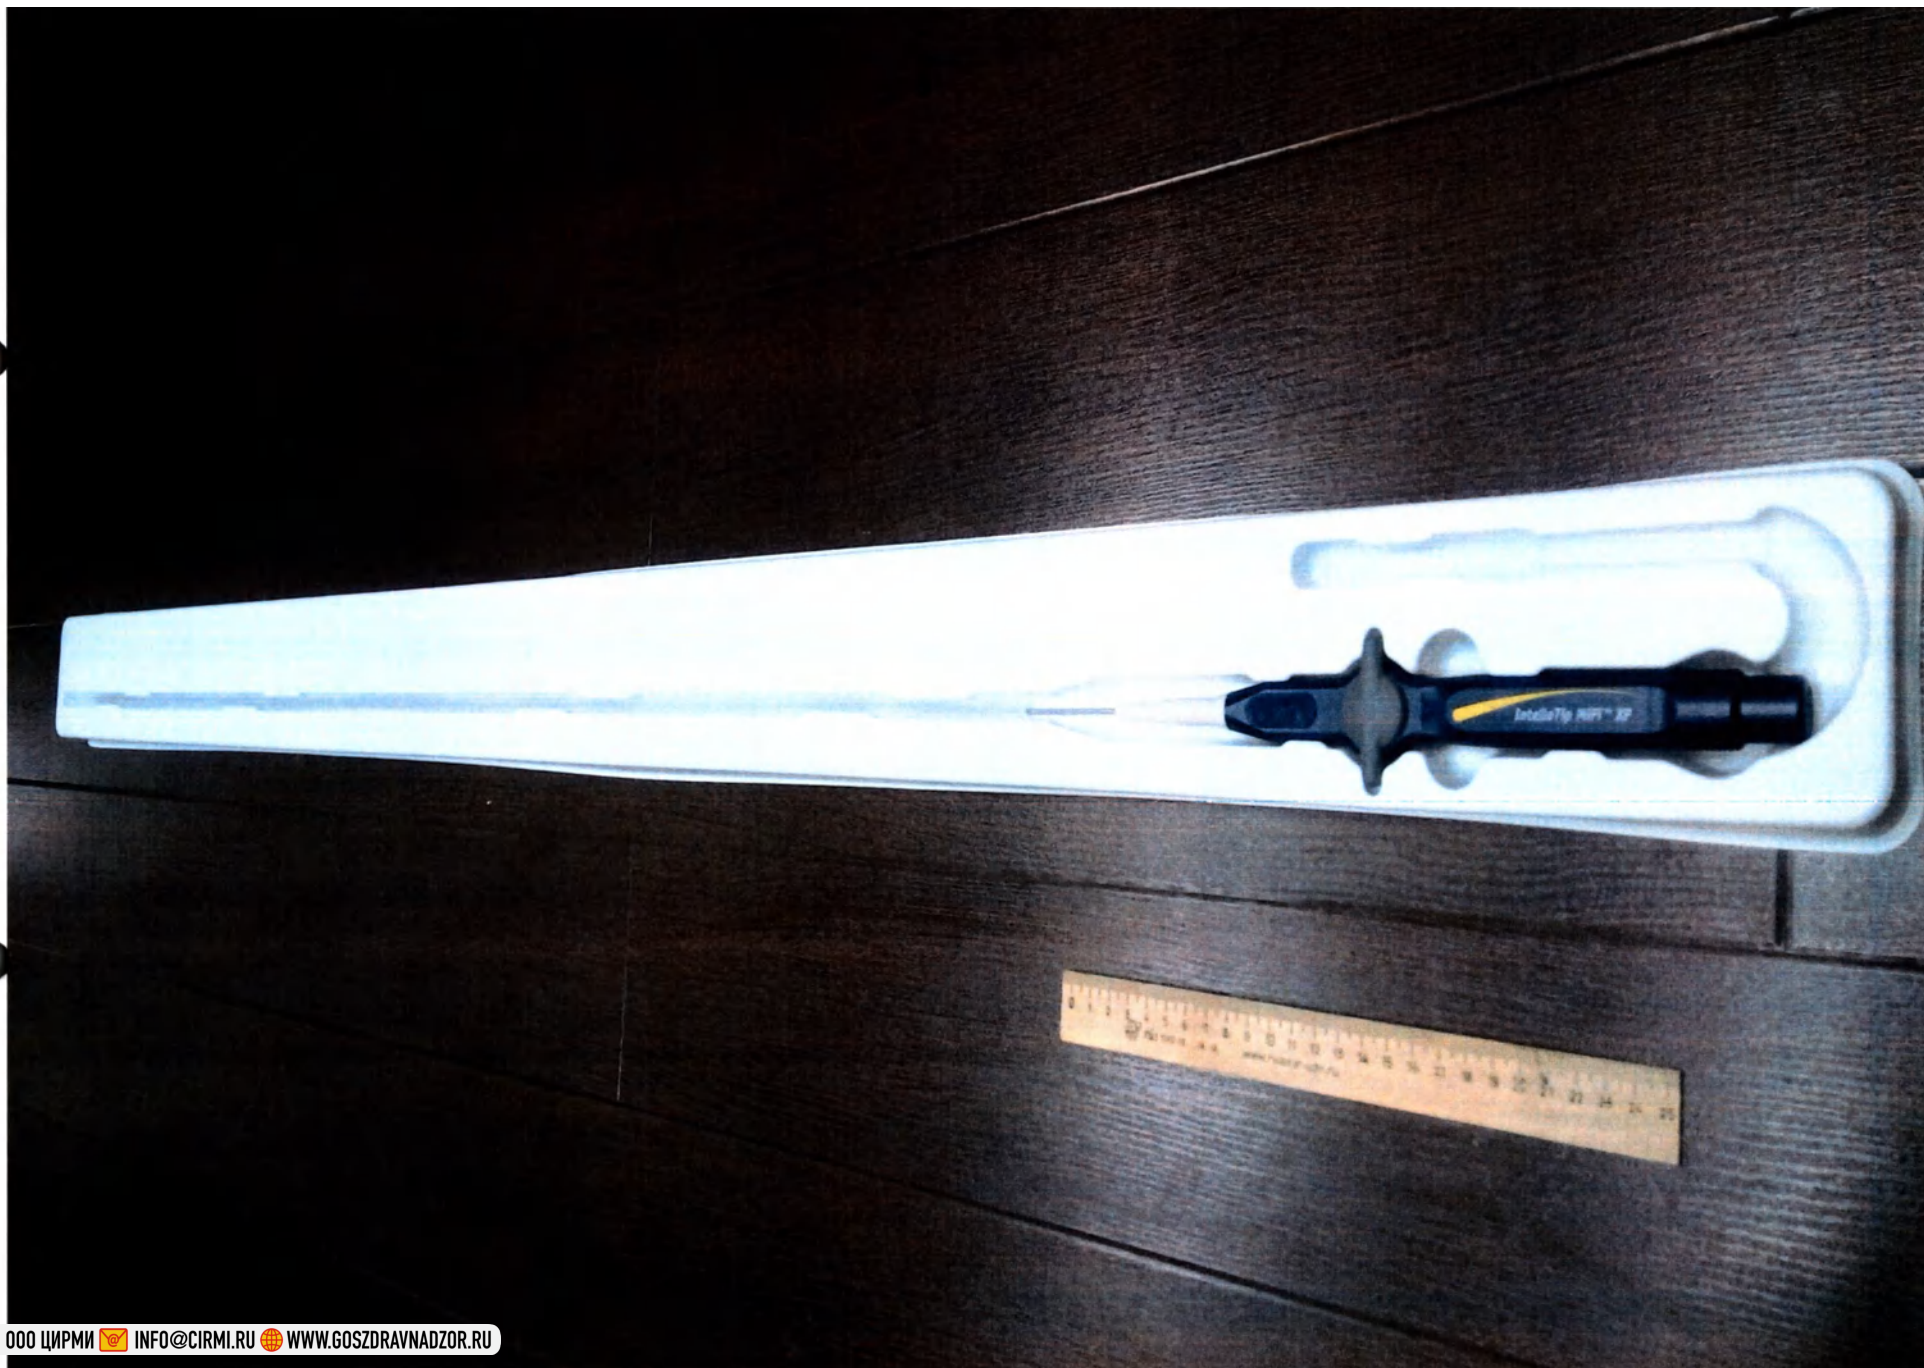


Катетер абляционный с температурным датчиком Intella Tip MiFi XR, размер электрода кончика: 8F (2.67 мм) x 8мм, 8F (2.67 мм) x 10мм, диаметр катетера 7F (2.33 мм), кривизна: стандартная, большая: запечатываемый пакет



Катетер абляционный с температурным датчиком Intella Tip MIFT XP, размер электрода кончика: 8F (2.67 мм) x 8мм, 8F (2.67 мм) x 10мм, диаметр катетера 7F (2.33 мм), кривизна: стандартная, большая: картонная коробка



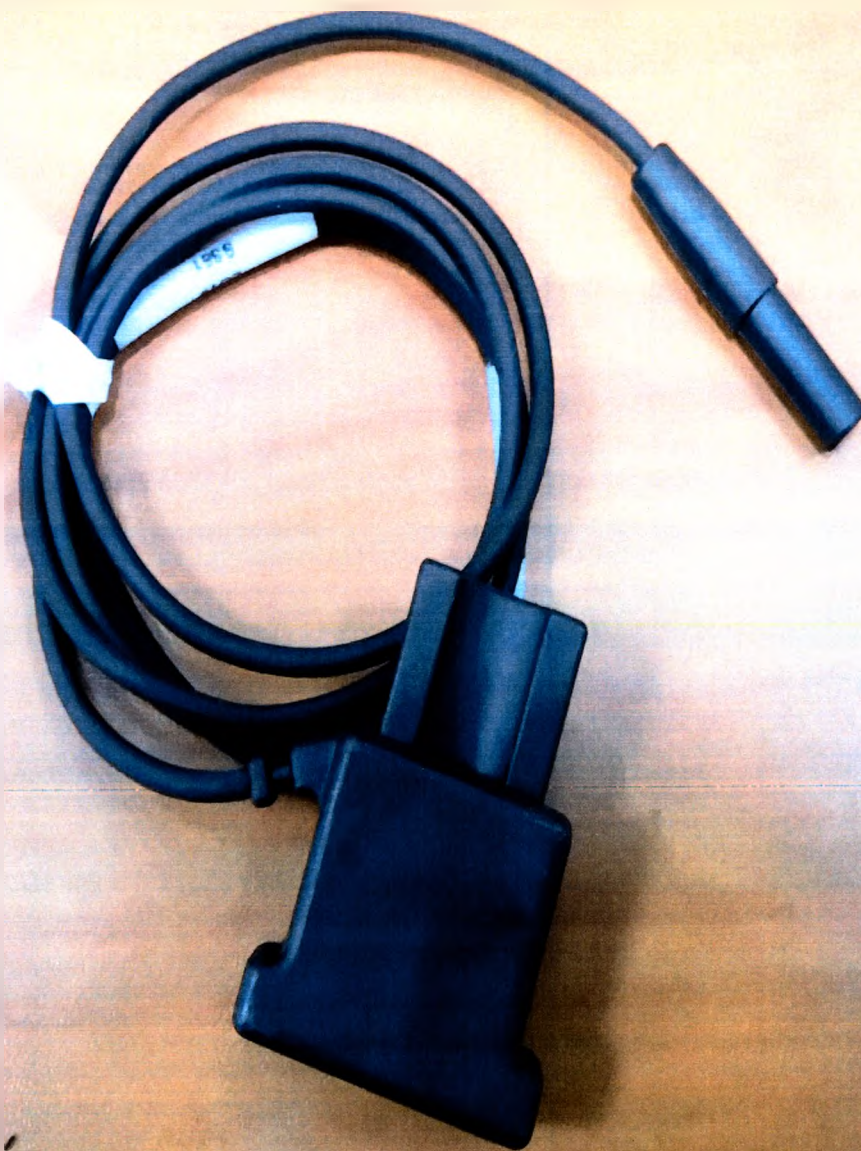

IntellaTip MiFi™ Reference Cable

Non-Sterile Electrophysiology Cable

Cable para electrofisiologia sin esterilizar, Câble d'électrophysiologie non stérile,
Nicht steriles Elektrophysiologie-Kabel, Cavo non sterile per studi elettrofisiologici,
Niet steriele elektrofysiologiekabel, 未滅菌電気生理検査用ケーブル,

Ikke-sterilt kabel til elektrofysiologi, Μη αποστειρωμένο καλώδιο ηλεκτροφυσιολογίας,

Cabo de Electrofisiologia Não Esterilizado, Ikke-steril elektrofysiologikabel,

Ne-steril, elektrofiziológias kábel, Nesterilni kabel pro elektrofiziologické systémy

Nieczysty przewód do zabiegów elektrofizjologicznych,

Ikke-steril elektrofysiologisk kabel, Steril Olmayan Elektrofizyoloji Kablosu

 Contents (1)



GTIN 08714729847946

LOT

17463187

REF

Catalog No.
M00436360



Date of
Manufacture 2015-04-03

EC REF

EU Authorized

P. ONLY





90950582-01

Internal BSC Bar Code

90968581-01A



10108714729647948111114111710117463187

GS1

Boston Scientific Limited
Ballybrit Business Park
Galway
IRELAND



Legal
Manufacturer

Boston Scientific Corporation
300 Boston Scientific Way
Marlborough, MA 01752
USA
USA Customer Service 888-272-1001



Consult instructions
for use.



Do not use if package
is damaged.



Recyclable
Package



Made in USA

47215 Lakeview Blvd
Fremont, CA 94538 USA

This product may be protected by one or more patents
Patent information can be obtained at
<http://www.bostonscientific.com/patents>







Cable, IntellaTip MiFi™ XP

12 SOCKET QUICK CONNECT TO 9 PIN AND 4 PIN QUICK CONNECTS

305cm (10ft)

Sterile Cable

Cable estéril: Cable estéril. Sterile kabel: Cabo estéril. Sterile kabel: 滅菌ケーブル (ip). Sterile kabel: Амортизирующий кабель стерилиз. Steril kabel: Steril kabel. Steril kabel: Kabeł steryliz. Steril kabel: Steril kabel.

Contents (1)



STERILE

10X

Reusable Reconnections

GTIN

08714729847953

REF

Catalog No.

M0046200



08714729847953 9 500000 1000000 1000

CE 0344

Made in USA
100 Street, Suite
100, 02044, Cambridge, MA

LOT

17684727

This product may be protected by one or more patents.
Patent information can be obtained at
<http://www.bostonscientific.com/patents>

Use By

2018-02-28

STERILE

Handled using
ethylene oxide

Cable, IntellaTip Multi XP

12 SOCKET QUICK CONNECT TO 9 PIN
AND 4 PIN QUICK CONNECTS

305cm (10ft)

Sterile Cable

Cable estéril, Câble stérile, Steriles Kabel, Cavo sterile, Steriele kabel,
滅菌ケーブル, Sterilt kabel, Αποστειρωμένο καλώδιο, Cabo
Esterilizado, Steril kabel, Steril kábel, Sterilní kabel, Kabel steryiny,
Steril kabel, Steril Kablo



Contents (1)



STERILE Σ

10x
Allowable Reesterilizations

GTIN

08714729847953

REF


Catalog No.

M0046200



Use By

2018-03-23

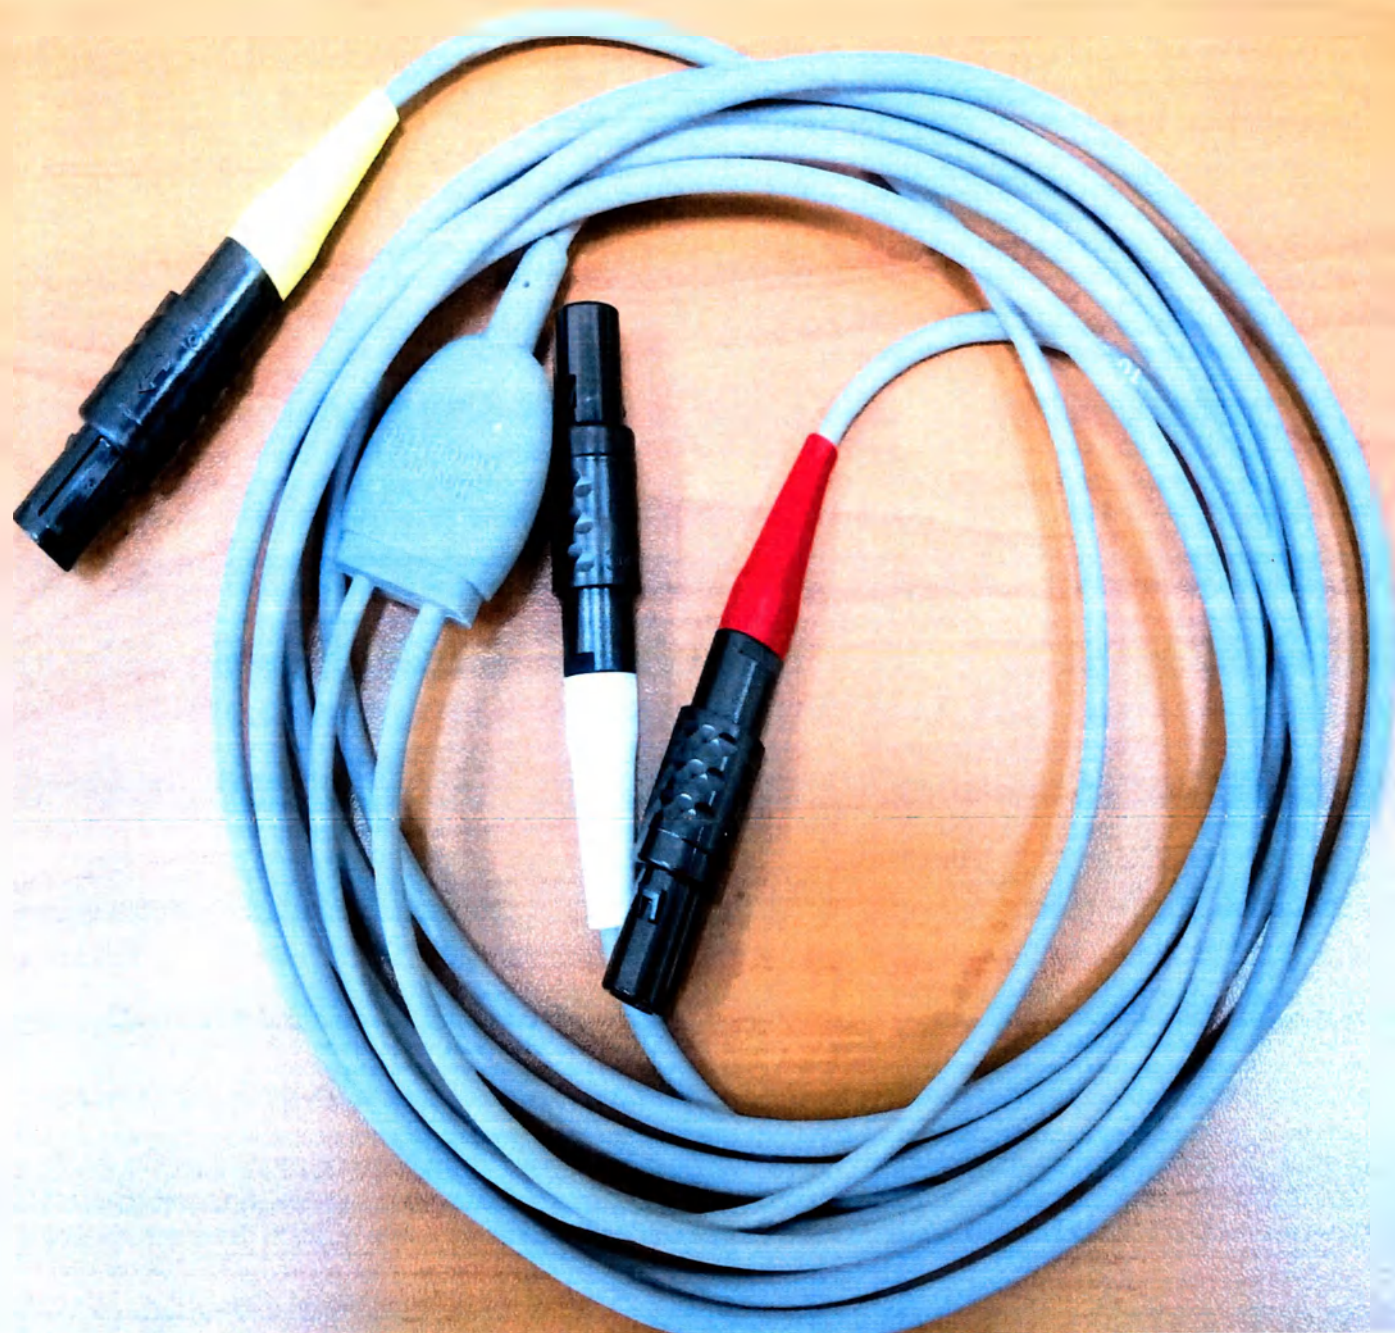

Cable, IntellaTip MiFi™ OI

IntellaTip MiFi OI to Stockert RF Generator

305cm (10ft)

Sterile Cable

Cable estéril, Câble stérile, Steriles Kabel, Cabo sterile, Stereile kabel, 滅菌ケーブル, Steril kabel, Амортизирующий кабель, Cabo Esterilizado, Steril kabel, Steril kabel, Steril kabel, Kabel sterilizing, Steril kabel, Steril Kabel.



Contents (1)



STERILE

10x

Allowable Resterilizations

GTIN 08714729848745

REF

Catalog No.

M0046210



IntellaTip MiFi OI
960213 02



08714729848745 1113004101950007 0 51

CE 0344

Made in COSTA RICA
302 Parkway
Global Park, Heredia
COSTA RICA

LOT

Use By

19553097

2019-08-04

This product may be protected by one or more patents.
Patent information can be obtained at
<http://www.bostonscientific.com/patents>

STERILE

Sterilized using ethylene oxide

Cable, IntellaTip MiFi™ OI

IntellaTip MiFi OI to Stockert RF Generator

305cm (10ft)

Sterile Cable

Cable estéril, Câble stérile, Steriles Kabel, Cavo sterile, Steriele kabel, 滅菌ケーブル, Sterilt kabel, Αποστειρωμένο καλώδιο, Cabo Esterilizado, Steril kabel, Steril kábel, Sterilní kabel, Kabel sterylony, Steril kabel, Steril Kablo



Contents (1)



STERILE

10x

Allowable Resterilizations

GTIN

08714729848745

REF

Catalog No.

M0046210



Use By

2019-08-04





Cable, IntellaTip MiFi™ OI
IntellaTip MiFi OI to Maestro 4000™

Sterile Cable
Cable length: 305 cm (10ft)
Sterile Cable

Contents (1)

STERILE **10x**
Antiseptic Reprocessing

GTIN 08714729877424 **REF 046270**

CE 0344
1945976
019-07-1

LOT **Use By**

Made in COSTA RICA
Goszdravnadzor, Havana
COSTA RICA

STERILE EO Sterilized using ethylene oxide

Boston
Scientific

Cable, IntellaTip MiFi™ OI

IntellaTip MiFi OI to Maestro 4000™

305cm (10ft)

Sterile Cable
Cable length: 305cm (10ft)
Cable length: 305cm (10ft)
Cable length: 305cm (10ft)
Cable length: 305cm (10ft)
Cable length: 305cm (10ft)

Contents (1)



STERILE 10x Allowable Reconnections

GTIN 08714729877424

REF Catalog No M0046270

Use By 2019-07-18



**Boston
Scientific**

Cable, IntellaNav™ Ablation Catheter

IntellaNav™ Catheter to Rhythmia™ Mapping System

200cm (6.6ft)

Sterile Cable

Capo a sterili. Căble sterilizate. Sterilizierter Kabel. Cabo sterile. Sterile kabel.
滅菌ケーブル。Steril kabel. Antiseptisch aufbereitetes Kabel. Steril
kabel. Steril kabel. Steril kabel. Steril kabel. Kabel sterilizing. Steril
kabel. Steril kabel. Steril kabel. Cable steril. Чрезвычайно чистый
Sterilizing kabel.

 **Contents (1)**




STERILE  **10X**
Antiseptisch aufbereitet

GTIN **08714729848783**

REF **Catalog No** **M004RARC010**

Use By **2019-07-08**

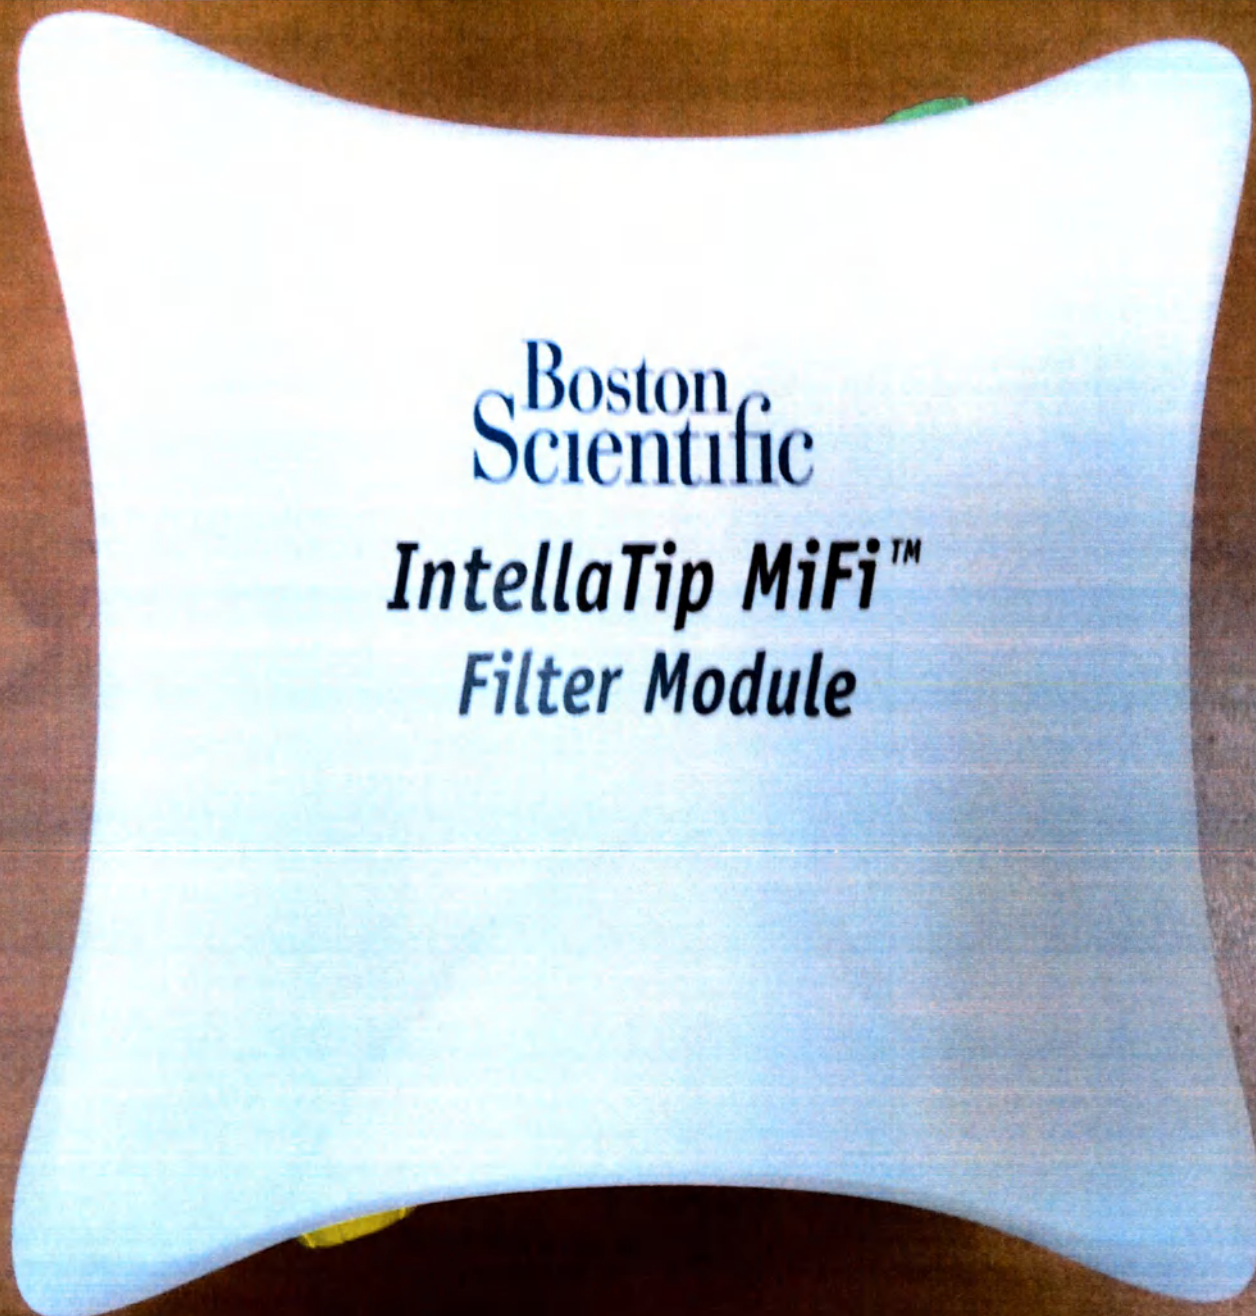

Boston
Scientific

IntellaTip MiFi™
Filter Module

LOT: 1463 SN: 1463



90953314-01B



Collection



Consult instructions
for use.

CE

Made in USA
47215 Lakeview Blvd
Fremont, CA 94538 USA

	This product may be protected by one or more patents. Patent information can be obtained at http://www.bostonscientific.com/patents
	

LOT 1463

SN Serial Number
1463

 Date of
Manufacture

2016-10-22



90910781-01



(01)08714729847939(11)160606(10)1463

GS1

Internal BSC Bar Code

90953314-01B



(21)1463

GS1

Accepted Material

Material #: M00412120



Desc: Filter Module

Batch No: 1463

Org Plant: M750



Date: 22-Oct-2016

Exp Date: 22-Oct-2043

Container Qty: 1



Rev: E

Container: 1 of 1



EU Authorized
Representative

Rx ONLY

Boston Scientific Medical
Equipment Business Park
Boston
MA 02128



Legal
Representative
Boston Scientific Corporation
200 Winter Street, 5th Floor
Boston, MA 02128
USA
Tel: 617 633 1000 ext 4000

**Boston
Scientific**

Генеральный директор
Шевчук Е.В.



ПРОШИТО И
ПРОНУМЕРОВАНО
30 ЛИСТОВ

