

Фотографические изображения медицинского изделия

**Система для клеточного анализа UniCel DxH Coulter: устройство подготовки и окрашивания
препаратов DxH Slidemaker Stainer II (DxH SMS II)**

1. Устройство подготовки и окрашивания препаратов DxH SlideMaker Stainer II (DxH SMS II) с тумбой.



2. Управляющая станция (компьютер) в комплекте с принадлежностями (при необходимости), в составе:



- компьютер




- клавиатура




- компьютерная «Мышь»




- кабель питания,

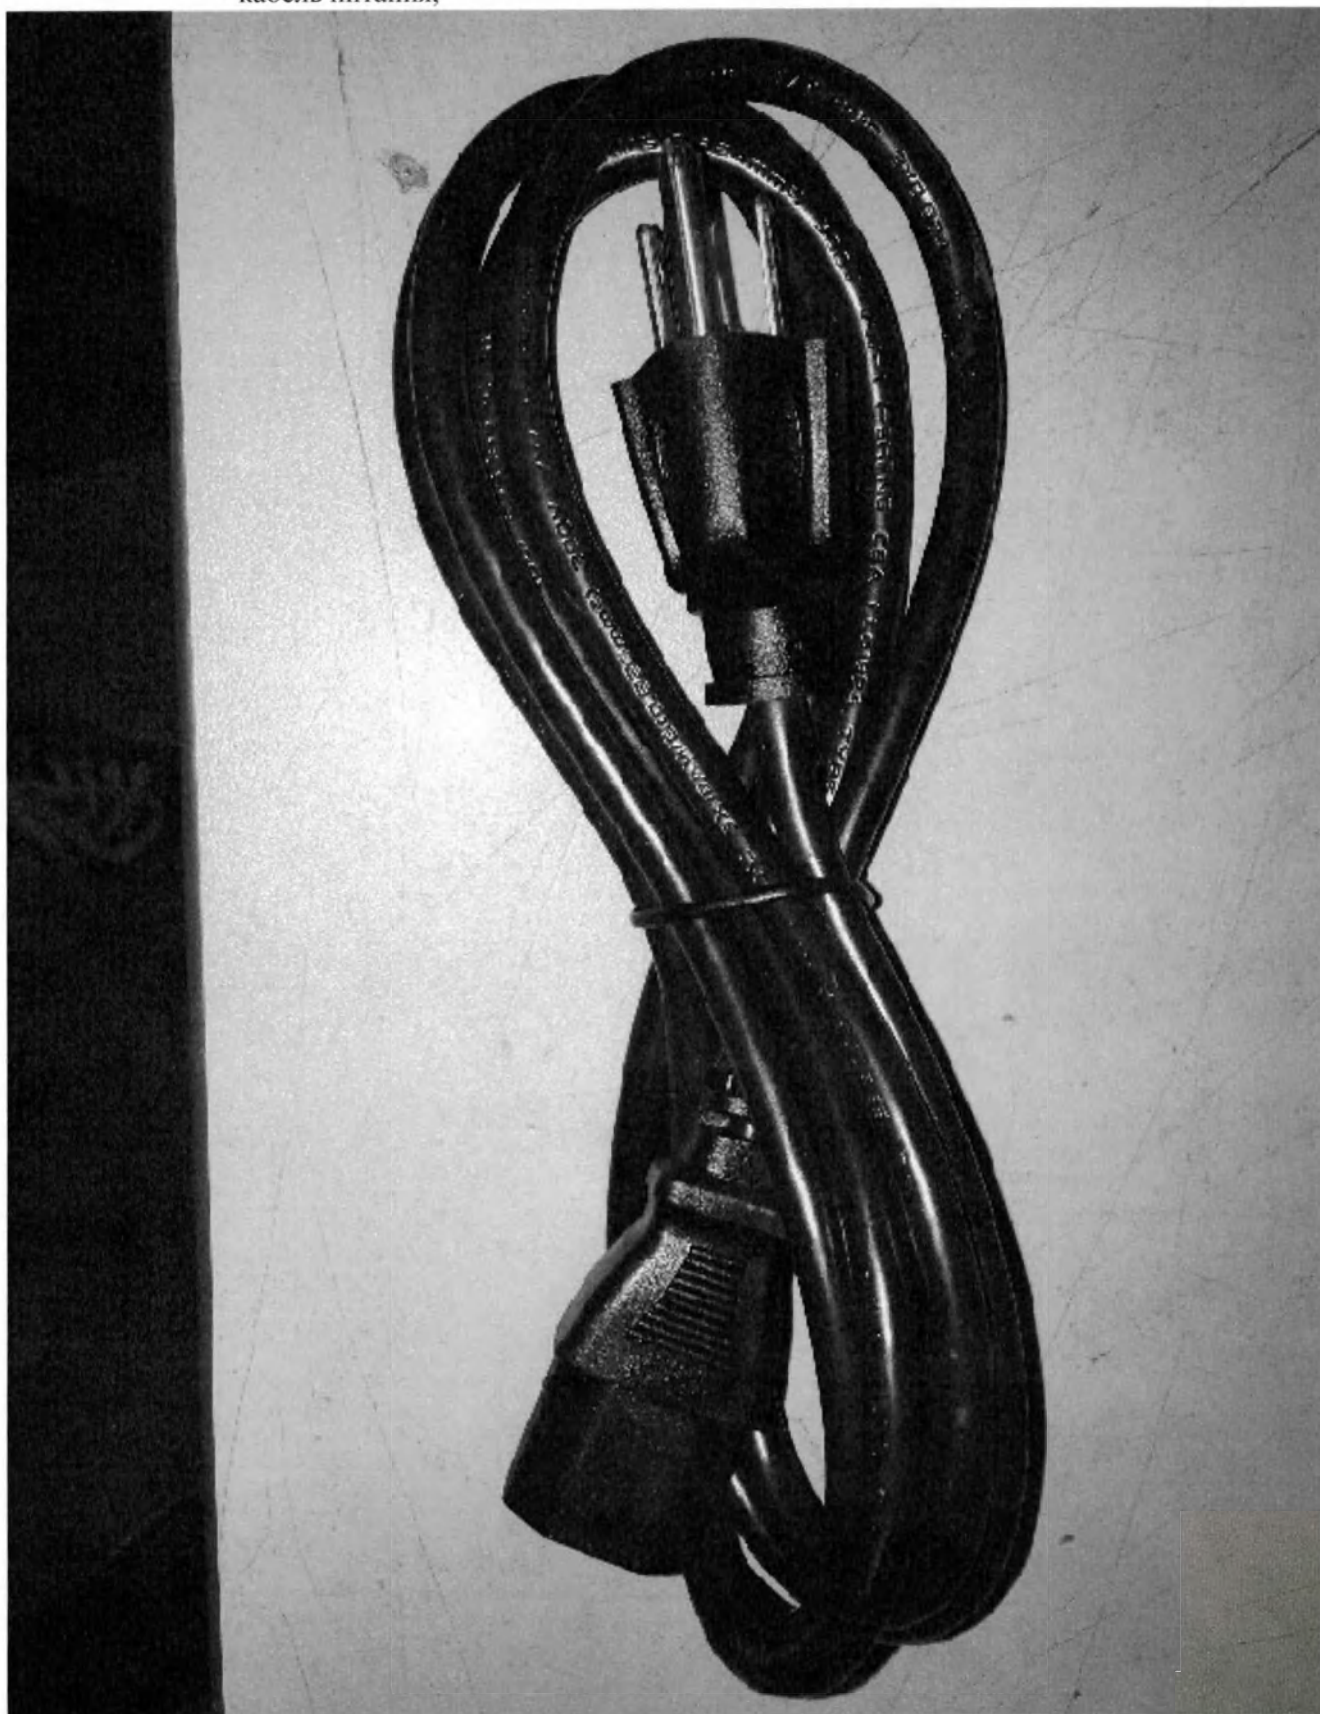

- CD-диски, не более 5-ти штук,

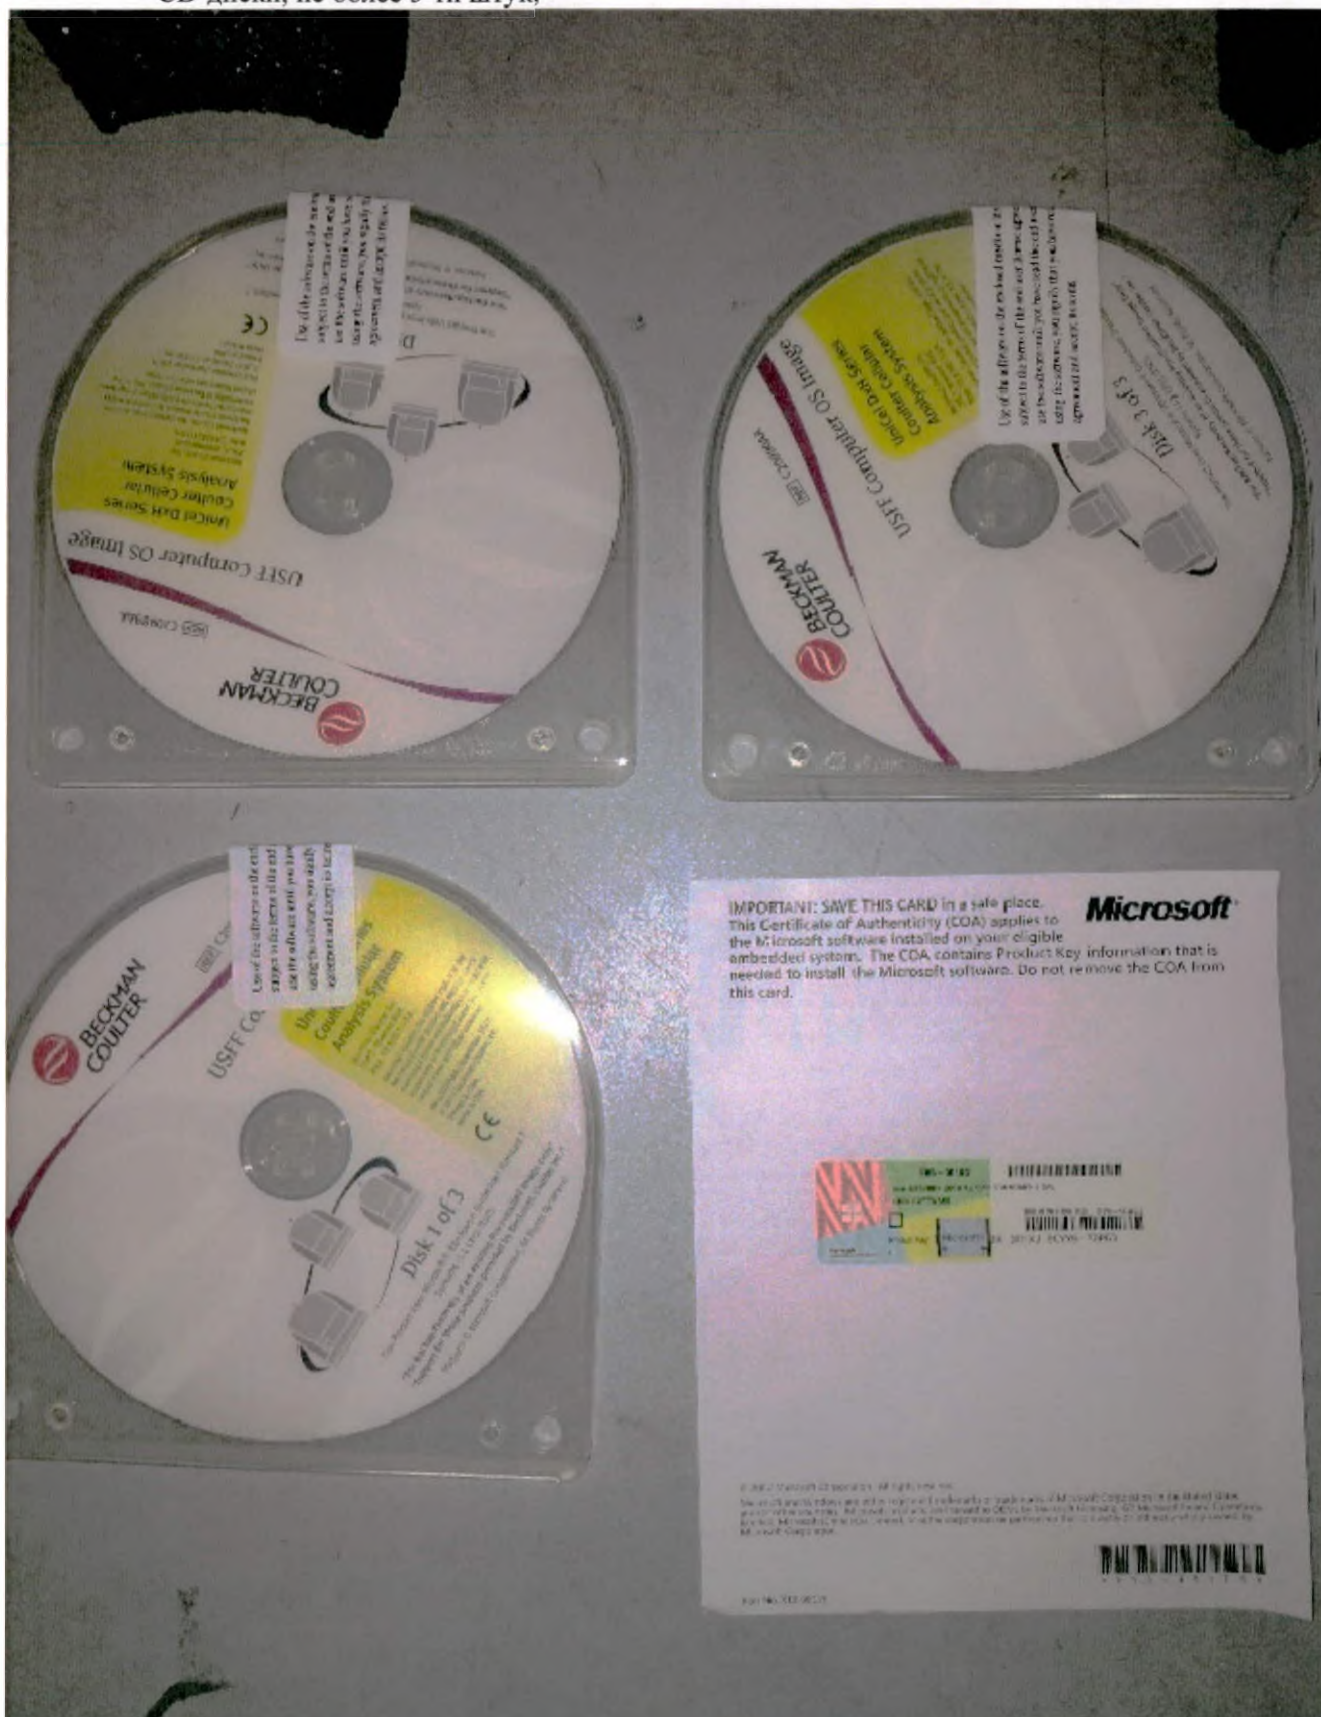



Symantec
 10000
 10000

Order Number: 10000000000000000000

Order Date: 2010-01-01

Order Status: Pending

Product Name: Symantec Endpoint Protection

Product Version: 10.0.0.100

Product License: 10000000000000000000

Microsoft

Microsoft Software License Agreement

Microsoft Corporation

One Microsoft Way

Redmond, WA 98073-0800

USA

Phone: (206) 936-6000

Fax: (206) 936-6001

Internet: www.microsoft.com

E-mail: licensing@microsoft.com

Technical Specifications

Item	Description	Value
1	Processor	Intel Core i7-2600K
2	Memory	16GB DDR3
3	Storage	1TB SATA
4	Operating System	Windows 7
5	Network Interface	10/100/1000 Ethernet
6	Power Supply	550W
7	Cases	Mid Tower
8	Peripherals	Keyboard, Mouse, Headset

Warranty Information

Warranty Period: 3 Years

Warranty Type: On-site

Warranty Start Date: 2010-01-01

Warranty End Date: 2012-12-31

Notes

1. All components are new unless otherwise specified.

2. All components are warranted by the manufacturer for a period of 3 years.

3. All components are warranted by the manufacturer for a period of 3 years.

4. All components are warranted by the manufacturer for a period of 3 years.

5. All components are warranted by the manufacturer for a period of 3 years.

6. All components are warranted by the manufacturer for a period of 3 years.


7. All components are warranted by the manufacturer for a period of 3 years.

8. All components are warranted by the manufacturer for a period of 3 years.

9. All components are warranted by the manufacturer for a period of 3 years.

10. All components are warranted by the manufacturer for a period of 3 years.

3. Стойка для установки монитора (при необходимости), в составе:
- монитор с тачскрином

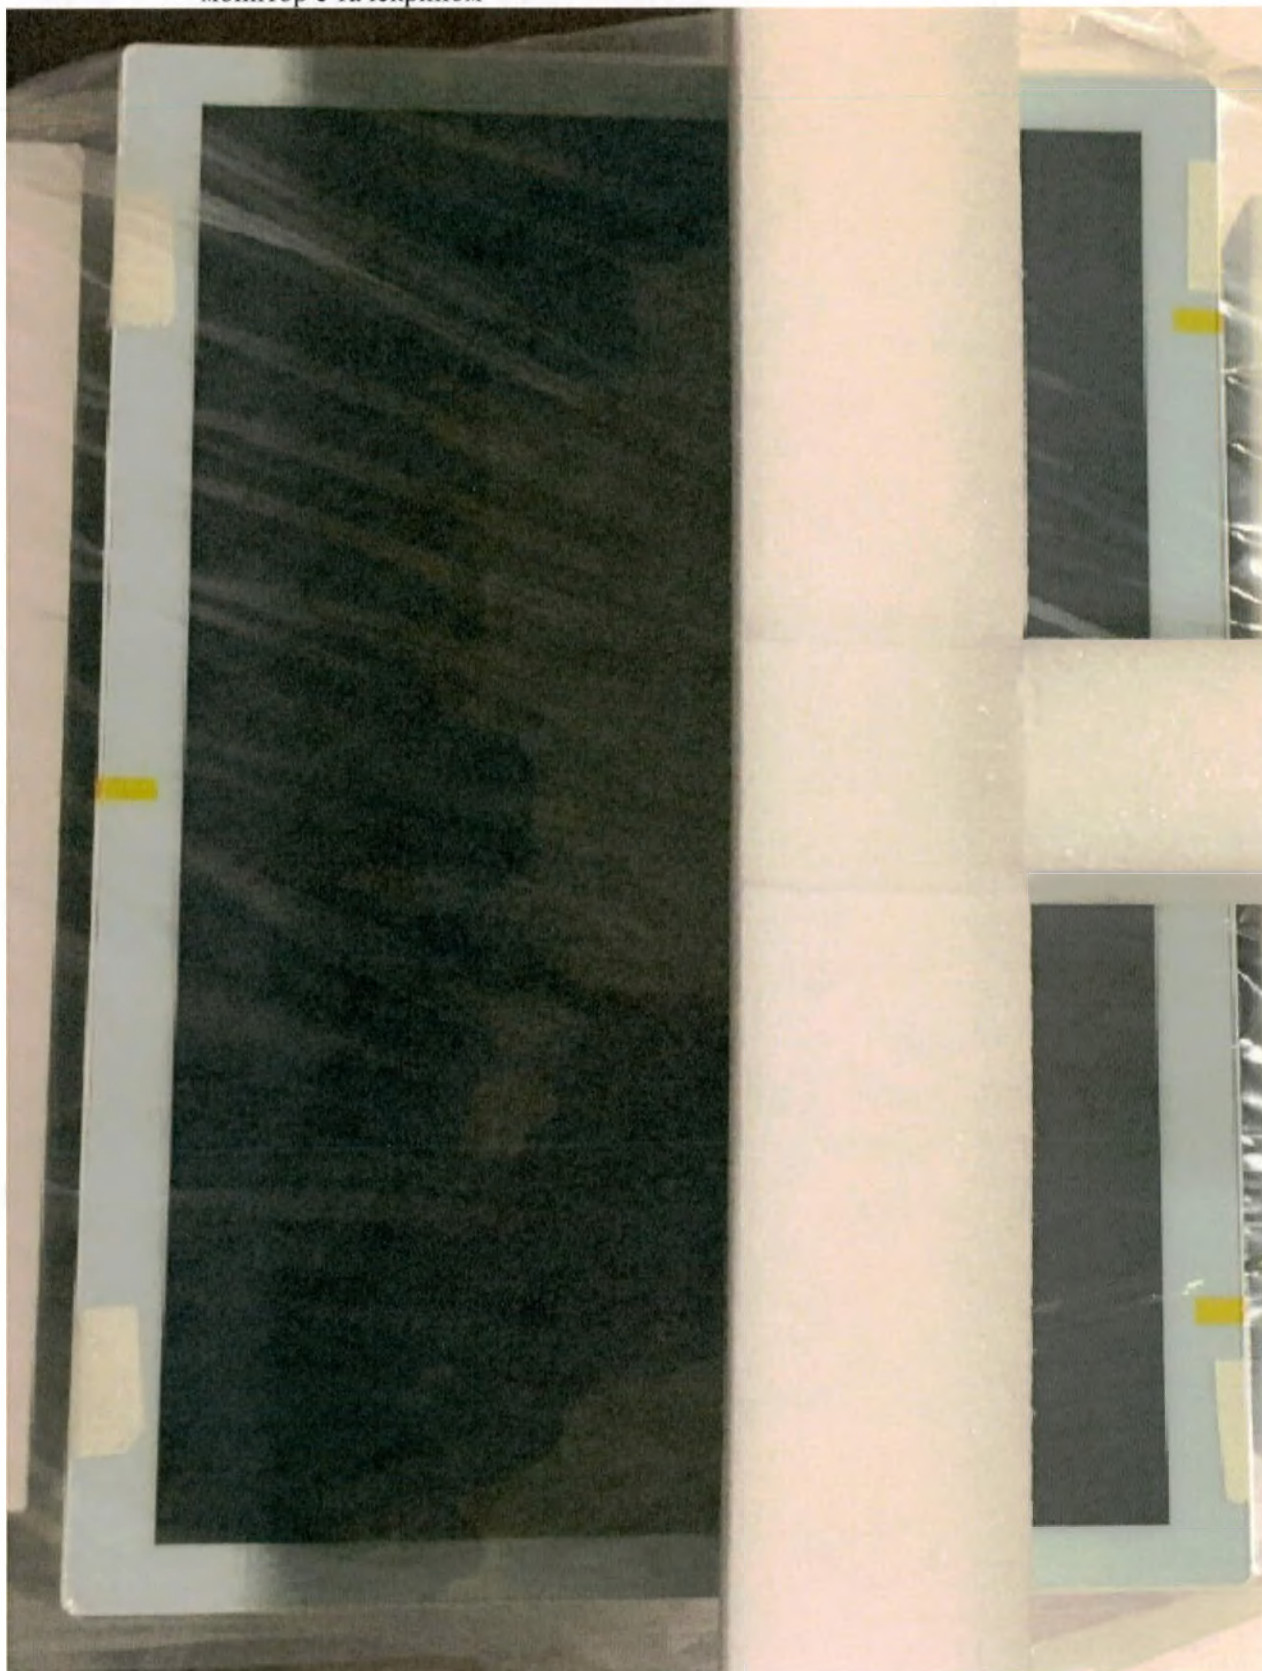


- компьютерная «Мышь»



- считыватель штрих-кодов ручной



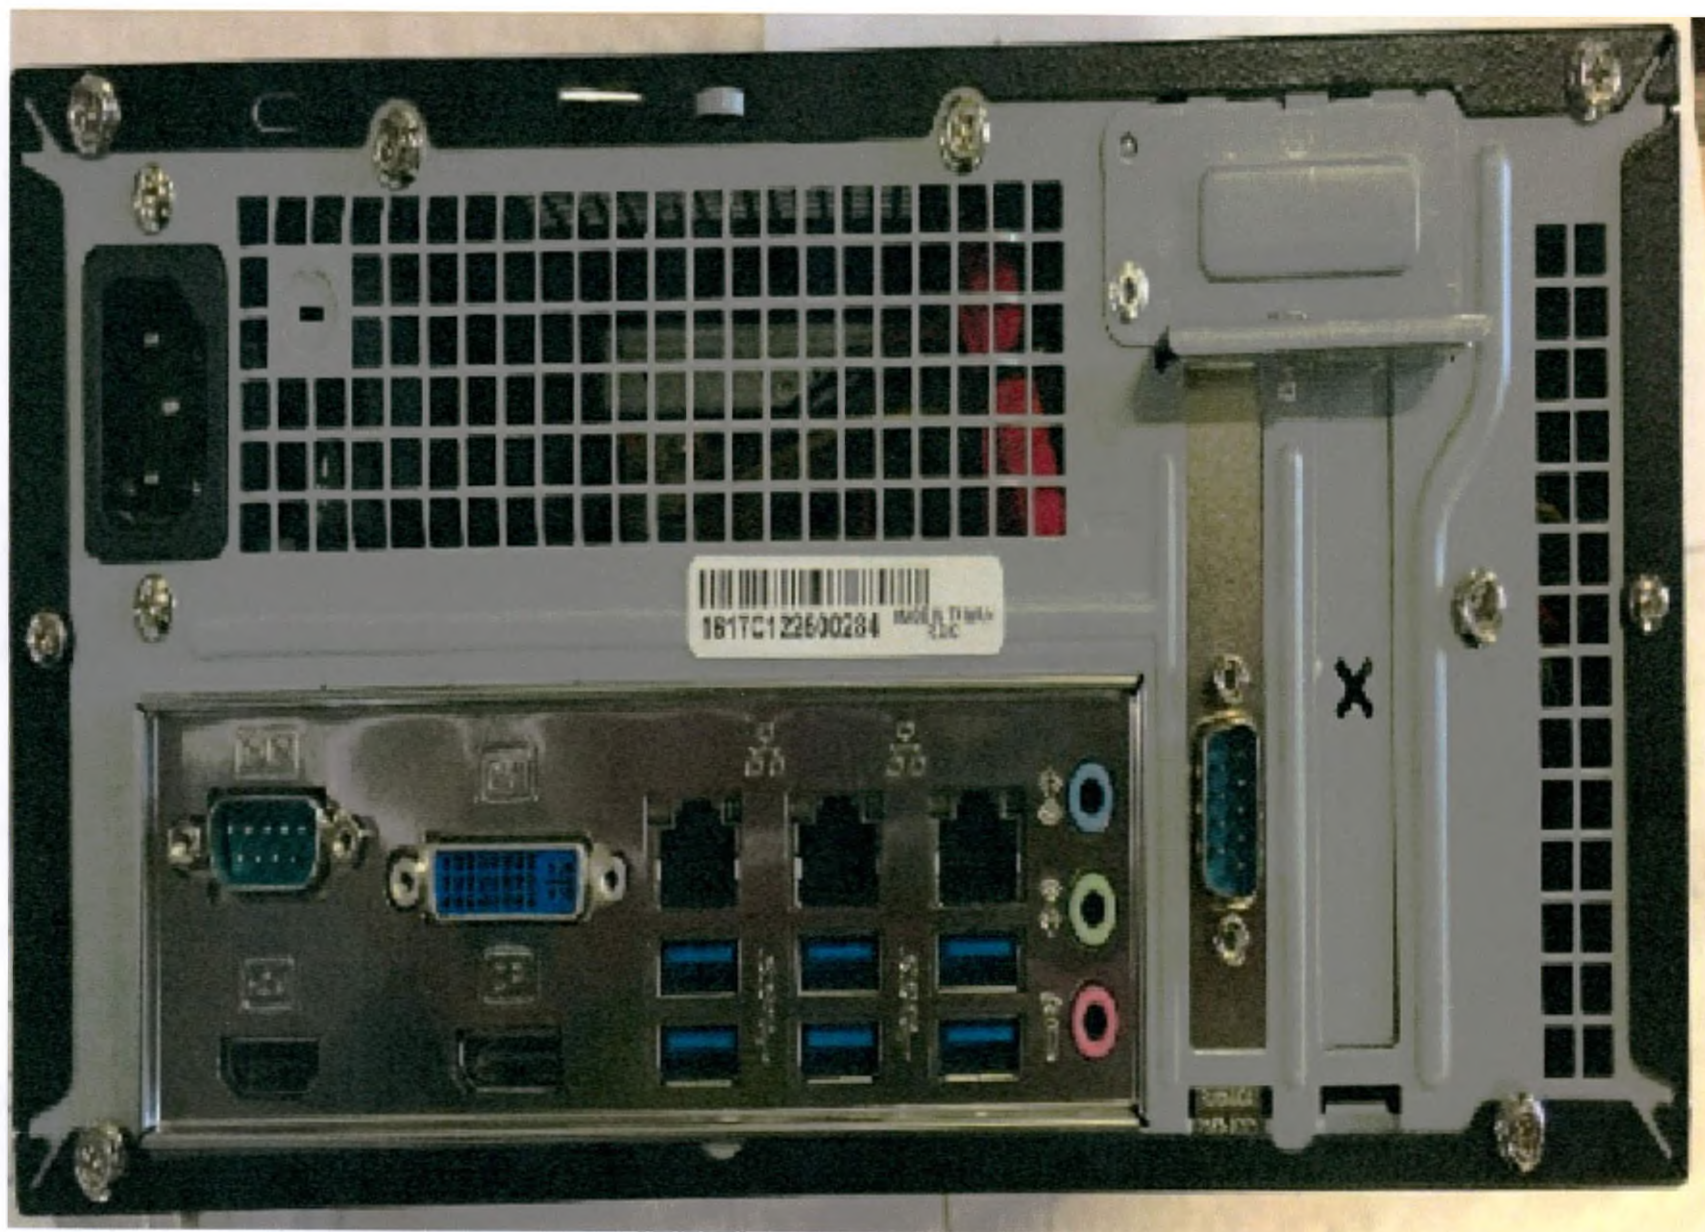


- Блок питания

- кабели, не более 7 шт.



- хомуты, не более 30 шт.

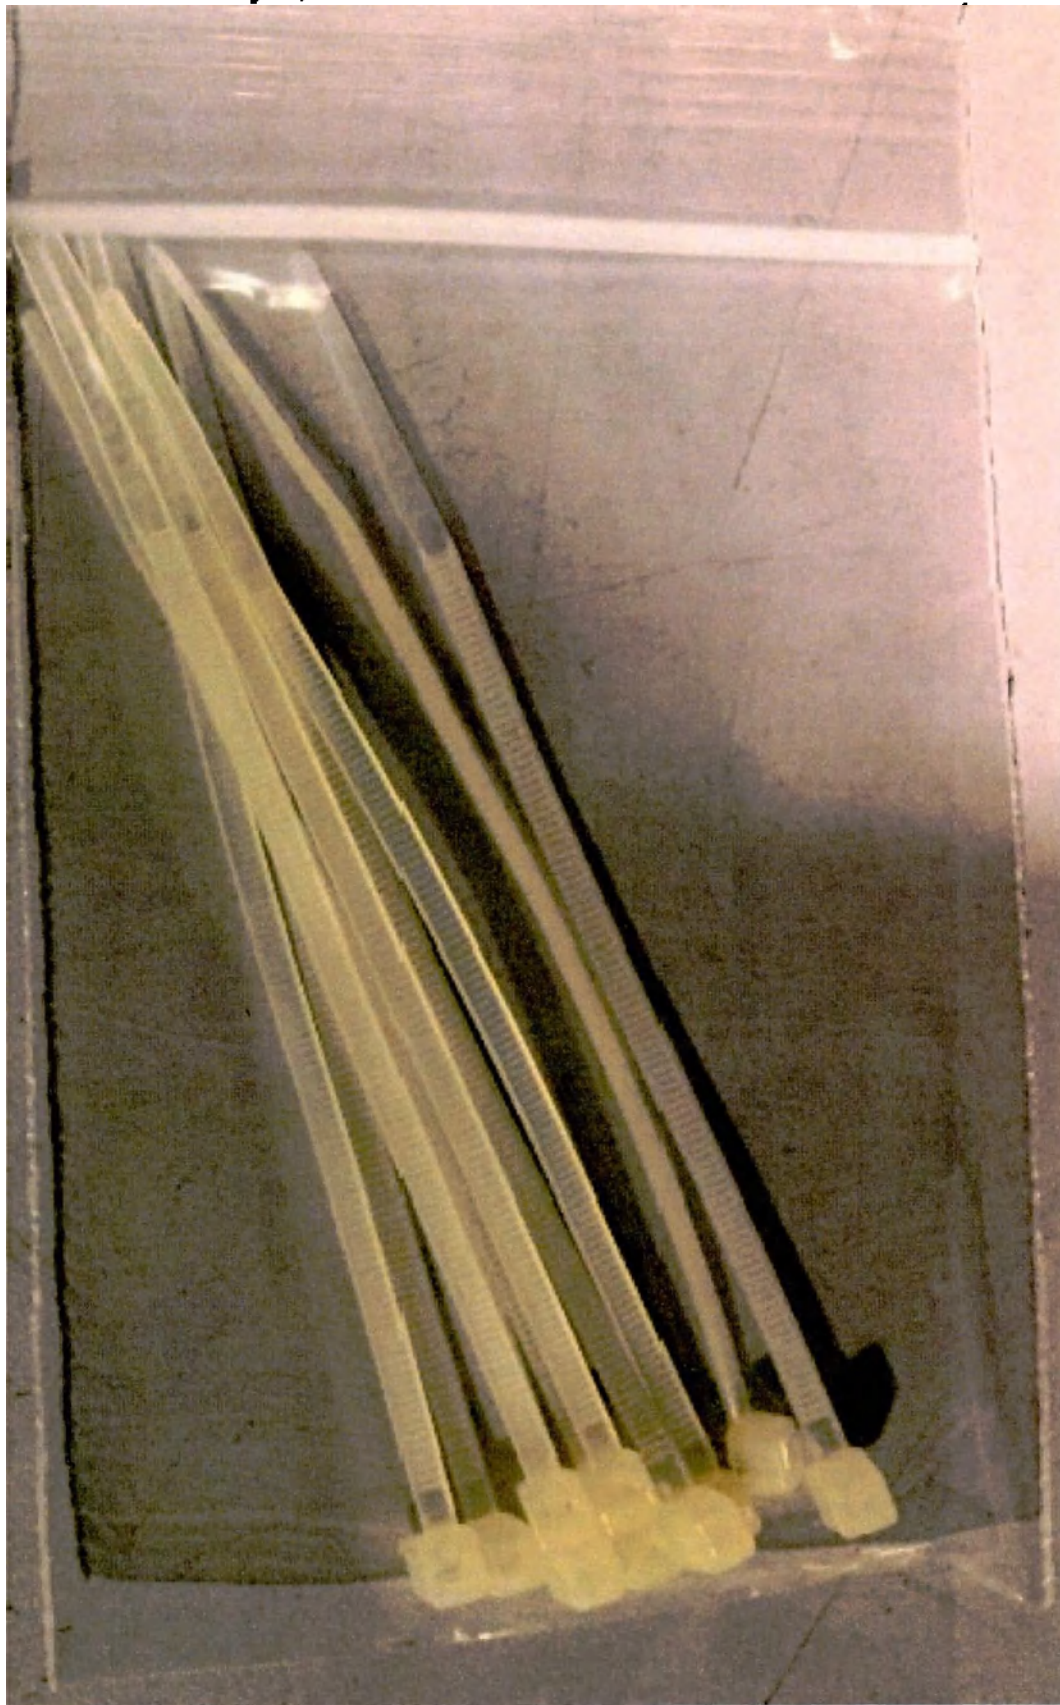

- стойка



- коврик для мыши



DxH 900



IMPORTANT PRODUCT NOTIFICATION for

UniCel® DxH™ Slidemaker Stainer Coulter® Cellular Analysis System, PN 775222
Using Beckman Coulter DxH Slides & Coulter TruColor Stains and Buffers

October 2013

Dear Beckman Coulter Customer,

Beckman Coulter has received reports of slide staining irregularities being experienced by some customers using Beckman Coulter DxH Slides and Coulter TruColor Stains and Buffers. This does not affect every lot of slides, stains or buffer.

Reported stain irregularities include:

- Red blood cells that appear hypochromic, refractile, or punched out.
- Excess precipitate that may be interpreted as increased cellular granularity in white blood cells, inclusions in red blood cells, and/or particles that interfere with platelet estimates.
- A dark blue/purple background stain that may interfere with the ability to read the slides.

These issues may impact frequency of maintenance, turnaround time and/or workflow. If you experience any staining irregularities, follow the recommendations listed below:

- To improve RBC morphology, add the information indicated below in bold print to the DxH SlideMaker Stainer Instructions for Use (IFU), Part Number A85371AD, Chapter 9, Cleaning Procedures, *Flushing Reagent lines and Stainer with Methanol*, before step 1.
... **IMPORTANT: Flushing water through the stainer lines may affect stain quality.**
Do not flush water through the reagent lines and stainer, except for Bath 5 rinse.
- To avoid excess precipitation and reduce background stain, closely follow the existing recommendations in PN A85371 AD – Appendix B, Table B.1 *Optimum Stain Quality Troubleshooting*.

Beckman Coulter is working to improve the quality of the slides.

Share this information with your laboratory staff and retain this notification as part of your laboratory Quality System documentation.

If you have any questions concerning this letter, please contact our Customer Support Center:

- Via our website, <http://www.beckmancoulter.com/customersupport/support>
- Via phone, call 800-526-7694 in the United States and Canada.
- Outside US and Canada, contact your local Beckman Coulter Representative.

We apologize for the inconvenience this issue has caused your laboratory. Thank you for your continued support of Beckman Coulter products.

Sincerely,

Caryl J. Campbell
Director of Technical Support Operations

4. Набор для установки (при необходимости), в составе:



- отвертка крестообразная




- отвертка прямой шлиц



- торцевой ключ



- острогубцы

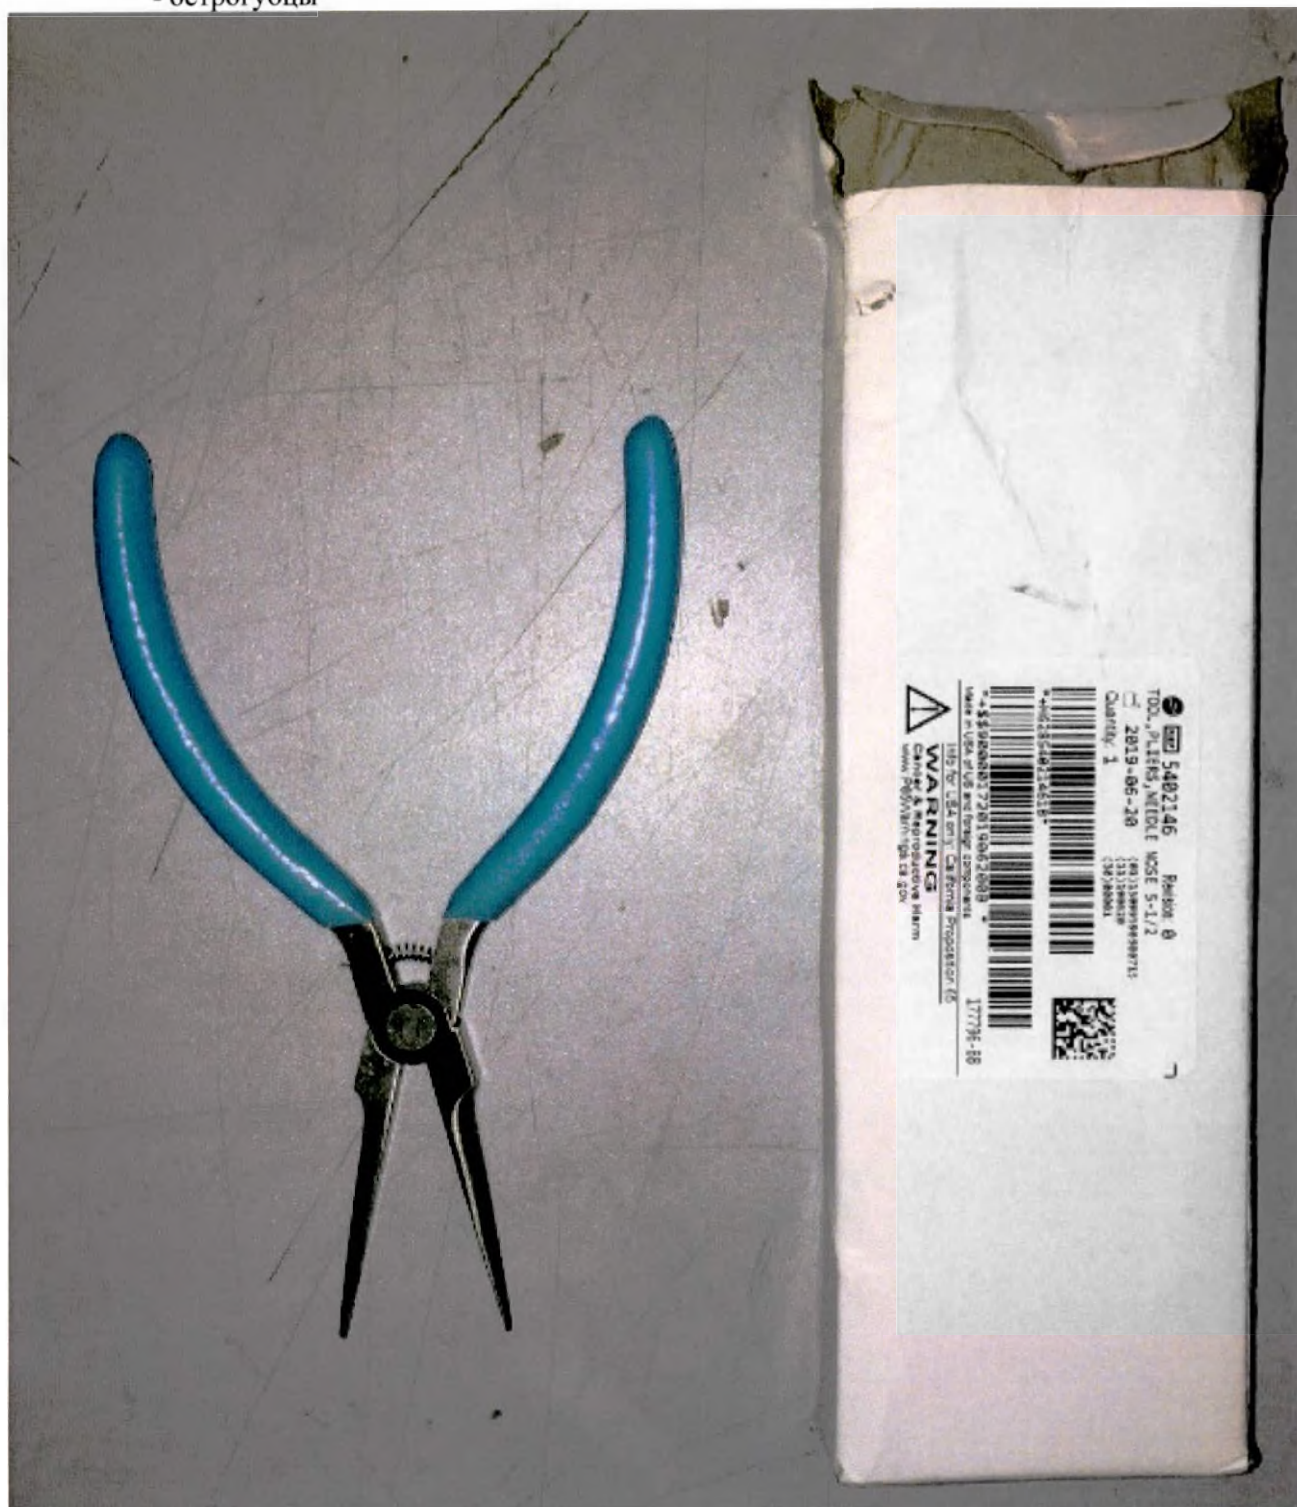

- переносной ящик




- кабели коммуникационные, не более 8 шт.



5. Программное обеспечение на CD/DVD дисках – не более 10 шт. (при необходимости).



6. Мерная кювета – не более 100 шт.

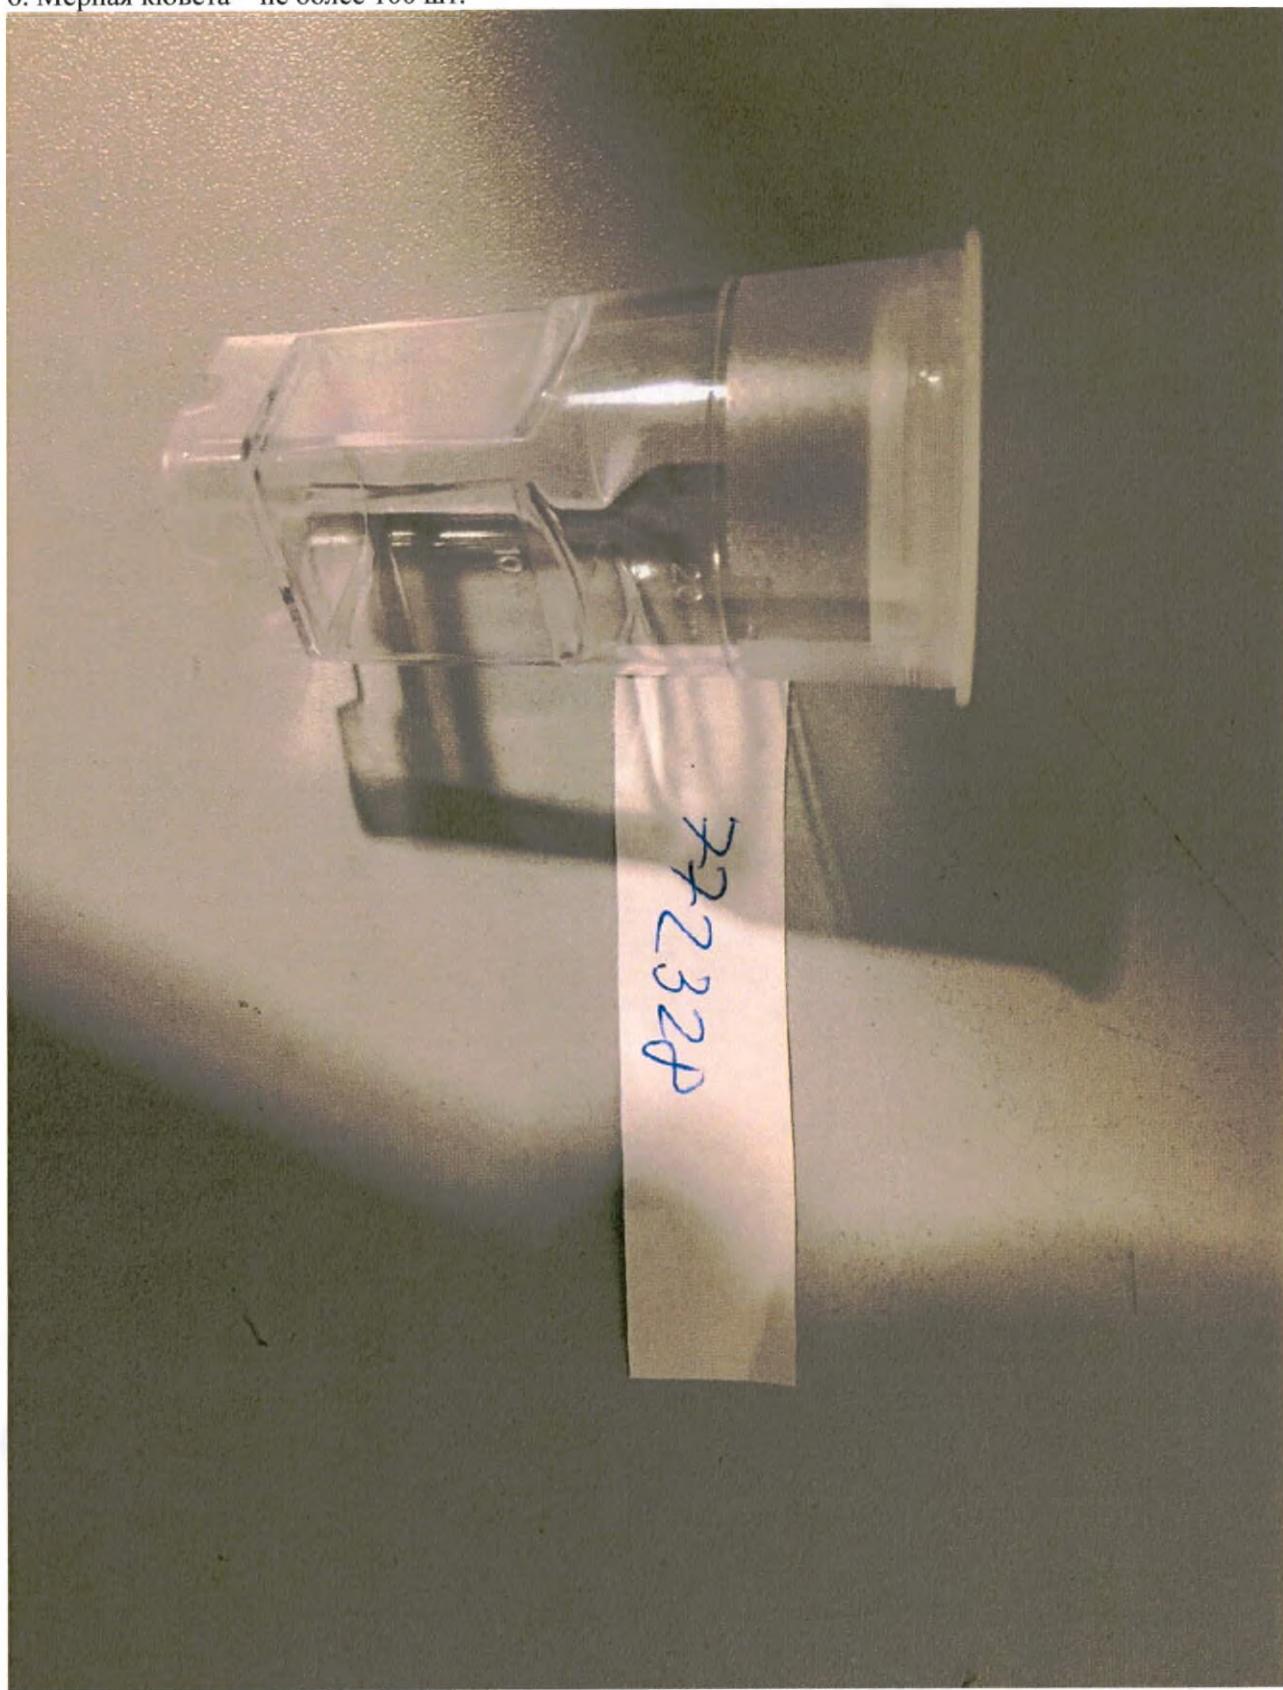

7. Дозаторы образца – не более 100 шт.



8. Кассеты для образцов типа А, 20 шт/уп - не более 100 уп.



9. Стекля для окрашивания препаратов 72 шт/уп. - не более 100 уп.



10. Пробоотборник для аспирации образца



Принадлежности:

- двойной скотч для крепления, не более 4 шт.

Ship To:

Republic Packaging of Florida
4570 NW 128th St. RD.
Opa Locka, FL, 33054

Ship To:

Republic Packaging of Florida
4570 NW 128th St. RD.
Opa Locka, FL, 33054

B24444
DXH SMS Packaging
Return Instructions

- 1) Unroll the roll of tape.
- 2) Remove the tape from the roll.
- 3) Cut the tape into 4 equal pieces.
- 4) Cut the tape into 4 equal pieces.
- 5) Cut the tape into 4 equal pieces.
- 6) Cut the tape into 4 equal pieces.
- 7) Cut the tape into 4 equal pieces.
- 8) Cut the tape into 4 equal pieces.
- 9) Cut the tape into 4 equal pieces.
- 10) Cut the tape into 4 equal pieces.
- 11) Cut the tape into 4 equal pieces.
- 12) Cut the tape into 4 equal pieces.

Place the 66
corrugated
the front of

Replace the plywood spreader plate on top of the top flap and place the tape on the pallet as shown, strap the kit together. Use the plastic banding included. Make sure to run the plastic banding through the Granding holes located on the pallet.



- Remove all "Name" and "Ship to" labels from packaging.
- Complete the "Shipped From" portion in the upper right corner of Conway Bill of Lading (BOL) and place them into the two self-adhesive envelopes included in this instruction kit and place them on the left and right side of the front corrugated panels.
- Place one "Ship to: Republic Packaging" self-adhesive label below the "Bill of Lading" envelope.
- Call Conway Central 1-800-421-4007 for crate pick up.
- Note: Have the completed BOL, pen and paper handy when you make the call.
- Conway will ask you for the address of the pickup location on the BOL.
- They may request you call another number for pick up.
- Request shipping and receiving to move packaged unit such that it can be picked up by Conway.
- Conway Central will pick up the crate within 24 hours.

RECONWAY
CORP.

820 PARTS NUMBER
A B24405


- металлический стержень (датчик) для определения уровня жидкости, не более 2 шт.



- пластины для дверцы, не более 4 шт.



- кисточка – не более 10 шт.

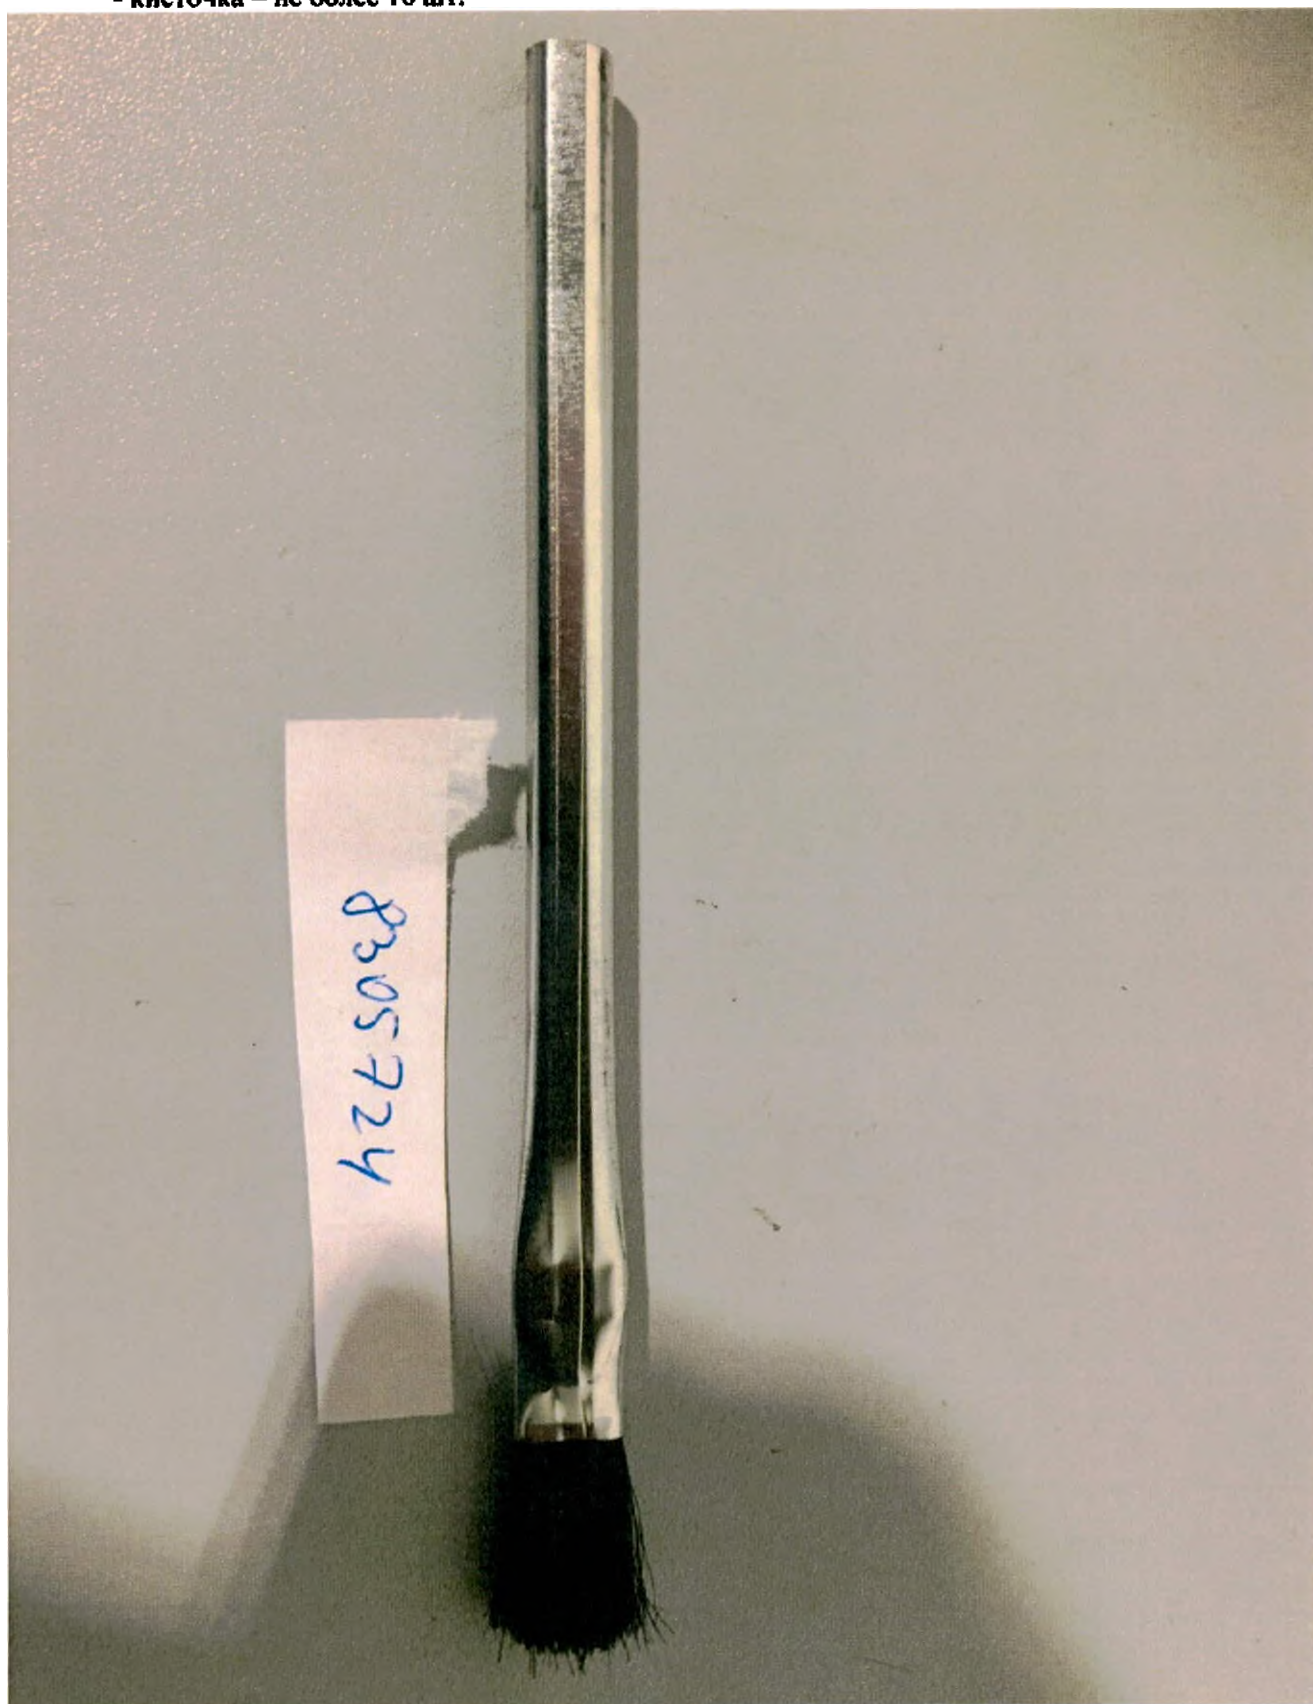

- хомуты, не более 10 шт.




- винты для крепления элементов системы, не более 20 шт.




- крышки бутылей пластиковые, не более 4 шт.



- световой индикатор состояния системы – не более 10 шт.

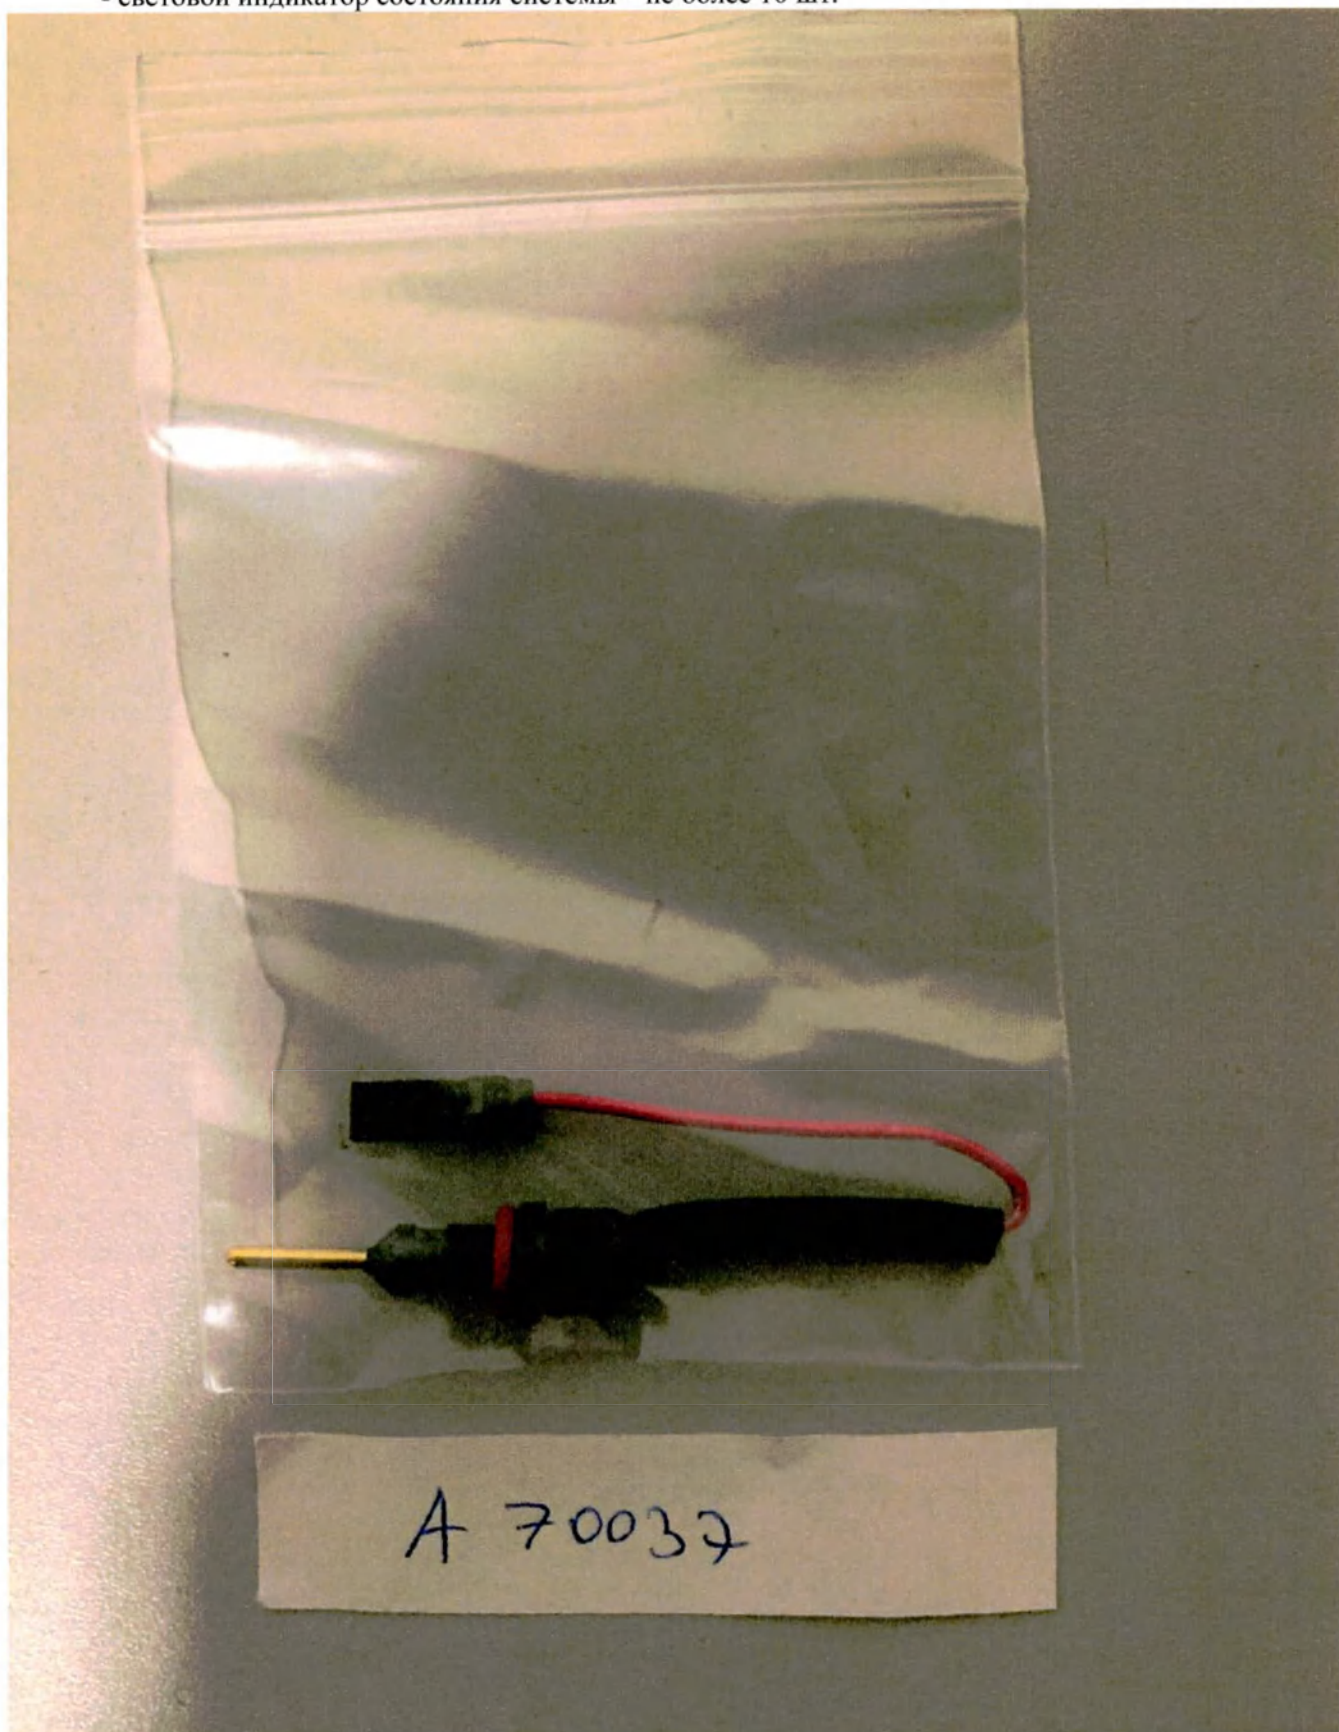

- трубка в сборе с обратным клапаном, коннектором и фильтром с этикетками и крышками – не более 10 шт.

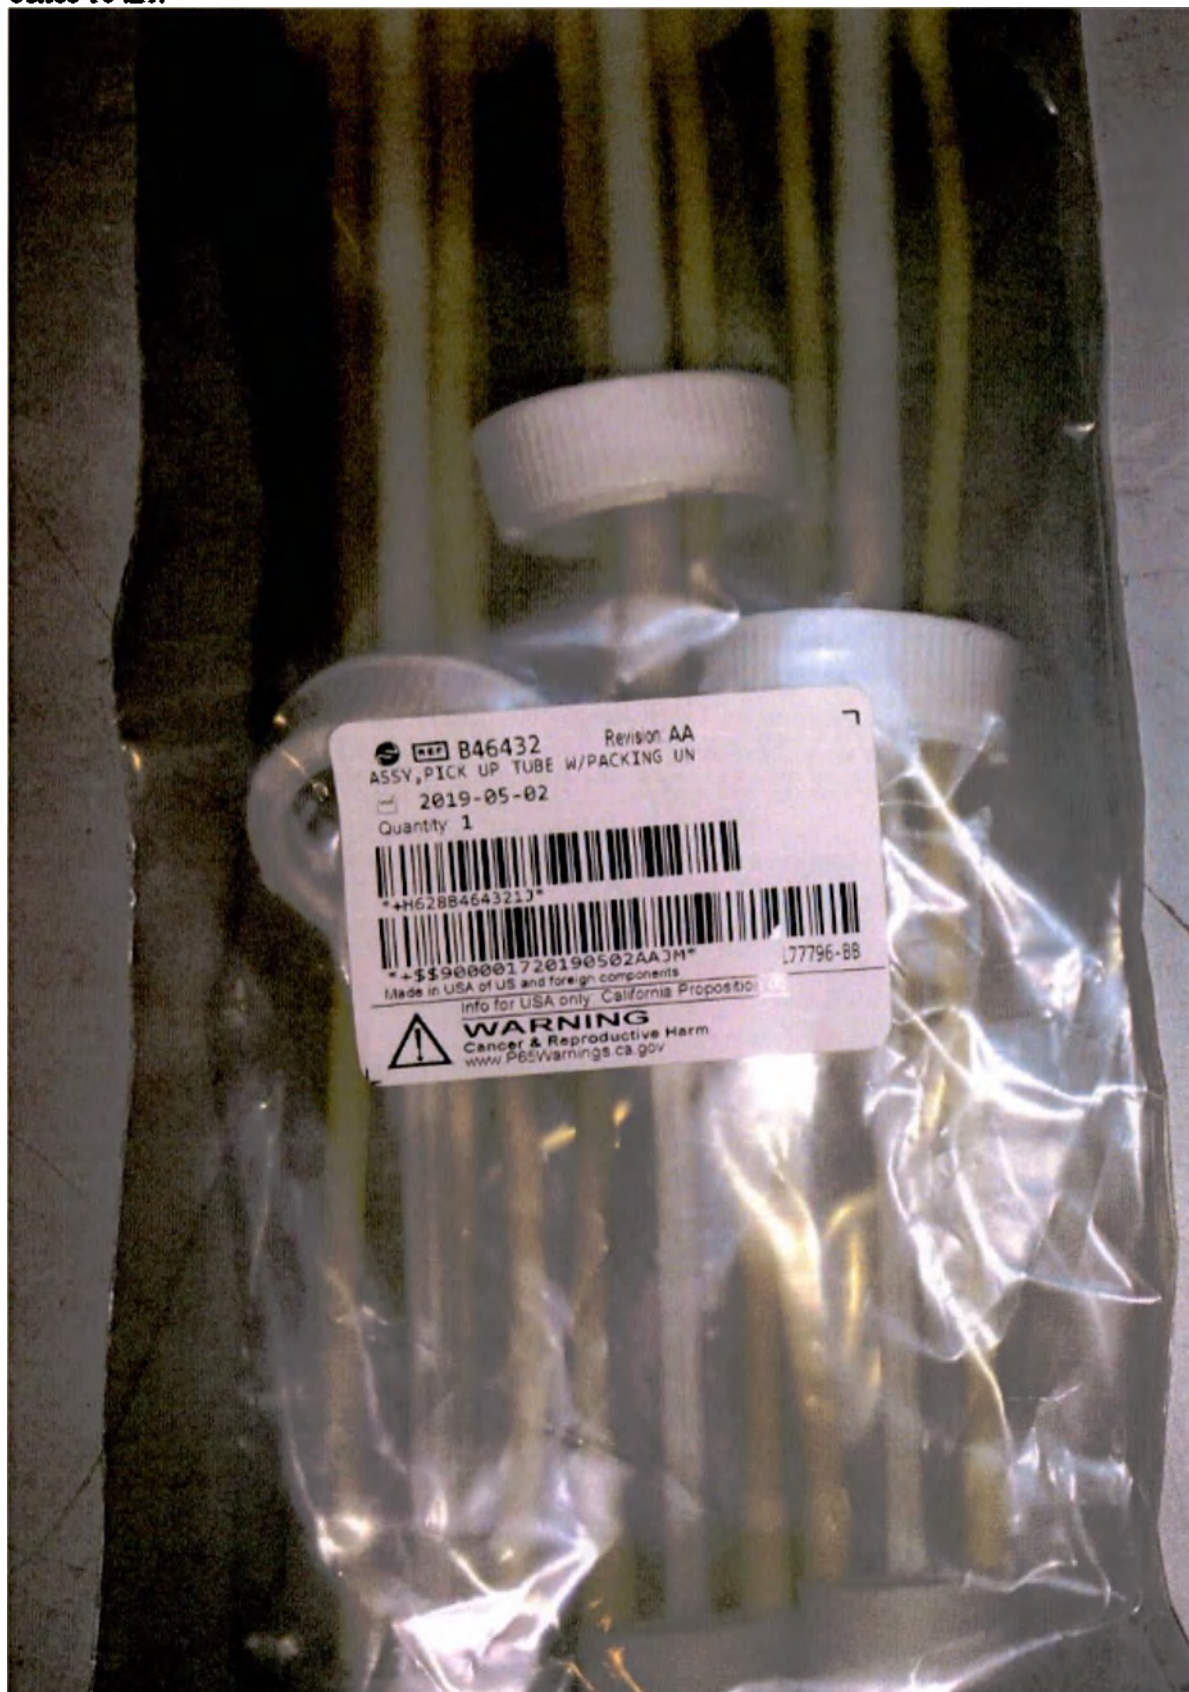

[illegible]


- картридж для встроенного матричного принтера (ленточный) – не более 10 шт.



- металлическая вставка – не более 10 шт.



- заглушки для разъемов, не более 6 шт.

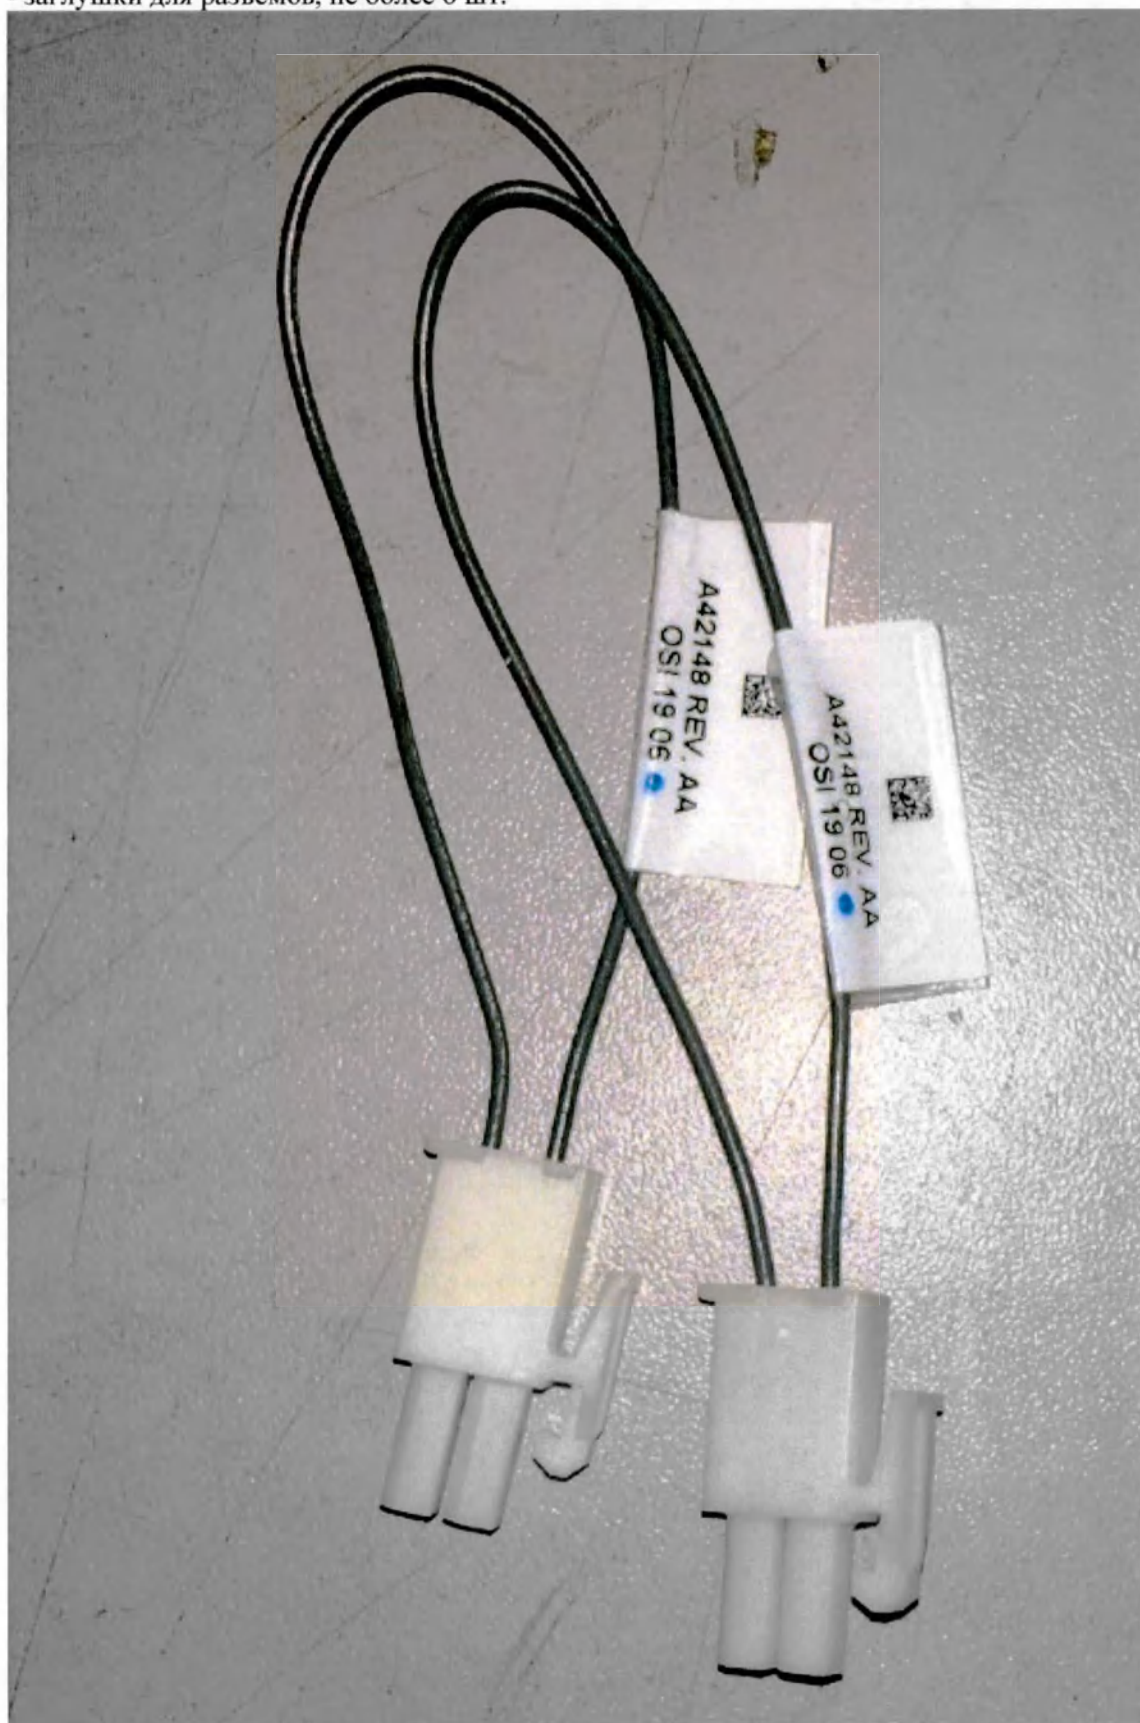


- наклейки, не более 2 листов




- трубка сброса отходов экранированная – не более 10 шт.



- воронки для перелива, не более 2 шт.

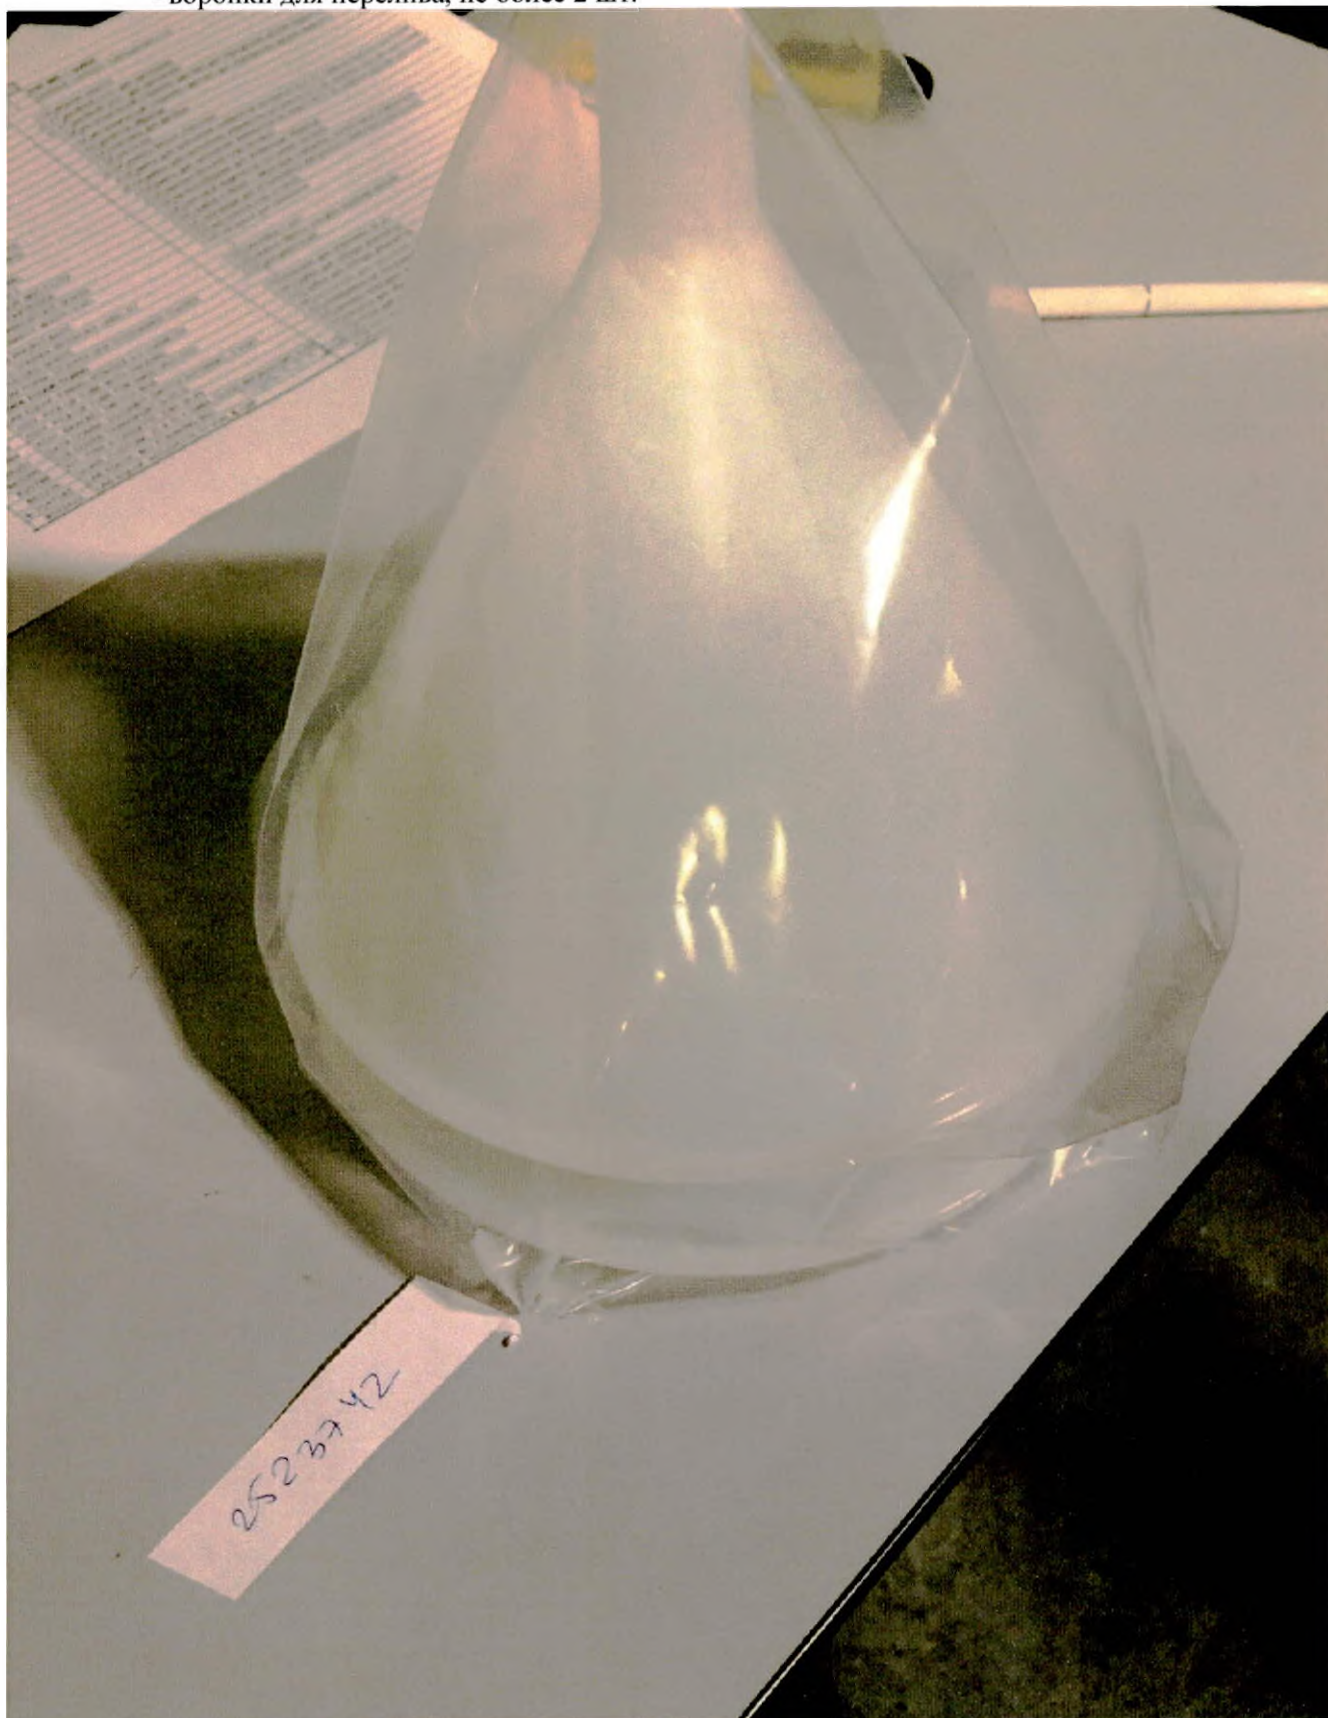

- трубки для отбора реагентов, не более 10 уп.

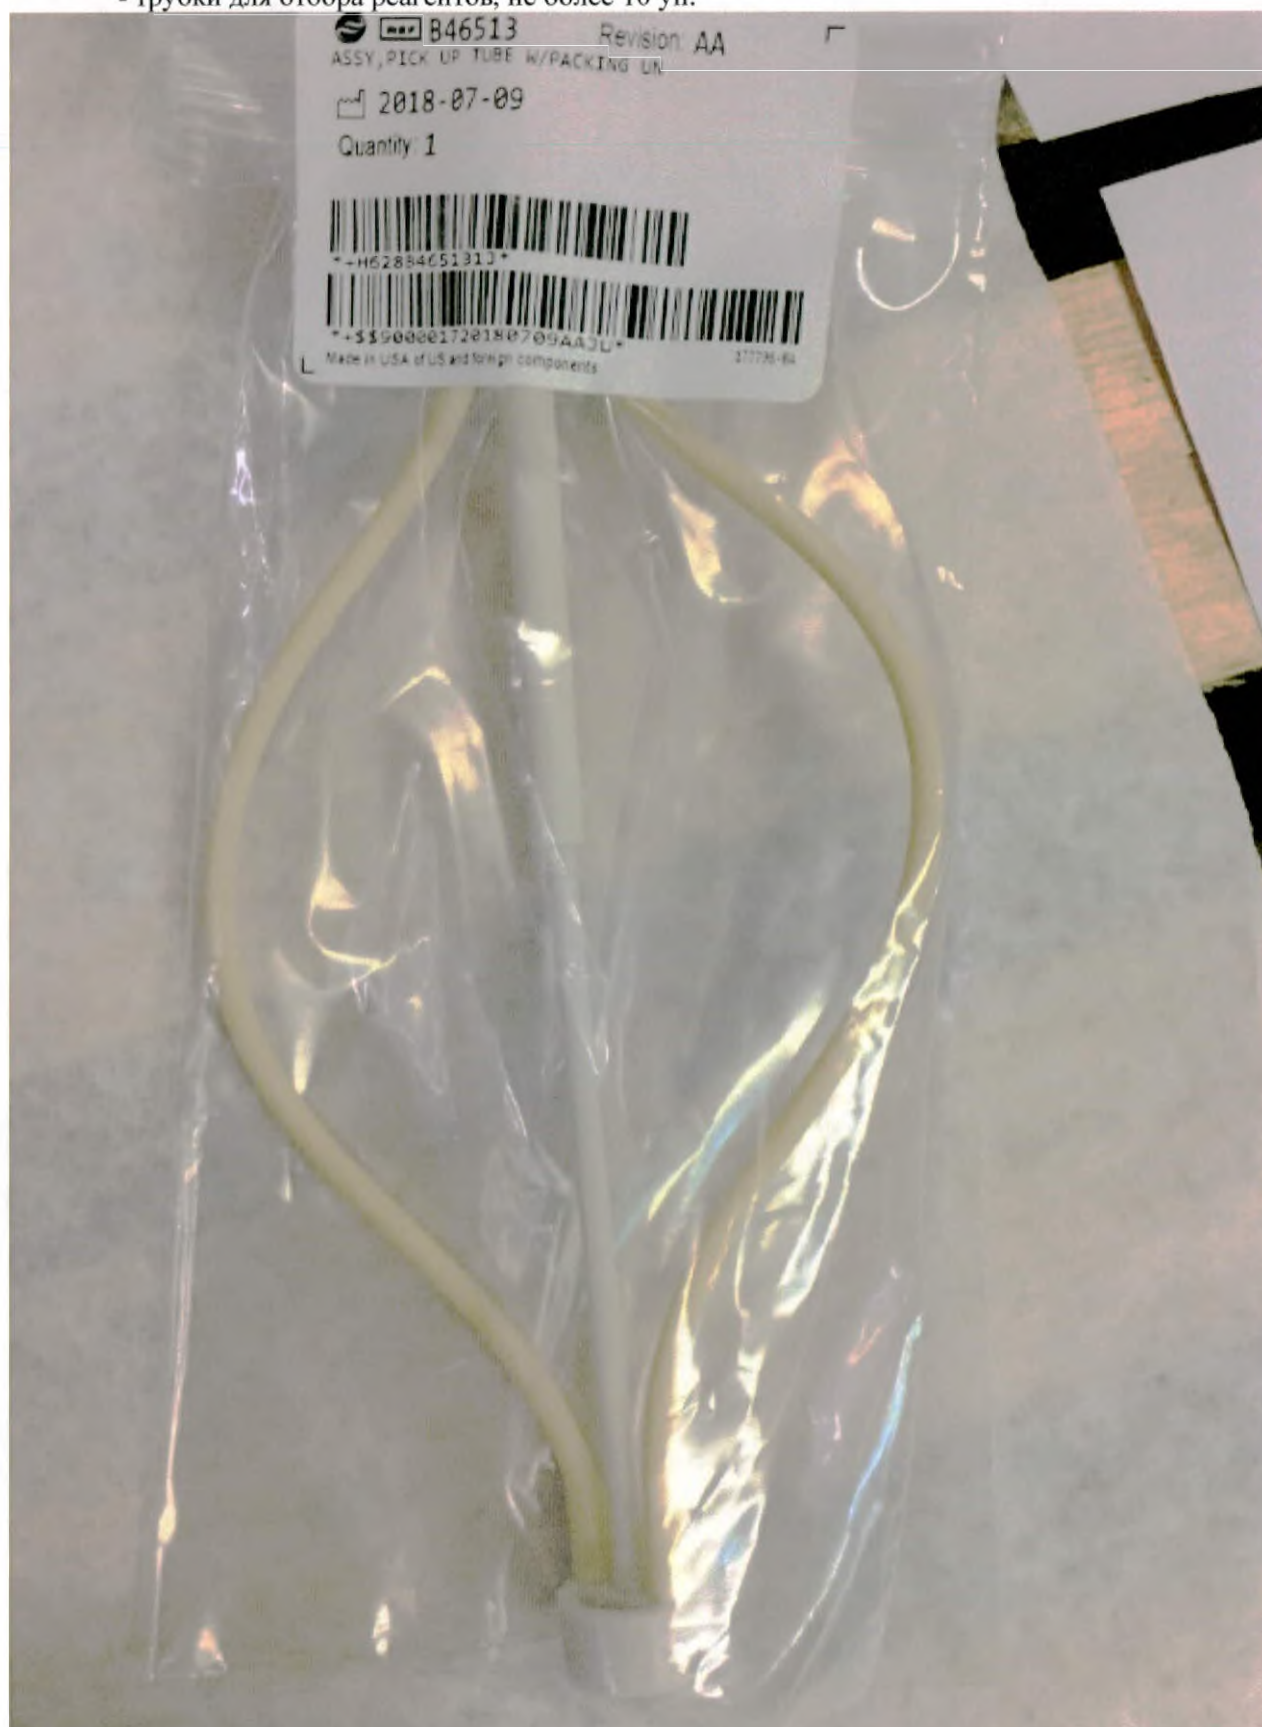

- кронштейн для крепления коммутатор локальной LAN сети – не более 10 шт.



- коммутатор локальной LAN сети, в комплекте с кабелем с блоком питания – не более 10 шт.

NETGEAR®

SOHO SWITCH SERIES

5-Port Gigabit Ethernet Switch Commutateur Ethernet Gigabit 5 ports


Plug and Play Prêt à l'emploi



Model No.
GS305


Ideal for Small Office and Home Office
Rugged metal case
LED on each port
Wall mountable

Idéal pour les petits bureaux
et les bureaux à la maison
Boîtier métallique robuste
Voyant sur chaque port
Adapté pour montage mural



Gigabit Ethernet Switch/Commutateur

- крышка передняя защитная – не более 10 шт.

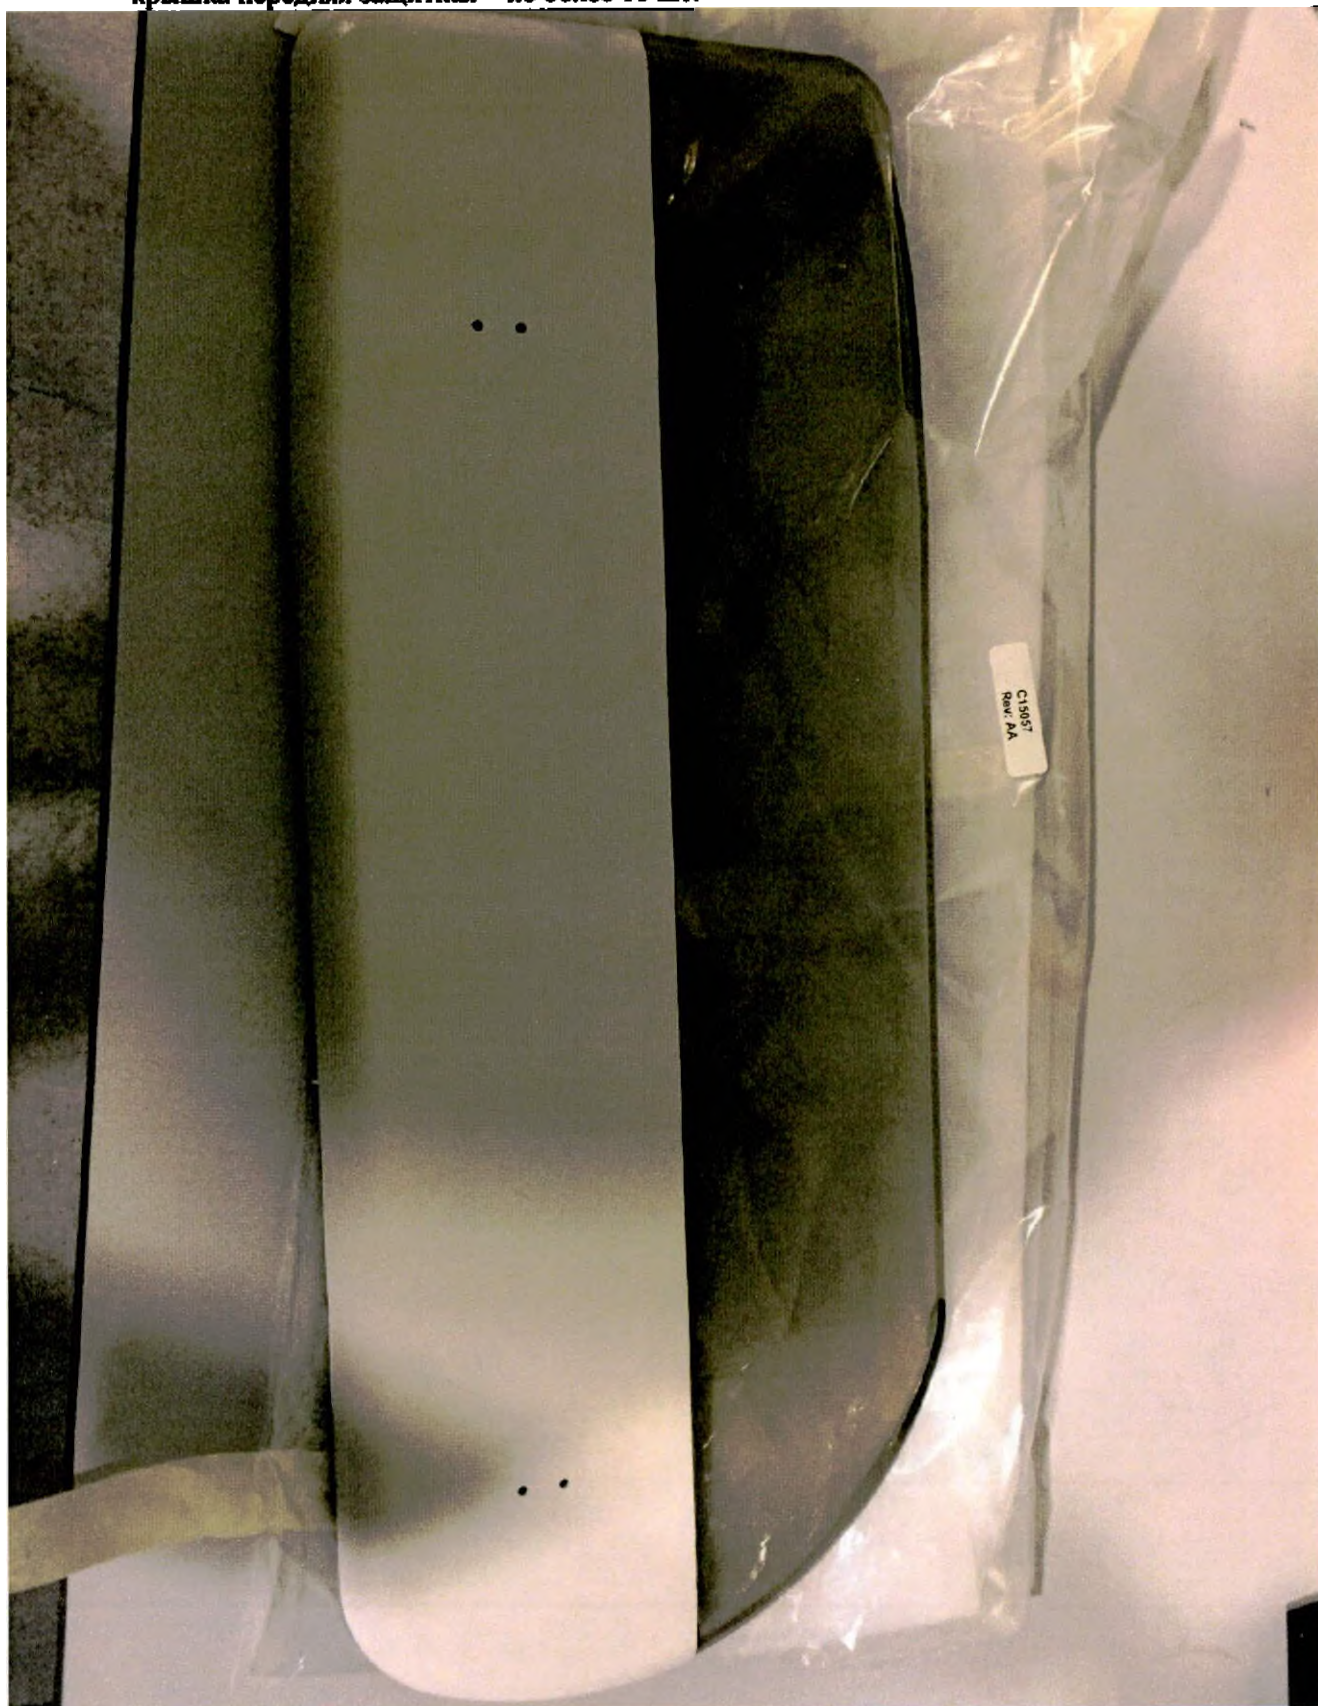

- канистры без крышек для окрашивающих реагентов, 1 л, не более 6 шт.



- канистры с крышками 5 л, не более 3 шт.



[illegible]

- канистры с крышками для окрашивающих реагентов, 2 л, не более 7 шт.




- боковые крышки в комплекте с винтами, не более 2 шт.



- пластиковая крышка модуля выгрузки кареток – не более 10 шт.



- ванны для окраски - не более 12 шт.

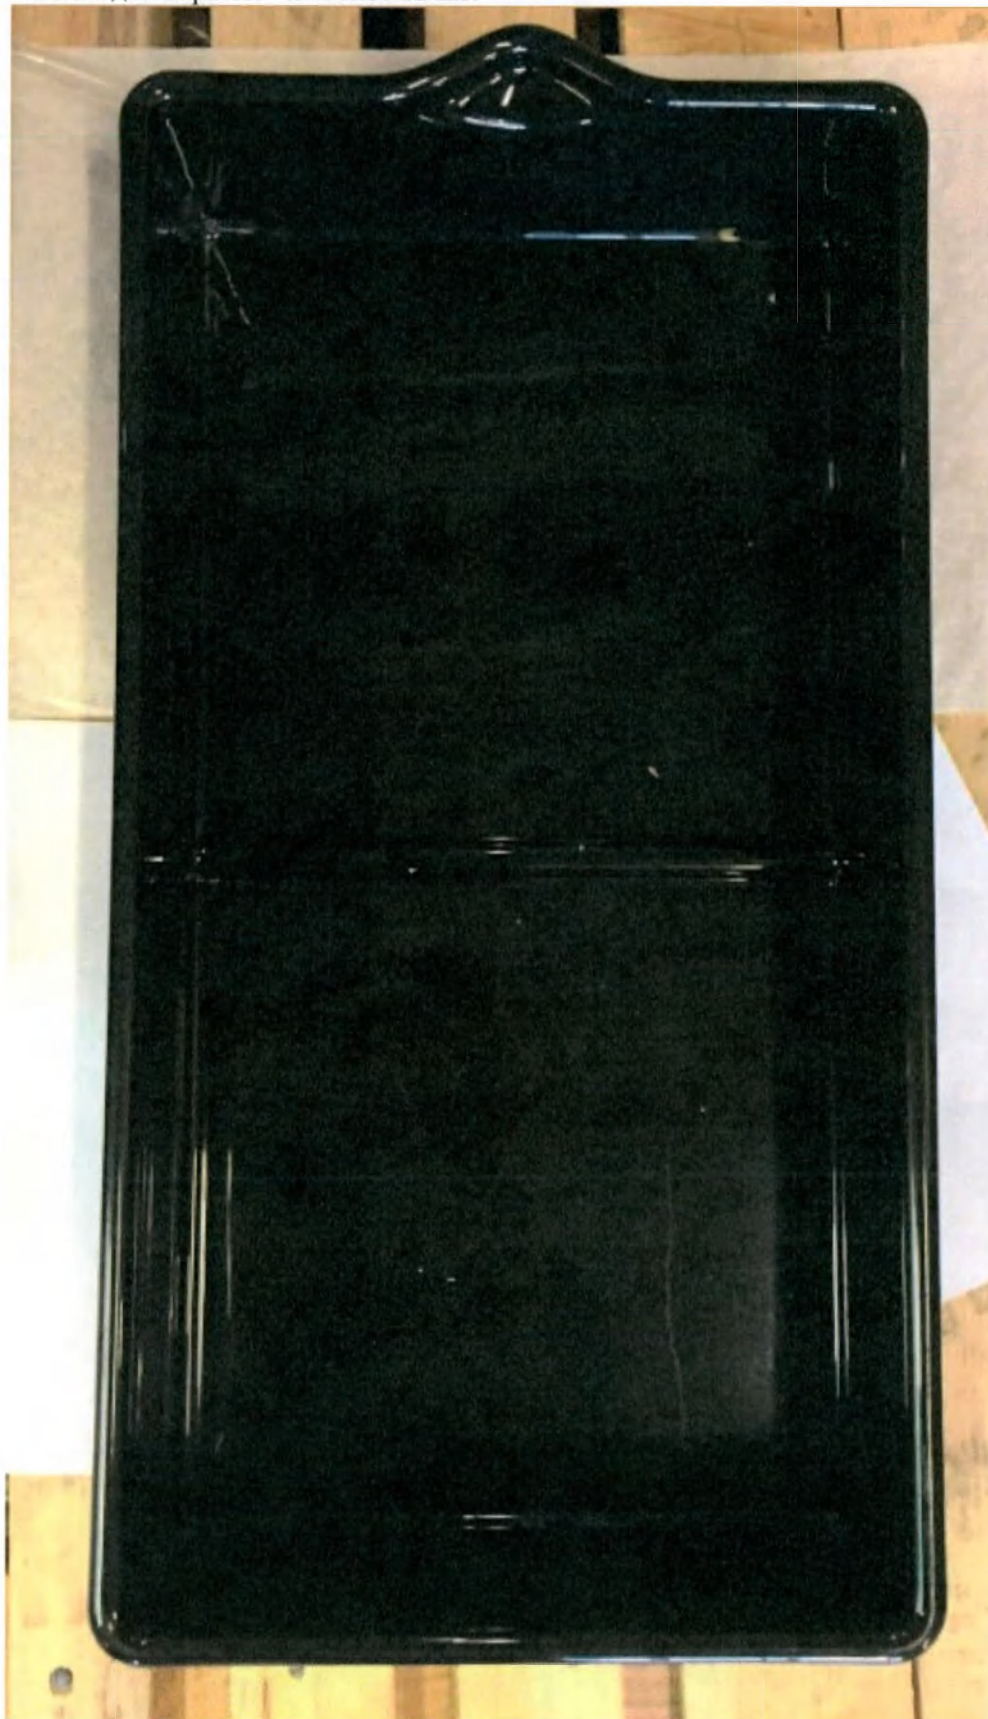


- каретки, не более 2 уп.




- поддоны для 5-ти малых ванн, не более 5 шт.




- этикетки, не более 2 листов

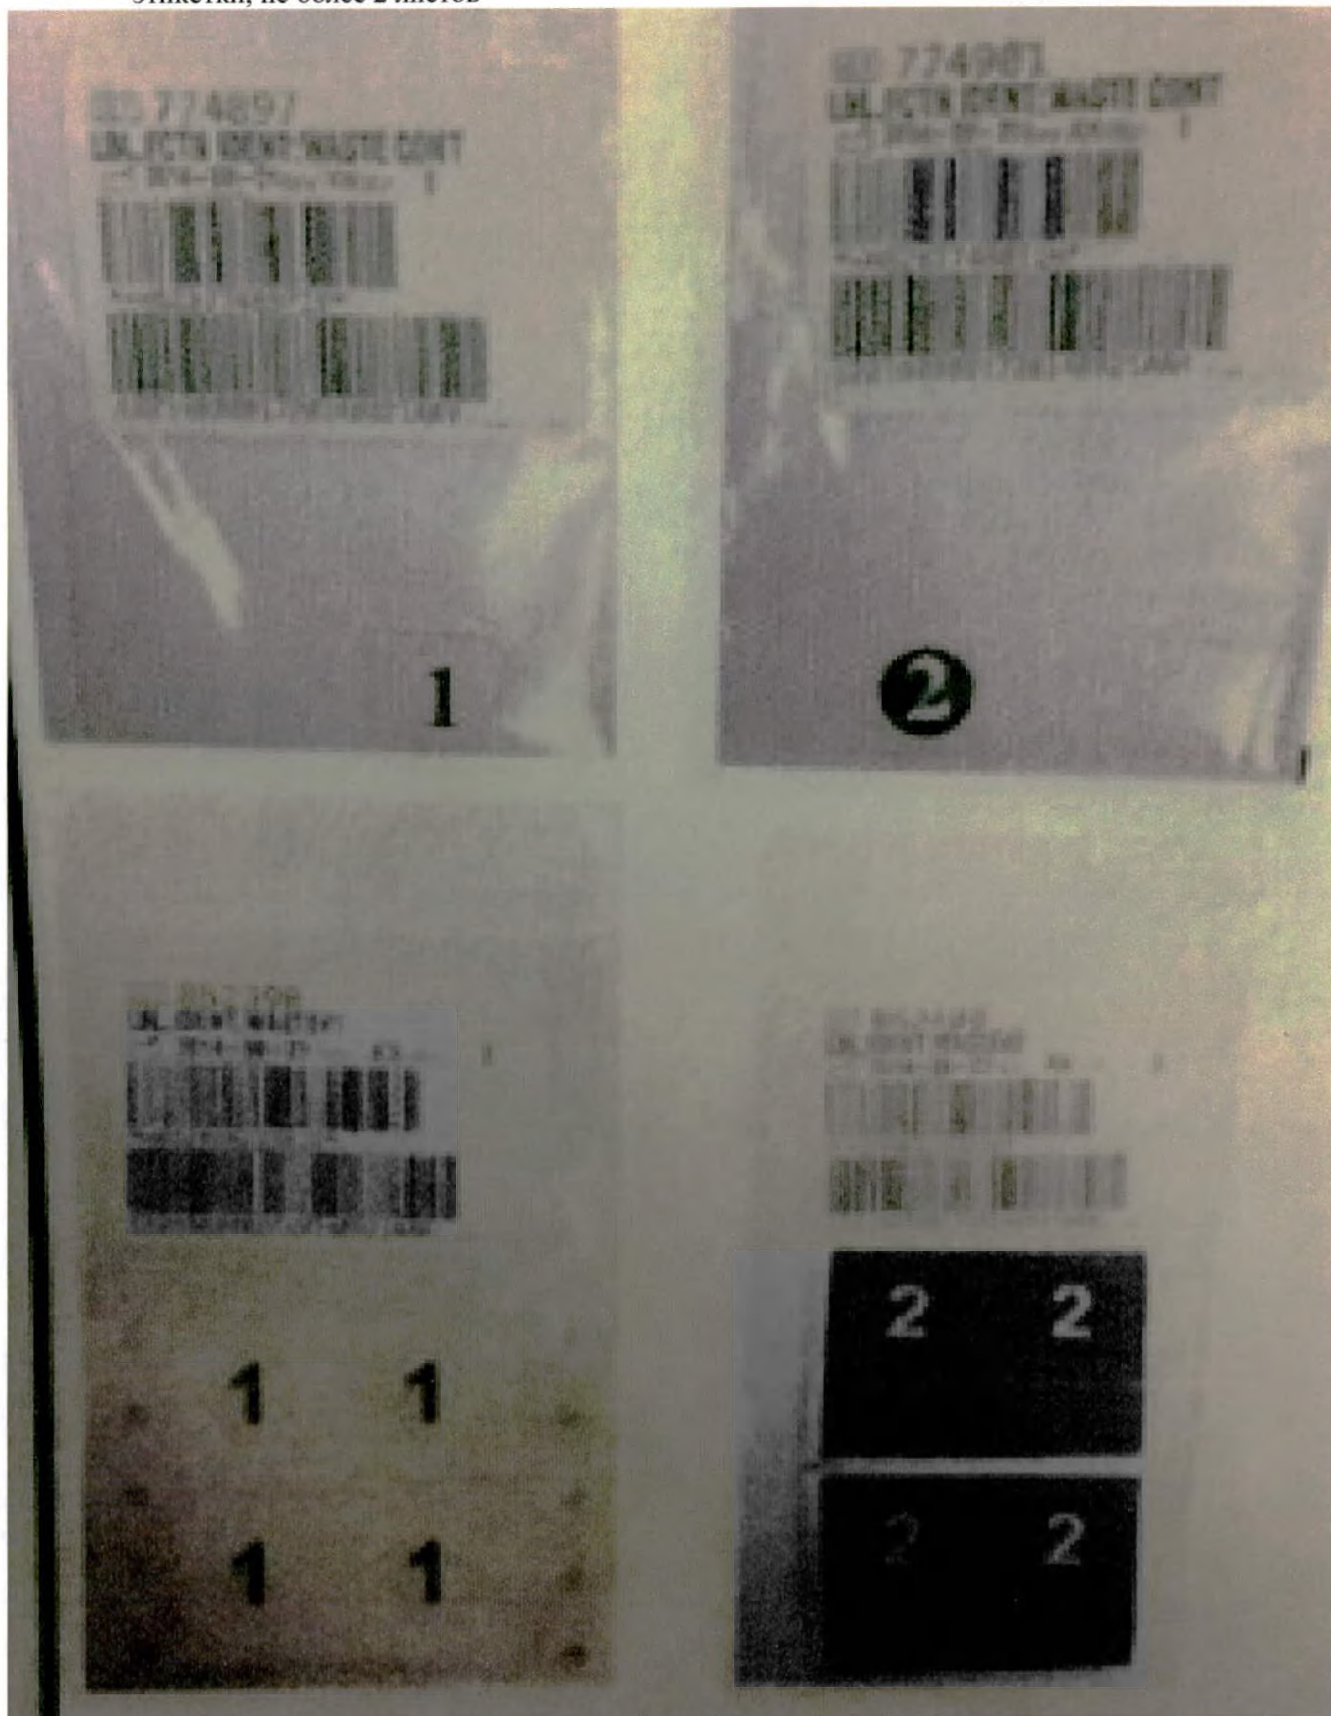

- ленты возвратные 2 шт. в комплекте с крепежными элементами 2 шт. и инструкцией – не более 10 шт.

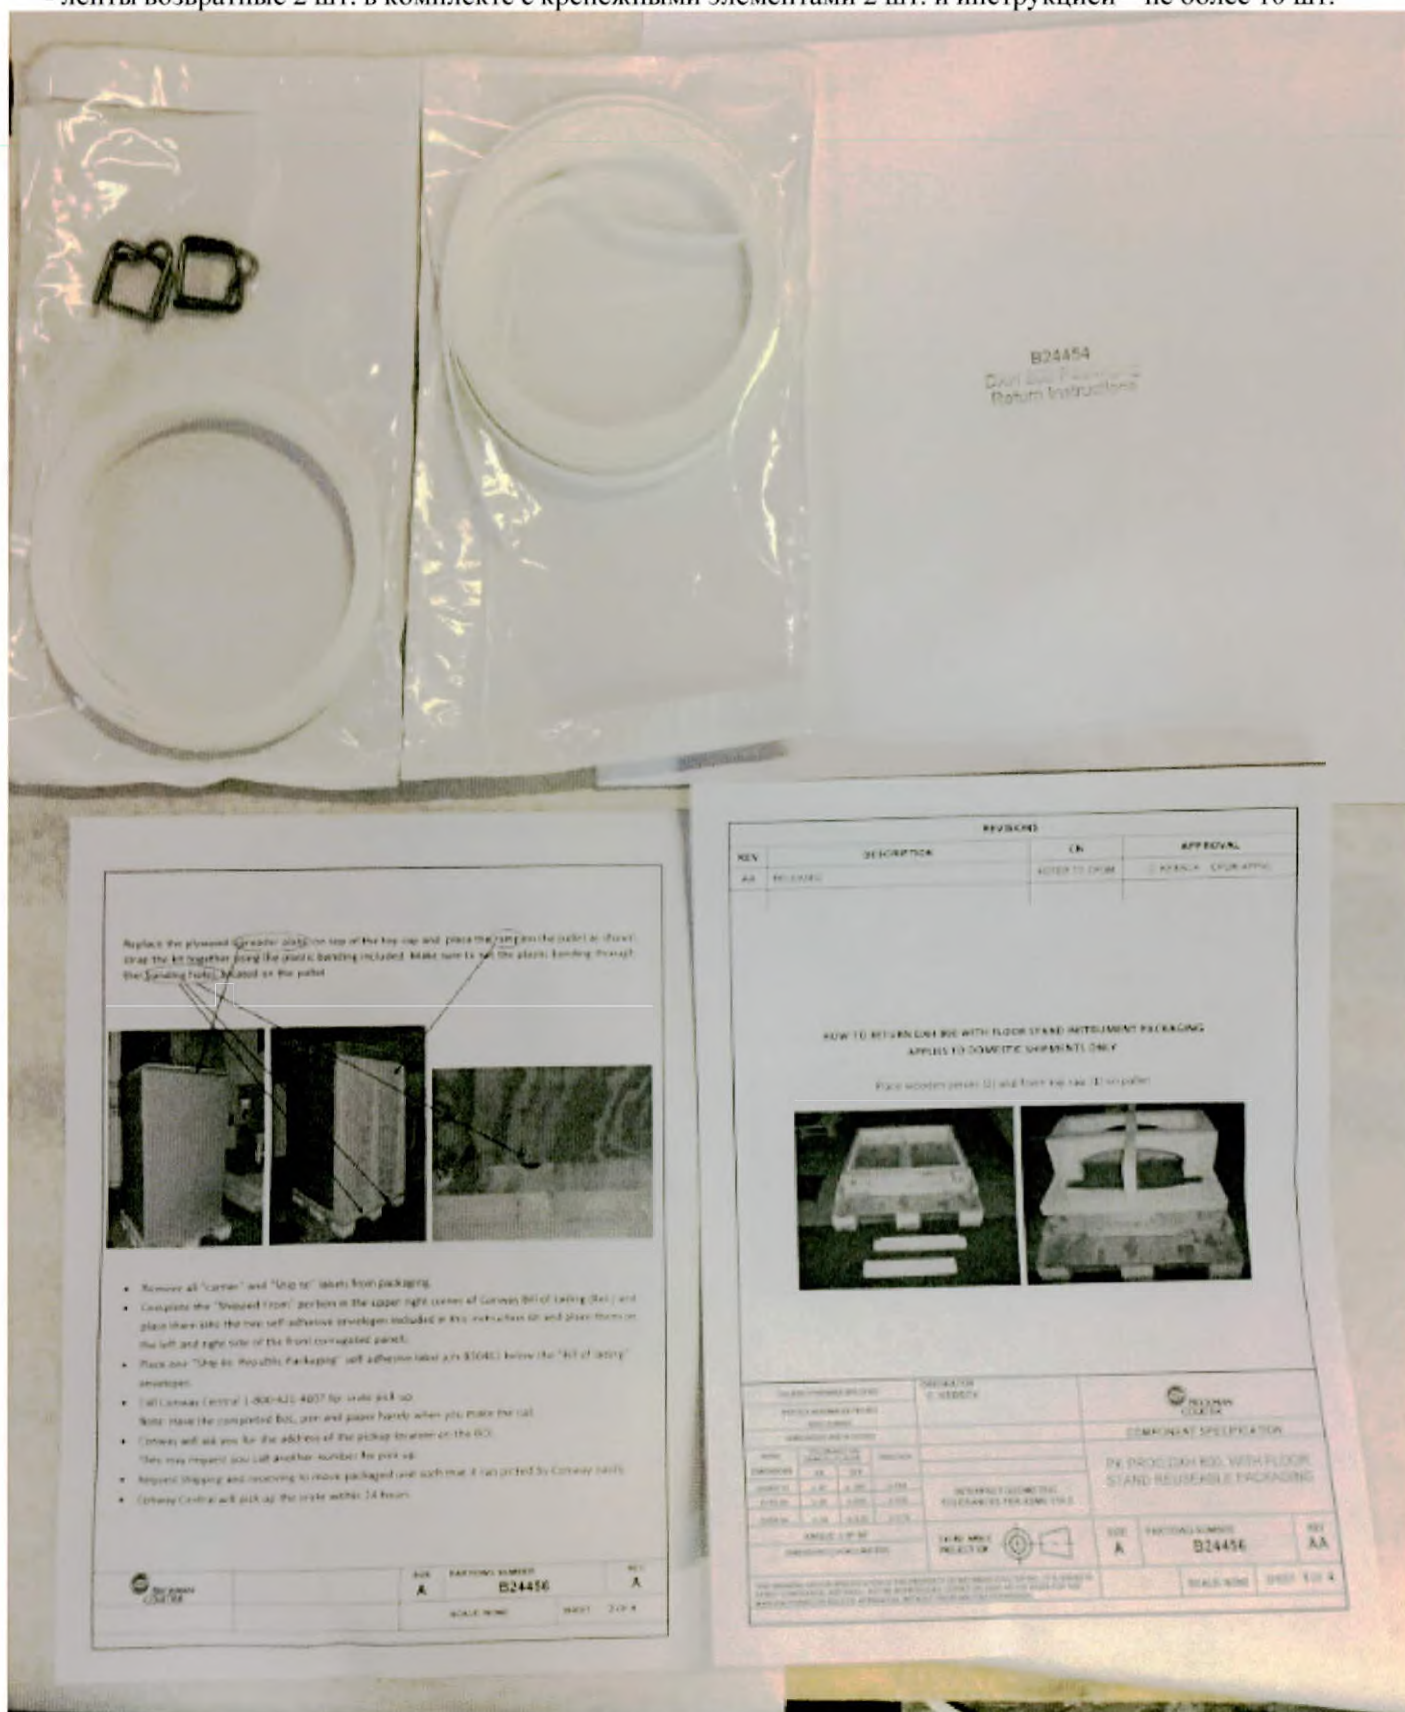

- Эксплуатационная документация – не более 5 шт..

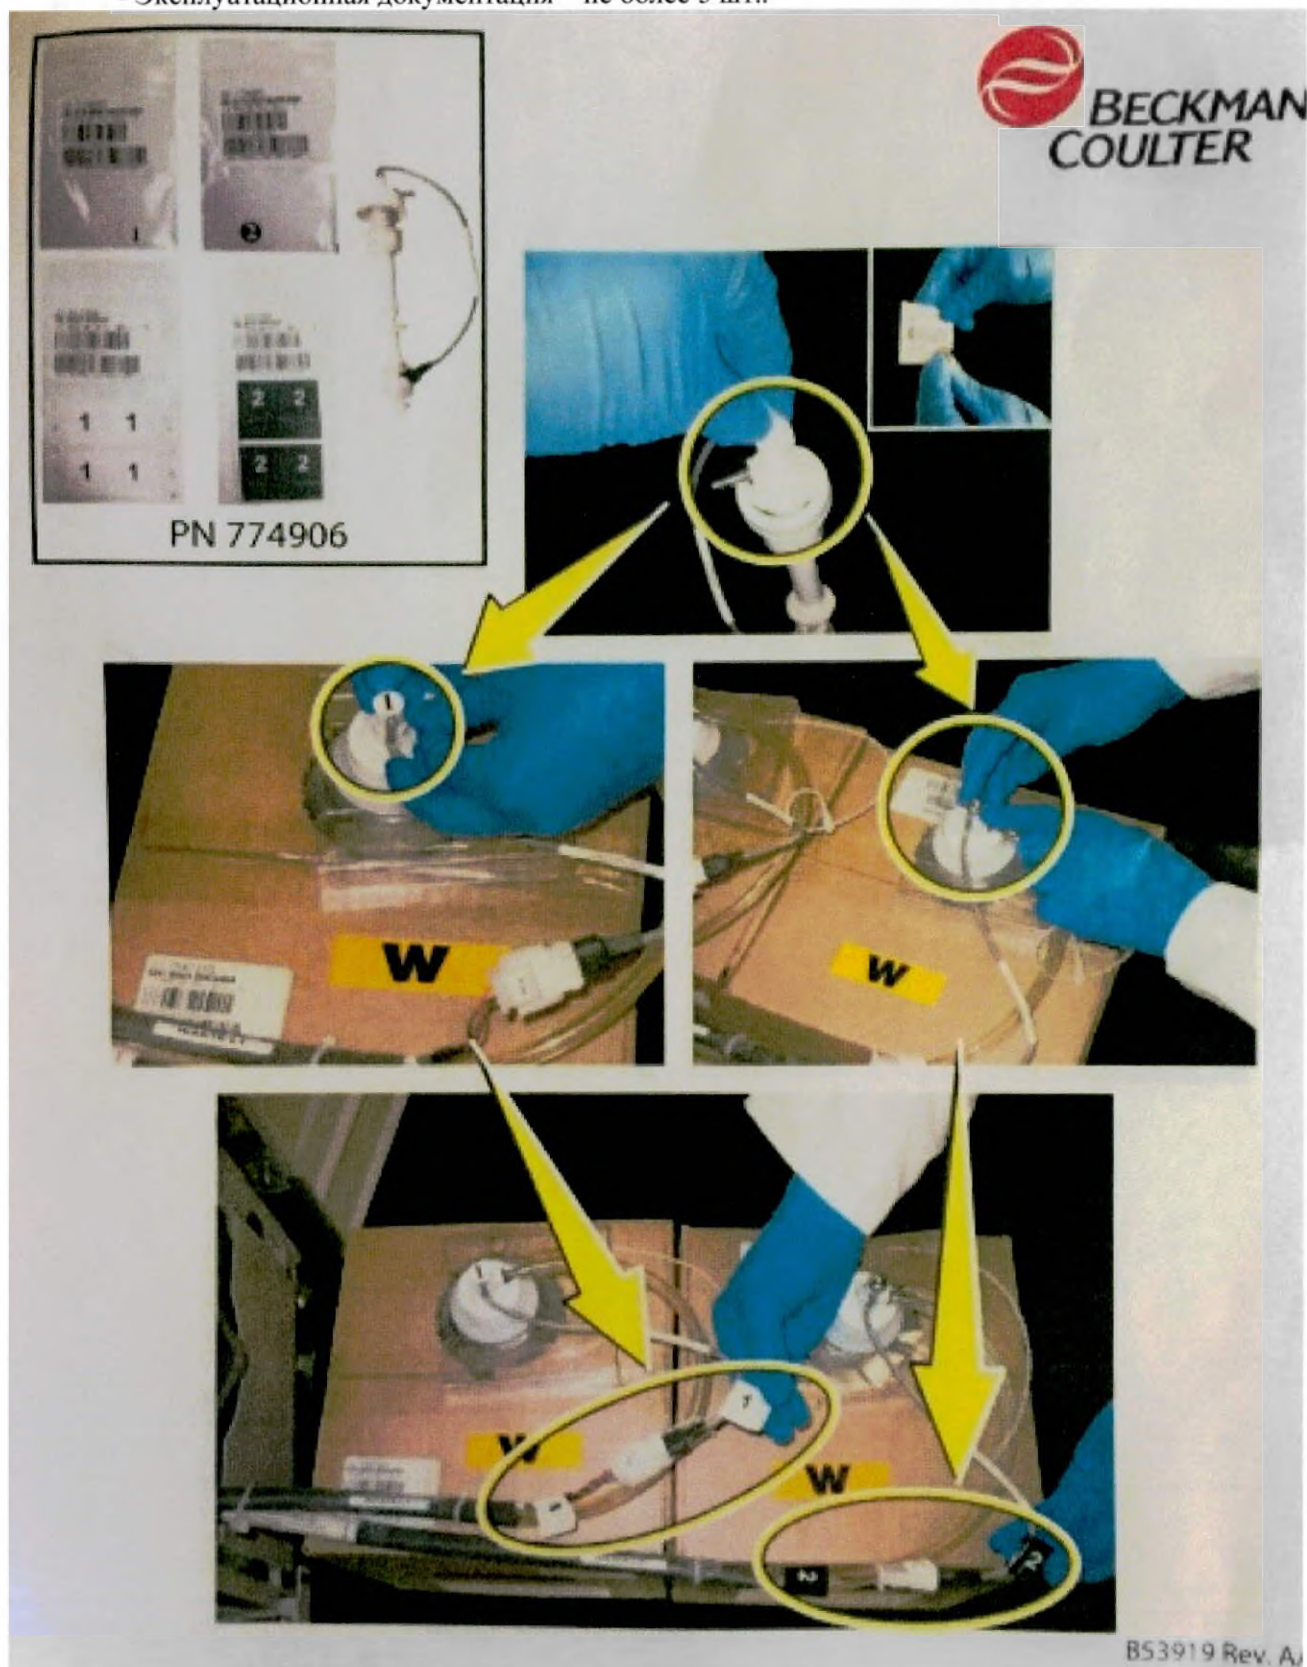

Фотография маркировки изделия на упаковке

PACKING SLIP
ENCLOSED IN
BOX NUMBER

Beckman Coulter, Inc.



REF C11477

Rx Only

TN,DXH SLIDEMAKER STAINER II
Serial No. BC24179



Beckman Coulter Inc.
250 S. Kraemer Blvd.
Brea, CA 92821 U.S.A.



2019-06-10

注意

运输/保存条件

温度: -10°C ~ 55°C

湿度: 30% ~ 95%

Made in USA of US and foreign components

177795-AF



Info for USA only: California Proposition 65

WARNING

Cancer & Reproductive Harm

www.P65Warnings.ca.gov



(01)15099590701567

(11)1190010

(21)BC24179

+H628C1147731

+BC2417910

Фотография маркировки изделия на обратной стороне



Макет маркировки изделия на русском языке



Регистрационное удостоверение:
РЗН XXXX/XXXXX от XX.XX.XXXX

Система для клеточного анализа UniCel DxH Coulter: устройство
подготовки и окрашивания препаратов DxH Slidemaker Stainer II (DxH
SMS II) с принадлежностями

DxH Slidemaker Stainer II (DxH SMS II)

Производитель:

Бекмен Култер, Инк. 250 S. Kraemer Blvd., Brea, CA 92821, США

Уполномоченный представитель производителя:

ООО "Бекмен Култер", Москва, Россия, 109004, Станиславского 21, стр.3

Кат. номер:

Серийный номер:

Дата производства:

Произведено в:

Дополнительная информация:

C11477

см. на оригинальной маркировке

см. на оригинальной маркировке

США

см. на оригинальной маркировке

Фотография упаковки изделия





ПРОШО, ПРОНУМЕРОВАНО
И СКРЕПЛЕНО ПЕЧАТЬЮ
63 ЛИСТОВ