

УТВЕРЖДАЮ

Генеральный директор
ООО «Компания «БиВи»

Т.А. Носова

29 августа 2023 г.





ПО ДОВЕРЕННОСТИ
77 АД 1754197
КУСАЙЛО Р. В.

Фотографические изображения изделия:

**Реагент лизирующий Z5 LB для анализатора автоматического гематологического
для диагностики in vitro (Lyse (Z5 LB))**

Zybio Inc. («Зибิโอ Инк.»), Китай

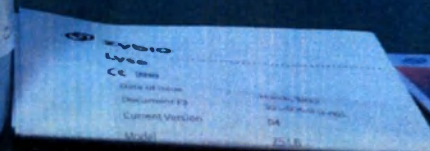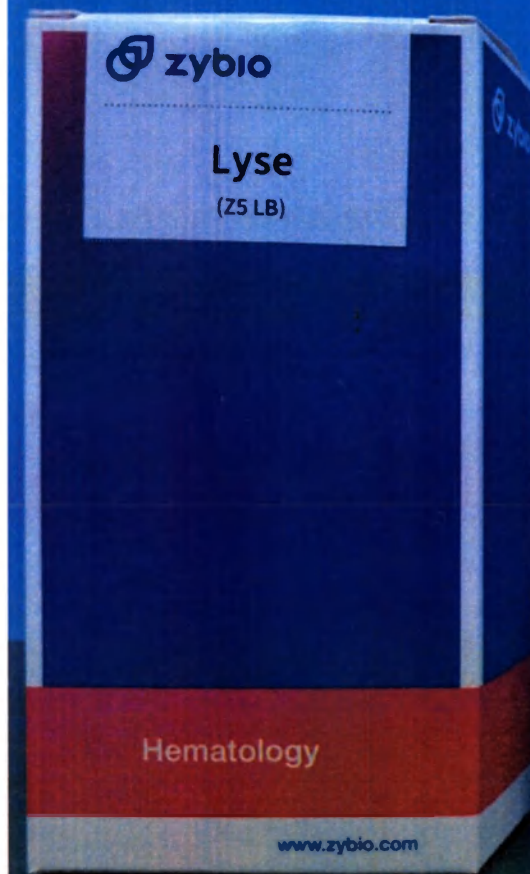

REF 01.09.31.05.Z5.05 LOT 230402

100mL × 1

 2023-04-11

 2025-04-10

Made in China



(01) 06973262865349

(11) 20230411

(17) 20250410

(10) 230402

(240) 01.09.31.05.Z5.05

(21) 2304020000001



30°C
4°C




GHS07




Zybio Inc.


Floor 1 to Floor 4, Building 30, No. 6 of Taikang Road, Block C of
Jianqiao Industrial Park, Dadukou District, 400082 Chongqing,
China

Lotus NL B.V.



Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague,
Netherlands.

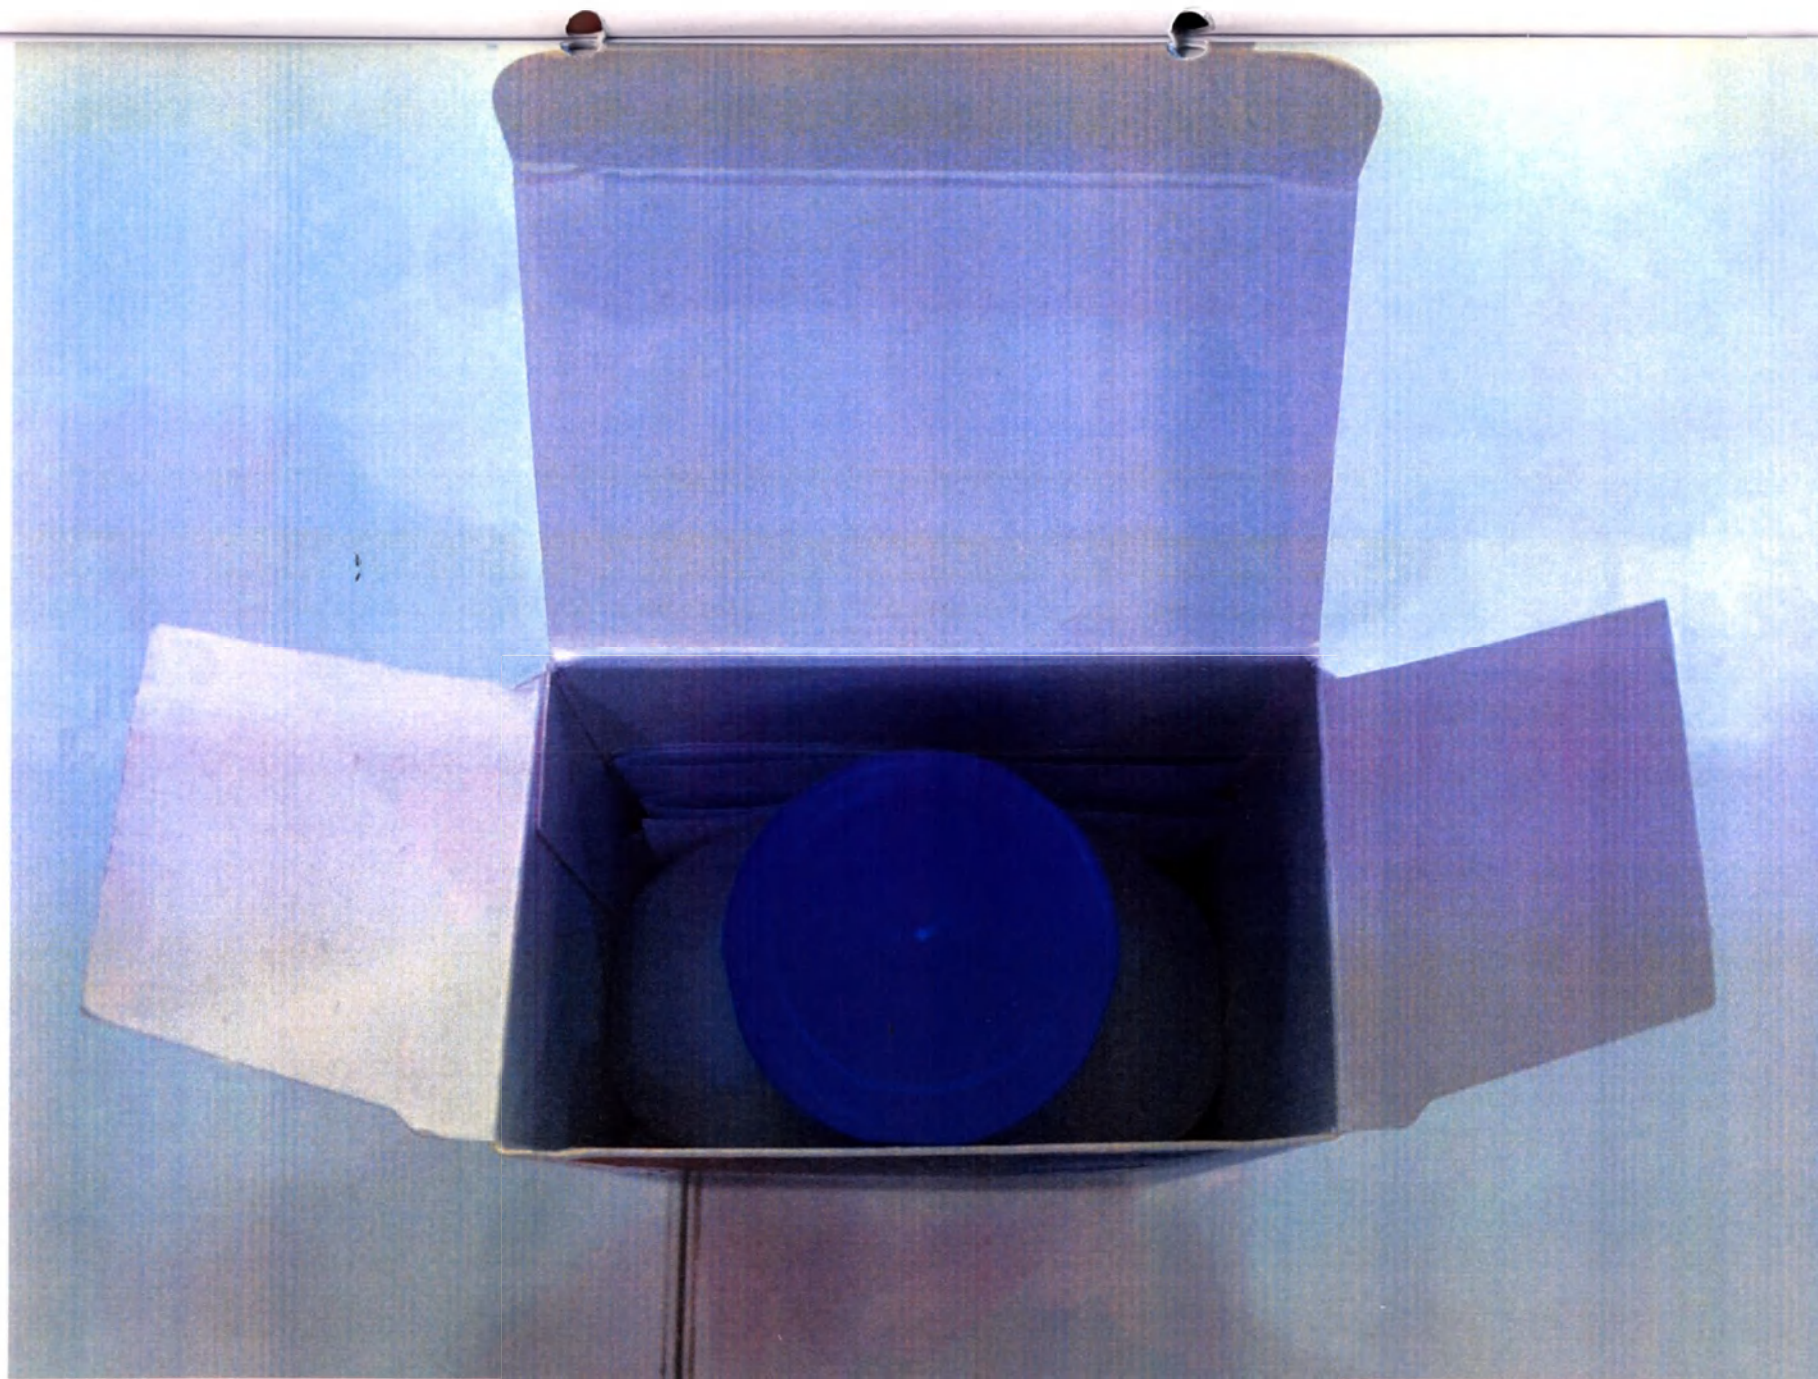

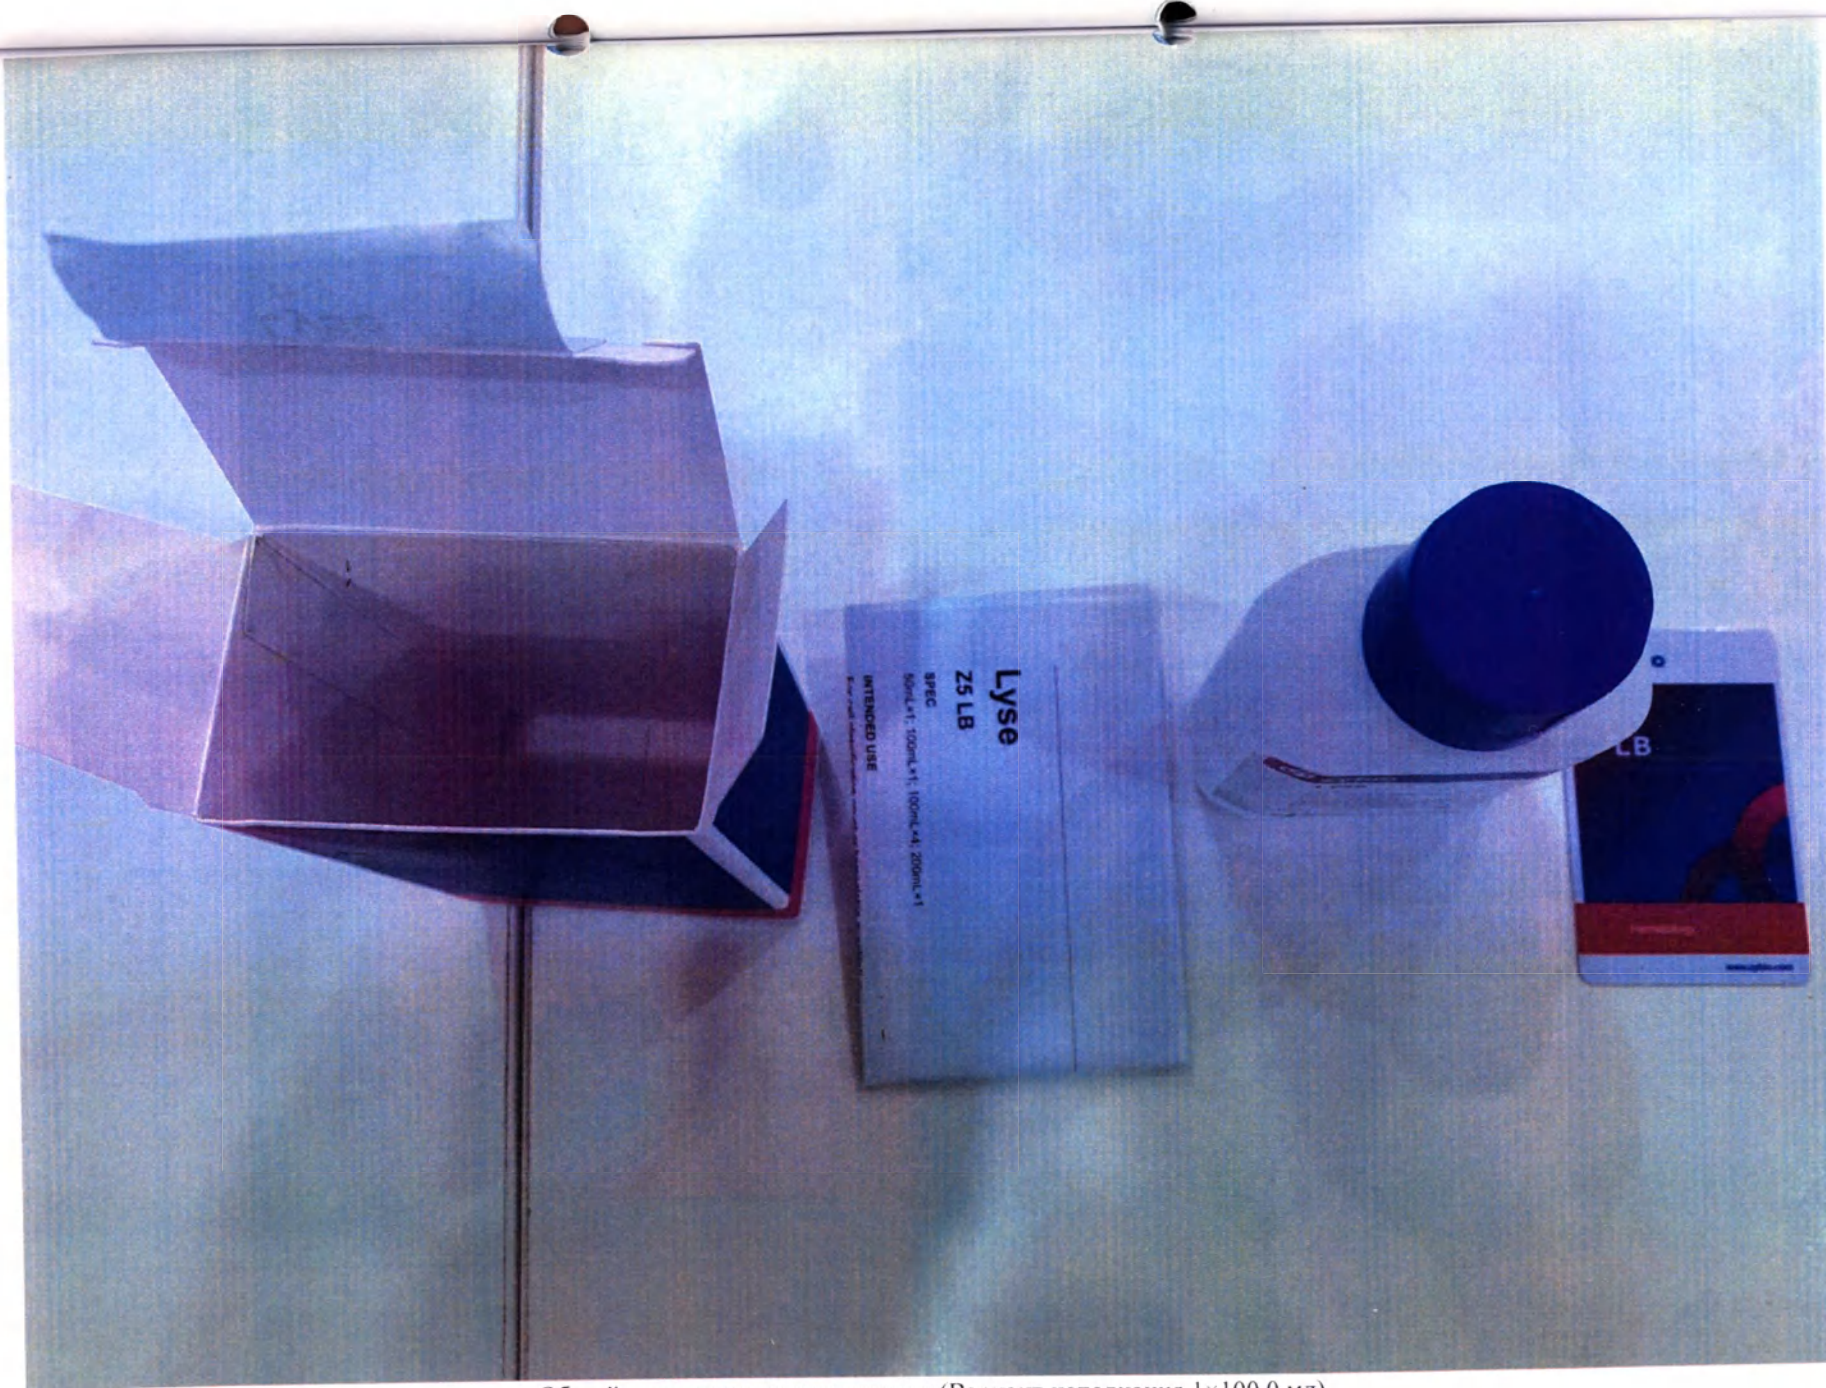

Общий вид медицинского изделия (Вариант исполнения 1×100,0 мл)



 **zybio**

Lyse

Z5 LB

Warnings and Precautions

1. For in vitro diagnostic use only. Do not ingest. Harmful if swallowed. Immediately with plenty of water and seek medical advice.
2. Considering volume proportion of reagents and samples a test should be appropriately increased or decreased according to varied conditions.
3. The waste liquid generated after reagent reaction and the unused reagent should be collected in a centralized manner and disposed of in accordance with relevant regulations.
4. Check before use, stop using if the flocculent sedimentation appears.
5. Don't expose without cover for a long time.
6. Any serious incident that has occurred in relation to the device should be reported to the competent authority of the Member State in which the user is located.


REF 01.09.31.05.Z5.05

LOT 230402






Реагент лизирующий Z5 LB (Вариант исполнения 1×100,0 мл)

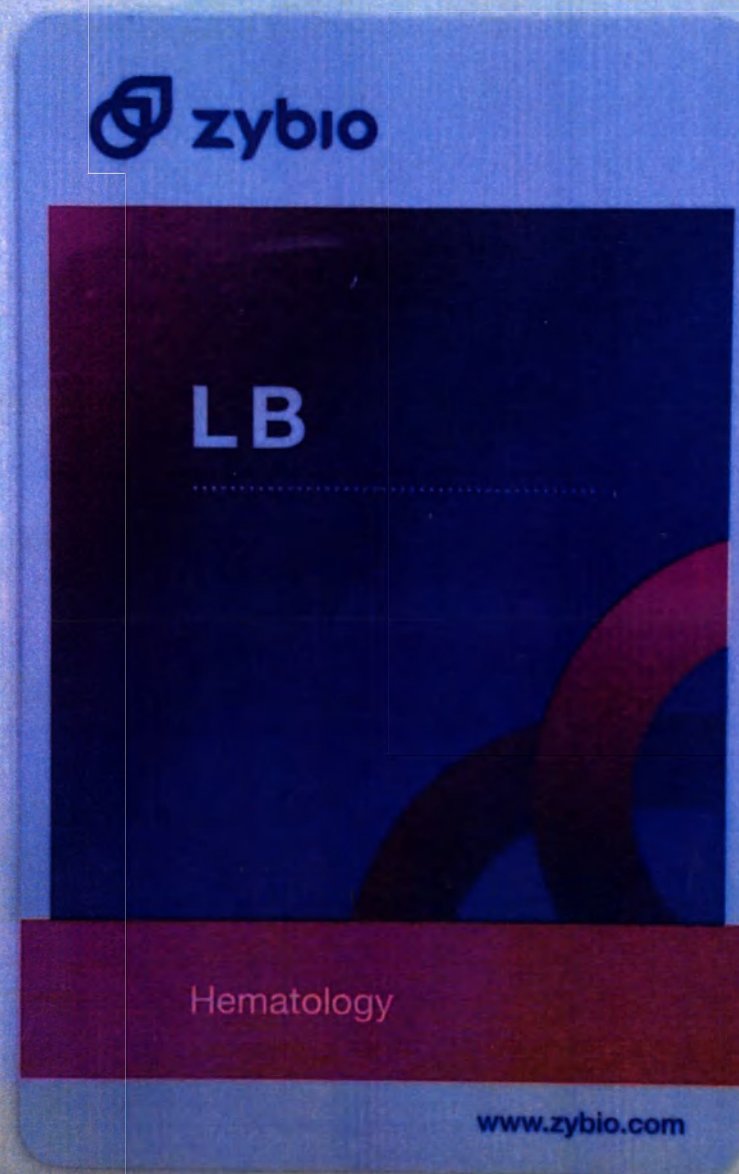

RFID-карта (Вариант исполнения 1×100,0 мл)

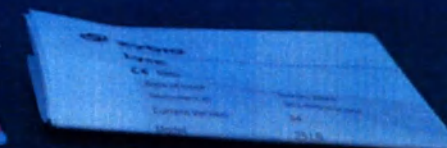

Lyse

(Z5 LB)

REF 01.09.31.05.Z5.36

LOT 230304

500mL×1

 2023-03-31

 2025-03-30



Made in China



(01) 06941967224365

(11) 20230331

(17) 20250330

(10) 230304

(240) 01.09.31.05.Z5.36

(21)2303040000001



IVD

30°C
4°C



GHS07

Zybio Inc.





Floor 1 to Floor 4, Building 30, No. 6 of Taikang Road, Block C of
Jianqiao Industrial Park, Dadukou District, 400082 Chongqing,
China

Lotus NL B.V.


EC REP

Koningin Julianaplein 10, 1e Verd, 2595AA, The Hague,
Netherlands.

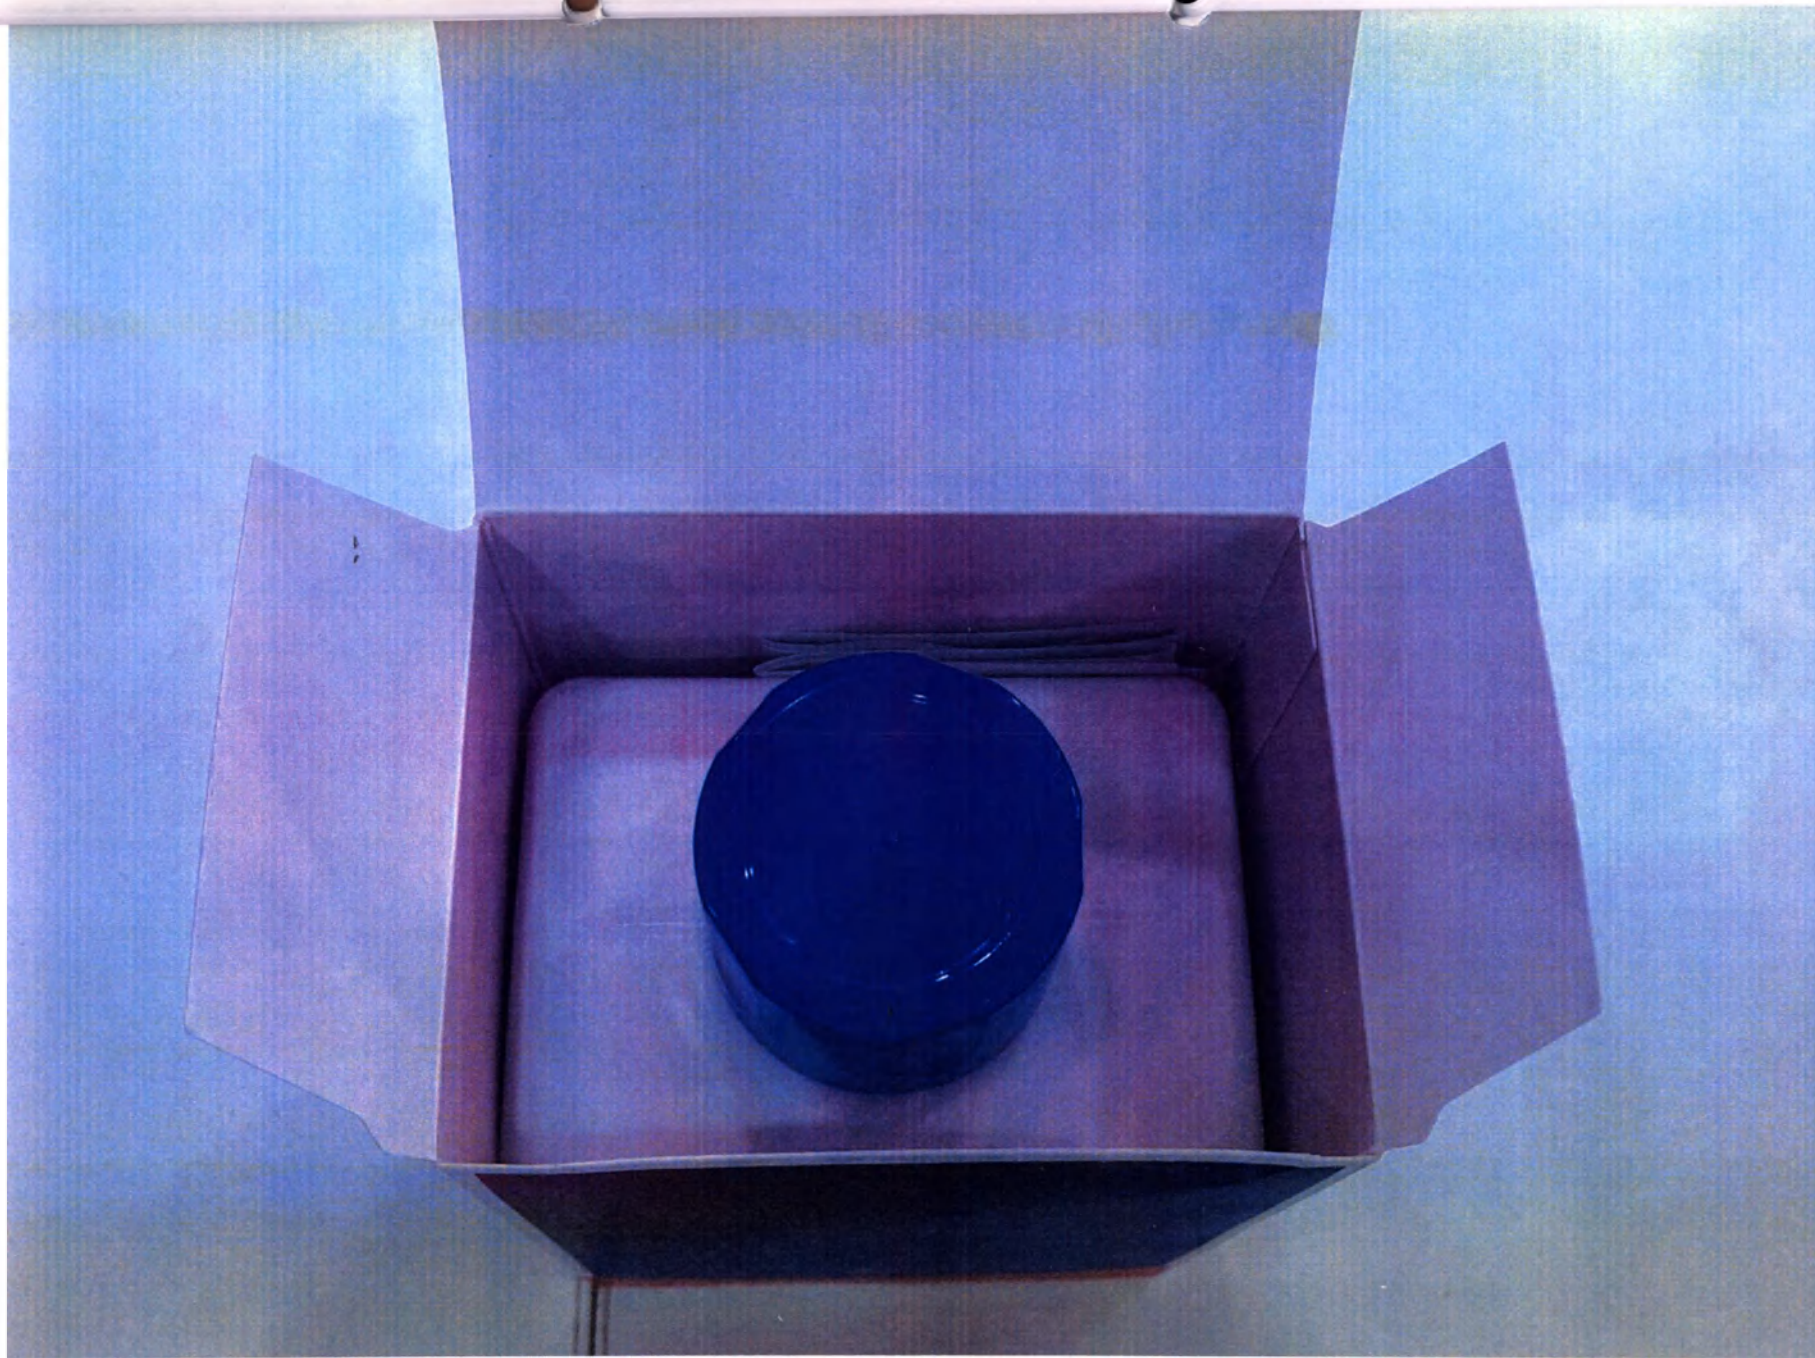

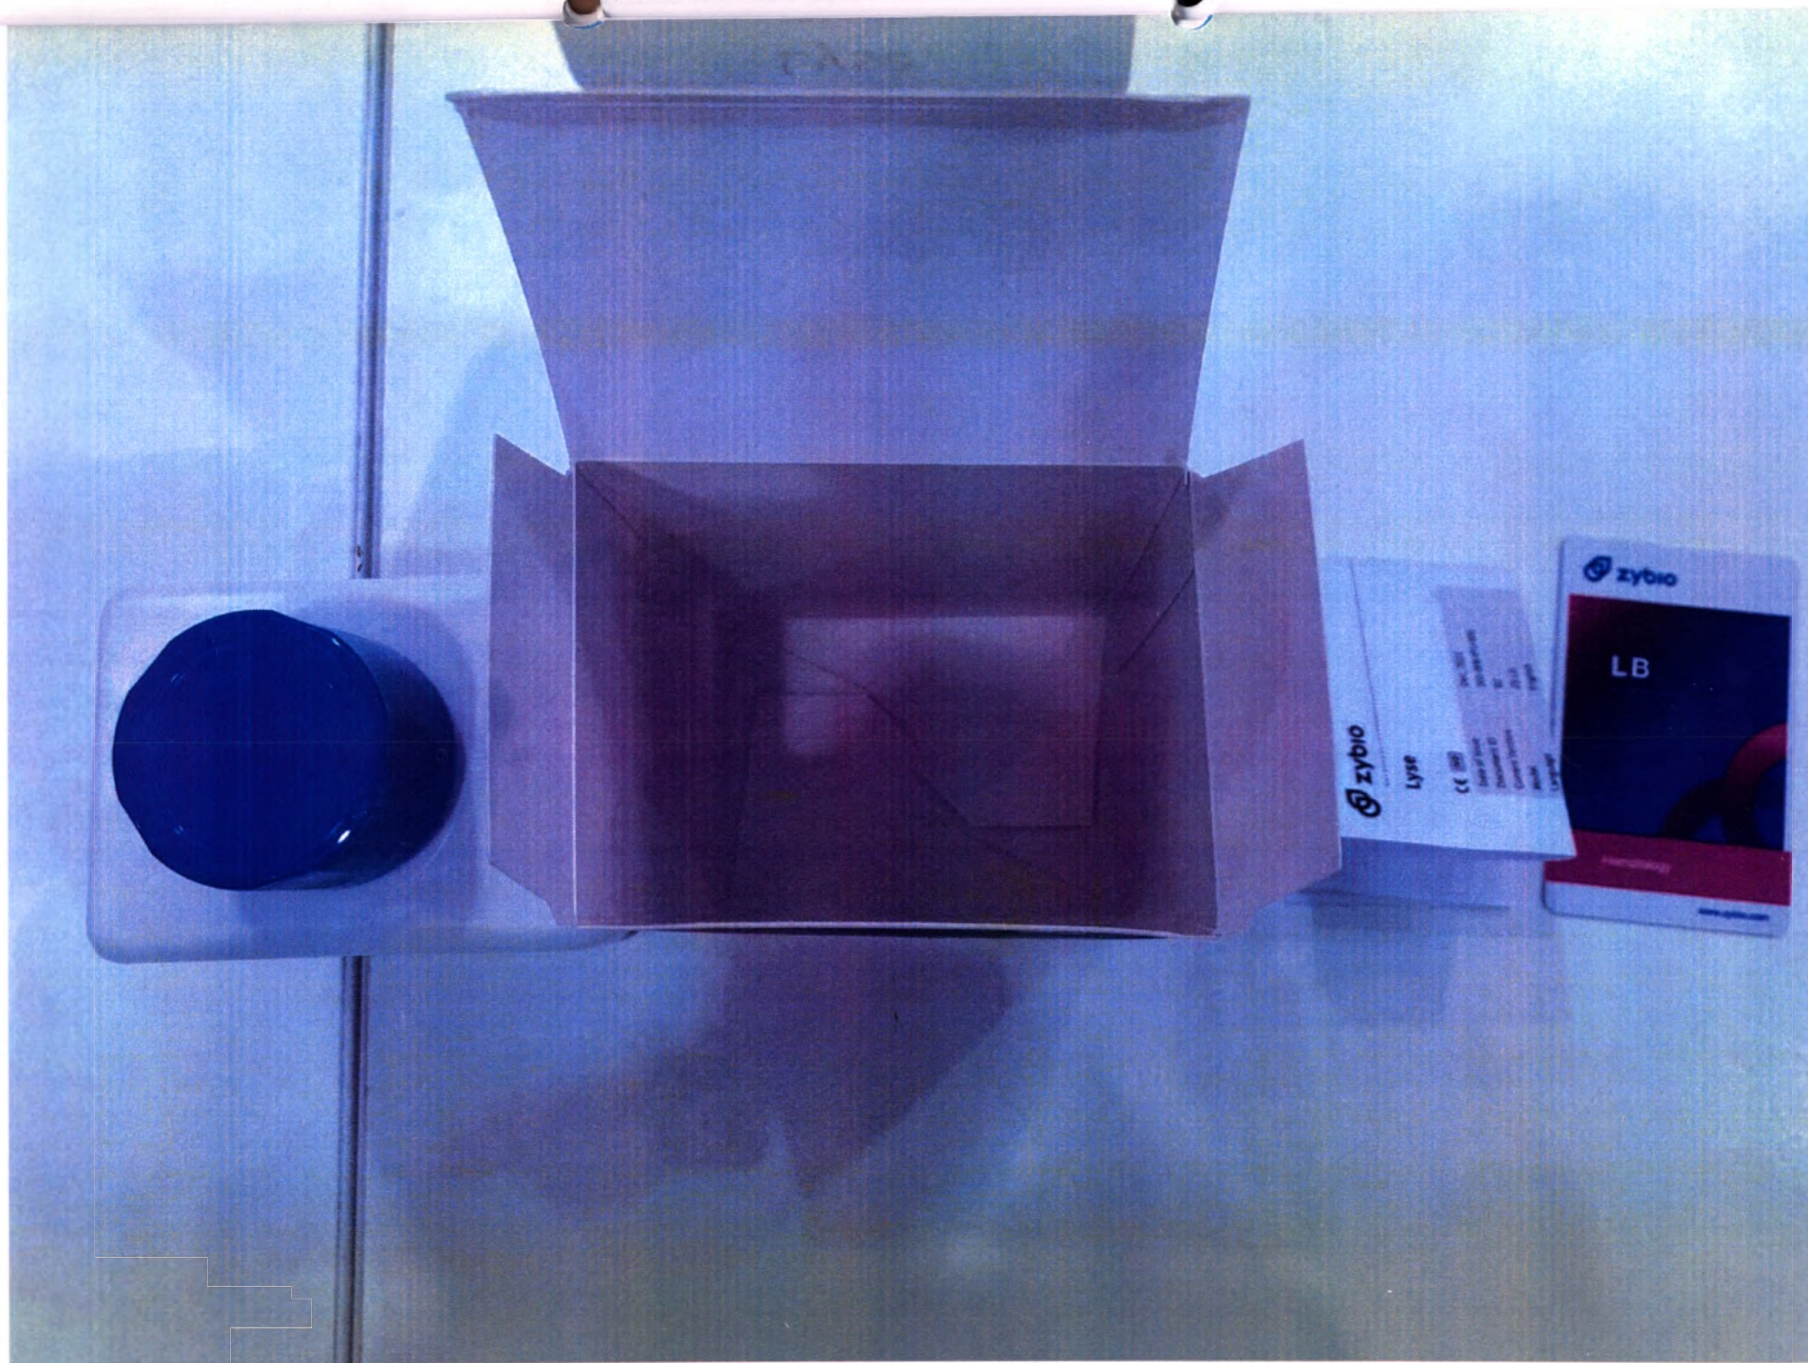

Общий вид медицинского изделия (Вариант исполнения 1×500,0 мл)



Lyse

Z5 LB



Warnings and Precautions

1. For in vitro diagnostic use only. Do not ingest. Harmful if swallowed. Rinse immediately with plenty of water and seek medical advice.
2. Considering volume proportion of reagents and samples is invariable, it is not necessary to increase or decrease according to varied instruments.
3. The waste liquid generated after reagent reaction and the used package should be collected in a centralized manner and disposed of in accordance with relevant regulations.
4. Check before use, stop using if the flocculent sedimentation, turbidity or other abnormal phenomena appear.
5. Don't expose without cover for a long time.
6. Any serious incident that has occurred in relation to the device should be reported to the competent authority of the Member State in which the user and operator are located.


REF 01.09.31.05.Z5.36

LOT 230304





Реагент лизирующий Z5 LB (Вариант исполнения 1×500,0 мл)

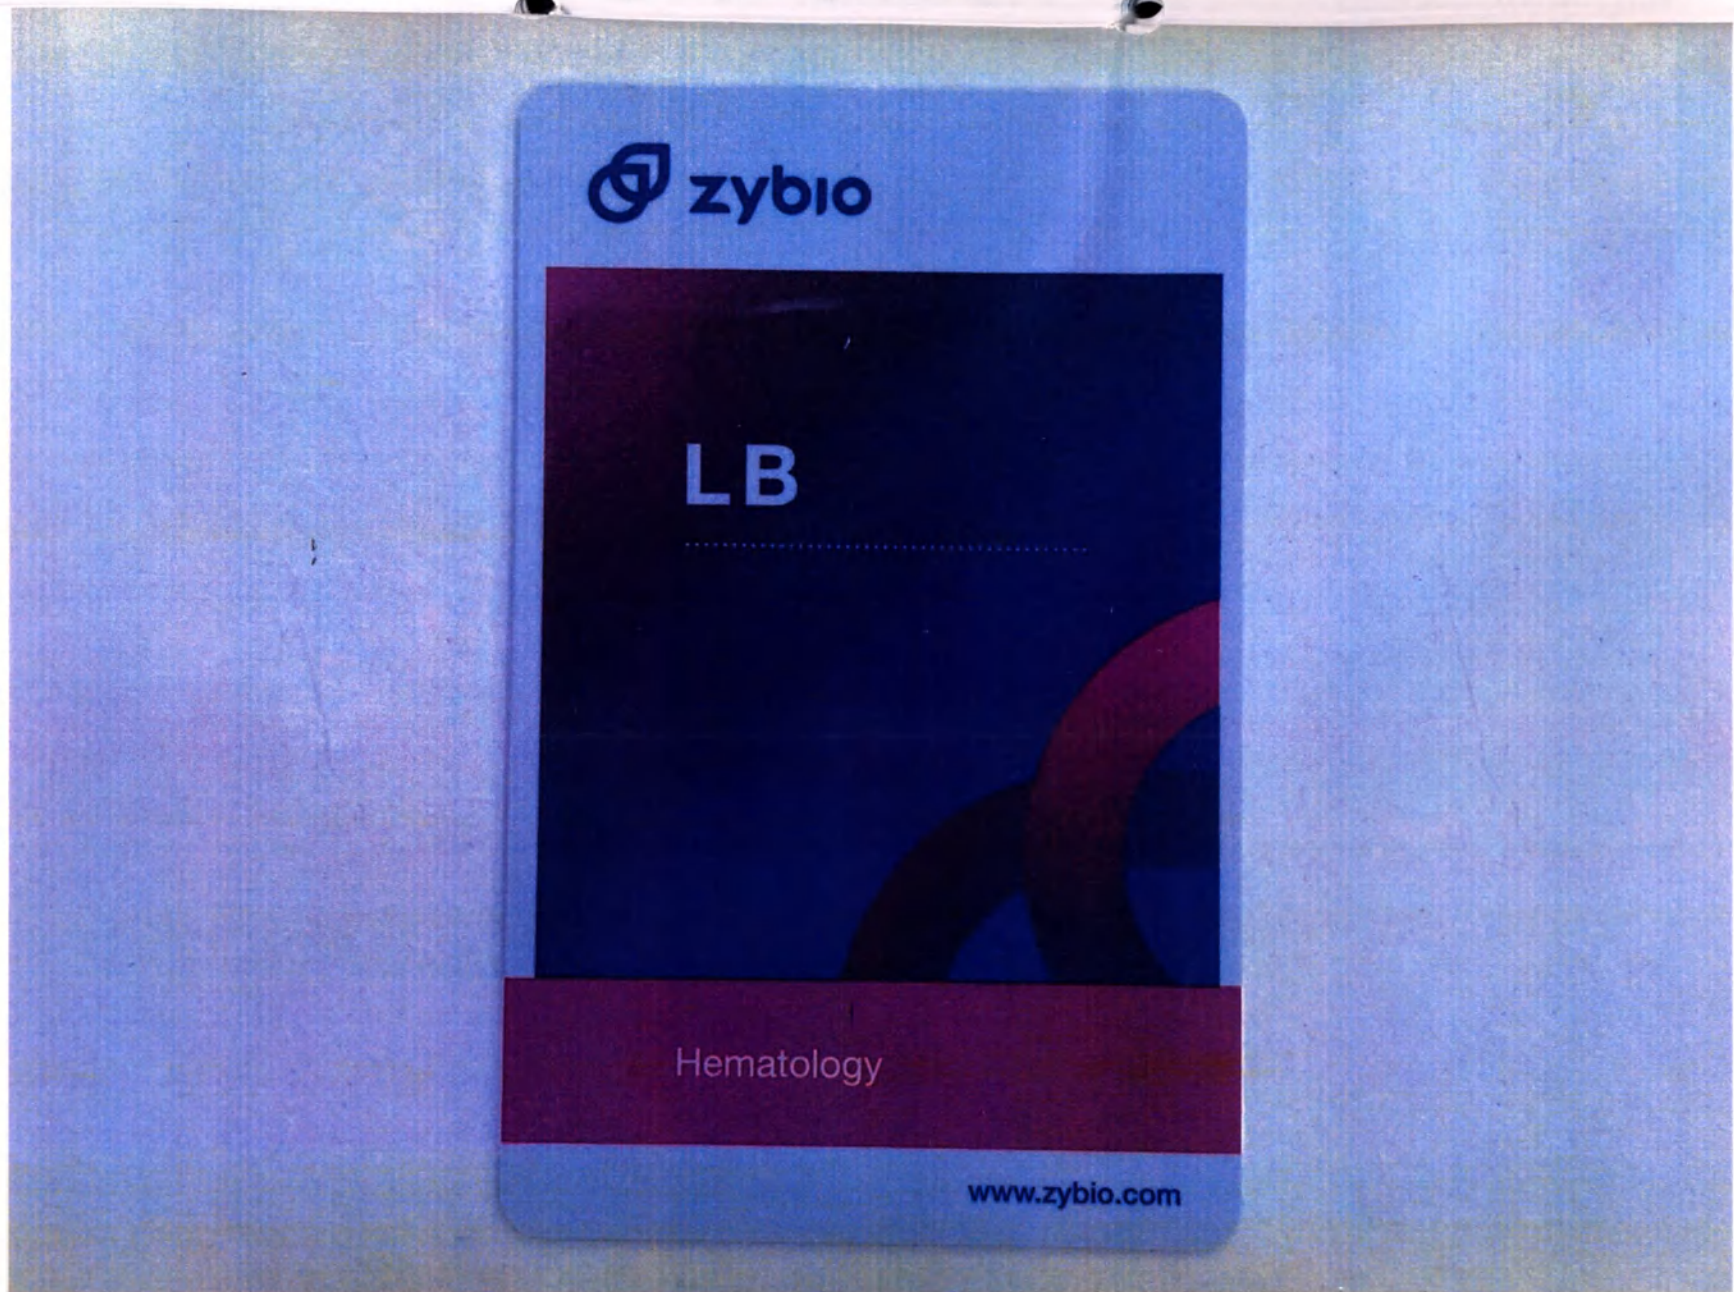

RFID-карта (Вариант исполнения 1×500,0 мл)

Всего прошито, пронумеровано и скреплено
печатью и подписью: 16 листа (-ов)

Генеральный директор _____ / Носова Т.А.
М.П.

