


ООО «Медтроник»
Башня на Набережной
ММДЦ «Москва-Сити»
Пресненская наб., д10, стр. С
123317, Москва, Россия

tel (+7 495) 580 73 77
fax (+7 495) 580 73 78
www.medtronic.ru


"УТВЕРЖДАЮ"

Генеральный директор
ООО «Медтроник»
Е. В. Плясунова
«1» ноября 2017 г.

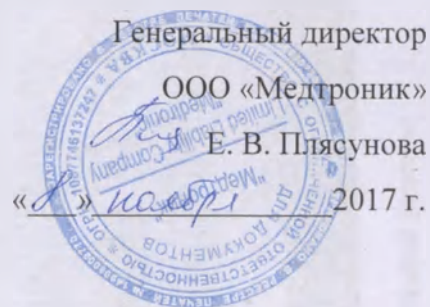





Фотографические изображения медицинского изделия

Микрокатетер, в различных вариантах исполнения Echelon, Rebar, Apollo,
Marathon, Orion 21



A	1.9 F .63 mm	B	150 cm
C	2.4 F .79 mm	D	.017 in .43 mm
E	3 cm	F	1.9 F .63 mm
G	.34 ml Dead Space Volume	H	.014" (.36mm) Max. Guidewire .063" (1.59mm) compatible Guiding Catheter I.D.


72-1562-814 Page 10/11



Microcatheter	Микрокатетер	Микрокатетер	МИКРО КАТЕТЕР
Mikrokatether	Mikrokatetri	Mikrocemik	마이크로 카테터
Mikrokateter	Mikrokateter	Mikro Kateter	
Micro Cateter	μικροκαθετήρας	Mikrokateter	ميكرو كاتيتير
Mikrokateter	Mikrokatetr	Mikrokateter	ميكرو كاتيتير
Mikrokatether	Mikrokateter	Mikrokateter	ميكرو كاتيتير

LOT A401198

CONTENTS



ev3 Echelon™-14, 45° Tip Shape [REF] 145-5092-150 [LOT] A4D1198
 3013006475385006270X17196512710104021198

ev3 Echelon™-14, 45° Tip Shape REF 145-5092-150 LOT A40119

 (01)J0847536006270(17)180117(10)A401190

ev3 Echelon™-14, 45° Tip Shape REF 145-5092-150 LOT A4011

Micro Catheter

Echelon™-14, 45° Tip Shape



A	1.9 F .63 mm	B	150 cm
C	2.4 F .79 mm	D	.017 in .43 mm
E	3 cm	F	1.9 F .63 mm
G	.34 ml	H	.014" L36mm, Max. Glycerine Dead Space Volume H ₂ O - 25mm ³ complete Guiding Catheter I.D.

REF 145-5092-150

LOT A401198

2019-01-17

CONTENTS



TIP
SHAPE 45°



Wort Technology, Inc.
8770 Lusk Way
Irvine, CA 92618 U.S.A.
Phone: +1 949 451 0700
Fax: +1 949 451 0701

Medtronic B.V.
Eurl. Medtronic B.V.
6422 PJ Heerlen
The Netherlands

Micro Catheter

Echelon™-14
1.9 F / 2.4 F

TIP SHAPE 45°

REF 145-5092-150

Usable Length
150 cm

LOT A401198

2019-01-17



Микрокатетер Echelon-14, форма наконечника 45° в лотке с крышкой



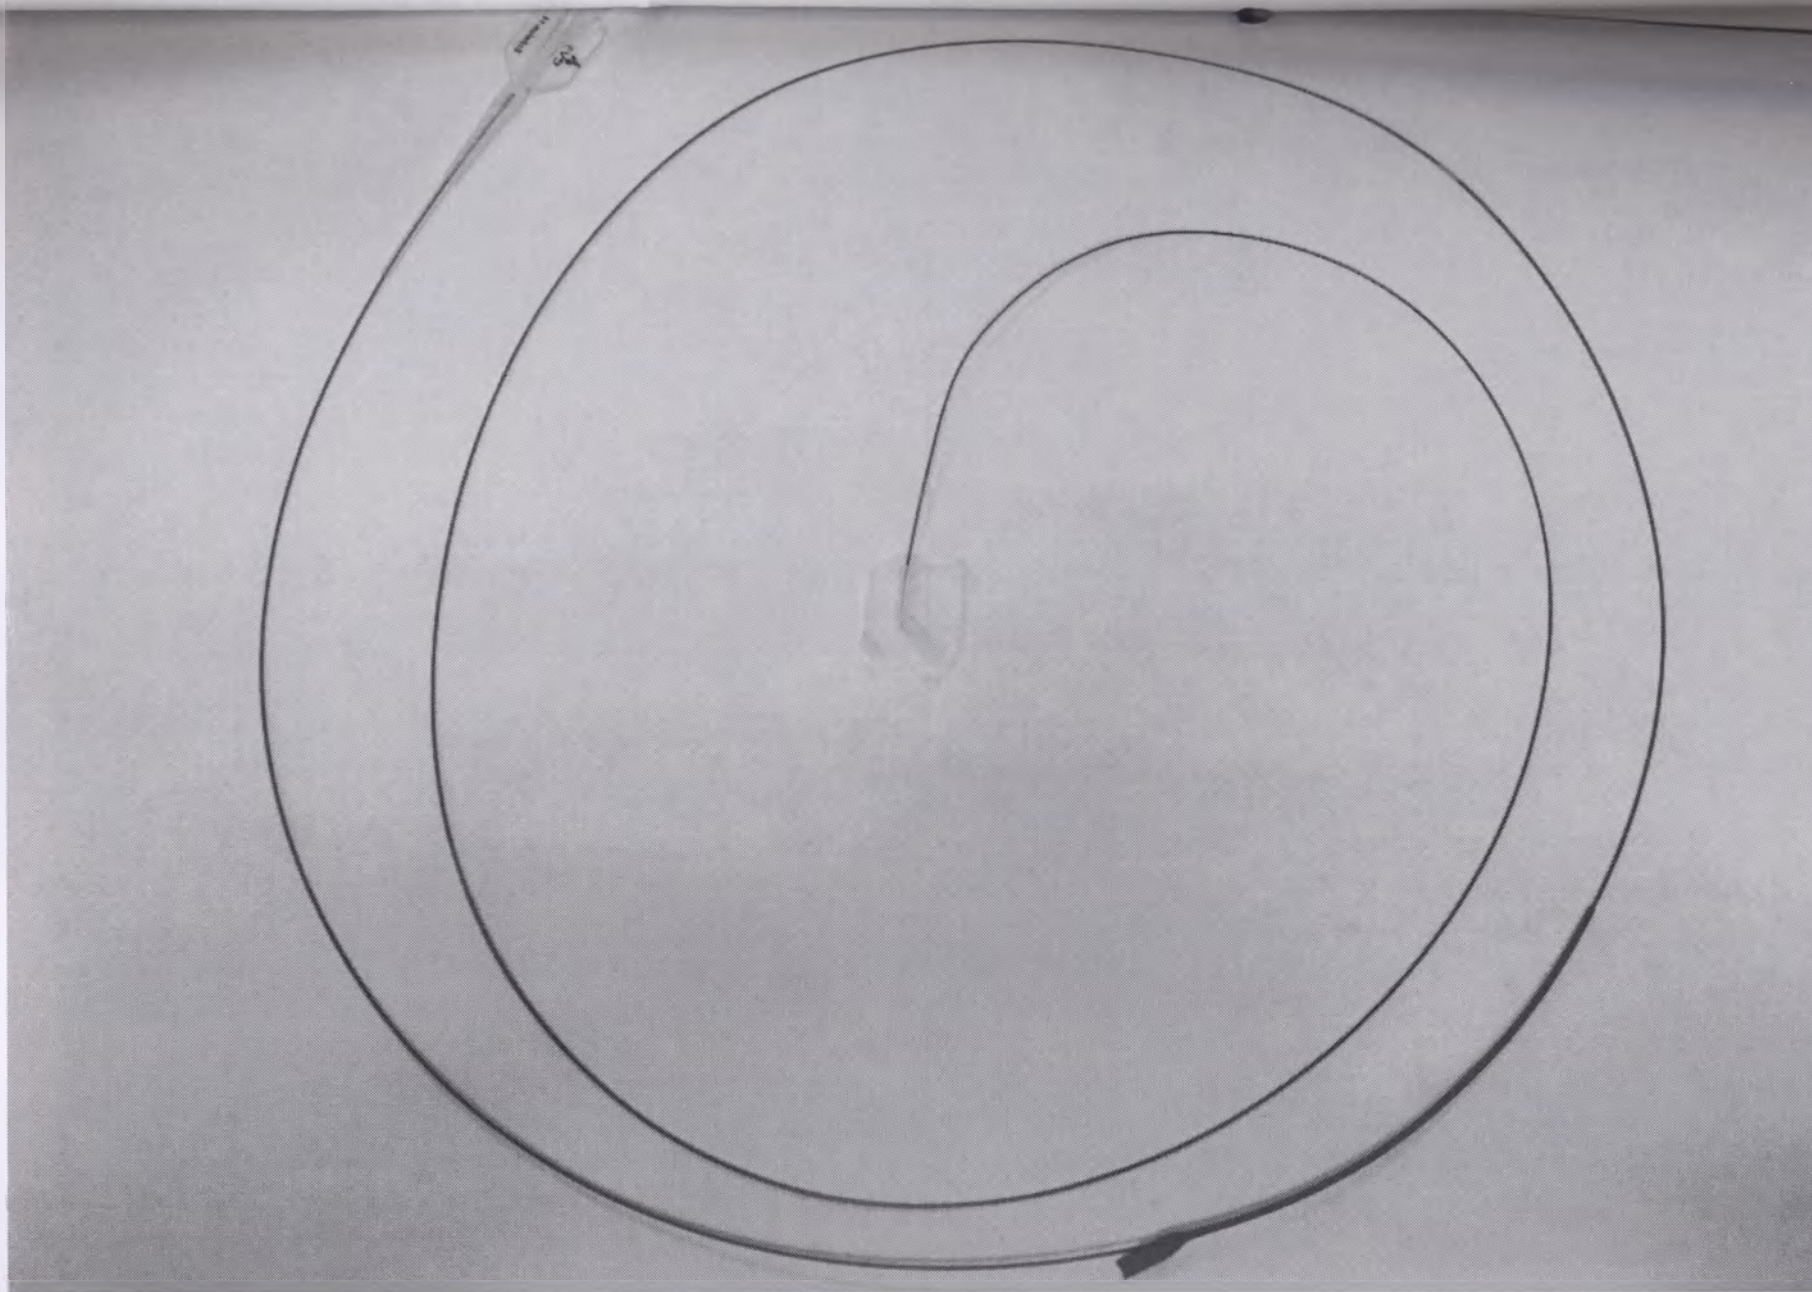


Фото Микрокатетера Echelon-14, форма наконечника 45°



Рабочая часть Микрокатетера Echelon-14, форма наконечника 45°

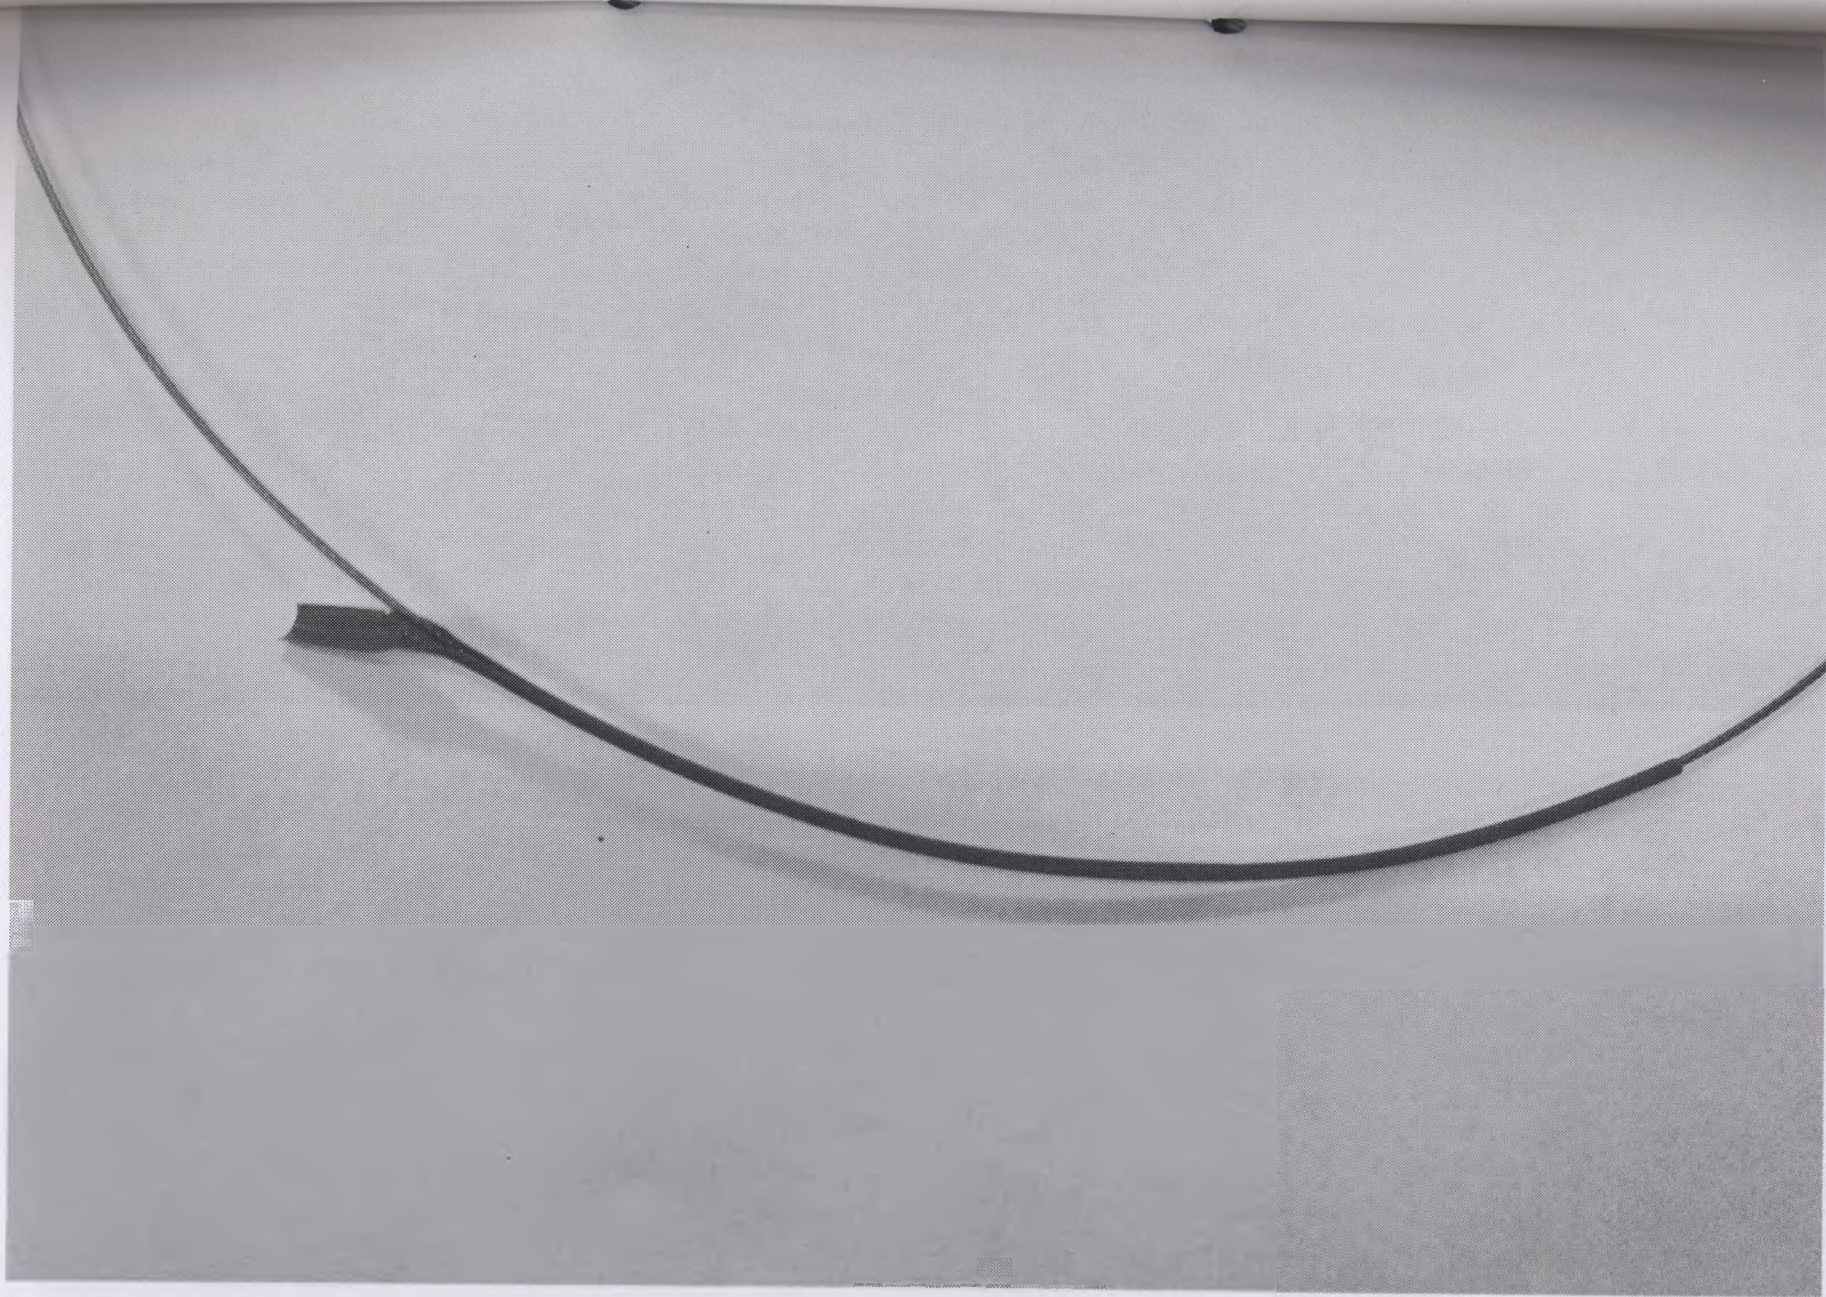

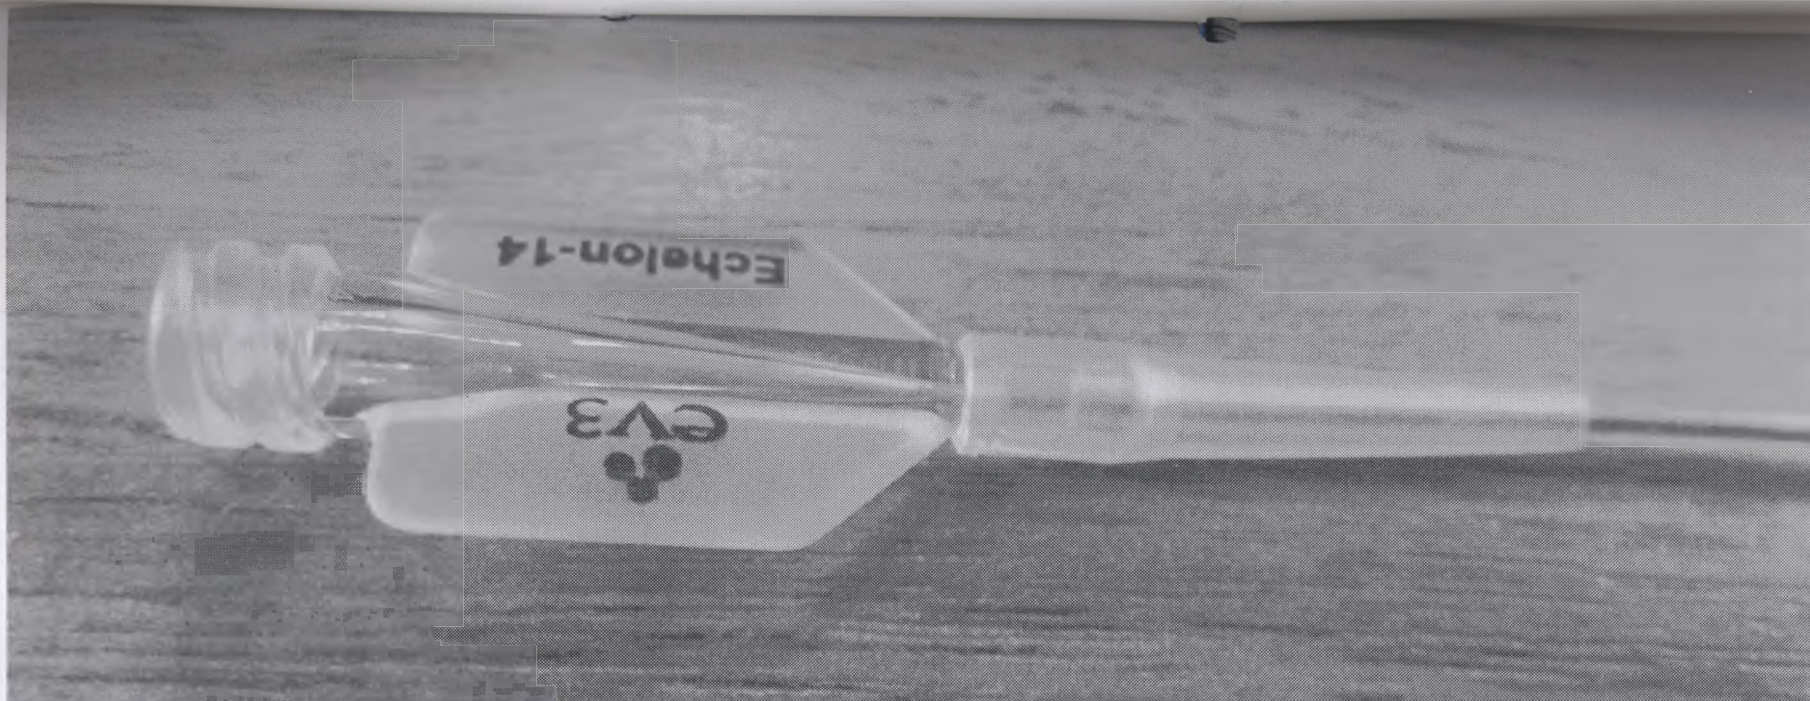

Втулка Микрокатетера Echelon-14, форма наконечника 45°

STEAM SHAPING MANDREL

INSTRUCTIONS FOR USE

In order to maintain catheter integrity and dimensional stability of the inner diameter, it is recommended that the user follow these instructions.


Warning! Shaping Mandrel is not intended for use in the human body.

Warning! Use only a steam source to shape the catheter tip. Do not use other heat sources.

Warning! Prior to use, inspect the catheter tip for any damage that may have resulted from shaping. Do not use a catheter that has been damaged in any way. Damaged catheters may rupture causing vessel trauma or tip detachment during steering maneuvers.

1. Remove shaping mandrel from card and insert into distal tip of the catheter.
2. Carefully bend catheter tip and shaping mandrel to desired shape. A slight over exaggeration of the shape may be required to accommodate for catheter relaxation.
3. Shape the catheter by holding the shaped portion approximately 1 inch (2.5 cm not less than 1 cm) from the steam source for about 20 seconds. (DO NOT EXCEED 30 SECONDS.)
4. Allow catheter tip to cool in air or saline prior to removing mandrel.
5. Remove mandrel from catheter and discard. Multiple shaping is not recommended.
6. Inspect the tip for any damage that may have resulted from steam shaping the catheter tip. If any damage is found, do not use the catheter.

30676 Rev. 07/07


EV3™

Мандрен с заостренным концом Микрокатетера Echelon



Syringe Adapter -
Echelon™ Micro Catheter

Adaptador
Adaptatore
Adaptateur
Adapter
Adapter

Adaptoru
Spraytheadapter
Łącznik
Adapter
Adapter

Adaptador
Προσφύλλο
注射器适配器
アダプター

REF 103-5095

LOT A310125

CONTENTS 1 X

2019-07-14

STERILE EO



Rx
ONLY



0297


Catheter	Minimum Dead Space	
	Catheter	Catheter + Adapter
Echelon 10/14	.34	.27

Micro Therapeutics, Inc.
d/b/a ev3 Neurovascular
9775 Toledo Way
Irvine, CA 92618 U.S.A.
Phone: +1-949-837-3700
Fax: +1-800-837-9775


EC REP

Medtronic B.V.
Eart Bakkenstraat 10
6422 PJ Heerlen
The Netherlands

20093-001 Rev. 08/13



Стерильная упаковка адаптера для шприца к микрокатетеру Echelon

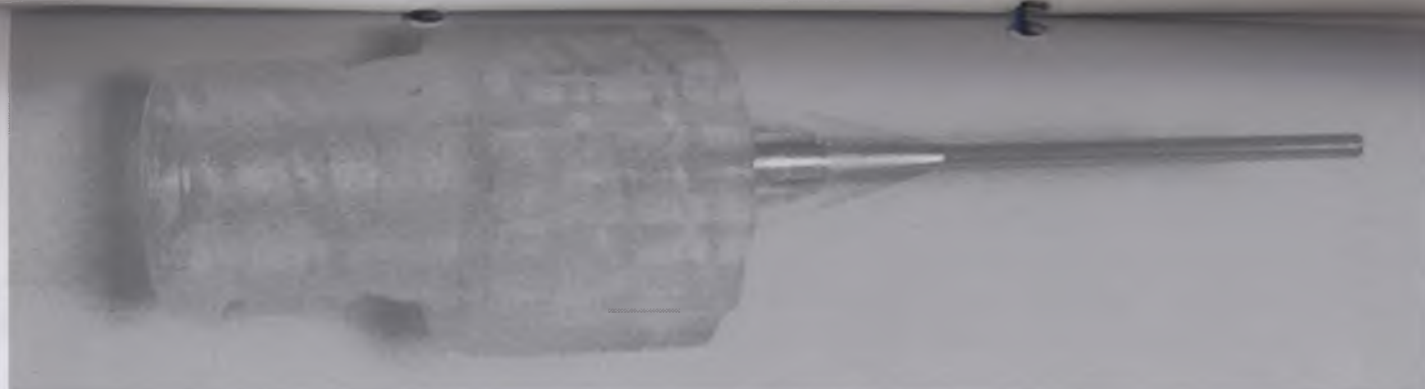

Адаптер к микрокатетеру Echelon



YOUR ENDOVASCULAR COMPANY

Micro Catheter




Rebar™-18 Micro Catheter

Microcatheter Microcatheter Микрокатетер 마이크로카테터
Mikrokatheter Mikrokatheter 마이크로카테터 마이크로카테터
Microcatheter Microcatheter Микрокатетер 마이크로카테터
Microcatheter Microcatheter Микрокатетер 마이크로카테터
Microcatheter Microcatheter Микрокатетер 마이크로카테터



A	2.4 F .81 mm	B	153 cm
C	2.7 F .91 mm	D	.021 in .53 mm
E	3 cm	F	2.4 F .81 mm
G	.49 ml Dead Space Volume	H	.018" (.46mm) Max. Guidewire .044" (1.13mm) compatible Guiding Catheter I.D.

REF 105-5081-153	LOT A418189
2019-02-21	CONTENTS 1X 1X



[illegible]

A	2.4 F .81 mm	B	153 cm
C	2.7 F .91 mm	D	.021 in .53 mm
E	3 cm	F	2.4 F .81 mm
G	.49 ml Dead Space Volume	H	.018" (.46mm) Max. Guidewire .044" (1.13mm) compatible Guiding Catheter I.D.

[illegible]

1992 ASME
 3120 14th Street, N.W.
 Washington, D.C. 20004-6145
 Tel: 202/295-6241
 Fax: 202/295-6242

Address: D.V.
 1000 University St.
 1000 University St.
 1000 University St.

Micro Catheter


Rebar™-18
24 F / 27 F

REF 105-5081-153

LOT A418189

2019-02-21

CONTENTS



ev3

ev3

Radax™ 18 **888** 185-6081-1352 **507** A418181

REF	Usable Length	LOT	A418189
105-5081-153	153 cm		2019-02-21

Микрокатетер Rebar -18, длина 130 см, в стерильной упаковке

STEAM SHAPING MANDREL

INSTRUCTIONS FOR USE

In order to maintain catheter integrity and dimensional stability of the inner diameter, it is recommended that the user follow these instructions.


Warning! Shaping Mandrel is not intended for use in the human body.

Warning! Use only a steam source to shape the catheter tip. Do not use other heat sources.

Warning! Prior to use, inspect the catheter tip for any damage that may have resulted from shaping. Do not use a catheter that has been damaged in any way. Damaged catheters may rupture causing vessel trauma or tip detachment during steering maneuvers.

1. Remove shaping mandrel from card and insert into distal tip of the catheter.
2. Carefully bend catheter tip and shaping mandrel to desired shape. A slight over exaggeration of the shape may be required to accommodate for catheter relaxation.
3. Shape the catheter by holding the shaped portion approximately 1 inch (2.5 cm not less than 1 cm) from the steam source for about 20 seconds. (DO NOT EXCEED 30 SECONDS.)
4. Allow catheter tip to cool in air or saline prior to removing mandrel.
5. Remove mandrel from catheter and discard. Multiple shaping is not recommended.
6. Inspect the tip for any damage that may have resulted from steam shaping the catheter tip. If any damage is found, do not use the catheter.

ev3™

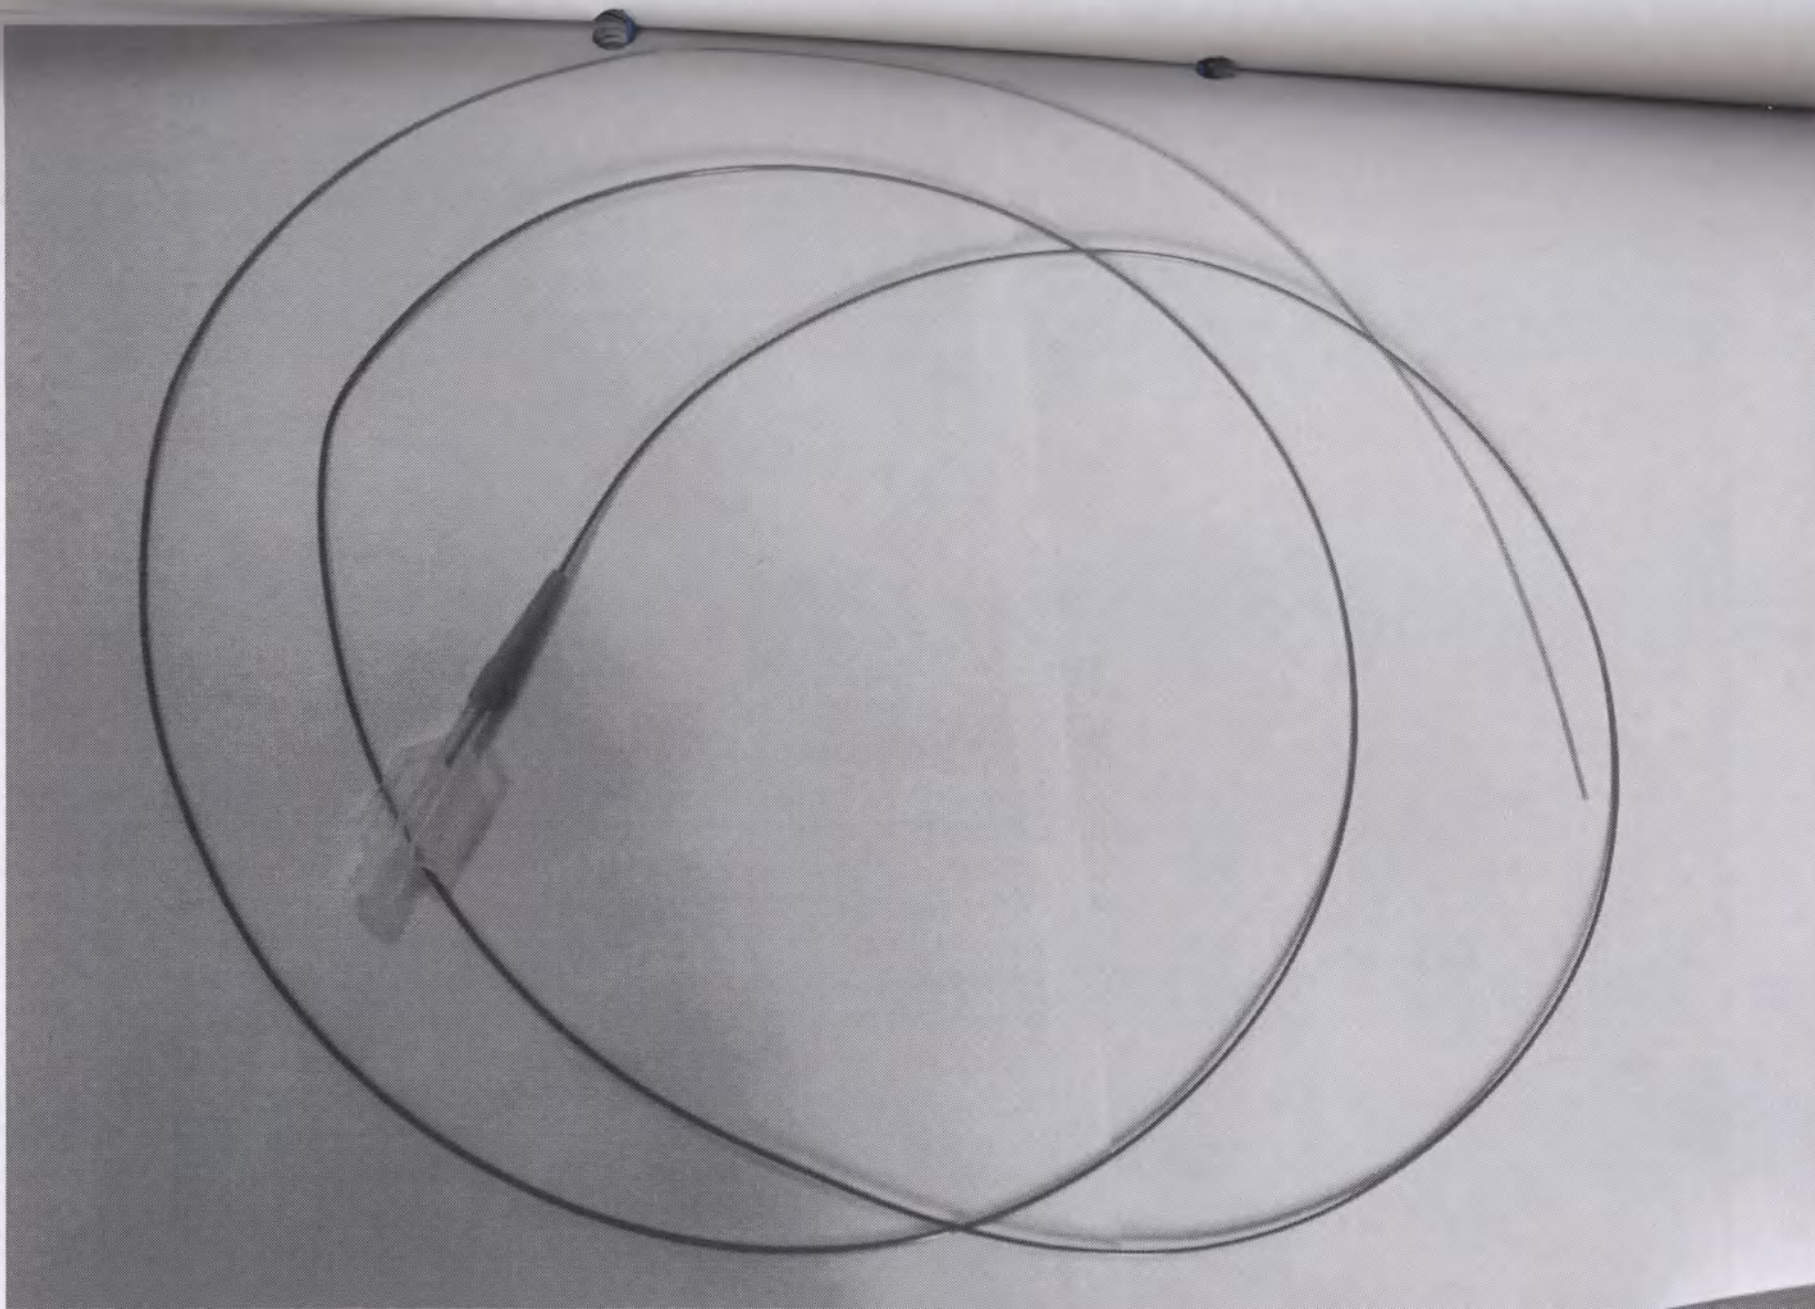



Рабочая часть Микрокатетера Rebar -18, длина 130 см



Втулка Микрокатетер Rebar -18, длина 130 см

STEAM SHAPING MANDREL

INSTRUCTIONS FOR USE

In order to maintain catheter integrity and dimensional stability of the inner diameter, it is recommended that the user follow these instructions.

Warning! Shaping Mandrel is not intended for use in the human body.

Warning! Use only a steam source to shape the catheter tip. Do not use other heat sources.

Warning! Prior to use, inspect the catheter tip for any damage that may have resulted from shaping. Do not use a catheter that has been damaged in any way. Damaged catheters may rupture causing vessel trauma or tip detachment during steering maneuvers.

1. Remove shaping mandrel from card and insert into distal tip of the catheter.
2. Gently bend catheter tip and shaping mandrel to desired shape. A slight over exaggeration of the shape may be required to accommodate for catheter relaxation.
3. Shape the catheter by holding the shaped portion approximately 1 inch (2.5 cm not less than 1 cm) from the steam source for about 20 seconds (DO NOT EXCEED 30 SECONDS.)
4. Allow catheter tip to cool in air or saline prior to removing mandrel.
5. Remove mandrel from catheter and discard. Multiple shaping is not recommended.
6. Inspect the tip for any damage that may have resulted from steam shaping the catheter tip. If any damage is found, do not use the catheter.

EV3™

Мандрен с заостренным концом микрокатетера Rebar



YOUR ENDOVASCULAR COMPANY

Micro Catheter

A 1.5 F (.51 mm)	B 165 cm
C 2.7 F (.91 mm)	D .013 in (.33 mm)
E 1.5 F (.51 mm)	F Distal Length 25 cm
G Detachable Tip Length 5.0 cm (50 mm)	H 0.5 mm
J 1.25 mm	K 1.9 F (.63 mm)
L .053" (1.35 mm) Compatible Guiding Catheter ID	M .23 ml Minimum Dead Space .20 ml Minimum Dead Space with Syringe Adapter

10988-001 Rev. 04/03




Micro Therapeutics, Inc.
8750 ev3 Neurovascular
9775 Toledo Way
Irvine, CA 92618 U.S.A.
Phone: +1-949-837-3700
Fax: +1-800-637-9775

Medtronic B.V.
Earl Bakkenstraat 10
6422 PJ Heerlen
The Netherlands

Apollo™ Onyx™ Delivery Micro Catheter

Microcatheter Mikrokatheter Mikrokatheter Mikrokatheter Mikrokatheter 마이크로 카테터
Microcatheter Mikrokatheter Mikrokatheter Mikrokatheter Mikrokatheter 마이크로 카테터
Microcatheter Mikrokatheter Mikrokatheter Mikrokatheter Mikrokatheter 마이크로 카테터

REF 105-5097-000 LOT A394039 CONTENTS 1X
2019-12-06 1X
1X

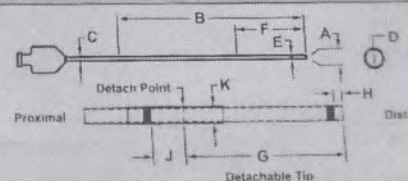

Apollo REF 105-5097-000 LOT A394039
ev3


Apollo REF 105-5097-000 LOT A394039
ev3

Apollo REF 105-5097-000 LOT A394039
ev3

Syringe Adapter - Apollo™ Onyx™ Delivery Micro Catheter

REF: 50414-001 LOT: A394129

CONTENTS: 1 X 2019-12-28





Catheter	Minimum Dead Space
Catheter	Catheter + Adapter
Apollo	23 20

Medtronic, Inc.
5115 Teller Way
Sunnyvale, CA 94088-1099
Phone: 1-800-451-5075
Fax: 1-415-451-5075

Medtronic B.V.
Eenheidsweg 10
5423 PZ Oss
The Netherlands
Phone: +31 (0)494 471 111
Fax: +31 (0)494 471 112

Micro Catheter

A 1.5 F (.51 mm)	B 165 cm
C 2.7 F (.91 mm)	D .013 in (.33 mm)
E 1.5 F (.51 mm)	F Distal Length 25 cm
G Distal Tip Length 5.0 cm (50 mm)	H 0.5 mm
J 1.25 mm	K 1.9 F (.63 mm)
L .022" (.56 mm) Compatible Guiding Catheter (I)	M .23 ml Minimum Dead Space .20 ml Minimum Dead Space with Syringe Adapter



Medtronic, Inc.
5115 Teller Way
Sunnyvale, CA 94088-1099
Phone: 1-800-451-5075
Fax: 1-415-451-5075



Medtronic B.V.
Eenheidsweg 10
5423 PZ Oss
The Netherlands
Phone: +31 (0)494 471 111
Fax: +31 (0)494 471 112

Micro Catheter


Apollo
1.5 F / 2.7 F
Tip Length 5.0 cm


Apollo™ Onyx™ Delivery Micro Catheter


REF: 105-5097-000 LOT: A394039
2019-12-06

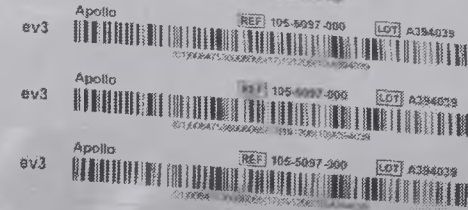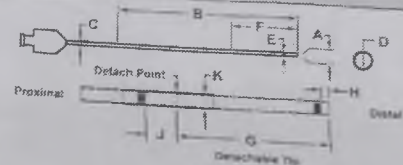



REF: 105-5097-000 LOT: A394039
Usable Length 165 cm
2019-12-06

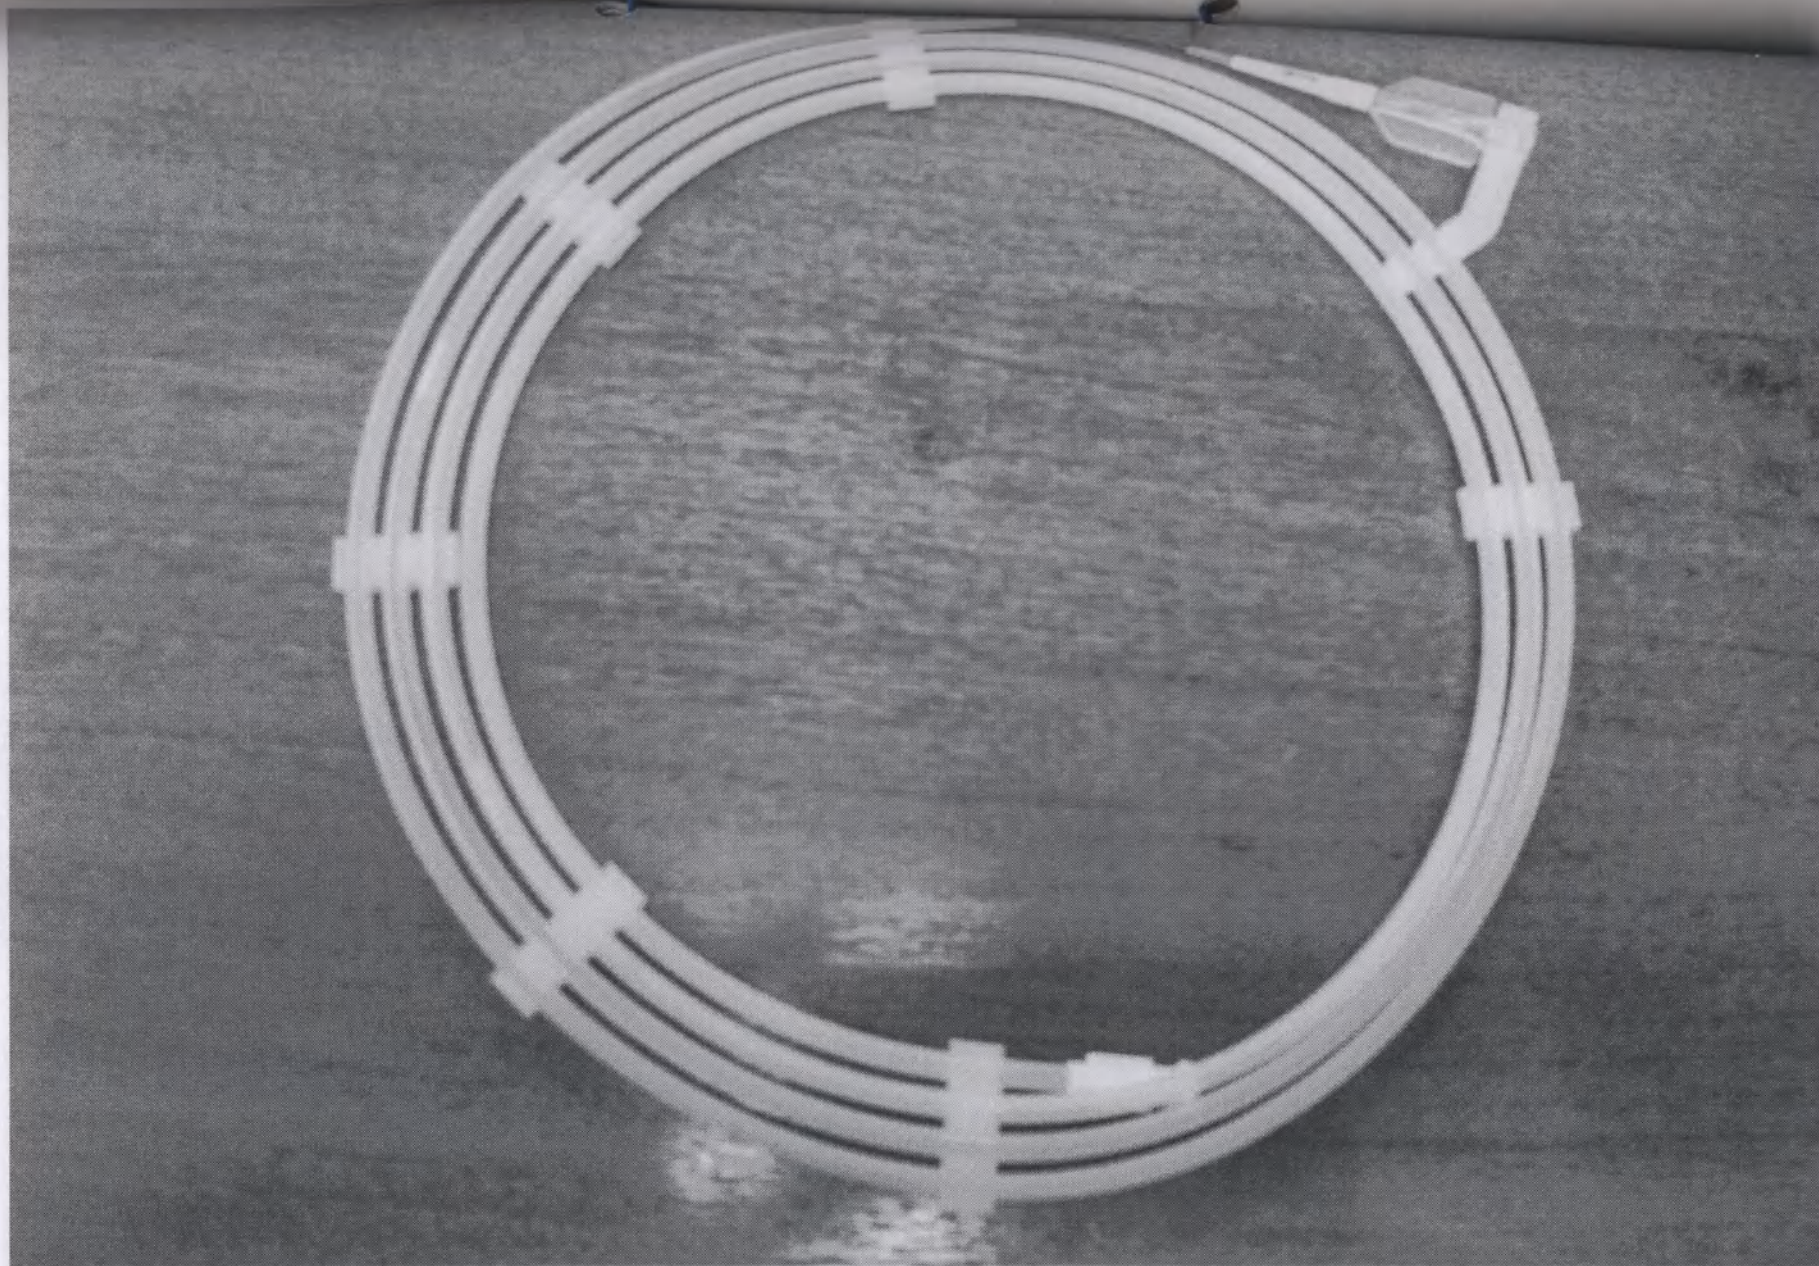

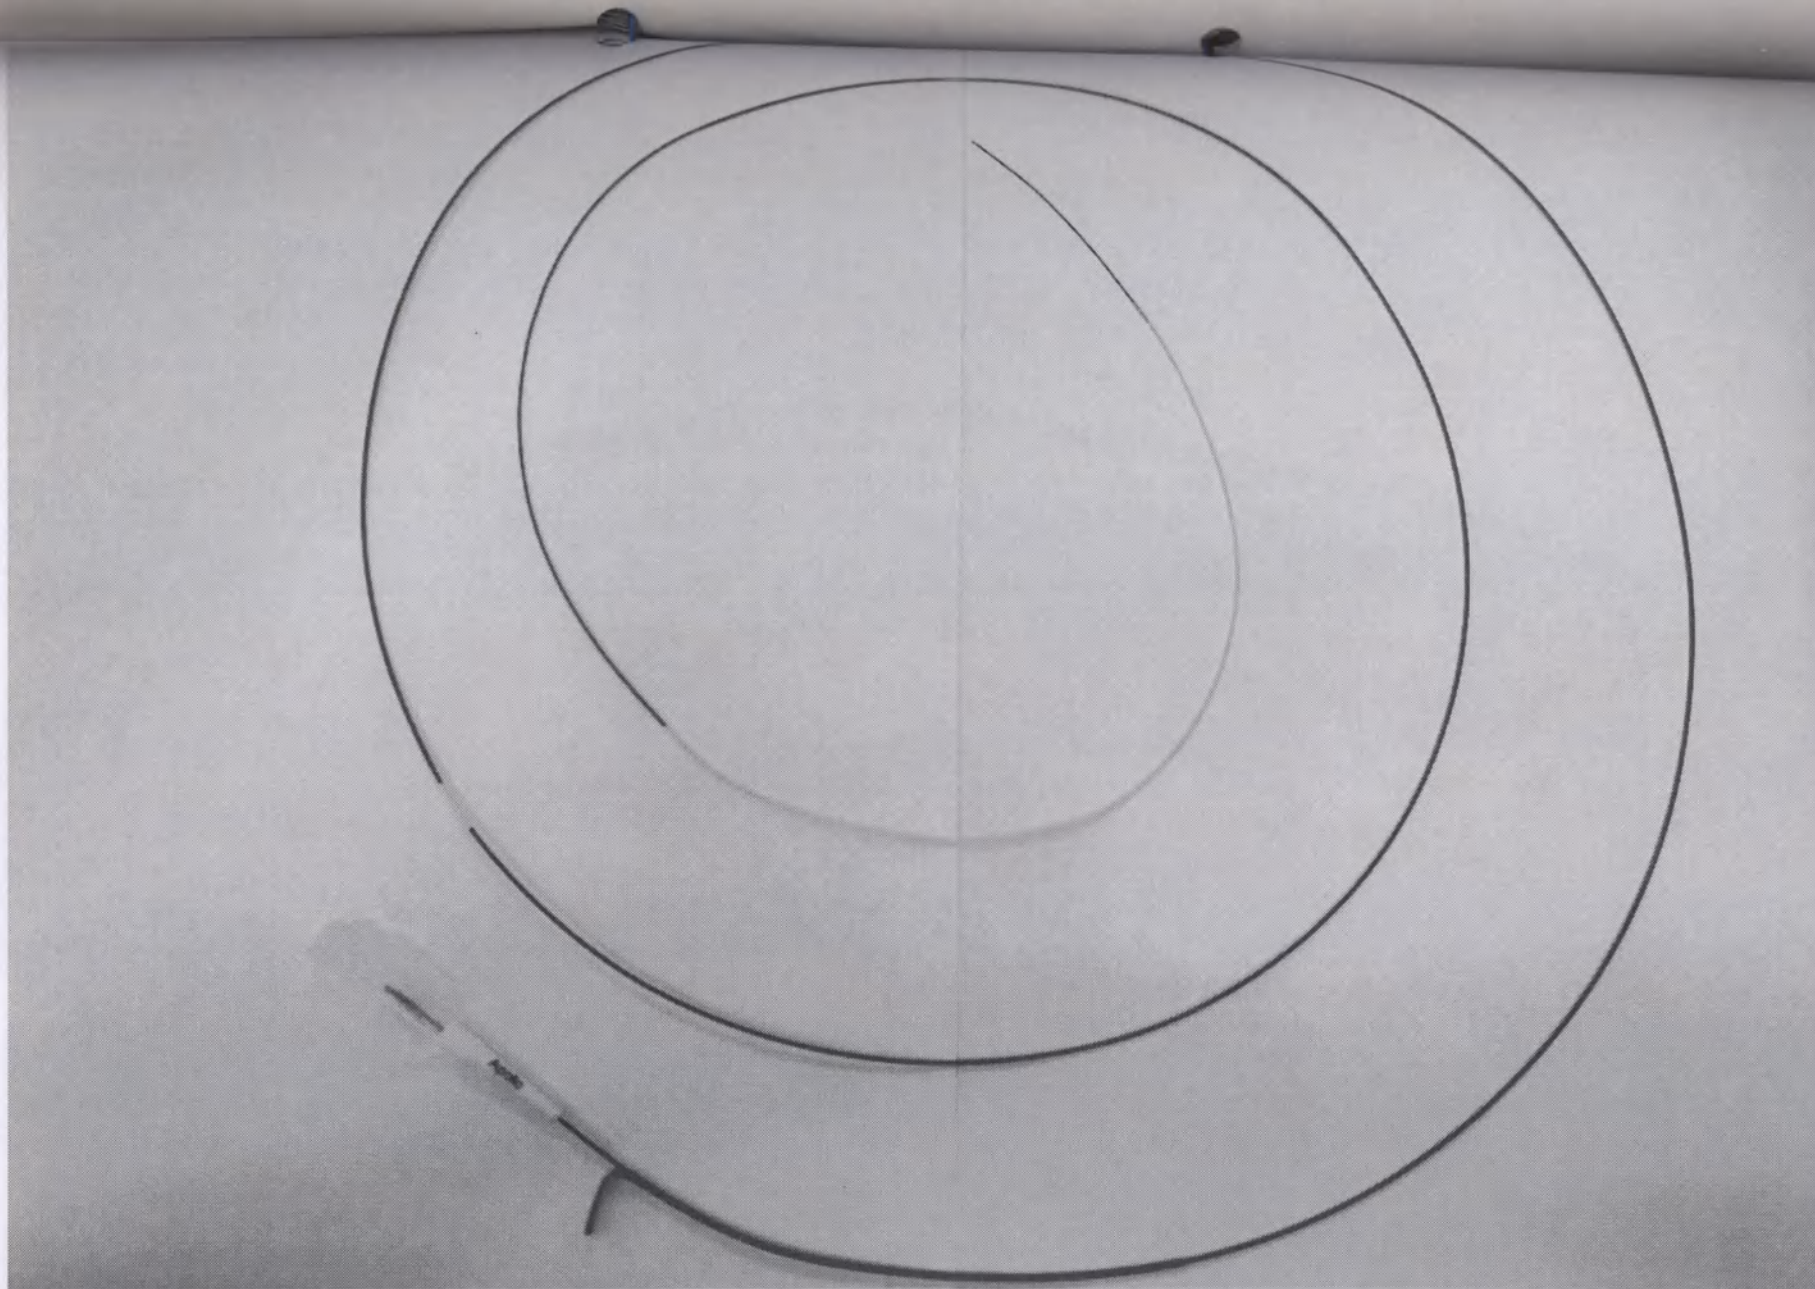


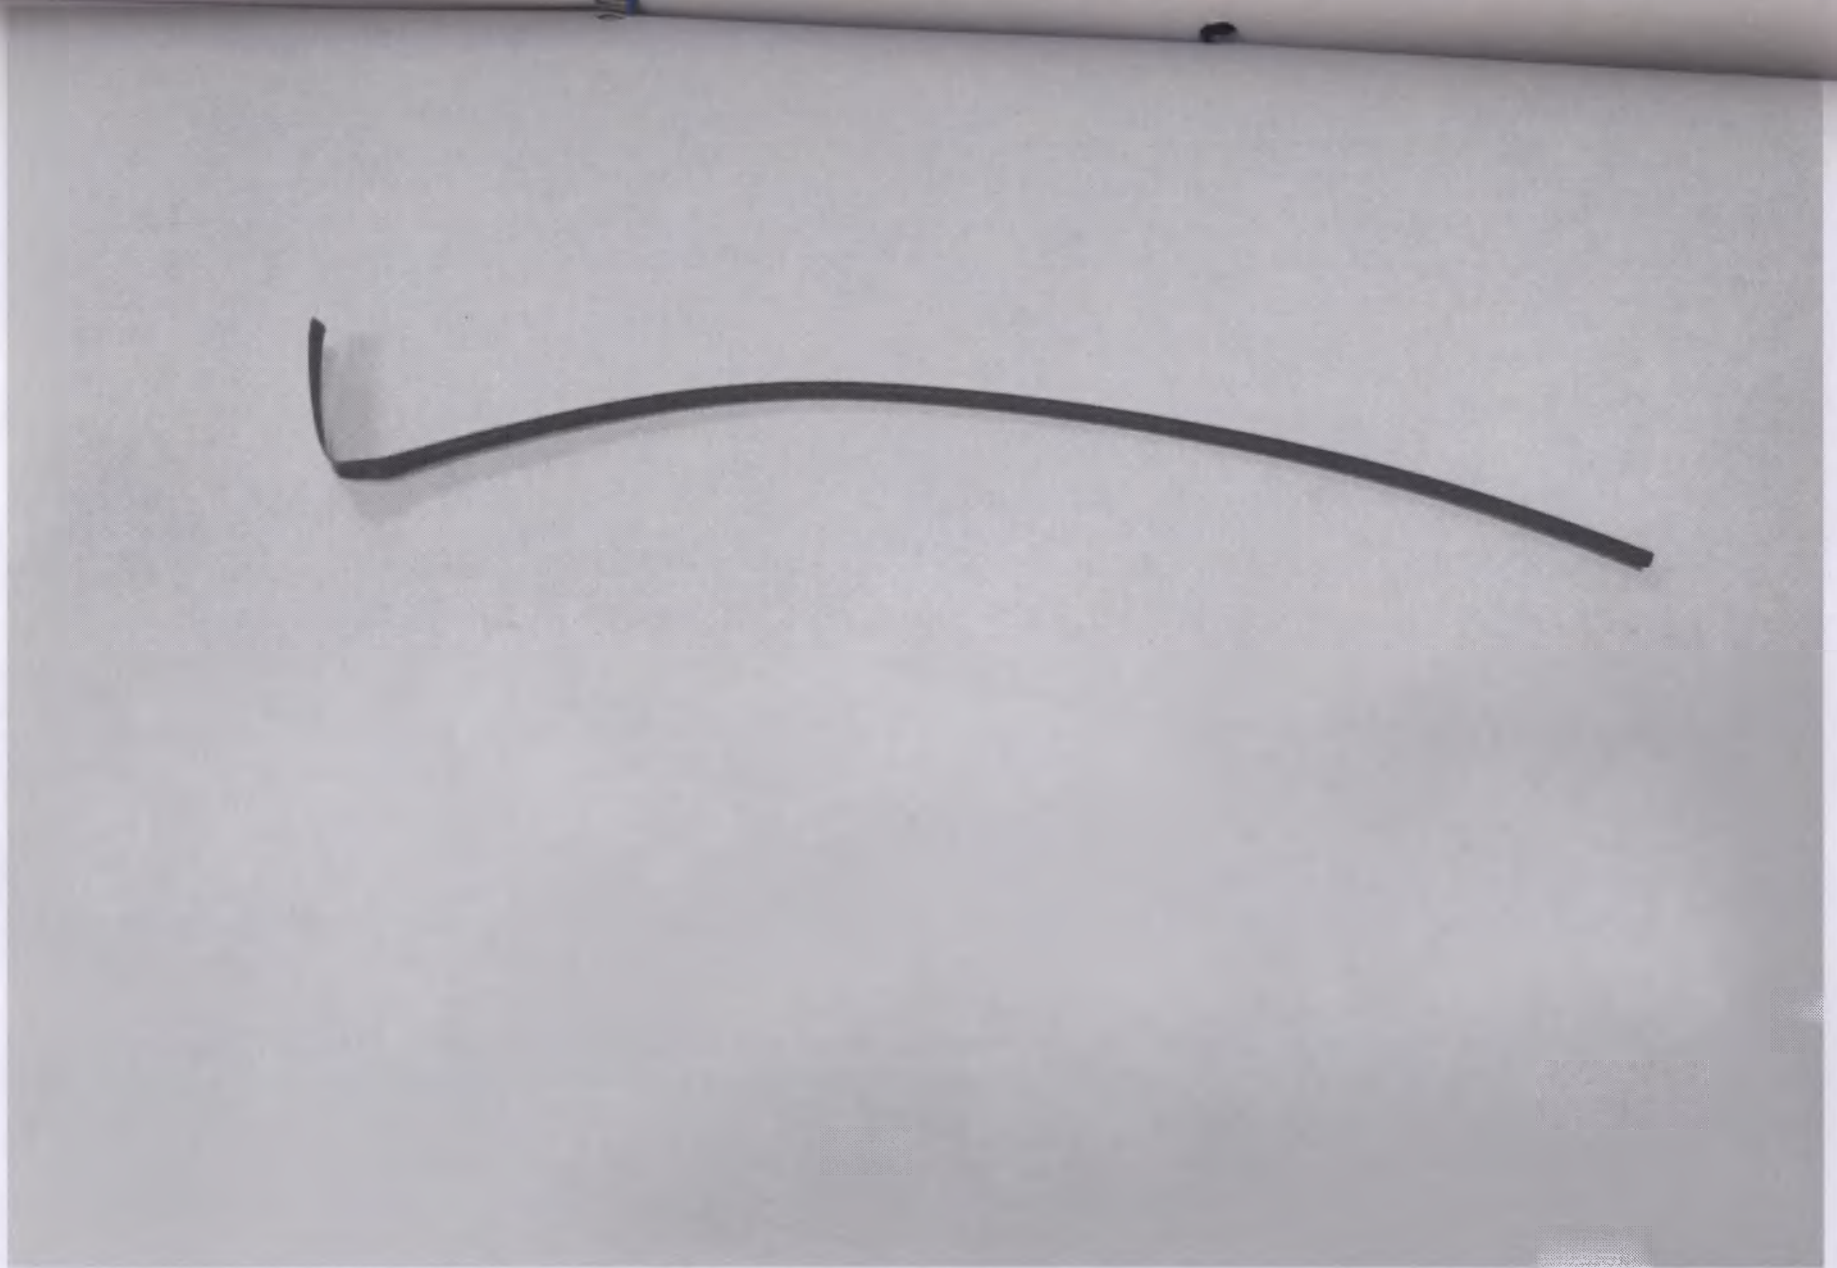

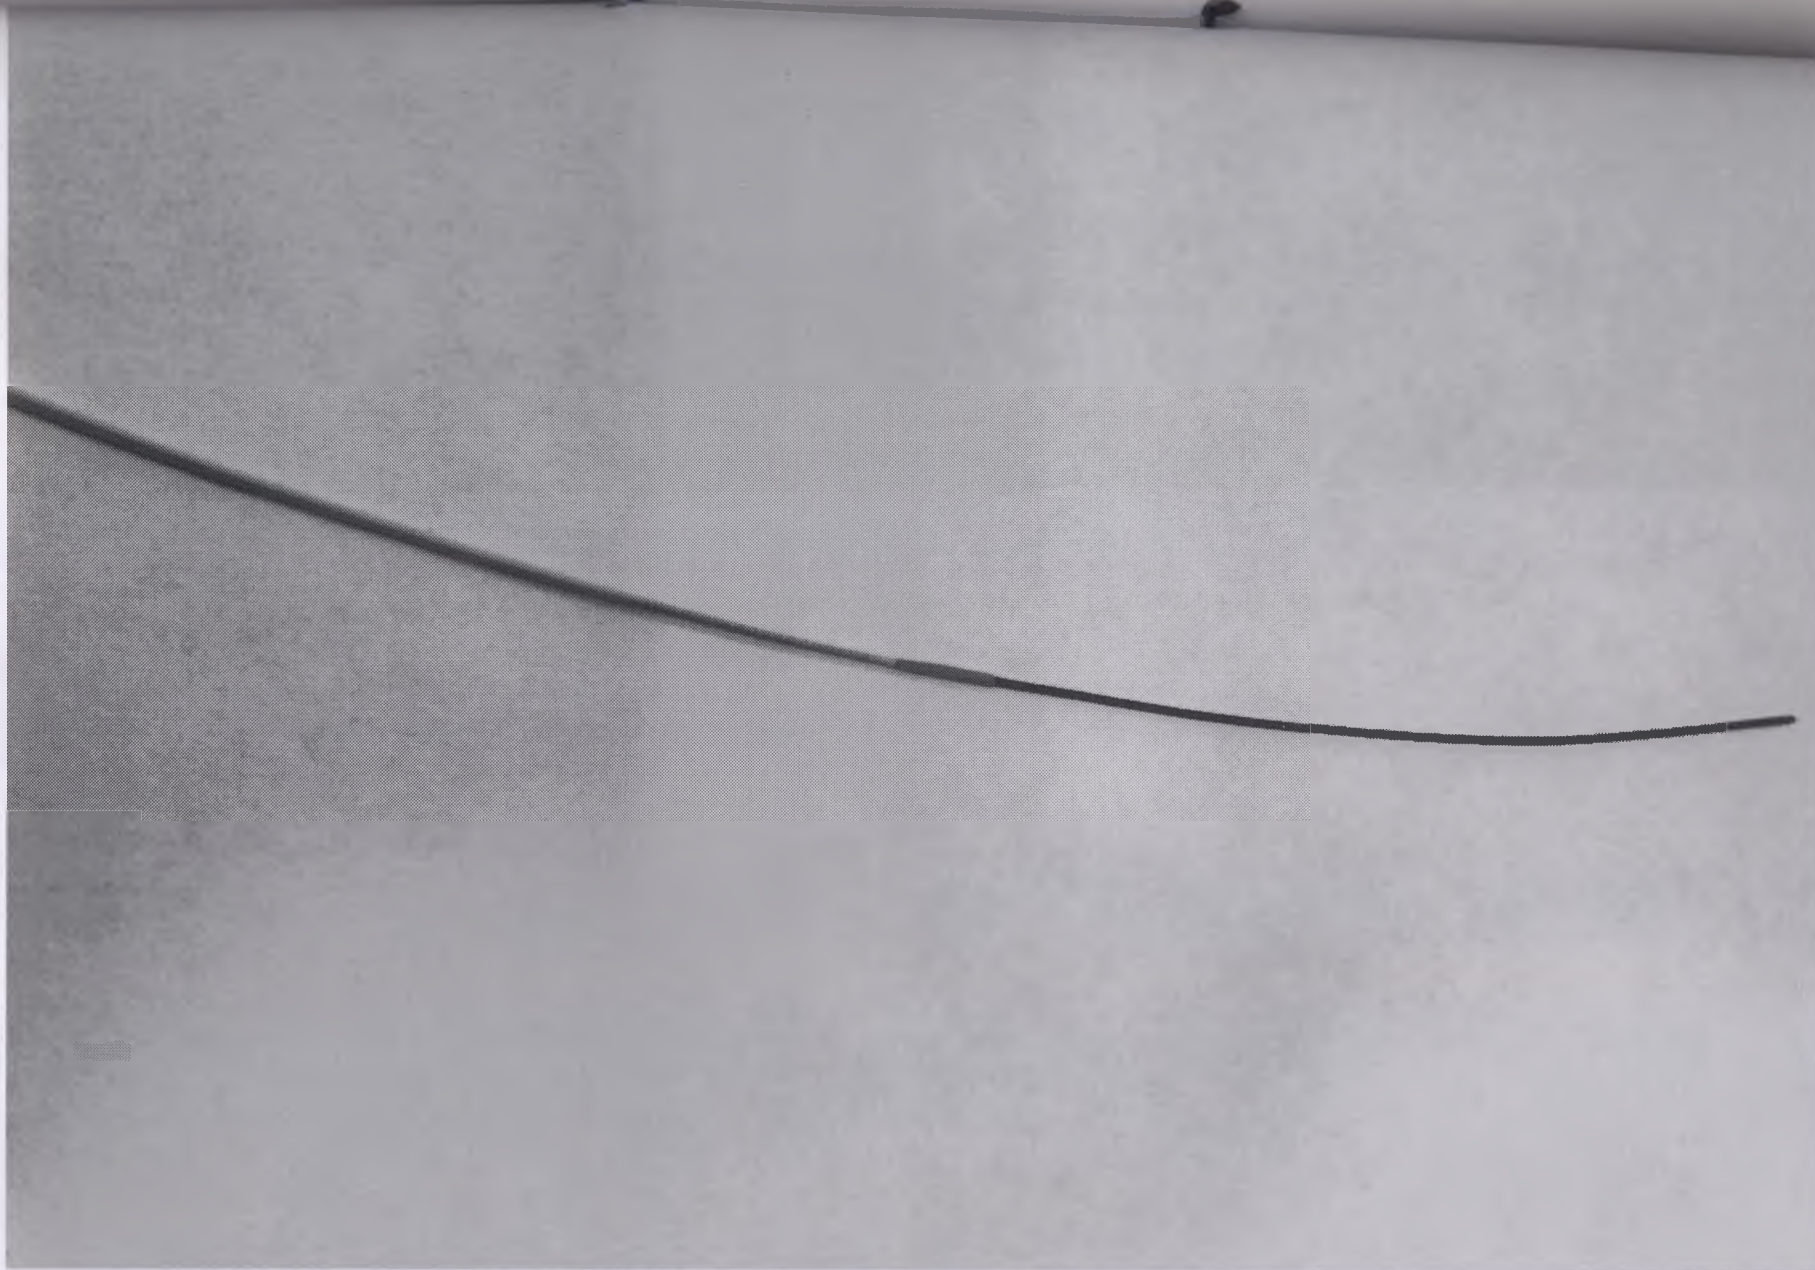


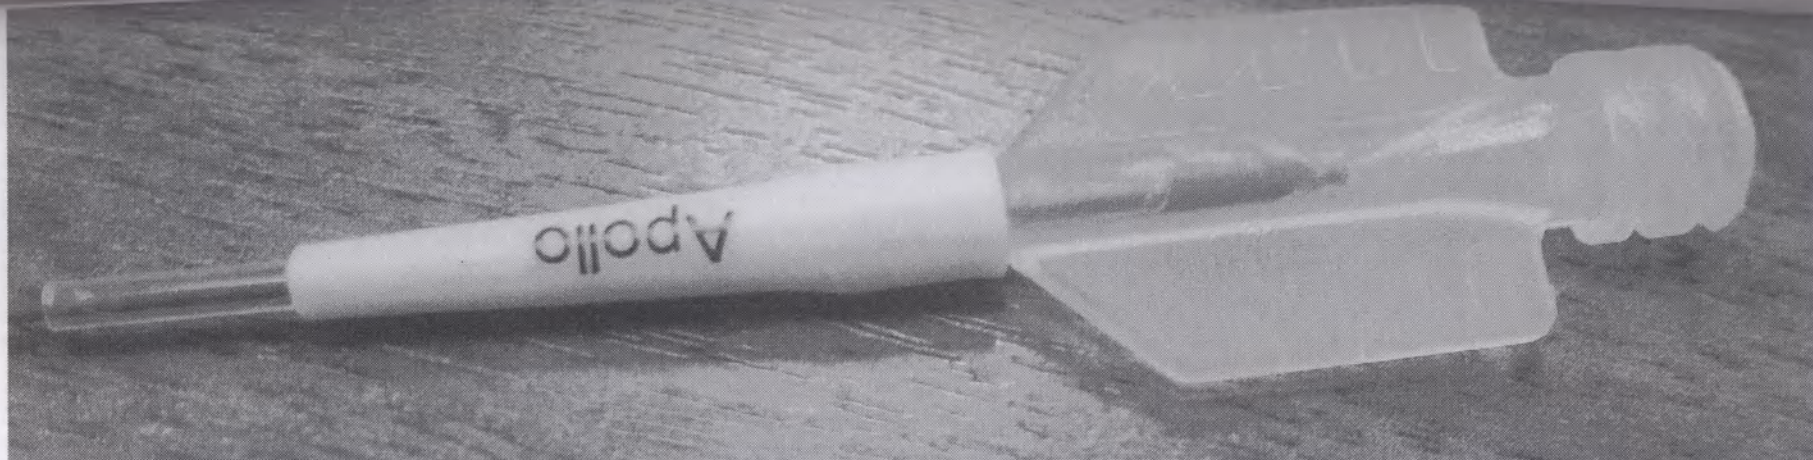


Втулка Микрокатетера Apollo для доставки вещества Онух, длина отсоединяемого наконечника 5,0 см

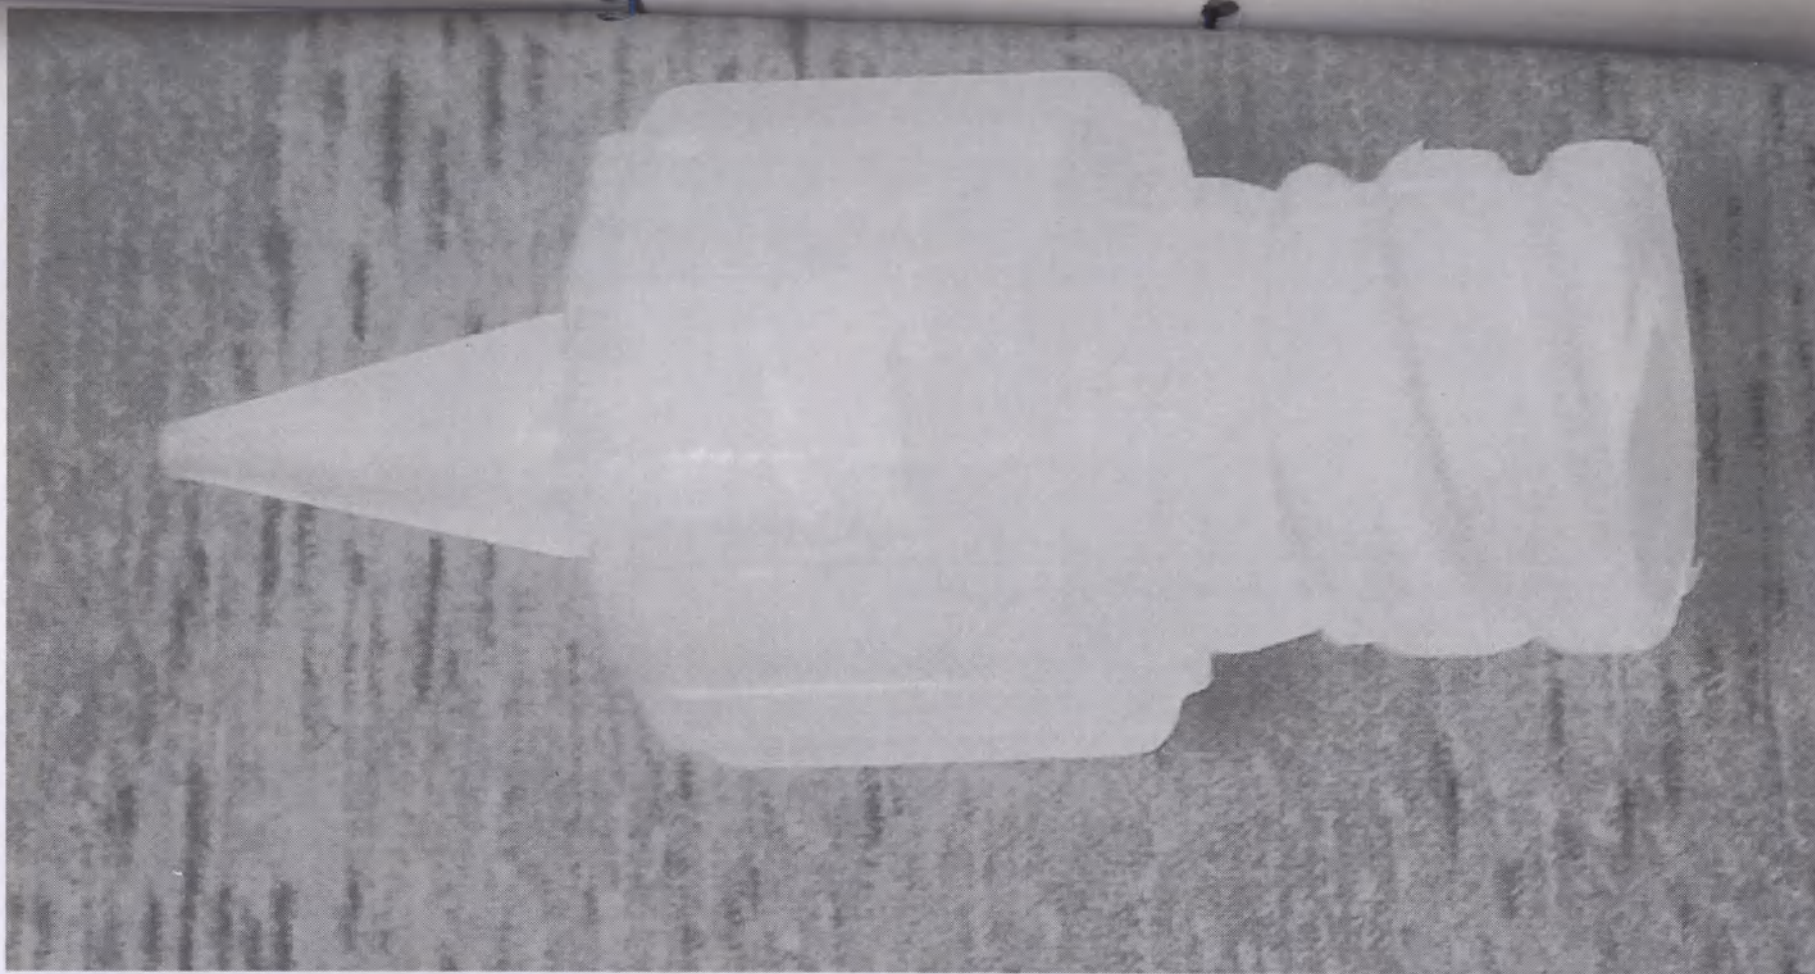

Адаптер для шприца к микрокатетеру Apollo




A	1.5 F .51 mm	B	165 cm
C	2.7 F .91 mm	D	.013 in .33 mm
E	1.5 F .51 mm	F	.23 ml Minimum Dead Space
G	25 cm Distal Length	H	.05" (1.35mm) compatible Guiding Catheter I.D.



Mikrokatēter	Mikrokatēter	Макрокатетер	Макрокатетер
Mikrokatētri	Mikrokatētri	Mikroceņnik	마이크로 카테터
Mikrokatēris	Mikrokatēris	Mikro Kateter	
Mikro Katēris	μκροκατετήριος	Mikrokatēter	مجاز لقسطرة أدقية
Mikrokatēter	Mikrokatēter	Mikrokatēter	
Mikrokatēter	Mikrokatēter	Mikrokatēter	

LOT A378548

CONTENTS



Marathon REF 105-5056 LOT A378548

Marathon REF 105-5056 LOT A378548


Marathon REF 105-5056 LOT A378542

A	1.5 F .51 mm	B	165 cm
C	2.7 F .91 mm	D	.013 in .33 mm
E	1.5 F .51 mm	F	.23 ml Minimum Dead Space
G	25 cm Total Length	H	.027 (1.35mm) compatible Guiding Catheter I.O

Microcatheter	Microcatheter	Microcatheter	Microcatheter
Mikrokatheter	Mikrokatheter	Mikrokateter	마이크로 카테터
Microcatheter	Microcatheter	Microkatheter	ميكرو كاتيتير
Micro Catheter	microcatheter	Microkatheter	ميكرو كاتيتير
Mikrokatheter	Mikrokateter	Microkatheter	ميكرو كاتيتير
Microcatheter	Microcatheter	Microcatheter	

LOT A378548

CONTENTS



Marathon REF 105-5056 LDT A378548
ev3

Marathon REV 105-5050 LOT A178548
8v3

Malatton REF 165-8854 LOT A378548
6v3


Stang International, Inc.
1000 West Main Street
07070 Teaneck, NJ
Tel: 201-261-8100 x 2
Fax: 201-261-5750
E-mail: info@stang.com

Micro Catheter Marathon
1.5 F / 2.7 F

STREET

Usable Length
165 cm

LOT A378548
2019-11-16

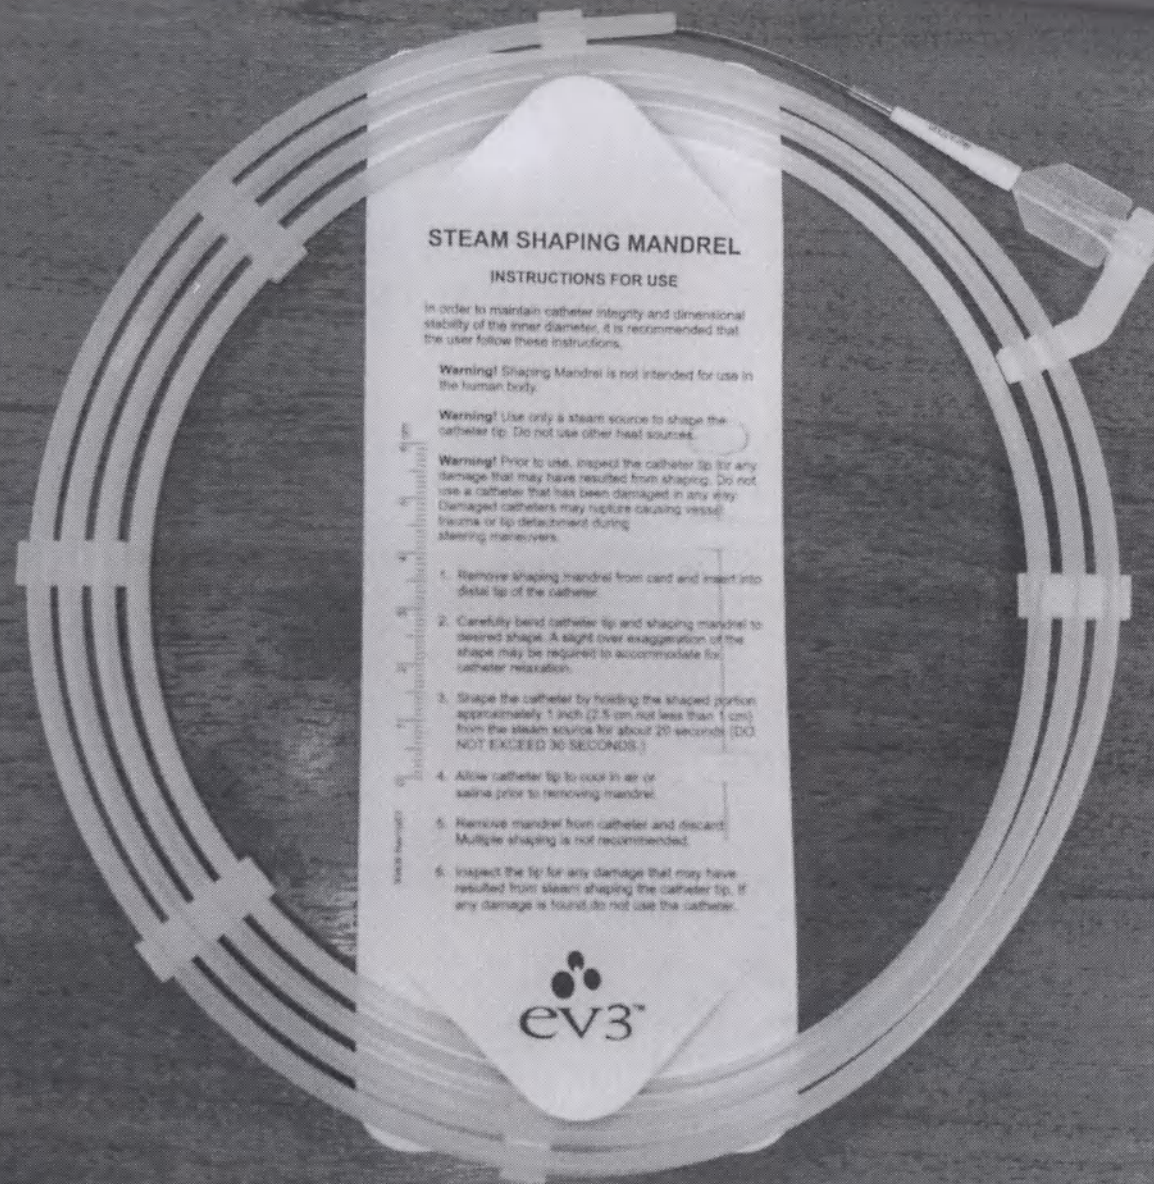

STEAM SHAPING MANDREL

INSTRUCTIONS FOR USE

In order to maintain catheter integrity and dimensional stability of the inner diameter, it is recommended that the user follow these instructions.


Warning! Shaping Mandrel is not intended for use in the human body.


Warning! Use only a steam source to shape the catheter tip. Do not use other heat sources.


Warning! Prior to use, inspect the catheter tip for any damage that may have resulted from shaping. Do not use a catheter that has been damaged in any way. Damaged catheters may rupture causing vessel trauma or tip detachment during steering maneuvers.

1. Remove shaping mandrel from cath and insert into distal tip of the catheter.
2. Carefully bend catheter tip and shaping mandrel to desired shape. A slight over exaggeration of the shape may be required to accommodate for catheter relaxation.
3. Shape the catheter by holding the shaped portion approximately 1 inch (2.5 cm not less than 1 cm) from the steam source for about 20 seconds (DO NOT EXCEED 30 SECONDS.)
4. Allow catheter tip to cool in air or saline prior to removing mandrel.
5. Remove mandrel from catheter and discard. Multiple shaping is not recommended.
6. Inspect the tip for any damage that may have resulted from steam shaping the catheter tip. If any damage is found, do not use the catheter.



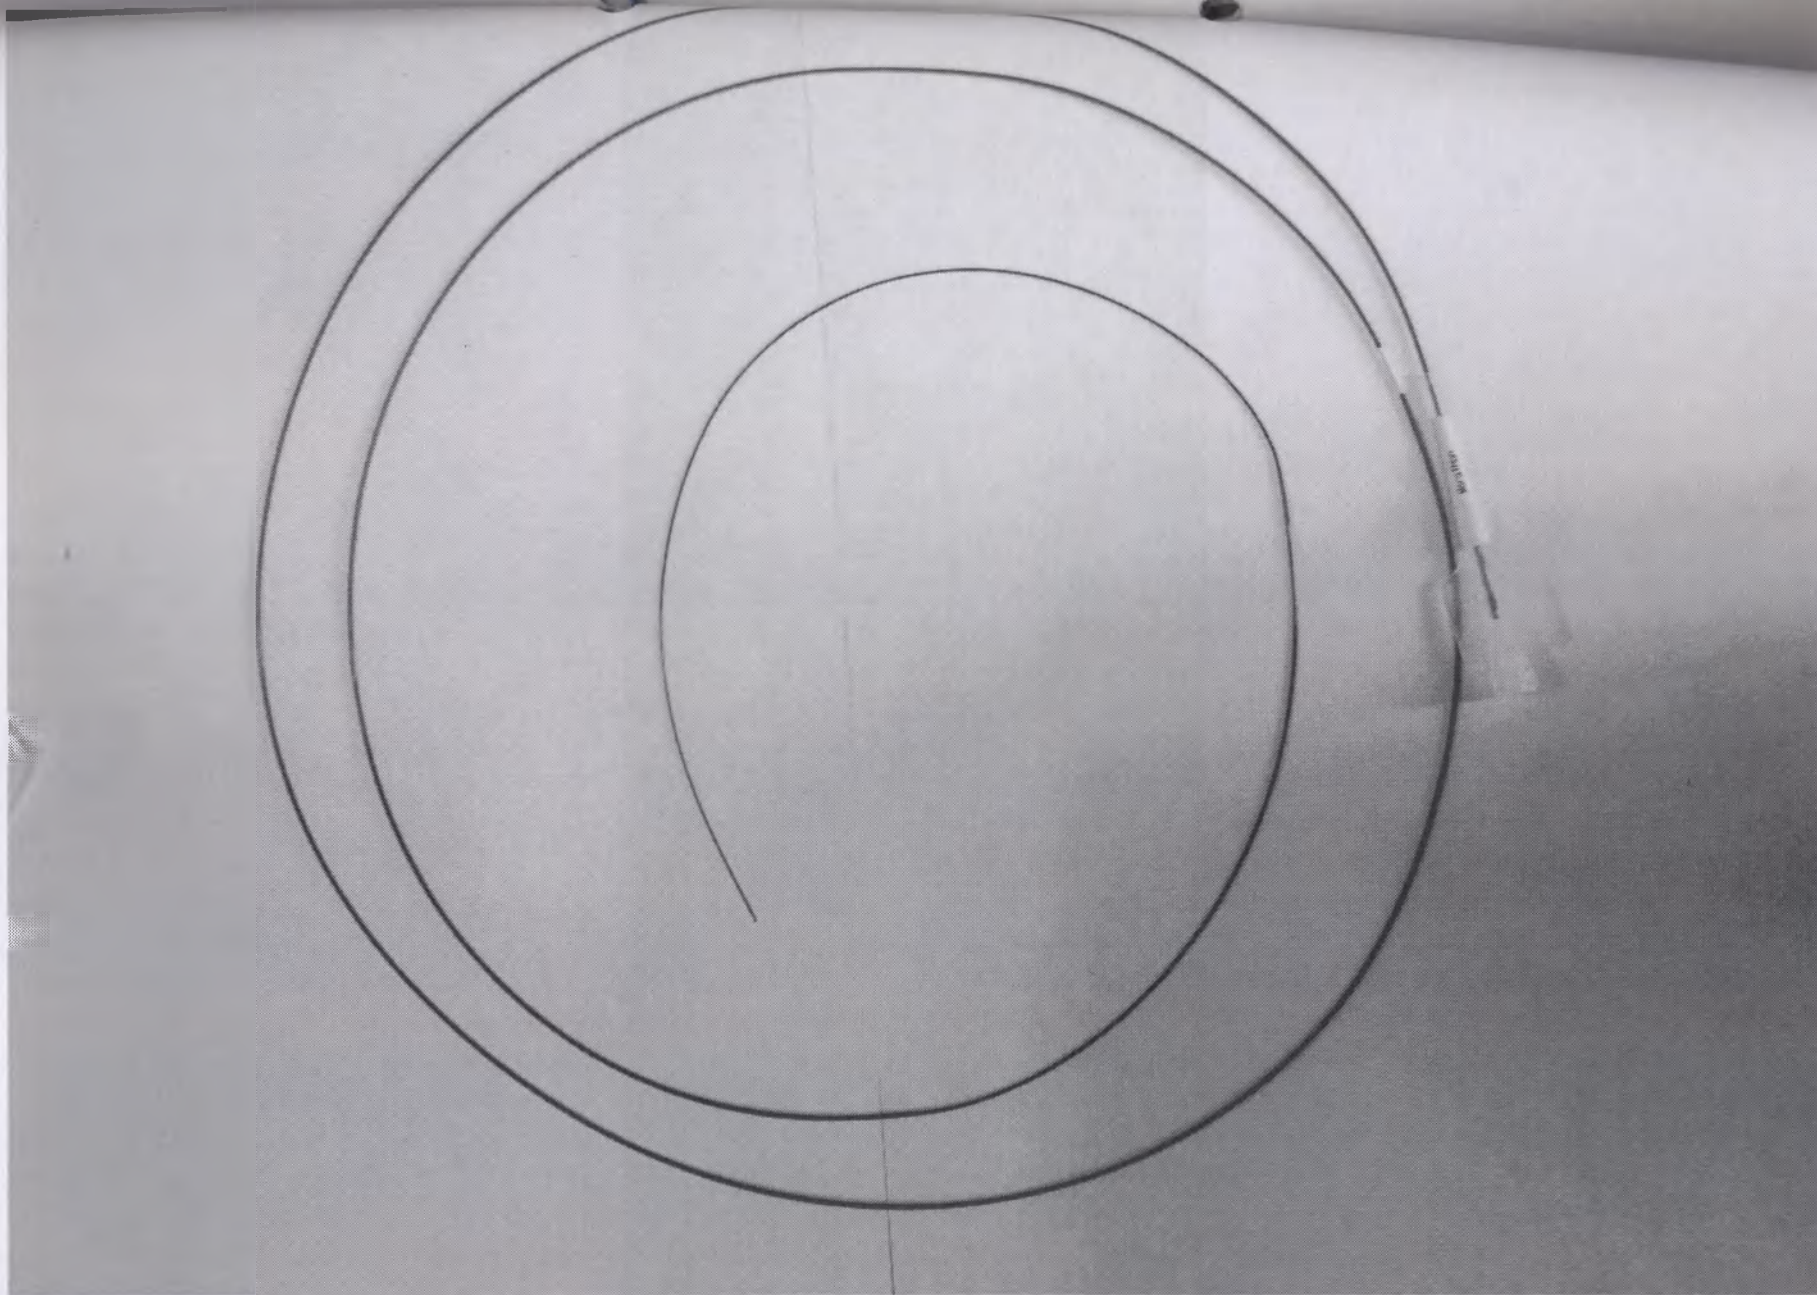

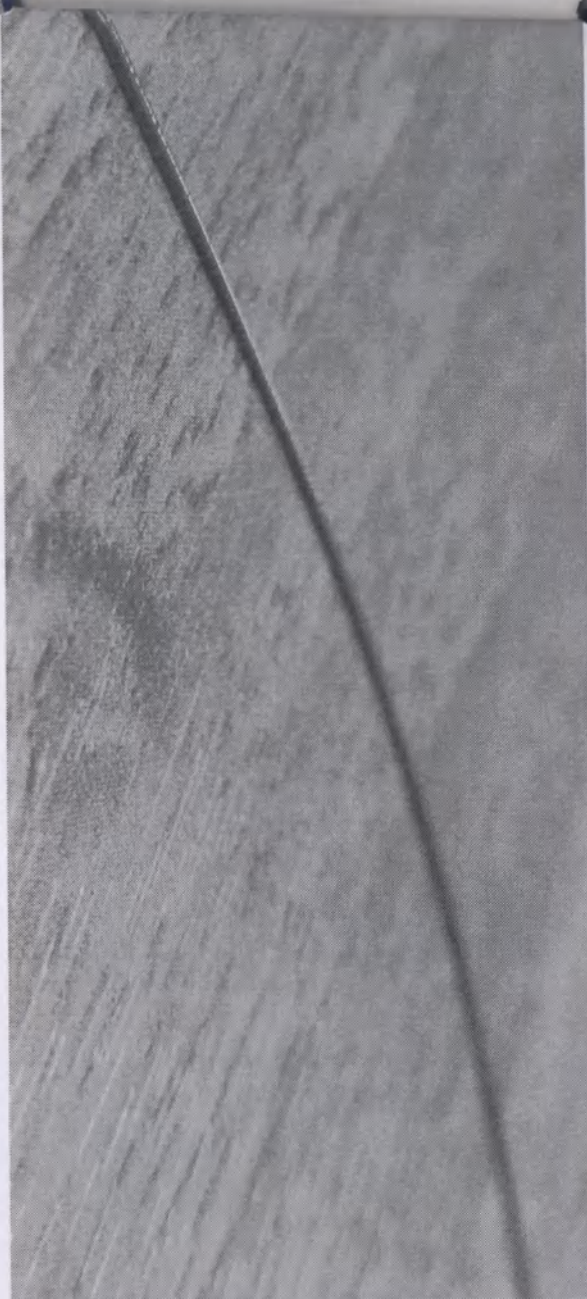

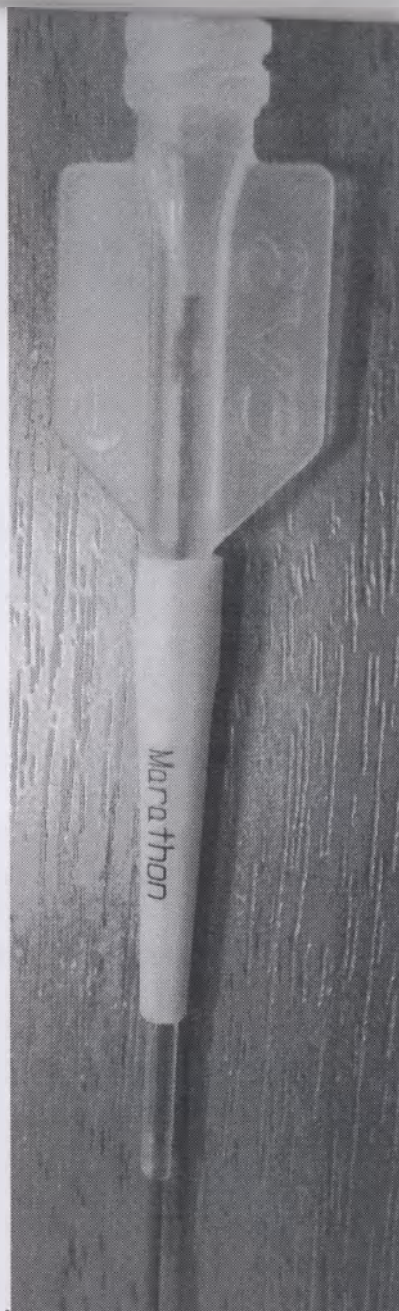

STEAM SHAPING MANDREL

INSTRUCTIONS FOR USE

In order to maintain catheter integrity and dimensional stability of the inner diameter, it is recommended that the user follow these instructions.

Warning! Shaping Mandrel is not intended for use in the human body.

Warning! Use only a steam source to shape the catheter tip. Do not use other heat sources.

Warning! Prior to use, inspect the catheter tip for any damage that may have resulted from shaping. Do not use a catheter that has been damaged in any way. Damaged catheters may rupture causing vessel trauma or tip detachment during steering maneuvers.

1. Remove shaping mandrel from card and insert into distal tip of the catheter.
2. Carefully bend catheter tip and shaping mandrel to desired shape. A slight over exaggeration of the shape may be required to accommodate for catheter relaxation.
3. Shape the catheter by holding the shaped portion approximately 1 inch (2.5 cm not less than 1 cm) from the steam source for about 20 seconds (DO NOT EXCEED 30 SECONDS.)
4. Allow catheter tip to cool in air or saline prior to removing mandrel.
5. Remove mandrel from catheter and discard. Multiple shaping is not recommended.
6. Inspect the tip for any damage that may have resulted from steam shaping the catheter tip. If any damage is found, do not use the catheter.

30409 Rev 1001


EV3™





YOUR ENDOVASCULAR COMPANY

Micro Catheter



A	2.6 F .88 mm	B	150 cm
C	2.4 F .81 mm	D	.021 in .53 mm
E	3 cm	F	2.6 F .88 mm
G	.48 ml Dead Space Volume	H	.018" (.46mm) Max. Guidewire .044" (1.13mm) compatible Guiding Catheter I.D.
I	82 cm Hypotube Length		

23089 901 Rev. 2411




Micro Therapeutics, Inc.
6052 ev3 Neurovascular
9775 Toledo Way
Irvine, CA 92618 U.S.A.
Phone: +1-949-837-3700
Fax: +1-800-637-9775

Madronic B.V.
Carl Bakkenstraat 10
6422 P.J. Heerlen
The Netherlands

Orion™-21 Micro Catheter

Microcatheter Microcatheter Микрокатетер 마이크로 카테터
Mikrokatheter Mikrokatheter Mikrosavniks 마이크로 카테터
Microcatheter Mikrokatheter Mikrosavniks 마이크로 카테터
Microcatheter Mikrokatheter Mikrosavniks 마이크로 카테터
Microcatheter Mikrokatheter Mikrosavniks 마이크로 카테터
Microcatheter Mikrokatheter Mikrosavniks 마이크로 카테터

REF	105-5098-150	LOT	A310292
2019-07-14		CONTENTS	1



Orion™-21 REF 105-5098-150 LOT A310292
ev3 (01)00847536027107(17)190714(10)A310292

Orion™-21 REF 105-5098-150 LOT A310292
ev3 (01)00847536027107(17)190714(10)A310292

Orion™-21 REF 105-5098-150 LOT A310292
ev3 (01)00847536027107(17)190714(10)A310292

Микрокатетер Orion 21 в картонной упаковке


A	2.6 F .88 mm	B	150 cm
C	2.4 F .81 mm	D	.021 in .53 mm
E	3 cm	F	2.6 F .88 mm
G	.48 ml Dead Space Volume	H	.018" (.46mm) Max. Guidewire .044" (1.13mm) compatible Guiding Catheter I.D.
I	82 cm Hypotube Length		

Microkaster	Microkaster	Микрокастер	Микрокастер
Microkaster	Микрокастери	Микрокастери	میکروکاستری
Microkaster	Микрокастер	Микрокастер	میکروکاستر
Microkaster	Микрокастер	Микрокастер	میکروکاستر
Microkaster	Микрокастер	Микрокастер	میکروکاستر
Microkaster	Микрокастер	Микрокастер	میکروکاستر

2019-07-14

2019-07-14

CONTENTS



Quantum™ 31 **REF** 195-0892-150 **A310292**

nv3 10721 219021400A310292

Onion™ 21 REF: 105-5098-150 LOT: A310292
av3

097 906-888-150 LOT A31029

097 906-888-150 LOT A31029

Micro Catheter

Orion™-21
2.6 F / 2.4 F

REF
105-5098-150

Usable Length
150 cm

LOT A310292
2019-07-14

STEAM SHAPING MANDREL

INSTRUCTIONS FOR USE

In order to maintain catheter integrity and dimensional stability of the inner diameter, it is recommended that the user follow these instructions.

Warning! Shaping Mandrel is not intended for use in the human body.


Warning! Use only a steam source to shape the catheter tip. Do not use other heat sources.

Warning! Prior to use, inspect the catheter tip for any damage that may have resulted from shaping. Do not use a catheter that has been damaged in any way. Damaged catheters may rupture causing vessel trauma or tip detachment during steering maneuvers.

1. Remove shaping mandrel from card and insert into distal tip of the catheter.
2. Carefully bend catheter tip and shaping mandrel to desired shape. A slight over exaggeration of the shape may be required to accommodate for catheter relaxation.
3. Shape the catheter by holding the shaped portion approximately 1 inch (2.5 cm not less than 1 cm) from the steam source for about 20 seconds (DO NOT EXCEED 30 SECONDS.)
4. Allow catheter tip to cool in air or saline prior to removing mandrel.
5. Remove mandrel from catheter and discard. Multiple shaping is not recommended.
6. Inspect the tip for any damage that may have resulted from steam shaping the catheter tip. If any damage is found, do not use the catheter.

ev3™

Рабочая часть микрокатетера Orion 21

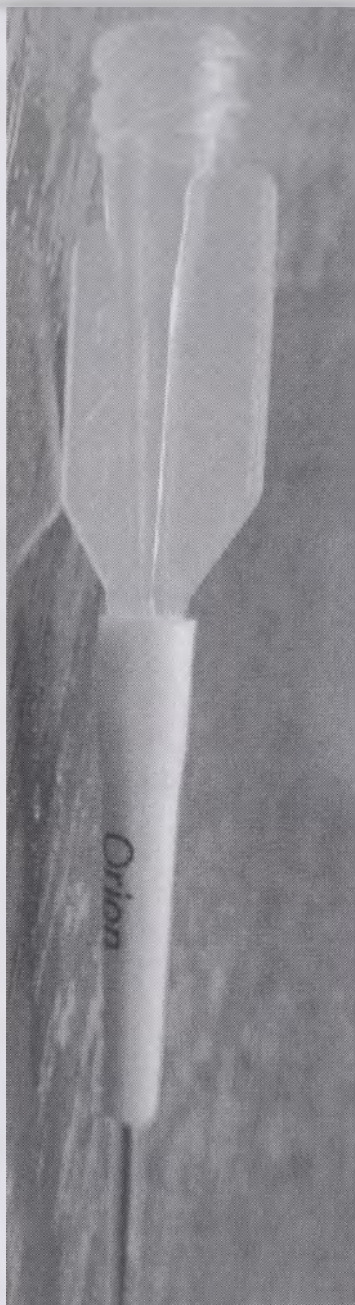

Всего прошнуровано,
пронумеровано и скреплено
печатью ООО «Медтроник»
37 листа(ов)

