

«УТВЕРЖДАЮ»

Генеральный директор
ООО "ЭТС-ПРО"



И.А. Копчинский


«06» февраля 2023 г.


М.П.

ФОТОГРАФИЧЕСКИЕ ИЗОБРАЖЕНИЯ МЕДИЦИНСКОГО ИЗДЕЛИЯ

Катетер баллонный Alwide™ Plus


(редакция 1.0)

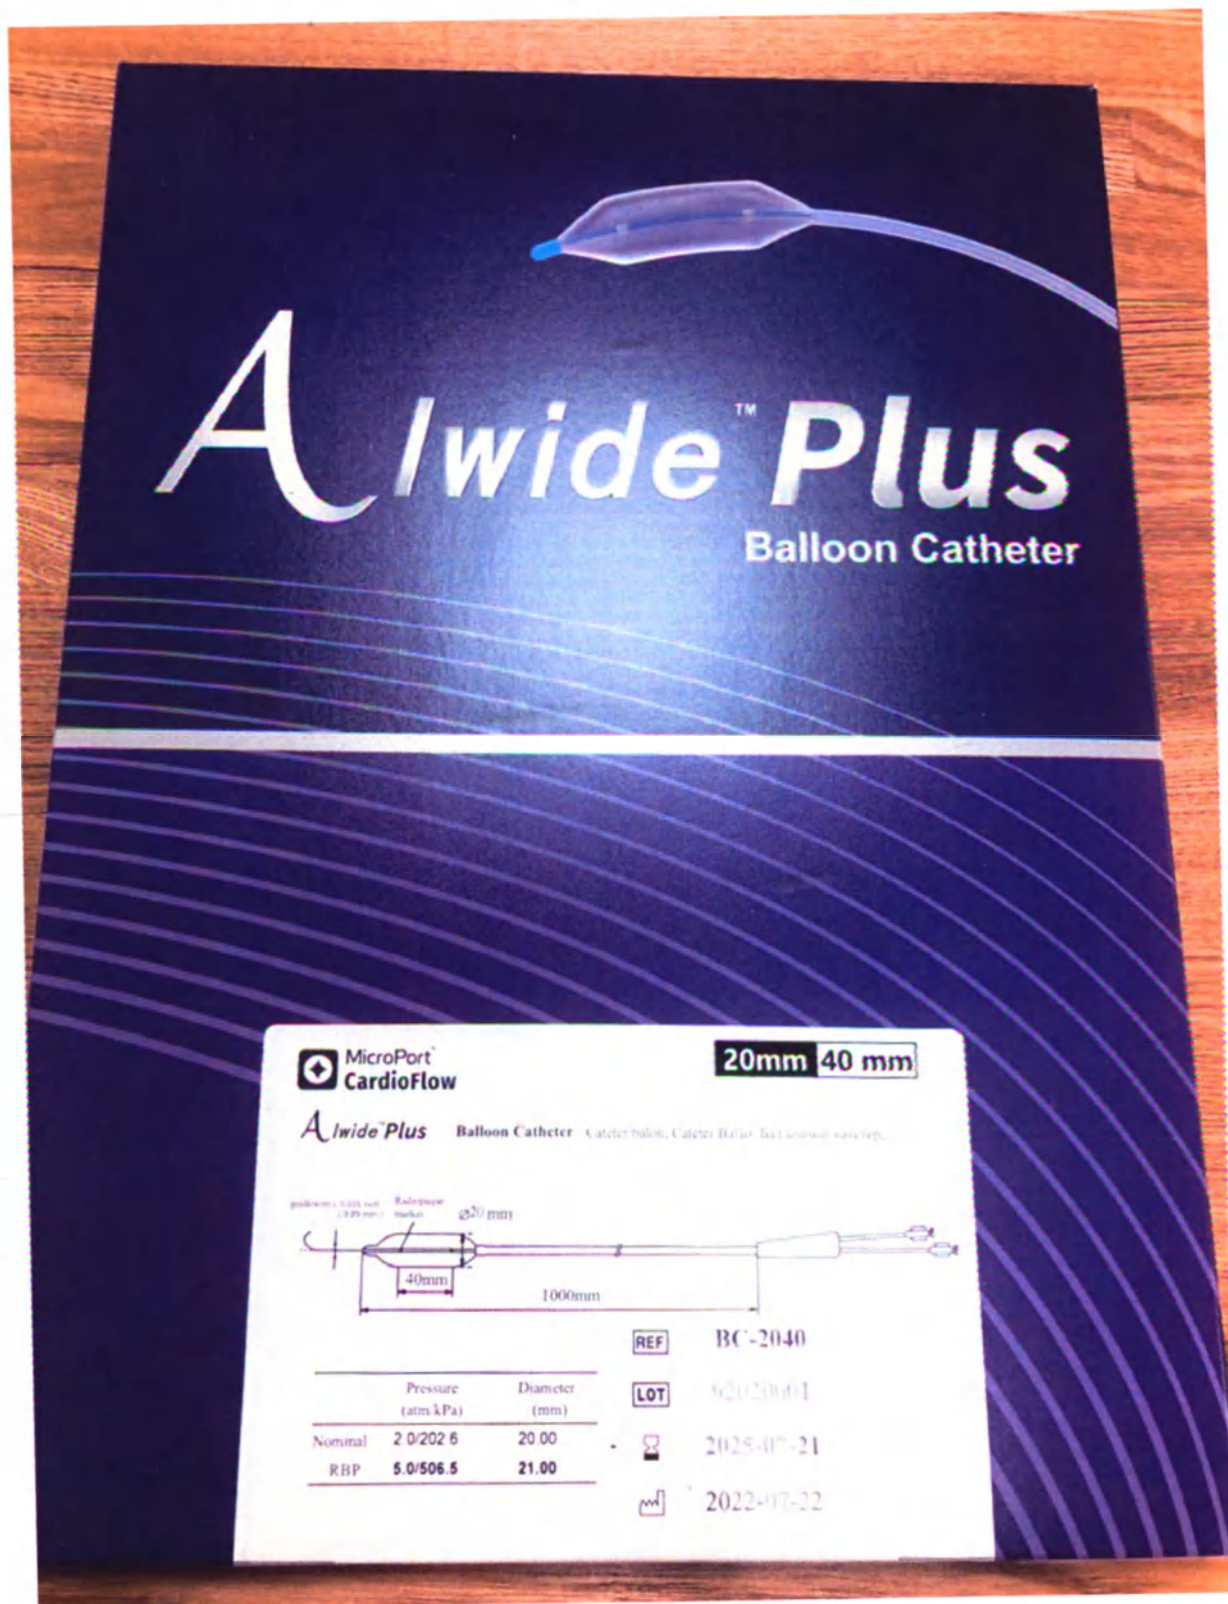

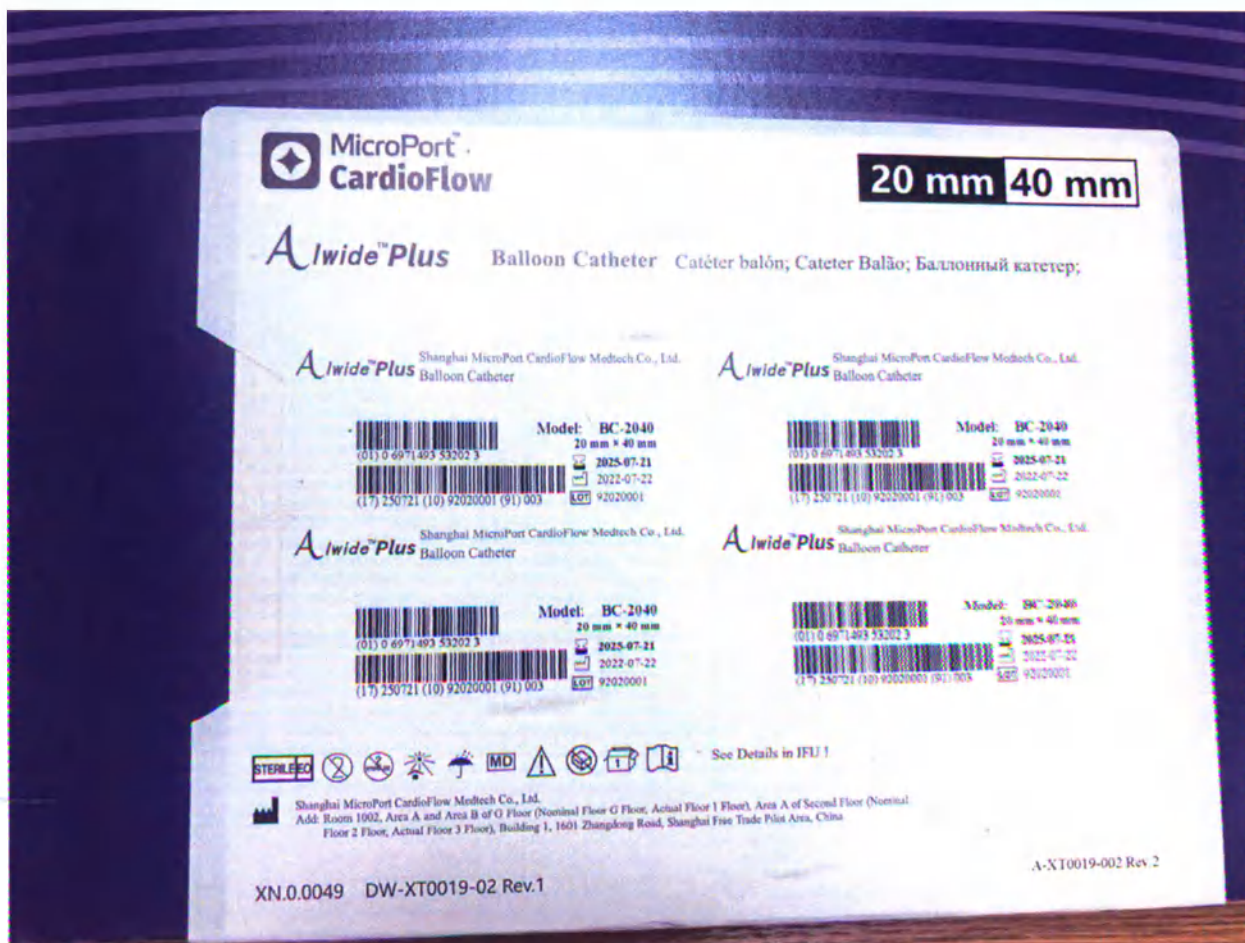



*см.макеты маркировок при поставке в РФ



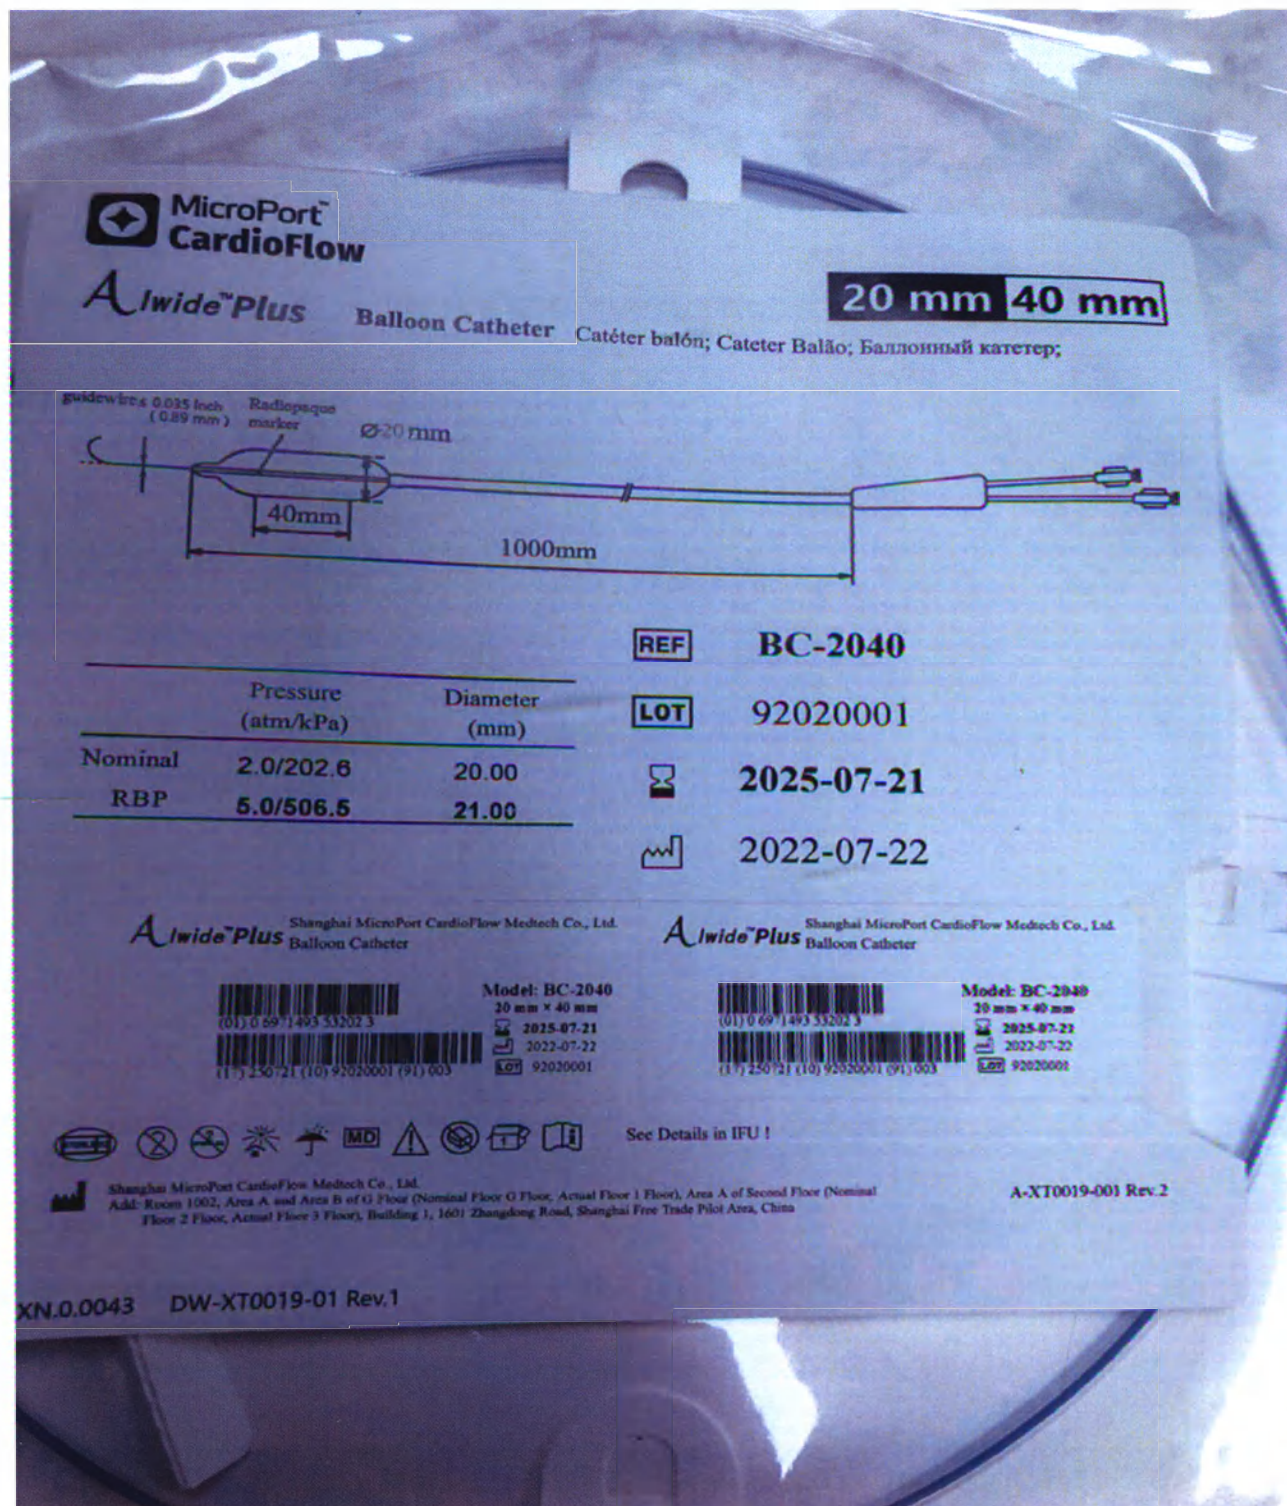


*см.макеты маркировок при поставке в РФ

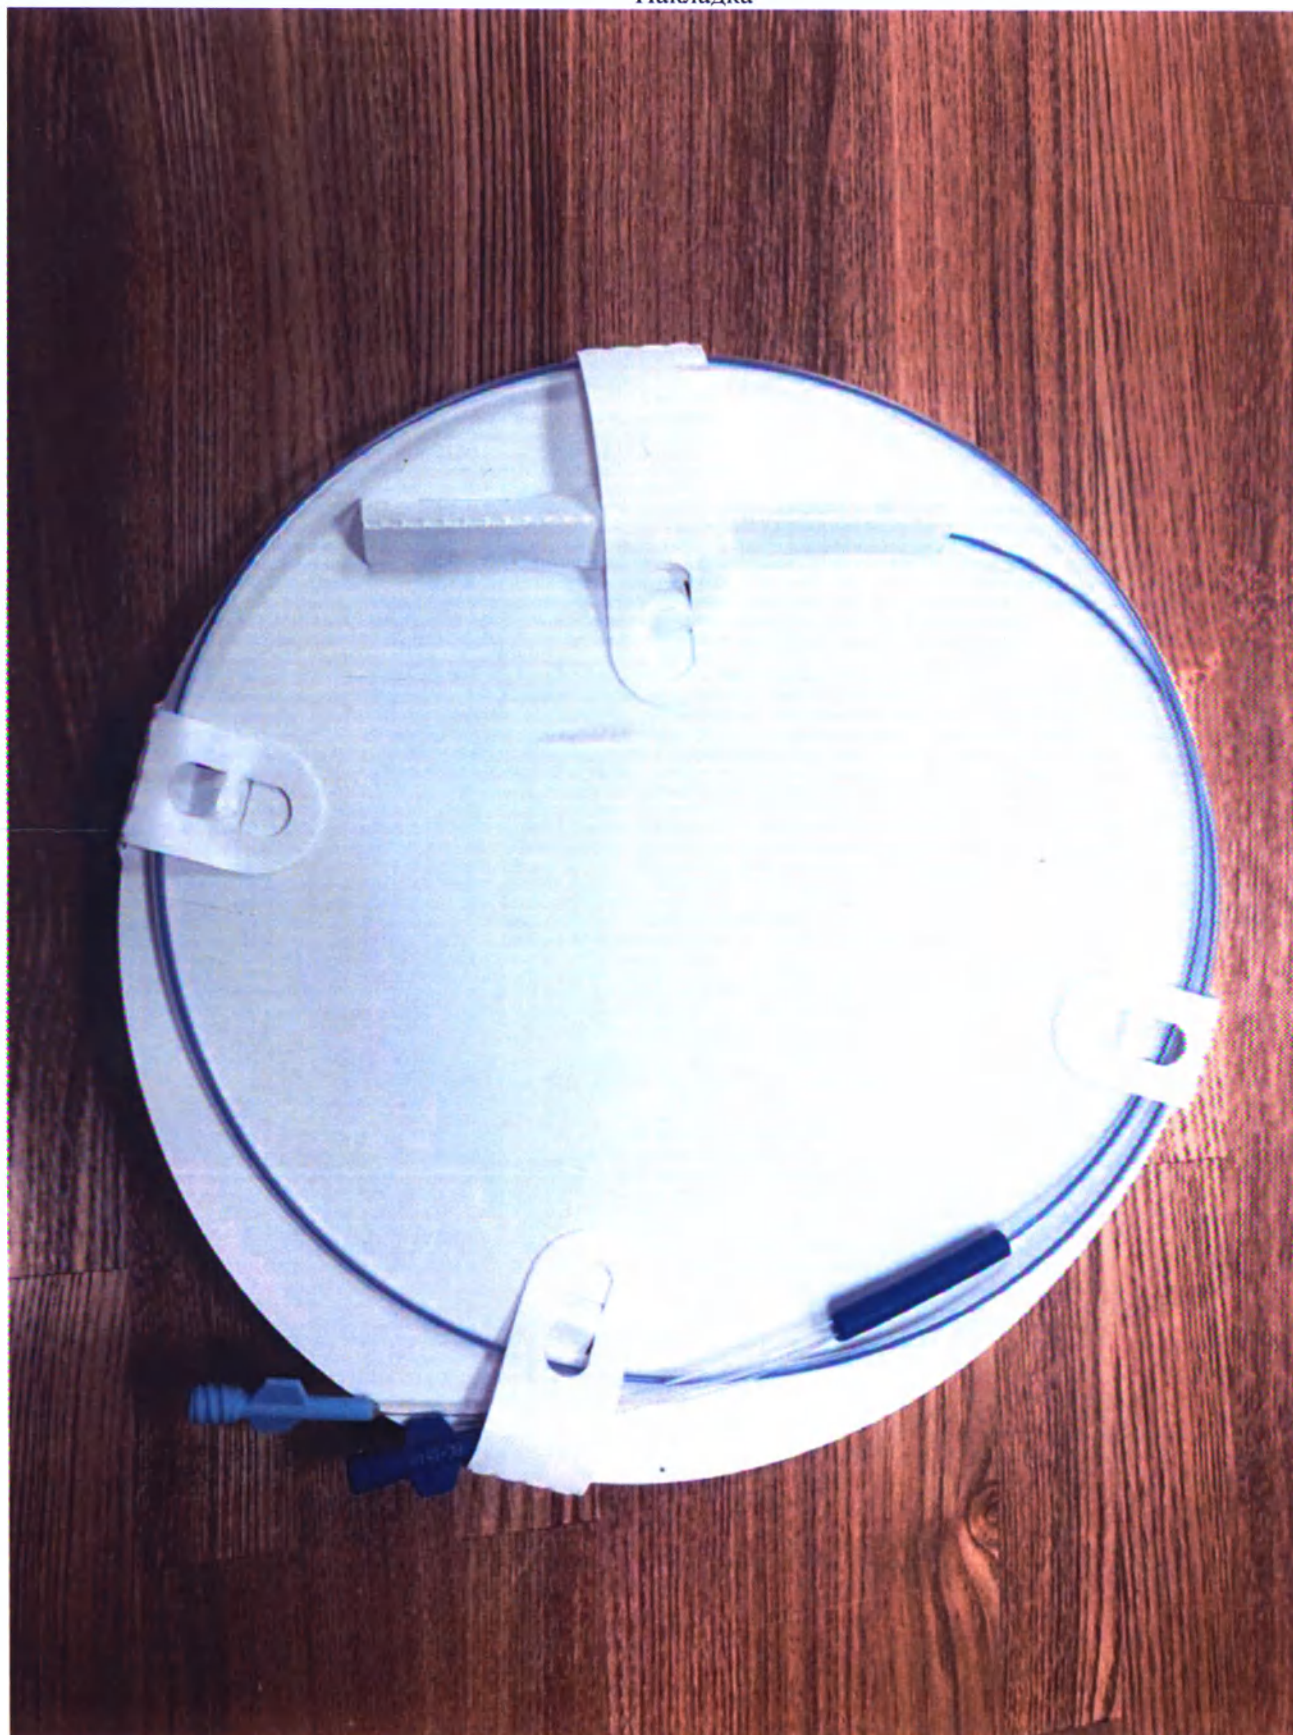

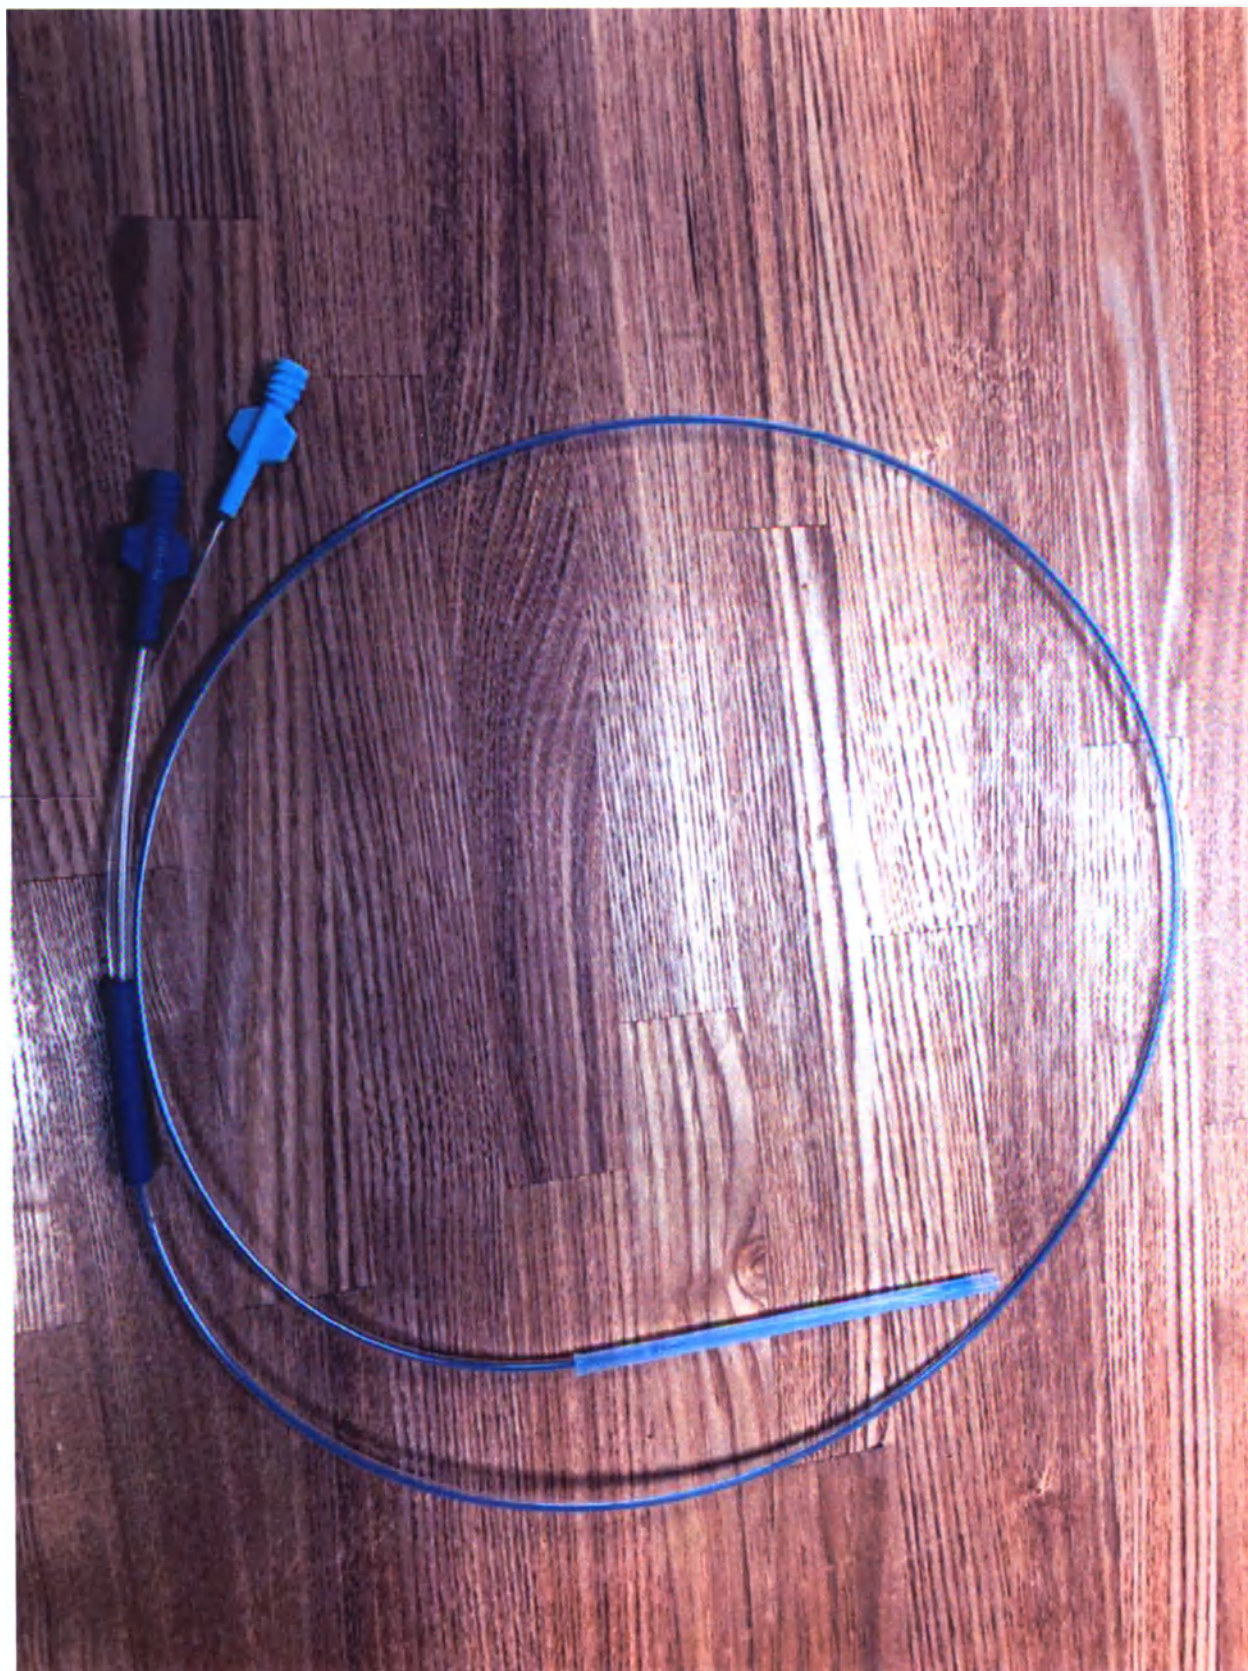



Общий вид баллона (в расправленном виде): Катетер баллонный Alwide™ Plus

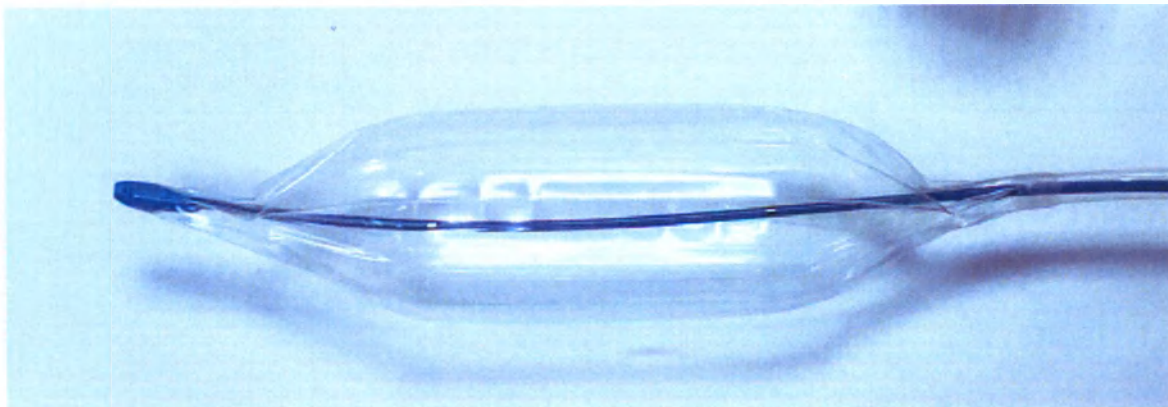

ПРИЛОЖЕНИЕ (СПРАВОЧНОЕ)
Маркировка медицинского изделия при поставке в РФ


Маркировка упаковочной коробки: Катетер баллонный Alwide™ Plus



18 mm 40 mm

Alwide™ Plus Balloon Catheter

Catèter balón; Cateter Balão; Катетер баллонный :

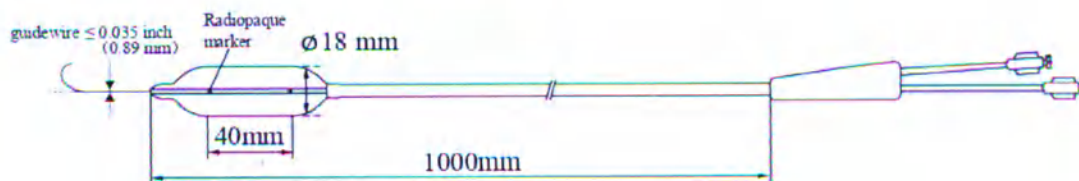

REF BC-1840

LOT



	Pressure (atm/kPa)	Diameter (mm)
Nominal	4.0/405.2	18.00
RBP	7.0/709.1	19.00

Shanghai MicroPort CardioFlow Medtech Co., Ltd.
Alwide™ Plus Balloon Catheter



(01) 0 6971493 53201 6



(17) 241110 (10) 92010001 (91) 001

Model: BC-1840
 18 mm × 40 mm



LOT

Shanghai MicroPort CardioFlow Medtech Co., Ltd.
Alwide™ Plus Balloon Catheter



(01) 0 6971493 53201 6



(17) 241110 (10) 92010001 (91) 001

Model: BC-1840
 18 mm × 40 mm



LOT



See Details in IFU !



Shanghai MicroPort CardioFlow Medtech Co., Ltd.
 Add: Room 1002, Area A and Area B of G Floor (Nominal Floor G Floor,
 Actual Floor 1 Floor), Area A of Second Floor (Nominal Floor 2 Floor,
 Actual Floor 3 Floor), Building 1, 1601 Zhangdong Road, Shanghai Free
 Trade Pilot Area, China


A-XT0019-001 Rev 1



18 mm 40 mm

Alwide™ Plus Balloon Catheter

Catéter balón; Cateter Balão; Катетер баллонный ;

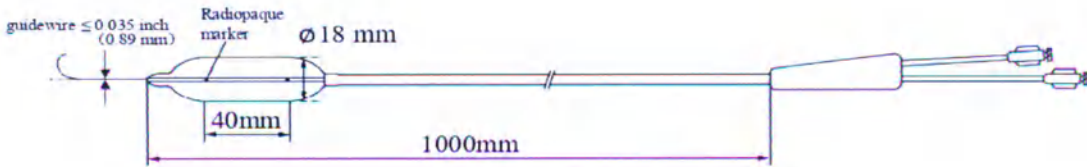

REF BC-1840

LOT



	Pressure (atm/kPa)	Diameter (mm)
Nominal	4.0/405.2	18.00
RBP	7.0/709.1	19.00



REF BC-1840



Alwide™ Plus Balloon Catheter



A-XI0019-002 Rev.1

Shanghai MicroPort CardioFlow Medical Co., Ltd.
Add: Room 1002, Area A and Area B of C Floor, Optical Floor C Floor, Actual Floor 1 Floor, Area A of Second Floor Optical
Floor 2 Floor, Actual Floor 3 Floor, Building 1, 1601 Zhongyuan Road, Shanghai Free Trade Pilot Area, China


See Details in IFU !



Shanghai MicroPort CardioFlow Medical Co., Ltd. Alwide™ Plus Balloon Catheter Model: BC-1840 18 mm × 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT	Shanghai MicroPort CardioFlow Medical Co., Ltd. Alwide™ Plus Balloon Catheter Model: BC-1840 18 mm × 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT
Shanghai MicroPort CardioFlow Medical Co., Ltd. Alwide™ Plus Balloon Catheter Model: BC-1840 18 mm × 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT	Shanghai MicroPort CardioFlow Medical Co., Ltd. Alwide™ Plus Balloon Catheter Model: BC-1840 18 mm × 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT

Alwide™ Plus Balloon Catheter
Catéter balón; Cateter Balão; Баллонный катетер;

18 mm 40 mm



Стикер для маркировки продукции при поставке в РФ
(место нанесения: упаковочная коробка):

Катетер баллонный Alwide™ Plus

НЕТОКСИЧНО, СТЕРИЛЬНО, АПИРОГЕННО

Условия хранения: +15°C до +25°C. Относительная влажность
воздуха: до 80%. Атмосферное давление: 900 гПа– 1100 гПа.

РУ №__ от ЧЧ.ММ.ГГГГ. Срок действия: Бессрочно.

Всего прошито, пронумеровано
и скреплено печатью 12 листов
Подпись 

«УТВЕРЖДАЮ»
Генеральный директор
ООО "ЭТС-ПРО"

А.А. Копчинский

«06» февраля 2023 г.

М.П.



МАКЕТЫ МАРКИРОВКИ МЕДИЦИНСКОГО ИЗДЕЛИЯ ПРИ ПОСТАВКЕ В РФ


Катетер баллонный Alwide™ Plus

(редакция 1.0)



18 mm 40 mm

Alwide™ Plus Balloon Catheter
Catéter balón; Cateter Balão; Катетер баллонный ;

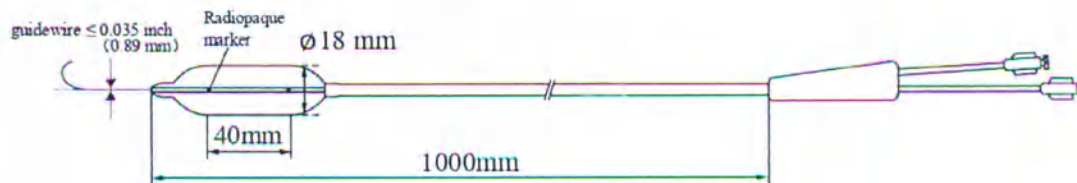

REF BC-1840

LOT



	Pressure (atm/kPa)	Diameter (mm)
Nominal	4.0/405.2	18.00
RBP	7.0/709.1	19.00

Shanghai MicroPort CardioFlow Medtech Co., Ltd.
Alwide™ Plus Balloon Catheter



(01) 0 6971493 33201 6



(17) 241110 (10) 92010001 (91) 001

Model: BC-1840
18 mm × 40 mm



LOT

Shanghai MicroPort CardioFlow Medtech Co., Ltd.
Alwide™ Plus Balloon Catheter



(01) 0 6971493 33201 6



(17) 241110 (10) 92010001 (91) 001

Model: BC-1840
18 mm × 40 mm



LOT



See Details in IFU¹




Shanghai MicroPort CardioFlow Medtech Co., Ltd.
Add: Room 1002, Area A and Area B of G Floor (Nominal Floor G Floor,
Actual Floor 1 Floor), Area A of Second Floor (Nominal Floor 2 Floor,
Actual Floor 3 Floor), Building 1, 1601 Zhangdong Road, Shanghai Free
Trade Pilot Area, China

A-XT0019-001 Rev: 1



18 mm 40 mm

Alwide™ Plus Balloon Catheter
Catéter balón; Cateter Balão; Катетер баллонный ;

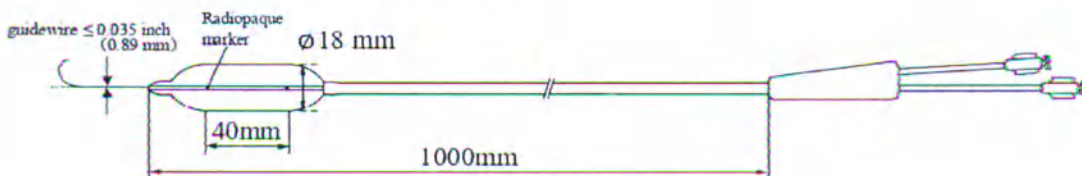

REF BC-1840

LOT



	Pressure (atm/kPa)	Diameter (mm)
Nominal	4.0/405.2	18.00
RBP	7.0/709.1	19.00



REF BC-1840



Alwide™ Plus Balloon Catheter



A-XI0019-002 Rev.1


Shanghai MicroPort CardioFlow Medtech Co., Ltd.
Add: Room 1002, Area A and Area B of C Floor (Nominal) Floor C Floor, Actual Floor 1 Floor, Area A of 5 second Floor (Nominal)
Floor 2 Floor, Actual Floor 3 Floor, Building 1, 1001 Zhenyuan Road, Shanghai Free Trade Area, China

See Details in IFU !



Shanghai MicroPort CardioFlow Medtech Co., Ltd. Model: BC-1840 18 mm x 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT Alwide™ Plus Balloon Catheter	Shanghai MicroPort CardioFlow Medtech Co., Ltd. Model: BC-1840 18 mm x 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT Alwide™ Plus Balloon Catheter
Shanghai MicroPort CardioFlow Medtech Co., Ltd. Model: BC-1840 18 mm x 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT Alwide™ Plus Balloon Catheter	Shanghai MicroPort CardioFlow Medtech Co., Ltd. Model: BC-1840 18 mm x 40 mm (01) 0 6971493 53201 6 (17) 241110 (10) 92010001 (91) 001 LOT Alwide™ Plus Balloon Catheter

Alwide™ Plus Balloon Catheter
Catéter balón; Cateter Balão; Баллонный катетер;



18 mm 40 mm

Стикер для маркировки продукции при поставке в РФ
(место нанесения: упаковочная коробка):

Катетер баллонный Alwide™ Plus

НЕТОКСИЧНО, СТЕРИЛЬНО, АПИРОГЕННО

Условия хранения: +15°C до +25°C. Относительная влажность
воздуха: до 80%. Атмосферное давление: 900 гПа– 1100 гПа.

РУ №__ от ЧЧ.ММ.ГГГГ. Срок действия: Бессрочно.

Всего прошито, пронумеровано
и скреплено печатью 4 листов
Подпись _____

