


«УТВЕРЖДАЮ»

**Генеральный директор
ООО «СП-КАРДИО»**


Шеенков В.В.
_____ 2024 г.




Фотографические изображения

медицинского изделия

Индефлятор для баллонного катетера

производства


**Shanghai Kindly Medical Instruments Co., Ltd., Китай
(Шанхай Кайндли Медикал Инструментс Ко., Лтд.)**

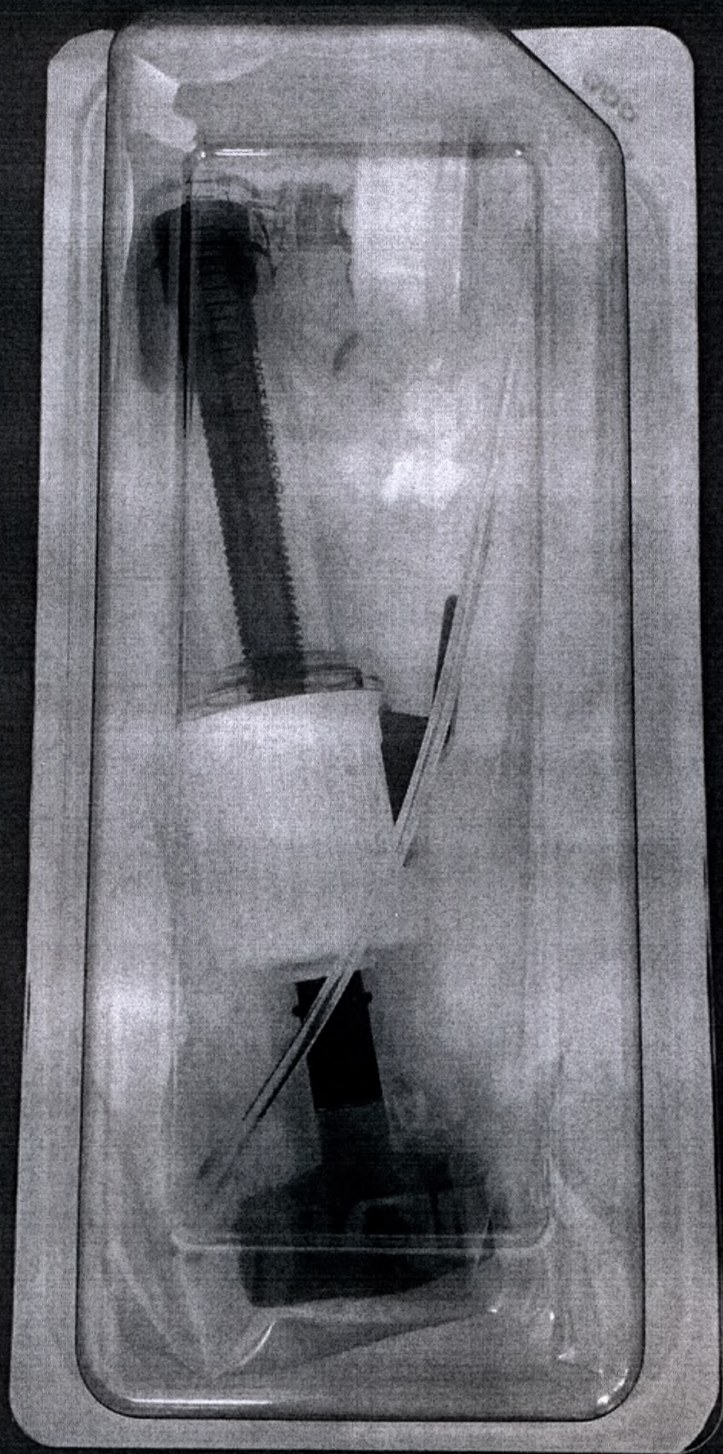


Индефлятор для баллонного катетера AI25 / AI25A в индивидуальной упаковке




Индефлятор для баллонного катетера AI25

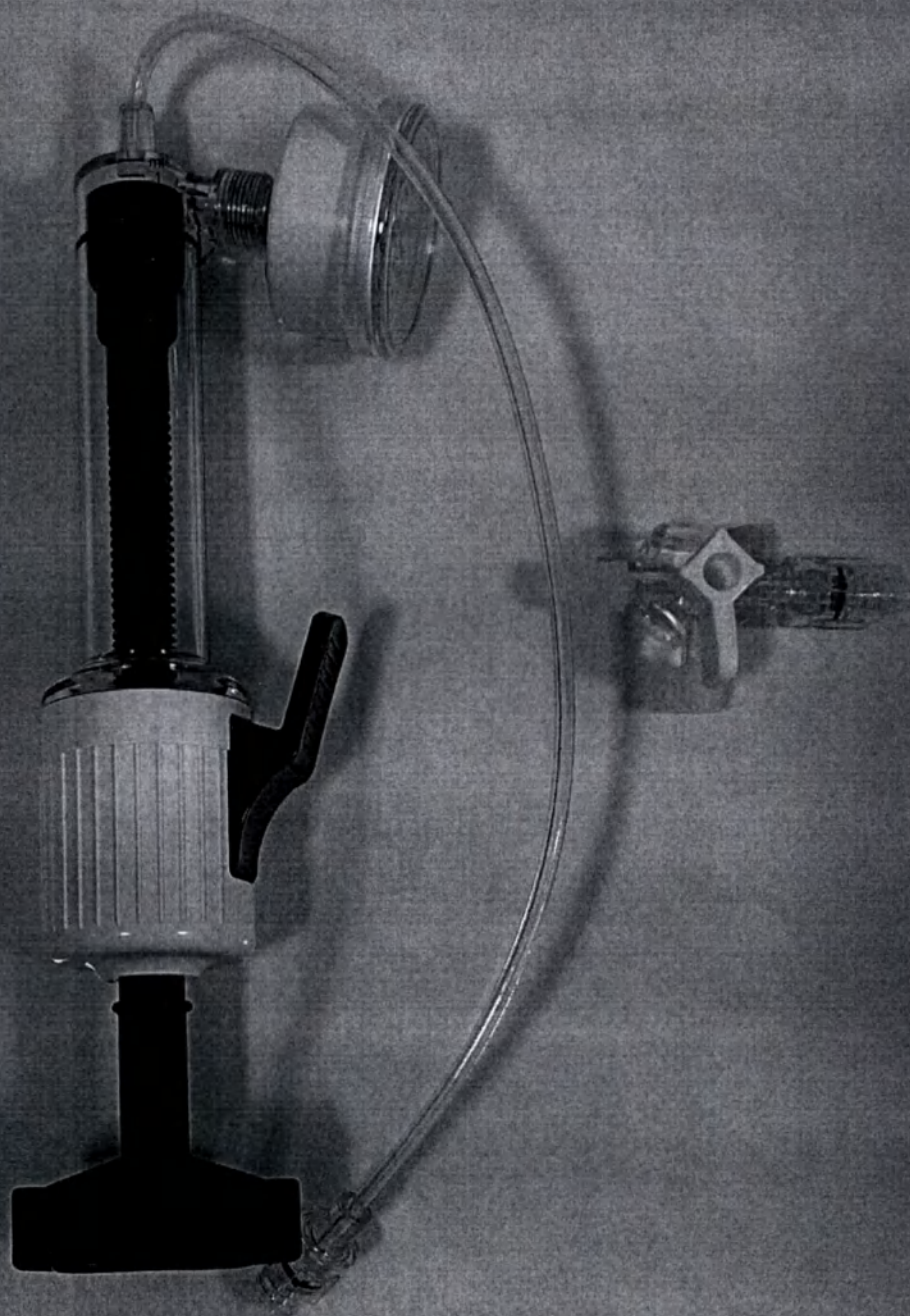



Индефлятор для баллонного катетера AI25

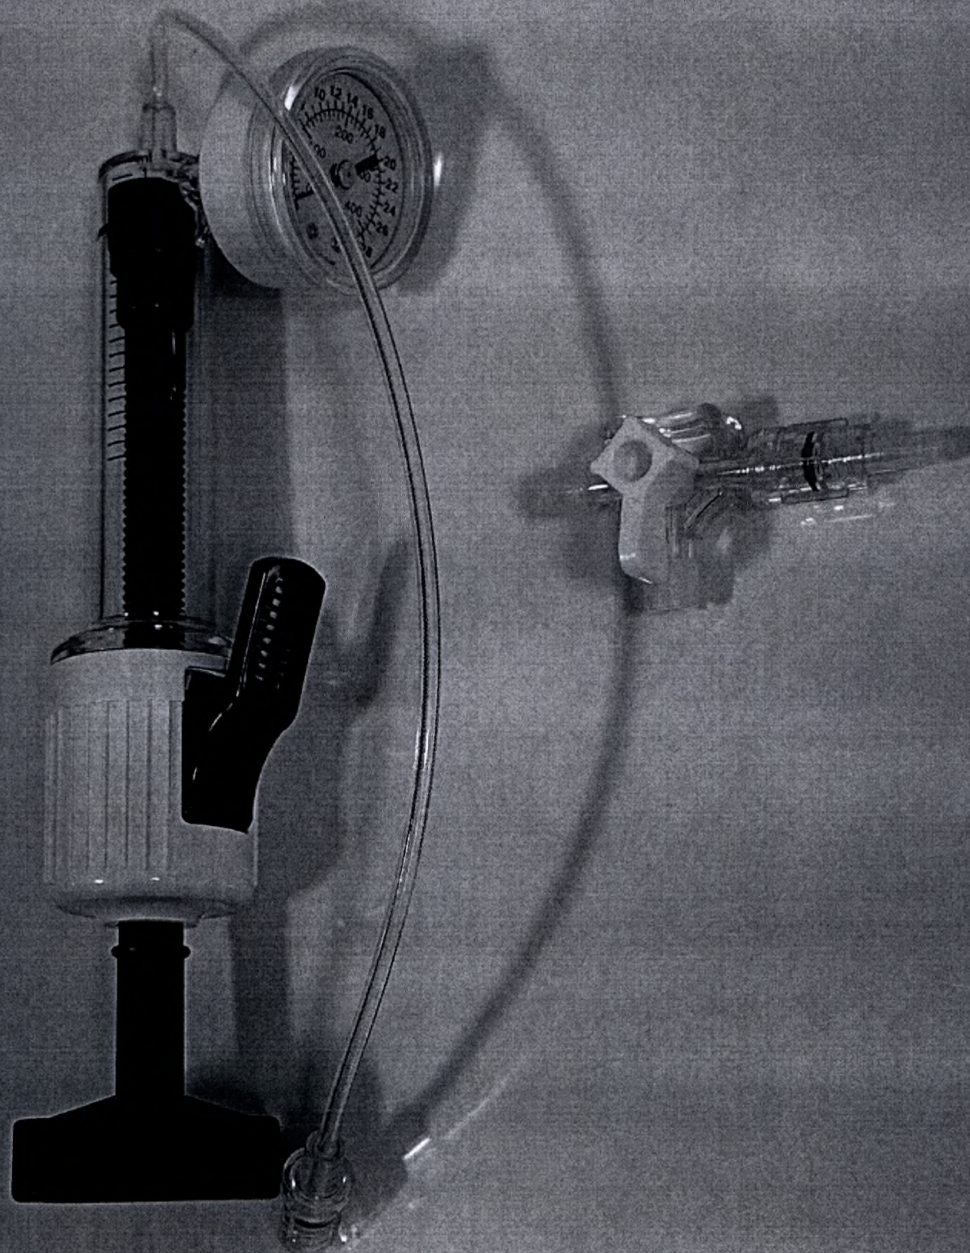


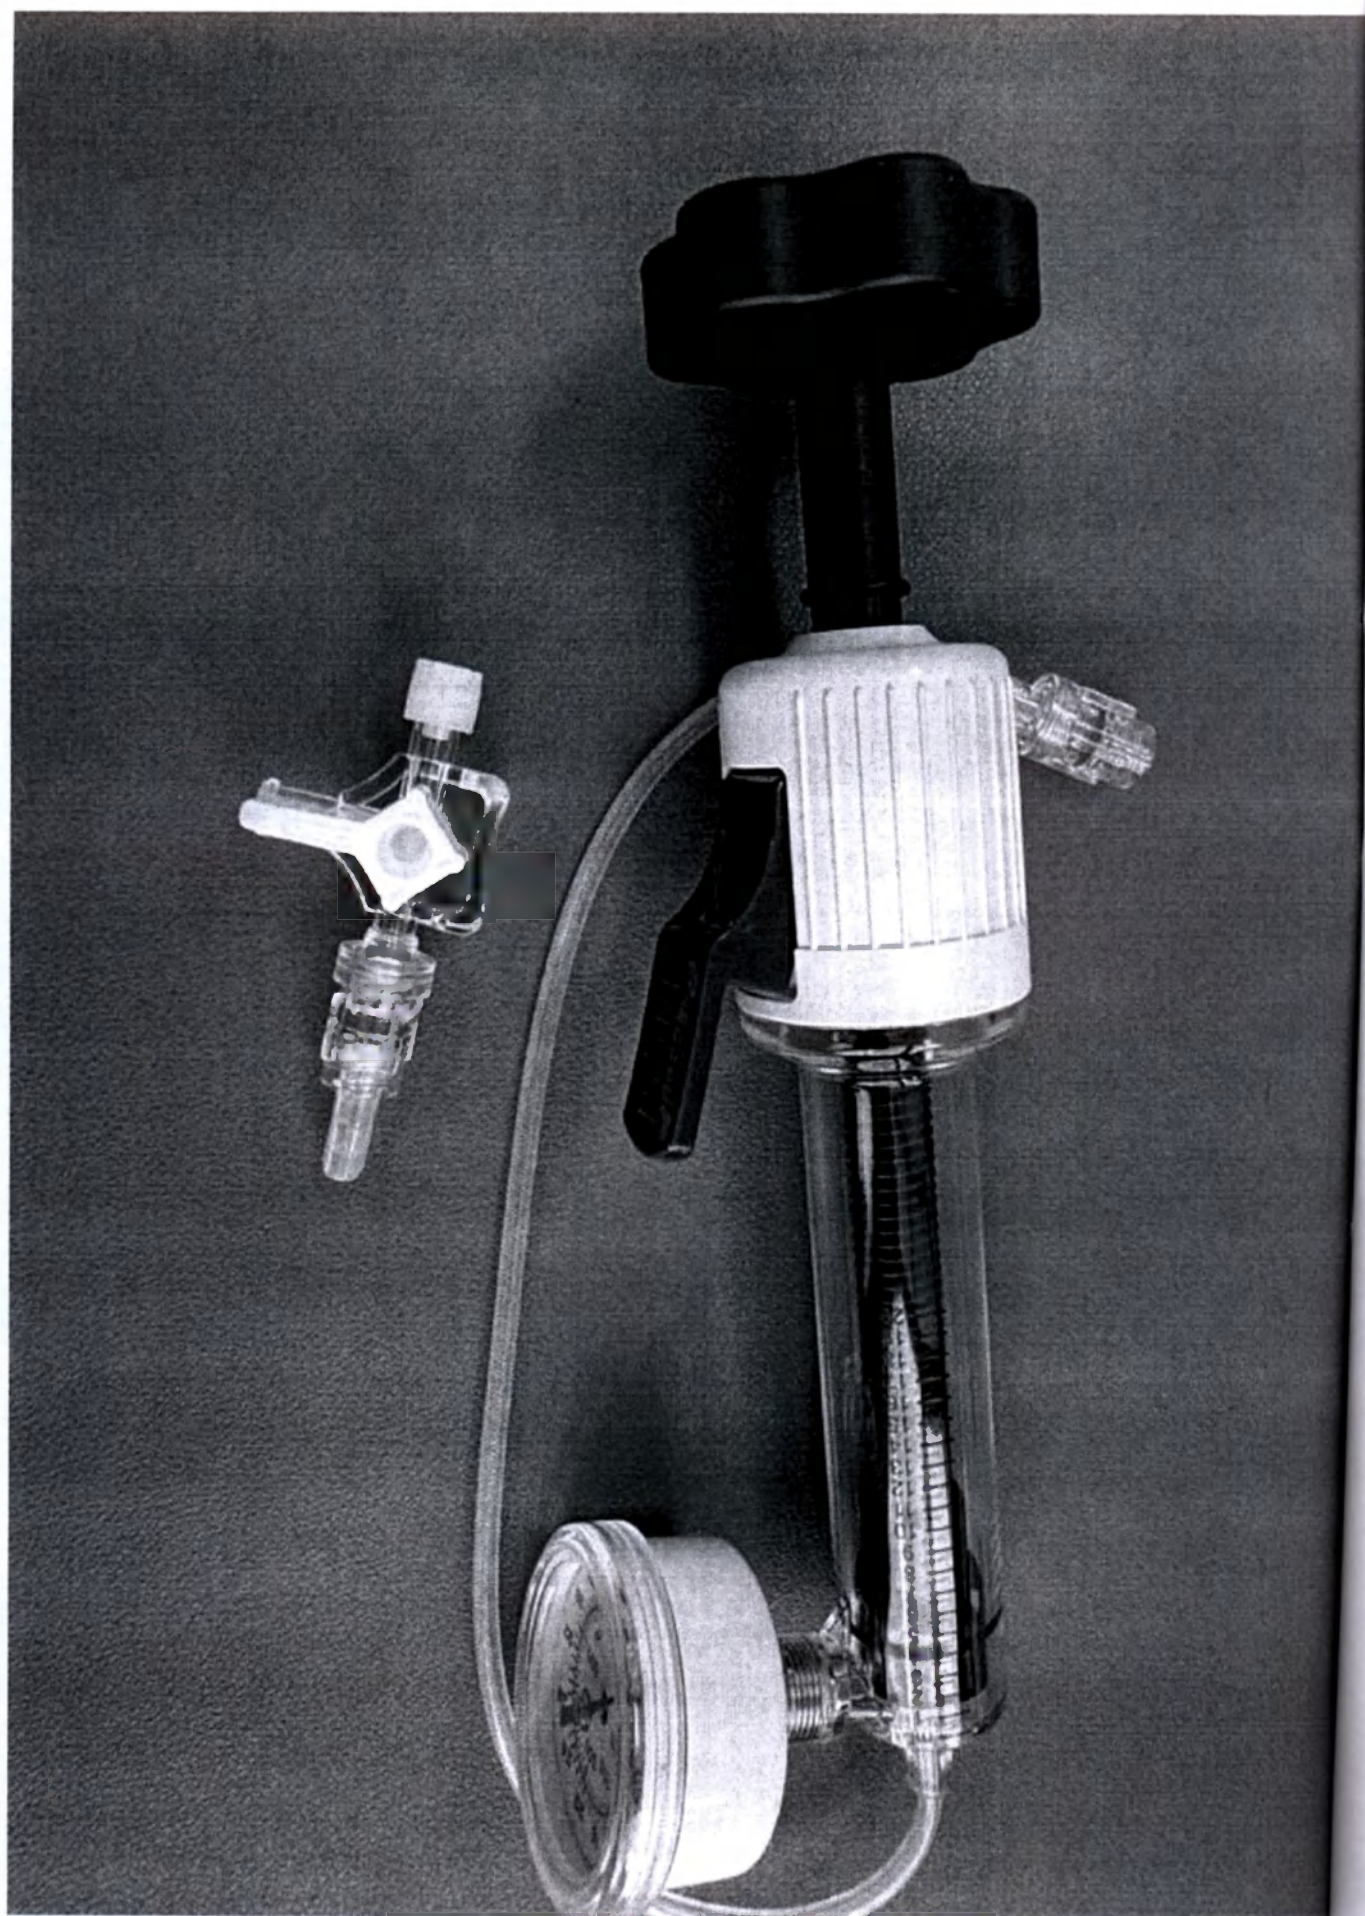


Индефлятор для баллонного катетера AI25A

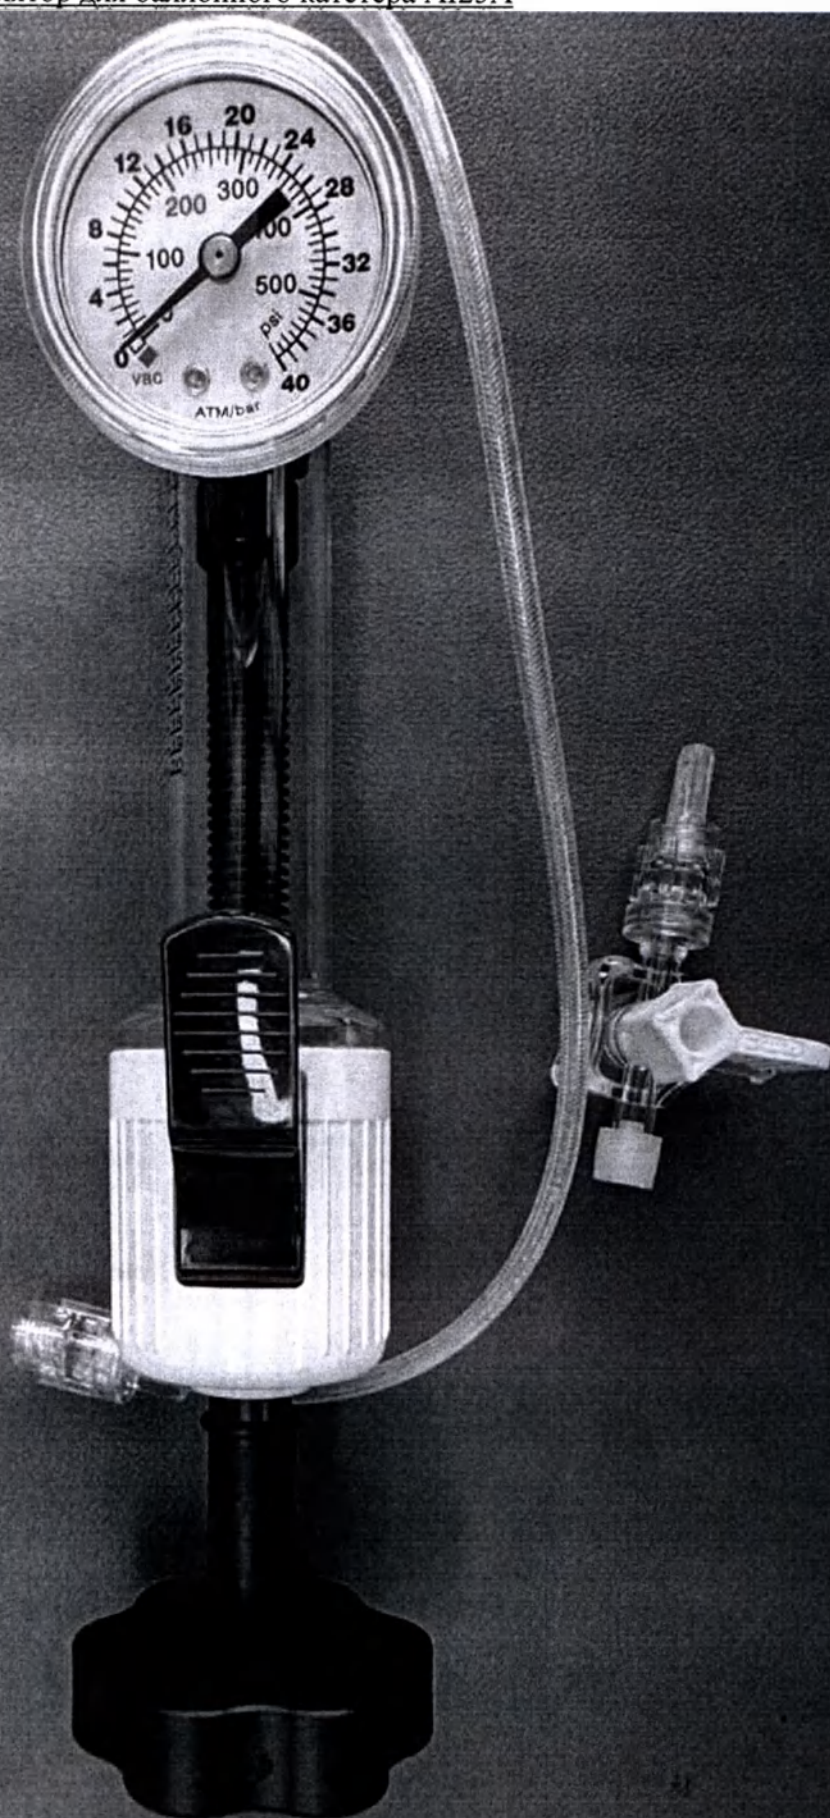


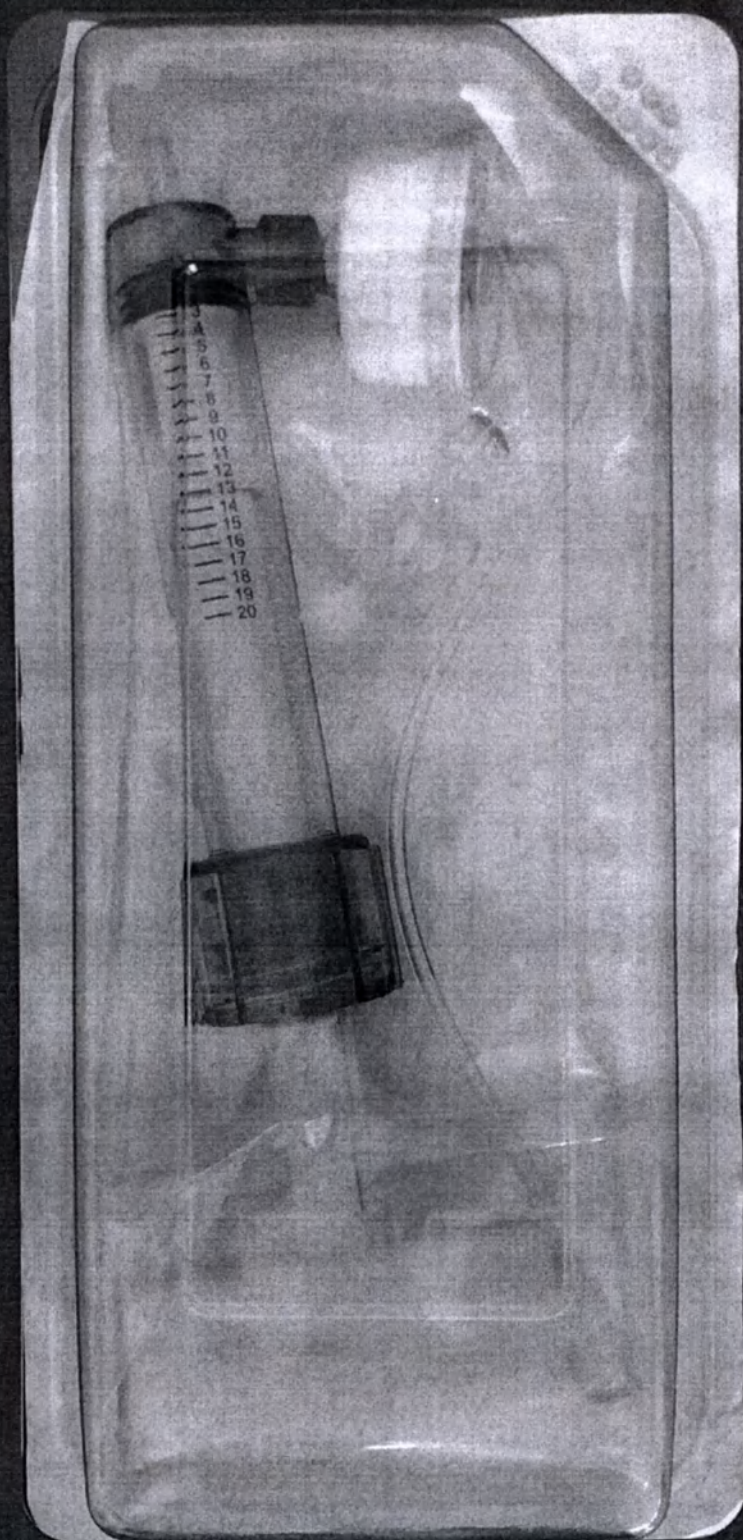

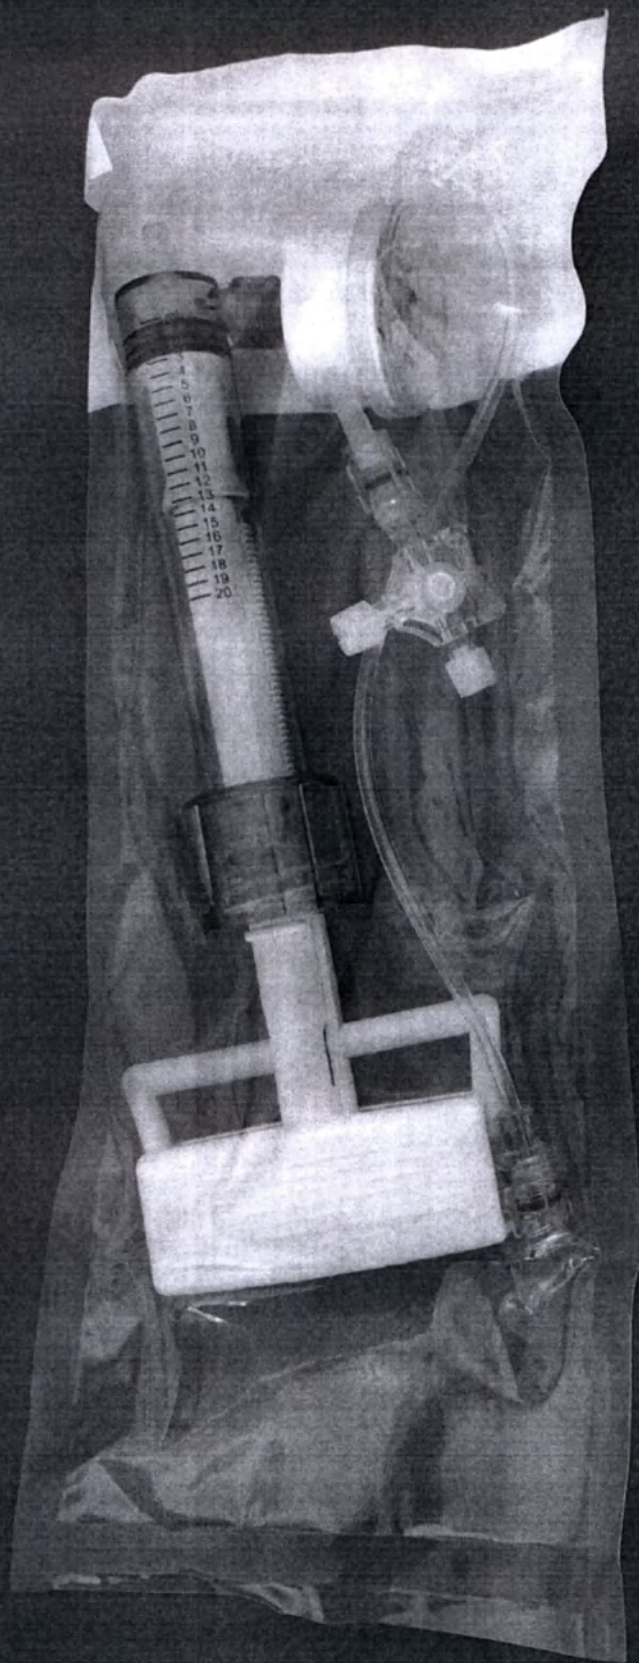


Индефлятор для баллонного катетера AI30

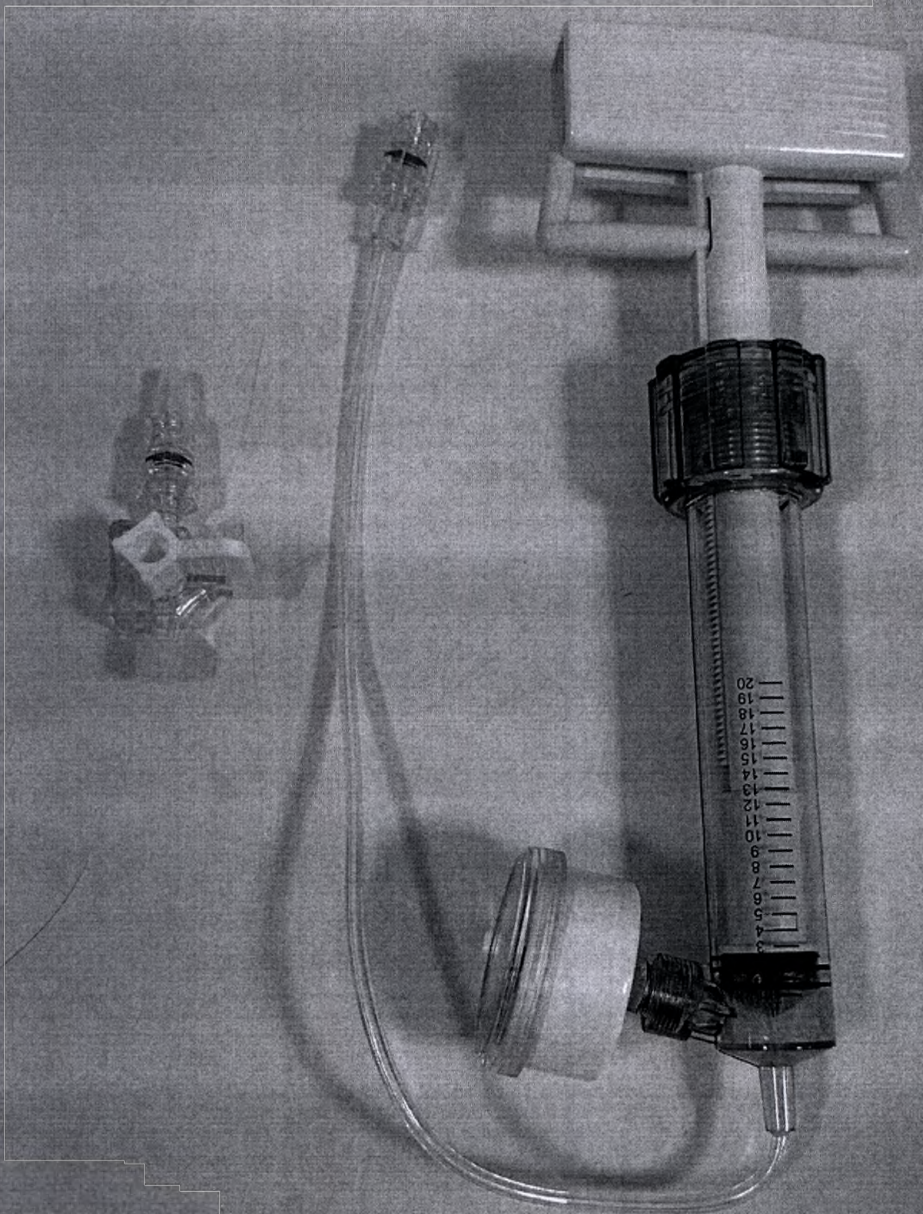

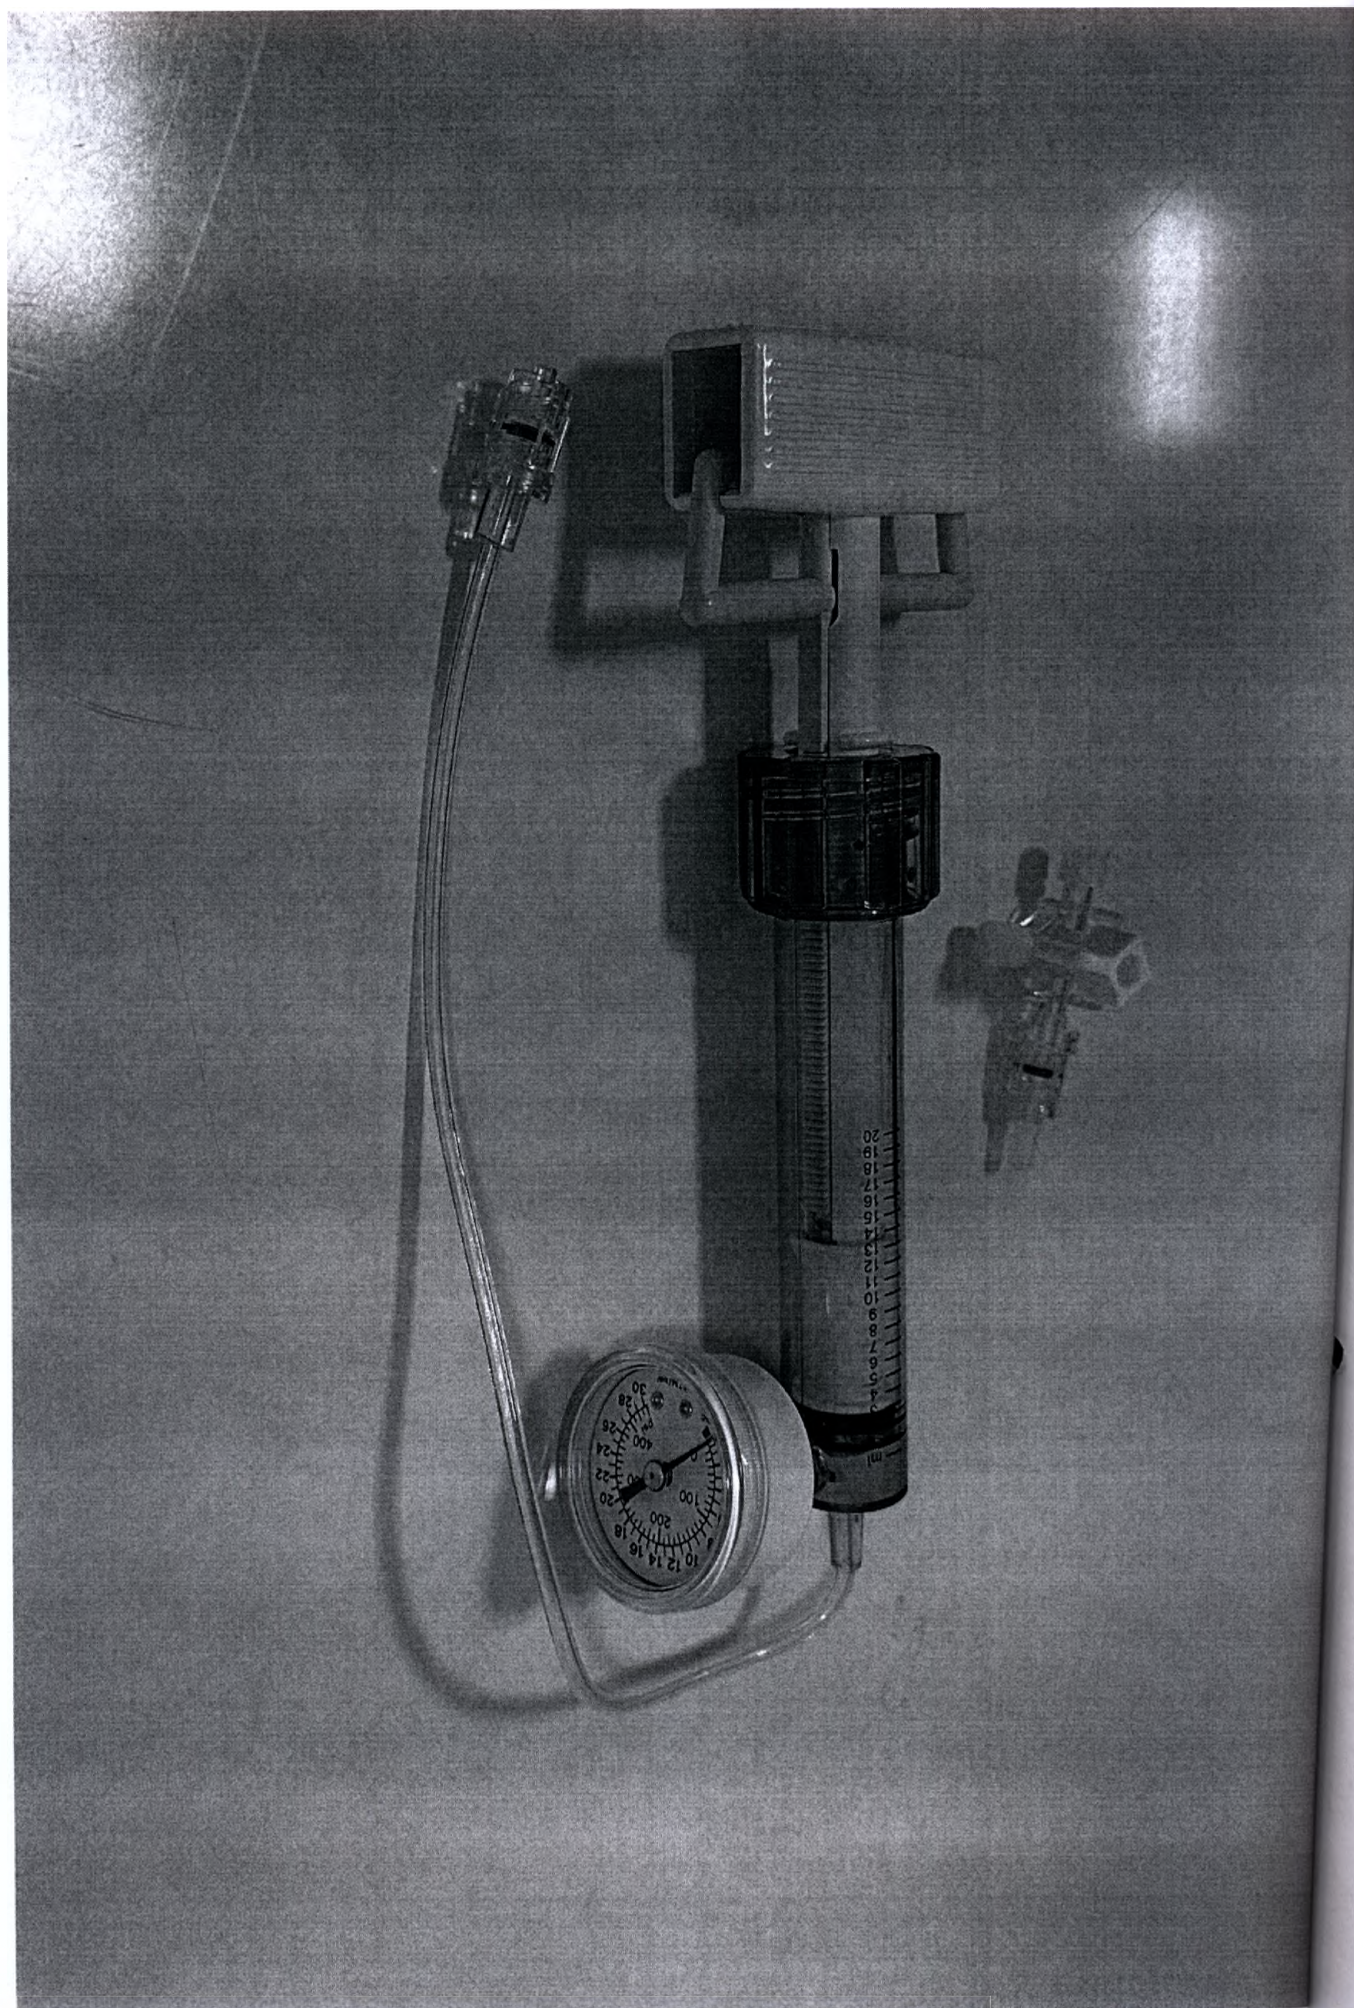


Индификатор для баллонного катетера А130


Индефлятор для баллонного катетера AI40

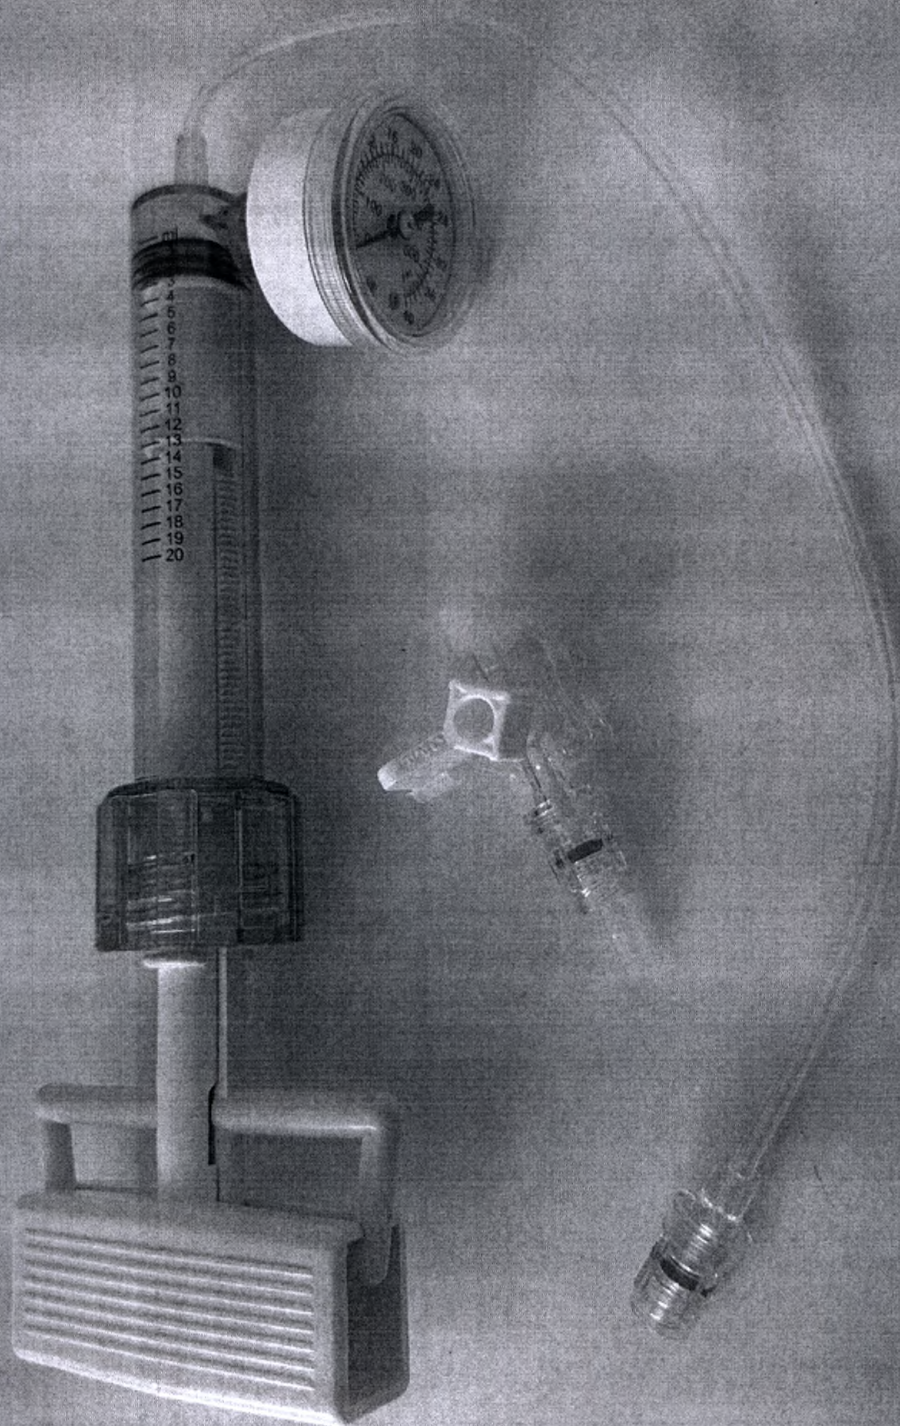


Шкала манометра индифляторов 30 атм

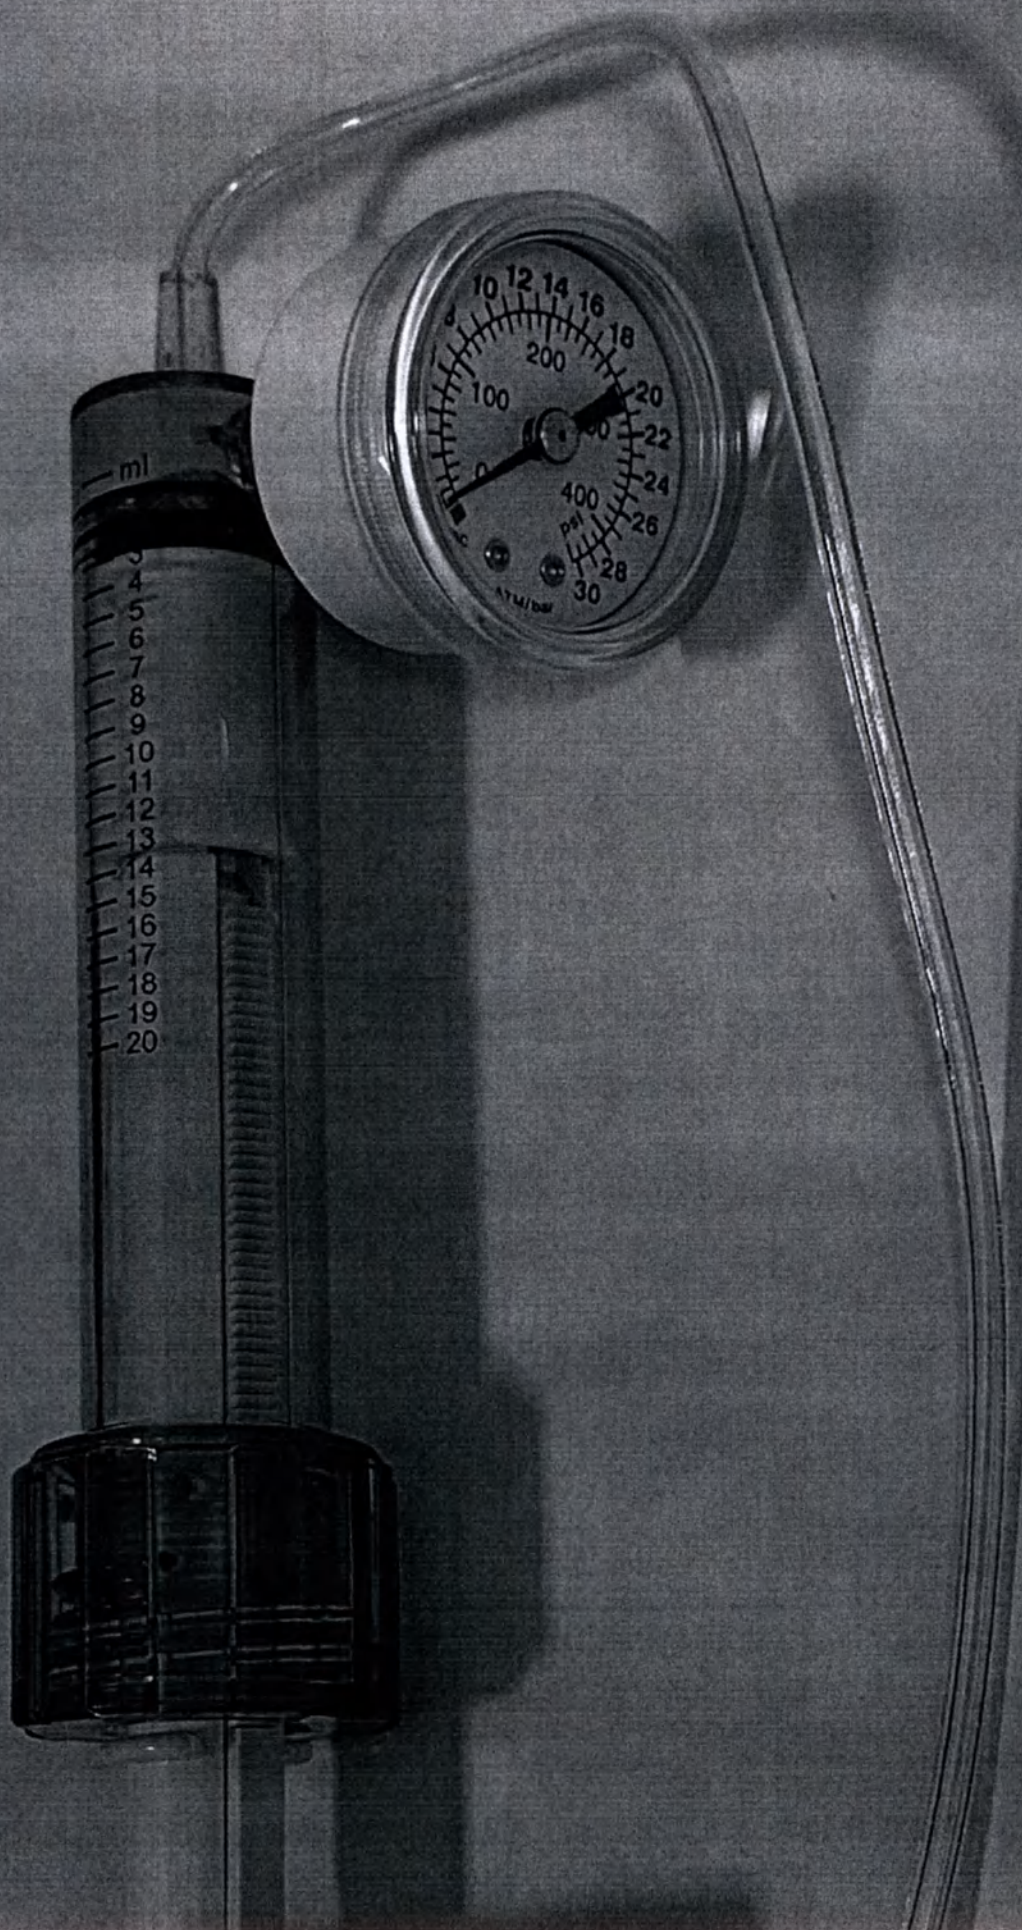


Шкала манометра индифляторов 40 атм

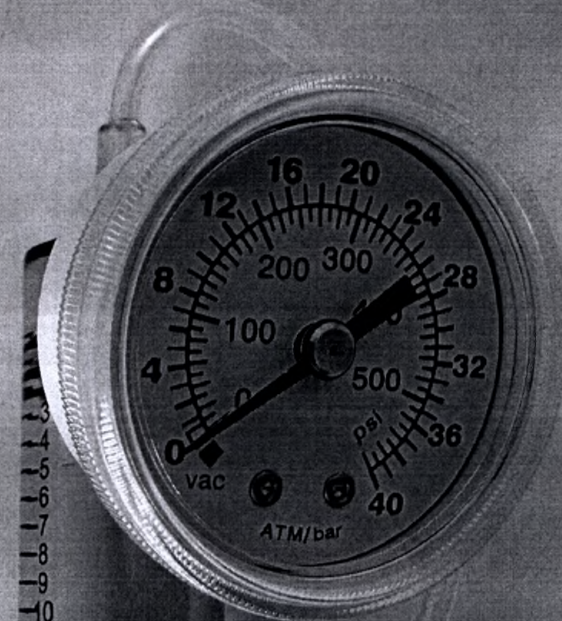



STERILE
INFLATION DEVICE
FOR SINGLE USE

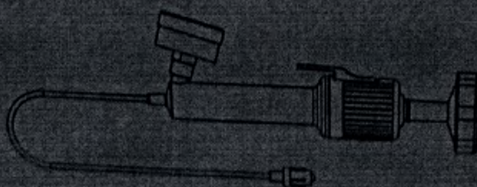

CE 0123

STERILE EO

Rev. 08/2022




Shanghai Kindly Medical Instruments Co., Ltd
Addr: No.925 Jinyuan yi Road, 201803 Shanghai, P.R.C.
Tel: +86-21-59140056




Shanghai International Holding Corp. GmbH (Europe)
Addr: Eilffestraße 80, 20537 Hamburg Germany
Tel: 0049-40-2613175

MADE IN CHINA



STERILE
INFLATION DEVICE
FOR SINGLE USE

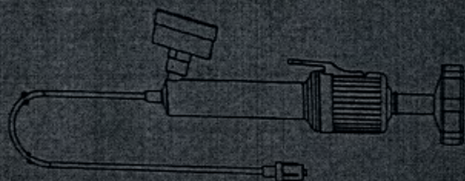

Rev. 08/2022

CE 0123

STERILE EO



Shanghai Kindly Medical Instruments Co., Ltd.
Addr: No. 925 Jinyuan yi Road, 201803 Shanghai, P.R. C.
Tel: +86-21-59140056



Shanghai International Holding Corp. GmbH (Europe)
Addr: Eiffestraße 80, 20537 Hamburg Germany
Tel: 0049-40-2513175

MADE IN CHINA



STERILE
INFLATION DEVICE
FOR SINGLE USE



30 ATM



(01) 06950900920011(17) 240427(11) 210428(10) 20210428

REF / CAT : AI30

MFG. DATE :

LOT LOT NO.:

EXP. DATE:

Warning

Re-use of single-use devices creates a potential risk of patient or user. It may lead to contamination and/or impairment of functional capability. Contamination and/or limited functionality of the device may lead to injury, illness or death of the patient.

STERILE EO

Sterilized using
ethylene oxide

CE 0123

2 Do not re-use

Do not use if package
is damaged



Shanghai Kindly Medical Instruments Co., Ltd.
Addr: No. 925 Jinyuan yi Road, 201803 Shanghai, P.R. C.
Tel: +86 21 59140056

EC REP

Shanghai International Holding Corp GmbH(Europe)
Addr: Eiffestraße 80, 20537 Hamburg Germany
Tel: 0049-40-2513175

MADE IN CHINA



STERILE
INFLATION DEVICE
FOR SINGLE USE



TYPE: AI25 (30atm)



06950900920011(17) 240427(11) 210428(10) 20210428

REF / CAT : AI25

MFG. DATE :

LOT LOT NO.:

EXP. DATE:

STERILE EO

Sterilized using
ethylene oxide



Do not use if package
is damaged



Do not re-use



Caution
consult the
instructions for use



0123

Warning

Re-use of single-use devices creates a potential risk of patient or user. It may lead to contamination and/or impairment of functional capability. Contamination and/or limited functionality of the device may lead to injury, illness or death of the patient.





Shanghai Kindly Medical Instruments Co., Ltd.
Addr: No.925 Jinyuan yi Road,201803 Shanghai,P.R.C.
Tel: +86- 21-59140056

EC REP

Shanghai International Holding Corp.GmbH(Europe)
Addr: Eiffestraße 80,20537 Hamburg Germany
Tel:0049-40-2513175

 STERILE INFLATION DEVICE FOR SINGLE USE   CE 0123 STERILE EO 2 Shanghai Kindly Medical Instruments Co., Ltd. Addr: No. 925 Jinyuan yi Road, 201803 Shanghai, P. R. C. Tel: +86 21 59140056 Shanghai International Holding Corp. GmbH(Europe) Addr: Eiffelstraße 80, 20537 Hamburg Germany Tel: 0049-40-2513175 EC REP	TYPE: AI25 (30atm) <table border="1"> <tr> <td>REF / CAT</td> <td>AI25</td> </tr> <tr> <td>LOT LOT NO</td> <td></td> </tr> <tr> <td>MFG. DATE</td> <td></td> </tr> <tr> <td>EXP. DATE</td> <td></td> </tr> <tr> <td>QTY.:</td> <td>5 pcs</td> </tr> </table> Rev: 02/2017	REF / CAT	AI25	LOT LOT NO		MFG. DATE		EXP. DATE		QTY.:	5 pcs	 STERILE INFLATION DEVICE FOR SINGLE USE   CE 0123 STERILE EO 2 Shanghai Kindly Medical Instruments Co., Ltd. Addr: No. 925 Jinyuan yi Road, 201803 Shanghai, P. R. C. Tel: +86 21 59140056 Shanghai International Holding Corp. GmbH(Europe) Addr: Eiffelstraße 80, 20537 Hamburg Germany Tel: 0049-40-2513175 EC REP	Caution: • Sterile. Non-pyrogenic. • Do not use if the package is open or damaged. • Do not store at extreme temperature. • Keep away from getting wet. • For single use only. discard after use. Warning: Re-use of single-use devices creates a potential risk of patient or user. It may lead to contamination and/or impairment of functional capability. Contamination and/or limited functionality of the device may lead to injury, illness or death of the patient.
REF / CAT	AI25												
LOT LOT NO													
MFG. DATE													
EXP. DATE													
QTY.:	5 pcs												

Макет этикетки транспортной коробки

 STERILE INFLATION DEVICE FOR SINGLE USE   CE 0123 STERILE EO 2 Shanghai Kindly Medical Instruments Co., Ltd. Addr: No. 925 Jinyuan yi Road, 201803 Shanghai, P. R. C. Tel: +86 21 59140056 Shanghai International Holding Corp. GmbH(Europe) Addr: Eiffelstraße 80, 20537 Hamburg Germany Tel: 0049-40-2513175 EC REP	Caution: • Sterile. Non-pyrogenic. • Do not use if the package is open or damaged. • Do not store at extreme temperature. • Keep away from getting wet. • For single use only. discard after use. Warning: Re-use of single-use devices creates a potential risk of patient or user. It may lead to contamination and/or impairment of functional capability. Contamination and/or limited functionality of the device may lead to injury, illness or death of the patient.	 STERILE INFLATION DEVICE FOR SINGLE USE   CE 0123 STERILE EO 2 Shanghai Kindly Medical Instruments Co., Ltd. Addr: No. 925 Jinyuan yi Road, 201803 Shanghai, P. R. C. Tel: +86 21 59140056 Shanghai International Holding Corp. GmbH(Europe) Addr: Eiffelstraße 80, 20537 Hamburg Germany Tel: 0049-40-2513175 EC REP	 TYPE: AI25 (30atm) <table border="1"> <tr> <td>REF / CAT</td> <td>AI25</td> </tr> <tr> <td>LOT LOT NO</td> <td></td> </tr> <tr> <td>MFG. DATE</td> <td></td> </tr> <tr> <td>EXP. DATE</td> <td></td> </tr> <tr> <td>QTY.:</td> <td>20 pcs</td> </tr> </table> GROSS WEIGHT: 7.05 kg MEASU: 61 X 30 X 33cm-G: 060cm³	REF / CAT	AI25	LOT LOT NO		MFG. DATE		EXP. DATE		QTY.:	20 pcs
REF / CAT	AI25												
LOT LOT NO													
MFG. DATE													
EXP. DATE													
QTY.:	20 pcs												

Индефлятор для баллонного катетера

Вариант исполнения: _____

Размеры: см. на упаковке.



Стерильно. Апирогенно. Не токсично внутри.

Условия транспортирования и хранения: см. инструкцию по применению.

Меры предосторожности: см. инструкцию по применению.

Расшифровка графических символов: см. инструкцию по применению.

LOT

Код партии: см. на упаковке.



Дата изготовления: см. на упаковке.



Использовать до: см. на упаковке.

Производитель:

Shanghai Kindly Medical Instruments Co., Ltd.

No. 925, Jinyuan Yi Road, 201803, Shanghai, China

Уполномоченный представитель производителя:

Общество с ограниченной ответственностью «СП-КАРДИО» (ООО «СП-КАРДИО»)

107076, Россия, г. Москва, ул. Матросская Тишина, д. 23, стр. 1

Тел: +7 (903) 616-15-71

e-mail: sp_cardio@rambler.ru

Регистрационное удостоверение № РЗН _____ / _____ от _____ 20__ года

Handwritten signature in blue ink.

Пронумеровано, прошито и скреплено печатью
21 (дварчатъ дин) листа(ов).

Генеральный директор
ООО «СП-КАРДИО»

 _____ Шеенков В.В.

