

УТВЕРЖДАЮ

Генеральный директор

ООО «Компания «БиВи»

Т.А. Носова

« 22 » декабря 2023 г.

ПО ДОВЕРЕННОСТИ
УАД 3555614

КУСАЙЛО Р. В.



Фотографические изображения изделия:

**Набор реагентов для количественного определения витамина B12
электрохемилюминесцентным методом на анализаторах ECL для диагностики in vitro
(Vitamin B12 (eCLIA) / Vitamin B12)**

«Shenzhen Lifotronic Technology Co., Ltd.»
(«Шэньчжэнь Лайфотроник Технолоджи Ко., Лтд.»), Китай

QC Pass

Lifotronic

Vitamin B12 (eCLIA)


Components	
Control Material (High)	1×2.0 mL
Control Material (Low)	1×2.0 mL
Calibrator (High)	1×1.0 mL
Calibrator (Low)	1×1.0 mL
MB	1×3.5 mL
RB	1×4.0 mL
RA	1×7.5 mL
RD	1×2.0 mL

P/N: 03-R05B840-00001

REF 0320500208

LOT A042300100


2025-01-27

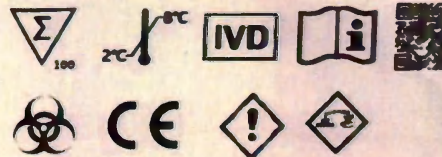


Shenzhen Lifotronic Technology Co., Ltd.
Unit A, 4th Floor, Building 15, Yijing Estate, No.1008, Songhai Road, Nanshan District, Shenzhen City,
Guangdong Province, 518055 P.R. China

BC REP


Shanghai International Holding Corp GmbH (Europe)
Edifício 80, 20537 Hamburg, Germany
Tel: +49-40-2513175 Fax: +49-40-255726



(01) 0 6975984 00253.2
(17) 250127
(10) A042300100

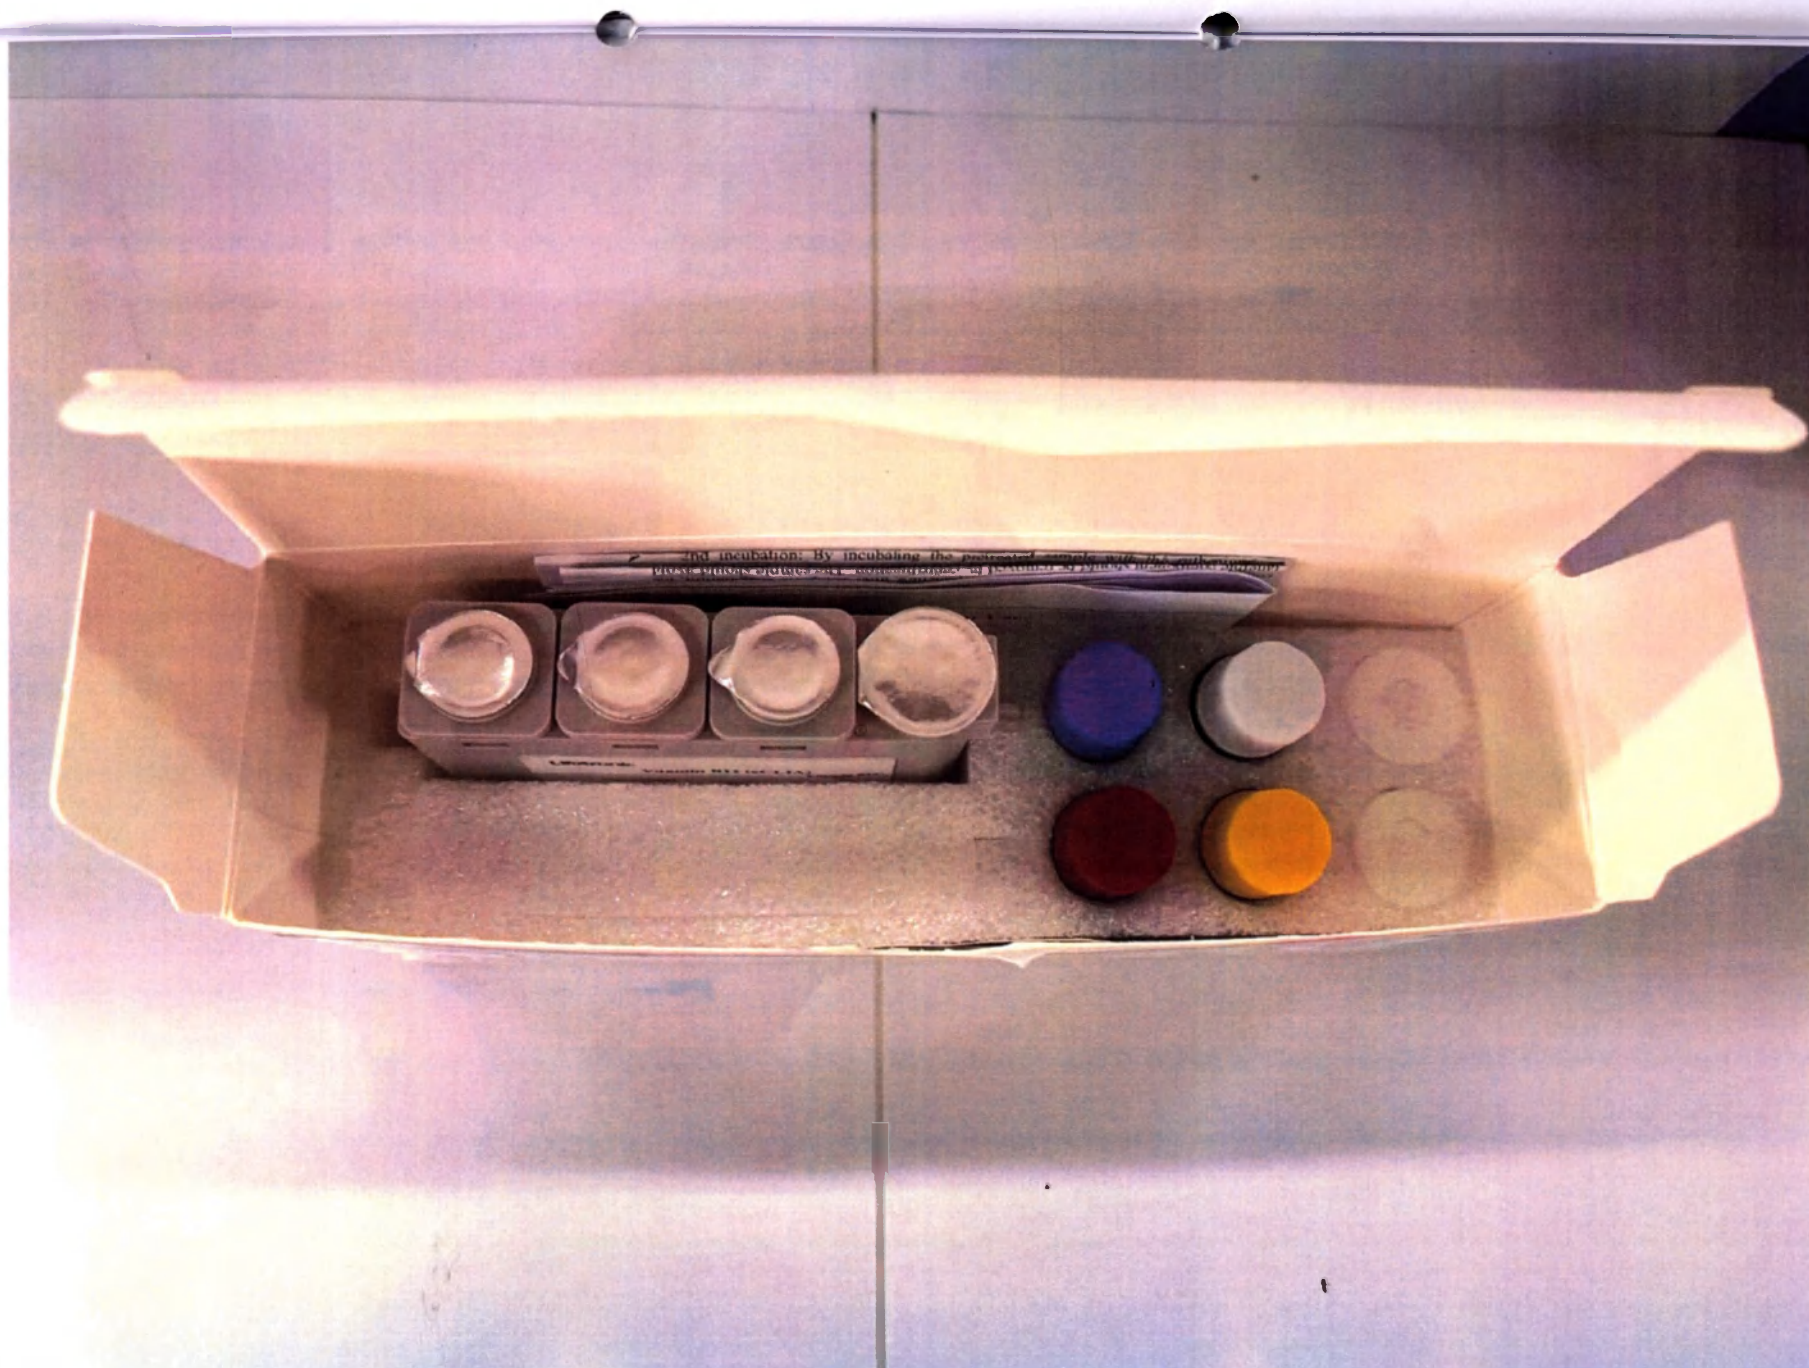


Набор реагентов для количественного определения витамина B12 электрохемилюминесцентным методом на анализаторах ECL для диагностики in vitro (Vitamin B12 (eCLIA) / Vitamin B12), в варианте исполнения 100 тестов

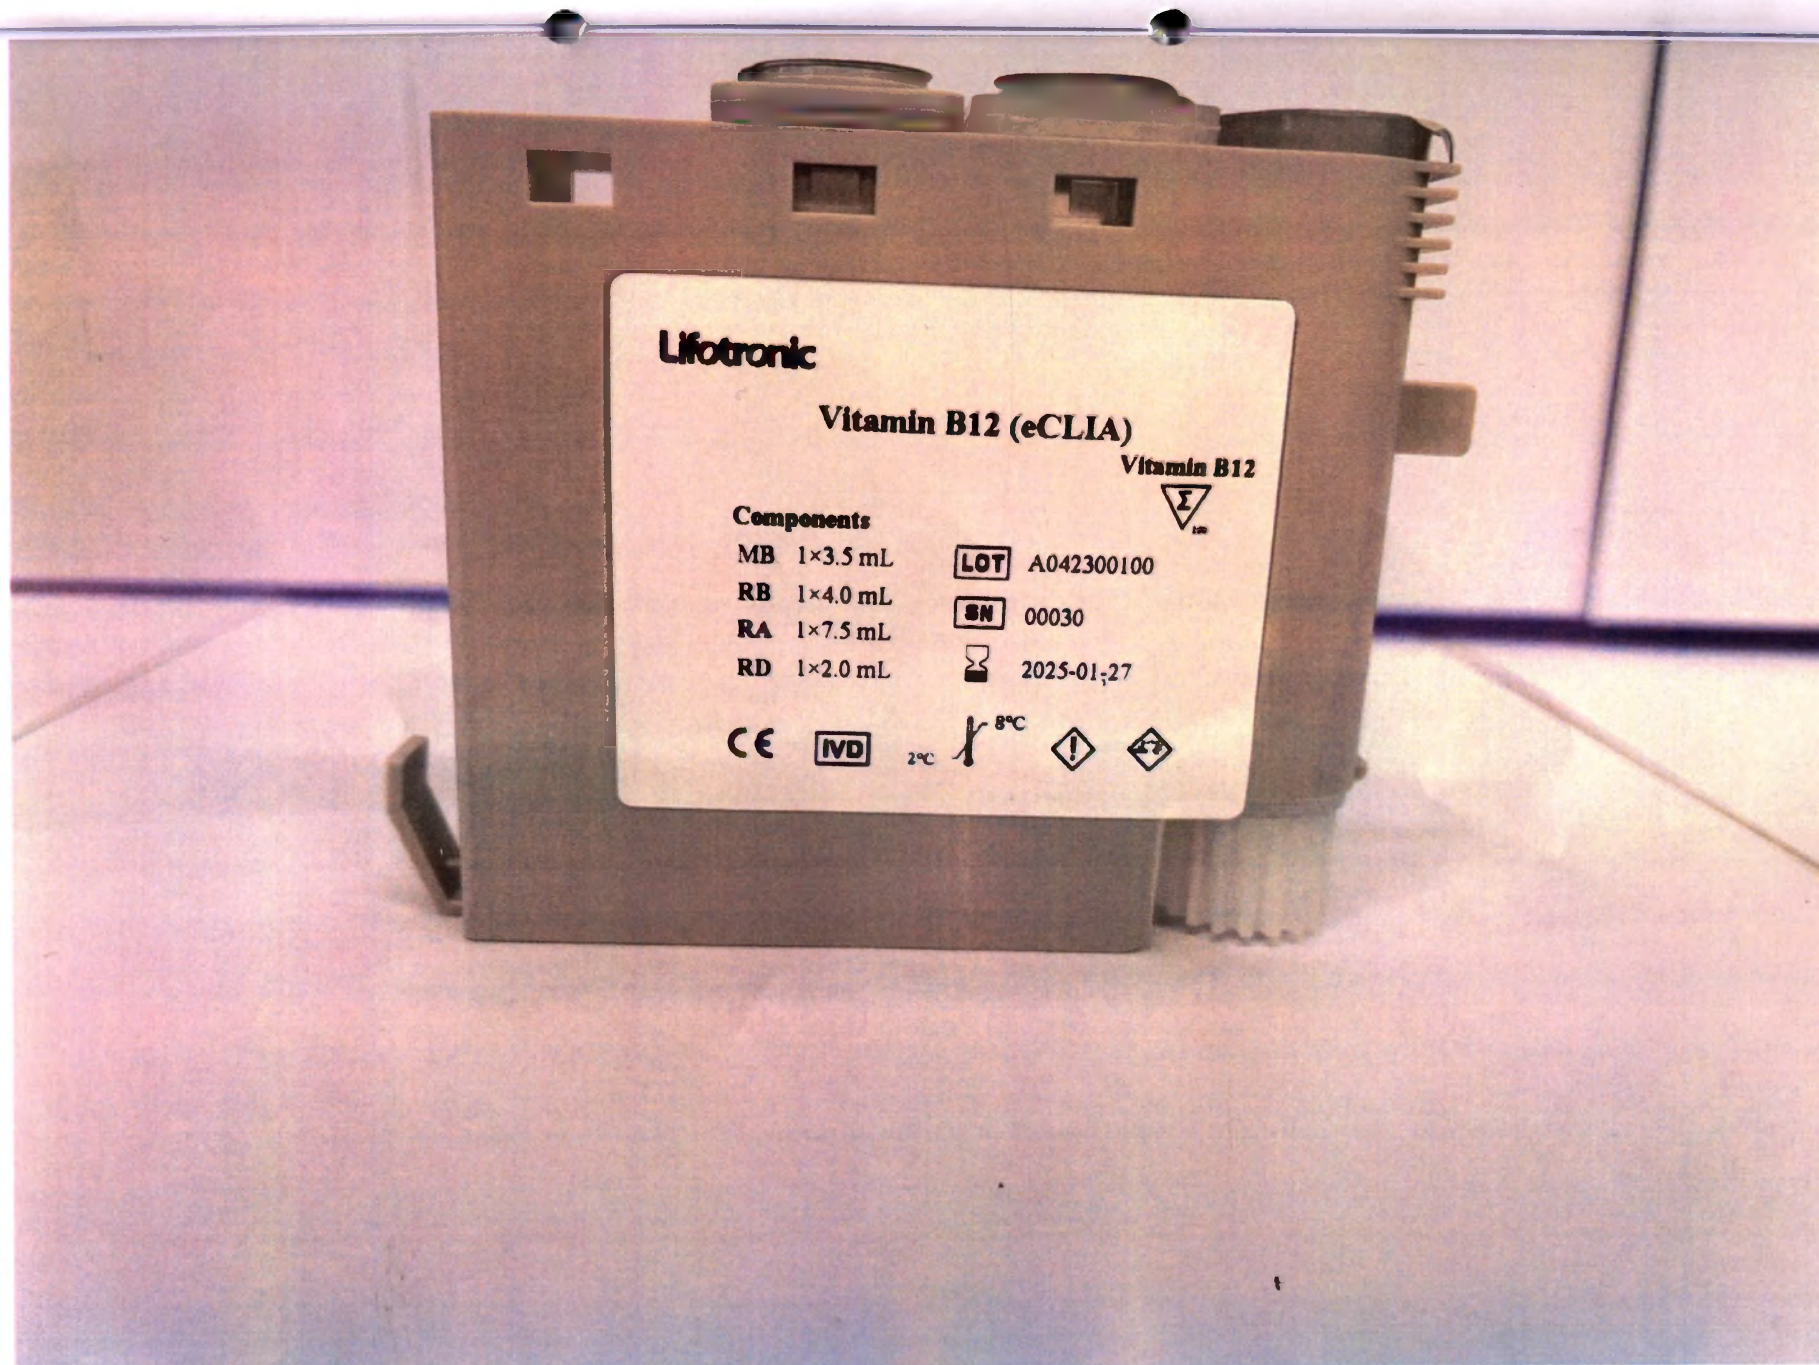

Кассета с реагентами



Калибратор (низкий уровень), Калибратор (высокий уровень), Материал контрольный (высокий уровень), Материал контрольный (низкий уровень)

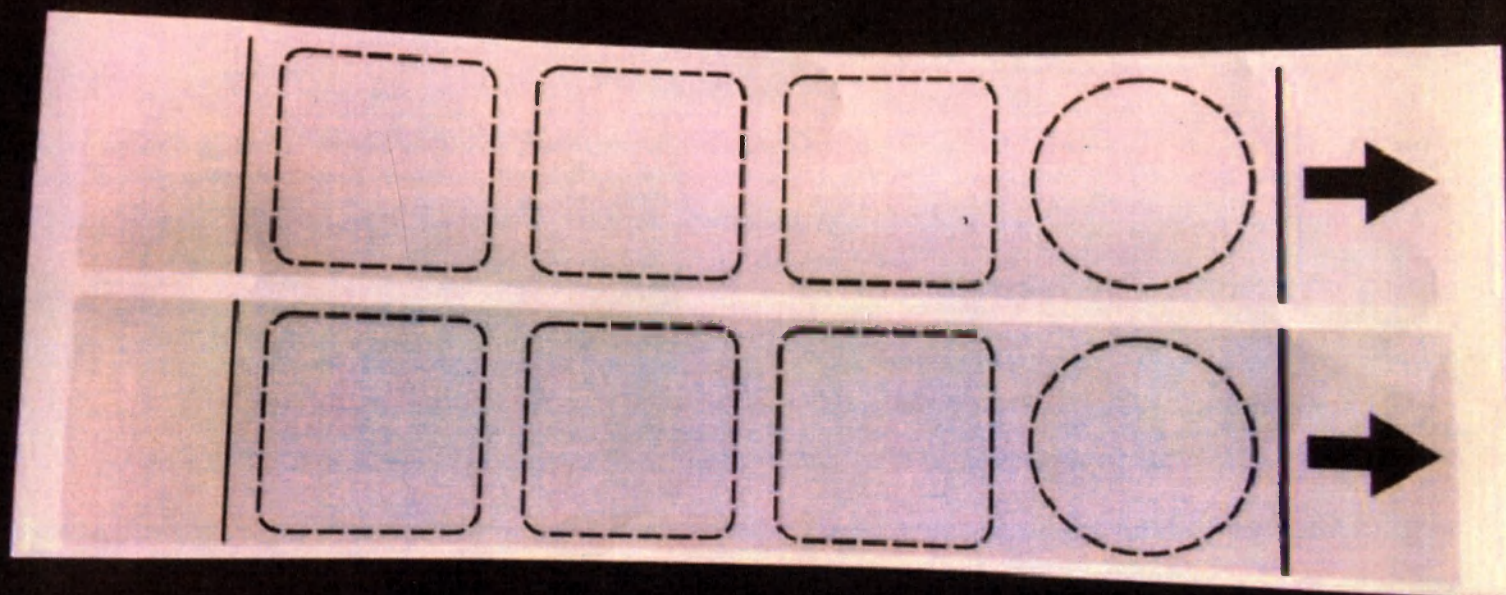

Этикетки для запечатывания флаконов

Vitamin B12 Control Material RFID

LOT A042300100  2025-01-27

QC Range (Low): 168.5-444.3 pg/mL

QC Range (High): 606.8~1127 pg/mL

Lifotronic

Lifotronic

Instruction For Use

【Product Name】

Vitamin B12 (eCLIA)

【Order Information】

REF NO.	Package Size
0320500207	50T
0320500208	100T
0320500203	2×50T
0320500204	2×100T

【Intended Use】

Immunoassay for in vitro quantitative determination of Vitamin B12 in human serum and plasma.

Vitamin B12, also known as cobalamin, is a corrin family compound with four pyrrole rings around a cobalt atom. As a complex organic compound, Vitamin B12 is mainly in the form of methylcobalamin in serum and 5'-deoxyadenosylcobalamin in cells, which is converted to cyanocobalamin in the

Инструкция по применению

Lifotronic

Vitamin B12 (eCLIA)

Components

Control Material (High)	1×2.0 mL
Control Material (Low)	1×2.0 mL
Calibrator (High)	1×1.0 mL
Calibrator (Low)	1×1.0 mL
MB	1×1.8 mL
RB	1×2.0 mL
RA	1×3.8 mL
RD	1×1.0 mL

P/N: 03-R05B840-00002

REF 0320500207


LOT A042300300

 2025-01-27




Shenzhen Lifotronic Technology Co., Ltd.
Unit A, 4th Floor, Building 15, Yijing Estate, No 1008, Songbai Road, Nanshan District, Shenzhen City,
Guangdong Province, 518055 P.R. China

Shanghai Inteconational Holding Corp. GmbH (Europe)
Exilstrasse 80, 20537 Hamburg, Germany
Tel. +49-40-2513175 Fax. +49-40-255726



(01) 0 6975984 06252 5
(17) 250127
(10) A042300300

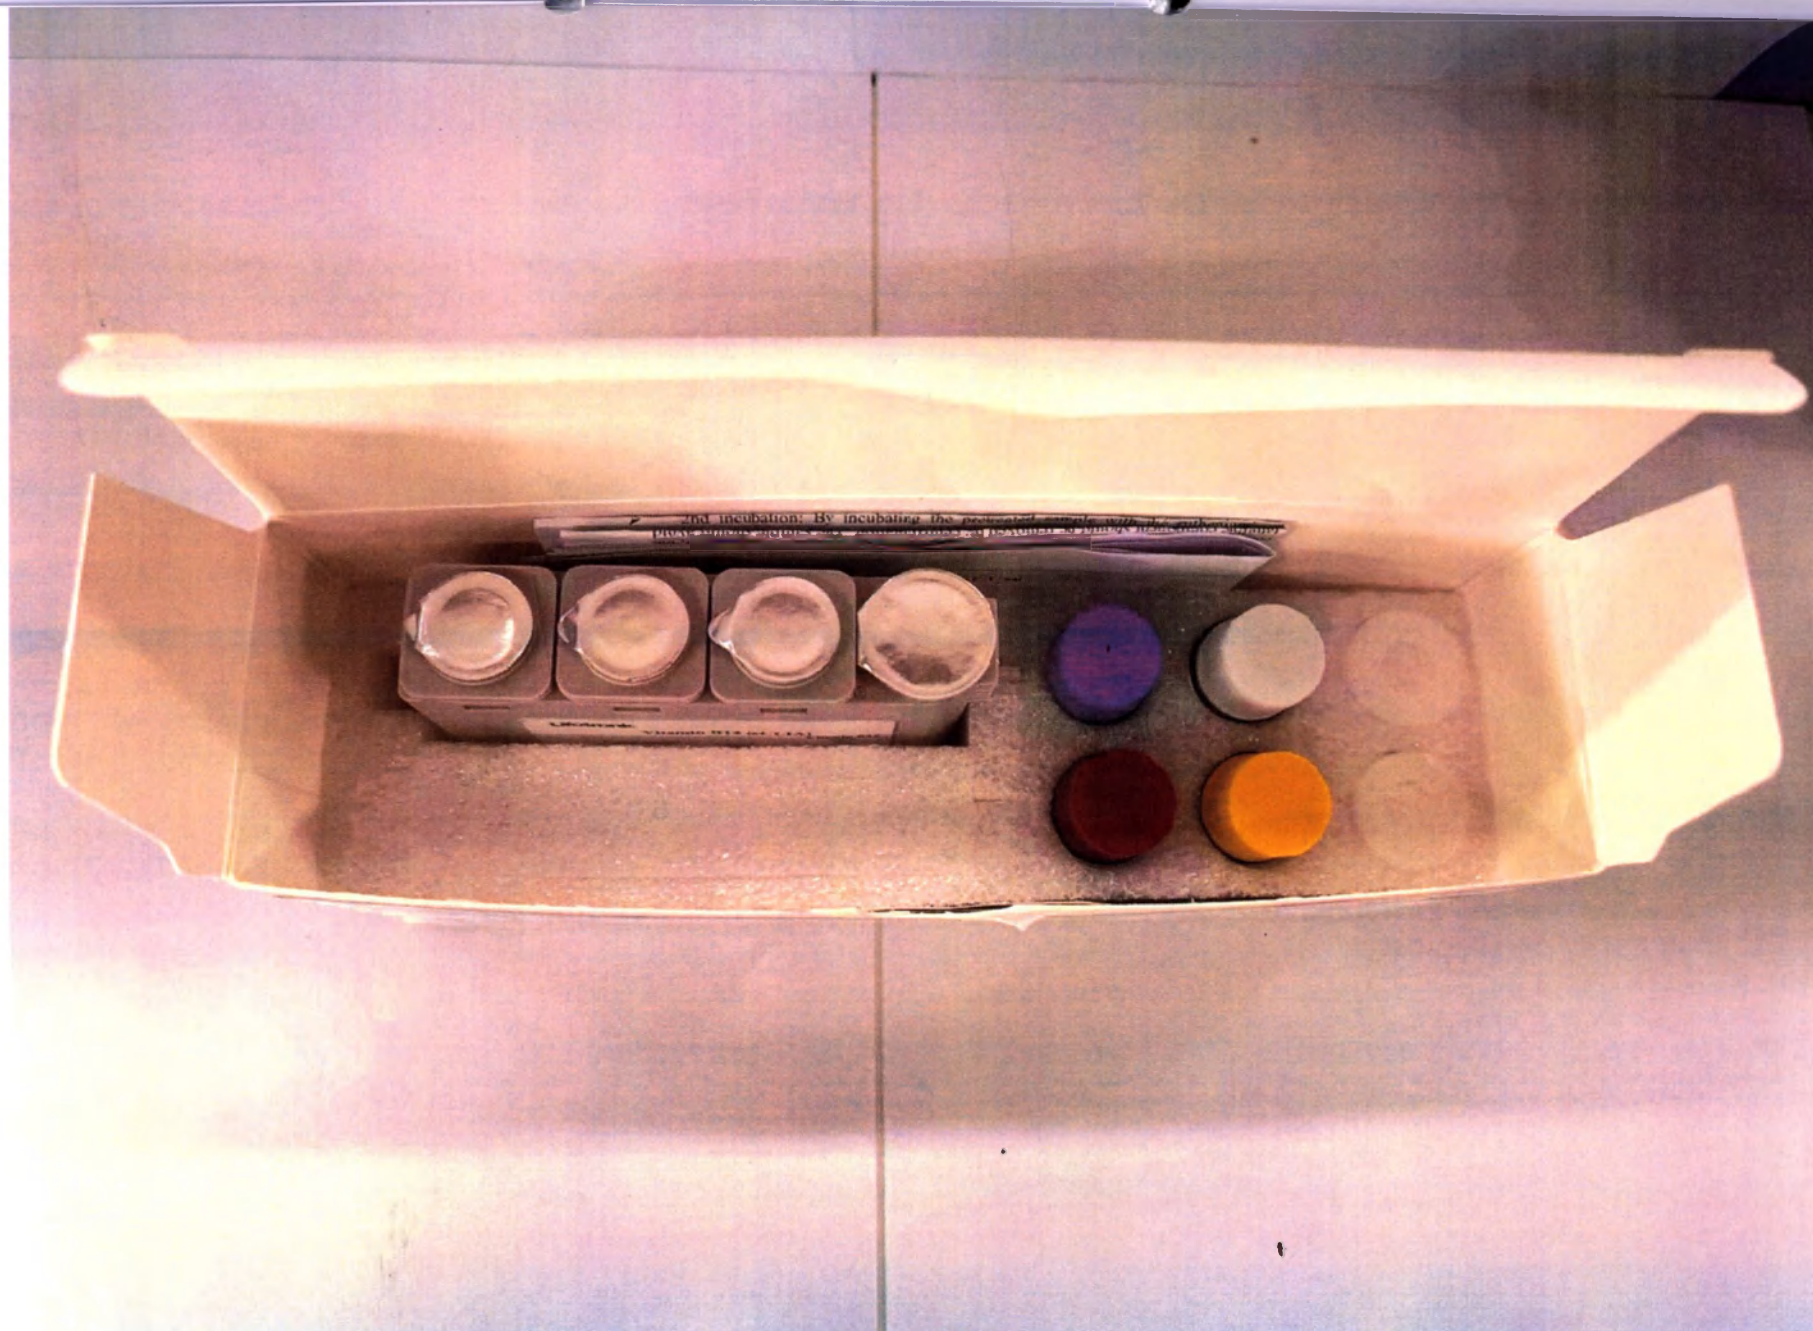

Набор реагентов для количественного определения витамина B12 электрохемилюминесцентным методом на анализаторах ECL для диагностики in vitro (Vitamin B12 (eCLIA) / Vitamin B12), в варианте исполнения 50 тестов

Lifotronic

Vitamin B12 (eCLIA)

Vitamin B12



Components

MB 1×1.8 mL

RB 1×2.0 mL

RA 1×3.8 mL

RD 1×1.0 mL

LOT A042300300

SN 00030

2025-01-27

CE

IVD

2°C


8°C



Кассета с реагентами



Калибратор (низкий уровень), Калибратор (высокий уровень), Материал контрольный (высокий уровень), Материал контрольный (низкий уровень)

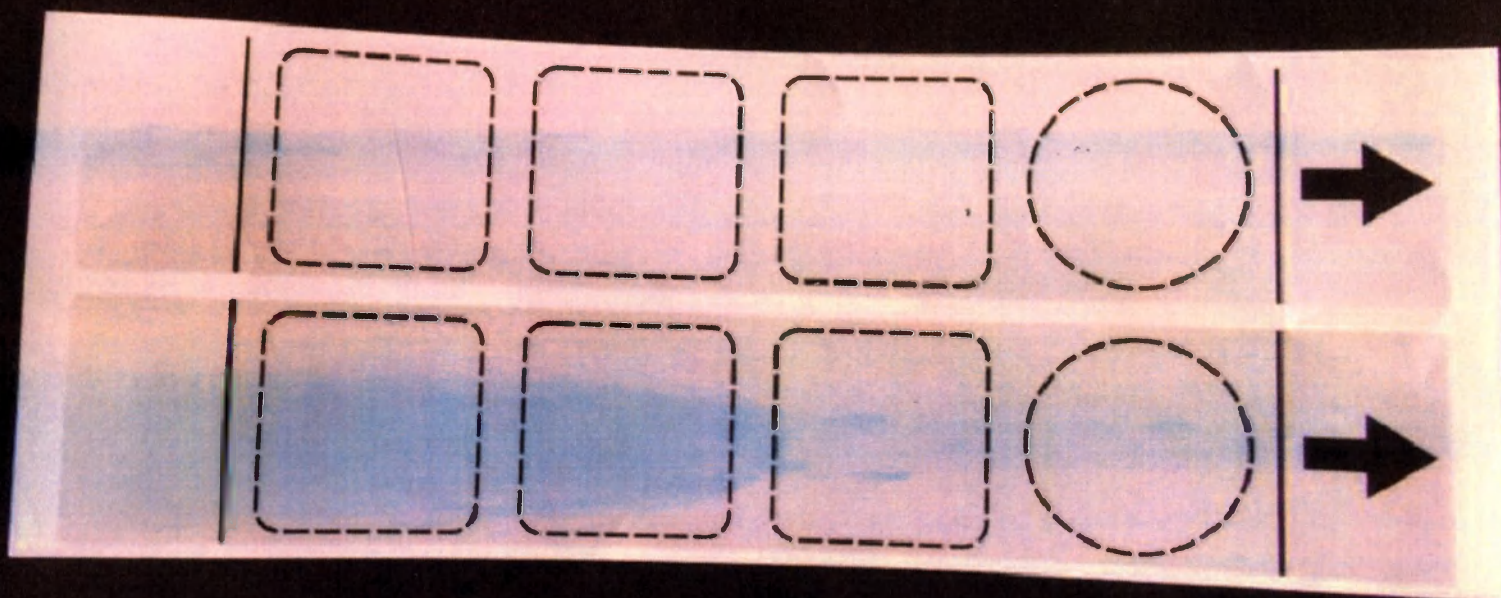

Этикетки для запечатывания флаконов

Vitamin B12 Control Material RFID



A042300300



2025-01-27

QC Range (Low): 168.5-444.3 pg/mL

QC Range (High): 606.8-1127 pg/mL

Lifotronic

Этикетка результатов значений материалов контрольных

Lifotronic

Instruction For Use

【Product Name】
Vitamin B12 (eCLIA)

【Order Information】

REF NO.	Package Size
0320500207	50T
0320500208	100T
0320500203	2×50T
0320500204	2×100T

【Intended Use】

Immunoassay for in vitro quantitative determination of Vitamin B12 in human serum and plasma.

Vitamin B12, also known as cobalamin, is a complex organometallic compound with four pyrrole rings around a cobalt atom. As a complex organometallic compound, VB12 is mainly in the form of methylcobalamin in serum and 5'-deoxyadenosylcobalamin in cells, which is converted to cyanocobalamin in the

Инструкция по применению

Всего прошито, пронумеровано и скреплено
печатью и подписью: 17 листа (-ов)

Генеральный директор _____ / Носова Т.А
М.П.

ПО ДОВЕРЕННОСТИ
77 АД 3555614
КУСАЙЛО Р.В.

