



ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru

УТВЕРЖДАЮ

Генеральный директор

ООО «ВУ ЯНГ МЕДИКАЛ РУС»

Е.В. Михеева



«28» декабря 2023 г.

ФОТОГРАФИЧЕСКИЕ ИЗОБРАЖЕНИЯ МЕДИЦИНСКОГО ИЗДЕЛИЯ

«Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы в вариантах исполнения»




ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru

Варианты исполнения медицинского изделия – первичная упаковка:

- 1) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P24A: диаметр катетера 24G (0,44 мм): длина катетера 19,05 мм, скорость потока 19 мл/мин – 50 шт, инструкция по применению – 1 шт.

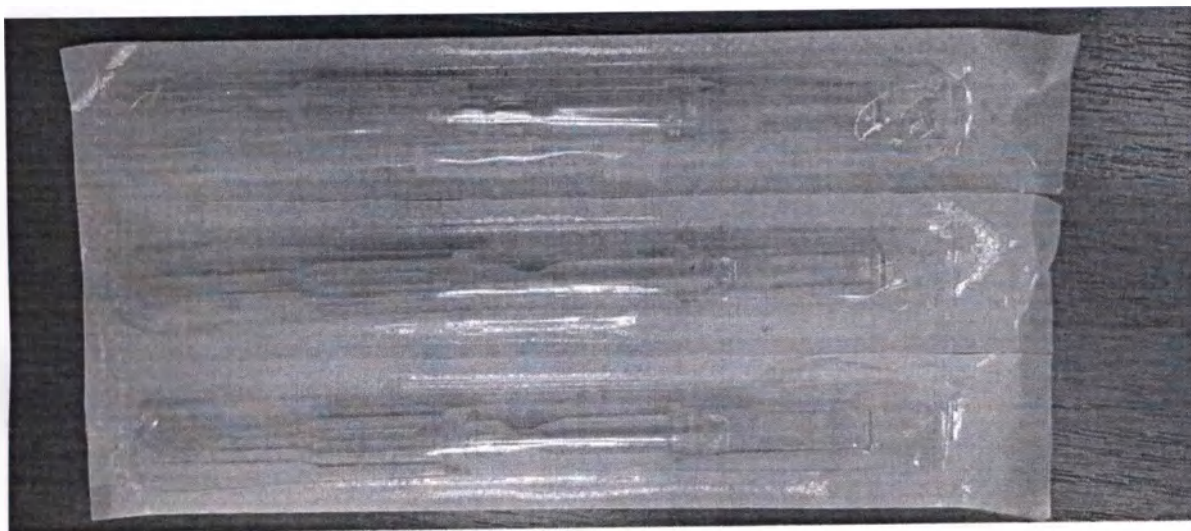


- 2) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P22B: диаметр катетера 22G (0,54 мм): длина катетера 25,40 мм, скорость потока 31 мл/мин – 50 шт, инструкция по применению – 1 шт.




ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru

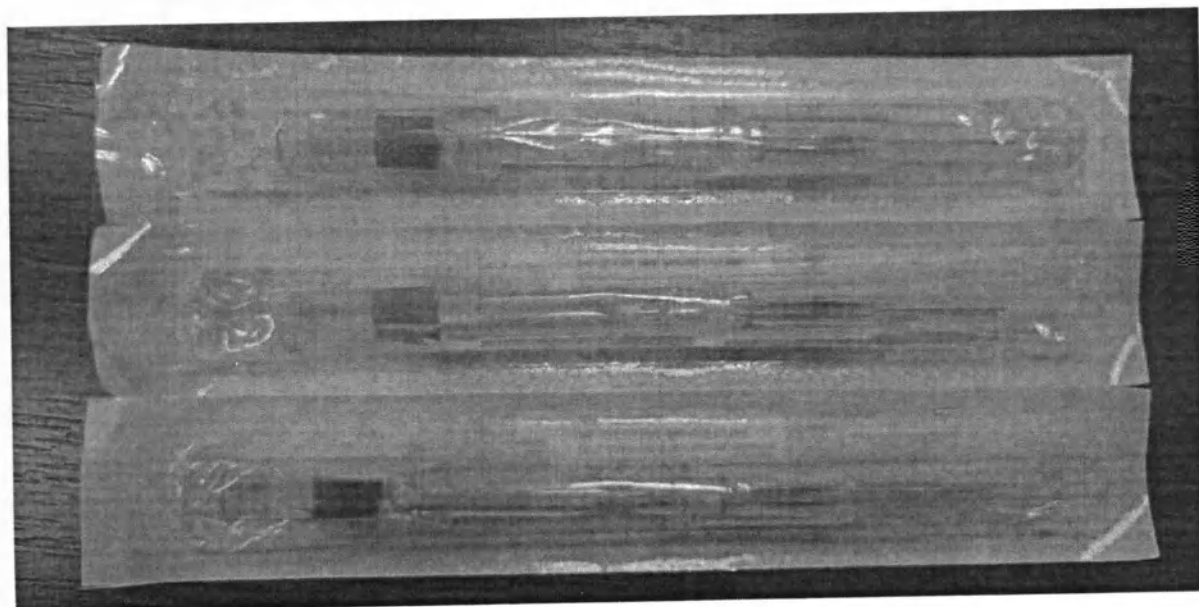

- 3) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P20C: диаметр катетера 20G (0,70 мм): длина катетера 29,46 мм, скорость потока 56 мл/мин – 50 шт, инструкция по применению – 1 шт.

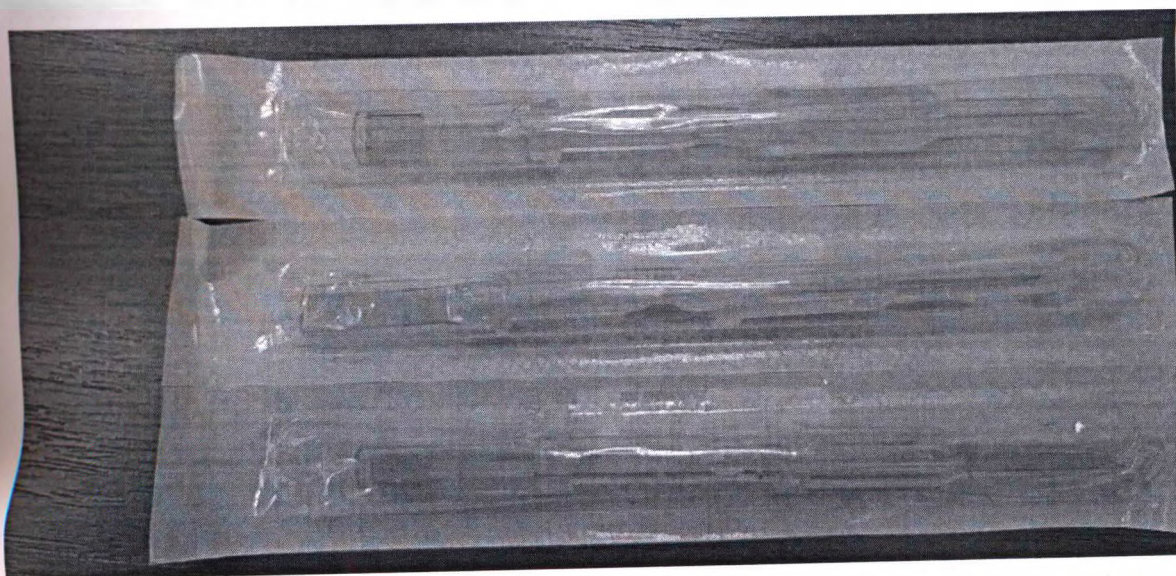




ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru



- 4) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P18C: диаметр катетера 18G (0,88 мм): длина катетера 29,46 мм, скорость потока 93 мл/мин – 50 шт, инструкция по применению – 1 шт.

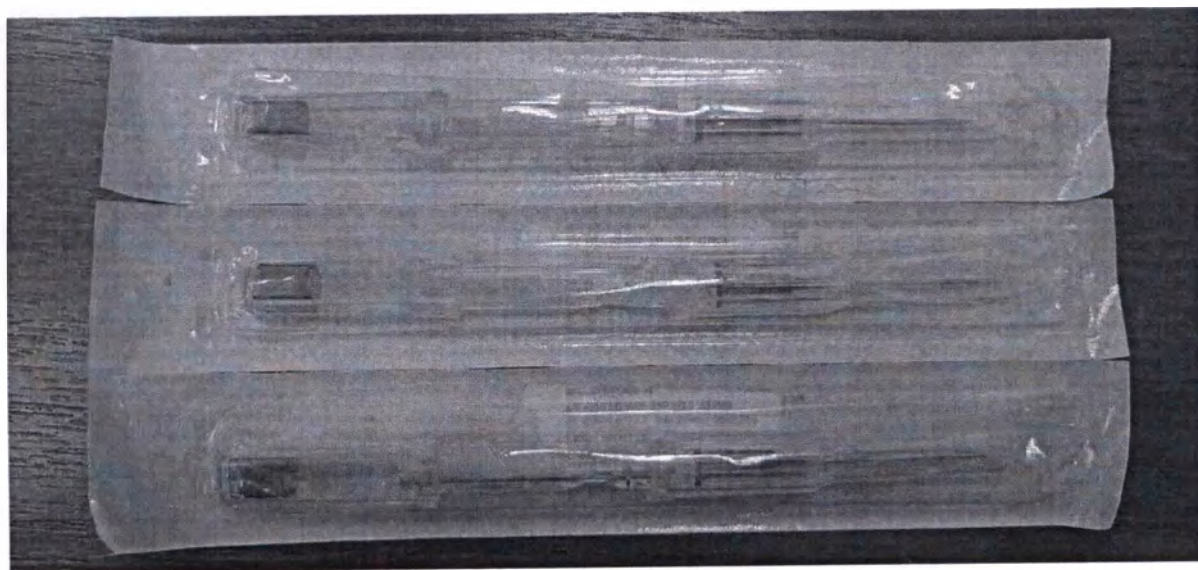

Варианты исполнения медицинского изделия – групповая упаковка:

- 1) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P24A: диаметр катетера 24G (0,44 мм): длина катетера 19,05 мм, скорость потока 19 мл/мин – 50 шт, инструкция по применению – 1 шт.



ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru



CE Rx
2460 Only

24G

MagiCath IITM


PU Safety I.V. Catheter

INDICATIONS OF USE

MagiCath II is inserted into the patient's vascular system for short-term use (less than 30 days) to sample blood, monitor blood pressure, or administer fluids intravenously. These catheters should be used for a patient with consideration given to the adequacy of vascular anatomy and appropriateness of the procedure.

CONTRAINDICATION

There are no absolute contraindications.

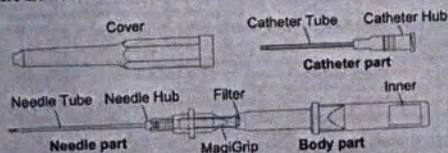


WARNINGS

1. Discard the device after single use according to local regulations. Do not reuse or re-sterilize. Reuse or re-sterilization may result in the slow or unpredictable flow of medication and result in infection.
2. Before using the device, please double check the specification indicated on the label. Using the wrong size may result in injury to the patient.
3. Do not use the unit if the packaging has been previously damaged or tampered with.
4. Do not use it if the expiration date has passed.
5. Always pay attention to needle stick injury and exposure of blood to avoid transmission and contaminations that can cause HIV, infection by viruses, germs or other inflammation.
6. Minimize the movement of a patient and inserted catheter at the puncture site. Otherwise, leak of solution to surrounding tissue or pain may occur.

HOW TO USE

1. Use aseptic technique.
2. Before unpacking, check the sterile packaging and product for damage and basic product information.
3. Remove cover carefully to avoid damage to the tip of needle and needle stick injury and then inspect catheter part whether catheter is bent or damaged.
4. Always place your hands behind the product during use to avoid needle stick injury.
5. Hold MagiGrip with bevel face up.



6. After checking separation of the catheter hub, fix the catheter hub firmly until it is removed from the patient.
7. Position a patient properly.
8. During venipuncture, make sure blood is visible along the needle hub.
9. Stabilize catheter and then pull out needle from the catheter hub.
10. To activate the safety function, lift the device upright and release the fingers holding MagiGrip. The needle part will retract inside the body part.
11. When you can see that needle tube entered into inner, discard it in a sharps disposal container immediately.
12. Connect and tighten the connectors or adapters which is in compliance with ISO requirements to catheter hub.
13. The puncture site should be monitored regularly by medical staff.
14. When the procedure is completed, remove and discard the catheter.



2) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P22B: диаметр катетера 22G (0,54 мм): длина катетера 25,40 мм, скорость потока 31 мл/мин – 50 шт, инструкция по применению – 1 шт.



ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru

WOO YOUNG MEDICAL

CE 2460 Rx Only 22G

MagiCathTM II

PU Safety I.V. Catheter

INDICATIONS OF USE
MagiCath II is inserted into the patient's vascular system for short-term use (less than 30 days) to sample blood, monitor blood pressure, or administer fluids intravenously. These catheters should be used for a patient with consideration given to the adequacy of vascular anatomy and appropriateness of the procedure.

CONTRAINDICATION
There are no absolute contraindications.

HOW TO USE

1. Use aseptic technique.
2. Before unpacking, check the sterile packaging and product for damage and basic product information.
3. Remove cover carefully to avoid damage to the tip of needle and needle stick injury and then inspect catheter part whether catheter is bent or damaged.
4. Always place your hands behind the product during use to avoid needle stick injury.
5. Hold MagiGrip with bevel face up.

Bevel down ✗ Bevel up ✓

WARNINGS

1. Discard the device after single use according to local regulations. Do not reuse or re-sterilize. Reuse or re-sterilization may result in the slow or unpredictable flow of medication and result in infection.
2. Before using the device, please double check the specification indicated on the label. Using the wrong size may result in injury to the patient.
3. Do not use the unit if the packaging has been previously damaged or tampered with.
4. Do not use it if the expiration date has passed.
5. Always pay attention to needle stick injury and exposure of blood to avoid transmission and contaminations that can cause HIV, infection by viruses, germs or other inflammation.
6. Minimize the movement of a patient and inserted catheter at the puncture site. Otherwise, leak of solution to surrounding tissue or pain may occur.

6. After checking separation of the catheter hub, fix the catheter hub firmly until is removed from the patient.
7. Position a patient properly.
8. During venipuncture, make sure blood is visible along the needle hub.
9. Stabilize catheter and then pull out needle from the catheter hub.
10. To activate the safety function, lift the device upright and release the fingers holding MagiGrip. The needle part will retract inside the body part.
11. When you can see that needle tube entered into inner, discard it in a sharps disposal container immediately.
12. Connect and tighten the connectors or adapters which is in compliance with ISO requirements to catheter hub.
13. The puncture site should be monitored regularly by medical staff.
14. When the procedure is completed, remove and discard the catheter.

3) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P20C: диаметр катетера 20G (0,70 мм): длина катетера 29,46 мм, скорость потока 56 мл/мин – 50 шт, инструкция по применению – 1 шт.



ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru



WOO YOUNG MEDICAL



2460

Rx Only

20G

MagiCathTM II


PU Safety I.V. Catheter

INDICATIONS OF USE

MagiCath II is inserted into the patient's vascular system for short-term use (less than 30 days) to sample blood, monitor blood pressure, or administer fluids intravenously. These catheters should be used for a patient with consideration given to the adequacy of vascular anatomy and appropriateness of the procedure.

CONTRAINDICATION

There are no absolute contraindications.

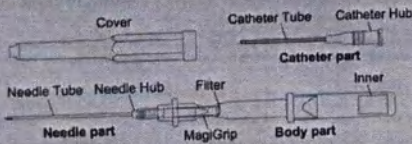

WARNINGS

1. Discard the device after single use according to local regulations. Do not reuse or re-sterilize. Reuse or re-sterilization may result in the slow or unpredictable flow of medication and result in infection.
2. Before using the device, please double check the specification indicated on the label. Using the wrong size may result in injury to the patient.
3. Do not use the unit if the packaging has been previously damaged or tampered with.
4. Do not use it if the expiration date has passed.
5. Always pay attention to needle stick injury and exposure of blood to avoid transmission and contaminations that can cause HIV, infection by viruses, germs or other inflammation.
6. Minimize the movement of a patient and inserted catheter at the puncture site. Otherwise, leak of solution to surrounding tissue or pain may occur.

HOW TO USE

1. Use aseptic technique.
2. Before unpacking, check the sterile packaging and product for damage and basic product information.
3. Remove cover carefully to avoid damage to the tip of needle and needle stick injury and then inspect catheter part whether catheter is bent or damaged.
4. Always place your hands behind the product during use to avoid needle stick injury.
5. Hold MagiGrip with bevel face up.

Bevel down ✗

Bevel up ✓

6. After checking separation of the catheter hub, fix the catheter hub firmly until is removed from the patient.
7. Position a patient properly.
8. During venipuncture, make sure blood is visible along the needle hub.
9. Stabilize catheter and then pull out needle from the catheter hub.
10. To activate the safety function, lift the device upright and release the fingers holding MagiGrip. The needle part will retract inside the body part.
11. When you can see that needle tube entered into inner, discard it in a sharps disposal container immediately.
12. Connect and tighten the connectors or adapters which is in compliance with ISO requirements to catheter hub.
13. The puncture site should be monitored regularly by medical staff.
14. When the procedure is completed, remove and discard the catheter.




4) Катетер внутривенный безопасный одноразовый стерильный MagiCath II с механизмом защиты от укола иглы модель 2P18C: диаметр катетера 18G (0,88 мм): длина катетера 29,46 мм, скорость потока 93 мл/мин – 50 шт, инструкция по применению – 1 шт.



ООО «ВУ ЯНГ МЕДИКАЛ РУС»

105064, город Москва, ул Нижний Сусальный переулок, д. 5, стр. 5А;
ИНН/КПП 7709482942/770901001; тел. +7(495) 909 24 61; www.wooyoungmed.ru



CE
2460

Rx
Only

18G


MagiCath IITM

INDICATIONS OF USE

MagiCath II is inserted into the patient's vascular system for short-term use (less than 30 days) to sample blood, monitor blood pressure, or administer fluids intravenously. These catheters should be used for a patient with consideration given to the adequacy of vascular anatomy and appropriateness of the procedure.

CONTRAINDICATION

There are no absolute contraindications.

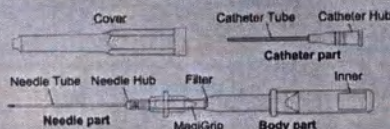


WARNINGS

1. Discard the device after single use according to local regulations. Do not reuse or re-sterilize. Reuse or re-sterilization may result in the slow or unpredictable flow of medication and result in infection.
2. Before using the device, please double check the specification indicated on the label. Using the wrong size may result in injury to the patient.
3. Do not use the unit if the packaging has been previously damaged or tampered with.
4. Do not use it if the expiration date has passed.
5. Always pay attention to needle stick injury and exposure of blood to avoid transmission and contaminations that can cause HIV, infection by viruses, germs or other inflammation.
6. Minimize the movement of a patient and inserted catheter at the puncture site. Otherwise, leak of solution to surrounding tissue or pain may occur.

HOW TO USE

1. Use aseptic technique.
2. Before unpacking, check the sterile packaging and product for damage and basic product information.
3. Remove cover carefully to avoid damage to the tip of needle and needle stick injury and then inspect catheter part whether catheter is bent or damaged.
4. Always place your hands behind the product during use to avoid needle stick injury.
5. Hold MagiGrip with bevel face up.



6. After checking separation of the catheter hub, fix the catheter hub firmly until is removed from the patient.
7. Position a patient properly.
8. During venipuncture, make sure blood is visible along the needle hub.
9. Stabilize catheter and then pull out needle from the catheter hub.
10. To activate the safety function, lift the device upright and release the fingers holding MagiGrip. The needle part will retract inside the body part.
11. When you can see that needle tube entered into inner, discard it in a sharps disposal container immediately.
12. Connect and tighten the connectors or adapters which is in compliance with ISO requirements to catheter hub.
13. The puncture site should be monitored regularly by medical staff.
14. When the procedure is completed, remove and discard the catheter.



Всего прошито, прочисловано
и скреплено печатью

8 листа

Генеральный директор
ООО «ВУ ЯНГ МЕДИКАЛ РУС»
Михеева Е.В.

