

Генеральный директор
ООО «Компания «БиВи»


«24» апреля 2023 г.



ПО ДОВЕРЕННОСТИ
77 АД 1754197
КУСАЙЛО Р. В.

Реагент лизирующий для анализаторов автоматических гематологических 3-Diff/5-Diff для диагностики in vitro (Hematology analyzer lyse (LYE-1/LYG-1))

Shenzhen Dymind Biotechnology Co., Ltd., («Шэньчжэнь Дайминд Биотекнолоджи Ко., Лтд.»),
Китай

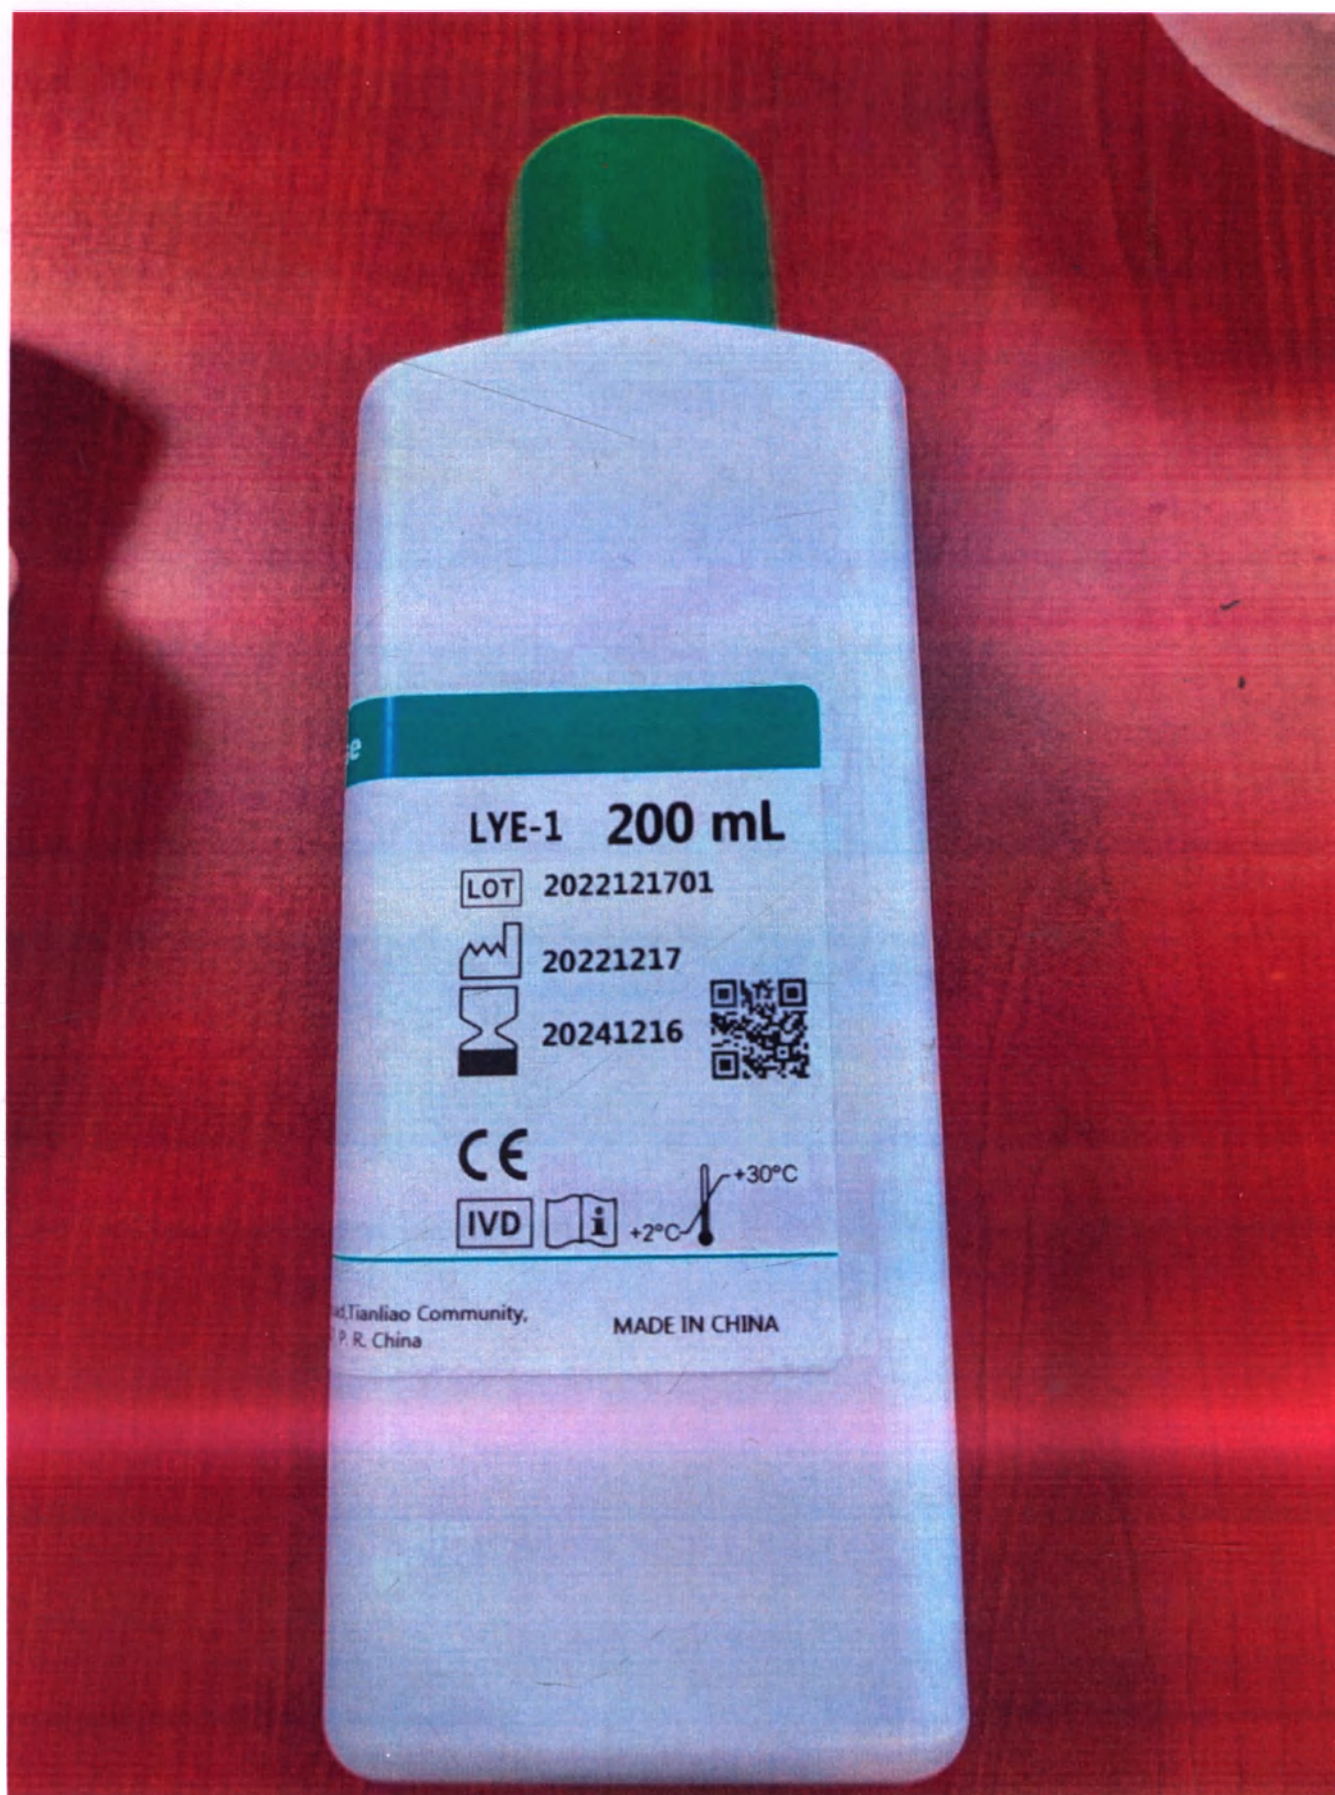

Реагент лизирующий LYE-1, 200 мл



Реагент лизирующий LYE-1, 200 мл



Hematology Analyzer Lyse

LYE-1 Lyse is applicable to the DH3X (where X represents the digit and/or letter) series hematology analyzers manufactured by Dymind. It is used to lyse (destroy) red blood cells for hemoglobin determinations or aid in the counting of white blood cells. Use the LYE-1 Lyse as instructed by the operation manual of the analyzer.

STORAGE AND STABILITY:

The product will be stable for 2 years when stored at 2°C to 30°C (35°F to 86°F).

If the operating environment is 15°C to 30°C (59°F to 86°F), discard opened container after 60 days.




Eunitor GmbH
Kennedydamm 5, 40476 Duesseldorf, Germany




Shenzhen Dymind Biotechnology Co., Ltd.
10th Floor, Building B, High-tech Park, Guangqiao Road,
Yutang Street, Guangming District, Shenzhen 518107, P.R.

Реагент лизирующий LYE-1, 200 мл

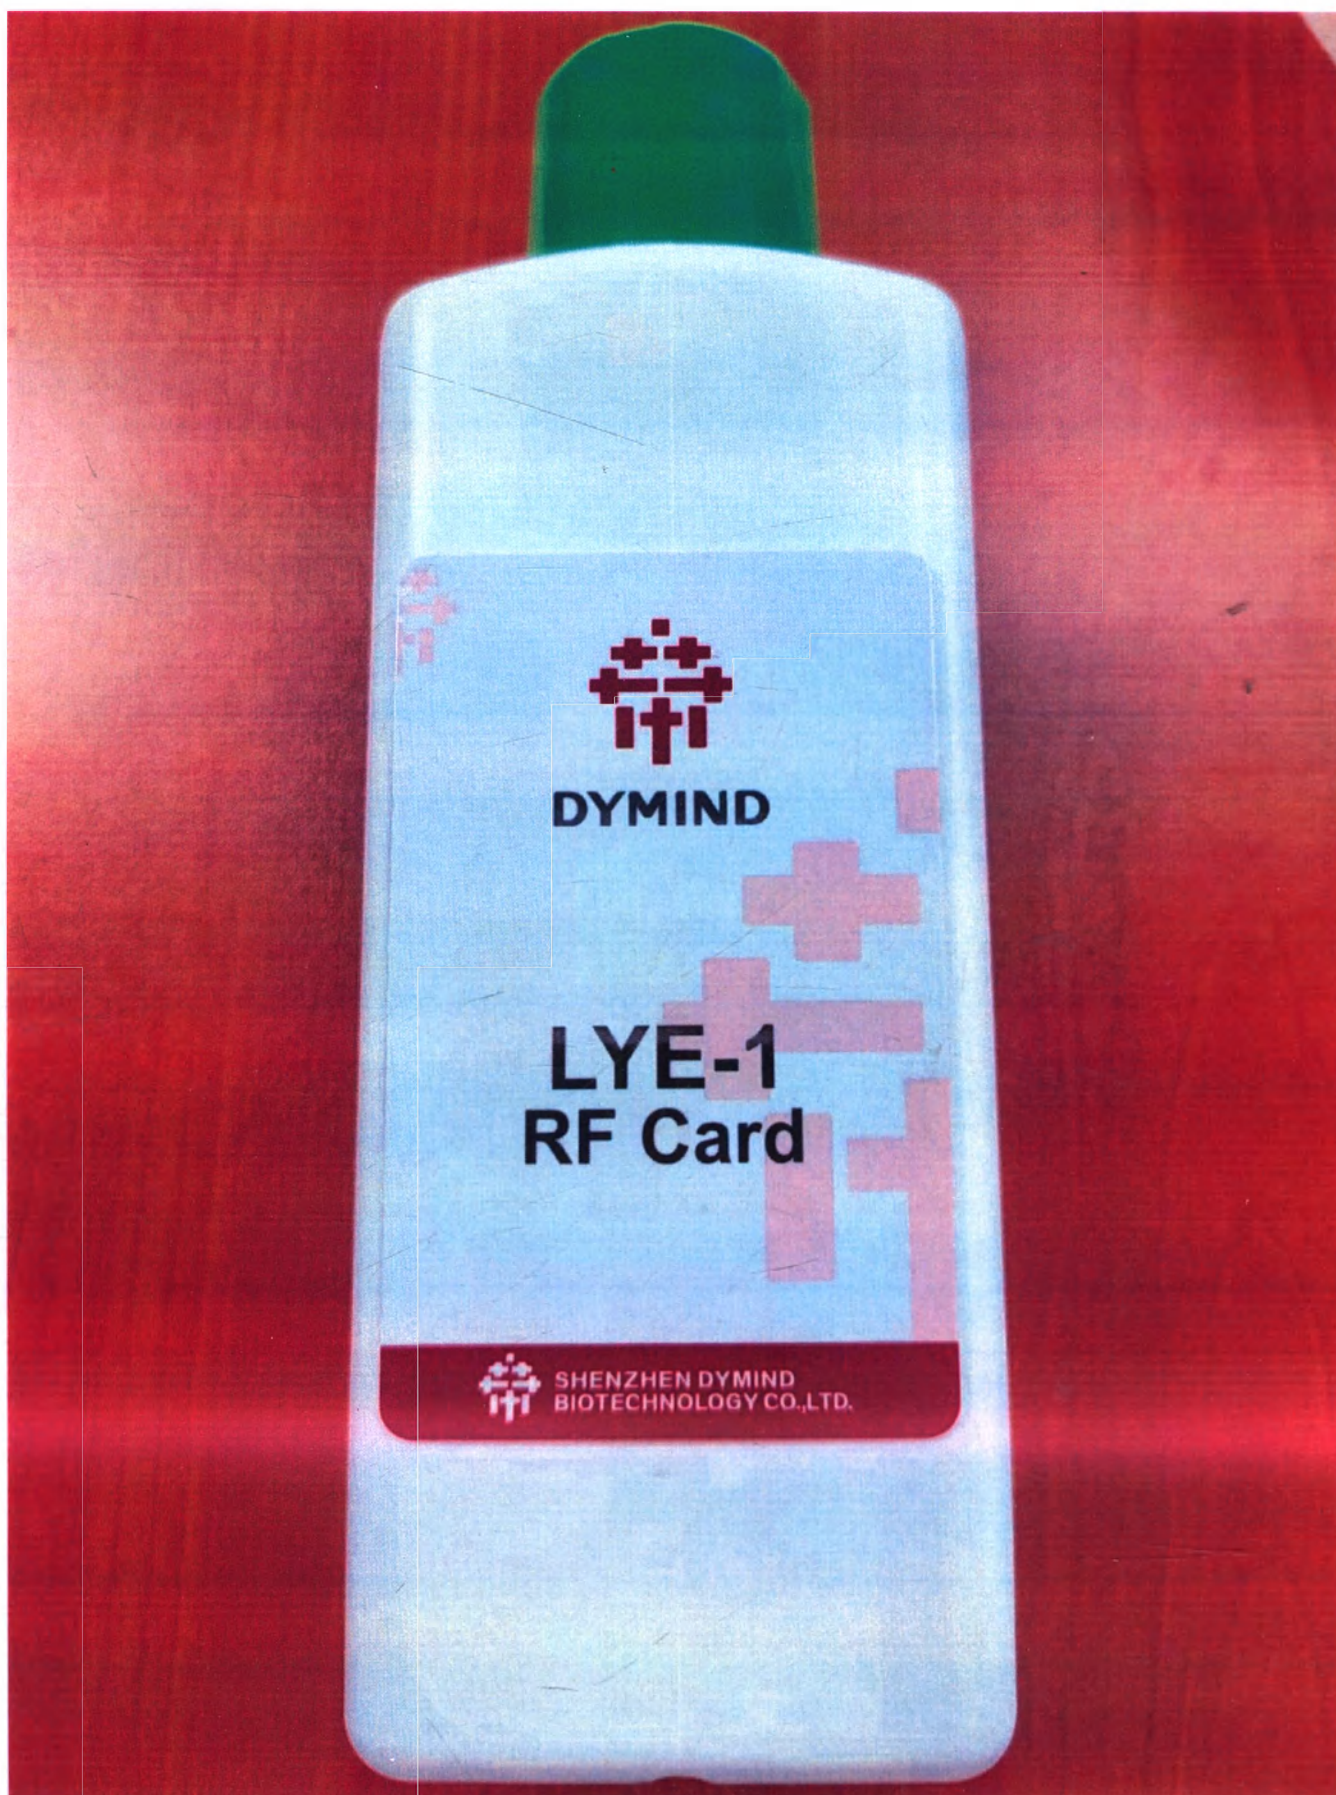

Реагент лизирующий LYE-1, 200 мл

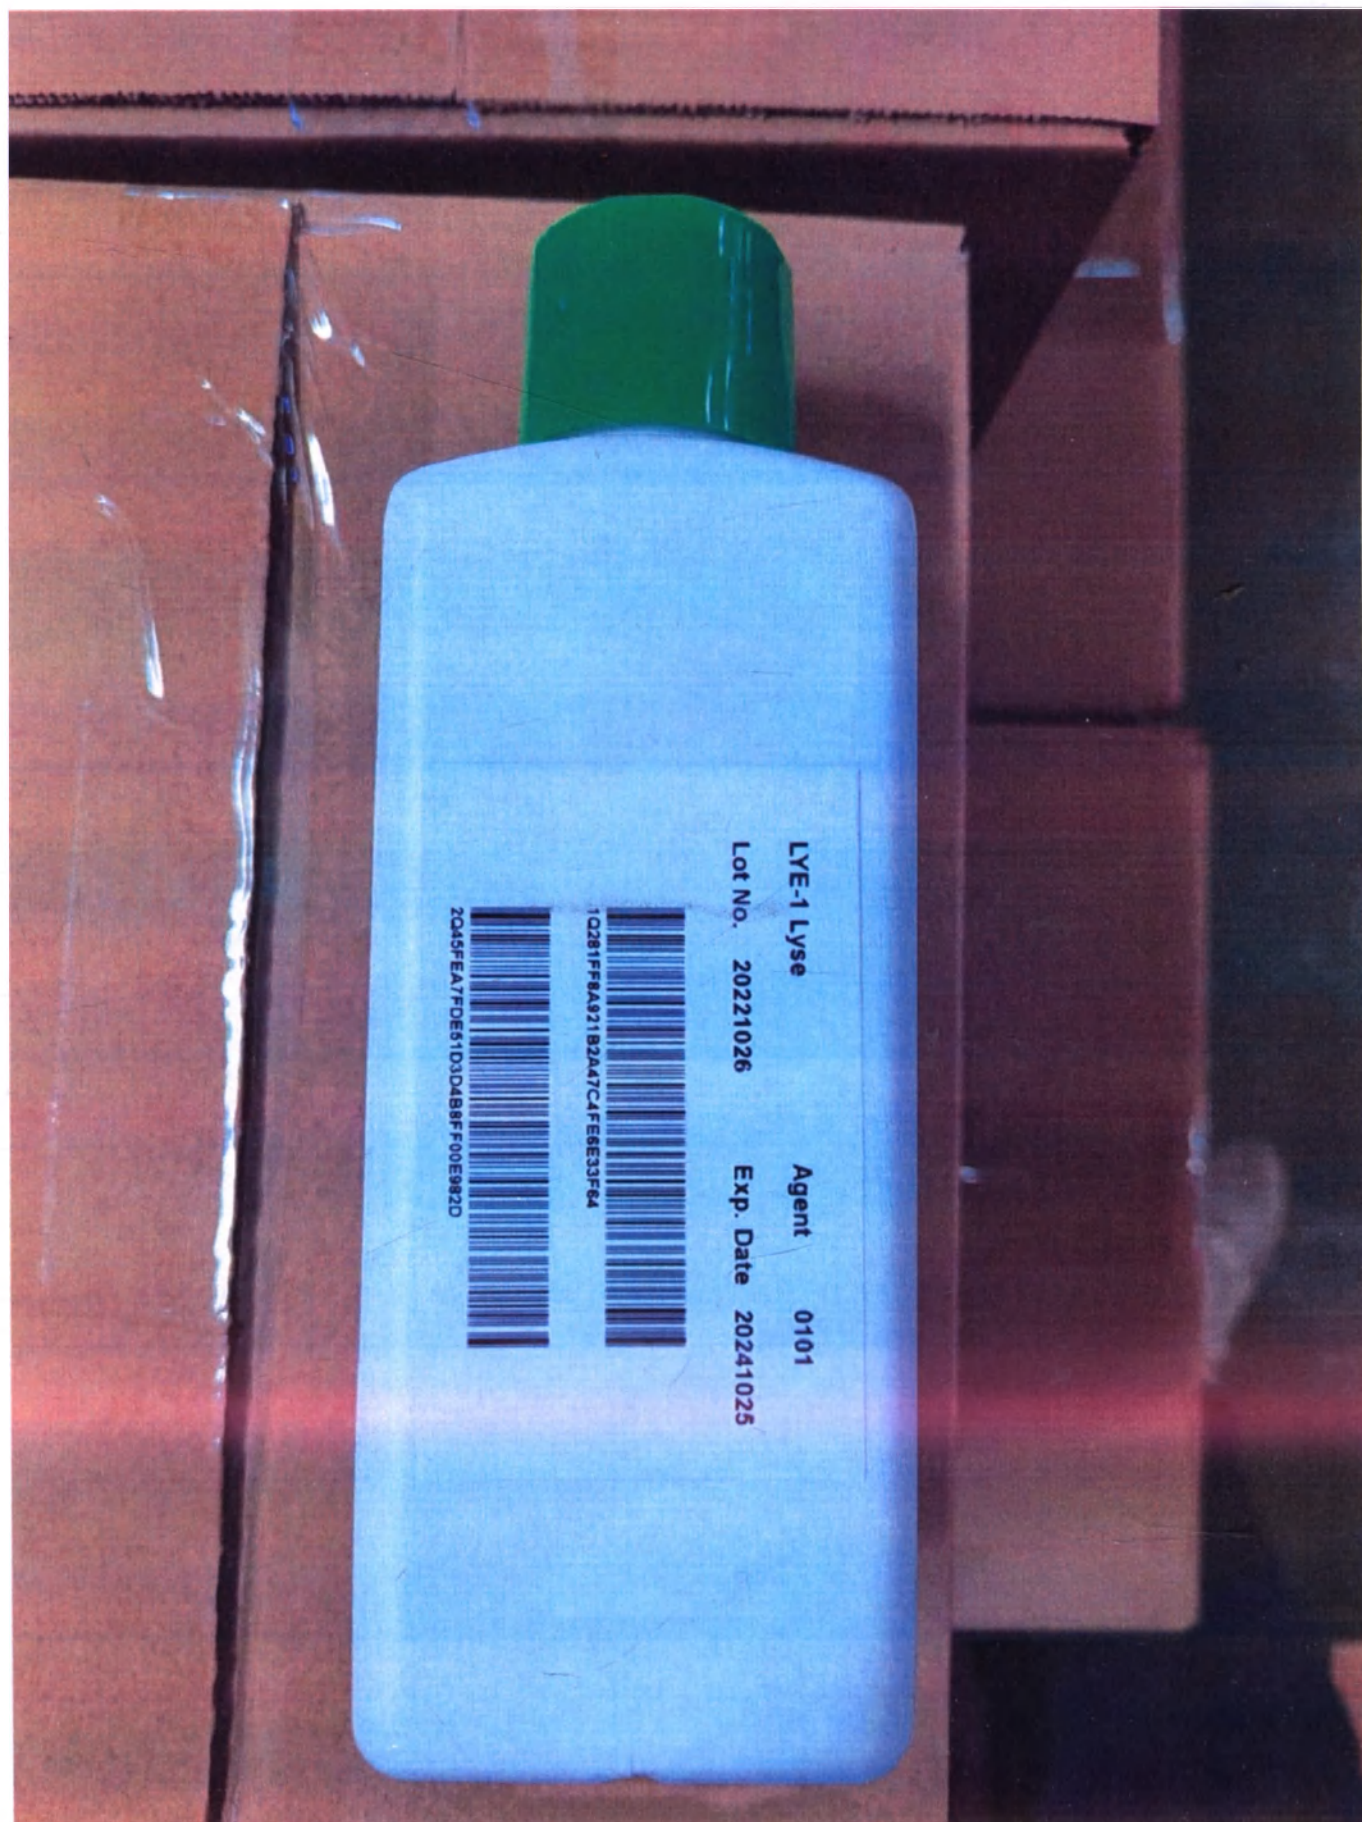


Реагент лизирующий LYE-1, 200 мл



Реагент лизирующий LYE-1, 200 мл



Реагент лизирующий LYE-1, 500 мл

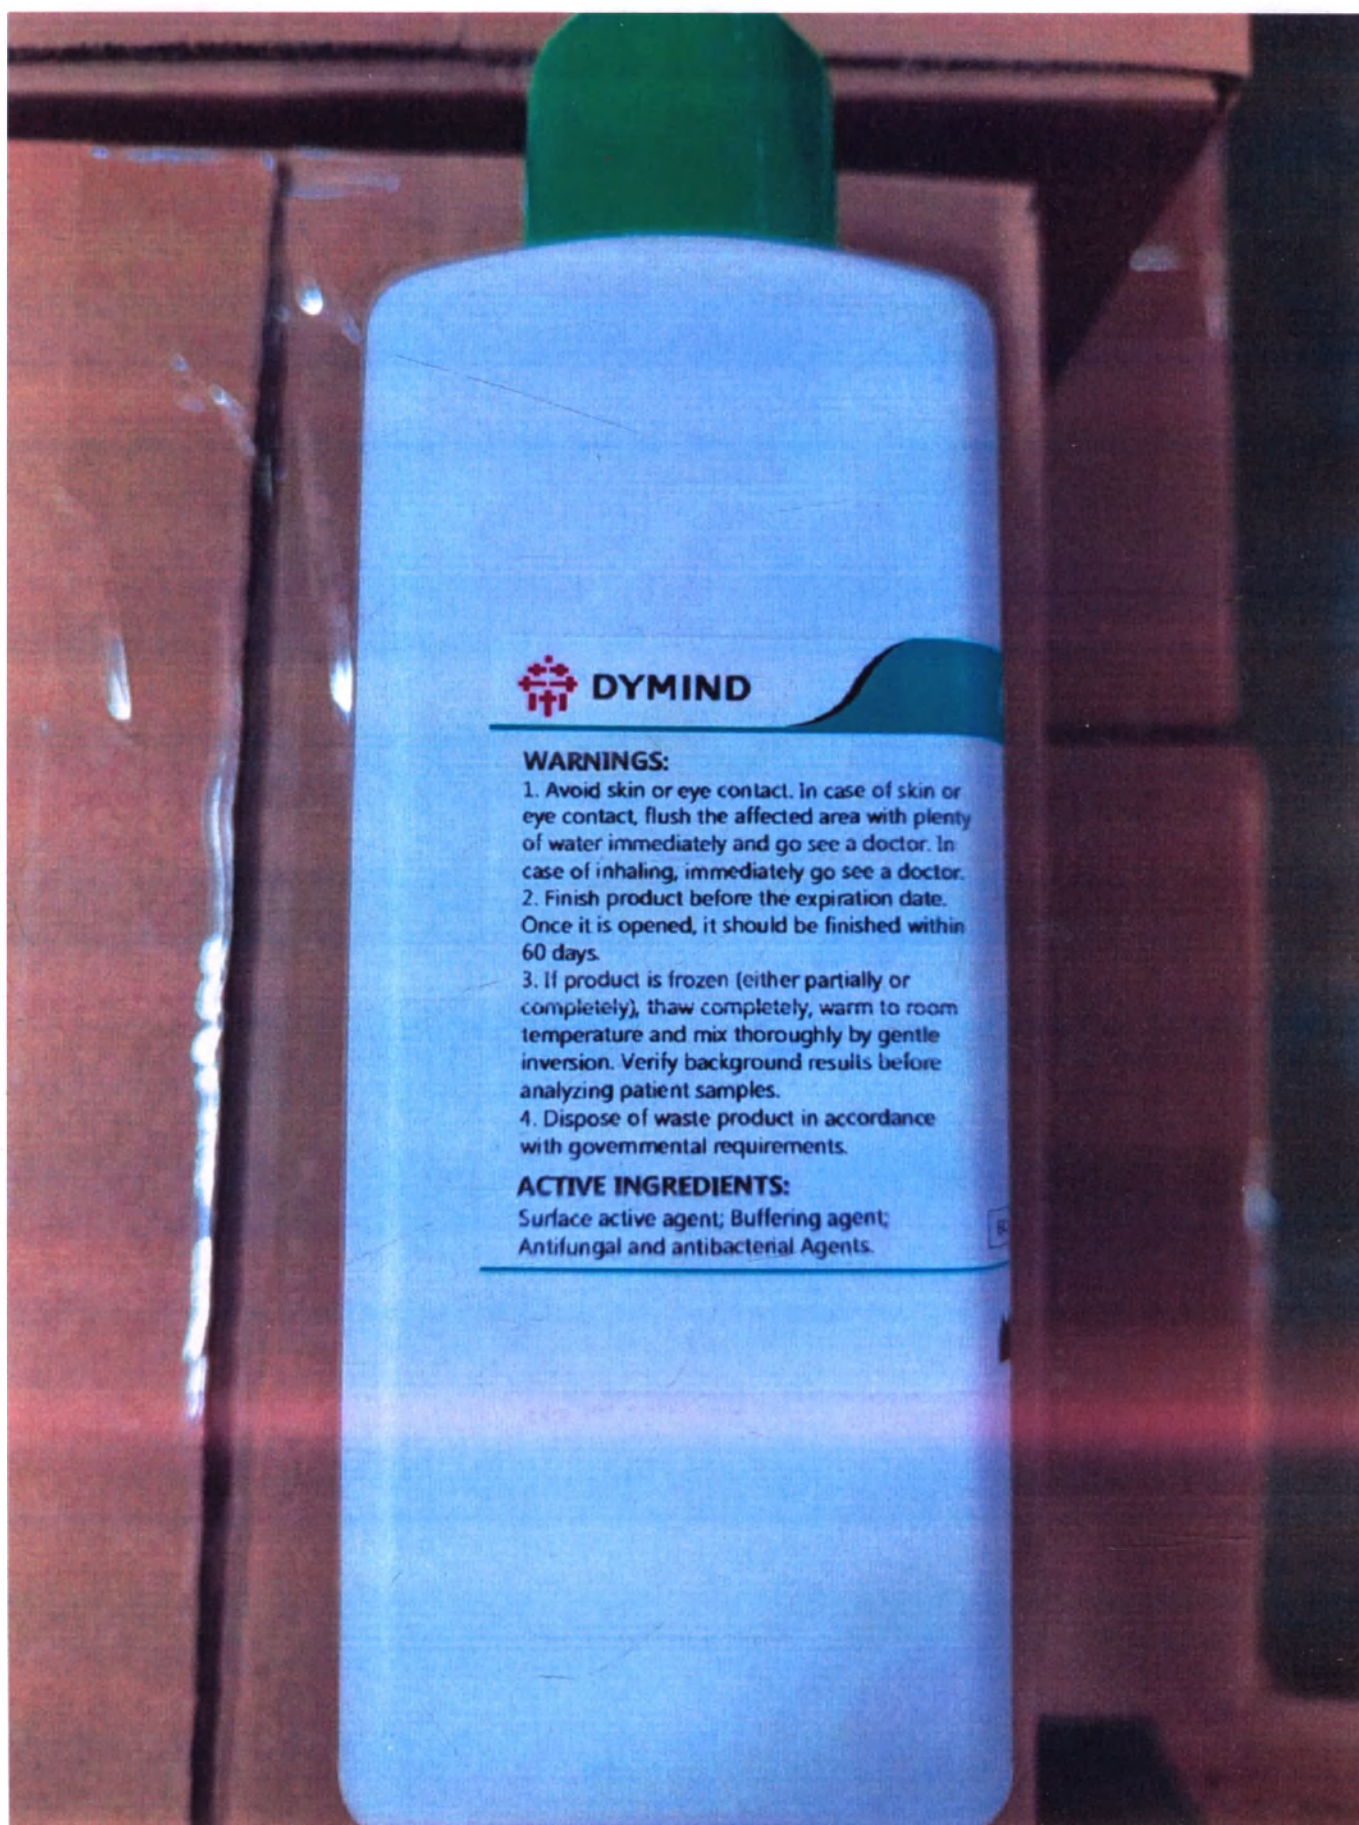

DYMIND


WARNINGS:

1. Avoid skin or eye contact. In case of skin or eye contact, flush the affected area with plenty of water immediately and go see a doctor. In case of inhaling, immediately go see a doctor.
2. Finish product before the expiration date. Once it is opened, it should be finished within 60 days.
3. If product is frozen (either partially or completely), thaw completely, warm to room temperature and mix thoroughly by gentle inversion. Verify background results before analyzing patient samples.
4. Dispose of waste product in accordance with governmental requirements.


ACTIVE INGREDIENTS:

Surface active agent; Buffering agent;
Antifungal and antibacterial Agents.

Реагент лизирующий LYE-1, 500 мл

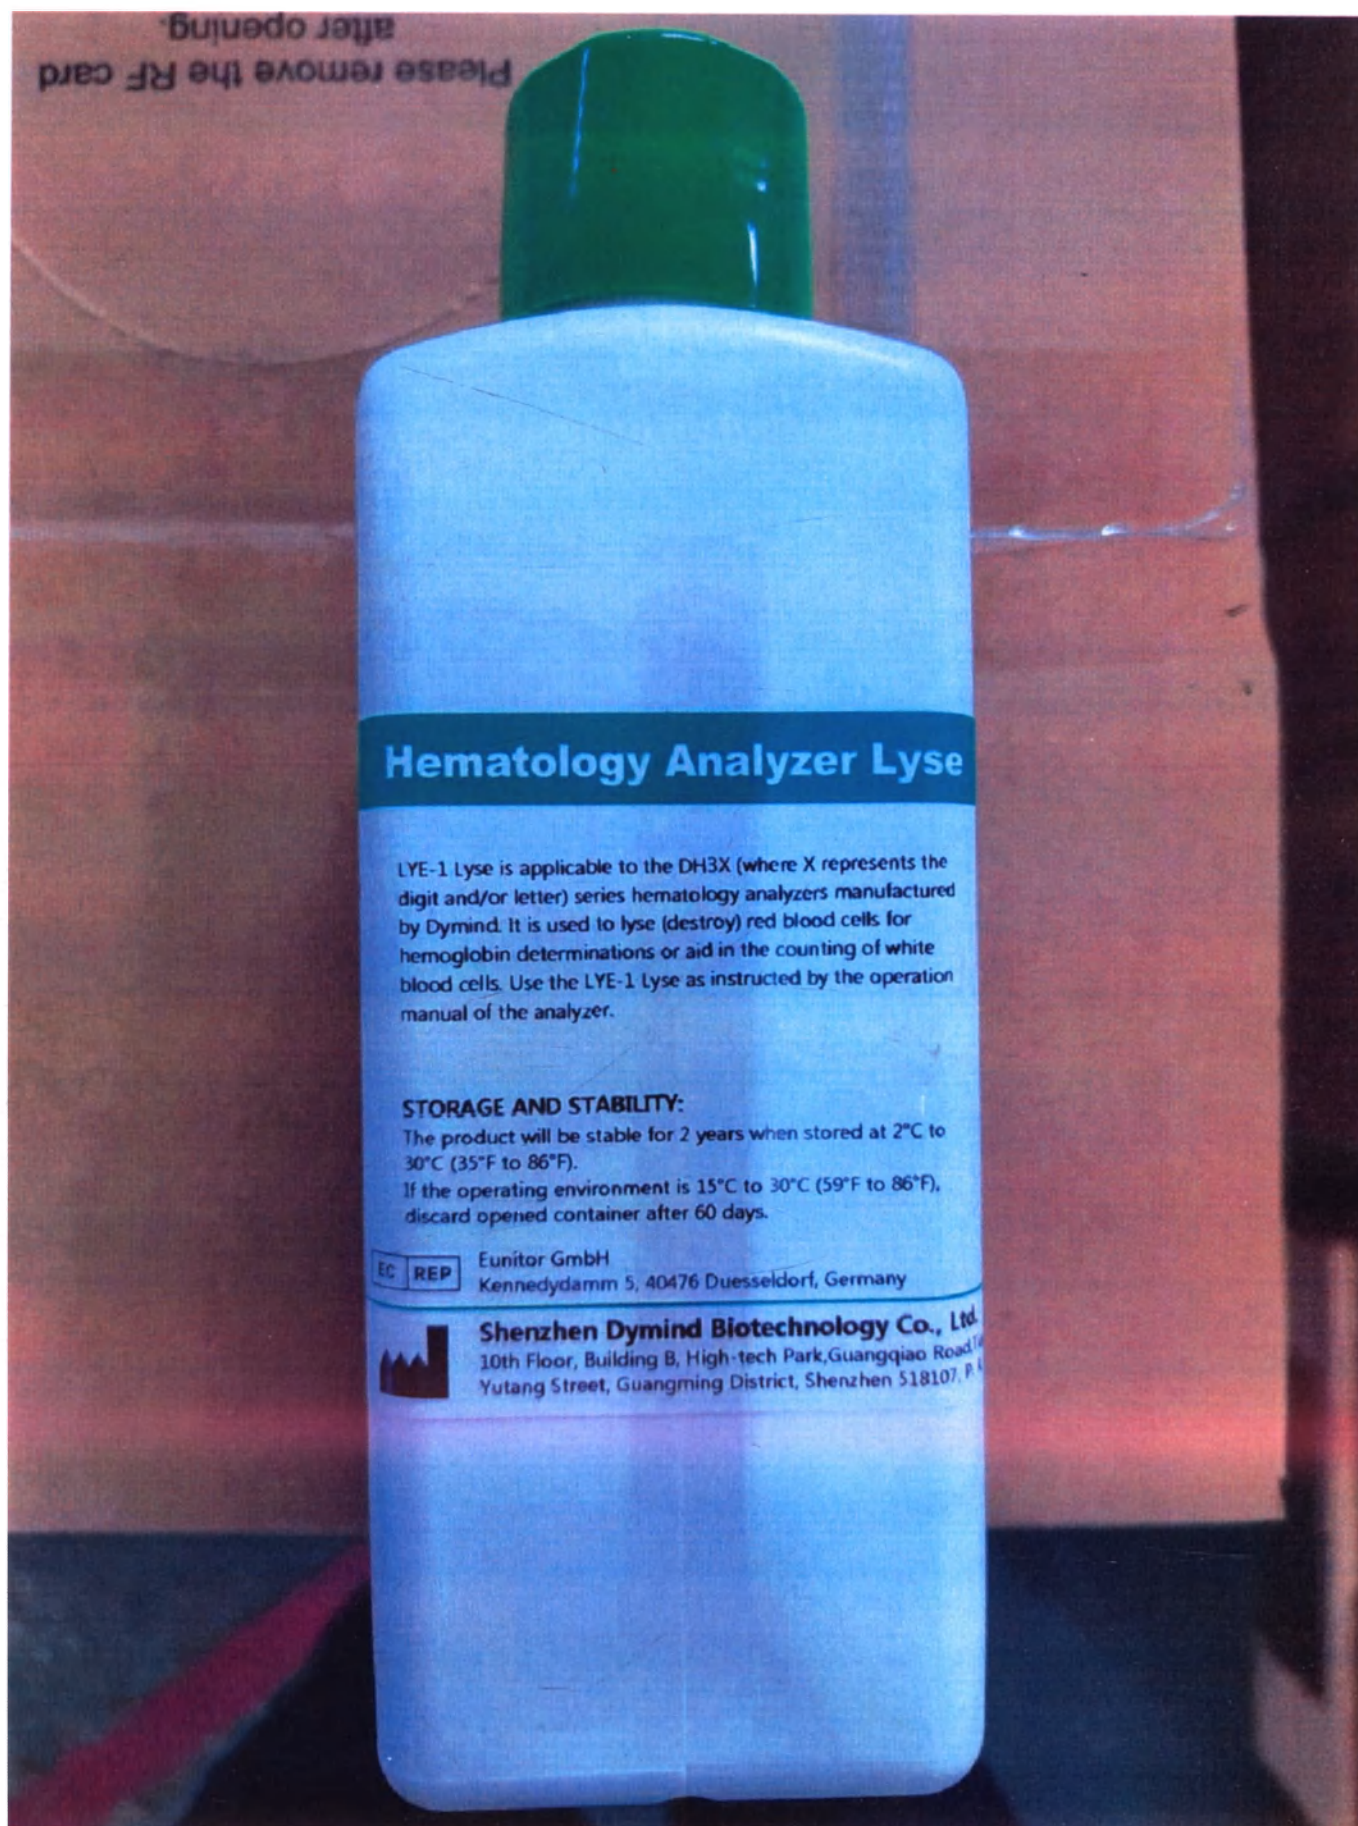


Реагент лизирующий LYE-1, 500 мл

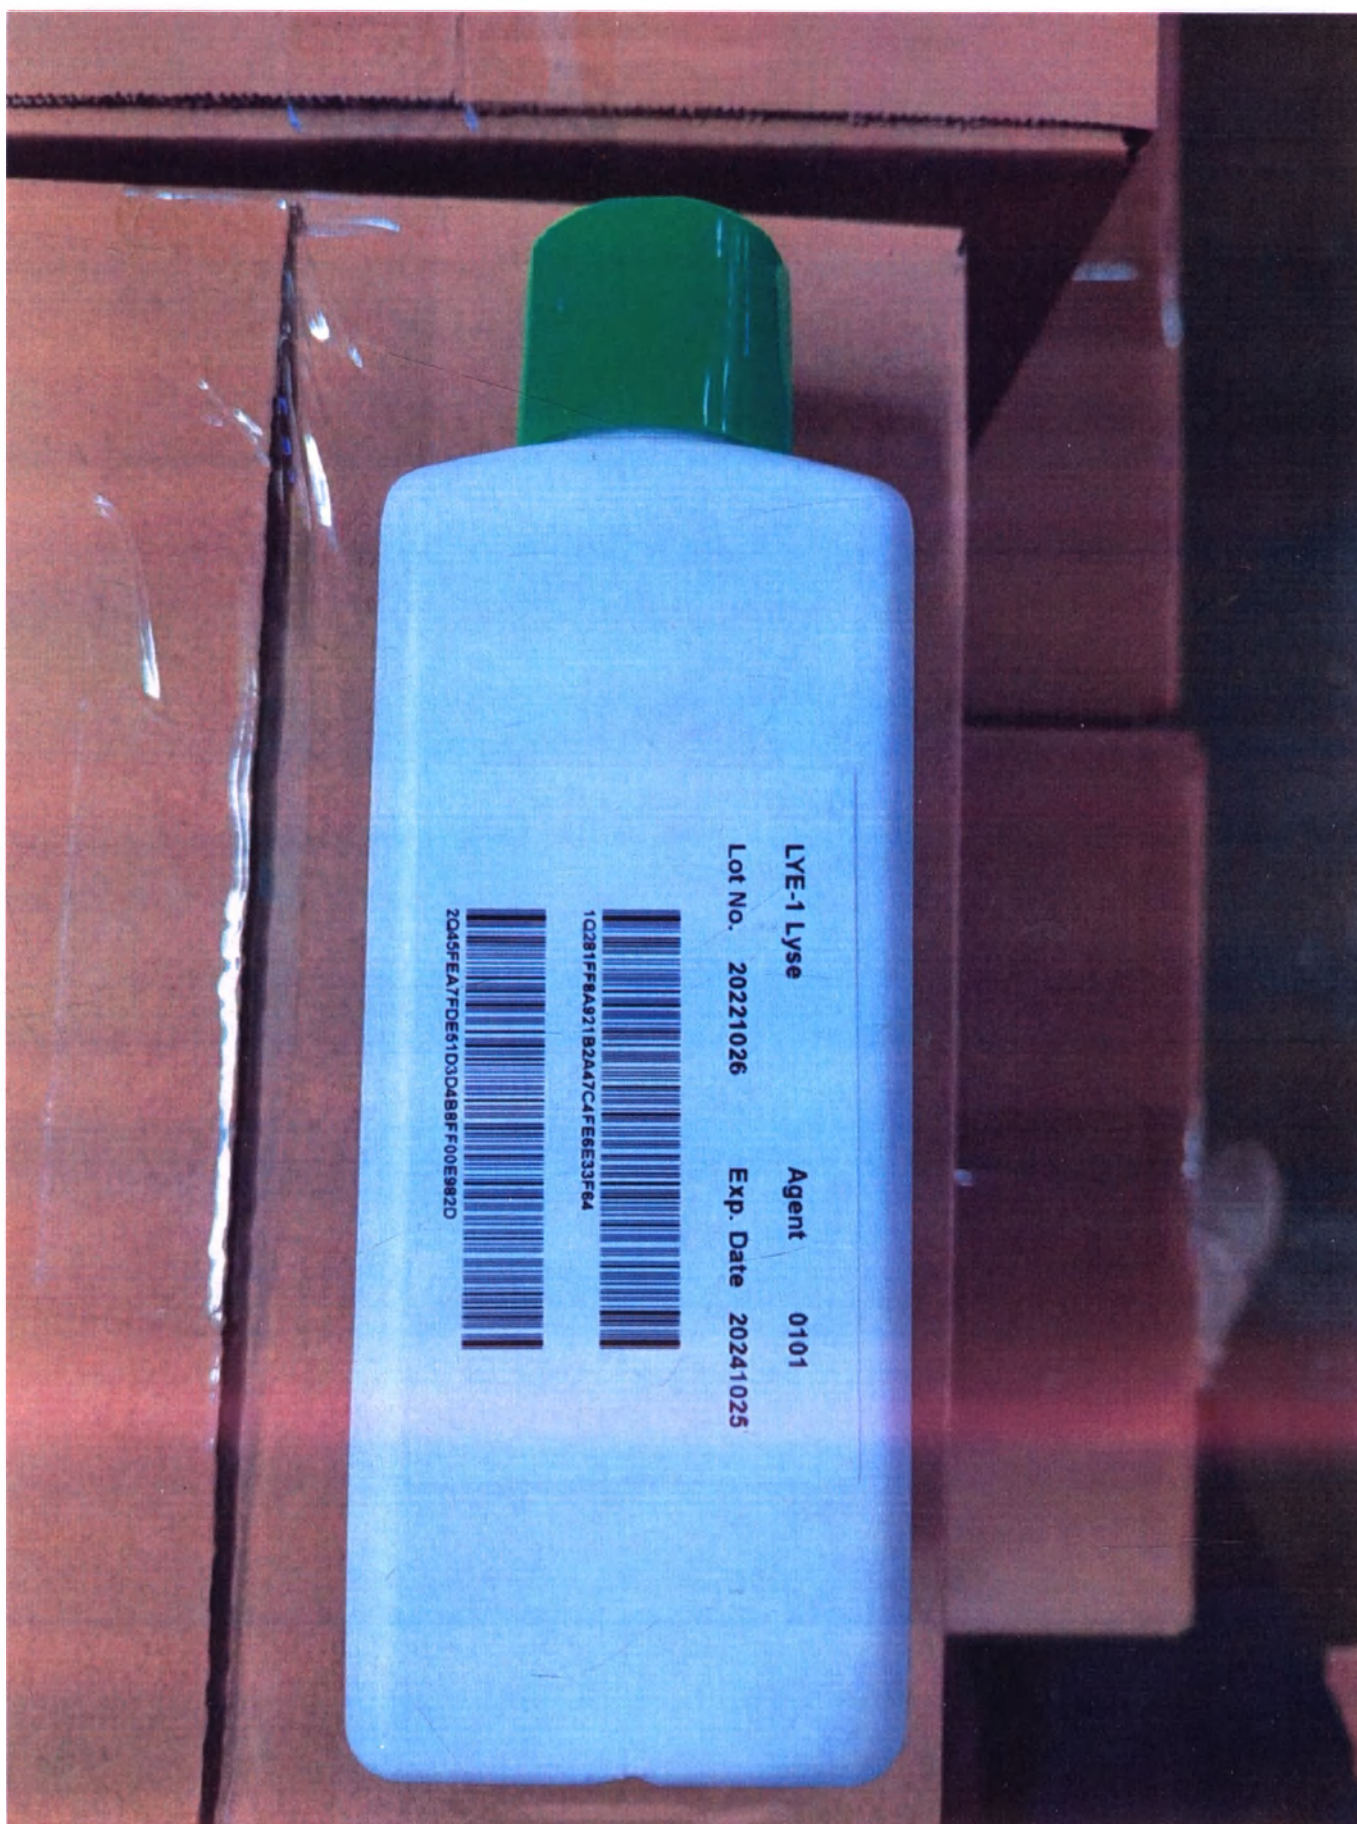

Реагент лизирующий LYE-1, 500 мл



Реагент лизирующий LYE-1, 500 мл

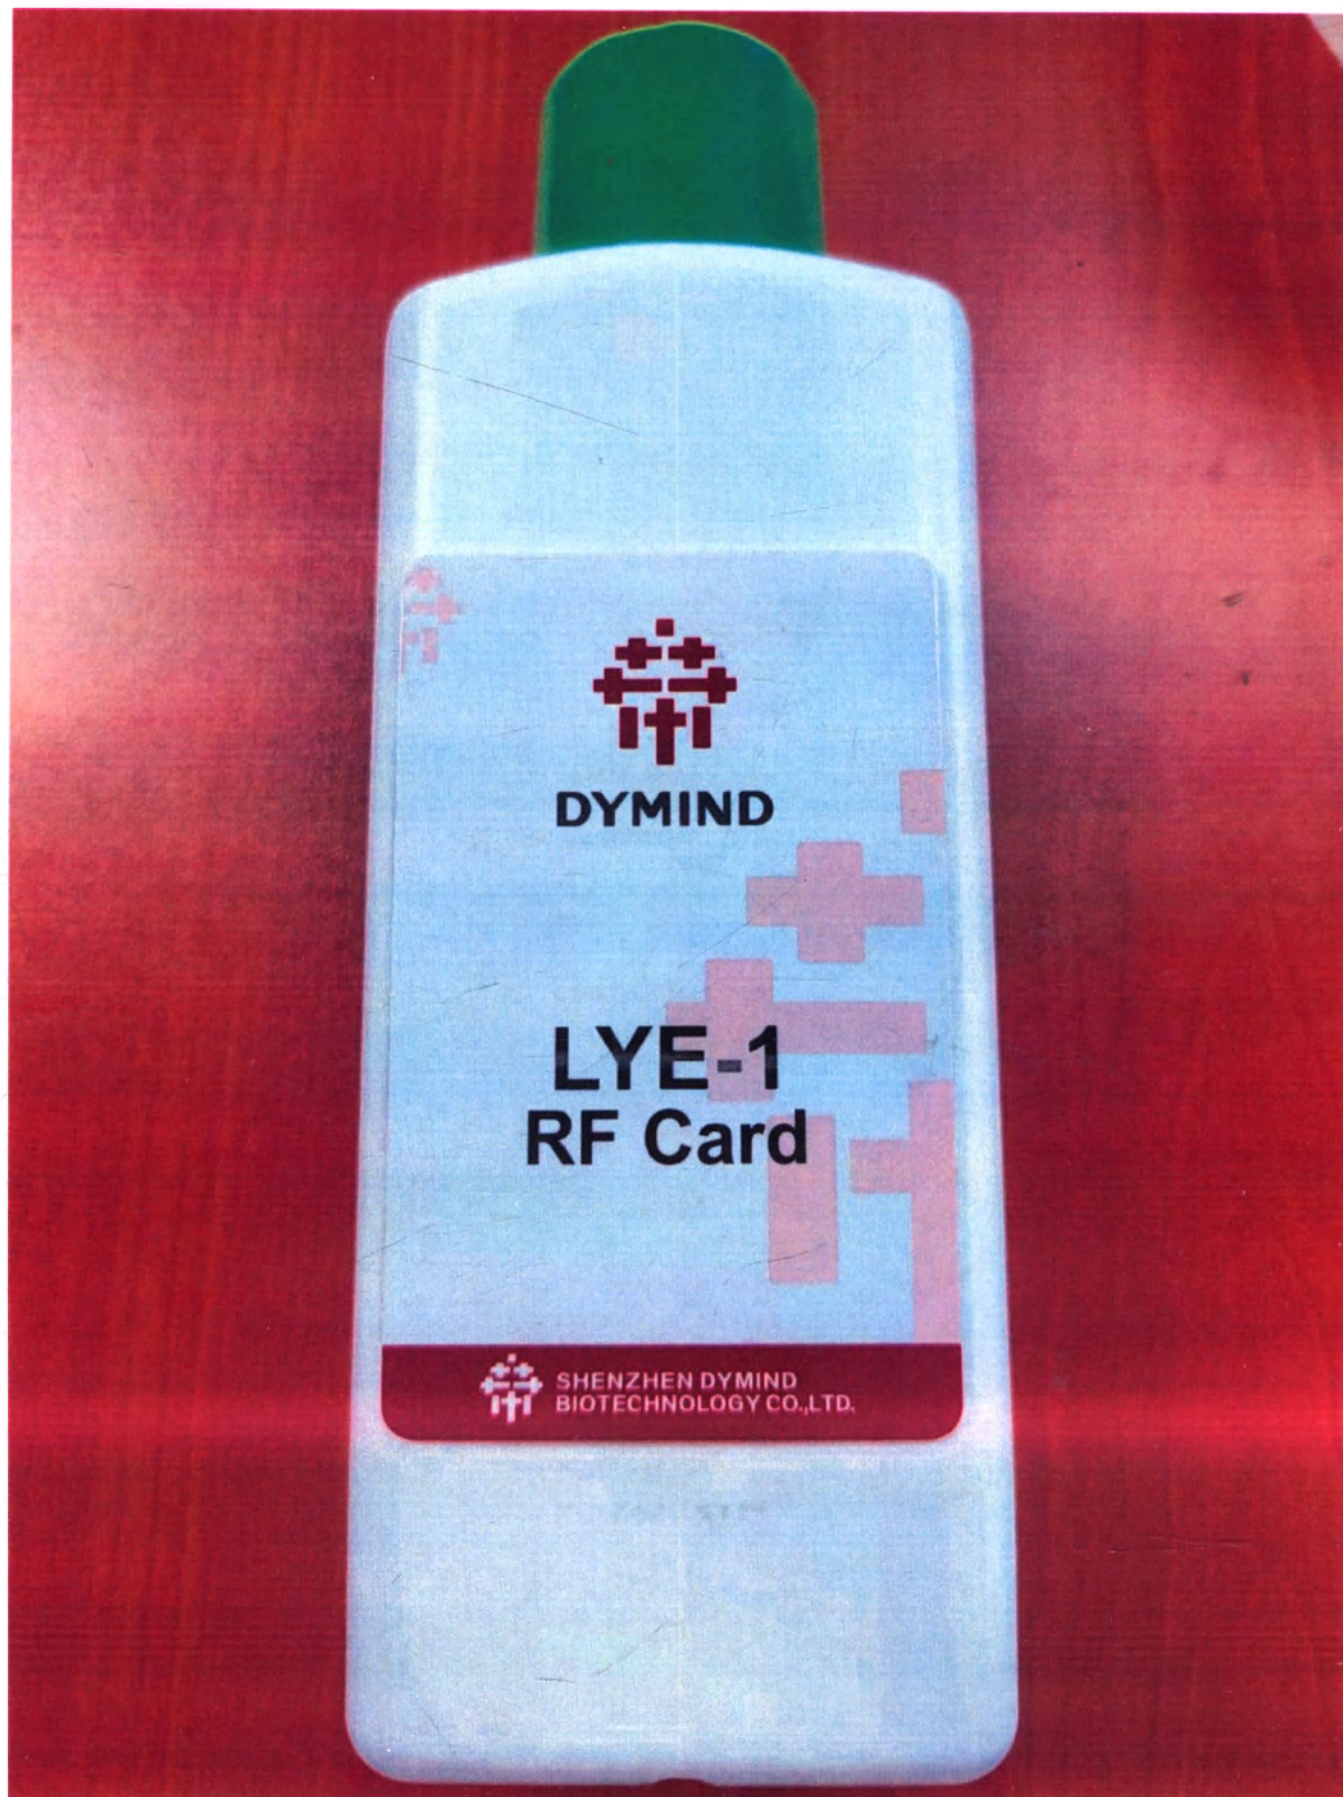

Реагент лизирующий LYE-1, 500 мл



Реагент лизирующий LYG-1, 200 мл

Hematology Analyzer Lyse

LYG-1 Lyse is applicable to the UN7X (where X represents the digit and/or letter) series hematology analyzers manufactured by Dymind. It is used to lyse (destroy) red blood cells for hemoglobin determinations or aid in the counting of white blood cells. Use the LYG-1 Lyse as instructed by the operation manual of the analyzer.

STORAGE AND STABILITY:

The product will be stable for 2 years when stored at 2°C to 30°C (35°F to 86°F).

If the operating environment is 15°C to 30°C (59°F to 86°F), discard opened container after 60 days.

EC REP

Eunitor GmbH
Kennedydamm 5, 40476 Duesseldorf, Germany



Shenzhen Dymind Biotechnology Co., Ltd.
10th Floor, Building B, High-tech Park, Guangqiao Road,
Yutang Street, Guangming District, Shenzhen 518107, P.R.

Реагент лизирующий LYG-1, 200 мл



DYMIND

WARNINGS:

1. Avoid skin or eye contact. In case of skin or eye contact, flush the affected area with plenty of water immediately and go see a doctor. In case of inhaling, immediately go see a doctor.
2. Finish product before the expiration date. Once it is opened, it should be finished within 60 days.
3. If product is frozen (either partially or completely), thaw completely, warm to room temperature and mix thoroughly by gentle inversion. Verify background results before analyzing patient samples.
4. Dispose of waste product in accordance with governmental requirements.

ACTIVE INGREDIENTS:

Surface active agent; Buffering agent;
Antifungal and antibacterial Agents

EC


Реагент лизирующий LYG-1, 200 мл



Реагент лизирующий LYG-1, 200 мл



Реагент лизирующий LYG-1, 200 мл

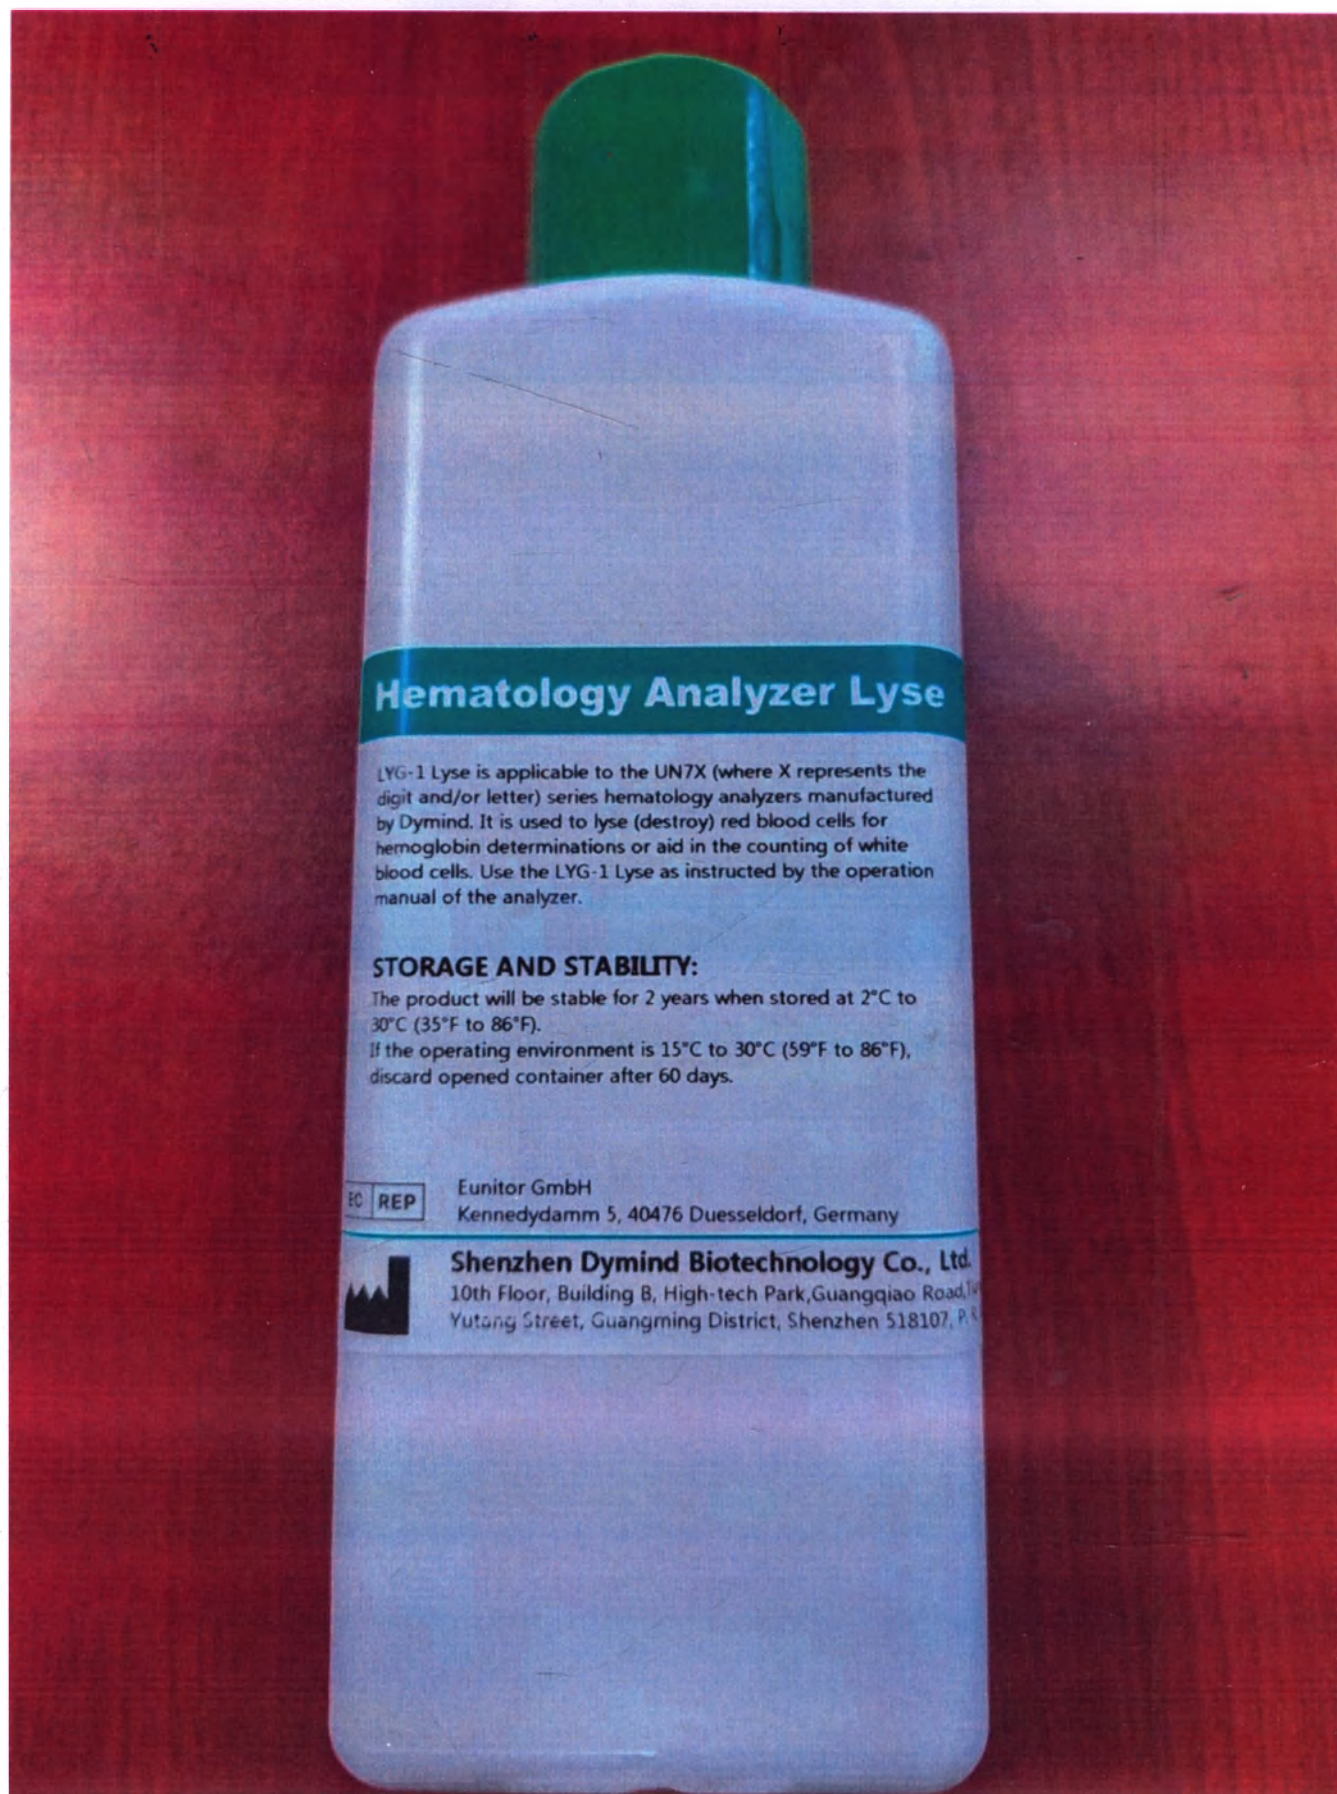

Hematology Analyzer Lyse

LYG-1 Lyse is applicable to the UN7X (where X represents the digit and/or letter) series hematology analyzers manufactured by Dymind. It is used to lyse (destroy) red blood cells for hemoglobin determinations or aid in the counting of white blood cells. Use the LYG-1 Lyse as instructed by the operation manual of the analyzer.

STORAGE AND STABILITY:

The product will be stable for 2 years when stored at 2°C to 30°C (35°F to 86°F).

If the operating environment is 15°C to 30°C (59°F to 86°F), discard opened container after 60 days.


EC REP

Eunitor GmbH
Kennedydamm 5, 40476 Duesseldorf, Germany



Shenzhen Dymind Biotechnology Co., Ltd.
10th Floor, Building B, High-tech Park, Guangqiao Road,
Yutang Street, Guangming District, Shenzhen 518107, P.R.

Реагент лизирующий LYG-1, 500 мл

**WARNINGS:**

1. Avoid skin or eye contact. In case of skin or eye contact, flush the affected area with plenty of water immediately and go see a doctor. In case of inhaling, immediately go see a doctor.
2. Finish product before the expiration date. Once it is opened, it should be finished within 60 days.
3. If product is frozen (either partially or completely), thaw completely, warm to room temperature and mix thoroughly by gentle inversion. Verify background results before analyzing patient samples.
4. Dispose of waste product in accordance with governmental requirements.

ACTIVE INGREDIENTS:

Surface active agent; Buffering agent;
Antifungal and antibacterial Agents

Реагент лизирующий LYG-1, 500 мл



Реагент лизирующий LYG-1, 500 мл




Реагент лизирующий LYG-1, 500 мл

Hematology Analyzer Lyse




DYMIND

List	Model	Specification	LOT	Production date	Expiry date	PCS
	LYE-1	200mL	2022052601	26.05.2022	25.05.2024	3
	LYE-1	200mL	2022052602	26.05.2022	25.05.2024	7
	LYG-1	200mL	2022052601	26.05.2022	25.05.2024	3
	LYG-1	200mL	2022052602	26.05.2022	25.05.2024	7



Made in China



Eunitor GmbH
Kennedydamm 5, 40476 Duesseldorf, Germany



Shenzhen Dymind Biotechnology Co., Ltd.

10th Floor, Building B, High-tech Park, Guangqiao Road, Tianliao Community, Yutang Street,
Guangming District, Shenzhen 518107, P.R.China

Country : Russia-Company BW, LLC

No : DM00000000

Транспортная маркировка

Всего прошито, пронумеровано и скреплено
печатью и подписью: 24 листа (-ов)

Генеральный директор _____ / Носова Т.А
М.П.

