


**Фотографические изображения общего вида
медицинского изделия**

**Калибраторы для обеспечения правильности количественного
определения аутоантител класса IgG к тиреоглобулину
иммунохемилюминесцентным методом в сыворотке и плазме крови
человека на иммунохимических анализаторах Alinity i
«Анти-ТГ Калибраторы (Alinity i Anti-Tg Calibrators)»**



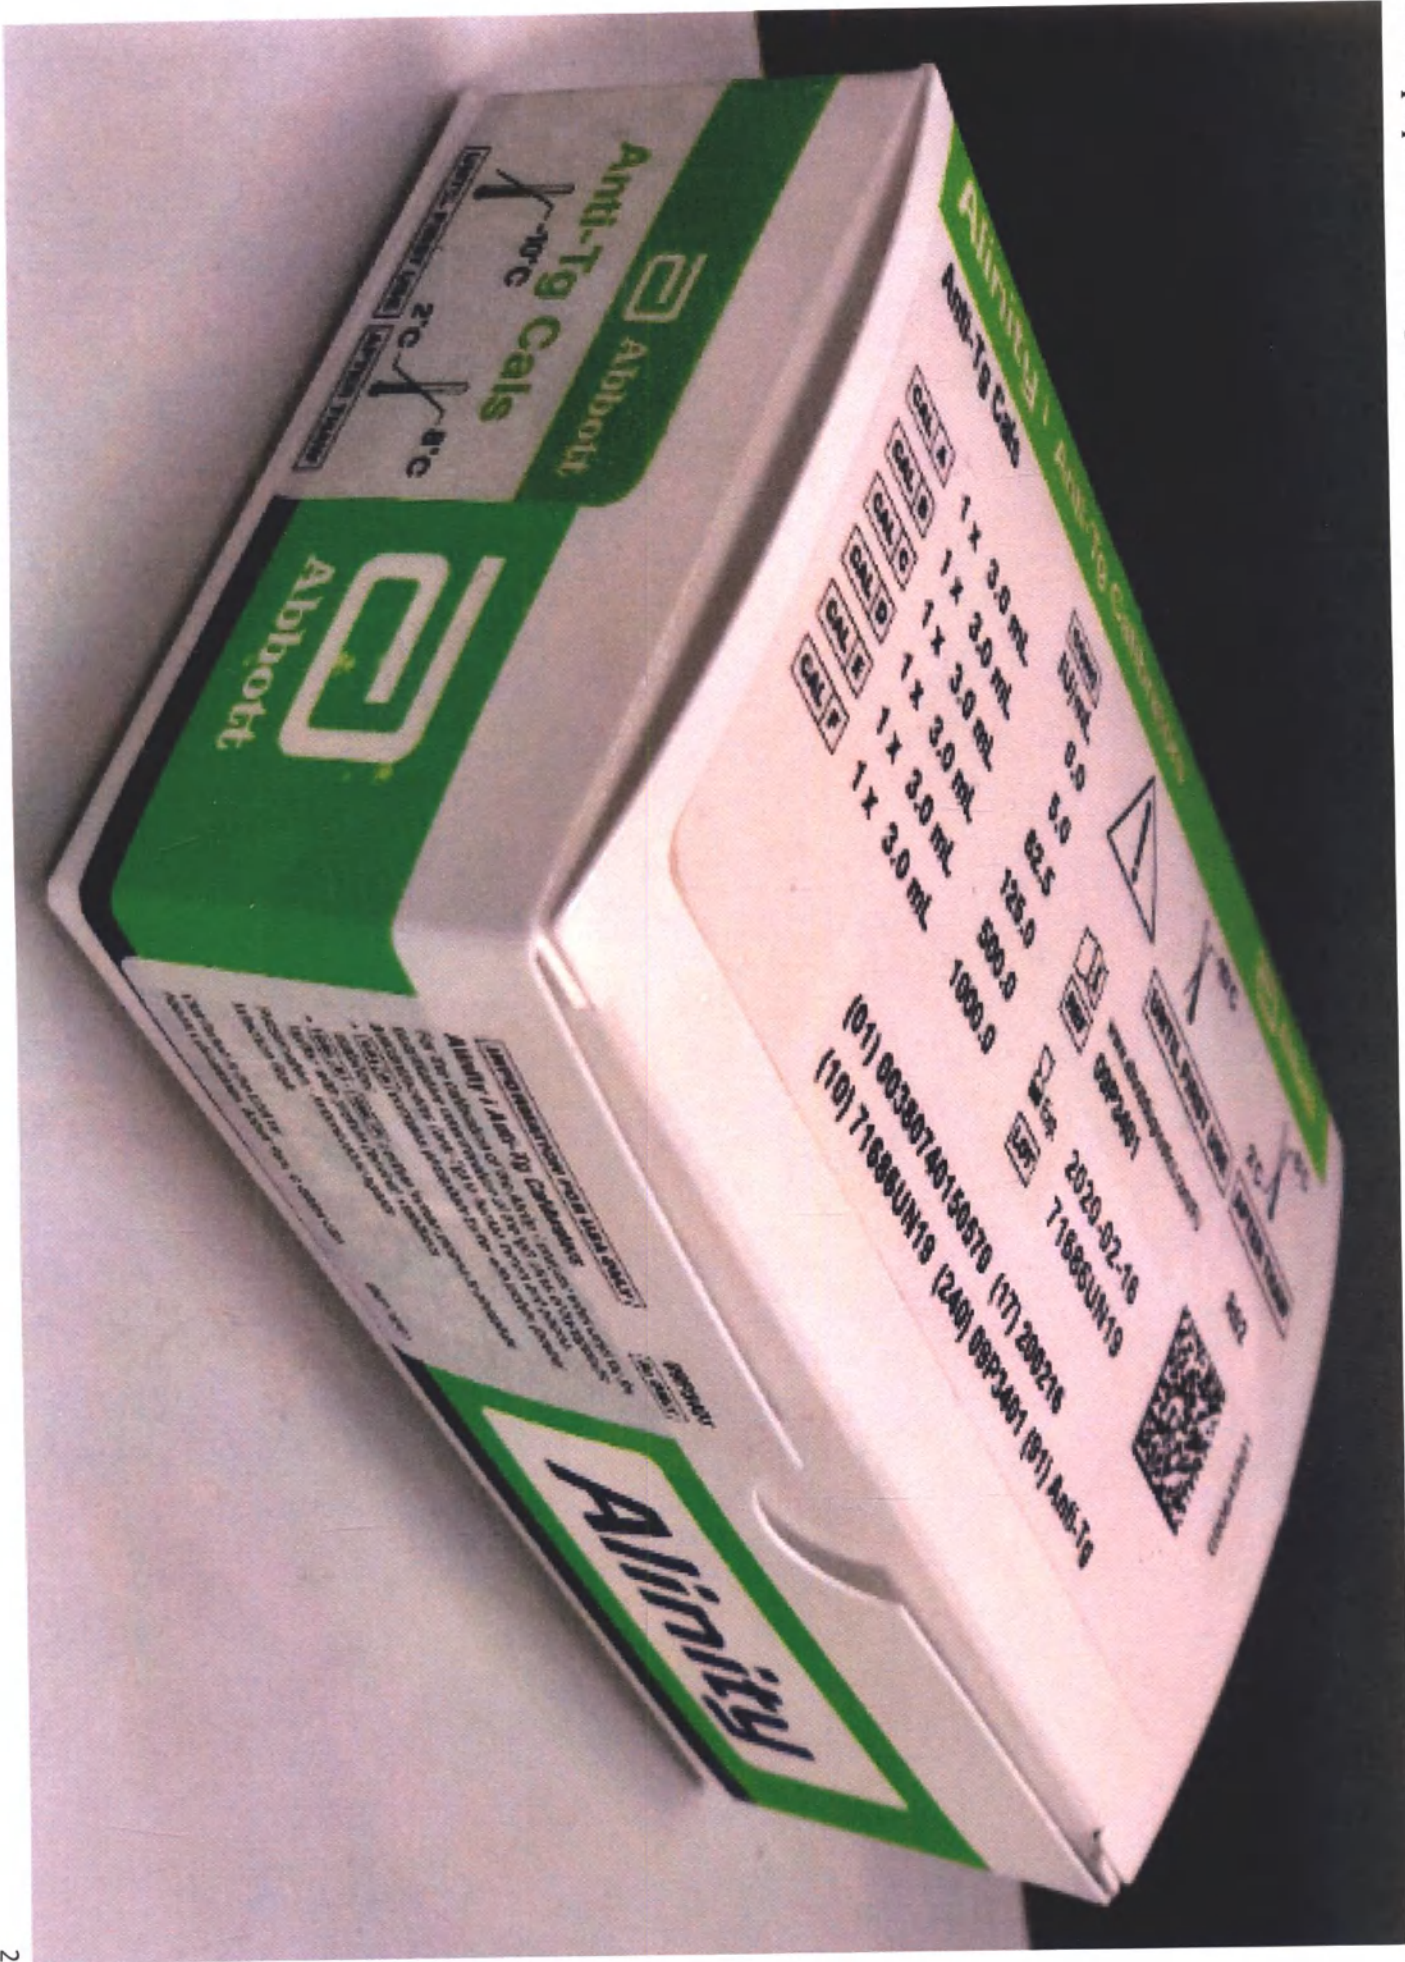

Anti-Tg Calibrators

Head Highlighted Changes: Revised March 2018

NAME

Activity 1 Anti-Tg Calibrators (also referred to as Anti-Tg Cal)

INTENDED USE

The Alinity i Anti-Ig Calibrators are for the calibration of the Alinity i analyzer when used for the quantitative determination of the IgG class of thyroglobulin autoantibodies (anti-Tg) in human serum and plasma.

For additional information, refer to the Alinity i Anti-Tg reagent insert and the Alinity ci-Series Operations Manual.

Conc	100	500.0	125.0	62.5	5.0	0.0
Cal. 8	1 x 3.0 mL					
Cal. 6	1 x 3.0 mL					
Cal. 5	1 x 3.0 mL					
Cal. 4	1 x 3.0 mL					
Cal. 3	1 x 3.0 mL					
Cal. 2	1 x 3.0 mL					
Cal. 1	1 x 3.0 mL					

Anti-Tg Cats

Alinutril

1

Abbott

UNTIL FIRST USE

216-1

MAIL FIRST CLASS
09P3401

2020-02-16
71000

71686UN19

UN19 (240) 08P2407 (31) ANN TO



Anti-Tg

1000-0000

918064AHO

19. dfg

Battery Data Sheets are available at www.safaribatteryusa.com or contact your local representative.

For a detailed discussion of safety precautions during system operation, refer to the Agency class-series Operations Manual, Section 8.

PREPARATION FOR USE

- Thaw completely at room temperature (15 to 30°C) for 45 to 60 minutes.

STORAGE



всего прошито, пронумеровано
и скреплено печатью

5 листов

Подпись _____

